


Appendix D


Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

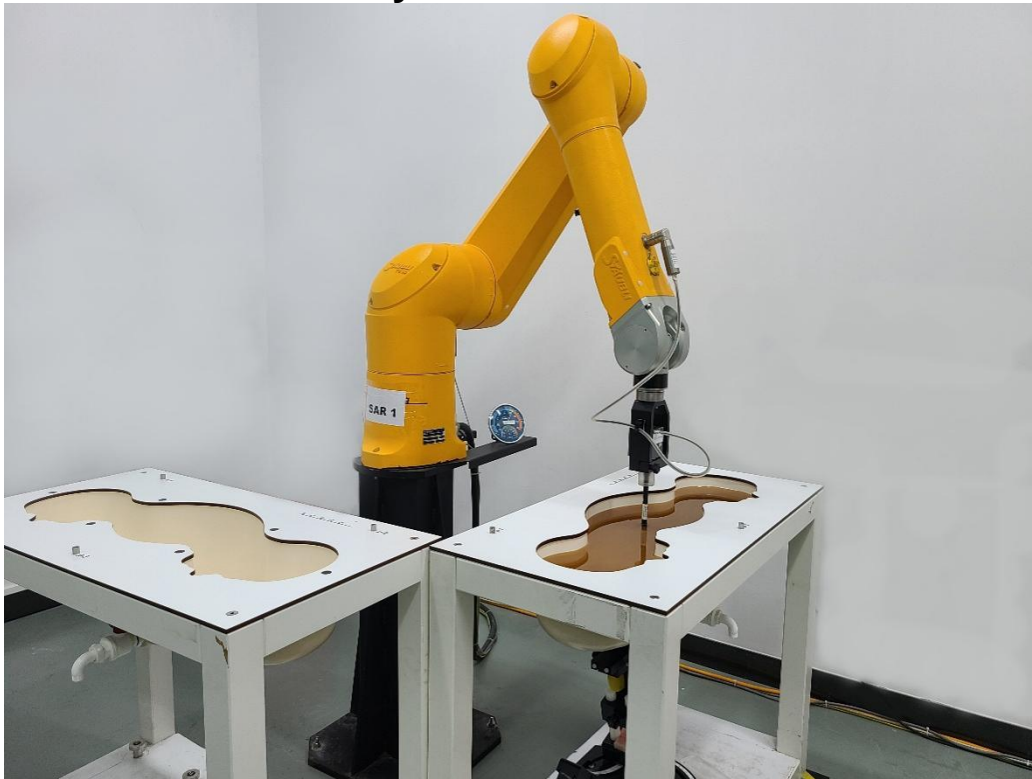

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
	NA

3. Photographs of EUT test position

Photo 2: Left Cheek

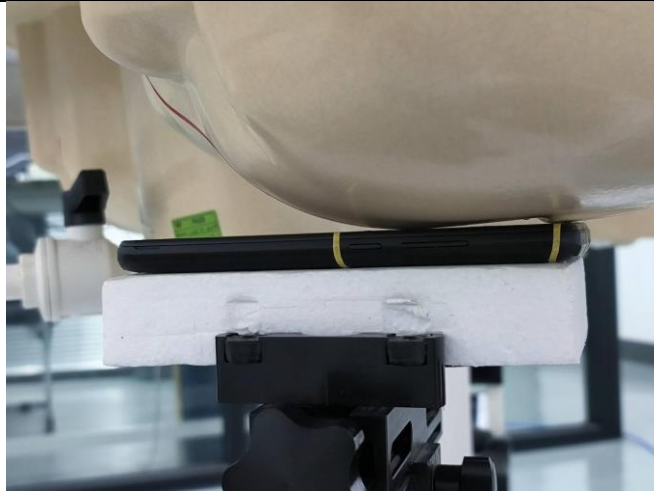


Photo 3: Left Tilted



Photo 4: Right Cheek

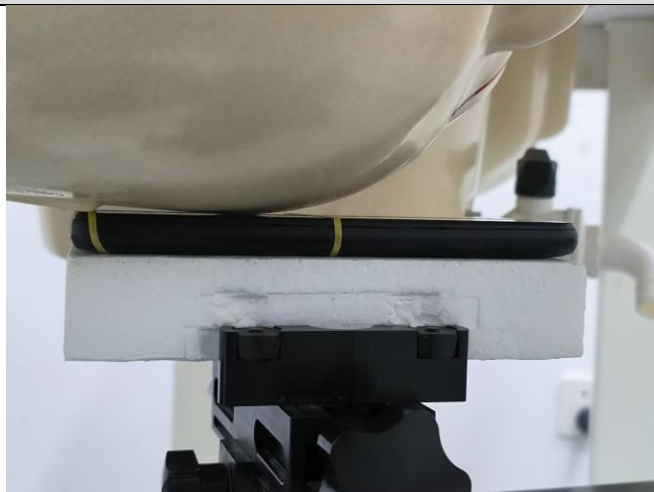


Photo 5: Right Tilted



Photo 6: Front side 15mm



Photo 7: Back side 15mm

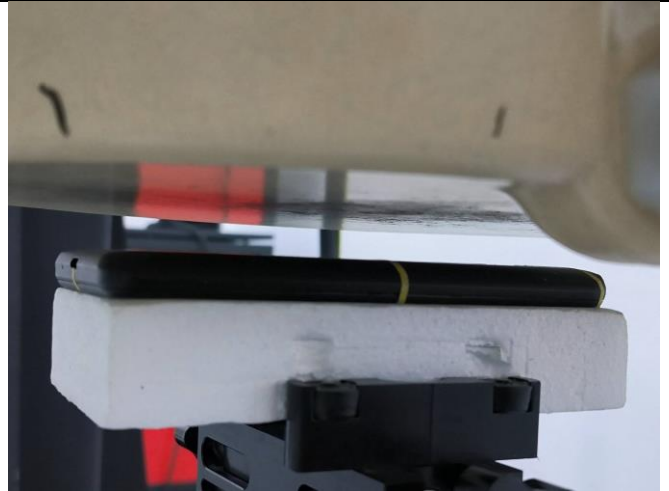


Photo 8: Front side 10mm



Photo 9: Back side 10mm



Photo 10: Left side 10mm

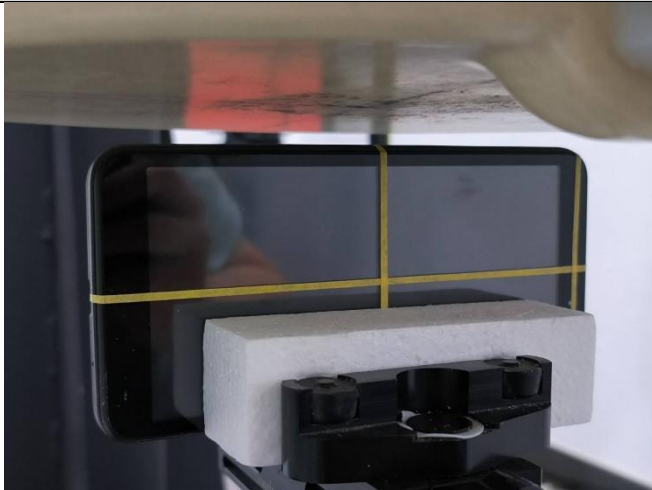


Photo 11: Right side 10mm

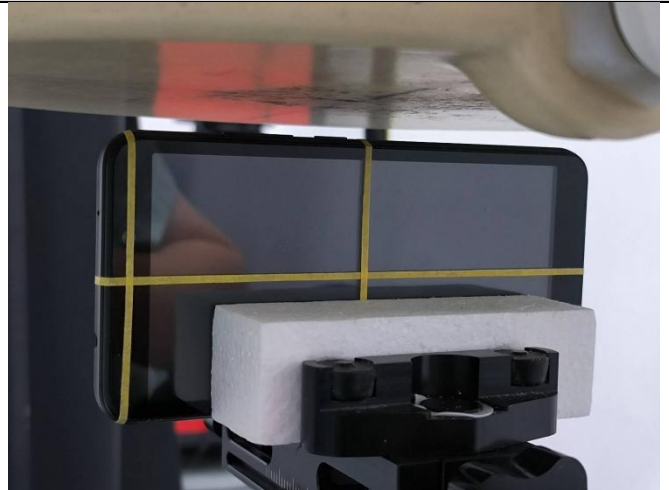


Photo 12: Top side 10mm



Photo 13: Back side 10mm



Photo 14: Front side 12mm



Photo 15: Front side 13mm



Photo 16: Left side 16mm

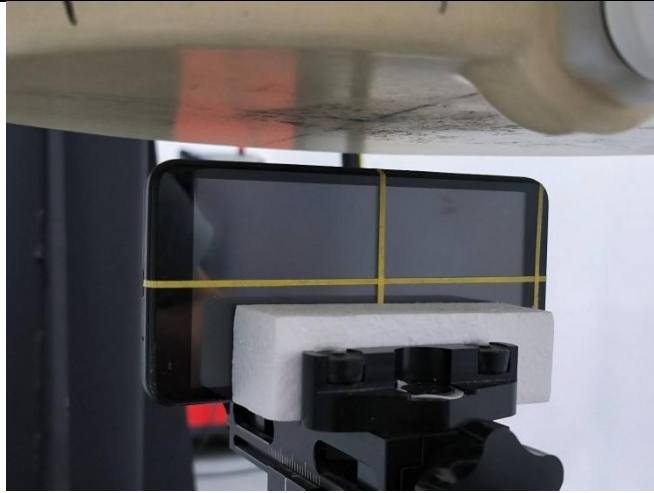


Photo 17: Right side 14mm

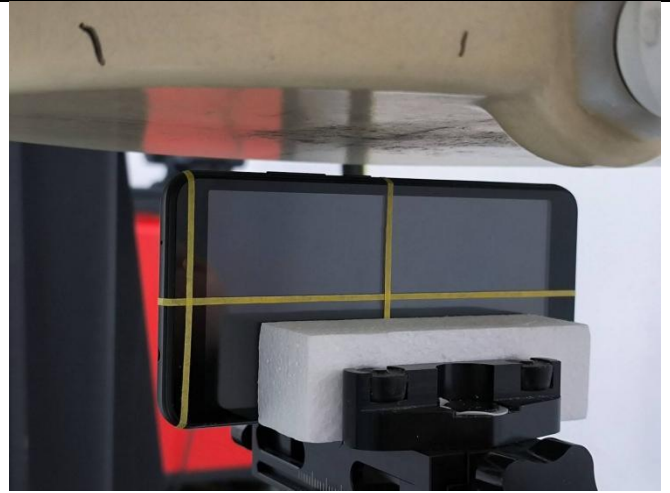


Photo 18: Top side 16mm



Photo 19: Top side 22mm



4. EUT Constructional Details

