

Appendix D for KSCR240600114701**Photographs**

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Antenna Locations
5. EUT Constructional Details

1. SAR measurement System

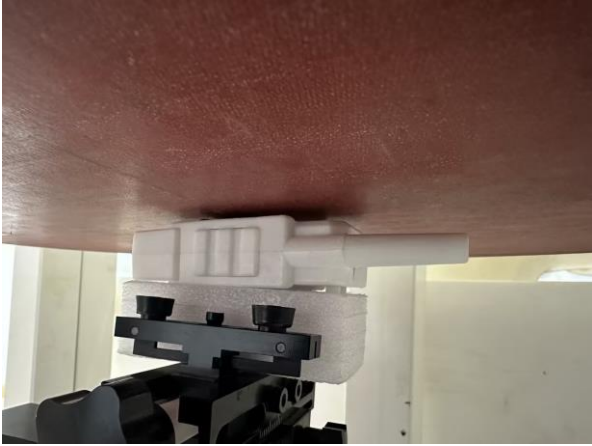
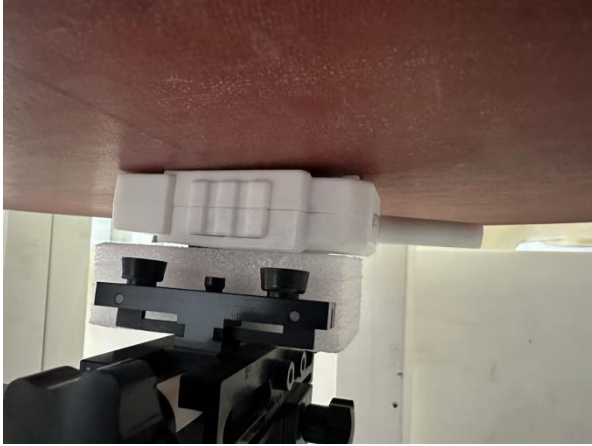


2. Photographs of Tissue Simulate Liquid

Tissue Simulant Liquid for Head 450

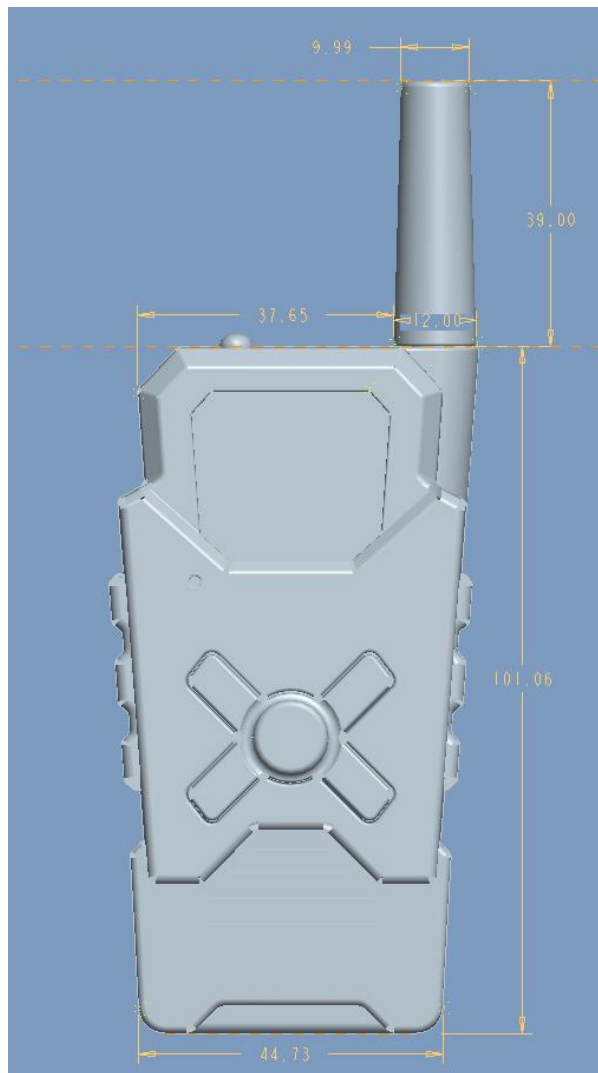


3. Photographs of EUT test position

Front Side 0mm	Back Side 0mm
 A photograph showing the front side of the EUT test position. The device is mounted on a black base, and a white plastic component is visible. The background is a reddish-brown surface.	 A photograph showing the back side of the EUT test position. The device is mounted on a black base, and a white plastic component is visible. The background is a reddish-brown surface.
Left Side 0mm	Right Side 0mm
 A photograph showing the left side of the EUT test position. The device is mounted on a black base, and a white plastic component with a black 'X' mark is visible. The background is a reddish-brown surface.	 A photograph showing the right side of the EUT test position. The device is mounted on a black base, and a white plastic component with a black 'X' mark is visible. The background is a reddish-brown surface.

Top Side 0mm	Bottom Side 0mm
	

4. EUT Antenna Locations



5. EUT Constructional Details

Refer to External and Internal Photos for SZCR2405001722AT.