



Appendix C for KSCR240600114701

Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date	Due date of calibration
Dipole	<input checked="" type="checkbox"/>	1	D450V3	1103	2024/06/03	2027/06/02
DAE	<input checked="" type="checkbox"/>	2	DAE4	918	2023/08/07	2024/08/06
Probe	<input checked="" type="checkbox"/>	3	EX3DV4	7767	2023/10/26	2024/10/25

1 Dipole

1.1 D450V3 - SN 1103

<div style="display: flex; justify-content: space-between; align-items: flex-start;"> <div style="width: 60%;"> <p>Calibration Laboratory of Schmid & Partner Engineering AG Engelshausstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: SGS Suzhou</p> <p>Certificate No: D450V3-1103_Jun24</p> </div> <div style="width: 35%; text-align: center;"> <p>S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service</p> <p>Accreditation No.: SCS 0108</p> </div> </div> <hr/> <div style="border: 1px solid black; padding: 5px;"> <p align="center">CALIBRATION CERTIFICATE</p> <p>Object: D450V3 - SN: 1103</p> <p>Calibration procedure(s): QA CAL-15 v11 Calibration Procedure for SAR Validation Sources below 700 MHz</p> <p>Calibration date: June 03, 2024</p> <p><small>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</small></p> <p><small>All calibrations have been conducted in the stated laboratory facility, environment temperature (22 ± 3)°C and humidity < 70%.</small></p> <p><small>Calibration Equipment used (MATE critical for calibration)</small></p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NP92</td> <td>SN: 104718</td> <td>26-Mar-24 (No. 211-046304037)</td> <td>Mar-25</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103244</td> <td>26-Mar-24 (No. 211-046306)</td> <td>Mar-25</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103245</td> <td>26-Mar-24 (No. 211-046307)</td> <td>Mar-25</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: 891284 (293)</td> <td>26-Mar-24 (No. 211-046488)</td> <td>Mar-25</td> </tr> <tr> <td>Type-N mismatch combination</td> <td>SN: 319882 / 00327</td> <td>26-Mar-24 (No. 211-046247)</td> <td>Mar-25</td> </tr> <tr> <td>Reference Probe EX320V4</td> <td>SN: 3077</td> <td>15-Jan-24 (No. EX3-3077_Jan24)</td> <td>Jan-25</td> </tr> <tr> <td>DAE4</td> <td>SN: 854</td> <td>15-Jan-24 (No. DAE4-854_Jan24)</td> <td>Jan-25</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power meter NP92</td> <td>SN: 107193</td> <td>08-Nov-21 (in house check Dec-22)</td> <td>In house check Dec-24</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 105052</td> <td>19-Dec-20 (in house check Dec-22)</td> <td>In house check Dec-24</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 105418</td> <td>01-Jan-24 (in house check Dec-22)</td> <td>In house check Dec-24</td> </tr> <tr> <td>RF generator HP 8548C</td> <td>SN: US3952001700</td> <td>04-Aug-19 (in house check Jun-22)</td> <td>In house check Jun-24</td> </tr> <tr> <td>Network Analyzer Agilent E8359A</td> <td>SN: USA100477</td> <td>31-Mar-14 (in house check Oct-22)</td> <td>In house check Oct-24</td> </tr> </tbody> </table> <p>Calibrated by: Jeffrey Kästman (Function: Laboratory Technician) [Signature]</p> <p>Approved by: Sven Kuhn (Function: Technical Manager)</p> <p align="right"><small>Issued: June 5, 2024</small></p> </div>	Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Power meter NP92	SN: 104718	26-Mar-24 (No. 211-046304037)	Mar-25	Power sensor NRP-Z91	SN: 103244	26-Mar-24 (No. 211-046306)	Mar-25	Power sensor NRP-Z91	SN: 103245	26-Mar-24 (No. 211-046307)	Mar-25	Reference 20 dB Attenuator	SN: 891284 (293)	26-Mar-24 (No. 211-046488)	Mar-25	Type-N mismatch combination	SN: 319882 / 00327	26-Mar-24 (No. 211-046247)	Mar-25	Reference Probe EX320V4	SN: 3077	15-Jan-24 (No. EX3-3077_Jan24)	Jan-25	DAE4	SN: 854	15-Jan-24 (No. DAE4-854_Jan24)	Jan-25	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Power meter NP92	SN: 107193	08-Nov-21 (in house check Dec-22)	In house check Dec-24	Power sensor NRP-Z91	SN: 105052	19-Dec-20 (in house check Dec-22)	In house check Dec-24	Power sensor NRP-Z91	SN: 105418	01-Jan-24 (in house check Dec-22)	In house check Dec-24	RF generator HP 8548C	SN: US3952001700	04-Aug-19 (in house check Jun-22)	In house check Jun-24	Network Analyzer Agilent E8359A	SN: USA100477	31-Mar-14 (in house check Oct-22)	In house check Oct-24	<div style="display: flex; justify-content: space-between; align-items: flex-start;"> <div style="width: 60%;"> <p>Calibration Laboratory of Schmid & Partner Engineering AG Engelshausstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: SGS Suzhou</p> <p>Certificate No: D450V3-1103_Jun24</p> </div> <div style="width: 35%; text-align: center;"> <p>S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service</p> <p>Accreditation No.: SCS 0108</p> </div> </div> <hr/> <p>Glossary:</p> <p>TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORM x,y,z N/A: not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards:</p> <ol style="list-style-type: none"> IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020. KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz" <p>Additional Documentation:</p> <p>c) DASY System Handbook</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <p><small>This reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</small></p>				
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																																																										
Power meter NP92	SN: 104718	26-Mar-24 (No. 211-046304037)	Mar-25																																																										
Power sensor NRP-Z91	SN: 103244	26-Mar-24 (No. 211-046306)	Mar-25																																																										
Power sensor NRP-Z91	SN: 103245	26-Mar-24 (No. 211-046307)	Mar-25																																																										
Reference 20 dB Attenuator	SN: 891284 (293)	26-Mar-24 (No. 211-046488)	Mar-25																																																										
Type-N mismatch combination	SN: 319882 / 00327	26-Mar-24 (No. 211-046247)	Mar-25																																																										
Reference Probe EX320V4	SN: 3077	15-Jan-24 (No. EX3-3077_Jan24)	Jan-25																																																										
DAE4	SN: 854	15-Jan-24 (No. DAE4-854_Jan24)	Jan-25																																																										
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																																																										
Power meter NP92	SN: 107193	08-Nov-21 (in house check Dec-22)	In house check Dec-24																																																										
Power sensor NRP-Z91	SN: 105052	19-Dec-20 (in house check Dec-22)	In house check Dec-24																																																										
Power sensor NRP-Z91	SN: 105418	01-Jan-24 (in house check Dec-22)	In house check Dec-24																																																										
RF generator HP 8548C	SN: US3952001700	04-Aug-19 (in house check Jun-22)	In house check Jun-24																																																										
Network Analyzer Agilent E8359A	SN: USA100477	31-Mar-14 (in house check Oct-22)	In house check Oct-24																																																										
<p>Measurement Conditions DASY system configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>DASY Version</th> <th>DASY5</th> <th>V52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>EL14 Flat Phantom</td> <td>Shell thickness: 2 ± 0.2 mm</td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>450 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p>Head TSL parameters The following parameters and calculations were applied:</p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>Nominal Head TSL parameters</th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td></td> <td>22.0 °C</td> <td>43.5</td> <td>0.87 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>45.0 ± 6 %</td> <td>0.87 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>< 0.5 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p>SAR result with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.15 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>4.63 W/kg ± 16.1 % (k=2)</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>SAR averaged over 10 cm³ (10 g) of Head TSL</th> <th>condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>0.765 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>3.08 W/kg ± 17.6 % (k=2)</td> </tr> </tbody> </table>	DASY Version	DASY5	V52.10.4	Extrapolation	Advanced Extrapolation		Phantom	EL14 Flat Phantom	Shell thickness: 2 ± 0.2 mm	Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	450 MHz ± 1 MHz		Nominal Head TSL parameters	Temperature	Permittivity	Conductivity		22.0 °C	43.5	0.87 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	45.0 ± 6 %	0.87 mho/m ± 6 %	Head TSL temperature change during test	< 0.5 °C	---	---	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	1.15 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	4.63 W/kg ± 16.1 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	condition		SAR measured	250 mW input power	0.765 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	3.08 W/kg ± 17.6 % (k=2)	<p>Appendix (Additional assessments outside the scope of SCS 0108)</p> <p>Antenna Parameters with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td>59.0 Ω ± 0.5 (k)</td> </tr> <tr> <td>Return Loss</td> <td>-21.6 dB</td> </tr> </tbody> </table> <p>General Antenna Parameters and Design</p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <tbody> <tr> <td>Electrical Delay (one direction)</td> <td>1.351 ns</td> </tr> </tbody> </table> <p><small>After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.</small></p> <p>Additional EUT Data</p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table>	Impedance, transformed to feed point	59.0 Ω ± 0.5 (k)	Return Loss	-21.6 dB	Electrical Delay (one direction)	1.351 ns	Manufactured by	SPEAG
DASY Version	DASY5	V52.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	EL14 Flat Phantom	Shell thickness: 2 ± 0.2 mm																																																											
Distance Dipole Center - TSL	15 mm	with Spacer																																																											
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																												
Frequency	450 MHz ± 1 MHz																																																												
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity																																																										
	22.0 °C	43.5	0.87 mho/m																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	45.0 ± 6 %	0.87 mho/m ± 6 %																																																										
Head TSL temperature change during test	< 0.5 °C	---	---																																																										
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	1.15 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	4.63 W/kg ± 16.1 % (k=2)																																																											
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition																																																												
SAR measured	250 mW input power	0.765 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	3.08 W/kg ± 17.6 % (k=2)																																																											
Impedance, transformed to feed point	59.0 Ω ± 0.5 (k)																																																												
Return Loss	-21.6 dB																																																												
Electrical Delay (one direction)	1.351 ns																																																												
Manufactured by	SPEAG																																																												
Certificate No: D450V3-1103_Jun24 Page 3 of 6	Certificate No: D450V3-1103_Jun24 Page 4 of 6																																																												

DASY5 Validation Report for Head TSL

Date: 03.06.2024

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1103


Communication System: UID 0 - CW; Frequency: 450 MHz
 Medium parameters used: $f = 450 \text{ MHz}$; $\sigma = 0.87 \text{ S/m}$; $\epsilon_s = 45.0$; $\rho = 1000 \text{ kg/m}^3$
 Phantom section: Flat Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.64, 10.64) @ 450 MHz; Calibrated: 10.01.2024
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 15.01.2024
- Phantom: ELJ v6.0; Type: QDOVA003AA; Serial: TP-2034
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue (d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0):


Measurement grid: $d_x=5\text{mm}$, $d_y=5\text{mm}$, $d_z=5\text{mm}$
 Reference Value = 39.05 V/m; Power Drift = 0.01 dB
 Peak SAR (extrapolated) = 1.79 W/kg
SAR1 (g) = 1.15 W/kg; SAR10 (g) = 0.765 W/kg
 Smallest distance from peaks to all points 3 dB below: Larger than measurement grid (> 15 mm)
 Ratio of SAR at M2 to SAR at M1 = 64.2%
 Maximum value of SAR (measured) = 1.55 W/kg

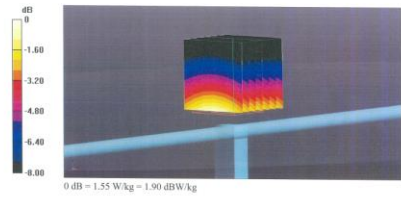

Certificate No: D450V3-1103_Jun24

Page 5 of 6

Impedance Measurement Plot for Head TSL

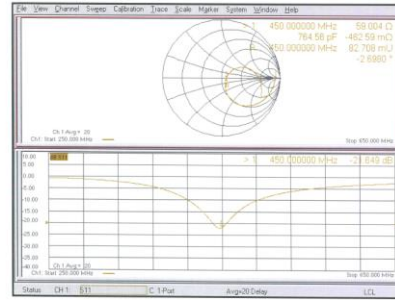

Certificate No: D450V3-1103_Jun24

Page 6 of 6

2 DAE4 - SN 918

<div style="display: flex; justify-content: space-between; align-items: center;"> <div style="text-align: center;"> <small>In Collaboration with CALIBRATION LABORATORY</small> <small>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42394833-2117 E-mail: emf@caict.ac.cn http://www.caict.ac.cn</small> </div> <div style="text-align: center;"> <small>中国合格评定委员会 CALIBRATION CNAS LISTED</small> </div> <div style="text-align: center;"> <small>中国科学院 国家认证 校准 CALIBRATION CNAS LISTED</small> </div> </div> <p style="text-align: center;">Client: Auden Certificate No: J23260347</p> <p>CALIBRATION CERTIFICATE</p> <p>Object: DAE4 - SN: 918</p> <p>Calibration Procedure(s): FF-Z11-002-01 Calibration Procedure for the Data Acquisition Electronics (DAEX)</p> <p>Calibration date: August 07, 2023</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C, and humidity<70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date(Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Process Calibrator 753</td> <td>1971018</td> <td>12-Jun-23 (CTTL No.J23X05436)</td> <td>Jun-24</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse; margin-top: 10px;"> <thead> <tr> <th>Calibrated by:</th> <th>Name</th> <th>Function</th> <th>Signature</th> </tr> </thead> <tbody> <tr> <td></td> <td>Yu Zongying</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <td>Reviewed by:</td> <td>Lin Hao</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <td>Approved by:</td> <td>Qi Dianyuan</td> <td>SAR Project Leader</td> <td></td> </tr> </tbody> </table> <p style="text-align: right;">Issued: August 13, 2023</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p style="font-size: small;">Certificate No: J23260347 Page 1 of 3</p>	Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration	Process Calibrator 753	1971018	12-Jun-23 (CTTL No.J23X05436)	Jun-24	Calibrated by:	Name	Function	Signature		Yu Zongying	SAR Test Engineer		Reviewed by:	Lin Hao	SAR Test Engineer		Approved by:	Qi Dianyuan	SAR Project Leader		<div style="display: flex; justify-content: space-between; align-items: center;"> <div style="text-align: center;"> <small>In Collaboration with CALIBRATION LABORATORY</small> <small>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42394833-2117 E-mail: emf@caict.ac.cn http://www.caict.ac.cn</small> </div> <div style="text-align: center;"> <small>中国科学院 国家认证 校准 CALIBRATION CNAS LISTED</small> </div> </div> <p style="text-align: center;">Client: Auden Certificate No: J23260347</p> <p>Glossary:</p> <p>DAE: data acquisition electronics Connector angle: information used in DASYS system to align probe sensor X to the robot coordinate system.</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> DC Voltage Measurement: Calibration Factor assessed for use in DASYS system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range. Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required. The report provide only calibration results for DAE, it does not contain other performance test results. <p style="font-size: small;">Certificate No: J23260347 Page 2 of 3</p>
Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration																						
Process Calibrator 753	1971018	12-Jun-23 (CTTL No.J23X05436)	Jun-24																						
Calibrated by:	Name	Function	Signature																						
	Yu Zongying	SAR Test Engineer																							
Reviewed by:	Lin Hao	SAR Test Engineer																							
Approved by:	Qi Dianyuan	SAR Project Leader																							
<div style="display: flex; justify-content: space-between; align-items: center;"> <div style="text-align: center;"> <small>In Collaboration with CALIBRATION LABORATORY</small> <small>Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42394833-2117 E-mail: emf@caict.ac.cn http://www.caict.ac.cn</small> </div> <div style="text-align: center;"> <small>中国科学院 国家认证 校准 CALIBRATION CNAS LISTED</small> </div> </div> <p style="text-align: center;">Client: Auden Certificate No: J23260347</p> <p>DC Voltage Measurement</p> <p>A/D Converter Resolution nominal: 1LSB = 8.1uV, full range = -100...+300 mV High Range: 1LSB = 81uV, full range = -1...+3mV Low Range: 1LSB = 810V, full range = -1...+3mV DASYS measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec.</p> <table border="1" style="width: 100%; border-collapse: collapse; margin-top: 10px;"> <thead> <tr> <th>Calibration Factors</th> <th>X</th> <th>Y</th> <th>Z</th> </tr> </thead> <tbody> <tr> <td>High Range</td> <td>404.345 ± 0.15% (k=2)</td> <td>404.521 ± 0.15% (k=2)</td> <td>404.051 ± 0.15% (k=2)</td> </tr> <tr> <td>Low Range</td> <td>4.01038 ± 0.7% (k=2)</td> <td>3.99083 ± 0.7% (k=2)</td> <td>4.00746 ± 0.7% (k=2)</td> </tr> </tbody> </table> <p>Connector Angle</p> <table border="1" style="width: 100%; border-collapse: collapse; margin-top: 10px;"> <tbody> <tr> <td>Connector Angle to be used in DASYS system</td> <td>321.5° ± 1°</td> </tr> </tbody> </table> <p style="font-size: small;">Certificate No: J23260347 Page 3 of 3</p>	Calibration Factors	X	Y	Z	High Range	404.345 ± 0.15% (k=2)	404.521 ± 0.15% (k=2)	404.051 ± 0.15% (k=2)	Low Range	4.01038 ± 0.7% (k=2)	3.99083 ± 0.7% (k=2)	4.00746 ± 0.7% (k=2)	Connector Angle to be used in DASYS system	321.5° ± 1°											
Calibration Factors	X	Y	Z																						
High Range	404.345 ± 0.15% (k=2)	404.521 ± 0.15% (k=2)	404.051 ± 0.15% (k=2)																						
Low Range	4.01038 ± 0.7% (k=2)	3.99083 ± 0.7% (k=2)	4.00746 ± 0.7% (k=2)																						
Connector Angle to be used in DASYS system	321.5° ± 1°																								

3 EX3DV4 - SN 7767

<div style="display: flex; justify-content: space-between; align-items: flex-start;"> <div style="font-size: 8px;"> <p>Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> </div> <div style="text-align: center;"> </div> <div style="font-size: 8px;"> <p>S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service</p> <p>Accreditation No.: SCS 0108</p> </div> </div> <div style="margin-top: 10px;"> <p>Client: SGS Kunshan</p> <p>Certificate No.: EX-7767_Oct23</p> </div> <div style="border: 1px solid black; padding: 5px; margin-top: 5px;"> <p align="center">CALIBRATION CERTIFICATE</p> </div> <div style="margin-top: 5px;"> <p>Object: EX3DV4 - SN:7767</p> <p>Calibration procedure(s): QA CAL-01 v1.0, QA CAL-12 v1.0, QA CAL-14 v7, QA CAL-23 v6, QA CAL-25 v6 Calibration procedure for dosimetric E-field probes</p> <p>Calibration date: October 26, 2023</p> <p>The calibration certificate documents the traceability to national standards, which relates the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature 22 ± 3°C and humidity < 70%. Calibration Equipment used (MATE critical for calibration)</p> <table border="1" style="width: 100%; font-size: 8px; border-collapse: collapse;"> <thead> <tr> <th>Primary Standards</th> <th>ID</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP-261</td> <td>SN: 104778</td> <td>30-Mar-23 (No. 217-03864-03956)</td> <td>Mar-24</td> </tr> <tr> <td>DCP GAK-12 (single lead)</td> <td>SN: 10384</td> <td>30-Mar-23 (No. 217-03864)</td> <td>Mar-24</td> </tr> <tr> <td>DCP GAK-12</td> <td>SN: 10318</td> <td>05-Oct-23 (DCP-DNA-12-1816, Oct23)</td> <td>Oct-24</td> </tr> <tr> <td>Reference SR 88 Attenuator</td> <td>SN: 025955 (200)</td> <td>30-Mar-23 (No. 217-03864)</td> <td>Mar-24</td> </tr> <tr> <td>DAE4</td> <td>SN: 660</td> <td>16-Mar-23 (No. SAE4-660, Mar23)</td> <td>Mar-24</td> </tr> <tr> <td>Reference Probe ES320X</td> <td>SN: 3013</td> <td>06-Jan-23 (No. ESS-3013_Jan23)</td> <td>Jan-24</td> </tr> </tbody> </table> <table border="1" style="width: 100%; font-size: 8px; border-collapse: collapse;"> <thead> <tr> <th>Secondary Standards</th> <th>ID</th> <th>Check Date (in hours)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power meter E44199</td> <td>SN: 0841208974</td> <td>06-Apr-16 (in house check Jun-20)</td> <td>10 hours check Jun-24</td> </tr> <tr> <td>Power sensor EA415A</td> <td>SN: NVA1488087</td> <td>06-Apr-16 (in house check Jun-20)</td> <td>10 hours check Jun-24</td> </tr> <tr> <td>Power sensor EA415A</td> <td>SN: 00011019</td> <td>06-Apr-16 (in house check Jun-20)</td> <td>10 hours check Jun-24</td> </tr> <tr> <td>RF generator HP 8840C</td> <td>SN: US304007700</td> <td>04-Aug-09 (in house check Jun-20)</td> <td>10 hours check Jun-24</td> </tr> <tr> <td>Network Analyzer E8508A</td> <td>SN: 11041098977</td> <td>31-Mar-14 (in house check Oct-22)</td> <td>10 hours check Oct-24</td> </tr> </tbody> </table> <div style="margin-top: 10px; font-size: 8px;"> <table style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 33%;">Calibrated by: Joanna Lishaj</td> <td style="width: 33%;">Function: Laboratory Technician</td> <td style="width: 33%;">Signature: </td> </tr> <tr> <td>Approved by: Sven Kuhn</td> <td>Technical Manager</td> <td></td> </tr> </table> <p align="right">Issued: October 26, 2023</p> <p align="center">This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> </div> </div>	Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration	Power meter NRP-261	SN: 104778	30-Mar-23 (No. 217-03864-03956)	Mar-24	DCP GAK-12 (single lead)	SN: 10384	30-Mar-23 (No. 217-03864)	Mar-24	DCP GAK-12	SN: 10318	05-Oct-23 (DCP-DNA-12-1816, Oct23)	Oct-24	Reference SR 88 Attenuator	SN: 025955 (200)	30-Mar-23 (No. 217-03864)	Mar-24	DAE4	SN: 660	16-Mar-23 (No. SAE4-660, Mar23)	Mar-24	Reference Probe ES320X	SN: 3013	06-Jan-23 (No. ESS-3013_Jan23)	Jan-24	Secondary Standards	ID	Check Date (in hours)	Scheduled Check	Power meter E44199	SN: 0841208974	06-Apr-16 (in house check Jun-20)	10 hours check Jun-24	Power sensor EA415A	SN: NVA1488087	06-Apr-16 (in house check Jun-20)	10 hours check Jun-24	Power sensor EA415A	SN: 00011019	06-Apr-16 (in house check Jun-20)	10 hours check Jun-24	RF generator HP 8840C	SN: US304007700	04-Aug-09 (in house check Jun-20)	10 hours check Jun-24	Network Analyzer E8508A	SN: 11041098977	31-Mar-14 (in house check Oct-22)	10 hours check Oct-24	Calibrated by: Joanna Lishaj	Function: Laboratory Technician	Signature:	Approved by: Sven Kuhn	Technical Manager		<div style="display: flex; justify-content: space-between; align-items: flex-start;"> <div style="font-size: 8px;"> <p>Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> </div> <div style="text-align: center;"> </div> <div style="font-size: 8px;"> <p>S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service</p> <p>Accreditation No.: SCS 0108</p> </div> </div> <div style="margin-top: 10px;"> <p>Glossary</p> <p>TSL: Virtual simulating liquid NORM_{x,y,z}: sensitivity in free space ConvF: sensitivity in TSL, NORM_{x,y,z} DCP: diode compression point CF: crest factor (1-Qu_{1,2}/Qu₀) of the RF signal A, B, C, D: modulation dependent linearization parameters Polarization ψ: ψ rotation around probe axis Polarization θ: θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e. $\theta = 0$ is normal to probe axis Connector Angle: information used in DASYS system to align probe sensor X to the robot coordinate system</p> </div> <div style="margin-top: 10px;"> <p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1528: "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020. b) KDB 865664: "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> </div> <div style="margin-top: 10px;"> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> • NORM_{x,y,z}: Assessed for E-field polarization $\theta = 0$ (± 90 MHz in TEM cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E-field uncertainty inside TSL (see table ConvF). • NORM_{x,y,z} = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASYS software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF. • DCP_{x,y,z}: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency nor media. • RAR: RAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics. • A_{0,x,y,z}; B_{0,x,y,z}; C_{0,x,y,z}; D_{0,x,y,z}; W_{0,x,y,z}: A, B, C, D are numerical linearization parameters assessed based on the data of calibration range expressed in RMS voltage across the diode. The parameters do not depend on frequency nor media. W₀ is the maximum power sweep for specific modulation signal. The parameters do not depend on frequency nor media. • ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f > 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASYS software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF, whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASYS version 4.4 and higher which allows extending the validity from 140 MHz to 100 MHz. • Spherical Isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna. • Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required. • Connector Angle: The angle is assessed using the information gained by determining the NORMs (no uncertainty required). </div>																														
Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration																																																																																						
Power meter NRP-261	SN: 104778	30-Mar-23 (No. 217-03864-03956)	Mar-24																																																																																						
DCP GAK-12 (single lead)	SN: 10384	30-Mar-23 (No. 217-03864)	Mar-24																																																																																						
DCP GAK-12	SN: 10318	05-Oct-23 (DCP-DNA-12-1816, Oct23)	Oct-24																																																																																						
Reference SR 88 Attenuator	SN: 025955 (200)	30-Mar-23 (No. 217-03864)	Mar-24																																																																																						
DAE4	SN: 660	16-Mar-23 (No. SAE4-660, Mar23)	Mar-24																																																																																						
Reference Probe ES320X	SN: 3013	06-Jan-23 (No. ESS-3013_Jan23)	Jan-24																																																																																						
Secondary Standards	ID	Check Date (in hours)	Scheduled Check																																																																																						
Power meter E44199	SN: 0841208974	06-Apr-16 (in house check Jun-20)	10 hours check Jun-24																																																																																						
Power sensor EA415A	SN: NVA1488087	06-Apr-16 (in house check Jun-20)	10 hours check Jun-24																																																																																						
Power sensor EA415A	SN: 00011019	06-Apr-16 (in house check Jun-20)	10 hours check Jun-24																																																																																						
RF generator HP 8840C	SN: US304007700	04-Aug-09 (in house check Jun-20)	10 hours check Jun-24																																																																																						
Network Analyzer E8508A	SN: 11041098977	31-Mar-14 (in house check Oct-22)	10 hours check Oct-24																																																																																						
Calibrated by: Joanna Lishaj	Function: Laboratory Technician	Signature:																																																																																							
Approved by: Sven Kuhn	Technical Manager																																																																																								
<p>EX3DV4 - SN:7767 October 26, 2023</p> <p>Parameters of Probe: EX3DV4 - SN:7767</p> <p>Basic Calibration Parameters</p> <table border="1" style="width: 100%; font-size: 8px; border-collapse: collapse;"> <thead> <tr> <th></th> <th>Sensor X</th> <th>Sensor Y</th> <th>Sensor Z</th> <th>Unc (k = 2)</th> </tr> </thead> <tbody> <tr> <td>Norm (uV/(m²)^{1/2}) A</td> <td>0.68</td> <td>0.72</td> <td>0.58</td> <td>±15.1%</td> </tr> <tr> <td>DCP (dBV) B</td> <td>103.4</td> <td>103.4</td> <td>108.6</td> <td>±4.7%</td> </tr> </tbody> </table> <p>Calibration Results for Modulation Response</p> <table border="1" style="width: 100%; font-size: 8px; border-collapse: collapse;"> <thead> <tr> <th rowspan="2">Mod</th> <th rowspan="2">Communication System Name</th> <th colspan="3">A</th> <th colspan="3">B</th> <th rowspan="2">VR</th> <th rowspan="2">Max dev.</th> <th rowspan="2">Max Unc[#]</th> </tr> <tr> <th>dB</th> <th>dB</th> <th>dB</th> <th>dB</th> <th>dB</th> <th>dB</th> </tr> </thead> <tbody> <tr> <td>0</td> <td>CW</td> <td>X</td> <td>0.00</td> <td>0.00</td> <td>1.00</td> <td>0.00</td> <td>120.0</td> <td>±1.9%</td> <td>±4.7%</td> </tr> <tr> <td></td> <td></td> <td>Y</td> <td>0.00</td> <td>0.00</td> <td>1.00</td> <td>0.00</td> <td>148.5</td> <td></td> <td></td> </tr> <tr> <td></td> <td></td> <td>Z</td> <td>0.00</td> <td>0.00</td> <td>1.00</td> <td>0.00</td> <td>136.6</td> <td></td> <td></td> </tr> </tbody> </table> <p>The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>¹ The uncertainties of Norm X, Y, Z do not show the E-field uncertainty inside TSL (see Page 6).</p> <p>² Coverage factor: uncertainty for maximum searched field strength.</p> <p>³ Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.</p>		Sensor X	Sensor Y	Sensor Z	Unc (k = 2)	Norm (uV/(m ²) ^{1/2}) A	0.68	0.72	0.58	±15.1%	DCP (dBV) B	103.4	103.4	108.6	±4.7%	Mod	Communication System Name	A			B			VR	Max dev.	Max Unc [#]	dB	dB	dB	dB	dB	dB	0	CW	X	0.00	0.00	1.00	0.00	120.0	±1.9%	±4.7%			Y	0.00	0.00	1.00	0.00	148.5					Z	0.00	0.00	1.00	0.00	136.6			<p>EX3DV4 - SN:7767 October 26, 2023</p> <p>Parameters of Probe: EX3DV4 - SN:7767</p> <p>Other Probe Parameters</p> <table border="1" style="width: 100%; font-size: 8px; border-collapse: collapse;"> <thead> <tr> <th>Parameter</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>Sensor Arrangement</td> <td>Triangular</td> </tr> <tr> <td>Connector Angle</td> <td>45°/9°</td> </tr> <tr> <td>Mechanical Surface Detection Mode</td> <td>enabled</td> </tr> <tr> <td>Optical Surface Detection Mode</td> <td>disabled</td> </tr> <tr> <td>Probe Overall Length</td> <td>337 mm</td> </tr> <tr> <td>Probe Body Diameter</td> <td>10 mm</td> </tr> <tr> <td>Tip Length</td> <td>9 mm</td> </tr> <tr> <td>Tip Diameter</td> <td>2.5 mm</td> </tr> <tr> <td>Probe Tip to Sensor X Calibration Point</td> <td>1 mm</td> </tr> <tr> <td>Probe Tip to Sensor Y Calibration Point</td> <td>1 mm</td> </tr> <tr> <td>Probe Tip to Sensor Z Calibration Point</td> <td>1 mm</td> </tr> <tr> <td>Recorded Measurement Distance from Surface</td> <td>1.4 mm</td> </tr> </tbody> </table> <p>Note: Measurement distance from surface can be increased to 3.4 mm for an Area Scan.</p>	Parameter	Value	Sensor Arrangement	Triangular	Connector Angle	45°/9°	Mechanical Surface Detection Mode	enabled	Optical Surface Detection Mode	disabled	Probe Overall Length	337 mm	Probe Body Diameter	10 mm	Tip Length	9 mm	Tip Diameter	2.5 mm	Probe Tip to Sensor X Calibration Point	1 mm	Probe Tip to Sensor Y Calibration Point	1 mm	Probe Tip to Sensor Z Calibration Point	1 mm	Recorded Measurement Distance from Surface	1.4 mm
	Sensor X	Sensor Y	Sensor Z	Unc (k = 2)																																																																																					
Norm (uV/(m ²) ^{1/2}) A	0.68	0.72	0.58	±15.1%																																																																																					
DCP (dBV) B	103.4	103.4	108.6	±4.7%																																																																																					
Mod	Communication System Name	A			B			VR	Max dev.	Max Unc [#]																																																																															
		dB	dB	dB	dB	dB	dB																																																																																		
0	CW	X	0.00	0.00	1.00	0.00	120.0	±1.9%	±4.7%																																																																																
		Y	0.00	0.00	1.00	0.00	148.5																																																																																		
		Z	0.00	0.00	1.00	0.00	136.6																																																																																		
Parameter	Value																																																																																								
Sensor Arrangement	Triangular																																																																																								
Connector Angle	45°/9°																																																																																								
Mechanical Surface Detection Mode	enabled																																																																																								
Optical Surface Detection Mode	disabled																																																																																								
Probe Overall Length	337 mm																																																																																								
Probe Body Diameter	10 mm																																																																																								
Tip Length	9 mm																																																																																								
Tip Diameter	2.5 mm																																																																																								
Probe Tip to Sensor X Calibration Point	1 mm																																																																																								
Probe Tip to Sensor Y Calibration Point	1 mm																																																																																								
Probe Tip to Sensor Z Calibration Point	1 mm																																																																																								
Recorded Measurement Distance from Surface	1.4 mm																																																																																								

EX3D04 - SN:7767 October 26, 2023

Parameters of Probe: EX3D04 - SN:7767

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz] ¹⁾	Relative Permittivity ²⁾	Conductivity ³⁾ [S/m]	CorrF X	CorrF Y	CorrF Z	Alpha ⁴⁾	Depth ⁵⁾ [mm]	Unc. [k=2]
150	52.3	0.78	13.37	13.37	13.37	0.00	1.25	±13.5%
450	43.5	0.87	11.82	11.82	11.82	0.10	1.30	±13.3%
750	41.9	0.89	10.54	10.54	10.87	0.59	1.27	±12.6%
850	41.5	0.90	10.39	9.85	10.00	0.36	1.27	±12.0%
900	41.5	0.97	10.29	9.75	9.99	0.58	1.27	±12.0%
1750	40.1	1.27	9.45	8.73	9.34	0.24	1.27	±12.0%
1900	40.0	1.40	8.54	7.56	8.42	0.26	1.27	±12.0%
2100	39.8	1.49	8.41	7.82	8.34	0.28	1.27	±12.0%
2300	39.5	1.67	8.70	8.12	8.61	0.29	1.27	±12.0%
2450	39.2	1.80	8.38	7.75	8.29	0.28	1.27	±12.0%
2800	38.0	1.98	8.01	7.49	7.95	0.27	1.27	±12.0%
3300	36.2	2.71	7.41	6.83	7.31	0.33	1.27	±14.0%
3500	37.9	2.91	7.54	7.07	7.52	0.34	1.27	±14.0%
3700	37.7	3.12	7.21	6.82	7.10	0.34	1.27	±14.0%
3900	37.5	3.32	7.17	6.59	7.08	0.34	1.27	±14.0%
4100	37.2	3.53	6.85	6.39	6.86	0.35	1.27	±14.0%
4200	37.1	3.63	6.64	6.09	6.55	0.35	1.27	±14.0%
4400	36.9	3.84	6.59	6.06	6.50	0.36	1.27	±14.0%
4600	36.7	4.04	6.45	6.11	6.57	0.36	1.27	±14.0%
4800	36.4	4.25	6.78	6.23	6.87	0.36	1.27	±14.0%
4900	36.2	4.40	6.43	6.17	6.30	0.39	1.28	±14.0%
5000	36.0	4.66	6.01	5.50	5.93	0.30	1.80	±14.0%
5300	35.9	4.76	5.80	5.38	5.75	0.29	1.67	±14.0%
5500	35.6	4.96	5.50	5.07	5.48	0.32	1.70	±14.0%
9800	35.5	5.07	5.25	4.78	5.18	0.34	1.75	±14.0%
5800	35.3	5.27	5.26	4.79	5.17	0.34	1.88	±14.0%

¹⁾ Frequency validity above 200 MHz and ±10 MHz only applies for D0307-4 and higher level probe (R2), else it is restricted to ±10 MHz. The uncertainty of the R22 of the CorrF factor varies at calibration frequency and the uncertainty for the rest of the frequency band. Frequency validity below 300 MHz is ±1%, 15, 45, 60 and 70 MHz for CorrF appearance at 0, 90, 180, 270 and 315 degrees respectively. Validity of CorrF assessed at 600 MHz, 1800 MHz, and 2500 MHz presented at 135 degrees > 0-90 MHz. Above 5.5 GHz frequency validity can be extended to ±10 MHz.

²⁾ The probe was calibrated using Relative Permittivity (R22) that deviate less or equal to the target value (the relative uncertainty is 11.1% for $0.7 - 2.5 \text{ GHz}$ and 13.1% for $3 - 6 \text{ GHz}$).

³⁾ AlphaDepth was determined during calibration. SPAD measures that the weighting correction due to the boundary effect after compensation is always less than 1% for frequencies below 3 GHz and below 40% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX-7767_0423 Page 5 of 9

EX3D04 - SN:7767 October 26, 2023

Frequency Response of E-Field

(TEM-Cell#1110 EXX, Waveguide:R22)

Uncertainty of Frequency Response of E-Field: ±6.3% (k=2)

Certificate No: EX-7767_0423 Page 6 of 9

EX3D04 - SN:7767 October 26, 2023

Receiving Pattern $(\theta) = 0^\circ$

1-600MHz, TEM, 0°

1-1900MHz, R22, 0°

Uncertainty of Axial Isotropy Assessment: ±0.5% (k=2)

Certificate No: EX-7767_0423 Page 7 of 9

EX3D04 - SN:7767 October 26, 2023

Dynamic Range I(SAR_{head})

(TEM cell, f_{cell} = 1900MHz)


Uncertainty of Linearity Assessment: ±0.6% (k=2)

Certificate No: EX-7767_0423 Page 8 of 9

EX3DN4 - SN:7767


October 26, 2023

Conversion Factor Assessment



Deviation from Isotropy in Liquid

Error (p, 0), I = 900 MHz



Certificate No: EX-7767_Oct23

Page 9 of 9