



Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details





1. SAR measurement System



2. Photographs of Tissue Simulate Liquid


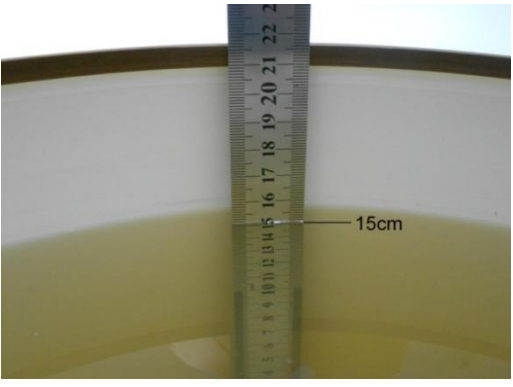




Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Head 2600
	

Photo 7: Tissue Simulant Liquid for Head 5-6GHz	NA
--	-----------





3. Photographs of EUT test position

Photo 8: Left touch cheek

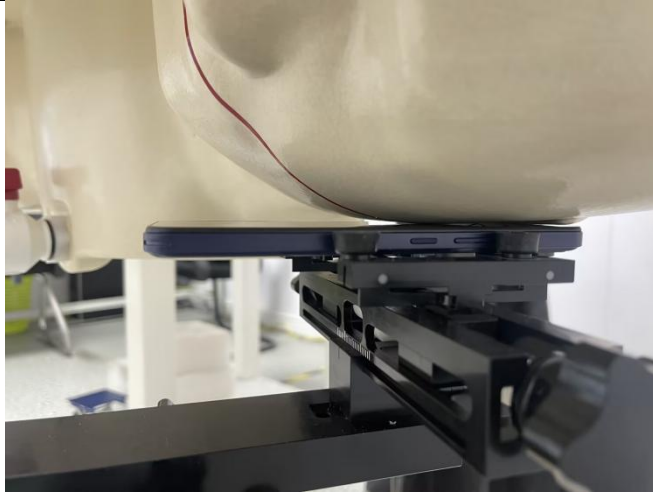


Photo 9: Left tilted 15 degree

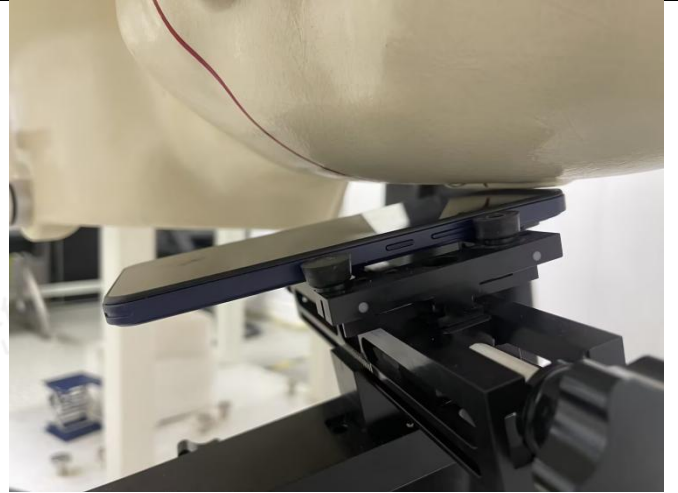


Photo 10: Right touch cheek

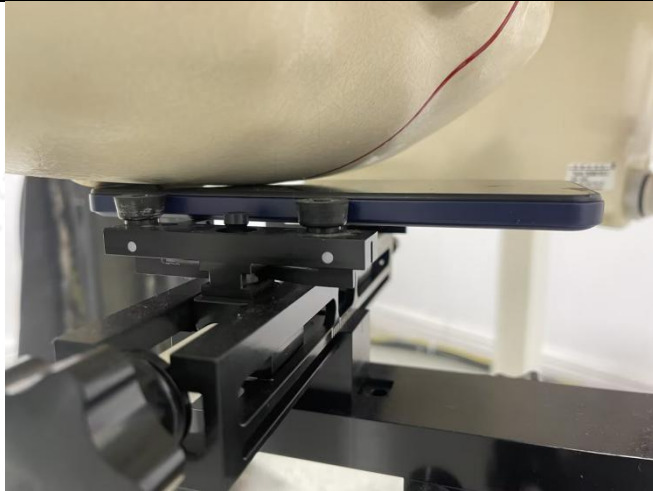


Photo 11: Right tilted 15 degree

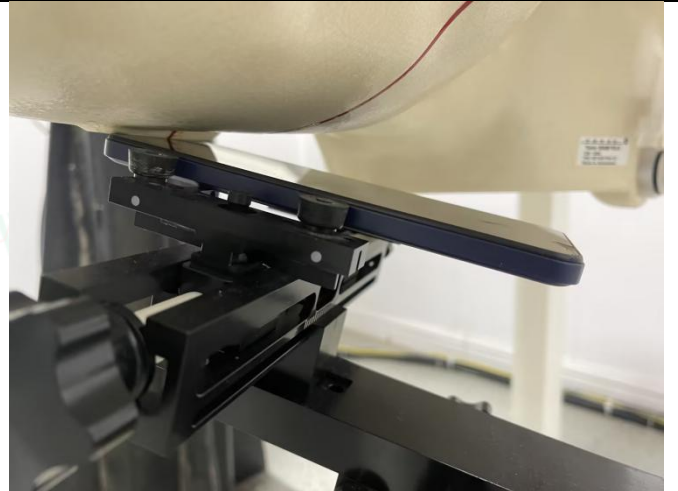


Photo 12: Front side 10mm



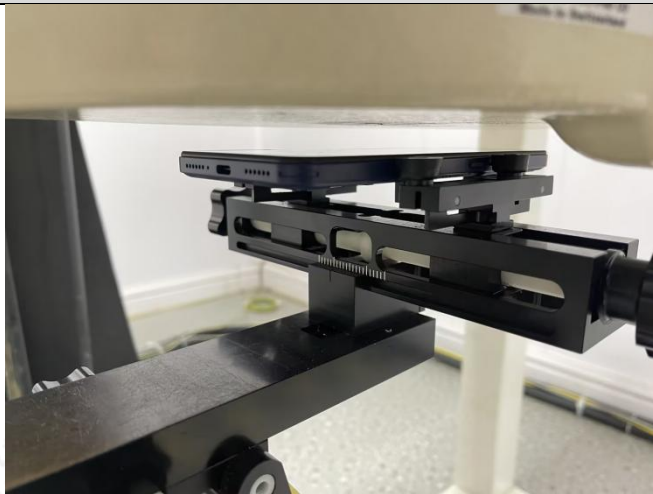


Photo 13: Back side 10mm



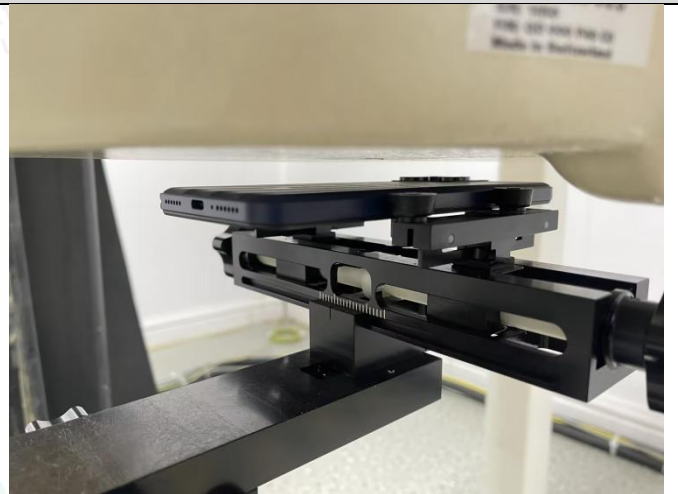

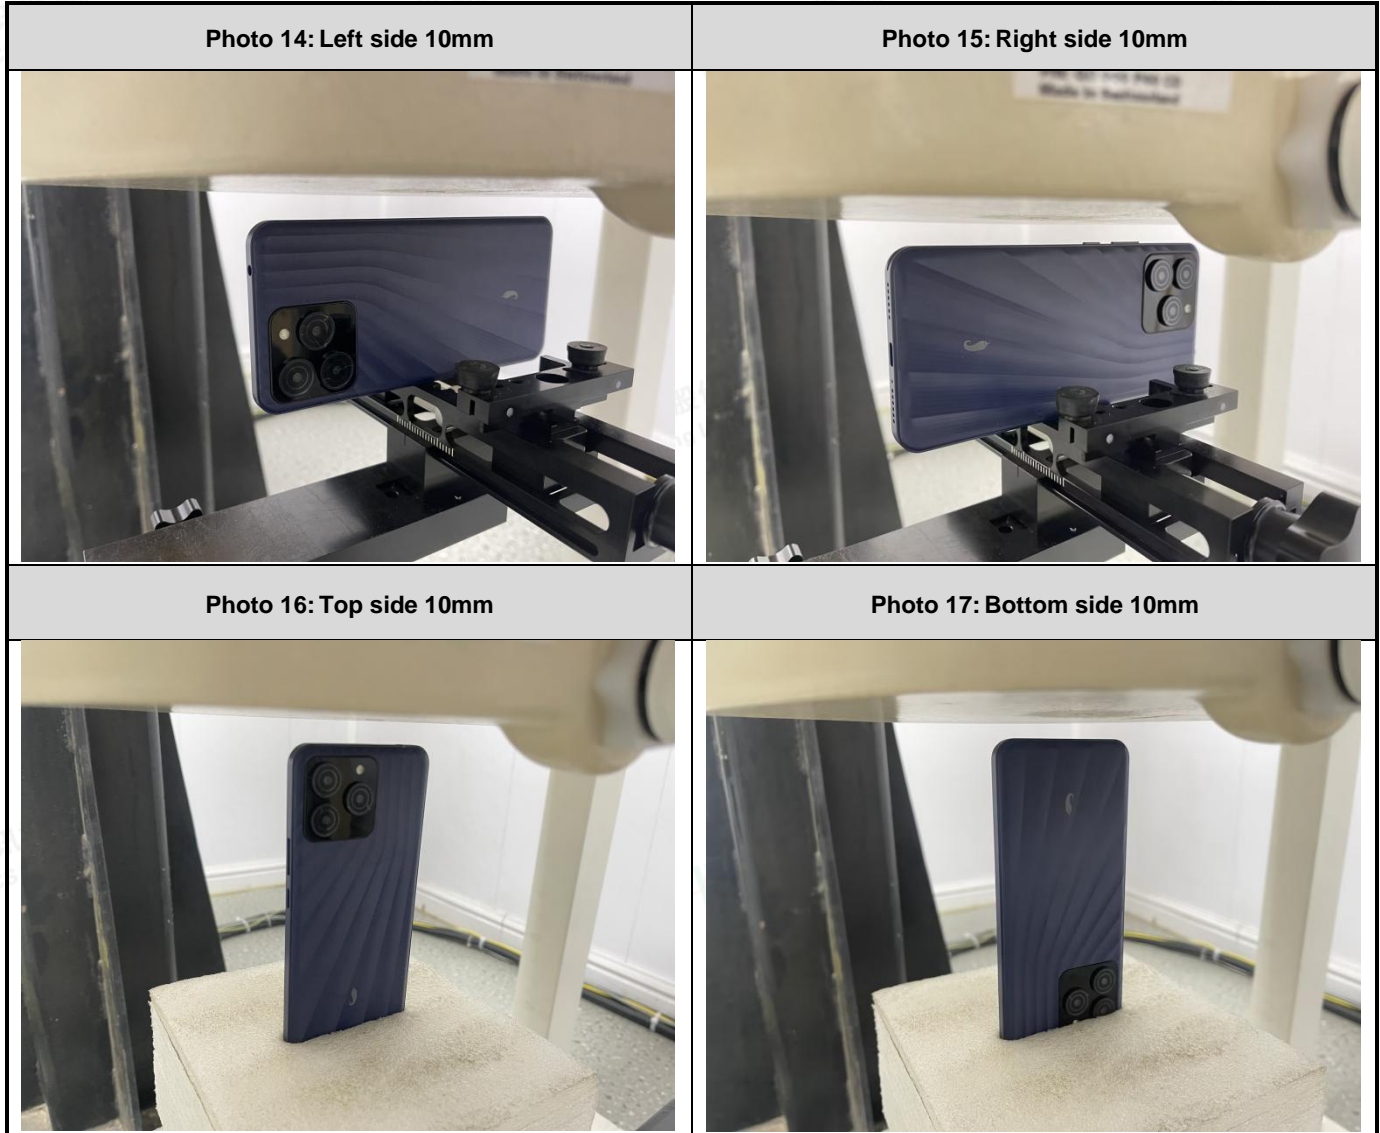

4. EUT Constructional Details

