尺寸:130*55mm

Visual WiFi Ear Endoscope


User Manual

FCC Statement This device complies with part 15 of the FCC rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation. Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment. NOTE: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures: Reorient or relocate the receiving antenna.

 Increase the separation between the equipment and Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.

The device has been evaluated to meet general RF exposure requirement. The device can be used in portable exposure condition without restriction.

Consult the dealer or an experienced radio/TV technician

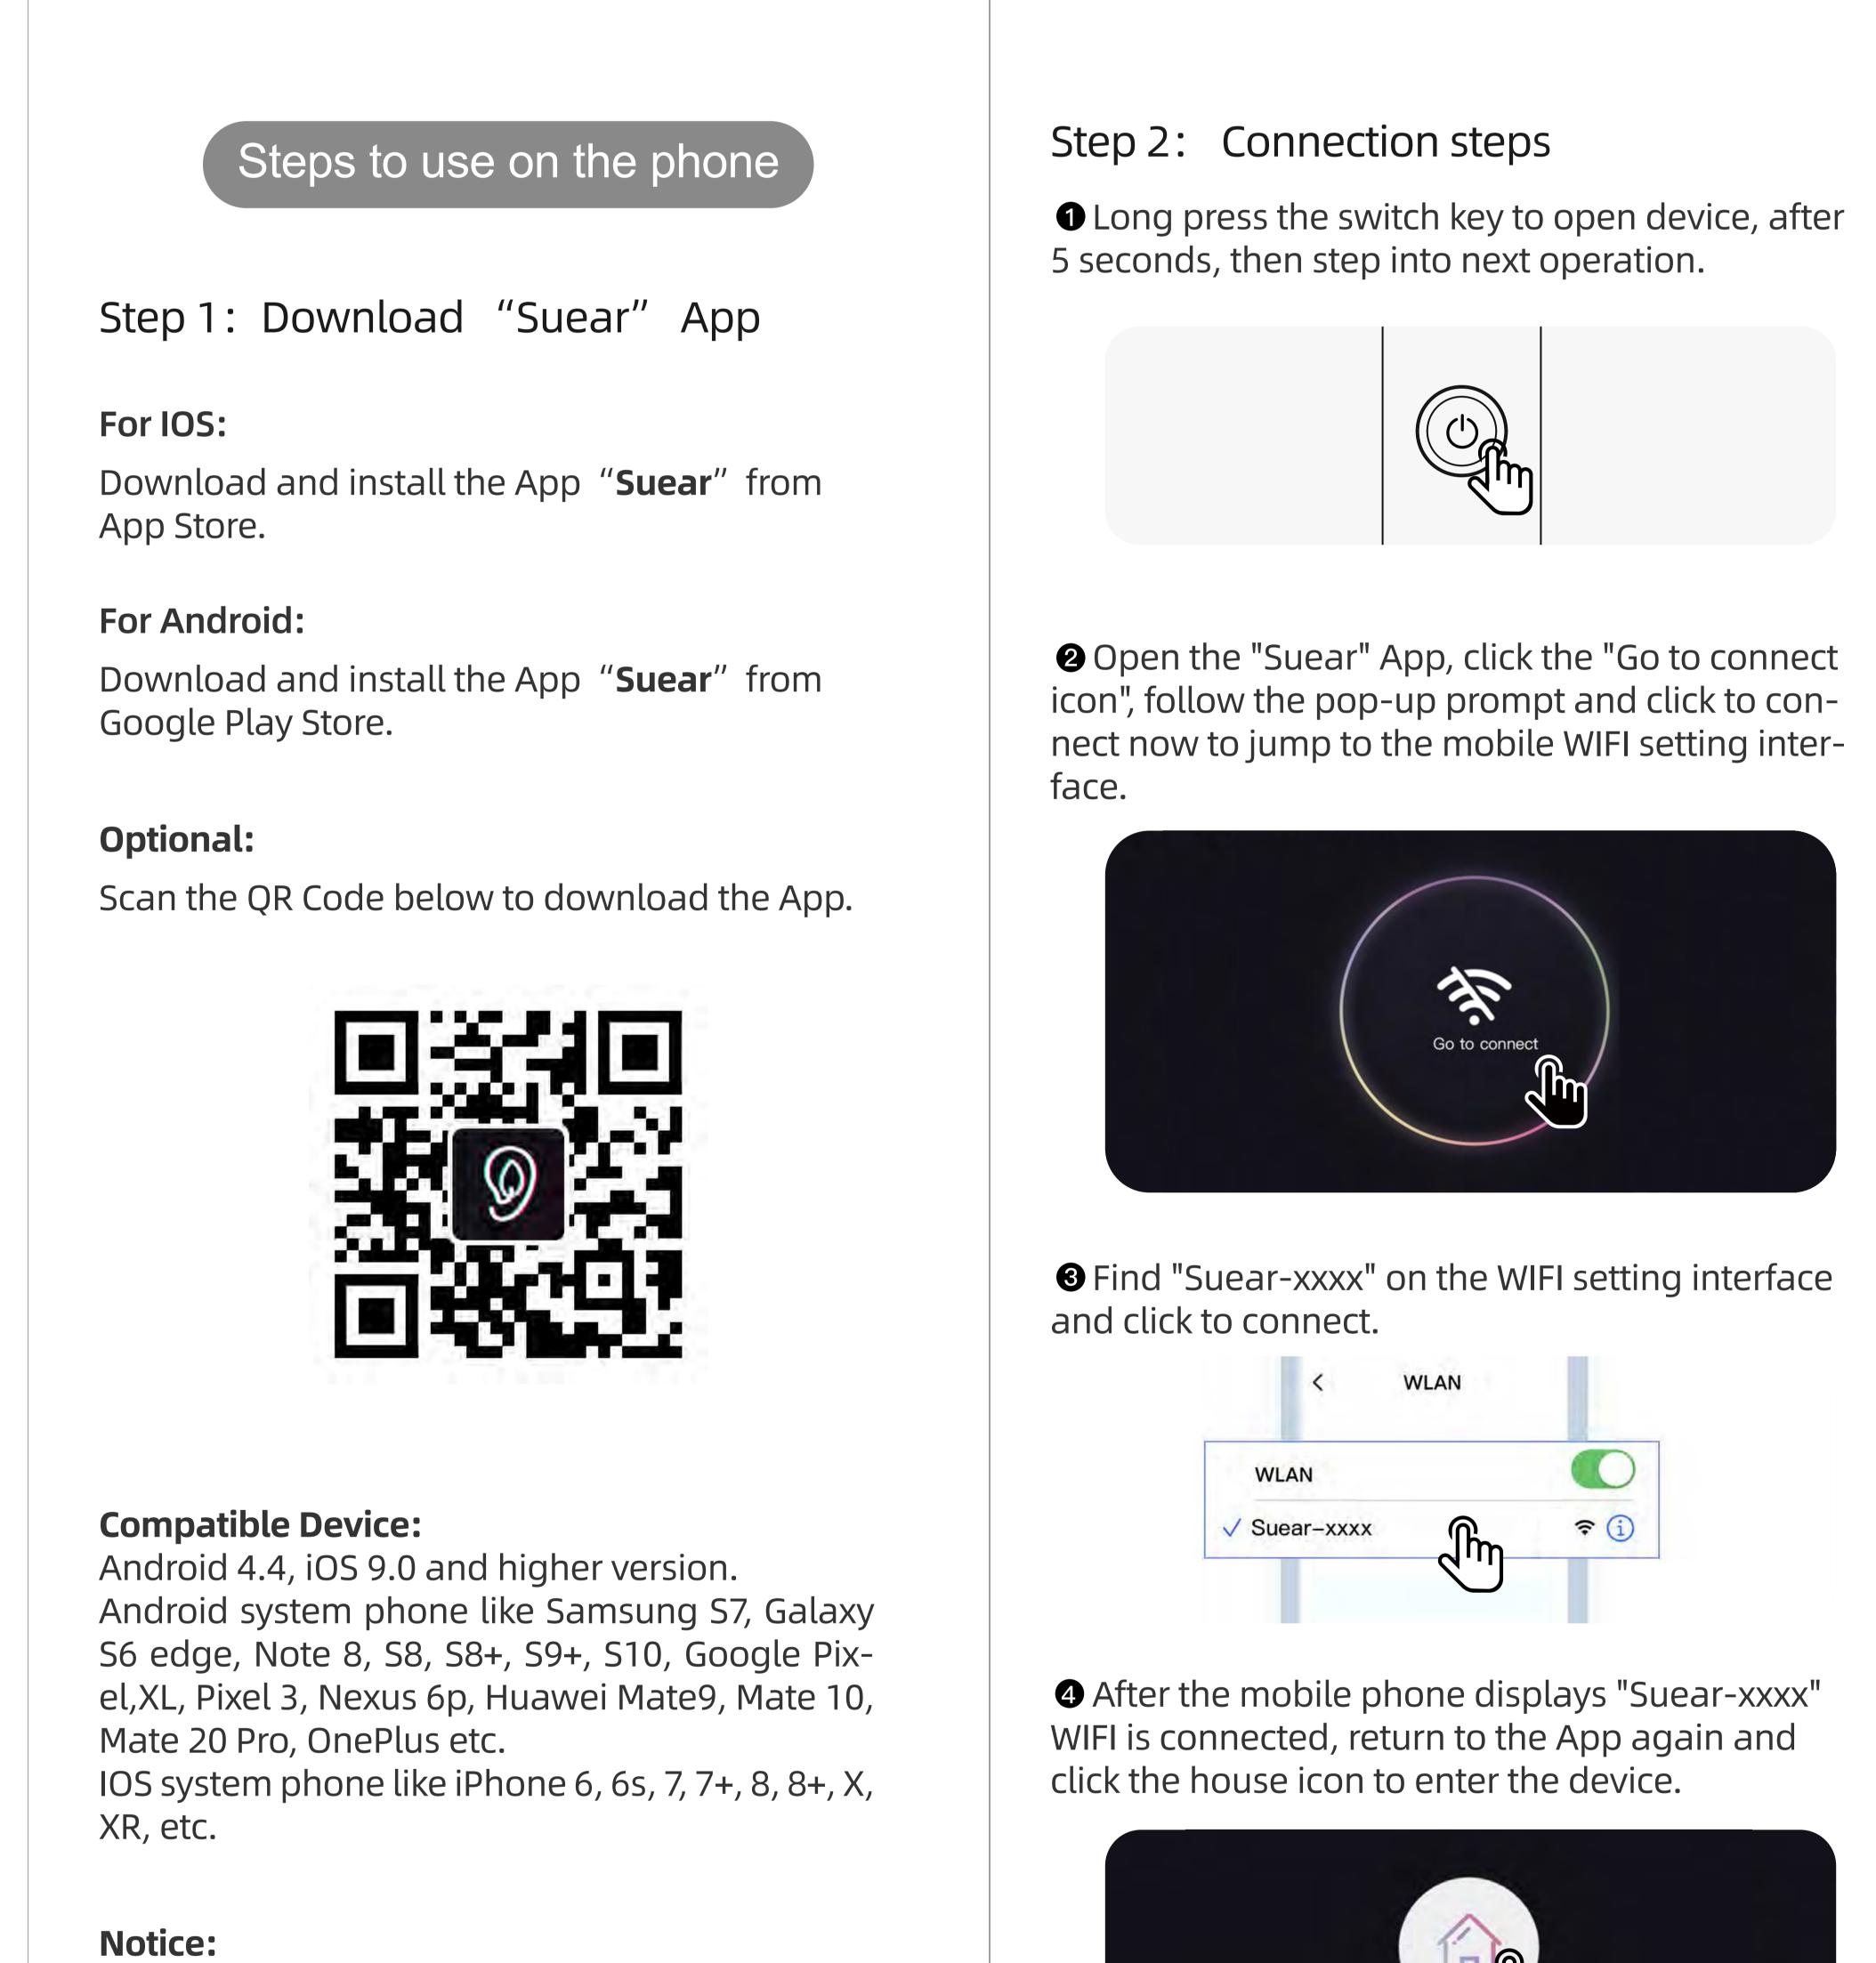



This model can't work for computer systems!

参

WLAN

√ Suear–xxxx

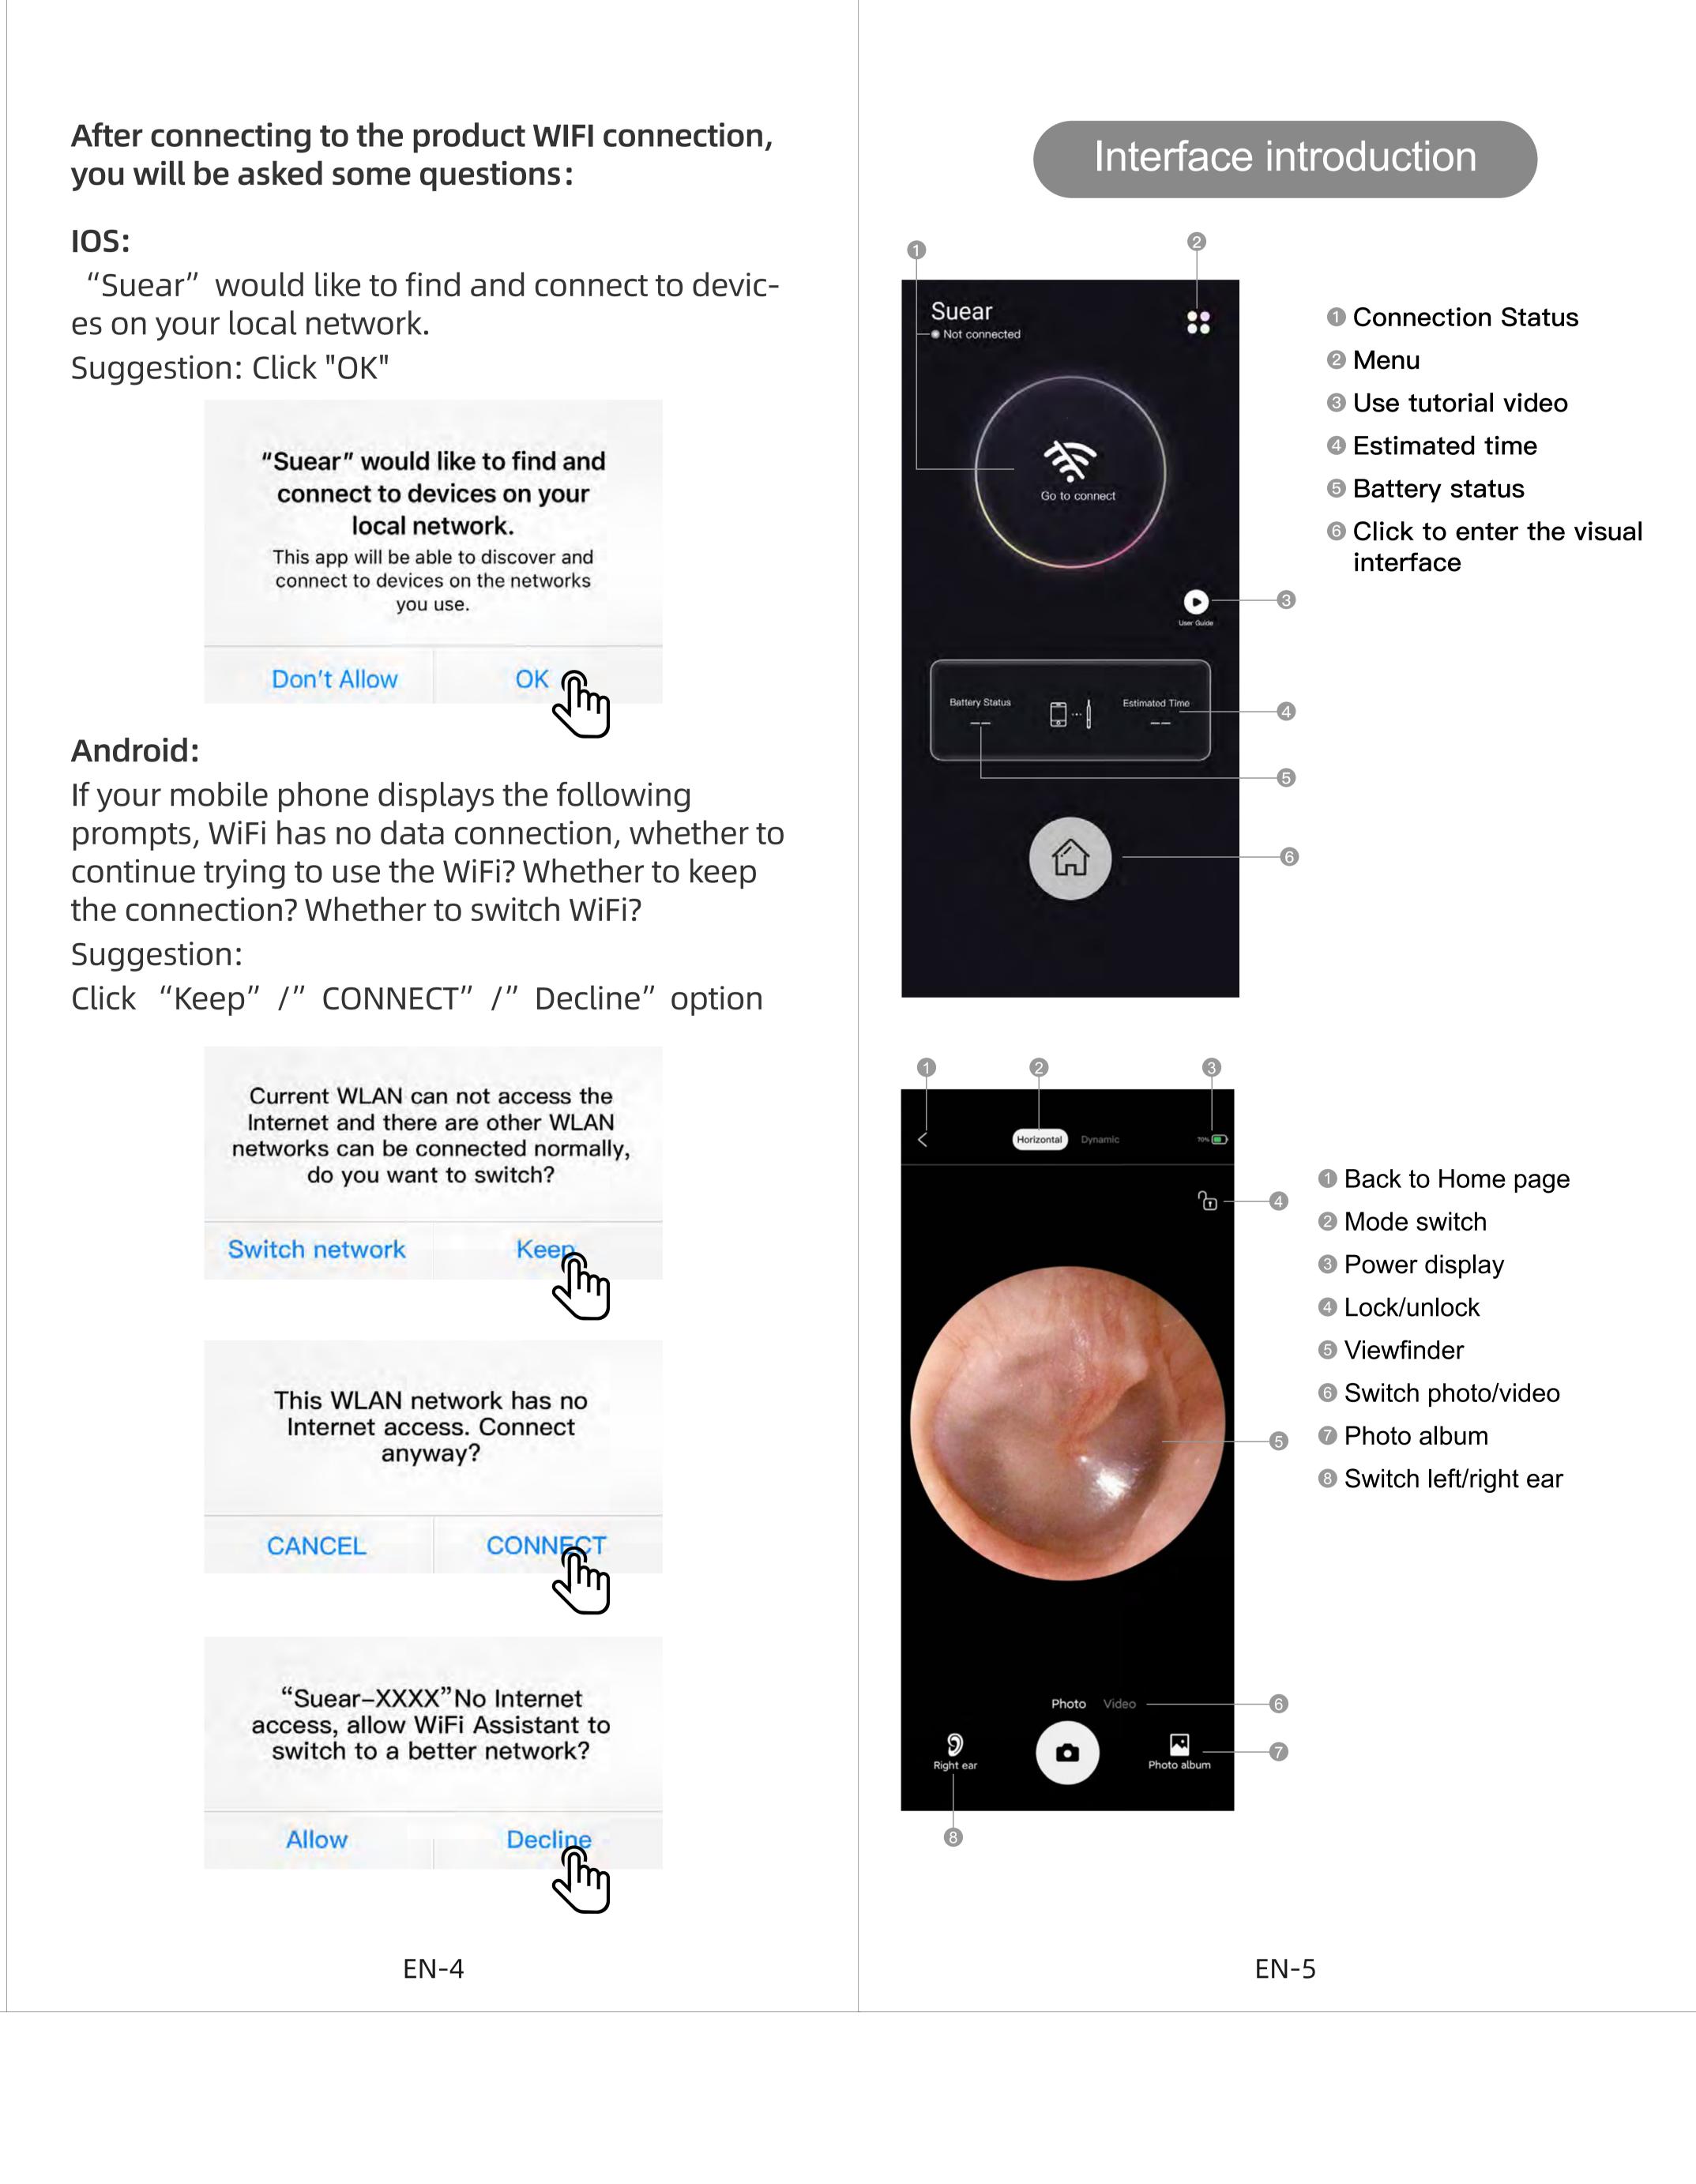

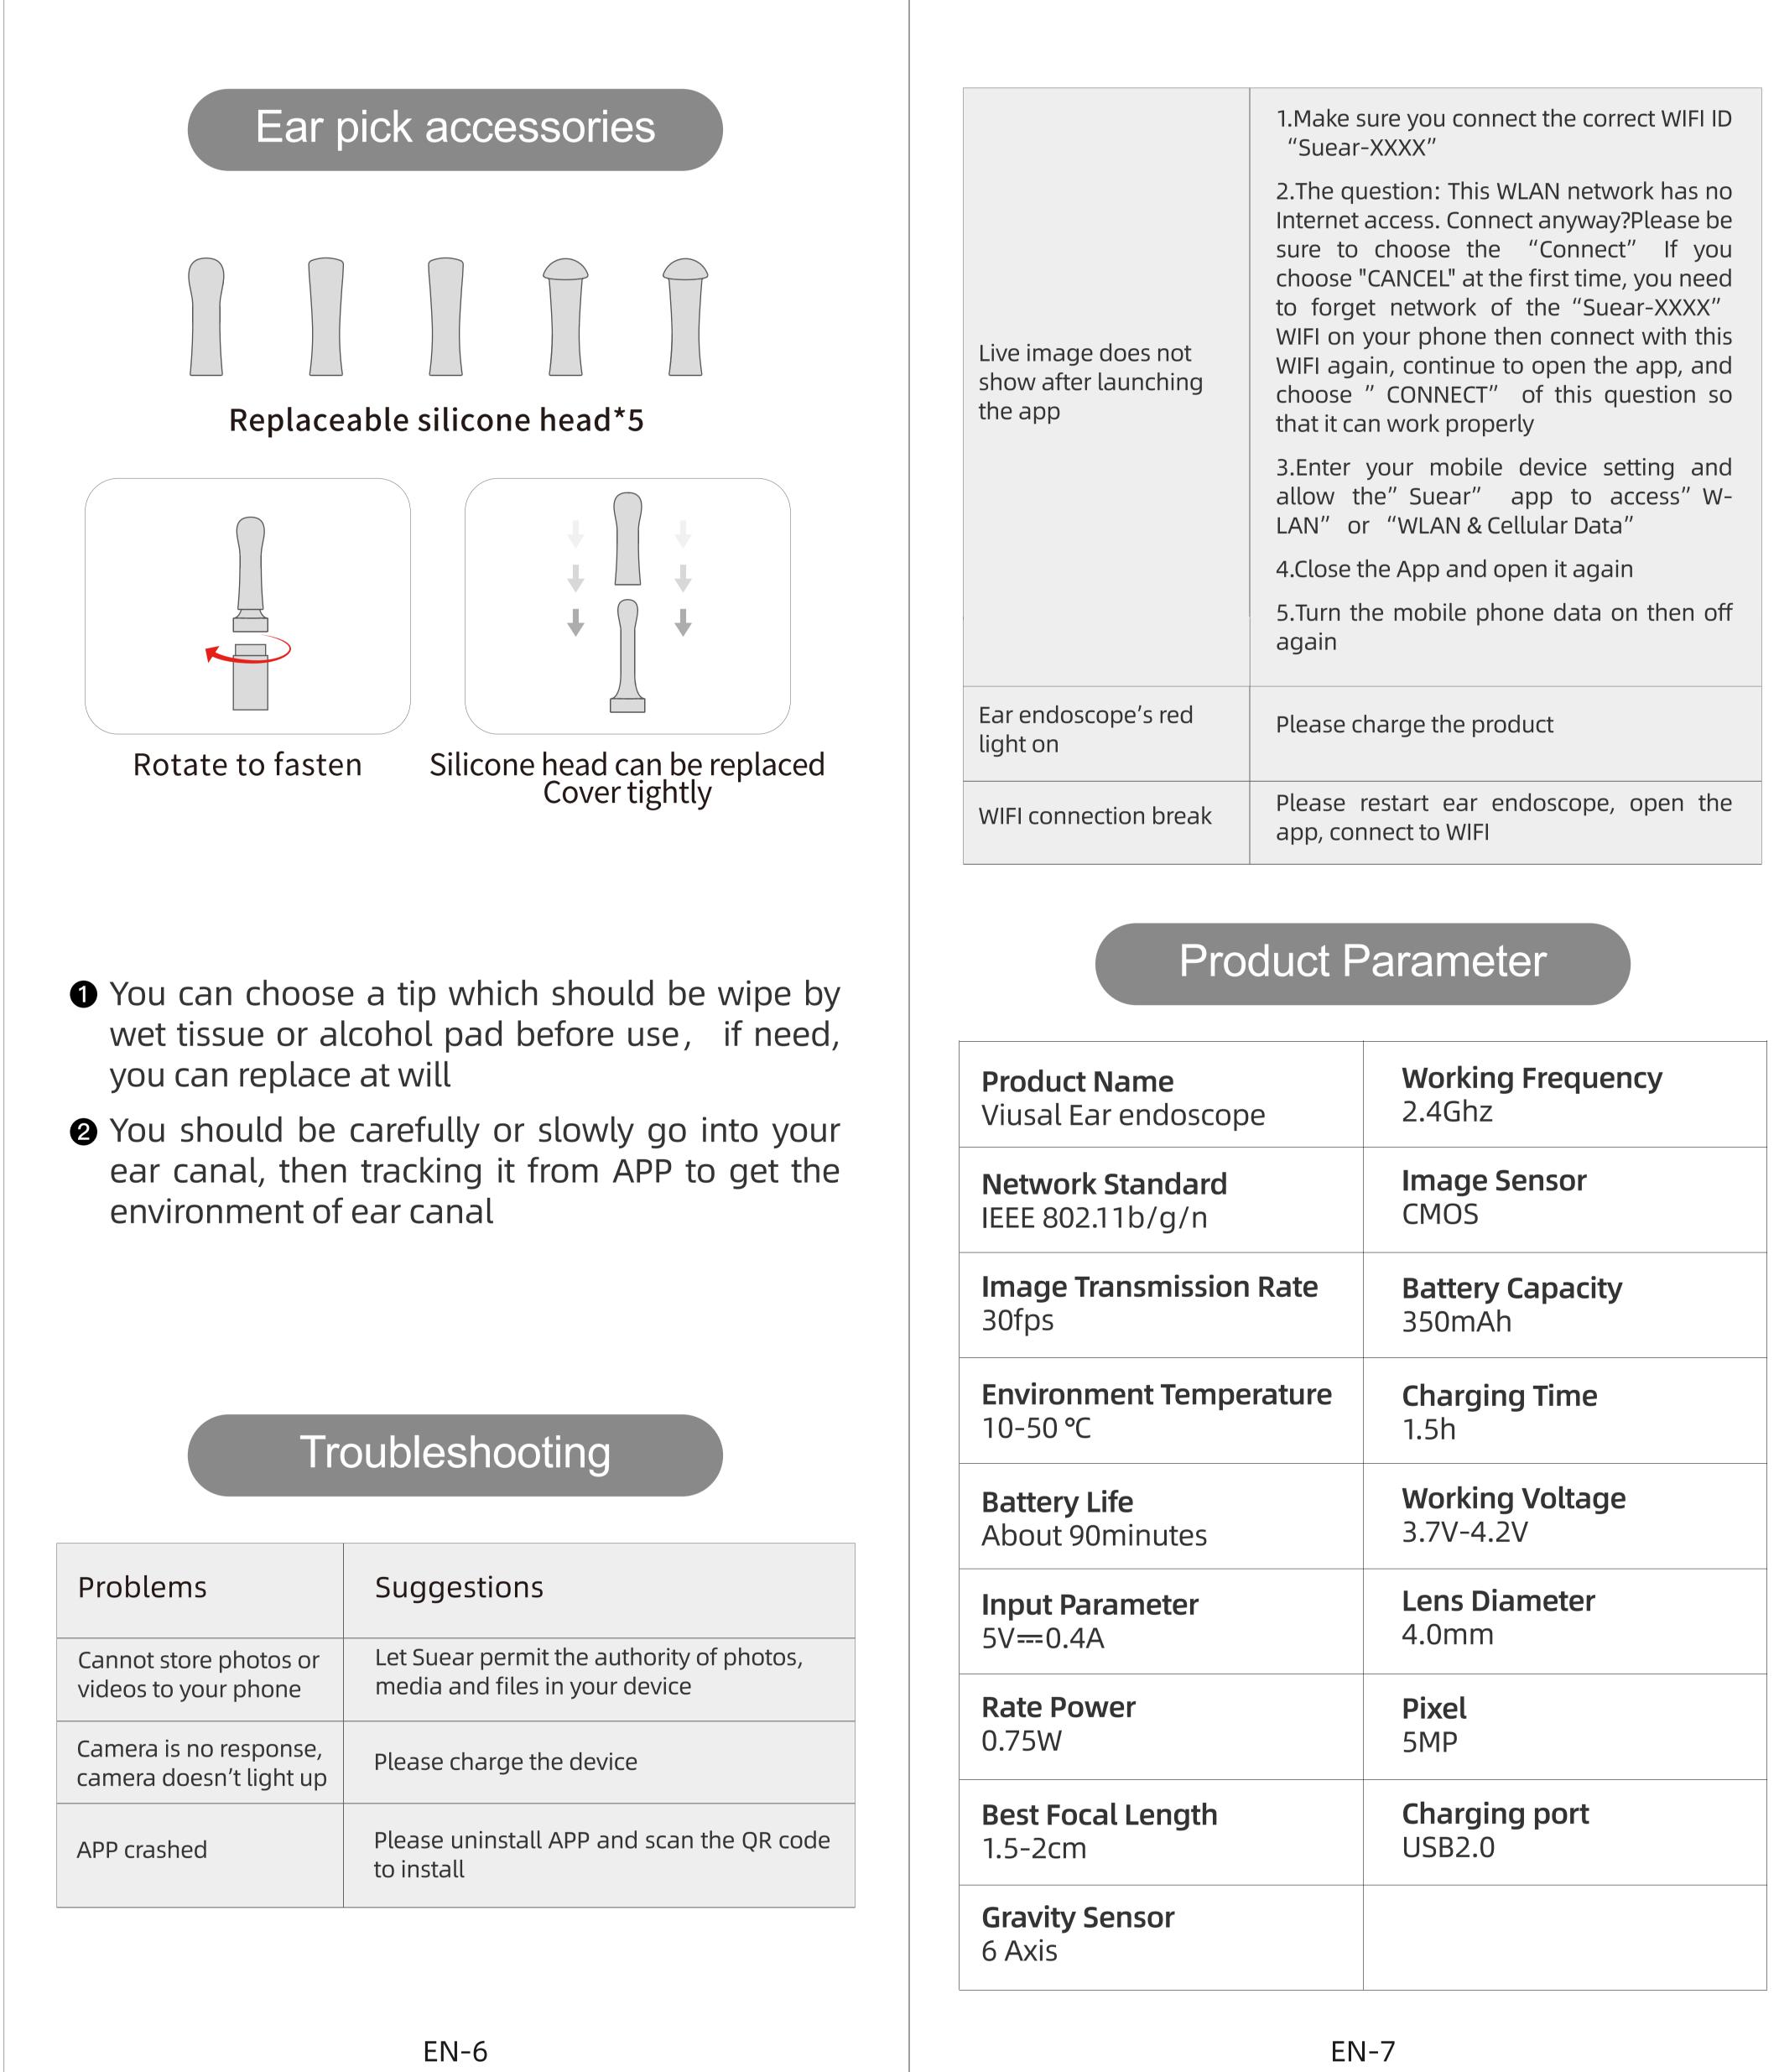

	4.Close the App and open it again 5.Turn the mobile phone data on then of again	
Ear endoscope's red light on	Please charge the product	
WIFI connection break	Please restart ear endoscope, open the app, connect to WIFI	
Pro	duct Para	meter
Product Name		orking Frequency
Viusal Ear endoscope		4Ghz
Network Standard		age Sensor
IEEE 802.11b/g/n		10S
Image Transmission Rate		attery Capacity
30fps		0mAh
Environment Temperature		narging Time
10-50 ℃		5h
Battery Life		orking Voltage
About 90minutes		7V-4.2V
Input Parameter		ns Diameter
5V==0.4A		Omm
Rate Power 0.75W	Pi : 5N	xel 1P
Best Focal Length		arging port
1.5-2cm		SB2.0
Gravity Sensor		