

# SAR TEST REPORT

For

**Magnetic Suspension Keyboard Case**

**Model Number: QM002**

**FCC ID:2A6TM-QM002**

**Report Number : WT228001223**

Test Laboratory : Shenzhen Academy of Metrology and Quality Inspection  
Site Location : NETC Building, No.4 Tongfa Road, Xili Town, Nanshan District, Shenzhen, Guangdong, China  
Tel : 0086-755-86928965  
Fax : 0086-755-86009898-31396  
Web : [www.smq.com.cn](http://www.smq.com.cn)  
Email : [emcrf@smq.com.cn](mailto:emcrf@smq.com.cn)

## Test report declaration

Applicant : SHENZHEN CITY KEXIN HUACHENG COMMUNICATION  
TECHNOLOGY CO.,LTD  
Plants 101 and 201 of Zhongkenuo Digital Technology Industrial Park,  
Address : No. 7 Road, East Of Guangming High Tech Park, Tianliao Community,  
Yutang Street, Guangming District, Shenzhen  
Manufacturer : SHENZHEN CITY KEXIN HUACHENG COMMUNICATION  
TECHNOLOGY CO.,LTD  
Plants 101 and 201 of Zhongkenuo Digital Technology Industrial Park,  
Address : No. 7 Road, East Of Guangming High Tech Park, Tianliao Community,  
Yutang Street, Guangming District, Shenzhen  
Model No. : QM002  
FCC ID : 2A6TM-QM002

### Test Standards:

FCC 47CFR Part 2(2.1093) IEEE Std 1528-2013 KDB 447498 D01v07 KDB 248227 D01v02r02 KDB  
865664 D01v01r04 KDB 865664 D02v01r02

The EUT described above is tested by Shenzhen Academy of Metrology and Quality Inspection EMC Laboratory to determine the compliance of the applicable standards stated above.

Shenzhen Academy of Metrology and Quality Inspection EMC Laboratory is assumed full responsibility for the accuracy of the test results.

The results documented in this report only apply to the tested sample, under the conditions and modes of operation as described herein.

The test report shall not be reproduced in part without written approval of the laboratory.

Project Engineer:




(Zhang Qiang)

Date:

May.24, 2022

Checked by:




(Shi Changda)

Date:

May.24, 2022

Approved by:



(Lin Yixiang)

Date:

May.24, 2022

## TABLE OF CONTENTS

<b>1. REPORTED SAR SUMMARY</b> .....	<b>5</b>
1.1. Statement of Compliance.....	5
1.2. RF exposure limits (ICNIRP Guidelines).....	6
1.3 Ratings and System Details.....	7
1.4 Product Function and Intended Use.....	7
1.5 Test specification(s).....	8
1.6 List of Test and Measurement Instruments.....	9
<b>2. GENERAL INFORMATION</b> .....	<b>10</b>
2.1. Report information.....	10
2.2. Laboratory Accreditation and Relationship to Customer.....	10
<b>3. SAR MEASUREMENT SYSTEM CONFIGURATION</b> .....	<b>11</b>
3.1. SAR Measurement Set-up.....	11
3.2. Probe description.....	12
3.3. Device holder description.....	14
<b>4. SAR MEASUREMENT PROCEDURE</b> .....	<b>14</b>
4.1. Scanning procedure.....	14
<b>7. SYSTEM VERIFICATION PROCEDURE</b> .....	<b>20</b>
7.1. Tissue Verification.....	20
<b>8. SAR MEASUREMENT VARIABILITY AND UNCERTAINTY</b> .....	<b>23</b>
8.1. SAR measurement variability.....	23
8.2. SAR measurement uncertainty.....	23
<b>9. Test Configuration</b> .....	<b>24</b>
<b>10. TUNE-UP LIMIT</b> .....	<b>25</b>
<b>11. MEASUREMENT RESULTS</b> .....	<b>26</b>
11.1. Conducted Power.....	26
11.2. BLE SAR results.....	27
11.3. Repeated SAR results.....	28
<b>12. EXPOSURE POSITIONS CONSIDERATION</b> .....	<b>29</b>
12.1. Multiple Transmitter Evaluation.....	29
<b>APPENDIX A: SYSTEM CHECKING SCANS</b> .....	<b>30</b>

**APPENDIX B.MEASUREMENT SCANS..... 32**  
**APPENDIX C: RELEVANT PAGES FROM PROBE CALIBRATION REPORT(S)..... 34**  
**APPENDIX D: RELEVANT PAGES FROM DAE& DIPOLE VALIDATION KIT REPORT(S)..... 47**  
    13. Photographs of the Test Set-Up..... 54

# 1. REPORTED SAR SUMMARY

## 1.1. Statement of Compliance

The maximum results of Specific Absorption Rate (SAR) found during testing are as follows.

Band	Max Reported SAR(W/kg)
	1-g Gap(0mm)
BLE	0.04

Table 1: Summary of test result

**Note:**

The SAR values listed on grants should be rounded to two decimal places. All SAR values less than 0.10 W/kg, after rounding, should be listed using the less-than symbol; for example, “The highest reported SAR value is < 0.10 W/kg.”

The device is in compliance with Specific Absorption Rate (SAR) for general population/ uncontrolled exposure limits according to the FCC rule 2.1093 , the ANSI/IEEE C95.1:1992, the NCRP Report Number 86 for uncontrolled environment, according to the Industry Canada Radio Standards Specification RSS-102 for General Population/ Uncontrolled exposure, and had been tested in accordance with the measurement methods and procedures specified in IEEE Std 1528-2013& IEEE Std 1528a-2005.

## 1.2. RF exposure limits (ICNIRP Guidelines)

Human Exposure	Uncontrolled Environment General Population	Controlled Environment Occupational
<b>Spatial Peak SAR*(Brain/Body)</b>	<b>1.60mW/g</b>	8.00mW/g
Spatial Average SAR** (Whole Body)	0.08mW/g	0.40mW/g
Spatial Peak SAR***(Limbs)	4.00mW/g	20.00mW/g

**Table 2: RF exposure limits**

The limit applied in this test report is shown in bold letters

Notes:

- \* The Spatial Peak value of the SAR averaged over any 1 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time
- \*\* The Spatial Average value of the SAR averaged over the whole body.
- \*\*\* The Spatial Peak value of the SAR averaged over any 1 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time. Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation.)

### 1.3 Ratings and System Details

Model No :	QM002	
IMEI No :	--	
Exposure category:	Uncontrolled environment / General population	
Test Device Production information	Production Unit	
Operating Mode(s)	BLE	
Test modulation	BLE(GFSK)	
Operating Frequency Range(s)	Transmitter Frequency Range	Receiver Frequency Range
Frequency:	Bluetooth Dual mode: 2402-2480MHz	
Power Class :	--	
Hardware version :	QM002-A	
Software version :	220522V1.0QM/BS	
Antenna type :	Internal antenna	
Battery information :	Dongguan Xinxin Electronic Technology Co., LTD	Battery model : 303450 Battery Specification:DC3.7V, 500mAh

### 1.4 Product Function and Intended Use

The Model No is an QM002, and it has BLE transmitter unit.

### 1.5 Test specification(s)

FCC 47CFR Part 2(2.1093)	Radiofrequency Radiation Exposure Evaluation: Portable Devices
IEEE Std 1528-2013	Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate(SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques
KDB 447498 D01v07	General RF Exposure Guidance No deviation
KDB 248227 D01v02r02	SAR Measurement Procedures for 802.11 Transmitters
KDB 865664 D01v01r04	SAR Measurement 100 MHz to 6 GHz
KDB 865664 D02v01r02	RF Exposure Reporting



## 1.6 List of Test and Measurement Instruments

	Equipment	Model No.	Serial No.	Manufacturer	Last Calibration Date	Period
☒	SAR test system	TX60L	F08/5AY8A1/A/01+F08/	SPEAG	NCR	NCR
☒	Electronic Data Transmitter	DAE4	1637	SPEAG	2021.11.05	1year
☒	SAR Probe	EX3DV4	3881	SPEAG	2021.07.23	1year
☒	Software	85070	--	Agilent	--	--
☒	Software	DASY5	--	SPEAG	--	--
☒	System Validation Dipole,2450MHz	D2450V2	818	SPEAG	2021.08.26	3year
☒	Dielectric Probe Kit	85070E	MY44300455	Agilent	NCR	NCR
☒	Dual-directional coupler,0.10-2.0GHz	778D	MY48220198	Agilent	NCR	NCR
☒	Dual-directional coupler,2.00-18GHz	772D	MY46151160	Agilent	NCR	NCR
☒	Power Amplifier	ZVE-8G	SC280800926	MINI-CIRCUITS	NCR	NCR
☒	Power Amplifier	ZHL42W	81709	MINI-CIRCUITS	NCR	NCR
☒	Signal Generator	SMR20	100047	R&S	2022.02.19	1year
☒	Power Sensor	NRP-Z21	102626	R&S	2021.06.04	1year
☒	Power Sensor	NRP-Z21	102627	R&S	2021.06.04	1year
☒	Call Tester	CMU 200	100110	R&S	2021.05.18	1year
☒	Network Analyzer	E5071C	MY46109550	Agilent	2022.02.19	1Year
☒	Flat Phantom	ELI4.0	TP-1904	SPEAG	NCR	NCR
☒	Twin Phantom	SAM	TP-1504	SPEAG	NCR	NCR
☒	Wideband Radio Communication Tester	CMW500	125469	R&S	2021.05.18	1Year
☒	Precision Thermometer	--	--	--	2021.08.07	1Year

**Table 3: List of Test and Measurement Equipment**

Note: All the test equipments are calibrated once a year, except the dipoles, which are calibrated every three years. Moreover, we have self-calibration every year to the dipoles.

## 2. GENERAL INFORMATION

### 2.1. Report information

This report is not a certificate of quality; it only applies to the sample of the specific product/equipment given at the time of its testing. The results are not used to indicate or imply that they are applicable to the similar items. In addition, such results must not be used to indicate or imply that SMQ approves, recommends or endorses the manufacture, supplier or use of such product/equipment, or that SMQ in any way guarantees the later performance of the product/equipment.

The sample/s mentioned in this report is/are supplied by Applicant, SMQ therefore assumes no responsibility for the accuracy of information on the brand name, model number, origin of manufacture or any information supplied.

Additional copies of the report are available to the Applicant at an additional fee. No third party can obtain a copy of this report through SMQ, unless the applicant has authorized SMQ in writing to do so.

The lab will not be liable for any loss or damage resulting from false, inaccurate, inappropriate or incomplete product information provided by the applicant/manufacture.

### 2.2. Laboratory Accreditation and Relationship to Customer

The testing reports were performed by the Shenzhen Academy of Metrology and Quality Inspection EMC Laboratory (Guangdong EMC compliance testing center), in their facilities located at NETC Building, No.4 Tongfa Rd., Xili, Nanshan, Shenzhen, China. At the time of testing, Laboratory is accredited by the following organizations:

China National Accreditation Service for Conformity Assessment (CNAS) accredits the Laboratory for conformance to FCC standards, EMC international standards and EN standards. The Registration Number is CNAS L0579.

The Laboratory is Accredited Testing Laboratory of FCC with Designation number CN1165 and Site registration number 582918.

The Laboratory is registered to perform emission tests with Innovation, Science and Economic Development (ISED), and the registration number is 11177A.

The Laboratory is registered to perform emission tests with VCCI, and the registration numbers are C-20048, G20076, R-20077, R-20078 and T-20047.

The Laboratory is Accredited Testing Laboratory of American Association for Laboratory Accreditation (A2LA) and certificate number is 3292.01.




- The generic twin phantom enabling the testing of left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- System checks dipoles allowing validating the proper functioning of the system.
- Test environment
- The DASY5 measurement system is placed at the head end of a room with dimensions: 4.5 x 4 x 3 m<sup>3</sup>, the SAM phantom is placed in a distance of 1.3 m from the side walls and 1.1m from the rear wall.

Picture 1 of the photo documentation shows a complete view of the test environment.

### 3.2. Probe description


Isotropic E-Field Probe EX3DV4 for Dosimetric Measurements

Construction	Symmetrical design with triangular core Interleaved sensors Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., DGBE)	
Calibration	ISO/IEC 17025 calibration service available.	
Frequency	10 MHz to >6 GHz (dosimetry); Linearity: ± 0.2 dB (30 MHz to 6 GHz)	
Directivity	± 0.3 dB in HSL (rotation around probe axis) ± 0.5 dB in tissue material (rotation normal to probe axis)	
Dynamic range	10 µW/g to > 100 mW/g; Linearity: ± 0.2 dB (noise: typically < 1 µW/g)	
Dimensions	Overall length: 337 mm (Tip: 20mm) Tip length: 2.5 mm (Body: 12mm) Typical distance from probe tip to dipole centers: 1mm	
Application	High precision dosimetric measurements in any exposure scenario (e.g., very strong gradient fields). Only probe which enables compliance testing for frequencies up to 6 GHz with precision of better 30%.	

### Phantom description

The used SAM Phantom meets the requirements specified in Edition 01-01 of Supplement C to OET Bulletin 65 for Specific Absorption Rate (SAR) measurements.

The phantom consists of a fibreglass shell integrated in a wooden table. It allows left-hand and right-hand head as well as body-worn measurements with a maximum liquid depth of 18 cm in head position and 22 cm in planar position (body measurements). The thickness of the Phantom shell is 2 mm +/- 0.1 mm.

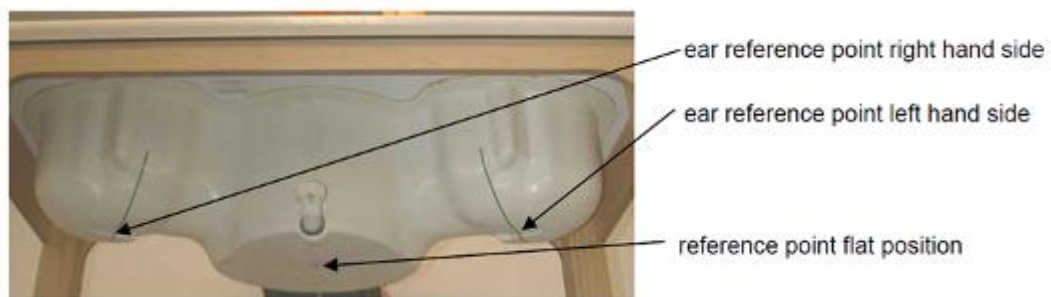

ELI4 Phantom

Shell Thickness	2mm+/- 0.2mm
Filling Volume	Approximately 30 liters
Measurement Areas	Flat phantom

The ELI4 phantom is intended for compliance testing of handheld and body-mounted wireless devices in the frequency range of 30MHz to 6GHz. ELI4 is fully compatible with the latest draft of the standard IEC 62209-2 and all known tissue simulating liquids.

The phantom shell material is resistant to all ingredients used in the tissue-equivalent liquid recipes. The shell of the phantom including ear spacers is constructed from low permittivity and low loss material, with a relative permittivity  $\leq 5$  and a loss tangent  $\leq 0.05$ .

### 3.3. Device holder description

The DASY5 device holder has two scales for device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear openings). The plane between



the ear openings and the mouth tip has a rotation angle of  $65^\circ$ . The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. This device holder is used for standard mobile phones or PDA's only. If necessary an additional support of polystyrene material is used.

Larger DUT's (e.g. notebooks) cannot be tested using this device holder. Instead a support of bigger polystyrene cubes and thin polystyrene plates is used to position the DUT in all relevant positions to find and measure spots with maximum SAR

values.

Therefore those devices are normally only tested at the flat part of the SAM.

## 4. SAR MEASUREMENT PROCEDURE

### 4.1. Scanning procedure

- The DASY5 installation includes predefined files with recommended procedures for measurements and system check. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.
- The reference and drift measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max.  $\pm 5\%$ .
- The surface check measurement tests the optical surface detection system of the DASY5 system by repeatedly detecting the surface with the optical and mechanical surface detector and comparing the results. The output gives the detecting heights of both systems, the difference between the two systems and the standard deviation of the detection repeatability. Air bubbles or refraction in the liquid due to separation of the sugar-water mixture gives poor repeatability (above  $\pm 0.1\text{mm}$ ). To prevent wrong results tests are only executed when the liquid is free of air bubbles. The difference between the optical surface detection and the actual surface depends on

the probe and is specified with each probe. (It does not depend on the surface reflectivity or the probe angle to the surface within  $\pm 30^\circ$ .)

- The area scan measures the SAR above the DUT or verification dipole on a parallel plane to the surface. It is used to locate the approximate location of the peak SAR with 2D spline interpolation. The robot performs a stepped movement along one grid axis while the local electrical field strength is measured by the probe. The probe is touching the surface of the SAM during acquisition of measurement values. The standard scan uses large grid spacing for faster measurement. Standard grid spacing for head measurements is 15 mm in x- and y- dimension ( $\leq 2\text{GHz}$ ), 12 mm in x- and y- dimension (2-4 GHz) and 10mm in x- and y- dimension (4-6GHz). If a finer resolution is needed, the grid spacing can be reduced. Grid spacing and orientation have no influence on the SAR result. For special applications where the standard scan method does not find the peak SAR within the grid, e.g. mobile phones with flip cover, the grid can be adapted in orientation.

Results of this coarse scan are shown in Appendix B.

- A “zoom scan” measures the field in a volume around the 2D peak SAR value acquired in the previous “coarse” scan. This is a fine grid with maximum scan spatial resolution:  $\Delta x_{\text{zoom}}$ ,  $\Delta y_{\text{zoom}} \leq 2\text{GHz} \leq 8\text{ mm}$ , 2-4GHz -  $\leq 5\text{ mm}$  and 4-6 GHz- $\leq 4\text{ mm}$ ;  $\Delta z_{\text{zoom}} \leq 3\text{GHz} - \leq 5\text{ mm}$ , 3-4 GHz-  $\leq 4\text{ mm}$  and 4-6GHz- $\leq 2\text{mm}$  where the robot additionally moves the probe along the z-axis away from the bottom of the Phantom. DASY5 is also able to perform repeated zoom scans if more than 1 peak is found during area scan. Test results relevant for the specified standard (see chapter 1.5.) are shown in table form in chapter 3.2.

- A Z-axis scan measures the total SAR value at the x-and y-position of the maximum SAR value found during the cube scan. The probe is moved away in z-direction from the bottom of the SAM phantom in 2mm steps. This measurement shows the continuity of the liquid and can – depending in the field strength- also show the liquid depth. A z-axis scan of the measurement with maximum SAR value is shown in Appendix B.

The following table summarizes the area scan and zoom scan resolutions per FCC KDB 865664D01:

Frequency	Maximum Area Scan resolution ( $\Delta x$ area, $\Delta y$ area)	Maximum Zoom Scan spatial resolution ( $\Delta x$ zoom, $\Delta y$ zoom)	Maximum Zoom Scan spatial resolution			Minimum zoom scan volume (x,y,z)
			Uniform Grid	Graded Grad		
			$\Delta$	$\Delta$	$\Delta z$ zoom (n>1)	

		zoom)	zzoom(n)	zzoom(1)		
≤2GHz	≤15mm	≤8mm	≤5mm	≤4mm	≤1.5*Δz zoom(n-1)	≥30mm
2-3GHz	≤12mm	≤5mm	≤5mm	≤4mm	≤ 1.5* Δ z zoom(n-1)	≥30mm
3-4GHz	≤10mm	≤5mm	≤4mm	≤3mm	≤ 1.5* Δ z zoom(n-1)	≥28mm
4-5GHz	≤10mm	≤4mm	≤3mm	≤2.5mm	≤ 1.5* Δ z zoom(n-1)	≥25mm
5-6GHz	≤10mm	≤4mm	≤2mm	≤2mm	≤ 1.5* Δ z zoom(n-1)	≥22mm

#### Spatial Peak SAR Evaluation

- The spatial peak SAR - value for 1 and 10 g is evaluated after the Cube measurements have been done. The bases of the evaluation are the SAR values measured at the points of the fine cube grid consisting of 5 x 5 x 7 points (with 8mm horizontal resolution) or 7 x 7 x 7 points (with 5mm horizontal resolution).
- The algorithm that finds the maximal averaged volume is separated into three different stages.
- The data between the dipole center of the probe and the surface of the phantom are extrapolated. This data cannot be measured since the center of the dipole is 2.7 mm away from the tip of the probe and the distance between the surface and the lowest measuring point is about 1 mm (see probe calibration sheet). The extrapolated data from a cube measurement can be visualized by selecting 'Graph Evaluated'.
- The maximum interpolated value is searched with a straight-forward algorithm. Around this maximum the SAR - values averaged over the spatial volumes (1g or 10 g) are computed using the 3d-spline interpolation algorithm. If the volume cannot be evaluated (i.e., if a part of the grid was cut off by the boundary of the measurement area) the evaluation will be started on the corners of the bottom plane of the cube.
- All neighboring volumes are evaluated until no neighboring volume with a higher average value is found.
- Extrapolation
- The extrapolation is based on a least square algorithm [W. Gander, Computermathematik, p.168-180]. Through the points in the first 3 cm along the z-axis, polynomials of order four are calculated. These polynomials are then used to evaluate the points between the surface and the





- Conversion factor                      ConvFi
- Diode compression point              Dcpi
- Device parameters:    - Frequency                      f
- Crest factor                              cf
- Media parameters:    - Conductivity                       $\sigma$
- Density                                       $\rho$

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY5 components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics.

If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot cf/dcpi$$

with  $V_i$  = compensated signal of channel  $i$  ( $i = x, y, z$ )

$U_i$  = input signal of channel  $i$  ( $i = x, y, z$ )

cf = crest factor of exciting field (DASY parameter)

dcpi = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes:                       $E_i = (V_i / Norm_i \cdot ConvF)^{1/2}$

H-field probes:                       $H_i = (V_i)^{1/2} \cdot (a_{i0} + a_{i1}f + a_{i2}f^2)/f$

with  $V_i$  = compensated signal of channel  $i$  ( $i = x, y, z$ )

Normi = sensor sensitivity of channel i (i = x, y, z)

[mV/(V/m)<sup>2</sup>] for E-field Probes

ConvF = sensitivity enhancement in solution

aij = sensor sensitivity factors for H-field probes

f = carrier frequency [GHz]

Ei = electric field strength of channel i in V/m

Hi = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = (E_x^2 + E_y^2 + E_z^2)^{1/2}$$

The primary field data are used to calculate the derived field units.

$$SAR = (E_{tot}^2 \cdot \sigma) / (\rho \cdot 1000)$$

with SAR = local specific absorption rate in mW/g

E<sub>tot</sub> = total field strength in V/m

σ = conductivity in [mho/m] or [Siemens/m]

ρ = equivalent tissue density in g/cm<sup>3</sup>

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid. The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = E_{tot}^2 / 3770 \quad \text{or} \quad P_{pwe} = H_{tot}^2 \cdot 37.7$$

with P<sub>pwe</sub> = equivalent power density of a plane wave in mW/cm<sup>2</sup>

E<sub>tot</sub> = total electric field strength in V/m

H<sub>tot</sub> = total magnetic field strength in A/m

## 7. SYSTEM VERIFICATION PROCEDURE

### 7.1. Tissue Verification

The simulating liquids should be checked at the beginning of a series of SAR measurements to determine if the dielectric parameters are within the tolerances of the specified target values. The measured conductivity and relative permittivity should be within  $\pm 5\%$  of the target values.

The following materials are used for producing the tissue-equivalent materials

Ingredient (% by weight )	Frequency Band
	2450
Tissue Type	Head
Water	62.7
Salt(NaCl)	0.5
Sugar	0.0
HEC	0.0
Bactericide	0.0
Triton X-100	0.0
DGBE	36.8

**Table 4 : Tissue Dielectric Properties**

Salt: 99+% Pure Sodium Chloride; Sugar: 98+% Pure Sucrose; Water: De-ionized, 16M $\Omega$ + resistivity

HEC: Hydroxyethyl Cellulose; DGBE: 99+% Di(ethylene glycol) butyl ether, [2-(2-butoxyethoxy)ethanol]

Triton X-100(ultra pure): Polyethylene glycol mono[4-(1,1,3,3-tetramethylbutyl)phenyl]ether

Head Tissue-equivalent liquid measurements:


Used Target Frequency	Target Tissue		Measured Tissue		Liquid Temp	Test Date
	$\epsilon_r$ (+/-5%)	$\sigma$ (S/m) (+/-5%)	$\epsilon_r$	$\sigma$ (S/m)		
2450MHz Head	39.2 (37.24~41.16)	1.80 (1.71~1.89)	39.01	1.73	22°C	2022.05.16
$\epsilon_r$ = Relative permittivity, $\sigma$ = Conductivity						

System checking, Head Tissue-equivalent liquid:

System Check	Target SAR (1W) (+/-10%)		Measured SAR (Normalized to 1W)		Liquid Temp.	Test Date
	1-g (W/kg)	10-g (W/kg)	1-g (W/kg)	10-g (W/kg)		
D2450V2 Head	51.6 (46.44~56.76)	23.64 (21.28~26.00)	52.16	23.80	22°C	2022.05.16

System Checking

The manufacturer calibrates the probes annually. A system check measurement was made following the determination of the dielectric parameters of the tissue-equivalent liquid, using the dipole validation kit. A power level of 250mW was supplied to the dipole antenna, which was placed under the flat section of the twin SAM phantom.

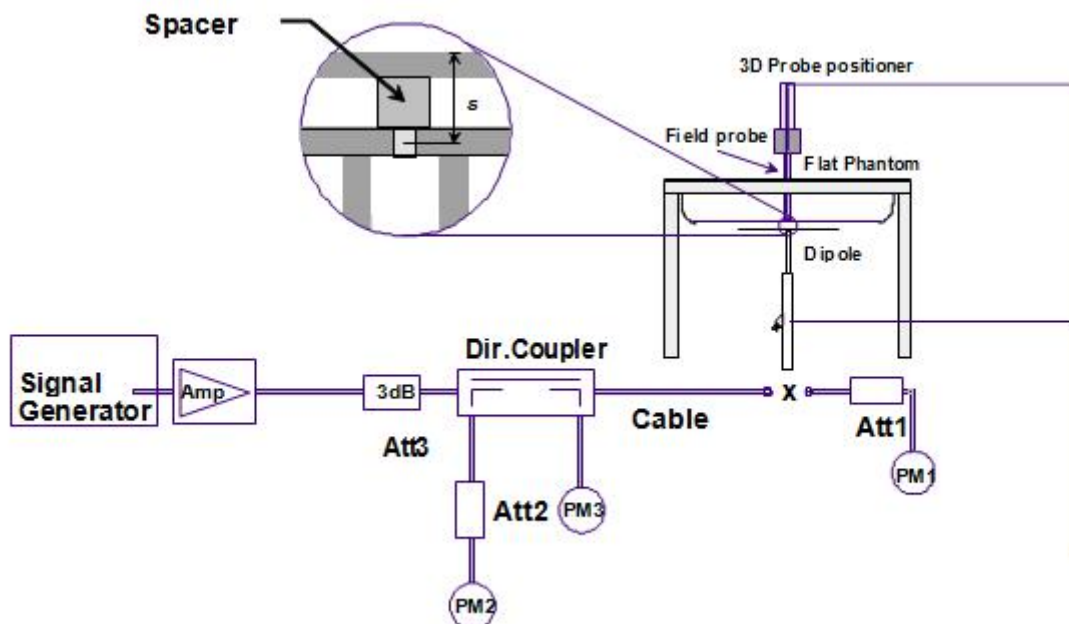

The system checking results (dielectric parameters and SAR values) are given in the table below.

The system check is performed for verifying the accuracy of the complete measurement system and performance of the software. The system check is performed with tissue equivalent material according to IEEE P1528 (described above). The following table shows system check results for all frequency bands and tissue liquids used during the tests (Graphic Plot(s) see Appendix A).

## 8. SAR MEASUREMENT VARIABILITY AND UNCERTAINTY

### 8.1. SAR measurement variability

Per KDB865664 D01 SAR measurement 100MHz to 6GHz v01r04, SAR measurement variability must be assessed for each frequency band, which is determined by the SAR probe calibration point and tissue-equivalent medium used for the device measurements. The additional measurements are repeated after the completion of all measurement requiring the same head or body tissue-equivalent medium in a frequency band. The test device should be returned to ambient conditions (normal room temperature) with the battery fully charged before it is re-mounted on the device holder for the repeated measurement(s) to minimize any unexpected variations in the repeated results.

- 1) Repeated measurement is not required when the original highest measured SAR is  $<0.80$  W/kg; step2) through 4) do not apply.
- 2) When the original highest measured SAR is  $\geq 0.8$  W/kg , repeat that measurement once.
- 3) Perform a second repeated measurement only if the ratio of largest to smallest SAR for the original and first repeated measurements is  $>1.20$  or when the original or repeated measurement is  $\geq 1.45$  W/kg (~10% from the 1-g SAR limit).
- 4) Perform a third repeated measurement only if the original, first or second repeated measurement is  $\geq 1.5$ W/kg and the ratio of largest to smallest SAR for the original, first and second repeated measurements is  $>1.20$ .

The same procedures should be adapted for measurements according to extremity and occupational exposure limits by applying a factor of 2.5 for extremity exposure and a factor of 5 for occupational exposure to the corresponding SAR thresholds.

### 8.2. SAR measurement uncertainty

Per KDB865664 D01 SAR Measurement 100MHz to 6GHz v01r03, when the highest measured 1-g SAR within a frequency band is  $<1.5$ W/kg, the extensive SAR measurement uncertainty analysis described in IEEE Std 1528-2003 is not required in SAR reports submitted for equipment approval. The equivalent ratio(1.5/1.6) is applied to extremity and occupational exposure conditions.

## 9. Test Configuration

Test positions as described in the tables above are in accordance with the specified test standard.

### **KDB 447498 D01 General RF Exposure Guidance:**

Testing of the required channels within the operating mode of a frequency band is not required when the reported 1-g or 10-g SAR for the mid band or highest output power channel is:

- $\leq 0.8\text{W/kg}$  or  $2.0\text{ W/kg}$  , for 1-g or 10-g respectively, when the transmission band is  $\leq 100\text{MHz}$
- $\leq 0.6\text{W/kg}$  or  $1.5\text{ W/kg}$  , for 1-g or 10-g respectively, when the transmission band is between  $100\text{MHz}$  and  $200\text{MHz}$
- $\leq 0.4\text{W/kg}$  or  $1.0\text{ W/kg}$  , for 1-g or 10-g respectively, when the transmission band is  $\geq 200\text{MHz}$



## 10. TUNE-UP LIMIT

Average Power	1M	2M
BLE	-0.5 [-1.0dB~~+1.0dB]	-0.5 [-1.0dB~~+1.0dB]

## 11. MEASUREMENT RESULTS

Date of testing : 2022.5.15-2022.5.17  
Ambient temperature : 20°C~22°C  
Relative humidity : 50~68%

### 11.1. Conducted Power

BLE2.4GHz(1M) Band Conducted Power		
Channel	Frequency(MHz)	Average Power (dBm)
CH 0	2,402	-0.17
CH 19	2,440	-0.35
CH 39	2,480	-0.59

BLE2.4GHz(2M) Band Conducted Power		
Channel	Frequency(MHz)	Average Power (dBm)
CH 0	2,402	-0.44
CH 19	2,440	-0.37
CH 39	2,480	-0.73

## 11.2.BLE SAR results

Body Exposure Condition (Separation Distance is 0 mm)

Mode	Test Position	Ch.	Freq. (MHz)	Burst Average Power (dBm)	Tune-Up Limit (dBm)	Scaling Factor	1g Measured SAR (W/kg)	1g Reported SAR (W/kg)
1M	Front Side	0	2402	-0.17	0.5	1.167	0.02	0.02
<b>1M</b>	<b>Back Side</b>	<b>0</b>	<b>2402</b>	<b>-0.17</b>	<b>0.5</b>	<b>1.167</b>	<b>0.03</b>	<b>0.04</b>
1M	Left Side	0	2402	-0.17	0.5	1.167	0.01	0.01
1M	Right Side	0	2402	-0.17	0.5	1.167	0.01	0.01
1M	Top Side	0	2402	-0.17	0.5	1.167	0.01	0.02
1M	Bottom Side	0	2402	-0.17	0.5	1.167	0.01	0.01

### 11.3.Repeated SAR results


Remark:

1. Per KDB 865664 D01v01r04, for each frequency band, repeated SAR measurement is required only when the measured SAR is  $\geq 0.8\text{W/kg}$ .
2. Per KDB 865664 D01v01r04, if the ratio among the repeated measurement is  $\leq 1.2$  and the measured SAR  $< 1.45\text{W/kg}$ , only one repeated measurement is required.
3. The ratio is the difference in percentage between original and repeated measured SAR.
4. All measurement SAR result is scaled-up to account for tune-up tolerance and is compliant.

Band	Mode	Test Position	Ch.	Freq. (MHz)	Average Power (dBm)	Tune-Up Limit (dBm)	Scaling Factor	Measured SAR (W/kg)	Reported SAR (W/kg)
--	--	--	--	--	--	--	--	--	--

## 12. EXPOSURE POSITIONS CONSIDERATION

### 12.1. Multiple Transmitter Evaluation

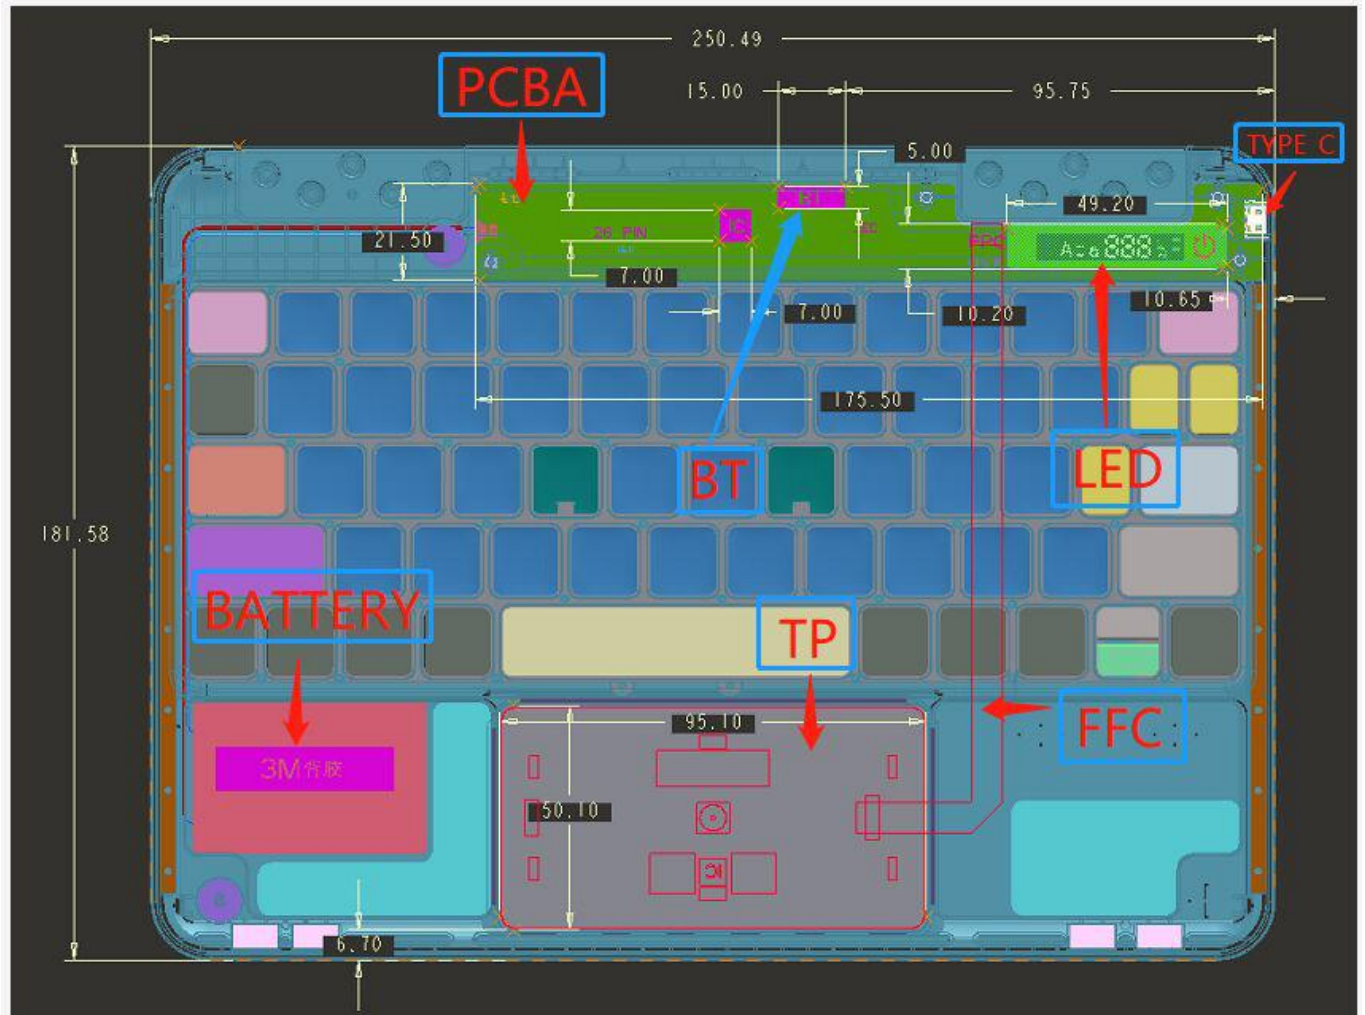

Antennas	Distance of the Antenna to the EUT surface edge					
	Front	Back	Left	Right	Top	Bottom
ANT	≤25mm	≤25mm	>25mm	>25mm	≤25mm	>25mm

**APPENDIX A: SYSTEM CHECKING SCANS**

**Dipole2450V2**


Communication System: UID 0, CW; Communication System Band: D2450 (2450.0 MHz); Frequency: 2450 MHz; Communication System PAR: 0 dB; PMF: 1  
 Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.73$  S/m;  $\epsilon_r = 39.01$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
 Phantom section: Flat Section  
 Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY Configuration:

- Probe: EX3DV4 - SN3881; ConvF(8.07, 8.07, 8.07) @ 2450 MHz; Calibrated: 2021-07-23
- Sensor-Surface: 4mm (Mechanical Surface Detection),  $z = 1.0, 31.0$
- Electronics: DAE4 Sn1637; Calibrated: 2021-11-05
- Phantom: SAM1; Type: QD 000 P41 AA;
- DASYS 52.10.4(1527); SEMCAD X 14.6.14(7483)

**Head/Dipole2450/Area Scan (61x61x1):** Interpolated grid:  $dx=1.500$  mm,  $dy=1.500$  mm  
 Reference Value = 109.4 V/m; Power Drift = -0.17 dB  
**Fast SAR: SAR(1 g) = 13.15 W/kg; SAR(10 g) = 6.03 W/kg**  
 Maximum value of SAR (interpolated) = 23.4 W/kg

**Head/Dipole2450/Zoom Scan (5x5x7)/Cube 0:** Measurement grid:  $dx=8$ mm,  $dy=8$ mm,  $dz=5$ mm  
 Reference Value = 109.4 V/m; Power Drift = -0.17 dB  
 Peak SAR (extrapolated) = 27.7 W/kg  
**SAR(1 g) = 13.04 W/kg; SAR(10 g) = 5.95 W/kg**  
 Smallest distance from peaks to all points 3 dB below = 9.3 mm  
 Ratio of SAR at M2 to SAR at M1 = 45.7%  
 Maximum value of SAR (measured) = 22.8 W/kg

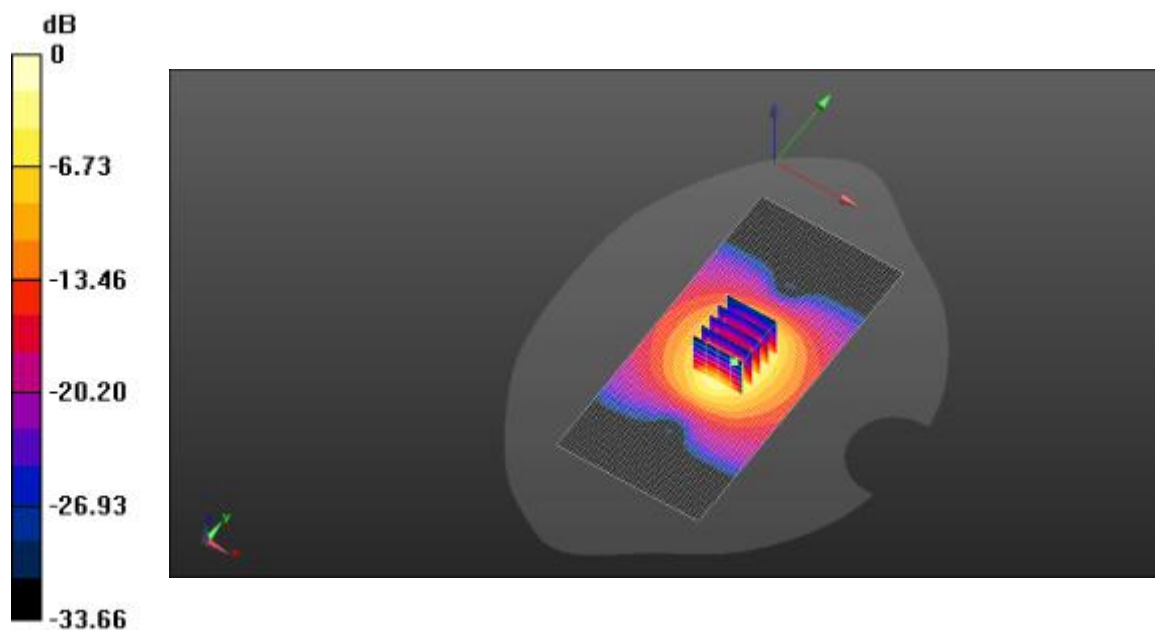

0 dB = 23.4 W/kg = 13.89 dBW/kg

**APPENDIX B. MEASUREMENT SCANS**



**BLE Body Facedown CH0**

Communication System: UID 10030 - CAA, IEEE 802.15.1 Bluetooth (GFSK, DH1); Communication System Band: ISM 2.4 GHz Band (2402.0 - 2480.0 MHz); Frequency: 2402 MHz; Communication System PAR: 5.295 dB; PMF: 1.83865

Medium parameters used:  $f = 2402$  MHz;  $\sigma = 1.89$  S/m;  $\epsilon_r = 38$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007)

DASY Configuration:

- Probe: EX3DV4 - SN3881; ConvF(8.07, 8.07, 8.07) @ 2450 MHz; Calibrated: 2021-07-23
- Sensor-Surface: 4mm (Mechanical Surface Detection),  $z = 1.0, 31.0$
- Electronics: DAE4 Sn1637; Calibrated: 2021-11-05
- Phantom: SAM1; Type: QD 000 P41 AA;
- DASYS 52.10.4(1527); SEMCAD X 14.6.14(7483)

**BLE Body Facedown/Area Scan (61x61x1):** Interpolated grid:  $dx=1.500$  mm,  $dy=1.500$  mm

Reference Value = 1.12 V/m; Power Drift = 0.02 dB

**Fast SAR: SAR(1 g) = 0.029 W/kg; SAR(10 g) = 0.017 W/kg**

Maximum value of SAR (interpolated) = 0.033 W/kg

**BLE Body Facedown/Zoom Scan (5x5x7)/Cube 0:** Measurement grid:  $dx=8$ mm,  $dy=8$ mm,  $dz=5$ mm

Reference Value = 1.12 V/m; Power Drift = 0.02 dB


Peak SAR (extrapolated) = 0.050 W/kg

**SAR(1 g) = 0.027 W/kg; SAR(10 g) = 0.016 W/kg**

Smallest distance from peaks to all points 3 dB below = 8.8 mm

Ratio of SAR at M2 to SAR at M1 = 51.1%

Maximum value of SAR (measured) = 0.033 W/kg

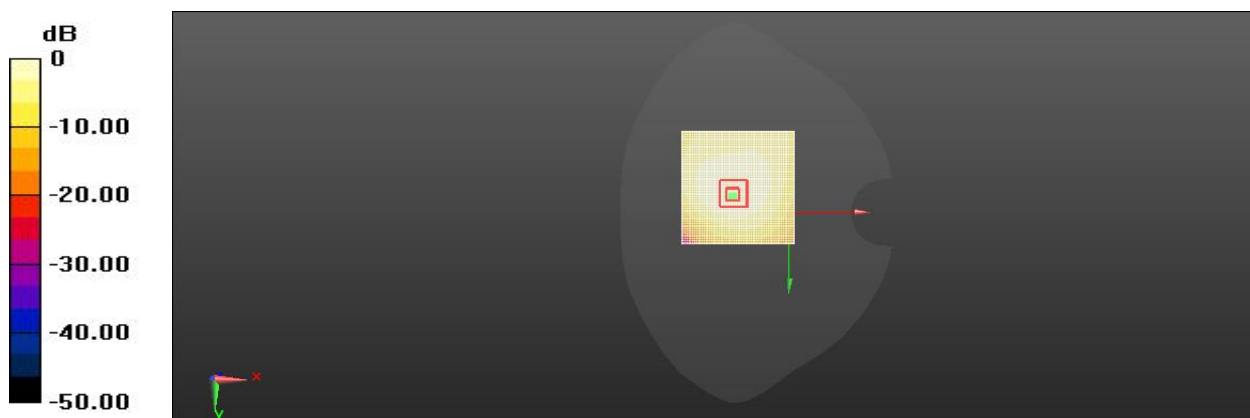

0 dB = 0.033 W/kg = -14.31 dBW/kg

## APPENDIX C: RELEVANT PAGES FROM PROBE CALIBRATION REPORT(S)



In Collaboration with  
**S P E A G**  
 CALIBRATION LABORATORY



中国认可  
 国际互认  
 校准  
 CALIBRATION  
 CNAS L0570

1810363

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
 E-mail: cntl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

Client **SMQ**

Certificate No: **Z21-60261**

### CALIBRATION CERTIFICATE

Object: EX3DV4 - SN : 3881

Calibration Procedure(s): FF-Z11-004-02  
 Calibration Procedures for Dosimetric E-field Probes

Calibration date: July 23, 2021

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	101919	15-Jun-21(CTTL, No.J21X04466)	Jun-22
Power sensor NRP-Z91	101547	15-Jun-21(CTTL, No.J21X04466)	Jun-22
Power sensor NRP-Z91	101548	15-Jun-21(CTTL, No.J21X04466)	Jun-22
Reference 10dBAttenuator	18N50W-10dB	10-Feb-20(CTTL, No.J20X00525)	Feb-22
Reference 20dBAttenuator	18N50W-20dB	10-Feb-20(CTTL, No.J20X00526)	Feb-22
Reference Probe EX3DV4	SN 3617	27-Jan-21(SPEAG, No.EX3-3617_Jan21)	Jan-22
DAE4	SN 1556	15-Jan-21(SPEAG, No.DAE4-1556_Jan21)	Jan-22
Secondary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
SignalGenerator MG3700A	6201052605	16-Jun-21(CTTL, No.J21X04467)	Jun-22
Network Analyzer E5071C	MY46110673	21-Jan-21(CTTL, No.J20X00515)	Jan-22

	Name	Function	Signature
Calibrated by:	Yu Zongying	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyuan	SAR Project Leader	

Issued: July 25, 2021

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z21-60261

Page 1 of 9



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com <http://www.chinattl.cn>

#### Glossary:

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A,B,C,D	modulation dependent linearization parameters
Polarization $\Phi$	$\Phi$ rotation around probe axis
Polarization $\theta$	$\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), $\theta=0$ is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

#### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>:** Assessed for E-field polarization  $\theta=0$  (fs900MHz in TEM-cell;  $f>1800$ MHz: waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not effect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>:** DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR:** PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; VR<sub>x,y,z</sub>; A,B,C** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for fs800MHz) and inside waveguide using analytical field distributions based on power measurements for  $f>800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$ MHz to  $\pm 100$ MHz.
- Spherical isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle:** The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).



In Collaboration with  
**s p e a g**  
**CALIBRATION LABORATORY**

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
 E-mail: cttl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

## DASY/EASY – Parameters of Probe: EX3DV4 – SN:3881

### Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup>	0.27	0.27	0.35	$\pm 10.0\%$
DCP(mV) <sup>B</sup>	101.1	100.1	105.5	

### Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB· $\mu\text{V}$	C	D dB	VR mV	Unc <sup>E</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	119.1	$\pm 2.9\%$
		Y	0.0	0.0	1.0		116.7	
		Z	0.0	0.0	1.0		141.2	

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X, Y, Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 4).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.





In Collaboration with  
**s p e a g**  
 CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
 E-mail: cntl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

## DASY/EASY – Parameters of Probe: EX3DV4 – SN:3881

### Calibration Parameter Determined in Head Tissue Simulating Media


f [MHz] <sup>c</sup>	Relative Permittivity <sup>f</sup>	Conductivity (S/m) <sup>f</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>g</sup>	Depth <sup>g</sup> (mm)	Unct. (k=2)
750	41.9	0.89	9.92	9.92	9.92	0.40	0.72	±12.1%
835	41.5	0.90	9.52	9.52	9.52	0.18	1.16	±12.1%
900	41.5	0.97	9.50	9.50	9.50	0.35	0.86	±12.1%
1750	40.1	1.37	8.29	8.29	8.29	0.22	0.95	±12.1%
1810	40.0	1.40	8.09	8.09	8.09	0.18	1.11	±12.1%
1900	40.0	1.40	7.99	7.99	7.99	0.21	1.16	±12.1%
2300	39.5	1.67	7.75	7.75	7.75	0.34	0.88	±12.1%
2450	39.2	1.80	7.56	7.56	7.56	0.40	0.85	±12.1%
2600	39.0	1.96	7.33	7.33	7.33	0.60	0.66	±12.1%
3300	38.2	2.71	7.05	7.05	7.05	0.41	0.89	±13.3%
3500	37.9	2.91	6.89	6.89	6.89	0.40	0.93	±13.3%
3700	37.7	3.12	6.59	6.59	6.59	0.35	1.10	±13.3%
3900	37.5	3.32	6.40	6.40	6.40	0.30	1.52	±13.3%
4200	37.1	3.63	6.31	6.31	6.31	0.35	1.38	±13.3%
4400	36.9	3.84	6.23	6.23	6.23	0.35	1.32	±13.3%
4600	36.7	4.04	6.15	6.15	6.15	0.40	1.30	±13.3%
4800	36.4	4.25	6.10	6.10	6.10	0.40	1.32	±13.3%
4950	36.3	4.40	5.91	5.91	5.91	0.40	1.32	±13.3%
5250	35.9	4.71	5.22	5.22	5.22	0.40	1.45	±13.3%
5600	35.5	5.07	4.72	4.72	4.72	0.45	1.45	±13.3%
5750	35.4	5.22	4.79	4.79	4.79	0.45	1.50	±13.3%

<sup>c</sup> Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>f</sup> At frequency below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>g</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)



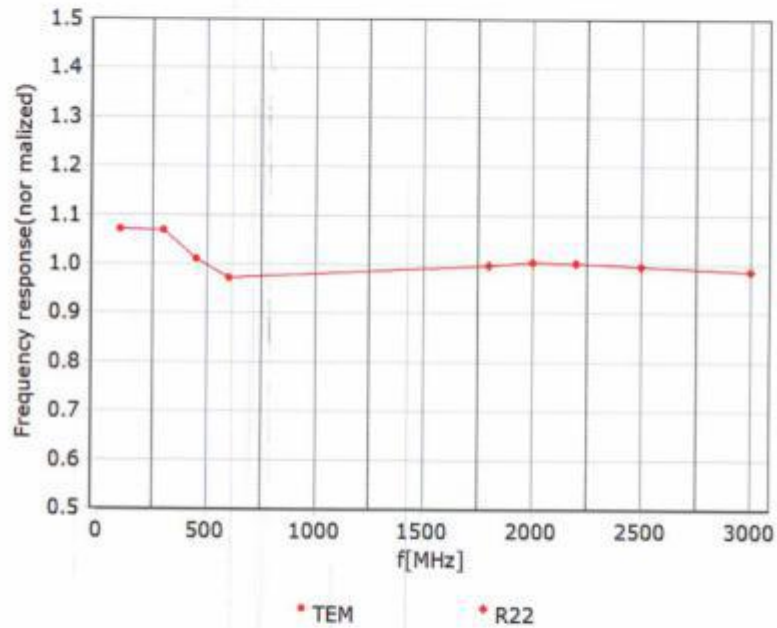


Uncertainty of Frequency Response of E-field:  $\pm 7.4\%$  ( $k=2$ )

### Receiving Pattern ( $\Phi$ ), $\theta=0^\circ$

**f=600 MHz, TEM**

**f=1800 MHz, R22**

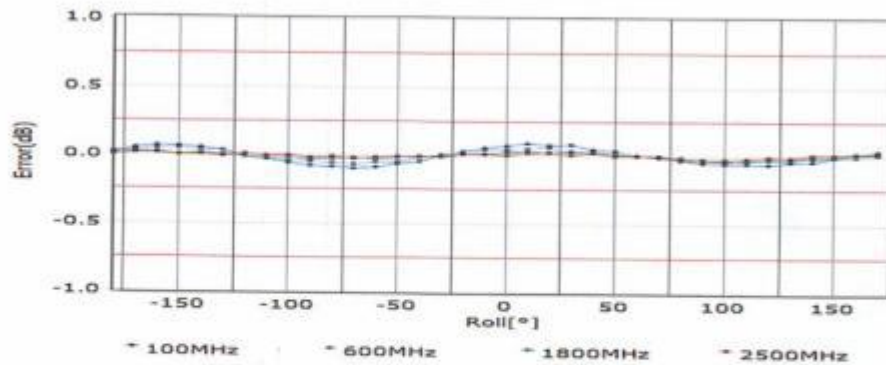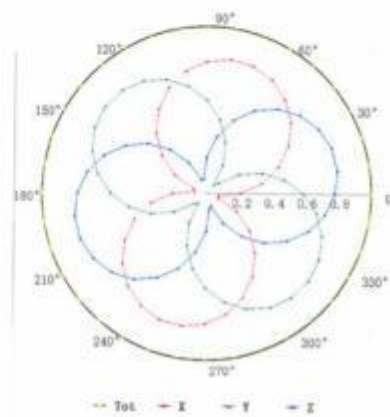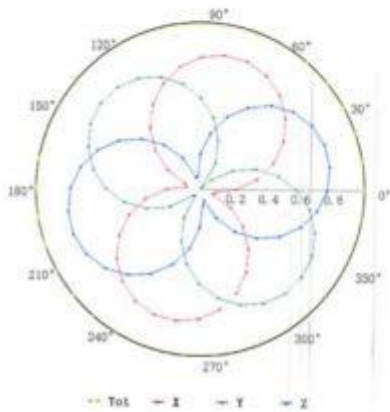

Uncertainty of Axial Isotropy Assessment:  $\pm 1.2\%$  ( $k=2$ )







In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: ccl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

### Dynamic Range f(SAR<sub>head</sub>) (TEM cell, f = 900 MHz)

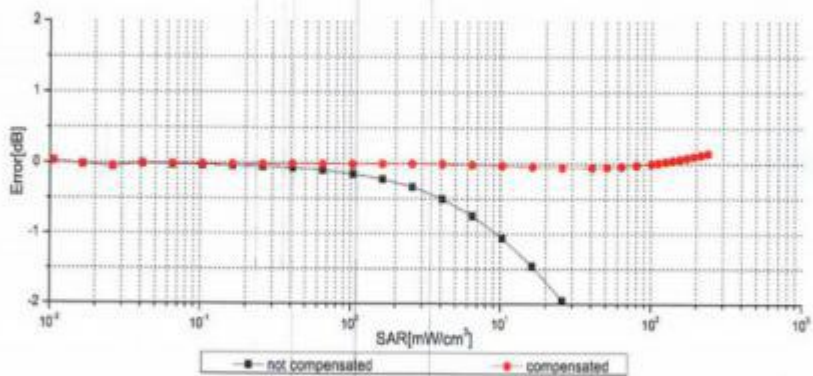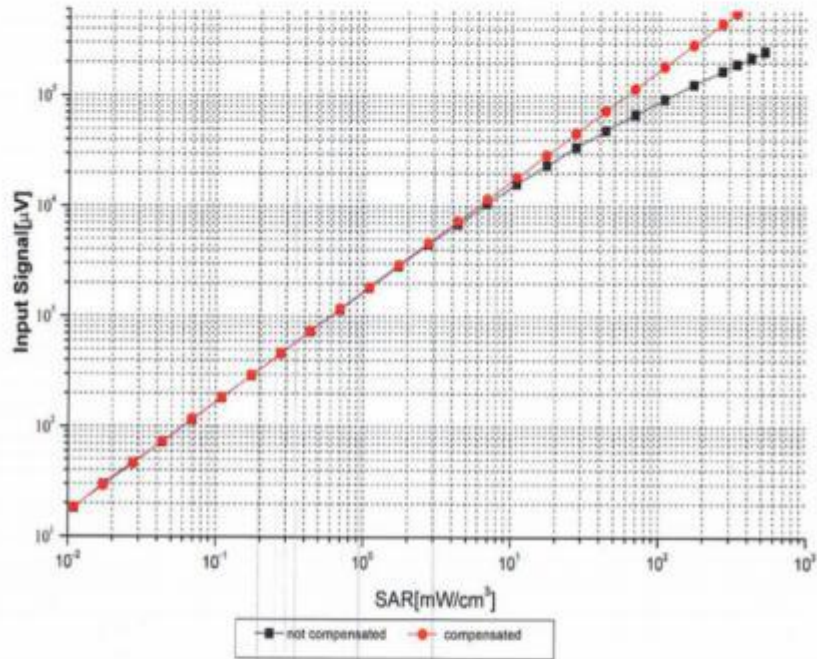

Uncertainty of Linearity Assessment: ±0.9% (k=2)





In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)


## Conversion Factor Assessment

f=750 MHz,WGLS R9(H\_convF)

f=1750 MHz,WGLS R22(H\_convF)

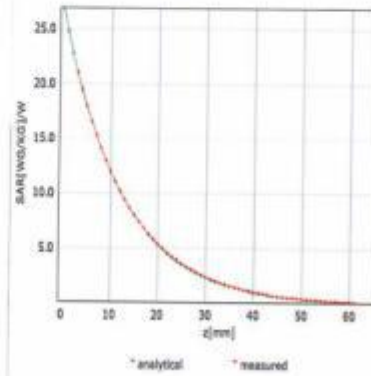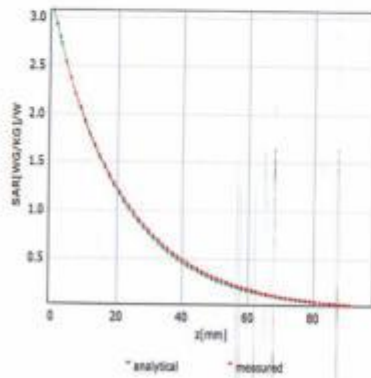

## Deviation from Isotropy in Liquid

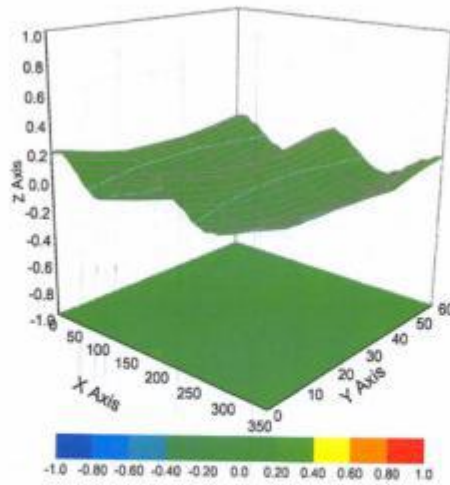

Uncertainty of Spherical Isotropy Assessment:  $\pm 3.2\%$  ( $k=2$ )

Certificate No.:Z21-60261

Page 8 of 9

## DASY/EASY – Parameters of Probe: EX3DV4 – SN:3881

### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	127
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	9mm
Tip Diameter	2.5mm
Probe Tip to Sensor X Calibration Point	1mm
Probe Tip to Sensor Y Calibration Point	1mm
Probe Tip to Sensor Z Calibration Point	1mm
Recommended Measurement Distance from Surface	1.4mm

4819052/08



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY



中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L0570

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: ttl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

Client : **SMQ**

Certificate No: **Z21-60443**

### CALIBRATION CERTIFICATE

Object: **DAE4 - SN: 1637**

Calibration Procedure(s): **FF-Z11-002-01**  
Calibration Procedure for the Data Acquisition Electronics (DAEx)

Calibration date: **November 05, 2021**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Process Calibrator 753	1971018	15-Jun-21 (CTTL, No.J21X04465)	Jun-22

	Name	Function	Signature
Calibrated by:	Yu Zongying	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyuan	SAR Project Leader	

Issued: November 07, 2021

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: ttl@chinatl.com Http://www.chinatl.cn

**Glossary:**

DAE data acquisition electronics  
Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

**Methods Applied and Interpretation of Parameters:**

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.

### DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 $\mu$ V, full range = -100...+300 mV  
Low Range: 1LSB = 61nV, full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	404.999 $\pm$ 0.15% (k=2)	404.815 $\pm$ 0.15% (k=2)	404.984 $\pm$ 0.15% (k=2)
Low Range	3.96454 $\pm$ 0.7% (k=2)	3.99368 $\pm$ 0.7% (k=2)	4.00497 $\pm$ 0.7% (k=2)

### Connector Angle

Connector Angle to be used in DASY system	23.5° $\pm$ 1°
---	----------------

**APPENDIX D: RELEVANT PAGES FROM DAE& DIPOLE VALIDATION KIT  
REPORT(S)**



486810/06



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY



中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L0570

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, Chi  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

Client

SMQ

Certificate No: Z21-60306

### CALIBRATION CERTIFICATE

Object: D2450V2 - SN: 818

Calibration Procedure(s): FF-Z11-003-01  
Calibration Procedures for dipole validation kits

Calibration date: August 26, 2021

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	23-Sep-20 (CTTL, No.J20X08336)	Sep-21
Power sensor NRP8S	104291	23-Sep-20 (CTTL, No.J20X08336)	Sep-21
Reference Probe EX3DV4	SN 7517	03-Feb-21(CTTL-SPEAG,No.Z21-60001)	Feb-22
DAE3	SN 536	06-Nov-20(CTTL-SPEAG,No.Z20-60452)	Nov-21
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	01-Feb-21 (CTTL, No.J21X00593)	Jan-22
NetworkAnalyzer E5071C	MY46110673	14-Jan-21 (CTTL, No.J21X00232)	Jan-22

	Name	Function	Signature
Calibrated by:	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyuan	SAR Project Leader	

Issued: August 31, 2021

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z21-60306

Page 1 of 6





In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

#### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
N/A	not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

#### Additional Documentation:

- DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution Corresponds to a coverage probability of approximately 95%.



In Collaboration with  
**s p e a g**  
 CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
 Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
 E-mail: cttl@chinattl.com http://www.chinattl.cn

**Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

**Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.0 ± 6 %	1.77 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	----	----

**SAR result with Head TSL**

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	12.9 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.2 W/kg ± 18.8 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.91 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.8 W/kg ± 18.7 % (k=2)



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com http://www.chinattl.cn

## Appendix (Additional assessments outside the scope of CNAS L0570)

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.7Ω+ 3.89jΩ
Return Loss	- 25.7dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.071 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG
-----------------	-------



In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: ctll@chinattl.com http://www.chinattl.cn

**DASY5 Validation Report for Head TSL**

Date: 08.26.2021

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 818**

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 2450$  MHz;  $\sigma = 1.772$  S/m;  $\epsilon_r = 40.04$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section

DASY5 Configuration:

- Probe: EX3DV4 - SN7517; ConvF(7.34, 7.34, 7.34) @ 2450 MHz; Calibrated: 2021-02-03
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn536; Calibrated: 2020-11-06
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm**

Reference Value = 107.9 V/m; Power Drift = -0.02 dB


Peak SAR (extrapolated) = 27.4 W/kg

**SAR(1 g) = 12.9 W/kg; SAR(10 g) = 5.91 W/kg**

Smallest distance from peaks to all points 3 dB below = 9 mm

Ratio of SAR at M2 to SAR at M1 = 46.9%

Maximum value of SAR (measured) = 22.0 W/kg

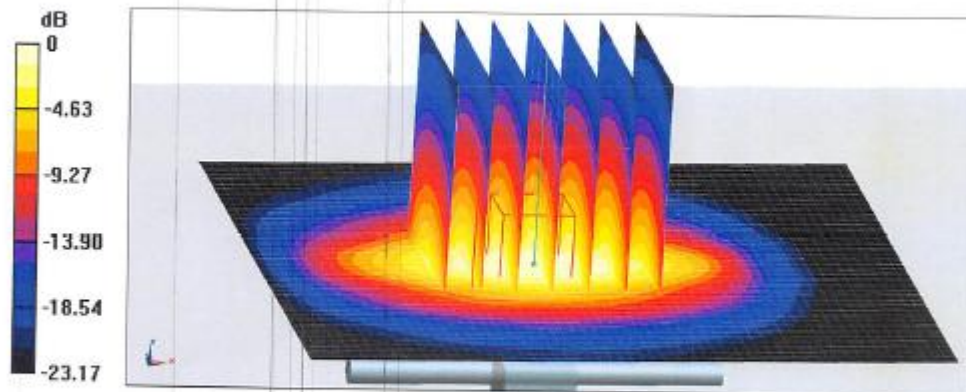

0 dB = 22.0 W/kg = 13.42 dBW/kg






In Collaboration with  
**s p e a g**  
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504  
E-mail: cctl@chinatl.com http://www.chinatl.cn

### Impedance Measurement Plot for Head TSL

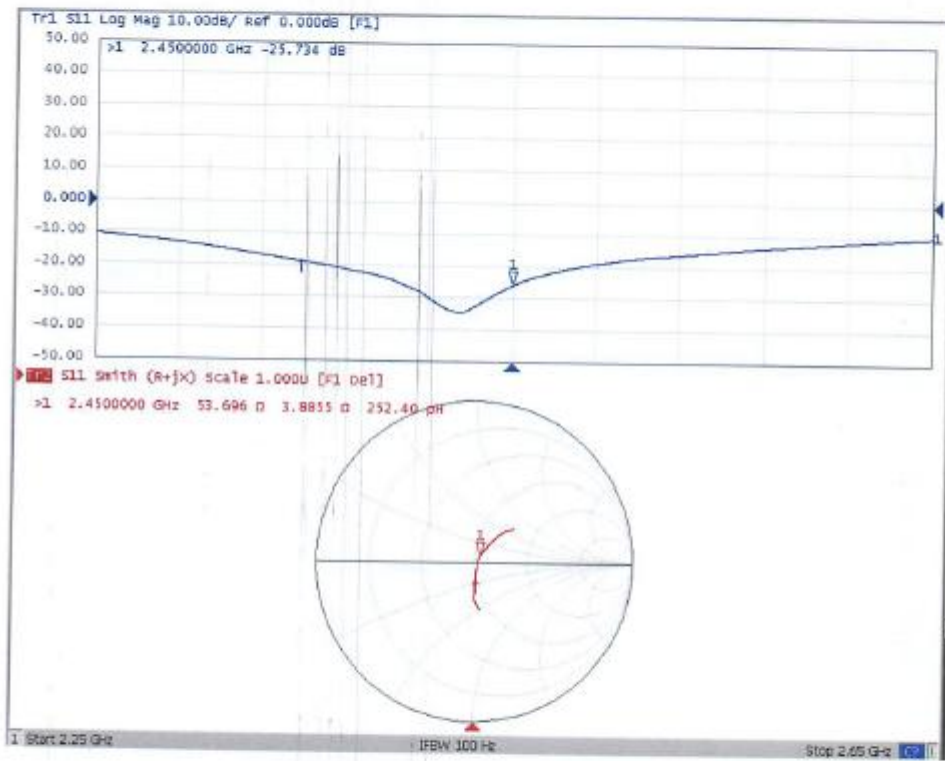

### 13. Photographs of the Test Set-Up


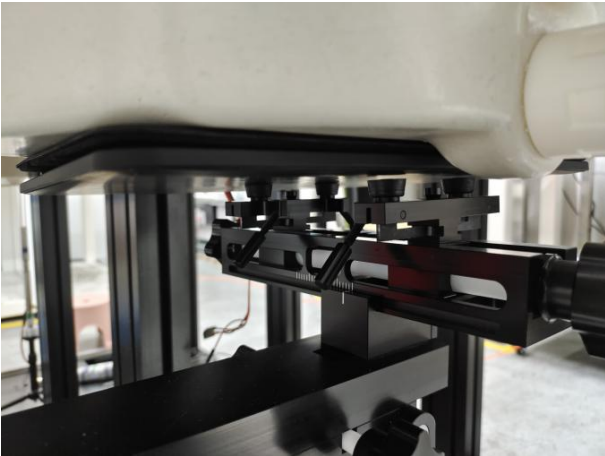
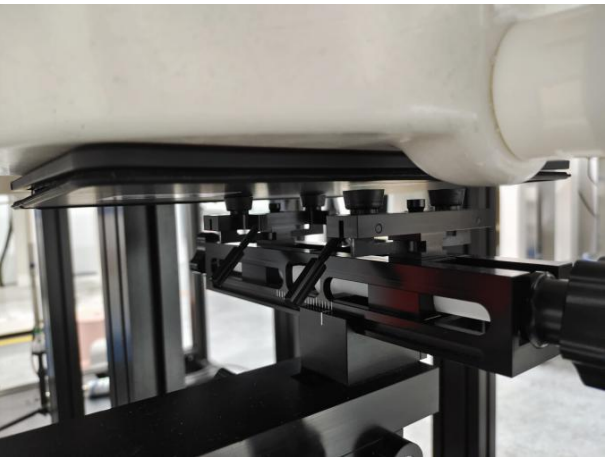
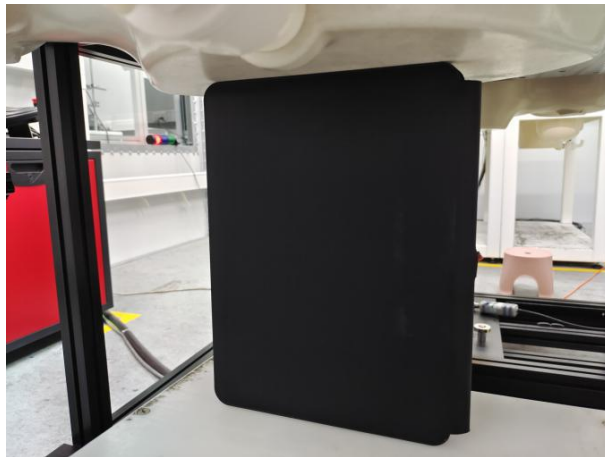
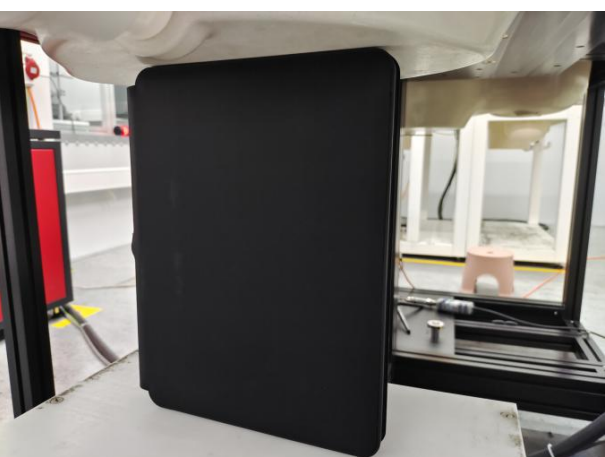

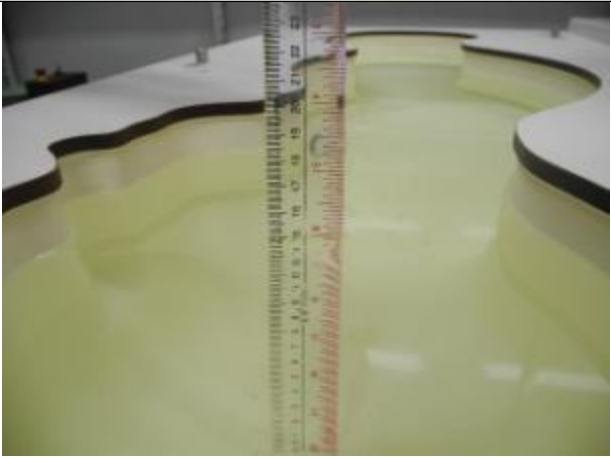
<p>Photo 1: Measurement System DASY5</p> 	<p>Photo 2: Front Side 0mm</p> 
<p>Photo 3: Rear View 0mm</p> 	<p>Photo 4: Left Side 0mm</p> 
<p>Photo 5: Right Side 0mm</p> 	<p>Photo 6: Top Side 0mm</p> 

Photo 7: Bottom Side 0mm



Photograph: Liquid depth

Photo 8: Head 2450 Depth (15.0cm)	N/A
	N/A
N/A	N/A
N/A	N/A