



Impedance Plot for SN 29/15 DIP 2G450-393
2450 Head

Calibrated impedance: $52.3\Omega + 3.4j\Omega$; Measurement impedance: $50.0\Omega + 5.0j\Omega$ (within 5Ω)

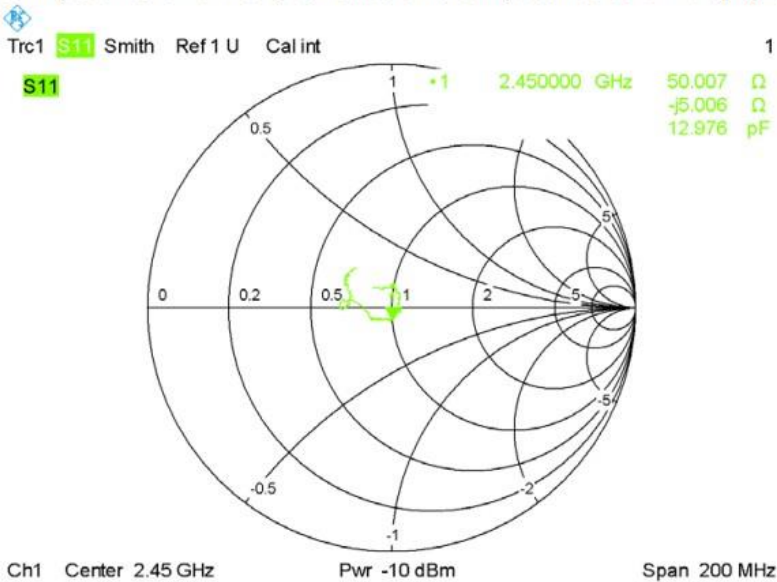

Date: 21.FEB.2024 19:04:50

Calibrated return loss: -27.80dB; Measurement return loss: -26.75dB (within 20%)

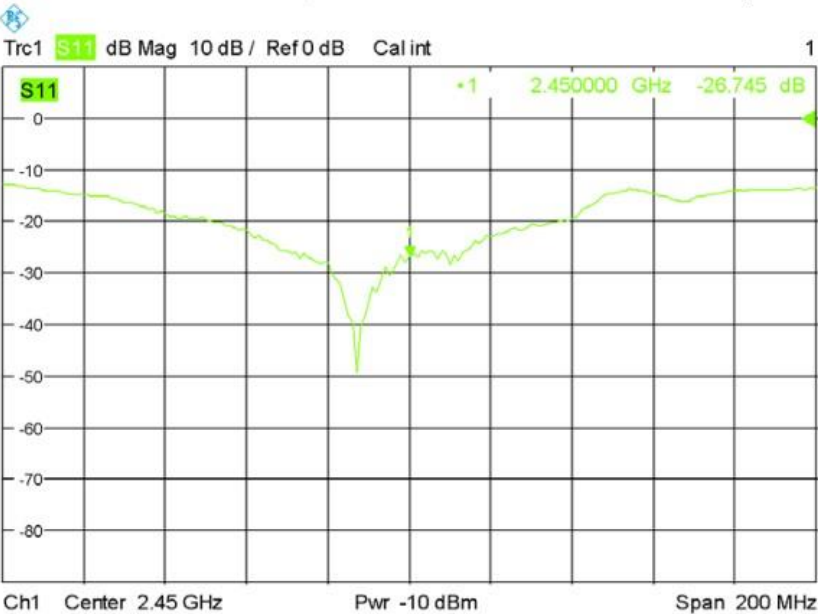


Date: 26.FEB.2024 19:28:46

Impedance Plot for SN17/22 DIP 5G000-671

5200 Head

Calibrated impedance: $54.06\Omega + 8.44j\Omega$; Measurement impedance: $55.03\Omega + 7.00j\Omega$ (within 5Ω)

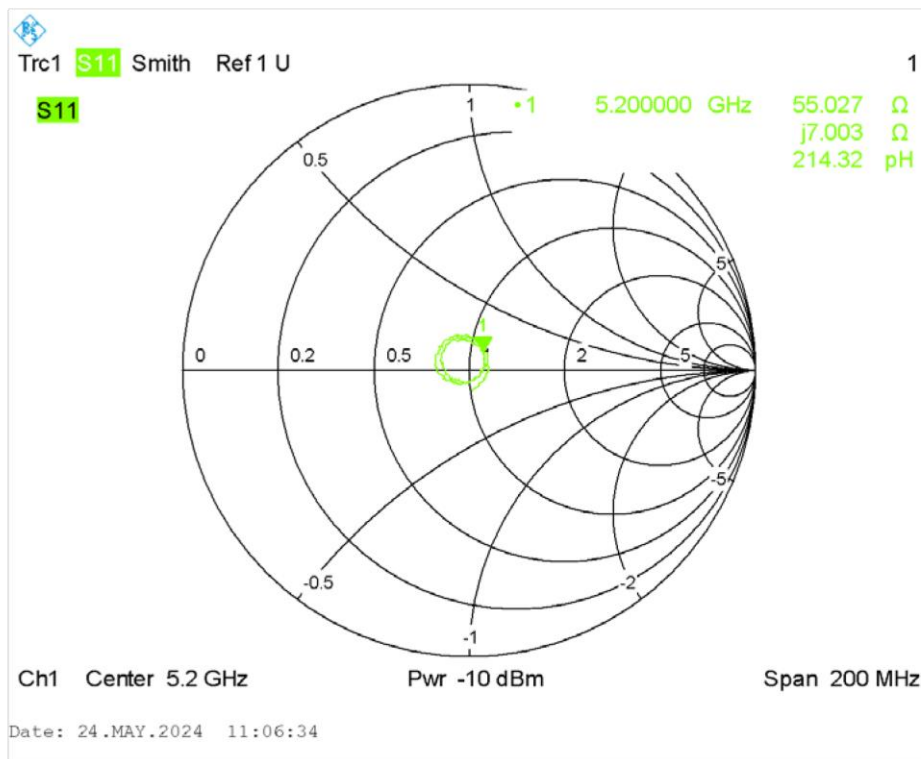

Calibrated return loss: -20.52dB; Measurement return loss: -21.29dB (within 20%)

