



SAR TEST REPORT

Product Name	RFID Handheld Reader
Model Name	PLATINO
Brand Name	Star Systems
FCC ID	2AA7KPLATINO-WF2014
Applicant	Star Systems International Limited
Manufacturer	Shenzhen Zoko Industry Development Company Limited
Date of issue	August 7, 2015

TA Technology (Shanghai) Co., Ltd.

Report No.: RXA1411-0262SAR01R1

GENERAL SUMMARY

Reference Standard(s)	FCC 47CFR §2.1093 Radiofrequency Radiation Exposure Evaluation: Portable Devices ANSI C95.1- 1992: Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz.(IEEE Std C95.1-1991) IEEE Std 1528™-2003: IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques. KDB 865664 D01 SAR measurement 100 MHz to 6 GHz v01r03: SAR Measurement Requirements for 100 MHz to 6 GHz KDB 447498 D01 Mobile Portable RF Exposure v05r02: Mobile and Portable Device RF Exposure Procedures and Equipment Authorization Policies
Conclusion	This portable wireless equipment has been measured in all cases requested by the relevant standards. Test results in Chapter 7 of this test report are below limits specified in the relevant standards for the tested bands only. General Judgment: Pass
Comment	The test result only responds to the measured sample.
Approved by	Kai Xu DirectorTiang peng Lan Jiangpeng LanPerformed byJie Li Jie Li

Director

SAR Manager

SAR Engineer

TA Technology (Shanghai) Co., Ltd. Test Report	
Report No.: RXA1411-0262SAR01R1	Page 3 of 65

TABLE OF CONTENT

1. General Information	5
1.1. Notes of the Test Report	5
1.2. Testing Laboratory	5
1.3. Applicant Information	6
1.4. Manufacturer Information	6
1.5. Information of EUT	7
1.6. EUT Antenna Locations	
1.7. The Maximum Reported SAR _{10g}	9
1.8. Test Date	9
2. SAR Measurements System Configuration	
2.1. SAR Measurement Set-up	10
2.2. DASY5 E-field Probe System	11
2.2.1. EX3DV4 Probe Specification	11
2.2.2. E-field Probe Calibration	
2.3. Other Test Equipment	
2.3.1. Device Holder for Transmitters	
2.3.2. Phantom	13
2.4. Scanning Procedure	13
2.5. Data Storage and Evaluation	15
2.5.1. Data Storage	15
2.5.2. Data Evaluation by SEMCAD	15
3. Laboratory Environment	17
4. Tissue-equivalent Liquid	
4.1. Tissue-equivalent Liquid Ingredients	
4.2. Tissue-equivalent Liquid Properties	
5. System Check	
5.1. Description of System Check	
5.2. System Check Results	
6. Operational Conditions during Test	
6.1. General Description of Test Procedures	
6.2. Test Positions	
6.3. Measurement Variability	
7. Test Results	
7.1. Conducted Power Results	
7.2. Standalone SAR Test Exclusion Considerations	
7.3. SAR Test Results	
7.3.1. RFID 900MHz	-
7.4. Simultaneous Transmission Conditions	
8. Measurement Uncertainty	
9. Main Test Instruments	

Report No.: RXA1411-0262SAR01R1	Page 4 of 65
ANNEX A: Test Layout	
ANNEX B: System Check Results	
ANNEX C: Highest Graph Results	
ANNEX D: Probe Calibration Certificate	
ANNEX E: D835V2 Dipole Calibration Certificate	
ANNEX F: DAE4 Calibration Certificate	
ANNEX G: The EUT Appearances and Test Configuration	61
ANNEX K: System Validation	65

1. General Information

1.1. Notes of the Test Report

TA Technology (Shanghai) Co., Ltd. has obtained the accreditation of China National Accreditation Service for Conformity Assessment (CNAS), and accreditation number: L2264.

TA Technology (Shanghai) Co., Ltd. guarantees the reliability of the data presented in this test report, which is the results of measurements and tests performed for the items under test on the date and under the conditions stated in this test report and is based on the knowledge and technical facilities available at TA Technology (Shanghai) Co., Ltd. at the time of execution of the test.

TA Technology (Shanghai) Co., Ltd. is liable to the client for the maintenance by its personnel of the confidentiality of all information related to the items under test and the results of the test. The sample under test was selected by the Client. This report only refers to the item that has undergone the test.

This report alone does not constitute or imply by its own an approval of the product by the certification Bodies or competent Authorities. This report cannot be used partially or in full for publicity and/or promotional purposes without previous written approval of **TA Technology (Shanghai) Co., Ltd.** and the Accreditation Bodies, if it applies.

If the electronic report is inconsistent with the printed one, it should be subject to the latter.

1.2. Testing Laboratory

Company:	TA Technology (Shanghai) Co., Ltd.
Address:	No.145, Jintang Rd, Tangzhen Industry Park, Pudong Shanghai, China
City:	Shanghai
Post code:	201201
Country:	P. R. China
Contact:	Xu Kai
Telephone:	+86-021-50791141/2/3
Fax:	+86-021-50791141/2/3-8000
Website:	http://www.ta-shanghai.com
E-mail:	xukai@ta-shanghai.com

1.3. Applicant Information

Company:	Star Systems International Limited
Address:	Unit A01, 24/F, Gold King Industrial Building, 35-41 Tai Lin Pai Road, Kwai
	Chung, New Territories, Hong Kong

1.4. Manufacturer Information

Company:Zoko Industry Development Company LimitedAddress:5/F, Administration Building, Jinxing Industry District, Dongbin Road,
Nanshan, Shenzhen, China


Page 7 of 65

1.5. Information of EUT General Information

Device Type:	Portable Device		
Exposure Category:	Uncontrolled Environment / General Population		
State of Sample:	Prototype Unit		
Product SN:	15013801		
Hardware Version:	ZKT960-V2.1		
Software Version:	V1.06		
Antenna Type:	Internal Antenna		
Device Operating Configurations :			
Test Mode(s):	RFID 900MHz		
Test Modulation:	DSB-ASK		
	Mode	Tx (MHz)	
Operating Frequency Range(s):	RFID 900MHz	902.75 ~ 927.25	
	WiFi	2412 ~ 2462	
Power Level set:	RFID 900MHz: 21dBm		

Page 8 of 65

1.6. EUT Antenna Locations

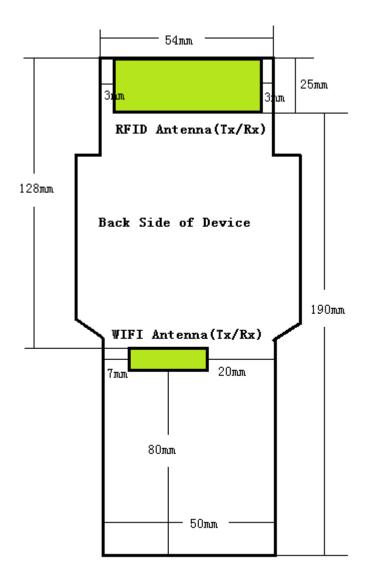

Page 9 of 65

1.7. The Maximum Reported SAR_{10g}

Body SAR Configuration

	Test Position	Channel /Frequency(MHz)	Limit SAR _{10g} 4 W/kg	
Mode			Measured SAR _{10g} (W/kg)	Reported SAR _{10g} (W/kg)
RFID 900MHz	Top Edge	1/902.75	1.430	2.086

1.8. Test Date

The test performed on January 25, 2015.

2. SAR Measurements System Configuration

2.1. SAR Measurement Set-up

The DASY5 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Stäubli RX family) with controller and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e. an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronic (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- A unit to operate the optical surface detector which is connected to the EOC.
- The Electro-Optical Coupler (EOC) performs the conversion from the optical into a digital electric signal of the DAE. The EOC is connected to the DASY5 measurement server.
- The DASY5 measurement server, which performs all real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operation. A computer operating Windows 2003
- DASY5 software and SEMCAD data evaluation software.
- Remote control with teach panel and additional circuitry for robot safety such as warning lamps, etc.
- The generic twin phantom enabling the testing of left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- System validation dipoles allowing to validate the proper functioning of the system.

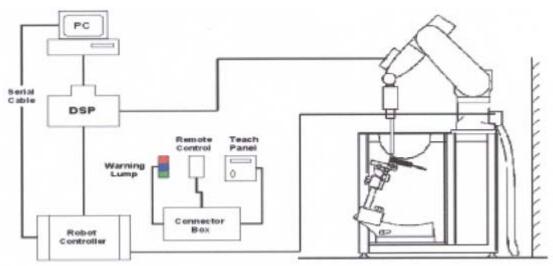


Figure 1 SAR Lab Test Measurement Set-up

2.2. DASY5 E-field Probe System

The SAR measurements were conducted with the dosimetric probe EX3DV4(manufactured by SPEAG), designed in the classical triangular configuration and optimized for dosimetric evaluation.

2.2.1. EX3DV4 Probe Specification

- Construction Symmetrical design with triangular core Built-in shielding against static charges PEEK enclosure material (resistant to organic solvents, e.g., DGBE)
- Calibration ISO/IEC 17025 calibration service available
- Frequency 10 MHz to > 6 GHz Linearity: ± 0.2 dB (30 MHz to 6 GHz)



Figure 2.EX3DV4 E-field Probe

- Directivity \pm 0.3 dB in HSL (rotation around probe axis) \pm 0.5 dB in tissue material (rotation normal to probe axis)
- Dynamic Range 10μ W/g to > 100 mW/g Linearity:
 - \pm 0.2dB (noise: typically < 1 μ W/g)
- Dimensions Overall length: 330 mm (Tip: 20 mm) Tip diameter: 2.5 mm (Body: 12 mm) Typical distance from probe tip to dipole centers: 1 mm
- Application High precision dosimetric measurements in any exposure scenario (e.g., very strong gradient fields). Only probe which enables compliance testing for frequencies up to 6 GHz with precision of better 30%.



Figure 3. EX3DV4 E-field probe

Report No.: RXA1411-0262SAR01R1

2.2.2. E-field Probe Calibration

Each probe is calibrated according to a dosimetric assessment procedure with accuracy better than \pm 10%. The spherical isotropy was evaluated and found to be better than \pm 0.25dB. The sensitivity parameters (NormX, NormY, NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested.

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies bellow 1 GHz, and in a wave guide above 1 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees.

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$\mathbf{SAR} = \mathbf{C} \frac{\Delta \mathbf{T}}{\Delta \mathbf{t}}$$

Where: Δt = Exposure time (30 seconds), C = Heat capacity of tissue (brain or muscle), ΔT = Temperature increase due to RF exposure. Or

$$\mathbf{SAR} = \frac{|\mathbf{E}|^2 \sigma}{\rho}$$

Where:

 σ = Simulated tissue conductivity,

 ρ = Tissue density (kg/m3).

2.3. Other Test Equipment

2.3.1. Device Holder for Transmitters

The DASY device holder is designed to cope with the die rent positions given in the standard.

It has two scales for device rotation (with respect to the body axis) and device inclination (with respect to the line between the ear reference points). The rotation centers for both scales is the ear reference point (ERP). Thus the device needs no repositioning when changing the angles. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the inference of the clamp on the test results could thus be lowered.




Figure 4 Device Holder

2.3.2. Phantom

Phantom for compliance testing of handheld andbody-mounted wireless devices in the frequency range of 30 MHz to 6 GHz. ELI is fully compatible with the IEC 62209-2 standard and all known tissue simulating liquids. ELI has been optimized regarding its performance and can be integrated into our standard phantom tables. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points. The phantom is compatible with all SPEAG dosimetric probes and dipoles.

Shell Thickness 2 ±0.2 mm Filling Volume Approx. 30 liters Dimensions 190×600×400 mm (H×L×W)



2.4. Scanning Procedure

Figure 5.ELI4 Phantom

The DASY5 installation includes predefined files with recommended procedures for measurements and validation. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.

- The "reference" and "drift" measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max. ± 5 %.
- The "surface check" measurement tests the optical surface detection system of the DASY5 system by repeatedly detecting the surface with the optical and mechanical surface detector and comparing the results. The output gives the detecting heights of both systems, the difference between the two systems and the standard deviation of the detection repeatability. Air bubbles or refraction in the liquid due to separation of the sugar-water mixture gives poor repeatability (above ± 0.1mm). To prevent wrong results tests are only executed when the liquid is free of air bubbles. The difference between the optical surface detection and the actual surface depends on the probe and is specified with each probe. (It does not depend on the surface reflectivity or the probe angle to the surface within ± 30°.)

Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values

Report No.: RXA1411-0262SAR01R1

before running a detailed measurement around the hot spot. Before starting the area scan a grid spacing is set according to FCC KDB Publication 865664. During scan the distance of the probe to the phantom remains unchanged.

After finishing area scan, the field maxima within a range of 2 dB will be ascertained.

Zoom Scan

After the maximum interpolated values were calculated between the points in the cube, the SAR was averaged over the spatial volume (1g or 10g) using a 3D-Spline interpolation algorithm. The 3D-spline is composed of three one-dimensional splines with the "Not a knot" condition (in x, y, and z directions). The volume was then integrated with the trapezoidal algorithm.

• Spatial Peak Detection

The procedure for spatial peak SAR evaluation has been implemented and can determine values of masses of 1g and 10g, as well as for user-specific masses. The DASY5 system allows evaluations that combine measured data and robot positions, such as:

- maximum search
- extrapolation
- boundary correction
- peak search for averaged SAR

During a maximum search, global and local maxima searches are automatically performed in 2-D after each Area Scan measurement with at least 6 measurement points. It is based on the evaluation of the local SAR gradient calculated by the Quadratic Shepard's method. The algorithm will find the global maximum and all local maxima within -2 dB of the global maxima for all SAR distributions.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. Several measurements at different distances are necessary for the extrapolation. Extrapolation routines require at least 10 measurement points in 3-D space. They are used in the Zoom Scan to obtain SAR values between the lowest measurement points and the inner phantom surface. The routine uses the modified Quadratic Shepard's method for extrapolation.

• A Z-axis scan measures the total SAR value at the x-and y-position of the maximum SAR value found during the cube scan. The probe is moved away in z-direction from the bottom of the SAM phantom in 5mm steps.

Frequency	Maximum Area Scan Resolution (mm) (∆x _{area} , ∆y _{area})	Maximum Zoom Scan Resolution (mm) (∆x _{zoom} , ∆y _{zoom})	Maximum Zoom Scan Spatial Resolution (mm) ∆z _{zoom} (n)	Minimum Zoom Scan Volume (mm) (x,y,z)
≤ 2 GHz	≤ 15	≤ 8	≤ 5	≥ 30
2-3 GHz	≤ 12	≤ 5	≤ 5	≥ 30
3-4 GHz	≤ 12	≤ 5	≤ 4	≥ 28
4-5 GHz	≤ 10	≤ 4	≤ 3	≥ 25
5-6 GHz	≤ 10	≤ 4	≤ 2	≥ 22

Table 1: Area and Zoom Scan Resolutions per FCC KDB Publication 865664 D01

2.5. Data Storage and Evaluation

2.5.1. Data Storage

The DASY5 software stores the acquired data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension ".DAE4". The software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of incorrect parameter settings. For example, if a measurement has been performed with a wrong crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be re-evaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type ([V/m], [A/m], [°C], [mW/g], [mW/cm²], [dBrel], etc.). Some of these units are not available in certain situations or show meaningless results, e.g., a SAR output in a lossless media will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

2.5.2. Data Evaluation by SEMCAD

The SEMCAD software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters:	,	Normi, a _{i0} , a _{i1} , a _{i2}
	- Conversion factor	ConvF _i
	- Diode compression point	Dcpi
Device parameters:	- Frequency	f
	- Crest factor	cf
Media parameters:	- Conductivity	

- Density

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY5 components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics.

Report No.: RXA1411-0262SAR01R1

If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot c f / d c p_i$$

With	V_i = compensated signal of channel i	(i = x, y, z)
	U _i = input signal of channel i	(i = x, y, z)
	<i>Cf</i> = crest factor of exciting field	(DASY parameter)
	dcp_i = diode compression point	(DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field p	robes:	$E_i = (V_i / Norm_i \cdot ConvF)^{1/2}$	
H-field p	robes:	$H_{i} = (V_{i})^{1/2} \cdot (a_{i0} + a_{i1}f + a_{i2}f^{2}) / f$	
With	V _i	= compensated signal of channel i	(i = x, y, z)

Norm _i	= sensor sensitivity of channel i	(i = x, y, z)
	[mV/(V/m) ²] for E-field Probes	

ConvF	= sensitivity enhancement in solution				
a _{ij}	= sensor sensitivity factors for H-field probes				
f	= carrier frequency [GHz]				
E i	= electric field strength of channel i in V/m				
H _i	= magnetic field strength of channel i in A/m				

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = (E_x^2 + E_y^2 + E_z^2)^{1/2}$$

The primary field data are used to calculate the derived field units.

$$SAR = (E_{tot})^2 \cdot \sigma / (\rho \cdot 1000)$$

Report No.: RXA1411-0262SAR01R1

- with **SAR** = local specific absorption rate in mW/g
 - **E**_{tot} = total field strength in V/m

= conductivity in [mho/m]

or [Siemens/m]

= equivalent tissue density

in g/cm³

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid. The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = E_{tot}^{2} / 3770$$
 or $P_{pwe} = H_{tot}^{2} \cdot 37.7$

with P_{pwe} = equivalent power density of a plane wave in mW/cm²

 E_{tot} = total electric field strength in V/m

 H_{tot} = total magnetic field strength in A/m

3. Laboratory Environment

Table 2: The Requirements of the Ambient Conditions

Temperature	Min. = 18°C, Max. = 25 °C
Relative humidity	Min. = 30%, Max. = 70%
Ground system resistance	< 0.5 Ω
Ambient noise is checked and found very low	w and in compliance with requirement of standards.
Reflection of surrounding objects is minimized	ed and in compliance with requirement of standards.

4. Tissue-equivalent Liquid

4.1. Tissue-equivalent Liquid Ingredients

The liquid is consisted of water, salt, Glycol, Sugar, Preventol and Cellulose. The liquid has previously been proven to be suited for worst-case. The table 3 show the detail solution. It's satisfying the latest tissue dielectric parameters requirements proposed by the KDB 865664 D01.

MIXTURE%	FREQUENCY(Body) 835MHz
Water	52.5
Sugar	45
Salt	1.4
Preventol	0.1
Cellulose	1.0
Dielectric Parameters Target Value	f=835MHz ε=55.2 σ=0.97

Page 19 of 65

4.2. Tissue-equivalent Liquid Properties

F	To of Doto	Temp	Measured Dielectric Parameters		Target Dielectric Parameters		Limit (Within ±5%)	
Frequency	Test Date	℃ ε _r	٤r	σ(s/m)	٤ _r	σ(s/m)	Dev ε _r (%)	Dev σ(%)
835MHz (body)	2015-1-25	21.5	55.9	0.99	55.2	0.97	1.27	2.06
915MHz (body)	2015-1-25	21.5	55.5	1.09	55.0	1.06	0.87	2.83

Table 4: Dielectric Performance of Tissue Simulating Liquid

5. System Check

5.1. Description of System Check

The manufacturer calibrates the probes annually. Dielectric parameters of the tissue simulates were measured every day using the dielectric probe kit and the network analyzer. A system check measurement was made following the determination of the dielectric parameters of the simulates, using the dipole validation kit. A power level of 250 mW was supplied to the dipole antenna, which was placed under the flat section of the twin SAM phantom. The system check results (dielectric parameters and SAR values) are given in the table 5.

System check results have to be equal or near the values determined during dipole calibration with the relevant liquids and test system (± 10 %).

System check is performed regularly on all frequency bands where tests are performed with the DASY5 system.

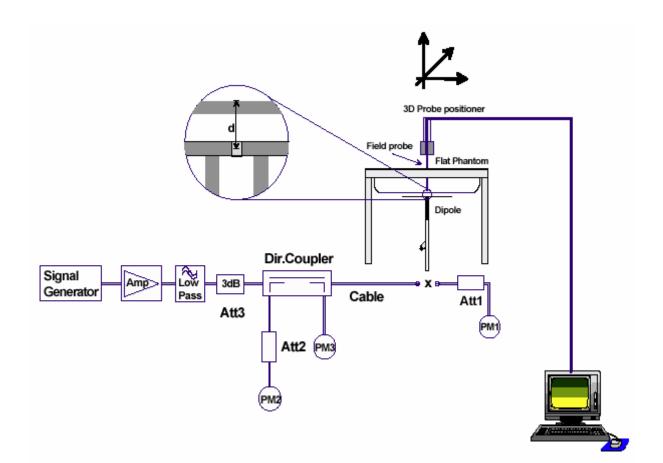


Figure 6 System Check Set-up

5.2. System Check Results

Table 5: System Check in Body Tissue Simulating Liquid

Frequency	Test Date	Diele Paran	ectric neters	250mW Measured SAR _{10g}	1W Normalized SAR _{10g}	1W Target SAR _{10g}	Limit (±10%
		٤r	σ(s/m)		(W/kg)		Deviation)
835MHz	2015-1-25	55.9	0.99	1.60	6.40	6.31	1.43
Note: 1. The graph results see ANNEX B.							
2. Tar	get Values use	d derive f	rom the ca	alibration certi	ficate		

6. Operational Conditions during Test

6.1. General Description of Test Procedures

The product use RFID technology. It can support 902-928MHz with duty cycle 100%, It has no voice call function.

For RFID SAR testing, RFID engineering testing software installed on the EUT can provide continuous transmitting RF signal with maximum output power.

6.2. Test Positions

According to a KDB inquiry, The EUT is tested at the following four test positions:

- Test Position 1: The back side of the EUT towards to the bottom of the flat phantom. The distance is 0mm. (ANNEX G Picture 4)
- Test Position 2: The left edge of the EUT towards to the bottom of the flat phantom. The distance is 0mm. (ANNEX G Picture 5)
- Test Position 3: The right edge of the EUT towards to the bottom of the flat phantom. The distance is 0mm. (ANNEX G Picture 6)
- Test Position 4: The top edge of the EUT towards to the bottom of the flat phantom. The distance is 0mm. (ANNEX G Picture 7)
- Test Position 5: The back side of the EUT antenna towards to the bottom of the flat phantom. The distance is 0mm. (ANNEX G Picture 8)

6.3. Measurement Variability

Per FCC KDB Publication 865664 D01, SAR measurement variability was assessed for each frequency band, which was determined by the SAR probe calibration point and tissue-equivalent medium used for the device measurements. When both head and body tissue-equivalent media were required for SAR measurements in a frequency band, the variability measurement procedures were applied to the tissue medium with the highest measured SAR, using the highest measured SAR configuration for that tissue-equivalent medium. These additional measurements were repeated after the completion of all measurements requiring the same head or body tissue-equivalent medium in a frequency band. The test device was returned to ambient conditions (normal room temperature) with the battery fully charged before it was re-mounted on the device holder for the repeated measurement(s) to minimize any unexpected variations in the repeated results.

SAR Measurement Variability was assessed using the following procedures for each frequency band: 1) When the original highest measured SAR is ≥ 0.80 W/kg, the measurement was repeated once. 2) A second repeated measurement was preformed only if the ratio of largest to smallest SAR for the original and first repeated measurements was > 1.20 or when the original or repeated measurement was \geq 1.45 W/kg (~ 10% from the 1-g SAR limit).

3) A third repeated measurement was performed only if the original, first or second repeated measurement was \ge 1.5 W/kg and the ratio of largest to smallest SAR for the original, first and second repeated measurements is > 1.20.

4) Repeated measurements are not required when the original highest measured SAR is < 0.80 W/kg

The same procedures should be adapted for measurements according to extremity and occupational exposure limits by applying a factor of 2.5 for extremity exposure and a factor of 5 for occupational exposure to the corresponding SAR thresholds.

7. Test Results

7.1. Conducted Power Results

Table 6: Conducted Power Measurement Results

	A	verage power(dBr	Bm)		
RFID 900MHz	Channel/Frequency(MHz)				
	1/902.75	26/914.75	51/927.25		
Test results	21.86	21.66	21.51		

Mode	Channel/ Frequency(MHz)	Data rate (Mbps)	AV Power (dBm)
		1	2.5
		2	2.3
	1	5.5	2.0
		11	2.1
		1	1.8
11b	6	2	1.9
	0	5.5	1.7
		11	1.8
		1	2.4
	11	2	2.3
		5.5	2.4
		11	2.3
		6	-3.9
		9	-4.0
		12	-4.0
	1	18	-4.1
	I	24	-4.5
		36	-4.2
		48	-4.1
		54	-4.3
11g		6	-4.3
iig		9	-4.6
		12	-4.5
	6	18	-4.5
	0	24	-4.6
		36	-4.3
		48	-4.8
		54	-4.0
	11	6	-5.0
		9	-5.1

Report No.: RXA1411-0262SAR01R1

Page 25 of 65

		40	4.0
		12	-4.8
		18	-4.6
		24	-4.6
		36	-4.5
		48	-4.3
		54	-4.4
		MCS 0	-1.4
		MCS 1	-1.6
		MCS 2	-1.8
	1	MCS 3	-1.9
		MCS 4	-1.6
		MCS 5	-1.5
		MCS 6	-1.5
		MCS 7	-1.6
		MCS 0	-1.5
		MCS 1	-1.8
		MCS 2	-1.6
11 × UT20	6	MCS 3	-1.7
11n HT20	0	MCS 4	-1.8
		MCS 5	-1.8
		MCS 6	-1.7
		MCS 7	-1.6
		MCS 0	-1.5
		MCS 1	-1.8
		MCS 2	-1.8
		MCS 3	-1.9
	11	MCS 4	-1.5
		MCS 5	-1.6
		MCS 6	-1.4
		MCS 7	-1.5
		MCS 0	-2.1
		MCS 1	-2.2
		MCS 2	-2.4
		MCS 3	-2.6
	3	MCS 4	-2.8
		MCS 5	-2.9
11n HT40		MCS 6	-2.5
		MCS 7	-2.6
		MCS 0	-2.7
		MCS 1	-2.5
	6	MCS 2	-2.3
		MCS 3	-2.1
		MCS 3 MCS 4	-2.1

Report No.: RXA1411-0262SAR01R1

Page 26 of 65

	MCS 5	-2.4
	MCS 6	-2.5
	MCS 7	-2.1
	MCS 0	-2.3
	MCS 1	-2.4
	MCS 2	-2.3 -2.4 -2.6 -2.7 -2.5 -2.4
0	MCS 3	-2.7
9	MCS 4	-2.5
	MCS 5	-2.4
	MCS 6	-2.1
	MCS 7	-2.2

7.2. Standalone SAR Test Exclusion Considerations

Per FCC KDB 447498 D01, the SAR exclusion threshold for distances <50mm is defined by the following equation:

(max. power of channel, including tune-up tolerance, mW) (min. test separation distance, mm) $*\sqrt{Frequency (GHz)} \leq 7.5$

	Band	Configuration	Frequency (MHz)	Maximum Power (dBm)	Separation Distance (mm)	Calculation Result	SAR Exclusion Thresholds	Standalone SAR
6	Wifi	Body	2462	3	5	0.63	7.5	No

7.3. SAR Test Results

7.3.1. RFID 900MHz

Table 7: SAR Values [RFID 900MHz]

- /	Channel/ Frequency (MHz)	Service		Maximum Allowed Power (dBm)	Conducted Power (dBm)	Drift \pm 0.21dB	Limit SAR _{10g} 4 W/kg			
Test Position			Duty Cycle			Drift (dB)	Measured SAR _{10g} (W/kg)	Scaling Factor	Reported SAR _{10g} (W/kg)	Graph Results
			1	Fest position	of Body (Di	stance 0mm)				
Back Side	1/902.75	DSB-ASK	1:1	23.5	21.86	-0.037	0.330	1.46	0.481	/
Front Side	NA	NA	NA	NA	NA	NA	NA	NA	NA	NA
Left Edge	1/902.75	DSB-ASK	1:1	23.5	21.86	0.090	0.744	1.46	1.085	/
Right Edge	1/902.75	DSB-ASK	1:1	23.5	21.86	0.033	0.581	1.46	0.848	/
	51/927.25	DSB-ASK	1:1	23.5	21.51	0.010	0.660	1.58	1.044	/
Top Edge	26/914.75	DSB-ASK	1:1	23.5	21.66	-0.010	0.954	1.53	1.457	/
	1/902.75	DSB-ASK	1:1	23.5	21.86	0.020	1.430	1.46	2.086	Figure 8
Bottom Edge	NA	NA	NA	NA	NA	NA	NA	NA	NA	NA
Position Antenna	1/902.75	DSB-ASK	1:1	23.5	21.86	-0.070	0.654	1.46	0.954	Figure 9
	Note: 1.The value with blue color is the maximum SAR Value of each test band. EUT has no voice call function.									

7.4. Simultaneous Transmission Conditions

RFID and WiFi antenna can not transmit simultaneously.

Page 30 of 65

8. Measurement Uncertainty

No.	source	Туре	Uncertaint y Value (%)	Probabilit y Distributio n	k	Ci	Standard Uncertai nty u _i (%)	Degree of freedom V _{eff} or v _i
1	System repetivity	А	0.5	Ν	1	1	0.5	9
		Meas	surement syst	tem				
2	-probe calibration	В	6.0	Ν	1	1	6.0	8
3	-axial isotropy of the probe	В	4.7	R	$\sqrt{3}$	$\sqrt{0.5}$	1.9	×
4	- Hemispherical isotropy of the probe	В	9.4	R	$\sqrt{3}$	$\sqrt{0.5}$	3.9	8
5	-boundary effect	В	1.9	R	$\sqrt{3}$	1	1.1	∞
6	-probe linearity	В	4.7	R	$\sqrt{3}$	1	2.7	∞
7	- System detection limits	В	1.0	R	$\sqrt{3}$	1	0.6	8
8	-readout Electronics	В	1.0	Ν	1	1	1.0	∞
9	-response time	В	0.8	R	$\sqrt{3}$	1	0.5	∞
10	-integration time	В	4.3	R	$\sqrt{3}$	1	2.5	∞
11	-RF Ambient noise	В	3.0	R	$\sqrt{3}$	1	1.7	∞
12	-RF Ambient Conditions	В	3.0	R	$\sqrt{3}$	1	1.7	∞
13	-Probe Positioner Mechanical Tolerance	В	0.4	R	$\sqrt{3}$	1	0.2	8
14	-Probe Positioning with respect to Phantom Shell	В	2.9	R	$\sqrt{3}$	1	1.7	8
15	-Extrapolation, interpolation and Integration Algorithms for Max. SAR Evaluation	В	3.9	R	$\sqrt{3}$	1	2.3	8
Test sample Related								
16	-Test Sample Positioning	А	2.9	Ν	1	1	2.9	71
17	-Device Holder Uncertainty	А	4.1	Ν	1	1	4.1	5
18	- Power drift	В	5.0	R	$\sqrt{3}$	1	2.9	∞
	Physical parameter							

Report No.: RXA1411-0262SAR01R1

Page 31 of 65

19	-phantom Uncertainty	В	4.0	R	$\sqrt{3}$	1	2.3	8
20	Algorithm for correcting SAR for deviations in permittivity and conductivity	В	1.9	N	1	0.84	0.9	8
21	-Liquid conductivity (measurement uncertainty)	В	2.5	Ν	1	0.71	1.8	9
22	-Liquid permittivity (measurement uncertainty)	В	2.5	Ν	1	0.26	0.7	9
23	-Liquid conductivity -temperature uncertainty	В	1.7	R	$\sqrt{3}$	0.71	0.7	8
24	-Liquid permittivity -temperature uncertainty	В	0.3	R	$\sqrt{3}$	0.26	0.05	8
Combined standard uncertainty		<i>u</i> _c =	$\sqrt{\sum_{i=1}^{24} c_i^2 u_i^2}$				11.34	
Expanded uncertainty (confidence interval of 95 %)		L	$u_e = 2u_c$	Ν	k=	=2	22.68	

9. Main Test Instruments

Table 8 [.]	l ist of	Main	Instruments
	LISCO	wan	matiumenta

No.	Name	Туре	Serial Number	Calibration Date	Expiration Time	Valid Period
01	Network analyzer	E5071B	MY42404014	2014-05-26	2015-05-25	1 year
02	Dielectric Probe Kit	Agilent 85070E	US44020115	No Cal	ibration Reques	sted
03	Power meter	Agilent E4417A	GB41291714	2014-03-09	2015-03-08	1 year
04	Power sensor	Agilent N8481H	MY50350004	2014-09-24	2015-09-23	1 year
05	Power sensor	E9327A	US40441622	2015-01-20	2016-01-19	1 year
06	Signal Generator	HP 8341B	2730A00804	2014-09-02	2015-09-01	1 year
07	Dual directional coupler	778D-012	50519	2014-03-24	2015-03-23	1 year
08	Amplifier	IXA-020	0401	No Calibration Requested		sted
09	Wideband radio communication tester	E5515C	MY48360957	2014-12-18	2015-12-17	1 year
10	E-field Probe	EX3DV4	3977	2014-02-17	2015-02-16	1 year
11	DAE	DAE4	1291	2014-11-14	2015-11-13	1 year
12	Validation Kit 835MHz	D835V2	4d020	2014-08-28	2017-08-27	3 years
13	Temperature Probe	JM222	AA1009129	2014-03-13	2015-03-12	1 year
14	Hygrothermograph	WS-1	64591	2014-09-25	2015-09-24	1 year

*****END OF REPORT *****

ANNEX A: Test Layout



Picture 1: Specific Absorption Rate Test Layout



Picture 2: Liquid depth in the flat Phantom (835MHz, 15.4cm depth)

ANNEX B: System Check Results

System Performance Check at 835 MHz Body TSL

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d020

Date: 1/25/2015 Communication System: CW; Frequency: 835 MHz;Duty Cycle: 1:1 Medium parameters used: f = 835 MHz; σ = 0.99 mho/m; ϵ_r = 55.9; ρ = 1000 kg/m³ Ambient Temperature:22.3 °C Liquid Temperature: 21.5 °C Phantom section: Flat Section DASY5 Configuration: Sensor-Surface: 4mm (Mechanical Surface Detection) Probe: EX3DV4 - SN3977; ConvF(9.74, 9.74, 9.74); Calibrated: 2/17/2014; Electronics: DAE4 Sn1291; Calibrated: 11/14/2014 Phantom: ELI 4.0; Type: QDOVA001BA; Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)


d=15mm, Pin=250mW/Area Scan (41x121x1): Measurement grid: dx=1.500 mm, dy=1.500 mm Maximum value of SAR (interpolated) = 2.58 mW/g


d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 51.9 V/m; Power Drift = -0.058 dB

Peak SAR (extrapolated) = 3.5 W/kg

SAR(1 g) = 2.41 mW/g; SAR(10 g) = 1.6 mW/g



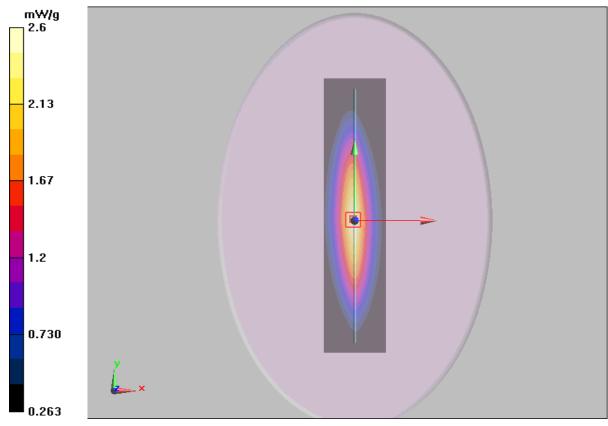

Page 35 of 65

ANNEX C: Highest Graph Results

RFID 900MHz Top Edge Low

Date: 1/25/2015 Communication System: UID 0, Frequency: 902.75 MHz;Duty Cycle: 1:1 Medium parameters used: f = 903 MHz; σ = 1.06 S/m; ϵ_r = 55.059; ρ = 1000 kg/m³ Ambient Temperature:22.3 °C Liquid Temperature: 21.5 °C Phantom section: Flat Section DASY5 Configuration: Sensor-Surface: 4mm (Mechanical Surface Detection) Probe: EX3DV4 - SN3977; ConvF(9.74, 9.74, 9.74); Calibrated: 2/17/2014; Electronics: DAE4 Sn1291; Calibrated: 11/14/2014 Phantom: ELI 4.0; Type: QDOVA001BA; Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Top Edge Low /Area Scan (51x91x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Maximum value of SAR (interpolated) = 2.71 W/kg

Top Edge Low /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 50.06 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 4.18 W/kg

SAR(1 g) = 2.31 W/kg; SAR(10 g) = 1.43 W/kg

Maximum value of SAR (measured) = 2.43 W/kg

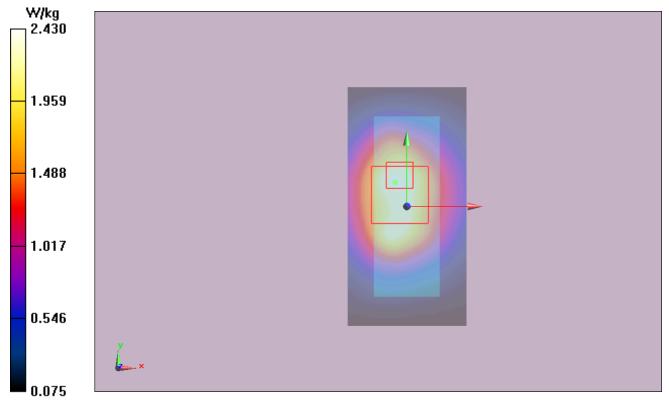


Figure 8 Body, Top Edge, RFID 900M Channel 1

ΓΑ Technology (Shanghai) Co.,	Ltd.
Test Report	

RFID 900MHz Position Antenna Low

Date: 1/25/2015 Communication System: UID 0, Frequency: 902.75 MHz;Duty Cycle: 1:1.21955 Medium parameters used: f = 903 MHz; σ = 1.06 S/m; ε_r = 55.059; ρ = 1000 kg/m³ Ambient Temperature:22.3 °C Liquid Temperature: 21.5 °C Phantom section: Flat Section DASY5 Configuration: Sensor-Surface: 4mm (Mechanical Surface Detection) Probe: EX3DV4 - SN3977; ConvF(9.74, 9.74, 9.74); Calibrated: 2/17/2014; Electronics: DAE4 Sn1291; Calibrated: 11/14/2014 Phantom: ELI 4.0; Type: QDOVA001BA; Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)


Position Antenna Low /Area Scan (51x91x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Maximum value of SAR (interpolated) = 0.969 W/kg


Position Antenna Low /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 0.2970 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 1.19 W/kg

SAR(1 g) = 0.863 W/kg; SAR(10 g) = 0.654 W/kg Maximum value of SAR (measured) = 0.911 W/kg

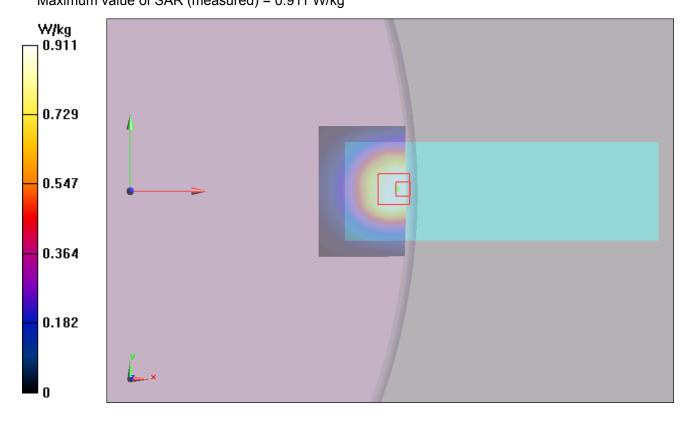



Report No.: RXA1411-0262SAR01R1

ANNEX D: Probe Calibration Certificate

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



9

Schweizerischer Kalibrierdienst S Service suisse d'étalonnage С Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

S

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

ATL (Auden) Client

Certificate No: EX3-3977_Feb14

CALIBRATION CERTIFICATE

Object	EX3DV4 - SN:39	77	AND
Calibration procedure(s)	QA CAL-25.v6	A CAL-12.v9, QA CAL-14.v4, QA dure for dosimetric E-field probes	CAL-23.v5,
Calibration date:	February 17, 201	4	
		onal standards, which realize the physical units robability are given on the following pages and	
		y facility: environment temperature (22 \pm 3)°C é	and humidity < 70%.
Calibration Equipment used (M			
Calibration Equipment used (M&	TE critical for calibration)	y facility: environment temperature (22 ± 3)°C a	And humidity < 70%.
Calibration Equipment used (M& Primary Standards Power meter E4419B	TE critical for calibration)	Cal Date (Certificate No.)	Scheduled Calibration
Calibration Equipment used (Ma Primary Standards Power meter E4419B Power sensor E4412A	TE critical for calibration)	Cal Date (Certificate No.) 04-Apr-13 (No. 217-01733)	Scheduled Calibration Apr-14
Calibration Equipment used (M8 Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator	TE critical for calibration) ID GB41293874 MY41498087	Cal Date (Certificate No.) 04-Apr-13 (No. 217-01733) 04-Apr-13 (No. 217-01733)	Scheduled Calibration Apr-14 Apr-14
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	ID GB41293874 MY41498087 SN: \$5054 (3c)	Cal Date (Certificate No.) 04-Apr-13 (No. 217-01733) 04-Apr-13 (No. 217-01733) 04-Apr-13 (No. 217-01737)	Scheduled Calibration Apr-14 Apr-14 Apr-14
Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator	ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5277 (20x) SN: S5277 (20x)	Cal Date (Certificate No.) 04-Apr-13 (No. 217-01733) 04-Apr-13 (No. 217-01733) 04-Apr-13 (No. 217-01737) 04-Apr-13 (No. 217-01735)	Scheduled Calibration Apr-14 Apr-14 Apr-14 Apr-14
Calibration Equipment used (M8 Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2	ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5277 (20x) SN: S5129 (30b)	Cal Date (Certificate No.) 04-Apr-13 (No. 217-01733) 04-Apr-13 (No. 217-01733) 04-Apr-13 (No. 217-01737) 04-Apr-13 (No. 217-01735) 04-Apr-13 (No. 217-01738)	Scheduled Calibration Apr-14 Apr-14 Apr-14 Apr-14 Apr-14
Calibration Equipment used (M& Primary Standards	ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5277 (20x) SN: S5129 (30b) SN: 3013	Cal Date (Certificate No.) 04-Apr-13 (No. 217-01733) 04-Apr-13 (No. 217-01733) 04-Apr-13 (No. 217-01737) 04-Apr-13 (No. 217-01735) 04-Apr-13 (No. 217-01738) 30-Dec-13 (No. ES3-3013_Dec13)	Scheduled Calibration Apr-14 Apr-14 Apr-14 Apr-14 Apr-14 Apr-14 Dec-14
Calibration Equipment used (Ma Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ID GB41293874 MY41498087 SN: \$5054 (3c) SN: \$5277 (20x) SN: \$5129 (30b) SN: \$5129 (30b) SN: 3013 SN: \$660 SN: \$660	Cal Date (Certificate No.) 04-Apr-13 (No. 217-01733) 04-Apr-13 (No. 217-01733) 04-Apr-13 (No. 217-01737) 04-Apr-13 (No. 217-01735) 04-Apr-13 (No. 217-01738) 30-Dec-13 (No. ES3-3013_Dec13) 13-Dec-13 (No. DAE4-660_Dec13)	Scheduled Calibration Apr-14 Apr-14 Apr-14 Apr-14 Apr-14 Dec-14 Dec-14

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	4F
Approved by:	Katja Pokovic	Technical Manager	Cliff
			Issued: February 19, 2014
This calibration certificate	e shall not be reproduced except in ful	I without written approval of the laboratory	

Certificate No: EX3-3977_Feb14

Report No.: RXA1411-0262SAR01R1

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



GNIS.C

BRP

S

C

S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

Giussaiy.	
TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization ϕ	φ rotation around probe axis
Polarization 9	9 rotation around an axis that is in the plane normal to probe axis (at measurement center),
	i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization ∂ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below *ConvF*).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx, y, z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom
 exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: EX3-3977_Feb14

Report No.: RXA1411-0262SAR01R1

EX3DV4 - SN:3977

February 17, 2014

Page 39 of 65

Probe EX3DV4

SN:3977

Manufactured: November 5, 2013 Calibrated: February 17, 2014

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: EX3-3977_Feb14

Page 3 of 11

5

EX3DV4-SN:3977

February 17, 2014

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3977

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)^A$	0.54	0.57	0.54	± 10.1 %
DCP (mV) ⁸	99.5	100.0	99.7	

Modulation Calibration Parameters

UID	JID Communication System Name		A dB	B dBõV	С	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	133.3	±3.3 %
		Y	0.0	0.0	1.0		134.9	
		Z	0.0	0.0	1.0	1	146.5	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

 ^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).
 ^B Numerical linearization parameter: uncertainty not required.
 ^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field uncertainty is determined using the max. field value.

EX3DV4- SN:3977

February 17, 2014

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3977

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
450	43.5	0.87	11.72	11.72	11.72	0.18	1.10	± 13.3 %
750	41.9	0.89	9.98	9.98	9.98	0.36	0.88	± 12.0 %
835	41.5	0.90	9.62	9.62	9.62	0.61	0.69	± 12.0 %
900	41.5	0.97	9.48	9.48	9.48	0.77	0.63	± 12.0 %
1750	40.1	1.37	8.14	8.14	8.14	0.78	0.60	± 12.0 %
1900	40.0	1.40	7.97	7.97	7.97	0.48	0.75	± 12.0 %
2000	40.0	1.40	7.93	7.93	7.93	0.69	0.63	± 12.0 %
2300	39.5	1.67	7.59	7.59	7.59	0.37	0.83	± 12.0 %
2450	39.2	1.80	7.24	7.24	7.24	0.27	1.10	± 12.0 %
2600	39.0	1.96	7.07	7.07	7.07	0.41	0.84	± 12.0 %
5200	36.0	4.66	5.09	5.09	5.09	0.35	1.80	± 13.1 %
5300	35.9	4.76	4.82	4.82	4.82	0.35	1.80	± 13.1 %
5500	35.6	4.96	4.76	4.76	4.76	0.35	1.80	± 13.1 %
5600	35.5	5.07	4.55	4.55	4.55	0.40	1.80	± 13.1 %
5800	35.3	5.27	4.52	4.52	4.52	0.40	1.80	± 13.1 %

Calibration Parameter Determined in Head Tissue Simulating Media

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.
 ^F At frequencies below 3 GHz, the validity of tissue parameters (and o) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (and o) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.
 ^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX3-3977_Feb14

Page 5 of 11

EX3DV4-SN:3977

ş

February 17, 2014

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3977

f (MHz) ^c	Relative Permittivity ^F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
450	56.7	0.94	12.47	12.47	12.47	0.11	1.10	± 13.3 %
750	55.5	0.96	9.78	9.78	9.78	0.45	0.86	± 12.0 %
835	55.2	0.97	9.74	9.74	9.74	0.48	0.83	± 12.0 %
900	55.0	1.05	9.46	9.46	9.46	0.41	0.89	± 12.0 %
1750	53.4	1.49	7.69	7.69	7.69	0.41	0.88	± 12.0 %
1900	53.3	1.52	7.37	7.37	7.37	0.34	0.89	± 12.0 %
2000	53.3	1.52	7.41	7.41	7.41	0.24	1.14	± 12.0 %
2300	52.9	1.81	7.12	7.12	7.12	0.66	0.64	± 12.0 %
2450	52.7	1.95	6.97	6.97	6.97	0.80	0.50	± 12.0 %
2600	52.5	2.16	6.68	6.68	6.68	0.80	0.50	± 12.0 %
5200	49.0	5.30	4.50	4.50	4.50	0.45	1.90	± 13.1 %
5300	48.9	5.42	4.28	4.28	4.28	0.45	1.90	± 13.1 %
5500	48.6	5.65	4.02	4.02	4.02	0.45	1.90	± 13.1 %
5600	48.5	5.77	3.87	3.87	3.87	0.45	1.90	± 13.1 %
5800	48.2	6.00	4.12	4.12	4.12	0.50	1.90	± 13.1 %

Calibration Parameter Determined in Body Tissue Simulating Media

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.
^F At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.
(ε and σ) is restricted to ± 5%. The uncertainty is the RSS of a Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


Certificate No: EX3-3977_Feb14

Page 6 of 11

EX3DV4-SN:3977

February 17, 2014


Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

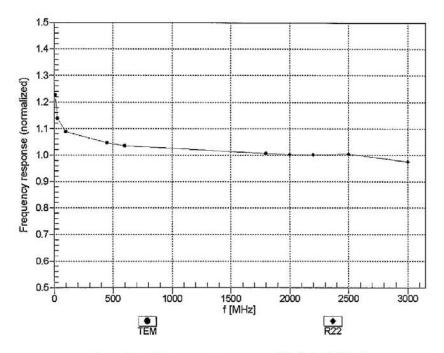

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Page 7 of 11

February 17, 2014

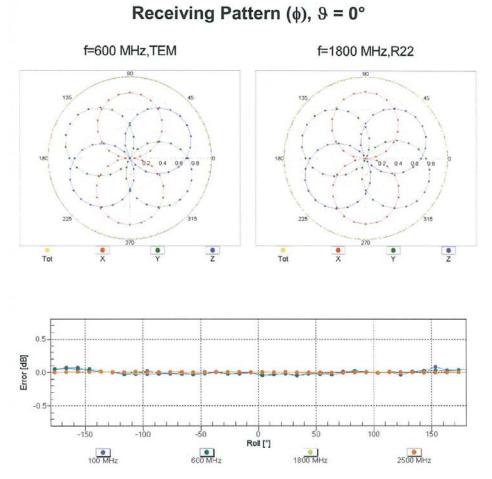


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: EX3-3977_Feb14

EX3DV4-SN:3977

February 17, 2014

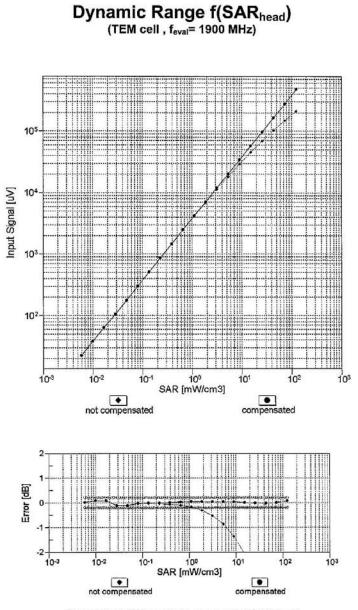

Uncertainty of Linearity Assessment: ± 0.6% (k=2)


Certificate No: EX3-3977_Feb14

Page 9 of 11

Report No.: RXA1411-0262SAR01R1

EX3DV4- SN:3977

February 17, 2014

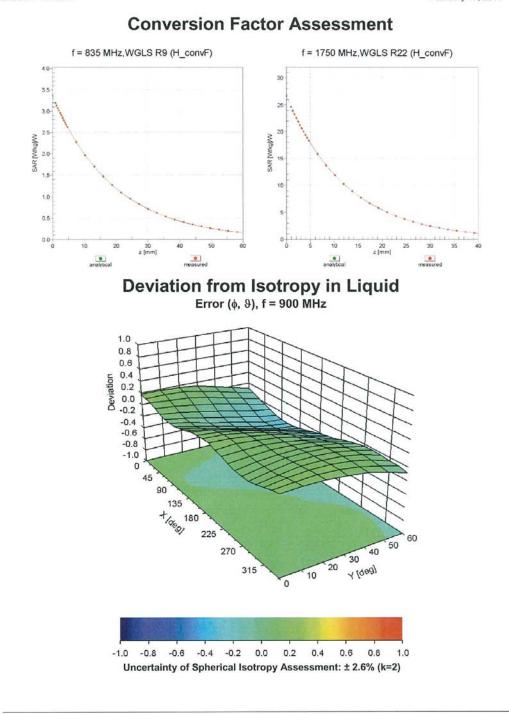

Certificate No: EX3-3977_Feb14

Page 10 of 11

EX3DV4-SN:3977

February 17, 2014

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3977

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	23.6
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm

۰.

ANNEX E: D835V2 Dipole Calibration Certificate

E-mail: cttl@chinattl.com Client TA(Shang	,	4441.941	
	ghai)	Certificate No: Z14-97073	
CALIBRATION C	ERTIFICATE		
Object	D835V2 -	SN: 4d020	
Calibration Procedure(s)	710 00		
	TMC-OS-	E-02-194 n procedure for dipole validation kits	
	Calibration		
Calibration date:	August 28	, 2014	
given on the following pag All calibrations have beer and humidity<70%.	es and are part of the	losed laboratory facility: environment tempera	
given on the following pag All calibrations have beer and humidity<70%. Calibration Equipment use	es and are part of the n conducted in the c ed (M&TE critical for o	e certificate. losed laboratory facility: environment tempera	ature(22±3)
given on the following pag All calibrations have beer and humidity<70%. Calibration Equipment use	es and are part of the n conducted in the c ed (M&TE critical for o	e certificate. losed laboratory facility: environment tempera calibration) e(Calibrated by, Certificate No.) Scheduled 11-Sep-13 (TMC, No.JZ13-443)	d Calibratio Sep-14
given on the following pag All calibrations have beer and humidity<70%. Calibration Equipment use Primary Standards	es and are part of the c n conducted in the c ed (M&TE critical for o ID # Cal Date	e certificate. losed laboratory facility: environment tempera calibration) c(Calibrated by, Certificate No.) Scheduled 11-Sep-13 (TMC, No.JZ13-443) 11-Sep-13 (TMC, No. JZ13-443)	d Calibratio Sep-14 Sep -14
given on the following pag All calibrations have been and humidity<70%. Calibration Equipment use Primary Standards Power Meter NRVD Power sensor NRV-Z5 Reference Probe ES3DV	es and are part of the n conducted in the c ed (M&TE critical for o ID # Cal Date 102083 100595 /3 SN 3149	e certificate. losed laboratory facility: environment tempera calibration) c(Calibrated by, Certificate No.) Scheduled 11-Sep-13 (TMC, No.JZ13-443) 11-Sep-13 (TMC, No. JZ13-443) 5- Sep-13 (SPEAG, No.ES3-3149_Sep13)	d Calibratio Sep-14 Sep -14 Sep -14
given on the following pag All calibrations have been and humidity<70%. Calibration Equipment use Primary Standards Power Meter NRVD Power sensor NRV-Z5 Reference Probe ES3DV DAE3	es and are part of the n conducted in the c ed (M&TE critical for o ID # Cal Date 102083 100595 /3 SN 3149 SN 536	e certificate. losed laboratory facility: environment tempera calibration) c(Calibrated by, Certificate No.) Scheduled 11-Sep-13 (TMC, No.JZ13-443) 11-Sep-13 (TMC, No. JZ13-443) 5- Sep-13 (SPEAG, No.ES3-3149_Sep13) 23-Jan-14 (SPEAG, DAE3-536_Jan14)	d Calibratio Sep-14 Sep-14 Sep-14 Jan -15
given on the following pag All calibrations have been and humidity<70%. Calibration Equipment use Primary Standards Power Meter NRVD Power sensor NRV-Z5 Reference Probe ES3DV DAE3 Signal Generator E443	es and are part of the n conducted in the c ed (M&TE critical for o ID # Cal Date 102083 100595 /3 SN 3149 SN 536 8C MY49070393	e certificate. losed laboratory facility: environment tempera calibration) c(Calibrated by, Certificate No.) Scheduled 11-Sep-13 (TMC, No.JZ13-443) 11-Sep-13 (TMC, No.JZ13-443) 5- Sep-13 (SPEAG, No.ES3-3149_Sep13) 23-Jan-14 (SPEAG, DAE3-536_Jan14) 13-Nov-13 (TMC, No.JZ13-394)	d Calibratio Sep-14 Sep-14 Sep-14 Jan -15 Nov-14
given on the following pag All calibrations have been and humidity<70%. Calibration Equipment use Primary Standards Power Meter NRVD Power sensor NRV-Z5 Reference Probe ES3DV DAE3	es and are part of the n conducted in the c ed (M&TE critical for o ID # Cal Date 102083 100595 /3 SN 3149 SN 536 8C MY49070393	e certificate. losed laboratory facility: environment tempera calibration) c(Calibrated by, Certificate No.) Scheduled 11-Sep-13 (TMC, No.JZ13-443) 11-Sep-13 (TMC, No. JZ13-443) 5- Sep-13 (SPEAG, No.ES3-3149_Sep13) 23-Jan-14 (SPEAG, DAE3-536_Jan14)	d Calibratio Sep-14 Sep-14 Sep-14 Jan -15
given on the following pag All calibrations have been and humidity<70%. Calibration Equipment use Primary Standards Power Meter NRVD Power sensor NRV-Z5 Reference Probe ES3DV DAE3 Signal Generator E4433 Network Analyzer E8362	es and are part of the n conducted in the c ed (M&TE critical for o ID # Cal Date 102083 100595 /3 SN 3149 SN 536 8C MY49070393	e certificate. losed laboratory facility: environment tempera calibration) c(Calibrated by, Certificate No.) Scheduled 11-Sep-13 (TMC, No.JZ13-443) 11-Sep-13 (TMC, No.JZ13-443) 5- Sep-13 (SPEAG, No.ES3-3149_Sep13) 23-Jan-14 (SPEAG, DAE3-536_Jan14) 13-Nov-13 (TMC, No.JZ13-394) 19-Oct-13 (TMC, No.JZ13-278)	d Calibratio Sep-14 Sep-14 Sep-14 Jan -15 Nov-14
given on the following pag All calibrations have been and humidity<70%. Calibration Equipment use Primary Standards Power Meter NRVD Power sensor NRV-Z5 Reference Probe ES3DV DAE3 Signal Generator E4433 Network Analyzer E8362	es and are part of the n conducted in the c ed (M&TE critical for of ID # Cal Date 100595 /3 SN 3149 SN 536 8C MY49070393 B MY43021135	e certificate. losed laboratory facility: environment tempera calibration) c(Calibrated by, Certificate No.) Scheduled 11-Sep-13 (TMC, No.JZ13-443) 11-Sep-13 (TMC, No.JZ13-443) 5- Sep-13 (SPEAG, No.ES3-3149_Sep13) 23-Jan-14 (SPEAG, DAE3-536_Jan14) 13-Nov-13 (TMC, No.JZ13-394) 19-Oct-13 (TMC, No.JZ13-278)	d Calibratio Sep-14 Sep -14 Sep -14 Jan -15 Nov-14 Oct-14
given on the following pag All calibrations have been and humidity<70%. Calibration Equipment use Primary Standards Power Meter NRVD Power sensor NRV-Z5 Reference Probe ES3DV DAE3 Signal Generator E443	es and are part of the n conducted in the c ed (M&TE critical for o ID # Cal Date 102083 100595 73 SN 3149 SN 536 8C MY49070393 B MY43021135	e certificate. losed laboratory facility: environment tempera calibration) c(Calibrated by, Certificate No.) Scheduled 11-Sep-13 (TMC, No.JZ13-443) 11-Sep-13 (TMC, No.JZ13-443) 5- Sep-13 (SPEAG, No.ES3-3149_Sep13) 23-Jan-14 (SPEAG, DAE3-536_Jan14) 13-Nov-13 (TMC, No.JZ13-394) 19-Oct-13 (TMC, No.JZ13-278) Function S	d Calibratio Sep-14 Sep -14 Sep -14 Jan -15 Nov-14 Oct-14

Certificate No: Z14-97073

Report No.: RXA1411-0262SAR01R1



CNAS CALIBRATION No. L0570

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com Http://www.chinattl.cn

Glossary:

TSL ConvF N/A tissue simulating liquid sensitivity in TSL / NORMx,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms
 oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z14-97073

Page 2 of 8

Report No.: RXA1411-0262SAR01R1

In Collaborat S D CALIBRATIO	ea	a g	-	lac	CNAS
	ct, Beijing, 6-10-62304 ww.chinatt	633-2504		"Inha	CALIBRATIO No. L0570
Measurement Conditions DASY system configuration, as far as not	aiven on r	1 and			
DASY Version	2.01 2)ASY52		52	2.8.8.1222
Extrapolation	Advance	d Extrapolation			
Phantom	Triple Fla	at Phantom 5.1C	7.) (. 7		
Distance Dipole Center - TSL	15 mm			with	ı Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm				
Frequency	835 N	1Hz±1 MHz			
Head TSL parameters		ar:: 10			
The following parameters and calculations		niea. Temperature	Permitti	vity	Conductivity
Nominal Head TSL parameters		22.0 °C	41.5	-	- 0.90 mho/m
Measured Head TSL parameters	0	22.0±0.2) °C	42.5 ±	:6 %	0.91 mho/m ±6 %
Head TSL temperature change during	y test	<1.0 °C	1.000		1
SAR result with Head TSL		SUCCESSO			ê de la companya de la
SAR averaged over 1 cm^3 (1g) of Hea	ad TSL	Condit	ion		
SAR measured		250 mW in	put power	2.39 mW/g	
SAR for nominal Head TSL parameters	9	normalized to 1W		9.54 mW/g ± 20.8 % (
SAR averaged over 10 cm^3 (10 g) of H	lead TSL	Condit	ion		
SAR measured		250 mW in	put power	1.57 mW/g	
SAR for nominal Head TSL parameters		normalized to 1W 6		6.26 r	mW/g ± 20.4 % (k=2)
Body TSL parameters The following parameters and calculations	: were anr	lied		anor	
	(7) (300)	Temperature	Permitti	vity	Conductivity
Nominal Body TSL parameters		22.0 °C	55.2		0.97 mho/m
Measured Body TSL parameters	(22.0±0.2) ℃	56.7 ±0	3 %	0.97 mho/m±6 %
Body TSL temperature change during	gtest	<1.0 °C			
SAR result with Body TSL					
SAR averaged over 1 cm ³ (1g) of Boo	dy TSL	Condit	ion		
SAR measured		250 mW in	put power		2.37 mW/g
SAR for nominal Body TSL parameters	}	normalize	d to 1W	9.54 1	nW/g ± 20.8 % (k=2)
SAR averaged over 10 cm^3 (10 g) of E	Body TSL	Condit	ion		
SAR measured		250 mW in	put power		1.57 mW/g
SAR for nominal Body TSL parameters		normalized to 1W 6.31 mW/g ± 20.4 % (k			mW/g±20.4 % (k=2)

Certificate No: Z14-97073

Page 3 of 8



Http://www.chinattl.cn



Appendix

Antenna Parameters with Head TSL

E-mail: cttl@chinattl.com

Impedance, transformed to feed point	48.6Ω + 2.75jΩ
Return Loss	- 30.1dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	54.0Ω +5.88jΩ
Return Loss	- 23.3dB

General Antenna Parameters and Design

42 ns
1.2-

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.


The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.


No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Report No.: RXA1411-0262SAR01R1

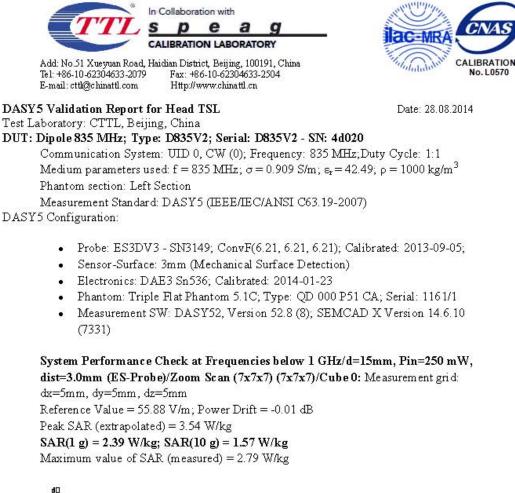


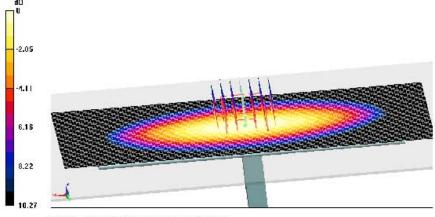

0 dB = 2.79 W/kg = 4.46 dBW/kg

Certificate No: Z14-97073


Report No.: RXA1411-0262SAR01R1







Impedance Measurement Plot for Head TSL

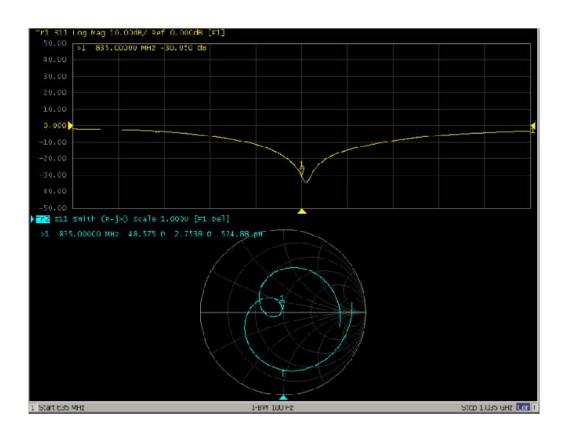

Certificate No: Z14-97073


Page 6 of 8

Report No.: RXA1411-0262SAR01R1



- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/2
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

System Performance Check at Frequencies below 1 GHz/d=15mm, Pin=250 mW, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 53.515 V/m; Power Drift = -0.01 dB Peak SAR (extrapolated) = 3.45 W/kg SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.57 W/kg Maximum value of SAR (measured) = 2.74 W/kg

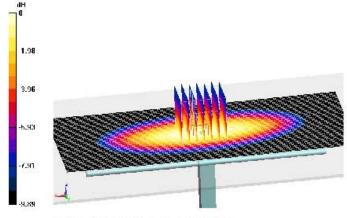

0 dB = 2.74 W/kg = 4.38 dBW/kg

Certificate No: Z14-97073


Page 7 of 8

Report No.: RXA1411-0262SAR01R1



Impedance Measurement Plot for Body TSL



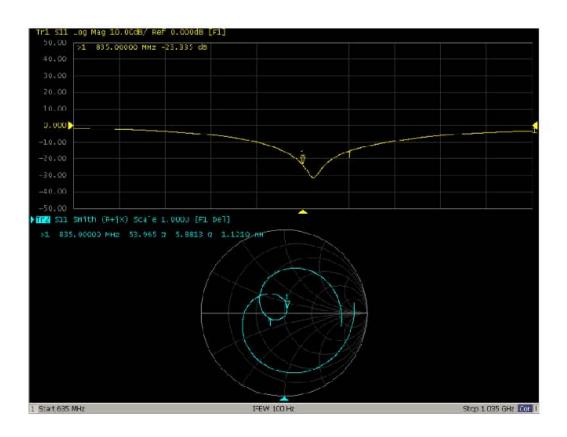

Certificate No: Z14-97073

Page 8 of 8

Report No.: RXA1411-0262SAR01R1

ANNEX F: DAE4 Calibration Certificate

Calibration Laboratory Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich		ACCMEA C. V. C. V.	 S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service 	
Accredited by the Swiss Accreditation Service (SAS) Accreditation No.: SCS 108 The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates				
Client TA-Shanghai (Auden) Certificate No: DAE4-1291_Nov14				
CALIBRATION C	ERTIFICATE			
Object	DAE4 - SD 000 D	04 BM - SN: 1291	· · · · · · ·	
Calibration procedure(s)	QA CAL-06.v28 Calibration proces	dure for the data acquisition ele	ectronics (DAE)	
Calibration date:	November 14, 20	14		
The measurements and the uncer	tainties with confidence pr	onal standards, which realize the physical obability are given on the following pages y facility: environment temperature (22 ± 3	and are part of the certificate.	
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	
Keithley Multimeter Type 2001	SN: 0810278	03-Oct-14 (No:15573)	Oct-15	
Secondary Standards Auto DAE Calibration Unit Calibrator Box V2.1		Check Date (in house) 07-Jan-14 (in house check) 07-Jan-14 (in house check)	Scheduled Check In house check: Jan-15 In house check: Jan-15	
Calibrated by:	Name Dominique Steffen	Function Technician	Signature	
Approved by:	Fin Bomholt	Deputy Technical Manager	1. V. Bellun	
This calibration certificate shall not	be reproduced except in f	ull without written approval of the laborato	Issued: November 14, 2014 bry.	

Certificate No: DAE4-1291_Nov14

Report No.: RXA1411-0262SAR01R1

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)



SWISS CZ RIGRAT S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Glossary

DAE Connector angle

data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement. Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - Power consumption: Typical value for information. Supply currents in various operating modes.

Report No.: RXA1411-0262SAR01R1

DC Voltage Measurement A/D - Converter Resolution non

A/D - Converter Reso	olution nominal				
High Range:	1LSB =	6.1µV,	full range =	-100+300 mV	
Low Range:	1LSB =	61nV .		-1+3mV	
DASY measurement	parameters: Aut	o Zero Time: 3	sec; Measuring	time: 3 sec	

Calibration Factors	X	Y	Z
High Range	402.613 ± 0.02% (k=2)	403.293 ± 0.02% (k=2)	403.205 ± 0.02% (k=2)
Low Range	3.97544 ± 1.50% (k=2)	3.93356 ± 1.50% (k=2)	3.99377 ± 1.50% (k=2)

Connector Angle

Connector Angle to be used in DASY system	308.5 ° ± 1 °

Appendix (Additional assessments outside the scope of SCS108)

1. DC Voltage Linearity

High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	200033.82	-3.10	-0.00
Channel X + Input	20004.15	-0.02	-0.00
Channel X - Input	-20004.31	1.85	-0.01
Channel Y + Input	200033.24	-3.41	-0.00
Channel Y + Input	20003.47	-0.54	-0.00
Channel Y - Input	-20006.08	0.19	-0.00
Channel Z + Input	200036.05	-0.73	-0.00
Channel Z + Input	20001.26	-2.68	-0.01
Channel Z - Input	-20007.69	-1.47	0.01

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	2000.57	-0.08	-0.00
Channel X + Input	200.57	-0.14	-0.07
Channel X - Input	-199.31	-0.00	0.00
Channel Y + Input	1999.81	-0.79	-0.04
Channel Y + Input	200.05	-0.62	-0.31
Channel Y - Input	-199.06	0.30	-0.15
Channel Z + Input	2001.14	0.56	0.03
Channel Z + Input	199.16	-1.42	-0.71
Channel Z - Input	-200.73	-1.23	0.62

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	9.64	7.77
	- 200	-6.77	-8.44
Channel Y	200	13.71	13.30
	- 200	-14.01	-14.19
Channel Z	200	-16.88	-16.56
	- 200	13.70	13.86

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (µV)	Channel Z (µV)
Channel X	200	-	3.91	-4.26
Channel Y	200	8.88	-	3.64
Channel Z	200	10.51	7.45	-

Certificate No: DAE4-1291_Nov14

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Rang e (LSB)	Low Range (LSB)
Channel X	16003	13374
Channel Y	15805	15470
Channel Z	16035	14317

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input 10M Ω

	Average (μV)	Average (μV) min. Offset (μV) max. O		Std. Deviation (µV)	
Channel X	0.37	-1.17	1.61	0.49	
Channel Y	0.25	-0.91	1.56	0.48	
Channel Z	-0.62	-1.83	0.60	0.47	

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)	
Channel X	200	200	
Channel Y	200	200	
Channel Z	200	200	

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)	
Supply (+ Vcc)	+0.01	+6	+14	
Supply (- Vcc)	-0.01	-8	-9	

ANNEX G: The EUT Appearances and Test Configuration






a: EUT

Picture 3: Constituents of EUT

Report No.: RXA1411-0262SAR01R1

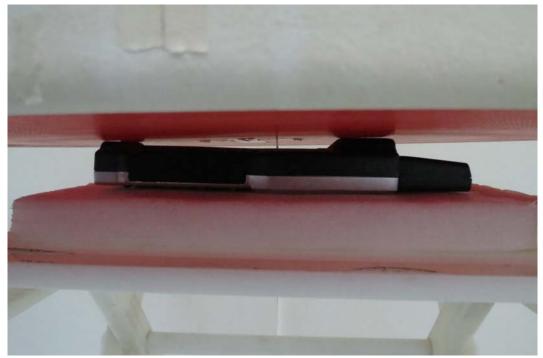

Picture 4: Back Side, the distance from EUT to the bottom of the Phantom is 0mm



Picture 5: Left Edge, the distance from EUT to the bottom of the Phantom is 0mm

Report No.: RXA1411-0262SAR01R1



Picture 6: Right Edge, the distance from EUT to the bottom of the Phantom is 0mm



Picture 7: Top Edge, the distance from EUT to the bottom of the Phantom is 0mm

Report No.: RXA1411-0262SAR01R1



Picture 8: Back Side, the distance from EUT antenna to the bottom of the Phantom is 0mm

ANNEX K: System Validation

The SAR system must be validated against its performance specifications before it is deployed. When SAR probes, system components or software are changed, upgraded or recalibrated, these must be validated with the SAR system(s) that operates with such components.

Table 9	: System	Validation	Part 1
---------	----------	------------	--------

System	Probe	Liquid	Validation	Frequency	Permittivity	Conductivity
No.	SN.	Name	Date	Point	٤	σ(s/m)
1	3977	835MHz (body)	February 17, 2014	835MHz	55.2	0.97

Table 10: System Validation Part 2

	Sensitivity	PASS	PASS
	Probe Linearity	PASS	PASS
cw	Probe Isotropy	PASS	PASS
Validation	MOD. Type	OFDM	OFDM
	Duty Factor	PASS	PASS
	PAR	PASS	PASS