




EMC TEST REPORT FCC 47 CFR Part 15B Industry Canada RSS-Gen Electromagnetic compatibility - Unintentional radiators	
Report Reference No.	G0M-1305-2859-EF01-V01
Testing Laboratory	Eurofins Product Service GmbH
Address	Storkower Str. 38c 15526 Reichenwalde Germany
Accreditation	<div style="text-align: center;">   </div> <p style="text-align: center;"> A2LA Accredited Testing Laboratory, Certificate No.: 1983.01 FCC Filed Test Laboratory, Reg.-No.: 96970 IC OATS Filing assigned code: 3470A </p>
Applicant's name	Bang & Olufsen Medicom A/S
Address	Gimsinglundvej 20 7600 Struer DENMARK
Test specification:	
Standard.....	47 CFR Part 15 Subpart B RSS-Gen, Issue 3, 2010-12 ANSI C63.4:2009
Equipment under test (EUT):	
Product description	Electronic Auto-injector
Model No.	betaCONNECT
Additional Models	None
Hardware version	B11
Firmware / Software version	None
	FCC-ID: 2AAGY-BETAC1 IC: 3775E-BETAC1
Test result	Passed

Possible test case verdicts:

- not applicable to test object: N/A
- test object does meet the requirement.....: P (Pass)
- test object does not meet the requirement.....: F (Fail)

Testing:

Date of receipt of test item: 2013-07-01
 Date (s) of performance of tests: 2013-07-03
 Compiled by : Antje Bartusch
 Tested by (+ signature)..... : Matthias Handrik
 Approved by (+ signature) : Jens Zimmermann
 Date of issue : 2013-08-30
 Total number of pages : 21

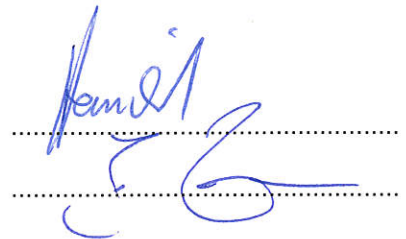
General remarks:

**The test results presented in this report relate only to the object tested.
 The results contained in this report reflect the results for this particular model and serial number. It is the responsibility of the manufacturer to ensure that all production models meet the intent of the requirements detailed within this report.**

This report shall not be reproduced, except in full, without the written approval of the Issuing testing laboratory.

Additional comments:

REPORT INDEX

1	EQUIPMENT (TEST ITEM) DESCRIPTION	4
1.1	Photos – Equipment external	5
1.1	Photos – Equipment internal	6
1.2	Photos – Test setup	8
1.3	Supporting Equipment Used During Testing	9
1.4	Operating Modes	10
1.5	Test Equipment Used During Testing	11
1.6	Sample emission level calculation	12
2	RESULT SUMMARY	13
3	TEST CONDITIONS AND RESULTS	14
3.1	Test Conditions and Results – Radiated emissions	14
3.2	Test Conditions and Results – AC power line conducted emissions	19

1 Equipment (Test item) Description

Description	Electronic Auto-injector	
Model	betaCONNECT	
Additional Models	None	
Serial number	None	
Hardware version	B11	
Software / Firmware version	None	
FCC-ID	2AAGY-BETAC1	
IC	3775E-BETAC1	
Power supply	120V AC/DC Adapter	
AC/DC-Adaptor	Model	ASUC30e-050100
	Vendor	Aquilstar Precision Industrial
	Input	100-240VAC, 50-60Hz
	Output	5.0V
Manufacturer	Bang & Olufsen Medicom A/S Gimsinglundvej 20 7600 Struer DENMARK	
Highest emission frequency	0.4 MHz	
Device classification	Class B	
Equipment type	Tabletop	
Number of tested samples	1	

1.3 Supporting Equipment Used During Testing

Product Type*	Device	Manufacturer	Model No.	Comments
None				
<p>*Note: Use the following abbreviations:</p> <p style="margin-left: 40px;">AE : Auxiliary/Associated Equipment, or</p> <p style="margin-left: 40px;">SIM : Simulator (Not Subjected to Test)</p> <p style="margin-left: 40px;">CABL : Connecting cables</p>				

1.4 Operating Modes

Mode #	Description
1	active; motor with load; charging, Bluetooth link

1.5 Test Equipment Used During Testing

Radiated emissions					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Biconical Antenna	R&S	HK 116	EF00012	2013-02	2016-02
LPD-Antenne	R&S	HL 223	EF00187	2011-02	2014-02
LPD-Antenna	R&S	HL 025	EF00327	2013-02	2016-02
EMI Test Receiver	R&S	ESU8	EF00379	2013-03	2014-03
EMI Test Receiver	R&S	ESCS 30	EF00297	2012-09	2013-09

Conducted emissions					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
AMN	R&S	ESH2-Z5	EF00182	2012-10	2014-10
AMN	R&S	ESH3-Z5	EF00036	2012-11	2014-11
EMI Test Receiver	R&S	ESCS 30	EF00297	2012-09	2013-09

1.6 Sample emission level calculation

The following is a description of terms and a sample calculation, as appears in the radiated emissions data table. The numbers used in the calculation are for example only. There is no direct correlation to the specific data taken for the product described in this document:

Reading:

This is the reading obtained on the spectrum analyzer in dB μ V. Any external preamplifiers used are taken into account through internal analyzer settings.

A.F.:

This is the antenna factor for the receiving antenna. It is a conversion factor, which converts electric fields strengths to voltages, which can be measured directly on the spectrum analyzer. It is treated as a loss in dB. Cable losses have been included with the A.F. to simplify the calculations. The antenna factor is used in calculations as follows:

$$\text{Reading on Analyzer (dB}\mu\text{V)} + \text{A.F. (dB)} = \text{Net field strength (dB}\mu\text{V/m)}$$

Net:

This is the net field strength measurement (as shown above).

Limit:

This is the FCC Class B radiated emission limit (in units of dB μ V/m). The FCC limits are given in units of μ V/m. The following formula is used to convert the units of μ V/m to dB μ V/m:

$$\text{Limit (dB}\mu\text{V/m)} = 20 * \log (\mu\text{V/m})$$

Margin:

This is the margin of compliance below the FCC limit. The units are given in dB. A negative margin indicates the emission was below the limit. A positive margin indicates that the emission exceeds the limit.

Example only:

$$\begin{array}{rclclcl} \text{Reading} & + & \text{AF} & = & \text{Net Reading} & : & \text{Net reading - FCC limit} & = & \text{Margin} \\ 21.5 \text{ dB}\mu\text{V} & + & 26 \text{ dB} & = & 47.5 \text{ dB}\mu\text{V/m} & : & 47.5 \text{ dB}\mu\text{V/m} - 57.0 \text{ dB}\mu\text{V/m} & = & -9.5 \text{ dB} \end{array}$$

2 Result Summary

FCC 47 CFR Part 15B, Industry Canada RSS-Gen				
Product Specific Standard	Requirement – Test	Reference Method	Result	Remarks
47 CFR 15.109 RSS-Gen 4.9 & 4.10	Radiated emissions	ANSI C 63.4	PASS	
47 CFR 15.107 RSS-Gen 7.2.4	AC power line conducted emissions	ANSI C63.4	PASS	
Remarks:				

3 Test Conditions and Results

3.1 Test Conditions and Results – Radiated emissions


Radiated emissions acc. FCC 47 CFR 15.109 / IC RSS-Gen		Verdict: PASS				
Laboratory Parameters:	Required prior to the test	During the test				
Ambient Temperature	15 to 35 °C	24°C				
Relative Humidity	30 to 60 %	53%				
Test according referenced standards	Reference Method					
	ANSI C63.4					
Sample is tested with respect to the requirements of the equipment class	Equipment class					
	Class B					
Test frequency range determined from highest emission frequency	Highest emission frequency					
	0.4 MHz					
Fully configured sample scanned over the following frequency range	Frequency range					
	30 MHz to 1 GHz					
Operating mode	1					
Limits and results Class B						
Frequency [MHz]	Quasi-Peak [dB μ V/m]	Result	Average [dB μ V/m]	Result	Peak [dB μ V/m]	Result
30 – 88	40	PASS	-		-	-
88 – 216	43.5	PASS	-		-	-
216 – 960	46	PASS	-		-	-
960 – 1000	54	PASS	-		-	-
Comments:						

Spurious emissions under normal conditions according to FCC 15B

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Handrik
 Test Conditions: Tnom: 22°C, Unom: 120V AC (AC/DC adaptor: ASUC30e-050100)
 Antenna: Rohde & Schwarz HK 116, Vertical
 Measurement distance: 3m
 Mode: active; motor with load; charging, Bluetooth link
 Test Date: 2013-07-03
 Note:

Index 10

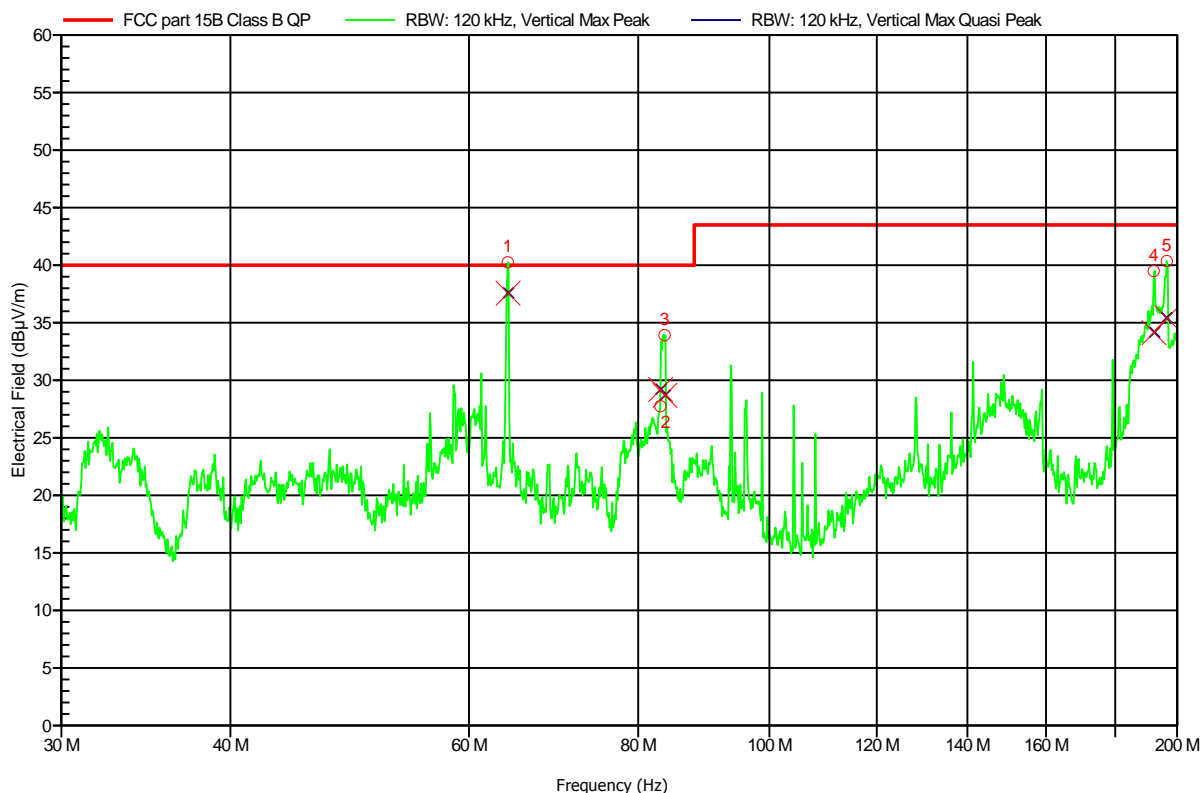

Nr	Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status
1	64.092 MHz	37.59 dBµV/m	40 dBµV/m	-2.41 dB	Pass
2	83.076 MHz	29.22 dBµV/m	40 dBµV/m	-10.78 dB	Pass
3	83.67 MHz	28.72 dBµV/m	40 dBµV/m	-11.28 dB	Pass
4	192.156 MHz	34.17 dBµV/m	43.5 dBµV/m	-9.33 dB	Pass
5	196.47 MHz	35.43 dBµV/m	43.5 dBµV/m	-8.07 dB	Pass

Test Report No.: G0M-1305-2859-EF01-V01


 Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Spurious emissions under normal conditions according to FCC 15B

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Handrik
 Test Conditions: Tnom: 22°C, Unom: 120V AC (AC/DC adaptor: ASUC30e-050100)
 Antenna: Rohde & Schwarz HK 116, Horizontal
 Measurement distance: 3m
 Mode: active; motor with load; charging, Bluetooth link
 Test Date: 2013-07-03
 Note:

Index 9

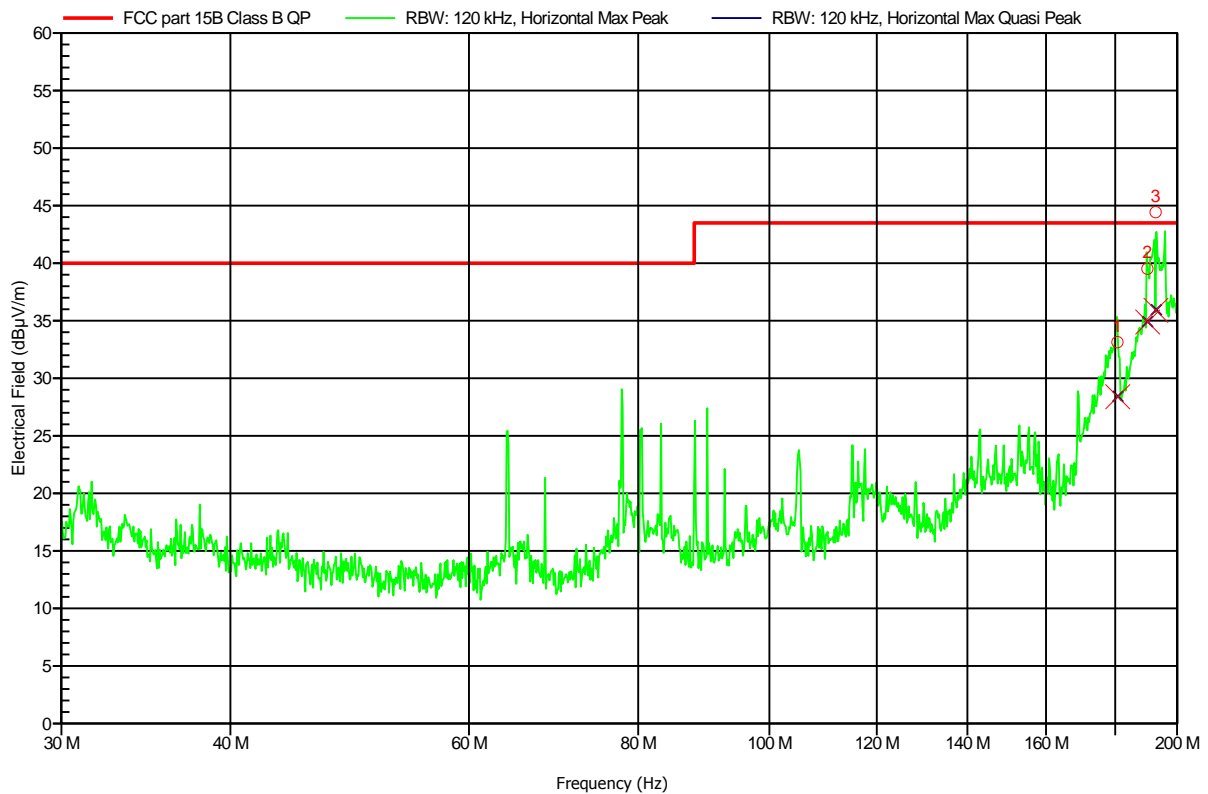


Nr	Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status
1	180.654 MHz	28.42 dBµV/m	43.5 dBµV/m	-15.08 dB	Pass
2	190.092 MHz	34.91 dBµV/m	43.5 dBµV/m	-8.59 dB	Pass
3	192.78 MHz	35.94 dBµV/m	43.5 dBµV/m	-7.56 dB	Pass

Spurious emissions under normal conditions according to FCC 15B

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Handrik
 Test Conditions: Tnom: 22°C, Unom: 120V AC (AC/DC adaptor: ASUC30e-050100)
 Antenna: Rohde & Schwarz HL 223, Vertical
 Measurement distance: 3m
 Mode: active; motor with load; charging, Bluetooth link
 Test Date: 2013-07-03
 Note:

Index 11

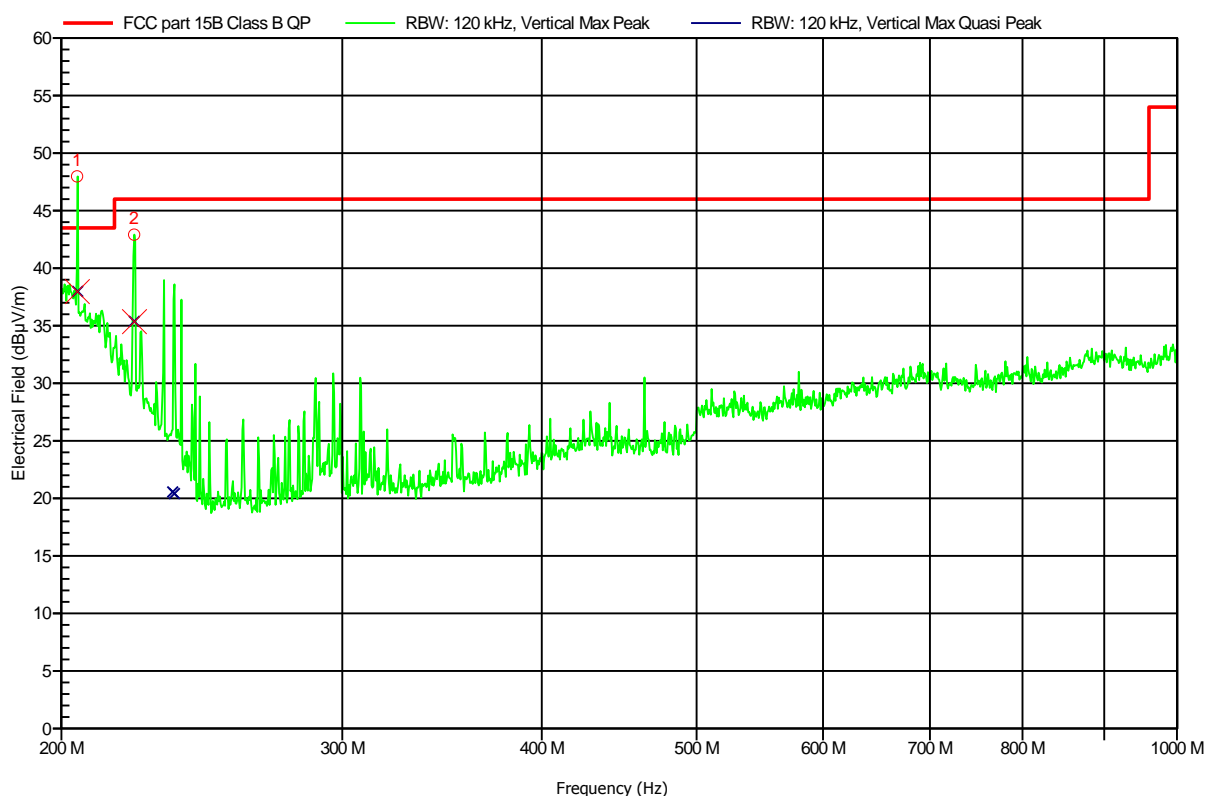


Nr	Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status
1	204.662 MHz	37.99 dBµV/m	43.5 dBµV/m	-5.51 dB	Pass
2	222.206 MHz	35.38 dBµV/m	46 dBµV/m	-10.62 dB	Pass

Spurious emissions under normal conditions according to FCC 15B

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Handrik
 Test Conditions: Tnom: 22°C, Unom: 120V AC (AC/DC adaptor: ASUC30e-050100)
 Antenna: Rohde & Schwarz HL 223, Horizontal
 Measurement distance: 3m
 Mode: active; motor with load; charging, Bluetooth link
 Test Date: 2013-07-03
 Note:

Index 12

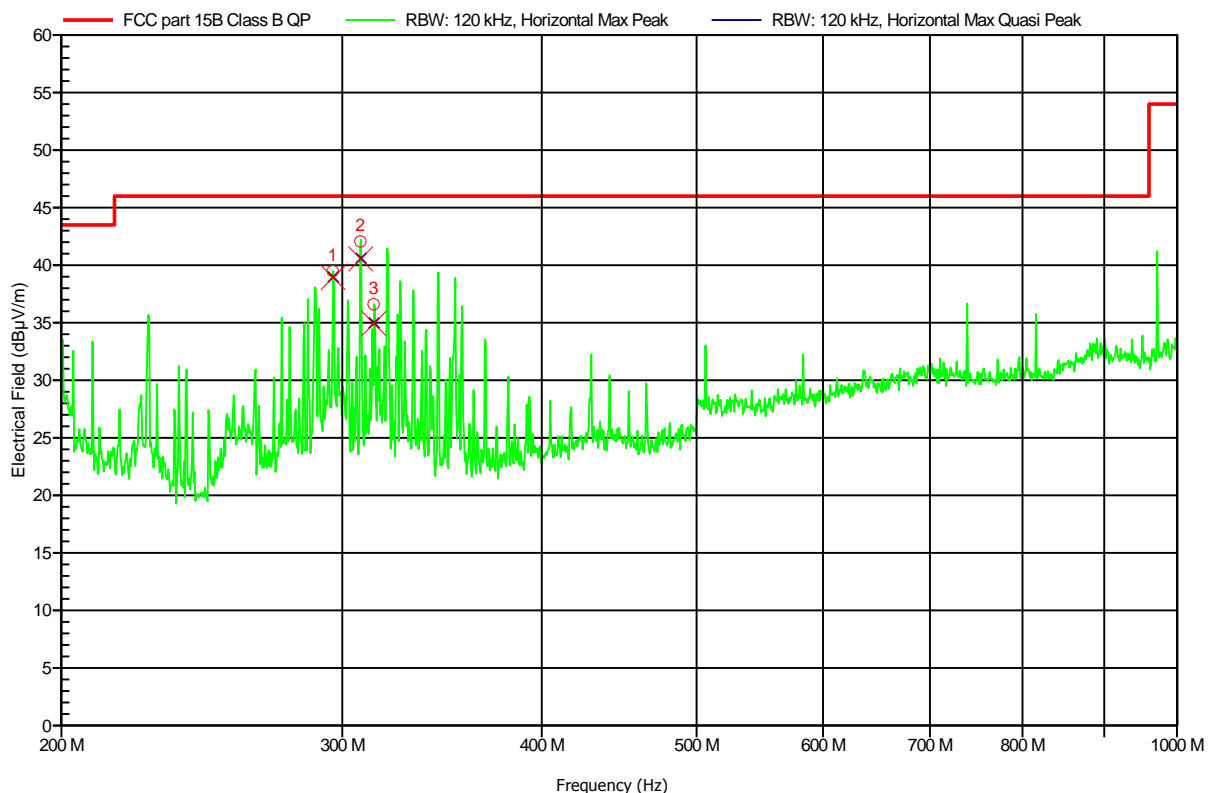

Nr	Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status
1	295.898 MHz	38.95 dBµV/m	46 dBµV/m	-7.05 dB	Pass
2	307.94 MHz	40.57 dBµV/m	46 dBµV/m	-5.43 dB	Pass
3	313.85 MHz	34.96 dBµV/m	46 dBµV/m	-11.04 dB	Pass

Test Report No.: G0M-1305-2859-EF01-V01

 Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

3.2 Test Conditions and Results – AC power line conducted emissions


Conducted emissions acc. FCC 47 CFR 15.107 / IC RSS-Gen			Verdict: PASS	
Laboratory Parameters:	Required prior to the test	During the test		
Ambient Temperature	15 to 35 °C	24°C		
Relative Humidity	30 to 60 %	53%		
Test according referenced standards	Reference Method			
	ANSI C63.4			
Fully configured sample scanned over the following frequency range	Frequency range			
	0.15 MHz to 30 MHz			
Sample is tested with respect to the requirements of the equipment class	Equipment class			
	Class B			
Points of Application	Application Interface			
AC Mains	LISN			
Operating mode	1			
Limits and results Class B				
Frequency [MHz]	Quasi-Peak [dB μ V]	Result	Average [dB μ V]	Result
0.15 to 5	66 to 56*	PASS	56 to 46*	PASS
0.5 to 5	56	PASS	46	PASS
5 to 30	60	PASS	50	PASS
Comments:				
* Limit decreases linearly with the logarithm of the frequency.				

EMI voltage test in the ac-mains according to FCC 15B

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Handrik
Test Conditions:	Tnom: 22°C, Unom: 120 V AC (AC/DC adaptor: ASUC30e-050100)
LISN:	ESH2-Z5 N
Mode:	active; motor with load; charging, Bluetooth link
Test Date:	2013-07-02
Note:	

Index 4

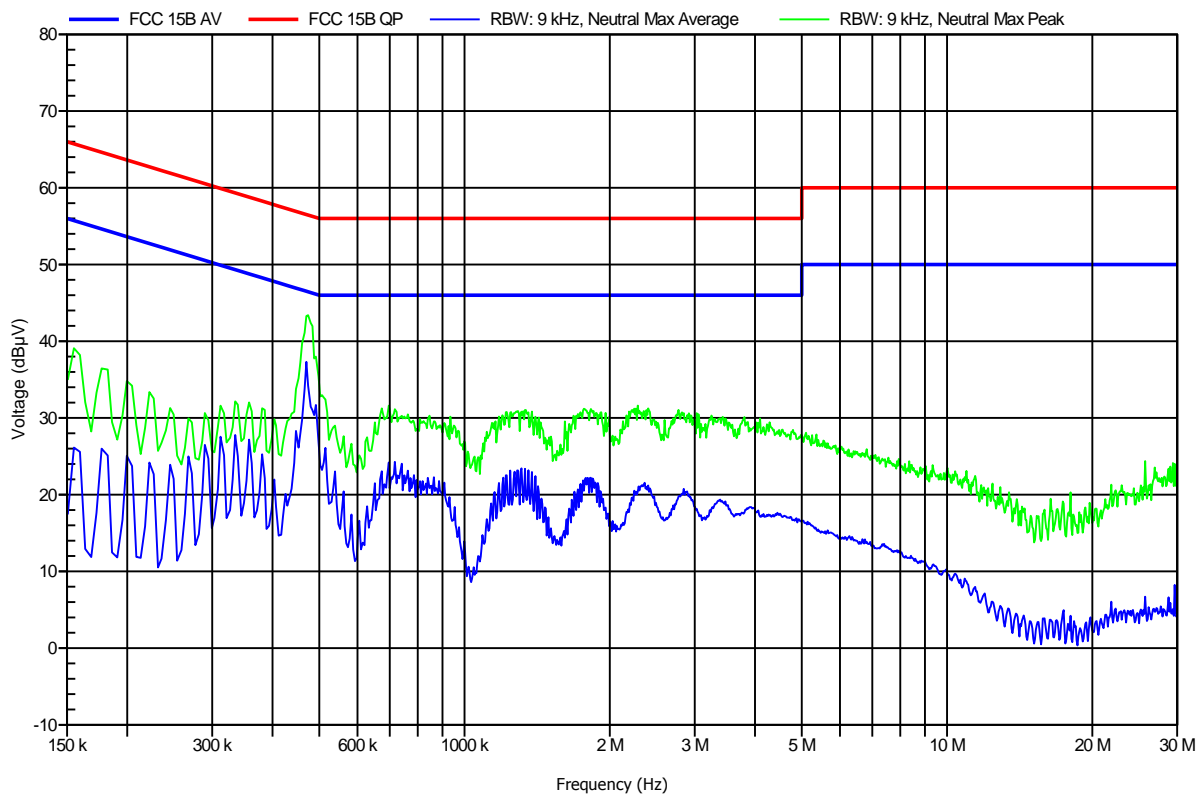

EMI voltage test in the ac-mains according to FCC 15B

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Handrik
Test Conditions:	Tnom: 22°C, Unom: 120 V AC (AC/DC adaptor: ASUC30e-050100)
LISN:	ESH2-Z5 L
Mode:	active; motor with load; charging, Bluetooth link
Test Date:	2013-07-02
Note:	

Index 5

