



FCC TEST REPORT FCC 47 CFR Part 15C Industry Canada RSS-210 Digital transmission systems operating within the 2400 – 2483.5 MHz band	
Report Reference No.	G0M-1305-2859-TFC247W-V02
Testing Laboratory	Eurofins Product Service GmbH
Address	Storkower Str. 38c 15526 Reichenwalde Germany
Accreditation	<div style="display: flex; justify-content: center; align-items: center;">   </div> <p style="text-align: center; margin-top: 5px;"> A2LA Accredited Testing Laboratory, Certificate No.: 1983.01 FCC Filed Test Laboratory, Reg.-No.: 96970 IC OATS Filing assigned code: 3470A </p>
Applicant's name	Bang & Olufsen Medicom A/S
Address	Gimsinglundvej 20 7600 Struer DENMARK
Test specification:	
Standard.....	47 CFR Part 15C KDB Publication No. 558074 RSS-210, Issue 8, 2010-12 RSS-Gen, Issue 3, 2010-12 ANSI C63.4:2009
Equipment under test (EUT):	
Product description	Electronic Auto-injector
Model No.	betaCONNECT
Hardware version	B11
Firmware / Software version	None
	FCC-ID: 2AAGY-BETAC1 IC: 3775E-BETAC1
Test result	Passed

Possible test case verdicts:	
- neither assessed nor tested	N/N
- required by standard but not appl. to test object.....	N/A
- required by standard but not tested.....	N/T
- not required by standard for the test object	N/R
- test object does meet the requirement.....	P (Pass)
- test object does not meet the requirement.....	F (Fail)
Testing:	
Date of receipt of test item	2013-07-01
Date (s) of performance of tests	2013-07-02 – 2013-07-03
Compiled by	Antje Bartusch
Tested by (+ signature)..... (Testing Manager)	Wilfried Treffke 
Approved by (+ signature)	Christian Weber 
Date of issue	2013-11-13
Total number of pages.....	82
General remarks:	
<p>The test results presented in this report relate only to the object tested.</p> <p>The results contained in this report reflect the results for this particular model and serial number. It is the responsibility of the manufacturer to ensure that all production models meet the intent of the requirements detailed within this report.</p>	
<p>This report shall not be reproduced, except in full, without the written approval of the Issuing testing laboratory.</p>	
Additional comments:	

Version History

Version	Issue Date	Remarks	Revised by
01	2013-08-30	Initial Release	
02	2013-11-13	Calibration dates corrected	C. Weber

REPORT INDEX

1	EQUIPMENT (TEST ITEM) DESCRIPTION	5
1.1	Photos – Equipment External	6
1.2	Photos – Equipment internal	7
1.3	Photos – Test setup	8
1.4	Supporting Equipment Used During Testing	9
1.5	Test Modes	10
1.6	Test Equipment Used During Testing	11
1.7	Sample emission level calculation	12
2	RESULT SUMMARY	13
3	TEST CONDITIONS AND RESULTS	14
3.1	Test Conditions and Results – Occupied Bandwidth	14
3.2	Test Conditions and Results – 6 dB Bandwidth	18
3.3	Test Conditions and Results – Maximum peak conducted power	22
3.4	Test Conditions and Results – Power spectral density	24
3.5	Test Conditions and Results – AC power line conducted emissions	25
3.6	Test Conditions and Results – Band edge compliance	28
3.7	Test Conditions and Results – Conducted spurious emissions	31
3.8	Test Conditions and Results – Transmitter radiated emissions	35
3.9	Test Conditions and Results – Receiver radiated emissions	37
ANNEX A	Transmitter radiated spurious emissions	39
ANNEX B	Receiver radiated spurious emissions	75

1 Equipment (Test item) Description

Description	Electronic Auto-injector	
Model	betaCONNECT	
Serial number	None	
Hardware version	B11	
Software / Firmware version	None	
FCC-ID	2AAGY-BETAC1	
IC	3775E-BETAC1	
Equipment type	Radio module	
Radio type	Transceiver	
Radio technology	Bluetooth 4.0 Low Energy	
Operating frequency range	2402 - 2480 MHz	
Assigned frequency band	2400 - 2483.5 MHz	
Main test frequencies	F _{LOW}	2402 MHz
	F _{MID}	2440 MHz
	F _{HIGH}	2480 MHz
Spreading	None	
Modulations	GFSK	
Number of channels	40	
Channel spacing	2MHz	
Number of antennas	1	
Antenna	Type	integrated
	Model	2450AT18B100
	Manufacturer	Johanson Technology
	Gain	-0.5 dBi (manufacturer declaration)
Manufacturer	Bang & Olufsen Medicom A/S Gimsinglundvej 20 7600 Struer DENMARK	
Power supply	V _{NOM}	3.7 VDC
	V _{MIN}	3.3 VDC
	V _{MAX}	4.2 VDC
AC/DC-Adaptor	Model	ASUC30e-050100
	Vendor	Aquilstar Precision Industrial
	Input	100-240VAC, 50-60Hz
	Output	5.0V

1.4 Supporting Equipment Used During Testing

Product Type*	Device	Manufacturer	Model No.	Comments
None				
<p>*Note: Use the following abbreviations:</p> <p style="padding-left: 40px;">AE : Auxiliary/Associated Equipment, or</p> <p style="padding-left: 40px;">SIM : Simulator (Not Subjected to Test)</p> <p style="padding-left: 40px;">CABL : Connecting cables</p>				

1.5 Test Modes

Mode #	Description	
Transmit	General conditions:	EUT powered by laboratory power supply.
	Radio conditions:	Mode = standalone transmit Spreading = None Modulation = GFSK Data rate = 1 Mbps Bandwidth = 2 MHz Duty cycle = 100 % Power level = Maximum
Receive	General conditions:	EUT powered by laboratory power supply.
	Radio conditions:	Mode = standalone receive (scan mode) Spreading = None Modulation = GFSK
AC-Powerline	General conditions:	EUT powered by commercial Laptop
	Radio conditions:	Mode = Transmit Spreading = None

1.6 Test Equipment Used During Testing

Occupied Bandwidth					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSP 30	EF00312	2013-01	2014-01

6dB Bandwidth					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSP 30	EF00312	2013-01	2014-01

Maximum peak conducted power					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSP 30	EF00312	2013-01	2014-01

Power spectral density					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSP 30	EF00312	2013-01	2014-01

Band edge compliance					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSP 30	EF00312	2013-01	2014-01

Conducted spurious emissions					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSP 30	EF00312	2013-01	2014-01

Radiated spurious emissions					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Semi-anechoic chamber	Frankonia	AC 5	EF00395	-	-
Spectrum Analyzer	R&S	FSIQ26	EF00242	2013-06	2014-06
Biconical Antenna	R&S	HK 116	EF00012	2013-02	2016-02
LPD Antenna	R&S	HL 223	EF00187	2011-02	2014-02
LPD Antenna	R&S	HL 025	EF00327	2013-02	2016-02

AC powerline conducted emissions					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
AMN	R&S	ESH2-Z5	EF00182	2012-10	2014-10
AMN	R&S	ESH3-Z5	EF00036	2012-11	2014-11
EMI Test Receiver	R&S	ESCS 30	EF00295	2012-08	2013-08

Test Report No.: G0M-1305-2859-TFC247W-V02

Eurofins Product Service GmbH
Storkower Str. 38c, D-15526 Reichenwalde, Germany

1.7 Sample emission level calculation

The following is a description of terms and a sample calculation, as appears in the radiated emissions data table. The numbers used in the calculation are for example only. There is no direct correlation to the specific data taken for the product described in this document:

Reading:

This is the reading obtained on the spectrum analyzer in dB μ V. Any external preamplifiers used are taken into account through internal analyzer settings.

A.F.:

This is the antenna factor for the receiving antenna. It is a conversion factor, which converts electric fields strengths to voltages, which can be measured directly on the spectrum analyzer. It is treated as a loss in dB. Cable losses have been included with the A.F. to simplify the calculations. The antenna factor is used in calculations as follows:

$$\text{Reading on Analyzer (dB}\mu\text{V)} + \text{A.F. (dB)} = \text{Net field strength (dB}\mu\text{V/m)}$$

Net:

This is the net field strength measurement (as shown above).

Limit:

This is the FCC Class B radiated emission limit (in units of dB μ V/m). The FCC limits are given in units of μ V/m. The following formula is used to convert the units of μ V/m to dB μ V/m:

$$\text{Limit (dB}\mu\text{V/m)} = 20 * \log (\mu\text{V/m})$$

Margin:

This is the margin of compliance below the FCC limit. The units are given in dB. A negative margin indicates the emission was below the limit. A positive margin indicates that the emission exceeds the limit.

Example only:


$$\begin{array}{rclcl} \text{Reading} & + & \text{AF} & = & \text{Net Reading} & : & \text{Net reading - FCC limit} & = & \text{Margin} \\ 21.5 \text{ dB}\mu\text{V} & + & 26 \text{ dB} & = & 47.5 \text{ dB}\mu\text{V/m} & : & 47.5 \text{ dB}\mu\text{V/m} - 57.0 \text{ dB}\mu\text{V/m} & = & -9.5 \text{ dB} \end{array}$$

2 Result Summary

FCC 47 CFR Part 15C, IC RSS-210				
Product Specific Standard Section	Requirement – Test	Reference Method	Result	Remarks
RSS-Gen 4.6.1	Occupied Bandwidth	RSS-Gen 4.6.1	N/R	Informational only
FCC § 15.247(a)(2) IC RSS-210 § A8.2	6dB Bandwidth	KDB Publication No. 558074	PASS	
FCC § 15.247(b)(3) IC RSS-210 § A8.4	Maximum peak conducted power	KDB Publication No. 558074	PASS	
FCC § 15.247(e) IC RSS-210 § A8.2	Power spectral density	KDB Publication No. 558074	PASS	
47 CFR 15.207 RSS-Gen 7.2.4	AC power line conducted emissions	KDB Publication No. 558074 / ANSI C63.4	PASS	
FCC § 15.247(d) IC RSS-210 § A8.5	Band edge compliance	KDB Publication No. 558074	PASS	
FCC § 15.247(d) IC RSS-210 § A8.5	Conducted spurious emissions	KDB Publication No. 558074	PASS	
FCC § 15.247(d) FCC § 15.209 IC RSS-210 A8.5 IC RSS-Gen 4.9 IC RSS-Gen 7.2.5	Transmitter radiated spurious emissions	KDB Publication No. 558074 / ANSI C 63.4	PASS	
IC RSS-Gen 4.10 IC RSS-Gen 6.1	Receiver radiated spurious emissions	ANSI C 63.4	PASS	
Remarks:				


3 Test Conditions and Results

3.1 Test Conditions and Results – Occupied Bandwidth

Occupied Bandwidth acc. IC RSS-Gen		Verdict: PASS	
Test according to measurement reference	Reference Method		
	RSS-Gen 4.6.1		
Test frequency range	Tested frequencies		
	$F_{\text{LOW}} / F_{\text{MID}} / F_{\text{HIGH}}$		
Limits			
None (Informational only)			
Test setup			
			
Test procedure			
<ol style="list-style-type: none"> 1. EUT set to test mode (Communication tester is used if needed) 2. Span set to at least twice the emission spectrum 3. Resolution bandwidth set to 1 % of span 4. Occupied Bandwidth (99 %) measurement with spectrum analyzer built in measurement function 			
Test results			
Channel	Frequency [MHz]	Mode	Occupied Bandwidth [kHz]
F_{LOW}	2402	Transmit	1.065
F_{MID}	2440	Transmit	1.017
F_{HIGH}	2480	Transmit	1.009
Comments:			

Occupied Bandwidth – F_{MID}
**RSS Gen
Occupied Bandwidth**


EUT	Electronic Auto-injector
Model	betaCONNECT
Approval Holder	Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
Temperature / Voltage	Tnom / Vnom
Test Site / Operator	Eurofins Product Service GmbH / Mr. Treffke
Test Specification	4.4.1 Occupied Bandwidth
Comment 1	Channel.: 2440 MHz
Comment 2	A spectrum analyzer with an integrated 99% power bandwidth function is used
Comment 3	GFSK

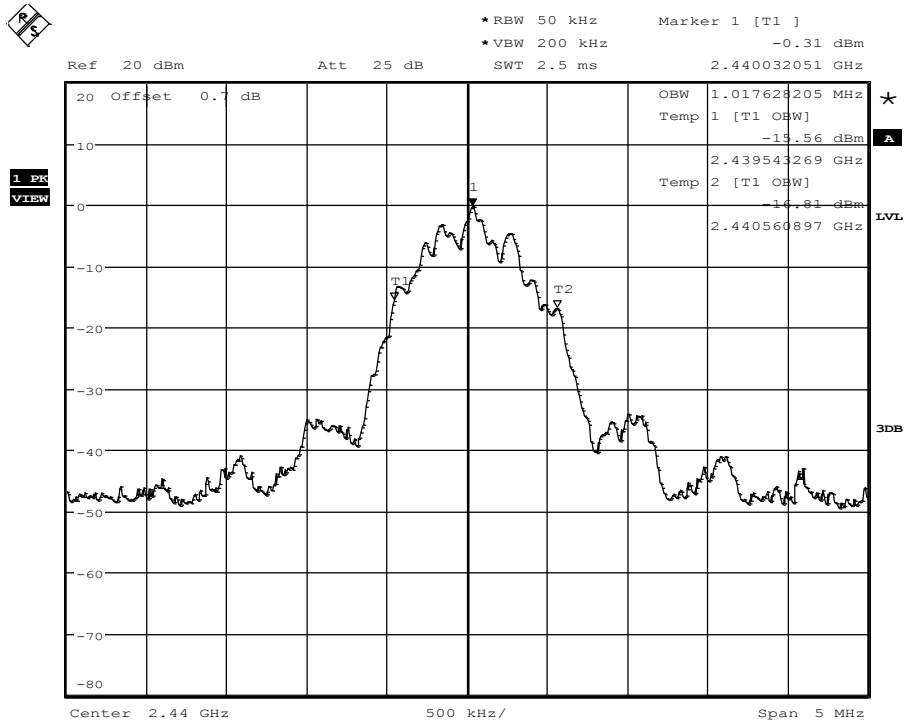

Occupied bandwidth: 1017.6 KHz
Date: 2.JUL.2013 14:01:37


Occupied Bandwidth – F_{HIGH}
**RSS Gen
Occupied Bandwidth**

EUT	Electronic Auto-injector
Model	betaCONNECT
Approval Holder	Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
Temperature / Voltage	Tnom / Vnom
Test Site / Operator	Eurofins Product Service GmbH / Mr. Treffke
Test Specification	4.4.1 Occupied Bandwidth
Comment 1	Channel.: 2480 MHz
Comment 2	A spectrum analyzer with an integrated 99% power bandwidth function is used
Comment 3	GFSK

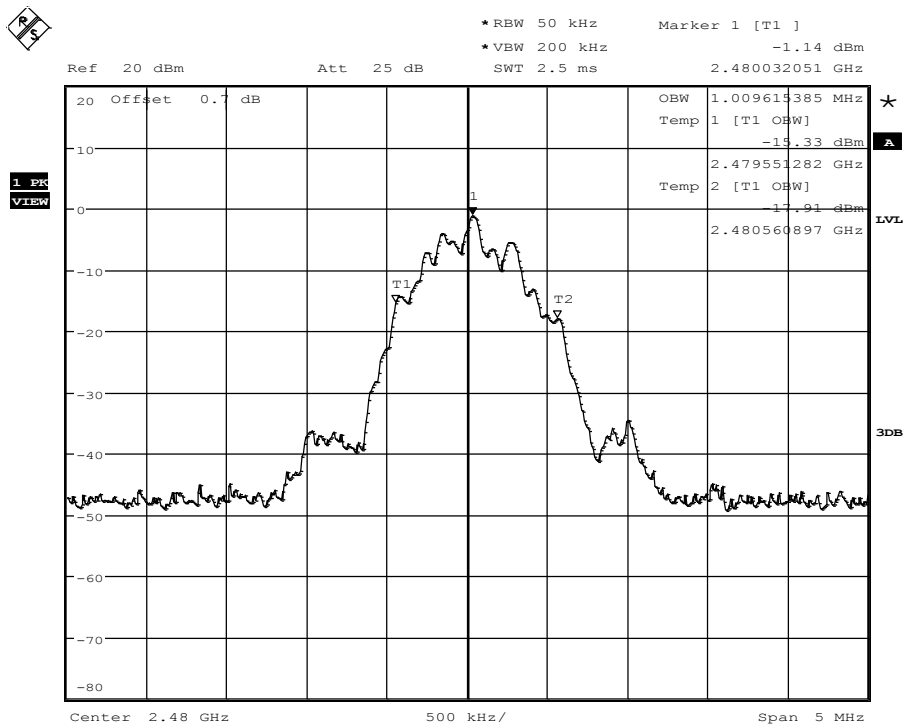


Occupied bandwidth: 1009.6 KHz
Date: 2.JUL.2013 14:03:07

3.2 Test Conditions and Results – 6 dB Bandwidth

6dB Bandwidth acc. FCC 15.247 / IC RSS-210				Verdict: PASS	
EUT requirement rule parts and clause	Reference				
	FCC 15.247(a)(2) / IC RSS-210 A8.2				
Test according to measurement reference	Reference Method				
	FCC KDB Publication No. 558074				
Test frequency range	Tested frequencies				
	$F_{LOW} / F_{MID} / F_{HIGH}$				
Limits					
Limit					
≥ 500kHz					
Test setup					
					
Test procedure					
<ol style="list-style-type: none"> 1. EUT set to test mode 2. Span set to at least twice the emission spectrum 3. Detector set to peak and max hold and RBW is set to 100 kHz 4. Envelope peak value of emission spectrum is selected 5. Marker on envelope of spectrum is set to level of -6 dB to the left of the peak 6. Marker on envelope of spectrum is set to level of -6 dB to the right of the peak 7. 6 dB Bandwidth is determined by marker frequency separation 					
Test results					
Channel	Frequency [MHz]	Mode	6 dB Bandwidth [kHz]	Limit [kHz]	Result
F_{LOW}	2402	Transmit	668.963	500	PASS
F_{MID}	2440	Transmit	668.907	500	PASS
F_{HIGH}	2480	Transmit	663.221	500	PASS
Comments:					

6 dB Bandwidth – F_{Low}
**FCC part 15.247 (a)2
Minimum 6 dB Bandwidth**

EUT	Electronic Auto-injector
Model	betaCONNECT
Approval Holder	Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
Temperature / Voltage	Tnom / Vnom
Test Site / Operator	Eurofins Product Service GmbH / Mr. Treffke
Test Specification	FCC part 15.247 (a)2
Comment 1	Minimum 6 dB Bandwidth
Comment 2	Channel 2402 MHz, GFSK
Comment 3	procedure 8.1 DTS BW (558074 D01 DTS)

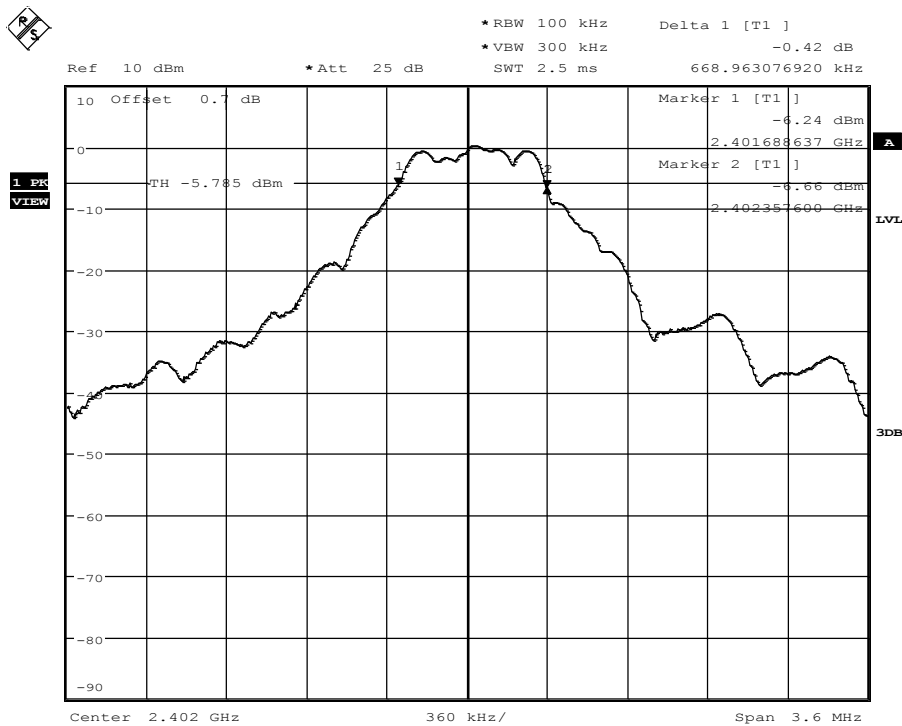


6 dB bandwidth: 669 KHz > 500 KHz; verdict: PASS
 Date: 2.JUL.2013 13:35:44

6 dB Bandwidth – F_{MID}

FCC part 15.247 (a)2
Minimum 6 dB Bandwidth


EUT	Electronic Auto-injector
Model	betaCONNECT
Approval Holder	Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
Temperature / Voltage	Tnom / Vnom
Test Site / Operator	Eurofins Product Service GmbH / Mr. Treffke
Test Specification	FCC part 15.247 (a)2
Comment 1	Minimum 6 dB Bandwidth
Comment 2	Channel 2440 MHz, GFSK
Comment 3	procedure 8.1 DTS BW (558074 D01 DTS)

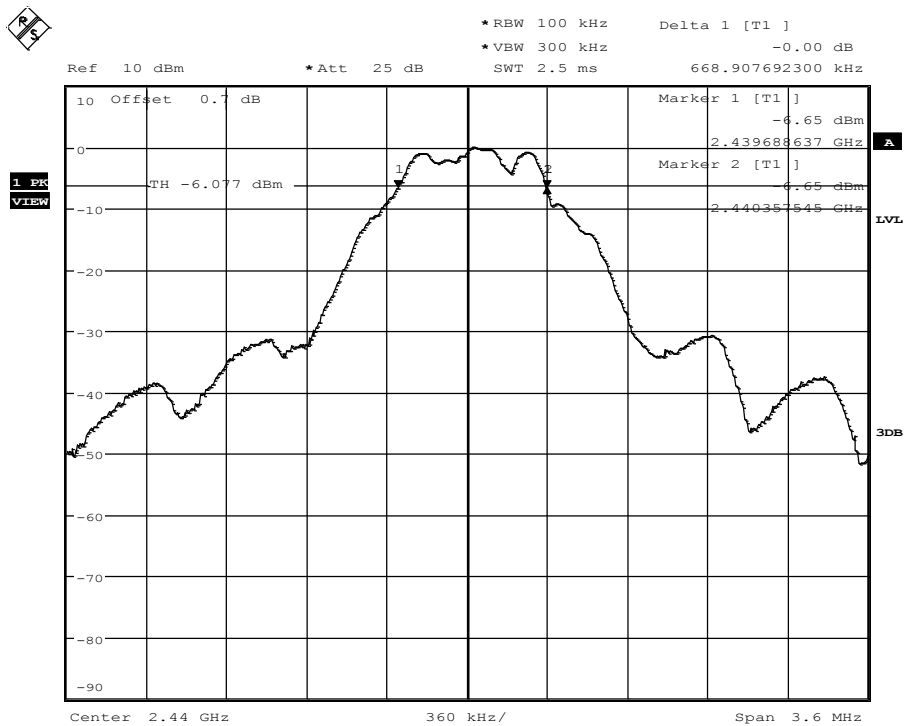

6 dB bandwidth: 668.9 KHz > 500 KHz; verdict: PASS
Date: 2.JUL.2013 13:32:55


6 dB Bandwidth – F_{HIGH}
**FCC part 15.247 (a)2
Minimum 6 dB Bandwidth**

EUT	Electronic Auto-injector
Model	betaCONNECT
Approval Holder	Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
Temperature / Voltage	Tnom / Vnom
Test Site / Operator	Eurofins Product Service GmbH / Mr. Treffke
Test Specification	FCC part 15.247 (a)2
Comment 1	Minimum 6 dB Bandwidth
Comment 2	Channel 2480 MHz, GFSK
Comment 3	procedure 8.1 DTS BW (558074 D01 DTS)

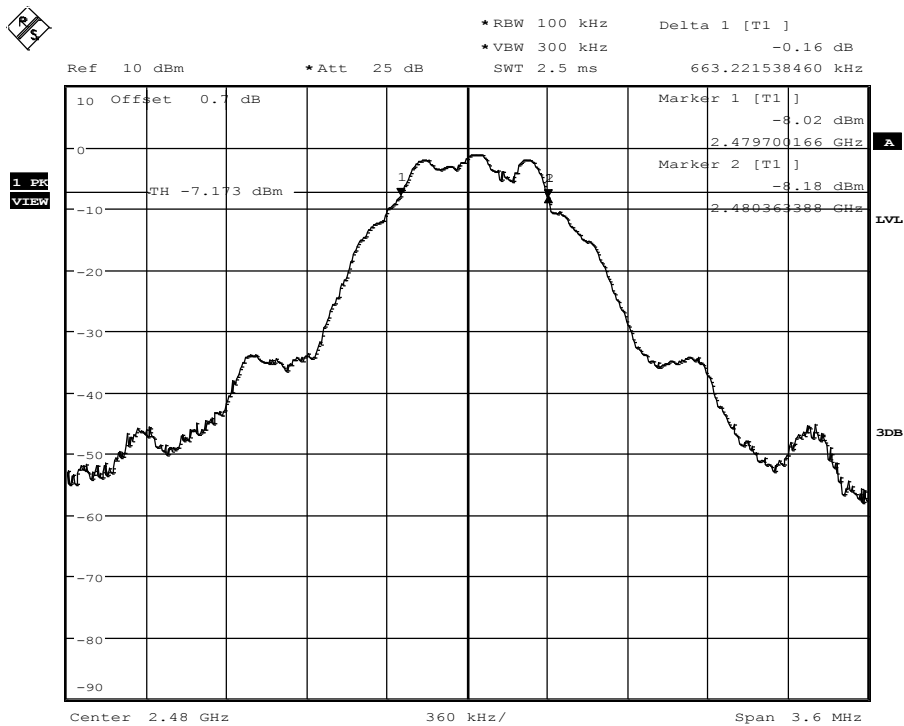


6 dB bandwidth: 663.2 KHz > 500 KHz; verdict: PASS
 Date: 2.JUL.2013 13:37:15

3.3 Test Conditions and Results – Maximum peak conducted power

Maximum peak conducted power acc. FCC 15.247 / IC RSS-210		Verdict: PASS
EUT requirement rule parts and clause	Reference	
	FCC 15.247(b)(3) / IC RSS-210 A8.4	
Test according to measurement reference	Reference Method	
	FCC KDB Publication No. 558074	
Test frequency range	Tested frequencies	
	$F_{\text{LOW}} / F_{\text{MID}} / F_{\text{HIGH}}$	
Measurement mode	Peak	
Maximum antenna gain	-0.5 dBi \Rightarrow Limit correction = 0 dB	
Limits		
1 W (30 dBm)		
<p>The conducted output power limit specified above is based on the use of antennas with directional gains that do not exceed 6 dBi. If transmitting antennas of directional gain greater than 6 dBi are used, the conducted output power from the intentional radiator shall be reduced below the stated values in the table, as appropriate, by the amount in dB that the directional gain of the antenna exceeds 6 dBi.</p>		
Test setup		
 <pre> graph LR SA[Spectrum Analyzer] --- EUT[EUT] </pre>		
Test procedure		
<ol style="list-style-type: none"> 1. EUT set to test mode (Communication tester is used if needed) 2. Center frequency set to test channel center frequency 3. Span set to twice the 20 dB bandwidth and detector to peak and max hold 4. Resolution bandwidth is set to 3 MHz 5. Peak conducted power is determined from peak of spectrum envelope 		

Test results							
Channel	Frequency [MHz]	Voltage	Mode	Peak power [dbm]	Peak power [W]	Limit [dBm]	Margin [dB]
F _{LOW}	2402	V _{NOM} = 3.7	Transmit	0.21	0.001	30	-29.79
F _{MID}	2442	V _{MIN} = 3.3	Transmit	0.21	0.001	30	-29.79
F _{HIGH}	2480	V _{MAX} =4.2	Transmit	0.20	0.001	30	-29.80
F _{LOW}	2402	V _{NOM} = 3.7	Transmit	-0.3	0.001	30	-30.30
F _{MID}	2442	V _{MIN} = 3.3	Transmit	-0.28	0.0009	30	-30.28
F _{HIGH}	2480	V _{MAX} =4.2	Transmit	-0.29	0.0009	30	-30.29
F _{LOW}	2402	V _{NOM} = 3.7	Transmit	-1.21	0.0007	30	-31.21
F _{MID}	2442	V _{MIN} = 3.3	Transmit	-1.21	0.0007	30	-31.21
F _{HIGH}	2480	V _{MAX} =4.2	Transmit	-1.22	0.0007	30	-31.22
Comment:							

3.4 Test Conditions and Results – Power spectral density

Power spectral density acc. FCC 15.247 / IC RSS-210				Verdict: PASS		
EUT requirement rule parts and clause	Reference					
	FCC 15.247(e) / IC RSS-210 A8.2					
Test according to measurement reference	Reference Method					
	FCC KDB Publication No. 558074					
Test frequency range	Tested frequencies					
	$F_{LOW} / F_{MID} / F_{HIGH}$					
Measurement mode	Peak					
Limits						
8 dBm / 3 kHz						
Test setup						
						
Test procedure						
<ol style="list-style-type: none"> 1. EUT set to test mode (Communication tester is used if needed) 2. Center frequency set to test channel center frequency 3. Span is set large enough to capture maximum emissions in passband, RBW is set to 3kHz 4. Peak power density is determined from peak emission of envelope 						
Test results						
Channel	Frequency [MHz]	Test mode	Peak frequency [MHz]	Peak power density [dBm]	Limit [dBm/3kHz]	Margin [dB]
F_{LOW}	2402	Transmit	2402.045	-15.02	8.0	-23.02
F_{MID}	2440	Transmit	2440.035	-15.6	8.0	-23.60
F_{HIGH}	2480	Transmit	2480.045	-16.5	8.0	-24.50
Comments:						

3.5 Test Conditions and Results – AC power line conducted emissions


Power line conducted emissions acc. FCC 47 CFR 15.207 / IC RSS-Gen		Verdict: PASS		
Test according referenced standards	Reference Method			
	ANSI C63.4			
Fully configured sample scanned over the following frequency range	Frequency range			
	0.15 MHz to 30 MHz			
Points of Application	Application Interface			
AC Mains	LISN			
EUT test mode	AC power line			
Limits and results				
Frequency [MHz]	Quasi-Peak [dB μ V]	Result	Average [dB μ V]	Result
0.15 to 5	66 to 56*	PASS	56 to 46*	PASS
0.5 to 5	56	PASS	46	PASS
5 to 30	60	PASS	50	PASS
Comments: * Limit decreases linearly with the logarithm of the frequency.				

Conducted Emissions
EMI voltage test in the ac-mains according to FCC 15B

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Handrik
Test Conditions:	Tnom: 22°C, Unom: 120 V AC (AC/DC adaptor: ASUC30e-050100)
LISN:	ESH2-Z5 N
Mode:	active; motor with load; charging, Bluetooth link
Test Date:	2013-07-02
Note:	

Index 4

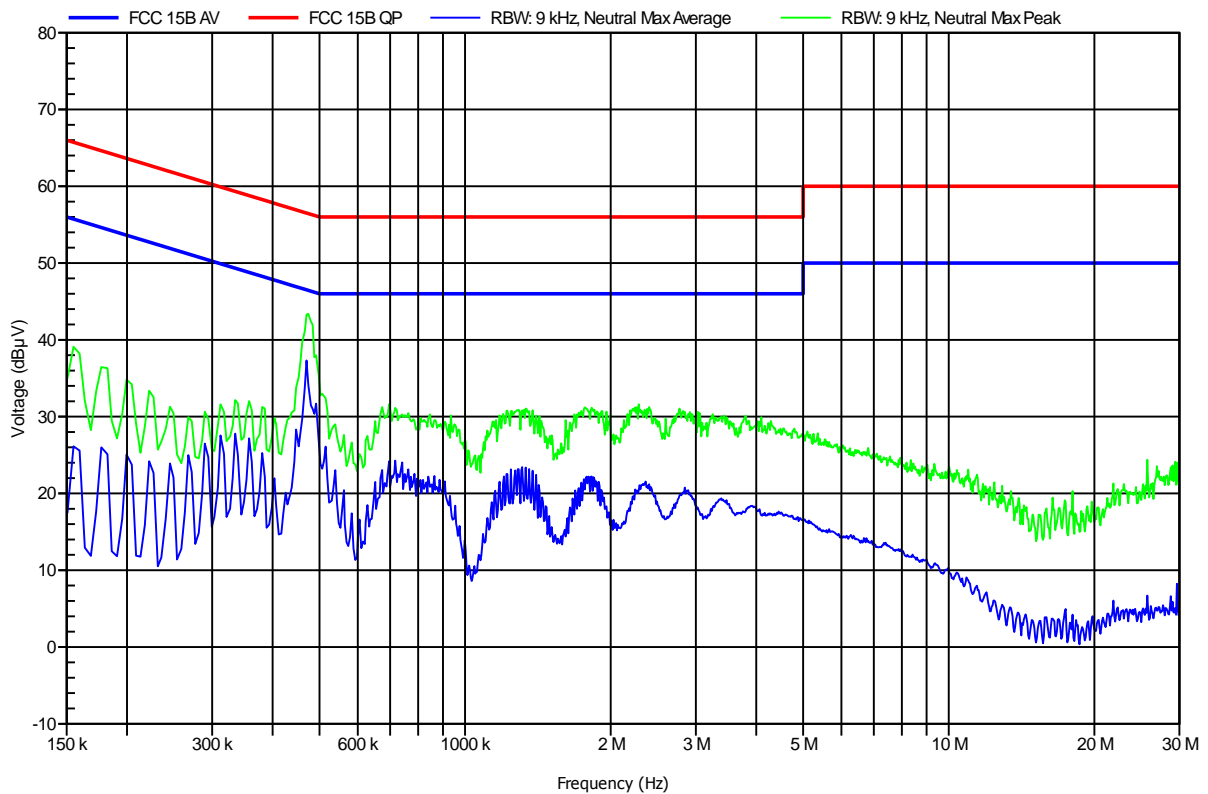


Conducted Emissions
EMI voltage test in the ac-mains according to FCC 15B


Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Handrik
 Test Conditions: Tnom: 22°C, Unom: 120 V AC (AC/DC adaptor: ASUC30e-050100)
 LISN: ESH2-Z5 L
 Mode: active; motor with load; charging, Bluetooth link
 Test Date: 2013-07-02
 Note:

Index 5

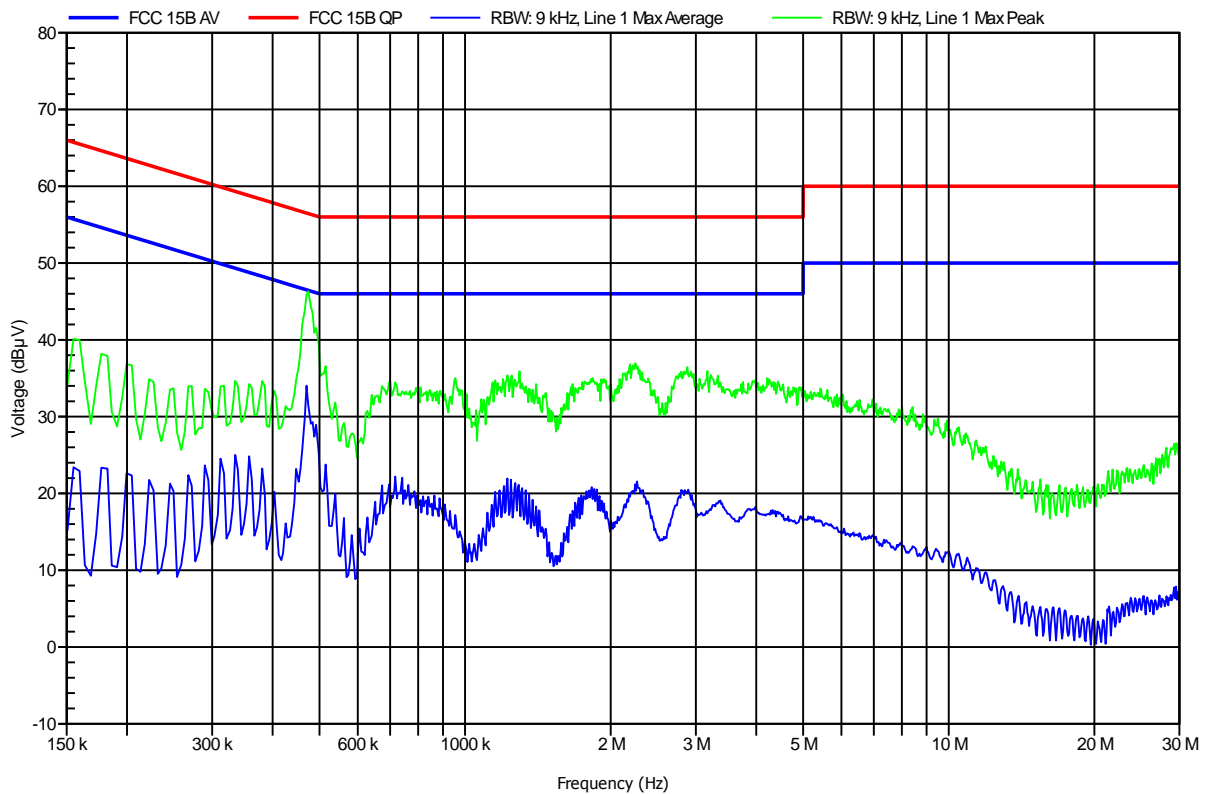


3.6 Test Conditions and Results – Band edge compliance

Band-edge compliance acc. FCC 15.247 / IC RSS-210				Verdict: PASS	
EUT requirement rule parts and clause		Reference			
		FCC 15.247(d) / IC RSS-210 A8.5			
Test according to measurement reference		Reference Method			
		FCC KDB Publication No. 558074			
Test frequency range		Tested frequencies			
		F_{LOW} / F_{HIGH}			
Measurement mode		Peak			
Limits					
Limit			Condition		
≤ -20 dB / 100 kHz			Peak power measurement detector = Peak		
≤ -30 dB / 100 kHz			Peak power measurement detector = RMS		
Test setup					
 <pre> graph LR SA[Spectrum Analyzer] --- EUT[EUT] </pre>					
Test procedure					
<ol style="list-style-type: none"> EUT set to test mode (Communication tester is used if needed) Span set around lower band edge and detector is set to peak and max hold Resolution bandwidth is set to 100 kHz Markers are set to peak emission levels within frequency band and outside frequency band Band edge attenuation is determined from level difference 					
Test results					
Channel	Frequency [MHz]	Mode	Level [dBc]	Limit [dBc]	Margin [dB]
F_{LOW}	2402	Transmit	-40.61	-20	-20.61
F_{HIGH}	2480	Transmit	-41.73	-20	-21.73
Comments:					

Band-edge compliance
FCC part 15.247
Band-edge compliance of RF conducted emissions

EUT	Electronic Auto-injector
Model	betaCONNECT
Approval Holder	Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
Temperature / Voltage	Tnom / Vnom
Test Site / Operator	Eurofins Product Service GmbH / Mr. Treffke
Test Specification	FCC part 15 section 247(c)
Comment 1	Band-edge compliance
Comment 2	Channel.: 2402 MHz
Comment 3	GFSK

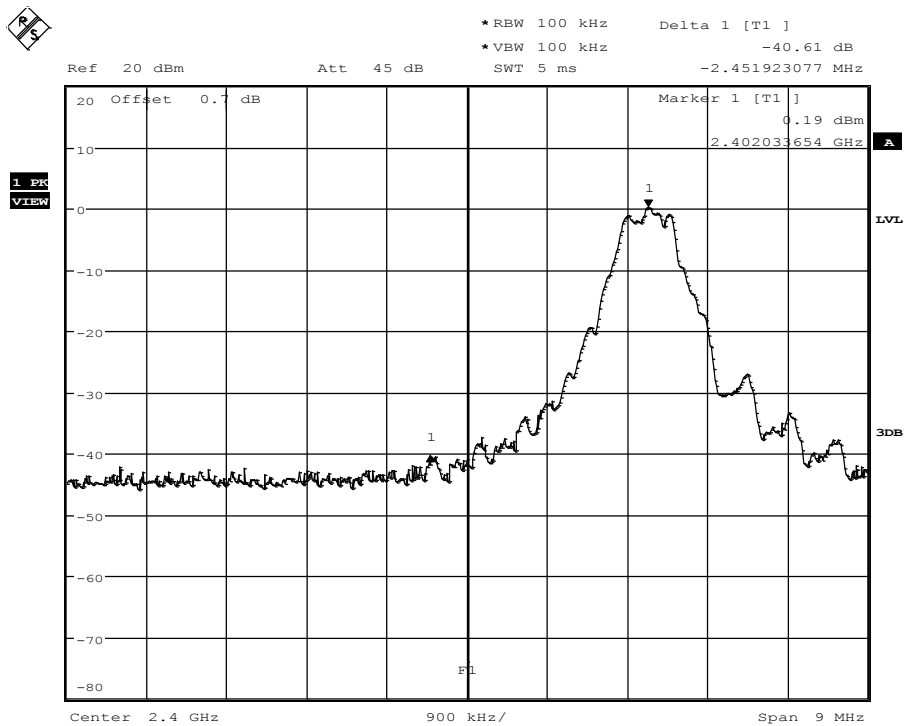


Limit: Marker Delta value >20 dB; Result: PASS

Date: 2.JUL.2013 14:07:14

Band-edge compliance
FCC part 15.247
Band-edge compliance of RF conducted emissions


EUT	Electronic Auto-injector
Model	betaCONNECT
Approval Holder	Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
Temperature / Voltage	Tnom / Vnom
Test Site / Operator	Eurofins Product Service GmbH / Mr. Treffke
Test Specification	FCC part 15 section 247(c)
Comment 1	Band-edge compliance
Comment 2	Channel.: 2480 MHz
Comment 3	GFSK

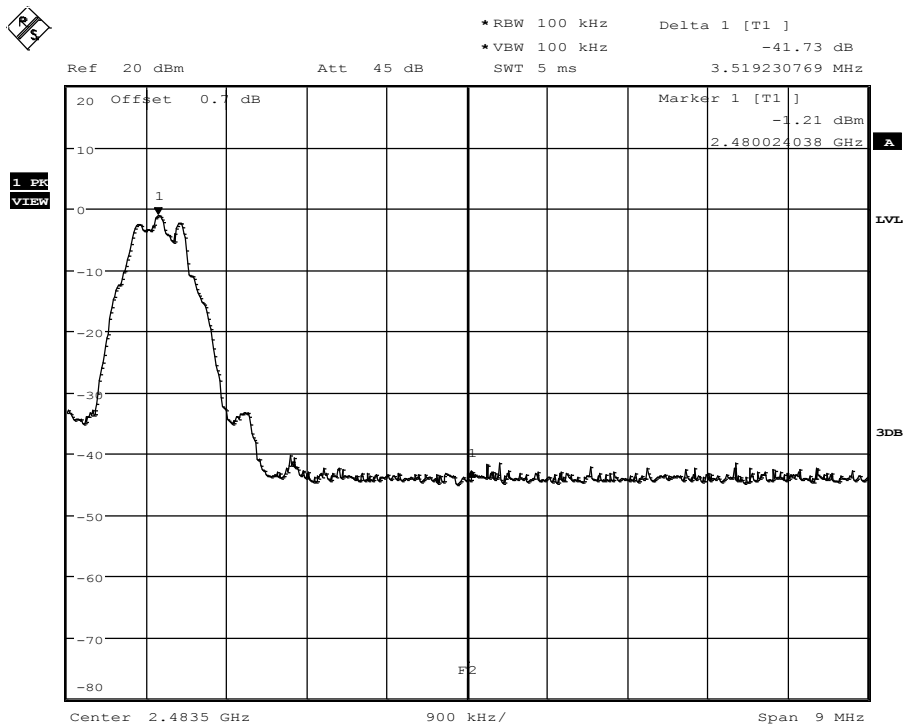

Limit: Marker Delta value >20 dB; Result: PASS



Date: 2.JUL.2013 14:05:01

3.7 Test Conditions and Results – Conducted spurious emissions

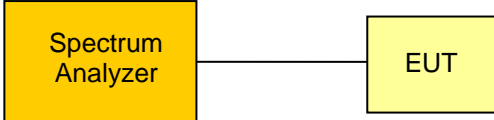Conducted spurious emissions acc. FCC 15.247 / IC RSS-210				Verdict: PASS			
EUT requirement rule parts and clause		Reference					
		FCC 15.247(d) / IC RSS-210 A8.5					
Test according to measurement reference		Reference Method					
		FCC KDB Publication No. 558074					
Test frequency range		Tested frequencies					
		10 MHz – 10 th Harmonic					
Measurement mode		Peak					
Limits							
Limit				Condition			
≤ -20 dB / 100 kHz				Peak power measurement detector = Peak			
≤ -30 dB /100 kHz				Peak power measurement detector = RMS			
Test setup							
							
Test procedure							
<ol style="list-style-type: none"> 1. EUT set to test mode (Communication tester is used if needed) 2. Span it set according to measurement range 3. Resolution bandwidth is set to 100 kHz and detector to peak and max hold 4. Markers are set to peak emission levels within frequency band 5. Emission level is determined by second marker on emission peak 6. Attenuation is determined from level difference 							
Test results							
Channel	Frequency [MHz]	Mode	Emission [MHz]	Emission Level [dbm]	Peak power [dBm]	Limit [dBm]	Margin [dB]
F _{LOW}	2402	Transmit	4800.74	-41.72	-0.16	-20.16	-21.56
F _{MID}	2440	Transmit	4884.78	-41.70	-1.43	-21.4	-20.30
F _{HIGH}	2480	Transmit	4968.83	-40.09	-1.77	-21.8	-18.29
Comments:							

Conducted spurious emissions – F_{Low}
**FCC part 15.247 (d)
Spurious Emissions**

EUT	Electronic Auto-injector
Model	betaCONNECT
Approval Holder	Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
Temperature / Voltage	Tnom / Vnom
Test Site / Operator	Eurofins Product Service GmbH / Mr. Treffke
Test Specification	FCC part 15.247 (d)
Comment 1	Spurious Emissions conducted
Comment 2	Channel 2402 MHz
Comment 3	Emissions in non-restricted frequency bands 558074 D01 Meas Guidance

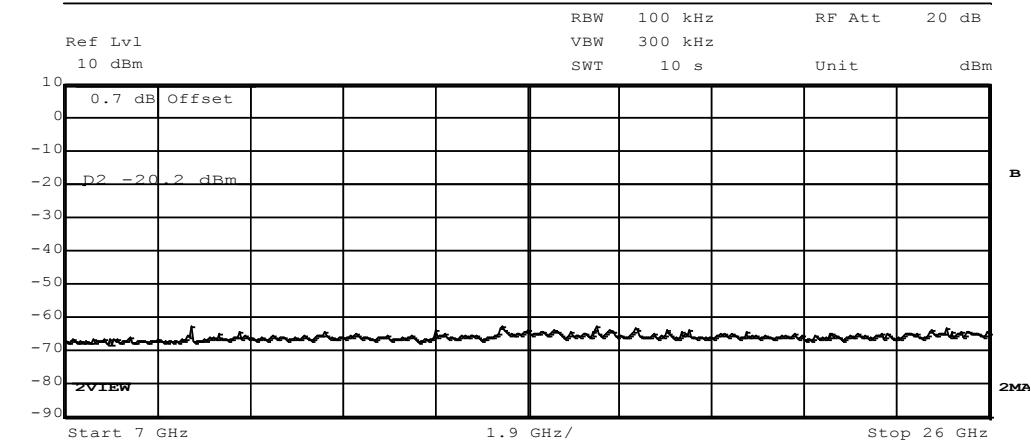
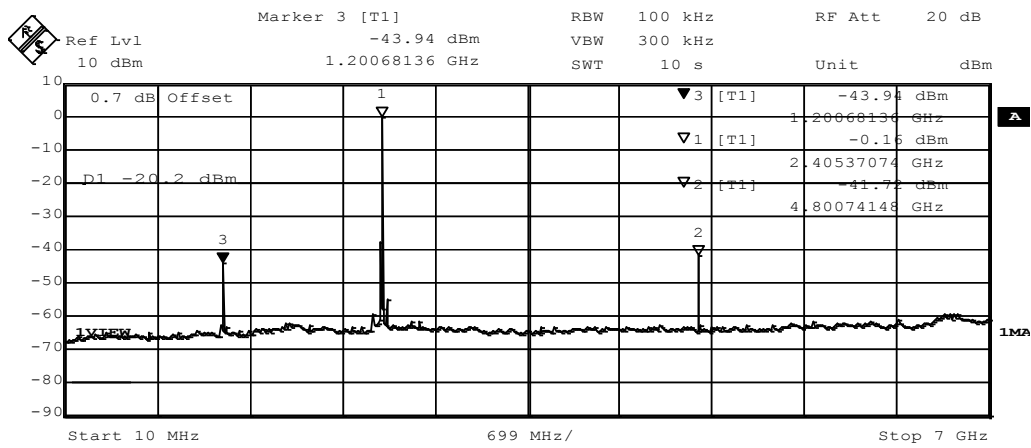


Date: 2.JUL.2013 14:21:51

Conducted spurious emissions – F_{MID}

FCC part 15.247 (d)
Spurious Emissions

EUT Electronic Auto-injector
 Model betaCONNECT
 Approval Holder Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
 Temperature / Voltage Tnom / Vnom
 Test Site / Operator Eurofins Product Service GmbH / Mr. Treffke
 Test Specification FCC part 15.247 (d)
 Comment 1 Spurious Emissions conducted
 Comment 2 Channel 2440 MHz
 Comment 3 Emissions in non-restricted frequency bands 558074 D01 Meas Guidance

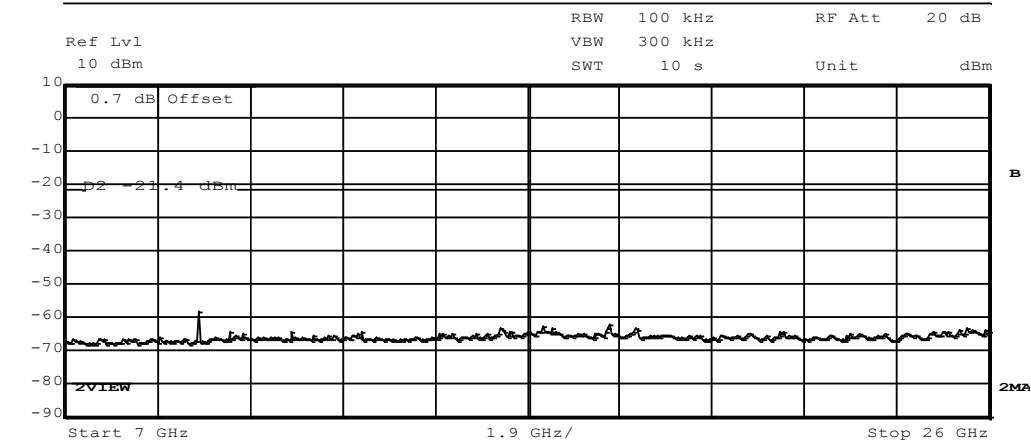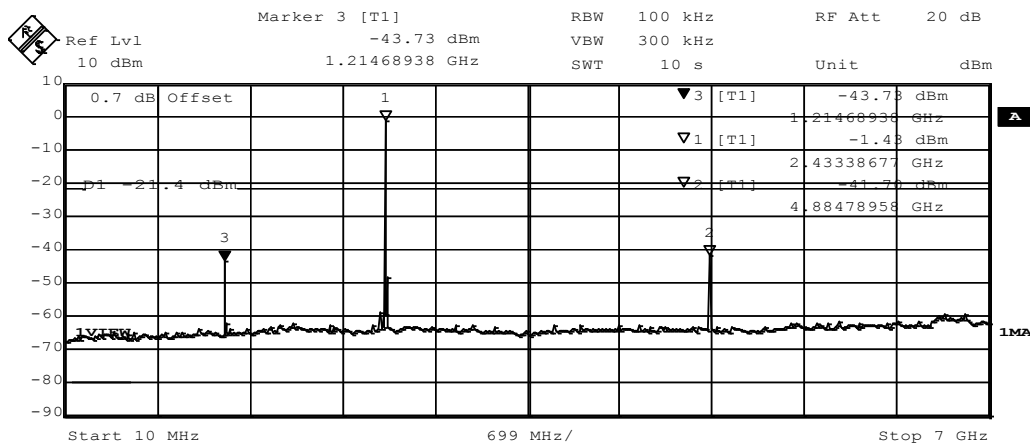


Date: 2.JUL.2013 14:19:06


Conducted spurious emissions – F_{HIGH}

FCC part 15.247 (d)
Spurious Emissions

EUT Electronic Auto-injector
 Model betaCONNECT
 Approval Holder Bang & Olufsen Medicom A/S / Ord.: G0M-1305-2859
 Temperature / Voltage Tnom / Vnom
 Test Site / Operator Eurofins Product Service GmbH / Mr. Treffke
 Test Specification FCC part 15.247 (d)
 Comment 1 Spurious Emissions conducted
 Comment 2 Channel 2480 MHz
 Comment 3 Emissions in non-restricted frequency bands 558074 D01 Meas Guidance

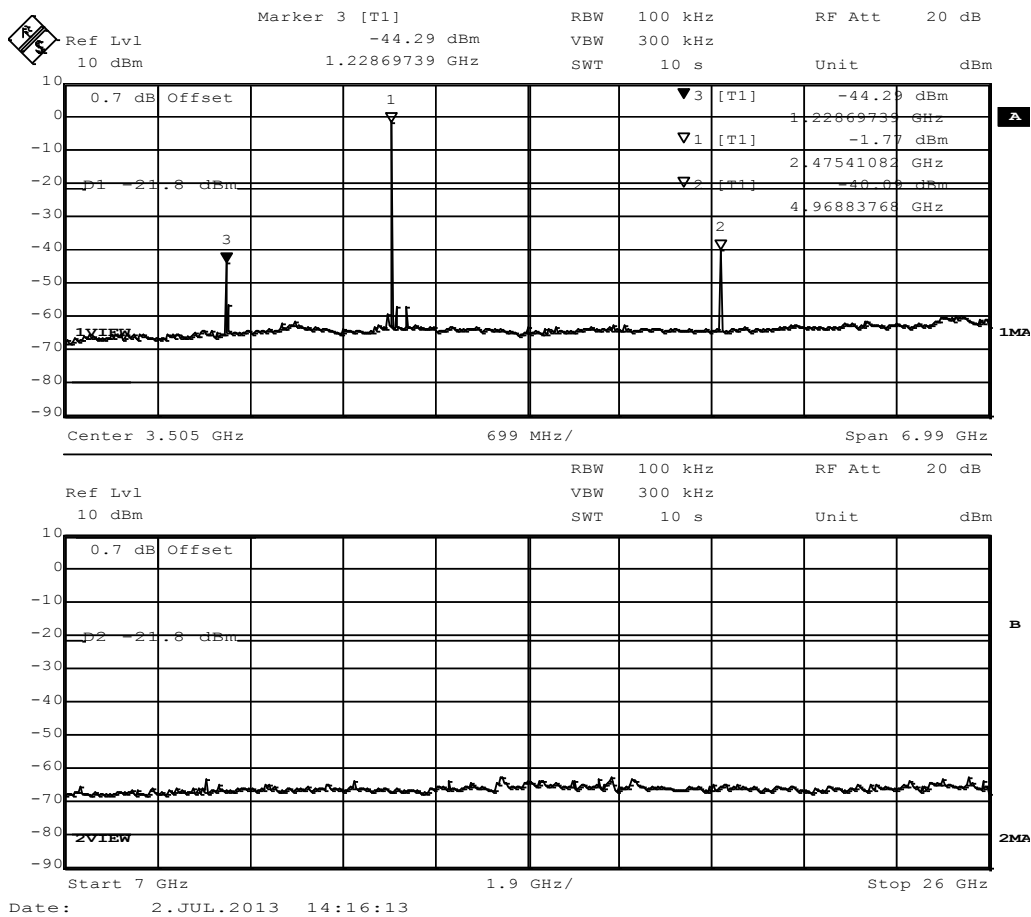

3.8 Test Conditions and Results – Transmitter radiated emissions

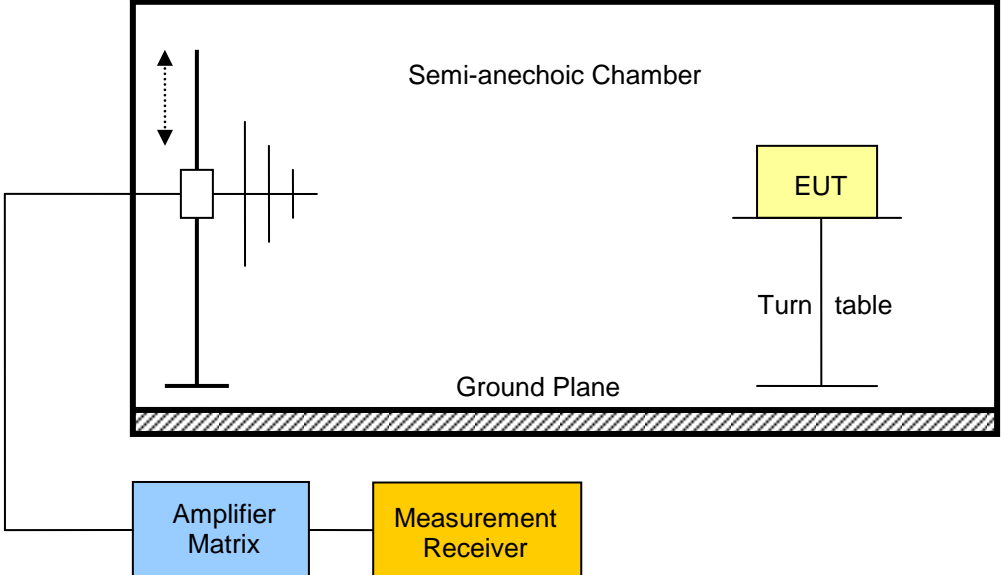Transmitter radiated emissions acc. FCC 47 CFR 15.247 / IC RSS-210				Verdict: PASS	
Test according referenced standards		Reference Method			
		FCC 15.247(d) / IC RSS-210 A8.5			
Test according to measurement reference		Reference Method			
		FCC KDB Publication No. 558074 / ANSI C63.4			
Test frequency range		Tested frequencies			
		30 MHz – 10 th Harmonic			
Limits					
Frequency range [MHz]	Detector	Limit [μ V/m]	Limit [dB μ V/m]	Limit Distance [m]	
30 – 88	Quasi-Peak	100	40	3	
88 – 216	Quasi-Peak	150	43.5	3	
216 – 960	Quasi-Peak	200	46	3	
960 – 1000	Quasi-Peak	500	54	3	
> 1000	Average	500	54	3	
<p>Radiated emissions which fall in the restricted bands, as defined in Section 15.205(a), must also comply with the radiated emission limits specified in Section 15.209(a) (see Section 15.205(c)).</p> <p>When average radiated emission measurements are specified, including average emission measurements below 1000 MHz, there also is a limit on the peak level of the radio frequency emissions. The limit on peak radio frequency emissions is 20 dB above the maximum permitted average emission limit applicable to the equipment under test.</p>					
Test setup					
 <p>The diagram illustrates the test setup. A Semi-anechoic Chamber is shown with a Ground Plane at the bottom. Inside the chamber, an Amplifier Matrix is connected to a Measurement Receiver. The EUT (Equipment Under Test) is placed on a Turn table. The chamber is labeled 'Semi-anechoic Chamber' and 'Ground Plane'.</p>					

Test procedure


1. EUT set to test mode (Communication tester is used if needed)
2. Span it set according to measurement range
3. Resolution bandwidth below 1 GHz is set according to CISPR 16 with peak/quasi-peak detector and RBW of 1 MHz with peak/average detector is used above 1 GHz
4. Markers are set to peak emission levels within restricted bands

Test results

Channel	Frequency [MHz]	Mode	Emission [MHz]	Level [dB μ V/m]	Det.	Pol.	Limit [dB μ V/m]	Limit dist. [m]*	Margin [dB]
F _{LOW}	2402	Transmit	37.804	31.02	pk	ver	40.00	3	-08.98
F _{LOW}	2402	Transmit	2336	37.94	pk	hor	74.00	3	-36.06
F _{LOW}	2402	Transmit	4804	54.81	pk	hor	74.00	3	-19.19
F _{LOW}	2402	Transmit	4804	53.00	avg	hor	54.00	3	-01.00
F _{LOW}	2402	Transmit	4804	52.68	pk	ver	74.00	3	-21.32
F _{LOW}	2402	Transmit	4804	50.31	avg	ver	54.00	3	-03.69
F _{MID}	2440	Transmit	4880	51.60	pk	ver	74.00	3	-22.40
F _{MID}	2440	Transmit	4880	48.82	avg	ver	54.00	3	-05.18
F _{HIGH}	2480	Transmit	2483.5	46.20	pk	hor	74.00	3	-27.80

Comments:

3.9 Test Conditions and Results – Receiver radiated emissions

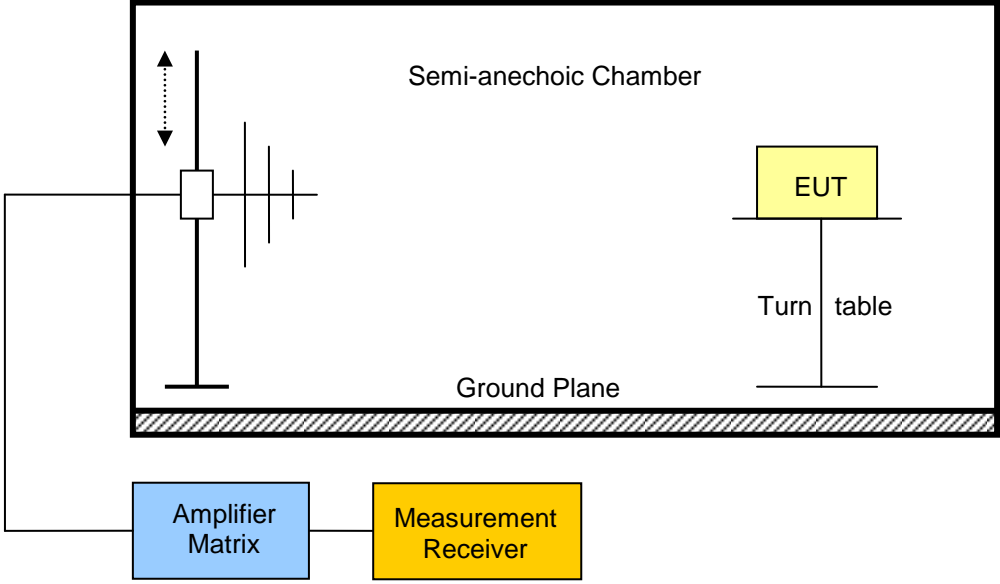Receiver radiated emissions acc. IC RSS-210			Verdict: PASS	
Test according referenced standards	Reference Method			
	IC RSS-210 A8.5			
Test according to measurement reference	Reference Method			
	ANSI C63.4			
Test frequency range	Tested frequencies			
	30 MHz – 3 th Harmonic			
EUT test mode	Receive			
Limits				
Frequency range [MHz]	Detector	Limit [$\mu\text{V}/\text{m}$]	Limit [$\text{dB}\mu\text{V}/\text{m}$]	Limit Distance [m]
30 – 88	Quasi-Peak	100	40	3
88 – 216	Quasi-Peak	150	43.5	3
216 – 960	Quasi-Peak	200	46	3
960 – 1000	Quasi-Peak	500	54	3
> 1000	Average	500	54	3
Test setup				
				

Test procedure

1. EUT set to receive mode (Communication tester is used if needed)
2. Span it set according to measurement range
3. Resolution bandwidth below 1 GHz is set according to CISPR 16 with peak/quasi-peak detector and RBW of 1 MHz with peak/average detector is used above 1 GHz
4. Markers are set to peak emission levels

Test results

Channel	Frequency [MHz]	Emission [MHz]	Emission Level [db μ V/m]	Emission Level [μ V/m]	Det.	Limit [μ V/m]	Margin [μ V/m]
F _{MID}	2440	32.715	31.65	38.24	pk	100	-61.76
F _{MID}	2440	59.86	34.24	51.52	pk	100	-48.48
F _{MID}	2440	551.297	27.33	23.25	pk	200	-176.75
F _{MID}	2440	575.25	26.43	20.97	pk	200	-179.03

Comments:

* Physical distance between EUT and measurement antenna.

** Emission level corresponds to ambient noise floor


ANNEX A Transmitter radiated spurious emissions

Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Rohde & Schwarz HK 116, Horizontal
Measurement distance:	3 m
Mode:	TX; ch. 0
Test Date:	2013-07-03
Note:	worst case

Index 74

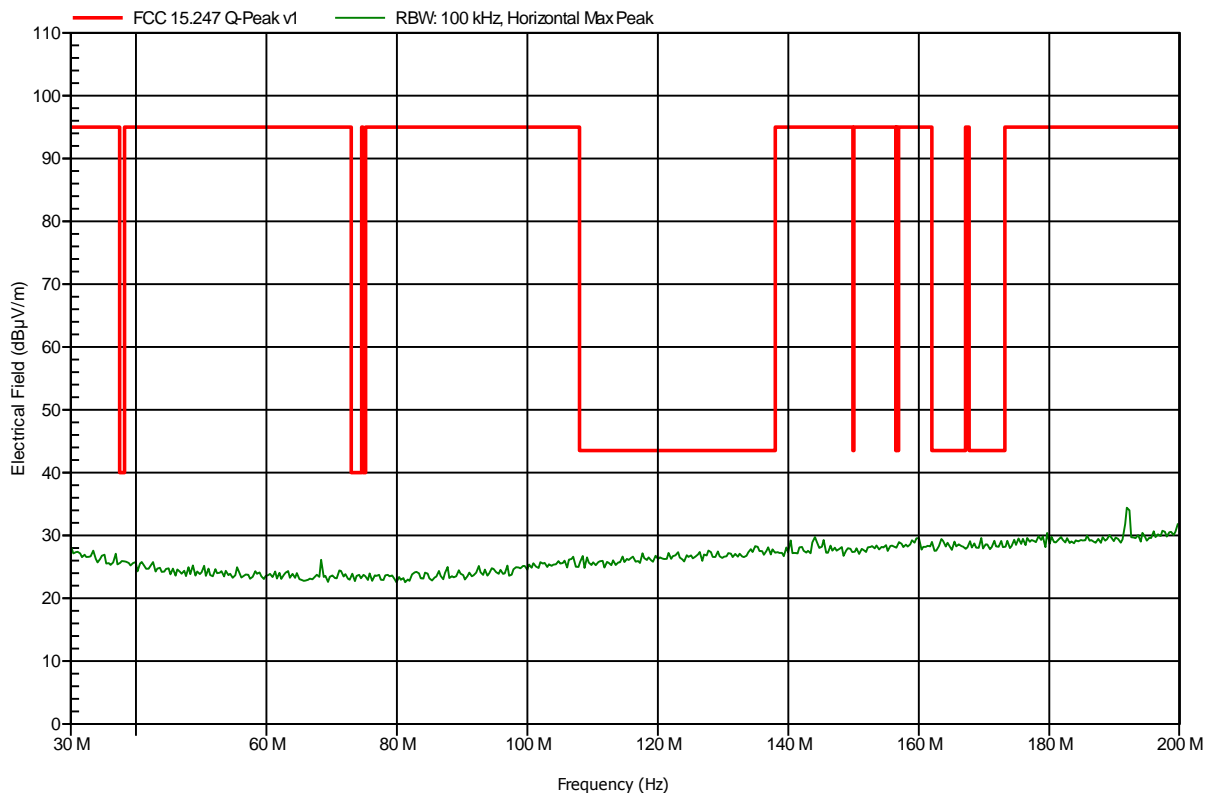


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HK 116, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note: worst case

Index 75

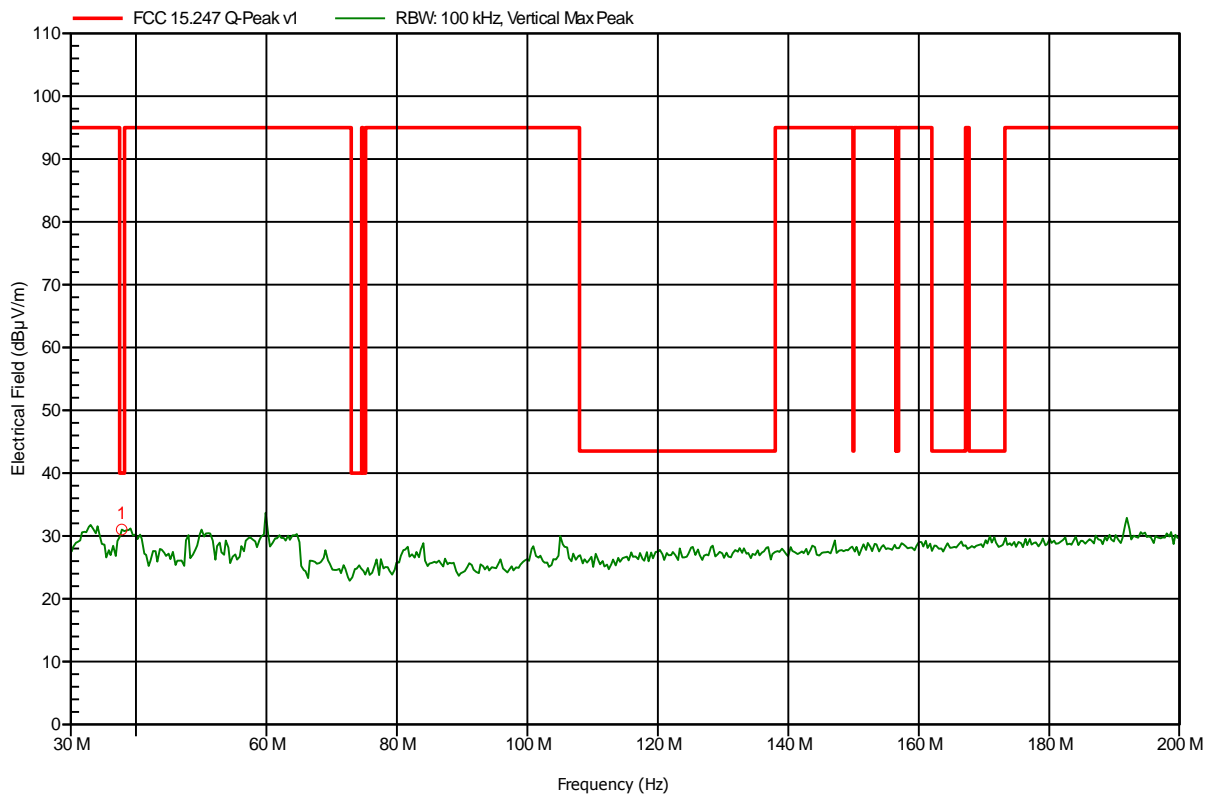


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
37.804 MHz	31.02 dBµV/m	40 dBµV/m	-8.98 dB	Pass

Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Rohde & Schwarz HL 223, Horizontal
Measurement distance:	3 m
Mode:	TX; ch. 0
Test Date:	2013-07-03
Note:	

Index 71

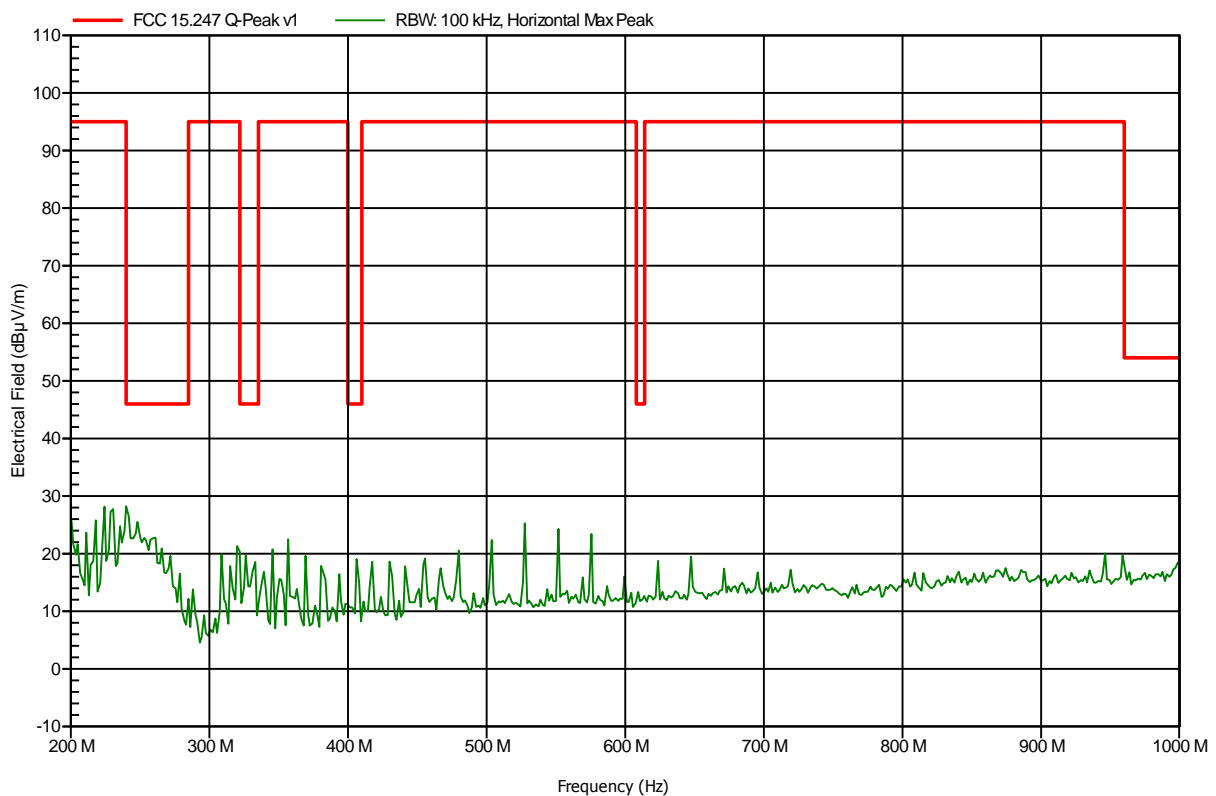


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Rohde & Schwarz HL 223, Vertical
Measurement distance:	3 m
Mode:	TX; ch. 0
Test Date:	2013-07-03
Note:	

Index 68

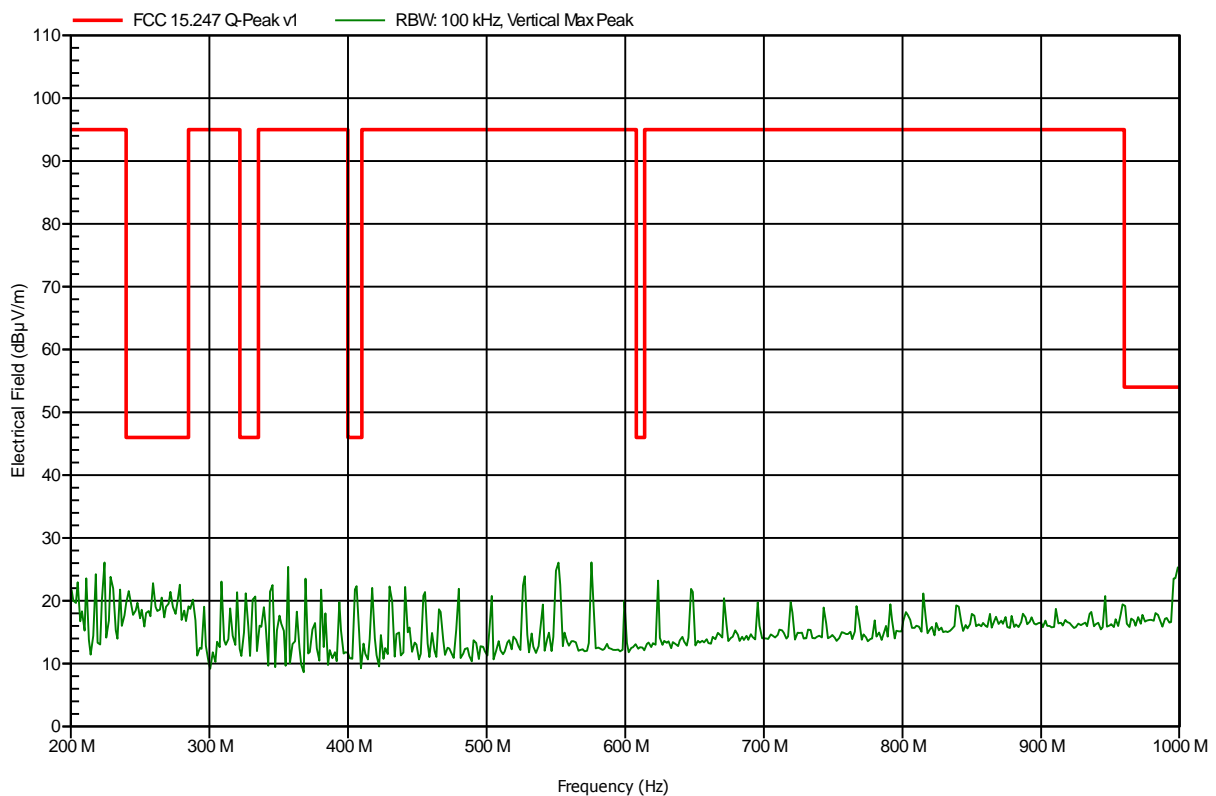


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 41

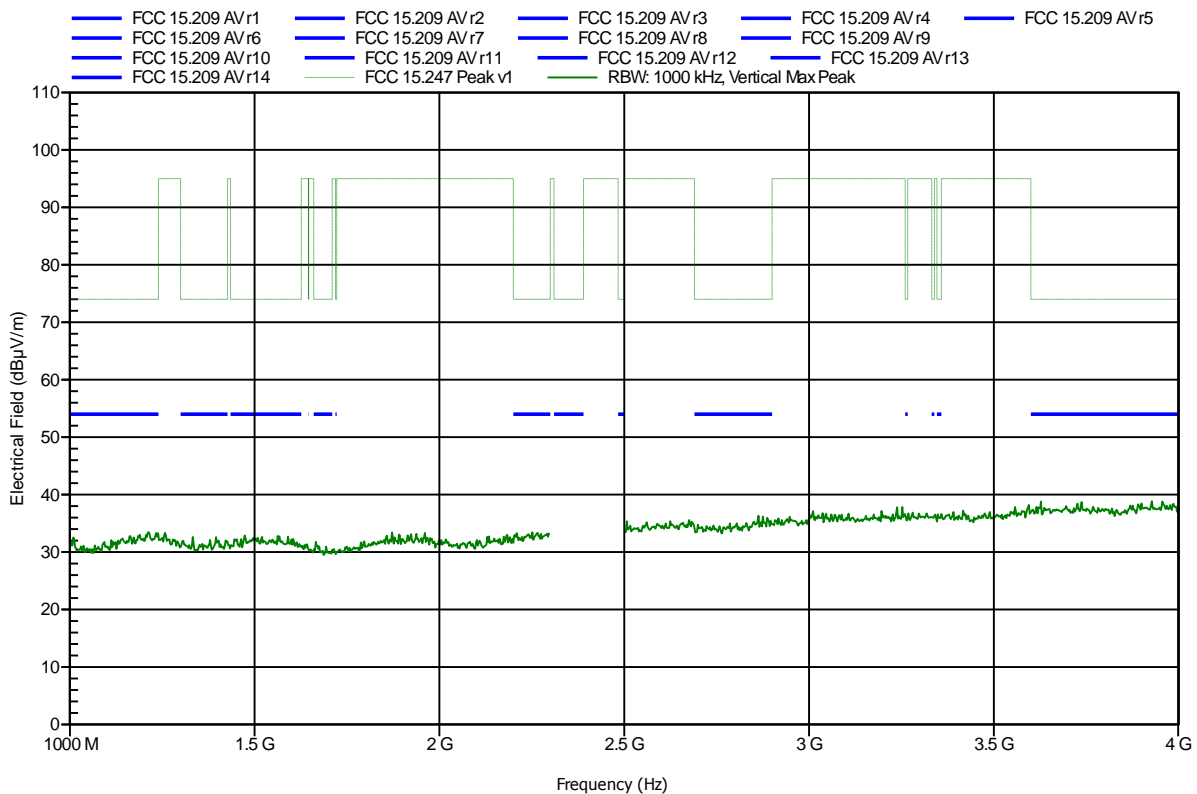


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 38

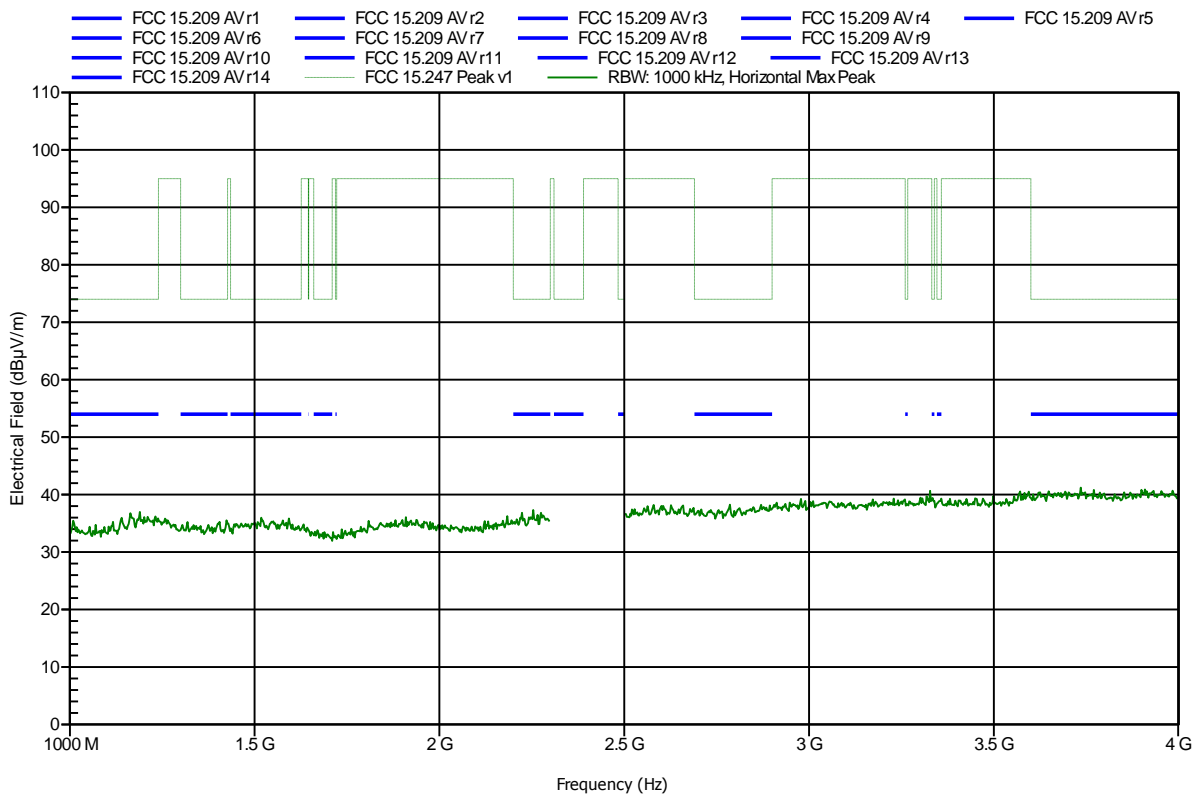


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note: lower bandedge

Index 39

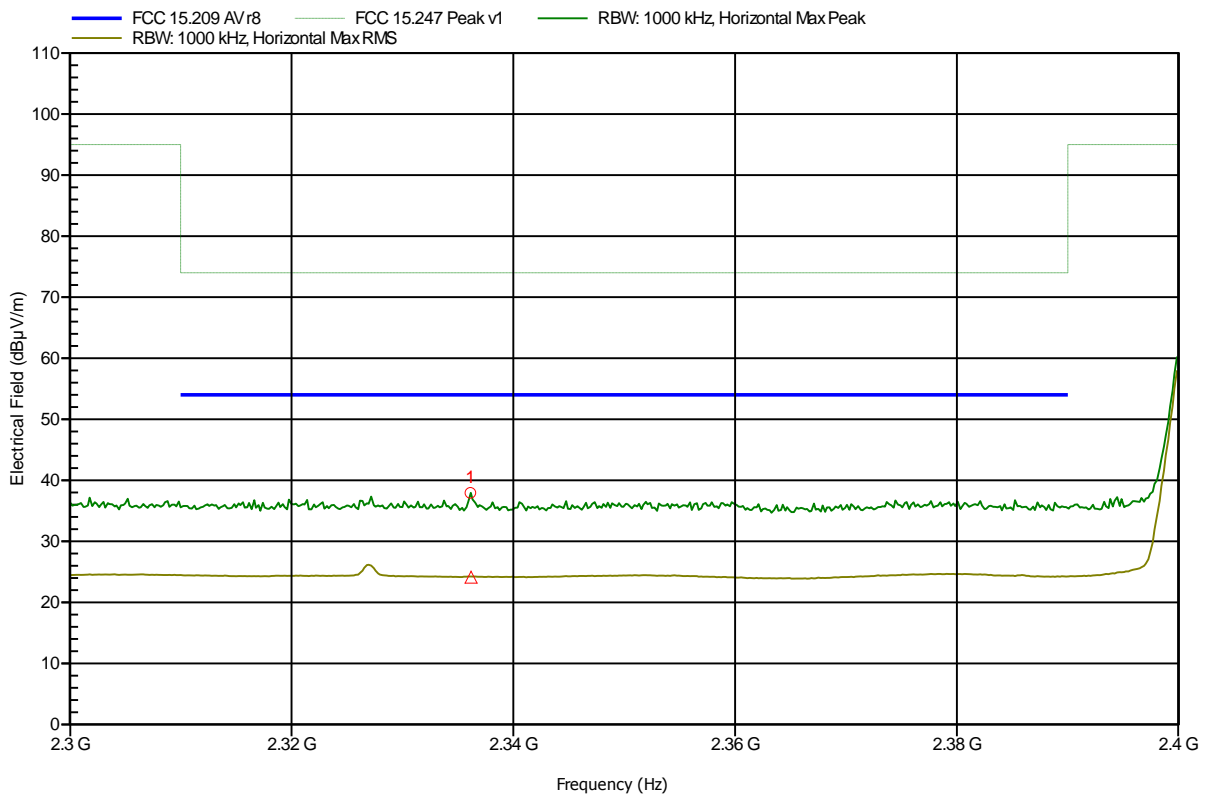


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
2.336 GHz	37.94 dBµV/m	74 dBµV/m	-36.06 dB	Pass

Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	3 m
Mode:	TX; ch. 0
Test Date:	2013-07-03
Note:	lower bandedge

Index 42

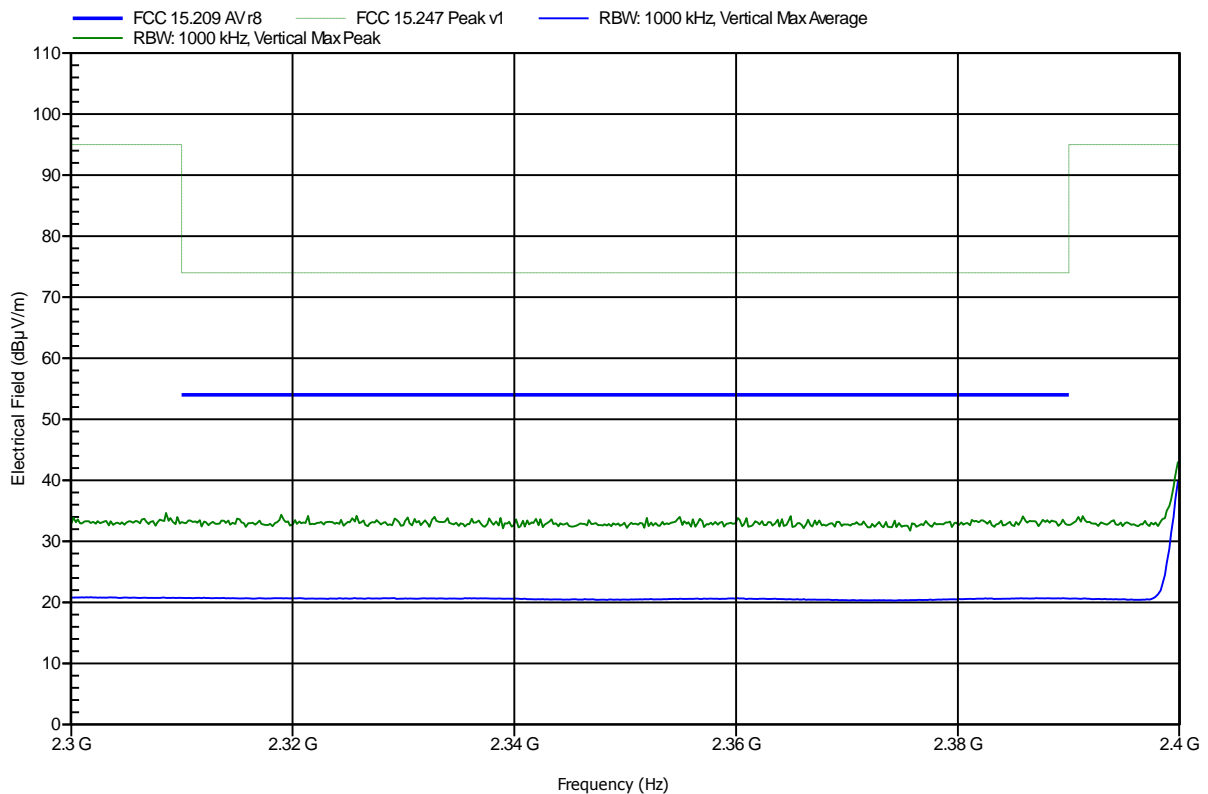


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 40

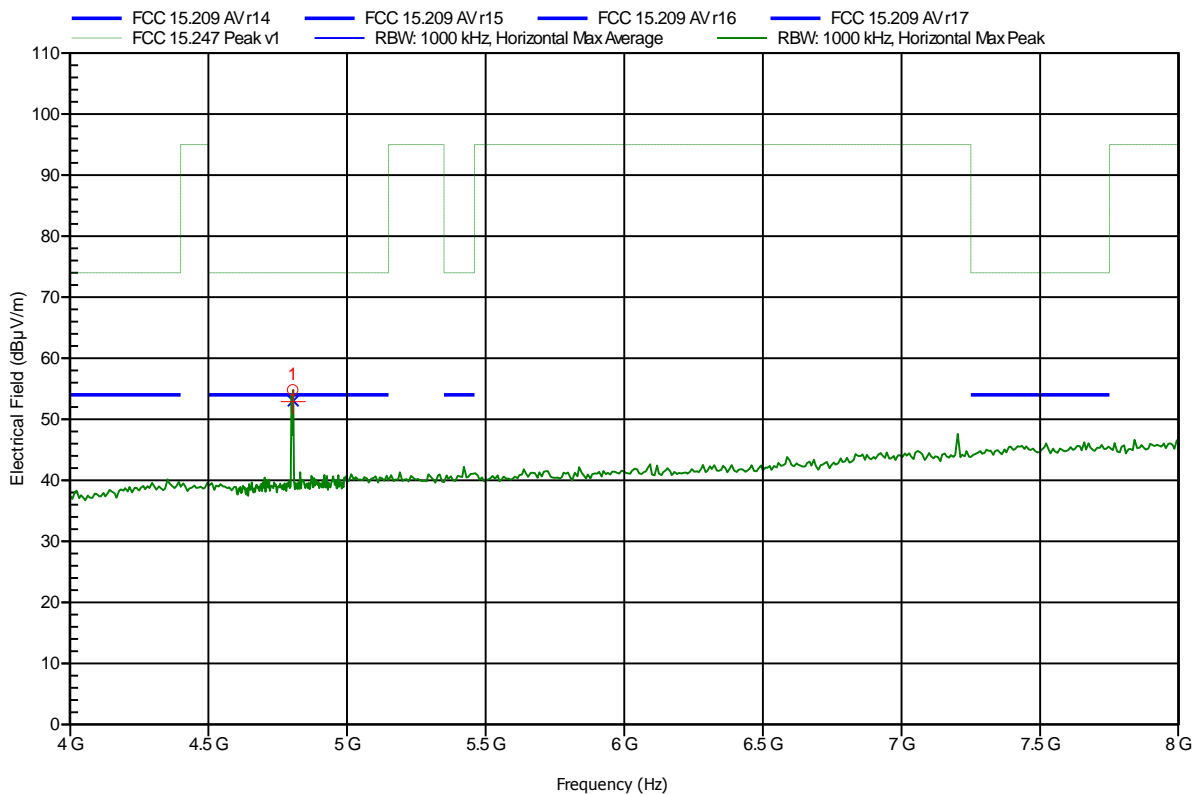


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
4.804 GHz	54.81 dBµV/m	74 dBµV/m	-19.19 dB	Pass
Frequency	Average	Average Limit	Average Difference	Average Status
4.804 GHz	53 dBµV/m	54 dBµV/m	-1 dB	Pass

Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 43

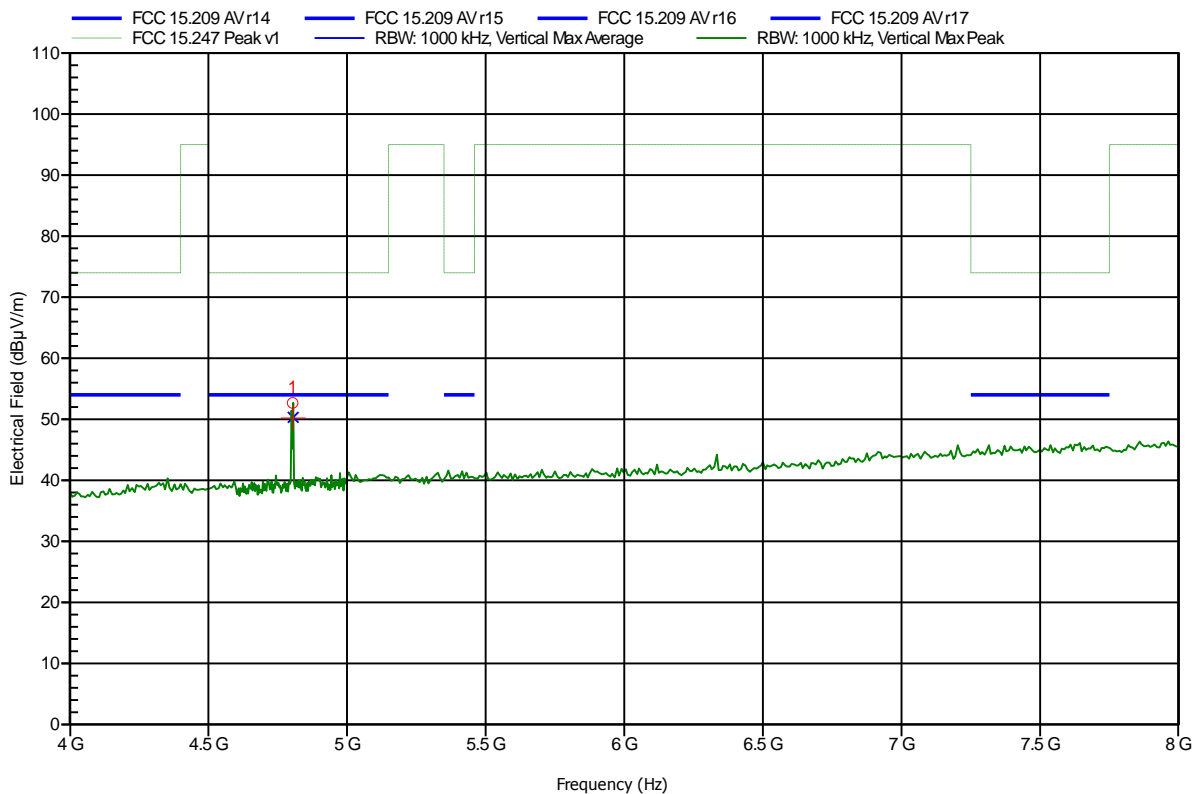


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
4.804 GHz	52.68 dBµV/m	74 dBµV/m	-21.32 dB	Pass
Frequency	Average	Average Limit	Average Difference	Average Status
4.804 GHz	50.31 dBµV/m	54 dBµV/m	-3.69 dB	Pass

Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 100 cm converted to 3m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 54

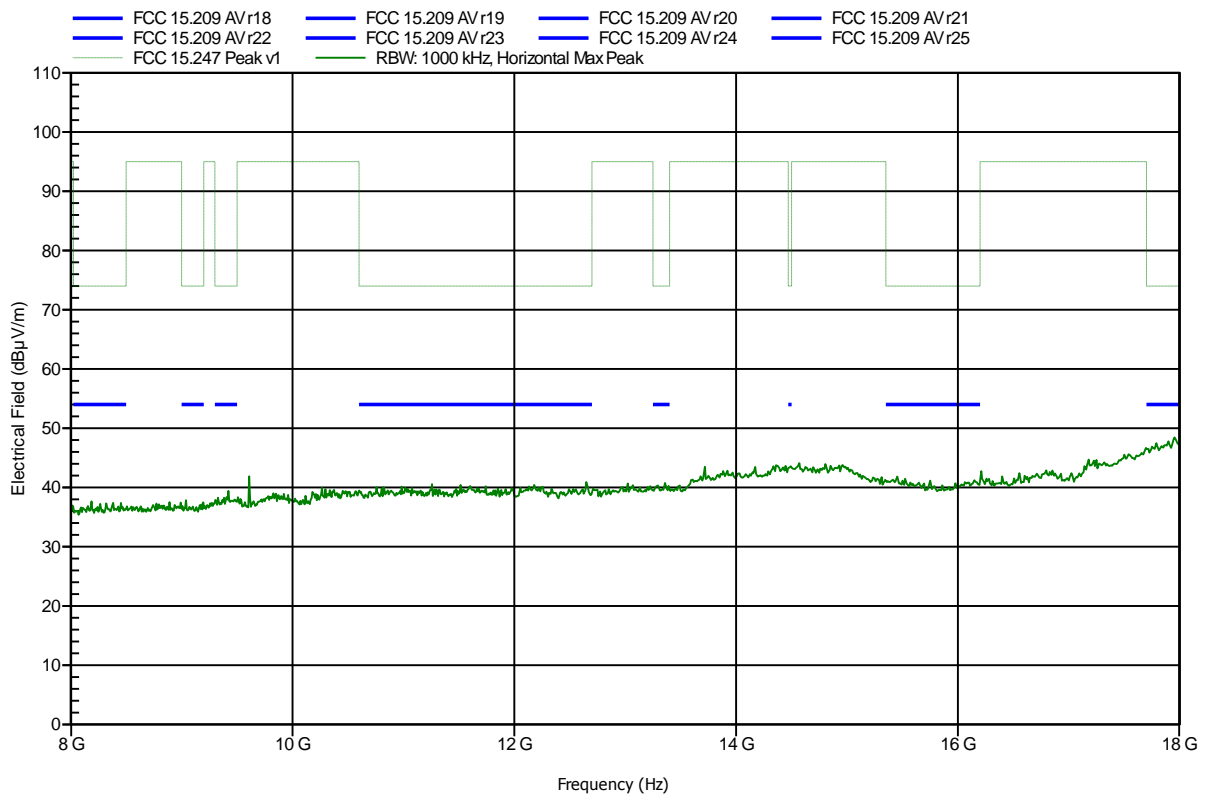


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 100 cm converted to 3m
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 56

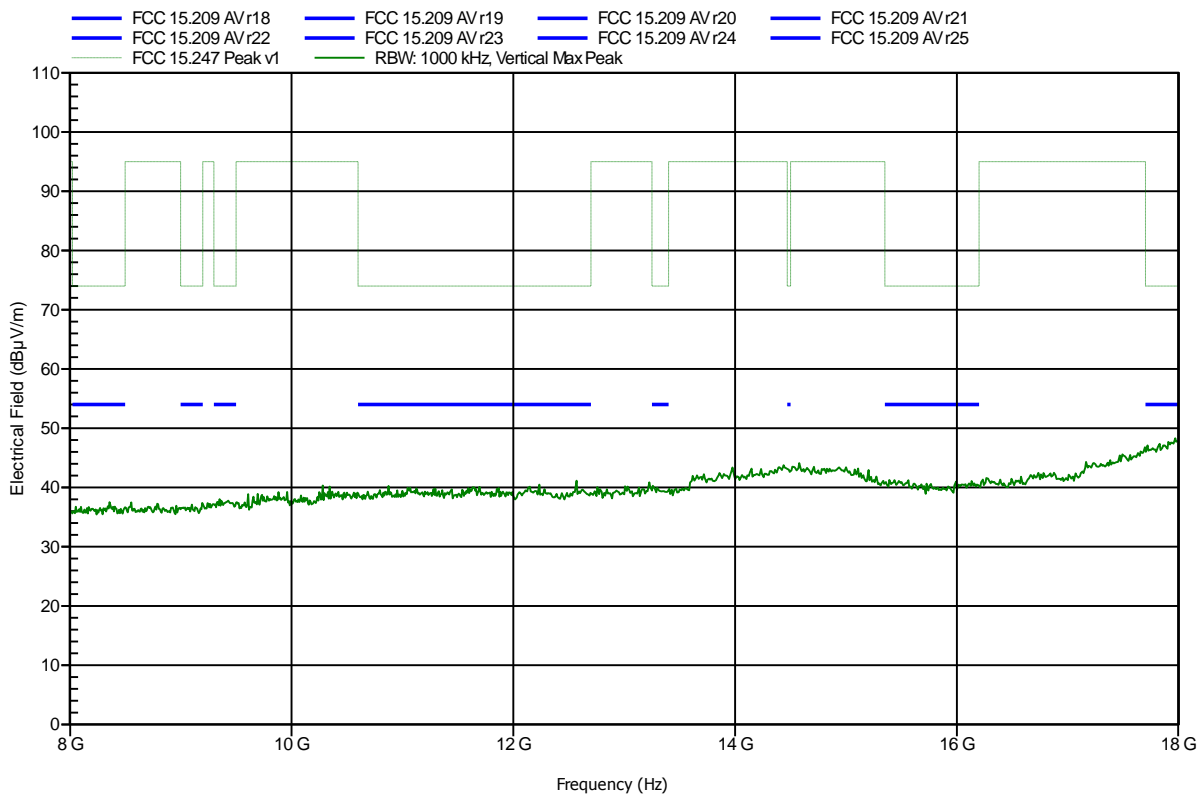


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 025, Horizontal
 Measurement distance: 100 cm
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 55

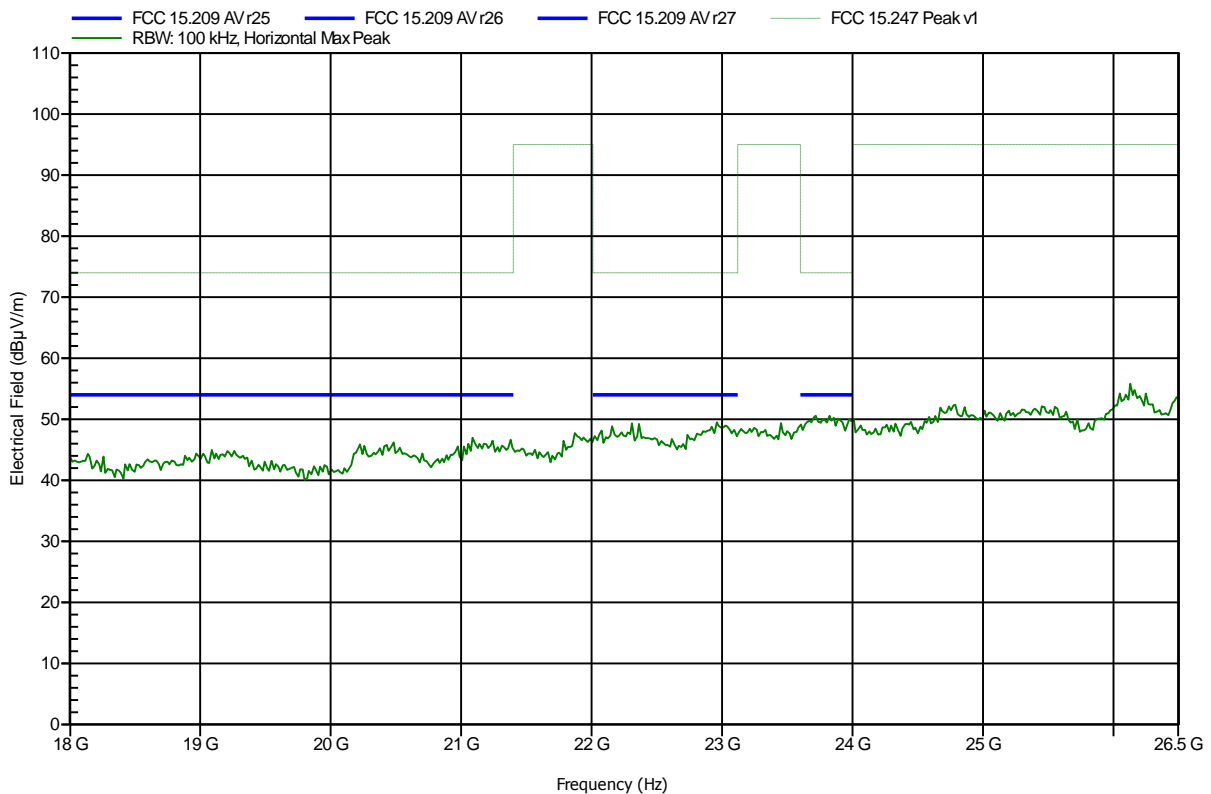


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 025, Vertical
 Measurement distance: 100 cm
 Mode: TX; ch. 0
 Test Date: 2013-07-03
 Note:

Index 57

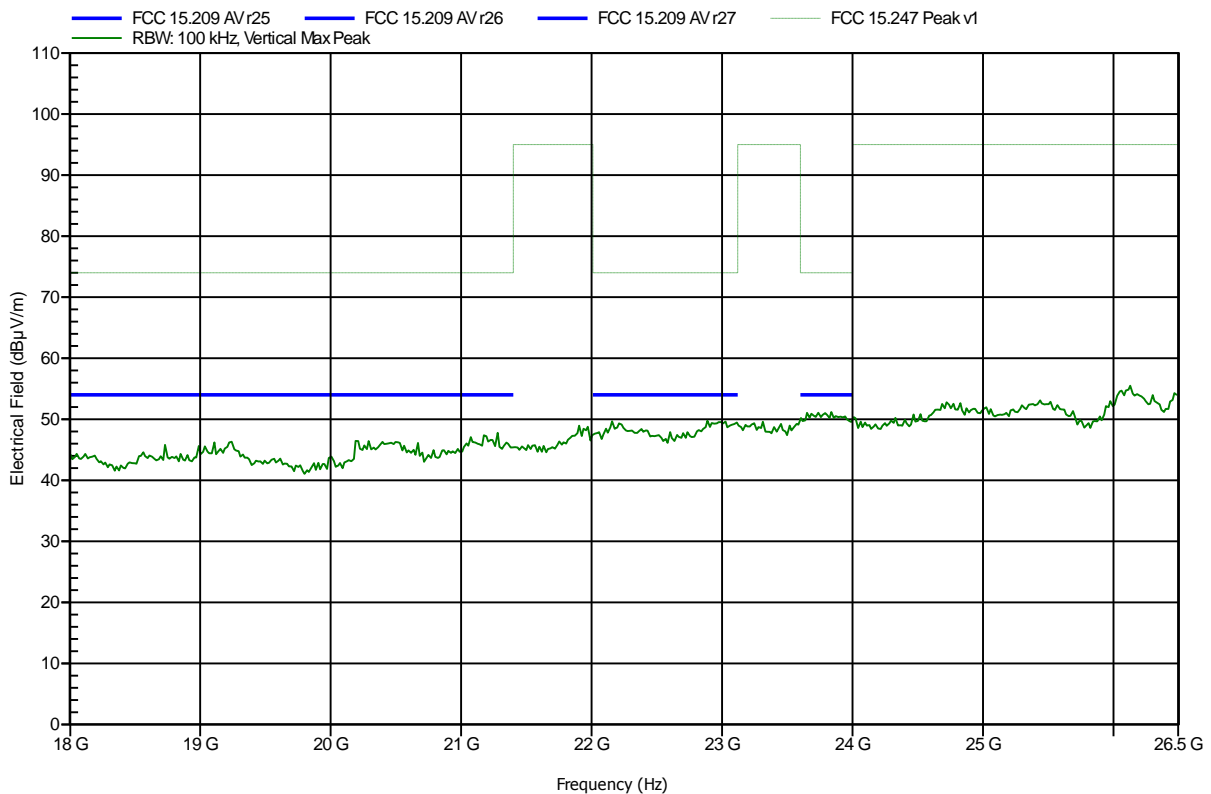


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Rohde & Schwarz HL 223, Horizontal
Measurement distance:	3 m
Mode:	TX; ch. 19
Test Date:	2013-07-03
Note:	

Index 70

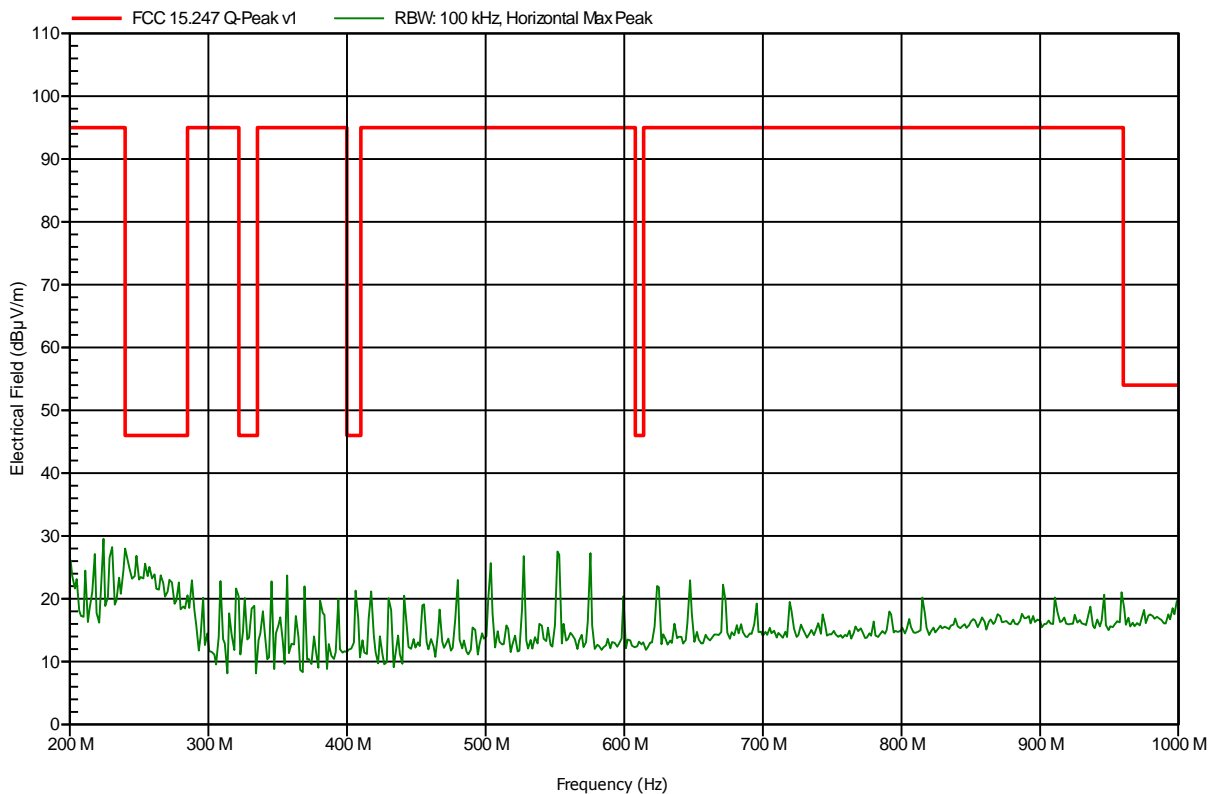


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Rohde & Schwarz HL 223, Vertical
Measurement distance:	3 m
Mode:	TX; ch. 19
Test Date:	2013-07-03
Note:	

Index 69

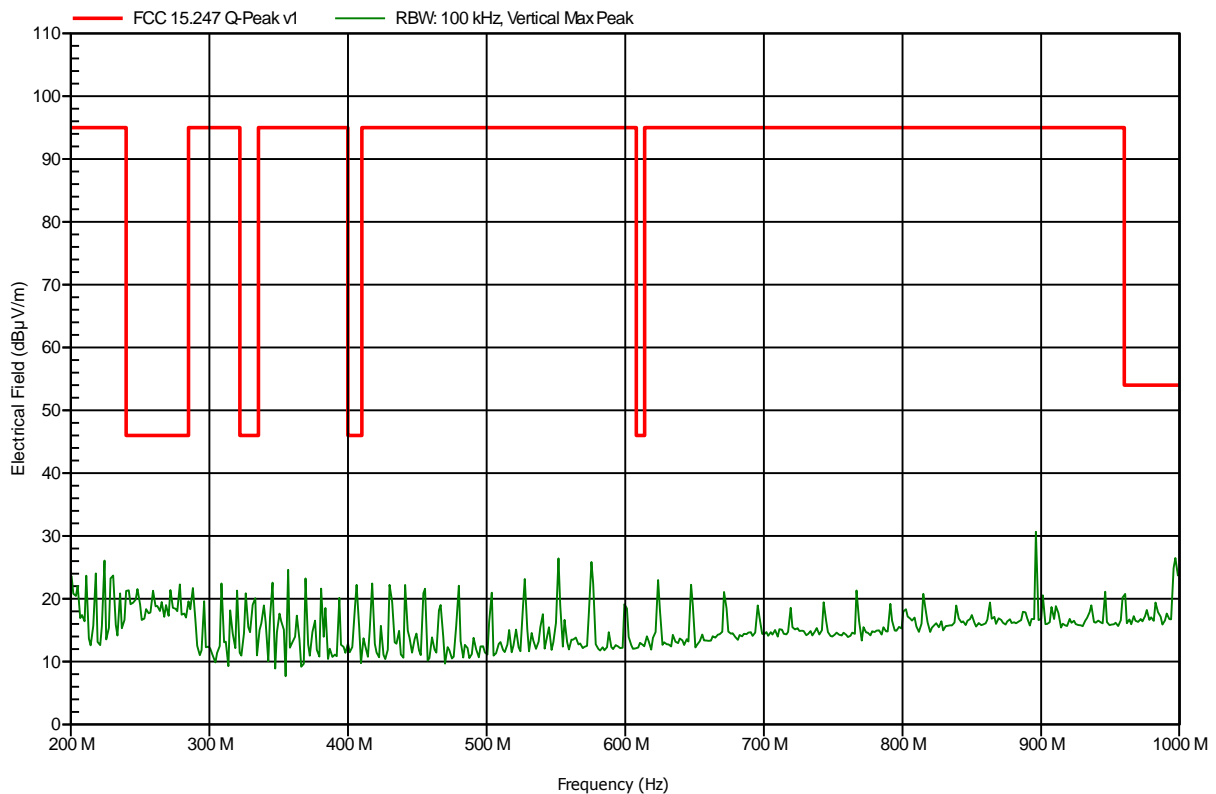


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 44

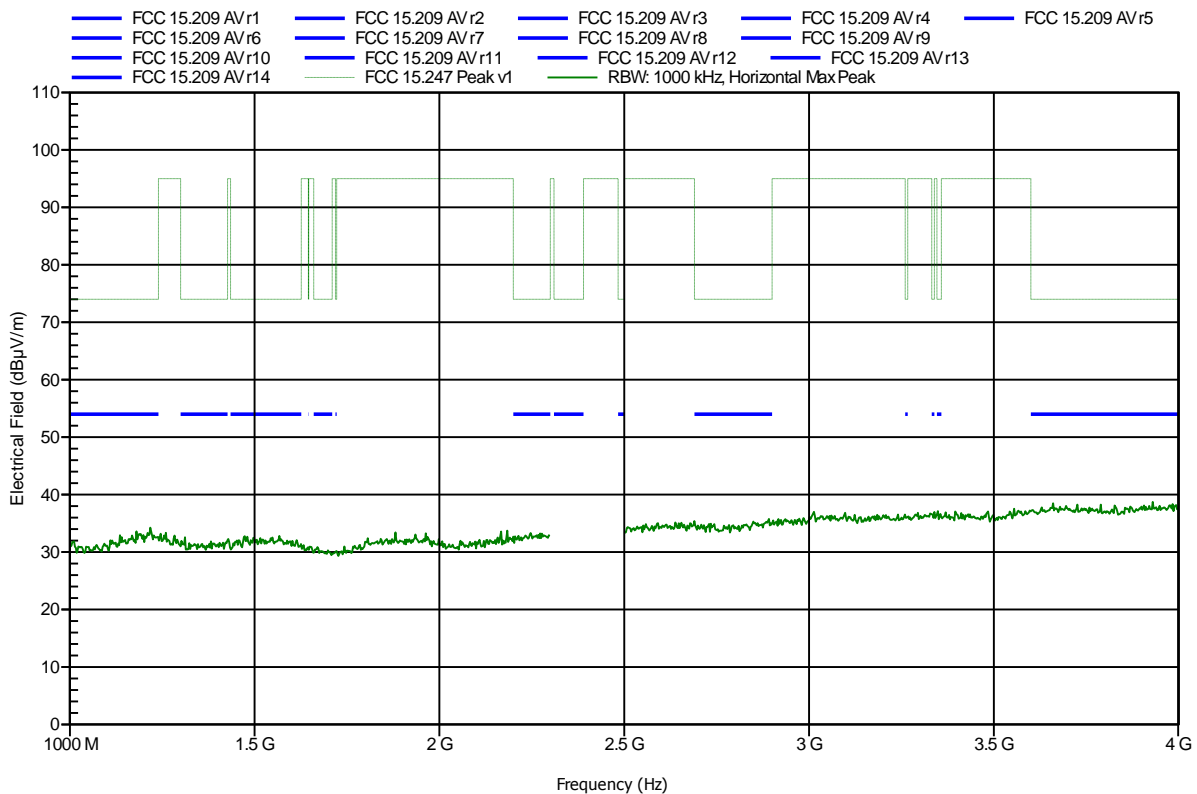


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 46

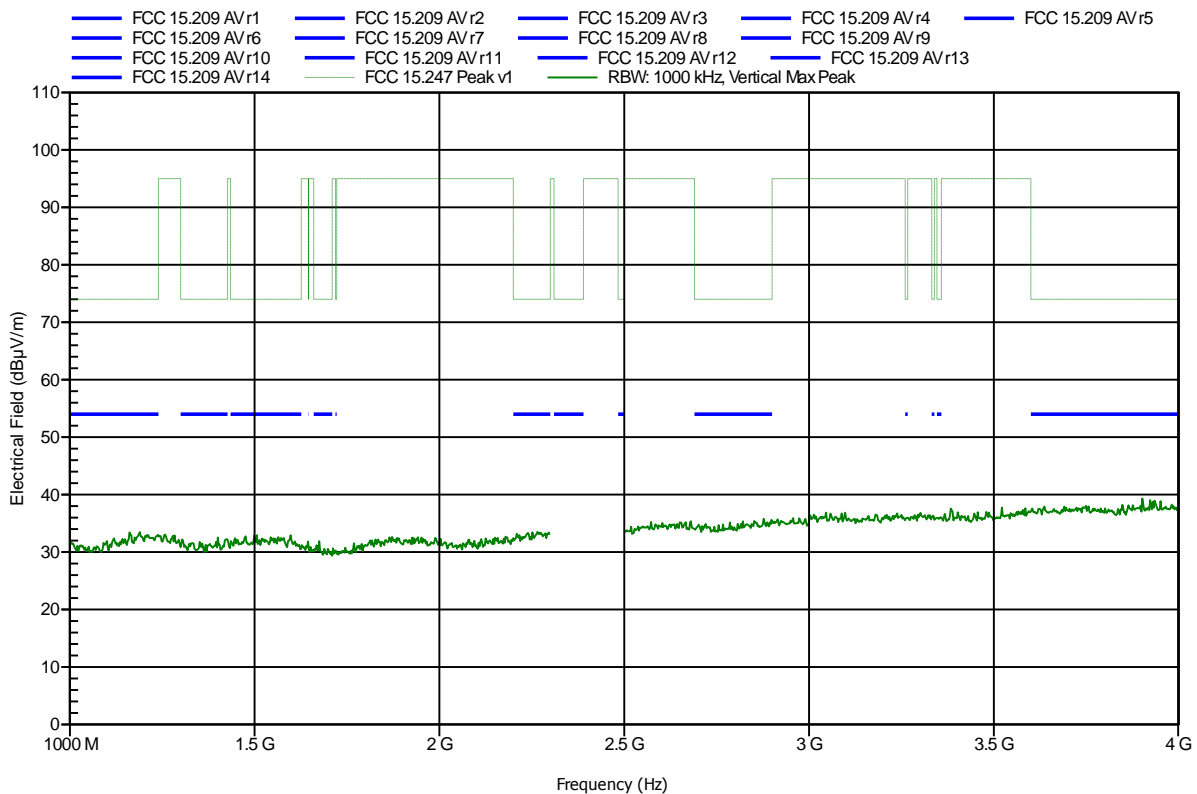


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 45

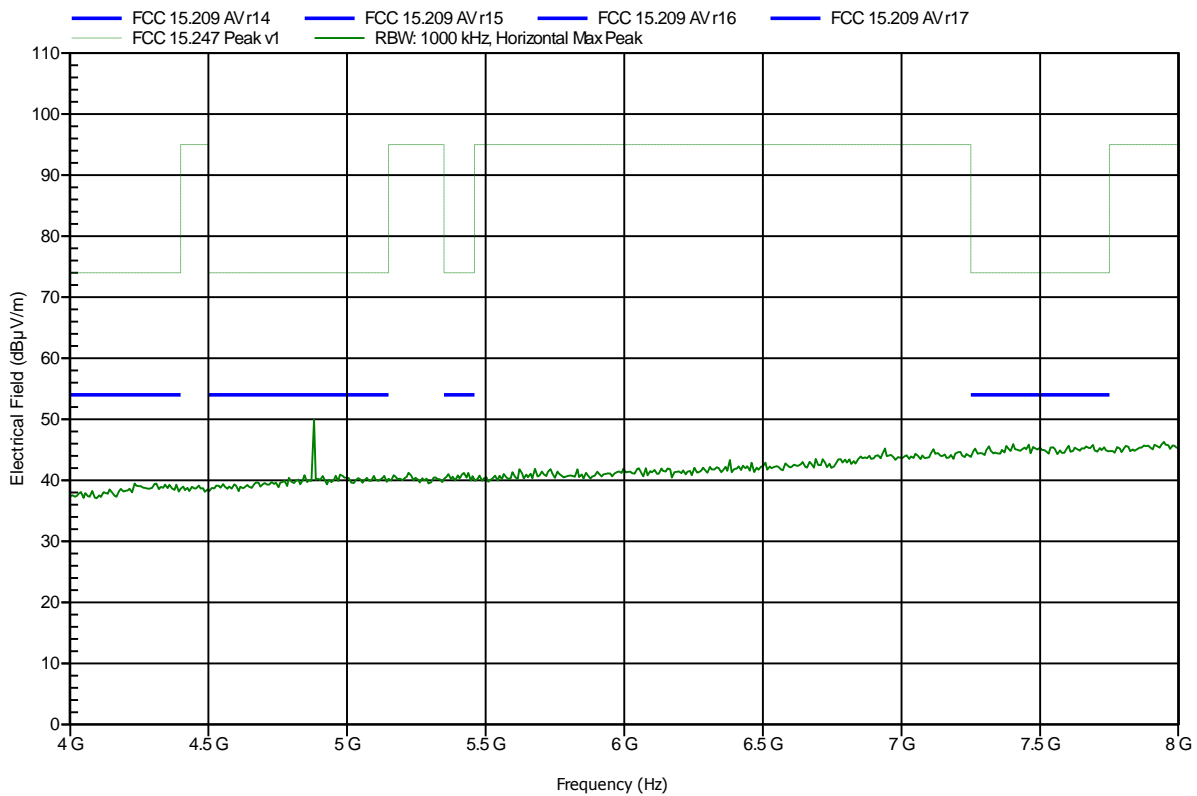


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 47

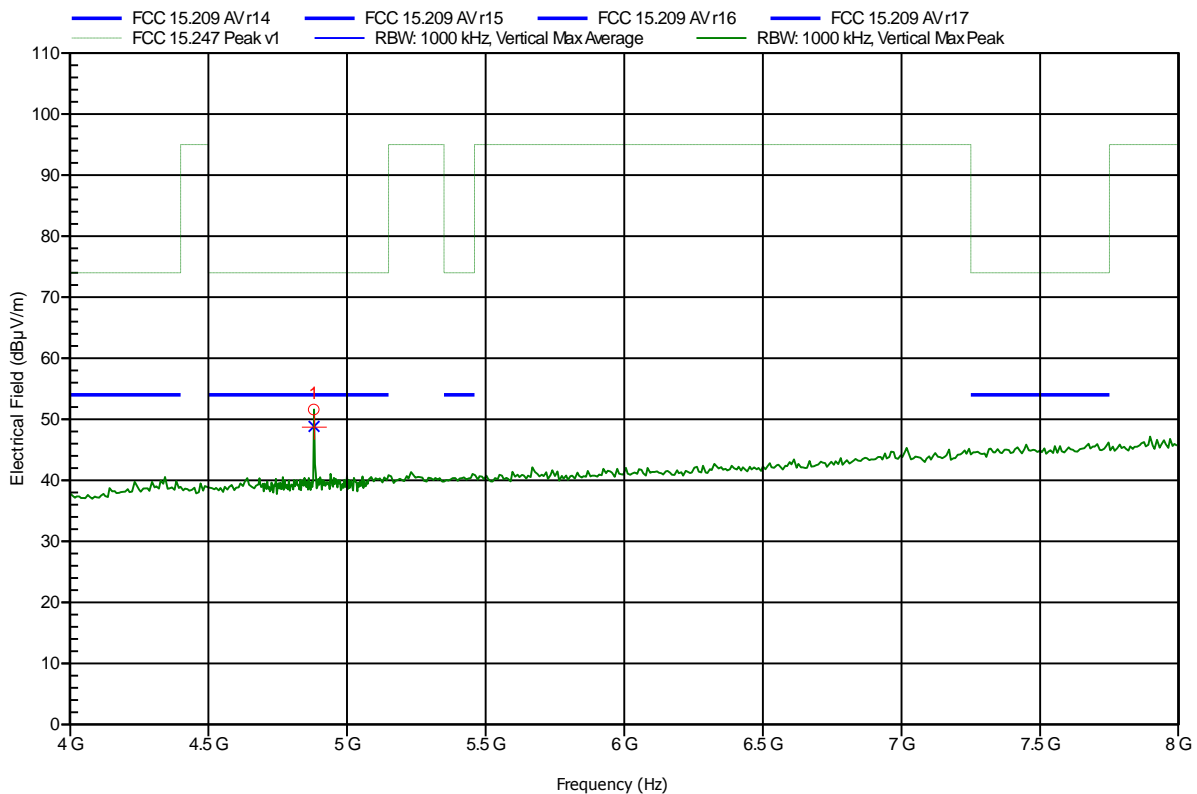


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
4.88 GHz	51.6 dBµV/m	74 dBµV/m	-22.4 dB	Pass
Frequency	Average	Average Limit	Average Difference	Average Status
4.88 GHz	48.82 dBµV/m	54 dBµV/m	-5.18 dB	Pass

Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 100 cm converted to 3m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 58

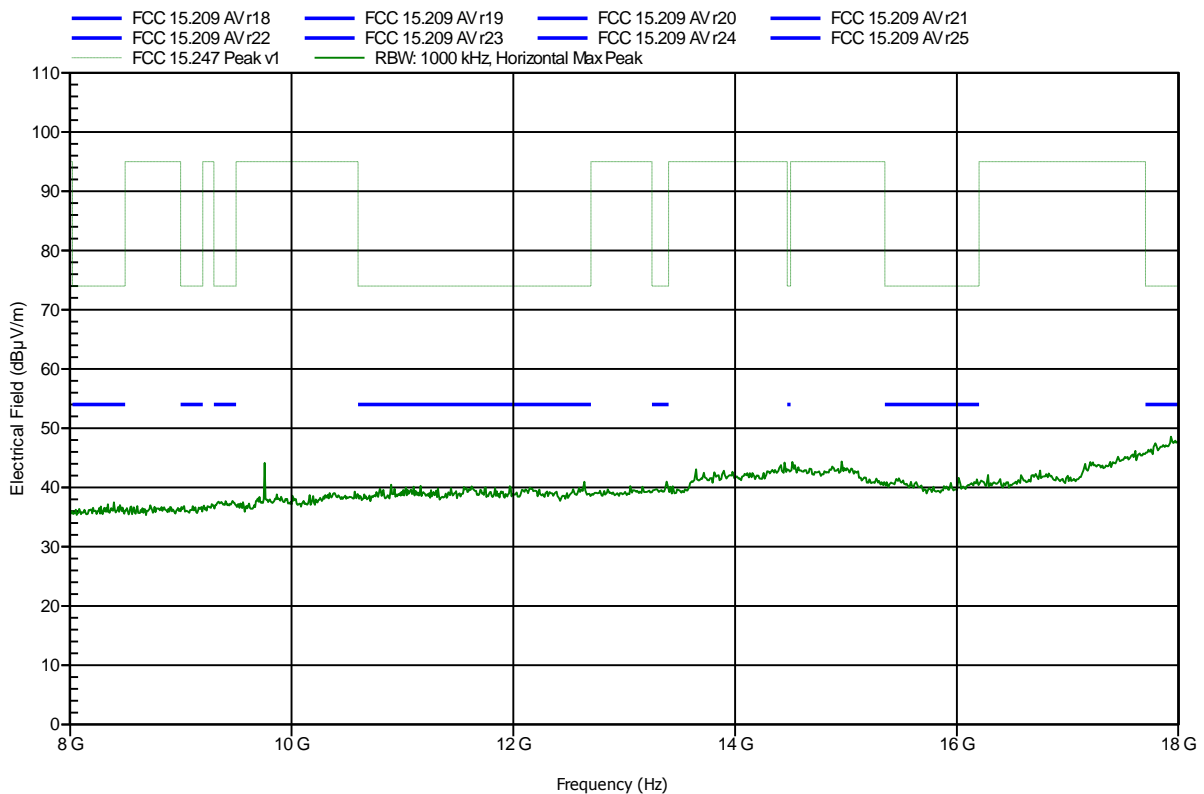


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 100 cm converted to 3m
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 61

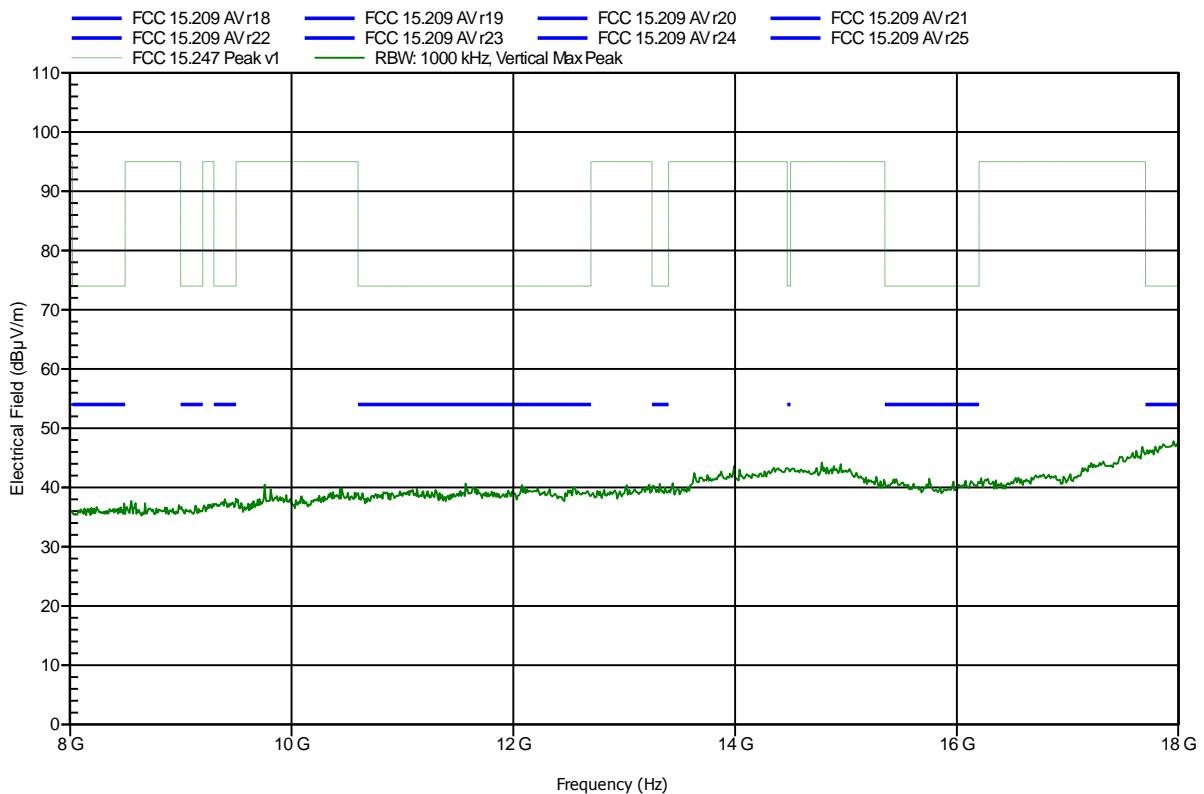


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 025, Horizontal
 Measurement distance: 100 cm
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 59

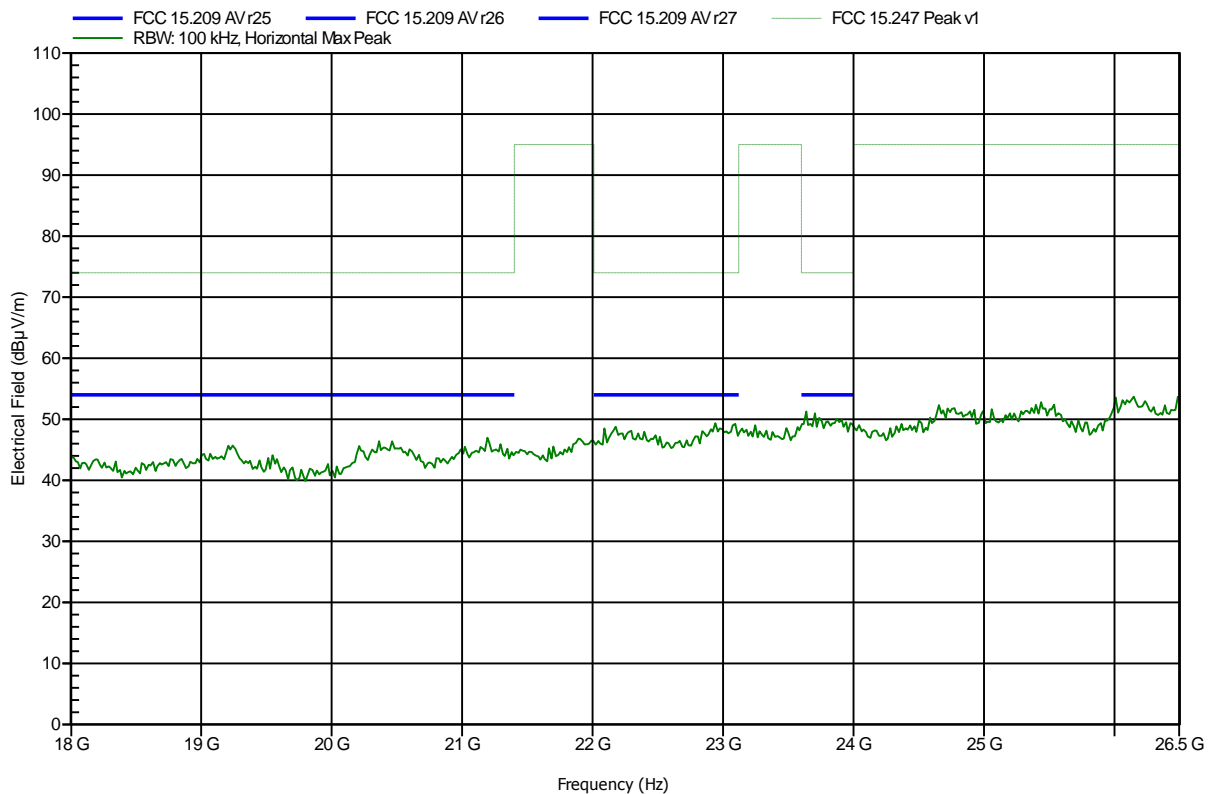


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 025, Vertical
 Measurement distance: 100 cm
 Mode: TX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 62

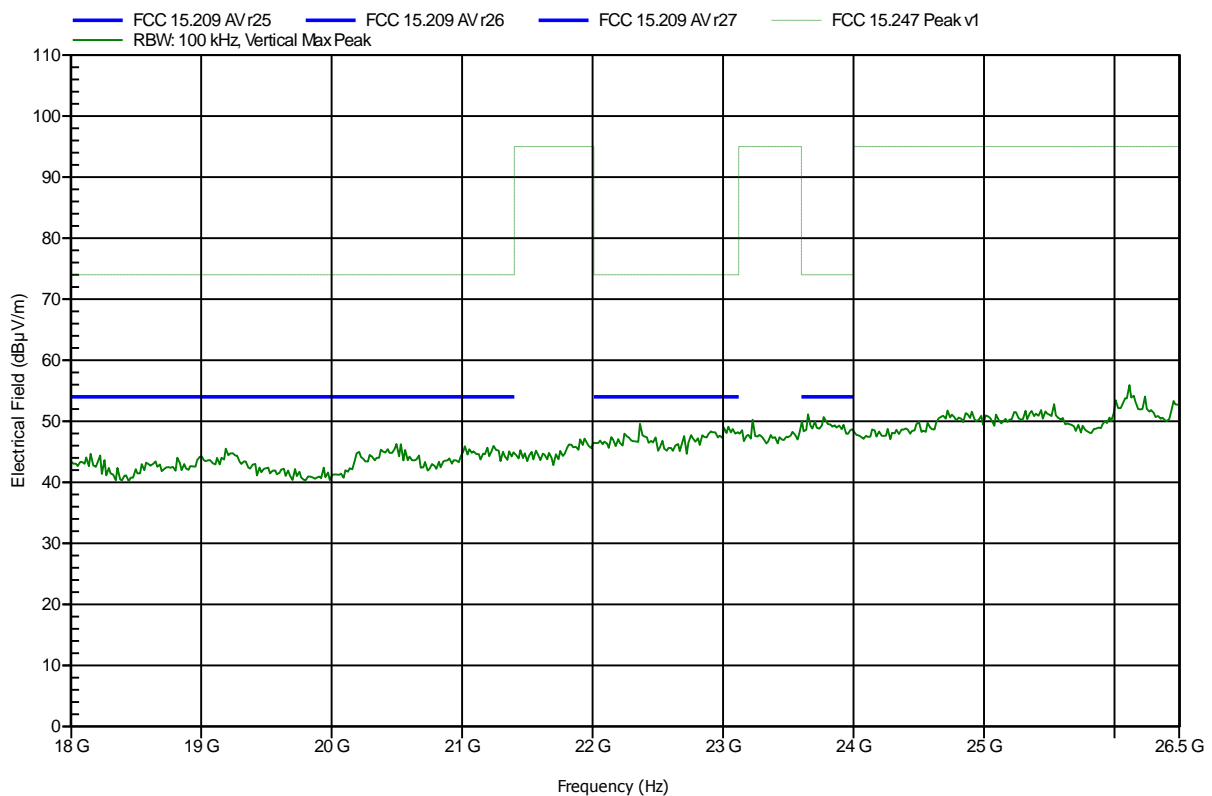


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Rohde & Schwarz HL 223, Horizontal
Measurement distance:	3 m
Mode:	TX; ch. 39
Test Date:	2013-07-03
Note:	

Index 72

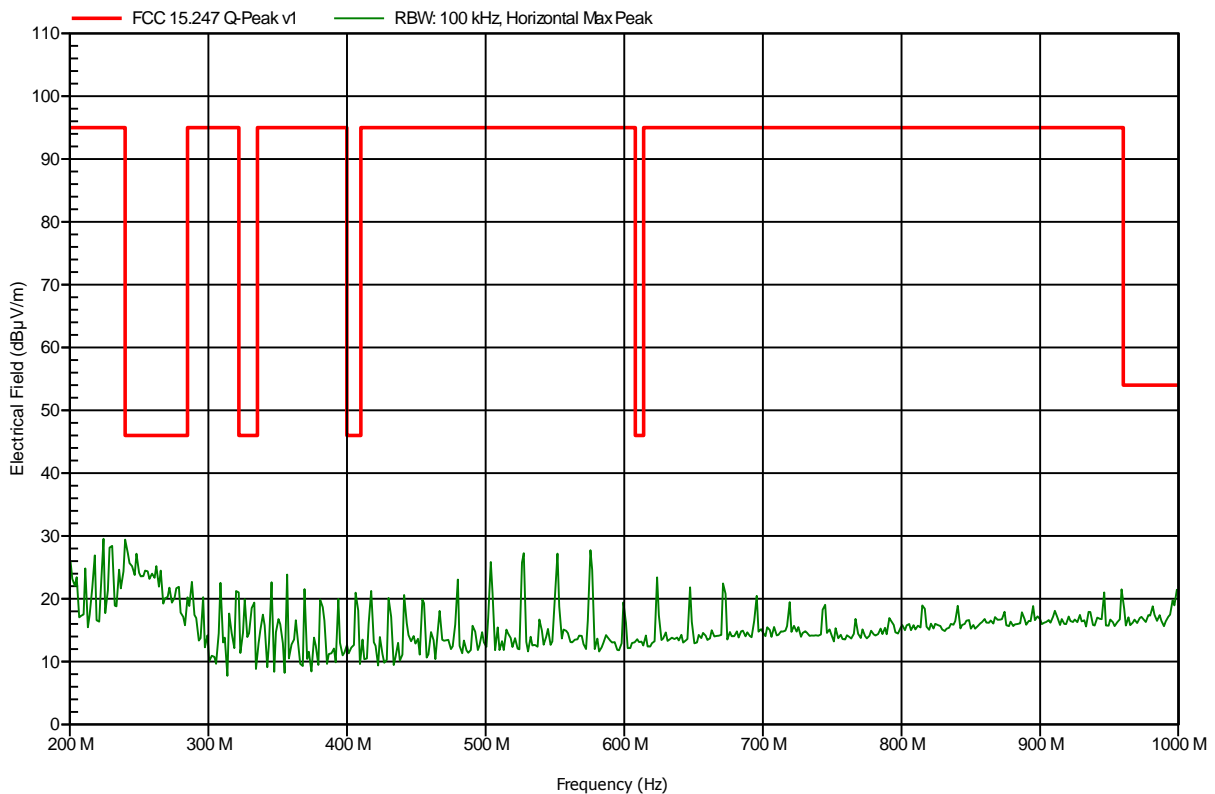


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Rohde & Schwarz HL 223, Vertical
Measurement distance:	3 m
Mode:	TX; ch. 39
Test Date:	2013-07-03
Note:	

Index 73

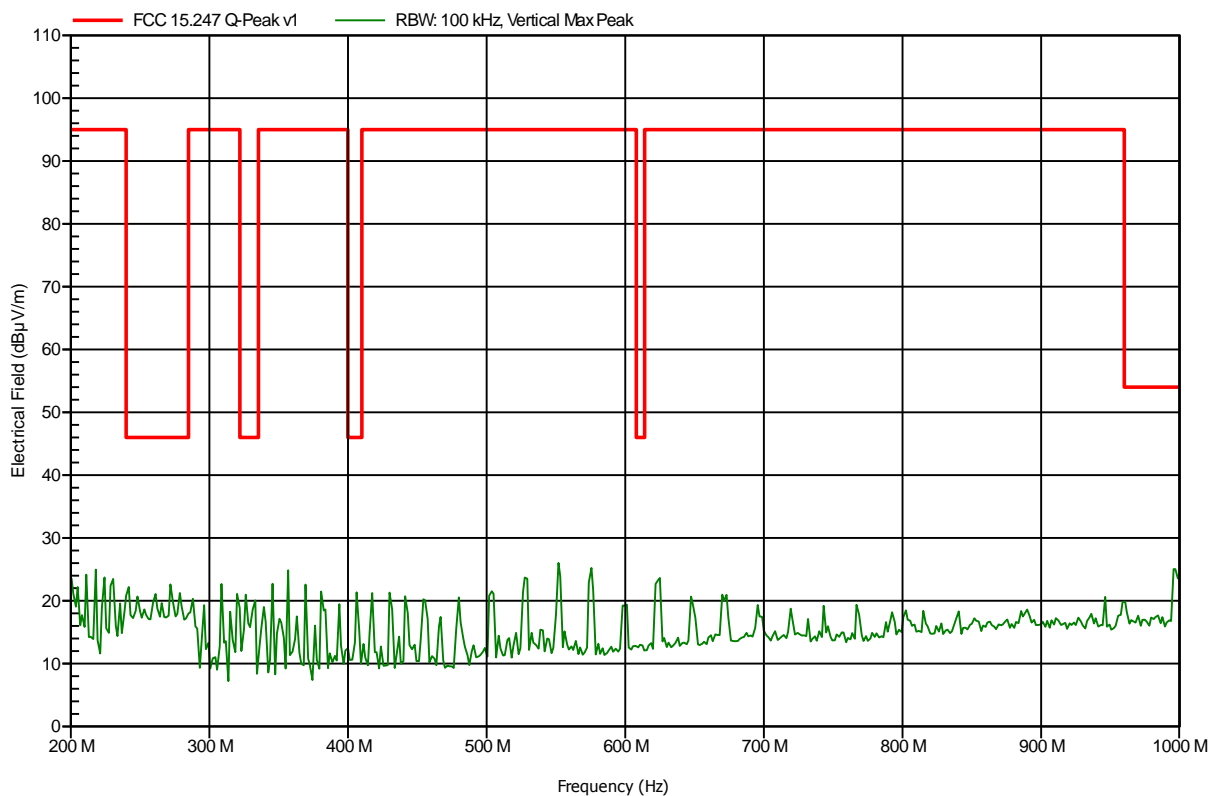


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 48

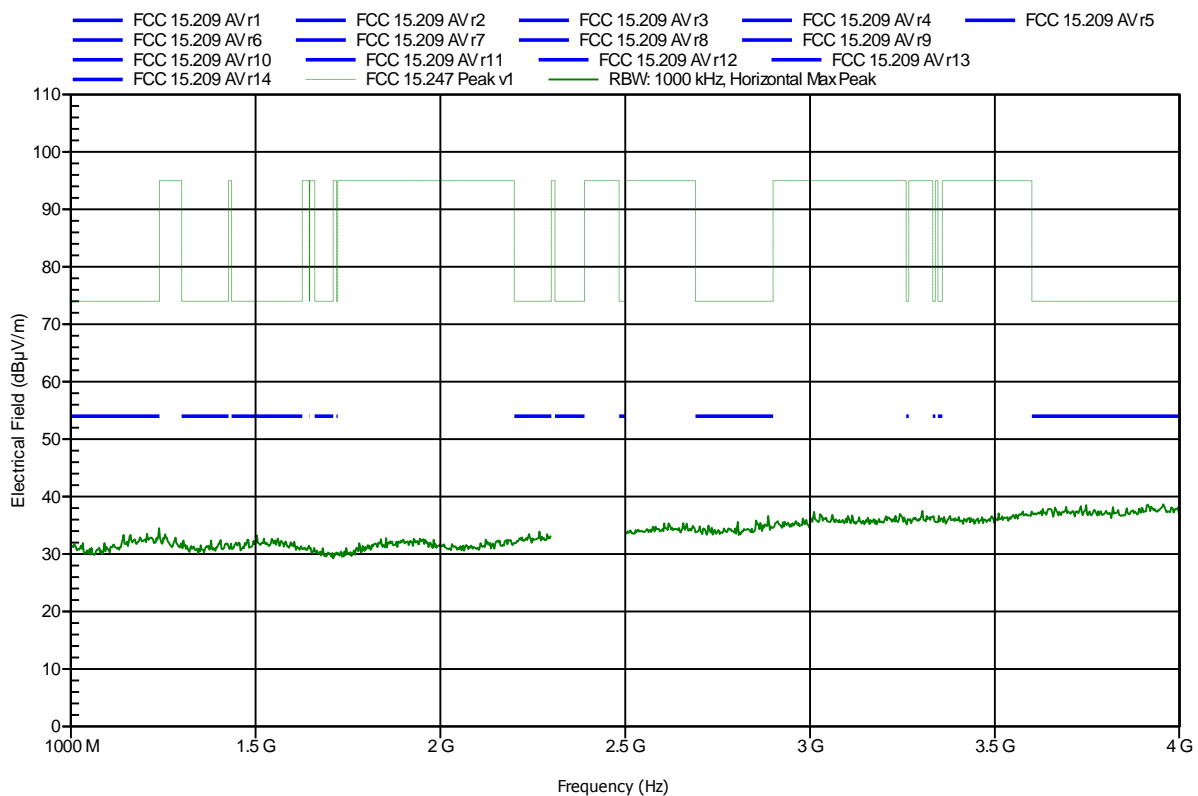


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 51

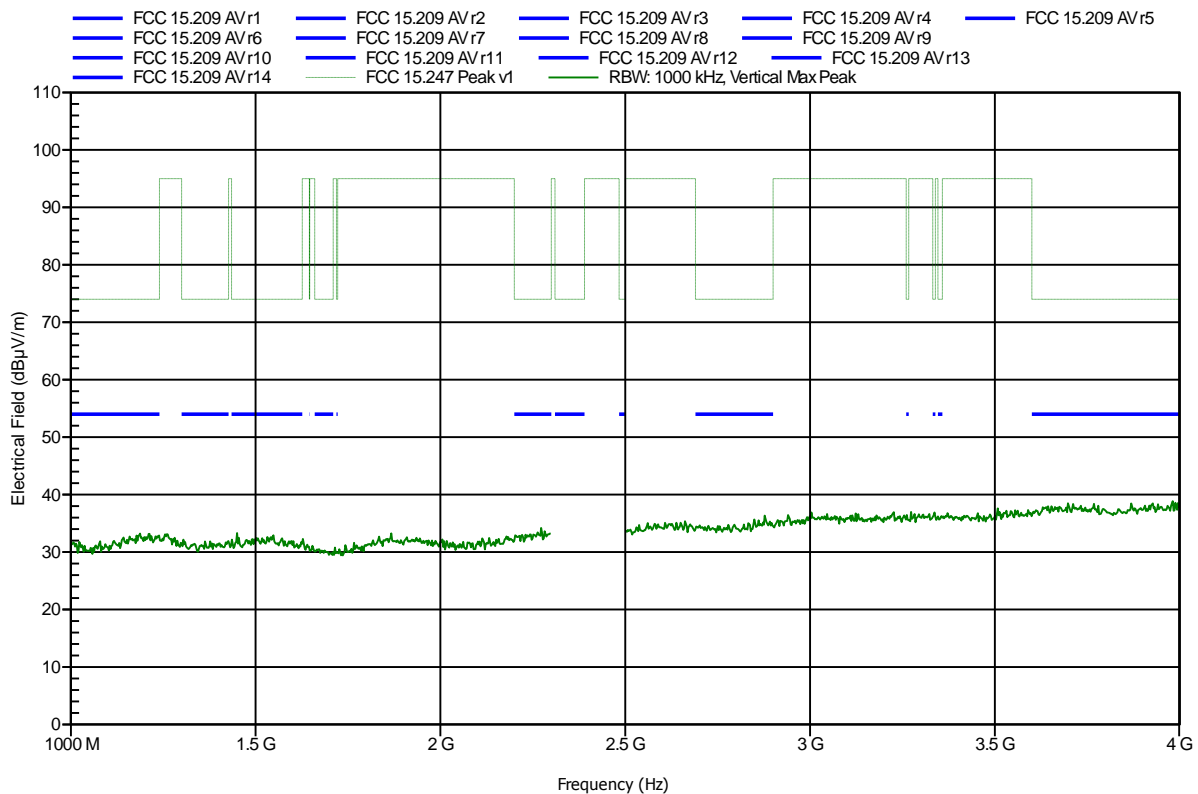


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note: upper bandedge

Index 49

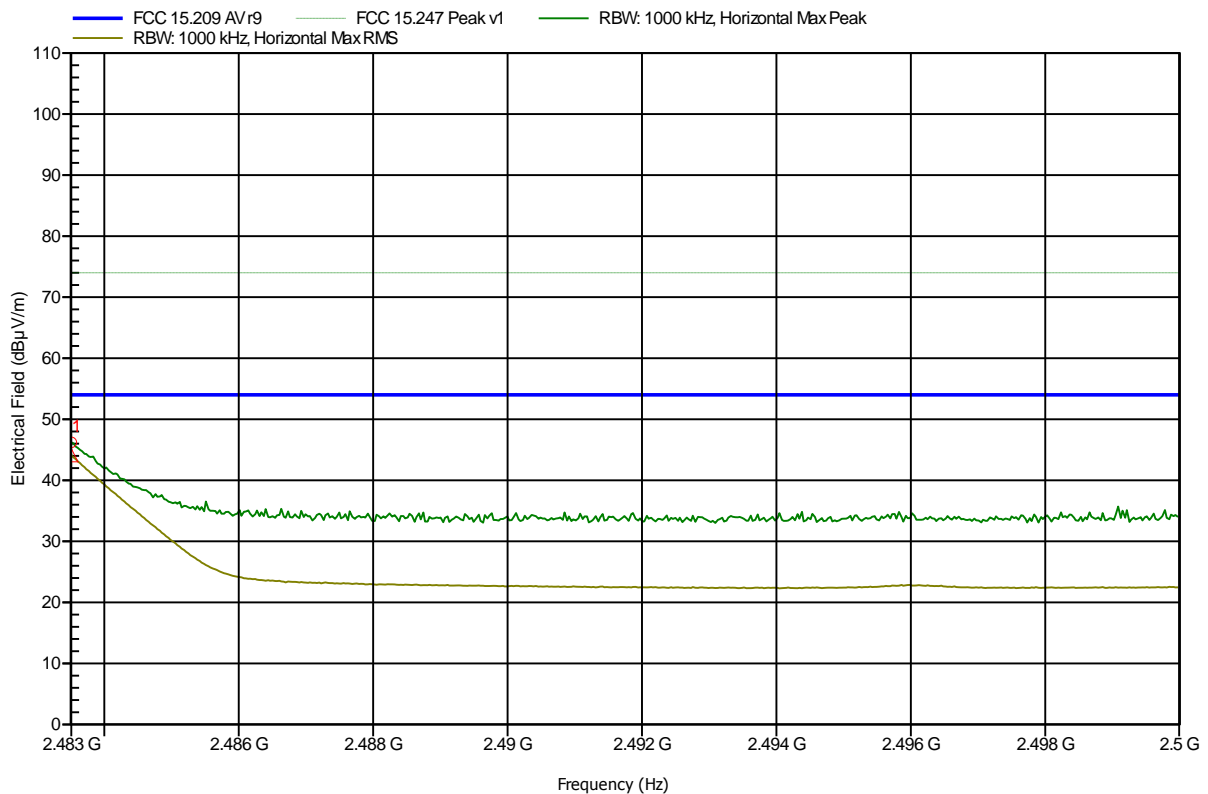


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
2.4835 GHz	46.2 dBµV/m	74 dBµV/m	-27.8 dB	Pass

Spurious emissions according to FCC 15.247

Project number: GOM-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	3 m
Mode:	TX; ch. 39
Test Date:	2013-07-03
Note:	upper bandedge

Index 52

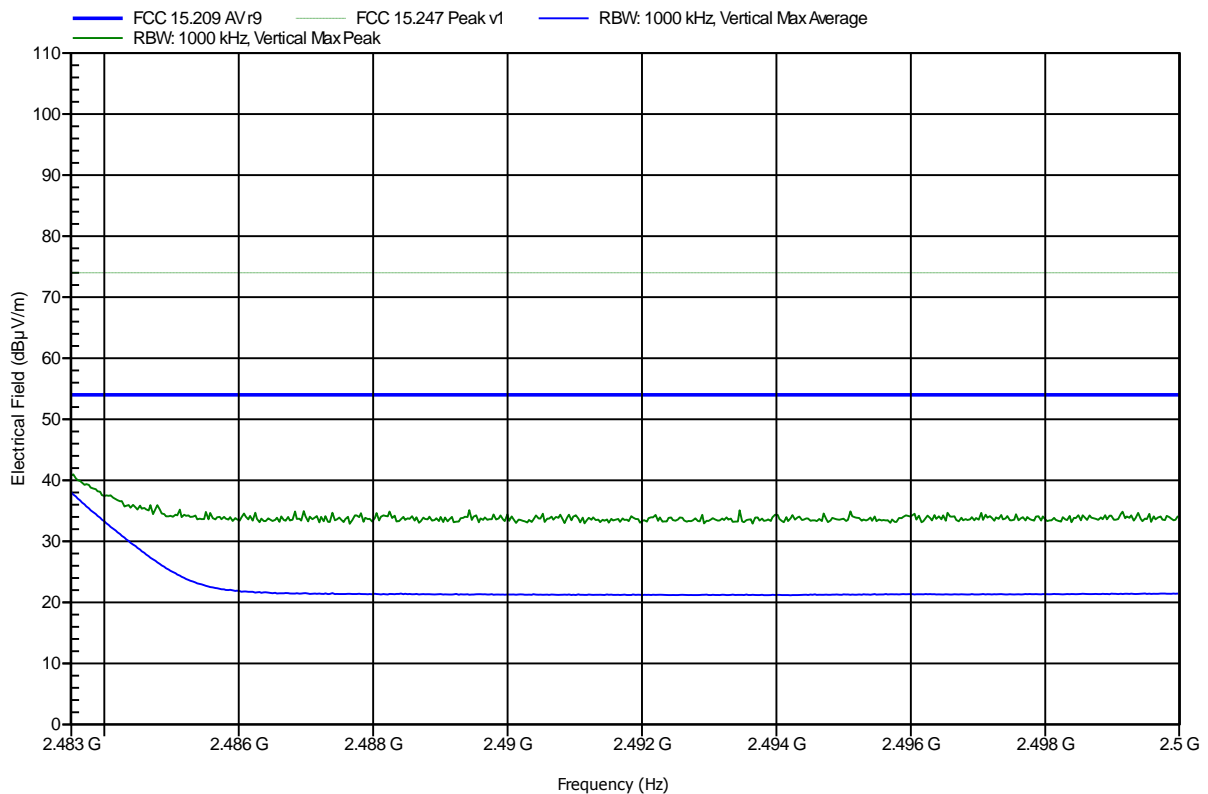


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 3 m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 50

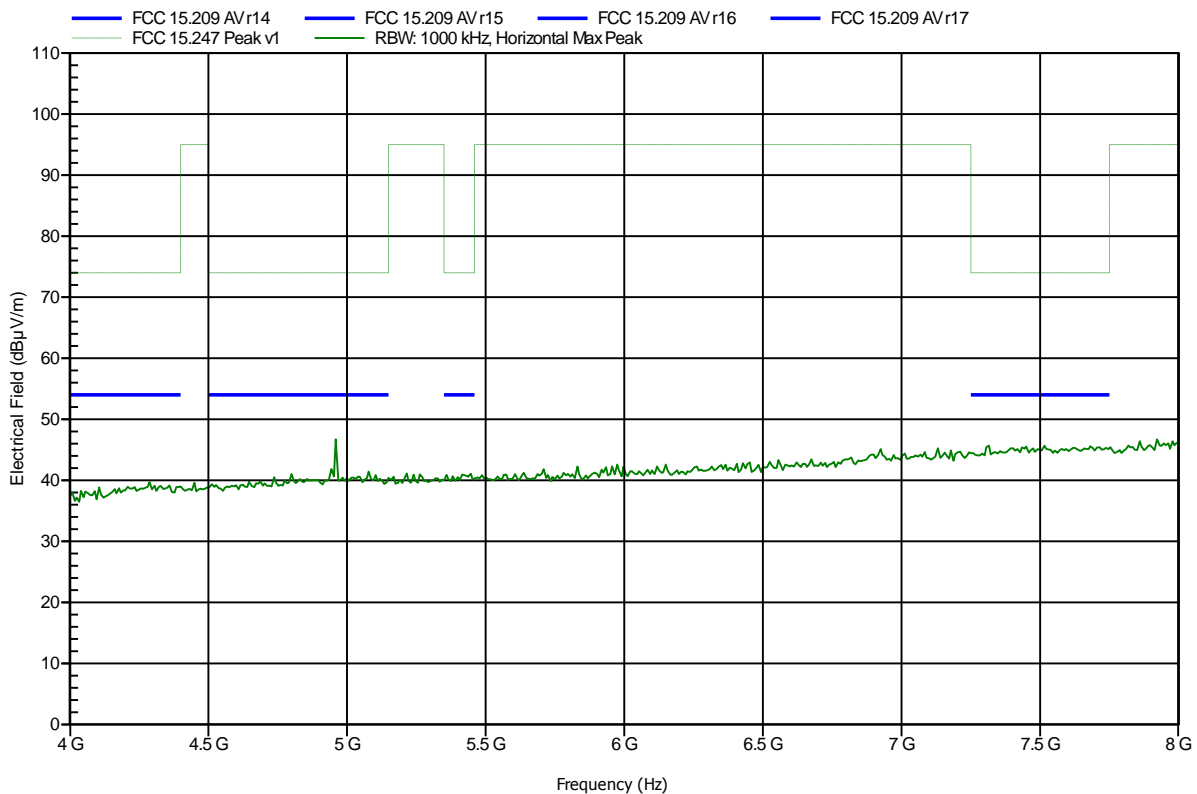


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 3 m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 53

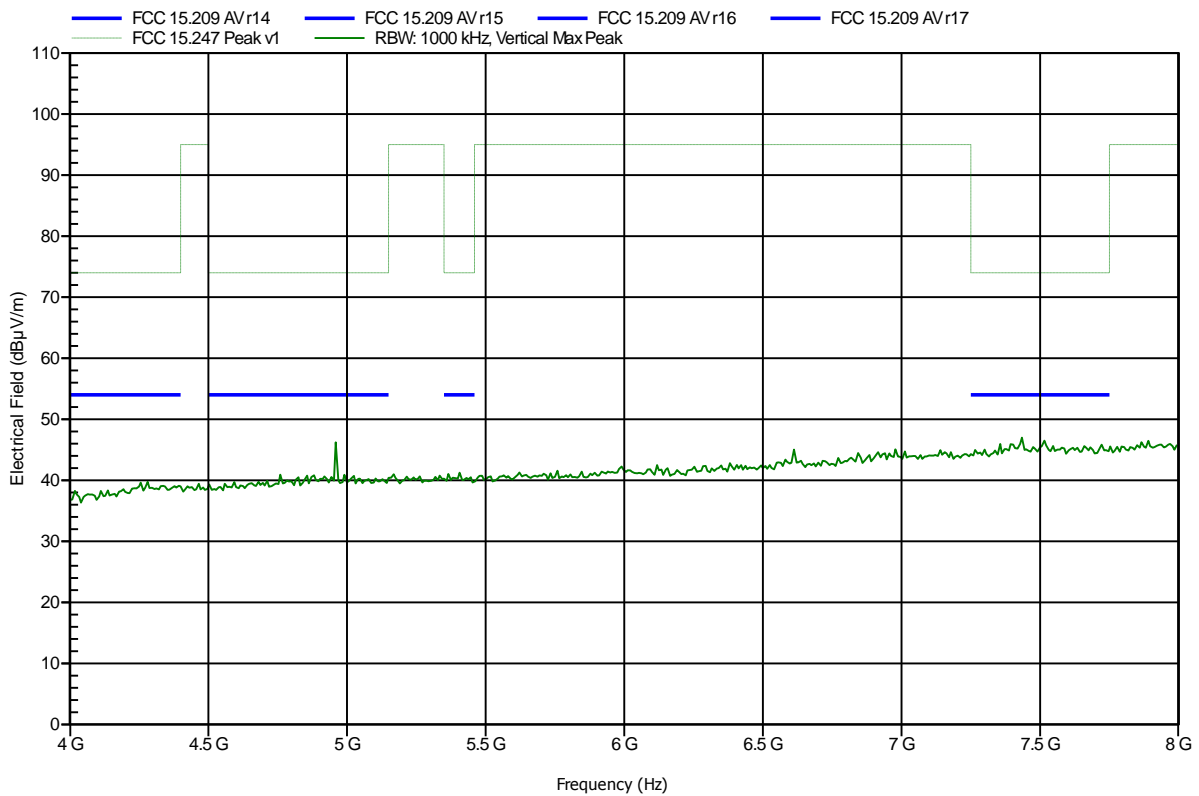


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Horizontal
 Measurement distance: 100 cm converted to 3m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 63

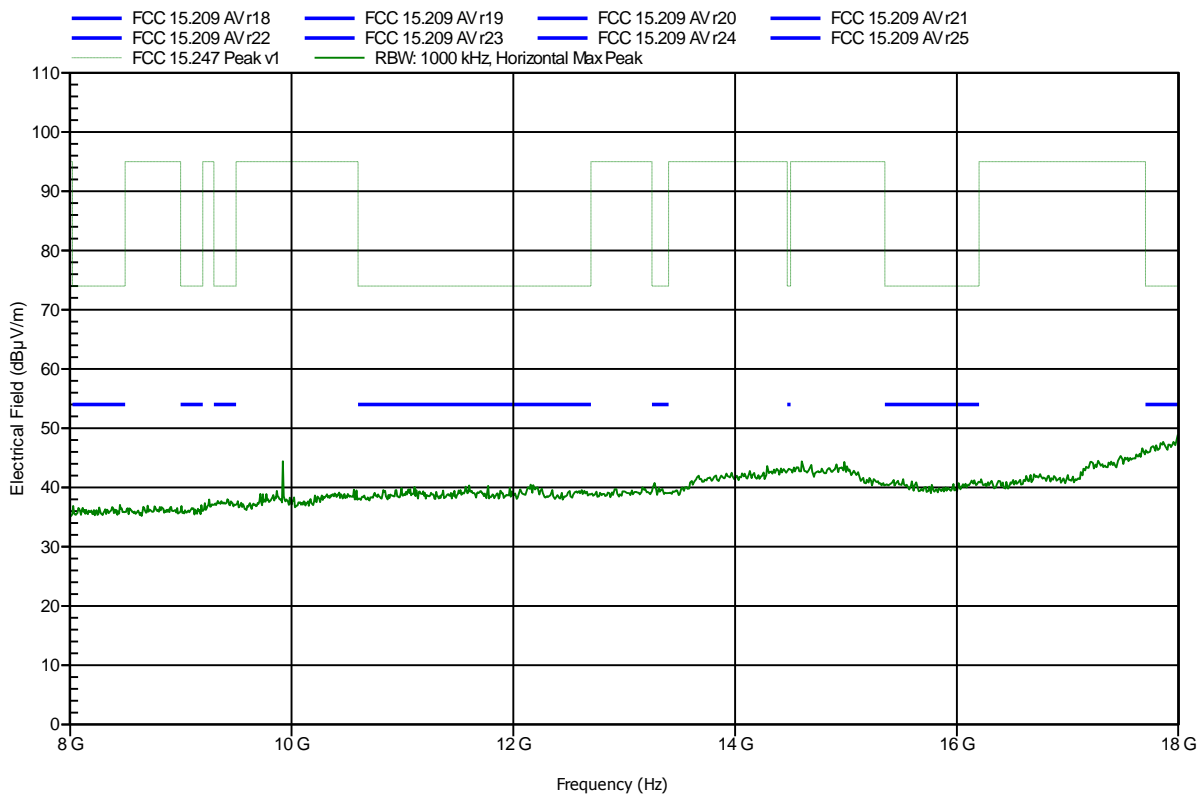


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Schwarzbeck BBHA 9120D, Vertical
 Measurement distance: 100 cm converted to 3m
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 65

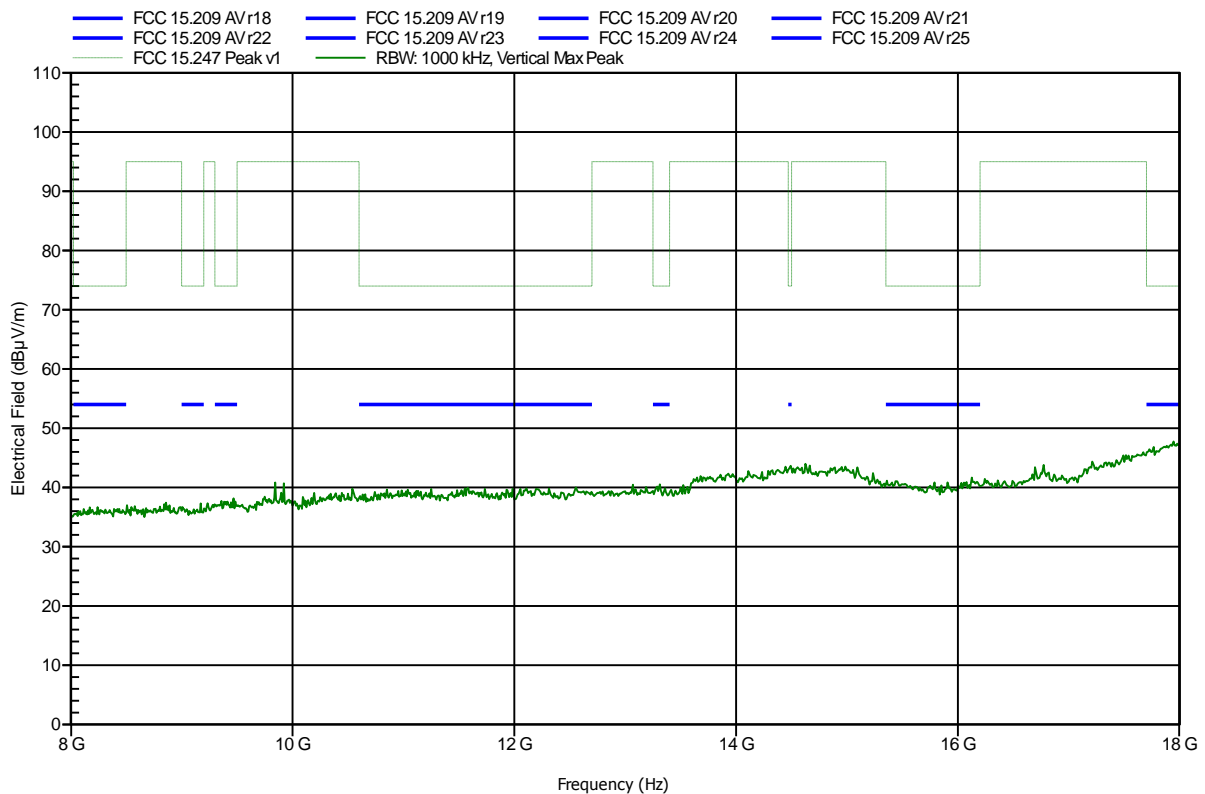


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 025, Horizontal
 Measurement distance: 100 cm
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 64

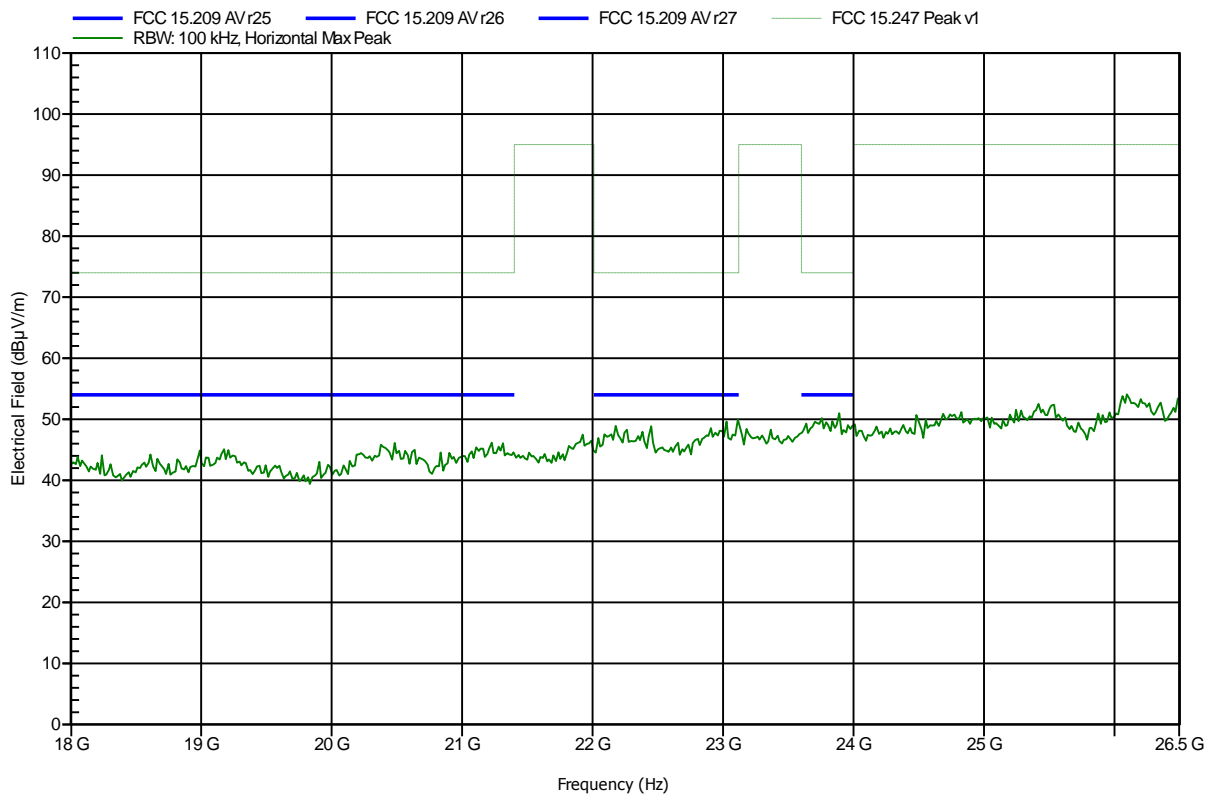


Spurious emissions according to FCC 15.247

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 025, Vertical
 Measurement distance: 100 cm
 Mode: TX; ch. 39
 Test Date: 2013-07-03
 Note:

Index 66

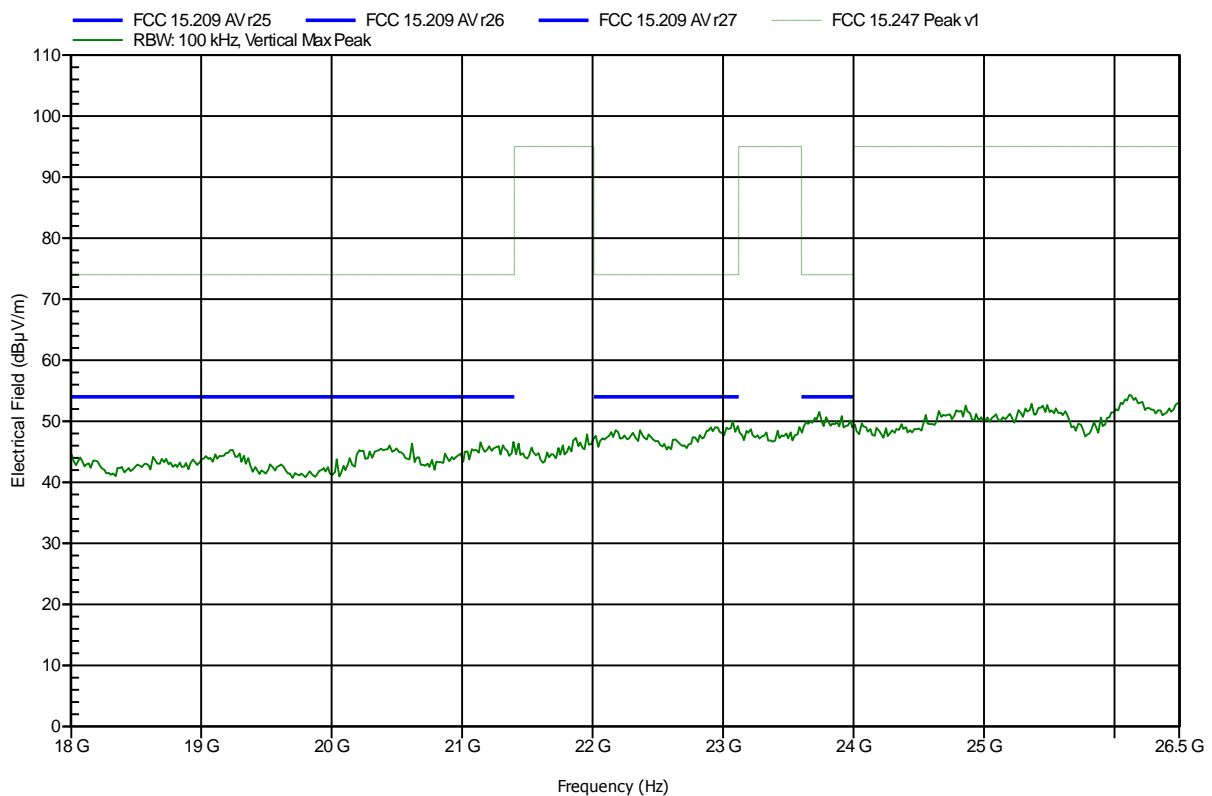


ANNEX B Receiver radiated spurious emissions

Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Rohde & Schwarz HK 116, Horizontal
Measurement distance:	3 m
Mode:	RX; ch. 19
Test Date:	2013-07-03
Note:	

Index 76

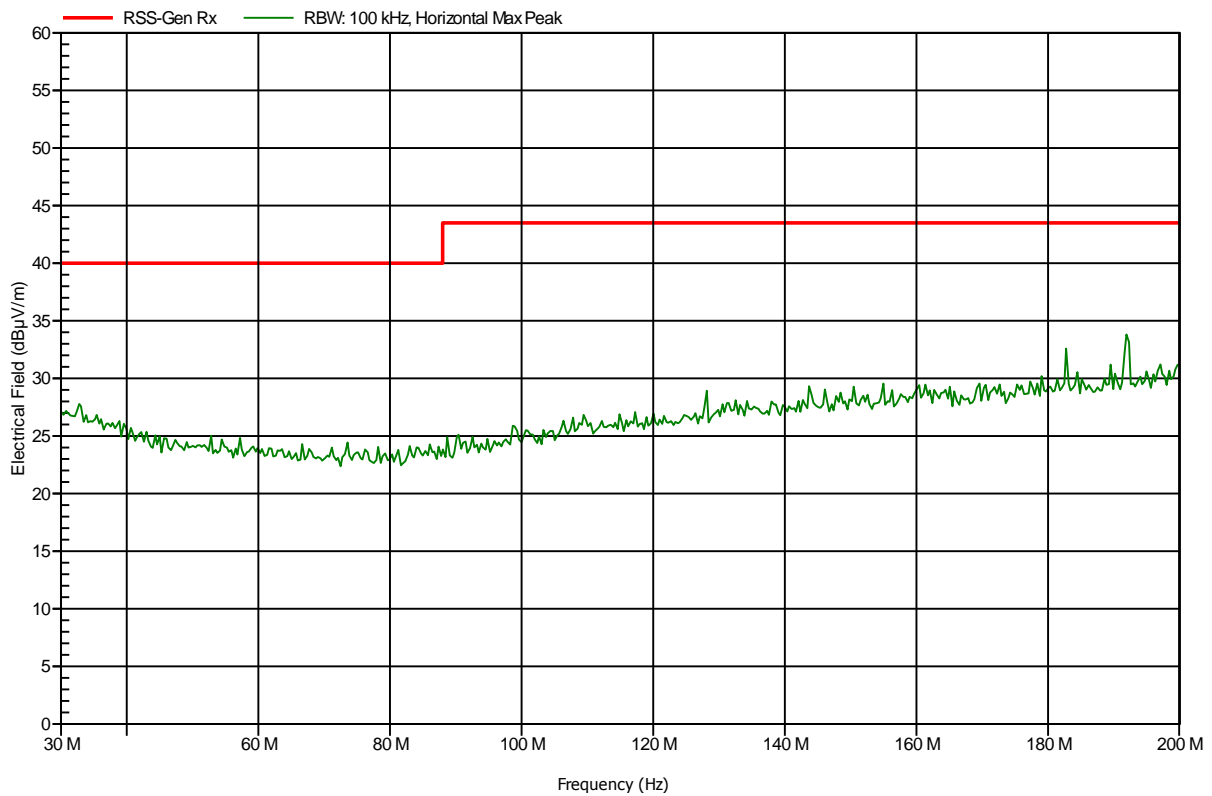


Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HK 116, Vertical
 Measurement distance: 3 m
 Mode: RX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 77

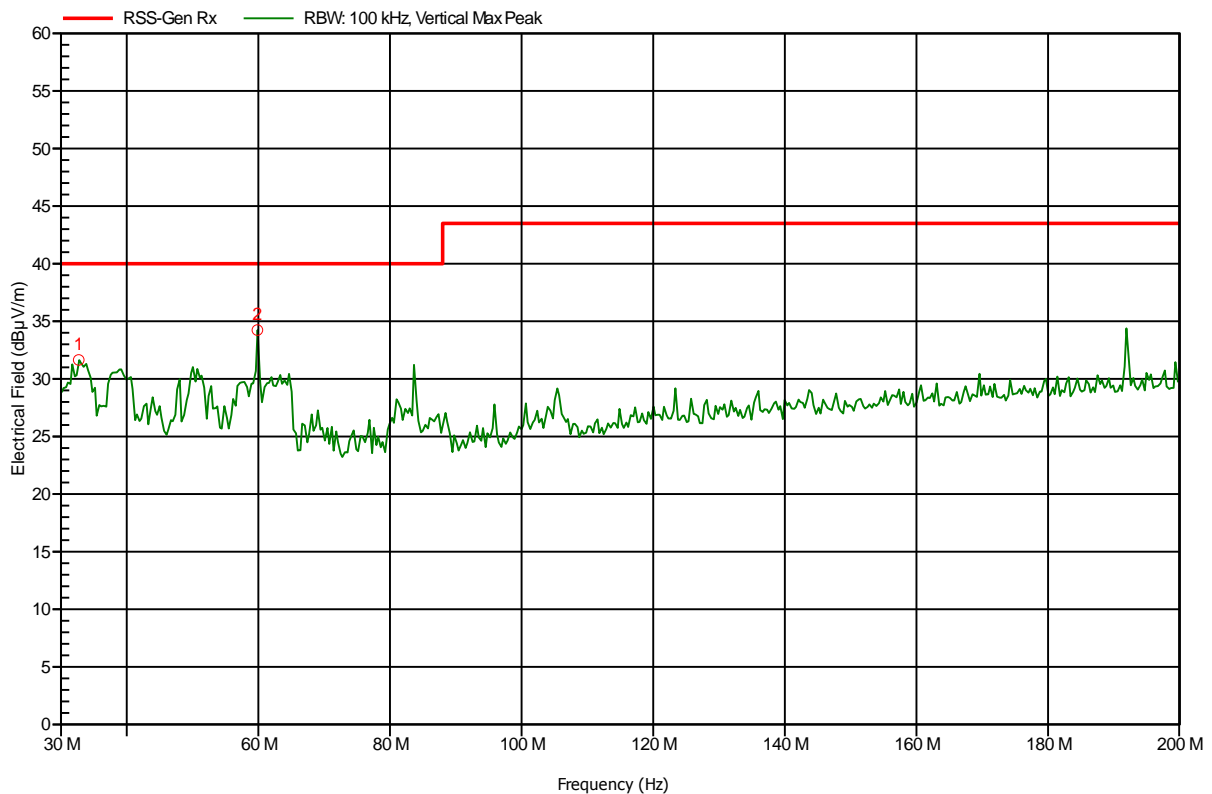


Frequency	Peak	Peak Limit	Peak Difference	Status
32.715 MHz	31.65 dBµV/m	40 dBµV/m	-8.35 dB	Pass
59.86 MHz	34.24 dBµV/m	40 dBµV/m	-5.76 dB	Pass

Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Rohde & Schwarz HL 223, Horizontal
Measurement distance:	3 m
Mode:	RX; ch. 19
Test Date:	2013-07-03
Note:	

Index 78

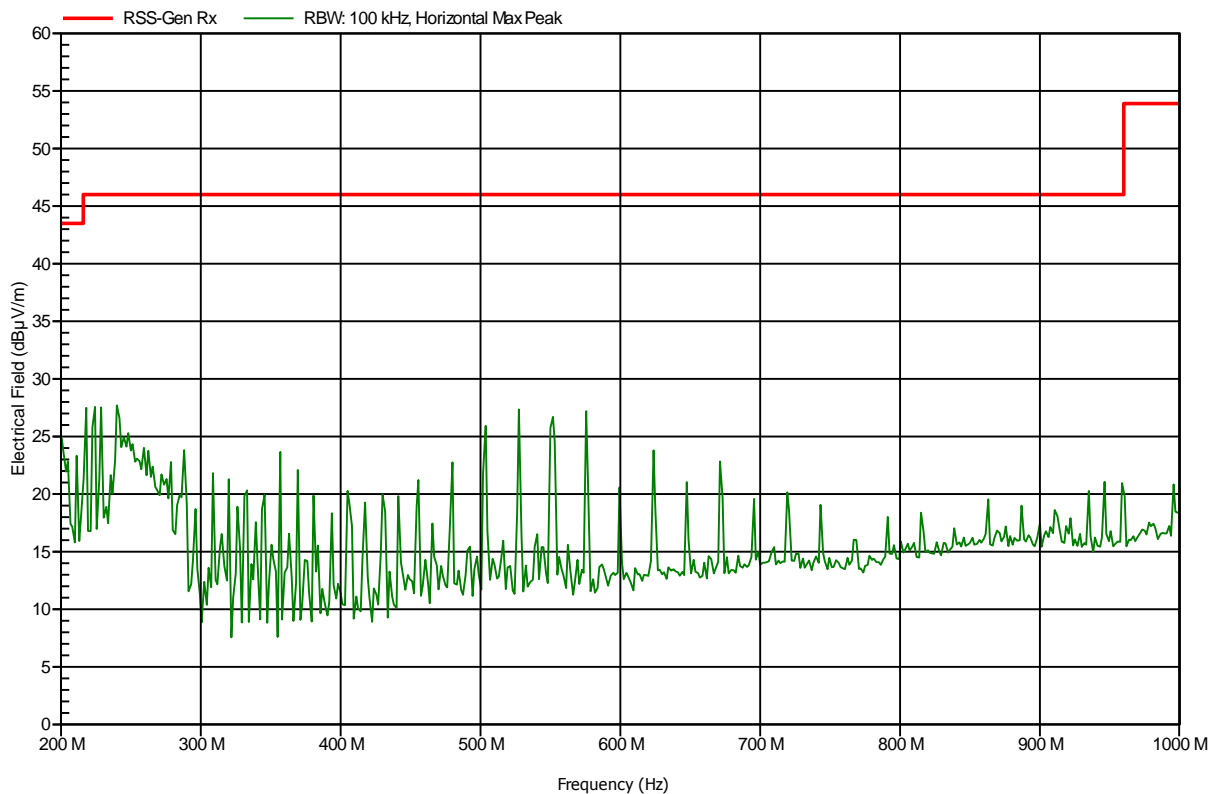


Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer: Bang & Olufsen Medicom A/S
 EUT Name: Electronic Auto-injector
 Model: betaCONNECT
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Treffke
 Test Conditions: Tnom: 20°C, Vnom: 3.7V DC lithium battery
 Antenna: Rohde & Schwarz HL 223, Vertical
 Measurement distance: 3 m
 Mode: RX; ch. 19
 Test Date: 2013-07-03
 Note:

Index 79

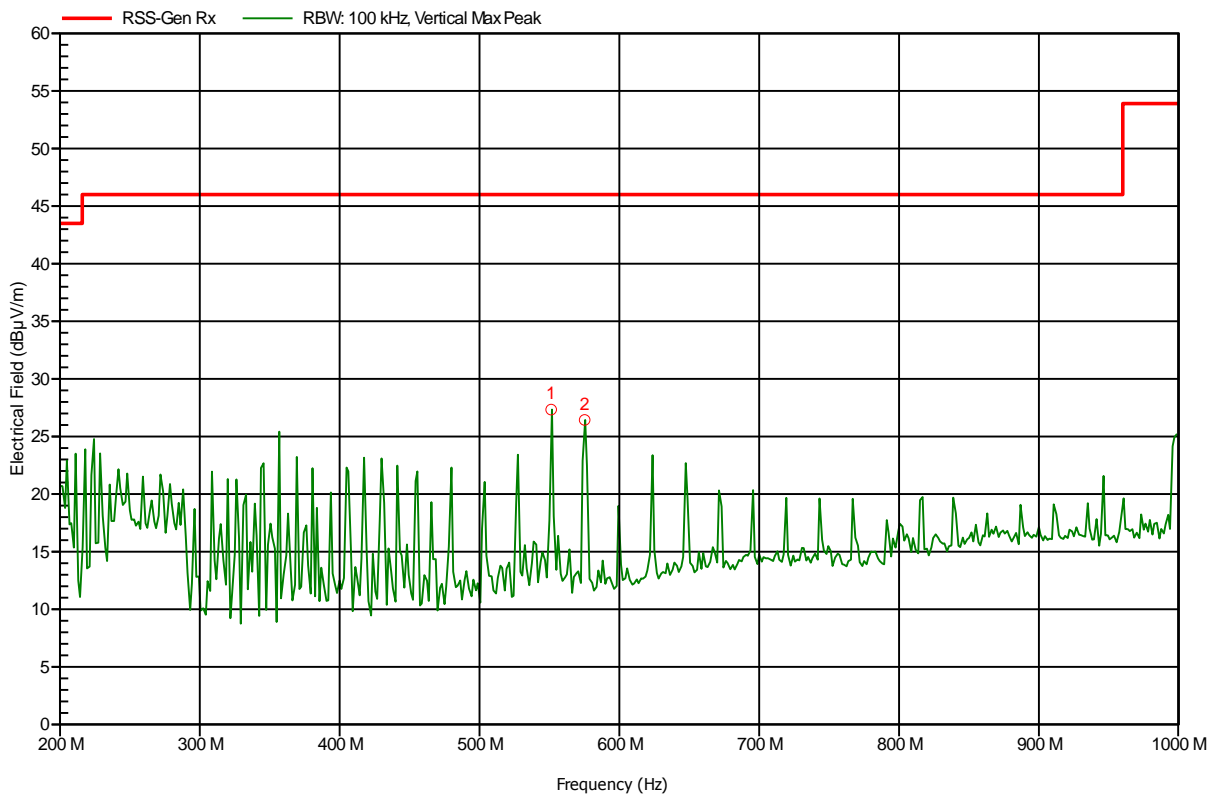


Frequency	Peak	Peak Limit	Peak Difference	Status
551.297 MHz	27.33 dBµV/m	46 dBµV/m	-18.67 dB	Pass
575.25 MHz	26.43 dBµV/m	46 dBµV/m	-19.57 dB	Pass

Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	3 m
Mode:	RX; ch. 19
Test Date:	2013-07-03
Note:	

Index 80

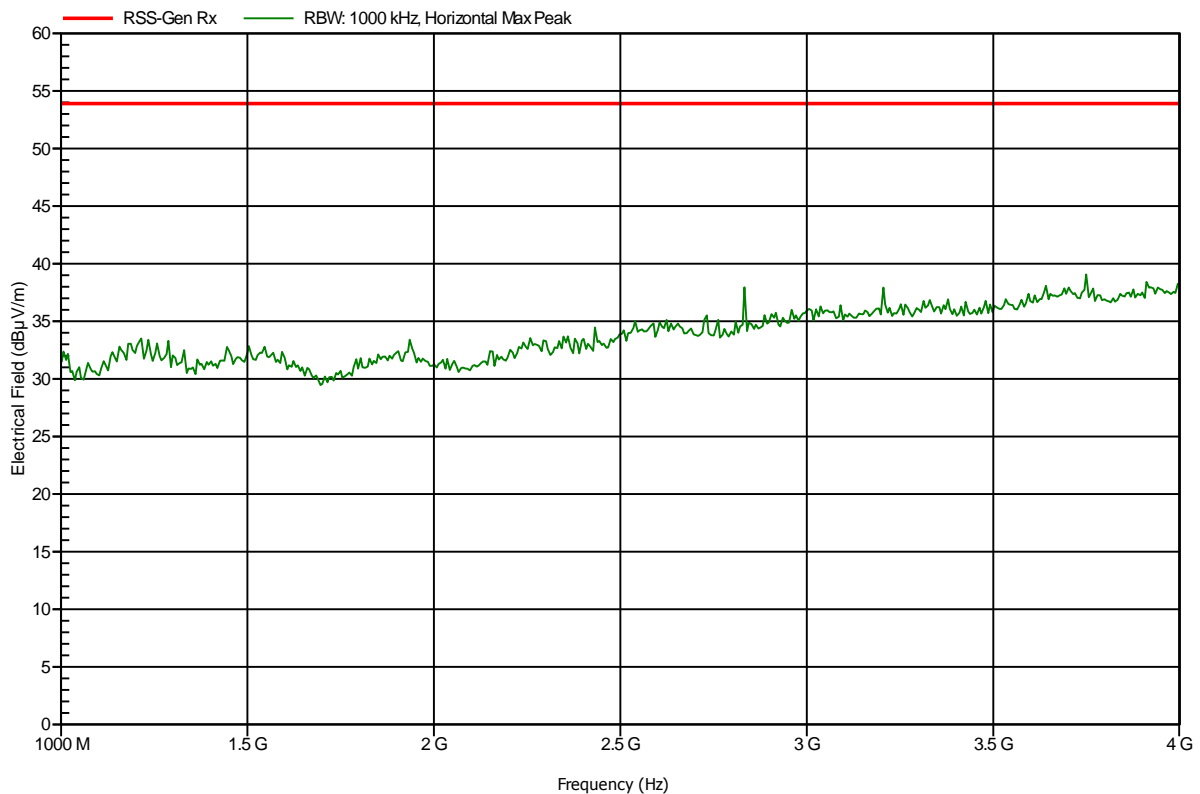


Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	3 m
Mode:	RX; ch. 19
Test Date:	2013-07-03
Note:	

Index 82

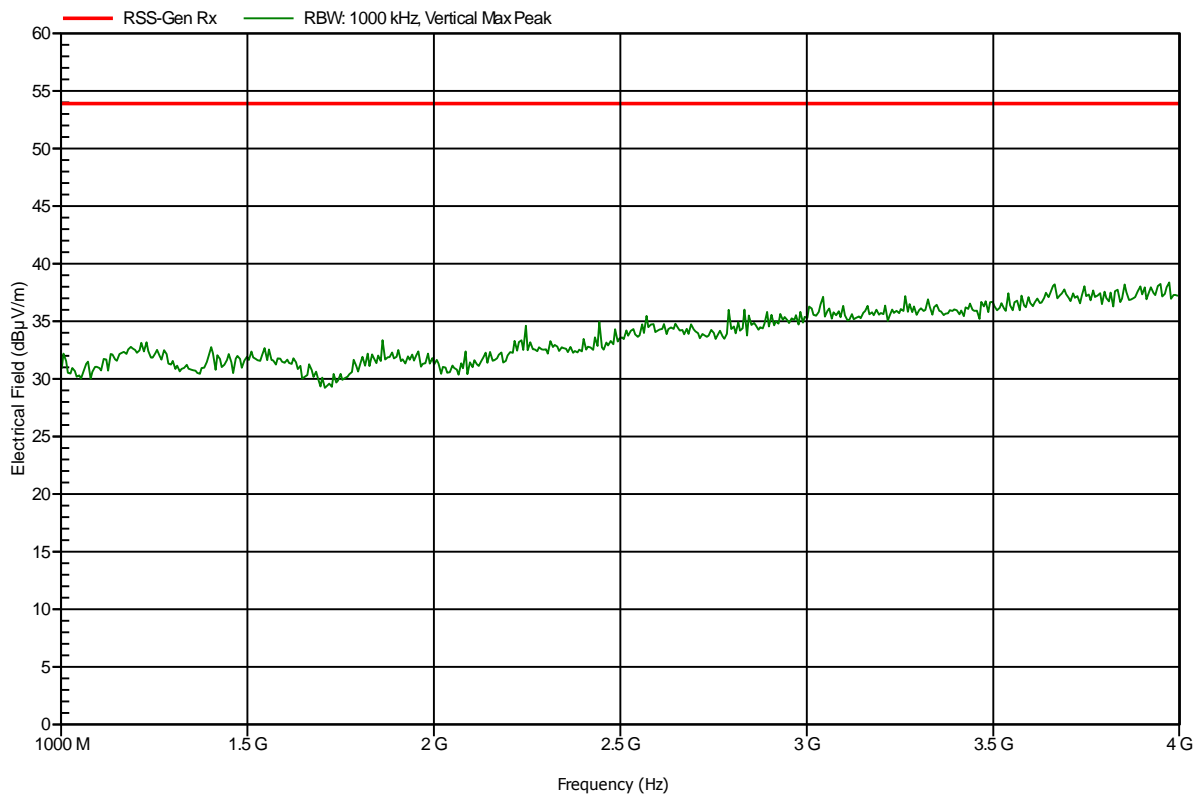


Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Schwarzbeck BBHA 9120D, Horizontal
Measurement distance:	3 m
Mode:	RX; ch. 19
Test Date:	2013-07-03
Note:	

Index 81

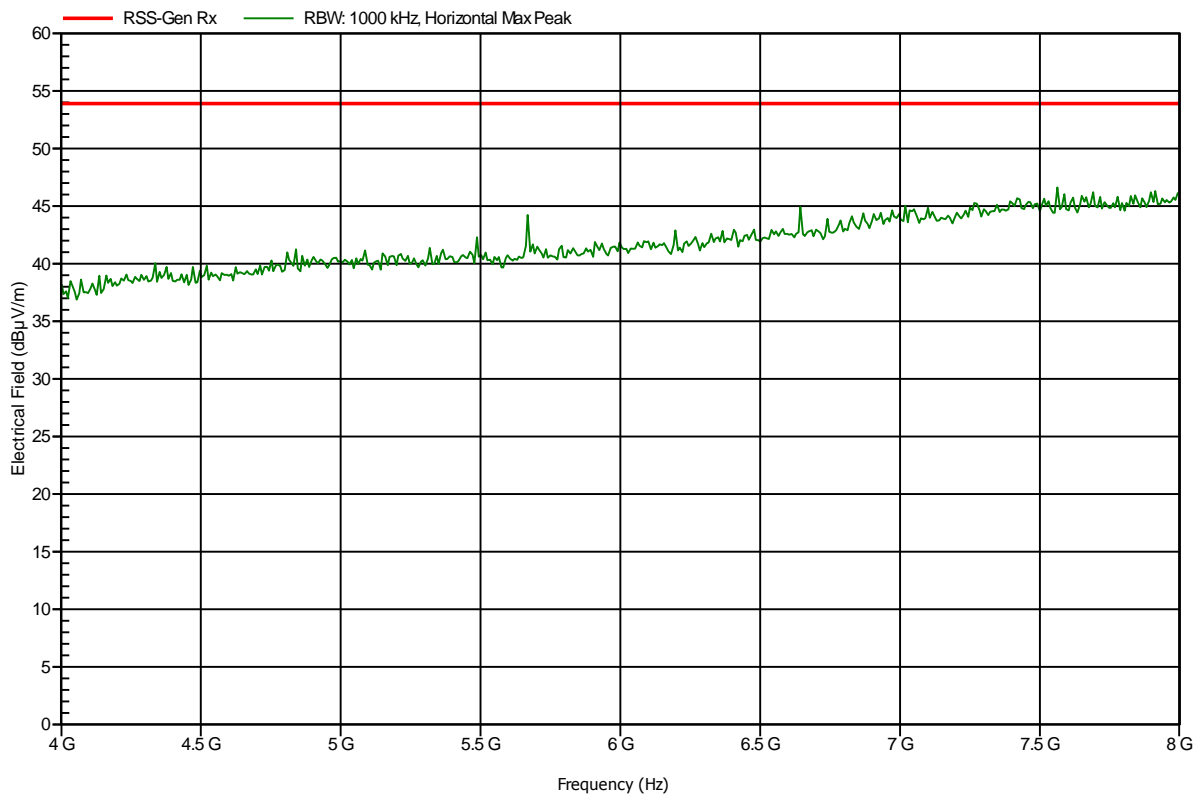

Spurious emissions according to RSS-GEN

Project number: G0M-1305-2859

Manufacturer:	Bang & Olufsen Medicom A/S
EUT Name:	Electronic Auto-injector
Model:	betaCONNECT
Test Site:	Eurofins Product Service GmbH
Operator:	Mr. Treffke
Test Conditions:	Tnom: 20°C, Vnom: 3.7V DC lithium battery
Antenna:	Schwarzbeck BBHA 9120D, Vertical
Measurement distance:	3 m
Mode:	RX; ch. 19
Test Date:	2013-07-03
Note:	

Index 83

