

Prepared by: LabTest Certification Inc.  
Date Issued: August 19, 2013  
Project No: 11404

Client: Orpyx Medical Technologies Inc.  
Report No.: 11404-1E  
Revision No.: 0

## APPENDIX C: Test setup photos


### - Test configuration for Conducted measurement



Prepared by: LabTest Certification Inc.  
Date Issued: August 19, 2013  
Project No: 11404

Client: Orpyx Medical Technologies Inc.  
Report No.: 11404-1E  
Revision No.: 0


**- Test configuration for Radiated measurement, over 1 GHz for Harmonics**

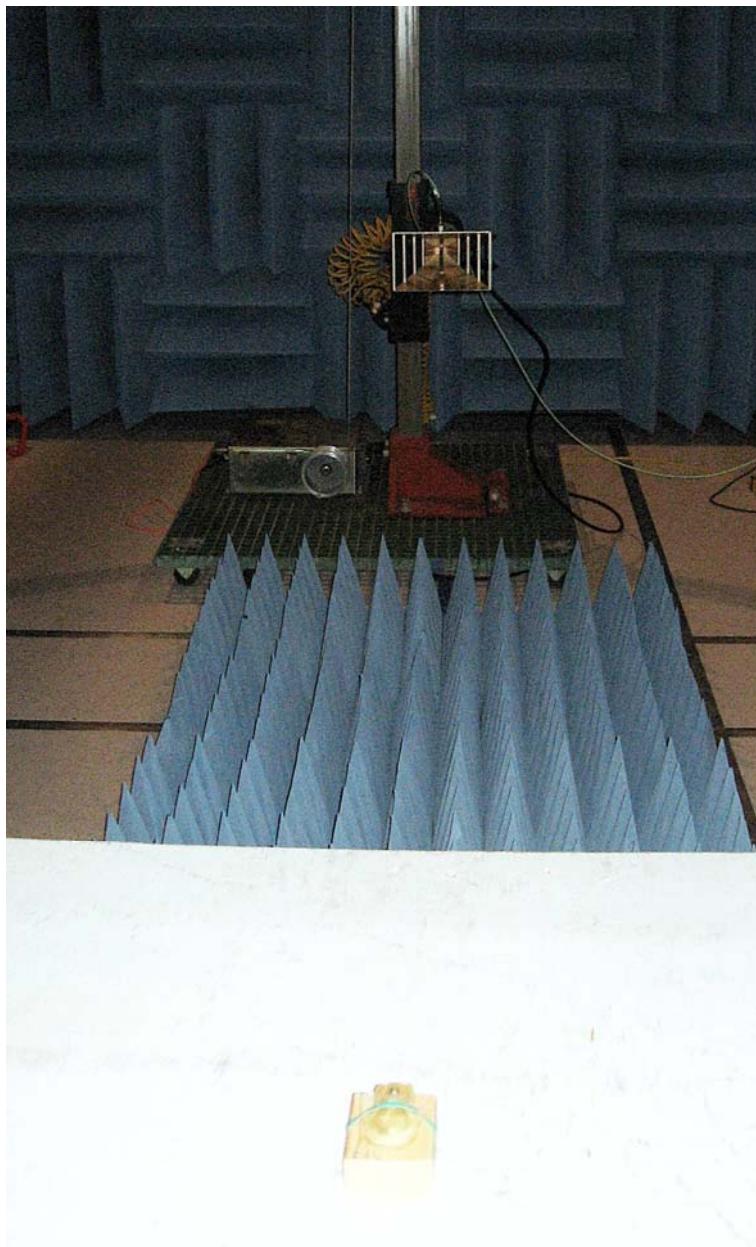

Prepared by: LabTest Certification Inc.  
Date Issued: August 19, 2013  
Project No: 11404

Client: Orpyx Medical Technologies Inc.  
Report No.: 11404-1E  
Revision No.: 0

**- Test configuration for Radiated measurement, 30 MHz to 1 GHz for Spurious and Receive Mode**

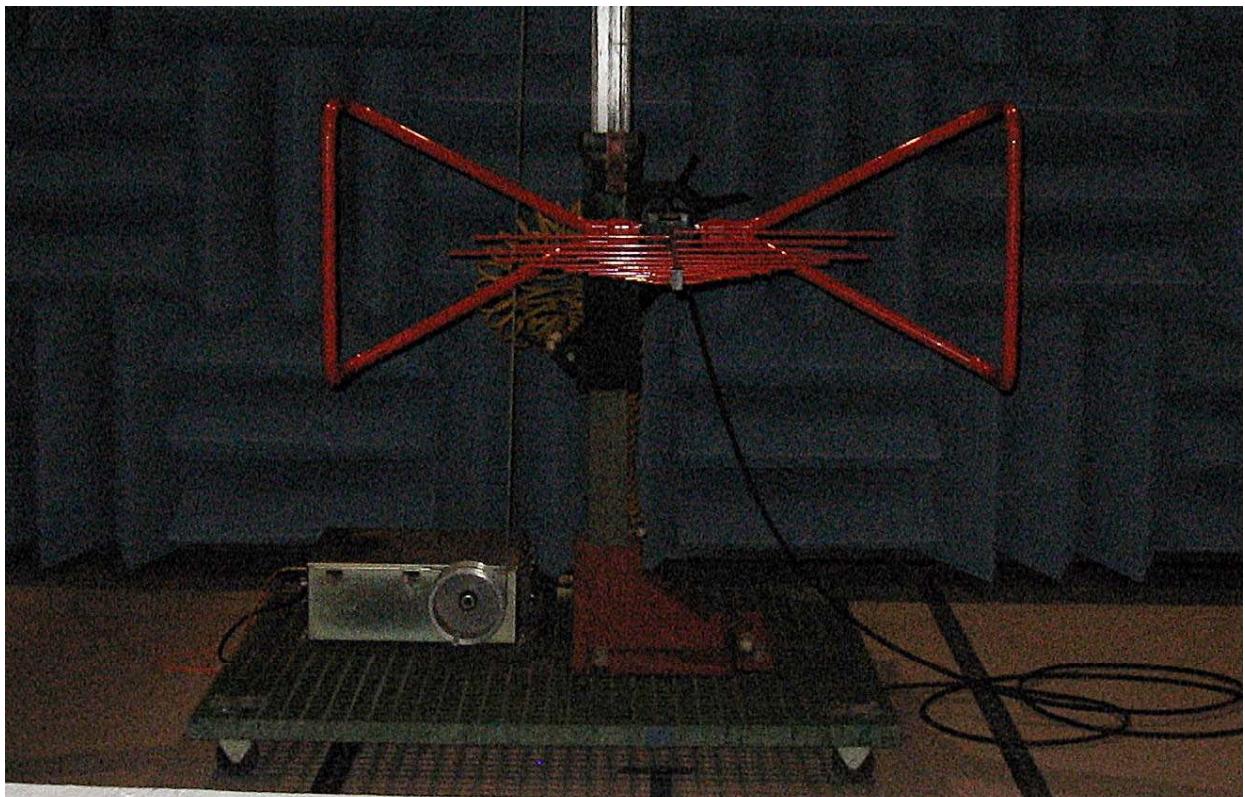

Prepared by: LabTest Certification Inc.  
Date Issued: August 19, 2013  
Project No: 11404

Client: Orpyx Medical Technologies Inc.  
Report No.: 11404-1E  
Revision No.: 0


**- Test configuration for Radiated measurement, under 30MHz for Intentional Emissions**



Prepared by: LabTest Certification Inc.  
Date Issued: August 19, 2013  
Project No: 11404

Client: Orpyx Medical Technologies Inc.  
Report No.: 11404-1E  
Revision No.: 0

**- Table setup for Radiated measurement, Orthogonal X**

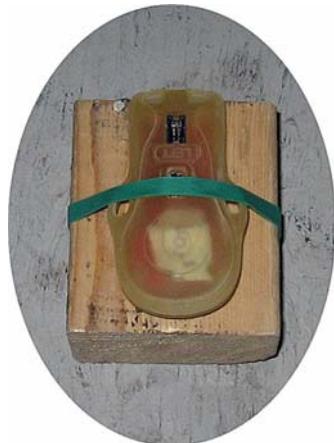

**- Table setup for Radiated measurement, Orthogonal Y**



**- Table setup for Radiated measurement, Orthogonal Z**

