



3.3 LOWER DETECTION LIMIT

The lower detection limit was assessed using the same measurement set up as used for the linearity measurement. The required lower detection limit is 10 mW/kg.

3.4 ISOTROPY

The axial isotropy was evaluated by exposing the probe to a reference wave from a standard dipole with the dipole mounted under the flat phantom in the test configuration suggested for system validations and checks. The probe was rotated along its main axis from 0 to 360 degrees in 15-degree steps. The hemispherical isotropy is determined by inserting the probe in a thin plastic box filled with tissue-equivalent liquid, with the plastic box illuminated with the fields from a half wave dipole. The dipole is rotated about its axis (0°-180°) in 15° increments. At each step the probe is rotated about its axis (0°-360°).

3.1 BOUNDARY EFFECT

The boundary effect is defined as the deviation between the SAR measured data and the expected exponential decay in the liquid when the probe is oriented normal to the interface. To evaluate this effect, the liquid filled flat phantom is exposed to fields from either a reference dipole or waveguide. With the probe normal to the phantom surface, the peak spatial average SAR is measured and compared to the analytical value at the surface.

The boundary effect uncertainty can be estimated according to the following uncertainty approximation formula based on linear and exponential extrapolations between the surface and d\_be + d\_step along lines that are approximately normal to the surface:

SAR\_uncertainty [%] = ΔSAR\_be \* ((d\_be + d\_step)^2 \* (e^-d\_be/δ)) / (2d\_step \* δ/2) for (d\_be + d\_step) < 10 mm

- where
SAR\_uncertainty is the uncertainty in percent of the probe boundary effect
d\_be is the distance between the surface and the closest zoom-scan measurement point, in millimetre
Δ\_step is the separation distance between the first and second measurement points that are closest to the phantom surface, in millimetre, assuming the boundary effect at the second location is negligible
δ is the minimum penetration depth in millimetres of the head tissue-equivalent liquids defined in this standard, i.e., δ ≈ 14 mm at 3 GHz;
ΔSAR\_be in percent of SAR is the deviation between the measured SAR value, at the distance d\_be from the boundary, and the analytical SAR value.

The measured worst case boundary effect SAR uncertainty[%] for scanning distances larger than 4mm is 1.0% Limit ,2%).





COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR.180.4.42.BES.A

4 MEASUREMENT UNCERTAINTY

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty associated with an E-field probe calibration using the waveguide technique. All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

| Uncertainty analysis of the probe calibration in waveguide |                       |                          |         |    |                          |
|--|-----------------------|--------------------------|---------|----|--------------------------|
| ERROR SOURCES  | Uncertainty value (%) | Probability Distribution | Divisor | ci | Standard Uncertainty (%) |
| Expanded uncertainty<br>95 % confidence level k = 2        |                       |                          |         |    | 14 %                     |

5 CALIBRATION MEASUREMENT RESULTS

| Calibration Parameters |             |
|------------------------|-------------|
| Liquid Temperature     | 20 +/- 1 °C |
| Lab Temperature        | 20 +/- 1 °C |
| Lab Humidity           | 30-70 %     |

5.1 SENSITIVITY IN AIR

| Normx dipole 1 (µV/(V/m)²) | Normy dipole 2 (µV/(V/m)²) | Normz dipole 3 (µV/(V/m)²) |
|----------------------------|----------------------------|----------------------------|
| 0.76                       | 0.78                       | 0.76                       |

| DCP dipole 1 (mV) | DCP dipole 2 (mV) | DCP dipole 3 (mV) |
|-------------------|-------------------|-------------------|
| 106               | 107               | 108               |

Calibration curves  $e_i=f(V)$  (i=1,2,3) allow to obtain E-field value using the formula:

$E = \sqrt{E_1^2 + E_2^2 + E_3^2}$

Template: ACR.DDD.N.YF.MVG.R.ISSUE\_COMOSAR\_Probe.v8

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.






COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR.180.4.42.BES.A


份  
Lab

Calibration curves

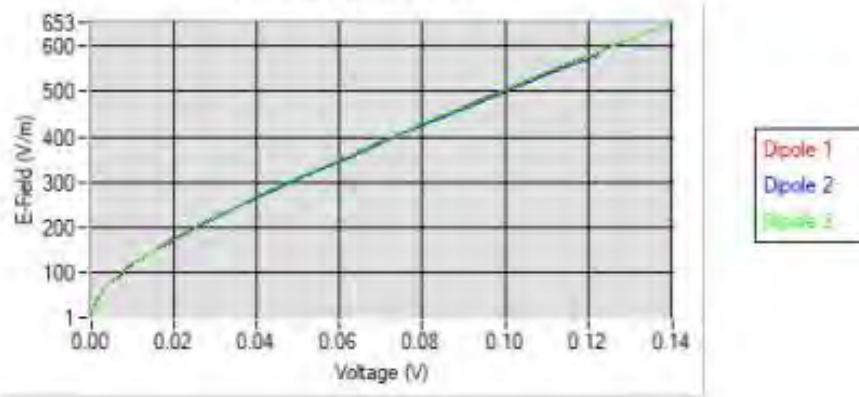

5.2 LINEARITY

Linearity

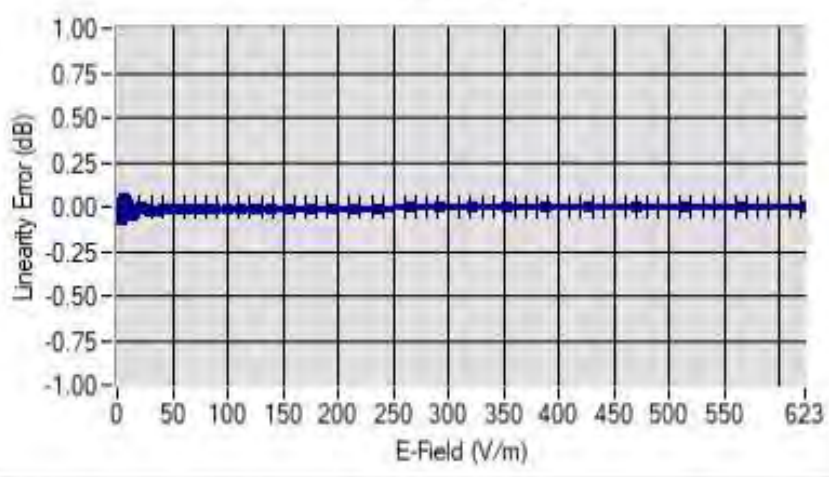

Linearity: +/-1.81% (+/-0.08dB)

Template: ACR.DDD-N.YY.MHGBLSSUE\_COMOSAR Probe v8

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.

份  
Lab





COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR.180.4.42.BESA

股份  
ng Lab

5.3 SENSITIVITY IN LIQUID

| Liquid | Frequency<br>(MHz +/-<br>100MHz) | ConvF |
|--------|----------------------------------|-------|
| HL450* | 450*                             | 1.74* |
| BL450* | 450*                             | 1.67* |
| HL750  | 750                              | 1.69  |
| BL750  | 750                              | 1.73  |
| HL850  | 835                              | 1.75  |
| BL850  | 835                              | 1.80  |
| HL900  | 900                              | 1.87  |
| BL900  | 900                              | 1.85  |
| HL1800 | 1800                             | 2.09  |
| BL1800 | 1800                             | 2.15  |
| HL1900 | 1900                             | 2.14  |
| BL1900 | 1900                             | 2.27  |
| HL2000 | 2000                             | 2.31  |
| BL2000 | 2000                             | 2.34  |
| HL2300 | 2300                             | 2.46  |
| BL2300 | 2300                             | 2.51  |
| HL2450 | 2450                             | 2.60  |
| BL2450 | 2450                             | 2.70  |
| HL2600 | 2600                             | 2.39  |
| BL2600 | 2600                             | 2.50  |
| HL5200 | 5200                             | 1.85  |
| BL5200 | 5200                             | 1.81  |
| HL5400 | 5400                             | 2.07  |
| BL5400 | 5400                             | 2.00  |
| HL5600 | 5600                             | 2.19  |
| BL5600 | 5600                             | 2.11  |
| HL5800 | 5800                             | 2.01  |
| BL5800 | 5800                             | 1.97  |

\* Frequency not cover by COFRAC scope, calibration not accredited

LOWER DETECTION LIMIT: 7mW/kg

Compliance: ACR.180.4.42.BESA\_COMOSAR Probe calibration

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.

股份  
ng Lab






COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR.180.4.42.BES.A

股份  
ig Lab

5.4 ISOTROPY

HL1800 MHz

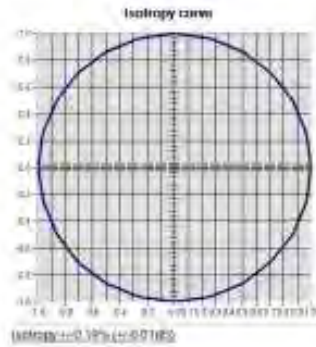

股份  
ig Lab

Template: ACR\_TEMPLATE\_VY.MVGR.ISSUE\_COMOSAR Probe 06

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.

股份  
ig Lab





COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR.180.4.42.BES.A

股份  
ig Lab

6 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                      |                         |   |   |
|------------------------------------|----------------------|-------------------------|---|---|
| Equipment Description              | Manufacturer / Model | Identification No.      | Current Calibration Date                      | Next Calibration Date                         |
| CALIPROBE Test Bench               | Version 2            | NA                      | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM  | 100203                  | 08/2021                                       | 08/2024                                       |
| Network Analyzer                   | Agilent 8753ES       | MY40003210              | 10/2022                                       | 10/2025                                       |
| Network Analyzer – Calibration kit | HP 85033D            | 3423A08186              | 06/2021                                       | 06/2027                                       |
| Multimeter                         | Keithley 2000        | 1160271                 | 02/2023                                       | 02/2026                                       |
| Signal Generator                   | Rohde & Schwarz SMB  | 106589                  | 03/2022                                       | 03/2025                                       |
| Amplifier                          | MVG                  | MODU-023-C-0002         | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680          | 170100013               | 06/2021                                       | 06/2024                                       |
| Power Meter                        | Rohde & Schwarz NRVD | 832839-056              | 11/2022                                       | 11/2025                                       |
| Directional Coupler                | Krytar 158020        | 131467                  | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Waveguide                          | MVG                  | SN 32/16 WG4_1          | Validated. No cal required.                   | Validated. No cal required.                   |
| Liquid transition                  | MVG                  | SN 32/16 WGLIQ_0G900_1  | Validated. No cal required.                   | Validated. No cal required.                   |
| Waveguide                          | MVG                  | SN 32/16 WG6_1          | Validated. No cal required.                   | Validated. No cal required.                   |
| Liquid transition                  | MVG                  | SN 32/16 WGLIQ_1G500_1  | Validated. No cal required.                   | Validated. No cal required.                   |
| Waveguide                          | MVG                  | SN 32/16 WG8_1          | Validated. No cal required.                   | Validated. No cal required.                   |
| Liquid transition                  | MVG                  | SN 32/16 WGLIQ_1G800B_1 | Validated. No cal required.                   | Validated. No cal required.                   |
| Liquid transition                  | MVG                  | SN 32/16 WGLIQ_1G800H_1 | Validated. No cal required.                   | Validated. No cal required.                   |
| Waveguide                          | MVG                  | SN 32/16 WG10_1         | Validated. No cal required.                   | Validated. No cal required.                   |
| Liquid transition                  | MVG                  | SN 32/16 WGLIQ_3G500_1  | Validated. No cal required.                   | Validated. No cal required.                   |
| Waveguide                          | MVG                  | SN 32/16 WG12_1         | Validated. No cal required.                   | Validated. No cal required.                   |

股份  
ig Lab

Page: 10/11

Template: ACR.DDU.8.11.10 08.15.16 E\_COMOSAR Probe v6

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.

股份  
ig Lab





COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR.180.442.BES.A

股份  
ig Lab

|                                  |              |                           |                                |                                |
|----------------------------------|--------------|---------------------------|--------------------------------|--------------------------------|
| Liquid transition                | MVG          | SN 32/16<br>WGLIQ_5G000_1 | Validated. No cal<br>required. | Validated. No cal<br>required. |
| Temperature / Humidity<br>Sensor | Testo 184 H1 | 44225320                  | 06/2021                        | 06/2024                        |

股份  
ig Lab

Template: ACR.DDD.N.YY.MYGB.ISSUE\_COMOSAR Probe v8

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.

股份  
ig Lab





### 5.1 SID750Dipole Calibration Certificate



## SAR Reference Dipole Calibration Report

Ref: ACR.287.3.14.SATU.A

### SHENZHEN LCS COMPLIANCE TESTING LABORATORY LTD.

1F., XINGYUAN INDUSTRIAL PARK, TONGDA ROAD,  
BAO'AN BLVD  
BAO'AN DISTRICT, SHENZHEN, GUANGDONG, CHINA  
**SATIMO COMOSAR REFERENCE DIPOLE**  
FREQUENCY: 750 MHZ  
SERIAL NO.: SN 07/14 DIP 0G750-302

Calibrated at SATIMO US  
2105 Barrett Park Dr. - Kennesaw, GA 30144



09/29/2021

*Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in SATIMO USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



测股份  
ting Lab

测股份  
ting Lab

测股份  
ting Lab





SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.3.14.SATU.A

股份  
g Lab

|                      | <i>Name</i>   | <i>Function</i> | <i>Date</i> | <i>Signature</i> |
|----------------------|---------------|-----------------|-------------|------------------|
| <i>Prepared by :</i> | Jérôme LUC    | Product Manager | 10/12/2021  |                  |
| <i>Checked by :</i>  | Jérôme LUC    | Product Manager | 10/12/2021  |                  |
| <i>Approved by :</i> | Kim RUTKOWSKI | Quality Manager | 10/12/2021  |                  |

|                       |   |
|-----------------------|---|
|                       | <i>Customer Name</i>                                  |
| <i>Distribution :</i> | Shenzhen LCS<br>Compliance Testing<br>Laboratory Ltd. |

| <i>Issue</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|----------------------|
| A            | 10/12/2021  | Initial release      |
|              |             |                      |
|              |             |                      |

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.  
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

股份  
g Lab





股份  
ig Lab

TABLE OF CONTENTS

1 Introduction..... 4

2 Device Under Test ..... 4

3 Product Description ..... 4

    3.1 General Information ..... 4

4 Measurement Method ..... 5

    4.1 Return Loss Requirements ..... 5

    4.2 Mechanical Requirements ..... 5

5 Measurement Uncertainty..... 5

    5.1 Return Loss ..... 5

    5.2 Dimension Measurement ..... 5

    5.3 Validation Measurement ..... 5

6 Calibration Measurement Results ..... 6

    6.1 Return Loss and Impedance ..... 6

    6.2 Mechanical Dimensions ..... 6

7 Validation measurement ..... 7

    7.1 Head Liquid Measurement ..... 7

    7.2 SAR Measurement Result With Head Liquid ..... 7

    7.3 Body Liquid Measurement ..... 9

    7.4 SAR Measurement Result With Body Liquid ..... 9

8 List of Equipment ..... 11

股份  
ig Lab

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO.  
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

股份  
ig Lab





## 1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

## 2 DEVICE UNDER TEST

| Device Under Test              |                                  |
|--------------------------------|----------------------------------|
| Device Type                    | COMOSAR 750 MHz REFERENCE DIPOLE |
| Manufacturer                   | Satimo                           |
| Model                          | SID750                           |
| Serial Number                  | SN 07/14 DIP 0G750-302           |
| Product Condition (new / used) | New                              |

A yearly calibration interval is recommended.

## 3 PRODUCT DESCRIPTION

### 3.1 GENERAL INFORMATION

Satimo's COMOSAR Validation Dipoles are built in accordance to the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards. The product is designed for use with the COMOSAR test bench only.



Figure 1 – Satimo COMOSAR Validation Dipole

Page: 4/11

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*





股份  
ig Lab

#### 4 MEASUREMENT METHOD

The IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

##### 4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards.

##### 4.2 MECHANICAL REQUIREMENTS

The IEEE Std. 1528 and CEI/IEC 62209 standards specify the mechanical components and dimensions of the validation dipoles, with the dimensions frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness.

#### 5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

##### 5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.1 dB                              |

##### 5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 3 - 300     | 0.05 mm                        |

##### 5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 20.3 %               |
| 10 g        | 20.1 %               |

Page: 5/11

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

股份  
ig Lab



股份  
ig Lab




SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.3.14.SATU.A

股份  
ig Lab

6 CALIBRATION MEASUREMENT RESULTS

6.1 RETURN LOSS AND IMPEDANCE

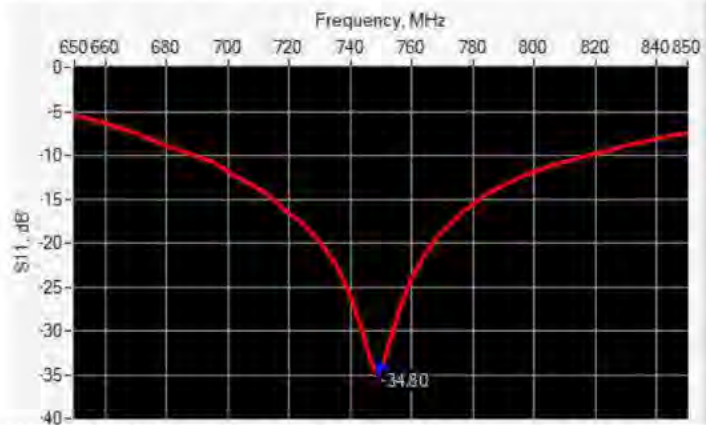

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance       |
|-----------------|------------------|------------------|-----------------|
| 750             | -34.80           | -20              | 50.7 Ω + 1.6 jΩ |

6.2 MECHANICAL DIMENSIONS

| Frequency MHz | L mm       |          | h mm       |          | d mm      |          |
|---------------|------------|----------|------------|----------|-----------|----------|
|               | required   | measured | required   | measured | required  | measured |
| 300           | 420.0 ±1 % |          | 250.0 ±1 % |          | 6.35 ±1 % |          |
| 450           | 290.0 ±1 % |          | 166.7 ±1 % |          | 6.35 ±1 % |          |
| 750           | 176.0 ±1 % | PASS     | 100.0 ±1 % | PASS     | 6.35 ±1 % | PASS     |
| 835           | 161.0 ±1 % |          | 89.8 ±1 %  |          | 3.6 ±1 %  |          |
| 900           | 149.0 ±1 % |          | 83.3 ±1 %  |          | 3.6 ±1 %  |          |
| 1450          | 89.1 ±1 %  |          | 51.7 ±1 %  |          | 3.6 ±1 %  |          |
| 1500          | 80.5 ±1 %  |          | 50.0 ±1 %  |          | 3.6 ±1 %  |          |
| 1640          | 79.0 ±1 %  |          | 45.7 ±1 %  |          | 3.6 ±1 %  |          |
| 1750          | 75.2 ±1 %  |          | 42.9 ±1 %  |          | 3.6 ±1 %  |          |
| 1800          | 72.0 ±1 %  |          | 41.7 ±1 %  |          | 3.6 ±1 %  |          |
| 1900          | 68.0 ±1 %  |          | 39.5 ±1 %  |          | 3.6 ±1 %  |          |
| 1950          | 66.3 ±1 %  |          | 38.5 ±1 %  |          | 3.6 ±1 %  |          |
| 2000          | 64.5 ±1 %  |          | 37.5 ±1 %  |          | 3.6 ±1 %  |          |
| 2100          | 61.0 ±1 %  |          | 35.7 ±1 %  |          | 3.6 ±1 %  |          |
| 2300          | 55.5 ±1 %  |          | 32.6 ±1 %  |          | 3.6 ±1 %  |          |
| 2450          | 51.5 ±1 %  |          | 30.4 ±1 %  |          | 3.6 ±1 %  |          |
| 2600          | 48.5 ±1 %  |          | 28.8 ±1 %  |          | 3.6 ±1 %  |          |
| 3000          | 41.5 ±1 %  |          | 25.0 ±1 %  |          | 3.6 ±1 %  |          |
| 3500          | 37.0 ±1 %  |          | 26.4 ±1 %  |          | 3.6 ±1 %  |          |
| 3700          | 34.7 ±1 %  |          | 26.4 ±1 %  |          | 3.6 ±1 %  |          |

Page: 6/11

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

股份  
ig Lab





股份  
g Lab

### 7 VALIDATION MEASUREMENT

The IEEE Std. 1528, OET 65 Bulletin C and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

#### 7.1 HEAD LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|--|----------|-------------------------------|----------|
|                  | required                               | measured | required                      | measured |
| 300              | 45.3 ±5 %                              |          | 0.87 ±5 %                     |          |
| 450              | 43.5 ±5 %                              |          | 0.87 ±5 %                     |          |
| 750              | 41.9 ±5 %                              | PASS     | 0.89 ±5 %                     | PASS     |
| 835              | 41.5 ±5 %                              |          | 0.90 ±5 %                     |          |
| 900              | 41.5 ±5 %                              |          | 0.97 ±5 %                     |          |
| 1450             | 40.5 ±5 %                              |          | 1.20 ±5 %                     |          |
| 1500             | 40.4 ±5 %                              |          | 1.23 ±5 %                     |          |
| 1640             | 40.2 ±5 %                              |          | 1.31 ±5 %                     |          |
| 1750             | 40.1 ±5 %                              |          | 1.37 ±5 %                     |          |
| 1800             | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 1900             | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 1950             | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 2000             | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 2100             | 39.8 ±5 %                              |          | 1.49 ±5 %                     |          |
| 2300             | 39.5 ±5 %                              |          | 1.67 ±5 %                     |          |
| 2450             | 39.2 ±5 %                              |          | 1.80 ±5 %                     |          |
| 2600             | 39.0 ±5 %                              |          | 1.96 ±5 %                     |          |
| 3000             | 38.5 ±5 %                              |          | 2.40 ±5 %                     |          |
| 3500             | 37.9 ±5 %                              |          | 2.91 ±5 %                     |          |

股份  
g Lab

#### 7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.

|   |   |
|---|---|
| Software                                  | OPENSAR V4  |
| Phantom                                   | SN 20/09 SAM71  |
| Probe                                     | SN 18/11 EPG122   |
| Liquid                                    | Head Liquid Values: $\epsilon_r$ : 42.1 $\sigma$ : 0.89 |
| Distance between dipole center and liquid | 15.0 mm   |
| Area scan resolution                      | dx=8mm/dy=8mm   |

Page: 7/11

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

股份  
g Lab





SAR REFERENCE DIPOLE CALIBRATION REPORT


Ref: ACR.287.3.14.SATIM.A

股份  
ig Lab

|                      |                     |
|----------------------|---------------------|
| Zoon Scan Resolution | dx=8mm/dy=8m/dz=5mm |
| Frequency            | 750 MHz             |
| Input power          | 20 dBm              |
| Liquid Temperature   | 21 °C               |
| Lab Temperature      | 21 °C               |
| Lab Humidity         | 45 %                |

| Frequency MHz | 1 g SAR (W/kg/W) |             | 10 g SAR (W/kg/W) |             |
|---------------|------------------|-------------|-------------------|-------------|
|               | required         | measured    | required          | measured    |
| 300           | 2.85             |             | 1.94              |             |
| 450           | 4.58             |             | 3.06              |             |
| 750           | 8.49             | 8.38 (0.84) | 5.55              | 5.53 (0.55) |
| 835           | 9.56             |             | 6.22              |             |
| 900           | 10.9             |             | 6.99              |             |
| 1450          | 29               |             | 16                |             |
| 1500          | 30.5             |             | 16.8              |             |
| 1640          | 34.2             |             | 18.4              |             |
| 1750          | 36.4             |             | 19.3              |             |
| 1800          | 38.4             |             | 20.1              |             |
| 1900          | 39.7             |             | 20.5              |             |
| 1950          | 40.5             |             | 20.9              |             |
| 2000          | 41.1             |             | 21.1              |             |
| 2100          | 43.6             |             | 21.9              |             |
| 2300          | 48.7             |             | 23.3              |             |
| 2450          | 52.4             |             | 24                |             |
| 2600          | 55.3             |             | 24.6              |             |
| 3000          | 63.8             |             | 25.7              |             |
| 3500          | 67.1             |             | 25                |             |

股份  
ig Lab

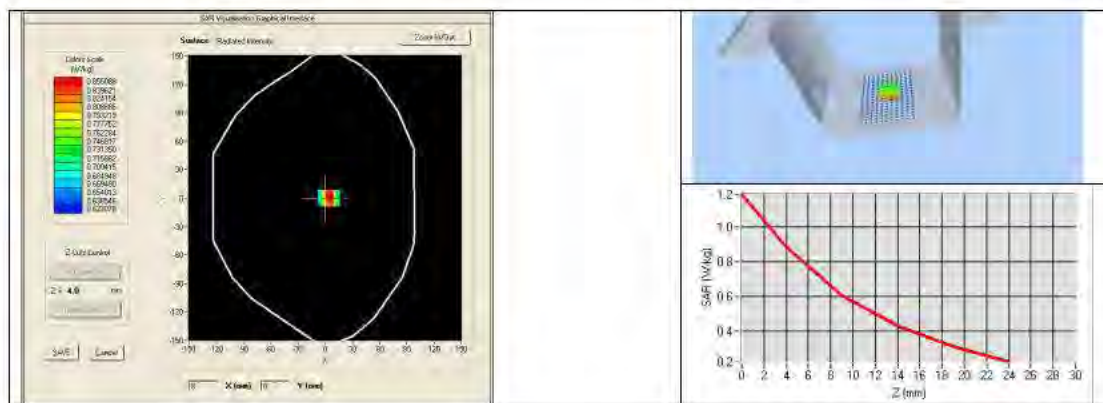

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.

股份  
ig Lab





SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.3.14.SATIMA

股份  
ig Lab

7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|--|----------|-------------------------------|----------|
|                  | required                               | measured | required                      | measured |
| 150              | 61.9 ±5 %                              |          | 0.80 ±5 %                     |          |
| 300              | 58.2 ±5 %                              |          | 0.92 ±5 %                     |          |
| 450              | 56.7 ±5 %                              |          | 0.94 ±5 %                     |          |
| 750              | 55.5 ±5 %                              | PASS     | 0.96 ±5 %                     | PASS     |
| 835              | 55.2 ±5 %                              |          | 0.97 ±5 %                     |          |
| 900              | 55.0 ±5 %                              |          | 1.05 ±5 %                     |          |
| 915              | 55.0 ±5 %                              |          | 1.06 ±5 %                     |          |
| 1450             | 54.0 ±5 %                              |          | 1.30 ±5 %                     |          |
| 1610             | 53.8 ±5 %                              |          | 1.40 ±5 %                     |          |
| 1800             | 53.3 ±5 %                              |          | 1.52 ±5 %                     |          |
| 1900             | 53.3 ±5 %                              |          | 1.52 ±5 %                     |          |
| 2000             | 53.3 ±5 %                              |          | 1.52 ±5 %                     |          |
| 2100             | 53.2 ±5 %                              |          | 1.62 ±5 %                     |          |
| 2450             | 52.7 ±5 %                              |          | 1.95 ±5 %                     |          |
| 2600             | 52.5 ±5 %                              |          | 2.16 ±5 %                     |          |
| 3000             | 52.0 ±5 %                              |          | 2.73 ±5 %                     |          |
| 3500             | 51.3 ±5 %                              |          | 3.31 ±5 %                     |          |
| 5200             | 49.0 ±10 %                             |          | 5.30 ±10 %                    |          |
| 5300             | 48.9 ±10 %                             |          | 5.42 ±10 %                    |          |
| 5400             | 48.7 ±10 %                             |          | 5.53 ±10 %                    |          |
| 5500             | 48.6 ±10 %                             |          | 5.65 ±10 %                    |          |
| 5600             | 48.5 ±10 %                             |          | 5.77 ±10 %                    |          |
| 5800             | 48.2 ±10 %                             |          | 6.00 ±10 %                    |          |

股份  
ig Lab

7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|   |   |
|---|---|
| Software                                  | OPENSAR V4  |
| Phantom                                   | SN 20/09 SAM71  |
| Probe                                     | SN 18/11 EPG122   |
| Liquid                                    | Body Liquid Values: $\epsilon_r$ : 56.6 $\sigma$ : 0.99 |
| Distance between dipole center and liquid | 15.0 mm   |
| Area scan resolution                      | $dx=8mm/dy=8mm$   |
| Zoon Scan Resolution                      | $dx=8mm/dy=8m/dz=5mm$                                   |
| Frequency                                 | 750 MHz   |
| Input power                               | 20 dBm  |
| Liquid Temperature                        | 21 °C   |
| Lab Temperature                           | 21 °C   |
| Lab Humidity                              | 45 %  |

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.

股份  
ig Lab








SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.3.14.SATL.A

股份  
ig Lab

| Frequency MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|---------------|------------------|-------------------|
|               | measured         | measured          |
| 750           | 8.77 (0.88)      | 5.78 (0.58)       |

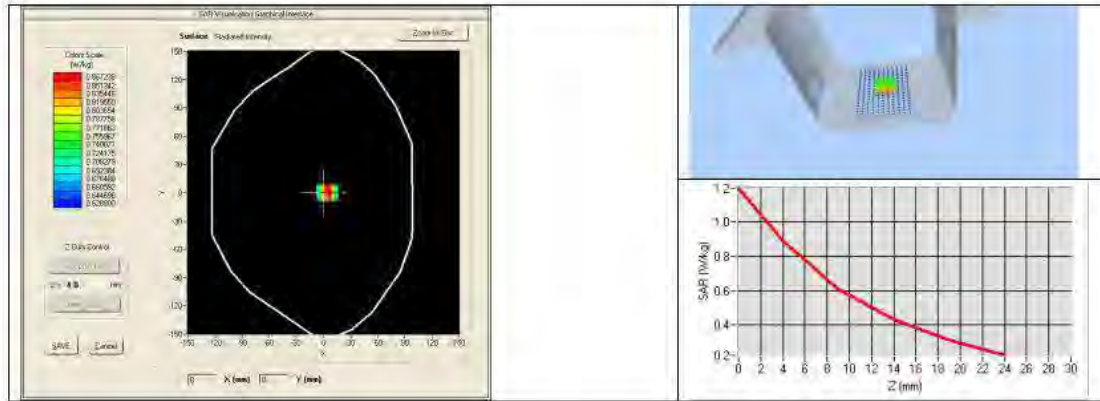

股份  
ig Lab

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

股份  
ig Lab





股份  
ig Lab

8 LIST OF EQUIPMENT

| Equipment Summary Sheet         |                      |                    |   |   |
|---------------------------------|----------------------|--------------------|---|---|
| Equipment Description           | Manufacturer / Model | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                     | Satimo               | SN-20/09-SAM71     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench              | Version 3            | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                | Rhode & Schwarz ZVA  | SN100132           | 02/2021                                       | 02/2024                                       |
| Calipers                        | Carrera              | CALIPER-01         | 12/2021                                       | 12/2024                                       |
| Reference Probe                 | Satimo               | EPG122 SN 18/11    | 10/2022                                       | 10/2025                                       |
| Multimeter                      | Keithley 2000        | 1188656            | 12/2021                                       | 12/2024                                       |
| Signal Generator                | Agilent E4438C       | MY49070581         | 12/2018                                       | 12/2024                                       |
| Amplifier                       | Aethercomm           | SN 046             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                     | HP E4418A            | US38261498         | 12/2021                                       | 12/2024                                       |
| Power Sensor                    | HP ECP-E26A          | US37181460         | 12/2021                                       | 12/2024                                       |
| Directional Coupler             | Narda 4216-20        | 01386              | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature and Humidity Sensor | Control Company      | 11-661-9           | 8/2021  | 8/2024  |

股份  
ig Lab

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.

股份  
ig Lab





### 5.2 SID835Dipole Calibration Certificate





### SAR Reference Dipole Calibration Report

Ref : ACR.287.4.14.SATU.A

**SHENZHEN LCS COMPLIANCE TESTING  
LABORATORY LTD.**  
**1F., XINGYUAN INDUSTRIAL PARK, TONGDA ROAD,  
BAO'AN BLVD**  
**BAO'AN DISTRICT, SHENZHEN, GUANGDONG, CHINA**  
**SATIMO COMOSAR REFERENCE DIPOLE**  
**FREQUENCY: 835 MHZ**  
**SERIAL NO.: SN 07/14 DIP 0G835-303**

**Calibrated at SATIMO US**  
**2105 Barrett Park Dr. - Kennesaw, GA 30144**




**09/29/2021**

*Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in SATIMO USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



股份  
ing Lab

股份  
ing Lab

股份  
ing Lab



SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.2874.14.SATIM.A

|               | Name          | Function        | Date       | Signature |
|---------------|---------------|-----------------|------------|-----------|
| Prepared by : | Jérôme LUC    | Product Manager | 10/12/2021 |           |
| Checked by :  | Jérôme LUC    | Product Manager | 10/12/2021 |           |
| Approved by : | Kim RUTKOWSKI | Quality Manager | 10/12/2021 |           |

|                | Customer Name                                   |
|----------------|---|
| Distribution : | Shenzhen LCS Compliance Testing Laboratory Ltd. |

| Issue | Date       | Modifications   |
|-------|------------|-----------------|
| A     | 10/12/2021 | Initial release |
|       |            |                 |
|       |            |                 |

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*





SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.4.14.SATL.A

TABLE OF CONTENTS

- 1 Introduction..... 4
- 2 Device Under Test ..... 4
- 3 Product Description ..... 4
  - 3.1 General Information ..... 4
- 4 Measurement Method ..... 5
  - 4.1 Return Loss Requirements ..... 5
  - 4.2 Mechanical Requirements ..... 5
- 5 Measurement Uncertainty..... 5
  - 5.1 Return Loss ..... 5
  - 5.2 Dimension Measurement ..... 5
  - 5.3 Validation Measurement ..... 5
- 6 Calibration Measurement Results ..... 6
  - 6.1 Return Loss and Impedance ..... 6
  - 6.2 Mechanical Dimensions ..... 6
- 7 Validation measurement ..... 7
  - 7.1 Head Liquid Measurement ..... 7
  - 7.2 SAR Measurement Result With Head Liquid ..... 7
  - 7.3 Body Liquid Measurement ..... 9
  - 7.4 SAR Measurement Result With Body Liquid ..... 9
- 8 List of Equipment ..... 11

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.





**1 INTRODUCTION**

This document contains a summary of the requirements set forth by the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

**2 DEVICE UNDER TEST**

| Device Under Test              |                                  |
|--------------------------------|----------------------------------|
| Device Type                    | COMOSAR 835 MHz REFERENCE DIPOLE |
| Manufacturer                   | Satimo                           |
| Model                          | SID835                           |
| Serial Number                  | SN 07/14 DIP 0G835-303           |
| Product Condition (new / used) | New                              |

A yearly calibration interval is recommended.

**3 PRODUCT DESCRIPTION**

**3.1 GENERAL INFORMATION**

Satimo's COMOSAR Validation Dipoles are built in accordance to the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards. The product is designed for use with the COMOSAR test bench only.



**Figure 1 – Satimo COMOSAR Validation Dipole**





**4 MEASUREMENT METHOD**

The IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

**4.1 RETURN LOSS REQUIREMENTS**

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards.

**4.2 MECHANICAL REQUIREMENTS**

The IEEE Std. 1528 and CEI/IEC 62209 standards specify the mechanical components and dimensions of the validation dipoles, with the dimensions frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness.

**5 MEASUREMENT UNCERTAINTY**

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

**5.1 RETURN LOSS**

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.1 dB                              |

**5.2 DIMENSION MEASUREMENT**

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 3 - 300     | 0.05 mm                        |

**5.3 VALIDATION MEASUREMENT**

The guidelines outlined in the IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 20.3 %               |
| 10 g        | 20.1 %               |








SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.4.14.SATU.A

6 CALIBRATION MEASUREMENT RESULTS

6.1 RETURN LOSS AND IMPEDANCE

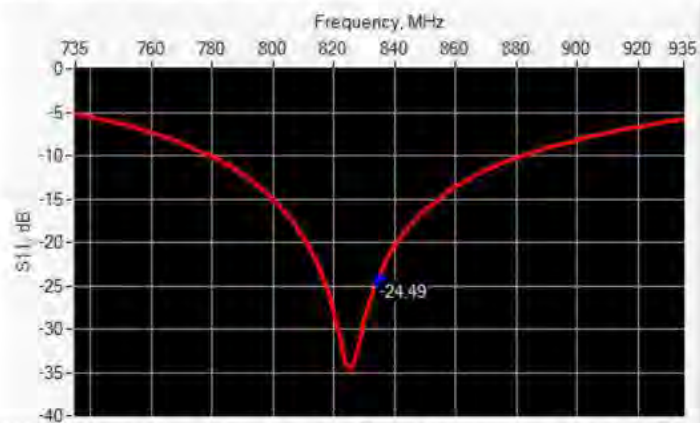

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance       |
|-----------------|------------------|------------------|-----------------|
| 835             | -24.49           | -20              | 54.9 Ω + 2.8 jΩ |

6.2 MECHANICAL DIMENSIONS

| Frequency MHz | L mm       |          | h mm       |          | d mm      |          |
|---------------|------------|----------|------------|----------|-----------|----------|
|               | required   | measured | required   | measured | required  | measured |
| 300           | 420.0 ±1 % |          | 250.0 ±1 % |          | 6.35 ±1 % |          |
| 450           | 290.0 ±1 % |          | 166.7 ±1 % |          | 6.35 ±1 % |          |
| 750           | 176.0 ±1 % |          | 100.0 ±1 % |          | 6.35 ±1 % |          |
| 835           | 161.0 ±1 % | PASS     | 89.8 ±1 %  | PASS     | 3.6 ±1 %  | PASS     |
| 900           | 149.0 ±1 % |          | 83.3 ±1 %  |          | 3.6 ±1 %  |          |
| 1450          | 89.1 ±1 %  |          | 51.7 ±1 %  |          | 3.6 ±1 %  |          |
| 1500          | 80.5 ±1 %  |          | 50.0 ±1 %  |          | 3.6 ±1 %  |          |
| 1640          | 79.0 ±1 %  |          | 45.7 ±1 %  |          | 3.6 ±1 %  |          |
| 1750          | 75.2 ±1 %  |          | 42.9 ±1 %  |          | 3.6 ±1 %  |          |
| 1800          | 72.0 ±1 %  |          | 41.7 ±1 %  |          | 3.6 ±1 %  |          |
| 1900          | 68.0 ±1 %  |          | 39.5 ±1 %  |          | 3.6 ±1 %  |          |
| 1950          | 66.3 ±1 %  |          | 38.5 ±1 %  |          | 3.6 ±1 %  |          |
| 2000          | 64.5 ±1 %  |          | 37.5 ±1 %  |          | 3.6 ±1 %  |          |
| 2100          | 61.0 ±1 %  |          | 35.7 ±1 %  |          | 3.6 ±1 %  |          |
| 2300          | 55.5 ±1 %  |          | 32.6 ±1 %  |          | 3.6 ±1 %  |          |
| 2450          | 51.5 ±1 %  |          | 30.4 ±1 %  |          | 3.6 ±1 %  |          |
| 2600          | 48.5 ±1 %  |          | 28.8 ±1 %  |          | 3.6 ±1 %  |          |
| 3000          | 41.5 ±1 %  |          | 25.0 ±1 %  |          | 3.6 ±1 %  |          |
| 3500          | 37.0 ±1 %  |          | 26.4 ±1 %  |          | 3.6 ±1 %  |          |
| 3700          | 34.7 ±1 %  |          | 26.4 ±1 %  |          | 3.6 ±1 %  |          |

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.





SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.4.14.SATIM.A

股份  
ig Lab

7 VALIDATION MEASUREMENT

The IEEE Std. 1528, OET 65 Bulletin C and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

7.1 HEAD LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|--|----------|-------------------------------|----------|
|                  | required                               | measured | required                      | measured |
| 300              | 45.3 ±5 %                              |          | 0.87 ±5 %                     |          |
| 450              | 43.5 ±5 %                              |          | 0.87 ±5 %                     |          |
| 750              | 41.9 ±5 %                              |          | 0.89 ±5 %                     |          |
| 835              | 41.5 ±5 %                              | PASS     | 0.90 ±5 %                     | PASS     |
| 900              | 41.5 ±5 %                              |          | 0.97 ±5 %                     |          |
| 1450             | 40.5 ±5 %                              |          | 1.20 ±5 %                     |          |
| 1500             | 40.4 ±5 %                              |          | 1.23 ±5 %                     |          |
| 1640             | 40.2 ±5 %                              |          | 1.31 ±5 %                     |          |
| 1750             | 40.1 ±5 %                              |          | 1.37 ±5 %                     |          |
| 1800             | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 1900             | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 1950             | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 2000             | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 2100             | 39.8 ±5 %                              |          | 1.49 ±5 %                     |          |
| 2300             | 39.5 ±5 %                              |          | 1.67 ±5 %                     |          |
| 2450             | 39.2 ±5 %                              |          | 1.80 ±5 %                     |          |
| 2600             | 39.0 ±5 %                              |          | 1.96 ±5 %                     |          |
| 3000             | 38.5 ±5 %                              |          | 2.40 ±5 %                     |          |
| 3500             | 37.9 ±5 %                              |          | 2.91 ±5 %                     |          |

股份  
ig Lab

7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.

|   |  |
|---|--|
| Software                                  | OPENSAR V4   |
| Phantom                                   | SN 20/09 SAM71   |
| Probe                                     | SN 18/11 EPG122  |
| Liquid                                    | Head Liquid Values: $\epsilon_{ps}^*$ : 42.3 $\sigma$ : 0.92 |
| Distance between dipole center and liquid | 15.0 mm  |
| Area scan resolution                      | $dx=8mm/dy=8mm$  |

Page: 7/11

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

股份  
ig Lab





SAR REFERENCE DIPOLE CALIBRATION REPORT


Ref: ACR.287.4.14.SATL.A

股份  
ig Lab

|                      |                     |
|----------------------|---------------------|
| Zoon Scan Resolution | dx=8mm/dy=8m/dz=5mm |
| Frequency            | 835 MHz             |
| Input power          | 20 dBm              |
| Liquid Temperature   | 21 °C               |
| Lab Temperature      | 21 °C               |
| Lab Humidity         | 45 %                |

| Frequency<br>MHz | 1 g SAR (W/kg/W) |             | 10 g SAR (W/kg/W) |             |
|------------------|------------------|-------------|-------------------|-------------|
|                  | required         | measured    | required          | measured    |
| 300              | 2.85             |             | 1.94              |             |
| 450              | 4.58             |             | 3.06              |             |
| 750              | 8.49             |             | 5.55              |             |
| 835              | 9.56             | 9.60 (0.96) | 6.22              | 6.20 (0.62) |
| 900              | 10.9             |             | 6.99              |             |
| 1450             | 29               |             | 16                |             |
| 1500             | 30.5             |             | 16.8              |             |
| 1640             | 34.2             |             | 18.4              |             |
| 1750             | 36.4             |             | 19.3              |             |
| 1800             | 38.4             |             | 20.1              |             |
| 1900             | 39.7             |             | 20.5              |             |
| 1950             | 40.5             |             | 20.9              |             |
| 2000             | 41.1             |             | 21.1              |             |
| 2100             | 43.6             |             | 21.9              |             |
| 2300             | 48.7             |             | 23.3              |             |
| 2450             | 52.4             |             | 24                |             |
| 2600             | 55.3             |             | 24.6              |             |
| 3000             | 63.8             |             | 25.7              |             |
| 3500             | 67.1             |             | 25                |             |

股份  
ig Lab

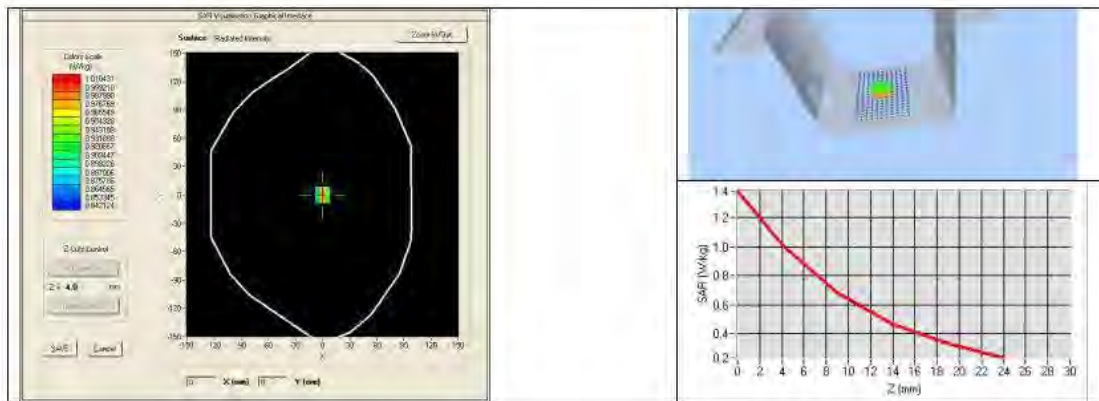

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.

股份  
ig Lab





SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.4.14.SATIMA

7.3 BODY LIQUID MEASUREMENT

| Frequency MHz | Relative permittivity ( $\epsilon_r$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|---------------|--|----------|-------------------------------|----------|
|               | required                               | measured | required                      | measured |
| 150           | 61.9 ±5 %                              |          | 0.80 ±5 %                     |          |
| 300           | 58.2 ±5 %                              |          | 0.92 ±5 %                     |          |
| 450           | 56.7 ±5 %                              |          | 0.94 ±5 %                     |          |
| 750           | 55.5 ±5 %                              |          | 0.96 ±5 %                     |          |
| 835           | 55.2 ±5 %                              | PASS     | 0.97 ±5 %                     | PASS     |
| 900           | 55.0 ±5 %                              |          | 1.05 ±5 %                     |          |
| 915           | 55.0 ±5 %                              |          | 1.06 ±5 %                     |          |
| 1450          | 54.0 ±5 %                              |          | 1.30 ±5 %                     |          |
| 1610          | 53.8 ±5 %                              |          | 1.40 ±5 %                     |          |
| 1800          | 53.3 ±5 %                              |          | 1.52 ±5 %                     |          |
| 1900          | 53.3 ±5 %                              |          | 1.52 ±5 %                     |          |
| 2000          | 53.3 ±5 %                              |          | 1.52 ±5 %                     |          |
| 2100          | 53.2 ±5 %                              |          | 1.62 ±5 %                     |          |
| 2450          | 52.7 ±5 %                              |          | 1.95 ±5 %                     |          |
| 2600          | 52.5 ±5 %                              |          | 2.16 ±5 %                     |          |
| 3000          | 52.0 ±5 %                              |          | 2.73 ±5 %                     |          |
| 3500          | 51.3 ±5 %                              |          | 3.31 ±5 %                     |          |
| 5200          | 49.0 ±10 %                             |          | 5.30 ±10 %                    |          |
| 5300          | 48.9 ±10 %                             |          | 5.42 ±10 %                    |          |
| 5400          | 48.7 ±10 %                             |          | 5.53 ±10 %                    |          |
| 5500          | 48.6 ±10 %                             |          | 5.65 ±10 %                    |          |
| 5600          | 48.5 ±10 %                             |          | 5.77 ±10 %                    |          |
| 5800          | 48.2 ±10 %                             |          | 6.00 ±10 %                    |          |

7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|   |  |
|---|--|
| Software                                  | OPENSAR V4   |
| Phantom                                   | SN 20/09 SAM71   |
| Probe                                     | SN 18/11 EPG122  |
| Liquid                                    | Body Liquid Values: $\epsilon_{ps}$ : 54.1 $\sigma$ : 0.97 |
| Distance between dipole center and liquid | 15.0 mm  |
| Area scan resolution                      | $dx=8mm/dy=8mm$  |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                     |
| Frequency                                 | 835 MHz  |
| Input power                               | 20 dBm   |
| Liquid Temperature                        | 21 °C  |
| Lab Temperature                           | 21 °C  |
| Lab Humidity                              | 45 %   |

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.






SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.4.14.SATL.A

| Frequency MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|---------------|------------------|-------------------|
|               | measured         | measured          |
| 835           | 9.90 (0.99)      | 6.39 (0.64)       |

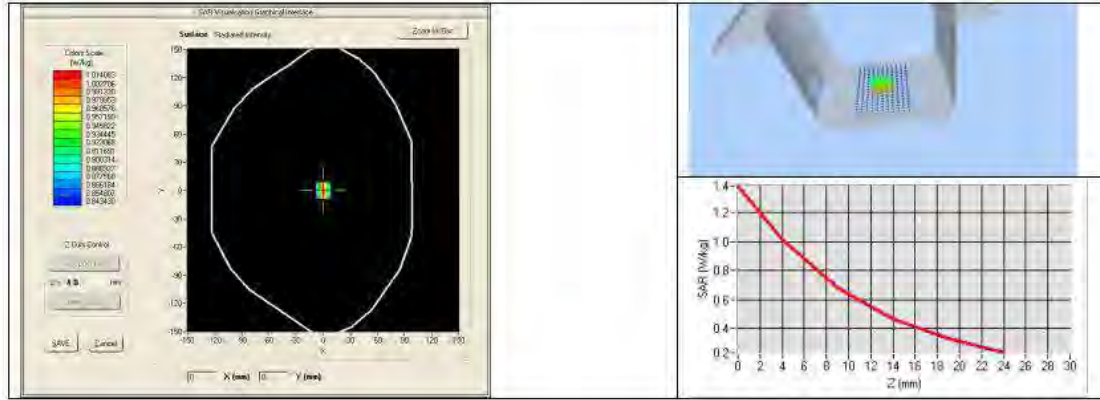

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.





SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR-2874-14-SATIMA

8 LIST OF EQUIPMENT

| Equipment Summary Sheet         |                      |                    |   |   |
|---------------------------------|----------------------|--------------------|---|---|
| Equipment Description           | Manufacturer / Model | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                     | Satimo               | SN-20/09-SAM71     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench              | Version 3            | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                | Rhode & Schwarz ZVA  | SN100132           | 02/2021                                       | 02/2024                                       |
| Calipers                        | Carrera              | CALIPER-01         | 12/2021                                       | 12/2024                                       |
| Reference Probe                 | Satimo               | EPG122 SN 18/11    | 10/2023                                       | 10/2024                                       |
| Multimeter                      | Keithley 2000        | 1188656            | 12/2021                                       | 12/2024                                       |
| Signal Generator                | Agilent E4438C       | MY49070581         | 12/2021                                       | 12/2024                                       |
| Amplifier                       | Aethercomm           | SN 046             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                     | HP E4418A            | US38261498         | 12/2021                                       | 12/2024                                       |
| Power Sensor                    | HP ECP-E26A          | US37181460         | 12/2021                                       | 12/2024                                       |
| Directional Coupler             | Narda 4216-20        | 01386              | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature and Humidity Sensor | Control Company      | 11-661-9           | 8/2021  | 8/2024  |

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*



### 5.3 SID1800 Dipole Calibration Certificate



## SAR Reference Dipole Calibration Report

Ref: ACR.287.6.14.SATU.A

**SHENZHEN LCS COMPLIANCE TESTING  
LABORATORY LTD.**  
**1F., XINGYUAN INDUSTRIAL PARK, TONGDA ROAD,  
BAO'AN BLVD**  
**BAO'AN DISTRICT, SHENZHEN, GUANGDONG, CHINA**  
**SATIMO COMOSAR REFERENCE DIPOLE**  
**FREQUENCY: 1800 MHZ**  
**SERIAL NO.: SN 07/14 DIP 1G800-301**

**Calibrated at SATIMO US**  
**2105 Barrett Park Dr. - Kennesaw, GA 30144**




**09/29/2021**

*Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in SATIMO USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



股份  
ing Lab

股份  
ing Lab

股份  
ing Lab



SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.6.14.SATU.A

|                      | <i>Name</i>   | <i>Function</i> | <i>Date</i> | <i>Signature</i>   |
|----------------------|---------------|-----------------|-------------|--------------------|
| <i>Prepared by :</i> | Jérôme LUC    | Product Manager | 10/12/2021  | <i>[Signature]</i> |
| <i>Checked by :</i>  | Jérôme LUC    | Product Manager | 10/12/2021  | <i>[Signature]</i> |
| <i>Approved by :</i> | Kim RUTKOWSKI | Quality Manager | 10/12/2021  | <i>[Signature]</i> |

|                       | <i>Customer Name</i>                            |
|-----------------------|---|
| <i>Distribution :</i> | Shenzhen LCS Compliance Testing Laboratory Ltd. |

| <i>Issue</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|----------------------|
| A            | 10/12/2021  | Initial release      |
|              |             |                      |
|              |             |                      |

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*







TABLE OF CONTENTS

- 1 Introduction..... 4
- 2 Device Under Test ..... 4
- 3 Product Description ..... 4
  - 3.1 General Information ..... 4
- 4 Measurement Method ..... 5
  - 4.1 Return Loss Requirements ..... 5
  - 4.2 Mechanical Requirements ..... 5
- 5 Measurement Uncertainty..... 5
  - 5.1 Return Loss ..... 5
  - 5.2 Dimension Measurement ..... 5
  - 5.3 Validation Measurement ..... 5
- 6 Calibration Measurement Results ..... 6
  - 6.1 Return Loss and Impedance ..... 6
  - 6.2 Mechanical Dimensions ..... 6
- 7 Validation measurement ..... 7
  - 7.1 Head Liquid Measurement ..... 7
  - 7.2 SAR Measurement Result With Head Liquid ..... 7
  - 7.3 Body Liquid Measurement ..... 9
  - 7.4 SAR Measurement Result With Body Liquid ..... 9
- 8 List of Equipment ..... 11

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.





**1 INTRODUCTION**

This document contains a summary of the requirements set forth by the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

**2 DEVICE UNDER TEST**

| Device Under Test              |                                   |
|--------------------------------|-----------------------------------|
| Device Type                    | COMOSAR 1800 MHz REFERENCE DIPOLE |
| Manufacturer                   | Satimo                            |
| Model                          | SID1800                           |
| Serial Number                  | SN 07/14 DIP 1G800-301            |
| Product Condition (new / used) | New                               |

A yearly calibration interval is recommended.

**3 PRODUCT DESCRIPTION**

**3.1 GENERAL INFORMATION**

Satimo's COMOSAR Validation Dipoles are built in accordance to the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards. The product is designed for use with the COMOSAR test bench only.



**Figure 1 – Satimo COMOSAR Validation Dipole**





**4 MEASUREMENT METHOD**

The IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

**4.1 RETURN LOSS REQUIREMENTS**

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards.

**4.2 MECHANICAL REQUIREMENTS**

The IEEE Std. 1528 and CEI/IEC 62209 standards specify the mechanical components and dimensions of the validation dipoles, with the dimensions frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness.

**5 MEASUREMENT UNCERTAINTY**

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

**5.1 RETURN LOSS**

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.1 dB                              |

**5.2 DIMENSION MEASUREMENT**

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 3 - 300     | 0.05 mm                        |

**5.3 VALIDATION MEASUREMENT**

The guidelines outlined in the IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 20.3 %               |
| 10 g        | 20.1 %               |






SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.6.14.SATU.A

6 CALIBRATION MEASUREMENT RESULTS

6.1 RETURN LOSS AND IMPEDANCE

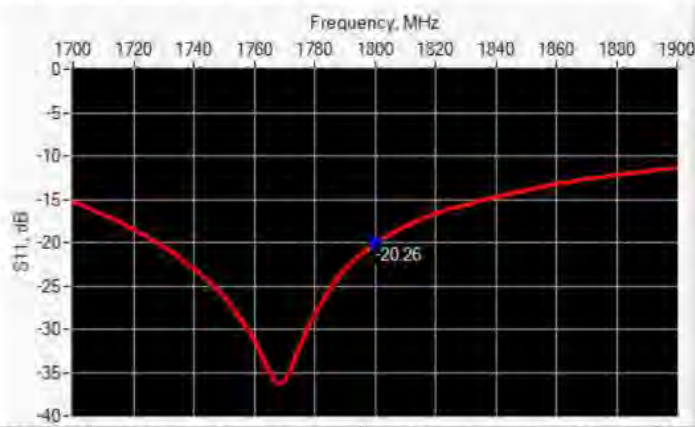

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance       |
|-----------------|------------------|------------------|-----------------|
| 1800            | -20.26           | -20              | 43.1 Ω + 6.9 jΩ |

6.2 MECHANICAL DIMENSIONS

| Frequency MHz | L mm       |          | h mm       |          | d mm      |          |
|---------------|------------|----------|------------|----------|-----------|----------|
|               | required   | measured | required   | measured | required  | measured |
| 300           | 420.0 ±1 % |          | 250.0 ±1 % |          | 6.35 ±1 % |          |
| 450           | 290.0 ±1 % |          | 166.7 ±1 % |          | 6.35 ±1 % |          |
| 750           | 176.0 ±1 % |          | 100.0 ±1 % |          | 6.35 ±1 % |          |
| 835           | 161.0 ±1 % |          | 89.8 ±1 %  |          | 3.6 ±1 %  |          |
| 900           | 149.0 ±1 % |          | 83.3 ±1 %  |          | 3.6 ±1 %  |          |
| 1450          | 89.1 ±1 %  |          | 51.7 ±1 %  |          | 3.6 ±1 %  |          |
| 1500          | 80.5 ±1 %  |          | 50.0 ±1 %  |          | 3.6 ±1 %  |          |
| 1640          | 79.0 ±1 %  |          | 45.7 ±1 %  |          | 3.6 ±1 %  |          |
| 1750          | 75.2 ±1 %  |          | 42.9 ±1 %  |          | 3.6 ±1 %  |          |
| 1800          | 72.0 ±1 %  | PASS     | 41.7 ±1 %  | PASS     | 3.6 ±1 %  | PASS     |
| 1900          | 68.0 ±1 %  |          | 39.5 ±1 %  |          | 3.6 ±1 %  |          |
| 1950          | 66.3 ±1 %  |          | 38.5 ±1 %  |          | 3.6 ±1 %  |          |
| 2000          | 64.5 ±1 %  |          | 37.5 ±1 %  |          | 3.6 ±1 %  |          |
| 2100          | 61.0 ±1 %  |          | 35.7 ±1 %  |          | 3.6 ±1 %  |          |
| 2300          | 55.5 ±1 %  |          | 32.6 ±1 %  |          | 3.6 ±1 %  |          |
| 2450          | 51.5 ±1 %  |          | 30.4 ±1 %  |          | 3.6 ±1 %  |          |
| 2600          | 48.5 ±1 %  |          | 28.8 ±1 %  |          | 3.6 ±1 %  |          |
| 3000          | 41.5 ±1 %  |          | 25.0 ±1 %  |          | 3.6 ±1 %  |          |
| 3500          | 37.0 ±1 %  |          | 26.4 ±1 %  |          | 3.6 ±1 %  |          |
| 3700          | 34.7 ±1 %  |          | 26.4 ±1 %  |          | 3.6 ±1 %  |          |

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.





7 VALIDATION MEASUREMENT

The IEEE Std. 1528, OET 65 Bulletin C and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

7.1 HEAD LIQUID MEASUREMENT

| Frequency MHz | Relative permittivity ( $\epsilon_r$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|---------------|--|----------|-------------------------------|----------|
|               | required                               | measured | required                      | measured |
| 300           | 45.3 ±5 %                              |          | 0.87 ±5 %                     |          |
| 450           | 43.5 ±5 %                              |          | 0.87 ±5 %                     |          |
| 750           | 41.9 ±5 %                              |          | 0.89 ±5 %                     |          |
| 835           | 41.5 ±5 %                              |          | 0.90 ±5 %                     |          |
| 900           | 41.5 ±5 %                              |          | 0.97 ±5 %                     |          |
| 1450          | 40.5 ±5 %                              |          | 1.20 ±5 %                     |          |
| 1500          | 40.4 ±5 %                              |          | 1.23 ±5 %                     |          |
| 1640          | 40.2 ±5 %                              |          | 1.31 ±5 %                     |          |
| 1750          | 40.1 ±5 %                              |          | 1.37 ±5 %                     |          |
| 1800          | 40.0 ±5 %                              | PASS     | 1.40 ±5 %                     | PASS     |
| 1900          | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 1950          | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 2000          | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 2100          | 39.8 ±5 %                              |          | 1.49 ±5 %                     |          |
| 2300          | 39.5 ±5 %                              |          | 1.67 ±5 %                     |          |
| 2450          | 39.2 ±5 %                              |          | 1.80 ±5 %                     |          |
| 2600          | 39.0 ±5 %                              |          | 1.96 ±5 %                     |          |
| 3000          | 38.5 ±5 %                              |          | 2.40 ±5 %                     |          |
| 3500          | 37.9 ±5 %                              |          | 2.91 ±5 %                     |          |

7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.

|   |  |
|---|--|
| Software                                  | OPENSAR V4   |
| Phantom                                   | SN 20/09 SAM71   |
| Probe                                     | SN 18/11 EPG122  |
| Liquid                                    | Head Liquid Values: $\epsilon_{ps}$ : 41.3 $\sigma$ : 1.38 |
| Distance between dipole center and liquid | 10.0 mm  |
| Area scan resolution                      | $dx=8mm/dy=8mm$  |

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*






SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.6.14.SATU.A

|                      |                     |
|----------------------|---------------------|
| Zoon Scan Resolution | dx=8mm/dy=8m/dz=5mm |
| Frequency            | 1800 MHz            |
| Input power          | 20 dBm              |
| Liquid Temperature   | 21 °C               |
| Lab Temperature      | 21 °C               |
| Lab Humidity         | 45 %                |

| Frequency MHz | 1 g SAR (W/kg/W) |              | 10 g SAR (W/kg/W) |              |
|---------------|------------------|--------------|-------------------|--------------|
|               | required         | measured     | required          | measured     |
| 300           | 2.85             |              | 1.94              |              |
| 450           | 4.58             |              | 3.06              |              |
| 750           | 8.49             |              | 5.55              |              |
| 835           | 9.56             |              | 6.22              |              |
| 900           | 10.9             |              | 6.99              |              |
| 1450          | 29               |              | 16                |              |
| 1500          | 30.5             |              | 16.8              |              |
| 1640          | 34.2             |              | 18.4              |              |
| 1750          | 36.4             |              | 19.3              |              |
| 1800          | 38.4             | 38.13 (3.81) | 20.1              | 20.20 (2.02) |
| 1900          | 39.7             |              | 20.5              |              |
| 1950          | 40.5             |              | 20.9              |              |
| 2000          | 41.1             |              | 21.1              |              |
| 2100          | 43.6             |              | 21.9              |              |
| 2300          | 48.7             |              | 23.3              |              |
| 2450          | 52.4             |              | 24                |              |
| 2600          | 55.3             |              | 24.6              |              |
| 3000          | 63.8             |              | 25.7              |              |
| 3500          | 67.1             |              | 25                |              |

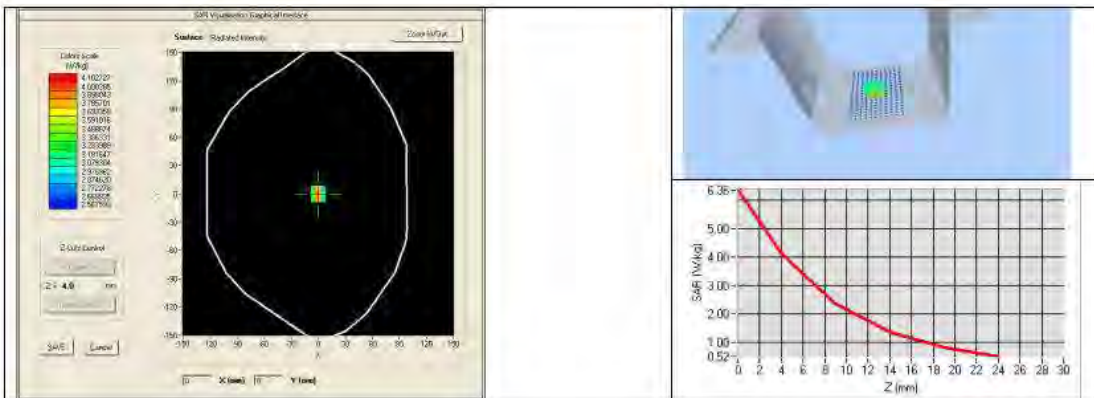

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.





SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR\_287.6.14.SATIMA

7.3 BODY LIQUID MEASUREMENT

| Frequency MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|---------------|---|----------|-------------------------------|----------|
|               | required                                | measured | required                      | measured |
| 150           | 61.9 ±5 %                               |          | 0.80 ±5 %                     |          |
| 300           | 58.2 ±5 %                               |          | 0.92 ±5 %                     |          |
| 450           | 56.7 ±5 %                               |          | 0.94 ±5 %                     |          |
| 750           | 55.5 ±5 %                               |          | 0.96 ±5 %                     |          |
| 835           | 55.2 ±5 %                               |          | 0.97 ±5 %                     |          |
| 900           | 55.0 ±5 %                               |          | 1.05 ±5 %                     |          |
| 915           | 55.0 ±5 %                               |          | 1.06 ±5 %                     |          |
| 1450          | 54.0 ±5 %                               |          | 1.30 ±5 %                     |          |
| 1610          | 53.8 ±5 %                               |          | 1.40 ±5 %                     |          |
| 1800          | 53.3 ±5 %                               | PASS     | 1.52 ±5 %                     | PASS     |
| 1900          | 53.3 ±5 %                               |          | 1.52 ±5 %                     |          |
| 2000          | 53.3 ±5 %                               |          | 1.52 ±5 %                     |          |
| 2100          | 53.2 ±5 %                               |          | 1.62 ±5 %                     |          |
| 2450          | 52.7 ±5 %                               |          | 1.95 ±5 %                     |          |
| 2600          | 52.5 ±5 %                               |          | 2.16 ±5 %                     |          |
| 3000          | 52.0 ±5 %                               |          | 2.73 ±5 %                     |          |
| 3500          | 51.3 ±5 %                               |          | 3.31 ±5 %                     |          |
| 5200          | 49.0 ±10 %                              |          | 5.30 ±10 %                    |          |
| 5300          | 48.9 ±10 %                              |          | 5.42 ±10 %                    |          |
| 5400          | 48.7 ±10 %                              |          | 5.53 ±10 %                    |          |
| 5500          | 48.6 ±10 %                              |          | 5.65 ±10 %                    |          |
| 5600          | 48.5 ±10 %                              |          | 5.77 ±10 %                    |          |
| 5800          | 48.2 ±10 %                              |          | 6.00 ±10 %                    |          |

7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|   |   |
|---|---|
| Software                                  | OPENSAR V4  |
| Phantom                                   | SN 20/09 SAM71  |
| Probe                                     | SN 18/11 EPG122   |
| Liquid                                    | Body Liquid Values: $\epsilon_{ps}'$ : 53.3 $\sigma$ : 1.51 |
| Distance between dipole center and liquid | 10.0 mm   |
| Area scan resolution                      | $dx=8mm/dy=8mm$   |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                      |
| Frequency                                 | 1800 MHz  |
| Input power                               | 20 dBm  |
| Liquid Temperature                        | 21 °C   |
| Lab Temperature                           | 21 °C   |
| Lab Humidity                              | 45 %  |

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.






SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.6.14.SATU.A

| Frequency MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|---------------|------------------|-------------------|
|               | measured         | measured          |
| 1800          | 39.03 (3.90)     | 20.65 (2.07)      |

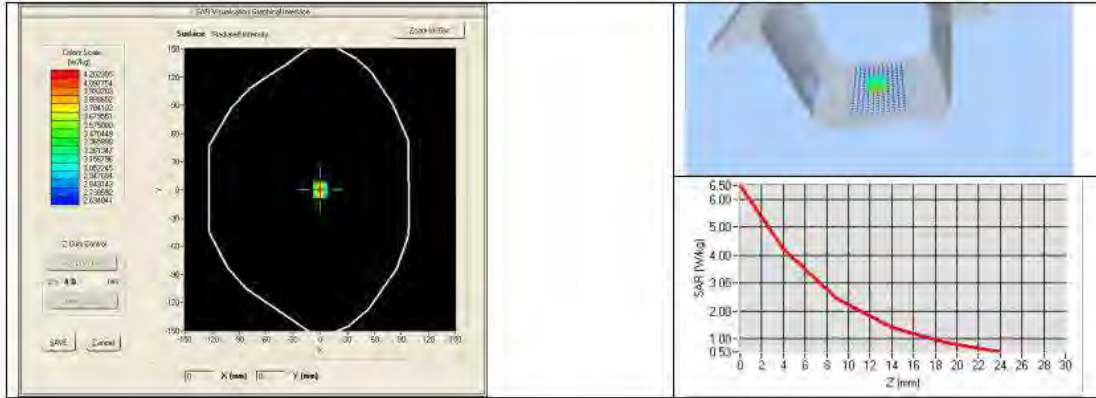

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*







8 LIST OF EQUIPMENT

| Equipment Summary Sheet         |                      |                    |   |   |
|---------------------------------|----------------------|--------------------|---|---|
| Equipment Description           | Manufacturer / Model | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                     | Satimo               | SN-20/09-SAM71     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench              | Version 3            | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                | Rhode & Schwarz ZVA  | SN100132           | 02/2021                                       | 02/2024                                       |
| Calipers                        | Carrera              | CALIPER-01         | 12/2021                                       | 12/2024                                       |
| Reference Probe                 | Satimo               | EPG122 SN 18/11    | 10/2023                                       | 10/2024                                       |
| Multimeter                      | Keithley 2000        | 1188656            | 12/2021                                       | 12/2024                                       |
| Signal Generator                | Agilent E4438C       | MY49070581         | 12/2021                                       | 12/2024                                       |
| Amplifier                       | Aethercomm           | SN 046             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                     | HP E4418A            | US38261498         | 12/2021                                       | 12/2024                                       |
| Power Sensor                    | HP ECP-E26A          | US37181460         | 12/2021                                       | 12/2024                                       |
| Directional Coupler             | Narda 4216-20        | 01386              | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature and Humidity Sensor | Control Company      | 11-661-9           | 8/2021  | 8/2024  |





### 5.4 SID1900 Dipole Calibration Certificate



## SAR Reference Dipole Calibration Report

Ref: ACR.273.2.18.SATU.A

**SHENZHEN LCS COMPLIANCE TESTING  
LABORATORY LTD.**  
**1F., XINGYUAN INDUSTRIAL PARK, TONGDA ROAD,  
BAO'AN BLVD**  
**BAO'AN DISTRICT, SHENZHEN, GUANGDONG, CHINA**  
**MVG COMOSAR REFERENCE DIPOLE**  
**FREQUENCY: 1900 MHZ**  
**SERIAL NO.: SN 38/18 DIP 1G900-466**

**Calibrated at MVG US**  
**2105 Barrett Park Dr. - Kennesaw, GA 30144**




**ACCREDITED**  
Calibration Cert #234802

**Calibration Date: 09/22/2021**

*Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



股份  
ing Lab

股份  
ing Lab

股份  
ing Lab





SAR REFERENCE DIPOLE CALIBRATION REPORT

RUE ACR.273.2.18.SATC.A

股份  
ig Lab

|                      | <i>Name</i>   | <i>Function</i> | <i>Date</i> | <i>Signature</i>   |
|----------------------|---------------|-----------------|-------------|--------------------|
| <i>Prepared by :</i> | Jérôme LUC    | Product Manager | 09/28/2021  | <i>[Signature]</i> |
| <i>Checked by :</i>  | Jérôme LUC    | Product Manager | 09/28/2021  | <i>[Signature]</i> |
| <i>Approved by :</i> | Kim RUTKOWSKI | Quality Manager | 09/28/2021  | <i>[Signature]</i> |

|                       | <i>Customer Name</i>                            |
|-----------------------|---|
| <i>Distribution :</i> | Shenzhen LCS Compliance Testing Laboratory Ltd. |

股份  
ig Lab

| <i>Issue</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|----------------------|
| A            | 09/28/2021  | Initial release      |
|              |             |                      |
|              |             |                      |

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.  
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*

股份  
ig Lab





SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.273.2.18.SATC.A

TABLE OF CONTENTS

1 Introduction..... 4

2 Device Under Test..... 4

3 Product Description ..... 4

    3.1 General Information ..... 4

4 Measurement Method ..... 5

    4.1 Return Loss Requirements ..... 5

    4.2 Mechanical Requirements ..... 5

5 Measurement Uncertainty..... 5

    5.1 Return Loss ..... 5

    5.2 Dimension Measurement ..... 5

    5.3 Validation Measurement ..... 5

6 Calibration Measurement Results ..... 6

    6.1 Return Loss and Impedance In Head Liquid ..... 6

    6.2 Return Loss and Impedance In Body Liquid ..... 6

    6.3 Mechanical Dimensions ..... 6

7 Validation measurement ..... 7

    7.1 Head Liquid Measurement ..... 7

    7.2 SAR Measurement Result With Head Liquid ..... 8

    7.3 Body Liquid Measurement ..... 9

    7.4 SAR Measurement Result With Body Liquid ..... 10

8 List of Equipment ..... 11

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.





股份  
ig Lab

**1 INTRODUCTION**

This document contains a summary of the requirements set forth by the IEEE 1528, FCC KDBs and CEI/IEC 62209 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

**2 DEVICE UNDER TEST**

| Device Under Test              |                                   |
|--------------------------------|-----------------------------------|
| Device Type                    | COMOSAR 1900 MHz REFERENCE DIPOLE |
| Manufacturer                   | MVG                               |
| Model                          | SID1900                           |
| Serial Number                  | SN 38/18 DIP 1G900-466            |
| Product Condition (new / used) | Used                              |

A yearly calibration interval is recommended.

**3 PRODUCT DESCRIPTION**

**3.1 GENERAL INFORMATION**

MVG's COMOSAR Validation Dipoles are built in accordance to the IEEE 1528, FCC KDBs and CEI/IEC 62209 standards. The product is designed for use with the COMOSAR test bench only.



**Figure 1 – MVG COMOSAR Validation Dipole**

股份  
ig Lab

股份  
ig Lab





**4 MEASUREMENT METHOD**

The IEEE 1528, FCC KDBs and CEI/IEC 62209 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

**4.1 RETURN LOSS REQUIREMENTS**

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards.

**4.2 MECHANICAL REQUIREMENTS**

The IEEE Std. 1528 and CEI/IEC 62209 standards specify the mechanical components and dimensions of the validation dipoles, with the dimensions frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness.

**5 MEASUREMENT UNCERTAINTY**

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

**5.1 RETURN LOSS**

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.1 dB                              |

**5.2 DIMENSION MEASUREMENT**

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 3 - 300     | 0.05 mm                        |

**5.3 VALIDATION MEASUREMENT**

The guidelines outlined in the IEEE 1528, FCC KDBs, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 20.3 %               |






SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.273.2.18.SATL.A

|      |        |
|------|--------|
| 10 g | 20.1 % |
|------|--------|


6 CALIBRATION MEASUREMENT RESULTS

6.1 RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

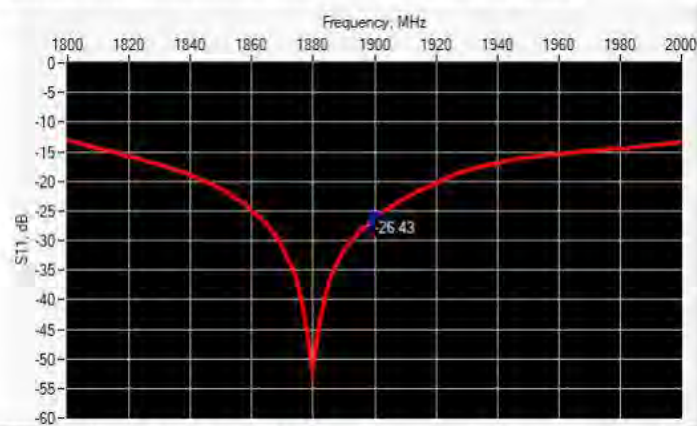

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance       |
|-----------------|------------------|------------------|-----------------|
| 1900            | -26.43           | -20              | 50.5 Ω + 4.7 jΩ |

6.2 RETURN LOSS AND IMPEDANCE IN BODY LIQUID

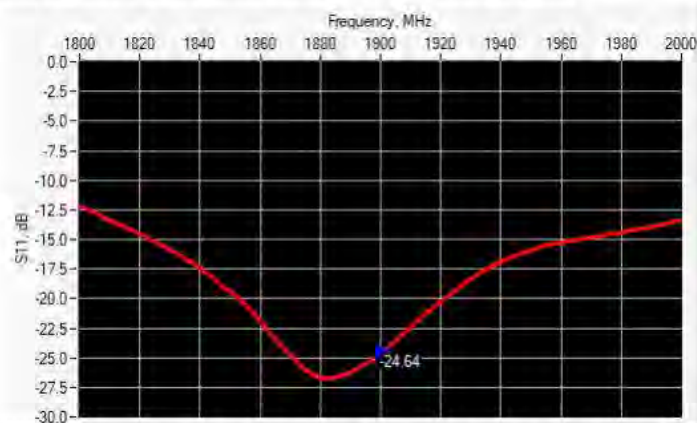

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance       |
|-----------------|------------------|------------------|-----------------|
| 1900            | -24.64           | -20              | 46.2 Ω + 4.4 jΩ |

6.3 MECHANICAL DIMENSIONS

| Frequency MHz | L mm       |          | h mm       |          | d mm      |          |
|---------------|------------|----------|------------|----------|-----------|----------|
|               | required   | measured | required   | measured | required  | measured |
| 300           | 420.0 ±1 % |          | 250.0 ±1 % |          | 6.35 ±1 % |          |

Page: 6/11

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.







SAR REFERENCE DIPOLE CALIBRATION REPORT

Rule ACR 273.2.18.SATL.A

股份  
ig Lab

|      |            |      |            |      |           |      |
|------|------------|------|------------|------|-----------|------|
| 450  | 290.0 ±1 % |      | 166.7 ±1 % |      | 6.35 ±1 % |      |
| 750  | 176.0 ±1 % |      | 100.0 ±1 % |      | 6.35 ±1 % |      |
| 835  | 161.0 ±1 % |      | 89.8 ±1 %  |      | 3.6 ±1 %  |      |
| 900  | 149.0 ±1 % |      | 83.3 ±1 %  |      | 3.6 ±1 %  |      |
| 1450 | 89.1 ±1 %  |      | 51.7 ±1 %  |      | 3.6 ±1 %  |      |
| 1500 | 80.5 ±1 %  |      | 50.0 ±1 %  |      | 3.6 ±1 %  |      |
| 1640 | 79.0 ±1 %  |      | 45.7 ±1 %  |      | 3.6 ±1 %  |      |
| 1750 | 75.2 ±1 %  |      | 42.9 ±1 %  |      | 3.6 ±1 %  |      |
| 1800 | 72.0 ±1 %  |      | 41.7 ±1 %  |      | 3.6 ±1 %  |      |
| 1900 | 68.0 ±1 %  | PASS | 39.5 ±1 %  | PASS | 3.6 ±1 %  | PASS |
| 1950 | 66.3 ±1 %  |      | 38.5 ±1 %  |      | 3.6 ±1 %  |      |
| 2000 | 64.5 ±1 %  |      | 37.5 ±1 %  |      | 3.6 ±1 %  |      |
| 2100 | 61.0 ±1 %  |      | 35.7 ±1 %  |      | 3.6 ±1 %  |      |
| 2300 | 55.5 ±1 %  |      | 32.6 ±1 %  |      | 3.6 ±1 %  |      |
| 2450 | 51.5 ±1 %  |      | 30.4 ±1 %  |      | 3.6 ±1 %  |      |
| 2600 | 48.5 ±1 %  |      | 28.8 ±1 %  |      | 3.6 ±1 %  |      |
| 3000 | 41.5 ±1 %  |      | 25.0 ±1 %  |      | 3.6 ±1 %  |      |
| 3500 | 37.0 ±1 %  |      | 26.4 ±1 %  |      | 3.6 ±1 %  |      |
| 3700 | 34.7 ±1 %  |      | 26.4 ±1 %  |      | 3.6 ±1 %  |      |

7 VALIDATION MEASUREMENT

The IEEE Std. 1528, FCC KDBs and CEM/IEC 62209 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

7.1 HEAD LIQUID MEASUREMENT

| Frequency MHz | Relative permittivity ( $\epsilon_r$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|---------------|--|----------|-------------------------------|----------|
|               | required                               | measured | required                      | measured |
| 300           | 45.3 ±5 %                              |          | 0.87 ±5 %                     |          |
| 450           | 43.5 ±5 %                              |          | 0.87 ±5 %                     |          |
| 750           | 41.9 ±5 %                              |          | 0.89 ±5 %                     |          |
| 835           | 41.5 ±5 %                              |          | 0.90 ±5 %                     |          |
| 900           | 41.5 ±5 %                              |          | 0.97 ±5 %                     |          |
| 1450          | 40.5 ±5 %                              |          | 1.20 ±5 %                     |          |
| 1500          | 40.4 ±5 %                              |          | 1.23 ±5 %                     |          |
| 1640          | 40.2 ±5 %                              |          | 1.31 ±5 %                     |          |
| 1750          | 40.1 ±5 %                              |          | 1.37 ±5 %                     |          |

Page: 7/11

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.  
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*

股份  
ig Lab





SAR REFERENCE DIPOLE CALIBRATION REPORT

RUE ACR.273.2.18.SATL.A

|      |           |      |           |      |
|------|-----------|------|-----------|------|
| 1800 | 40.0 ±5 % |      | 1.40 ±5 % |      |
| 1900 | 40.0 ±5 % | PASS | 1.40 ±5 % | PASS |
| 1950 | 40.0 ±5 % |      | 1.40 ±5 % |      |
| 2000 | 40.0 ±5 % |      | 1.40 ±5 % |      |
| 2100 | 39.8 ±5 % |      | 1.49 ±5 % |      |
| 2300 | 39.5 ±5 % |      | 1.67 ±5 % |      |
| 2450 | 39.2 ±5 % |      | 1.80 ±5 % |      |
| 2600 | 39.0 ±5 % |      | 1.96 ±5 % |      |
| 3000 | 38.5 ±5 % |      | 2.40 ±5 % |      |
| 3500 | 37.9 ±5 % |      | 2.91 ±5 % |      |

7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.

|   |   |
|---|---|
| Software                                  | OPENSAR V4  |
| Phantom                                   | SN 20/09 SAM71  |
| Probe                                     | SN 18/11 EPG122   |
| Liquid                                    | Head Liquid Values: $\epsilon_{ps} = 38.5$ $\sigma_{\text{rel}} = 1.45$ |
| Distance between dipole center and liquid | 10.0 mm   |
| Area scan resolution                      | $dx=8\text{mm}/dy=8\text{mm}$   |
| Zoon Scan Resolution                      | $dx=8\text{mm}/dy=8\text{mm}/dz=5\text{mm}$                             |
| Frequency                                 | 1900 MHz  |
| Input power                               | 20 dBm  |
| Liquid Temperature                        | 21 °C   |
| Lab Temperature                           | 21 °C   |
| Lab Humidity                              | 45 %  |

| Frequency MHz | 1 g SAR (W/kg/W) |          | 10 g SAR (W/kg/W) |          |
|---------------|------------------|----------|-------------------|----------|
|               | required         | measured | required          | measured |
| 300           | 2.85             |          | 1.94              |          |
| 450           | 4.58             |          | 3.06              |          |
| 750           | 8.49             |          | 5.55              |          |
| 835           | 9.56             |          | 6.22              |          |
| 900           | 10.9             |          | 6.99              |          |
| 1450          | 29               |          | 16                |          |
| 1500          | 30.5             |          | 16.8              |          |
| 1640          | 34.2             |          | 18.4              |          |
| 1750          | 36.4             |          | 19.3              |          |
| 1800          | 38.4             |          | 20.1              |          |

Page: 8/11

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.






SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.273.2.18.SATC.A

股份  
ig Lab

|      |      |              |      |              |
|------|------|--------------|------|--------------|
| 1900 | 39.7 | 40.03 (4.00) | 20.5 | 20.55 (2.06) |
| 1950 | 40.5 |              | 20.9 |              |
| 2000 | 41.1 |              | 21.1 |              |
| 2100 | 43.6 |              | 21.9 |              |
| 2300 | 48.7 |              | 23.3 |              |
| 2450 | 52.4 |              | 24   |              |
| 2600 | 55.3 |              | 24.6 |              |
| 3000 | 63.8 |              | 25.7 |              |
| 3500 | 67.1 |              | 25   |              |
| 3700 | 67.4 |              | 24.2 |              |

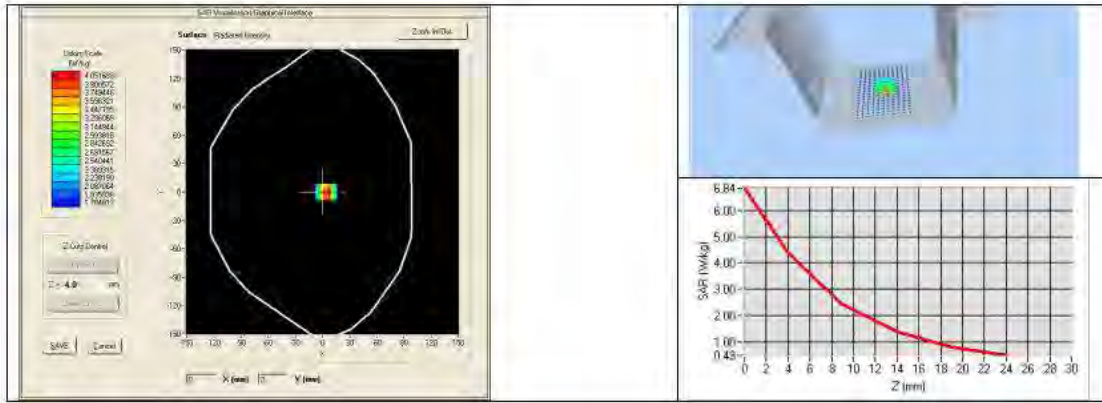

股份  
ig Lab

7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|---|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 150              | 61.9 ±5 %                               |          | 0.80 ±5 %                     |          |
| 300              | 58.2 ±5 %                               |          | 0.92 ±5 %                     |          |
| 450              | 56.7 ±5 %                               |          | 0.94 ±5 %                     |          |
| 750              | 55.5 ±5 %                               |          | 0.96 ±5 %                     |          |
| 835              | 55.2 ±5 %                               |          | 0.97 ±5 %                     |          |
| 900              | 55.0 ±5 %                               |          | 1.05 ±5 %                     |          |
| 915              | 55.0 ±5 %                               |          | 1.06 ±5 %                     |          |
| 1450             | 54.0 ±5 %                               |          | 1.30 ±5 %                     |          |
| 1610             | 53.8 ±5 %                               |          | 1.40 ±5 %                     |          |
| 1800             | 53.3 ±5 %                               |          | 1.52 ±5 %                     |          |
| 1900             | 53.3 ±5 %                               | PASS     | 1.52 ±5 %                     | PASS     |
| 2000             | 53.3 ±5 %                               |          | 1.52 ±5 %                     |          |
| 2100             | 53.2 ±5 %                               |          | 1.62 ±5 %                     |          |

Page: 9/11

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.

股份  
ig Lab





SAR REFERENCE DIPOLE CALIBRATION REPORT


Ref: ACR.273.2.18.SATL.A

|      |            |  |            |
|------|------------|--|------------|
| 2300 | 52.9 ±5 %  |  | 1.81 ±5 %  |
| 2450 | 52.7 ±5 %  |  | 1.95 ±5 %  |
| 2600 | 52.5 ±5 %  |  | 2.16 ±5 %  |
| 3000 | 52.0 ±5 %  |  | 2.73 ±5 %  |
| 3500 | 51.3 ±5 %  |  | 3.31 ±5 %  |
| 3700 | 51.0 ±5 %  |  | 3.55 ±5 %  |
| 5200 | 49.0 ±10 % |  | 5.30 ±10 % |
| 5300 | 48.9 ±10 % |  | 5.42 ±10 % |
| 5400 | 48.7 ±10 % |  | 5.53 ±10 % |
| 5500 | 48.6 ±10 % |  | 5.65 ±10 % |
| 5600 | 48.5 ±10 % |  | 5.77 ±10 % |
| 5800 | 48.2 ±10 % |  | 6.00 ±10 % |

7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|   |  |
|---|--|
| Software                                  | OPENSAR V4   |
| Phantom                                   | SN 20/09 SAM71   |
| Probe                                     | SN 18/11 EPG122  |
| Liquid                                    | Body Liquid Values: $\epsilon_{ps}$ : 53.3 $\sigma$ : 1.56 |
| Distance between dipole center and liquid | 10.0 mm  |
| Area scan resolution                      | $dx=8mm/dy=8mm$  |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                     |
| Frequency                                 | 1900 MHz   |
| Input power                               | 20 dBm   |
| Liquid Temperature                        | 21 °C  |
| Lab Temperature                           | 21 °C  |
| Lab Humidity                              | 45 %   |

| Frequency MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|---------------|------------------|-------------------|
|               | measured         | measured          |
| 1900          | 40.91 (4.09)     | 21.40 (2.14)      |

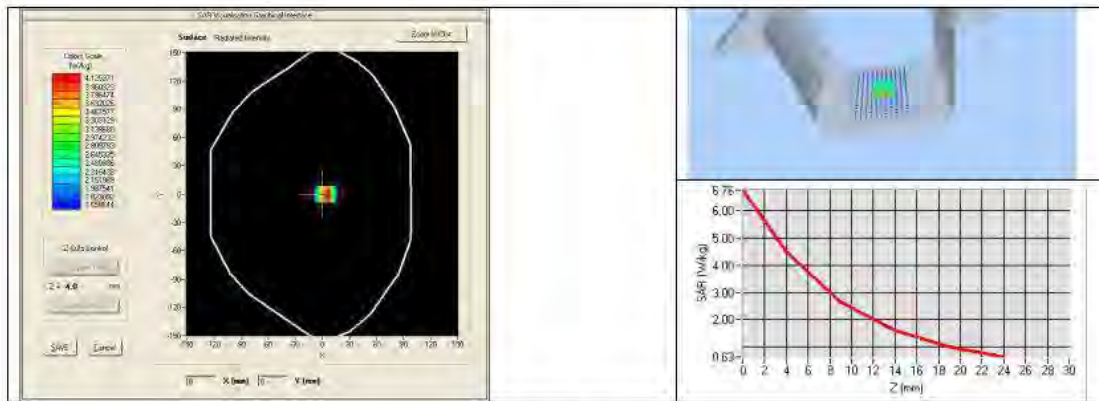

Page: 10/11

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.





SAR REFERENCE DIPOLE CALIBRATION REPORT

RUE ACR.273.2.18.SATL.A

8 LIST OF EQUIPMENT

| Equipment Summary Sheet         |                      |                    |   |   |
|---------------------------------|----------------------|--------------------|---|---|
| Equipment Description           | Manufacturer / Model | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                     | MVG                  | SN-20/09-SAM71     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench              | Version 3            | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                | Rhode & Schwarz ZVA  | SN100132           | 06/2021                                       | 06/2024                                       |
| Calipers                        | Carrera              | CALIPER-01         | 01/2023                                       | 01/2026                                       |
| Reference Probe                 | MVG                  | EPG122 SN 18/11    | 08/2023                                       | 08/2024                                       |
| Multimeter                      | Keithley 2000        | 1188656            | 01/2023                                       | 01/2026                                       |
| Signal Generator                | Agilent E4438C       | MY49070581         | 01/2023                                       | 01/2026                                       |
| Amplifier                       | Aethercomm           | SN 046             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                     | HP E4418A            | US38261498         | 11/2023                                       | 11/2026                                       |
| Power Sensor                    | HP ECP-E26A          | US37181460         | 01/2023                                       | 01/2026                                       |
| Directional Coupler             | Narda 4216-20        | 01386              | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature and Humidity Sensor | Control Company      | 150798832          | 11/2023                                       | 11/2026                                       |

*This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*





### 5.5 SID2450 Dipole Calibration Certificate



## SAR Reference Dipole Calibration Report

Ref : ACR.287.8.14.SATU.A

**SHENZHEN LCS COMPLIANCE TESTING  
LABORATORY LTD.**  
**1F., XINGYUAN INDUSTRIAL PARK, TONGDA ROAD,  
BAO'AN BLVD**  
**BAO'AN DISTRICT, SHENZHEN, GUANGDONG, CHINA**  
**SATIMO COMOSAR REFERENCE DIPOLE**  
**FREQUENCY: 2450 MHZ**  
**SERIAL NO.: SN 07/14 DIP 2G450-306**

**Calibrated at SATIMO US**  
**2105 Barrett Park Dr. - Kennesaw, GA 30144**




**09/29/2021**

*Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in SATIMO USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



股份  
ing Lab

股份  
ing Lab

股份  
ing Lab



SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.8.14.SATL.A

股份  
ig Lab

|               | Name          | Function        | Date       | Signature            |
|---------------|---------------|-----------------|------------|----------------------|
| Prepared by : | Jérôme LUC    | Product Manager | 10/12/2021 | <i>JL</i>            |
| Checked by :  | Jérôme LUC    | Product Manager | 10/12/2021 | <i>JL</i>            |
| Approved by : | Kim RUTKOWSKI | Quality Manager | 10/12/2021 | <i>Kim Rutkowski</i> |

|                | Customer Name                                   |
|----------------|---|
| Distribution : | Shenzhen LCS Compliance Testing Laboratory Ltd. |

| Issue | Date       | Mod. fications  |
|-------|------------|-----------------|
| A     | 10/12/2021 | Initial release |
|       |            |                 |
|       |            |                 |

股份  
ig Lab

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*

股份  
ig Lab









SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.B.14.SATL.A

TABLE OF CONTENTS

- 1 Introduction..... 4
- 2 Device Under Test ..... 4
- 3 Product Description ..... 4
  - 3.1 General Information ..... 4
- 4 Measurement Method ..... 5
  - 4.1 Return Loss Requirements ..... 5
  - 4.2 Mechanical Requirements ..... 5
- 5 Measurement Uncertainty..... 5
  - 5.1 Return Loss ..... 5
  - 5.2 Dimension Measurement ..... 5
  - 5.3 Validation Measurement ..... 5
- 6 Calibration Measurement Results ..... 6
  - 6.1 Return Loss and Impedance ..... 6
  - 6.2 Mechanical Dimensions ..... 6
- 7 Validation measurement ..... 7
  - 7.1 Head Liquid Measurement ..... 7
  - 7.2 SAR Measurement Result With Head Liquid ..... 7
  - 7.3 Body Liquid Measurement ..... 9
  - 7.4 SAR Measurement Result With Body Liquid ..... 9
- 8 List of Equipment ..... 11

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.





**1 INTRODUCTION**

This document contains a summary of the requirements set forth by the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

**2 DEVICE UNDER TEST**

| Device Under Test              |                                   |
|--------------------------------|-----------------------------------|
| Device Type                    | COMOSAR 2450 MHz REFERENCE DIPOLE |
| Manufacturer                   | Satimo                            |
| Model                          | SID2450                           |
| Serial Number                  | SN 07/14 DIP 2G450-306            |
| Product Condition (new / used) | New                               |

A yearly calibration interval is recommended.

**3 PRODUCT DESCRIPTION**

**3.1 GENERAL INFORMATION**

Satimo's COMOSAR Validation Dipoles are built in accordance to the IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards. The product is designed for use with the COMOSAR test bench only.



**Figure 1 – Satimo COMOSAR Validation Dipole**





**4 MEASUREMENT METHOD**

The IEEE 1528, OET 65 Bulletin C and CEI/IEC 62209 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

**4.1 RETURN LOSS REQUIREMENTS**

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards.

**4.2 MECHANICAL REQUIREMENTS**

The IEEE Std. 1528 and CEI/IEC 62209 standards specify the mechanical components and dimensions of the validation dipoles, with the dimensions frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness.

**5 MEASUREMENT UNCERTAINTY**

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

**5.1 RETURN LOSS**

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.1 dB                              |

**5.2 DIMENSION MEASUREMENT**

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 3 - 300     | 0.05 mm                        |

**5.3 VALIDATION MEASUREMENT**

The guidelines outlined in the IEEE 1528, OET 65 Bulletin C, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 20.3 %               |
| 10 g        | 20.1 %               |

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*






SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.8.14.SATL.A

6 CALIBRATION MEASUREMENT RESULTS

6.1 RETURN LOSS AND IMPEDANCE

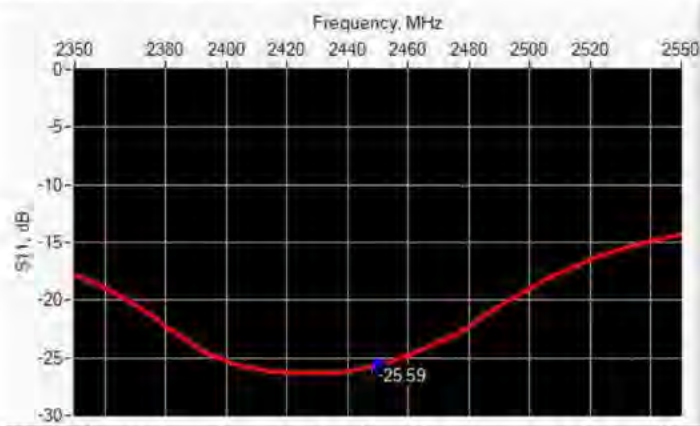

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance       |
|-----------------|------------------|------------------|-----------------|
| 2450            | -25.59           | -20              | 44.7 Ω - 1.1 jΩ |

6.2 MECHANICAL DIMENSIONS

| Frequency MHz | L mm       |          | h mm       |          | d mm      |          |
|---------------|------------|----------|------------|----------|-----------|----------|
|               | required   | measured | required   | measured | required  | measured |
| 300           | 420.0 ±1 % |          | 250.0 ±1 % |          | 6.35 ±1 % |          |
| 450           | 290.0 ±1 % |          | 166.7 ±1 % |          | 6.35 ±1 % |          |
| 750           | 176.0 ±1 % |          | 100.0 ±1 % |          | 6.35 ±1 % |          |
| 835           | 161.0 ±1 % |          | 89.8 ±1 %  |          | 3.6 ±1 %  |          |
| 900           | 149.0 ±1 % |          | 83.3 ±1 %  |          | 3.6 ±1 %  |          |
| 1450          | 89.1 ±1 %  |          | 51.7 ±1 %  |          | 3.6 ±1 %  |          |
| 1500          | 80.5 ±1 %  |          | 50.0 ±1 %  |          | 3.6 ±1 %  |          |
| 1640          | 79.0 ±1 %  |          | 45.7 ±1 %  |          | 3.6 ±1 %  |          |
| 1750          | 75.2 ±1 %  |          | 42.9 ±1 %  |          | 3.6 ±1 %  |          |
| 1800          | 72.0 ±1 %  |          | 41.7 ±1 %  |          | 3.6 ±1 %  |          |
| 1900          | 68.0 ±1 %  |          | 39.5 ±1 %  |          | 3.6 ±1 %  |          |
| 1950          | 66.3 ±1 %  |          | 38.5 ±1 %  |          | 3.6 ±1 %  |          |
| 2000          | 64.5 ±1 %  |          | 37.5 ±1 %  |          | 3.6 ±1 %  |          |
| 2100          | 61.0 ±1 %  |          | 35.7 ±1 %  |          | 3.6 ±1 %  |          |
| 2300          | 55.5 ±1 %  |          | 32.6 ±1 %  |          | 3.6 ±1 %  |          |
| 2450          | 51.5 ±1 %  | PASS     | 30.4 ±1 %  | PASS     | 3.6 ±1 %  | PASS     |
| 2600          | 48.5 ±1 %  |          | 28.8 ±1 %  |          | 3.6 ±1 %  |          |
| 3000          | 41.5 ±1 %  |          | 25.0 ±1 %  |          | 3.6 ±1 %  |          |
| 3500          | 37.0 ±1 %  |          | 26.4 ±1 %  |          | 3.6 ±1 %  |          |
| 3700          | 34.7 ±1 %  |          | 26.4 ±1 %  |          | 3.6 ±1 %  |          |

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.





SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.E.14.SATIM.A

7 VALIDATION MEASUREMENT

The IEEE Std. 1528, OET 65 Bulletin C and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

7.1 HEAD LIQUID MEASUREMENT

| Frequency MHz | Relative permittivity ( $\epsilon_r$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|---------------|--|----------|-------------------------------|----------|
|               | required                               | measured | required                      | measured |
| 300           | 45.3 ±5 %                              |          | 0.87 ±5 %                     |          |
| 450           | 43.5 ±5 %                              |          | 0.87 ±5 %                     |          |
| 750           | 41.9 ±5 %                              |          | 0.89 ±5 %                     |          |
| 835           | 41.5 ±5 %                              |          | 0.90 ±5 %                     |          |
| 900           | 41.5 ±5 %                              |          | 0.97 ±5 %                     |          |
| 1450          | 40.5 ±5 %                              |          | 1.20 ±5 %                     |          |
| 1500          | 40.4 ±5 %                              |          | 1.23 ±5 %                     |          |
| 1640          | 40.2 ±5 %                              |          | 1.31 ±5 %                     |          |
| 1750          | 40.1 ±5 %                              |          | 1.37 ±5 %                     |          |
| 1800          | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 1900          | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 1950          | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 2000          | 40.0 ±5 %                              |          | 1.40 ±5 %                     |          |
| 2100          | 39.8 ±5 %                              |          | 1.49 ±5 %                     |          |
| 2300          | 39.5 ±5 %                              |          | 1.67 ±5 %                     |          |
| 2450          | 39.2 ±5 %                              | PASS     | 1.80 ±5 %                     | PASS     |
| 2600          | 39.0 ±5 %                              |          | 1.96 ±5 %                     |          |
| 3000          | 38.5 ±5 %                              |          | 2.40 ±5 %                     |          |
| 3500          | 37.9 ±5 %                              |          | 2.91 ±5 %                     |          |

7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.

|   |   |
|---|---|
| Software                                  | OPENSAR V4  |
| Phantom                                   | SN 20/09 SAM71  |
| Probe                                     | SN 18/11 EPG122   |
| Liquid                                    | Head Liquid Values: $\epsilon_{ps}^*$ : 39.0 sigma : 1.77 |
| Distance between dipole center and liquid | 10.0 mm   |
| Area scan resolution                      | dx=8mm/dy=8mm   |

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*







SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.8.14.SATL.A

|                      |                      |
|----------------------|----------------------|
| Zoon Scan Resolution | dx=8mm/dy=8mm/dz=5mm |
| Frequency            | 2450 MHz             |
| Input power          | 20 dBm               |
| Liquid Temperature   | 21 °C                |
| Lab Temperature      | 21 °C                |
| Lab Humidity         | 45 %                 |

| Frequency MHz | 1 g SAR (W/kg/W) |              | 10 g SAR (W/kg/W) |              |
|---------------|------------------|--------------|-------------------|--------------|
|               | required         | measured     | required          | measured     |
| 300           | 2.85             |              | 1.94              |              |
| 450           | 4.58             |              | 3.06              |              |
| 750           | 8.49             |              | 5.55              |              |
| 835           | 9.56             |              | 6.22              |              |
| 900           | 10.9             |              | 6.99              |              |
| 1450          | 29               |              | 16                |              |
| 1500          | 30.5             |              | 16.8              |              |
| 1640          | 34.2             |              | 18.4              |              |
| 1750          | 36.4             |              | 19.3              |              |
| 1800          | 38.4             |              | 20.1              |              |
| 1900          | 39.7             |              | 20.5              |              |
| 1950          | 40.5             |              | 20.9              |              |
| 2000          | 41.1             |              | 21.1              |              |
| 2100          | 43.6             |              | 21.9              |              |
| 2300          | 48.7             |              | 23.3              |              |
| 2450          | 52.4             | 53.89 (5.39) | 24                | 24.15 (2.42) |
| 2600          | 55.3             |              | 24.6              |              |
| 3000          | 63.8             |              | 25.7              |              |
| 3500          | 67.1             |              | 25                |              |

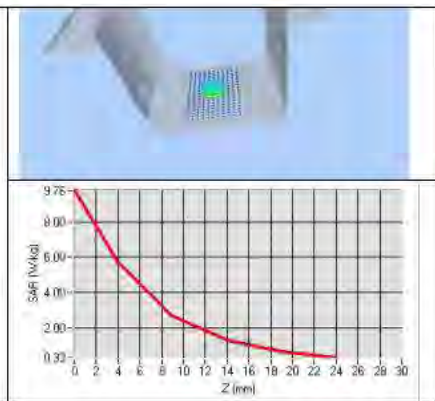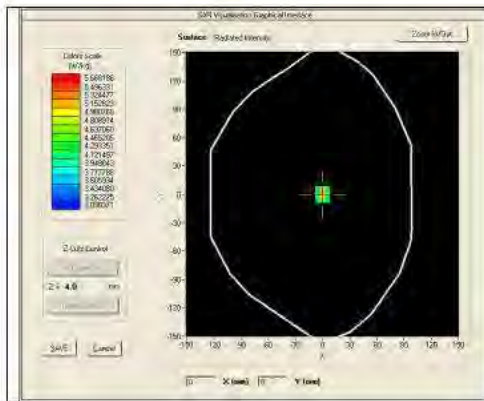

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.





SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.E.14.SATIM.A

7.3 BODY LIQUID MEASUREMENT

| Frequency MHz | Relative permittivity ( $\epsilon_r$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|---------------|--|----------|-------------------------------|----------|
|               | required                               | measured | required                      | measured |
| 150           | 61.9 ±5 %                              |          | 0.80 ±5 %                     |          |
| 300           | 58.2 ±5 %                              |          | 0.92 ±5 %                     |          |
| 450           | 56.7 ±5 %                              |          | 0.94 ±5 %                     |          |
| 750           | 55.5 ±5 %                              |          | 0.96 ±5 %                     |          |
| 835           | 55.2 ±5 %                              |          | 0.97 ±5 %                     |          |
| 900           | 55.0 ±5 %                              |          | 1.05 ±5 %                     |          |
| 915           | 55.0 ±5 %                              |          | 1.06 ±5 %                     |          |
| 1450          | 54.0 ±5 %                              |          | 1.30 ±5 %                     |          |
| 1610          | 53.8 ±5 %                              |          | 1.40 ±5 %                     |          |
| 1800          | 53.3 ±5 %                              |          | 1.52 ±5 %                     |          |
| 1900          | 53.3 ±5 %                              |          | 1.52 ±5 %                     |          |
| 2000          | 53.3 ±5 %                              |          | 1.52 ±5 %                     |          |
| 2100          | 53.2 ±5 %                              |          | 1.62 ±5 %                     |          |
| 2450          | 52.7 ±5 %                              | PASS     | 1.95 ±5 %                     | PASS     |
| 2600          | 52.5 ±5 %                              |          | 2.16 ±5 %                     |          |
| 3000          | 52.0 ±5 %                              |          | 2.73 ±5 %                     |          |
| 3500          | 51.3 ±5 %                              |          | 3.31 ±5 %                     |          |
| 5200          | 49.0 ±10 %                             |          | 5.30 ±10 %                    |          |
| 5300          | 48.9 ±10 %                             |          | 5.42 ±10 %                    |          |
| 5400          | 48.7 ±10 %                             |          | 5.53 ±10 %                    |          |
| 5500          | 48.6 ±10 %                             |          | 5.65 ±10 %                    |          |
| 5600          | 48.5 ±10 %                             |          | 5.77 ±10 %                    |          |
| 5800          | 48.2 ±10 %                             |          | 6.00 ±10 %                    |          |

7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|   |   |
|---|---|
| Software                                  | OPENSAR V4  |
| Phantom                                   | SN 20/09 SAM71  |
| Probe                                     | SN 18/11 EPG122   |
| Liquid                                    | Body Liquid Values: $\epsilon_r$ : 53.0 $\sigma$ : 1.93 |
| Distance between dipole center and liquid | 10.0 mm   |
| Area scan resolution                      | $dx=8mm/dy=8mm$   |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                  |
| Frequency                                 | 2450 MHz  |
| Input power                               | 20 dBm  |
| Liquid Temperature                        | 21 °C   |
| Lab Temperature                           | 21 °C   |
| Lab Humidity                              | 45 %  |

This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.






SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.287.8.14.SATL.A

| Frequency MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|---------------|------------------|-------------------|
|               | measured         | measured          |
| 2450          | 54.65 (5.46)     | 24.58 (2.46)      |

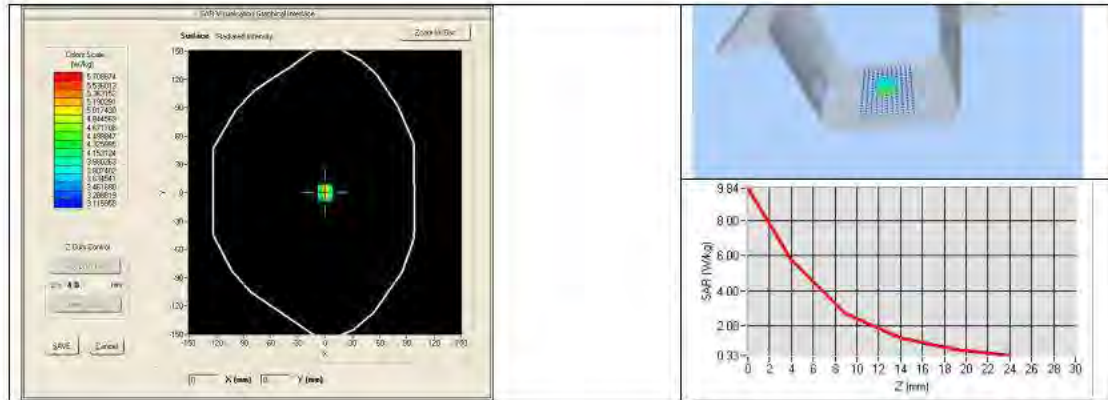

*This document shall not be reproduced, except in full or in part, without the written approval of SATIMO. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of SATIMO.*







8 LIST OF EQUIPMENT

| Equipment Summary Sheet         |                      |                    |   |   |
|---------------------------------|----------------------|--------------------|---|---|
| Equipment Description           | Manufacturer / Model | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                     | Satimo               | SN-20/09-SAM71     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench              | Version 3            | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                | Rhode & Schwarz ZVA  | SN100132           | 02/2021                                       | 02/2024                                       |
| Calipers                        | Carrera              | CALIPER-01         | 12/2021                                       | 12/2023                                       |
| Reference Probe                 | Satimo               | EPG122 SN 18/11    | 10/2023                                       | 10/2024                                       |
| Multimeter                      | Keithley 2000        | 1188656            | 12/2021                                       | 12/2023                                       |
| Signal Generator                | Agilent E4438C       | MY49070581         | 12/2021                                       | 12/2023                                       |
| Amplifier                       | Aethercomm           | SN 046             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                     | HP E4418A            | US38261498         | 12/2021                                       | 12/2023                                       |
| Power Sensor                    | HP ECP-E26A          | US37181460         | 12/2021                                       | 12/2023                                       |
| Directional Coupler             | Narda 4216-20        | 01386              | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature and Humidity Sensor | Control Company      | 11-661-9           | 8/2021  | 8/2024  |





### 5.6 SID2600 Dipole Calibration Certificate



## SAR Reference Dipole Calibration Report

Ref: ACR.273.4.18.SATU.A

**SHENZHEN LCS COMPLIANCE TESTING  
LABORATORY LTD.**  
**1F., XINGYUAN INDUSTRIAL PARK, TONGDA ROAD,  
BAO'AN BLVD**  
**BAO'AN DISTRICT, SHENZHEN, GUANGDONG, CHINA**  
**MVG COMOSAR REFERENCE DIPOLE**  
**FREQUENCY: 2600 MHZ**  
**SERIAL NO.: SN 38/18 DIP 2G600-468**

**Calibrated at MVG US**  
**2105 Barrett Park Dr. - Kennesaw, GA 30144**



**Calibration Date: 09/22/2021**

*Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



股份  
ing Lab

股份  
ing Lab

股份  
ing Lab





SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.273.4.18.SATC.A

股份  
ig Lab

|                      | <i>Name</i>   | <i>Function</i> | <i>Date</i> | <i>Signature</i> |
|----------------------|---------------|-----------------|-------------|------------------|
| <i>Prepared by :</i> | Jérôme LUC    | Product Manager | 09/28/2021  |                  |
| <i>Checked by :</i>  | Jérôme LUC    | Product Manager | 09/28/2021  |                  |
| <i>Approved by :</i> | Kim RUTKOWSKI | Quality Manager | 09/28/2021  |                  |

|                       | <i>Customer Name</i>                            |
|-----------------------|---|
| <i>Distribution :</i> | Shenzhen LCS Compliance Testing Laboratory Ltd. |

股份  
ig Lab

| <i>Issue</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|----------------------|
| A            | 09/28/2021  | Initial release      |
|              |             |                      |
|              |             |                      |
|              |             |                      |

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.

股份  
ig Lab





SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.273.4.18.SATC.A

TABLE OF CONTENTS

1 Introduction..... 4

2 Device Under Test..... 4

3 Product Description ..... 4

    3.1 General Information ..... 4

4 Measurement Method ..... 5

    4.1 Return Loss Requirements ..... 5

    4.2 Mechanical Requirements ..... 5

5 Measurement Uncertainty..... 5

    5.1 Return Loss ..... 5

    5.2 Dimension Measurement ..... 5

    5.3 Validation Measurement ..... 5

6 Calibration Measurement Results ..... 6

    6.1 Return Loss and Impedance In Head Liquid ..... 6

    6.2 Return Loss and Impedance In Body Liquid ..... 6

    6.3 Mechanical Dimensions ..... 6

7 Validation measurement ..... 7

    7.1 Head Liquid Measurement ..... 7

    7.2 SAR Measurement Result With Head Liquid ..... 8

    7.3 Body Liquid Measurement ..... 9

    7.4 SAR Measurement Result With Body Liquid ..... 10

8 List of Equipment ..... 11

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.





**1 INTRODUCTION**

This document contains a summary of the requirements set forth by the IEEE 1528, FCC KDBs and CEI/IEC 62209 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

**2 DEVICE UNDER TEST**

| Device Under Test              |                                   |
|--------------------------------|-----------------------------------|
| Device Type                    | COMOSAR 2600 MHz REFERENCE DIPOLE |
| Manufacturer                   | MVG                               |
| Model                          | SID2600                           |
| Serial Number                  | SN 38/18 DIP 2G600-468            |
| Product Condition (new / used) | Used                              |

A yearly calibration interval is recommended.

**3 PRODUCT DESCRIPTION**

**3.1 GENERAL INFORMATION**

MVG's COMOSAR Validation Dipoles are built in accordance to the IEEE 1528, FCC KDBs and CEI/IEC 62209 standards. The product is designed for use with the COMOSAR test bench only.



Figure 1 – MVG COMOSAR Validation Dipole





**4 MEASUREMENT METHOD**

The IEEE 1528, FCC KDBs and CEI/IEC 62209 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

**4.1 RETURN LOSS REQUIREMENTS**

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards.

**4.2 MECHANICAL REQUIREMENTS**

The IEEE Std. 1528 and CEI/IEC 62209 standards specify the mechanical components and dimensions of the validation dipoles, with the dimensions frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness.

**5 MEASUREMENT UNCERTAINTY**

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

**5.1 RETURN LOSS**

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.1 dB                              |

**5.2 DIMENSION MEASUREMENT**

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 3 - 300     | 0.05 mm                        |

**5.3 VALIDATION MEASUREMENT**

The guidelines outlined in the IEEE 1528, FCC KDBs, CENELEC EN50361 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 20.3 %               |

*This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*






SAR REFERENCE DIPOLE CALIBRATION REPORT

Rev. ACR.273.4.18.SATL.A

|      |        |
|------|--------|
| 10 g | 20.1 % |
|------|--------|


6 CALIBRATION MEASUREMENT RESULTS

6.1 RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

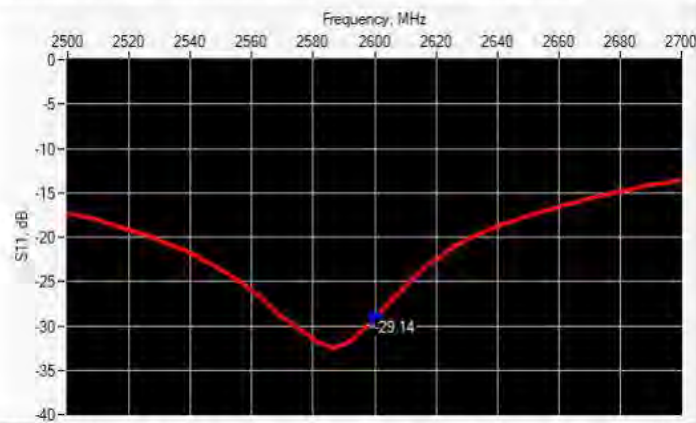

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance       |
|-----------------|------------------|------------------|-----------------|
| 2600            | -29.14           | -20              | 49.2 Ω + 3.4 jΩ |

6.2 RETURN LOSS AND IMPEDANCE IN BODY LIQUID

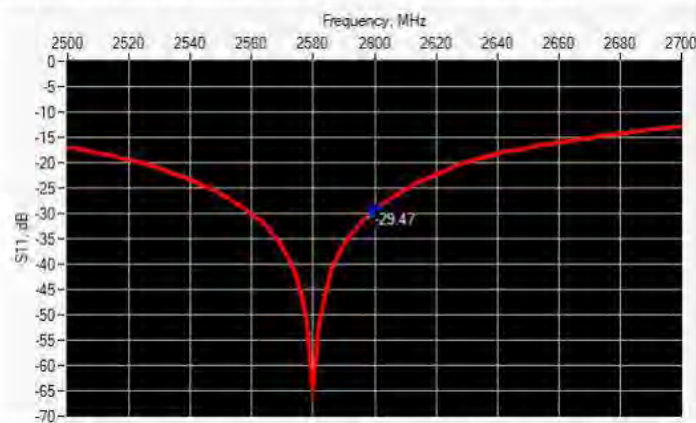

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance       |
|-----------------|------------------|------------------|-----------------|
| 2600            | -29.47           | -20              | 47.5 Ω + 2.2 jΩ |

6.3 MECHANICAL DIMENSIONS

| Frequency MHz | L mm       |          | h mm       |          | d mm      |          |
|---------------|------------|----------|------------|----------|-----------|----------|
|               | required   | measured | required   | measured | required  | measured |
| 300           | 420.0 ±1 % |          | 250.0 ±1 % |          | 6.35 ±1 % |          |

Page: 6/11

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.







SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR-2734-18-SATC-A

|      |            |      |            |      |           |      |
|------|------------|------|------------|------|-----------|------|
| 450  | 290.0 ±1 % |      | 166.7 ±1 % |      | 6.35 ±1 % |      |
| 750  | 176.0 ±1 % |      | 100.0 ±1 % |      | 6.35 ±1 % |      |
| 835  | 161.0 ±1 % |      | 89.8 ±1 %  |      | 3.6 ±1 %  |      |
| 900  | 149.0 ±1 % |      | 83.3 ±1 %  |      | 3.6 ±1 %  |      |
| 1450 | 89.1 ±1 %  |      | 51.7 ±1 %  |      | 3.6 ±1 %  |      |
| 1500 | 80.5 ±1 %  |      | 50.0 ±1 %  |      | 3.6 ±1 %  |      |
| 1640 | 79.0 ±1 %  |      | 45.7 ±1 %  |      | 3.6 ±1 %  |      |
| 1750 | 75.2 ±1 %  |      | 42.9 ±1 %  |      | 3.6 ±1 %  |      |
| 1800 | 72.0 ±1 %  |      | 41.7 ±1 %  |      | 3.6 ±1 %  |      |
| 1900 | 68.0 ±1 %  |      | 39.5 ±1 %  |      | 3.6 ±1 %  |      |
| 1950 | 66.3 ±1 %  |      | 38.5 ±1 %  |      | 3.6 ±1 %  |      |
| 2000 | 64.5 ±1 %  |      | 37.5 ±1 %  |      | 3.6 ±1 %  |      |
| 2100 | 61.0 ±1 %  |      | 35.7 ±1 %  |      | 3.6 ±1 %  |      |
| 2300 | 55.5 ±1 %  |      | 32.6 ±1 %  |      | 3.6 ±1 %  |      |
| 2450 | 51.5 ±1 %  |      | 30.4 ±1 %  |      | 3.6 ±1 %  |      |
| 2600 | 48.5 ±1 %  | PASS | 28.8 ±1 %  | PASS | 3.6 ±1 %  | PASS |
| 3000 | 41.5 ±1 %  |      | 25.0 ±1 %  |      | 3.6 ±1 %  |      |
| 3500 | 37.0 ±1 %  |      | 26.4 ±1 %  |      | 3.6 ±1 %  |      |
| 3700 | 34.7 ±1 %  |      | 26.4 ±1 %  |      | 3.6 ±1 %  |      |

7 VALIDATION MEASUREMENT

The IEEE Std. 1528, FCC KDBs and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

7.1 HEAD LIQUID MEASUREMENT

| Frequency MHz | Relative permittivity (ε <sub>r</sub> ) |          | Conductivity (σ) S/m |          |
|---------------|---|----------|----------------------|----------|
|               | required                                | measured | required             | measured |
| 300           | 45.3 ±5 %                               |          | 0.87 ±5 %            |          |
| 450           | 43.5 ±5 %                               |          | 0.87 ±5 %            |          |
| 750           | 41.9 ±5 %                               |          | 0.89 ±5 %            |          |
| 835           | 41.5 ±5 %                               |          | 0.90 ±5 %            |          |
| 900           | 41.5 ±5 %                               |          | 0.97 ±5 %            |          |
| 1450          | 40.5 ±5 %                               |          | 1.20 ±5 %            |          |
| 1500          | 40.4 ±5 %                               |          | 1.23 ±5 %            |          |
| 1640          | 40.2 ±5 %                               |          | 1.31 ±5 %            |          |
| 1750          | 40.1 ±5 %                               |          | 1.37 ±5 %            |          |

Page: 7/11

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.





SAR REFERENCE DIPOLE CALIBRATION REPORT

RUE ACR.273.4.18.SATC.A

|      |           |      |           |      |
|------|-----------|------|-----------|------|
| 1800 | 40.0 ±5 % |      | 1.40 ±5 % |      |
| 1900 | 40.0 ±5 % |      | 1.40 ±5 % |      |
| 1950 | 40.0 ±5 % |      | 1.40 ±5 % |      |
| 2000 | 40.0 ±5 % |      | 1.40 ±5 % |      |
| 2100 | 39.8 ±5 % |      | 1.49 ±5 % |      |
| 2300 | 39.5 ±5 % |      | 1.67 ±5 % |      |
| 2450 | 39.2 ±5 % |      | 1.80 ±5 % |      |
| 2600 | 39.0 ±5 % | PASS | 1.96 ±5 % | PASS |
| 3000 | 38.5 ±5 % |      | 2.40 ±5 % |      |
| 3500 | 37.9 ±5 % |      | 2.91 ±5 % |      |

7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.

|   |   |
|---|---|
| Software                                  | OPENSAR V4  |
| Phantom                                   | SN 20/09 SAM71  |
| Probe                                     | SN 18/11 EPG122   |
| Liquid                                    | Head Liquid Values: $\sigma_{ps}^2$ : 39.8 $\sigma_{\text{sigma}}$ : 1.99 |
| Distance between dipole center and liquid | 10.0 mm   |
| Area scan resolution                      | dx=8mm/dy=8mm   |
| Zoon Scan Resolution                      | dx=5mm/dy=5mm/dz=5mm  |
| Frequency                                 | 2600 MHz  |
| Input power                               | 20 dBm  |
| Liquid Temperature                        | 21 °C   |
| Lab Temperature                           | 21 °C   |
| Lab Humidity                              | 45 %  |

| Frequency MHz | 1 g SAR (W/kg/W) |          | 10 g SAR (W/kg/W) |          |
|---------------|------------------|----------|-------------------|----------|
|               | required         | measured | required          | measured |
| 300           | 2.85             |          | 1.94              |          |
| 450           | 4.58             |          | 3.06              |          |
| 750           | 8.49             |          | 5.55              |          |
| 835           | 9.56             |          | 6.22              |          |
| 900           | 10.9             |          | 6.99              |          |
| 1450          | 29               |          | 16                |          |
| 1500          | 30.5             |          | 16.8              |          |
| 1640          | 34.2             |          | 18.4              |          |
| 1750          | 36.4             |          | 19.3              |          |
| 1800          | 38.4             |          | 20.1              |          |

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.








SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.273.4.18.SATU.A

股份  
ig Lab

|      |      |              |      |              |
|------|------|--------------|------|--------------|
| 1900 | 39.7 |              | 20.5 |              |
| 1950 | 40.5 |              | 20.9 |              |
| 2000 | 41.1 |              | 21.1 |              |
| 2100 | 43.6 |              | 21.9 |              |
| 2300 | 48.7 |              | 23.3 |              |
| 2450 | 52.4 |              | 24   |              |
| 2600 | 55.3 | 56.91 (5.69) | 24.6 | 24.69 (2.47) |
| 3000 | 63.8 |              | 25.7 |              |
| 3500 | 67.1 |              | 25   |              |
| 3700 | 67.4 |              | 24.2 |              |

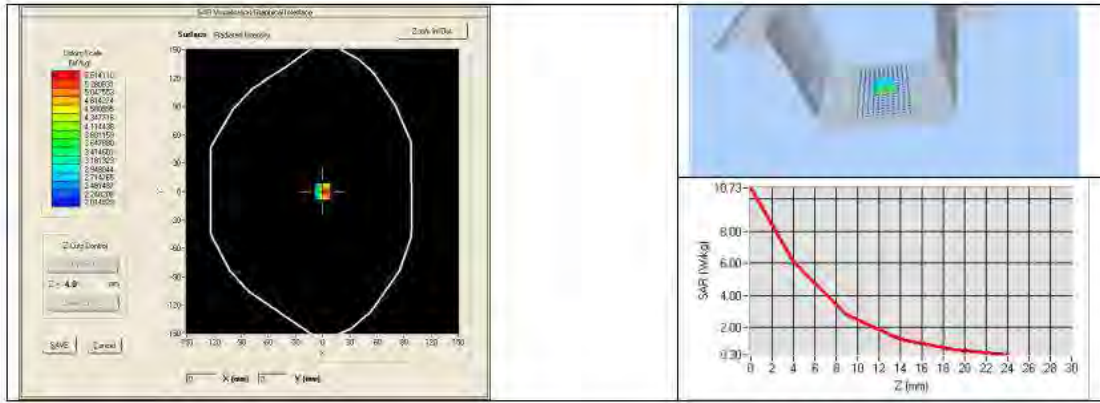

股份  
ig Lab

7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|---|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 150              | 61.9 ±5 %                               |          | 0.80 ±5 %                     |          |
| 300              | 58.2 ±5 %                               |          | 0.92 ±5 %                     |          |
| 450              | 56.7 ±5 %                               |          | 0.94 ±5 %                     |          |
| 750              | 55.5 ±5 %                               |          | 0.96 ±5 %                     |          |
| 835              | 55.2 ±5 %                               |          | 0.97 ±5 %                     |          |
| 900              | 55.0 ±5 %                               |          | 1.05 ±5 %                     |          |
| 915              | 55.0 ±5 %                               |          | 1.06 ±5 %                     |          |
| 1450             | 54.0 ±5 %                               |          | 1.30 ±5 %                     |          |
| 1610             | 53.8 ±5 %                               |          | 1.40 ±5 %                     |          |
| 1800             | 53.3 ±5 %                               |          | 1.52 ±5 %                     |          |
| 1900             | 53.3 ±5 %                               |          | 1.52 ±5 %                     |          |
| 2000             | 53.3 ±5 %                               |          | 1.52 ±5 %                     |          |
| 2100             | 53.2 ±5 %                               |          | 1.62 ±5 %                     |          |

Page: 9/11

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.

股份  
ig Lab





SAR REFERENCE DIPOLE CALIBRATION REPORT


Ref: ACR.273.4.18.SATU.A

|      |            |      |            |      |
|------|------------|------|------------|------|
| 2300 | 52.9 ±5 %  |      | 1.81 ±5 %  |      |
| 2450 | 52.7 ±5 %  |      | 1.95 ±5 %  |      |
| 2600 | 52.5 ±5 %  | PASS | 2.16 ±5 %  | PASS |
| 3000 | 52.0 ±5 %  |      | 2.73 ±5 %  |      |
| 3500 | 51.3 ±5 %  |      | 3.31 ±5 %  |      |
| 3700 | 51.0 ±5 %  |      | 3.55 ±5 %  |      |
| 5200 | 49.0 ±10 % |      | 5.30 ±10 % |      |
| 5300 | 48.9 ±10 % |      | 5.42 ±10 % |      |
| 5400 | 48.7 ±10 % |      | 5.53 ±10 % |      |
| 5500 | 48.6 ±10 % |      | 5.65 ±10 % |      |
| 5600 | 48.5 ±10 % |      | 5.77 ±10 % |      |
| 5800 | 48.2 ±10 % |      | 6.00 ±10 % |      |

7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|   |  |
|---|--|
| Software                                  | OPENSAR V4                                   |
| Phantom                                   | SN 20/09 SAM71                               |
| Probe                                     | SN 18/11 EPG122                              |
| Liquid                                    | Body Liquid Values: eps' : 52.5 sigma : 2.23 |
| Distance between dipole center and liquid | 10.0 mm                                      |
| Area scan resolution                      | dx=8mm/dy=8mm                                |
| Zoon Scan Resolution                      | dx=5mm/dy=5mm/dz=5mm                         |
| Frequency                                 | 2600 MHz                                     |
| Input power                               | 20 dBm                                       |
| Liquid Temperature                        | 21 °C  |
| Lab Temperature                           | 21 °C  |
| Lab Humidity                              | 45 %   |

| Frequency MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|---------------|------------------|-------------------|
|               | measured         | measured          |
| 2600          | 54.14 (5.41)     | 24.13 (2.41)      |

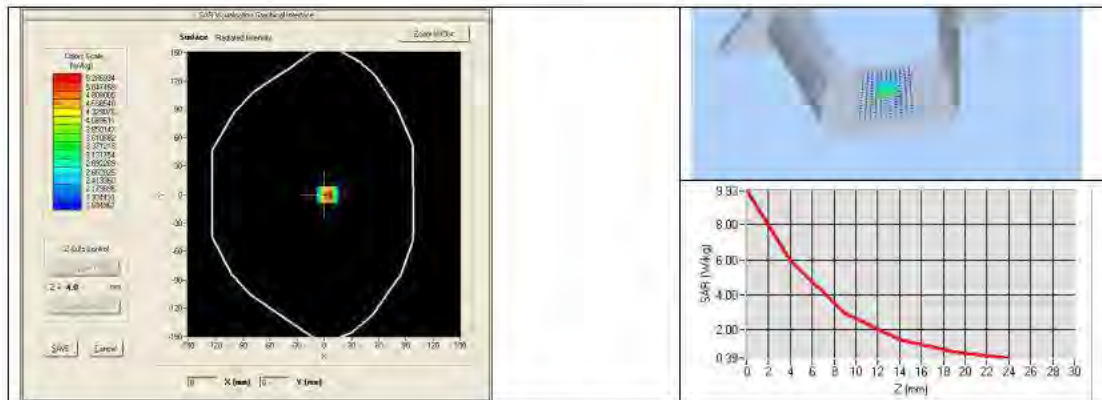

Page: 10/11

This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.





SAR REFERENCE DIPOLE CALIBRATION REPORT

RUE ACR.273.4.18.SATL.A

8 LIST OF EQUIPMENT

| Equipment Summary Sheet         |                      |                    |   |   |
|---------------------------------|----------------------|--------------------|---|---|
| Equipment Description           | Manufacturer / Model | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                     | MVG                  | SN-20/09-SAM71     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench              | Version 3            | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                | Rhode & Schwarz ZVA  | SN100132           | 06/2021                                       | 06/2024                                       |
| Calipers                        | Carrera              | CALIPER-01         | 01/2023                                       | 01/2026                                       |
| Reference Probe                 | MVG                  | EPG122 SN 18/11    | 08/2023                                       | 08/2024                                       |
| Multimeter                      | Keithley 2000        | 1188656            | 01/2023                                       | 01/2026                                       |
| Signal Generator                | Agilent E4438C       | MY49070581         | 01/2023                                       | 01/2026                                       |
| Amplifier                       | Aethercomm           | SN 046             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                     | HP E4418A            | US38261498         | 11/2023                                       | 11/2026                                       |
| Power Sensor                    | HP ECP-E26A          | US37181460         | 01/2023                                       | 01/2026                                       |
| Directional Coupler             | Narda 4216-20        | 01386              | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature and Humidity Sensor | Control Company      | 150798832          | 11/2023                                       | 11/2026                                       |


*This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*



## 6. SAR System PHOTOGRAPHS



Liquid depth  $\geq 15\text{cm}$

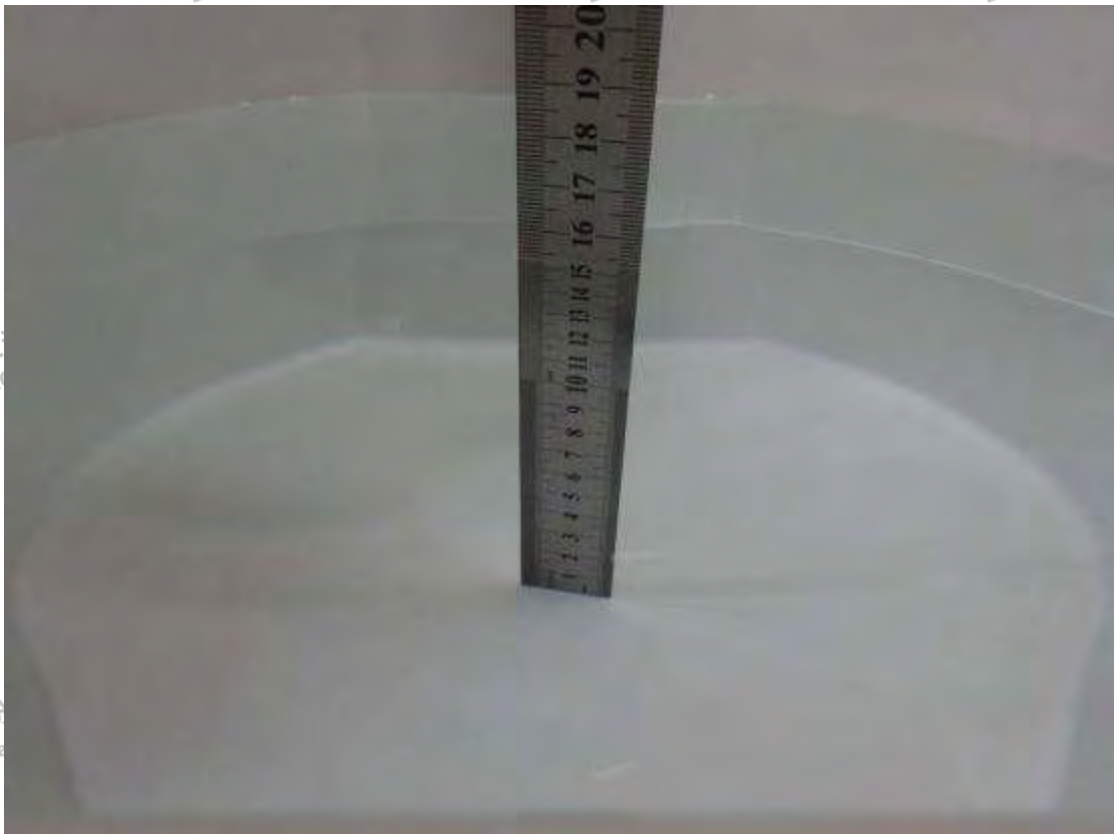



## 7. SETUP PHOTOGRAPHS

Please refer to separated files for Test Setup Photos of SAR.







### 8. EUT PHOTOGRAPHS

Please refer to separated files for Test Setup Photos of SAR

.....The End of Test Report.....

