

EMC Test Report

Application for Grant of Equipment Authorization

Industry Canada RSS-Gen Issue 3 / RSS 210 Issue 8 FCC Part 15 Subpart C

RFID Model ACCRX01

IC CERTIFICATION #: 11508A-ACCRX01
FCC ID: 2AAZF-ACCRX01

APPLICANT: Intuitive Surgical Inc.
1266 Kifer Road
Sunnyvale, CA 94086

TEST SITE(S): National Technical Systems - Silicon Valley
41039 Boyce Road.
Fremont, CA. 94538-2435

IC SITE REGISTRATION #: 2845B-3, 2845B-4

REPORT DATE: December 26, 2013

REISSUE DATE: January 15, 2013

FINAL TEST DATES: November 8 and 13 and December 6, 2013

TOTAL NUMBER OF PAGES: 34

PROGRAM MGR /
TECHNICAL REVIEWER:

QUALITY ASSURANCE DELEGATE /
FINAL REPORT PREPARER:



Mark E Hill
Staff Engineer



David Guidotti
Senior Technical Writer



National Technical Systems - Silicon Valley is accredited by the A2LA, certificate number 0214.26, to perform the test(s) listed in this report, except where noted otherwise. This report and the information contained herein represent the results of testing test articles identified and selected by the client performed to specifications and/or procedures selected by the client. National Technical Systems (NTS) makes no representations, expressed or implied, that such testing is adequate (or inadequate) to demonstrate efficiency, performance, reliability, or any other characteristic of the articles being tested, or similar products. This report should not be relied upon as an endorsement or certification by NTS of the equipment tested, nor does it represent any statement whatsoever as to its merchantability or fitness of the test article, or similar products, for a particular purpose. This report shall not be reproduced except in full

REVISION HISTORY

Rev#	Date	Comments	Modified By
-	12/26/2013	First release	
1	12/31/2013	Reissued to correct test dates on pages 1 and 8	Dave Guidotti
2	1/15/2014	Corrected RSS-GEN/RSS-210 Standard references	Dave Guidotti Mark Hill

TABLE OF CONTENTS

REVISION HISTORY	2
TABLE OF CONTENTS	3
SCOPE.....	4
OBJECTIVE	4
STATEMENT OF COMPLIANCE.....	5
DEVIATIONS FROM THE STANDARDS.....	5
TEST RESULTS SUMMARY	6
DEVICES OPERATING UNDER THE GENERAL LIMITS	6
GENERAL REQUIREMENTS APPLICABLE TO ALL BANDS.....	6
MEASUREMENT UNCERTAINTIES.....	7
EQUIPMENT UNDER TEST (EUT) DETAILS.....	8
GENERAL.....	8
ANTENNA SYSTEM	8
ENCLOSURE.....	8
MODIFICATIONS.....	8
SUPPORT EQUIPMENT	8
EUT INTERFACE PORTS	9
EUT OPERATION	9
TEST SITE.....	10
GENERAL INFORMATION.....	10
CONDUCTED EMISSIONS CONSIDERATIONS	10
RADIATED EMISSIONS CONSIDERATIONS	10
MEASUREMENT INSTRUMENTATION	11
RECEIVER SYSTEM	11
INSTRUMENT CONTROL COMPUTER	11
LINE IMPEDANCE STABILIZATION NETWORK (LISN).....	11
FILTERS/ATTENUATORS	12
ANTENNAS.....	12
ANTENNA MAST AND EQUIPMENT TURNTABLE	12
INSTRUMENT CALIBRATION.....	12
TEST PROCEDURES	13
EUT AND CABLE PLACEMENT	13
CONDUCTED EMISSIONS.....	13
RADIATED EMISSIONS.....	14
BANDWIDTH MEASUREMENTS	15
SPECIFICATION LIMITS AND SAMPLE CALCULATIONS	16
CONDUCTED EMISSIONS SPECIFICATION LIMITS: FCC 15.207; FCC 15.107(A), RSS GEN	16
GENERAL TRANSMITTER RADIATED EMISSIONS SPECIFICATION LIMITS	17
SAMPLE CALCULATIONS - CONDUCTED EMISSIONS	17
SAMPLE CALCULATIONS - RADIATED EMISSIONS.....	18
SAMPLE CALCULATIONS - FIELD STRENGTH TO EIRP CONVERSION.....	19
APPENDIX A TEST EQUIPMENT CALIBRATION DATA	20
APPENDIX B TEST DATA	21
END OF REPORT	34

SCOPE

An electromagnetic emissions test has been performed on the Intuitive Surgical Inc. RFID model ACCRX01, pursuant to the following rules:

Industry Canada RSS-Gen Issue 3

RSS 210 Issue 8 "Low-power Licence-exempt Radiocommunication Devices (All Frequency Bands): Category I Equipment"

FCC Part 15 Subpart C

Conducted and radiated emissions data has been collected, reduced, and analyzed within this report in accordance with measurement guidelines set forth in the following reference standards and as outlined in National Technical Systems - Silicon Valley test procedures:

ANSI C63.10-2009

The intentional radiator above has been tested in a simulated typical installation to demonstrate compliance with the relevant Industry Canada performance and procedural standards.

Final system data was gathered in a mode that tended to maximize emissions by varying orientation of EUT, orientation of power and I/O cabling, antenna search height, and antenna polarization.

Every practical effort was made to perform an impartial test using appropriate test equipment of known calibration. All pertinent factors have been applied to reach the determination of compliance.

OBJECTIVE

The primary objective of the manufacturer is compliance with the regulations outlined in the previous section.

Prior to marketing in the USA, all unlicensed transmitters and transceivers require certification. Receive-only devices operating between 30 MHz and 960 MHz are subject to either certification or a manufacturer's declaration of conformity, with all other receive-only devices exempt from the technical requirements.

Prior to marketing in Canada, Class I transmitters, receivers and transceivers require certification. Class II devices are required to meet the appropriate technical requirements but are exempt from certification requirements.

Certification is a procedure where the manufacturer submits test data and technical information to a certification body and receives a certificate or grant of equipment authorization upon successful completion of the certification body's review of the submitted documents. Once the equipment authorization has been obtained, the label indicating compliance must be attached to all identical units, which are subsequently manufactured.

Maintenance of compliance is the responsibility of the manufacturer. Any modification of the product which may result in increased emissions should be checked to ensure compliance has been maintained (i.e., printed circuit board layout changes, different line filter, different power supply, harnessing or I/O cable changes, etc.).

STATEMENT OF COMPLIANCE

The tested sample of Intuitive Surgical Inc. RFID model ACCRX01 complied with the requirements of the following regulations:

Industry Canada RSS-Gen Issue 3
RSS 210 Issue 8 “Low-power Licence-exempt Radiocommunication Devices (All Frequency Bands): Category I Equipment”
FCC Part 15 Subpart C

Maintenance of compliance is the responsibility of the manufacturer. Any modifications to the product should be assessed to determine their potential impact on the compliance status of the device with respect to the standards detailed in this test report.

The test results recorded herein are based on a single type test of Intuitive Surgical Inc. RFID model ACCRX01 and therefore apply only to the tested sample. The sample was selected and prepared by Bryan Blair of Intuitive Surgical Inc.

DEVIATIONS FROM THE STANDARDS

No deviations were made from the published requirements listed in the scope of this report.

TEST RESULTS SUMMARY**DEVICES OPERATING UNDER THE GENERAL LIMITS**

FCC Rule Part	RSS Rule Part	Description	Measured Value / Comments	Limit / Requirement	Result
15.209	RSS 210 2.5.1 – RSS- GEN Table 6	Transmitter Fundamental Signal Emissions, 13.56 MHz	4.00 dB μ V/m @ 13.561 MHz	Refer to table in limits section	Complies
15.209	RSS 210 2.5.1 – RSS- GEN Table 5 and 6	Transmitter Radiated Spurious Emissions, 9kHz - 150 MHz	35.6 dB μ V/m @ 135.60 MHz	Refer to table in limits section	Complies

GENERAL REQUIREMENTS APPLICABLE TO ALL BANDS

FCC Rule Part	RSS Rule part	Description	Measured Value / Comments	Limit / Requirement	Result (margin)
15.203	-	RF Connector	Integral Antenna	Unique or integral antenna required	Complies
15.207	RSS GEN 7.2.4 Table 4	AC Conducted Emissions	46.2 dB μ V @ 0.150 MHz (-19.8 dB)	Refer to page 16	Complies
15.109	RSS GEN 6.1 Table 2	Receiver spurious emissions	N/A – Receiver tunes below 30MHz		
15.247 (b) (5) 15.407 (f)	RSS 102	RF Exposure Requirements	Refer to RSS 102 declaration	Refer to OET 65, FCC Part 1 and RSS 102	Complies
-	RSP 100 RSS GEN 7.1.2	User Manual	Refer to manual	Statement required regarding non- interference	Complies
-	RSP 100 RSS GEN 7.1.2	User Manual	Antenna is integral	Statement for products with detachable antenna	N/A
-	RSP 100 RSS GEN 4.6.1	99% Bandwidth	221 Hz	Information only	N/A

MEASUREMENT UNCERTAINTIES

ISO/IEC 17025 requires that an estimate of the measurement uncertainties associated with the emissions test results be included in the report. The measurement uncertainties given below are based on a 95% confidence level and were calculated in accordance with UKAS document LAB 34.

Measurement Type	Measurement Unit	Frequency Range	Expanded Uncertainty
RF power, conducted (power meter)	dBm	25 to 7000 MHz	± 0.52 dB
RF power, conducted (Spectrum analyzer)	dBm	25 to 7000 MHz	± 0.7 dB
Conducted emission of transmitter	dBm	25 to 26500 MHz	± 0.7 dB
Conducted emission of receiver	dBm	25 to 26500 MHz	± 0.7 dB
Radiated emission (substitution method)	dBm	25 to 26500 MHz	± 2.5 dB
Radiated emission (field strength)	dB μ V/m	25 to 1000 MHz	± 3.6 dB
		1000 to 40000 MHz	± 6.0 dB
Conducted Emissions (AC Power)	dB μ V	0.15 to 30 MHz	± 2.4 dB

EQUIPMENT UNDER TEST (EUT) DETAILS

GENERAL

The Intuitive Surgical Inc. RFID model ACCRX01 is an RFID 13.56MHz transceiver module for use in the Endoscopic Instrument Control System, model IS4000, intended to assist in the accurate control of endoscopic instruments.

It would be installed in and powered from the Patient Side Cart (PSC). The electrical rating for the PSC is 100-230V, 50/60Hz, 12A.

The sample was received on November 8, 2013 and tested on November 8 and 13 and December 6, 2013. The EUT consisted of the following component(s):

Company	Model	Description	Serial Number	FCC ID
Intuitive Surgical	ACCRX01	RFID Module	P113460366	2AAZF-ACCRX01

ANTENNA SYSTEM

The antenna is integral to the module.

ENCLOSURE

The module does not have an enclosure. It is intended to be mounted in the PSC of the IS4000 system.

MODIFICATIONS

No modifications were made to the EUT during the time the product was at NTS Silicon Valley.

SUPPORT EQUIPMENT

The following equipment was used as support equipment for testing:

Company	Model	Description	Serial Number	FCC ID
Dell	Latitude E6410	Laptop	GYN8XN1	-

EUT INTERFACE PORTS

The I/O cabling configuration during testing was as follows:

Port		Cable(s)		
From	To	Description	Shielded/Unshielded	Length(m)
Laptop USB	EUT	Power/Data Cable	Shielded	2.13

EUT OPERATION

The EUT was configured to continuously transmit in a read/write cycle at 13.56MHz.

TEST SITE**GENERAL INFORMATION**

Final test measurements were taken at the test sites listed below. Pursuant to section 2.948 of the FCC's Rules and section 3.3 of RSP-100, construction, calibration, and equipment data has been filed with the Commission and with industry Canada.

Site	Registration Numbers		Location
	FCC	Canada	
Chamber 3	769238	2845B-3	41039 Boyce Road Fremont, CA 94538-2435
Chamber 4	211948	2845B-4	

ANSI C63.4 recommends that ambient noise at the test site be at least 6 dB below the allowable limits. Ambient levels are below this requirement. The test site(s) contain separate areas for radiated and conducted emissions testing. Considerable engineering effort has been expended to ensure that the facilities conform to all pertinent requirements of ANSI C63.4.

CONDUCTED EMISSIONS CONSIDERATIONS

Conducted emissions testing is performed in conformance with ANSI C63.10. Measurements are made with the EUT connected to the public power network through a nominal, standardized RF impedance, which is provided by a line impedance stabilization network, known as a LISN. A LISN is inserted in series with each current-carrying conductor in the EUT power cord.

RADIATED EMISSIONS CONSIDERATIONS

The FCC has determined that radiation measurements made in a shielded enclosure are not suitable for determining levels of radiated emissions. Radiated measurements are performed in an open field environment or in a semi-anechoic chamber. The test sites are maintained free of conductive objects within the CISPR defined elliptical area incorporated in ANSI C63.4 guidelines and meet the Normalized Site Attenuation (NSA) requirements of ANSI C63.4.

MEASUREMENT INSTRUMENTATION

RECEIVER SYSTEM

An EMI receiver as specified in CISPR 16-1-1 is used for emissions measurements. The receivers used can measure over the frequency range of 9 kHz up to 2000 MHz. These receivers allow both ease of measurement and high accuracy to be achieved. The receivers have Peak, Average, and CISPR (Quasi-peak) detectors built into their design so no external adapters are necessary. The receiver automatically sets the required bandwidth for the CISPR detector used during measurements. If the repetition frequency of the signal being measured is below 20Hz, peak measurements are made in lieu of Quasi-Peak measurements.

For measurements above the frequency range of the receivers, a spectrum analyzer is utilized because it provides visibility of the entire spectrum along with the precision and versatility required to support engineering analysis. Average measurements above 1000MHz are performed on the spectrum analyzer using the linear-average method with a resolution bandwidth of 1 MHz and a video bandwidth of 10 Hz, unless the signal is pulsed in which case the average (or video) bandwidth of the measuring instrument is reduced to onset of pulse desensitization and then increased.

INSTRUMENT CONTROL COMPUTER

The receivers utilize either a Rohde & Schwarz EZM Spectrum Monitor/Controller or contain an internal Spectrum Monitor/Controller to view and convert the receiver measurements to the field strength at an antenna or voltage developed at the LISN measurement port, which is then compared directly with the appropriate specification limit. This provides faster, more accurate readings by performing the conversions described under Sample Calculations within the Test Procedures section of this report. Results are printed in a graphic and/or tabular format, as appropriate. A personal computer is used to record all measurements made with the receivers.

The Spectrum Monitor provides a visual display of the signal being measured. In addition, the controller or a personal computer run automated data collection programs which control the receivers. This provides added accuracy since all site correction factors, such as cable loss and antenna factors are added automatically.

LINE IMPEDANCE STABILIZATION NETWORK (LISN)

Line conducted measurements utilize a fifty microhenry Line Impedance Stabilization Network as the monitoring point. The LISN used also contains a 250 uH CISPR adapter. This network provides for calibrated radio frequency noise measurements by the design of the internal low pass and high pass filters on the EUT and measurement ports, respectively.

FILTERS/ATTENUATORS

External filters and precision attenuators are often connected between the receiving antenna or LISN and the receiver. This eliminates saturation effects and non-linear operation due to high amplitude transient events.

ANTENNAS

A loop antenna is used below 30 MHz. For the measurement range 30 MHz to 1000 MHz either a combination of a biconical antenna and a log periodic or a bi-log antenna is used. Above 1000 MHz, horn antennas are used. The antenna calibration factors to convert the received voltage to an electric field strength are included with appropriate cable loss and amplifier gain factors to determine an overall site factor, which is then programmed into the test receivers or incorporated into the test software.

ANTENNA MAST AND EQUIPMENT TURNTABLE

The antennas used to measure the radiated electric field strength are mounted on a non-conductive antenna mast equipped with a motor-drive to vary the antenna height. Measurements below 30 MHz are made with the loop antenna at a fixed height of 1m above the ground plane.

ANSI C63.10 specifies that the test height above ground for table mounted devices shall be 80 centimeters. Floor mounted equipment shall be placed on the ground plane if the device is normally used on a conductive floor or separated from the ground plane by insulating material from 3 to 12 mm if the device is normally used on a non-conductive floor as specified in ANSI C63.4. During radiated measurements, the EUT is positioned on a motorized turntable in conformance with this requirement.

INSTRUMENT CALIBRATION

All test equipment is regularly checked to ensure that performance is maintained in accordance with the manufacturer's specifications. All antennas are calibrated at regular intervals with respect to tuned half-wave dipoles. An exhibit of this report contains the list of test equipment used and calibration information.

TEST PROCEDURES

EUT AND CABLE PLACEMENT

The regulations require that interconnecting cables be connected to the available ports of the unit and that the placement of the unit and the attached cables simulate the worst case orientation that can be expected from a typical installation, so far as practicable. To this end, the position of the unit and associated cabling is varied within the guidelines of ANSI C63.10, and the worst-case orientation is used for final measurements.

CONDUCTED EMISSIONS

Conducted emissions are measured at the plug end of the power cord supplied with the EUT. Excess power cord length is wrapped in a bundle between 30 and 40 centimeters in length near the center of the cord. Preliminary measurements are made to determine the highest amplitude emission relative to the specification limit for all the modes of operation. Placement of system components and varying of cable positions are performed in each mode. A final peak mode scan is then performed in the position and mode for which the highest emission was noted on all current carrying conductors of the power cord.

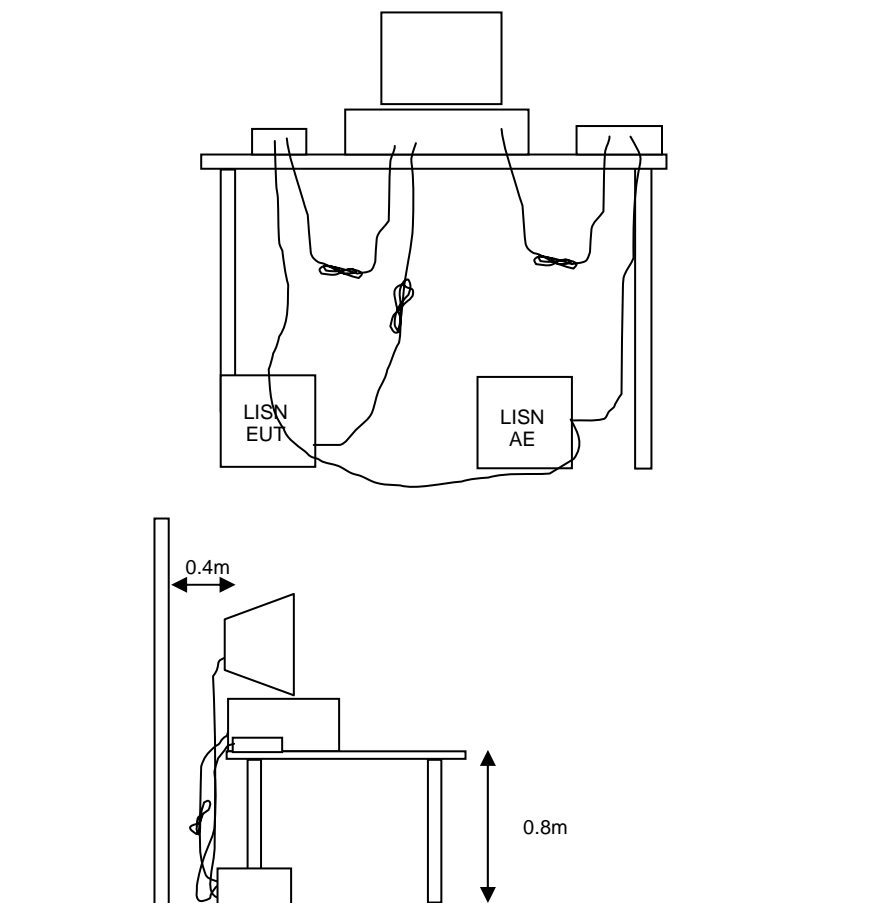


Figure 1 Typical Conducted Emissions Test Configuration


RADIATED EMISSIONS

A preliminary scan of the radiated emissions is performed in which all significant EUT frequencies are identified with the system in a nominal configuration. At least two scans are performed, one scan for each antenna polarization (horizontal and vertical; loop parallel and perpendicular to the EUT). During the preliminary scans, the EUT is rotated through 360°, the antenna height is varied (for measurements above 30 MHz) and cable positions are varied to determine the highest emission relative to the limit. Preliminary scans may be performed in a fully anechoic chamber for the purposes of identifying the frequencies of the highest emissions from the EUT.


A speaker is provided in the receiver to aid in discriminating between EUT and ambient emissions. Other methods used during the preliminary scan for EUT emissions involve scanning with near field magnetic loops, monitoring I/O cables with RF current clamps, and cycling power to the EUT.

Final maximization is a phase in which the highest amplitude emissions identified in the spectral search are viewed while the EUT azimuth angle is varied from 0 to 360 degrees relative to the receiving antenna. The azimuth, which results in the highest emission is then maintained while varying the antenna height from one to four meters (for measurements above 30 MHz, measurements below 30 MHz are made with the loop antenna at a fixed height of 1m). The result is the identification of the highest amplitude for each of the highest peaks. Each recorded level is corrected in the receiver using appropriate factors for cables, connectors, antennas, and preamplifier gain.

When testing above 18 GHz, the receive antenna is located at 1 meter from the EUT and the antenna height is restricted to a maximum of 2.5 meters.

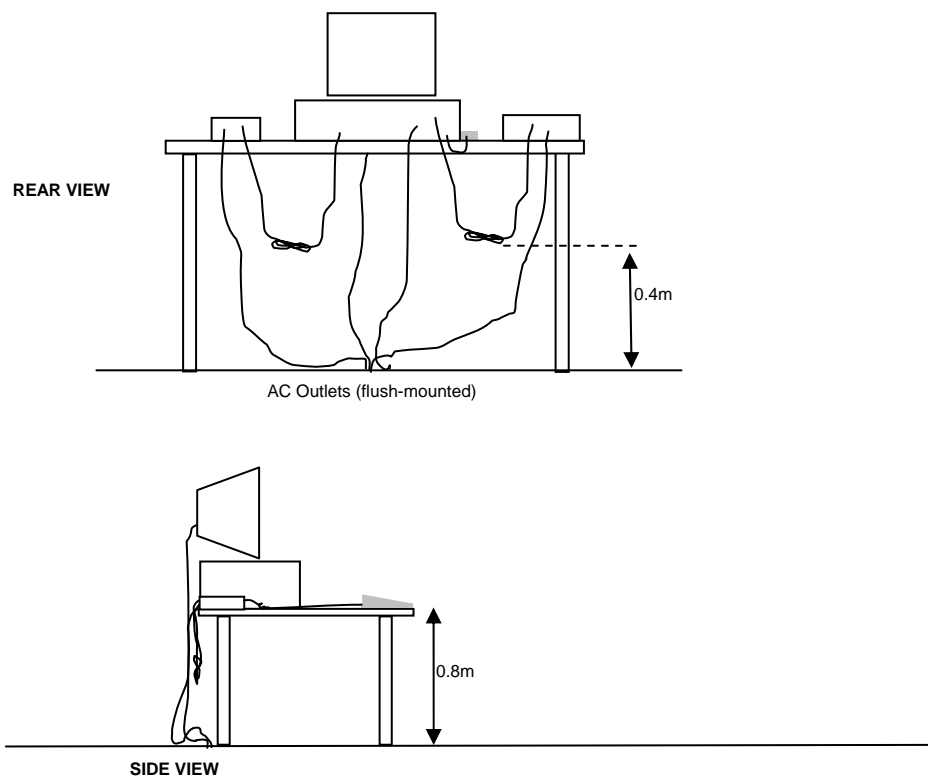


Typical Test Configuration for Radiated Field Strength Measurements

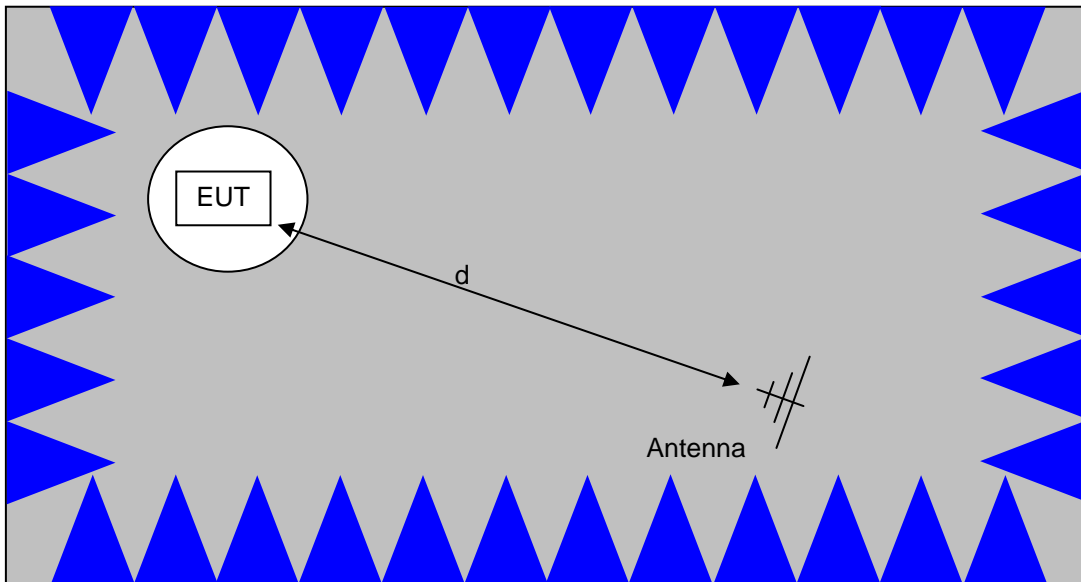

The anechoic materials on the walls and ceiling ensure compliance with the normalized site attenuation requirements of CISPR 16 / CISPR 22 / ANSI C63.4 for an alternate test site at the measurement distances used.

Floor-standing equipment is placed on the floor with insulating supports between the unit and the ground plane.

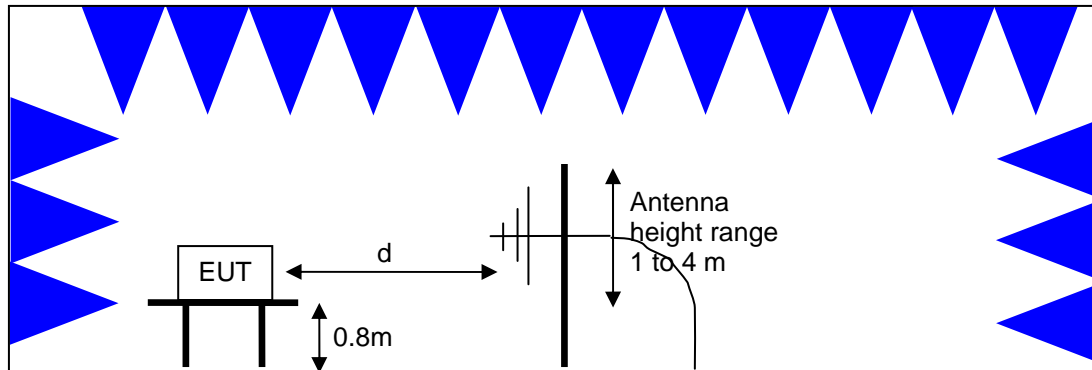

Test Configuration for Radiated Field Strength Measurements
Semi-Anechoic Chamber, Plan and Side Views

BANDWIDTH MEASUREMENTS

The 6dB, 20dB, 26dB and/or 99% signal bandwidth are measured using the bandwidths recommended by ANSI C63.10 and RSS GEN.

SPECIFICATION LIMITS AND SAMPLE CALCULATIONS

The limits for conducted emissions are given in units of microvolts, and the limits for radiated emissions are given in units of microvolts per meter at a specified test distance. Data is measured in the logarithmic form of decibels relative to one microvolt, or dB microvolts (dBuV). For radiated emissions, the measured data is converted to the field strength at the antenna in dB microvolts per meter (dBuV/m). The results are then converted to the linear forms of uV and uV/m for comparison to published specifications.

For reference, converting the specification limits from linear to decibel form is accomplished by taking the base ten logarithm, then multiplying by 20. These limits in both linear and logarithmic form are as follows:

CONDUCTED EMISSIONS SPECIFICATION LIMITS: FCC 15.207; FCC 15.107(a), RSS GEN

The table below shows the limits for the emissions on the AC power line from an intentional radiator and a receiver.

Frequency (MHz)	Average Limit (dBuV)	Quasi Peak Limit (dBuV)
0.150 to 0.500	Linear decrease on logarithmic frequency axis between 56.0 and 46.0	Linear decrease on logarithmic frequency axis between 66.0 and 56.0
0.500 to 5.000	46.0	56.0
5.000 to 30.000	50.0	60.0

GENERAL TRANSMITTER RADIATED EMISSIONS SPECIFICATION LIMITS

The table below shows the limits for the spurious emissions from transmitters that fall in restricted bands¹ (with the exception of transmitters operating under FCC Part 15 Subpart D and RSS 210 Annex 9), the limits for all emissions from a low power device operating under the general rules of RSS 310 (tables 3 and 4), RSS 210 (table 2) and FCC Part 15 Subpart C section 15.209.

Frequency Range (MHz)	Limit (uV/m)	Limit (dBuV/m @ 3m)
0.009-0.490	2400/F _{KHz} @ 300m	67.6-20*log ₁₀ (F _{KHz}) @ 300m
0.490-1.705	24000/F _{KHz} @ 30m	87.6-20*log ₁₀ (F _{KHz}) @ 30m
1.705 to 30	30 @ 30m	29.5 @ 30m
30 to 88	100 @ 3m	40 @ 3m
88 to 216	150 @ 3m	43.5 @ 3m
216 to 960	200 @ 3m	46.0 @ 3m
Above 960	500 @ 3m	54.0 @ 3m

SAMPLE CALCULATIONS - CONDUCTED EMISSIONS

Receiver readings are compared directly to the conducted emissions specification limit (decibel form) as follows:

$$R_r - S = M$$

where:

R_r = Receiver Reading in dBuV

S = Specification Limit in dBuV

M = Margin to Specification in +/- dB

¹ The restricted bands are detailed in FCC 15.203, RSS 210 Table 1 and RSS 310 Table 2

SAMPLE CALCULATIONS - RADIATED EMISSIONS

Receiver readings are compared directly to the specification limit (decibel form). The receiver internally corrects for cable loss, preamplifier gain, and antenna factor. The calculations are in the reverse direction of the actual signal flow, thus cable loss is added and the amplifier gain is subtracted. The Antenna Factor converts the voltage at the antenna coaxial connector to the field strength at the antenna elements.

A distance factor, when used for electric field measurements above 30MHz, is calculated by using the following formula:

$$F_d = 20 * \text{LOG}_{10} (D_m/D_s)$$

where:

$$F_d = \text{Distance Factor in dB}$$

$$D_m = \text{Measurement Distance in meters}$$

$$D_s = \text{Specification Distance in meters}$$

For electric field measurements below 30MHz the extrapolation factor is either determined by making measurements at multiple distances or a theoretical value is calculated using the formula:

$$F_d = 40 * \text{LOG}_{10} (D_m/D_s)$$

Measurement Distance is the distance at which the measurements were taken and Specification Distance is the distance at which the specification limits are based. The antenna factor converts the voltage at the antenna coaxial connector to the field strength at the antenna elements.

The margin of a given emission peak relative to the limit is calculated as follows:

$$R_c = R_r + F_d$$

and

$$M = R_c - L_s$$

where:

$$R_r = \text{Receiver Reading in dBuV/m}$$

$$F_d = \text{Distance Factor in dB}$$

$$R_c = \text{Corrected Reading in dBuV/m}$$

$$L_s = \text{Specification Limit in dBuV/m}$$

$$M = \text{Margin in dB Relative to Spec}$$

SAMPLE CALCULATIONS - FIELD STRENGTH TO EIRP CONVERSION

Where the radiated electric field strength is expressed in terms of the equivalent isotropic radiated power (eirp), or where a field strength measurement of output power is made in lieu of a direct measurement, the following formula is used to convert between eirp and field strength at a distance of d (meters) from the equipment under test:

$$E = \frac{1000000 \sqrt{30 P}}{d} \quad \text{microvolts per meter}$$

where P is the eirp (Watts)

For a measurement at 3m the conversion from a logarithmic value for field strength (dBuV/m) to an eirp power (dBm) is -95.3dB.

Appendix A Test Equipment Calibration Data**Radiated Emissions, .009 - 150 MHz, 08-Nov-13**

<u>Manufacturer</u>	<u>Description</u>	<u>Model</u>	<u>Asset #</u>	<u>Cal Due</u>
EMCO	Magnetic Loop Antenna, 10 kHz-30 MHz	6502	296	4/8/2015
EMCO	Magnetic Loop Antenna, 10 kHz-30 MHz	6502	1299	2/5/2015
Rohde & Schwarz	EMI Test Receiver, 20 Hz-7 GHz	ESIB7	1630	6/22/2014
Sunol Sciences	Biconilog, 30-3000 MHz	JB3	2237	8/23/2014
Com-Power	Preamplifier, 30-1000 MHz	PA-103A	2359	2/20/2014

Conducted Emissions – AC Power Ports, 06-Dec-13

<u>Manufacturer</u>	<u>Description</u>	<u>Model #</u>	<u>Asset #</u>	<u>Cal Due</u>
EMCO	LISN, 10 kHz-100 MHz	3825/2	1293	14-Feb-14
Rohde & Schwarz	Pulse Limiter	ESH3 Z2	1401	15-May-14
Rohde & Schwarz	EMI Test Receiver, 20 Hz-7 GHz	ESIB7	1756	08-Jun-14

Appendix B Test Data

T93665 Pages 22 - 33



EMC Test Data

Client:	Intuitive Surgical, Inc.	Job Number:	J92885
Product:	RFID Model ACCRX01	T-Log Number:	T93665
		Account Manager:	Sheareen Jacobs
Contact:	Bryan Blair		
Emissions Standard(s):	15.225 / RSS-210 Annex A2.6 / EN 300 330	Class:	B
Immunity Standard(s):		Environment:	

EMC Test Data

For The

Intuitive Surgical, Inc.

Product

RFID Model ACCRX01

Date of Last Test: 11/13/2013



EMC Test Data

Client:	Intuitive Surgical, Inc.	Job Number:	J92885
Model:	RFID Model ACCRX01	T-Log Number:	T93665
Contact:	Bryan Blair	Project Manager:	Sheareen Jacobs
Standard:	15.225 / RSS-210 Annex A2.6 / EN 300 330	Project Coordinator:	-
		Class:	N/A

Radiated Emissions

Test Specific Details

Objective: The objective of this test session is to perform engineering evaluation testing of the EUT with respect to the specification listed above.

General Test Configuration

The EUT was located on the turntable for radiated emissions testing. The EUT was tested in all three orthogonal orientations.

The test distance and extrapolation factor (if applicable) are detailed under each run description.

Note, preliminary testing indicates that the emissions were maximized by orientation of the EUT and elevation of the measurement antenna. Maximized testing indicated that the emissions were maximized by orientation of the EUT, elevation of the measurement antenna, and manipulation of the EUT's interface cables.

Ambient Conditions: Temperature: 24 °C
 Rel. Humidity: 42 %

Summary of Results

Run #	Test Performed	Limit	Result	Value / Margin
1	Fundamental Signal Field Strength / Spectral Mask	FCC 15.209 & RSS 210/RSS GEN	Pass	4.00 dBμV/m @ 13.561 MHz (-25.5 dB)
2	Transmitter Radiated Spurious Emissions, 9kHz - 30 MHz, E-Field	FCC 15.209 & RSS 210/RSS GEN	Pass	-2.70 dBμV/m @ 30.00 MHz (-32.2 dB)
3	Transmitter Radiated Spurious Emissions, 30 - 1000 MHz	FCC 15.209 & RSS 210/RSS GEN	Pass	35.6 dBμV/m @ 135.60 MHz (-7.9 dB)
4	99% Bandwidth (center channel)	RSS-GEN	N/A	221 Hz

Modifications Made During Testing

No modifications were made to the EUT during testing

Deviations From The Standard

No deviations were made from the requirements of the standard.



EMC Test Data

Client:	Intuitive Surgical, Inc.	Job Number:	J92885
Model:	RFID Model ACCRX01	T-Log Number:	T93665
		Project Manager:	Sheareen Jacobs
Contact:	Bryan Blair	Project Coordinator:	-
Standard:	15.225 / RSS-210 Annex A2.6 / EN 300 330	Class:	N/A

Run #1: Fundamental Signal Field Strength / Spectral Mask

Date of Test: 11/8/2013
 Test Engineer: John Caizzi
 Test Location: Chamber 3

Config. Used: 1
 Config Change: none
 EUT Voltage:

Frequency Range	Test Distance	Limit Distance	Extrapolation Factor
12.56 - 14.56 MHz	3	30	40.0

Fundamental Field Strength

Frequency MHz	Level dB μ V/m	Pol v/h	FCC 15.209		Detector Pk/QP/Avg	Azimuth degrees	Height meters	Comments
			Limit	Margin				
13.563	-6.4	O	29.5	-35.9	Pk	152	1.37	EUT vert
13.563	2.4	C	29.5	-27.1	Pk	217	1.37	EUT vert
13.561	4.0	O	29.5	-25.5	Pk	89	1.37	EUT hor
13.559	3.3	C	29.5	-26.2	Pk	1	1.37	EUT hor
13.561	4.0	O	29.5	-25.5	Pk	349	1.37	EUT side
13.559	3.7	C	29.5	-25.8	Pk	269	1.37	EUT side

Client:	Intuitive Surgical, Inc.	Job Number:	J92885
Model:	RFID Model ACCRX01	T-Log Number:	T93665
Contact:	Bryan Blair	Project Manager:	Sheareen Jacobs
Standard:	15.225 / RSS-210 Annex A2.6 / EN 300 330	Project Coordinator:	-
		Class:	N/A


Run #2: 9 kHz - 30 MHz E-Field Radiated Emissions

Date of Test: 11/8/2013
 Test Engineer: John Caizzi
 Test Location: Chamber 3



Config. Used: 1
 Config Change: none
 EUT Voltage:

Frequency Range	Test Distance	Limit Distance	Extrapolation Factor
0.009 - 0.490 MHz	10	300	-59.1
0.490 - 1.705 MHz	3	30	-40.0
1.705 - 30.0 MHz	3	30	-40.0


Note - the extrapolation factor is based on $40\log(\text{test distance}/\text{limit distance})$ as permitted by FCC 15.31

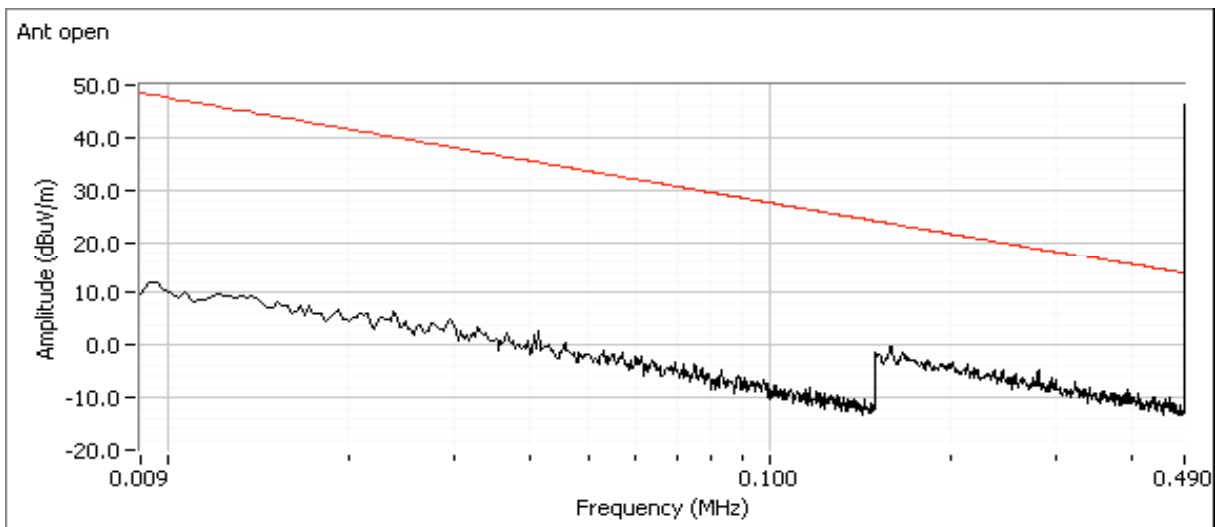

Client: Intuitive Surgical, Inc.	Job Number: J92885
Model: RFID Model ACCRX01	T-Log Number: T93665
Contact: Bryan Blair	Project Manager: Sheareen Jacobs
Standard: 15.225 / RSS-210 Annex A2.6 / EN 300 330	Project Coordinator: -
	Class: N/A

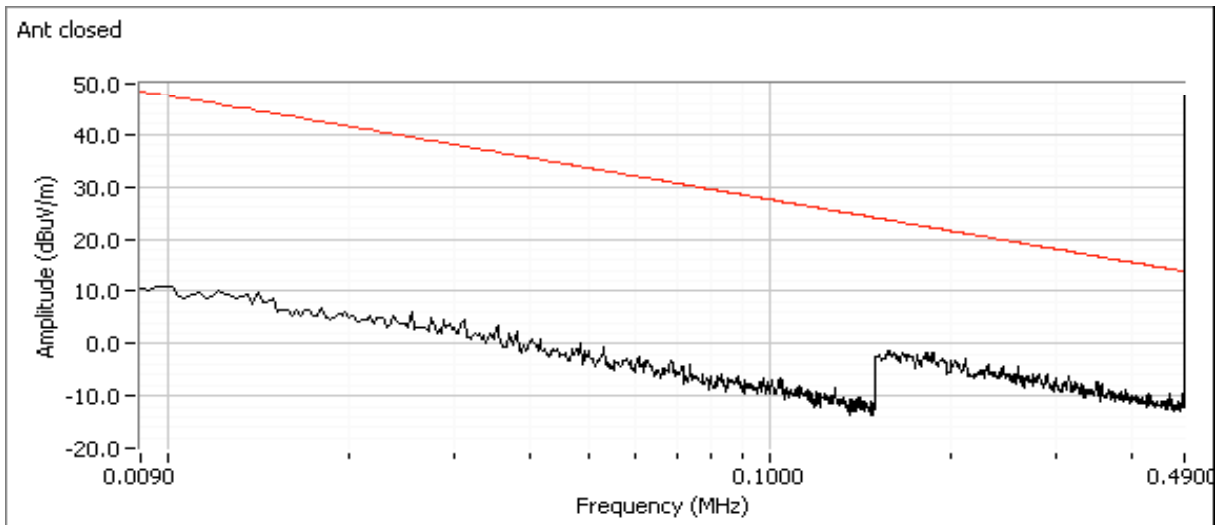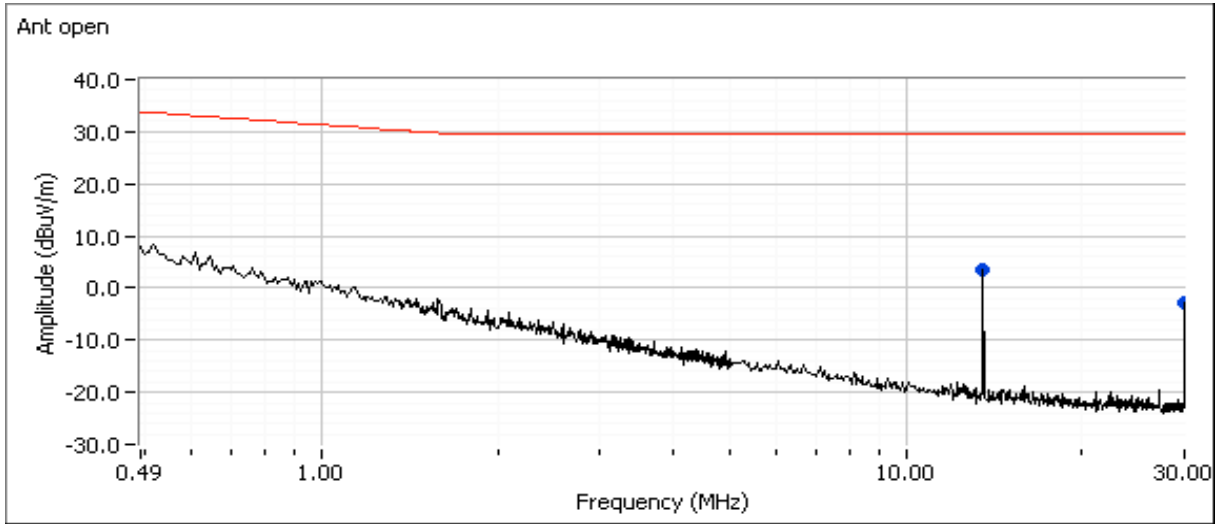

Client:	Intuitive Surgical, Inc.	Job Number:	J92885
Model:	RFID Model ACCRX01	T-Log Number:	T93665
Contact:	Bryan Blair	Project Manager:	Sheareen Jacobs
Standard:	15.225 / RSS-210 Annex A2.6 / EN 300 330	Project Coordinator:	-
		Class:	N/A

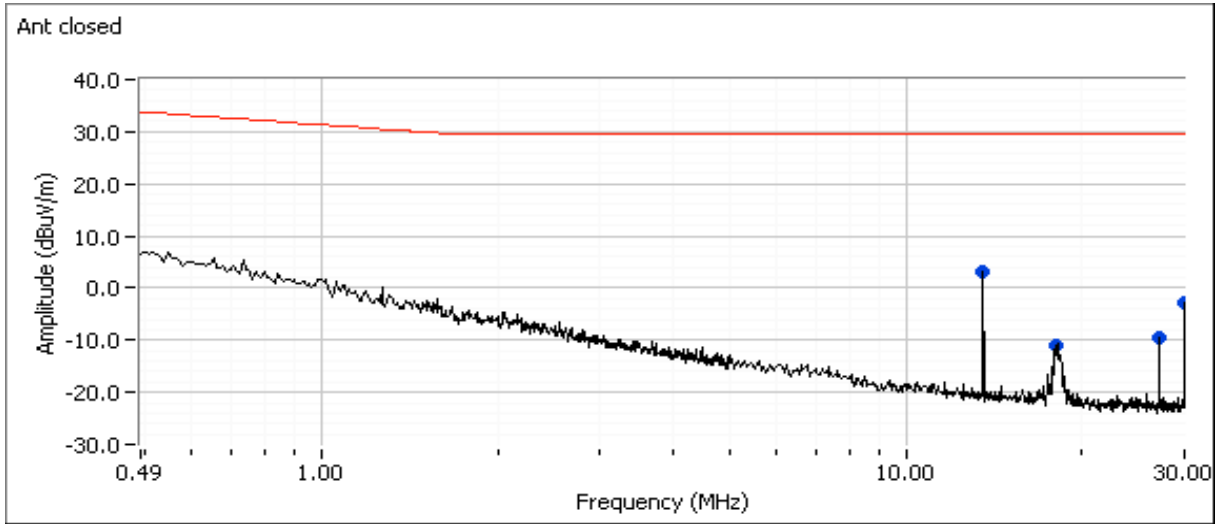

Preliminary readings

Frequency	Level	Pol	FCC 15.209		Detector	Azimuth	Height	Comments
MHz	dB μ V/m	v/h	Limit	Margin	Pk/QP/Avg	degrees	meters	
13.567	3.6	O	29.5	-25.9	Peak	358	1.37	Fundamental
13.567	3.3	C	29.5	-26.2	Peak	282	1.37	Fundamental
18.026	-11.0	C	29.5	-40.5	Peak	291	1.37	
27.144	-9.5	C	29.5	-39.0	Peak	272	1.37	
30.000	-2.7	C	29.5	-32.2	Peak	252	1.37	
30.000	-2.7	O	29.5	-32.2	Peak	213	1.37	

Note 1: The emission limits shown in the above table are based on measurements employing a CISPR quasi-peak detector except for the frequency bands 9-90 kHz, 110-490 kHz and above 1000 MHz. Radiated emission limits in these three bands are based on measurements employing an average detector, with a peak limit 20dB above the average limit.

Note 1: QP measurements not taken since all peak readings were below QP limit.



EMC Test Data


Client: Intuitive Surgical, Inc.	Job Number: J92885
Model: RFID Model ACCRX01	T-Log Number: T93665
Contact: Bryan Blair	Project Manager: Sheareen Jacobs
Standard: 15.225 / RSS-210 Annex A2.6 / EN 300 330	Project Coordinator: -
	Class: N/A

Run #3a: Maximized Readings - Transmitter Spurious Emissions, 30 - 150 MHz

Date of Test: 11/8/2013
 Test Engineer: John Caizzi
 Test Location: Chamber 3

Config. Used: 1
 Config Change: none
 EUT Voltage: 3.3 VDC

Frequency Range	Test Distance	Limit Distance	Extrapolation Factor
30 - 150 MHz	3	3	0.0

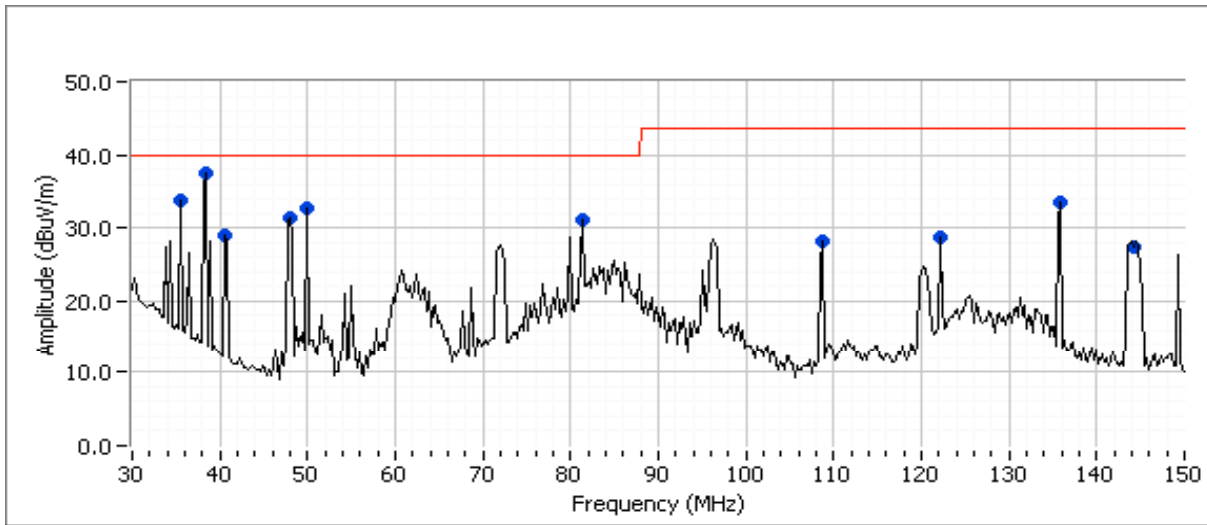

Preliminary Readings

Frequency MHz	Level dB μ V/m	Pol v/h	RSS 210 / FCC 15.209		Detector Pk/QP/Avg	Azimuth degrees	Height meters	Comments
			Limit	Margin				
81.369	31.0	V	40.0	-9.0	Peak	267	1.0	
135.600	33.6	V	43.5	-9.9	Peak	312	1.0	
40.686	29.1	V	40.0	-10.9	Peak	359	1.5	
122.045	28.6	V	43.5	-14.9	Peak	309	1.0	
108.483	28.3	V	43.5	-15.2	Peak	0	1.0	
35.531	33.7	H	40.0	-6.3	Peak	255	4.0	Not related to the radio
38.417	37.6	H	40.0	-2.4	Peak	262	2.0	Not related to the radio
48.036	31.4	V	40.0	-8.6	Peak	267	1.0	Not related to the radio
49.960	32.8	H	40.0	-7.2	Peak	224	4.0	Not related to the radio
144.228	27.5	V	43.5	-16.0	Peak	280	1.0	Not related to the radio



EMC Test Data

Client:	Intuitive Surgical, Inc.	Job Number:	J92885
Model:	RFID Model ACCRX01	T-Log Number:	T93665
		Project Manager:	Sheareen Jacobs
Contact:	Bryan Blair	Project Coordinator:	-
Standard:	15.225 / RSS-210 Annex A2.6 / EN 300 330	Class:	N/A

Maximized readings (includes manipulation of EUT interface cables)

Frequency	Level	Pol	RSS 210 / FCC 15.209		Detector	Azimuth	Height	Comments
MHz	dB μ V/m	v/h	Limit	Margin	Pk/QP/Avg	degrees	meters	
135.600	35.6	V	43.5	-7.9	QP	327	1.00	
81.369	30.6	V	40.0	-9.4	QP	289	1.00	
40.686	29.9	V	40.0	-10.1	QP	359	1.00	
122.045	29.8	V	43.5	-13.7	QP	352	1.00	
108.483	28.4	V	43.5	-15.1	QP	351	1.00	



EMC Test Data

Client: Intuitive Surgical, Inc.	Job Number: J92885
Model: RFID Model ACCRX01	T-Log Number: T93665
Contact: Bryan Blair	Project Manager: Sheareen Jacobs
Standard: 15.225 / RSS-210 Annex A2.6 / EN 300 330	Project Coordinator: -
	Class: N/A


Run #4: Bandwidth Measurement(s)

Date of Test: 11/13/2013
 Test Engineer: John Caizzi
 Test Location: Lab 4A

Config. Used:
 Config Change:
 EUT Voltage: 5 VDC

Power Setting	Frequency (MHz)	Resolution Bandwidth	Video Bandwidth	99% Bandwidth
Max	13.56	100Hz	300Hz	221

Note 1: 99% bandwidth measured in accordance with RSS GEN, with RB > 1% of the span and VB > 3xRB

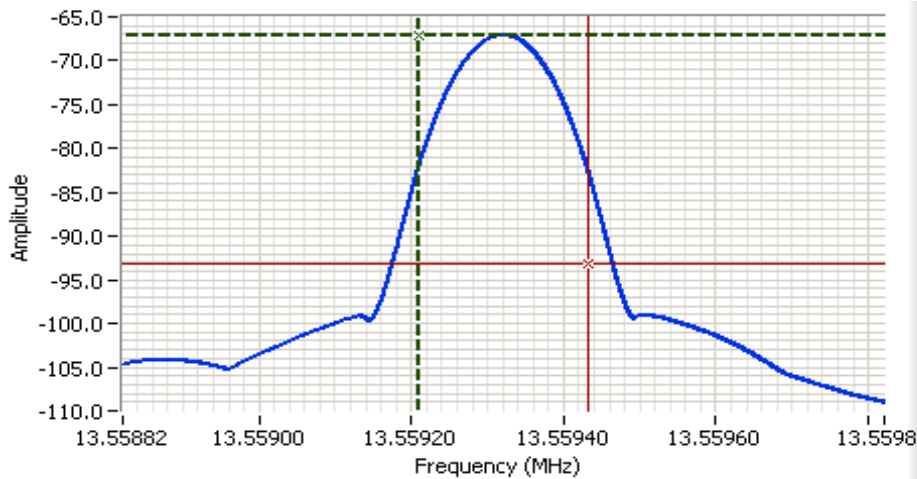

Analyzer Settings
 Agilent Technologies, E4446A
 CF: 13.559 MHz
 SPAN: 1.00 kHz
 RB: 100 Hz
 VB: 300 Hz
 Detector: POS
 Attn: 0 DB
 RL Offset: 0.0 DB
 Sweep Time: 18.6ms
 Ref Lvl: -50.0 DBM

Comments
 99% power BW: 221 Hz
 Power over span: -67.01dBm

Cursor 1	13.5592	-67.08	
Cursor 2	13.5594	-93.08	

Delta Freq. 221 Hz
 Delta Amplitude 26.00





EMC Test Data

Client: Intuitive Surgical, Inc.	Job Number: J92885
Model: RFID Model ACCRX01	T-Log Number: T93665
	Project Manager: Sheareen Jacobs
Contact: Bryan Blair	Project Coordinator: -
Standard: 15.225 / RSS-210 Annex A2.6 / EN 300 330	Class: B

Conducted Emissions

(Elliott Laboratories Fremont Facility, Semi-Anechoic Chamber)

Test Specific Details

Objective: The objective of this test session is to perform final qualification testing of the EUT with respect to the specification listed above.

Date of Test: 12/6/2013	Config. Used: 1
Test Engineer: Chris Groat	Config Change: none
Test Location: Fremont Chamber #4	EUT Voltage: 120V/60Hz

General Test Configuration

For tabletop equipment, the EUT was located on a wooden table inside the semi-anechoic chamber, 40 cm from a vertical coupling plane and 80cm from the LISN. A second LISN was used for all local support equipment. Remote support equipment was located outside of the semi-anechoic chamber. Any cables running to remote support equipment were routed through metal conduit and when possible passed through a ferrite clamp upon exiting the chamber.

Ambient Conditions:

Temperature:	21 °C
Rel. Humidity:	34 %

Summary of Results

Run #	Test Performed	Limit	Result	Margin
1	CE, AC Power, 120V/60Hz	15.207	Pass	46.2 dB μ V @ 0.150 MHz (-19.8 dB)

Modifications Made During Testing

No modifications were made to the EUT during testing



9

Deviations From The Standard

No deviations were made from the requirements of the standard.

Client: Intuitive Surgical, Inc.	Job Number: J92885
Model: RFID Model ACCRX01	T-Log Number: T93665
Contact: Bryan Blair	Project Manager: Sheareen Jacobs
Standard: 15.225 / RSS-210 Annex A2.6 / EN 300 330	Project Coordinator: -
	Class: B

Run #1: AC Power Port Conducted Emissions, 0.15 - 30MHz, 120V/60Hz
RFID Module

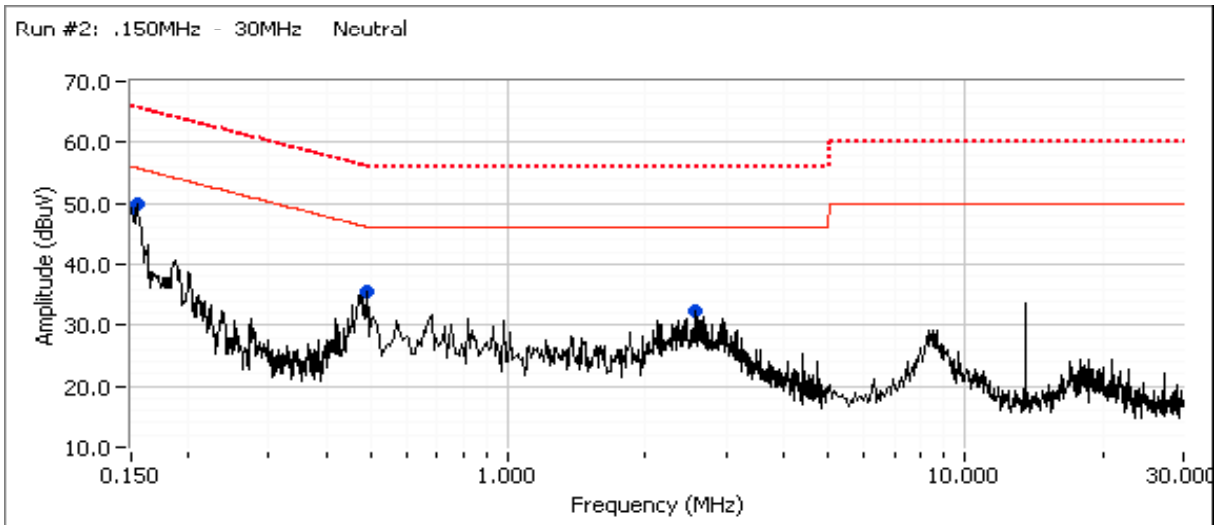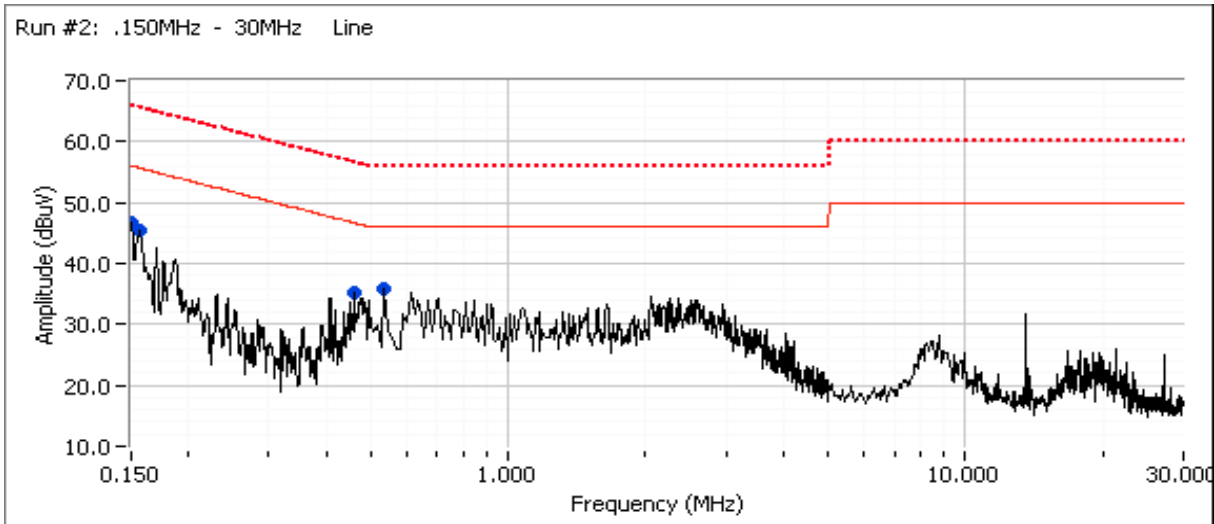



EMC Test Data

Client: Intuitive Surgical, Inc.	Job Number: J92885
Model: RFID Model ACCRX01	T-Log Number: T93665
	Project Manager: Sheareen Jacobs
Contact: Bryan Blair	Project Coordinator: -
Standard: 15.225 / RSS-210 Annex A2.6 / EN 300 330	Class: B

Run #2: AC Power Port Conducted Emissions, 0.15 - 30MHz, 120V/60Hz
RFID Module

Preliminary peak readings captured during pre-scan (peak readings vs. average limit)

Frequency MHz	Level dB μ V	AC Line	FCC 15.207		Detector QP/Ave	Comments
			Limit	Margin		
0.155	50.0	Neutral	55.7	-5.7	Peak	
0.150	49.4	Neutral	56.0	-6.6	Peak	
0.150	46.7	Line 1	56.0	-9.3	Peak	
0.538	35.8	Line 1	46.0	-10.2	Peak	
0.156	45.3	Line 1	55.6	-10.3	Peak	
0.492	35.6	Neutral	46.1	-10.5	Peak	
0.462	35.2	Line 1	46.7	-11.5	Peak	
2.575	32.3	Neutral	46.0	-13.7	Peak	

Final quasi-peak and average readings

Frequency MHz	Level dB μ V	AC Line	FCC 15.207		Detector QP/Ave	Comments
			Limit	Margin		
0.150	46.2	Neutral	66.0	-19.8	QP	QP (1.00s)
0.155	44.2	Neutral	65.7	-21.5	QP	QP (1.00s)
0.150	44.0	Line 1	66.0	-22.0	QP	QP (1.00s)
0.156	42.0	Line 1	65.7	-23.7	QP	QP (1.00s)
0.462	21.5	Line 1	46.7	-25.2	AVG	AVG (0.10s)
0.492	30.9	Neutral	56.1	-25.2	QP	QP (1.00s)
0.155	30.3	Neutral	55.7	-25.4	AVG	AVG (0.10s)
0.492	20.2	Neutral	46.1	-25.9	AVG	AVG (0.10s)
2.575	20.1	Neutral	46.0	-25.9	AVG	AVG (0.10s)
0.462	30.2	Line 1	56.7	-26.5	QP	QP (1.00s)
0.150	29.3	Line 1	56.0	-26.7	AVG	AVG (0.10s)
2.575	29.2	Neutral	56.0	-26.8	QP	QP (1.00s)
0.150	28.3	Neutral	56.0	-27.7	AVG	AVG (0.10s)
0.538	26.0	Line 1	56.0	-30.0	QP	QP (1.00s)
0.156	25.6	Line 1	55.7	-30.1	AVG	AVG (0.10s)
0.538	15.2	Line 1	46.0	-30.8	AVG	AVG (0.10s)

End of Report

This page is intentionally blank and marks the last page of this test report.