



Appendix D


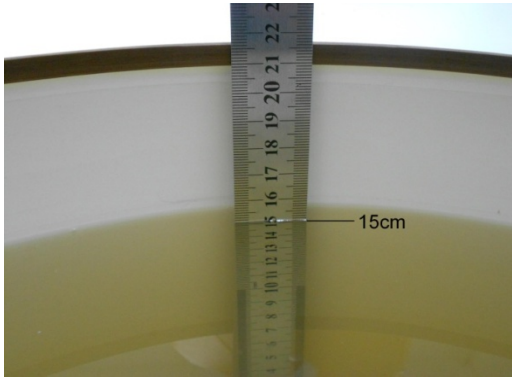



Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details







1. SAR measurement System



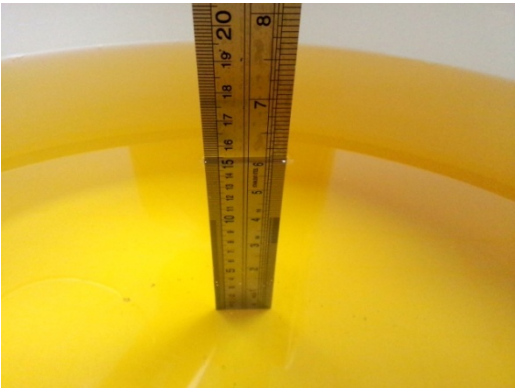



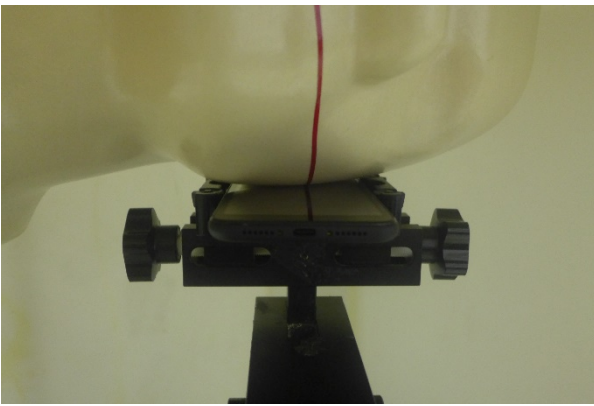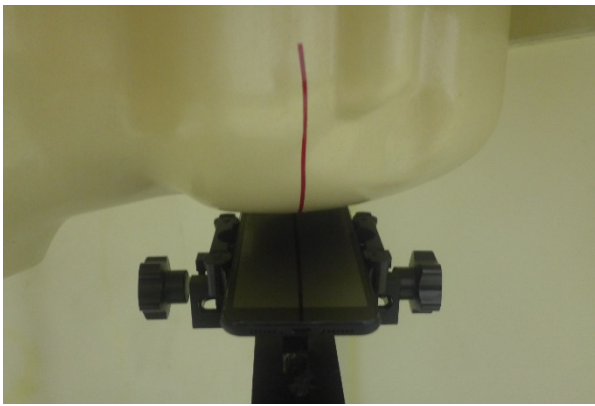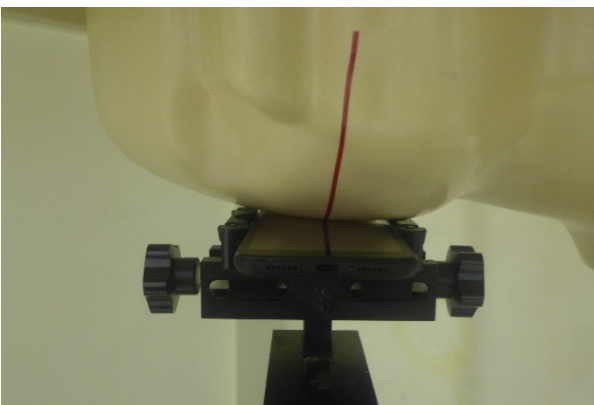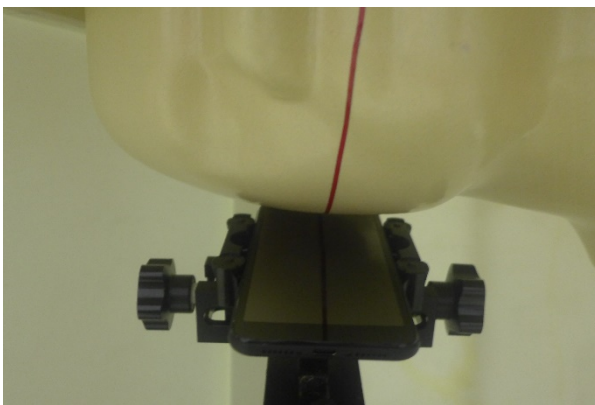

2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 750</p>	<p>Photo 2: Tissue Simulant Liquid for Head 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1750</p>	<p>Photo 4: Tissue Simulant Liquid for Head 1900</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2450</p>	<p>NA</p>
	<p>NA</p>

3. Photographs of EUT test position

<p>Photo 6: Left touch cheek</p>	<p>Photo 7: Left tilted 15 degree</p>
	
<p>Photo 8: Right touch cheek</p>	<p>Photo 9: Right tilted 15 degree</p>
	
<p>Photo 10: Front side 15mm</p>	<p>Photo 11: Back side 15mm</p>
	

<p>Photo 12: Front side 10mm</p>	<p>Photo 13: Back side 10mm</p>
	
<p>Photo 14: Left side 10mm</p>	<p>Photo 15: Right side 10mm</p>
	
<p>Photo 16: Top side 10mm</p>	<p>Photo 17: Bottom side 10mm</p>
	

4. EUT Constructional Details

