## Compliance Certification Services Inc. Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

## ANSI/IEEE Std. C95.1-1992 In accordance with the requirements of FCC Report and Order: ET Docket 93-62; FCC 47 CFR Part 2 (2.1093)

## FCC SAR TEST REPORT

For

Product Name: Mobile Phone

Brand Name: Sky Devices

Model No.: Sky 5.5W

Series Model: N/A

Test Report Number: C141229S01-SF

Issued for

Sky Phone LLC

1348 Washington Av. #350 Miami Beach, FL 33139 United States

Issued by

**Compliance Certification Services Inc.** 

Kun Shan Laboratory No.10 Weiye Rd., Innovation park, Eco&Tec, Development Zone, Kunshan City, Jiangsu, China TEL: 86-512-57355888

FAX: 86-512-57370818



Note: This report shall not be reproduced except in full, without the written approval of Compliance Certification Services Inc. This document may be altered or revised by Compliance Certification Services Inc. personnel only, and shall be noted in the revision section of the document. The client should not use it to claim product endorsement by A2LA or any government agencies. The test results in the report only apply to the tested sample.

Page 1 of 126



# ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue :January 26, 2015

## **Revision History**

Revision	REPORT NO.	Date	Page Revised	Contents
Original	C141229S01-SF	January 26, 2015	N/A	N/A

# ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue : January 26, 2015

## **TABLE OF CONTENTS**

1.	CERTIFICATE OF COMPLIANCE (SAR EVALUATION)	4
2.	EUT DESCRIPTION	5
3.	REQUIREMENTS FOR COMPLIANCE TESTING DEFINED BY THE FCC	6
4.	TEST METHODOLOGY	6
5.	TEST CONFIGURATION	6
6.	DOSIMETRIC ASSESSMENT SETUP	7
	6.1 MEASUREMENT SYSTEM DIAGRAM	
	6.2 SYSTEM COMPONENTS	9
7.	EVALUATION PROCEDURES	
8.	MEASUREMENT UNCERTAINTY	
9.	EXPOSURE LIMIT	
10.		
	10.1 ANTHROPOMORPHIC HEAD PHANTOM	-
	10.2 DEFINITION OF THE "CHEEK/TOUCH" POSITION	
	10.3 DEFINITION OF THE "TILTED" POSITION	
11.	MEASUREMENT RESULTS	21
	11.1 TEST LIQUIDS CONFIRMATION	21
	11.2 LIQUID MEASUREMENT RESULTS	
	11.3 SYSTEM PERFORMANCE CHECK	23
	11.4 EUT TUNE-UP PROCEDURES AND TEST MODE	25
	11.5 SAR TEST CONFIGURATIONS	
	11.6 EUT SETUP PHOTOS	
	11.7 SAR MEASUREMENT RESULTS	
	11.8 REPEATED SAR MEASUREMENT	
	11.9 SAR HANDSETS MULTI XMITER ASSESSMENT	42
EU	ГРНОТО	
12.	EQUIPMENT LIST & CALIBRATION STATUS	52
13.	FACILITIES	53
14.	REFERENCES	53
15.	ATTACHMENTS	54
Арр	pendix A: Plots of Performance Check	55
Арр	pendix B: DASY Calibration Certificate	64
Арр	pendix C: Plots of SAR Test Result	

# **1. CERTIFICATE OF COMPLIANCE (SAR EVALUATION)**

Product Name:	Mobile Phone						
Brand Name:	Sky Devices	Sky Devices					
Model Name.:	Sky 5.5W						
Series Model:	N/A						
Devices supporting GPRS/EDGE:	Class B	Class B					
Description Test Modes(worst case ):	simultaneous work, only su	The product has two SIM, SIM 1 and SIM 2 sharing a chipset does not support simultaneous work, only supports a single transmitter SIM1 or SIM 2, using SIM 1, SIM 2 will be suspended until select SIM 2, stop using the SIM 1, SIM 2 only would working.					
Device Category:	PORTABLE DEVICES						
Exposure Category:	GENERAL POPULATION/UNCONTROLLED EXPOSURE						
Date of Test:	January 5, 2015 to January 8, 2015						
Applicant:	Sky Phone LLC 1348 Washington Av. #350 Miami Beach, FL 33139 United States						
Manufacturer:		Shenzhen Konka Telecommunications Technology Co., Ltd. No.9008 Shennan Road, Overseas Chinese Town, ShenZhen, Guangdong, China					
Application Type:	Certification						
	APPLICABLE STANDARD	S AND TEST PROCEDURES					
STANDARDS AND	TEST PROCEDURES	TEST RESULT					
ANSI/IEEE	E C95.1-1992	No non-compliance noted					
	Deviation from A	pplicable Standard					
None							
and procedures specified stated device/equipment.	l in KDB 865664 The test re	vices Inc. in accordance with the measurement methods sults in this report apply only to the tested sample of the ent will not necessarily produce the same results due to					
<b></b>							

Approved by:	Tested by:		
Jeff fang	Kevin. Hua		
Jeff.fang RF Manager Compliance Certification Services Inc.	Kevin.hua Test Engineer Compliance Certification Services Inc.		

# 2. EUT DESCRIPTION

Product Name:	Mobile Phone					
Brand Name:	Sky Devices					
Model Name.:	Sky 5.5W					
Series Model:	N/A					
Model Discrepancy:	N/A					
FCC ID:	2ABOSSKY55W					
Power reduction:	NO					
DTM Description:	N/A					
Device Category:	Production unit					
Frequency Range:	GSM 850: 824.2 ~ 848.8 MHz PCS1900: 1850.2 ~ 1909.8 MHz WCDMA Band II:1852.4~1907.6MHz WCDMA Band IV:1712.4~1752.6MHz WCDMA Band V:826.4~846.6 MHz WLAN 2.4G: 2412 ~ 2462 MHz Bluetooth: 2402 ~ 2480 MHz					
Transmit Power(Average):	GSM 850: 32.76 dBm         802.11b: 14.92 dBm           PCS 1900: 29.39 dBm         802.11g: 14.33 dBm           WCDMA Band II: 21 84 dBm         802.11n HT20: 13.86					
Max. Reported SAR(1g):	Head:         Body:           GSM 850: 0.380 W/kg         GSM 850: 0.998 W/kg           PCS 1900: 0.336 W/kg         PCS 1900: 0.483 W/kg           WCDMA Band II: 0.613 W/kg         WCDMA Band II: 0.786 W/kg           WCDMA Band IV: 0.263 W/kg         WCDMA Band IV: 0.281 W/WCDMA Band V: 0.342 W/kg					
Modulation Technique:	WLAN 2.4G: 0.906 W/kgWLAN 2.4G: 0.096 W/kgGSM/GPRS/EDGE: GMSKEDGE:8PSKRMC/AMR: QPSKHSDPA: QPSKHSUPA: QPSKIEEE 802.11b: DSSS (CCK, DQPSK, DBPSK)IEEE 802.11g: DSSS (CCK, DQPSK, DBPSK)+OFDM (QPSK, BPSK, 16-QAM, 64-QAM)IEEE 802.11n: OFDM(MCS 0-7)Bluetooth 3.0: GFSK + π/4DQPSK+8DPSKBLE 4.0: GFSK					
Accessories:	Battery (rating) :					
Antenna Specification:	Capacitance: 3.8V 2400mAh GSM&WCDMA: PIFA Antenna Wifi&Bluetooth: CHIP Antenna					
Operating Mode:	Maximum continuous output					

Date of Issue : January 26, 2015

## 3. REQUIREMENTS FOR COMPLIANCE TESTING DEFINED BY **THE FCC**

The US Federal Communications Commission has released the report and order "Guidelines for Evaluating the Environmental Effects of RF Radiation", ET Docket No. 93-62 in August 1996. The order requires routine SAR evaluation prior to equipment authorization of portable transmitter devices, including portable telephones. For consumer products, the applicable limit is 1.6 W/Kg for an uncontrolled environment and 8.0 W/Kg for an occupational/controlled environment as recommended by the ANSI/IEEE standard C95.1-1992.

# 4. TEST METHODOLOGY

The Specific Absorption Rate (SAR) testing specification, method and procedure for this device is in accordance with the following standards:

K FCC 47 CFR Part 2 ( 2.1093)

ANSI/IEEE C95.1-1992

SAR Measurement Procedures for 802.11 a/b/g Transmitters KDB 248227 D01v01r02 KDB 447498 D01v05r02 General RF Exposure Guidance KDB 648474 D04v01r02 Handset SAR KDB 865664 D01v01r03 SAR Measurement 100 MHz to 6 GHz KDB 865664 D02v01r01 **RF Exposure Reporting** KDB 941225 D01v03 **3G SAR Procedures** KDB 941225 D06v02 Hot Spot SAR

# 5. TEST CONFIGURATION

For WWAN SAR testing The device was controlled by using a base station emulator R&S CMU200. Communication between the device and the emulator was established by air link. The distance between the DUT and the antenna of the emulator is larger than 50 cm and the output power radiated from the emulator antenna is at least 30 dB smaller than the output power of DUT. The DUT was set from the emulator to radiate maximum output power during all tests.

During WLAN SAR testing EUT is configured with the WLAN continuous TX tool, and the transmission duty factor was monitored on the spectrum analyzer with zero-span setting For WLAN SAR testing, WLAN engineering test software installed on the EUT can provide continuous transmitting RF signal.

Date of Issue : January 26, 2015

# 6. DOSIMETRIC ASSESSMENT SETUP

These measurements were performed with the automated near-field scanning system DASY 5 from ATTENNESSA. The system is based on a high precision robot (working range greater than 0.9 m), which positions the probes with a positional repeatability of better than ± 0.02 mm. Special E- and H-field probes have been developed for measurements close to material discontinuity, the sensors of which are directly loaded with a Schottky diode and connected via highly resistive lines to the data acquisition unit. The SAR measurements were conducted with the E-field PROBE EX3DV4 (manufactured by SPEAG), designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe has been calibrated according to the procedure described in [7] with accuracy of better than  $\pm 10\%$ . The spherical isotropy was evaluated with the procedure described in [8] and found to be better than ±0.25 dB. The phantom used was the SAM Twin Phantom as described in FCC supplement C, IEE P1528 and CENELEC EN 62209.

Ingredients	Frequency (MHz)									
(% by weight)	4	50	83	35	9	15	19	00	24	50
Tissue Type	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body
Water	38.56	51.16	41.45	52.4	41.05	56.0	54.9	40.4	62.7	73.2
Salt (NaCl)	3.95	1.49	1.45	1.4	1.35	0.76	0.18	0.5	0.5	0.04
Sugar	56.32	46.78	56.0	45.0	56.5	41.76	0.0	58.0	0.0	0.0
HEC	0.98	0.52	1.0	1.0	1.0	1.21	0.0	1.0	0.0	0.0
Bactericide	0.19	0.05	0.1	0.1	0.1	0.27	0.0	0.1	0.0	0.0
Triton X-100	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	36.8	0.0
DGBE	0.0	0.0	0.0	0.0	0.0	0.0	44.92	0.0	0.0	26.7
Dielectric Constant	43.42	58.0	42.54	56.1	42.0	56.8	39.9	54.0	39.8	52.5
Conductivity (S/m)	0.85	0.83	0.91	0.95	1.0	1.07	1.42	1.45	1.88	1.78


### The following table gives the recipes for tissue simulating liquids.

Compliance Certification Services Inc.

Report No: C141229S01-SF

Date of Issue :January 26, 2015

## **6.1 MEASUREMENT SYSTEM DIAGRAM**

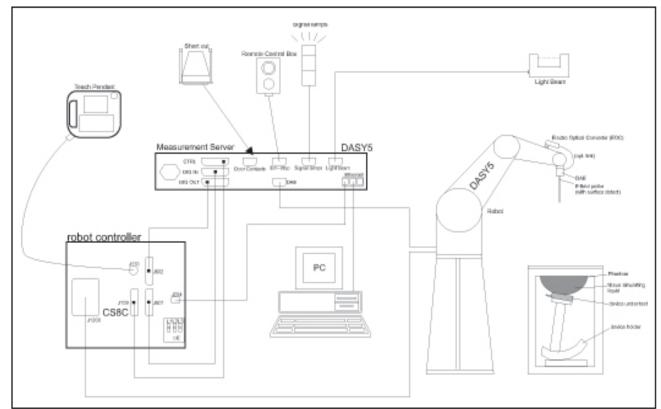

FCC ID: 2ABOSSKY55W


#### The DASY5 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (St"aubli RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows 7.
- DASY5 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM twin phantom enabling testing left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing validating the proper functioning of the system.

Page 8 of 126

Date of Issue : January 26, 2015

## **6.2 SYSTEM COMPONENTS**

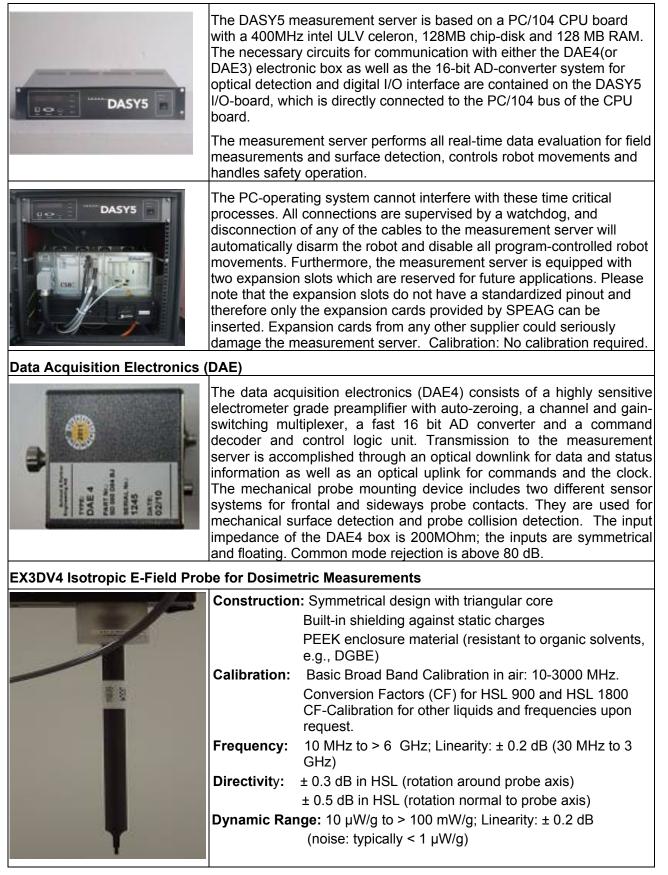

## **Compliance Certification Services Inc.** Report No: C141229S01-SF



FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

- **Dimensions:** Overall length: 337 mm (Tip: 9 mm) Tip diameter: 2.5 mm (Body: 10 mm) Distance from probe tip to dipole centers: 1 mm Application: High precision dosimetric measurements in any exposure scenario (e.g., very strong
  - gradient fields). Only probe which enables compliance testing for frequencies up to 6 GHz with precision of better 30%.



## SAM Twin Phantom

## Construction:

The shell corresponds to the specifications of the Specific Anthropomorphic Mannequin (SAM) phantom defined in IEEE 1528-200X, CENELEC 50360 and IEC 62209. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents evaporation of the liquid. Reference markings on the phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points with the robot.

Shell Thickness: 2 ±0.2 mm

Filling Volume: Approx. 25 liters

Height: 850mm; Length: 1000mm; Width: Dimensions: 750mm

#### SAM Phantom (ELI4 v4.0) **Description Construction:**

Phantom for compliance testing of handheld and bodymounted wireless devices in the frequency range of 30 MHz to 6 GHz. ELI4 is fully compatible with the latest draft of the standard IEC 62209 Part II and all known tissue simulating liquids. ELI4 has been optimized regarding its performance and can be integrated into our standard phantom tables. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points. The phantom is supported by software version DASY4/DASY5.5 and higher and is compatible with all SPEAG dosimetric probes and dipoles

Shell Thickness: Filling Volume: Dimensions: Minor axis:

 $2.0 \pm 0.2$  mm (sagging: <1%) Approx. 25 liters Major ellipse axis: 600 mm 400 mm 500mm



Page 10 of 126

Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W

## Device Holder for SAM Twin Phantom

Construction: In combination with the Twin SAM Phantom, the Mounting Device (made from POM) enables the rotation of the mounted transmitter in spherical coordinates, whereby the rotation point is the ear opening. The devices can be easily and accurately positioned according to IEC, IEEE, CENELEC, FCC or other specifications. The device holder can be locked at different phantom locations (left head, right head, and flat phantom).



## System Validation Kits for SAM Twin Phantom

**Construction:** Symmetrical dipole with I/4 balun Enables measurement of feedpoint impedance with NWA Matched for use near flat phantoms filled with brain simulating solutions Includes distance holder and tripod adaptor.

900,1800,2450,5800 MHz Frequency:

ReTune loss: > 20 dB at specified validation position

**Power capability:** > 100 W (f < 1 GHz); > 40 W (f > 1 GHz)

## Dimensions:

D835V2: dipole length: 161 mm; overall height: 340 mm D1800V2: dipole length: 72.5 mm; overall height: 300 mm D1900V2: dipole length: 67.7 mm; overall height: 300 mm D2450V2: dipole length: 51.5 mm; overall height: 290 mm D5GHzV2: dipole length: 20.6 mm; overall height: 300mm



## System Validation Kits for ELI4 phantom

Construction: Symmetrical dipole with I/4 balun Enables measurement of feedpoint impedance with NWA Matched for use near flat phantoms filled with brain simulating solutions Includes distance holder and tripod adaptor.

Frequency: 900, 1800, 2450, 5800 MHz

ReTune loss: > 20 dB at specified validation position

**Power capability:** > 100 W (f < 1 GHz); > 40 W (f > 1 GHz)

Dimensions:

D835V2: dipole length: 161 mm; overall height: 340 mm D1800V2: dipole length: 72.5 mm; overall height: 300 mm D1900V2: dipole length: 67.7 mm; overall height: 300 mm D2450V2: dipole length: 51.5 mm; overall height: 290 mm D5GHzV2: dipole length: 20.6 mm; overall height: 300 mm



## 7. EVALUATION PROCEDURES

## **DATA EVALUATION**

The DASY 5 post processing software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters:	- Sensitivity	Norm <sub>i</sub> , $a_{i0}$ , $a_{i1}$ , $a_{i2}$
	- Conversion factor	ConvF <sub>i</sub>
	- Diode compression point	dcpi
Device parameters:	- Frequency	f
	- Crest factor	cf
Media parameters:	- Conductivity	σ
	- Density	ρ

These parameters must be set correctly in the software. They can be found in the component documents or be imported into the software from the configuration files issued for the DASY 5 components. In the direct measuring mode of the multi-meter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with  $V_i$ 

= Compensated signal of channel i(i = x, y, z)= Input signal of channel i = Crest factor of exciting field

(i = x, y, z)(DASY 5 parameter) (DASY 5 parameter)

 $dcp_i$  = Diode compression point

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes:

Ui

cf

$$E_i = \sqrt{\frac{V_i}{Norm_i \bullet ConvF}}$$

H-field probes:

$$H_i = \sqrt{Vi} \cdot \frac{a_{i10} + a_{i11}f + a_{i12}f}{f}$$

with  $V_i$ = Compensated signal of channel i(i = x, y, z)

*Norm*<sub>i</sub> = Sensor sensitivity of channel i (i = x, y, z)

 $\mu$ V/(V/m)<sup>2</sup> for E0field Probes

ConvF

= Sensitivity enhancement in solution

- = Sensor sensitivity factors for H-field probes aii
- = Carrier frequency (GHz) f
- Ei = Electric field strength of channel i in V/m
- Hi = Magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

 $E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$ 

Page 12 of 126

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with SAR = local specific absorption rate in mW/g

 $E_{tot}$  = total field strength in V/m

= conductivity in [mho/m] or [Siemens/m] σ

= equivalent tissue density in  $g/cm^3$ ρ

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid.

The power flow density is calculated assuming the excitation field as a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$
 or  $P_{pwe} = H_{tot}^2 \cdot 37.7$ 

with  $P_{pwe}$  = Equivalent power density of a plane wave in mW/cm<sup>2</sup>

= total electric field strength in V/m  $E_{tot}$ 

= total magnetic field strength in A/m H<sub>tot</sub>

## SAR EVALUATION PROCEDURES

The procedure for assessing the peak spatial-average SAR value consists of the following steps:

#### **Power Reference Measurement**

The reference and drift jobs are useful jobs for monitoring the power drift of the device under test in the batch process. Both jobs measure the field at a specified reference position, at a selectable distance from the phantom surface. The reference position can be either the selected section's grid reference point or a user point in this section. The reference job projects the selected point onto the phantom surface, orients the probe perpendicularly to the surface, and approaches the surface using the selected detection method.

### Area Scan

The area scan is used as a fast scan in two dimensions to find the area of high field values, before doing a finer measurement around the hot spot. The sophisticated interpolation routines implemented in DASY 5 software can find the maximum locations even in relatively coarse grids. The scan area is defined by an editable grid. This grid is anchored at the grid reference point of the selected section in the phantom. When the area scan's property sheet is brought-up, grid was at to 15 mm by 15 mm and can be edited by a user.

### Zoom Scan

Zoom scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The default zoom scan measures 5 x 5 x 7 points within a cube whose base faces are centered around the maximum found in a preceding area scan job within the same procedure. If the preceding Area Scan job indicates more then one maximum, the number of Zoom Scans has to be enlarged accordingly (The default number inserted is 1).

### Power Drift measurement

The drift job measures the field at the same location as the most recent reference job within the same procedure, and with the same settings. The drift measurement gives the field difference in dB from the reading conducted within the last reference measurement. Several drift measurements are possible for one reference measurement. This allows a user to monitor the power drift of the device under test within a batch process. In the properties of the Drift job, the user can specify a limit for the drift and have DASY 5 software stop the measurements if this limit is exceeded.

## Z-Scan

The Z Scan job measures points along a vertical straight line. The line runs along the Z-axis of a one-dimensional grid. A user can anchor the grid to the current probe location. As with any other grids, the local Z-axis of the anchor location establishes the Z-axis of the grid.

## SPATIAL PEAK SAR EVALUATION

Report No: C141229S01-SF

The procedure for spatial peak SAR evaluation has been implemented according to the IEEE1529 standard. It can be conducted for 1 g and 10 g.

The DASY 5 system allows evaluations that combine measured data and robot positions, such as:

- maximum search
- extrapolation
- boundary correction
- peak search for averaged SAR

During a maximum search, global and local maximum searches are automatically performed in 2-D after each Area Scan measurement with at least 6 measurement points. It is based on the evaluation of the local SAR gradient calculated by the Quadratic Shepard's method. The algorithm will find the global maximum and all local maxima within -2 dB of the global maxima for all SAR distributions.

## Extrapolation

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. Several measurements at different distances are necessary for the extrapolation.

Extrapolation routines require at least 10 measurement points in 3-D space. They are used in the Cube Scan to obtain SAR values between the lowest measurement points and the inner phantom surface. The routine uses the modified Quadratic Shepard's method for extrapolation. For a grid using 5x5x7 measurement points with 5mm resolution amounting to 343 measurement points, the uncertainty of the extrapolation routines is less than 1% for 1 g and 10 g cubes.

### **Boundary effect**

For measurements in the immediate vicinity of a phantom surface, the field coupling effects between the probe and the boundary influence the probe characteristics. Boundary effect errors of different dosimetric probe types have been analyzed by measurements and using a numerical probe model. As expected, both methods showed an enhanced sensitivity in the immediate vicinity of the boundary. The effect strongly depends on the probe dimensions and disappears with increasing distance from the boundary. The sensitivity can be approximately given as:

$$S \approx S_o + S_b exp(-\frac{z}{a})cos(\pi \frac{z}{\lambda})$$

Since the decay of the boundary effect dominates for small probes ( $a <<\lambda$ ), the cos-term can be omitted. Factors *Sb* (parameter Alpha in the DASY 5 software) and *a* (parameter Delta in the DASY 5 software) are assessed during probe calibration and used for numerical compensation of the boundary effect. Several simulations and measurements have confirmed that the compensation is valid for different field and boundary configurations.

This simple compensation procedure can largely reduce the probe uncertainty near boundaries. It works well as long as:

- the boundary curvature is small
- the probe axis is angled less than 30\_ to the boundary normal
- the distance between probe and boundary is larger than 25% of the probe diameter
- the probe is symmetric (all sensors have the same offset from the probe tip)

Since all of these requirements are fulfilled in a DASY 5 system, the correction of the probe boundary effect in the vicinity of the phantom surface is performed in a fully automated manner via the measurement data extraction during post processing.

Page 15 of 126

# ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue :January 26, 2015

## 8. MEASUREMENT UNCERTAINTY

Measurement uncertainty for 30 MHz to 3 GHz averaged over 1 gram						
Uncertainty Component	Uncertainty	Prob.	Div.	<b>C</b> <sub>i (1g)</sub>	Std. Unc.(1-g)	Vi or Veff
Measurement System						
Probe Calibration ( <i>k</i> =1)	6.00	Normal	1	1	6.00	8
Probe Isotropy	4.70	Rectangular	√3	0.7	1.90	8
Modulation Response	2.40	Rectangular	√3	1	1.39	∞
Hemispherical Isotropy	9.60	Rectangular	√3	0.7	3.88	∞
Boundary Effect	2.00	Rectangular	√3	1	1.15	∞
Linearity	4.70	Rectangular	√3	1	2.71	∞
System Detection Limit	1.00	Rectangular	√3	1	0.58	∞
Readout Electronics	0.30	Normal	1	1	0.30	∞
Response Time	0.80	Rectangular	√3	1	0.46	∞
Integration Time	2.60	Rectangular	√3	1	1.50	∞
RF Ambient Noise	3.00	Rectangular	√3	1	1.73	∞
RF Ambient Reflections	3.00	Rectangular	√3	1	1.73	∞
Probe Positioner	0.40	Rectangular	√3	1	0.23	∞
Probe Positioning	2.90	Rectangular	√3	1	1.67	∞
Max. SAR Evaluation	2.00	Rectangular	√3	1	1.15	∞
Test sample Related						
Test sample Positioning	2.9	Normal	1	1	2.9	145
Device Holder Uncertainty	3.6	Normal	1	1	3.6	5
Power drift	5	Rectangular	√3	1	2.89	∞
Power Scaling	0	Rectangular	√3	1	0.00	∞
Phantom and Tissue Parameters						
Phantom Uncertainty	6.1	Rectangular	√3	1	3.52	∞
SAR correction	1.9	Rectangular	√3	1	1.10	∞
Liquid Conductivity (target)	5	Rectangular	√3	0.64	1.85	∞
Liquid Conductivity (meas)	3.42	Rectangular	√3	0.78	1.54	∞
Liquid Permittivity (target)	5	Rectangular	√3	0.6	1.73	∞
Liquid Permittivity (meas)	-3.18	Rectangular	√3	0.26	-0.48	∞
Temp. unc Conductivity	3.4	Rectangular	√3	0.78	1.53	∞
Temp. unc Permittivity	0.4	Rectangular	√3	0.23	0.05	∞
Combined Std. Uncertainty		RSS			11.53	361
Expanded STD Uncertainty		<i>k</i> =2			23.07	'%
Expanded STD Uncertainty		<i>k</i> =2			1.800	B

Table: Worst-case uncertainty for DASY5 assessed according to IEEE1528-2003.

The budge is valid for the frequency range 30 MHz to 3G Hz and represents a worst-case analysis.

## 9. EXPOSURE LIMIT

(A). Limits for Occupational/Controlled Exposure (W/kg)

Whole-Body	Partial-Body	Hands, Wrists, Feet and Ankles
0.4	8.0	20.0

(B). Limits for General Population/Uncontrolled Exposure (W/kg)

Whole-Body	Partial-Body	Hands, Wrists, Feet and Ankles
0.08	1.6	4.0

Note: Whole-Body SAR is averaged over the entire body, partial-body SAR is averaged over any 1 gram of tissue defined as a tissue volume in the shape of a cube. SAR for hands, wrists, feet and ankles is averaged over any 10 grams of tissue defined as a tissue volume in the shape of a cube.

Population/Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure.

Occupational/Controlled Environments are defined as locations where there is exposure that may be incurred by people who are aware of the potential for exposure, (i.e. as a result of employment or occupation).

NOTE					
GENERAL POPULATION/UNCONTROLLED EXPOSURE					
PARTIAL BODY LIMIT					
1.6 W/kg					

Date of Issue : January 26, 2015

#### EUT ARRANGEMENT 10.

Please refer to IEEE1528-2003 illustration below.

## 10.1 ANTHROPOMORPHIC HEAD PHANTOM

Figure 7-1a shows the front, back and side views of SAM. The point "M" is the reference point for the center of mouth, "LE" is the left ear reference point (ERP), and "RE" is the right ERP. The ERPs are 15 mm posterior to the entrance to ear canal (EEC) along the B-M line (Back-Mouth), as shown in Figure 7-1b. The plane passing through the two ear reference points and M is defined as the Reference Plane. The line N-F (Neck-Front) perpendicular to the reference plane and passing through the RE (or LE) is called the Reference Pivoting Line (see Figure 7-1c). Line B-M is perpendicular to the N-F line. Both N-F and B-M lines should be marked on the external phantom shell to facilitate handset positioning. Posterior to the N-F line, the thickness of the phantom shell with the shape of an ear is a flat surface 6 mm thick at the ERPs. Anterior to the N-F line, the ear is truncated as illustrated in Figure 7-1b. The ear truncation is introduced to avoid the handset from touching the ear lobe, which can cause unstable handset positioning at the cheek.

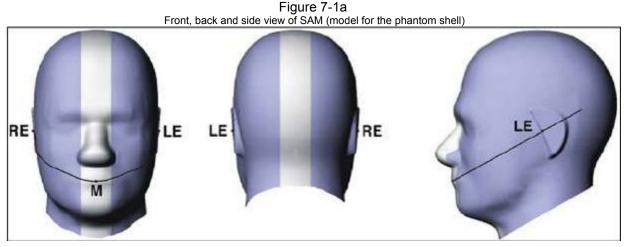


Figure 7-1b Close up side view of phantom showing the ear region






Figure 7-1b Close up side view of phantom showing the ear region

Figure 7-1c Side view of the phantom showing relevant markings and the 7 cross sectional plane locations





## 10.2 DEFINITION OF THE "CHEEK/TOUCH" POSITION

The "cheek" or "touch" position is defined as follows:

- a. Ready the handset for talk operation, if necessary. For example, for handsets with a cover piece, open the cover. (If the handset can also be used with the cover closed both configurations must be tested.)
- b. Define two imaginary lines on the handset: the vertical centerline and the horizontal line. The vertical centerline passes through two points on the front side of the handset: the midpoint of the width wt of the handset at the level of the acoustic output (point A on Figures 7-2a and 7-2b), and the midpoint of the width wb of the bottom of the handset (point B). The horizontal line is perpendicular to the vertical centerline and passes through the center of the acoustic output (see Figure 7-2a). The two lines intersect at point A. Note that for many handsets, point A coincides with the center of the acoustic output. However, the acoustic output may be located elsewhere on the horizontal line. Also note that the vertical centerline is not necessarily parallel to the front face of the handset (see Figure 7-2b), especially for clamshell handsets, handsets with flip pieces, and other irregularly-shaped handsets.
- c. Position the handset close to the surface of the phantom such that point A is on the (virtual) extension of the line passing through points RE and LE on the phantom (see Figure 7-2c), such that the plane defined by the vertical center line and the horizontal line of the handset is approximately parallel to the sagittal plane of the phantom.
- d. Translate the handset towards the phantom along the line passing through RE and LE until the handset touches the pinna.
- e. e) While maintaining the handset in this plane, rotate it around the LE-RE line until the vertical centerline is in the plane normal to MB-NF including the line MB (called the reference plane).
- f. Rotate the handset around the vertical centerline until the handset (horizontal line) is symmetrical with respect to the line NF.
- g. While maintaining the vertical centerline in the reference plane, keeping point A on the line passing through RE and LE and maintaining the handset contact with the pinna, rotate the handset about the line NF until any point on the handset is in contact with a phantom point below the pinna (cheek). See Figure 7-2c. The physical angles of rotation should be noted.


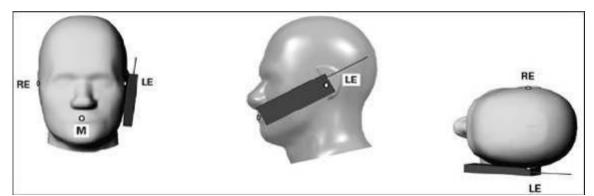


Figure 7.2c

Phone "cheek" or "touch" position. The reference points for the right ear (RE), left ear (LE) and mouth (M), which define the reference plane for handset positioning, are indicated.

Compliance Certification Services Inc.

Date of Issue :January 26, 2015

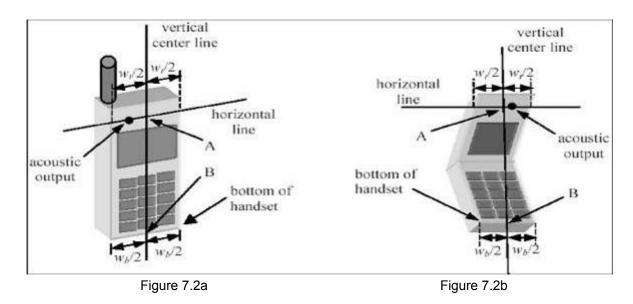


FCC ID: 2ABOSSKY55W

## **10.3 DEFINITION OF THE "TILTED" POSITION**

The "tilted" position is defined as follows:

Report No: C141229S01-SF

- a. Repeat steps (a) (g) of 7.2 to place the device in the "cheek position."
- b. While maintaining the orientation of the handset move the handset away from the pinna along the line passing through RE and LE in order to enable a rotation of the handset by 15 degrees.
- c. Rotate the handset around the horizontal line by 15 degrees.
- d. While maintaining the orientation of the handset, move the handset towards the phantom on a line passing through RE and LE until any part of the handset touches the ear. The tilted position is obtained when the contact is on the pinna. If the contact is at any location other than the pinna (e.g., the antenna with the back of the phantom head), the angle of the handset should be reduced. In this case, the tilted position is obtained if any part of the handset is in contact with the pinna as well as a second part of the handset is contact with the phantom (e.g., the antenna with the back of the handset is contact with the phantom (e.g., the antenna with the back of the handset is contact with the phantom (e.g., the antenna with the back of the handset is contact with the phantom (e.g., the antenna with the back of the handset is contact with the phantom (e.g., the antenna with the back of the head).

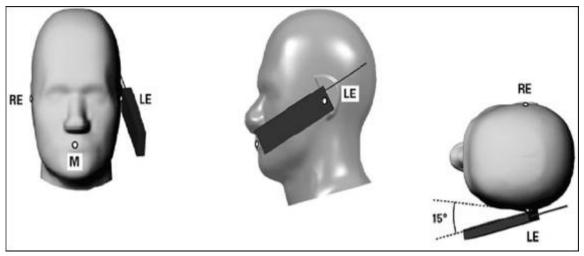

## Figure 7-3

Phone "tilted" position. The reference points for the right ear (RE), left ear (LE) and mouth (M), which define the reference plane for handset positioning, are indicated.

#### **MEASUREMENT RESULTS** 11.

#### 11.1 **TEST LIQUIDS CONFIRMATION**

## SIMULATED TISSUE LIQUID PARAMETER CONFIRMATION

The dielectric parameters were checked prior to assessment using the HP85070C dielectric probe kit. The dielectric parameters measured are reported in each correspondent section.

## **KDB865664 D01 RECOMMENDED TISSUE DIELECTRIC PARAMETERS**

The head and Body tissue dielectric parameters recommended by the KDB865664 D01 have been incorporated in the following table.

Target Frequency	Не	ad	Body		
(MHz)	ε <sub>r</sub>	σ (S/m)	ε <sub>r</sub>	σ (S/m)	
150	52.3	0.76	61.9	0.80	
300	45.3	0.87	58.2	0.92	
450	43.5	0.87	56.7	0.94	
835	41.5	0.90	55.2	0.97	
900	41.5	0.97	55.0	1.05	
915	41.5	0.98	55.0	1.06	
1450	40.5	1.20	54.0	1.30	
1610	40.3	1.29	53.8	1.40	
1800-2000	40.0	1.40	53.3	1.52	
2450	39.2	1.80	52.7	1.95	
3000	38.5	2.40	52.0	2.73	
5800	35.3	5.27	48.2	6.00	

( $\varepsilon_r$  = relative permittivity,  $\sigma$  = conductivity and  $\rho$  = 1000 kg/m<sup>3</sup>)

## 11.2 LIQUID MEASUREMENT RESULTS

## The following table show the measuring results for simulating liquid:


Liquid Type	Liquid Temp. (°C)	Parameters	Target	Measured	Deviation (%)	Limited (%)	Measured Date	
Head835	21.5	Permitivity(ε )	41.50	40.846	-1.58	± 5	2015-1-6	
Heau035	21.5	Conductivity(o)	0.90	0.911	1.22	± 5	2015-1-0	
Body835	21.5	Permitivity(ε )	55.20	53.445	-3.18	± 5	2015-1-8	
Douyoss	21.5	Conductivity(σ)	0.97	0.978	0.82	± 5	2013-1-0	
Head1800	21.5	Permitivity(ε )	40.00	40.015	0.04	± 5	2015-1-6	
Tieau 1000	21.5	Conductivity(σ)	1.40	1.439	2.79	± 5	2013-1-0	
Body1800	21.5	Permitivity(ε)	53.30	54.172	1.64	± 5	2015-1-7	
Body 1800	21.5	Conductivity(σ)	1.52	1.572	3.42	± 5	2015-1-7	
Head1900	21.5	Permitivity(ε )	40.00	39.062	-2.35	± 5	2015 1 6	
Tieau 1900	21.5	Conductivity(σ)	1.40	1.431	2.21	± 5	2015-1-6	
Body1900	21.5	Permitivity(ε )	53.30	54.749	2.72	± 5	2015-1-7	
Dody1900	21.5	Conductivity(σ)	1.52	1.571	3.36	± 5	2013-1-7	
Head2450	21.5	Permitivity(ε )	39.20	39.128	-0.18	± 5	2015-1-5	
116402450	21.0	Conductivity(σ)	1.80	1.832	1.78	± 5	2013-1-5	
Body2450	21.5	Permitivity(ɛ)	52.70	51.708	-1.88	± 5	2015-1-5	
B00y2430	21.0	Conductivity( $\sigma$ )	1.95	1.978	1.44	± 5	2010-1-0	

#### SYSTEM PERFORMANCE CHECK 11.3

The system performance check is performed prior to any usage of the system in order to guarantee reproducible results. The system performance check verifies that the system operates within its specifications of ±10%. The system performance check results are tabulated below. And also the corresponding SAR plot is attached as well in the SAR plots files.

## SYSTEM PERFORMANCE CHECK MEASUREMENT CONDITIONS

- The measurements were performed in the flat section of the SAM twin phantom filled with head • and body simulating liquid of the following parameters.
- The DASY5 system withan E-fileld probe EX3DV4 SN: 3798 was used for the measurements. .
- The dipole was mounted on the small tripod so that the dipole feed point was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15 mm (below 1 GHz) and 10 mm (above 1 GHz) from dipole center to the simulating liquid surface.
- The coarse grid with a grid spacing of 10mm was aligned with the dipole.
- Special 7x7x7 fine cube was chosen for cube integration (dx= 5 mm, dy= 5 mm, dz= 5 mm). •
- Distance between probe sensors and phantom surface was set to 2 mm. .
- The dipole input power was 250mW±3%.
- The results are normalized to 1 W input power.

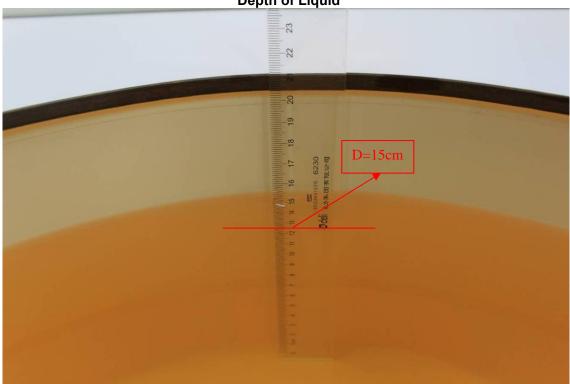

Note: For SAR testing, the depth is 15cm shown above

## **Depth of Liquid**

## SYSTEM PERFORMANCE CHECK RESULTS

Liquid Type	Ambient Temp. (° C)	Liquid Temp. (°C)	Input Power (W)	Measured SAR1g (W/Kg)	1W Target SAR¹g(W/Kg)	1W Normalized SAR1g(W/Kg)	Deviation (%)	Limited (%)	Date
Head835	22	21.5	0.25	2.21	9.50	8.84	-6.95	± 10	2015-1-6
Body835	22	21.5	0.25	2.43	9.53	9.72	1.99	± 10	2015-1-8
Head1800	22	21.5	0.25	9.86	38.60	39.44	2.18	± 10	2015-1-6
Body1800	22	21.5	0.25	9.75	39.30	39.00	-0.76	± 10	2015-1-7
Head1900	22	21.5	0.25	9.92	40.40	39.68	-1.78	± 10	2015-1-6
Body1900	22	21.5	0.25	10.80	40.50	43.20	6.67	± 10	2015-1-7
Head2450	22	21.5	0.25	13.40	52.60	53.60	1.90	± 10	2015-1-5
Body2450	22	21.5	0.25	12.90	49.20	51.60	4.88	± 10	2015-1-5

Date of Issue : January 26, 2015

## **11.4 EUT TUNE-UP PROCEDURES AND TEST MODE**

The following procedure had been used to prepare the EUT for the SAR test.

To setup the desire channel frequency and the maximum output power. A Radio Communication Tester "CMU200" was used to program the EUT.

#### **General Note:**

- 1. Per KDB 447498 D01v05r02, the maximum output power channel is used for SAR testing and for further SAR test reduction.
- 2. For head SAR testing, the EUT was set in GSM Voice for GSM850 and PCS1900 due to its highest frame-average power.
- 3. For body worn SAR testing, the EUT was set in GPRS 4 Tx slots for GSM850 and GPRS 4 Tx PCS1900 due to its highest frame-average power.

### GSM Conducted output power(dBm):

Band		GSM 850			GSM 1900	1			
Channel	128	190	251	512	661	810			
Frequency(MHz)	824.2	836.6	848.8	1850.2	1880.0	1909.8			
Maximum Burst-Averaged Output Power									
GSM(GMSK,1Uplink)	32.65	32.65	32.74	29.11	29.35	29.39			
GPRS 8 (GMSK,1 Uplink)	32.67	32.67	32.76	29.29	29.13	28.77			
GPRS 10 (GMSK,2 Uplink)	31.76	31.77	31.88	28.40	28.24	27.90			
GPRS 11 (GMSK,3 Uplink)	30.07	30.08	30.20	26.58	26.72	26.73			
GPRS 12 (GMSK,4 Uplink)	29.27	29.26	29.43	25.84	25.95	25.97			
EDGE 8 (GMSK,1 Uplink)	32.64	32.63	32.75	29.26	29.11	28.75			
EDGE 10 (GMSK,2 Uplink)	31.73	31.75	31.85	28.38	28.21	27.87			
EDGE 11 (GMSK,3 Uplink)	30.04	30.05	30.17	26.55	26.69	26.71			
EDGE 12 (GMSK,4 Uplink)	29.25	29.24	29.41	25.81	25.92	25.95			
EDGE 8 (8PSK,1 Uplink)	27.75	27.73	27.85	26.23	25.99	25.76			
EDGE 10 (8PSK,2 Uplink)	26.59	26.59	26.67	25.44	25.18	24.85			
EDGE 11 (8PSK,3 Uplink)	24.62	24.45	24.49	23.42	23.02	22.71			
EDGE 12 (8PSK,4 Uplink)	23.05	23.08	23.23	22.00	21.66	21.47			
Maxin	num Frame	e-Averageo	d Output P	ower					
GSM(GMSK,1Uplink)	23.63	23.63	23.72	20.09	20.33	20.37			
GPRS 8 (GMSK,1 Uplink)	23.64	23.64	23.73	20.26	20.10	19.74			
GPRS 10 (GMSK,2 Uplink)	25.73	25.74	25.85	22.37	22.21	21.87			
GPRS 11 (GMSK,3 Uplink)	25.81	25.82	25.94	22.32	22.46	22.47			
GPRS 12 (GMSK,4 Uplink)	26.26	26.25	26.42	22.83	22.94	22.96			
EDGE 8 (GMSK,1 Uplink)	23.61	23.60	23.72	20.23	20.08	19.72			
EDGE 10 (GMSK,2 Uplink)	25.71	25.73	25.83	22.36	22.19	21.85			
EDGE 11 (GMSK,3 Uplink)	25.78	25.79	25.91	22.29	22.43	22.45			
EDGE 12 (GMSK,4 Uplink)	26.24	26.23	26.40	22.80	22.91	22.94			
EDGE 8 (8PSK,1 Uplink)	18.72	18.70	18.82	17.20	16.96	16.73			
EDGE 10 (8PSK,2 Uplink)	20.57	20.57	20.65	19.42	19.16	18.83			
EDGE 11 (8PSK,3 Uplink)	20.36	20.19	20.23	19.16	18.76	18.45			
EDGE 12 (8PSK,4 Uplink)	20.04	20.07	20.22	18.99	18.65	18.46			

<sup>4.</sup> For hotspot SAR testing, the EUT was set in GPRS 4 Tx slots for GSM850 and GPRS 4 Tx PCS1900 due to its highest frame-average power.

Compliance Certification Services Inc. Report No: C141229S01-SF FCC ID: 2ABOSSKY55W Date of Issue :Ja

Date of Issue : January 26, 2015

**Remark:** The frame-averaged power is linearly scaled the maximum burst-averaged power based on

time slots. The calculated methods are shown as below:

Frame-averaged power = Burst-averaged power (1 Uplink) – 9.03 dBm

Frame-averaged power = Burst averaged power (2 Uplink) – 6.02 dBm

Frame-averaged power = Burst-averaged power (3 Uplink) – 4.26 dBm

Frame-averaged power = Burst averaged power (4 Uplink) – 3.01 dBm

**Note:** Per KDB 447498 D01v05r02, the maximum output power channel is used for SAR testing and for further SAR test reduction.

## WCDMA Conducted output power(dBm):

As the SAR body tests for WCDMA Band II, Band IV and Band V, we established the radio link through call processing. The maximum output power were verified on high, middle and low channels for each test band according to 3GPP TS 34.121 with the following configuration:a 12.2kbps RMC, 64,144,384 kbps RMC with TPC set to all "all '1's"b Test loop Mode 1 The following procedures had been used to prepare the EUT for the SAR test.

## **HSDPA Setup Configuration:**

Table C.10.1.4: β values for transmitter characteristics tests with HS-DPCCH

Sub-test	βc	βa	βd (SF)	β₀/β₫	βHS (Note1, Note 2)	CM (dB) (Note 3)	MPR (dB) (Note 3)
1	2/15	15/15	64	2/15	4/15	0.0	0.0
2	12/15	15/15	64	12/15	24/15	1.0	0.0
	(Note 4)	(Note 4)		(Note 4)			
3	15/15	8/15	64	15/8	30/15	1.5	0.5
4	15/15	4/15	64	15/4	30/15	1.5	0.5
	discontinuity with $\beta_{bc} = 2$		13.1AA, Δack	and $\Delta_{NACK} = 30/1$	5 with $\beta_{hs}$ =	30/15 * $eta_c$ , and	d ∆cqi = 24/15
Note 3:	CM = 1 for $\beta$ DPCCH the	_/β <sub>d</sub> =12/15, MPR is base		. For all other con ative CM differenc r releases.			
Note 4:	For subtest 2	2 the β₀/β₀ ra	atio of 12/15 f	or the TFC during factors for the re			

## **HSUPA Setup Configuration:**

Table C.11.1.3: β values for transmitter characteristics tests with HS-DPCCH and E-DCH

Sub- test	βc	βa	βd (SF)	βc/βd	<mark>βнs</mark> (Note1)	β <sub>ec</sub>	β <sub>ed</sub> (Note 5) (Note 6)	β <sub>ed</sub> (SF)	β <sub>ed</sub> (Codes)	CM (dB) (Note 2)	MPR (dB) (Note 2)	AG Index (Note 6)	E- TFCI
1	11/15 (Note 3)	15/15 (Note 3)	64	11/15 (Note 3)	22/15	209/2 25	1309/225	4	1	1.0	0.0	20	75
2	6/15	15/15	64	6/15	12/15	12/15	94/75	4	1	3.0	2.0	12	67
3	15/15	9/15	64	15/9	30/15	30/15	β <sub>ed</sub> 1: 47/15 β <sub>ed</sub> 2: 47/15	4 4	2	2.0	1.0	15	92
4	2/15	15/15	64	2/15	4/15	2/15	56/75	4	1	3.0	2.0	17	71
5	15/15 (Note 4)	15/15 (Note 4)	64	15/15 (Note 4)	30/15	24/15	134/15	4	1	1.0	0.0	21	81
Note 1	: Даск, 4	ANACK and	d Δ <sub>CQI</sub> =	= 30/15 w	vith $\beta_{\scriptscriptstyle hs}$	= 30/15 *	$\beta_c$ .						
Note 2							ner combinatio CM difference		DPDCH, [	OPCCH,	HS- DPC	CCH, E-D	PDCH
Note 3							during the mo TFC (TF1, T				· · · ·		by
Note 4	Note 4: For subtest 5 the $\beta_c/\beta_d$ ratio of 15/15 for the TFC during the measurement period (TF1, TF0) is achieved by setting the signalled gain factors for the reference TFC (TF1, TF1) to $\beta_c = 14/15$ and $\beta_d = 15/15$ .												
Note 5: In case of testing by UE using E-DPDCH Physical Layer category 1, Sub-test 3 is omitted according to TS25.306 Table 5.1g.													
			_			bsolute C							

# ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue :January 26, 2015

Band	W	CDMA Band	ll k	W	CDMA Band	IV
Channel	9262	9400	9538	1312	1413	1513
Frequency(MHz)	1852.4	1880	1907.6	1712.4	1732.6	1752.6
RMC12.2K	21.58	21.84	21.83	20.59	20.05	20.28
HSDPA Subtest-1	20.58	20.84	20.87	20.08	19.58	19.78
HSDPA Subtest-2	20.32	20.65	20.68	19.98	19.23	19.38
HSDPA Subtest-3	20.25	20.47	20.52	19.85	19.09	19.15
HSDPA Subtest-4	20.44	20.72	20.76	20.02	19.47	19.71
HSUPA Subtest-1	20.58	20.87	20.92	20.10	19.73	19.92
HSUPA Subtest-2	20.52	20.81	20.93	20.03	19.28	19.45
HSUPA Subtest-3	20.43	20.66	20.85	19.96	19.29	19.35
HSUPA Subtest-4	20.29	20.44	20.58	20.21	20.03	20.14
HSUPA Subtest-5	20.45	20.61	20.76	20.08	19.96	20.01

Band	W	CDMA Band	V I
Channel	4132	4182	4233
Frequency(MHz)	826.4	836.4	846.6
RMC12.2K	22.43	22.47	22.19
HSDPA Subtest-1	21.36	21.30	21.16
HSDPA Subtest-2	21.53	21.69	21.46
HSDPA Subtest-3	21.65	21.71	21.47
HSDPA Subtest-4	21.52	21.75	21.61
HSUPA Subtest-1	21.46	21.50	21.22
HSUPA Subtest-2	21.56	21.78	20.43
HSUPA Subtest-3	21.62	21.83	21.35
HSUPA Subtest-4	21.53	21.72	21.25
HSUPA Subtest-5	21.82	21.89	21.66

Note:

Per KDB 941225 D01, RMC 12.2kbps setting is used to evaluate SAR. If HSDPA/HSUPA output power is < 0.25dB higher than RMC, HSDPA/HSUPA SAR evaluation can be excluded.

## WLAN 2.4G Conducted output power(dBm):

Mode	Channel	Frequence	Average power(dBm)
	1	2412 MHZ	14.92
802.11 b	6	2437 MHZ	14.81
	11	2462 MHZ	14.74
	1	2412 MHZ	13.97
802.11 g	6	2437 MHZ	14.02
	11	2462 MHZ	14.33
000.44 -	1	2412 MHZ	13.56
802.11 n 20M	6	2437 MHZ	13.73
20101	11	2462 MHZ	13.86
000.44	3	2422 MHZ	11.68
802.11 n 40M	7	2442 MHZ	12.51
10101	11	2462 MHZ	12.56

### Bluetooth 3.0 Conducted output power(dBm):

		Average power(dBm)					
Channel	Frequency						
		1Mbps	3Mbps				
CH00	2402MHZ	5.42	4.57	4.79			
CH39	2441MHZ	5.93	5.19	5.36			
CH78	2480MHZ	6.01	5.30	5.48			

## BLE 4.0 Conducted output power(dBm):

Channel	Frequency	Average power(dBm)
Channel	Frequency	Date Rate(1Mbps)
CH00	2402MHZ	-1.90
CH19	2440MHZ	-1.19
CH39	2480MHZ	-1.04

According to KDB447498 D01: The 1-g and 10-g SAR test exclusion thresholds for 100 MHz to 6 GHz at test separation distances  $\leq$  50 mm are determined by:

[(max. power of channel, including tune-up tolerance, mW)/(min. test separation distance,

*mm*)]  $\cdot \left[\sqrt{f_{(GHz)}}\right] \le 3.0$  for 1-g SAR and  $\le 7.5$  for 10-g extremity SAR,24 where

- f(GHz) is the RF channel transmit frequency in GHz
- Power and distance are rounded to the nearest mW and mm before calculation25
- The result is rounded to one decimal place for comparison
- 3.0 and 7.5 are referred to as the numeric thresholds in the step 2 below
- · If the test separation distance (antenna-user) is < 5mm, 5mm is used for excluded SAR calculation

	Wireless Interface	Bluetooth
Ti	une-up Maximum power (dBm)	7
Tun	e-up Maximum rated power (mW)	5.012
	Antenna to user (mm)	5
Head	Frequency(GHz)	2.480
	SAR exclusion threshold	1.579
	Antenna to user (mm)	10
Body	Frequency(GHz)	2.480
	SAR exclusion threshold	0.789

Per KDB 447498 D01v05r02 exclusion thresholds is[(max. power of channel, including tune-up tolerance: 5.012 mW)/(min. test separation distance: 5mm)] · [ $\sqrt{2.480}$ ] =1.579< 3, Bluetooth RF exposure evaluation is not required.

# ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue : January 26, 2015

Mode	The Tune-up Maximum Power(Customer Declared)(dBm)	Range	Measured Conduct Maximum Power(dBm)
GSM 850	32+/-1	31~33	32.74
GPRS(GMSK) 850-1TS	32+/-1	31~33	32.76
GPRS(GMSK) 850-2TS	31+/-1	30~32	31.88
GPRS(GMSK) 850-3TS	30+/-1	29~31	30.20
GPRS(GMSK) 850-4TS	29+/-1	28~30	29.43
EDGE(GMSK) 850-1TS	32+/-1	31~33	32.75
EDGE(GMSK) 850-2TS	31+/-1	30~32	31.85
EDGE(GMSK) 850-3TS	30+/-1	29~31	30.17
EDGE(GMSK) 850-4TS	29+/-1	28~30	29.41
EDGE(8PSK) 850-1TS	27+/-1	26~28	27.85
EDGE(8PSK) 850-2TS	26+/-1	25~27	26.67
EDGE(8PSK) 850-3TS	24+/-1	23~25	24.62
EDGE(8PSK) 850-4TS	23+/-1	22~24	23.23
PCS 1900	29+/-1	29~30	29.39
GPRS(GMSK) 1900-1TS	29+/-1	29~30	29.29
GPRS(GMSK) 1900-2TS	28+/-1	27~29	28.40
GPRS(GMSK) 1900-3TS	26+/-1	25~27	26.73
GPRS(GMSK) 1900-4TS	26+/-1	25~27	25.97
EDGE(GMSK) 1900-1TS	29+/-1	29~30	29.26
EDGE(GMSK) 1900-2TS	28+/-1	27~29	28.38
EDGE(GMSK) 1900-3TS	26+/-1	25~27	26.71
EDGE(GMSK) 1900-4TS	26+/-1	25~27	25.95
EDGE(8PSK) 1900-1TS	26+/-1	25~27	26.23
EDGE(8PSK) 1900-2TS	25+/-1	24~26	25.44
EDGE(8PSK) 1900-3TS	23+/-1	22~24	23.42
EDGE(8PSK) 1900-4TS	22+/-1	21~23	22.00
WCDMA Band II RMC 12.2K	21 +/-1	20~22	21.84
HSDPA Band II	20 +/-1	19~21	20.87
HSUPA Band II	20 +/-1	19~21	20.93
WCDMA Band IV RMC 12.2K	20 +/-1	19~21	20.59
HSDPA Band IV	20 +/-1	19~21	20.08
HSUPA Band IV	20 +/-1	19~21	20.21
WCDMA Band V RMC 12.2K	22+/-1	21~23	22.47
HSDPA Band V	21 +/-1	20~22	21.75
HSUPA Band V	21 +/-1	20~22	21.89
IEEE 802.11b	14+/-1	13~15	14.92
IEEE 802.11g	14+/-1	13~15	14.33
IEEE 802.11n(20M)	13+/-1	12~14	13.86

Page 31 of 126

IEEE 802.11n(40M)	12+/-1	11~13	12.56
Bluetooth 1Mbps	6+/-1	5~7	6.01
Bluetooth 2Mbps	5+/-1	4~6	5.30
Bluetooth 3Mbps	5+/-1	4~6	5.48
BLE 4.0	-1+/-1	-2~0	-1.04

So, they are in tune-up range and complied.

Date of Issue :January 26, 2015

## **11.5 SAR TEST CONFIGURATIONS**

## **Body-Worn Accessory Exposure Conditions**


Report No: C141229S01-SF

Body-worn accessory exposure is typically related to voice mode operations when handsets are carried in body-worn accessories. The body-worn accessory procedures in KDB 447498 are used to test for body-worn accessory SAR compliance, without a headset connected to it. This enables the test results for such configuration to be compatible with that required for hotspot mode when the body-worn accessory test separation distance is greater than or equal to that required for hotspot mode. When the reported SAR for a body-worn accessory, measured without a headset connected to the handset, is > 1.2 W/kg, the highest reported SAR configuration for that wireless mode and frequency band should be repeated for that body-worn accessory with a headset attached to the handset.

Body-worn accessories that do not contain metallic or conductive components may be tested according to worst-case exposure configurations, typically according to the smallest test separation distance required for the group of body-worn accessories with similar operating and exposure characteristics. All body-worn accessories containing metallic components are tested in conjunction with the host device.

Body-worn accessory SAR compliance is based on a single minimum test separation distance for all wireless and operating modes applicable to each body-worn accessory used by the host, and according to the relevant voice and/or data mode transmissions and operations. If a body-worn accessory supports voice only operations in its normal and expected use conditions, testing of data mode for body-worn compliance is not required.


A conservative minimum test separation distance for supporting off-the-shelf body-worn accessories that may be acquired by users of consumer handsets is used to test for body-worn accessory SAR compliance. This distance is determined by the handset manufacturer, according to the requirements of Supplement C 01-01. Devices that are designed to operate on the body of users using lanyards and straps, or without requiring additional body-worn accessories, will be tested using a conservative minimum test separation distance <= 5 mm to support compliance.

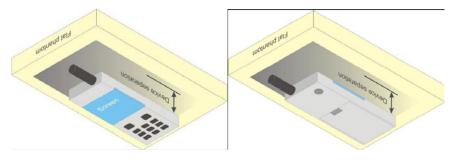


#### **Illustration for Body Worn Position**

## **Hotspot Mode Exposure conditions**

For handsets that support hotspot mode operations, with wireless router capabilities and various web browsing functions, the relevant hand and body exposure conditions are tested according to the hotspot SAR procedures in KDB 941225 D06. A test separation distance of 10 mm is required between the phantom and all surfaces and edges with a transmitting antenna located within 25 mm from that surface or edge. When the form factor of a handset is smaller than 9 cm x 5 cm, a test separation distance of 5 mm (instead of 10 mm) is required for testing hotspot mode. When the separation distance required for body-worn accessory testing is larger than or equal to that tested for hotspot mode, in the same wireless mode and for the same surface of the phone, the hotspot mode SAR data may be used to support body-worn accessory SAR compliance for that particular configuration (surface).



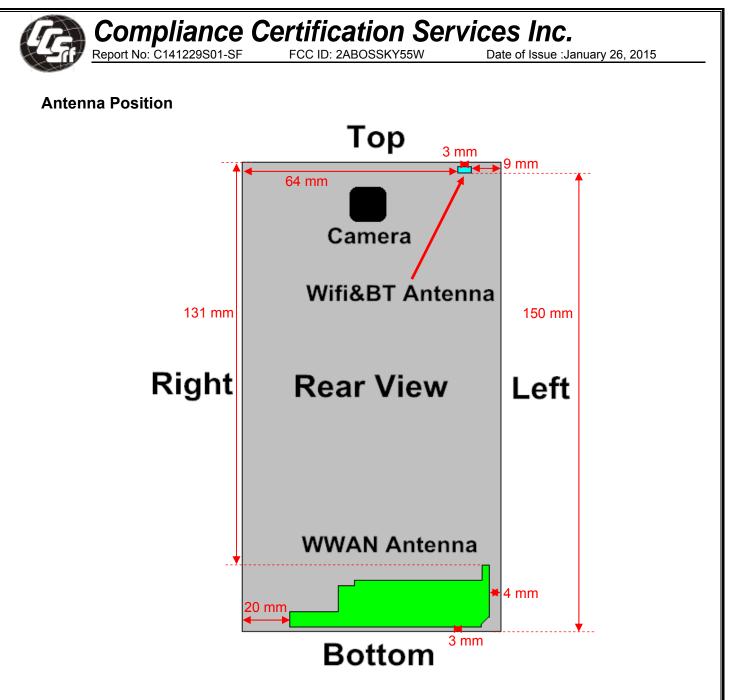

## Device dimensions (H x W): 155 x 78 mm

Antenna	Wireless Interface	
WWAN Antenna	GSM850 PCS1900 WCDMA Band II WCDMA Band IV WCDMA Band V	
Wifi&BT Antenna	WLAN 2.4G Bluetooth	

#### **Test Mode**

GSM 850/PCS1900	Data transmission mode(GPRS)/Voice mode(GSM)		
WCDMA Band II WCDMA Band IV WCDMA Band V	Data transmission mode(12.2k RMC)		
IEEE 802.11b	Data transmission mode(802.11b)		

Page 34 of 126

# ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue : January 26, 2015

## Body Exposure Condition

Distance of the Antenna to the EUT surface/edge						
Test distance: 10 mm						
Antenna	Front	Rear	Right side	Left side	Top side	Bottom side
	( <b>mm</b> )	(mm)				
WWAN	6<25	2<25	20<25	4<25	131>25	3<25
WLAN	6<25	2<25	64>25	9<25	3<25	150>25

## Body test position


Distance of the Antenna to the EUT surface/edge Test distance: 10 mm						
Antenna	Front	Rear	Right side	Left side	Top side	Bottom side
WWAN	Yes	Yes	Yes	Yes	No	Yes
WLAN	Yes	Yes	No	Yes	Yes	No

# Compliance Certification Services Inc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue :January 26, 2015


## **11.6 EUT SETUP PHOTOS**

## Head position

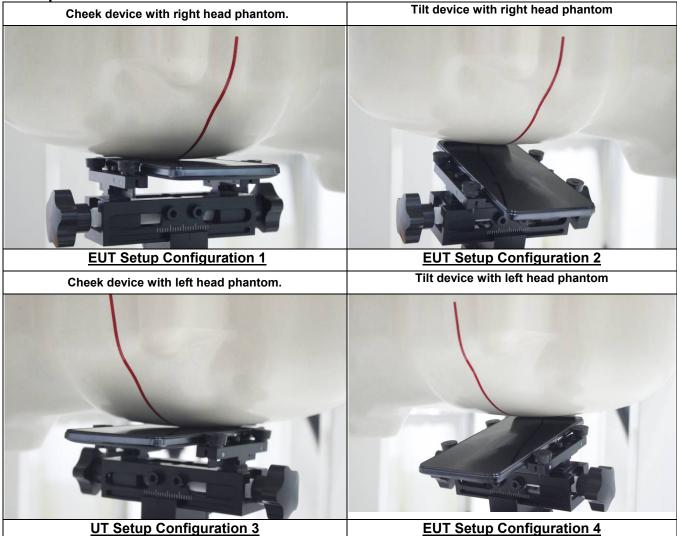

Date of Issue :January 26, 2015

## Body positon

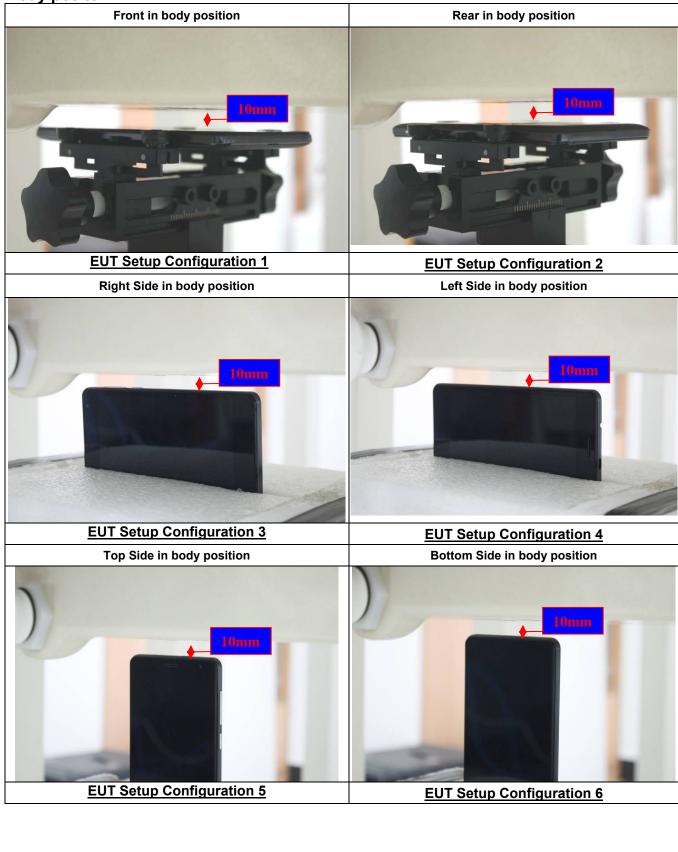

Date of Issue :January 26, 2015

## **11.7 SAR MEASUREMENT RESULTS**

## **Head SAR Test Records**

Band	Mode	Test Position	Ch.	Freq. (MHZ)	max Power (dBm)	Tune- Up Limit (dBm)	Scaling Factor	Power Drift (dB)	SAR1g (mW/g)	Scaled SAR1g (mW/g)
GSM850	Voice	Right Cheek	251	848.8	32.74	33	1.062	-0.02	0.358	0.380
GSM850	Voice	Right Tilted	251	848.8	32.74	33	1.062	-0.05	0.238	0.253
GSM850	Voice	Left Cheek	251	848.8	32.74	33	1.062	-0.08	0.322	0.342
GSM850	Voice	Left Tilted	251	848.8	32.74	33	1.062	-0.11	0.252	0.268
PCS1900	Voice	Right Cheek	810	1909.8	29.39	30	1.151	-0.15	0.169	0.194
PCS1900	Voice	Right Tilted	810	1909.8	29.39	30	1.151	-0.12	0.154	0.177
PCS1900	Voice	Left Cheek	810	1909.8	29.39	30	1.151	-0.09	0.292	0.336
PCS1900	Voice	Left Tilted	810	1909.8	29.39	30	1.151	-0.13	0.148	0.170
WCDMA II	RMC 12.2k	Right Cheek	9400	1880	21.84	22	1.038	-0.04	0.355	0.368
WCDMA II	RMC 12.2k	Right Tilted	9400	1880	21.84	22	1.038	-0.02	0.331	0.343
WCDMA II	RMC 12.2k	Left Cheek	9400	1880	21.84	22	1.038	-0.03	0.591	0.613
WCDMA II	RMC 12.2k	Left Tilted	9400	1880	21.84	22	1.038	0.04	0.259	0.269
WCDMA IV	RMC 12.2k	Right Cheek	1312	1712.4	20.59	21	1.099	-0.15	0.153	0.168
WCDMA IV	RMC 12.2k	Right Tilted	1312	1712.4	20.59	21	1.099	-0.03	0.119	0.131
WCDMA IV	RMC 12.2k	Left Cheek	1312	1712.4	20.59	21	1.099	0.09	0.239	0.263
WCDMA IV	RMC 12.2k	Left Tilted	1312	1712.4	20.59	21	1.099	0.08	0.094	0.103
WCDMA V	RMC 12.2k	Right Cheek	4182	836.6	22.47	23	1.130	0.10	0.303	0.342
WCDMA V	RMC 12.2k	Right Tilted	4182	836.6	22.47	23	1.130	0.06	0.147	0.166
WCDMA V	RMC 12.2k	Left Cheek	4182	836.6	22.47	23	1.130	-0.10	0.258	0.291
WCDMA V	RMC 12.2k	Left Tilted	4182	836.6	22.47	23	1.130	0.04	0.176	0.199
WLAN 2.4G	802.11 b	Right Cheek	1	2412	14.92	15	1.019	0.03	0.889	0.906
WLAN 2.4G	802.11 b	Right Cheek	6	2437	14.81	15	1.045	-0.07	0.714	0.746
WLAN 2.4G	802.11 b	Right Cheek	11	2462	14.74	15	1.062	0.08	0.578	0.614
WLAN 2.4G	802.11 b	Right Tilted	1	2412	14.92	15	1.019	-0.05	0.689	0.702
WLAN 2.4G	802.11 b	Left Cheek	1	2412	14.92	15	1.019	0.11	0.364	0.371
WLAN 2.4G	802.11 b	Left Tilted	1	2412	14.92	15	1.019	0.12	0.329	0.335

Date of Issue :January 26, 2015

## SAR for Body-Worn Test Records

Band	Mode	Test Position	Dist. (mm)	Ch.	Freq. (MHZ)	max Power (dBm)	Tune-Up Limit (dBm)	Scaling Factor	Power Drift (dB)	SAR1g (mW/g)	Scaled SAR1g (mW/g)
GSM850	GPRS 4slots	Front	10	251	848.8	29.43	30	1.140	-0.11	0.563	0.642
GSM850	GPRS 4slots	Rear	10	128	824.2	29.27	30	1.183	-0.01	0.792	0.937
GSM850	GPRS 4slots	Rear	10	190	836.6	29.26	30	1.186	-0.09	0.804	0.953
GSM850	GPRS 4slots	Rear	10	251	848.8	29.43	30	1.140	0.07	0.875	0.998
PCS1900	GPRS 4slots	Front	10	810	1909.8	25.97	27	1.268	-0.06	0.350	0.444
PCS1900	GPRS 4slots	Rear	10	810	1909.8	25.97	27	1.268	0.03	0.381	0.483
WCDMA II	RMC 12.2k	Front	10	9400	1880	21.84	22	1.038	-0.01	0.661	0.686
WCDMA II	RMC 12.2k	Rear	10	9400	1880	21.84	22	1.038	0.03	0.758	0.786
WCDMA IV	RMC 12.2k	Front	10	1312	1712.4	20.59	21	1.099	0.08	0.210	0.231
WCDMA IV	RMC 12.2k	Rear	10	1312	1712.4	20.59	21	1.099	-0.03	0.256	0.281
WCDMA V	RMC 12.2k	Front	10	4182	836.6	22.47	23	1.130	0.00	0.277	0.313
WCDMA V	RMC 12.2k	Rear	10	4182	836.6	22.47	23	1.130	-0.14	0.450	0.508
WLAN 2.4G	802.11 b	Front	10	1	2412	14.92	15	1.019	-0.05	0.083	0.085
WLAN 2.4G	802.11 b	Rear	10	1	2412	14.92	15	1.019	0.06	0.094	0.096

## Note:

According to October 2013TCB Workshop, For GSM / GPRS / EGPRS, the number of time slots to test for SAR should correspond to the highest source-based time-averaged maximum output power configuration, Considering the possibility of e.g. 3rd party VoIP operation for body-worn SAR testing, the EUT was set in GPRS (4Tx slots) for GSM850/GSM1900 band due to its highest frame-average power.

Date of Issue :January 26, 2015

## **SAR for Hotspot Test Records**

0/11/10	πιοισμοι τ	0011000	140								
Band	Mode	Test Position	Dist. (mm)	Ch.	Freq. (MHZ)	max Power (dBm)	Tune- Up Limit (dBm)	Scaling Factor	Power Drift (dB)	SAR1g (mW/g)	Scaled SAR1g (mW/g)
GSM850	GPRS 4slots	Front	10	251	848.8	29.43	30	1.140	-0.11	0.563	0.642
GSM850	GPRS 4slots	Rear	10	128	824.2	29.27	30	1.183	-0.01	0.792	0.937
GSM850	GPRS 4slots	Rear	10	190	836.6	29.26	30	1.186	-0.09	0.804	0.953
GSM850	GPRS 4slots	Rear	10	251	848.8	29.43	30	1.140	0.07	0.875	0.998
GSM850	GPRS 4slots	Right	10	251	848.8	29.43	30	1.140	0.05	0.645	0.735
GSM850	GPRS 4slots	Left	10	251	848.8	29.43	30	1.140	0.04	0.426	0.486
GSM850	GPRS 4slots	Bottom	10	251	848.8	29.43	30	1.140	0.08	0.215	0.245
PCS1900	GPRS 4slots	Front	10	810	1909.8	25.97	27	1.268	-0.06	0.350	0.444
PCS1900	GPRS 4slots	Rear	10	810	1909.8	25.97	27	1.268	0.03	0.381	0.483
PCS1900	GPRS 4slots	Right	10	810	1909.8	25.97	27	1.268	-0.10	0.115	0.146
PCS1900	GPRS 4slots	Left	10	810	1909.8	25.97	27	1.268	-0.02	0.322	0.408
PCS1900	GPRS 4slots	Bottom	10	810	1909.8	25.97	27	1.268	-0.08	0.157	0.199
WCDMA II	RMC 12.2k	Front	10	9400	1880	21.84	22	1.038	-0.01	0.661	0.686
WCDMA II	RMC 12.2k	Rear	10	9400	1880	21.84	22	1.038	0.03	0.758	0.786
WCDMA II	RMC 12.2k	Right	10	9400	1880	21.84	22	1.038	0.08	0.256	0.266
WCDMA II	RMC 12.2k	Left	10	9400	1880	21.84	22	1.038	0.04	0.572	0.593
WCDMA II	RMC 12.2k	Bottom	10	9400	1880	21.84	22	1.038	-0.06	0.275	0.285
WCDMA IV	RMC 12.2k	Front	10	1312	1712.4	20.59	21	1.099	0.08	0.210	0.231
WCDMA IV	RMC 12.2k	Rear	10	1312	1712.4	20.59	21	1.099	-0.03	0.256	0.281
WCDMA IV	RMC 12.2k	Right	10	1312	1712.4	20.59	21	1.099	-0.05	0.076	0.084
WCDMA IV	RMC 12.2k	Left	10	1312	1712.4	20.59	21	1.099	0.11	0.158	0.174
WCDMA IV	RMC 12.2k	Bottom	10	1312	1712.4	20.59	21	1.099	0.06	0.121	0.133
WCDMA V	RMC 12.2k	Front	10	4182	836.6	22.47	23	1.130	0.00	0.277	0.313
WCDMA V	RMC 12.2k	Rear	10	4182	836.6	22.47	23	1.130	-0.14	0.450	0.508
WCDMA V	RMC 12.2k	Right	10	4182	836.6	22.47	23	1.130	-0.15	0.329	0.372
WCDMA V	RMC 12.2k	Left	10	4182	836.6	22.47	23	1.130	-0.04	0.212	0.240
WCDMA V	RMC 12.2k	Bottom	10	4182	836.6	22.47	23	1.130	-0.10	0.078	0.088
WLAN 2.4G	802.11 b	Front	10	1	2412	14.92	15	1.019	-0.05	0.083	0.085
WLAN 2.4G	802.11 b	Rear	10	1	2412	14.92	15	1.019	0.06	0.094	0.096
WLAN 2.4G	802.11 b	Left	10	1	2412	14.92	15	1.019	0.01	0.047	0.048
WLAN 2.4G	802.11 b	Тор	10	1	2412	14.92	15	1.019	0.03	0.093	0.095

## **Repeated SAR Test Records**

Band	Mode	Test Position	Dist. (mm)	Ch.	Freq. (MHZ)	max Power (dBm)	Tune- Up Limit (dBm)	Scaling Factor	Power Drift (dB)	SAR1g (mW/g)	Scaled SAR1g (mW/g)
WLAN 2.4G	802.11 b	Right Cheek	0	1	2412	14.92	15	1.019	0.11	0.887	0.903
GSM850	GPRS 4slots	Rear	10	251	848.8	29.43	30	1.140	0.06	0.861	0.982

Report No: C141229S01-SF

Date of Issue : January 26, 2015

## **11.8 REPEATED SAR MEASUREMENT**

Band	Mode	Test Position	Dist. (mm)	Ch.	Original Measured SAR1g (mW/g)	1st Repeated SAR1g (mW/g)	Ratio	Original Measured SAR1g (mW/g)	2nd Repeated SAR1g (mW/g)	Ratio
WLAN 2.4G	802.11 b	Right Cheek	0	1	0.889	0.887	1.002			
GSM850	GPRS 4slots	Rear	10	251	0.875	0.861	1.016			

## Note:

- 1. Per KDB 865664 D01v01, for each frequence band, repeated SAR measurement is required only when the measured SAR is  $\geq 0.8W/Kg$
- 2. Per KDB 865664 D01v01, if the ratio of largest to smallest SAR for the original and first repeated measurement is ≤1.2 and the measured SAR <1.45W/Kg,only one repeated measurement is required.
- 3. Perform a second repeated measurement only if the ratio of largest to smallest SAR for the original and first repeated measurements is > 1.20 or when the original or repeated measurement is ≥ 1.45 W/kg
- 4. The ratio is the difference in percentage between original and repeated measured SAR.

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

## **11.9 SAR HANDSETS MULTI XMITER ASSESSMENT**

	Position	Applicable Combination				
		WWAN + WLAN				
	Head	WWAN + BT				
Simultaneous		WWAN + WLAN				
Transmission	Body-worn	WWAN + BT				
		WWAN + WLAN				
	Hotspot	WWAN + BT				

Note:

- 1. 2.4GHz WLAN and BT share the same antenna, and cannot transmit simultaneously.
- 2. The reported SAR summation is calculated based on the same configuration and test position.
- 3. For simultaneous transmission analysis, Bluetooth SAR is estimated per KDB 447498 D01v05 based on the formula below.

(max. power of channel, including tune-up tolerance, mW)/(min. test separation distance, mm)] • [ \sqrt{f(GHz)/x]} W/kg for test separation distances  $\leq$  50 mm; where x = 7.5 for 1-g SAR, and x = 18.75 for 10-g SAR.

0.4 W/kg for 1-g SAR and 1.0 W/kg for 10-g SAR, when the test separation distances is > 50 mm.

#### Bluetooth:

	Max power	Head (5mm distance)	Body (10mm distance)
Estimated SAR (W/kg)	7 dBm	0.210 W/kg	0.105 W/kg

4. Per KDB 447498 D01v05, simultaneous transmission SAR is compliant if,

1) Scalar SAR summation < 1.6W/kg.

2) SPLSR = (SAR1 + SAR2)1.5 / (min. separation distance, mm), and the peak separation distance is determined from the square root of [(x1-x2)2 + (y1-y2)2 + (z1-z2)2], where (x1, y1, z1) and (x2, y2, z2) are the coordinates of the extrapolated peak SAR locations in the zoom scan

If SPLSR  $\leq$  0.04, simultaneously transmission SAR is compliant

3) Simultaneously transmission SAR measurement, and the reported multi-band SAR < 1.6W/kg

Date of Issue : January 26, 2015

## Result of SUM ∑SAR1g of Head

	SUM ∑SAR1g (GSM850+WLAN(2.4G) or Bluetooth)										
Position	Distance	Stand a	alone SAR(1g	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]						
[mm]		GSM850	WLAN 2.4G	Bluetooth	WWAN + WLAN(2.4G)	WWAN + Bluetooth					
Right Cheek	0	0.380	0.906	0.210	1.286	0.590					
Right Tilted	0	0.253	0.702	0.210	0.955	0.463					
Left Cheek	0	0.342	0.371	0.210	0.713	0.552					
Left Tilted	0	0.268	0.335	0.210	0.603	0.478					

	SUM ∑SAR1g (PCS1900+WLAN(2.4G) or Bluetooth)										
Position	Distance	Stand a	Stand alone SAR(1g) [W/kg] SUM SUM SUM SAR(1g)[W/kg] SAR(1g)								
i contoni	[mm]	PCS 1900	WLAN 2.4G	Bluetooth	WWAN + WLAN(2.4G)	WWAN + Bluetooth					
Right Cheek	0	0.194	0.906	0.210	1.100	0.404					
Right Tilted	0	0.177	0.702	0.210	0.879	0.387					
Left Cheek	0	0.336	0.371	0.210	0.707	0.546					
Left Tilted	0	0.170	0.335	0.210	0.505	0.380					

	SUM ∑SAR1g (WCDMA Band II+WLAN(2.4G) or Bluetooth)										
Position	Distance	Stand a	lone SAR(1g	) [W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]					
	[mm]	WCDMA II	WLAN 2.4G	Bluetooth	WWAN + WLAN(2.4G)	WWAN + Bluetooth					
Right Cheek	0	0.368	0.906	0.210	1.274	0.578					
Right Tilted	0	0.343	0.702	0.210	1.045	0.553					
Left Cheek	0	0.613	0.371	0.210	0.984	0.823					
Left Tilted	0	0.269	0.335	0.210	0.604	0.479					



Date of Issue :January 26, 2015

	SUM ∑SAR1g (WCDMA Band IV+WLAN(2.4G) or Bluetooth)										
Position	Distance	Stand a	lone SAR(1g	) [W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]					
	[mm]	WCDMA IV	WLAN 2.4G	Bluetooth	WWAN + WLAN(2.4G)	WWAN + Bluetooth					
Right Cheek	0	0.168	0.906	0.210	1.074	0.378					
Right Tilted	0	0.131	0.702	0.210	0.833	0.341					
Left Cheek	0	0.263	0.371	0.210	0.634	0.473					
Left Tilted	0	0.103	0.335	0.210	0.438	0.313					

	SUM ∑SAR1g (WCDMA Band V+WLAN(2.4G) or Bluetooth)									
Position	Distance	Stand a	Stand alone SAR(1g) [W/kg] SUM SAR(1g)[W/kg] SAR(1							
	[mm]	WCDMA V	WLAN 2.4G	Bluetooth	WWAN + WLAN(2.4G)	WWAN + Bluetooth				
Right Cheek	0	0.342	0.906	0.210	1.248	0.552				
Right Tilted	0	0.166	0.702	0.210	0.868	0.376				
Left Cheek	0	0.291	0.371	0.210	0.662	0.501				
Left Tilted	0	0.199	0.199 0.335 0.210 0.534 0.409							

Date of Issue : January 26, 2015

## Result of SUM ∑SAR1g for Body worn

	SUM ∑SAR1g (GSM850+WLAN(2.4G) or Bluetooth)						
Position	Distance	Stand	alone SAR(1g	) [W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]	
	[mm]	GSM850	GSM850 WLAN 2.4G Bluetooth		WWAN + WLAN(2.4G)	WWAN + Bluetooth	
Front	10	0.642 0.085 0.105		0.727	0.747		
Rear	10	0.998 0.096 0.105			1.094	1.103	

	SUM ∑SAR1g (PCS1900+WLAN(2.4G) or Bluetooth)						
Position	Distance	Stand a	lone SAR(1g)	[W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]	
	[mm]	PCS1900	WLAN 2.4G	Bluetooth	WWAN + WLAN(2.4G)	WWAN + Bluetooth	
Front	10	0.444	0.444 0.085 0.105			0.549	
Rear	10	0.483	0.483 0.096 0.105 0.579 0.588				

SUM ∑SAR1g (WCDMA Band II+WLAN(2.4G) or Bluetooth)						
Position	Distance	Stand a	lone SAR(1g	) [W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]
	[mm]	WCDMA II	WCDMA II WLAN Bluetooth			WWAN + Bluetooth
Front	10	0.686 0.085 0.105			0.771	0.791
Rear	10	0.786 0.096 0.105 0.882 0.891				0.891

	SUM ∑SAR1g (WCDMA Band IV+WLAN(2.4G) or Bluetooth)						
Position	Distance	Stand a	lone SAR(1g	) [W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]	
	[mm]	WCDMA IV	Bluetooth			WWAN + Bluetooth	
Front	10	0.231 0.085 0.105			0.316	0.336	
Rear	10	0.281 0.096 0.105 0.377 0.386					

	SUM ∑SAR1g (WCDMA Band V+WLAN(2.4G) or Bluetooth)						
Position	Distance	Stand a	lone SAR(1g	) [W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]	
	[mm]	WCDMA V	WCDMA V WLAN Bluetooth			WWAN + Bluetooth	
Front	10	0.313 0.085 0.105		0.398	0.418		
Rear	10	0.508	0.508 0.096 0.105 0.604 0.613				

Date of Issue : January 26, 2015

## Result of SUM ∑SAR1g for Hotspot

	SUM ∑SAR1g (GSM850+WLAN(2.4G) or Bluetooth)							
Position	Distance	Stand	Stand alone SAR(1g) [W/kg]			SUM SAR(1g)[W/kg]		
	[mm]	GPRS850	GPRS850 WLAN Bluetooth		WWAN + WLAN(2.4G)	WWAN + Bluetooth		
Front	10	0.642	0.085	0.105	0.727	0.747		
Rear	10	0.998	0.096	0.105	1.094	1.103		
Right Side	10	0.735		0.105		0.840		
Left Side	10	0.486	0.486 0.048		0.534	0.591		
Top side	10	0.095 0.105		0.105				
Bottom side	10	0.245 0.105			0.350			

	SUM ∑SAR1g (PCS1900+WLAN(2.4G) or Bluetooth)							
Position	Distance	Stand a	lone SAR(1g)	) [W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]		
FOSILION	[mm]	GPRS 1900	Bluetooth		WWAN + WLAN(2.4G)	WWAN + Bluetooth		
Front	10	0.444	0.085	0.105	0.529	0.549		
Rear	10	0.483	0.096	0.105	0.579	0.588		
Right Side	10	0.146		0.105		0.251		
Left Side	10	0.408	0.408 0.048 0.105		0.456	0.513		
Top side	10		0.095 0.105					
Bottom side	10	0.199	0.199 0.105			0.304		

	SUM ∑SAR1g (WCDMA Band II+WLAN(2.4G) or Bluetooth)							
Position	Distance	Stand a	Stand alone SAR(1g) [W/kg]			SUM SAR(1g)[W/kg]		
FOSILION	[mm]	WCDMA II	WCDMA II WLAN 2.4G Bluetooth		WWAN + WLAN(2.4G)	WWAN + Bluetooth		
Front	10	0.686	0.085	0.105	0.771	0.791		
Rear	10	0.786	0.096	0.105	0.882	0.891		
Right Side	10	0.266		0.105		0.371		
Left Side	10	0.593	0.593 0.048 0.10		0.641	0.698		
Top side	10	0.095 0.105						
Bottom side	10	0.285		0.105		0.390		



Date of Issue : January 26, 2015

	SUM ∑SAR1g (WCDMA Band IV+WLAN(2.4G) or Bluetooth)						
Position	Distance	Stand al	one SAR(1g)	[W/kg]	SUM SAR(1g)[W/kg]	SUM SAR(1g)[W/kg]	
FOSILION	[mm]	WCDMA IV	WCDMA IV WLAN 2.4G Bluetooth		WWAN + WLAN(2.4G)	WWAN + Bluetooth	
Front	10	0.231	0.085	0.105	0.316	0.336	
Rear	10	0.281	0.096	0.105	0.377	0.386	
Right Side	10	0.084		0.105		0.189	
Left Side	10	0.174	0.174 0.048 0.105		0.222	0.279	
Top side	10	0.095 0.105					
Bottom side	10	0.133 0.105			0.238		

	SUM ∑SAR1g (WCDMA Band V+WLAN(2.4G) or Bluetooth)							
Position	Distance	Stand a	Stand alone SAR(1g) [W/kg]			SUM SAR(1g)[W/kg]		
FOSILION	[mm]	WCDMA V	VCDMA V WLAN Bluetooth		WWAN + WLAN(2.4G)	WWAN + Bluetooth		
Front	10	0.313	0.085	0.105	0.398	0.418		
Rear	10	0.508	0.096	0.105	0.604	0.613		
Right Side	10	0.372		0.105		0.477		
Left Side	10	0.240	0.240 0.048 0.105		0.288	0.345		
Top side	10		0.095 0.105					
Bottom side	10	0.088		0.105		0.193		


Date of Issue :January 26, 2015

# **EUT PHOTO**






Date of Issue :January 26, 2015

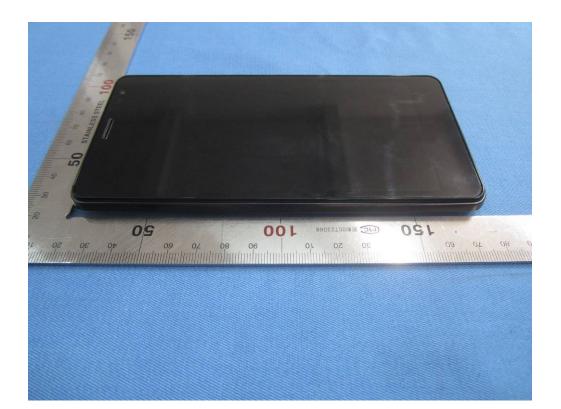






Date of Issue :January 26, 2015

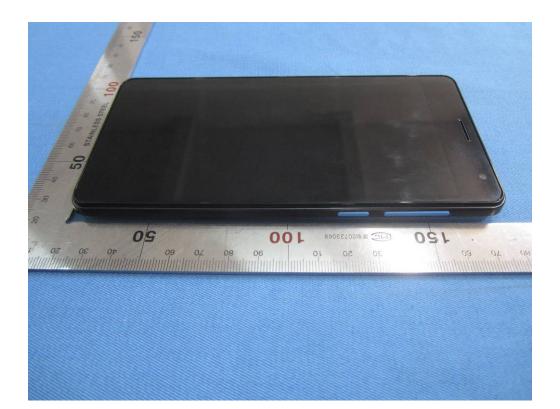


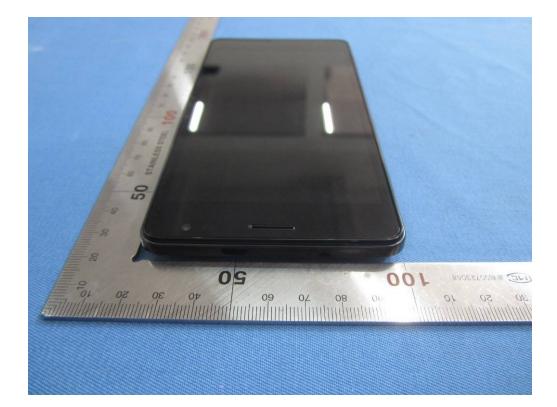



Date of Issue :January 26, 2015



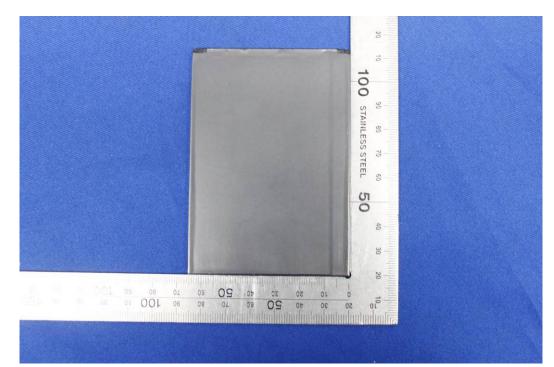

Date of Issue :January 26, 2015

#### **EQUIPMENT LIST & CALIBRATION STATUS** 12.

Name of Equipment	Manufacturer	Type/Model	Serial Number	Last Calibration	Calibration Due
PC	HP	Core(rm)3.16G	CZCO48171H	N/A	N/A
Signal Generator	Agilent	83732B	US37101915	05/30/2014	05/29/2015
S-Parameter Network Analyzer	Agilent	E5071B	MY42301382	03/17/2014	03/16/2015
Wireless Communication Test Set	R&S	CMU200	SN:109525	01/24/2014	01/23/2015
Power Meter	Agilent	E4416A	GB41292714	03/18/2014	03/17/2015
Peak & Average sensor	Agilent	E9327A	us40441788	03/18/2014	03/17/2015
E-field PROBE	SPEAG	EX3DV4	3798	07/28/2014	07/27/2015
DAE	SPEAG	DEA4	1245	07/22/2014	07/23/2015
DIPOLE 835MHZ ANTENNA	SPEAG	D835V2	4d114	07/30/2013	07/28/2015
DIPOLE 1800MHZ ANTENNA	SPEAG	D1800V2	2d170	07/31/2013	07/29/2015
DIPOLE 1900MHZ ANTENNA	SPEAG	D1900V2	5d136	07/22/2013	07/20/2015
DIPOLE 2450MHZ ANTENNA	SPEAG	D2450V2	817	07/31/2013	07/29/2015
DUMMY PROBE	SPEAG	DP_2	SPDP2001AA	N/A	N/A
SAM PHANTOM (ELI4 v4.0)	SPEAG	QDOVA001BB	1102	N/A	N/A
Twin SAM Phantom	SPEAG	QD000P40CD	1609	N/A	N/A
ROBOT	SPEAG	TX60	F10/5E6AA1/A101	N/A	N/A
ROBOT KRC	SPEAG	CS8C	F10/5E6AA1/C101	N/A	N/A
LIQUID CALIBRATION KIT	ANTENNESSA	41/05 OCP9	00425167	N/A	N/A

Date of Issue : January 26, 2015

# 13. FACILITIES

Report No: C141229S01-SF

All measurement facilities used to collect the measurement data are located at

🔀 No.10, Weiye Rd., Innovation Park, Eco & Tec. Development Part, Kunshan City, Jiangsu Province, China.

#### REFERENCES 14

- [1] Federal Communications Commission, Report and order: Guidelines for evaluating the environ-mental effects of radiofrequency radiation", Tech. Rep. FCC 96-326, FCC, Washington, D.C. 20554, 1996.
- David L. Means Kwok Chan, Robert F. Cleveland, \Evaluating compliance with FCC guidelines [2] for human exposure to radiofrequency electromagnetic fields", Tech. Rep., Federal Communication Commision, O\_ce of Engineering & Technology, Washington, DC, 1997.
- Thomas Schmid, Oliver Egger, and Niels Kuster, \Automated E- eld scanning system for [3] dosimetric assessments", IEEE Transactions on Microwave Theory and Techniques, vol. 44, pp. 105{113, Jan. 1996.
- Niels Kuster, Ralph K.astle, and Thomas Schmid, \Dosimetric evaluation of mobile [4] communications equipment with known precision", IEICE Transactions on Communications, vol. E80-B, no. 5, pp. 645{652, May 1997.
- [5] CENELEC. Considerations for evaluating of human exposure to electromagnetic fields (EMFs) from mobile telecommunication equipment (MTE) in the frequency range 30MHz - 6GHz", Tech. Rep., CENELEC, European Committee for Electrotechnical Standardization, Brussels, 1997.
- [6] ANSI, ANSI/IEEE C95.1-1999: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz, The Institute of Electrical and Electronics Engineers, Inc., New York, NY 10017, 1992.
- [7] Katja Pokovic, Thomas Schmid, and Niels Kuster, \Robust setup for precise calibration of Eeld probes in tissue simulating liquids at mobile communications frequencies", in ICECOM 97, Dubrovnik, October 15{17, 1997, pp. 120{124.
- Katja Pokovic, Thomas Schmid, and Niels Kuster, \E- eld probe with improved isotropy in [8] brain simulating liquids", in Proceedings of the ELMAR, Zadar, Croatia, 23(25 June, 1996, pp. 172{175.
- Volker Hombach, Klaus Meier, Michael Burkhardt, Eberhard K. uhn, and Niels Kuster, \The [9] dependence of EM energy absorption upon human head modeling at 900 MHz", IEEE Transactions on Microwave Theory and Techniques, vol. 44, no. 10, pp. 1865(1873, Oct. 1996.
- [10] Klaus Meier, Ralf Kastle, Volker Hombach, Roger Tay, and Niels Kuster, \The dependence of EM energy absorption upon human head modeling at 1800 MHz", IEEE Transactions on Microwave Theory and Techniques, Oct. 1997, in press.
- [11] W. Gander, Computermathematik, Birkhaeuser, Basel, 1992.
- [12] W. H. Press, S. A. Teukolsky, W. T. Vetterling, and B. P. Flannery, Numerical Receptes in C, The Art of Scientific Computing, Second Edition, Cambridge University Press, 1992...Dosimetric Evaluation of Sample device, month 1998 9
- [13] NIS81 NAMAS, \The treatment of uncertainity in EMC measurement", Tech. Rep., NAMAS Executive, National Physical Laboratory, Teddington, Middlesex, England, 1994.
- [14] Barry N. Taylor and Christ E. Kuyatt, \Guidelines for evaluating and expressing the uncertainty of NIST measurement results", Tech. Rep., National Institute of Standards and Technology, 1994. Dosimetric Evaluation of Sample device, month 1998 10

Page 53 of 126

Date of Issue :January 26, 2015

#### **ATTACHMENTS** 15.

Exhibit	Content
1	System Performance Check Plots
2	Dipole calibration report D835V2 SN:4d114
3	Dipole calibration report D1800V2 SN: 2d170
4	Dipole calibration report D1900V2-SN:5d136
5	Dipole calibration report D2450V2 SN: 817
6	Probe calibration report EX3DV4 SN3798
7	DAE calibration report DEA4 SD000D04BM SN:1245
8	SAR Test Plots



## **APPENDIX A: PLOTS OF PERFORMANCE CHECK**


The plots are showing as followings.

Compliance Certification Services Inc. FCC ID: 2ABOSSKY55W

Report No: C141229S01-SF

Date of Issue : January 26, 2015

Test Laboratory: Compliance Certification Services Inc. Date: 1/6/2015 SystemPerformanceCheck-Head D835 DUT: Dipole 835 MHz D835V2; Type: D835V2; Serial: 4d114 Communication System: UID 0, CW; Communication System Band: D835 (835.0 MHz); Frequency: 835 MHz; Duty Cycle: 1:1 Medium parameters used: f = 835 MHz;  $\sigma$  = 0.911 S/m;  $\varepsilon_r$  = 40.846;  $\rho$  = 1000 kg/m<sup>3</sup> Room Ambient Temperature: 22°C; Liguid Temperature: 21.5°C Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY Configuration: Probe: EX3DV4 - SN3798; ConvF(9.3, 9.3, 9.3); Calibrated: 7/28/2014; Sensor-Surface: 2mm (Mechanical Surface Detection) • Electronics: DAE4 Sn1245; Calibrated: 7/22/2014 • Phantom: Twin SAM Phantom; Type: QD 000 P40 CD; Serial: 1609 • DASY52 52.8.8(1222); • SEMCAD X Version 14.6.10 (7331) System Performance Check at Frequencies Low 1 GHz/Pin=250 mW, dist=15 mm (EX-Probe)/Area Scan (7x12x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 2.72 W/kg System Performance Check at Frequencies Low 1 GHz/Pin=250 mW, dist=15 mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 59.67 V/m; Power Drift = -0.04 dB Peak SAR (extrapolated) = 3.24 W/kg SAR(1 g) = 2.21 W/kg; SAR(10 g) = 1.46 W/ka Maximum value of SAR (measured) = 2.77 W/kg

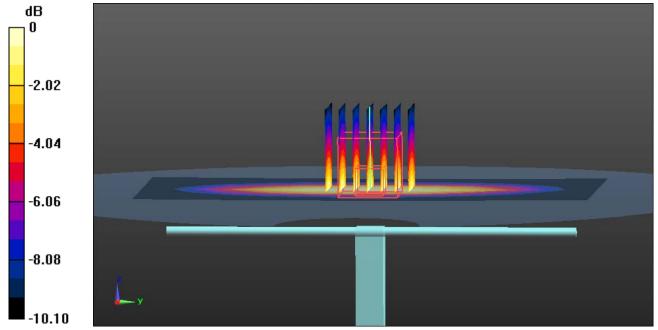

0 dB = 2.77 W/kg = 4.42 dBW/kg

Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W


Date of Issue : January 26, 2015

Test Laboratory: Compliance Certification Services Inc. Date: 1/8/2015 SystemPerformanceCheck-Body D835 DUT: Dipole 835 MHz D835V2; Type: D835V2; Serial: 4d114 Communication System: UID 0, CW; Communication System Band: D835 (835.0 MHz); Frequency: 835 MHz; Duty Cycle: 1:1 Medium parameters used: f = 835 MHz;  $\sigma$  = 0.978 S/m;  $\epsilon_r$  = 53.445;  $\rho$  = 1000 kg/m<sup>3</sup> Room Ambient Temperature: 22°C; Liguid Temperature: 21.5°C Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY Configuration: Probe: EX3DV4 - SN3798; ConvF(9.22, 9.22, 9.22); Calibrated: 7/28/2014; Sensor-Surface: 2mm (Mechanical Surface Detection) • Electronics: DAE4 Sn1245; Calibrated: 7/22/2014 • Phantom: Twin SAM Phantom; Type: QD 000 P40 CD; Serial: 1609 • DASY52 52.8.8(1222); • SEMCAD X Version 14.6.10 (7331)

System Performance Check at Frequencies Low 1 GHz/dist=15mm, Pin=250 mW(EX-Probe)/Area Scan (7x12x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 3.00 W/kg

## System Performance Check at Frequencies Low 1 GHz/dist=15mm, Pin=250 mW(EX-

Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 56.59 V/m; Power Drift = 0.09 dB Peak SAR (extrapolated) = 3.57 W/kg SAR(1 g) = 2.43 W/kg; SAR(10 g) = 1.61 W/kg Maximum value of SAR (measured) = 3.06 W/kg

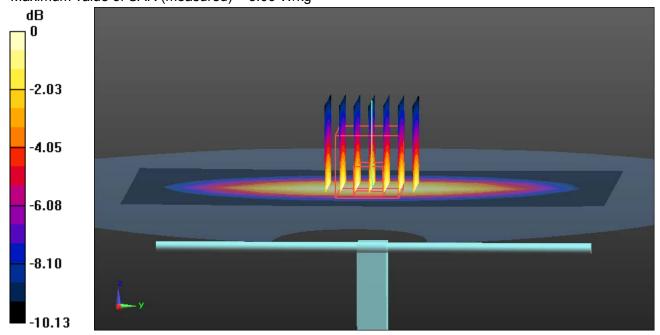

0 dB = 3.06 W/kg = 4.86 dBW/kg

**Compliance Certification Services Inc.** FCC ID: 2ABOSSKY55W

Report No: C141229S01-SF

SystemPerformanceCheck-Head D1800

Test Laboratory: Compliance Certification Services Inc.

Date of Issue : January 26, 2015

Date: 1/6/2015

DUT: Dipole 1800 MHz D1800V2; Type: D1800V2; Serial: D1800V2 - SN:2d170 Communication System: UID 10000, CW; Communication System Band: D1800 (1800.0 MHz); Frequency: 1800 MHz; Duty Cycle: 1:1 Medium parameters used (extrapolated): f = 1800 MHz;  $\sigma$  = 1.439 S/m;  $\epsilon_r$  = 40.015;  $\rho$  = 1000 kg/m<sup>3</sup> Room Ambient Temperature: 22°C; Liguid Temperature: 21.5°C Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY Configuration: Probe: EX3DV4 - SN3798; ConvF(7.82, 7.82, 7.82); Calibrated: 7/28/2014; Sensor-Surface: 3mm (Mechanical Surface Detection) • Electronics: DAE4 Sn1245; Calibrated: 7/22/2014 • Phantom: Twin SAM Phantom; Type: QD 000 P40 CD; Serial: 1609 • DASY52 52.8.8(1222); • SEMCAD X Version 14.6.10 (7331) System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW,(EX-Probe)/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm Info: Extrapolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 11.8 W/kg System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW,(EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 90.04 V/m; Power Drift = -0.05 dB Peak SAR (extrapolated) = 18.1 W/kg SAR(1 g) = 9.86 W/kg; SAR(10 g) = 5.19 W/kg Info: Extrapolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 12.5 W/kg dB 0 -3.43-6.86-10.30-13.73

0 dB = 12.5 W/kg = 10.97 dBW/kg

-17.16

Compliance Certification Services Inc. FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

Test Laboratory: Compliance Certification Services Inc. Date: 1/7/2015 SystemPerformanceCheck-Body D1800 DUT: Dipole 1800 MHz D1800V2; Type: D1800V2; Serial: D1800V2 - SN:2d052 Communication System: UID 10000, CW; Communication System Band: D1800 (1800.0 MHz); Frequency: 1800 MHz; Duty Cycle: 1:1 Medium parameters used (extrapolated): f = 1800 MHz;  $\sigma$  = 1.572 S/m;  $\epsilon_r$  = 54.172;  $\rho$  = 1000 kg/m<sup>3</sup> Room Ambient Temperature: 22°C; Liguid Temperature: 21.5°C Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY Configuration: Probe: EX3DV4 - SN3798; ConvF(7.26, 7.26, 7.26); Calibrated: 7/28/2014; Sensor-Surface: 1.4mm (Mechanical Surface Detection) • Electronics: DAE4 Sn1245; Calibrated: 7/22/2014 • Phantom: Twin SAM Phantom; Type: QD 000 P40 CD; Serial: 1609 • DASY52 52.8.8(1222); •

SEMCAD X Version 14.6.10 (7331)

Report No: C141229S01-SF


System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe) (23.6 dBm)/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm


Info: Extrapolated medium parameters used for SAR evaluation.

Maximum value of SAR (measured) = 15.0 W/kg

System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe) (23.6 dBm)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 103.4 V/m; Power Drift = -0.17 dB Peak SAR (extrapolated) = 17.9 W/kg SAR(1 g) = 9.75 W/kg; SAR(10 g) = 5.11 W/kg Info: Extrapolated medium parameters used for SAR evaluation. Maximum value of SAR (measured) = 15.1 W/kg

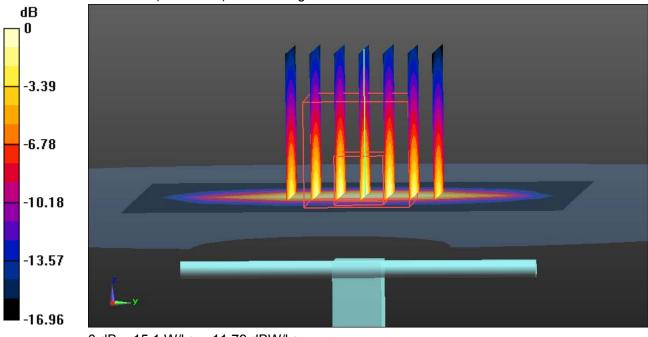



FCC ID: 2ABOSSKY55W


Date of Issue : January 26, 2015

Test Laboratory: Compliance Certification Services Inc. Date: 1/6/2015 SystemPerformanceCheck-Head D1900 DUT: Dipole 1900 MHz D1900V2; Type: D1900V2; Serial: 5d136 Communication System: UID 0, CW; Communication System Band: D1900 (1900.0 MHz); Frequency: 1900 MHz; Duty Cycle: 1:1 Medium parameters used: f = 1900 MHz;  $\sigma$  = 1.431 S/m;  $\epsilon_r$  = 39.062;  $\rho$  = 1000 kg/m<sup>3</sup> Room Ambient Temperature: 22°C; Liguid Temperature: 21.5°C Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY Configuration: Probe: EX3DV4 - SN3798; ConvF(7.75, 7.75, 7.75); Calibrated: 7/28/2014; Sensor-Surface: 2mm (Mechanical Surface Detection) • Electronics: DAE4 Sn1245; Calibrated: 7/22/2014 • Phantom: Twin SAM Phantom; Type: QD 000 P40 CD; Serial: 1609 • DASY52 52.8.8(1222); • SEMCAD X Version 14.6.10 (7331) System Performance Check at Frequencies above 1 GHz/Pin=250 mW, dist=10mm (EX-Probe)/Area Scan (7x8x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 13.3 W/kg

Report No: C141229S01-SF

System Performance Check at Frequencies above 1 GHz/Pin=250 mW, dist=10mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 101.7 V/m; Power Drift = 0.01 dB Peak SAR (extrapolated) = 18.6 W/kg SAR(1 g) = 9.92 W/kg; SAR(10 g) = 5.11 W/kg Maximum value of SAR (measured) = 14.4 W/kg

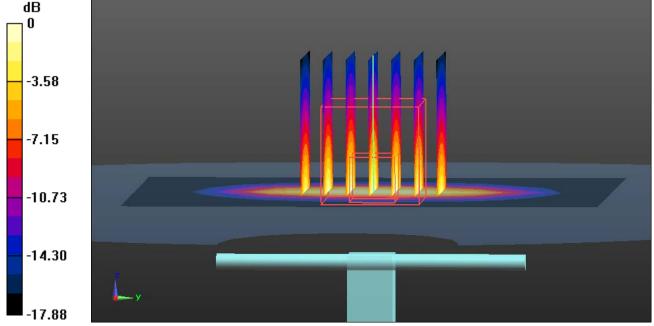

0 dB = 14.4 W/kg = 11.58 dBW/kg


FCC ID: 2ABOSSKY55W

Report No: C141229S01-SF

Date of Issue :January 26, 2015

Test Laboratory: Compliance Certification Services Inc. Date: 1/7/2015 SystemPerformanceCheck-Body D1900 DUT: Dipole 1900 MHz D1900V2; Type: D1900V2; Serial: 5d136 Communication System: UID 0, CW; Communication System Band: D1900 (1900.0 MHz); Frequency: 1900 MHz; Duty Cycle: 1:1 Medium parameters used: f = 1900 MHz;  $\sigma$  = 1.571 S/m;  $\epsilon_r$  = 54.749;  $\rho$  = 1000 kg/m<sup>3</sup> Room Ambient Temperature: 22°C; Liguid Temperature: 21.5°C Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY Configuration: Probe: EX3DV4 - SN3798; ConvF(7.09, 7.09, 7.09); Calibrated: 7/28/2014; Sensor-Surface: 2mm (Mechanical Surface Detection) • Electronics: DAE4 Sn1245; Calibrated: 7/22/2014 • Phantom: Twin SAM Phantom; Type: QD 000 P40 CD; Serial: 1609 • DASY52 52.8.8(1222); • SEMCAD X Version 14.6.10 (7331) System Performance Check at Frequencies above 1 GHz/Pin=250 mW, dist=10mm (EX-Probe)/Area Scan (7x8x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (measured) = 14.6 W/kg System Performance Check at Frequencies above 1 GHz/Pin=250 mW, dist=10mm (EX-

Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 101.5 V/m; Power Drift = -0.05 dB Peak SAR (extrapolated) = 20.0 W/kg SAR(1 g) = 10.8 W/kg; SAR(10 g) = 5.53 W/kg Maximum value of SAR (measured) = 15.5 W/kg

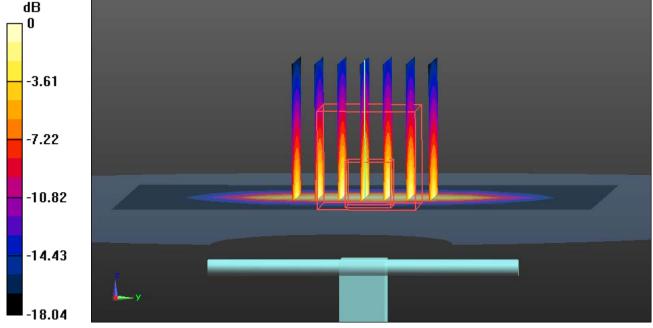

0 dB = 15.5 W/kg = 11.90 dBW/kg

FCC ID: 2ABOSSKY55W

Date of Issue :January 26, 2015


Test Laboratory: Compliance Certification Services Inc. Date: 1/5/2015 SystemPerformanceCheck-Head D2450 DUT: Dipole 2450 MHz D2450V2; Type: D2450V2; Serial: 817 Communication System: UID 0, CW; Communication System Band: D2450 (2450.0 MHz); Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz;  $\sigma$  = 1.832 S/m;  $\epsilon_r$  = 39.128;  $\rho$  = 1000 kg/m<sup>3</sup> Room Ambient Temperature: 22°C; Liguid Temperature: 21.5°C Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY Configuration: Probe: EX3DV4 - SN3798; ConvF(7.04, 7.04, 7.04); Calibrated: 7/28/2014; Sensor-Surface: 2mm (Mechanical Surface Detection) • Electronics: DAE4 Sn1245; Calibrated: 7/22/2014 • Phantom: Twin SAM Phantom; Type: QD 000 P40 CD; Serial: 1609 • DASY52 52.8.8(1222); •

• SEMCAD X Version 14.6.10 (7331)

Report No: C141229S01-SF

System Performance Check at Frequencies above 1 GHz/Pin=250 mW, dist=10mm (EX-Probe)/Area Scan (9x10x1): Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 19.4 W/kg

System Performance Check at Frequencies above 1 GHz/Pin=250 mW, dist=10mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 108.6 V/m; Power Drift = 0.00 dB Peak SAR (extrapolated) = 29.2 W/kg SAR(1 g) = 13.4 W/kg; SAR(10 g) = 6.01 W/kg Maximum value of SAR (measured) = 21.0 W/kg

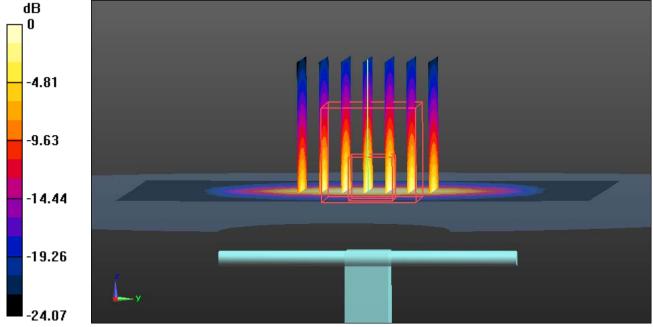

0 dB = 21.0 W/kg = 13.22 dBW/kg

FCC ID: 2ABOSSKY55W


Report No: C141229S01-SF

Date of Issue :January 26, 2015

Test Laboratory: Compliance Certification Services Inc. Date: 1/5/2015 SystemPerformanceCheck-Body D2450 DUT: Dipole 2450 MHz D2450V2; Type: D24500V2; Serial: 817 Communication System: UID 0, CW; Communication System Band: D2450 (2450.0 MHz); Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz;  $\sigma$  = 1.978 S/m;  $\epsilon_r$  = 51.708;  $\rho$  = 1000 kg/m<sup>3</sup> Room Ambient Temperature: 22°C; Liguid Temperature: 21.5°C Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY Configuration: Probe: EX3DV4 - SN3798; ConvF(6.82, 6.82, 6.82); Calibrated: 7/28/2014; Sensor-Surface: 2mm (Mechanical Surface Detection) • Electronics: DAE4 Sn1245; Calibrated: 7/22/2014 • Phantom: Twin SAM Phantom; Type: QD 000 P40 CD; Serial: 1609 • DASY52 52.8.8(1222); • SEMCAD X Version 14.6.10 (7331)

System Performance Check at Frequencies above 1 GHz/Pin=250 mW, dist=10mm (EX-Probe)/Area Scan (9x10x1): Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (measured) = 18.5 W/kg

System Performance Check at Frequencies above 1 GHz/Pin=250 mW, dist=10mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 102.3 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 28.5 W/kg SAR(1 g) = 12.9 W/kg; SAR(10 g) = 5.74 W/kg Maximum value of SAR (measured) = 20.3 W/kg

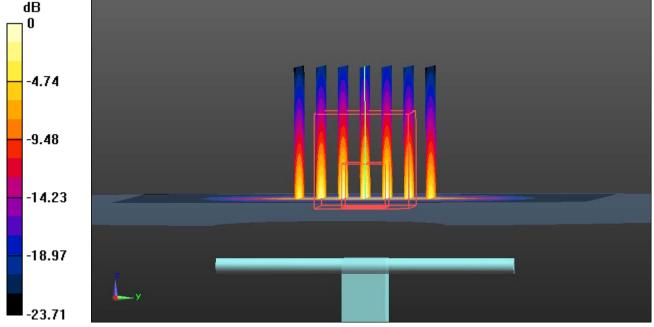

0 dB = 20.3 W/kg = 13.07 dBW/kg



## Date of Issue :January 26, 2015

## **APPENDIX B: DASY CALIBRATION CERTIFICATE**

The DASY Calibration Certificates are showing as followings .

Calibration Laboratory Schmid & Partner	y of	SMISS S	Want from the Barrier of State Sector and
Engineering AG Zeughausstrasse 43, 8004 Zurich	n, Switzerland	C C Z Z C	Servizio svizzero di taratura
Accredited by the Swiss Accreditat The Swiss Accreditation Service Multilateral Agreement for the re	is one of the signatories	s to the EA	n No.: SCS 108
Client CCS-CN (Auder	n)	Certificate N	le: D835V2-4d114_Jul1
CALIBRATION C	ERTIFICATE		
Object	D835V2 - SN: 4d	114	
Calibration procedure(s)	QA CAL-05.v9 Calibration proce	dure for dipole validation kits ab	ove 700 MHz
	1944 - C. M. C. L. C. C. C. C. C. M. C. M	onal standards, which realize the physical u robability are given on the following pages a	
This calibration certificate docum The measurements and the unce All calibrations have been conduc	ents the traceability to nati rtainties with confidence p cted in the closed laborator		and are part of the certificate.
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T	ents the traceability to nati rtainties with confidence p cted in the closed laborator FE critical for calibration)	robability are given on the following pages a y facility: environment temperature ( $22 \pm 3$ )	and are part of the certificate.
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards	ents the traceability to nati rtainties with confidence p sted in the closed laborator FE critical for calibration)	robability are given on the following pages a y facility: environment temperature (22 ± 3) Cal Date (Certificate No.)	and are part of the certificate.
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T	ents the traceability to nati rtainties with confidence p cted in the closed laborator FE critical for calibration)	robability are given on the following pages a y facility: environment temperature ( $22 \pm 3$ )	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPN-442A Power sensor HP 8481A Reference 20 dB Attenuator	ents the traceability to nati itainties with confidence p ated in the closed laborator FE critical for calibration) ID # GB37480704 US37292783 SN: 5056 (20k)	Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736)	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination	ents the traceability to nati intainties with confidence p ated in the closed laborator FE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327	Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739)	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPN-442A Power sensor HP 8481A Reference 20 dB Attenuator	ents the traceability to nati itainties with confidence p ated in the closed laborator FE critical for calibration) ID # GB37480704 US37292783 SN: 5056 (20k)	Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736)	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	ents the traceability to nati intainties with confidence p ated in the closed laborator FE critical for calibration) ID # GB37480704 US37292785 SN: 5056 (20k) SN: 5047.3 / 06327 SN: 3205	Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12)	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPN-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4	ents the traceability to nati rtainties with confidence p ated in the closed laborator FE critical for calibration) ID # GB37480704 US37292783 SN: 5056 (20k) SN: 50547.3 / 06327 SN: 505 SN: 601	Cal Date (Certificate No.)           01-Nov-12 (No. 217-01640)           01-Nov-12 (No. 217-01640)           04-Apr-13 (No. 217-01640)           04-Apr-13 (No. 217-01736)           04-Apr-13 (No. 217-01739)           28-Dec-12 (No. ES3-3205_Dec12)           25-Apr-13 (No. DAE4-601_Apr13)           Check Date (in house)           18-Oct-02 (in house check Oct-11)	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPN-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards	ents the traceability to nati intainties with confidence p ated in the closed laborator FE critical for calibration) ID # GB37480704 US37292785 SN: 5056 (20k) SN: 5056 (20k)	robability are given on the following pages a y facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house)	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPN-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A Rif generator R&S SMT-06	ents the traceability to nati intainties with confidence p ated in the closed laborator IE critical for calibration) ID # GB37480704 US37292785 SN: 5056 (20k) SN: 601 ID # MY41092317 100005	colability are given on the following pages a           y facility: environment temperature (22 ± 3)           Cal Date (Certificate No.)           01-Nov-12 (No. 217-01640)           01-Nov-12 (No. 217-01640)           04-Apr-13 (No. 217-01736)           04-Apr-13 (No. 217-01736)           28-Dec-12 (No. ES3-3205_Dec12)           25-Apr-13 (No. DAE4-601_Apr13)           Check Date (in house)           18-Oct-02 (in house check Oct-11)           04-Aug-99 (in house check Oct-11)	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPN-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A Rif generator R&S SMT-06	ents the traceability to nati intainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292785 SN: 5056 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005 US37390585 S4206	robability are given on the following pages a y facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 237-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11) 18-Oct-01 (in house check Oct-12)	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-13
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPN-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	ents the traceability to nati intainties with confidence p ated in the closed laborator TE critical for calibration) ID # GB37480704 US37292785 SN: 5056 (20k) SN: 5056 (20k) SN: 5047.3 / 06327 SN: 3206 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name	Cal Date (Certificate No.)           01-Nov-12 (No. 217-01640)           01-Nov-12 (No. 217-01640)           04-Apr-13 (No. 217-01640)           04-Apr-13 (No. 217-01736)           04-Apr-13 (No. 217-01739)           28-Dec-12 (No. ES3-3205_Dec12)           25-Apr-13 (No. DAE4-601_Apr13)           Check Date (in house)           18-Oct-02 (in house check Oct-11)           04-Aug-99 (in house check Oct-11)           18-Oct-01 (in house check Oct-12)	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-13

Compliance Certification Services Inc. Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





s

C

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

### Glossarv:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

## Additional Documentation:

d) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D835V2-4d114\_Jul13

Page 2 of 8

Page op of 120

Date of Issue :January 26, 2015

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

## Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.8 ± 6 %	0.92 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	****	

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.41 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.50 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL SAR measured	condition 250 mW input power	1.58 W/kg

### **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.9 ± 6 %	1.00 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

#### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.44 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.53 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.61 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.32 W/kg ± 16.5 % (k=2)

Certificate No: D835V2-4d114\_Jul13

Page 3 of 8

rage or or 120

Date of Issue : January 26, 2015

## Appendix

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.1 Ω - 1.3 jΩ	
Return Loss	- 32.1 dB	

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.2 Ω - 3.0 μΩ	
Return Loss	- 29.1 dB	

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.399 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	June 29, 2010

Page 4 of 8

## Compliance Certification Services Inc. Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

## DASY5 Validation Report for Head TSL

Date: 30.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland


### DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d114

Communication System: UID 0 - CW ; Frequency: 835 MHz Medium parameters used: f = 835 MHz;  $\sigma = 0.92$  S/m;  $\varepsilon_r = 41.8$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(6.05, 6.05, 6.05); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013 .
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001 .
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 56.702 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 3.60 W/kg SAR(1 g) = 2.41 W/kg; SAR(10 g) = 1.58 W/kg Maximum value of SAR (measured) = 2.81 W/kg

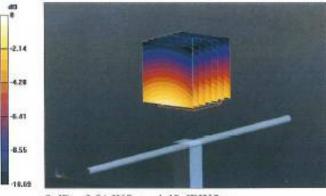


0 dB = 2.81 W/kg = 4.49 dBW/kg

Certificate No: D835V2-4d114\_Jul13

Page 5 of 8

Page 69 OF 126

Date of Issue :January 26, 2015

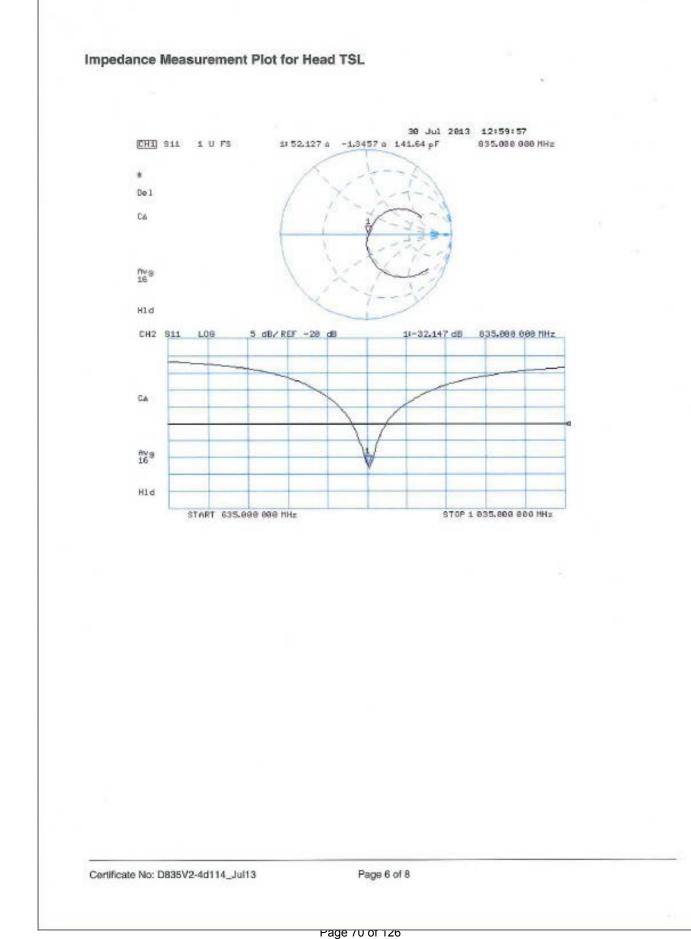

## Compliance Certification Services Inc. Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

## DASY5 Validation Report for Body TSL

Date: 22.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland


### DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d114

Communication System: UID 0 - CW ; Frequency: 835 MHz Medium parameters used: f = 835 MHz;  $\sigma = 1$  S/m;  $\varepsilon_r = 54.9$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(6.04, 6.04, 6.04); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 54.853 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 3.56 W/kg SAR(1 g) = 2.44 W/kg; SAR(10 g) = 1.61 W/kg Maximum value of SAR (measured) = 2.83 W/kg

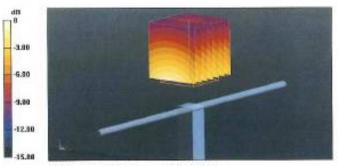

0 dB = 2.83 W/kg = 4.52 dBW/kg


Certificate No: D835V2-4d114\_Jul13

Page 7 of 8

Page / 1 01 120

# ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac Date of Issue :January 26, 2015

Impedance Measurement Plot for Body TSL

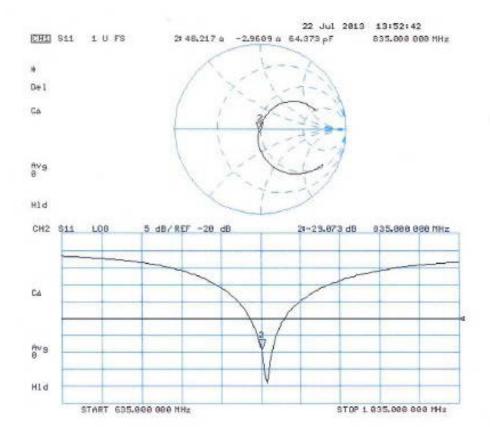

Certificate No: D835V2-4d114\_Jul13

Page 8 of 8

Date of Issue : January 26, 2015

## D835V2, Serial No.4d114 Extended Dipole Calibrations

Per IEEE Std 1528-2003, the dipole should have a return loss better than -20dB at the test frequency to reduce uncertainty in the power measurement

Per KDB 865664 D01, if dipoles are verified in return loss(<-20dB, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

## Justification of the extended calibration

		D850	V2 Serial No.4	d114		
			850 Head			
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (ohm)	Delta (ohm)
7.30.2013	-32.147		52.127		-1.346	
7.29.2014	-32.293	0.45	48.878	3.249	-2.134	0.788

		D850	V2 Serial No.4	d114		
			850 Body			
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (ohm)	Delta (ohm)
7.30.2013	-29.073		48.217		-2.961	
7.29.2014	-27.435	5.63	46.911	1.306	-2.689	0.272


The return loss is < -20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.


# Compliance Certification Services Inc. Report No: C141229S01-SF FCC ID: 2ABOSSKY55W Date of Issue :Jac

Date of Issue : January 26, 2015

## Dipole Verification Data D850V2 Serial No.4d114



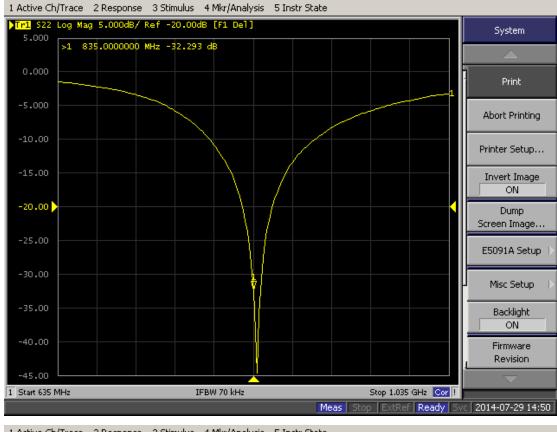


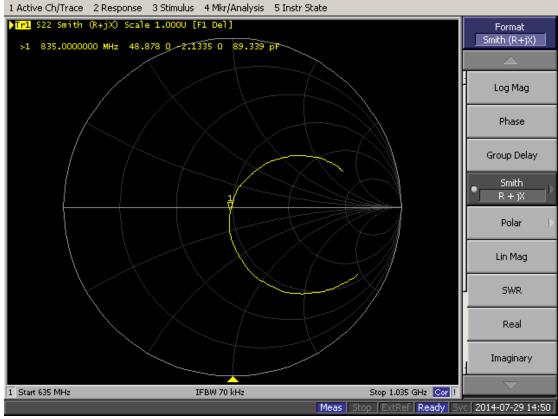


# Compliance Certification Services Inc. Report No: C141229S01-SF FCC ID: 2ABOSSKY55W Date of Issue : Jac

Date of Issue : January 26, 2015

## 850MHz-Body

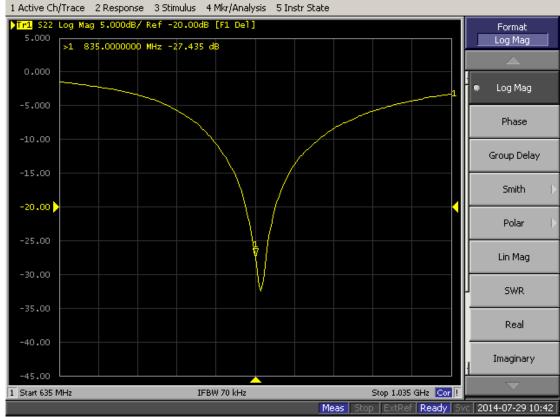

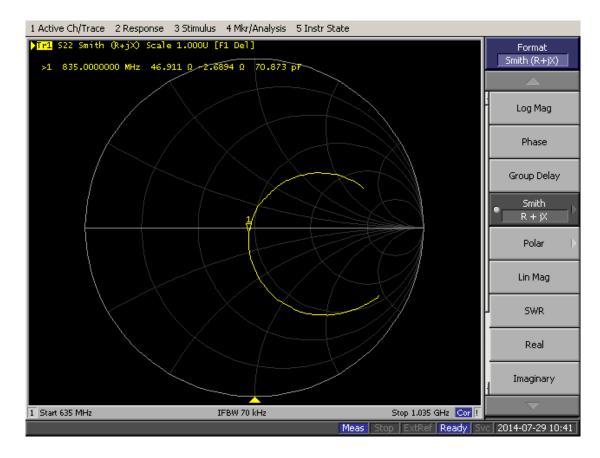

Calibration Laborator Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurict	i kanana H	BICHRA (Q T Z)	S Schweizerischer Kalibrierdie Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
Accredited by the Swiss Accredita The Swiss Accreditation Service Multilateral Agreement for the re	is one of the signatorie	s to the EA	on No.: SCS 108
client CCS-CN (Aude	<	119-21-010-122-2	No: D1800V2-2d170_Jul
CALIBRATION C	ERTIFICATE		
Object	D1800V2 - SN: 2	d170	
Calibration procedure(s)	QA CAL-05.v9 Calibration proce	dure for dipole validation kits al	bove 700 MHz
The measurements and the unce	rtainties with confidence p	onal standards, which realize the physical robability are given on the following pages ty facility: environment temperature (22 ± 3	and are part of the certificate.
This calibration certificate docum The measurements and the unce	ents the traceability to nati rtainties with confidence p sted in the closed laborato		and are part of the certificate.
This calibration certificate docum The measurements and the unce All calibrations have been conduc	ents the traceability to nati rtainties with confidence p sted in the closed laborato	robability are given on the following pages	and are part of the certificate.
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A	ents the traceability to nati rtainties with confidence p sted in the closed laborato FE critical for calibration) ID # GB37480704	robability are given on the following pages ry facility: environment temperature (22 ± 3 <u>Cal Date (Certificate No.)</u> 01-Nov-12 (No. 217-01640)	and are part of the certificate, i)°C and humidity < 70%, Scheduled Calibration Oct-13
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A	ents the traceability to nati rtainties with confidence p sted in the closed laborato FE critical for calibration) ID # GB37480704 US37292783	robability are given on the following pages ry facility: environment temperature (22 ± 3 <u>Cal Date (Certificate No.)</u> 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640)	and are part of the certificate, i)°C and humidity < 70%, Scheduled Calibration Oct-13 Oct-13
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A	ents the traceability to nati rtainties with confidence p sted in the closed laborato FE critical for calibration) ID # GB37480704	robability are given on the following pages ry facility: environment temperature (22 ± 3 <u>Cal Date (Certificate No.)</u> 01-Nov-12 (No. 217-01640)	and are part of the certificate. I)°C and humidity < 70%. Scheduled Calibration Oct-13
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attonuator Type-N mismatch combination Reference Probe ES3DV3	ents the traceability to nati rtainties with confidence p sted in the closed laborato FE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205	Cal Date (Certificate No.)           01-Nov-12 (No. 217-01840)           01-Nov-12 (No. 217-01640)           04-Apr-13 (No. 217-01736)           04-Apr-13 (No. 217-01739)           28-Dec-12 (No. ES3-3205_Dec12)	and are part of the certificate. I)°C and humidity < 70%. Scheduled Calibration Oci-13 Oci-13 Oci-13 Apr-14 Apr-14 Dec-13
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attonuator Type-N mismatch combination	ents the traceability to nati rtainties with confidence p sted in the closed laborato FE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327	robability are given on the following pages ry facility: environment temperature (22 ± 3 <u>Cal Date (Certificate No.)</u> 01-Nov-12 (No. 217-01840) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739)	and are part of the certificate. I)°C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attonuator Type-N mismatch combination Reference Probe ES3DV3	ents the traceability to nati rtainties with confidence p sted in the closed laborato FE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205	Cal Date (Certificate No.)           01-Nov-12 (No. 217-01840)           01-Nov-12 (No. 217-01640)           04-Apr-13 (No. 217-01736)           04-Apr-13 (No. 217-01739)           28-Dec-12 (No. ES3-3205_Dec12)	and are part of the certificate. I)°C and humidity < 70%. Scheduled Calibration Oci-13 Oci-13 Oci-13 Apr-14 Apr-14 Dec-13
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A	ents the traceability to nati rtainties with confidence p sted in the closed laborato IE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # MY41092317	robability are given on the following pages ty facility: environment temperature (22 ± 3 Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11)	and are part of the certificate. I)°C and humidity < 70%. Scheduled Calibration Oci-13 Oci-13 Oci-13 Apr-14 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attonuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards	ents the traceability to nati rtainties with confidence p sted in the closed laborato IE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5058 (20k) SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID #	robability are given on the following pages ry facility: environment temperature (22 ± 3 <u>Cal Date (Certificate No.)</u> 01-Nov-12 (No. 217-01840) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house)	and are part of the certificate. I)°C and humidity < 70%. Scheduled Calibration Oci-13 Oci-13 Oci-13 Apr-14 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Scheduled Check
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	ents the traceability to nati rtainties with confidence p sted in the closed laborato FE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 5047.3 / 06327 SN: 504 SN: 601 ID # MY41092317 100005	robability are given on the following pages ty facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-95 (in house check Oct-11)	and are part of the certificate. I)°C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Dec-13 Dec
This calibration certificate docum The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	ents the traceability to nati rtainties with confidence p sted in the closed laborato ID # GB37480704 US37292783 SN: 5056 (20k) SN: 5047.3 / 06327 SN: 5047.3 / 06327 SN: 5047.3 / 06327 SN: 5047.3 / 06327 SN: 601 ID # MY41092317 100005 US37390585 S4206	robability are given on the following pages by facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-95 (in house check Oct-11) 18-Oct-01 (in house check Oct-12) Function	and are part of the certificate. I)°C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-13
This calibration certificate docum The measurements and the unos All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	ents the traceability to nati rtainties with confidence p sted in the closed laborato PE critical for calibration) ID # GE37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name	robability are given on the following pages by facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-95 (in house check Oct-11) 18-Oct-01 (in house check Oct-12) Function	and are part of the certificate. I)°C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-13

Compliance Certification Services Inc.

G

FCC ID: 2ABOSSKY55W

Date of Issue :January 26, 2015

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Report No: C141229S01-SF



CRUSS CRUSRATT

s

C

S

Schweizerischer Kalibrierdienst

Service suisse d'étalonnege Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

## Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

## Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

## Additional Documentation:

d) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- · SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D1800V2-2d170\_Jul13

Page 2 of 8

Page // 01 120

Date of Issue :January 26, 2015

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1800 MHz ± 1 MHz	

## Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	$38.7\pm6~\%$	1.37 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.59 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	38.6 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL SAR measured	condition 250 mW input power	5.07 W/kg

## Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.4 ± 6 %	1.53 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.94 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	39.3 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 c) of Body TSL	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL SAR measured	condition 250 mW input power	5.25 W/kg

Certificate No: D1800V2-2d170\_Jul13

Page 3 of 8

Page / 8 of 126

Date of Issue : January 26, 2015

## Appendix

## Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.7 Ω - 3.3 jΩ	
Return Loss	- 29.5 dB	

1

## Antenna Parameters with Body TSL

Impedance, transformed to feed point	45.7 Ω - 3.4 jΩ
Return Loss	- 24.8 dB

## General Antenna Parameters and Design

Electrical Delay (one direction)	1.212 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

## Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	July 04, 2008	

Page 4 of 8

Page /9 01 120

## Compliance Certification Services Inc. Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

## DASY5 Validation Report for Head TSL

Date: 31.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland


DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d170

Communication System: UID 0 - CW; Frequency: 1800 MHz Medium parameters used: f = 1800 MHz;  $\sigma = 1.37 \text{ S/m}$ ;  $\varepsilon_r = 38.7$ ;  $\rho = 1000 \text{ kg/m}^3$ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63,19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(5.04, 5.04, 5.04); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection) .
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013 .
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164) .

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 94.137 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 17.2 W/kg SAR(1 g) = 9.59 W/kg; SAR(10 g) = 5.07 W/kg Maximum value of SAR (measured) = 11.9 W/kg

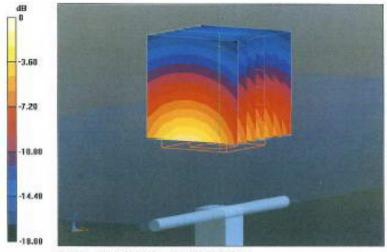

0 dB = 11.9 W/kg = 10.76 dBW/kg


Certificate No: D1800V2-2d170\_Jul13

Page 5 of 8

Page ou or 120

# ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue :January 26, 2015

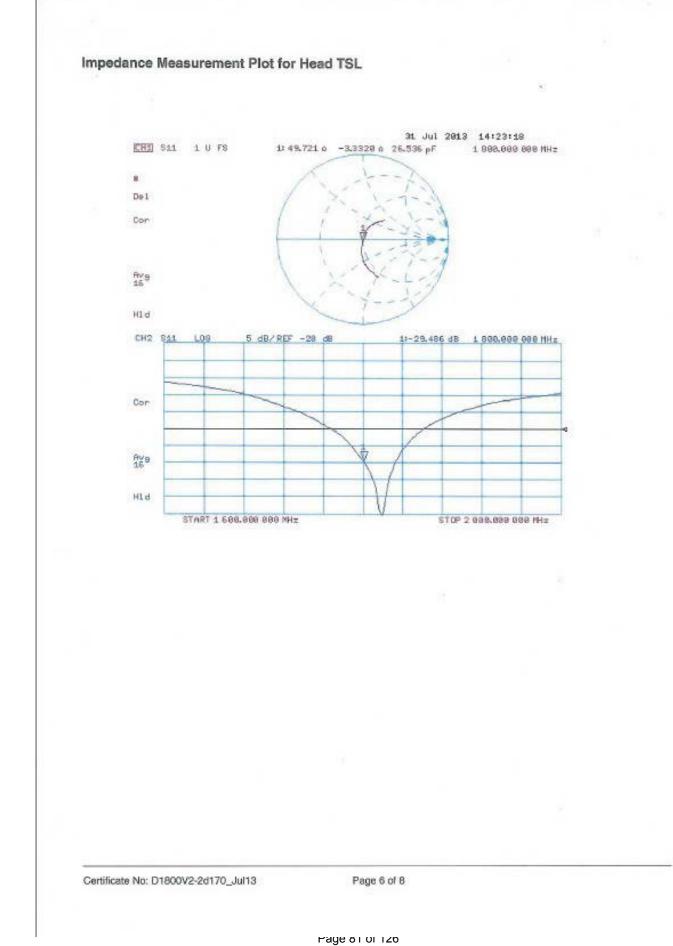

## Compliance Certification Services Inc. Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

Date: 31.07.2013

## DASY5 Validation Report for Body TSL

Test Laboratory: SPEAG, Zurich, Switzerland


## DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d170

Communication System: UID 0 - CW; Frequency: 1800 MHz Medium parameters used: f = 1800 MHz;  $\sigma = 1.53 \text{ S/m}$ ;  $\epsilon_r = 51.4$ ;  $\rho = 1000 \text{ kg/m}^3$ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- ٠ Probe: ES3DV3 - SN3205; ConvF(4.73, 4.73, 4.73); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 94.137 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 17.6 W/kg SAR(1 g) = 9.94 W/kg; SAR(10 g) = 5.25 W/kg Maximum value of SAR (measured) = 12.6 W/kg

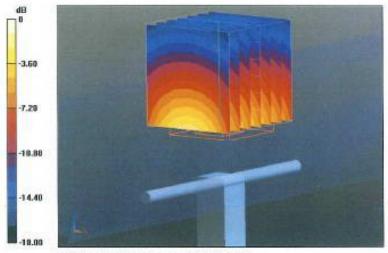

0 dB = 12.6 W/kg = 11.00 dBW/kg

Certificate No: D1800V2-2d170 Jul13


Page 7 of 8

Page 82 of 126

# ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue :January 26, 2015

## Impedance Measurement Plot for Body TSL

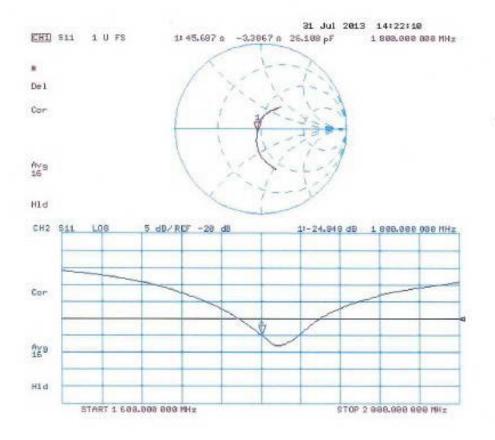

Certificate No: D1800V2-2d170\_Jul13

Page 8 of 8

rage os or 120

Date of Issue : January 26, 2015

## D1800V2, Serial No.2d170 Extended Dipole Calibrations

Per IEEE Std 1528-2003, the dipole should have a return loss better than -20dB at the test frequency to reduce uncertainty in the power measurement

Per KDB 865664 D01, if dipoles are verified in return loss(<-20dB, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Justification of the extended calibration

D1800V2 Serial No.2d170						
	1800 Head					
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (ohm)	Delta (ohm)
7.31.2013	-29.486		49.721		-3.332	
7.30.2014	-28.220	4.29	47.613	2.108	-2.974	0.358

D1800V2 Serial No.2d170						
	1800 Body					
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (ohm)	Delta (ohm)
7.31.2013	-24.848		45.687		-3.387	
7.30.2014	-24.010	3.37	44.951	0.736	-3.237	0.15


The return loss is < -20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.


# Compliance Certification Services Inc. Report No: C141229S01-SF FCC ID: 2ABOSSKY55W Date of Issue :Jac

Date of Issue : January 26, 2015

## Dipole Verification Data D1800V2 Serial No.2d170

## 1800MHz-Head

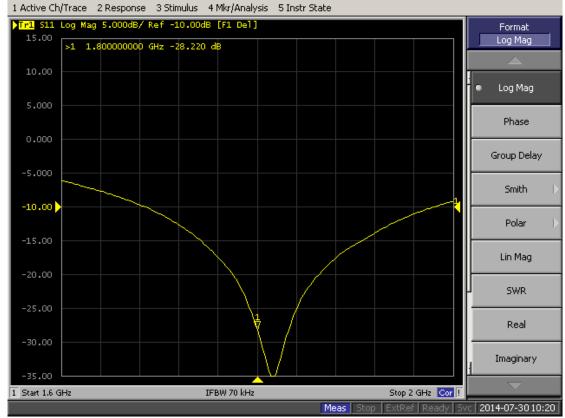


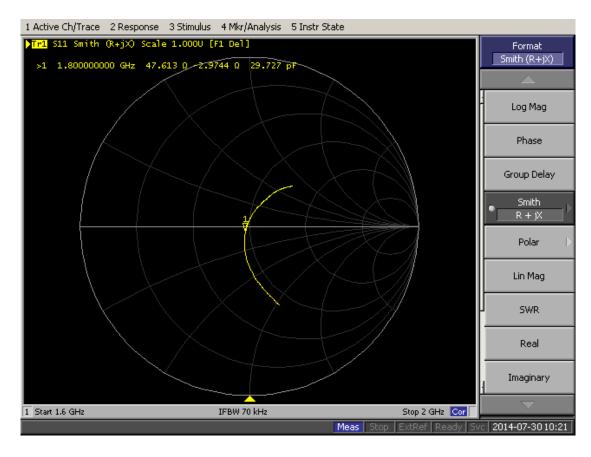


## Compliance Certification Services Inc. Report No: C141229S01-SF FCC ID: 2ABOSSKY55W Date of Issue 14 Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

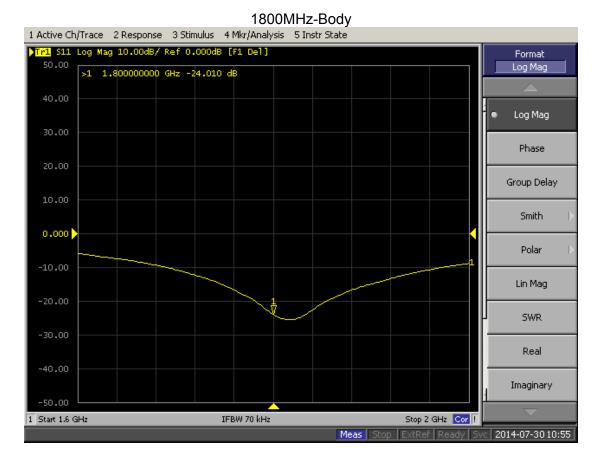

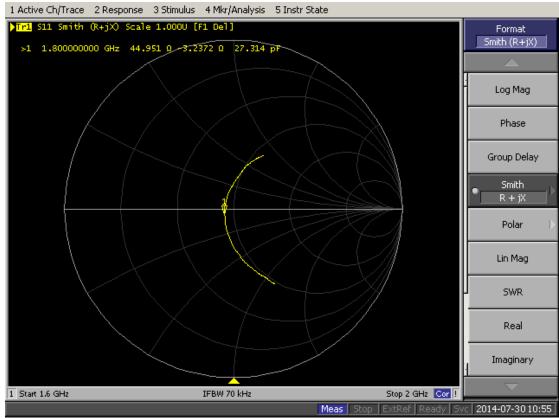

Calibration Laborator Schmid & Partner Engineering AG Coughousstrasse 43, 8004 Zuric		HAC MRA	Schweizerischer Kalibrierdien Service sulsse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
Accredited by the Swiss Accredita The Swiss Accreditation Servic Multilateral Agreement for the r	e is one of the signatorie	s to the EA	No.: SCS 108
Client CCS-CN (Aude			: D1900V2-5d136_Jul1
CALIBRATION (	CERTIFICATE		
Object	D1900V2 - SN: 5	d136	-
Calibration procedure(s)	QA CAL-05.v9 Calibration proce	dure for dipole validation kits abo	ove 700 MHz
Calibration date:	July 22, 2013		
This calibration certificate docum The measurements and the unco	rents the traceability to nati entainties with confidence p oted in the closed laborator	onal standards, which realize the physical ur robability are given on the following pages ar ry facility: environment temperature (22 ± 3) <sup>o</sup> Cal Date (Certificate No.)	nd are part of the certificate.
This calibration certificate docum The measurements and the unco All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A	nents the traceability to nati entainties with confidence p acted in the closed laborator TE critical for calibration) ID # GB37480704	robability are given on the following pages ar ny facility: environment temperature (22 ± 3) <sup>o</sup> Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-13
This calibration certificate docum The measurements and the unco All calibrations have been condu Calibration Equipment used (M& Primary Standards	nents the traceability to nati entainties with confidence p acted in the closed laborator TE critical for calibration)	robability are given on the following pages ar ry facility: environment temperature (22 ± 3) <sup>o</sup> Cal Date (Certificate No.)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8461A Reference 20 dB Attenuator Type-N mismatch combination	tents the traceability to nati entainties with confidence p acted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327	robability are given on the following pages ar ry facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8461A Reference 20 dB Attenuator	nents the traceability to nati entainties with confidence p acted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k)	robability are given on the following pages ar ry facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Deo-12 (No. ES3-3205_Dec12)	Ind are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4	ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5041	robability are given on the following pages ar ry facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 29-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13)	Ind are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards	tents the traceability to nati entainties with confidence p acted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5058 (20k) SN: 5047.3 / 06327 SN: 5047.3 / 06327 SN: 3205 SN: 601	robability are given on the following pages ar ry facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 29-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A	tents the traceability to nati entainties with confidence p acted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5058 (20k) SN: 5047.3 / 06327 SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # MY41092317	robability are given on the following pages ar ry facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Deo-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards	tents the traceability to nati entainties with confidence p acted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5058 (20k) SN: 5047.3 / 06327 SN: 5047.3 / 06327 SN: 3205 SN: 601	robability are given on the following pages ar ry facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 29-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& <u>Primary Standards</u> Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 <u>Secondary Standards</u> Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	nents the traceability to nati entainties with confidence p acted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name	robability are given on the following pages ar ty facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Nor-12 (No. 217-01640) 01-Nor-12 (No. 217-01640) 04-Apr-13 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11) 18-Oct-01 (in house check Oct-12) Function	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	nents the traceability to nati entainties with confidence p acted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005 US37390585 S4206	robability are given on the following pages ar ty facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Nor-12 (No. 217-01640) 01-Nor-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11) 18-Oct-01 (in house check Oct-12)	nd are part of the certificate. C and humidity < 70%. Cot+13 Oct+13 Oct+13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-13
This calibration certificate docum The measurements and the unco All calibrations have been condu Calibration Equipment used (M& <u>Primary Standards</u> Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by:	nents the traceability to nati entainties with confidence p acted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name Jeton Kastrati	robability are given on the following pages ar ty facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Nor-12 (No. 217-01640) 01-Nor-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11) 18-Oct-01 (in house check Oct-12) Function Laboratory Technician	nd are part of the certificate. C and humidity < 70%. Cot-13 Oct-13 Oct-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-13
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& <u>Primary Standards</u> Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 <u>Secondary Standards</u> Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	nents the traceability to nati entainties with confidence p acted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name	robability are given on the following pages ar ty facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Nor-12 (No. 217-01640) 01-Nor-12 (No. 217-01640) 04-Apr-13 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11) 18-Oct-01 (in house check Oct-12) Function	nd are part of the certificate. C and humidity < 70%. Cot-13 Oct-13 Oct-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-13

Compliance Certification Services Inc.

FCC ID: 2ABOSSKY55W Date of

Date of Issue :January 26, 2015

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Report No: C141229S01-SF



SNISS S C

Schweizerischer Kalibrierdienst

- Service suisse d'étalonnage
- Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service Is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

## Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

## Additional Documentation:

d) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- · SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D1900V2-5d136\_Jul13

Page 2 of 8

Page oo or 120

Date of Issue :January 26, 2015

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.9 ± 6 %	1.36 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.0 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.4 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>*</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.29 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 16.5 % (k=2)

## **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.4 ± 6 %	1.49 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

## SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.0 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	40.5 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.37 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.6 W/kg ± 16.5 % (k=2)

Certificate No: D1900V2-5d136\_Jul13

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

## Appendix

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.9 Ω + 7.2 jΩ	
Return Loss	- 22.5 dB	

## Antenna Parameters with Body TSL

Impedance, transformed to feed point	47.7 Ω + 7.3 jΩ
Return Loss	- 22.1 dB

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.203 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

## Additional EUT Data

Manufactured by	SPEAG
Manufactured on	April 14, 2010

Page 4 of 8

## Compliance Certification Services Inc. Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

## DASY5 Validation Report for Head TSL

Date: 22.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland

## DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d136


Communication System: UID 0 - CW ; Frequency: 1900 MHz Medium parameters used: f = 1900 MHz;  $\sigma = 1.36 \text{ S/m}$ ;  $\varepsilon_r = 38.9$ ;  $\rho = 1000 \text{ kg/m}^3$ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.98, 4.98, 4.98); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

## Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.803 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 18.1 W/kg SAR(1 g) = 10 W/kg; SAR(10 g) = 5.29 W/kg Maximum value of SAR (measured) = 12.4 W/kg

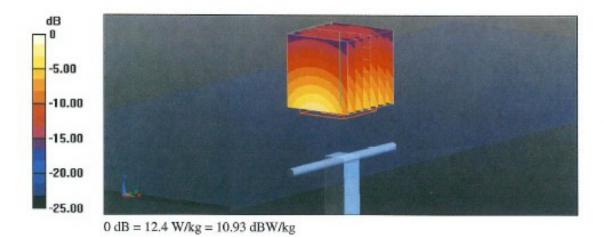


Certificate No: D1900V2-5d136\_Jul13

Page 5 of 8

Page 91 01 120

ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue :January 26, 2015

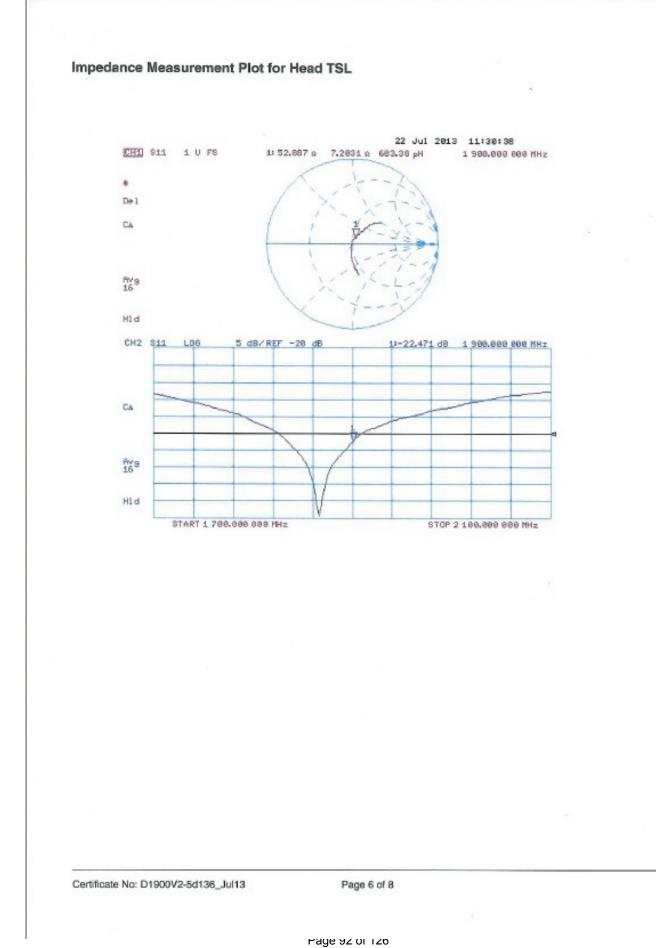

## **Compliance Certification Services Inc.** Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

Date: 22.07.2013

## DASY5 Validation Report for Body TSL

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d136


Communication System: UID 0 - CW ; Frequency: 1900 MHz Medium parameters used: f = 1900 MHz;  $\sigma = 1.49 \text{ S/m}$ ;  $\varepsilon_r = 53.4$ ;  $\rho = 1000 \text{ kg/m}^3$ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.6, 4.6, 4.6); Calibrated: 28.12.2012; .
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002 ٠
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

## Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.803 V/m; Power Drift = 0.00 dB Peak SAR (extrapolated) = 17.0 W/kg SAR(1 g) = 10 W/kg; SAR(10 g) = 5.37 W/kg Maximum value of SAR (measured) = 12.5 W/kg

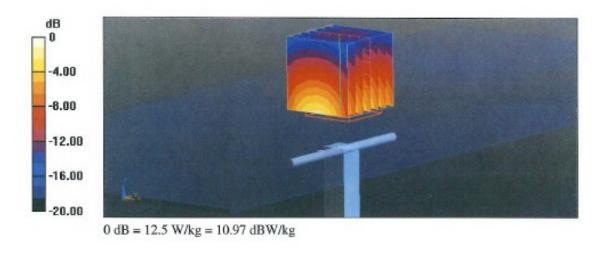


Certificate No: D1900V2-5d136\_Jul13

Page 7 of 8

Page 93 of 126

# Compliance Certification Services Inc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue :January 26, 2015

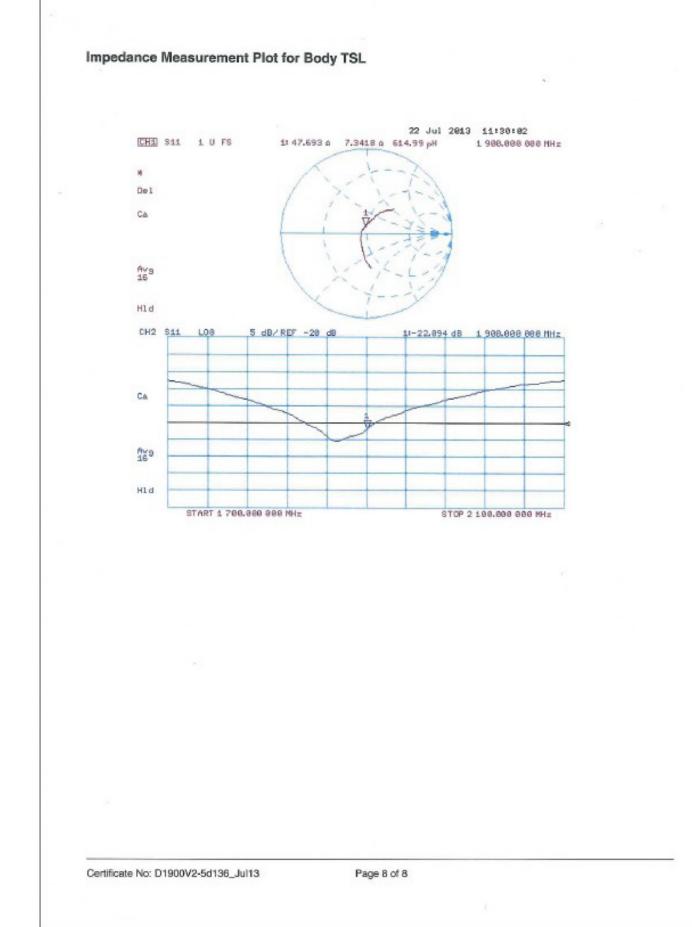

Page 94 0T 126

Date of Issue : January 26, 2015

## D1900V2, Serial No.5d136 Extended Dipole Calibrations

Per IEEE Std 1528-2003, the dipole should have a return loss better than -20dB at the test frequency to reduce uncertainty in the power measurement

Per KDB 865664 D01, if dipoles are verified in return loss(<-20dB, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

## Justification of the extended calibration

		D1900	V2 Serial No.	5d136		
1900 Head						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (ohm)	Delta (ohm)
7.22.2013	-22.471		52.887		7.2031	
7.21.2014	-23.930	6.49	51.667	1.22	6.2513	0.9518

		D1900	V2 Serial No.	5d136		
1900 Body						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (ohm)	Delta (ohm)
7.22.2013	-22.094		47.693		7.3418	
7.21.2014	-22.704	2.76	47.761	0.068	6.8096	0.5322


The return loss is < -20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.


# Compliance Certification Services Inc. Report No: C141229S01-SF FCC ID: 2ABOSSKY55W Date of Issue :Jabossky55W

Date of Issue : January 26, 2015

## Dipole Verification Data D1900V2 Serial No.5d136

## 1900MHz-Head

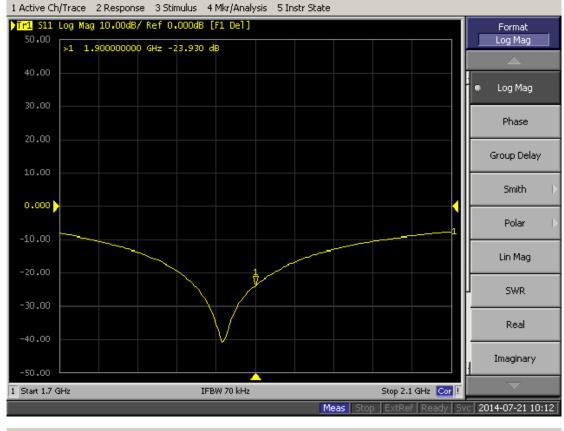


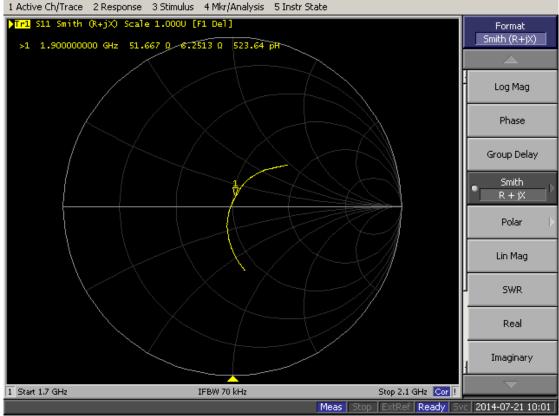


# Compliance Certification Services Inc. Report No: C141229S01-SF FCC ID: 2ABOSSKY55W Date of Issue :Jac

Date of Issue : January 26, 2015

## 1900MHz-Body

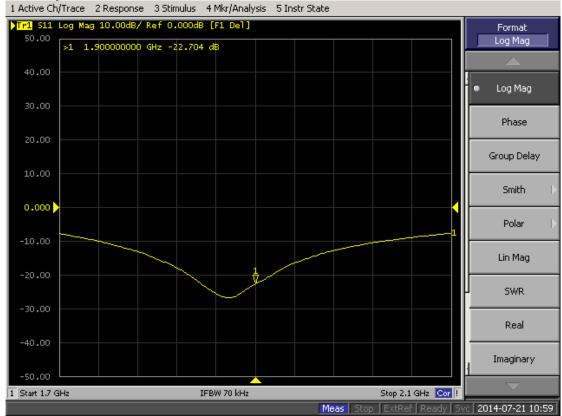

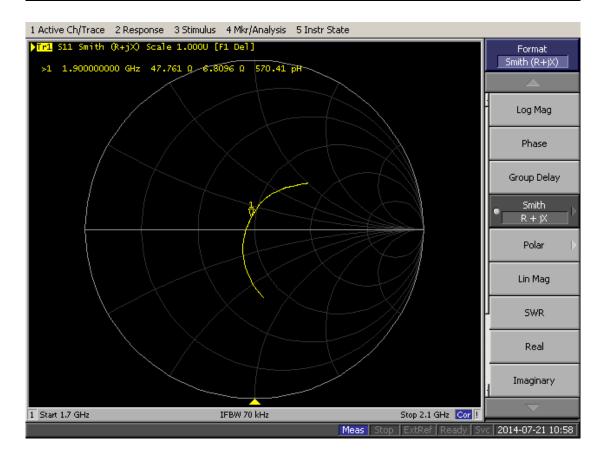

Page 97 of 126

Calibration Laborator Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zuric		HAC MEA	Servizio svizzero di taratura
Accredited by the Swiss Accredit The Swiss Accreditation Servic Multilateral Agreement for the r	e is one of the signatorie	s to the EA	n No.: SCS 108
Client CCS-CN (Aude	n)	Certificate N	lo: D2450V2-817_Jul13
CALIBRATION C	CERTIFICATE		
Object	D2450V2 - SN: 8	17	
Calibration procedure(s)	QA CAL-05.v9 Calibration proce	dure for dipole validation kits ab	ove 700 MHz
Calibration date:	July 31, 2013		
The measurements and the unce	ertainties with confidence p	onal standards, which realize the physical u robability are given on the following pages a ry facility: environment temperature (22 ± 3)	ind are part of the certificate.
The measurements and the unor All calibrations have been condu Calibration Equipment used (MS	etainties with confidence p cted in the closed laborato TE critical for calibration)	robability are given on the following pages a ry facility: environment temperature ( $22 \pm 3$ )	ind are part of the certificate.
The measurements and the unor All calibrations have been condu Calibration Equipment used (MS Primary Standards	etainties with confidence p cted in the closed laborator TE critical for calibration)	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.)	ind are part of the certificate. °C and humidity < 70%. Scheduled Calibration
The measurements and the unor All calibrations have been condu Calibration Equipment used (MS	etainties with confidence p cted in the closed laborato TE critical for calibration)	robability are given on the following pages a ry facility: environment temperature ( $22 \pm 3$ )	ind are part of the certificate.
The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	etainties with confidence p cted in the closed laborator TE critical for calibration) ID # QB37480704 US37292783 SN: 5058 (20k)	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736)	Ind are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13
The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination	etainties with confidence p cted in the closed laborator TE critical for calibration) ID # QB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739)	Ind are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14
The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	etainties with confidence p cted in the closed laborator TE critical for calibration) ID # QB37480704 US37292783 SN: 5058 (20k)	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736)	Ind are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14
The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4	etainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 U537292783 SN: 5058 (20k) SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 501	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13)	Ind are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-18 Oct-18 Oct-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14
The measurements and the unce All calibrations have been condu Calibration Equipment used (MS Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID #	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house)	Ind are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check
The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4	etainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 U537292783 SN: 5058 (20k) SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 501	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13)	Ind are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14
The measurements and the unor All calibrations have been condu Calibration Equipment used (MS Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 3205 SN: 601 ID # MY41092317	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11)	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14 Dec-13 Apr-14
The measurements and the unor All calibrations have been condu Calibration Equipment used (MS Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	etainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 505	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-12) Function	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Oct-13 Apr-14 Dec-13 Apr-14 Apr-1
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	etainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 505	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-12)	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-18 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-13
The measurements and the unor All calibrations have been condu Calibration Equipment used (MS Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	etainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5058 (20k) SN: 505	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-12) Function	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-18 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-13
The measurements and the unce All calibrations have been condu Calibration Equipment used (MS Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by: Approved by:	etainties with confidence p cted in the closed laborator TE critical for calibration) ID # QB37480704 US37292783 SN: 5058 (20k) SN: 5057 (20k) SN: 5058 (20k) SN: 505	robability are given on the following pages a ry facility: environment temperature (22 ± 3) Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11) 18-Oct-01 (in house check Oct-12) Function Laboratory Technician	and are part of the certificate. *C and humidity < 70%. Scheduled Calibration Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-13 Signature Mrau CI-Dae Mrau CI-Dae Marana

Compliance Certification Services Inc.

FCC ID: 2ABOSSKY55W Date of Issue :January 26, 2015

S

C

NIS

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Report No: C141229S01-SF



Schweizerlacher Kalibrierdienst Service suisse d'étalonnece

- Service suisse d'etalonnage Servizio svizzero di taratura
- Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

## Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

## Additional Documentation:

d) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- · SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-817\_Jul13

Page 2 of 8

наде ээ ог izo

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.8 ± 6 %	1.81 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.3 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.6 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL SAR measured	condition 250 mW input power	6.18 W/kg

## Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	50.5 ± 6 %	2.01 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	****	

### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition		
SAR measured	250 mW input power	12.6 W/kg	
SAR for nominal Body TSL parameters	normalized to 1W	49.2 W/kg ± 17.0 % (k=2)	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition		
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL SAR measured	condition 250 mW input power	5.87 W/kg	

Certificate No: D2450V2-817\_Jul13

Page 3 of 8

Page 100 of 120

FCC ID: 2ABOSSKY55W

### Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.5 Ω + 2.9 jΩ		
Return Loss	- 27.1 dB		

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.7 Ω + 4.5 jΩ
Return Loss	- 27.0 dB

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.159 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions' paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG		
Manufactured on	October 23, 2007		

Page 4 of 8

#### Compliance Certification Services Inc. Report No: C141229S01-SF Date of Issue : January 26, 2015

FCC ID: 2ABOSSKY55W

## DASY5 Validation Report for Head TSL

Date: 31.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland


### DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817

Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz;  $\sigma = 1.81 \text{ S/m}$ ;  $\varepsilon_r = 37.8$ ;  $\rho = 1000 \text{ kg/m}^3$ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63,19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.52, 4.52, 4.52); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013 .
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164) .

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 99.781 V/m; Power Drift = 0.06 dB Peak SAR (extrapolated) = 27.7 W/kg SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.18 W/kg Maximum value of SAR (measured) = 16.8 W/kg

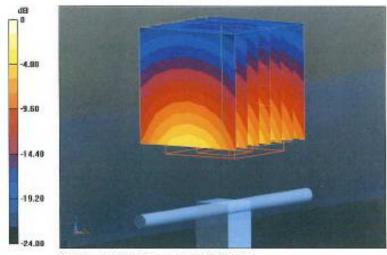

0 dB = 16.8 W/kg = 12.25 dBW/kg

Certificate No: D2450V2-817\_Jul13


Page 5 of 8

Page 102 OT 120

# ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue :January 26, 2015

## Impedance Measurement Plot for Head TSL

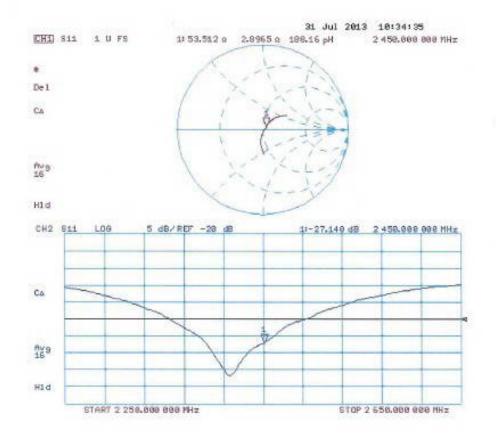

Certificate No: D2450V2-817\_Jul13

Page 6 of 8

Page 103 of 126

## Compliance Certification Services Inc. Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

## DASY5 Validation Report for Body TSL

Date: 31.07.2013

Test Laboratory: SPEAG, Zurich, Switzerland


## DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817

Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz;  $\sigma = 2.01 \text{ S/m}$ ;  $\epsilon_r = 50.5$ ;  $\rho = 1000 \text{ kg/m}^3$ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63,19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.42, 4.42, 4.42); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164) .

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 94.151 V/m; Power Drift = 0.06 dB Peak SAR (extrapolated) = 26.3 W/kg SAR(1 g) = 12.6 W/kg; SAR(10 g) = 5.87 W/kg Maximum value of SAR (measured) = 16.7 W/kg

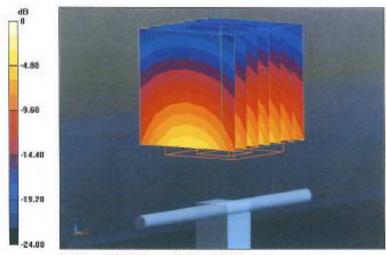

0 dB = 16.7 W/kg = 12.23 dBW/kg


Certificate No: D2450V2-817\_Jul13

Page 7 of 8

Page 104 of 126

## ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac Date of Issue :January 26, 2015

Impedance Measurement Plot for Body TSL

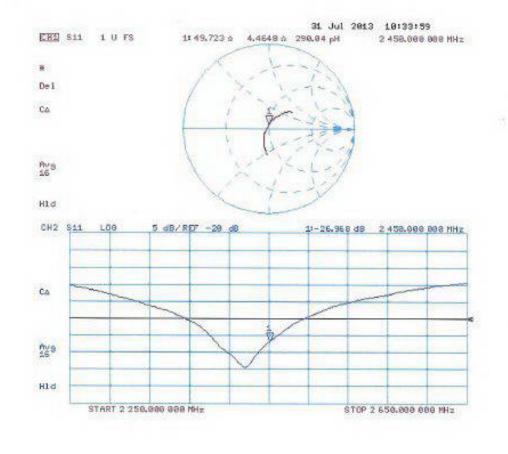

Certificate No: D2450V2-817\_Jui13

Page 8 of 8

Page 105 OF 120

Date of Issue : January 26, 2015

## D2450V2, Serial No.817 Extended Dipole Calibrations

Per IEEE Std 1528-2003, the dipole should have a return loss better than -20dB at the test frequency to reduce uncertainty in the power measurement.

Per KDB 865664 D01, if dipoles are verified in return loss(<-20dB, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

## Justification of the extended calibration

D2450V2 Serial No.817						
2450 Head						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (ohm)	Delta (ohm)
7.31.2013	-27.140		53.512		2.897	
7.30.2014	-26.620	1.92	52.828	0.684	3.898	0.911

D2450V2 Serial No.817						
2450 Body						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (ohm)	Delta (ohm)
7.31.2013	-26.968		49.723		4.465	
7.30.2014	-25.469	5.56	49.237	0.486	5.234	0.769


The return loss is < -20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.


# Compliance Certification Services Inc. Report No: C141229S01-SF FCC ID: 2ABOSSKY55W Date of Issue :Jabossky55W

Date of Issue : January 26, 2015

## Dipole Verification Data D2450V2 Serial No.817

## 2450 MHz-Head

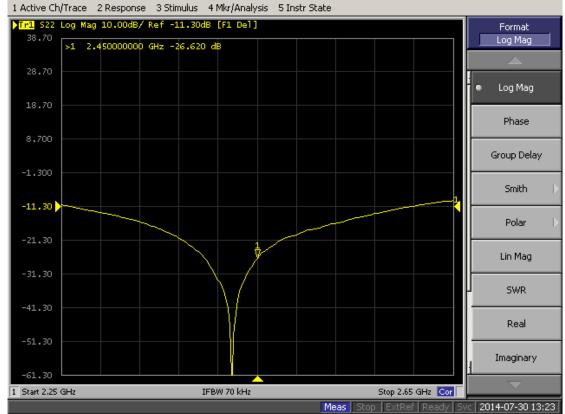


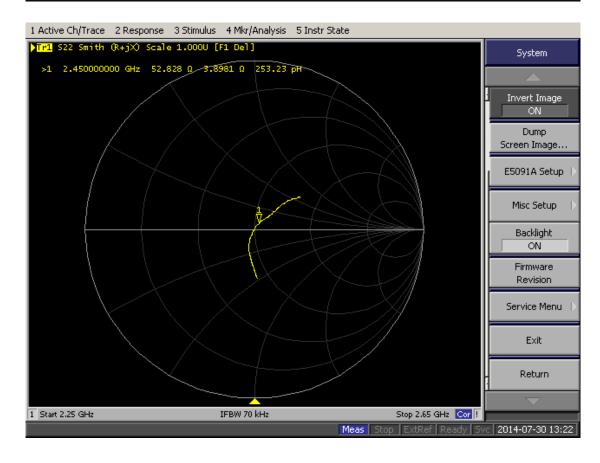


# Compliance Certification Services Inc. Report No: C141229S01-SF FCC ID: 2ABOSSKY55W Date of Issue : Jac

Date of Issue : January 26, 2015

## 2450 MHz-Body

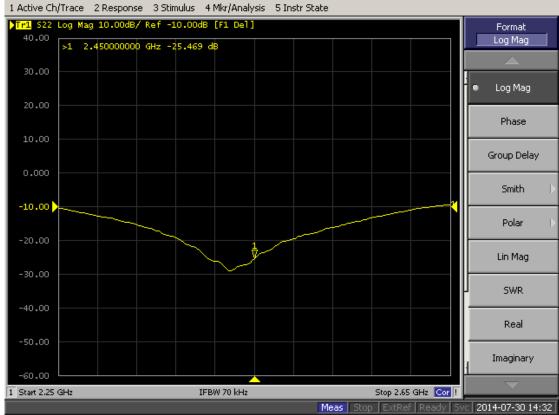

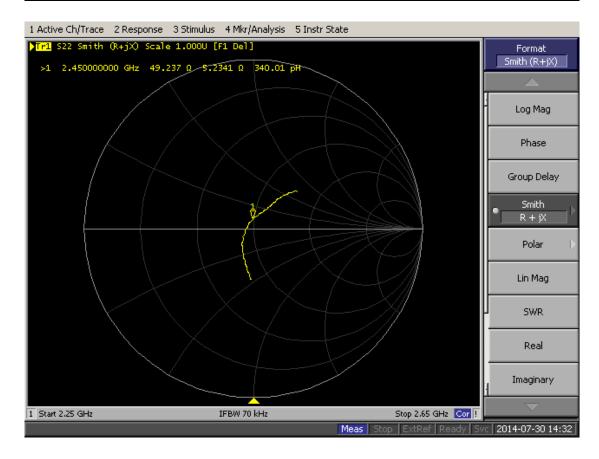

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

Schmid & Partner Engineering AG

Report No: C141229S01-SF

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 info@speag.com, http://www.speag.com

## IMPORTANT NOTICE

s

e

а

#### USAGE OF THE DAE 4

The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:

Battery Exchange: The battery cover of the DAE4 unit is closed using a screw, over tightening the screw may cause the threads inside the DAE to wear out.

Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an antistatic bag. This antistatic bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.

E-Stop Failures: Touch detection may be maifunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements.

Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect.

DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file.

#### Important Note:

Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer.

#### Important Note:

Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the Estop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure.

#### Important Note:

To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.

Schmid & Partner Engineering

TN\_BR040315AD DAE4.doc

11.12.2009

Page 109 of 126

Calibration Laboratory Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich		HAC MEA CROREND S	Schweizerischer Kalibrierdiens Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
Accredited by the Swiss Accreditat The Swiss Accreditation Service Multilateral Agreement for the re	is one of the signatories	to the EA	No.: SCS 108
Client CCS-CN (Aude			»: DAE4-1245_Jul14
CALIBRATION C	ERTIFICATE		
Object	DAE4 - SD 000 D	04 BM - SN: 1245	
Calibration procedure(s)	QA CAL-06.v26 Calibration proces	dure for the data acquisition elec	stronics (DAE)
Calibration date:	July 22, 2014		
The measurements and the uncer	tainties with confidence pr	nal standards, which realize the physical un obability are given on the following pages ar r facility: environment temperature (22 ± 3) <sup>o</sup>	d are part of the certificate.
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T	tainties with confidence protect in the closed laboratory E critical for calibration)	obability are given on the following pages ar y facility: environment temperature (22 ± 3) <sup>c</sup> )	nd are part of the certificate. C and humidity < 70%.
The measurements and the uncer All calibrations have been conduc	tainlifes with confidence protection of the closed laboratory	obability are given on the following pages ar	d are part of the certificate.
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards	tainties with confidence protection in the closed laboratory E critical for calibration) ID # SN: 0810278 ID # SE UWS 053 AA 1001	obability are given on the following pages ar y facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Oct-13 (No:13976) Check Date (in house)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T Primary Standards Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit Calibrator Box V2.1	tainties with confidence protection in the closed laboratory E critical for calibration) ID # SN: 0810278 ID # SE UWS 053 AA 1001 SE UMS 006 AA 1002 Name	obability are given on the following pages an (facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Oct-13 (No:13976) Check Date (in house) 07-Jan-14 (in house check) 07-Jan-14 (in house check) Function	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-14 Scheduled Check In house check: Jan-15 In house check: Jan-15
The measurements and the uncer All calibrations have been conduct Calibration Equipment used (M&T Primary Standards Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit	tainties with confidence protect in the closed laboratory E critical for calibration) ID # SN: 0810278 ID # SE UWS 053 AA 1001 SE UMS 006 AA 1002	obability are given on the following pages an (facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Oct-13 (No:13976) Check Date (in house) 07-Jan-14 (in house check) 07-Jan-14 (in house check)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-14 Scheduled Check In house check: Jan-15 In house check: Jan-15 In house check: Jan-15
The measurements and the uncer All calibrations have been conduct Calibration Equipment used (M&T Primary Standards Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit Calibrator Box V2.1	tainties with confidence protection in the closed laboratory E critical for calibration) ID # SN: 0810278 ID # SE UWS 053 AA 1001 SE UMS 006 AA 1002 Name	obability are given on the following pages an (facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Oct-13 (No:13976) Check Date (in house) 07-Jan-14 (in house check) 07-Jan-14 (in house check) Function	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-14 Scheduled Check In house check: Jan-15 In house check: Jan-15
The measurements and the uncer All calibrations have been conduc Calibration Equipment used (M&T <u>Primary Standards</u> Keithley Multimeter Type 2001 <u>Secondary Standards</u> Auto DAE Calibration Unit Calibrator Bex V2.1	tainties with confidence protect in the closed laboratory E critical for calibration) ID # SN: 0610276 ID # SE UWS 053 AA 1001 SE UWS 055 AA 1002 Name R Mayoraz Fin Bomholt	obability are given on the following pages an (facility: environment temperature (22 ± 3) <sup>4</sup> Cal Date (Certificate No.) 01-Oct-13 (No:13876) Check Date (in house) 07-Jan-14 (in house check) 07-Jan-14 (in house check) Function Technician	Ad are part of the certificate. C and humidity < 70%. <u>Scheduled Calibration</u> Oct-14 <u>Scheduled Check</u> In house check: Jan-15 In house check: Jan-15 Signature <i>Editypy</i> <i>i.v. Job Ulf</i> Issued: July 22, 2014

Compliance Certification Services Inc. Report No: C141229S01-SF

FCC ID: 2ABOSSKY55W

Date of Issue : January 26, 2015

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst s Service suisse d'étalonnage C Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary

DAE Connector angle

data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

#### Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a . result from the performance test and require no uncertainty.
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of . the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on • the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an . input voltage.
  - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-1245 Jul14

Page 2 of 5

Page 111 of 126

Date of Issue :January 26, 2015

### **DC Voltage Measurement**

A/D - Converter Reso	lution nominal			
High Range:	1LSB =	6.1µV,	full range =	-100+300 mV
Low Range:	1LSB =	61nV ,	full range =	-1+3mV
DASY measurement	parameters: Aut	to Zero Time: 3	sec; Measuring	time: 3 sec

Calibration Factors	x	Y	z
High Range	405.988 ± 0.02% (k=2)	404.710 ± 0.02% (k=2)	405.849 ± 0.02% (k=2)
Low Range	4.00335 ± 1.50% (k=2)	3.98492 ± 1.50% (k=2)	4.02547 ± 1.50% (k=2)

#### **Connector Angle**

Connector Angle to be used in DASY system	30.5 ° ± 1 °

Certificate No: DAE4-1245\_Jul14

Page 3 of 5

ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue :January 26, 2015

#### Appendix (Additional assessments outside the scope of SCS108)

#### 1. DC Voltage Linearity

High Range		Reading (µV)	Difference (µV)	Error (%)
Channel X	+ Input	199996.75	-0.27	-0.00
Channel X	+ Input	20001.39	1.15	0.01
Channel X	- Input	-20000.78	0.74	-0.00
Channel Y	+ Input	199998.13	1.27	0.00
Channel Y	+ Input	20000.37	0.12	0.00
Channel Y	- Input	-20002.24	-0.66	0.00
Channel Z	+ Input	199998.24	1.21	0.00
Channel Z	+ Input	20000.36	0.20	0.00
Channel Z	- Input	-20001.75	-0.03	0.00

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	2000.33	-0.09	-0.00
Channel X + Input	200.90	0.40	0.20
Channel X - Input	-198.83	0.46	-0.23
Channel Y + Input	2000.00	-0.26	-0.01
Channel Y + Input	199.61	-0.91	-0.45
Channel Y - Input	-200.08	-0.81	0.41
Channel Z + Input	2001.30	1.40	0.07
Channel Z + Input	200.05	-0.31	-0.15
Channel Z - Input	-200.89	-1.31	0.66

#### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Ingut Voltage (mV)	High Range Average Reading (µV)	Low Range Average Reading (µV)
Channel X	200	-7.83	-9.32
	- 200	10.88	9.44
Channel Y	200	-7.71	-8.33
	- 200	5.77	5.63
Channel Z	200	-5.90	-5.96
	- 200	4.79	4.74

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200		2.85	-2.60
Channel Y	200	9.53		4.34
Channel Z	200	9.98	6.64	-

Certificate No: DAE4-1245\_Jul14

Page 4 of 5

15939

Date of Issue : January 26, 2015

16860

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec High Range (LSB) Low Range (LSB) Channel X 15875 16740 Channel Y 16455 16504

#### 5. Input Offset Measurement

Channel Z

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input 10MΩ

	Average (µV)	min. Offset (µV)	max. Offset (µV)	Std. Deviation (µV)
Channel X	1.16	-0.50	2.34	0.49
Channel Y	-0.81	-2.25	0.40	0.49
Channel Z	-0.59	-1.82	0.83	0.56

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

#### 8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

#### 9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

	1-SF FCC		
Calibration Laborator Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zuric		BOCHEA CONSS S CONSS S CONSS S CONSS S	Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
Accredited by the Swiss Accredita The Swiss Accreditation Servic Multilateral Agreement for the r	e is one of the signatorie	s to the EA	Io.: SCS 108
Client CCS-CN (Aude	in)	Certificate No:	EX3-3798_Jul14
CALIBRATION	CERTIFICATI	E	and the second second
Object	EX3DV4 - SN:37	'98	Contraction of the
Calibration procedure(s)		DA CAL-14.v4, QA CAL-23.v5, QA edure for dosimetric E-field probes	CAL-25.v6
-			
		ional standaids, which realize the physical units robability are given on the following pages and	
This calibration certificate docum The measurements and the uno	ents the traceability to nat artainties with confidence p cted in the closed laborato		are part of the certificate.
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M&	ents the traceability to nat artainties with confidence p cted in the closed laborato TE critical for calibration)	vobability are given on the following pages and ny facility: environment temperature (22 ± 3)°C	are part of the certificate. and humidity < 70%.
This calibration certificate docum The measurements and the unor All calibrations have been condu	ents the traceability to nat artainties with confidence p cted in the closed laborato	robability are given on the following pages and	are part of the certificate.
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards	ents the traceability to nat artainties with confidence p cted in the closed laborato TE critical for calibration)	robability are given on the following pages and ry facility: environment temperature (22 ± 3)*C Cal Date (Certificate No.)	are part of the certificate. and humidity < 70%. Scheduled Calibration
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198	ents the traceability to nat artainties with confidence p cted in the closed laborato TE critical for calibration) ID GB41293874	Cal Date (Certificate No.) 03-Apr-14 (No. 217-01911)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter E44198 Power sensor E44198 Reference 3 dB Attenuator Reference 3 dB Attenuator	ents the traceability to nat attainties with confidence p cted in the closed laborato TE critical for calibration) ID GB41293874 MY41496087 SN: S5054 (3c) SN: S5277 (20x)	cobability are given on the following pages and ry facility: environment temperature (22 ± 3)*C           Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01919)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator	ents the traceability to nat attainties with confidence p cted in the closed laborato TE critical for calibration) ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5277 (20x) SN: S5129 (30b)	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Apr-15
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power mater E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2	tents the traceability to nat attainties with confidence p cted in the closed laborato TE critical for calibration) GB41293874 MY41496087 SN: S5054 (3c) SN: S5054 (3c) SN: S5277 (20x) SN: S5129 (30b) SN: 3013	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-13 (No. ES3-3013_Dec13)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Dec-14
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator	ents the traceability to nat attainties with confidence p cted in the closed laborato TE critical for calibration) ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5277 (20x) SN: S5129 (30b)	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Apr-15
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power mater E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2	tents the traceability to nat attainties with confidence p cted in the closed laborato TE critical for calibration) GB41293874 MY41496087 SN: S5054 (3c) SN: S5054 (3c) SN: S5277 (20x) SN: S5129 (30b) SN: 3013	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-13 (No. ES3-3013_Dec13)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Dec-14
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ents the traceability to nat attainties with confidence p cted in the closed laborato TE critical for calibration) ID GB41293874 MY4149087 SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: 3013 SN: 660	Cal Date (Certificate No.) Cal Date (Certificate No.) 03-Apr-14 (No. 217-01911) 03-Apr-14 (No. 217-01911) 03-Apr-14 (No. 217-01915) 03-Apr-14 (No. 217-01915) 03-Apr-14 (No. 217-01919) 03-Apr-14 (No. 217-01920) 30-Dec-13 (No. ES3-3013_Dec13) 13-Dec-13 (No. DAE4-660_Dec13)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Dec-14 Dec-14
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E44194 Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES30V2 DAE4	ents the traceability to nat attainties with confidence p cted in the closed laborato TE critical for calibration) ID G841293874 MY41498087 SN: 55064 (3c) SN: 55064 (3c) SN: 55129 (30b) SN: 3013 SN: 660 ID	Cal Date (Certificate No.) Cal Date (Certificate No.) 03-Apt-14 (No. 217-01911) 03-Apt-14 (No. 217-01911) 03-Apt-14 (No. 217-01915) 03-Apt-14 (No. 217-01915) 03-Apt-14 (No. 217-01919) 03-Apt-14 (No. 217-01919) 03-Apt-14 (No. 217-01920) 30-Dec-13 (No. ES3-3013_Dec13) 13-Dec-13 (No. DAE4-660_Dec13) Check Date (in house)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Dec-14 Dec-14 Scheduled Check
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E44194 Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 90 dB Attenuator Reference Probe ES30V2 DAE4 Secondary Standards RF generator HP 9648C	ents the traceability to nat artainties with confidence p cted in the closed laborato TE critical for calibration) ID GB41293874 MY41496087 SN: 55064 (3c) SN: 55054 (3c) SN: 55129 (30b) SN:	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01920)           03-Apr-14 (No. 217-01920)           03-Apr-14 (No. 217-01920)           03-Apr-13 (No. ES3-3013_Dec13)           13-Dac-13 (No. DAE4-660_Dec13)           13-Dac-13 (No. DAE4-660_Dec13)           18-Oct-01 (in house check Apr-13)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Dec-14 Dec-14 Scheduled Check In house check: Oct-14
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E44194 Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 90 dB Attenuator Reference Probe ES30V2 DAE4 Secondary Standards RF generator HP 9648C	ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: 3013 SN: 660 ID US3642001700	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-13 (No. EB3-3013_Dec13)           13-Dac-13 (No. DAE4-660_Dec13)           Check Date (in house)           4-Aug-99 (in house check Apr-13)	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Dec-14 Dec-14 Scheduled Check In house check: Apr-16
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 \$econdary Standards RF generator HP 9648C Network Analyzer HP 8753E	ents the traceability to nat attainties with confidence p cted in the closed laborato TE critical for calibration) ID GB41293874 MY41496087 SN: 55054 (3c) SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 3013 SN: 660 ID US3642U01700 US37390585 Name	Cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01920)           90-Dec-13 (No. ES3-3013_Dec13)           13-Dec-13 (No. DAE4-660_Dec13)           04-Aug-99 (in house)           4-Aug-99 (in house check Apr-13)           18-Oct-01 (in house check Apr-13)           Function	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Dec-14 Dec-14 Scheduled Check In house check: Oct-14
This calibration certificate docum The measurements and the unor All calibrations have been condu Calibration Equipment used (M& Primary Standards Power mater E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 90 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E Calibrated by:	ents the traceability to nat attainties with confidence p cted in the closed laborato TE critical for calibration) G6841293874 MY41498087 SN: S5064 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: S5129 (30b) SN: 3013 SN: 660 ID US3642U01700 US3642U01700 US37390585 Name Claudio Lauther	cal Date (Certificate No.)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01911)           03-Apr-14 (No. 217-01915)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01919)           03-Apr-14 (No. 217-01920)           30-Dec-13 (No. ES3-3013_Dec13)           13-Dec-13 (No. DAE4-660_Dec13)           18-Oct-01 (in house check Apr-13)           18-Oct-01 (in house check Apr-13)           Eunction           Laboratory Technician	are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Apr-15 Dec-14 Dec-14 Scheduled Check In house check: Oct-14

Certificate No: EX3-3798\_Jul14

Page 1 of 11

Compliance Certification Services Inc.

FCC ID: 2ABOSSKY55W

Date of Issue :January 26, 2015

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Report No: C141229S01-SF



Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

s

C

s

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx, y.z
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization @	o rotation around probe axis
Polarization 3	9 rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., 9 = 0 is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

#### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques\*, June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 8 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz; R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This linearization is
  implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
  in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z; A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical lsotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom
  exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: EX3-3798\_Jul14

Page 2 of 11

Page 116 of 126



## ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Jac

Date of Issue : January 26, 2015

EX3DV4 - SN:3798

July 28, 2014

# Probe EX3DV4

## SN:3798

Manufactured: April 5, 2011 Calibrated:

July 28, 2014

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: EX3-3798\_Jul14

Page 3 of 11

Date of Issue : January 26, 2015

EX3DV4- SN:3798

July 28, 2014

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3798

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m) <sup>2</sup> ) <sup>A</sup>	0.54	0.51	0.59	± 10.1 %
DCP (mV) <sup>®</sup>	97.6	99.3	96.2	

#### **Modulation Calibration Parameters**

UID	Communication System Name		A dB	B dBõV	С	D dB	VR mV	Unc <sup>E</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	145.7	\$2.7 %
		Y	0.0	0.0	1.0	1000000	142.0	-
		Z	0.0	0.0	1.0		132.7	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>6</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).
<sup>6</sup> Numerical linearization parameter: uncertainty not required.
<sup>6</sup> Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the section. field value.

Certificate No: EX3-3798\_Jul14

Page 4 of 11

Date of Issue : January 26, 2015

EX3DV4-SN:3798

#### July 28, 2014

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3798

f (MHz) <sup>c</sup>	Relative Permittivity	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>C</sup> (mm)	Unct. (k=2)
835	41.5	0.90	9.30	9.30	9.30	0.28	1.12	± 12.0 %
900	41.5	0.97	9.13	9.13	9.13	0.58	0.68	± 12.0 %
1810	40.0	1.40	7.82	7.82	7.82	0.41	0.81	± 12.0 %
1900	40.0	1.40	7.75	7.75	7.75	0.40	0.83	± 12.0 %
2450	39.2	1.80	7.04	7.04	7.04	0.33	0.92	± 12.0 %
5200	36.0	4.66	4.81	4.81	4.81	0.40	1.80	± 13.1 %
5300	35.9	4.76	4.60	4.60	4.60	0.40	1.80	± 13.1 %
5500	35.6	4.96	4.67	4.67	4.67	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.56	4.56	4.56	0.40	1.80	± 13.1 %
5800	35.3	5.27	4.55	4.55	4.55	0.40	1.80	± 13.1 %

Calibration Parameter Determined in Head Tissue Simulating Media

<sup>6</sup> Frequency velidity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the Com/F uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for Com/F assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.
<sup>7</sup> At frequencies below 3 GHz, the validity of tissue perameters (s and o) can be relaxed to ± 10% if iquid companiation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue perameters (s and o) is restricted to ± 5%. The uncertainty is the RSS of the Com/F uncertainty is the RSS of the Com/F uncertainty is the RSS of the Com/F.

<sup>10</sup> Alpha/Depth are determined during celibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always loss than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX3-3798\_Jul14

Page 5 of 11

Date of Issue : January 26, 2015

EX3DV4- SN:3798

#### July 28, 2014

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3798

f (MHz) <sup>c</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>®</sup> (mm)	Unct. (k=2)
835	55.2	0.97	9.22	9.22	9.22	0.32	1.07	± 12.0 %
900	55.0	1.05	8.96	8.96	8.96	0.55	0.76	± 12.0 %
1810	53.3	1.52	7.26	7.26	7.26	0.46	0.80	± 12.0 %
1900	53.3	1.52	7.09	7.09	7.09	0.38	0.87	± 12.0 %
2450	52.7	1.95	6.82	6.82	6.82	0.77	0.58	± 12.0 %
5200	49.0	5.30	4.41	4.41	4.41	0.45	1.90	± 13,1 %
5300	48.9	5.42	4.23	4.23	4.23	0.45	1.90	± 13.1 %
5500	48.6	5.65	3.91	3.91	3.91	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.75	3.75	3.75	0.50	1.90	±13.1 %
5800	48.2	6.00	4.09	4.09	4.09	0.50	1.90	± 13.1 %

#### Calibration Parameter Determined in Body Tissue Simulating Media

<sup>6</sup> Frequency veildity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity calibration formula to ± 10 MHz.
<sup>7</sup> At the puncies below 3 GHz, the validity of tissue parameters (s and σ) can be relaxed to ± 10% if liquid compensation formula is applied to the ConvF assessments. At requencies above 3 GHz, the validity of tissue parameters (s and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF and the RSS of the ConvF assessments.

the ConvF uncertainty for indicated target tissue parameters. <sup>6</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX3-3798 Jul14


Page 6 of 11



EX3DV4-- SN:3798

July 28, 2014


#### Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

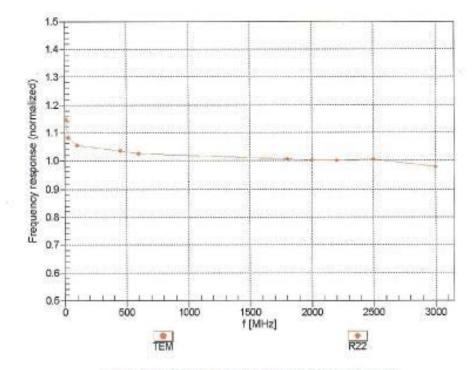

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: EX3-3798\_Jul14


Page 7 of 11

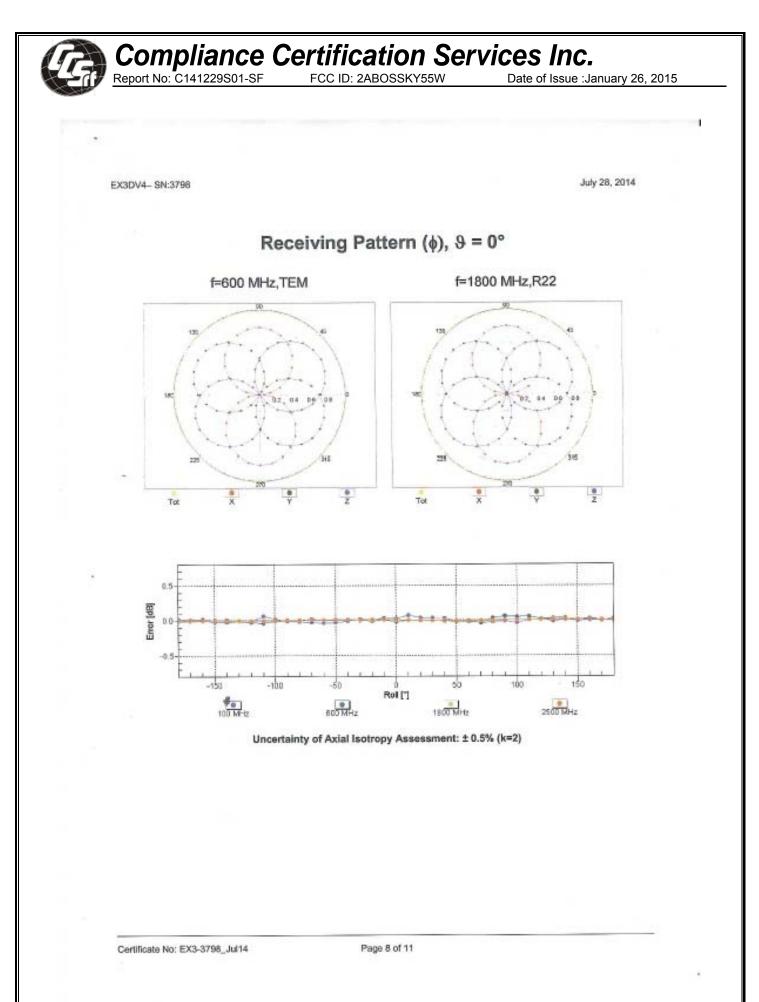




EX3DV4- SN:3798

July 28, 2014

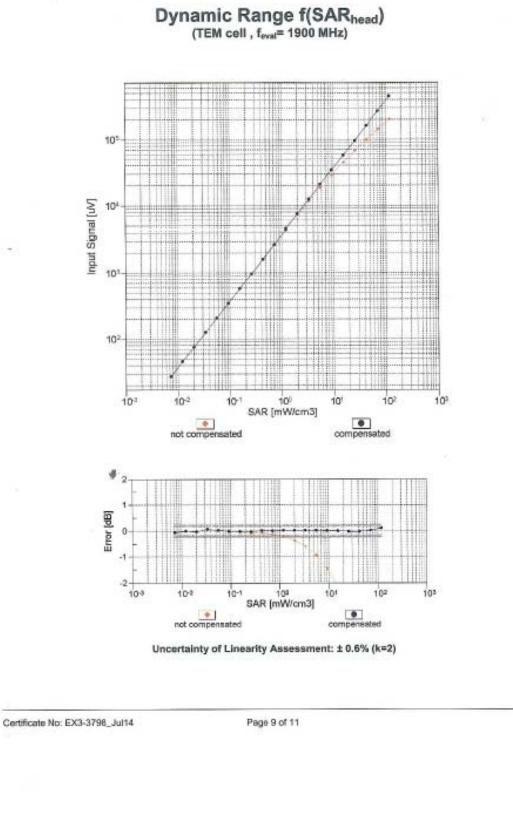

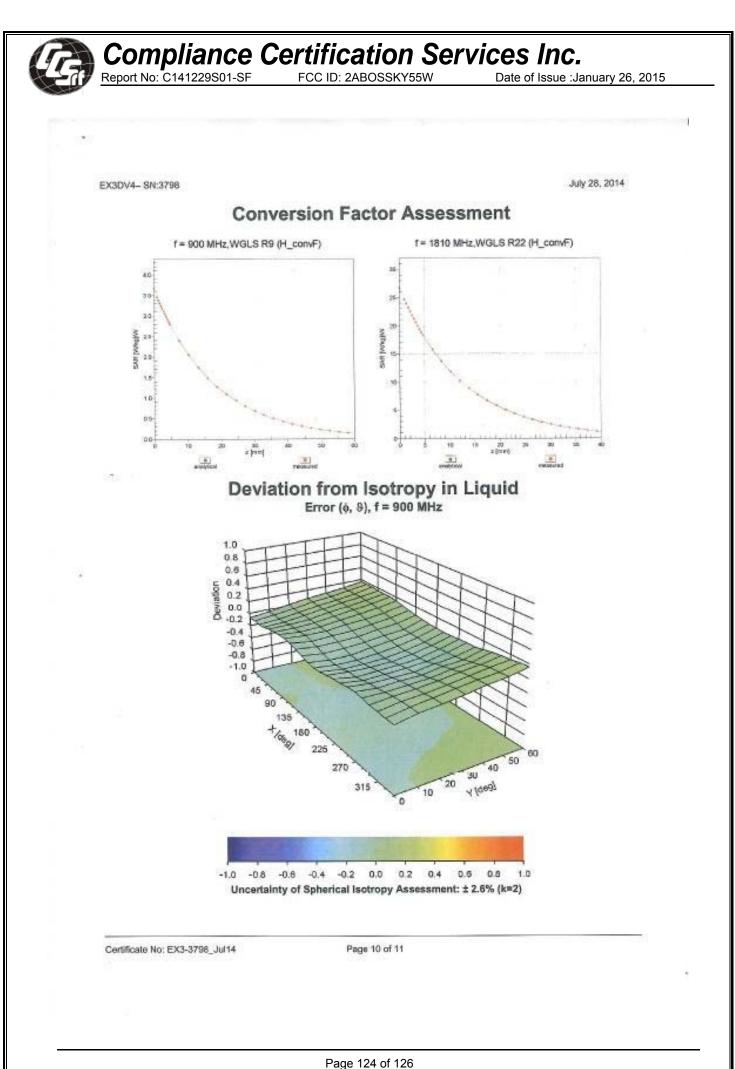



Date of Issue :January 26, 2015

EX3DV4- SN:3798

July 28, 2014

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3798

#### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-39.7
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Certificate No: EX3-3798\_Jul14

Page 11 of 11

# ComplianceCertificationServicesInc.Report No: C141229S01-SFFCC ID: 2ABOSSKY55WDate of Issue :Ja

Date of Issue :January 26, 2015

## **APPENDIX C: PLOTS OF SAR TEST RESULT**

The plots are showing in the file named Appendix C Plots of SAR Test Result

### **END REPORT**