

# FCC Test Report

Product Name	Automatic Wrist Blood Pressure Monitor
Model No.	HL158VA
FCC ID.	2ABTAHNL15VA

Applicant	HEALTH & LIFE CO.,LTD.
Address	9F., No.186, Jian Yi Road, Zhonghe District, New Taipei City, Taiwan

Date of Receipt	Jan. 13, 2016
Issued Date	Feb. 03, 2016
Report No.	1610230R-RFUSP01V00
Report Version	V1.0



The test results relate only to the samples tested.

The test results shown in the test report are traceable to the national/international standard through the calibration report of the equipment and evaluated measurement uncertainty herein.

This report must not be used to claim product endorsement by TAF or any agency of the government.

The test report shall not be reproduced without the written approval of QuieTek Corporation.

# Test Report

Issued Date: Feb. 03, 2016

Report No.: 1610230R-RFUSP01V00



Product Name	Automatic Wrist Blood Pressure Monitor
Applicant	HEALTH & LIFE CO.,LTD.
Address	9F., No.186, Jian Yi Road, Zhonghe District, New Taipei City, Taiwan
Manufacturer	HEALTH & LIFE CO.,LTD.
Address	9F., No.186, Jian Yi Road, Zhonghe District, New Taipei City, Taiwan
Name and address of factory (ies) :	#1 Health & Life (Suzhou) Co., Ltd. No.1428 Xiang Jiang Road, Suzhou New District, Suzhou City 215129, Jiangsu Province, China #2 LIVING SCIENCE CO., LTD. No.1428 Xiang Jiang Road, Suzhou New District Suzhou City 215129, Jiangsu Province, China
Model No.	HL158VA
FCC ID.	2ABTAHNL15VA
EUT Rated Voltage	DC by Battery 1.5V*2
EUT Test Voltage	DC by Battery 1.5V*2
Trade Name	Health & Life
Applicable Standard	FCC CFR Title 47 Part 15 Subpart C: 2014 ANSI C63.4: 2014, ANSI C63.10: 2013 KDB 558074 D01 DTS Meas Guidance v03r04
Test Result	Complied

Documented By : Jinn Chen  
( Senior Adm. Specialist / Jinn Chen )

Tested By : Nova chu  
( Engineer / Nova Chu )

Approved By : Vincent Lin  
( Director / Vincent Lin )

## TABLE OF CONTENTS

Description	Page
<b>1. GENERAL INFORMATION .....</b>	<b>4</b>
1.1. EUT Description.....	4
1.2. Operational Description.....	6
1.3. Tested System Details.....	7
1.4. Configuration of Tested System .....	7
1.5. EUT Exercise Software .....	7
1.6. Test Facility .....	8
<b>2. CONDUCTED EMISSION .....</b>	<b>9</b>
2.1. Test Equipment .....	9
2.2. Test Setup .....	9
2.3. Limits.....	10
2.4. Test Procedure .....	10
2.5. Uncertainty .....	10
2.6. Test Result of Conducted Emission.....	11
<b>3. PEAK POWER OUTPUT .....</b>	<b>12</b>
3.1. Test Equipment .....	12
3.2. Test Setup .....	12
3.3. Limit .....	12
3.4. Test Procedure .....	12
3.5. Uncertainty .....	12
3.6. Test Result of Peak Power Output .....	13
<b>4. RADIATED EMISSION .....</b>	<b>14</b>
4.1. Test Equipment .....	14
4.2. Test Setup .....	15
4.3. Limits.....	16
4.4. Test Procedure .....	17
4.5. Uncertainty .....	17
4.6. Test Result of Radiated Emission.....	18
<b>5. RF ANTENNA CONDUCTED TEST .....</b>	<b>22</b>
5.1. Test Equipment .....	22
5.2. Test Setup .....	22
5.3. Limits.....	22
5.4. Test Procedure .....	22
5.5. Uncertainty .....	22
5.6. Test Result of RF Antenna Conducted Test .....	23
<b>6. BAND EDGE .....</b>	<b>24</b>
6.1. Test Equipment .....	24
6.2. Test Setup .....	24
6.3. Limit .....	25
6.4. Test Procedure .....	25
6.5. Uncertainty .....	25
6.6. Test Result of Band Edge .....	26
<b>7. OCCUPIED BANDWIDTH (6DB BW).....</b>	<b>30</b>
7.1. Test Equipment .....	30
7.2. Test Setup .....	30
7.3. Limits.....	30
7.4. Test Procedure .....	30
7.5. Uncertainty .....	30
7.6. Test Result of Occupied Bandwidth .....	31
<b>8. POWER DENSITY .....</b>	<b>33</b>
8.1. Test Equipment .....	33
8.2. Test Setup .....	33
8.3. Limits.....	33
8.4. Test Procedure .....	33
8.5. Uncertainty .....	33
8.6. Test Result of Power Density .....	34
<b>9. EMI REDUCTION METHOD DURING COMPLIANCE TESTING .....</b>	<b>36</b>
Attachment 1: EUT Test Photographs	
Attachment 2: EUT Detailed Photographs	

**1. GENERAL INFORMATION**

**1.1. EUT Description**

Product Name	Automatic Wrist Blood Pressure Monitor
Trade Name	Health & Life
Model No.	HL158VA
FCC ID.	2ABTAHNL15VA
Frequency Range	2402 – 2480MHz
Channel Number	V4.0: 40CH
Type of Modulation	V4.0: GFSK(1Mbps)
Antenna Type	PCB Antenna
Channel Control	Auto
Antenna Gain	Refer to the table “Antenna List”

**Antenna List**

No.	Manufacturer	Model No.	Antenna Type	Peak Gain
1	SIGNAL	SMD8105-A0X	PCB Antenna	-2.39556dBi for 2.4 GHz

Note:

1. The antenna of EUT is conform to FCC 15.203.

Center Frequency of Each Channel: (For V4.0)

Channel	Frequency	Channel	Frequency	Channel	Frequency	Channel	Frequency
Channel 00:	2402 MHz	Channel 01:	2404 MHz	Channel 02:	2406 MHz	Channel 03:	2408 MHz
Channel 04:	2410 MHz	Channel 05:	2412 MHz	Channel 06:	2414 MHz	Channel 07:	2416 MHz
Channel 08:	2418 MHz	Channel 09:	2420 MHz	Channel 10:	2422 MHz	Channel 11:	2424 MHz
Channel 12:	2426 MHz	Channel 13:	2428 MHz	Channel 14:	2430 MHz	Channel 15:	2432 MHz
Channel 16:	2434 MHz	Channel 17:	2436 MHz	Channel 18:	2438 MHz	Channel 19:	2440 MHz
Channel 20:	2442 MHz	Channel 21:	2444 MHz	Channel 22:	2446 MHz	Channel 23:	2448 MHz
Channel 24:	2450 MHz	Channel 25:	2452 MHz	Channel 26:	2454 MHz	Channel 27:	2456 MHz
Channel 28:	2458 MHz	Channel 29:	2460 MHz	Channel 30:	2462 MHz	Channel 31:	2464 MHz
Channel 32:	2466 MHz	Channel 33:	2468 MHz	Channel 34:	2470 MHz	Channel 35:	2472 MHz
Channel 36:	2474 MHz	Channel 37:	2476 MHz	Channel 38:	2478 MHz	Channel 39:	2480 MHz

Note:

1. The EUT is a Automatic Wrist Blood Pressure Monitor with a built-in Bluetooth V4.0 transceiver.
2. These tests were conducted on a sample for the purpose of demonstrating compliance of Bluetooth transmitter with Part 15 Subpart C Paragraph 15.247 for spread spectrum devices.
3. Regarding to the operation frequency, the lowest, middle and highest frequency are selected to perform the test.

Test Mode	Mode 1: Transmit - BLE (GFSK)
-----------	-------------------------------

### 1.3. Tested System Details


The types for all equipment, plus descriptions of all cables used in the tested system (including inserted cards) are:

Product	Manufacturer	Model No.	Serial No.	Power Cord
N/A				

Signal Cable Type	Signal cable Description
N/A	

### 1.4. Configuration of Tested System

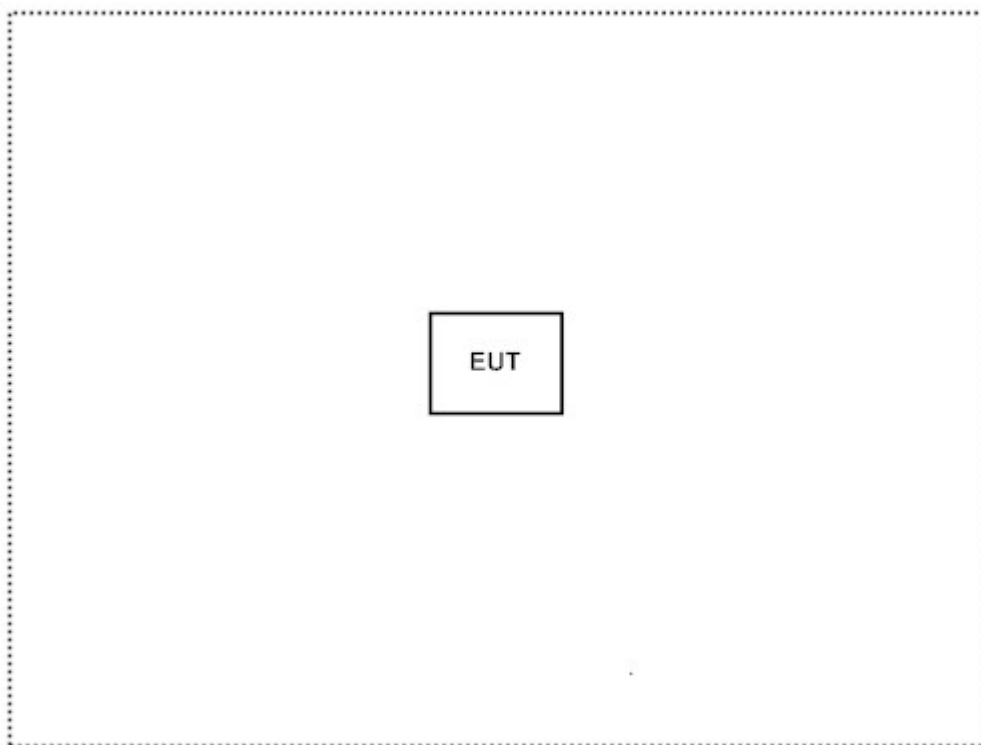

### 1.5. EUT Exercise Software

1. Setup the EUT as shown in Section 1.4.
2. Press the button to continue transmitter on the EUT
3. Check the test mode, the test channel, and the data rate.
4. Verify that the EUT works properly.

**1.6. Test Facility**

Ambient conditions in the laboratory:

Items	Required (IEC 68-1)	Actual
Temperature (°C)	15-35	20-35
Humidity (%RH)	25-75	30-65
Barometric pressure (mbar)	860-1060	950-1000

The related certificate for our laboratories about the test site and management system can be downloaded from

QuieTek Corporation's Web Site: <http://www.quietek.com/chinese/about/certificates.aspx?bval=5>

The address and introduction of Quietek Corporation's laboratories can be founded in our Web site:

<http://www.quietek.com/>

Site Description: File on  
Federal Communications Commission  
FCC Engineering Laboratory  
7435 Oakland Mills Road  
Columbia, MD 21046  
Registration Number: 92195

Site Name: Quietek Corporation  
Site Address: No.5-22, Ruishukeng,  
Linkou Dist. New Taipei City 24451,  
Taiwan, R.O.C.  
TEL: 886-2-8601-3788 / FAX : 886-2-8601-3789  
E-Mail : [service@quietek.com](mailto:service@quietek.com)

FCC Accreditation Number: TW1014

## 2. Conducted Emission


### 2.1. Test Equipment

	Equipment	Manufacturer	Model No. / Serial No.	Last Cal	Remark
X	Test Receiver	R & S	ESCS 30 / 825442/018	Sep., 2015	
X	Artificial Mains Network	R & S	ENV4200 / 848411/10	Feb., 2016	Peripherals
X	LISN	R & S	ESH3-Z5 / 825562/002	Feb., 2016	EUT
	DC LISN	Schwarzbeck	8226 / 176	Mar., 2015	EUT
X	Pulse Limiter	R & S	ESH3-Z2 / 357.8810.52	Feb., 2016	
	No.1 Shielded Room				

Note:

1. All equipments are calibrated with traceable calibrations. Each calibration is traceable to the national or international standards.
2. The test instruments marked with “X” are used to measure the final test results.
3. All equipments are calibrated every one year.

### 2.2. Test Setup

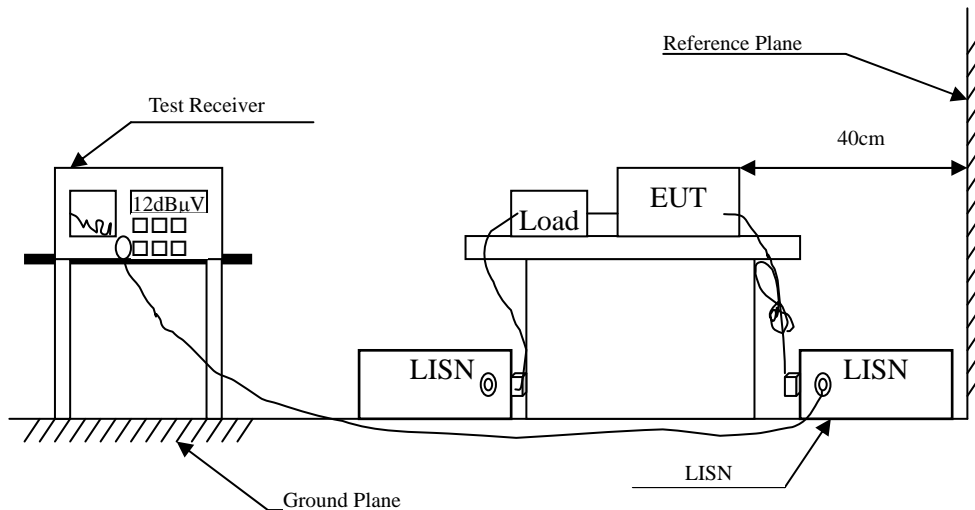



**2.3. Limits**

<b>FCC Part 15 Subpart C Paragraph 15.207 (dBµV) Limit</b>		
Frequency MHz	Limits	
	QP	AV
0.15 - 0.50	66-56	56-46
0.50-5.0	56	46
5.0 - 30	60	50

Remarks: In the above table, the tighter limit applies at the band edges.

**2.4. Test Procedure**

The EUT and Peripherals are connected to the main power through a line impedance stabilization network (L.I.S.N.). This provides a 50 ohm /50uH coupling impedance for the measuring equipment. The peripheral devices are also connected to the main power through a LISN that provides a 50ohm /50uH coupling impedance with 50ohm termination. (Please refer to the block diagram of the test setup and photographs.)

Both sides of A.C. line are checked for maximum conducted interference. In order to find the maximum emission, the relative positions of equipment and all the interface cables must be changed according to ANSI C63.4: 2014 on conducted measurement.

Conducted emissions were investigated over the frequency range from 0.15MHz to 30MHz using a receiver bandwidth of 9kHz.

The EUT was setup according to ANSI C63.4, 2014 and tested according to DTS test procedure of FCC KDB-558074 for compliance to FCC 47CFR 15.247 requirements.

**2.5. Uncertainty**

± 2.26 dB

## **2.6. Test Result of Conducted Emission**

Owing to the EUT use battery supply voltage, this test item is not performed.

### 3. Peak Power Output


#### 3.1. Test Equipment

	Equipment	Manufacturer	Model No. / Serial No.	Last Cal
X	Power Meter	Anritsu	ML2495A/6K00003357	May, 2015
X	Power Sensor	Anritsu	MA2411B/0738448	Jun., 2015

Note:

1. All equipments are calibrated with traceable calibrations. Each calibration is traceable to the national or international standards.
2. The test instruments marked with “X” are used to measure the final test results.
3. All equipments are calibrated every one year.

#### 3.2. Test Setup

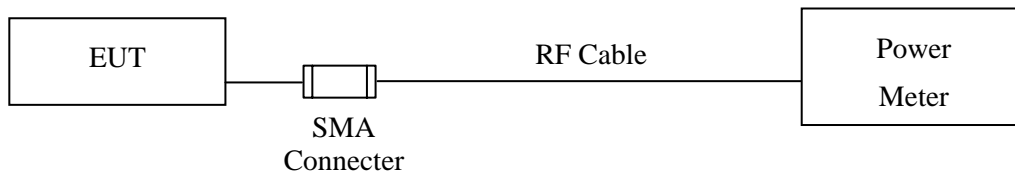

#### 3.3. Limit

The maximum peak power shall be less 1Watt.

#### 3.4. Test Procedure

Tested according to DTS test procedure of KDB 558074 for compliance to FCC 47CFR 15.247 requirements. The maximum peak conducted output power using KDB 558074 section 9.1.2 PKPM1 Peak power meter method.

#### 3.5. Uncertainty

± 1.27 dB

### 3.6. Test Result of Peak Power Output

Product : Automatic Wrist Blood Pressure Monitor  
 Test Item : Peak Power Output  
 Test Site : No.3 OATS  
 Test Mode : Mode 1: Transmit - BLE (GFSK)

Channel No.	Frequency (MHz)	Measurement (dBm)	Required Limit	Result
Channel 00	2402.00	-5.96	1 Watt= 30 dBm	Pass
Channel 19	2440.00	-6.34	1 Watt= 30 dBm	Pass
Channel 39	2480.00	-7.52	1 Watt= 30 dBm	Pass

#### 4. Radiated Emission

##### 4.1. Test Equipment

The following test equipments are used during the radiated emission test:

Test Site		Equipment	Manufacturer	Model No./Serial No.	Last Cal
☒ Site # 3	X	Loop Antenna	Teseq	HLA6120 / 26739	Jul., 2015
	X	Bilog Antenna	Schaffner Chase	CBL6112B/2673	Sep., 2015
	X	Horn Antenna	Schwarzbeck	BBHA9120D/D305	Sep., 2015
	X	Horn Antenna	Schwarzbeck	BBHA9170/208	Jul., 2015
	X	Pre-Amplifier	Agilent	8447D/2944A09549	Sep., 2015
	X	Spectrum Analyzer	Agilent	E4407B / US39440758	May, 2015
	X	Test Receiver	R & S	ESCS 30/ 825442/018	Sep., 2015
	X	Coaxial Cable	QuieTek	QTK-CABLE/ CAB5	Feb., 2016
	X	Controller	QuieTek	QTK-CONTROLLER/ CTRL3	N/A
X	Coaxial Switch	Anritsu	MP59B/6200265729	N/A	


Test Site		Equipment	Manufacturer	Model No./Serial No.	Last Cal.
☒ CB # 8	X	Spectrum Analyzer	R&S	FSP40/ 100339	Oct, 2015
	X	Horn Antenna	ETS-Lindgren	3117/ 35205	Mar, 2015
	X	Horn Antenna	Schwarzbeck	BBHA9170/209	Jan, 2016
	X	Horn Antenna	TRC	AH-0801/95051	Aug, 2015
	X	Pre-Amplifier	EMCI	EMC012630SE/980210	Jan, 2016
	X	Pre-Amplifier	MITEQ	JS41-001040000-58-5P/153945	Jul, 2015
	X	Pre-Amplifier	NARDA	DBL-1840N506/013	Jul, 2015

Note:


1. All equipments are calibrated with traceable calibrations. Each calibration is traceable to the national or international standards.
2. The test instruments marked with "X" are used to measure the final test results.
3. All equipments are calibrated every one year.

## 4.2. Test Setup

Below 1GHz

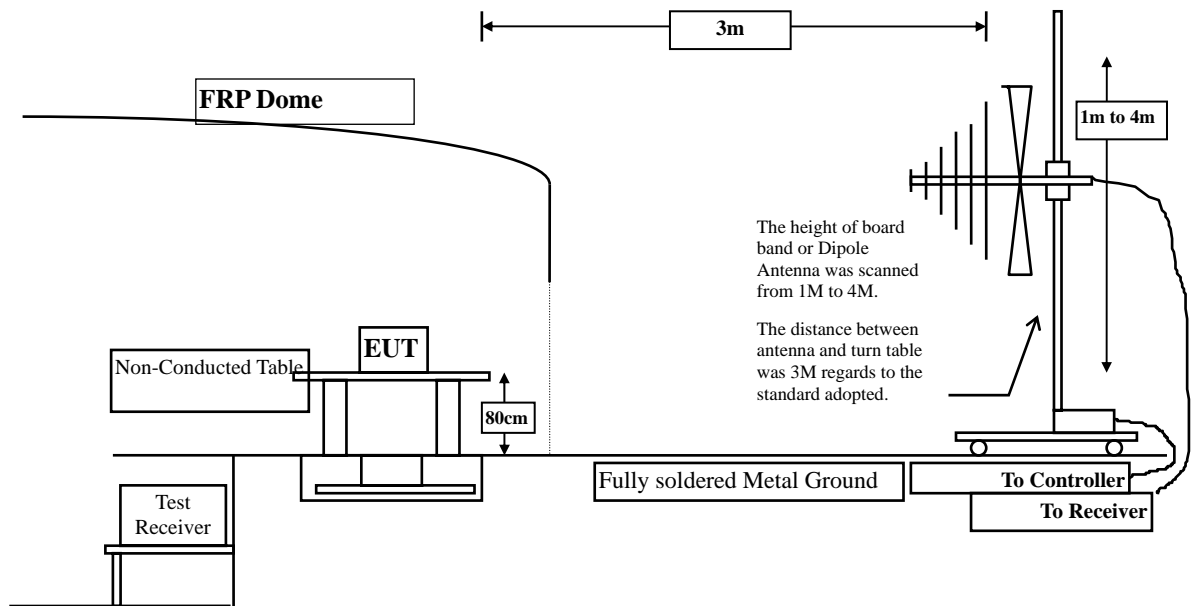

Above 1GHz

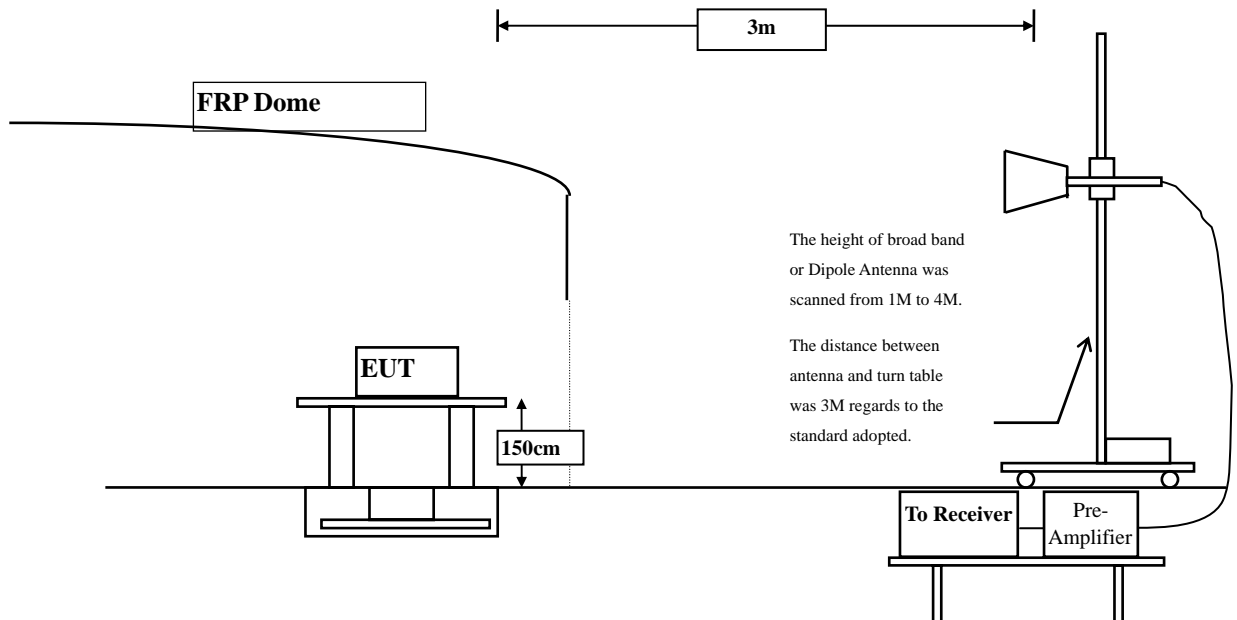

**4.3. Limits**

➤ **General Radiated Emission Limits**

Emissions radiated outside of the specified frequency bands, except for harmonics, shall be attenuated by at least 20dB below the level of the fundamental or to the general radiated emission limits in paragraph 15.209, whichever is the lesser attenuation.

<b>FCC Part 15 Subpart C Paragraph 15.209 Limits</b>		
Frequency MHz	Field strength (microvolts/meter)	Measurement distance (meter)
0.009-0.490	2400/F(kHz)	300
0.490-1.705	24000/F(kHz)	30
1.705-30	30	30
30-88	100	3
88-216	150	3
216-960	200	3
Above 960	500	3

- Remarks:
1. RF Voltage (dBμV) = 20 log RF Voltage (uV)
  2. In the Above Table, the tighter limit applies at the band edges.
  3. Distance refers to the distance in meters between the measuring instrument antenna and the closed point of any part of the device or system.

#### **4.4. Test Procedure**

The EUT was setup according to ANSI C63.10: 2013 and tested according to DTS test procedure of KDB558074 for compliance to FCC 47CFR 15.247 requirements.

Measuring the frequency range below 1GHz, the EUT is placed on a turn table which is 0.8 meter above ground, when measuring the frequency range above 1GHz, the EUT is placed on a turn table which is 1.5 meter above ground.

The turn table is rotated 360 degrees to determine the position of the maximum emission level.

The EUT was positioned such that the distance from antenna to the EUT was 3 meters.

The antenna is scanned between 1 meter and 4 meters to find out the maximum emission level. This is repeated for both horizontal and vertical polarization of the antenna. In order to find the maximum emission, all of the interface cables were manipulated according to ANSI C63.10: 2013 on radiated measurement.

The resolution bandwidth below 30MHz setting on the field strength meter is 9kHz and 30MHz~1GHz is 120kHz and above 1GHz is 1MHz.

Radiated emission measurements below 30MHz are made using Loop Antenna and 30MHz~1GHz are made using broadband Bilog antenna and above 1GHz are made using Horn Antennas.

The measurement is divided into the Preliminary Measurement and the Final Measurement.

The suspected frequencies are searched for in Preliminary Measurement with the measurement antenna kept pointed at the source of the emission both in azimuth and elevation, with the polarization of the antenna oriented for maximum response. The antenna is pointed at an angle towards the source of the emission, and the EUT is rotated in both height and polarization to maximize the measured emission. The emission is kept within the illumination area of the 3 dB bandwidth of the antenna.

The worst radiated emission is measured in the Open Area Test Site on the Final Measurement.

The measurement frequency range from 9kHz - 10th Harmonic of fundamental was investigated.

#### **4.5. Uncertainty**

± 3.9 dB above 1GHz

± 3.8 dB below 1GHz



**4.6. Test Result of Radiated Emission**

Product : Automatic Wrist Blood Pressure Monitor  
 Test Item : Harmonic Radiated Emission  
 Test Site : No.3 OATS  
 Test Mode : Mode 1: Transmit - BLE (GFSK)(2402MHz)

Frequency MHz	Correct Factor dB	Reading Level dBμV	Measurement Level dBμV/m	Margin dB	Limit dBμV/m
<b>Horizontal</b>					
<b>Peak Detector:</b>					
4804.000	3.327	41.440	44.767	-29.233	74.000
7206.000	10.136	30.960	41.096	-32.904	74.000
9608.000	13.706	31.230	44.936	-29.064	74.000
<b>Average Detector:</b>					
--					
<b>Vertical</b>					
<b>Peak Detector:</b>					
4804.000	6.638	37.340	43.977	-30.023	74.000
7206.000	11.005	30.820	41.825	-32.175	74.000
9608.000	14.103	31.550	45.653	-28.347	74.000
<b>Average Detector:</b>					
--					

Note:

1. All Readings below 1GHz are Quasi-Peak, above 1GHz are performed with peak and/or average measurements as necessary.
2. Peak measurements: RBW = 1MHz, VBW = 3 MHz, Sweep: Auto.
3. Average measurements: RBW = 1MHz, VBW = 10 Hz, Sweep: Auto.
4. Measurement Level = Reading Level + Correct Factor.
5. Correct Factor = Antenna factor + Cable loss – Amplifier gain.
6. The average measurement was not performed when the peak measured data under the limit of average detection.
7. The emission levels of other frequencies are very lower than the limit and not show in test report.

Product : Automatic Wrist Blood Pressure Monitor  
 Test Item : Harmonic Radiated Emission  
 Test Site : No.3 OATS  
 Test Mode : Mode 1: Transmit - BLE (GFSK) (2440MHz)

Frequency MHz	Correct Factor dB	Reading Level dB $\mu$ V	Measurement Level dB $\mu$ V/m	Margin dB	Limit dB $\mu$ V/m
------------------	-------------------------	--------------------------------	--------------------------------------	--------------	-----------------------

**Horizontal**

**Peak Detector:**

4880.000	3.010	41.840	44.850	-29.150	74.000
7320.000	11.833	31.770	43.604	-30.396	74.000
9760.000	12.580	31.270	43.851	-30.149	74.000

**Average**

**Detector:**

--

**Vertical**

**Peak Detector:**

4880.000	5.738	37.070	42.808	-31.192	74.000
7320.000	12.703	31.320	44.023	-29.977	74.000
9760.000	13.052	30.800	43.852	-30.148	74.000

**Average**

**Detector:**

--

Note:

1. All Readings below 1GHz are Quasi-Peak, above 1GHz are performed with peak and/or average measurements as necessary.
2. Peak measurements: RBW = 1MHz, VBW = 3 MHz, Sweep: Auto.
3. Average measurements: RBW = 1MHz, VBW = 10 Hz, Sweep: Auto.
4. Measurement Level = Reading Level + Correct Factor.
5. Correct Factor = Antenna factor + Cable loss – Amplifier gain.
6. The average measurement was not performed when the peak measured data under the limit of average detection.
7. The emission levels of other frequencies are very lower than the limit and not show in test report.

Product : Automatic Wrist Blood Pressure Monitor  
 Test Item : Harmonic Radiated Emission  
 Test Site : No.3 OATS  
 Test Mode : Mode 1: Transmit - BLE (GFSK) (2480MHz)

Frequency MHz	Correct Factor dB	Reading Level dB $\mu$ V	Measurement Level dB $\mu$ V/m	Margin dB	Limit dB $\mu$ V/m
<b>Horizontal</b>					
<b>Peak Detector:</b>					
4960.000	2.760	40.370	43.130	-30.870	74.000
7440.000	12.567	32.590	45.156	-28.844	74.000
9920.000	13.456	32.360	45.816	-28.184	74.000
<b>Average Detector:</b>					
--					
<b>Vertical</b>					
<b>Peak Detector:</b>					
4960.000	5.557	36.110	41.667	-32.333	74.000
7440.000	13.426	32.200	45.625	-28.375	74.000
9920.000	13.958	32.190	46.148	-27.852	74.000
<b>Average Detector:</b>					
--					

Note:

1. All Readings below 1GHz are Quasi-Peak, above 1GHz are performed with peak and/or average measurements as necessary.
2. Peak measurements: RBW = 1MHz, VBW = 3 MHz, Sweep: Auto.
3. Average measurements: RBW = 1MHz, VBW = 10 Hz, Sweep: Auto.
4. Measurement Level = Reading Level + Correct Factor.
5. Correct Factor = Antenna factor + Cable loss – Amplifier gain.
6. The average measurement was not performed when the peak measured data under the limit of average detection.
7. The emission levels of other frequencies are very lower than the limit and not show in test report.

Product : Automatic Wrist Blood Pressure Monitor  
 Test Item : General Radiated Emission  
 Test Site : No.3 OATS  
 Test Mode : Mode 1: Transmit - BLE (GFSK) (2440MHz)

Frequency MHz	Correct Factor dB	Reading Level dB $\mu$ V	Measurement Level dB $\mu$ V/m	Margin dB	Limit dB $\mu$ V/m
<b>Horizontal</b>					
143.490	-7.665	37.059	29.394	-14.106	43.500
261.830	-5.466	34.742	29.276	-16.724	46.000
341.370	-2.946	35.010	32.064	-13.936	46.000
464.560	2.914	36.069	38.983	-7.017	46.000
658.560	1.892	26.762	28.654	-17.346	46.000
852.560	7.106	23.739	30.845	-15.155	46.000
<b>Vertical</b>					
90.140	-4.175	38.959	34.784	-8.716	43.500
257.950	-4.952	33.860	28.908	-17.092	46.000
341.370	-1.116	33.332	32.216	-13.784	46.000
460.680	-1.930	28.578	26.648	-19.352	46.000
611.030	2.009	26.692	28.702	-17.298	46.000
771.080	2.766	24.021	26.788	-19.212	46.000

Note:

1. All Readings below 1GHz are Quasi-Peak, above 1GHz are performed with peak and/or average measurements as necessary.
2. Peak measurements: RBW = 1MHz, VBW = 3 MHz, Sweep: Auto.
3. Average measurements: RBW = 1MHz, VBW = 10 Hz, Sweep: Auto.
4. Measurement Level = Reading Level + Correct Factor.
5. Correct Factor = Antenna factor + Cable loss – Amplifier gain.
6. The average measurement was not performed when the peak measured data under the limit of average detection.
7. The emission levels of other frequencies are very lower than the limit and not show in test report.
8. No emission found between lowest internal used/generated frequency to 30MHz.

## 5. RF Antenna Conducted Test


### 5.1. Test Equipment

	Equipment	Manufacturer	Model No./Serial No.	Last Cal.
	Spectrum Analyzer	R&S	FSP40 / 100170	Jun., 2015
	Spectrum Analyzer	Agilent	E4407B / US39440758	Jun., 2015
X	Spectrum Analyzer	Agilent	N9010A / MY48030495	Apr., 2015

Note:

1. All equipments are calibrated with traceable calibrations. Each calibration is traceable to the national or international standards.
2. The test instruments marked with “X” are used to measure the final test results.
3. All equipments are calibrated every one year.

### 5.2. Test Setup

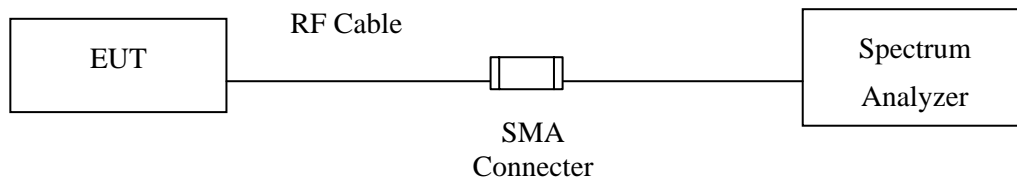

### 5.3. Limits

According to FCC Section 15.247(d). In any 100 kHz bandwidth outside the frequency band in which the spread spectrum or digitally modulated intentional radiator is operating, the radio frequency power that is produced by the intentional radiator shall be at least 20 dB below that in the 100 kHz bandwidth within the band that contains the highest level of the desired power, based on either an RF conducted or measurement, provided the transmitter demonstrates compliance with the peak conducted power limits. If the transmitter complies with the conducted power limits based on the use of RMS averaging over a time interval, the attenuation required under this paragraph shall be 30 dB instead of 20 dB.

### 5.4. Test Procedure

The EUT was tested according to DTS test procedure of KDB558074 for compliance to FCC 47CFR 15.247 requirements.


### 5.5. Uncertainty

± 150Hz


### 5.6. Test Result of RF Antenna Conducted Test

Product : Automatic Wrist Blood Pressure Monitor  
 Test Item : RF Antenna Conducted Test  
 Test Site : No.3 OATS  
 Test Mode : Mode 1: Transmit - BLE (GFSK)


**Figure Channel 00:**

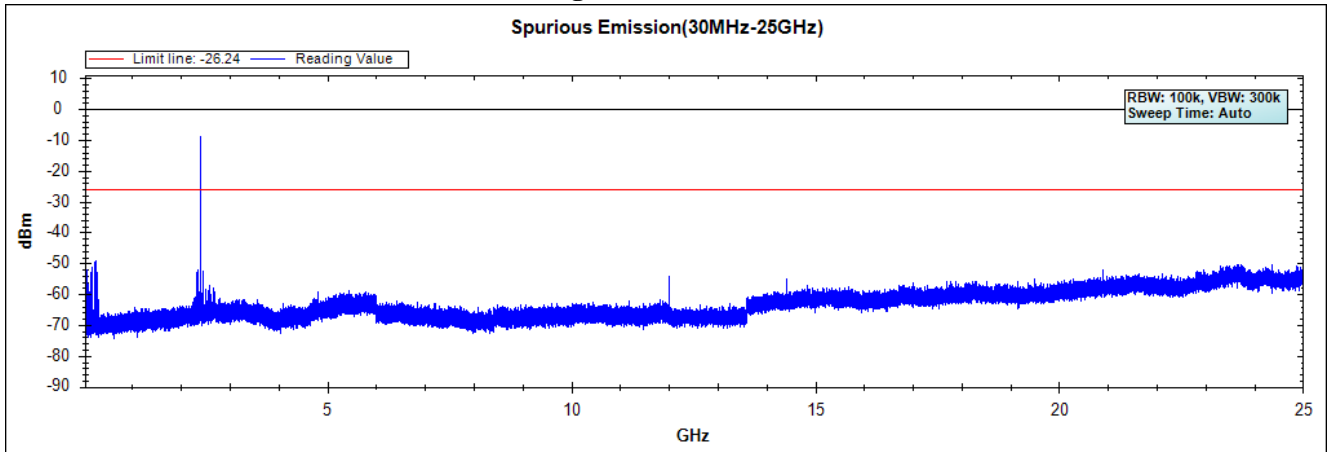

**Figure Channel 19:**

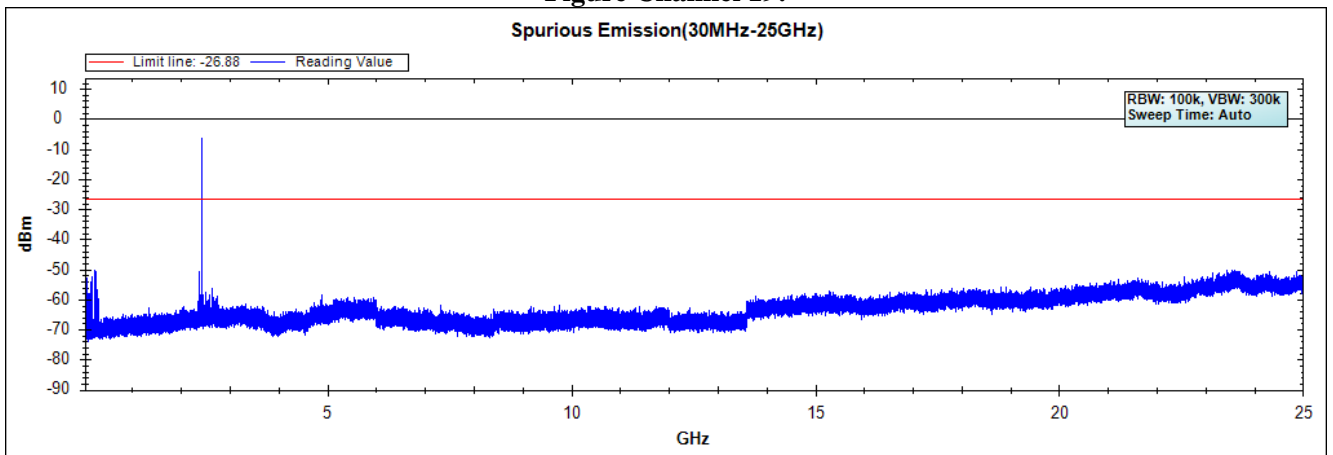

**Figure Channel 39:**

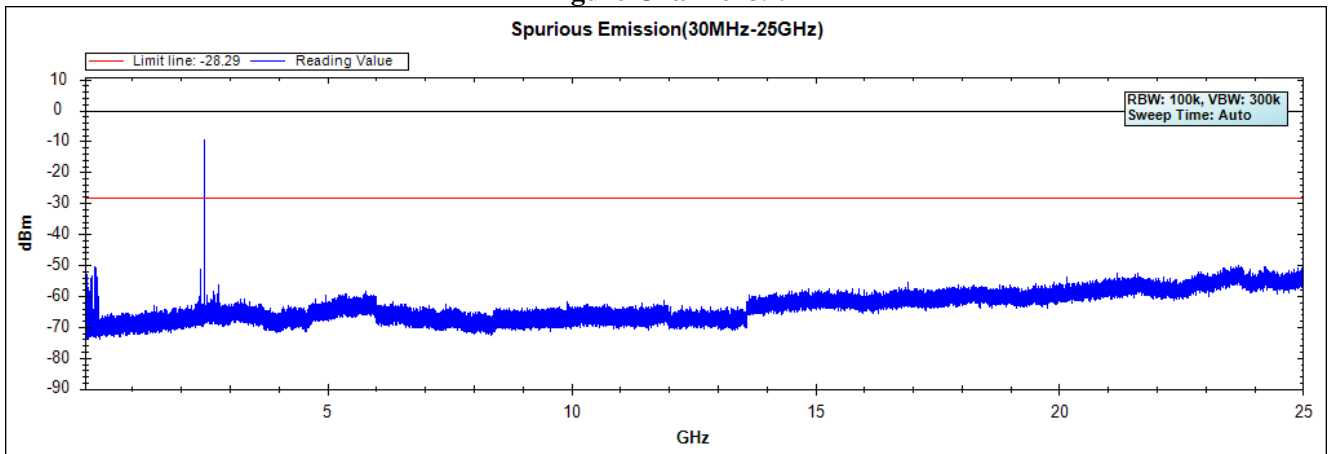

Note: The above test pattern is synthesized by multiple of the frequency range.

## 6. Band Edge

### 6.1. Test Equipment

#### RF Radiated Measurement:

The following test equipments are used during the band edge tests:

Test Site	Equipment	Manufacturer	Model No./Serial No.	Last Cal.
☒ CB # 8	X Spectrum Analyzer	R&S	FSP40/ 100339	Oct, 2015
	X Horn Antenna	ETS-Lindgren	3117/ 35205	Mar, 2015
	X Horn Antenna	Schwarzbeck	BBHA9170/209	Jan, 2016
	X Horn Antenna	TRC	AH-0801/95051	Aug, 2015
	X Pre-Amplifier	EMCI	EMC012630SE/980210	Jan, 2016
	X Pre-Amplifier	MITEQ	JS41-001040000-58-5P/153945	Jul, 2015
	X Pre-Amplifier	NARDA	DBL-1840N506/013	Jul, 2015


Note:

1. All equipments are calibrated with traceable calibrations. Each calibration is traceable to the national or international standards.
2. The test instruments marked with “X” are used to measure the final test results.
3. All equipments are calibrated every one year.

### 6.2. Test Setup

#### RF Radiated Measurement:

Above 1GHz

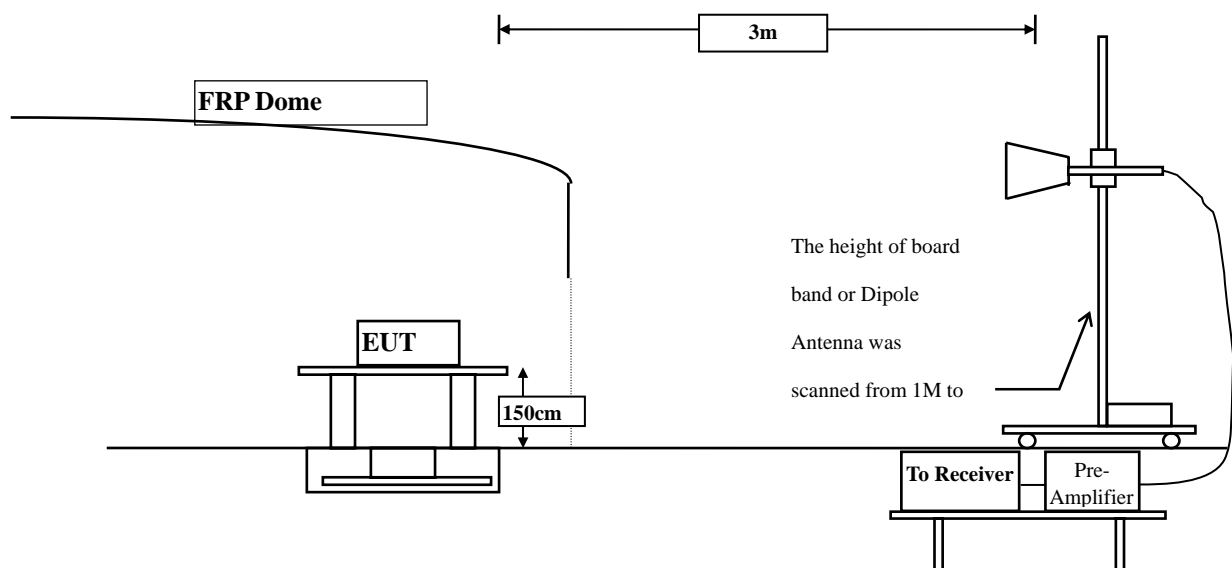

### **6.3. Limit**

In any 100 kHz bandwidth outside the frequency band in which the spread spectrum intentional radiator is operating, the radio frequency power that is produced by the intentional radiator shall be at least 20 dB below that in the 100 kHz bandwidth within the band that contains the highest level of the desired power, based on either an RF conducted or a radiated measurement. Attenuation below the general limits specified in Section 15.209(a) is not required. In addition, radiated emissions which fall in the restricted bands, as defined in Section 15.205(a), must also comply with the radiated emission limits specified in Section 15.209(a) (see Section 15.205(c)).

### **6.4. Test Procedure**

The EUT was setup according to ANSI C63.10, 2013 and tested according to DTS test procedure of KDB558074 for compliance to FCC 47CFR 15.247 requirements.

The EUT is placed on a turn table which is 1.5 meter above ground. The turn table is rotated 360 degrees to determine the position of the maximum emission level. The EUT was positioned such that the distance from antenna to the EUT was 3 meters.

The antenna is scanned from 1 meter to 4 meters to find out the maximum emission level. This is repeated for both horizontal and vertical polarization of the antenna. In order to find the maximum emission, all of the interface cables were manipulated according to ANSI C63.10:2013 on radiated measurement.

### **6.5. Uncertainty**

± 3.9 dB above 1GHz

± 3.8 dB below 1GHz




### 6.6. Test Result of Band Edge

Product : Automatic Wrist Blood Pressure Monitor  
 Test Item : Band Edge  
 Test Site : No.3 OATS  
 Test Mode : Mode 1: Transmit - BLE (GFSK) (2402MHz)


#### RF Radiated Measurement (Horizontal):

Channel No.	Frequency (MHz)	Correct Factor (dB)	Reading Level (dBμV)	Emission Level (dBμV/m)	Peak Limit (dBμV/m)	Average Limit (dBμV/m)	Result
00 (Peak)	2370.290	-1.208	36.370	35.162	74.00	54.00	Pass
00 (Peak)	2390.000	-1.131	33.367	32.236	74.00	54.00	Pass
00 (Peak)	2400.000	-1.084	57.227	56.144	--	--	--
00 (Peak)	2401.739	-1.074	79.030	77.956	--	--	--
00 (Average)	2370.145	-1.209	28.172	26.963	74.00	54.00	Pass
00 (Average)	2390.000	-1.131	21.708	20.577	74.00	54.00	Pass
00 (Average)	2400.000	-1.084	43.180	42.097	--	--	--
00 (Average)	2402.029	-1.073	78.179	77.107	--	--	--

**Figure Channel 00: Horizontal (Peak)**

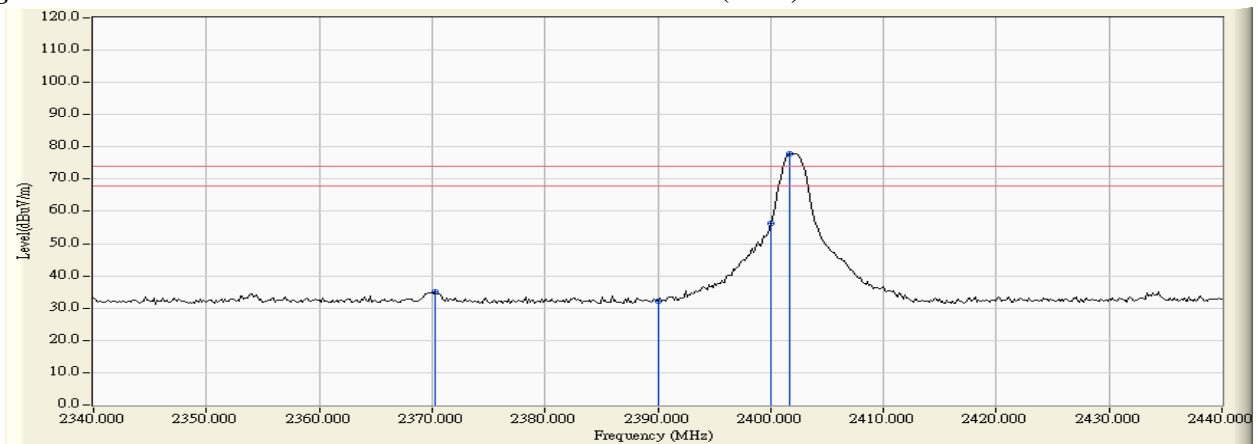

**Figure Channel 00: Horizontal (Average)**

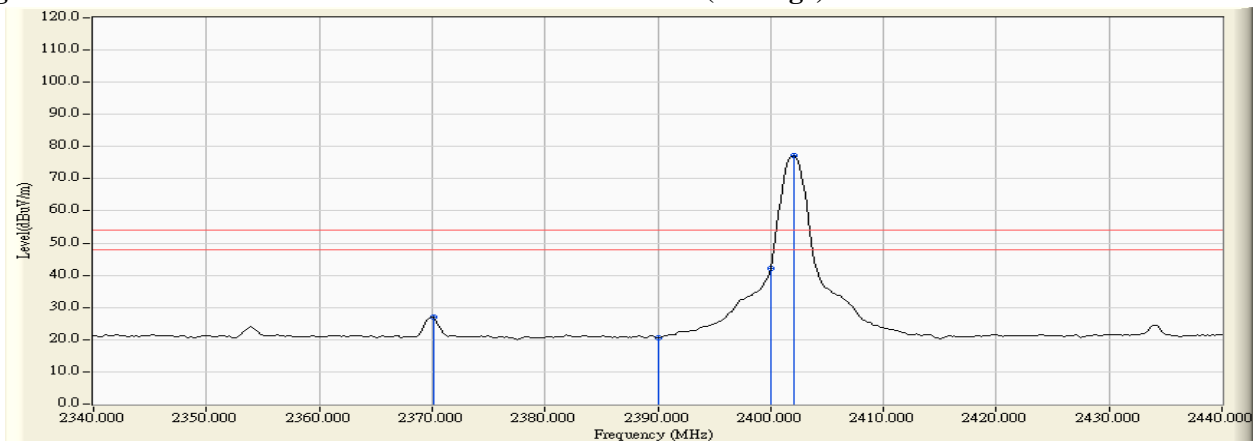

Note:


1. All readings above 1GHz are performed with peak and/or average measurements as necessary.
2. Peak measurements: RBW = 1MHz, VBW = 3 MHz, Sweep: Auto.
3. Average measurements: RBW = 1MHz, VBW = 10 Hz, Sweep: Auto.
4. “ \* ”, means this data is the worst emission level.
5. Measurement Level = Reading Level + Correct Factor.
6. The average measurement was not performed when the peak measured data under the limit of average detection.

Product : Automatic Wrist Blood Pressure Monitor  
 Test Item : Band Edge  
 Test Site : No.3 OATS  
 Test Mode : Mode 1: Transmit - BLE (GFSK) (2402MHz)


**RF Radiated Measurement (Vertical):**

Channel No.	Frequency (MHz)	Correct Factor (dB)	Reading Level (dBμV)	Emission Level (dBμV/m)	Peak Limit (dBμV/m)	Average Limit (dBμV/m)	Result
00 (Peak)	2370.145	-1.633	36.954	35.321	74.00	54.00	Pass
00 (Peak)	2390.000	-1.725	33.912	32.187	74.00	54.00	Pass
00 (Peak)	2400.000	-1.733	59.777	58.045	--	--	--
00 (Peak)	2402.319	-1.728	81.780	80.052	--	--	--
00 (Average)	2370.000	-1.632	30.436	28.804	74.00	54.00	Pass
00 (Average)	2390.000	-1.725	21.608	19.883	74.00	54.00	Pass
00 (Average)	2400.000	-1.733	45.774	44.042	--	--	--
00 (Average)	2402.029	-1.729	80.994	79.265	--	--	--

**Figure Channel 00: Vertical (Peak)**

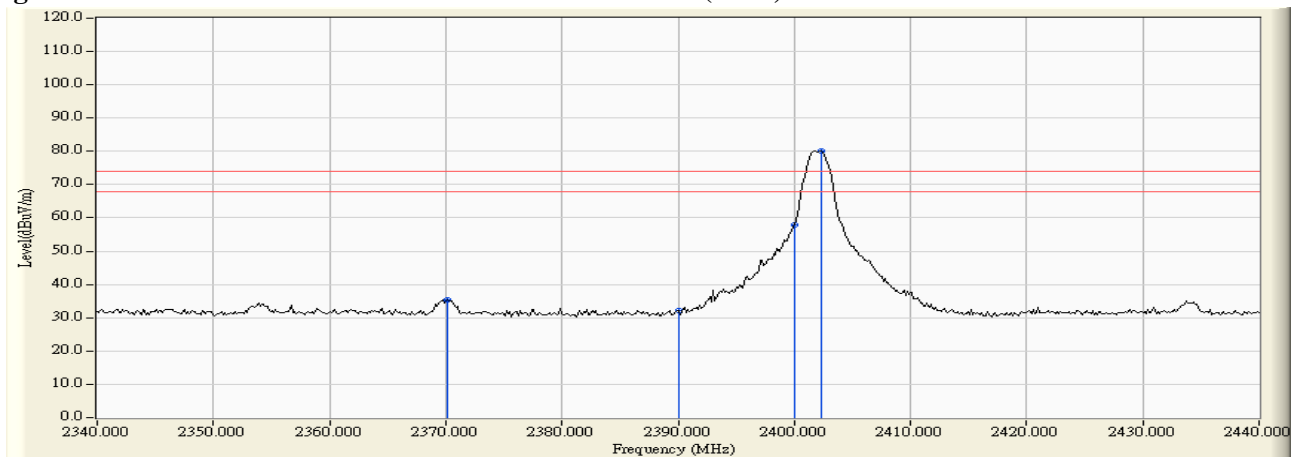

**Figure Channel 00: Vertical (Average)**

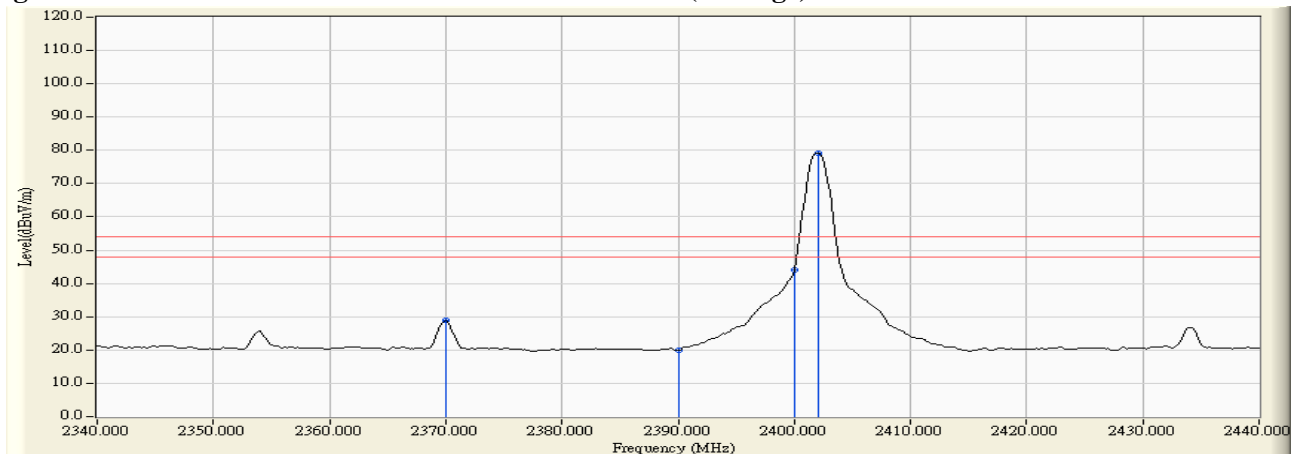

Note:


1. All readings above 1GHz are performed with peak and/or average measurements as necessary.
2. Peak measurements: RBW = 1MHz, VBW = 3 MHz, Sweep: Auto.
3. Average measurements: RBW = 1MHz, VBW = 10 Hz, Sweep: Auto.
4. “ \* ”, means this data is the worst emission level.
5. Measurement Level = Reading Level + Correct Factor.
6. The average measurement was not performed when the peak measured data under the limit of average detection.

Product : Automatic Wrist Blood Pressure Monitor  
 Test Item : Band Edge  
 Test Site : No.3 OATS  
 Test Mode : Mode 1: Transmit - BLE (GFSK) (2480MHz)


**RF Radiated Measurement (Horizontal):**

Channel No.	Frequency (MHz)	Correct Factor (dB)	Reading Level (dBμV)	Emission Level (dBμV/m)	Peak Limit (dBμV/m)	Average Limit (dBμV/m)	Result
39 (Peak)	2479.732	-0.582	76.247	75.665	--	--	--
39 (Peak)	2483.500	-0.558	47.067	46.509	74.00	54.00	Pass
39 (Average)	2480.022	-0.580	74.895	74.315	--	--	--
39 (Average)	2483.500	-0.558	28.945	28.387	74.00	54.00	Pass
39 (Average)	2484.225	-0.554	30.826	30.272	74.00	54.00	Pass

**Figure Channel 39: Horizontal (Peak)**

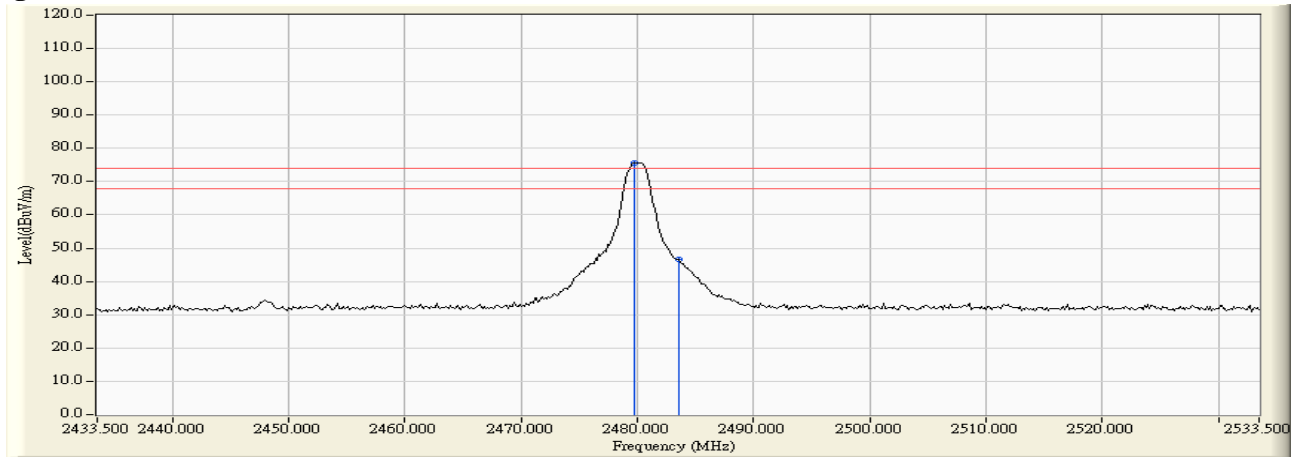

**Figure Channel 39: Horizontal (Average)**

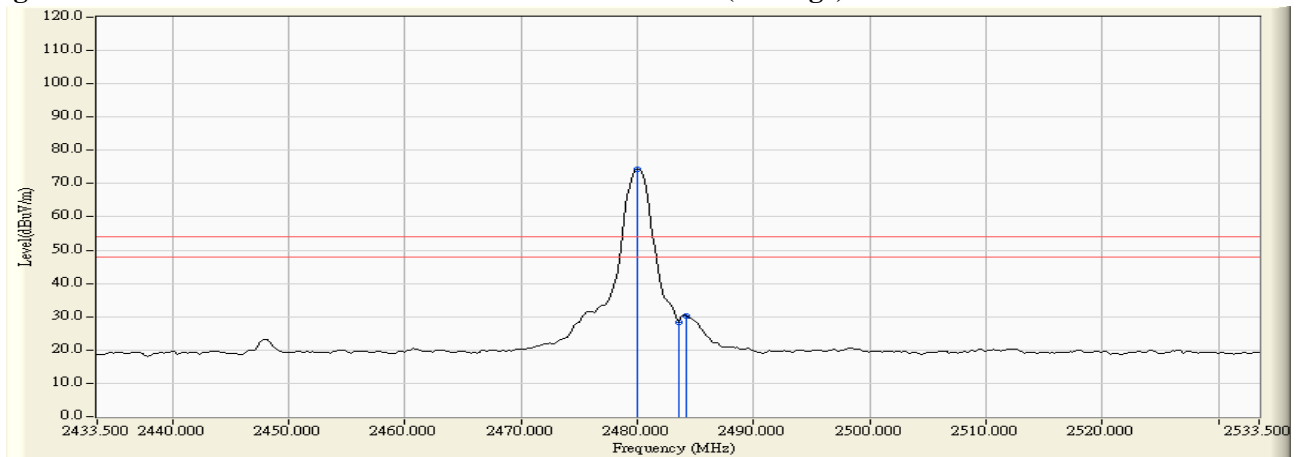

**Note:**


1. All readings above 1GHz are performed with peak and/or average measurements as necessary.
2. Peak measurements: RBW = 1MHz, VBW = 3 MHz, Sweep: Auto.
3. Average measurements: RBW = 1MHz, VBW = 10 Hz, Sweep: Auto.
4. “ \* ”, means this data is the worst emission level.
5. Measurement Level = Reading Level + Correct Factor.
6. The average measurement was not performed when the peak measured data under the limit of average detection.

Product : Automatic Wrist Blood Pressure Monitor  
 Test Item : Band Edge  
 Test Site : No.3 OATS  
 Test Mode : Mode 1: Transmit - BLE (GFSK) (2480MHz)


**RF Radiated Measurement (Vertical):**

Channel No.	Frequency (MHz)	Correct Factor (dB)	Reading Level (dBμV)	Emission Level (dBμV/m)	Peak Limit (dBμV/m)	Average Limit (dBμV/m)	Result
39 (Peak)	2480.167	-1.323	80.260	78.937	--	--	--
39 (Peak)	2483.500	-1.305	50.743	49.438	74.00	54.00	Pass
39 (Average)	2480.167	-1.323	78.893	77.570	--	--	--
39 (Average)	2483.500	-1.305	33.197	31.892	74.00	54.00	Pass

**Figure Channel 39: Vertical (Peak)**

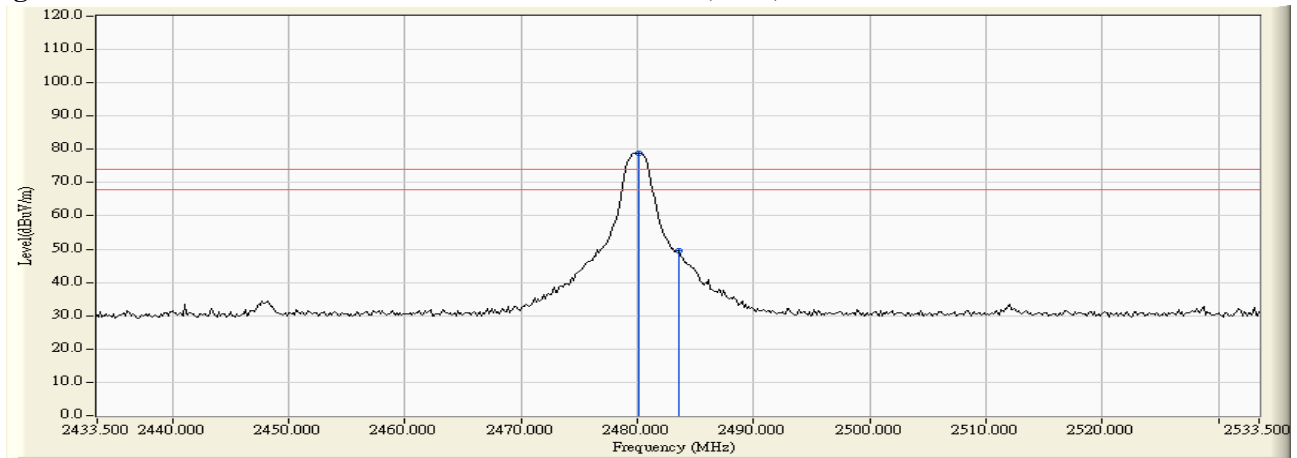

**Figure Channel 39: Vertical (Average)**

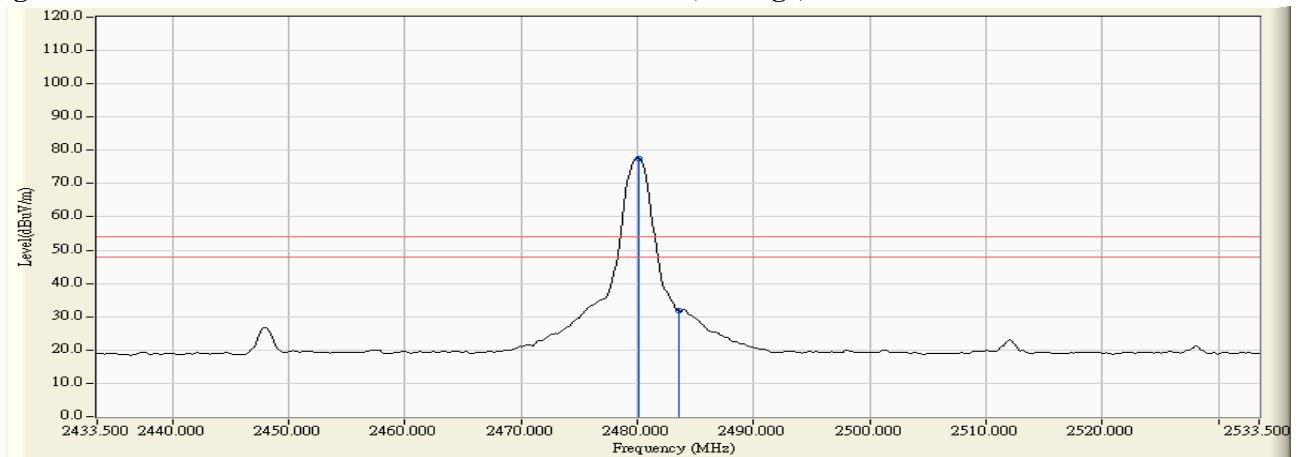

Note:

1. All readings above 1GHz are performed with peak and/or average measurements as necessary.
2. Peak measurements: RBW = 1MHz, VBW = 3 MHz, Sweep: Auto.
3. Average measurements: RBW = 1MHz, VBW = 10 Hz, Sweep: Auto.
4. “ \* ”, means this data is the worst emission level.
5. Measurement Level = Reading Level + Correct Factor.
6. The average measurement was not performed when the peak measured data under the limit of average detection.

## 7. Occupied Bandwidth (6dB BW)


### 7.1. Test Equipment

	Equipment	Manufacturer	Model No./Serial No.	Last Cal.
	Spectrum Analyzer	R&S	FSP40 / 100170	Jun., 2015
	Spectrum Analyzer	Agilent	E4407B / US39440758	Jun., 2015
X	Spectrum Analyzer	Agilent	N9010A / MY48030495	Apr., 2015

Note:

1. All equipments are calibrated with traceable calibrations. Each calibration is traceable to the national or international standards.
2. The test instruments marked with “X” are used to measure the final test results.
3. All equipments are calibrated every one year.

### 7.2. Test Setup

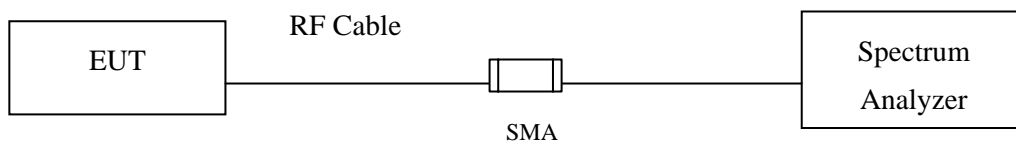

### 7.3. Limits

The minimum bandwidth shall be at least 500 kHz.

### 7.4. Test Procedure

The EUT was setup according to ANSI C63.10 2013; tested according to DTS test procedure of KDB558074 for compliance to FCC 47CFR 15.247 requirements.

Set RBW = 1-5% of the emission bandwidth, VBW ≥ 3\*RBW

### 7.5. Uncertainty

± 150Hz

### 7.6. Test Result of Occupied Bandwidth

Product : Automatic Wrist Blood Pressure Monitor  
 Test Item : Occupied Bandwidth Data  
 Test Site : No.3 OATS  
 Test Mode : Mode 1: Transmit - BLE (GFSK)

Channel No.	Frequency (MHz)	Measurement Level (kHz)	Required Limit (kHz)	Result
00	2402	740.0	>500	Pass
19	2440	730.0	>500	Pass
39	2480	740.0	>500	Pass

**Figure Channel 00:**

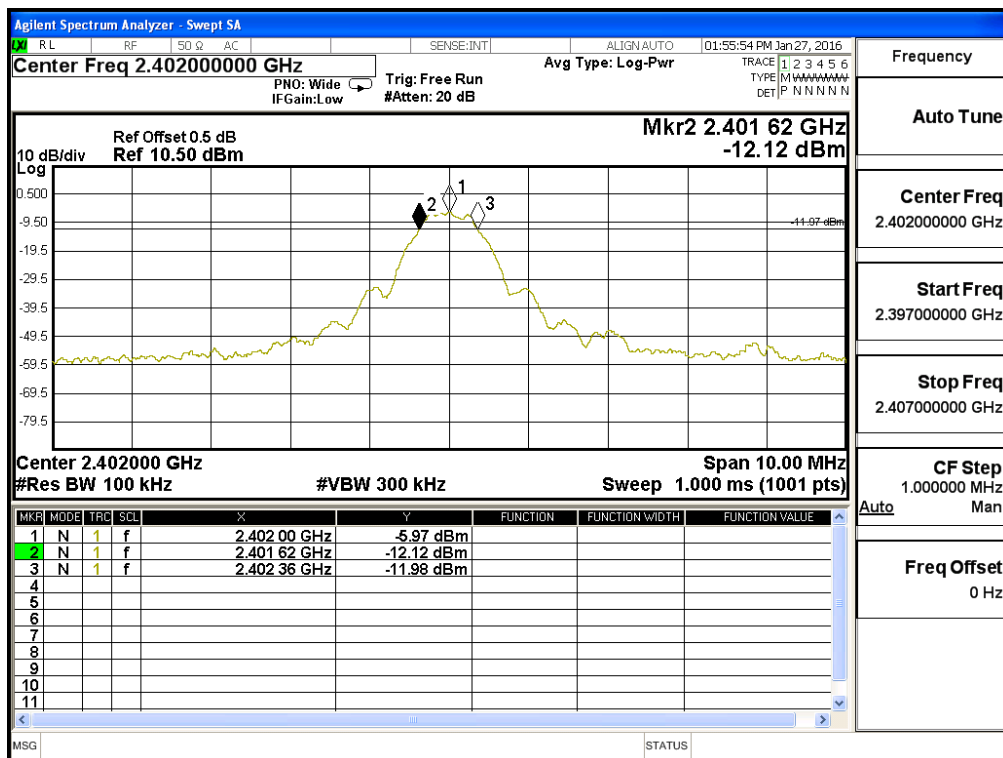


Figure Channel 19:


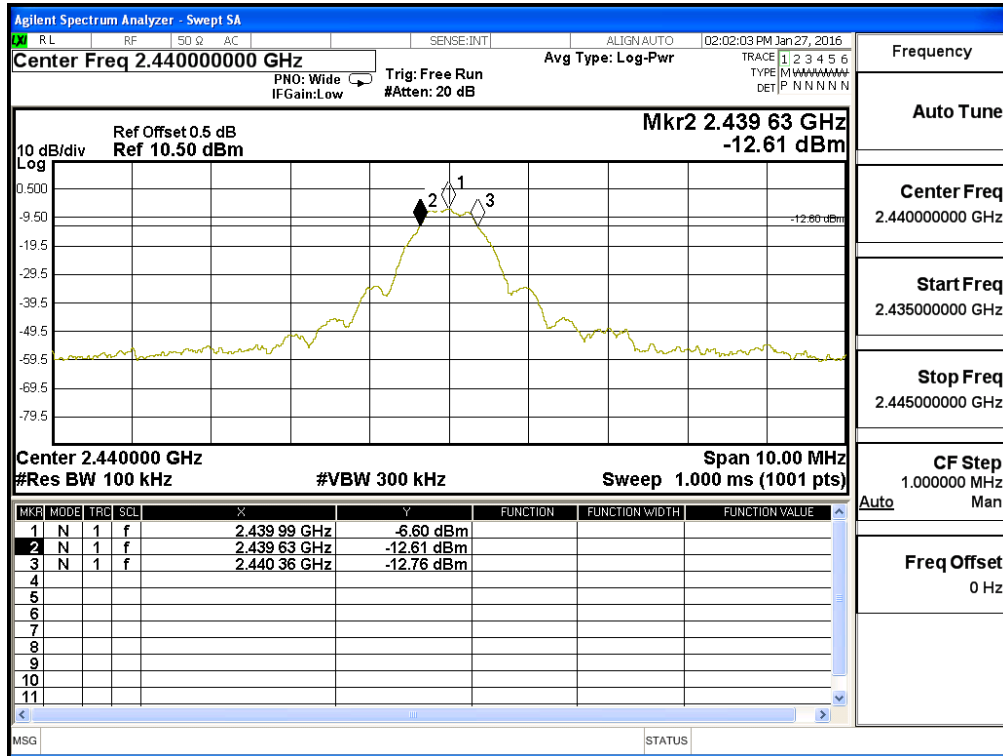


Figure Channel 39:

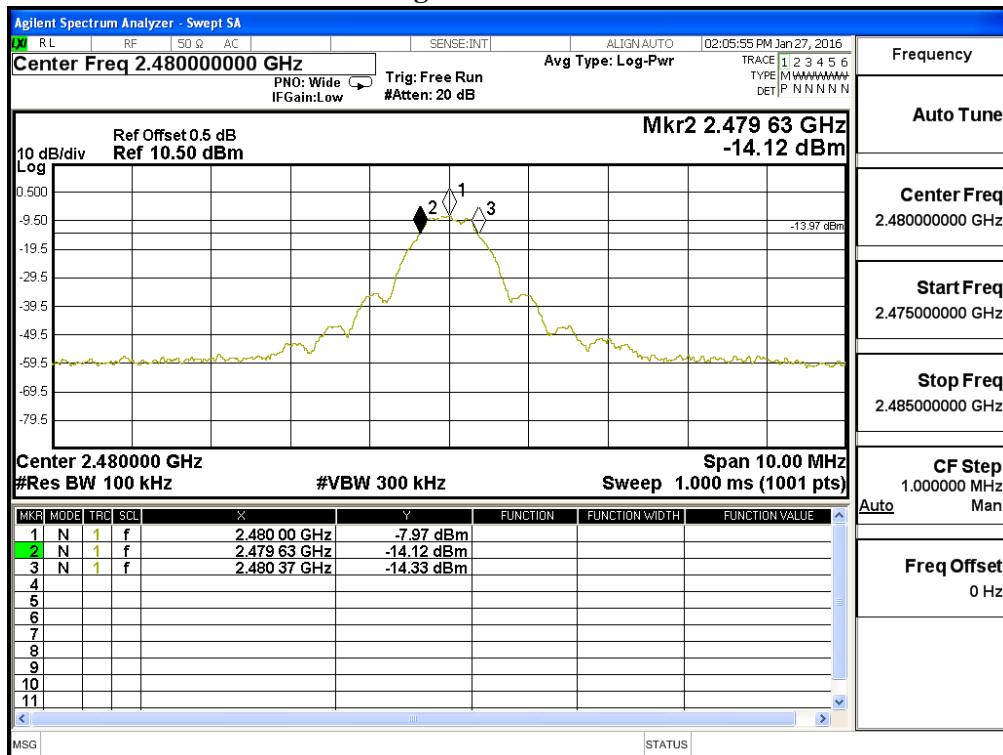

## 8. Power Density


### 8.1. Test Equipment

	Equipment	Manufacturer	Model No./Serial No.	Last Cal.
	Spectrum Analyzer	R&S	FSP40 / 100170	Jun., 2015
	Spectrum Analyzer	Agilent	E4407B / US39440758	Jun., 2015
X	Spectrum Analyzer	Agilent	N9010A / MY48030495	Apr., 2015

Note:

1. All equipments are calibrated with traceable calibrations. Each calibration is traceable to the national or international standards.
2. The test instruments marked with “X” are used to measure the final test results.
3. All equipments are calibrated every one year.

### 8.2. Test Setup

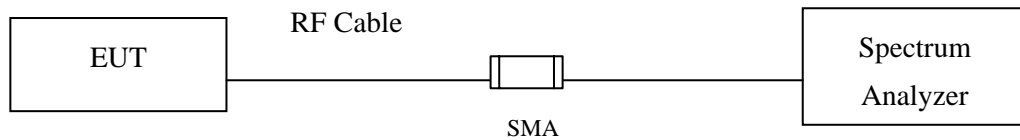

### 8.3. Limits

The transmitted power density averaged over any 1 second interval shall not be greater +8dBm in any 3kHz bandwidth.

### 8.4. Test Procedure

The EUT was setup according to ANSI C63.10: 2013, the maximum power spectral density using KDB 558074 section 10.2 PKPSD (peak PSD) method.

### 8.5. Uncertainty

± 1.27 dB



### 8.6. Test Result of Power Density

Product : Automatic Wrist Blood Pressure Monitor  
 Test Item : Power Density Data  
 Test Site : No.3 OATS  
 Test Mode : Mode 1: Transmit - BLE (GFSK)

Channel No.	Frequency (MHz)	Measure Level (dBm)	Limit (dBm)	Result
00	2402	-6.240	< 8dBm	Pass
19	2440	-6.880	< 8dBm	Pass
39	2480	-8.290	< 8dBm	Pass

**Figure Channel 00:**

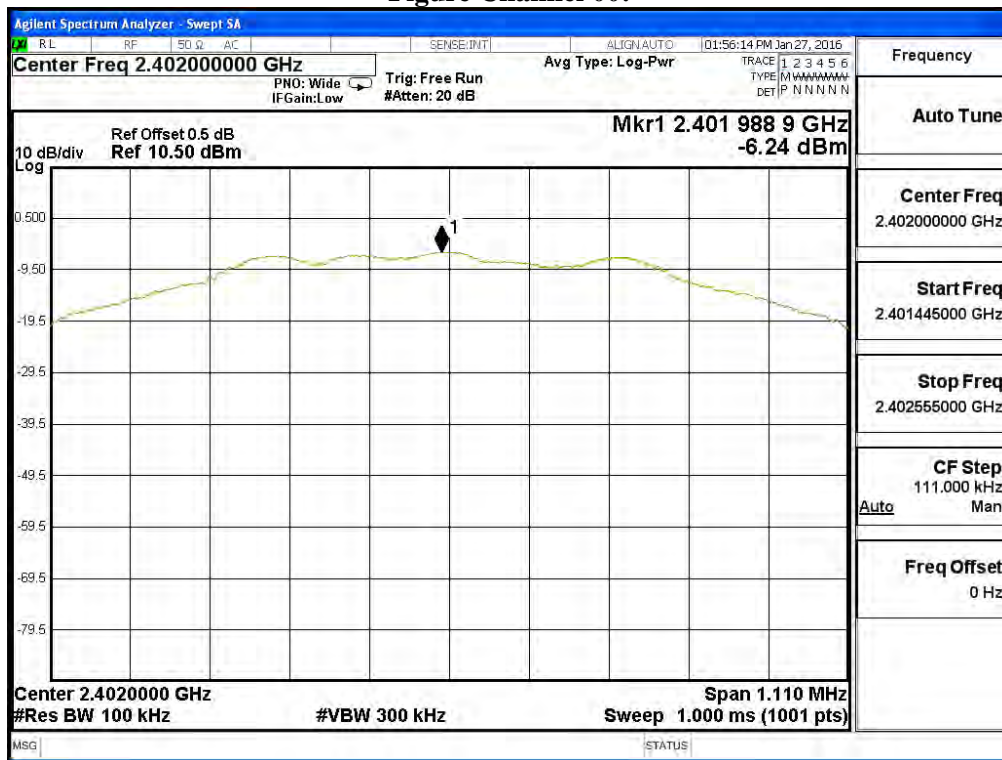


Figure Channel 19:


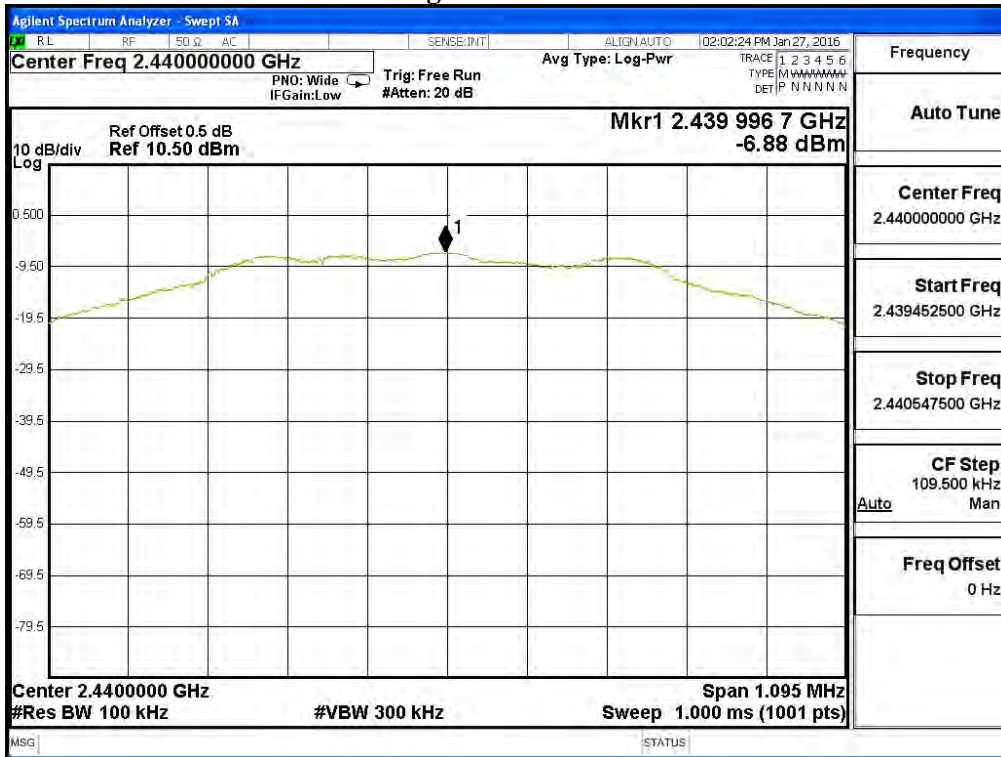


Figure Channel 39:

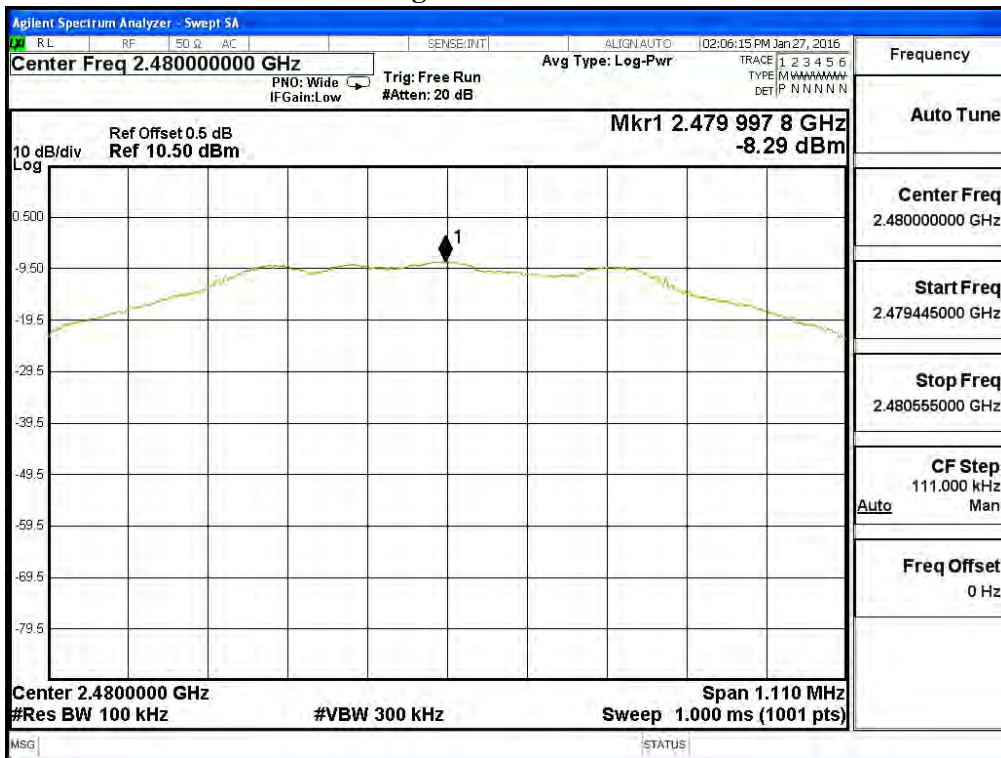

**9. EMI Reduction Method During Compliance Testing**

No modification was made during testing.