Calibration Laboratory of Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland

Sporton

Client



Schweizerischer Kalibrierdienst

- S Service suisse d'étalonnage
- C Servizio svizzero di taratura
- S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Certificate No: D6.5GHzV2-1026_Jan21

CALIBRATION CERTIFICATE

Object	D6.5GHzV2 - SN:	1026	
Calibration procedure(s)	QA CAL-22.v5 Calibration Procee	dure for SAR Validation Sources	between 3-10 GHz
Calibration date:	January 29, 2021		
The measurements and the uncertain	ainties with confidence pr	onal standards, which realize the physical unit obability are given on the following pages and y facility: environment temperature (22 ± 3)°C	I are part of the certificate.
	D#	Cal Date (Certificate No.)	Scheduled Calibration
Primary Standards Power meter NRP	SN: 104778	01-Apr-20 (No. 217-03100/03101)	Apr-21
Power sensor NRP-Z91	SN: 103244	01-Apr-20 (No. 217-03100)	Apr-21
Power sensor NRP-Z91	SN: 103245	01-Apr-20 (No. 217-03101)	Apr-21
Reference 20 dB Attenuator	SN: BH9394 (20k)	31-Mar-20 (No. 217-03106)	Apr-21
	SN: 310982 / 06327	31-Mar-20 (No. 217-03104)	Apr-21
Type-N mismatch combination	SN: 7405	30-Dec-20 (No. EX3-7405_Dec20)	Dec-21
Reference Probe EX3DV4 DAE4	SN: 908	14-Aug-20 (No. DAE4-908_Aug20)	Aug-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor R&S NRP33T	SN: 100967	17-Oct-16 (in house check Dec-18)	In house check: Dec-21
RF generator Anapico APSIN20G	SN: 669	28-Mar-17 (in house check Dec-18)	In house check: Dec-21
	SN: 101093	10-May-12 (in house check Dec-18)	In house check: Dec-21
Network Analyzer R&S ZVL13	T. Street and the second	To may 12 (in house one in sec. 19)	In house check. Dec 21
Network Analyzer R&S ZVL13	Name	Function	Signature
Network Analyzer R&S ZVL13 Calibrated by:			
	Name	Function	

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst

S Service suisse d'étalonnage

С Servizio svizzero di taratura

S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossarv:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528 ED1, "Measurement procedure for the assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-worn wireless communication devices - Part 1528: Human models, instrumentation and procedures (Frequency range of 4 MHz to 10 GHz)", draft 2019

Additional Documentation:

b) DASY6 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.
- The absorbed power density (APD): The absorbed power density is evaluated according to Samaras T, Christ A, Kuster N, "Compliance assessment of the epithelial or absorbed power density above 6 GHz using SAR measurement systems", Bioelectromagnetics, 2021 (submitted). The additional evaluation uncertainty of 0.55 dB (rectangular distribution) is considered.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Accreditation No.: SCS 0108

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY6	V6.14
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	5 mm	with Spacer
Zoom Scan Resolution	dx, dy = 3.4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	6500 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	34.5	6.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	6.20 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	12222	N ativi

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	29.0 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	290 W/kg ± 24.7 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition		
SAR measured	100 mW input power	5.33 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	53.4 W/kg ± 24.4 % (k=2)	

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.4 Ω - 4.8 jΩ		
Return Loss	- 25.9 dB		

APD (Absorber Power Density)

APD averaged over 1 cm ²	Condition	
APD measured	100 mW input power	290 W/m ²
APD measured	normalized to 1W	2900 W/m ² ± 29.2 % (k=2)

APD averaged over 4 cm ²	condition		
APD measured	100 mW input power	133 W/m ²	
APD measured	normalized to 1W	1330 W/m ² ± 28.9 % (k=2)	

*The reported APD values have been derived using psSAR10g. cDASY6 V6.16+ will use psSAR8g resulting in more accurate estimation of the APD values. The estimated offset is less than - 0.15 dB.

General Antenna Parameters and Design

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.


Additional EUT Data

Manufactured by	SPEAG
	A


DASY6 Validation Report for Head TSL

Measurement Report for D6.5GHz-1026, UID 0 -, Channel 6500 (6500.0MHz)

Device under 1							
Name, Manufa	acturer D	imensions	[mm]	IMEI	DUT Typ	e	
D6.5GHz	3	16.0 x 6.0 x	300.0	SN: 1026	35		
Exposure Cond	ditions						
Phantom	Position, Test	Band	Group,	Frequency	Conversion	TSL Cond.	TSL
Section, TSL	Distance [mm]		UID	[MHz]	Factor	[S/m]	Permittivity
Flat, HSL	5.00	Band	CW,	6500	5.75	6.20	34.8
Hardware Set	up						
Phantom		TSL		Probe, Ca	libration Date	DAE, Calib	oration Date
MFP V8.0 Cent	ter - 1182	HBBL600-10	0000V6	EX3DV4 - 5	SN7405, 2020-12-30	DAE4 Sn9	08, 2020-08-14
Scan Setup				Measurem	nent Results		
			Zoom S	ican			Zoom Scan
Grid Extents	[mm]		22.0 x 22.0 x 2	22.0 Date		2	021-01-21, 10:31
Grid Steps [n			3.4 x 3.4 x	1.4 psSAR1g	[W/Kg]		29.0
Sensor Surfa	100 B			1.4 psSAR10	g [W/Kg]		5.33
Graded Grid				Yes Power D	rift [dB]		0.00
Grading Ratio	0			1.4 Power So	caling		Disabled
MAIA				N/A Scaling F	actor [dB]		
Surface Dete	ection		VMS	+ 6p TSL Corr	ection		Enabled
Scan Method	Y.		Meas	ured M2/M1	[%]		50.3
ಂದುವ ಮಾಲುಗಳಿಗೆ ಕಿಂದ ಗಳಲ್ಲಿ ನಿನ				Dist 3dB	Peak [mm]		4.8

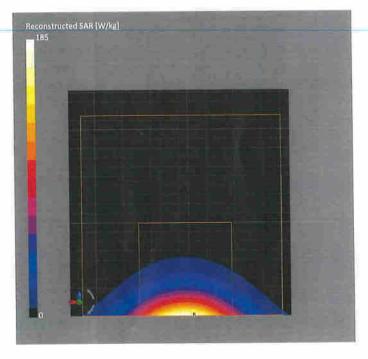

Impedance Measurement Plot for Head TSL

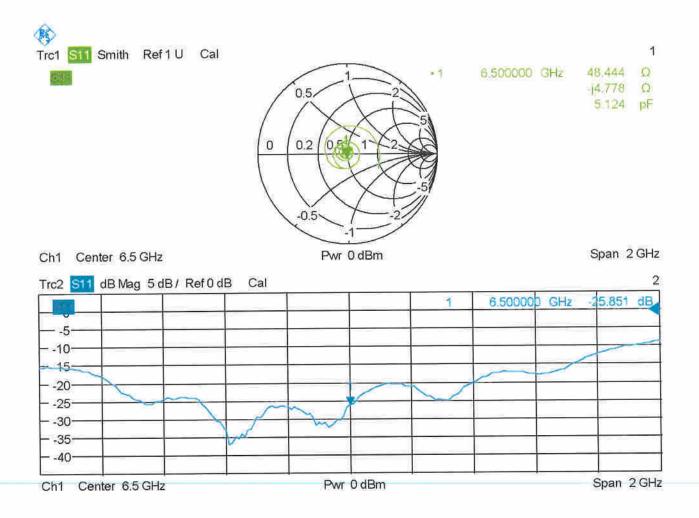



D6.5GV2, Serial No. 1026 Extended Dipole Calibrations

Referring to KDB 865664 D01, if dipoles are verified in return loss (<-20dB, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

D6.5GV2 – serial no. 1026							
		6.5G Head					
Date of Measurement	Return-Loss (dB)	Delta (%) Real Impedance (ohm) Delta (ohm)					
2021.1.29	-25.9		48.4		-4.8		
2022.1.28	-26.2	1.2%	48.5	-0.1	-4.6	-0.2	


<Justification of the extended calibration>

The return loss is < -20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.



Dipole Verification Data> D6.5V2, serial no. 1026

6.5GHz – Head----2022.1.28

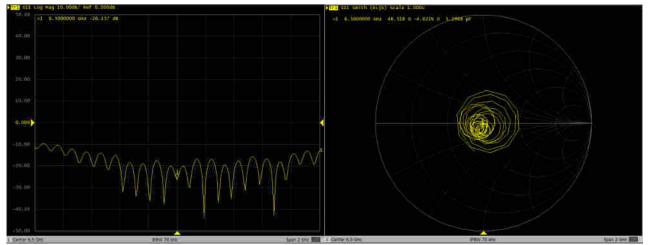

Calibration Laboratory of Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst

Service suisse d'étalonnage

S

С Servizio svizzero di taratura S

Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client Sporton

Certificate No: 5G-Veri10-2002_Nov21

CALIBRATION CERTIFICATE

Object	5G Verification So	urce 10 GHz - SN: 2002	-19 Million - 19 M
Calibration procedure(s)	QA CAL-45.v3 Calibration proced	lure for sources in air above 6 GHz	
Calibration date:	November 26, 202	21	
		nal standards, which realize the physical units of m bability are given on the following pages and are p	0.2
All calibrations have been conducte	ed in the closed laboratory	facility: environment temperature (22 \pm 3)°C and I	numidity < 70%.
Calibration Equipment used (M&TE	critical for calibration)		
Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Reference Probe EUmmWV3	SN: 9374	2020-12-30(No. EUmmWV3-9374_Dec20)	Dec-21
DAE4ip	SN: 1602	SN: 1602 2021-06-25 (No. DAE4ip-1602_Jun21)	
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Calibrated by:	Name Leif Klysner	Function Laboratory Technician	Signature Set Tiler
Approved by:	Niels Kuster	Quality Manager	1 And
50% CB			
This calibration certificate shall not	be reproduced except in t	full without written approval of the laboratory.	Issued: November 29, 2021

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S

Schweizerischer Kalibrierdienst

Service suisse d'étalonnage C

Servizio svizzero di taratura

Accreditation No.: SCS 0108

S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossarv

CW

Continuous wave

Calibration is Performed According to the Following Standards

- Internal procedure QA CAL-45-5Gsources
- IEC TR 63170 ED1. "Measurement procedure for the evaluation of power density related to . human exposure to radio frequency fields from wireless communication devices operating between 6 GHz and 100 GHz", January 2018

Methods Applied and Interpretation of Parameters

- Coordinate System: z-axis in the waveguide horn boresight, x-axis is in the direction of the E-field, y-axis normal to the others in the field scanning plane parallel to the horn flare and horn flange.
- Measurement Conditions: (1) 10 GHz: The radiated power is the forward power to the horn antenna minus ohmic and mismatch loss. During the measurements, the horn is directly connected to the cable and the antenna ohmic and mismatch losses are determined by farfield measurements. (2) 30, 45, 60 and 90 GHz: The verification sources are switched on for at least 30 minutes. Absorbers are used around the probe cub and at the ceiling to minimize reflections.
- Horn Positioning: The waveguide horn is mounted vertically on the flange of the waveguide source to allow vertical positioning of the EUmmW probe during the scan. The plane is parallel to the phantom surface. Probe distance is verified using mechanical gauges positioned on the flare of the horn.
- E- field distribution: E field is measured in two x-y-plane (10mm, 10mm + $\lambda/4$) with a vectorial E-field probe. The E-field value stated as calibration value represents the E-fieldmaxima and the averaged (1cm² and 4cm²) power density values at 10mm in front of the horn.
- Field polarization: Above the open horn, linear polarization of the field is expected. This is verified graphically in the field representation.

Calibrated Quantity

- Local peak E-field (V/m) and average of peak spatial components of the poynting vector (W/m^2) averaged over the surface area of 1 cm² and 4cm² at the nominal operational
- frequency of the verification source. Both square and circular averaging results are listed.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	cDASY6 Module mmWave	V2.4
Phantom	5G Phantom	PERSONAL AND A CONTRACT OF
Distance Horn Aperture - plane	10 mm	
XY Scan Resolution	dx, dy = 7.5 mm	
Number of measured planes	2 (10mm, 10mm + λ/4)	
Frequency	10 GHz ± 10 MHz	

Calibration Parameters, 10 GHz

Circular Averaging

Distance Horn Aperture	Prad ¹	Max E-field	Uncertainty	Avg Power Density		Uncertainty
to Measured Plane	(mW)	(V/m)	(k = 2)	Avg (psPDn+, psPDtot+, psPDmod+)		(k = 2)
				(W/m ²)		
				1 cm ²	4 cm ²	
10 mm	125	266	1.27 dB	187	151	1.28 dB

Square Averaging

Distance Horn Aperture to Measured Plane	Prad¹ (mW)	Max E-field (V/m)	Uncertainty (k = 2)	Avg (psPDn+, psl	er Density ^{PDtot+, psPDmod+)} /m ²)	Uncertainty (k = 2)
				1 cm ²	4 cm ²	
10 mm	125	266	1.27 dB	188	150	1.28 dB

 $^{^{\}rm I}$ Assessed ohmic and mismatch loss plus numerical offset: 0.95 dB

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

Device under Test Pro	operties				
Name, Manufacturer	Dimensions [mm	1]	IME	DUT Type	
SG Verification Source 10 G	iHz 100.0 x 100.0 x 1	100.0	SN: 2002		
Exposure Conditions					
Phantom Section	Position, Test Distance [mm]	Band	Group,	Frequency [MHz], Channel Number	Conversion Factor
5G -	10.0 mm	Validation band	CW	10000.0, 10000	1.0
Hardware Setup	Medium				
mmWave Phantom - 1002	Air		Probe, Calibra EUmmWV3 - 5 2020-12-30	stion Date SN9374_F1-78GHz,	DAE, Calibration Date DAE4ip Sn1602, 2021-06-25
Scan Setup			Measurem	ent Results	
		5G S	can		5G Scan
Grid Extents [mm]		120.0 x 12	20.0 Date		2021-11-26, 12:09
Grid Steps [lambda]		0.25 x (m²]	1.00
Sensor Surface [mm]			LO.0 psPDn+ (W/	m²]	187
MAIA		MAIA not u	sed psPDtot+ [W	//m²]	187

psPDmod+ [W/m²]


Power Drift [dB]

E_{max} [V/m]

188


266

0.02

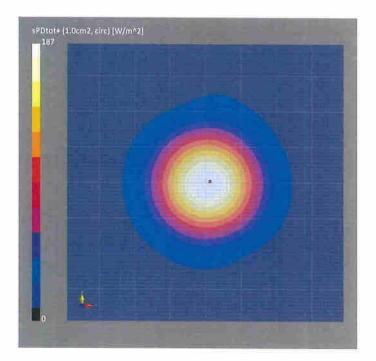


Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

Name, Manufacturer	Dimensions [mm	1	IMEI	DUT Type	
5G Verification Source 10 (GHz 100.0 x 100.0 x 1	100.0	SN: 2002	3	
Exposure Conditions					
Phantom Section	Position, Test Distance [mm]	Band	Group,	Frequency [MHz], Channel Number	Conversion Factor
5G -	10.0 mm	Validation band	CW	10000.0, 10000	1.0
Hardware Setup					
Phantom	Medium		Probe, Calib	ration Date	DAE, Calibration Date
mmWave Phantom - 1002	Air		EUmmWV3 2020-12-30	- SN9374_F1-78GHz,	DAE4ip Sn1602, 2021-06-25
Scan Setup			Measurer	nent Results	
		5G S			5G Scan
Grid Extents [mm]		120.0 x 12			2021-11-26, 12:09
Grid Steps [lambda]		0.25 x 0	the second se		4.00
Sensor Surface [mm]			0.0 psPDn+ [W	01002/322	150
MAIA		MAIA not u	Conservation and the second se		150
			psPDmod+		153
			Emax [V/m]		266

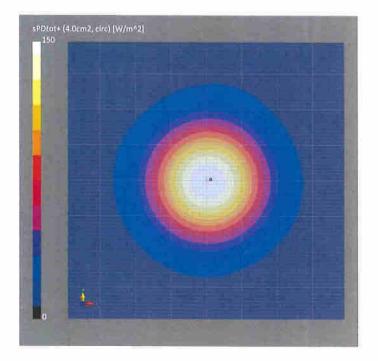


Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

Device under Test Pro Name, Manufacturer	Dimensions [mm	a) U	IMEL	DUITT	
5G Verification Source 10 G			SN: 2002	DUT Type	
			511. 2002	352	
Exposure Conditions					
Phantom Section	Position, Test Distance [mm]	Band	Group,	Frequency [MHz], Channel Number	Conversion Factor
5G -	10.0 mm	Validation band	CW	10000.0, 10000	1.0
Hardware Setup					
Phantom	Medium		Probe, Calib	ration Date	DAE, Calibration Date
mmWave Phantom - 1002	Air		EUmmWV3 2020-12-30	- SN9374_F1-78GHz,	DAE4ip Sn1602, 2021-06-25
Scan Setup			Measurer	nent Results	
		5G S	can		5G Scan
Grid Extents [mm]		120.0 x 12	0.0 Date		2021-11-26, 12:09
Grid Steps [lambda]		0.25 x 0			1.00
Sensor Surface [mm]			0.0 psPDn+[W	//m²]	187
MAIA		MAIA not u	25-CH 25-SA 5-SA (A)		187
			psPDmod+		189
			E _{max} [V/m]		266
			Power Drif	t [dB]	0.02

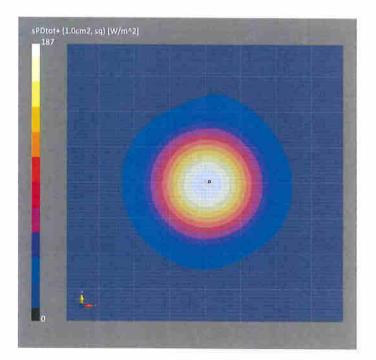

Measurement Report for 5G Verification Source 10 GHz, UID 0 -, Channel 10000 (10000.0MHz)

Device under Test Pro Name, Manufacturer	Dimensions (mm	a l	IMEI		
5G Verification Source 10 G		Second and the second s	SN: 2002	DUT Type	
Exposure Conditions					
Phantom Section	Position, Test Distance [mm]	Band	Group,	Frequency [MHz], Channel Number	Conversion Factor
5G -	10.0 mm	Validation band	CW	10000.0, 10000	1.0
Hardware Setup					
Phantom	Medium		Probe, Calib	ration Date	DAE, Calibration Date
mmWave Phantom - 1002	Air		The second se	- SN9374 F1-78GHz,	DAE4ip Sn1602,
			2020-12-30	245.05555557.55 4 - 240737876525705780	2021-06-25
Scan Setup			Measurer	ment Results	
		5G S		lient Results	5G Scan
Grid Extents [mm]		120.0 x 12			2021-11-26, 12:09
Grid Steps [lambda]		0.25 × 0		cm ²]	2021-11-26, 12:09
Sensor Surface [mm]			0.0 psPDn+ [W		4.00
MAIA		MAIA not us	2262 AAAAAAAAAAAAAAAAAAAAAAAAAAAAAAAAAA		149
			psPDmod+		153
			E _{max} [V/m]		266
			Power Drif		0.02

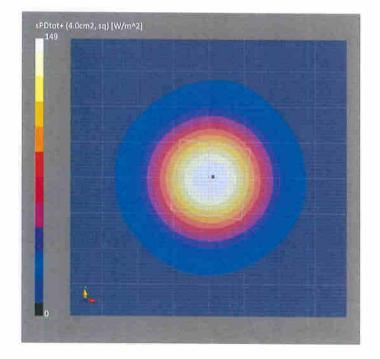

Schmid & Partner Engineering AG

pe a S 0

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 www.speag.swiss, info@speag.swiss

IMPORTANT NOTICE

USAGE OF THE DAE4

The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:

Battery Exchange: The battery cover of the DAE4 unit is fixed using a screw, over tightening the screw may cause the threads inside the DAE to wear out.

Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an antistatic bag. This antistatic bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.

E-Stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements.

Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect.

DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file.

Important Note:

Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer.

Important Note:

Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the Estop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure.

Important Note:

To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst

Service suisse d'étalonnage

Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client Sporton

Certificate No: DAE4-1210_Apr22

CALIBRATION CERTIFICATE

	DAE4 - SD 000 D	04 BM - SN: 1210	
Calibration procedure(s)		dure for the data acquisition elec	stronics (DAE)
Calibration date:	April 12, 2022		
The measurements and the unce	rtainties with confidence pro	nal standards, which realize the physical un obability are given on the following pages ar r facility: environment temperature (22 ± 3)°(id are part of the certificate.
Primary Standards	ID #	Cal Date (Certificate No.)	
AND		odi Dato (Oortinicate 140.)	Scheduled Calibration
AND	SN: 0810278	31-Aug-21 (No:31368)	Aug-22
Keithley Multimeter Type 2001 Secondary Standards	SN: 0810278	31-Aug-21 (No:31368)	Aug-22
Keithley Multimeter Type 2001		31-Aug-21 (No:31368) Check Date (in house) 24-Jan-22 (in house check)	
Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit	ID # SE UWS 053 AA 1001 SE UMS 006 AA 1002	31-Aug-21 (No:31368) Check Date (in house) 24-Jan-22 (in house check) 24-Jan-22 (in house check) Function	Aug-22 Scheduled Check In house check: Jan-23
Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit Calibrator Box V2.1	ID # SE UWS 053 AA 1001 SE UMS 006 AA 1002	31-Aug-21 (No:31368) Check Date (in house) 24-Jan-22 (in house check) 24-Jan-22 (in house check)	Aug-22 Scheduled Check In house check: Jan-23 In house check: Jan-23
Keithley Multimeter Type 2001 Secondary Standards Auto DAE Calibration Unit Calibrator Box V2.1	ID # SE UWS 053 AA 1001 SE UMS 006 AA 1002	31-Aug-21 (No:31368) Check Date (in house) 24-Jan-22 (in house check) 24-Jan-22 (in house check) Function	Aug-22 Scheduled Check In house check: Jan-23 In house check: Jan-23

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst

- C Service suisse d'étalonnage
 - Servizio svizzero di taratura
- S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary DAE data acquisition electronics Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle*: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - Power consumption: Typical value for information. Supply currents in various operating modes.

DC Voltage Measurement

Calibration Factors	X	Y	Z
High Range	404.304 ± 0.02% (k=2)	405.025 ± 0.02% (k=2)	404.439 ± 0.02% (k=2)
Low Range	3.98747 ± 1.50% (k=2)	3.97254 ± 1.50% (k=2)	3.98649 ± 1.50% (k=2)

Connector Angle

Connector Angle to be used in DASY system	345.5 ° ± 1 °

Appendix (Additional assessments outside the scope of SCS0108)

High Range		Reading (µV)	Difference (µV)	Error (%)
Channel X	+ Input	200034.27	-4.82	-0.00
Channel X	+ Input	20007.80	1.97	0.01
Channel X	- Input	-20003.01	2.83	-0.01
Channel Y	+ Input	200040.96	6.66	0.00
Channel Y	+ Input	20003.50	-2.14	-0.01
Channel Y	- Input	-20008.78	-2.75	0.01
Channel Z	+ Input	200032.00	-2.42	-0.00
Channel Z	+ Input	20004.35	-1.29	-0.01
Channel Z	- Input	-20006.24	-0.09	0.00

1. DC Voltage Linearity

Low Range		Reading (μV)	Difference (µV)	Error (%)
Channel X	+ Input	2001.09	-0.27	-0.01
Channel X	+ Input	201.46	0.11	0.06
Channel X	- Input	-198.65	0.03	-0.01
Channel Y	+ Input	2001.07	-0.17	-0.01
Channel Y	+ Input	200.38	-0.79	-0.39
Channel Y	- Input	-199.94	-1.09	0.55
Channel Z	+ Input	2001.26	0.13	0.01
Channel Z	+ Input	200.60	-0.46	-0.23
Channel Z	- Input	-199.35	-0.48	0.24

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	24.21	22.26
	- 200	-22.93	-23.92
Channel Y	200	-10.72	-10.99
	- 200	9.31	8.79
Channel Z	200	-15.35	-15.84
	- 200	14.57	14.52

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Υ (μV)	Channel Z (μV)
Channel X	200	-	2.48	-3.75
Channel Y	200	7.94	-	3.86
Channel Z	200	9.70	6.29	-

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15716	15644
Channel Y	16222	16304
Channel Z	15930	16151

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input 10MΩ

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (μV)
Channel X	1.09	-1.13	2.70	0.57
Channel Y	-0.58	-1.47	0.64	0.43
Channel Z	-0.33	-2.37	0.63	0.44

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Calibration Laboratory of Schmid & Partner Engineering AG

Sporton

Client

Zeughausstrasse 43, 8004 Zurich, Switzerland

Iac MRA



S Schweizerischer Kalibrierdienst

- C Service suisse d'étalonnage
- Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 0108

Certificate No

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accredited by the Swiss Accreditation Service (SAS)

EX-3935_Jun22

CALIBRATION CERTIFICATE

Object	EX3DV4 - SN:3935
Calibration procedure(s)	QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v6, QA CAL-23.v5, QA CAL-25.v7 Calibration procedure for dosimetric E-field probes
Calibration date	June 20, 2022
This calibration certificate doc	suments the traceability to national standards, which realize the physical units of measurements (SI).

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3) °C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-22 (No. 217-03525/03524)	Apr-23
Power sensor NRP-Z91	SN: 103244	04-Apr-22 (No. 217-03524)	Apr-23
OCP DAK-3.5 (weighted)	SN: 1249	20-Oct-21 (OCP-DAK3.5-1249 Oct21)	Oct-22
OCP DAK-12	SN: 1016	20-Oct-21 (OCP-DAK12-1016 Oct21)	Oct-22
Reference 20 dB Attenuator	SN: CC2552 (20x)	04-Apr-22 (No. 217-03527)	Apr-23
DAE4	SN: 660	13-Oct-21 (No. DAE4-660_Oct21)	Oct-22
Reference Probe ES3DV2	SN: 3013	27-Dec-21 (No. ES3-3013 Dec21)	Dec-22

Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-20)	In house check: Jun-22
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-20)	In house check: Jun-22
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-20)	In house check: Jun-22
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-20)	In house check: Jun-22
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-20)	In house check: Oct-22

	Name	Function	Signature
Calibrated by	Jeton Kastrati	Laboratory Technician	felle
Approved by	Sven Kühn	Technical Manager	5.2
This calibration certificate	e shall not be reproduced except in	n full without written approval of the lat	Issued: June 24, 2022 poratory.

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst

- Service suisse d'étalonnage
- С Servizio svizzero di taratura
- S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization <i>9</i>	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization
 ∂ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E2-field uncertainty inside TSL (see below ConvF).
- NORM(f)x, y, z = NORMx, y, z * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- · DCPx, y, z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency nor media.
- · PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- · Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx, y, z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ±50 MHz to ±100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- · Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc $(k = 2)$
Norm (µV/(V/m) ²) ^A	0.50	0.53	0.48	±10.1%
DCP (mV) ^B	104.0	103.0	104.0	±4.7%

Calibration Results for Modulation Response

UID	Communication System Name		A dB	B dBõV	С	D dB	VR mV	Max dev.	Max Unc ^E k = 2
0	CW	X	0.00	0.00	1.00	0.00	141.0	±2.7%	±4.7%
		Y	0.00	0.00	1.00	1	149.2		
		Z	0.00	0.00	1.00		141.9	1	
10352	Pulse Waveform (200Hz, 10%)	X	20.00	92.32	21.85	10.00	60.0	±3.0%	±9.6%
		Y	20.00	90.25	21.10	-	60.0		
		Z	20.00	92.40	21.82		60.0	1	
10353	Pulse Waveform (200Hz, 20%)	X	20.00	93.64	21.28	6.99	80.0	±1.6%	±9.6%
		Y	20.00	89.88	19.93		80.0		
		Z	20.00	93.42	21.15		80.0	1	
10354	Pulse Waveform (200Hz, 40%)	X	20.00	96.56	21.10	3.98	95.0	±1.2%	±9.6%
	±2	Y	20.00	91.11	19.26		95.0	1.575.007.007.0	
		Z	20.00	95.65	20.71		95.0		
10355	Pulse Waveform (200Hz, 60%)	X	20.00	94.32	18.56	2.22	120.0	±1.0%	±9.6%
		Y	20.00	93.51	19.15	=x=2751	120.0		20.070
		Z	20.00	96.57	19.67		120.0		
10387	QPSK Waveform, 1 MHz	X	1.53	65.53	14.15	1.00	150.0	±2.9%	±9.6%
		Y	1.67	66.29	15.01	1 12000	150.0		20.070
		Z	1.43	63.95	13.43	6	150.0		
10388	QPSK Waveform, 10 MHz	X	2.06	67.20	15.01	0.00	150.0	±0.8%	±9.6%
		Y	2.25	68.34	15.78	21.5.5	150.0	20.070	20.070
		Z	2.07	66.87	14.75		150.0		
10396	64-QAM Waveform, 100 kHz	X	2.68	68.76	17.82	3.01	150.0	±0.7%	±9.6%
		Y	3.24	72.12	19.60	2.5	150.0		20.070
		Z	2.96	70.93	18.85		150.0		
10399	64-QAM Waveform, 40 MHz	X	3.40	66.88	15.44	0.00	150.0	±2.5%	±9.6%
		Y	3.51	67.28	15.79		150.0		-0.070
		Z	3.42	66.79	15.33		150.0		
10414	WLAN CCDF, 64-QAM, 40 MHz	X	4.79	65.69	15.41	0.00	150.0	±4.3%	±9.6%
		Y	4.88	65.78	15.56		150.0	1.070	10.078
		Z	4.63	64.93	14.97	-	150.0		

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

^B Linearization parameter uncertainty for maximum specified field strength. ^E Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Sensor Model Parameters

	fF	C2 fF	v ^{−1}	11 msV ⁻²	T2 ms V ⁻¹	T3 ms	T4 V ⁻²	T5 V ⁻¹	Т6
x	42.0	309.00	34.59	14.62	0.52	5.10	0,10	0.44	1.01
У	47.0	347.17	34.86	29.21	0.40	5.10	1.00	0.44	10.75
Z	44.9	329.88	34.43	15.66	0.43	5.10	1.61	0.34	1.01

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle	-134.4°
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	
Probe Overall Length	disabled
Probe Body Diameter	337 mm
Tip Length	10 mm
Tip Diameter	9 mm
Probe Tip to Sensor X Calibration Point	2.5 mm
	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm
	Germin

Note: Measurement distance from surface can be increased to 3-4 mm for an Area Scan job.

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity ^F (S/m)	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unc (k = 2)
750	41.9	0.89	10.37	10.37	10.37	0.50	0.80	±12.0%
835	41.5	0.9	10.10	10.10	10.10	0.46	0.80	±12.0%
900	41.5	0.97	9.85	9.85	9.85	0.38	0.96	±12.0%
1450	40.5	1.2	8.89	8.89	8.89	0.49	0.80	±12.0%
1750	40.1	1.37	8.80	8.80	8.80	0.35	0.86	±12.0%
1900	40.0	1.4	8.50	8.50	8.50	0.34	0.86	±12.0%
2000	40.0	1.4	8.41	8.41	8.41	0.41	0.86	±12.0%
2300	39.5	1.67	8.14	8.14	8.14	0.39	0.90	±12.0%
2450	39.2	1.8	7.69	7.69	7.69	0.41	0.90	±12.0%
2600	39.0	1.96	7.56	7.56	7.56	0.45	0.90	±12.0%
3300	38.2	2.71	7.35	7.35	7.35	0.25	1.30	±13.1%
3500	37.9	2.91	7.00	7.00	7.00	0.25	1.30	±13.1%
3700	37.7	3.12	6.99	6.99	6.99	0.30	1.35	±13.1%
3900	37.5	3.32	6.96	6.96	6.96	0.30	1.30	±13.1%
4100	37.2	3.53	6.89	6.89	6.89	0.35	1.50	±13.1%
4200	37.1	3.63	6.80	6.80	6.80	0.35	1.50	±13.1%
4400	36.9	3.84	6.53	6.53	6.53	0.40	1.60	±13.1%
4600	36.7	4.04	6.40	6.40	6.40	0.40	1.60	±13.1%
4800	36.4	4.25	6.39	6.39	6.39	0.40	1.80	±13.1%
4950	36.3	4.4	6.15	6.15	6.15	0.40	1.80	±13.1%
5250	35.9	4.71	5.02	5.02	5.02	0.40	1.80	±13.1%
5600	35.5	5.07	4.75	4.75	4.75	0.40	1.80	±13.1%
5750	35.4	5.22	4.70	4.70	4.70	0.40	1.80	±13.1%

^C Frequency validity above 300 MHz of ±100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ±50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10 , 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Validity of ConvF assessed at 6 MHz is 4-9 MHz, and ConvF assessed at 13 MHz is 9-19 MHz. Above 5 GHz frequency validity can be extended to ± 100 MHz. F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 100 MHz.

values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz and below ±2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity ^F (S/m)	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unc (k = 2)
6500	34.5	6.07	5.80	5.80	5.80	0.20	2.50	±18.6%

C Frequency validity at 6.5 GHz is -600/+700 MHz, and ±700 MHz at or above 7 GHz. The uncertainty is the RSS of the ConvF uncertainty at calibration F At frequencies 6–10 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR


values. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz; below ±2% for frequencies between 3-6 GHz; and below ±4% for frequencies between 6-10 GHz at any distance larger than half the probe tip diameter from the boundary.

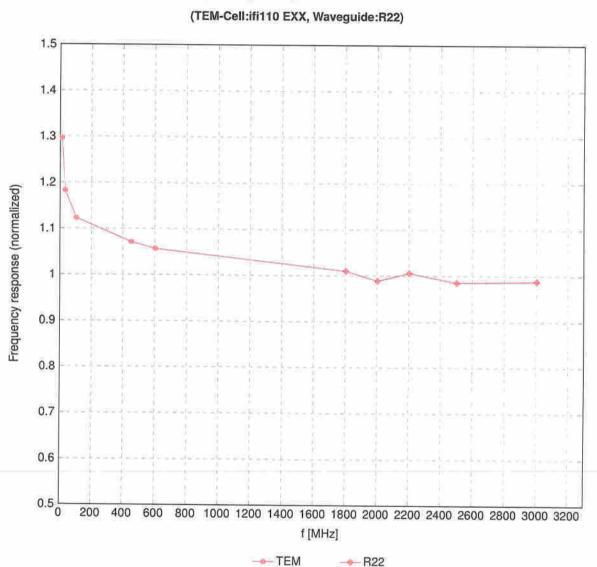


Frequency Response of E-Field

Uncertainty of Frequency Response of E-field: ±6.3% (k=2)

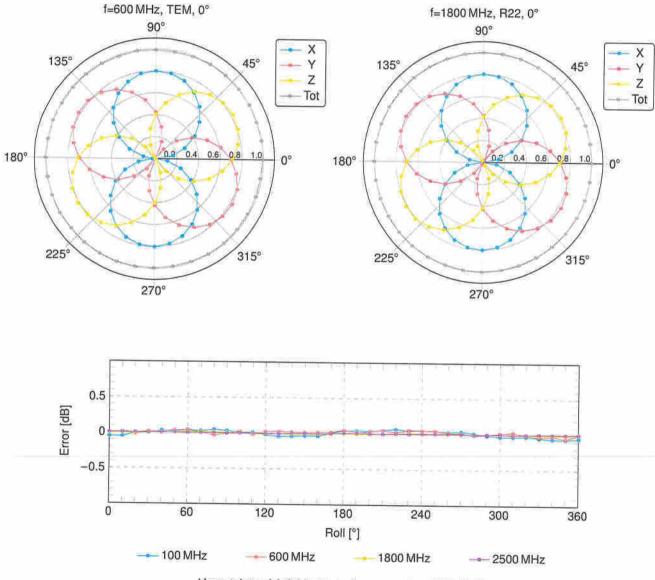

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

Uncertainty of Axial Isotropy Assessment: ±0.5% (k=2)

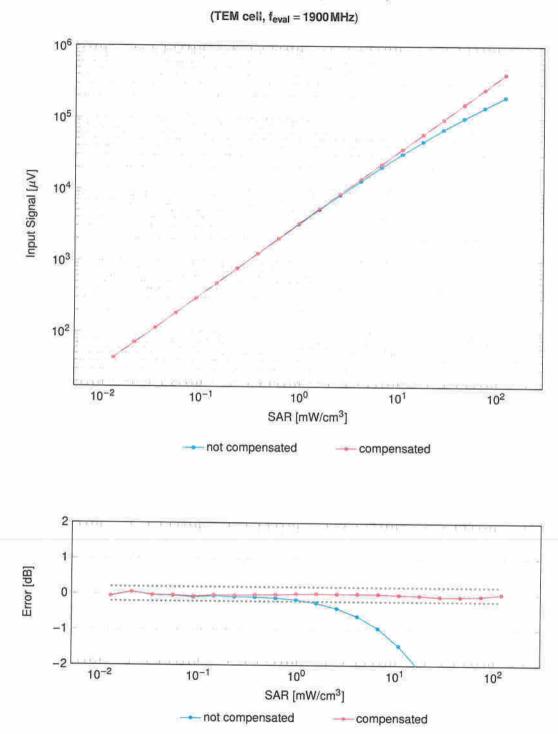


Dynamic Range f(SAR_{head})

Uncertainty of Linearity Assessment: ±0.6% (k=2)

f=1900 MHz, WGLS R22 (H_convF) 30 25 SAR [(W/kg)/W] 20 15 10 5 00 10 20 30 40 z [mm] ---- analytical ---- measured Deviation from Isotropy in Liquid Error (ϕ , θ), f = 900 MHz

Conversion Factor Assessment

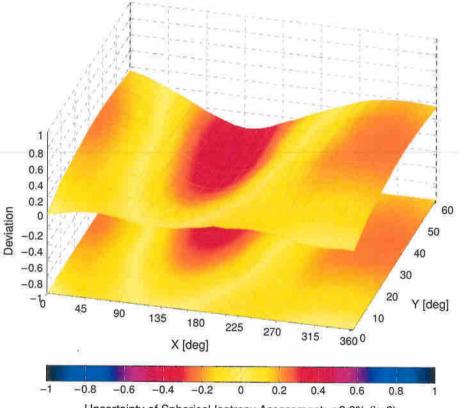

Uncertainty of Spherical Isotropy Assessment: ±2.6% (k=2)

Appendix: Modulation Calibration Parameters

UID	Rev	Communication System Name	Group	PAR (dB)	$Unc^{E} k = 1$
0		CW	CW	0.00	±4.7
10010	CAA	SAR Validation (Square, 100 ms, 10 ms)	Test	10.00	±9.6
10011	CAB	UMTS-FDD (WCDMA)	WCDMA	2.91	±9.6
10012	CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	WLAN	1.87	±9.6
10013	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps)	WLAN	9.46	±9.6
10021	DAC	GSM-FDD (TDMA, GMSK)	GSM	9.39	±9.6
10023	DAC	GPRS-FDD (TDMA, GMSK, TN 0)	GSM	9.57	±9.6
10024	DAC	GPRS-FDD (TDMA, GMSK, TN 0-1)	GSM	6.56	±9.6
10025	DAC	EDGE-FDD (TDMA, 8PSK, TN 0)	GSM	12.62	±9.6
10026	DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1)	GSM	9.55	±9.6
10027	DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	GSM	4.80	±9.6
10028	DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	GSM	3.55	±9.6
10029	DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2)	GSM	7.78	±9.6
10030	CAA	IEEE 802.15.1 Bluetooth (GFSK, DH1)	Bluetooth	5.30	±9.6
10031	CAA	IEEE 802.15.1 Bluetooth (GFSK, DH3)	Bluetooth	1.87	the second second second
10032	CAA	IEEE 802.15.1 Bluetooth (GFSK, DH5)	Bluetooth		±9.6
10033	CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH1)		1.16	±9.6
0034	CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH3)	Bluetooth	7.74	±9.6
0035	CAA	IEEE 802.15.1 Bluetooth (Pl/4-DQPSK, DH3)	Bluetooth	4.53	±9.6
0036	CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH1)	Bluetooth	3.83	±9.6
0036	CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH1) IEEE 802.15.1 Bluetooth (8-DPSK, DH3)	Bluetooth	8.01	±9.6
0037	CAA		Bluetooth	4.77	±9.6
5ea 1 e 1 a Aos	1.5777-7950)	IEEE 802.15.1 Bluetooth (8-DPSK, DH5)	Bluetooth	4.10	±9.6
0039	CAB	CDMA2000 (1xRTT, RC1)	CDMA2000	4.57	±9.6
0042	CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4-DQPSK, Halfrate)	AMPS	7.78	±9.6
0044	CAA	IS-91/EIA/TIA-553 FDD (FDMA, FM)	AMPS	0.00	±9.6
0048	CAA	DECT (TDD, TDMA/FDM, GFSK, Full Slot, 24)	DECT	13.80	±9.6
0049	CAA	DECT (TDD, TDMA/FDM, GFSK, Double Slot, 12)	DECT	10.79	±9.6
0056	CAA	UMTS-TDD (TD-SCDMA, 1.28 Mcps)	TD-SCDMA	11.01	±9.6
0058	DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2-3)	GSM	6.52	±9.6
0059	CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps)	WLAN	2.12	±9.6
0060	CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps)	WLAN	2.83	±9.6
0061	CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps)	WLAN	3.60	±9.6
0062	CAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps)	WLAN	8.68	±9.6
0063	CAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps)	WLAN	8.63	±9.6
0064	CAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps)	WLAN	9.09	±9.6
0065	CAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps)	WLAN	9.00	±9.6
0066	CAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps)	WLAN	9.38	±9.6
0067	CAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps)	WLAN	10.12	±9.6
0068	CAD	IEEE 802.11a/h WiFi 5GHz (OFDM, 48 Mbps)	WLAN	10.12	
0069	CAD	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps)	WLAN	10.24	±9.6
0071	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 9 Mbps)		1.52.535.0	±9.6
0072	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 12 Mbps)	WLAN	9.83	±9.6
0073	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 12 Mbps)	WLAN	9.62	±9.6
0074	CAB		WLAN	9.94	±9.6
0075	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 24 Mbps)	WLAN	10.30	±9.6
0075	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 36 Mbps)	WLAN	10.77	±9.6
0076	CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 48 Mbps)	WLAN	10.94	±9.6
C		IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 54 Mbps)	WLAN	11.00	±9.6
0081	CAB	CDMA2000 (1xRTT, RC3)	CDMA2000	3.97	±9.6
0082	CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4-DQPSK, Fullrate)	AMPS	4.77	±9.6
0090	DAC	GPRS-FDD (TDMA, GMSK, TN 0-4)	GSM	6.56	±9.6
0097	CAC	UMTS-FDD (HSDPA)	WCDMA	3.98	±9.6
8600	DAC	UMTS-FDD (HSUPA, Subtest 2)	WCDMA	3.98	±9.6
	CAC	EDGE-FDD (TDMA, 8PSK, TN 0-4)	GSM	9.55	±9.6
	CAC	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	LTE-FDD	5.67	±9.6
101	CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	LTE-FDD	6.42	±9.6
0102	CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	LTE-FDD	6.60	±9.6
0103	DAC	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	LTE-TDD	9.29	±9.6
0104	CAE	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	LTE-TDD	9.97	±9.6
105	CAE	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	LTE-TDD	10.01	±9.6
	CAE	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	LTE-FDD	_	ALC: NOT ALC: NOT
	CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	LTE-FDD	5.80	±9.6
	CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)		6.43	±9.6
)111	and the second se	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	LTE-FDD LTE-FDD	5.75	±9.6

UID	Rev	Communication System Name	Group	PAR (dB)	Unc ^E k =
10112	CAG	(For the first for the formation of Gravity)	LTE-FDD	6.59	±9.6
10113	CAG	(Contraction of the other that the other the	LTE-FDD	6.62	±9.6
10114	CAG	The second s	WLAN	8.10	±9.6
10115		the second of the second of the bas, to control of	WLAN	8.46	±9.6
10116	CAG	and an and an and an and an	WLAN	8.15	±9.6
10118	CAG		WLAN	8.07	±9.6
10119	CAD	The second s	WLAN	8.59	±9.6
10119	CAD	IEEE 802.11n (HT Mixed, 135 Mbps, 64-QAM)	WLAN	8.13	±9.6
10140	1000000000	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	LTE-FDD	6.49	±9.6
10141	CAD	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	LTE-FDD	6.53	±9.6
10142	CAD	LTE-FDD (SC-FDMA, 100% RB, 3MHz, QPSK)	LTE-FDD	5.73	±9.6
10143	CAC	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	LTE-FDD	6.35	±9.6
10145	CAC	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	LTE-FDD	6.65	±9.6
10146	CAC	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	LTE-FDD	5.76	±9.6
10147	CAC	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	LTE-FDD	6.41	±9.6
10149	CAE	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.72	±9.6
10150	CAE	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	LTE-FDD	6.42	±9.6
10151	CAE	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	LTE-FDD	6.60	±9.6
10152	CAE	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	LTE-TDD	9.28	±9.6
10152	CAE	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	LTE-TDD	9.92	±9.6
10154	CAF	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	LTE-TDD	10.05	±9.6
10155	CAF	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	LTE-FDD	5.75	±9.6
10156	CAF	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	LTE-FDD	6.43	±9.6
10157	CAE	LTE-FDD (SC-FDMA, 50% RB, 5MHz, QPSK)	LTE-FDD	5.79	±9.6
10158	CAE	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	LTE-FDD	6.49	±9.6
10159	CAE	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM)	LTE-FDD	6.62	±9.6
10160	CAG	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM)	LTE-FDD	6.56	±9.6
10161	CAG	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	LTE-FDD	5.82	±9.6
0162	CAG	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	LTE-FDD	6.43	±9.6
0166	CAG	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM)	LTE-FDD	6.58	±9.6
0167		LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	LTE-FDD	5.46	±9.6
0168	CAG	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	LTE-FDD	6.21	±9.6
0169	CAG	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.79	±9.6
0170	CAG	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	LTE-FDD	5.73	±9.6
0170	Cartonet	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	LTE-FDD	6.52	±9.6
0172	CAE	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	LTE-FDD	6.49	±9.6
0172	CAE	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	LTE-TDD	9.21	±9.6
0174	CAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	LTE-TDD	9.48	±9.6
0175	CAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	LTE-TDD	10.25	±9.6
0175	CAF	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	LTE-FDD	5.72	±9.6
0178	CAE	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	LTE-FDD	6.52	±9.6
and the second second	101121	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	LTE-FDD	5.73	±9.6
0178	CAE	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	LTE-FDD	6.52	±9.6
ALCONTRACT.	AAE	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	LTE-FDD	6.50	±9.6
0180	CAG	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	LTE-FDD	6.50	±9.6
0181	CAG	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	LTE-FDD	5.72	±9.6
0182	CAG	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	LTE-FDD	6.52	±9.6
0183	CAG	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	LTE-FDD	6.50	±9.6
	CAG	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	LTE-FDD	5.73	±9.6
0185	CAI	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	LTE-FDD	6.51	±9.6
186	CAG	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	LTE-FDD	6.50	±9.6
0187	CAG	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	LTE-FDD	5.73	±9.6
0188	CAG	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	LTE-FDD	6.52	±9.6
193	CAE	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	LTE-FDD	6.50	±9.6
	CAE	IEEE 802.11n (HT Greenfield, 6.5 Mbps, BPSK)	WLAN	8.09	±9.6
194	AAD	IEEE 802.11n (HT Greenfield, 39 Mbps, 16-QAM)	WLAN	8.12	±9.6
195	CAE	IEEE 802.11n (HT Greenfield, 65 Mbps, 64-QAM)	WLAN	8.21	±9.6
196	CAE	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	WLAN	8.10	±9.6
	AAE	IEEE 802.11n (HT Mixed, 39 Mbps, 16-QAM)	WLAN	8.13	±9.6
	CAF	IEEE 802.11n (HT Mixed, 65 Mbps, 64-QAM)	WLAN	8.27	±9.6
219	CAF	IEEE 802.11n (HT Mixed, 7.2 Mbps, BPSK)	WLAN	8.03	±9.6
A CONTRACTOR OF	AAF	IEEE 802.11n (HT Mixed, 43.3 Mbps, 16-QAM)	WLAN	8.13	±9.6
and the second sec	CAC	IEEE 802.11n (HT Mixed, 72.2 Mbps, 64-QAM)	WLAN	8.27	±9.6
		IEEE 802.11n (HT Mixed, 15 Mbps, BPSK)	WLAN	8.06	±9.6
	CAD	IEEE 802.11n (HT Mixed, 90 Mbps, 16-QAM)	WLAN	8.48	±9.6
224	CAD	IEEE 802.11n (HT Mixed, 150 Mbps, 64-QAM)	WLAN	8.08	±9.6