



## EX3DV4- SN:3617

#### January 30, 2020

10727	AAA	IEEE 802.11ax (80MHz, MCS8, 90pc duty cycle)	WLAN	8.66	± 9.6 %
10728	AAA	IEEE 802.11ax (80MHz, MCS9, 90pc duty cycle)	WLAN	8.65	± 9.6 %
10729	AAA	IEEE 802.11ax (80MHz, MCS10, 90pc duty cycle)	WLAN	8.64	± 9.6 %
10730	AAA	IEEE 802.11ax (80MHz, MCS11, 90pc duty cycle)	WLAN	8.67	± 9.6 %
10731	AAA	IEEE 802.11ax (80MHz, MCS0, 99pc duty cycle)	WLAN	8.42	± 9.6 %
0732	AAA	IEEE 802.11ax (80MHz, MCS1, 99pc duty cycle)	WLAN	8.46	± 9.6 %
10733	AAA	IEEE 802.11ax (80MHz, MCS2, 99pc duty cycle)	WLAN	8.40	± 9.6 %
10734	AAA	IEEE 802.11ax (80MHz, MCS3, 99pc duty cycle)	WLAN	8.25	± 9.6 %
10735	AAA	IEEE 802.11ax (80MHz, MCS3, 99pc duty cycle)	WLAN	8.33	± 9.6 %
10736	AAA	IEEE 802.11ax (80MHz, MCS4, 99pc duty cycle)	WLAN	8.27	± 9.6 %
	AAA		WLAN	8.36	± 9.6 %
0737		IEEE 802.11ax (80MHz, MCS6, 99pc duty cycle)			
0738	AAA	IEEE 802.11ax (80MHz, MCS7, 99pc duty cycle)	WLAN	8.42	± 9.6 %
0739	AAA	IEEE 802.11ax (80MHz, MCS8, 99pc duty cycle)	WLAN	8.29	± 9.6 %
10740	AAA	IEEE 802.11ax (80MHz, MCS9, 99pc duty cycle)	WLAN	8.48	± 9.6 %
10741	AAA	IEEE 802.11ax (80MHz, MCS10, 99pc duty cycle)	WLAN	8.40	± 9.6 %
10742	AAA	IEEE 802.11ax (80MHz, MCS11, 99pc duty cycle)	WLAN	8.43	± 9.6 %
10743	AAA	IEEE 802.11ax (160MHz, MCS0, 90pc duty cycle)	WLAN	8.94	± 9.6 %
10744	AAA	IEEE 802.11ax (160MHz, MCS1, 90pc duty cycle)	WLAN	9.16	± 9.6 %
10745	AAA	IEEE 802.11ax (160MHz, MCS2, 90pc duty cycle)	WLAN	8.93	± 9.6 %
10746	AAA	IEEE 802.11ax (160MHz, MCS3, 90pc duty cycle)	WLAN	9.11	± 9.6 %
10747	AAA	IEEE 802.11ax (160MHz, MCS4, 90pc duty cycle)	WLAN	9.04	± 9.6 %
10748	AAA	IEEE 802.11ax (160MHz, MCS5, 90pc duty cycle)	WLAN	8.93	±9.6 %
10749	AAA	IEEE 802.11ax (160MHz, MCS6, 90pc duty cycle)	WLAN	8.90	± 9.6 %
10750	AAA	IEEE 802.11ax (160MHz, MCS7, 90pc duty cycle)	WLAN	8.79	± 9.6 %
10751	AAA	IEEE 802.11ax (160MHz, MCS8, 90pc duty cycle)	WLAN	8.82	± 9.6 %
10752	AAA	IEEE 802.11ax (160MHz, MCS9, 90pc duty cycle)	WLAN	8.81	± 9.6 %
10753	AAA	IEEE 802.11ax (160MHz, MCS10, 90pc duty cycle)	WLAN	9.00	± 9.6 %
10754	AAA	IEEE 802.11ax (160MHz, MCS11, 90pc duty cycle)	WLAN	8.94	± 9.6 %
10755	AAA	IEEE 802.11ax (160MHz, MCS0, 99pc duty cycle)	WLAN	8.64	± 9.6 %
10756	AAA	IEEE 802.11ax (160MHz, MCS1, 99pc duty cycle)	WLAN	8.77	± 9.6 %
10757					
	AAA	IEEE 802.11ax (160MHz, MCS2, 99pc duty cycle)	WLAN	8.77	± 9.6 %
10758	AAA	IEEE 802.11ax (160MHz, MCS3, 99pc duty cycle)	WLAN	8.69	± 9.6 %
10759	AAA	IEEE 802.11ax (160MHz, MCS4, 99pc duty cycle)	WLAN	8.58	± 9.6 %
10760	AAA	IEEE 802.11ax (160MHz, MCS5, 99pc duty cycle)	WLAN	8.49	± 9.6 %
10761	AAA	IEEE 802.11ax (160MHz, MCS6, 99pc duty cycle)	WLAN	8.58	± 9.6 %
10762	AAA	IEEE 802.11ax (160MHz, MCS7, 99pc duty cycle)	WLAN	8.49	± 9.6 %
10763	AAA	IEEE 802.11ax (160MHz, MCS8, 99pc duty cycle)	WLAN	8.53	± 9.6 %
10764	AAA	IEEE 802.11ax (160MHz, MCS9, 99pc duty cycle)	WLAN	8.54	± 9.6 %
10765	AAA	IEEE 802.11ax (160MHz, MCS10, 99pc duty cycle)	WLAN	8.54	± 9.6 %
10766	AAA	IEEE 802.11ax (160MHz, MCS11, 99pc duty cycle)	WLAN	8.51	± 9.6 %
10767	AAB	5G NR (CP-OFDM, 1 RB, 5 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	7.99	± 9.6 %
10768	AAB	5G NR (CP-OFDM, 1 RB, 10 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.01	± 9.6 %
10769	AAB	5G NR (CP-OFDM, 1 RB, 15 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.01	± 9.6 %
10770	AAB	5G NR (CP-OFDM, 1 RB, 20 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.02	± 9.6 %
10771	AAB	5G NR (CP-OFDM, 1 RB, 25 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.02	± 9.6 %
10772	AAB	5G NR (CP-OFDM, 1 RB, 30 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.23	± 9.6 %
10773	AAB	5G NR (CP-OFDM, 1 RB, 40 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.03	± 9.6 %
10774	AAB	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.02	± 9.6 %
10776	AAB	5G NR (CP-OFDM, 50% RB, 10 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.30	± 9.6 %
10778	AAB	5G NR (CP-OFDM, 50% RB, 20 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.34	± 9.6 9
10780	AAB	5G NR (CP-OFDM, 50% RB, 30 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.38	± 9.6 9
10781	AAB	5G NR (CP-OFDM, 50% RB, 40 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.38	± 9.6 °

Certificate No: EX3-3617\_Jan20/2

Page 20 of 23





10700				0.40	
10782	AAB	5G NR (CP-OFDM, 50% RB, 50 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.43	± 9.6 %
10783	AAB	5G NR (CP-OFDM, 100% RB, 5 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.31	± 9.6 %
10784	AAB	5G NR (CP-OFDM, 100% RB, 10 MHz, QPSK, 15 kHz)	5G NR FR1 TDD	8.29	± 9.6 %
10785	AAB	5G NR (CP-OFDM, 100% RB, 15 MHz, QPSK, 15 kHz)~	5G NR FR1	8.40	± 9.6 %
10786	AAB	5G NR (CP-OFDM, 100% RB, 20 MHz, QPSK, 15 kHz)	TDD 5G NR FR1	8.35	± 9.6 %
10787	AAB	5G NR (CP-OFDM, 100% RB, 25 MHz, QPSK, 15 kHz)	TDD 5G NR FR1	8.44	± 9.6 %
10788	AAB	5G NR (CP-OFDM, 100% RB, 30 MHz, QPSK, 15 kHz)	TDD 5G NR FR1	8.39	± 9.6 %
10789	AAB	5G NR (CP-OFDM, 100% RB, 40 MHz, QPSK, 15 kHz)	TDD 5G NR FR1	8.37	± 9.6 %
10790	AAB	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 15 kHz)	TDD 5G NR FR1	8.39	± 9.6 %
		the state of the second second second with and the second se	TDD		
10791	AAB	5G NR (CP-OFDM, 1 RB, 5 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.83	± 9.6 %
10792	AAB	5G NR (CP-OFDM, 1 RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.92	± 9.6 %
10793	AAB	5G NR (CP-OFDM, 1 RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.95	± 9.6 %
10794	AAB	5G NR (CP-OFDM, 1 RB, 20 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.82	± 9.6 %
10795	AAB	5G NR (CP-OFDM, 1 RB, 25 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	7.84	± 9.6 %
10796	AAB	5G NR (CP-OFDM, 1 RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1	7.82	± 9.6 %
10797	AAB	5G NR (CP-OFDM, 1 RB, 40 MHz, QPSK, 30 kHz)	TDD 5G NR FR1	8.01	± 9.6 %
10798	AAB	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 30 kHz)	TDD 5G NR FR1	7.89	± 9.6 %
10799	AAB	5G NR (CP-OFDM, 1 RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1	7.93	± 9.6 %
10801	AAB	5G NR (CP-OFDM, 1 RB, 80 MHz, QPSK, 30 kHz)	TDD 5G NR FR1	7.89	± 9.6 %
10802	AAB	5G NR (CP-OFDM, 1 RB, 90 MHz, QPSK, 30 kHz)	TDD 5G NR FR1	7.87	± 9.6 9
10803	AAB		TDD 5G NR FR1	7.93	± 9.6 9
		5G NR (CP-OFDM, 1 RB, 100 MHz, QPSK, 30 kHz)	TDD		
10805	AAB	5G NR (CP-OFDM, 50% RB, 10 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.34	± 9.6 9
10806	AAB	5G NR (CP-OFDM, 50% RB, 15 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.37	± 9.6 °
10809	AAB	5G NR (CP-OFDM, 50% RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.34	± 9.6 °
10810	AAB	5G NR (CP-OFDM, 50% RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.34	± 9.6 °
10812	AAB	5G NR (CP-OFDM, 50% RB, 60 MHz, QPSK, 30 kHz)	5G NR FR1	8.35	± 9.6 °
10817	AAB	5G NR (CP-OFDM, 100% RB, 5 MHz, QPSK, 30 kHz)	TDD 5G NR FR1	8.35	± 9.6
10818	AAB	5G NR (CP-OFDM, 100% RB, 10 MHz, QPSK, 30 kHz)	TDD 5G NR FR1	8.34	± 9.6
10819	AAB	5G NR (CP-OFDM, 100% RB, 15 MHz, QPSK, 30 kHz)	TDD 5G NR FR1	8.33	± 9.6
10820	AAB	5G NR (CP-OFDM, 100% RB, 20 MHz, QPSK, 30 kHz)	TDD 5G NR FR1	8.30	± 9.6
10821	AAB	5G NR (CP-OFDM, 100% RB, 25 MHz, QPSK, 30 kHz)	TDD 5G NR FR1	8.41	± 9.6
			TDD		
10822	AAB	5G NR (CP-OFDM, 100% RB, 30 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.41	± 9.6
10823	AAB	5G NR (CP-OFDM, 100% RB, 40 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.36	± 9.6

Certificate No: EX3-3617\_Jan20/2

Page 21 of 23





10824	AAB	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 30 kHz)	5G NR FR1	8.39	± 9.6 %
10825	AAB	5G NR (CP-OFDM, 100% RB, 60 MHz, QPSK, 30 kHz)	TDD 5G NR FR1	8.41	± 9.6 %
			TDD		
10827	AAB	5G NR (CP-OFDM, 100% RB, 80 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.42	± 9.6 %
10828	AAB	5G NR (CP-OFDM, 100% RB, 90 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	8.43	± 9.6 %
10829	AAB	5G NR (CP-OFDM, 100% RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1	8.40	± 9.6 %
10830	AAB	5G NR (CP-OFDM, 1 RB, 10 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	7.63	± 9.6 %
10831	AAB	5G NR (CP-OFDM, 1 RB, 15 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	7.73	± 9.6 %
10832	AAB	5G NR (CP-OFDM, 1 RB, 20 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	7.74	± 9.6 %
10833	AAB	5G NR (CP-OFDM, 1 RB, 25 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	7.70	± 9.6 %
		Contraction Contraction and the second price in the second product of the second second product of the second se	TDD	2/2020/000	1.0000 000 Date
10834	AAB	5G NR (CP-OFDM, 1 RB, 30 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.75	± 9.6 %
10835	AAB	5G NR (CP-OFDM, 1 RB, 40 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.70	± 9.6 %
10836	AAB	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	7.66	± 9.6 %
10837	AAB	5G NR (CP-OFDM, 1 RB, 60 MHz, QPSK, 60 kHz)	5G NR FR1	7.68	± 9.6 %
10839	AAB	5G NR (CP-OFDM, 1 RB, 80 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	7.70	± 9.6 %
10840	AAB	5G NR (CP-OFDM, 1 RB, 90 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	7.67	± 9.6 %
10841	AAB	5G NR (CP-OFDM, 1 RB, 100 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	7.71	± 9.6 %
10843	AAB	5G NR (CP-OFDM, 50% RB, 15 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	8.49	± 9.6 %
10844	AAB		TDD 5G NR FR1	8.34	
		5G NR (CP-OFDM, 50% RB, 20 MHz, QPSK, 60 kHz)	TDD		± 9.6 %
10846	AAB	5G NR (CP-OFDM, 50% RB, 30 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.41	± 9.6 %
10854	AAB	5G NR (CP-OFDM, 100% RB, 10 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.34	± 9.6 %
10855	AAB	5G NR (CP-OFDM, 100% RB, 15 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.36	± 9.6 %
10856	AAB	5G NR (CP-OFDM, 100% RB, 20 MHz, QPSK, 60 kHz)	5G NR FR1	8.37	± 9.6 %
10857	AAB	5G NR (CP-OFDM, 100% RB, 25 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	8.35	± 9.6 %
10858	AAB	5G NR (CP-OFDM, 100% RB, 30 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	8.36	± 9.6 %
10859	AAB	5G NR (CP-OFDM, 100% RB, 40 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	8.34	± 9.6 %
10860	AAB	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	8.41	± 9.6 %
10861	AAB	5G NR (CP-OFDM, 100% RB, 60 MHz, QPSK, 60 kHz)	TDD 5G NR FR1	8.40	± 9.6 %
			TDD		-
10863	AAB	5G NR (CP-OFDM, 100% RB, 80 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.41	± 9.6 %
10864	AAB	5G NR (CP-OFDM, 100% RB, 90 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.37	± 9.6 %
10865	AAB	5G NR (CP-OFDM, 100% RB, 100 MHz, QPSK, 60 kHz)	5G NR FR1 TDD	8.41	± 9.6 %
10866	AAB	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1 TDD	5.68	± 9.6 %
10868	AAB	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, QPSK, 30 kHz)	5G NR FR1	5.89	± 9.6 %
10869	AAC	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, QPSK, 120 kHz)	TDD 5G NR FR2	5.75	± 9.6 %

Certificate No: EX3-3617\_Jan20/2

Page 22 of 23





10870	AAC	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.86	± 9.6 %
10871	AAC	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	5.75	± 9.6 %
10872	AAC	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	6.52	± 9.6 %
10873	AAC	5G NR (DFT-s-OFDM, 1 RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.61	± 9.6 %
10874	AAC	5G NR (DFT-s-OFDM, 100% RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.65	± 9.6 %
10875	AAC	5G NR (CP-OFDM, 1 RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	7.78	± 9.6 %
10876	AAC	5G NR (CP-OFDM, 100% RB, 100 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	8.39	± 9.6 %
10877	AAC	5G NR (CP-OFDM, 1 RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	7.95	± 9.6 %
10878	AAC	5G NR (CP-OFDM, 100% RB, 100 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	8.41	± 9.6 %
10879	AAC	5G NR (CP-OFDM, 1 RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.12	± 9.6 %
10880	AAC	5G NR (CP-OFDM, 100% RB, 100 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.38	± 9.6 %
10881	AAC	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.75	± 9.6 %
10882	AAC	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	5.96	± 9.6 %
10883	AAC	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	6.57	± 9.6 %
10884	AAC	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	6.53	± 9.6 %
10885	AAC	5G NR (DFT-s-OFDM, 1 RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.61	± 9.6 %
10886	AAC	5G NR (DFT-s-OFDM, 100% RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	6.65	± 9.6 %
10887	AAC	5G NR (CP-OFDM, 1 RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	7.78	± 9.6 %
10888	AAC	5G NR (CP-OFDM, 100% RB, 50 MHz, QPSK, 120 kHz)	5G NR FR2 TDD	8.35	± 9.6 %
10889	AAC	5G NR (CP-OFDM, 1 RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	8.02	± 9.6 9
10890	AAC	5G NR (CP-OFDM, 100% RB, 50 MHz, 16QAM, 120 kHz)	5G NR FR2 TDD	8.40	± 9.6 °
10891	AAC	5G NR (CP-OFDM, 1 RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.13	± 9.6
10892	AAC	5G NR (CP-OFDM, 100% RB, 50 MHz, 64QAM, 120 kHz)	5G NR FR2 TDD	8.41	± 9.6 °

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: EX3-3617\_Jan20/2

Page 23 of 23





# L.9 Dipole Calibration Certificate 750 MHz Dipole Calibration Certificate

	CALIBRA	TION LABORATORY	AC MRA	<b>CNAS</b>	国际互认
Add: No.51 Xueyua Tel: +86-10-623046 E-mail: cttl@chinatt	33-2079 Fax: +	trict, Beijing, 100191, China 86-10-62304633-2504 /www.chinattl.cn	All Contractions		CALIBRATION CNAS L0570
Client AUD	DEN	Cer	tificate No:	Z20-60219	
CALIBRATION CE	ERTIFICAT	E			
Object	D750V	3 - SN: 1078			
Calibration Procedure(s)	FE-711	-003-01			
		tion Procedures for dipole	e validation kits		
Calibration date:	June 1	8, 2020			
neasurements(SI). The mea bages and are part of the ce All calibrations have been humidity<70%.	ertificate.	the closed laboratory fa	acility: environn	nent temperature	9(22±3)°C and
bages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used	conducted in (M&TE critical fr	or calibration)			
bages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used Primary Standards	conducted in (M&TE critical fr	or calibration) Cal Date(Calibrated by	y, Certificate No.	.) Schedulec	Calibration
bages and are part of the ce All calibrations have been humidity<70%. Calibration Equipment used	conducted in (M&TE critical fr	or calibration) Cal Date(Calibrated by 04-Sep-19 (CTTL, No.J	/, Certificate No. 19X07825)	.) Schedulec S	I Calibration ep-20
Pages and are part of the ce NI calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2	conducted in (M&TE critical fr ID # 106277	or calibration) Cal Date(Calibrated by	7, Certificate No. 19X07825) 19X07825)	.) Schedulec S S	Calibration
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S	conducted in (M&TE critical fr ID # 106277 104291	or calibration) Cal Date(Calibrated by 04-Sep-19 (CTTL, No.J 04-Sep-19 (CTTL, No.J	7, Certificate No. 19X07825) 19X07825) KG,No.Z19-6030	.) Schedulec S S 06) S	I Calibration ep-20 ep-20
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S ReferenceProbe EX3DV4	ID # 106277 104291 SN 7514	or calibration) Cal Date(Calibrated by 04-Sep-19 (CTTL, No.J 04-Sep-19 (CTTL, No.J 27-Sep-19(CTTL-SPEA	r, Certificate No. 19X07825) 19X07825) 19X07825) 19X07825) 19X07825) 19X07825) 19X07825 19X0785 19X0775 19X0775 19X0775 19X0775 19X075 19X	.) Schedulec S S 06) S 05) A	I Calibration ep-20 ep-20 iep-20
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	rtificate. conducted in (M&TE critical fr 106277 104291 SN 7514 SN 1555 ID # MY49071430	Cal Date(Calibrated by 04-Sep-19 (CTTL, No.J 04-Sep-19 (CTTL, No.J 27-Sep-19(CTTL-SPEA 22-Aug-19(CTTL-SPEA Cal Date(Calibrated by, 25-Feb-20 (CTTL, No.J	/, Certificate No. 19X07825) 19X07825) (G,No.Z19-6030 (G,No.Z19-6029 Certificate No.) 20X00516)	.) Scheduled S S 06) S 05) A 0 Scheduled F	I Calibration ep-20 ep-20 Sep-20 ug-20 I Calibration eb-21
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S ReferenceProbe EX3DV4 DAE4 Secondary Standards	rtificate. conducted in (M&TE critical fo 106277 104291 SN 7514 SN 1555 ID #	Cal Date(Calibrated by 04-Sep-19 (CTTL, No.J 04-Sep-19 (CTTL, No.J 27-Sep-19(CTTL-SPEA 22-Aug-19(CTTL-SPEA Cal Date(Calibrated by, 25-Feb-20 (CTTL, No.J	/, Certificate No. 19X07825) 19X07825) (G,No.Z19-6030 (G,No.Z19-6029 Certificate No.) 20X00516)	.) Scheduled S S 06) S 05) A 0 Scheduled F	I Calibration ep-20 ep-20 Sep-20 ug-20 ug-20
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	rtificate. conducted in (M&TE critical fr 106277 104291 SN 7514 SN 1555 ID # MY49071430	Cal Date(Calibrated by 04-Sep-19 (CTTL, No.J 04-Sep-19 (CTTL, No.J 27-Sep-19(CTTL-SPEA 22-Aug-19(CTTL-SPEA Cal Date(Calibrated by, 25-Feb-20 (CTTL, No.J	/, Certificate No. 19X07825) 19X07825) (G,No.Z19-6030 (G,No.Z19-6029 Certificate No.) 20X00516)	.) Scheduled S S 06) S 05) A 0 Scheduled F	I Calibration ep-20 ep-20 sep-20 ug-20 I Calibration eb-21 eb-21
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power Sensor NRP8S ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	ertificate. conducted in (M&TE critical fr 106277 104291 SN 7514 SN 1555 ID # MY49071430 MY46107873	Cal Date(Calibrated by 04-Sep-19 (CTTL, No.J 04-Sep-19 (CTTL, No.J 27-Sep-19 (CTTL-SPEA 22-Aug-19(CTTL-SPEA Cal Date(Calibrated by, 25-Feb-20 (CTTL, No.J 10-Feb-20 (CTTL, No.J	y, Certificate No. 19X07825) 19X07825) G,No.Z19-6030 G,No.Z19-6029 Certificate No.) 20X00516) 20X00515)	.) Scheduled S S 06) S 05) A <u>Scheduled</u> F F	I Calibration ep-20 ep-20 sep-20 ug-20 I Calibration eb-21 eb-21
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	ertificate. conducted in (M&TE critical fr 106277 104291 SN 7514 SN 1555 ID # MY49071430 MY46107873 Name	Cal Date(Calibrated by 04-Sep-19 (CTTL, No.J 04-Sep-19 (CTTL, No.J 27-Sep-19(CTTL-SPEA 22-Aug-19(CTTL-SPEA Cal Date(Calibrated by, 25-Feb-20 (CTTL, No.J 10-Feb-20 (CTTL, No.J	y, Certificate No. (19X07825) (19X07825) (G,No.Z19-6030 (G,No.Z19-6029 Certificate No.) 20X00516) 20X00515) er	.) Scheduled S S 06) S 05) A <u>Scheduled</u> F F	I Calibration ep-20 ep-20 sep-20 ug-20 I Calibration eb-21 eb-21
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power Sensor NRP8S ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	Artificate. conducted in (M&TE critical fr 106277 104291 SN 7514 SN 1555 ID # MY49071430 MY46107873 Name Zhao Jing	Cal Date(Calibrated by 04-Sep-19 (CTTL, No.J 04-Sep-19 (CTTL, No.J 27-Sep-19(CTTL-SPEA 22-Aug-19(CTTL-SPEA Cal Date(Calibrated by, 25-Feb-20 (CTTL, No.J 10-Feb-20 (CTTL, No.J Function SAR Test Enginee	r, Certificate No. (19X07825) (19X07825) (G,No.Z19-6030 (G,No.Z19-6029 Certificate No.) 20X00516) 20X00515) er	.) Scheduled S S 06) S 05) A <u>Scheduled</u> F F	I Calibration ep-20 ep-20 sep-20 ug-20 I Calibration eb-21 eb-21







#### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORMx,y,z
N/A	not applicable or not measured

## Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- d) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

#### Additional Documentation:

e) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z20-60219

Page 2 of 6







#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz ± 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permitti	vity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.9		0.89 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.9 ± 6	5 %	0.87 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C			<u></u>
R result with Head TSL				
SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condi	tion		
SAR measured	250 mW in	put power		2.08 W/kg
SAR for nominal Head TSL parameters	normalize	ed to 1W	8.44	W/kg ± 18.8 % ( <i>k</i> =2)
SAR averaged over 10 $cm^3$ (10 g) of Head T	SL Condi	tion		
SAR measured	250 mW in	put power		1.37 W/kg
SAR for nominal Head TSL parameters	normalize	ed to 1W	5.55	W/kg ± 18.7 % ( <i>k</i> =2)

Certificate No: Z20-60219

Page 3 of 6







#### Appendix (Additional assessments outside the scope of CNAS L0570)

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.6Ω+ 0.22jΩ	
Return Loss	- 27.1dB	

#### General Antenna Parameters and Design

Electrical Delay (one direction)	0.899 ns	

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

## Additional EUT Data

Manufactured by		SPEAG	
rtificate No: Z20-60219	Page 4 of 6		







#### **DASY5 Validation Report for Head TSL** Test Laboratory: CTTL, Beijing, China

Date: 06.18.2020


**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1078** Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1 Medium parameters used: f = 750 MHz;  $\sigma = 0.867$  S/m;  $\varepsilon_r = 40.88$ ;  $\rho = 1000$  kg/m3 Phantom section: Right Section

DASY5 Configuration:

- Probe: EX3DV4 SN7514; ConvF(9.7, 9.7, 9.7) @ 750 MHz; Calibrated: 2019-09-27
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1555; Calibrated: 2019-08-22
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

**Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 54.84 V/m; Power Drift = -0.01 dB Peak SAR (extrapolated) = 3.25 W/kg SAR(1 g) = 2.08 W/kg; SAR(10 g) = 1.37 W/kg Smallest distance from peaks to all points 3 dB below = 21.2 mm Ratio of SAR at M2 to SAR at M1 = 64.4% Maximum value of SAR (measured) = 2.83 W/kg

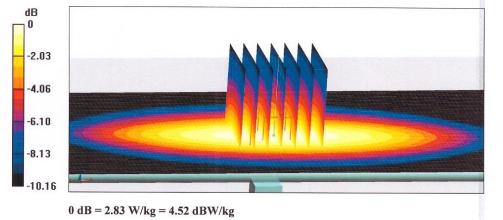

Certificate No: Z20-60219


Page 5 of 6







## Impedance Measurement Plot for Head TSL

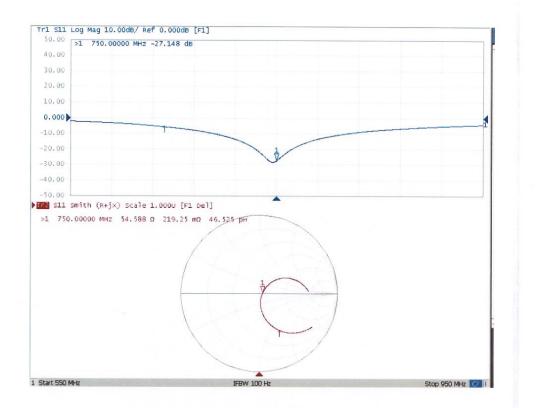

#### Certificate No: Z20-60219

Page 6 of 6





## 1750 MHz Dipole Calibration Certificate

Client AUDE	ttl.com http:/	+86-10-62304633-2504 /www.ehinattl.en Certificate No: Z20	CNAS L0570
		Continioute No. LEO	)-60155
ONEIBIGATION O	ERTIFICAT	ſE	
Object	D1750	V2 - SN: 1111	
Calibration Procedure(s)		-003-01	
Calibration date:		tion Procedures for dipole validation kits 9, 2020	
measurements(SI). The me pages and are part of the co		the uncertainties with confidence probability	are given on the following
humidity<70%.		the closed laboratory facility: environment	temperature(22±3)°C and
humidity<70%. Calibration Equipment usec	d (M&TE critical f	or calibration)	
humidity<70%. Calibration Equipment usec		or calibration) Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
numidity<70%. Calibration Equipment used Primary Standards	I (M&TE critical f	or calibration)	Scheduled Calibration Sep-20
numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2	I (M&TE critical f	or calibration) Cal Date(Calibrated by, Certificate No.) 04-Sep-19 (CTTL, No.J19X07825)	Scheduled Calibration Sep-20 Sep-20
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S	ID # 106277 104291	Cal Date(Calibrated by, Certificate No.) 04-Sep-19 (CTTL, No.J19X07825) 04-Sep-19 (CTTL, No.J19X07825)	Scheduled Calibration Sep-20
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S ReferenceProbe EX3DV4	ID # 106277 104291 SN 7307	Cal Date(Calibrated by, Certificate No.) 04-Sep-19 (CTTL, No.J19X07825) 04-Sep-19 (CTTL, No.J19X07825) 24-May-19(SPEAG,No.EX3-7307_May19)	Scheduled Calibration Sep-20 Sep-20 May-20
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S ReferenceProbe EX3DV4 DAE4	ID# 106277 104291 SN 7307 SN 1555 ID# MY49071430	Cal Date(Calibrated by, Certificate No.) 04-Sep-19 (CTTL, No.J19X07825) 04-Sep-19 (CTTL, No.J19X07825) 24-May-19(SPEAG,No.EX3-7307_May19) 22-Aug-19(CTTL-SPEAG,No.Z19-60295)	Scheduled Calibration Sep-20 Sep-20 May-20 Aug-20
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	d (M&TE critical f ID # 106277 104291 SN 7307 SN 1555 ID # MY49071430 MY46110673	Cal Date(Calibrated by, Certificate No.) 04-Sep-19 (CTTL, No.J19X07825) 04-Sep-19 (CTTL, No.J19X07825) 24-May-19(SPEAG,No.EX3-7307_May19) 22-Aug-19(CTTL-SPEAG,No.Z19-60295) Cal Date(Calibrated by, Certificate No.) 25-Feb-20 (CTTL, No.J20X00516) 10-Feb-20 (CTTL, No.J20X00515)	Scheduled Calibration Sep-20 Sep-20 May-20 Aug-20 Scheduled Calibration Feb-21 Feb-21
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	ID# 106277 104291 SN 7307 SN 1555 ID# MY49071430	Cal Date(Calibrated by, Certificate No.) 04-Sep-19 (CTTL, No.J19X07825) 04-Sep-19 (CTTL, No.J19X07825) 24-May-19(SPEAG,No.EX3-7307_May19) 22-Aug-19(CTTL-SPEAG,No.Z19-60295) Cal Date(Calibrated by, Certificate No.) 25-Feb-20 (CTTL, No.J20X00516)	Scheduled Calibration Sep-20 Sep-20 May-20 Aug-20 Scheduled Calibration Feb-21
humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	d (M&TE critical f ID # 106277 104291 SN 7307 SN 1555 ID # MY49071430 MY46110673 Name	Cal Date(Calibrated by, Certificate No.) 04-Sep-19 (CTTL, No.J19X07825) 04-Sep-19 (CTTL, No.J19X07825) 24-May-19 (SPEAG, No.EX3-7307_May19) 22-Aug-19 (CTTL-SPEAG, No.Z19-60295) Cal Date(Calibrated by, Certificate No.) 25-Feb-20 (CTTL, No.J20X00516) 10-Feb-20 (CTTL, No.J20X00515) Function	Scheduled Calibration Sep-20 Sep-20 May-20 Aug-20 Scheduled Calibration Feb-21 Feb-21

Certificate No: Z20-60155

Page 1 of 6







#### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORMx,y,z
N/A	not applicable or not measured

## Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- d) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

#### Additional Documentation:

e) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z20-60155

Page 2 of 6







#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	V52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	1750 MHz ± 1 MHz		

## **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.1	1.37 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.35 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

#### SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	8.80 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	35.5 W/kg ± 18.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	4.64 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	18.7 W/kg ± 18.7 % (k=2)

Certificate No: Z20-60155

Page 3 of 6







Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com http://www.chinattl.cn

#### Appendix (Additional assessments outside the scope of CNAS L0570)

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	47.7Ω- 3.24 jΩ	
Return Loss	- 27.8 dB	

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.084 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

## Additional EUT Data

Manufactured by	SPEAG

Certificate No: Z20-60155

Page 4 of 6







#### **DASY5 Validation Report for Head TSL** Test Laboratory: CTTL, Beijing, China

Date: 04.29.2020

**DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN: 1111** Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1 Medium parameters used: f = 1750 MHz;  $\sigma = 1.348$  S/m;  $\varepsilon_r = 39.78$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Right Section

DASY5 Configuration:


- Probe: EX3DV4 SN7307; ConvF(8.86, 8.86, 8.86) @ 1750 MHz; Calibrated: 2019-05-24
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1555; Calibrated: 2019-08-22
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

System Performance Check/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 93.73 V/m; Power Drift = -0.01 dB Peak SAR (extrapolated) = 16.6 W/kg SAR(1 g) = 8.8 W/kg; SAR(10 g) = 4.64 W/kg

Smallest distance from peaks to all points 3 dB below = 10 mm

Ratio of SAR at M2 to SAR at M1 = 53.5%

Maximum value of SAR (measured) = 13.7 W/kg

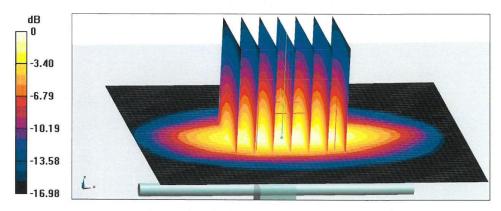

0 dB = 13.7 W/kg = 11.37 dBW/kg

Certificate No: Z20-60155

Page 5 of 6







#### **DASY5 Validation Report for Head TSL** Test Laboratory: CTTL, Beijing, China

Date: 04.29.2020

**DUT: Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2 - SN: 1111** Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1 Medium parameters used: f = 1750 MHz;  $\sigma = 1.348$  S/m;  $\varepsilon_r = 39.78$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Right Section


DASY5 Configuration:

- Probe: EX3DV4 SN7307; ConvF(8.86, 8.86, 8.86) @ 1750 MHz; Calibrated: 2019-05-24
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1555; Calibrated: 2019-08-22
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

System Performance Check/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 93.73 V/m; Power Drift = -0.01 dB Peak SAR (extrapolated) = 16.6 W/kg SAR(1 g) = 8.8 W/kg; SAR(10 g) = 4.64 W/kg

Smallest distance from peaks to all points 3 dB below = 10 mmRatio of SAR at M2 to SAR at M1 = 53.5%

Maximum value of SAR (measured) = 13.7 W/kg

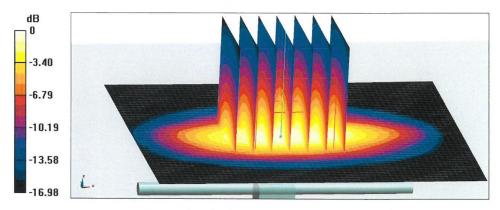

0 dB = 13.7 W/kg = 11.37 dBW/kg

Certificate No: Z20-60155

Page 5 of 6





## **1900 MHz Dipole Calibration Certificate**

<b>Calibration Laboratory</b> Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich,		BC-MRA NGININA	<ul> <li>S Schweizerischer Kalibrierdienst</li> <li>Service suisse d'étalonnage</li> <li>Servizio svizzero di taratura</li> <li>S Swiss Calibration Service</li> </ul>		
Accredited by the Swiss Accreditation The Swiss Accreditation Service in Multilateral Agreement for the rec	s one of the signatorie		Accreditation No.: SCS 0108		
Client Auden Certificate No: D1900V2-5d142_Jun20					
CALIBRATION CI	ERTIFICATE				
Object	D1900V2 - SN:50	1142			
Calibration procedure(s) QA CAL-05.v11 Calibration Procedure for SAR Validation Sources between 0.7-3 GHz					
Calibration date:	June 24, 2020				
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration)					
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration		
Power meter NRP	SN: 104778	01-Apr-20 (No. 217-03100/03101)	Apr-21		
Power sensor NRP-Z91	SN: 103244	01-Apr-20 (No. 217-03100)	Apr-21		
Power sensor NRP-Z91	SN: 103245	01-Apr-20 (No. 217-03101)	Apr-21		
Reference 20 dB Attenuator	SN: BH9394 (20k)	31-Mar-20 (No. 217-03106)	Apr-21		
Type-N mismatch combination	SN: 310982 / 06327	31-Mar-20 (No. 217-03104)	Apr-21		
Reference Probe EX3DV4	SN: 7405	31-Dec-19 (No. EX3-7405_Dec19)	Dec-20		
DAE4	SN: 601	27-Dec-19 (No. DAE4-601_Dec19)	Dec-20		
Secondary Standards ID # Check Date (in house) Scheduled Check					
Power meter E4419B	SN: GB39512475	Check Date (in house) 30-Oct-14 (in house check Feb-19)	In house check: Oct-20		
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-18)	In house check: Oct-20		
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-18)	In house check: Oct-20		
RF generator R&S SMT-06	SN: 100972		In house check: Oct-20		
Network Analyzer Agilent E8358A	SN: US41080477	15-Jun-15 (in house check Oct-18) 31-Mar-14 (in house check Oct-19)			
Network Analyzer Agilent L0000A	1314.0341000477	ST-Mar-14 (IT House check Oct-19)	In house check: Oct-20		
Name Function Signature					
Calibrated by:	Michael Weber	Laboratory Technician	Milleser		
Approved by:	Katja Pokovic	Technical Manager	Ally		
This calibration certificate shall not	be reproduced except in	full without written approval of the labor	Issued: June 25, 2020 atory.		

Certificate No: D1900V2-5d142\_Jun20

Page 1 of 6