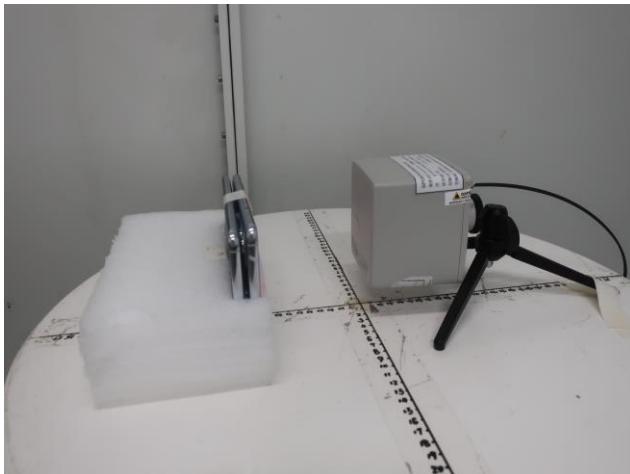
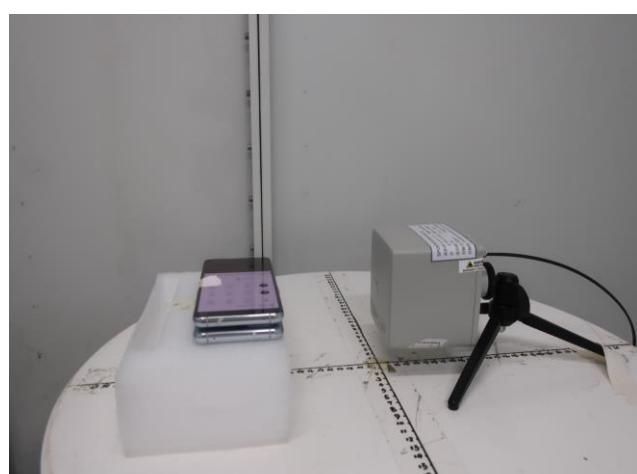
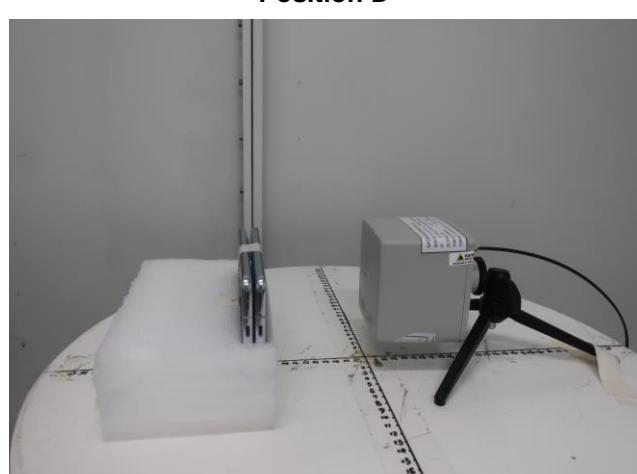


Appendix A. Test Setup Photos**<H-field Test Setup Photos>**

The equipment under test was placed on a wooden desk inside of shield room. The isotropic field probe was used to measure the field strength for 6 EUT surfaces, and during measurement a separation of 10cm is maintained between EUT surface and the center of the field probe.

**Position A****Position B****Position C****Position D****Position E****Position F**