

Appendix C for KSCR231100216803

Calibration Certificate

| Object | Apply | No | Model | SN | Calibration Date | Due date of calibration |
|--------|-------------------------------------|----|---------|-------|------------------|-------------------------|
| Dipole | <input type="checkbox"/> | 1 | CLA150 | 4025 | 2021/04/26 | 2024/04/25 |
| | <input type="checkbox"/> | 2 | D450V3 | 1103 | 2021/04/21 | 2024/04/20 |
| | <input type="checkbox"/> | 3 | D750V3 | 1188 | 2022/03/29 | 2025/03/28 |
| | <input type="checkbox"/> | 4 | D835V2 | 4d114 | 2022/03/31 | 2025/03/30 |
| | <input type="checkbox"/> | 5 | D900V2 | 1d079 | 2022/06/07 | 2025/06/06 |
| | <input type="checkbox"/> | 6 | D1800V2 | 2d170 | 2022/03/31 | 2025/03/30 |
| | <input type="checkbox"/> | 7 | D1900V2 | 5d136 | 2022/06/07 | 2025/06/06 |
| | <input type="checkbox"/> | 8 | D2000V2 | 1041 | 2022/06/06 | 2025/06/05 |
| | <input type="checkbox"/> | 9 | D2300V2 | 1096 | 2022/03/31 | 2025/03/30 |
| | <input checked="" type="checkbox"/> | 10 | D2450V2 | 817 | 2022/04/01 | 2025/03/31 |
| | <input type="checkbox"/> | 11 | D2600V2 | 1158 | 2022/03/31 | 2025/03/30 |
| | <input type="checkbox"/> | 12 | D5GHzV2 | 1095 | 2022/06/01 | 2025/05/31 |
| DAE | <input checked="" type="checkbox"/> | 13 | DAE4 | 1305 | 2023/04/13 | 2024/04/12 |
| Probe | <input checked="" type="checkbox"/> | 14 | EX3DV4 | 7767 | 2023/10/26 | 2024/10/25 |

1 Dipole

1.1 CLA150 - SN 4025

| <p>Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: SGS-CN (Auden) Certificate No: CLA150-4025_Apr21</p> <p style="text-align: right;">Accreditation No.: SCS 0108</p> <hr/> <p style="text-align: center;">CALIBRATION CERTIFICATE</p> <p>Object: CLA150 - SN: 4025</p> <p>Calibration procedure(s): QA CAL-15.v9 Calibration Procedure for SAR Validation Sources below 700 MHz</p> <p>Calibration date: April 26, 2021</p> <p>The calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.</p> <p>Calibration Equipment used (M&E critical for calibration)</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Schedule / Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP</td> <td>SN: 10475</td> <td>09-Apr-21 (No. 217-03201.00292)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP Z01</td> <td>SN: 103344</td> <td>09-Apr-21 (No. 217-03201)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP Z01</td> <td>SN: 103345</td> <td>09-Apr-21 (No. 217-03202)</td> <td>Apr-22</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: C22962 (20)</td> <td>09-Apr-21 (No. 217-03343)</td> <td>Apr-22</td> </tr> <tr> <td>Type-N mismatch combination</td> <td>SN: 310952 / 00327</td> <td>09-Apr-21 (No. 217-03344)</td> <td>Apr-22</td> </tr> <tr> <td>Reference Probe EX3004 (DIE4)</td> <td>SN: 3877</td> <td>30-Dec-20 (No. EX3-3877_Dec20)</td> <td>Dec-21</td> </tr> <tr> <td></td> <td>SN: 664</td> <td>26-Jun-20 (No. DMS4-656_Jun20)</td> <td>Jun-21</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power meter E4118B</td> <td>SN: G814282874</td> <td>06-Apr-18 (in house check Jun-20)</td> <td>in house check Jun-22</td> </tr> <tr> <td>Power sensor E4112A</td> <td>SN: MY4148067</td> <td>06-Apr-18 (in house check Jun-20)</td> <td>in house check Jun-22</td> </tr> <tr> <td>Power sensor E4112A</td> <td>SN: 000100210</td> <td>06-Apr-18 (in house check Jun-20)</td> <td>in house check Jun-22</td> </tr> <tr> <td>RF generator HP 85940D</td> <td>SN: U53840310700</td> <td>04-Aug-09 (in house check Jun-20)</td> <td>in house check Jun-22</td> </tr> <tr> <td>Network Analyzer Agilent E8363A</td> <td>SN: U541000477</td> <td>31-Mar-14 (in house check Oct-20)</td> <td>in house check Oct-21</td> </tr> </tbody> </table> <p>Calibrated by: Jeffrey Katzman Function: Laboratory Technician Signature: <i>[Signature]</i></p> <p>Approved by: Kate Polovic Technical Manager <i>[Signature]</i></p> <p style="text-align: right;">Issued: April 26, 2021</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: CLA150-4025_Apr21 Page 1 of 6</p> | Primary Standards | ID # | Cal Date (Certificate No.) | Schedule / Calibration | Power meter NRP | SN: 10475 | 09-Apr-21 (No. 217-03201.00292) | Apr-22 | Power sensor NRP Z01 | SN: 103344 | 09-Apr-21 (No. 217-03201) | Apr-22 | Power sensor NRP Z01 | SN: 103345 | 09-Apr-21 (No. 217-03202) | Apr-22 | Reference 20 dB Attenuator | SN: C22962 (20) | 09-Apr-21 (No. 217-03343) | Apr-22 | Type-N mismatch combination | SN: 310952 / 00327 | 09-Apr-21 (No. 217-03344) | Apr-22 | Reference Probe EX3004 (DIE4) | SN: 3877 | 30-Dec-20 (No. EX3-3877_Dec20) | Dec-21 | | SN: 664 | 26-Jun-20 (No. DMS4-656_Jun20) | Jun-21 | Secondary Standards | ID # | Check Date (in house) | Scheduled Check | Power meter E4118B | SN: G814282874 | 06-Apr-18 (in house check Jun-20) | in house check Jun-22 | Power sensor E4112A | SN: MY4148067 | 06-Apr-18 (in house check Jun-20) | in house check Jun-22 | Power sensor E4112A | SN: 000100210 | 06-Apr-18 (in house check Jun-20) | in house check Jun-22 | RF generator HP 85940D | SN: U53840310700 | 04-Aug-09 (in house check Jun-20) | in house check Jun-22 | Network Analyzer Agilent E8363A | SN: U541000477 | 31-Mar-14 (in house check Oct-20) | in house check Oct-21 | <p>Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Accreditation No.: SCS 0108</p> <hr/> <p>Glossary:</p> <p>TSL: Issue simulating liquid sensitivity in TSL / NORM x,y,z</p> <p>ConvF: not applicable or not measured</p> <p>N/A: not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards:</p> <ol style="list-style-type: none"> IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013 IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016 IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010 KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz" <p>Additional Documentation:</p> <ol style="list-style-type: none"> DASY4/5 System Handbook <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in this certificate are valid at the frequency indicated. Antenna Parameters with TSL: The source is mounted in a touch configuration below the center marking of the flat phantom. Return Loss: This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <div style="border: 1px solid black; padding: 5px; margin-top: 10px;"> <p>The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> </div> <p>Certificate No: CLA150-4025_Apr21 Page 2 of 6</p> | | |
|--|------------------------------|-----------------------------------|----------------------------|------------------------|------------------------|-----------|---------------------------------|------------------|-----------------------------|-----------------|---------------------------|--------|----------------------|------------------------------|----------------------------------|-----------|----------------------------|-----------------|---------------------------|-------------|-----------------------------|--------------------|-----------------------------|---------|-------------------------------|------------|--------------------------------|-----------------|------------|------------------|---|----------|---------------------|------|---|-----------------|--------------------|----------------|-----------------------------------|-----------------------|-------------------------------------|------------------|-----------------------------------|---|---------------------|---------------|-----------------------------------|-----------------------|------------------------|-------------------------------------|-----------------------------------|--------------------------|---|--------------------------------------|-----------------------------------|-----------------------|--|-----------------|-------|
| Primary Standards | ID # | Cal Date (Certificate No.) | Schedule / Calibration | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power meter NRP | SN: 10475 | 09-Apr-21 (No. 217-03201.00292) | Apr-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor NRP Z01 | SN: 103344 | 09-Apr-21 (No. 217-03201) | Apr-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor NRP Z01 | SN: 103345 | 09-Apr-21 (No. 217-03202) | Apr-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reference 20 dB Attenuator | SN: C22962 (20) | 09-Apr-21 (No. 217-03343) | Apr-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Type-N mismatch combination | SN: 310952 / 00327 | 09-Apr-21 (No. 217-03344) | Apr-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reference Probe EX3004 (DIE4) | SN: 3877 | 30-Dec-20 (No. EX3-3877_Dec20) | Dec-21 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | SN: 664 | 26-Jun-20 (No. DMS4-656_Jun20) | Jun-21 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Secondary Standards | ID # | Check Date (in house) | Scheduled Check | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power meter E4118B | SN: G814282874 | 06-Apr-18 (in house check Jun-20) | in house check Jun-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor E4112A | SN: MY4148067 | 06-Apr-18 (in house check Jun-20) | in house check Jun-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor E4112A | SN: 000100210 | 06-Apr-18 (in house check Jun-20) | in house check Jun-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| RF generator HP 85940D | SN: U53840310700 | 04-Aug-09 (in house check Jun-20) | in house check Jun-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Network Analyzer Agilent E8363A | SN: U541000477 | 31-Mar-14 (in house check Oct-20) | in house check Oct-21 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <p>Measurement Conditions DASY system configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>DASY Version</th> <th>DASY5</th> <th>V52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>ELN Flat Phantom</td> <td>Shell thickness: 2 ± 0.2 mm</td> </tr> <tr> <td>EUT Positioning</td> <td>Touch Position</td> <td></td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy = 4.0 mm, dz = 1.4 mm</td> <td>Graded Ratio = 1.4 (Z direction)</td> </tr> <tr> <td>Frequency</td> <td>150 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p>Head TSL parameters The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>52.3</td> <td>0.75 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>51.1 ± 6 %</td> <td>0.75 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>< 0.5 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p>SAR result with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>1 W input power</td> <td>3.90 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>3.88 W/kg ± 18.4 % (k=2)</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>SAR averaged over 10 cm³ (10 g) of Head TSL</th> <th>condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>1 W input power</td> <td>2.60 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>2.59 W/kg ± 18.0 % (k=2)</td> </tr> </tbody> </table> <p>Certificate No: CLA150-4025_Apr21 Page 3 of 6</p> | DASY Version | DASY5 | V52.10.4 | Extrapolation | Advanced Extrapolation | | Phantom | ELN Flat Phantom | Shell thickness: 2 ± 0.2 mm | EUT Positioning | Touch Position | | Zoom Scan Resolution | dx, dy = 4.0 mm, dz = 1.4 mm | Graded Ratio = 1.4 (Z direction) | Frequency | 150 MHz ± 1 MHz | | | Temperature | Permittivity | Conductivity | Nominal Head TSL parameters | 22.0 °C | 52.3 | 0.75 mho/m | Measured Head TSL parameters | (22.0 ± 0.2) °C | 51.1 ± 6 % | 0.75 mho/m ± 6 % | Head TSL temperature change during test | < 0.5 °C | --- | --- | SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | | SAR measured | 1 W input power | 3.90 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 3.88 W/kg ± 18.4 % (k=2) | SAR averaged over 10 cm ³ (10 g) of Head TSL | condition | | SAR measured | 1 W input power | 2.60 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 2.59 W/kg ± 18.0 % (k=2) | <p>Appendix (Additional assessments outside the scope of SCS 0108)</p> <p>Antenna Parameters with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Impedance, transformed to feed point</th> <th>47.8 Ω ± 1.5 Ω</th> </tr> </thead> <tbody> <tr> <td>Return Loss</td> <td>-31.4 dB</td> </tr> </tbody> </table> <p>Additional EUT Data</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table> <p>Certificate No: CLA150-4025_Apr21 Page 4 of 6</p> | Impedance, transformed to feed point | 47.8 Ω ± 1.5 Ω | Return Loss | -31.4 dB | Manufactured by | SPEAG |
| DASY Version | DASY5 | V52.10.4 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Extrapolation | Advanced Extrapolation | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Phantom | ELN Flat Phantom | Shell thickness: 2 ± 0.2 mm | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| EUT Positioning | Touch Position | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Zoom Scan Resolution | dx, dy = 4.0 mm, dz = 1.4 mm | Graded Ratio = 1.4 (Z direction) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Frequency | 150 MHz ± 1 MHz | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | Temperature | Permittivity | Conductivity | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Nominal Head TSL parameters | 22.0 °C | 52.3 | 0.75 mho/m | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 51.1 ± 6 % | 0.75 mho/m ± 6 % | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Head TSL temperature change during test | < 0.5 °C | --- | --- | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 1 W input power | 3.90 W/kg | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 3.88 W/kg ± 18.4 % (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 10 cm ³ (10 g) of Head TSL | condition | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 1 W input power | 2.60 W/kg | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 2.59 W/kg ± 18.0 % (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Impedance, transformed to feed point | 47.8 Ω ± 1.5 Ω | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Return Loss | -31.4 dB | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Manufactured by | SPEAG | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

DASY5 Validation Report for Head TSL

Date: 26.04.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4025

Communication System: UID 0 - CW; Frequency: 150 MHz
 Medium parameters used: $f = 150 \text{ MHz}$; $\sigma = 0.76 \text{ S/m}$; $\epsilon = 51.1$; $\rho = 1000 \text{ kg/m}^3$
 Phantom section: Flat Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(12.51, 12.51, 12.51) @ 150 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA54 Snt54; Calibrated: 26.06.2020
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP.1003
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan, dist=1.4mm (8x10x8)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
 Reference Value = 85.93 W/m; Power Drift = -0.02 dB
 Peak SAR (extrapolated) = 7.36 W/kg
SAR(1 g) = 3.90 W/kg; SAR(10 g) = 2.60 W/kg
 Smallest distance from peaks to all points 3 dB below: Larger than measurement grid (> 30mm)
 Ratio of SAR at M2 to SAR at M1 = 80.4%
 Maximum value of SAR (measured) = 5.48 W/kg

Certificate No: CLA150-4025_Apr21 Page 5 of 6

Certificate No: CLA150-4025_Apr21 Page 6 of 6

1.2 D450V3 - SN 1103

Calibration Laboratory of Schmid & Partner Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client: **SGS-CN (Aude)** Certificate No: **D450V3-1103_Apr21**

CALIBRATION CERTIFICATE

Object: **D450V3 - SN:1103**

Calibration procedure(s): **QA CAL-15_v9**
 Calibration Procedure for SAR Validation Sources below 700 MHz

Calibration date: **April 21, 2021**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 0.1) °C and humidity < 70%.

Calibration Equipment used (MPE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|----------------------------|--------------------|----------------------------------|-----------------------|
| Power meter NRP | SN: 104778 | 09-Apr-21 (No. 217-03021/03030) | Apr-22 |
| Power sensor NRP-291 | SN: 103244 | 09-Apr-21 (No. 217-03021) | Apr-22 |
| Power sensor NRP-291 | SN: 103245 | 09-Apr-21 (No. 217-03020) | Apr-22 |
| Reference 20 dB Attenuator | SN: CC2852 (200) | 09-Apr-21 (No. 217-03345) | Apr-22 |
| Type-N mission combination | SN: 310982 / 06327 | 09-Apr-21 (No. 217-03344) | Apr-22 |
| Reference Probe E3030A | SN: 3877 | 30-Dec-20 (No. E303-2077_Dece20) | Dec-21 |
| DAEA | SN: 654 | 26-Jan-20 (No. DAE4-654_Jan20) | Jan-21 |

| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
|---------------------------------|------------------|-----------------------------------|-----------------------|
| Power meter E4418B | SN: GB41200274 | 06-Apr-16 (in house check Jun-20) | In house check Jun-22 |
| Power sensor E4412A | SN: MY41496027 | 06-Apr-16 (in house check Jun-20) | In house check Jun-22 |
| Power sensor E4412A | SN: 000100210 | 06-Apr-16 (in house check Jun-20) | In house check Jun-22 |
| RF generator HP 8448C | SN: U53406101700 | 04-Aug-09 (in house check Jun-20) | In house check Jun-22 |
| Network Analyzer Agilent E8358A | SN: U541980427 | 31-Mar-14 (in house check Oct-20) | In house check Oct-21 |

Calibrated by: **Christof Leuber** (Function: Laboratory Technician)

Approved by: **Katja Polovic** (Function: Technical Manager)

This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued: April 23, 2021

Certificate No: D450V3-1103_Apr21 Page 1 of 6

Calibration Laboratory of Schmid & Partner Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0106**

Glossary:

TSL: Issue simulating liquid
 ConvF: sensitivity in TSL / NORM x,y,z
 N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices; Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D450V3-1103_Apr21 Page 2 of 6

Measurement Conditions
 DASY5 system configuration, as far as not given on page 1.

| | | |
|------------------------------|------------------------|-----------------------------|
| DASY Version | DASY5 | V82.10.4 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | ELJ4 Flat Phantom | Shell thickness: 2 ± 0.2 mm |
| Distance Dipole Center - TSL | 15 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 450 MHz ± 1 MHz | |

Head TSL parameters
 The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|-----------------|--------------|------------------|
| Nominal Head TSL parameters | 22.0 °C | 43.5 | 0.57 mho/m |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 43.1 ± 6 % | 0.67 mho/m ± 8 % |
| Head TSL temperature change during test | < 0.5 °C | --- | --- |

SAR result with Head TSL

| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
|---|--------------------|--------------------------|
| SAR measured | 250 mW input power | 1.14 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 4.56 W/kg ± 18.1 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
|---|--------------------|--------------------------|
| SAR measured | 250 mW input power | 0.757 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 3.06 W/kg ± 17.6 % (k=2) |

Certificate No: D450V3-1103_Apr21 Page 3 of 6

Appendix (Additional assessments outside the scope of SCS 0106)

Antenna Parameters with Head TSL

| | |
|--------------------------------------|-----------------|
| Impedance, transformed to feed point | 57.1 Ω - 2.6 jΩ |
| Return Loss | -23.0 dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.346 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.
 The dipole is made of standard straight coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is set according to the Standard.
 No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

| | |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Certificate No: D450V3-1103_Apr21 Page 4 of 6

DASY5 Validation Report for Head TSL

Test Laboratory: SPEAG, Zurich, Switzerland
 Date: 21.04.2021

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1103
 Communication System: UID 0 - CW; Frequency: 450 MHz
 Medium parameters used: f = 450 MHz, α = 0.87 S/m; ε = 43.1; ρ = 1000 kg/m³
 Phantom section: Flat Section
 Measurement Standard: DASY5 (IEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.64, 10.64, 10.64) @ 450 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 26.06.2020
- Phantom: ELJ v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:
 Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 39.18 V/m; Power Drift = -0.08 dB
 Peak SAR (extrapolated) = 1.76 W/kg
 SAR(1 g) = 1.14 W/kg; SAR(10 g) = 0.767 W/kg
 Smallest distance from peaks to all points 3 dB below: Larger than measurement grid
 Ratio of SAR at M2 to SAR at M1 = 64.9%
 Maximum value of SAR (measured) = 1.53 W/kg

0 dB = 1.53 W/kg = 1.85 dBW/kg

Certificate No: D450V3-1103_Apr21 Page 5 of 6

Certificate No: D450V3-1103_Apr21 Page 6 of 6

1.3 D750V3 - SN 1188

| <div style="display: flex; justify-content: space-between;"> </div> <p> Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4236633-2112 Fax: +86-10-4236633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn </p> <p> Client: SGS-CN Certificate No: Z22-60103 </p> <h3>CALIBRATION CERTIFICATE</h3> <p> Object: D750V3 - SN: 1188 </p> <p> Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits </p> <p> Calibration date: March 28, 2022 </p> <p> This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. </p> <p> All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%. </p> <p> Calibration Equipment used (M&TE critical for calibration) </p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>102277</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP88</td> <td>104291</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21(SPEAG.No.EX3-7307_May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22(CTTL-SPEAG.No.Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4439C</td> <td>MY49671430</td> <td>13-Jan-22 (CTTL No.J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110973</td> <td>14-Jan-22 (CTTL No.J22X00409)</td> <td>Jan-23</td> </tr> </tbody> </table> <p> Calibrated by: Zhao Jing, SAR Test Engineer (Signature) </p> <p> Reviewed by: Lin Hao, SAR Test Engineer (Signature) </p> <p> Approved by: Qi Dianyuan, SAR Project Leader (Signature) </p> <p> Issued: April 3, 2022 </p> <p> This calibration certificate shall not be reproduced except in full without written approval of the laboratory. </p> <p> Certificate No: Z22-60103 Page 1 of 6 </p> | Primary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration | Power Meter NRP2 | 102277 | 24-Sep-21 (CTTL No.J21X08326) | Sep-22 | Power sensor NRP88 | 104291 | 24-Sep-21 (CTTL No.J21X08326) | Sep-22 | Reference Probe EX3DV4 | SN 7307 | 26-May-21(SPEAG.No.EX3-7307_May21) | May-22 | DAE4 | SN 1556 | 12-Jan-22(CTTL-SPEAG.No.Z22-60007) | Jan-23 | Secondary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration | Signal Generator E4439C | MY49671430 | 13-Jan-22 (CTTL No.J22X00409) | Jan-23 | Network Analyzer E5071C | MY46110973 | 14-Jan-22 (CTTL No.J22X00409) | Jan-23 | <div style="display: flex; justify-content: space-between;"> </div> <p> Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4236633-2079 Fax: +86-10-4236633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn </p> <p> Glossary: TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORMx.yz N/A: not applicable or not measured </p> <p> Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865684, "SAR Measurement Requirements for 100 MHz to 6 GHz" </p> <p> Additional Documentation: c) DASy4/5 System Handbook </p> <p> Methods Applied and Interpretation of Parameters: <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. </p> <div style="border: 1px solid black; padding: 5px;"> <p> The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%. </p> </div> <p> Certificate No: Z22-60103 Page 2 of 6 </p> | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
|---|--------------------------|--|--|-----------------------|------------------------|--------|-------------------------------|--------------------------|--------------------|------------------------------|-------------------------------|-------------|------------------------|-------------------|------------------------------------|-----------|-----------------|---------|------------------------------------|-------------|---------------------|--------------|--|-----------------------|-------------------------|------------|-------------------------------|-----------------|-------------------------|------------------|---|---------|---|-----|---|-----------|--|--------------|--------------------|-----------|-------------------------------------|------------------|---------------------------|---|-----------|--|--------------|--------------------|-----------|-------------------------------------|------------------|---------------------------|--|--------------------------------------|---------------|-------------|---------|----------------------------------|----------|--|--|-----------------|-------|--|--|
| Primary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power Meter NRP2 | 102277 | 24-Sep-21 (CTTL No.J21X08326) | Sep-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor NRP88 | 104291 | 24-Sep-21 (CTTL No.J21X08326) | Sep-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reference Probe EX3DV4 | SN 7307 | 26-May-21(SPEAG.No.EX3-7307_May21) | May-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| DAE4 | SN 1556 | 12-Jan-22(CTTL-SPEAG.No.Z22-60007) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Secondary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Signal Generator E4439C | MY49671430 | 13-Jan-22 (CTTL No.J22X00409) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Network Analyzer E5071C | MY46110973 | 14-Jan-22 (CTTL No.J22X00409) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <div style="display: flex; justify-content: space-between;"> </div> <p> Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4236633-2079 Fax: +86-10-4236633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn </p> <p> Measurement Conditions DASy system configuration, as far as not given on page 1. </p> <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY52</th> <th>V52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>750 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p> Head TSL parameters The following parameters and calculations were applied. </p> <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>42.0</td> <td>0.90 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>41.4 ± 0.6 %</td> <td>0.89 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p> SAR result with Head TSL </p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm² (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.07 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>8.27 W/kg ± 18.8 %, (k=2)</td> </tr> <tr> <th>SAR averaged over 10 cm² (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.37 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>5.48 W/kg ± 18.7 %, (k=2)</td> </tr> </tbody> </table> <p> Certificate No: Z22-60103 Page 3 of 6 </p> | DASY Version | DASY52 | V52.10.4 | Extrapolation | Advanced Extrapolation | | Phantom | Triple Flat Phantom 5.1C | | Distance Dipole Center - TSL | 15 mm | with Spacer | Zoom Scan Resolution | dx, dy, dz = 5 mm | | Frequency | 750 MHz ± 1 MHz | | | Temperature | Permittivity | Conductivity | Nominal Head TSL parameters | 22.0 °C | 42.0 | 0.90 mho/m | Measured Head TSL parameters | (22.0 ± 0.2) °C | 41.4 ± 0.6 % | 0.89 mho/m ± 6 % | Head TSL temperature change during test | <1.0 °C | --- | --- | SAR averaged over 1 cm ² (1 g) of Head TSL | Condition | | SAR measured | 250 mW input power | 2.07 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 8.27 W/kg ± 18.8 %, (k=2) | SAR averaged over 10 cm ² (10 g) of Head TSL | Condition | | SAR measured | 250 mW input power | 1.37 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 5.48 W/kg ± 18.7 %, (k=2) | <div style="display: flex; justify-content: space-between;"> </div> <p> Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4236633-2079 Fax: +86-10-4236633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn </p> <p> Appendix (Additional assessments outside the scope of CNAS L0570) </p> <p> Antenna Parameters with Head TSL </p> <table border="1"> <thead> <tr> <th>Impedance, transformed to feed point</th> <th>53.60- 1.13jΩ</th> </tr> </thead> <tbody> <tr> <td>Return Loss</td> <td>-28.7dB</td> </tr> </tbody> </table> <p> General Antenna Parameters and Design </p> <table border="1"> <thead> <tr> <th>Electrical Delay (one direction)</th> <th>0.947 ns</th> </tr> </thead> <tbody> <tr> <td>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</td> <td></td> </tr> </tbody> </table> <p> The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. </p> <p> Additional EUT Data </p> <table border="1"> <thead> <tr> <th>Manufactured by</th> <th>SPEAG</th> </tr> </thead> <tbody> <tr> <td></td> <td></td> </tr> </tbody> </table> <p> Certificate No: Z22-60103 Page 4 of 6 </p> | Impedance, transformed to feed point | 53.60- 1.13jΩ | Return Loss | -28.7dB | Electrical Delay (one direction) | 0.947 ns | After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. | | Manufactured by | SPEAG | | |
| DASY Version | DASY52 | V52.10.4 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Extrapolation | Advanced Extrapolation | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Phantom | Triple Flat Phantom 5.1C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Distance Dipole Center - TSL | 15 mm | with Spacer | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Frequency | 750 MHz ± 1 MHz | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | Temperature | Permittivity | Conductivity | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Nominal Head TSL parameters | 22.0 °C | 42.0 | 0.90 mho/m | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 41.4 ± 0.6 % | 0.89 mho/m ± 6 % | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Head TSL temperature change during test | <1.0 °C | --- | --- | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 1 cm ² (1 g) of Head TSL | Condition | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 250 mW input power | 2.07 W/kg | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 8.27 W/kg ± 18.8 %, (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 10 cm ² (10 g) of Head TSL | Condition | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 250 mW input power | 1.37 W/kg | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 5.48 W/kg ± 18.7 %, (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Impedance, transformed to feed point | 53.60- 1.13jΩ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Return Loss | -28.7dB | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Electrical Delay (one direction) | 0.947 ns | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Manufactured by | SPEAG | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

TTL Speaq CALIBRATION LABORATORY
 In Collaboration with **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62506633-2079 Fax: +86-10-62506633-2564
 E-mail: cti@china.ttl.com http://www.chinatit.com

DASY5 Validation Report for Head TSL Date: 2022-03-29
 Test Laboratory: CTTL, Beijing, China
 DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN: 1188
 Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 750 \text{ MHz}$; $\sigma = 0.888 \text{ S/m}$; $\epsilon_r = 41.36$; $\rho = 1000 \text{ kg/m}^3$
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(10.31, 10.31, 10.31) @ 750 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 S01556; Calibrated: 2022-01-12
- Phantom: MFP-V5.1C (20kg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52.52.10.4(1535); SEMCADX 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 55.06 V/m; Power Drift = 0.00 dB
 Peak SAR (extrapolated) = 3.07 W/kg
 SAR(1 g) = 2.07 W/kg; SAR(10 g) = 1.37 W/kg
 Smallest distance from peaks to all points 3 dB below = 18.9 mm
 Ratio of SAR at M2 to SAR at M1 = 67.1%
 Maximum value of SAR (measured) = 2.74 W/kg

Certificate No: Z22-60103 Page 5 of 6

TTL Speaq CALIBRATION LABORATORY
 In Collaboration with **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62506633-2079 Fax: +86-10-62506633-2564
 E-mail: cti@china.ttl.com http://www.chinatit.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60103 Page 6 of 6

1.4 D835V2 - SN 4d114

TTL Speaq CALIBRATION LABORATORY
 In Collaboration with **CAICT** and **CNAS**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191
 Tel: +86-10-62506633-2079 Fax: +86-10-62506633-2564
 E-mail: cti@china.ttl.com http://www.chinatit.com

Client: **SGS-CN** Certificate No: **Z22-60104**

CALIBRATION CERTIFICATE

Object: D835V2 - SN: 4d114
 Calibration Procedure(s): FF-Z11-003-01
 Calibration Procedures for dipole validation kits
 Calibration date: March 31, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|------------------------|---------|---|-----------------------|
| Power Meter NRP2 | 106277 | 24-Sep-21 (CTTL, No.J21X08326) | Sep-22 |
| Power sensor NRPBS | 104291 | 24-Sep-21 (CTTL, No.J21X08326) | Sep-22 |
| Reference Probe EX3DV4 | SN 7307 | 26-May-21(SPEAG.No.EX3-7307_May21) | May-22 |
| DAE4 | SN 1556 | 12-Jan-22(CTTL-SPEAG.No.Z22-60007) | Jan-23 |

| Secondary Standards | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration |
|-------------------------|------------|---|-----------------------|
| Signal Generator E4438C | MY49071430 | 13-Jan-22 (CTTL, No.J22X00409) | Jan-23 |
| Network Analyzer E5071C | MY46110673 | 14-Jan-22 (CTTL, No.J22X00409) | Jan-23 |

Calibrated by: Zhao Jing, SAR Test Engineer
 Reviewed by: Lin Hao, SAR Test Engineer
 Approved by: Qi Dianyuan, SAR Project Leader

Issued: April 6, 2022
 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60104 Page 1 of 6

TTL Speaq CALIBRATION LABORATORY
 In Collaboration with **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-62506633-2079 Fax: +86-10-62506633-2564
 E-mail: cti@china.ttl.com http://www.chinatit.com

Glossary:
 TSL: tissue simulating liquid
 ConvF: sensitivity in TSL / NORMx.yz
 N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
 a) IEC/IEEE 62208-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
 b) KDB 685864, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:
 c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60104 Page 2 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@china.ttl.com http://www.china.ttl.com

Measurement Conditions
 DASY system configuration, as far as not given on page 1.

| | | |
|------------------------------|--------------------------|-------------|
| DASY Version | DASY52 | VS2 10.4 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Triple Flat Phantom 5.1C | |
| Distance Dipole Center - TSL | 15 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 835 MHz ± 1 MHz | |

Head TSL parameters
 The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|-----------------|--------------|------------------|
| Nominal Head TSL parameters | 22.0 °C | 41.5 | 0.90 mho/m |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 41.0 ± 5 % | 0.91 mho/m ± 8 % |
| Head TSL temperature change during test | <1.0 °C | --- | --- |

SAR result with Head TSL

| | | |
|---|--------------------|---------------------------------|
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 2.37 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 6.40 W/kg ± 18.6 % (k=2) |
| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 1.54 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 6.12 W/kg ± 18.7 % (k=2) |

Certificate No: Z22-60104 Page 3 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@china.ttl.com http://www.china.ttl.com

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

| | |
|--------------------------------------|----------------|
| Impedance, transformed to feed point | 48.70 - 5.22jΩ |
| Return Loss | -25.3dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.307 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

| | |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Certificate No: Z22-60104 Page 4 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@china.ttl.com http://www.china.ttl.com

DASY5 Validation Report for Head TSL Date: 2022-03-31
 Test Laboratory: CTTL, Beijing, China
 DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d114
 Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1
 Medium parameters used: f = 835 MHz; σ = 0.907 S/m; ε_r = 40.98; ρ = 1000 kg/m³
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(10.13, 10.13, 10.13) @ 835 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA4 Sni 1556; Calibrated: 2022-01-12
- Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 57.88 V/m; Power Drift = 0.04 dB
 Peak SAR (extrapolated) = 3.56 W/kg
SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.54 W/kg
 Smallest distance from peaks to all points 3 dB below = 15.8 mm
 Ratio of SAR at M2 to SAR at M1 = 66.2%
 Maximum value of SAR (measured) = 3.17 W/kg

0 dB = 3.17 W/kg = 5.01 dBW/kg

Certificate No: Z22-60104 Page 5 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@china.ttl.com http://www.china.ttl.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60104 Page 6 of 6

1.5 D900V2 - SN 1d079

| <div style="display: flex; justify-content: space-between; align-items: center;"> <div style="text-align: center;"> <small>In Collaboration with CALIBRATION LABORATORY</small> <small>ADD: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42306633-2117 E-mail: cti@ttest.com</small> </div> <div style="text-align: center;"> <small>中国合格评定国家认可委员会 CALIBRATION CLASS 1070</small> </div> <div style="text-align: center;"> <small>中国信息通信研究院 CALIBRATION CLASS 1070</small> </div> </div> <p style="text-align: center;">Client: SGS-CN Certificate No: Z22-60184</p> <h3 style="text-align: center;">CALIBRATION CERTIFICATE</h3> <p>Object: D900V2 - SN: 1d079</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: June 7, 2022</p> <p>The calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7464</td> <td>26-Jan-22 (SPEAG No. EX3-7464_Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAE4</td> <td>SN 1566</td> <td>12-Jan-22 (CTTL-SPEAG No. Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4438C</td> <td>M146071430</td> <td>13-Jan-22 (CTTL No. J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>M146110673</td> <td>14-Jan-22 (CTTL No. J22X00409)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>Calibrated by:</th> <th>Name</th> <th>Function</th> <th>Signature</th> </tr> </thead> <tbody> <tr> <td></td> <td>Zhao Jing</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <td>Reviewed by:</td> <td>Lin Hao</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <td>Approved by:</td> <td>Qi Diqiyuan</td> <td>SAR Project Leader</td> <td></td> </tr> </tbody> </table> <p style="text-align: center;">Issued: June 13, 2022</p> <p style="text-align: center;">The calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p style="text-align: center;">Certificate No: Z22-60184 Page 1 of 6</p> | Primary Standards | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration | Power Meter NRP2 | 106277 | 24-Sep-21 (CTTL No. J21X08326) | Sep-22 | Power sensor NRP8S | 104291 | 24-Sep-21 (CTTL No. J21X08326) | Sep-22 | Reference Probe EX3DV4 | SN 7464 | 26-Jan-22 (SPEAG No. EX3-7464_Jan22) | Jan-23 | DAE4 | SN 1566 | 12-Jan-22 (CTTL-SPEAG No. Z22-60007) | Jan-23 | Secondary Standards | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration | Signal Generator E4438C | M146071430 | 13-Jan-22 (CTTL No. J22X00409) | Jan-23 | Network Analyzer E5071C | M146110673 | 14-Jan-22 (CTTL No. J22X00409) | Jan-23 | Calibrated by: | Name | Function | Signature | | Zhao Jing | SAR Test Engineer | | Reviewed by: | Lin Hao | SAR Test Engineer | | Approved by: | Qi Diqiyuan | SAR Project Leader | | <div style="display: flex; justify-content: space-between; align-items: center;"> <div style="text-align: center;"> <small>In Collaboration with CALIBRATION LABORATORY</small> <small>ADD: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42306633-2117 E-mail: cti@ttest.com</small> </div> <div style="text-align: center;"> <small>中国信息通信研究院 CALIBRATION CLASS 1070</small> </div> </div> <p style="text-align: center;">Certificate No: Z22-60184 Page 2 of 6</p> <p>Glossary:</p> <p>TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORM_{x,y,z} N/A: not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Additional Documentation:</p> <p>c) DASY4/S System Handbook</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in this certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <div style="border: 1px solid black; padding: 5px; margin-top: 10px;"> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> </div> <p style="text-align: center;">Certificate No: Z22-60184 Page 2 of 6</p> | | | | | | | | | | | | |
|--|--------------------------|---|---|-----------------------|------------------------|--------|--------------------------------|--------------------------|--------------------|------------------------------|--------------------------------|-------------|------------------------|---------------|--------------------------------------|-----------|-----------------|---------|--------------------------------------|-------------|---------------------|--------------|---|-----------------------|-------------------------|------------|--------------------------------|-----------------|-------------------------|------------------|---|---------|----------------|------|---|-----------|--|--------------|--------------------|-----------|-------------------------------------|------------------|--------------------------|---|--------------|-------------|--------------------|--------------------|---|-------------------------------------|------------------|--------------------------|---|--------------------------------------|----------------|-------------|----------|----------------------------------|----------|-----------------|-------|
| Primary Standards | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power Meter NRP2 | 106277 | 24-Sep-21 (CTTL No. J21X08326) | Sep-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor NRP8S | 104291 | 24-Sep-21 (CTTL No. J21X08326) | Sep-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reference Probe EX3DV4 | SN 7464 | 26-Jan-22 (SPEAG No. EX3-7464_Jan22) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| DAE4 | SN 1566 | 12-Jan-22 (CTTL-SPEAG No. Z22-60007) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Secondary Standards | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Signal Generator E4438C | M146071430 | 13-Jan-22 (CTTL No. J22X00409) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Network Analyzer E5071C | M146110673 | 14-Jan-22 (CTTL No. J22X00409) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Calibrated by: | Name | Function | Signature | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | Zhao Jing | SAR Test Engineer | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reviewed by: | Lin Hao | SAR Test Engineer | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Approved by: | Qi Diqiyuan | SAR Project Leader | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <div style="display: flex; justify-content: space-between; align-items: center;"> <div style="text-align: center;"> <small>In Collaboration with CALIBRATION LABORATORY</small> <small>ADD: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42306633-2117 E-mail: cti@ttest.com</small> </div> <div style="text-align: center;"> <small>中国信息通信研究院 CALIBRATION CLASS 1070</small> </div> </div> <p>Measurement Conditions</p> <p>DASY system configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>DASY Version</th> <th>DASY52</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dk, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>900 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p>Head TSL parameters</p> <p>The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>41.5</td> <td>0.07 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>42.1 ± 6 %</td> <td>0.08 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p>SAR result with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.70 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>11.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.73 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>7.09 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p style="text-align: center;">Certificate No: Z22-60184 Page 3 of 6</p> | DASY Version | DASY52 | 52.10.4 | Extrapolation | Advanced Extrapolation | | Phantom | Triple Flat Phantom 5.1C | | Distance Dipole Center - TSL | 15 mm | with Spacer | Zoom Scan Resolution | dk, dz = 5 mm | | Frequency | 900 MHz ± 1 MHz | | | Temperature | Permittivity | Conductivity | Nominal Head TSL parameters | 22.0 °C | 41.5 | 0.07 mho/m | Measured Head TSL parameters | (22.0 ± 0.2) °C | 42.1 ± 6 % | 0.08 mho/m ± 6 % | Head TSL temperature change during test | <1.0 °C | --- | --- | SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | | SAR measured | 250 mW input power | 2.70 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 11.0 W/kg ± 18.8 % (k=2) | SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | | SAR measured | 250 mW input power | 1.73 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 7.09 W/kg ± 18.7 % (k=2) | <div style="display: flex; justify-content: space-between; align-items: center;"> <div style="text-align: center;"> <small>In Collaboration with CALIBRATION LABORATORY</small> <small>ADD: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42306633-2117 E-mail: cti@ttest.com</small> </div> <div style="text-align: center;"> <small>中国信息通信研究院 CALIBRATION CLASS 1070</small> </div> </div> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td>48.10 - 8.48jΩ</td> </tr> <tr> <td>Return Loss</td> <td>-23.3 dB</td> </tr> </tbody> </table> <p>General Antenna Parameters and Design</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tbody> <tr> <td>Electrical Delay (one direction)</td> <td>1.312 ns</td> </tr> </tbody> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table> <p style="text-align: center;">Certificate No: Z22-60184 Page 4 of 6</p> | Impedance, transformed to feed point | 48.10 - 8.48jΩ | Return Loss | -23.3 dB | Electrical Delay (one direction) | 1.312 ns | Manufactured by | SPEAG |
| DASY Version | DASY52 | 52.10.4 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Extrapolation | Advanced Extrapolation | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Phantom | Triple Flat Phantom 5.1C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Distance Dipole Center - TSL | 15 mm | with Spacer | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Zoom Scan Resolution | dk, dz = 5 mm | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Frequency | 900 MHz ± 1 MHz | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | Temperature | Permittivity | Conductivity | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Nominal Head TSL parameters | 22.0 °C | 41.5 | 0.07 mho/m | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 42.1 ± 6 % | 0.08 mho/m ± 6 % | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Head TSL temperature change during test | <1.0 °C | --- | --- | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 250 mW input power | 2.70 W/kg | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 11.0 W/kg ± 18.8 % (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 250 mW input power | 1.73 W/kg | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 7.09 W/kg ± 18.7 % (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Impedance, transformed to feed point | 48.10 - 8.48jΩ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Return Loss | -23.3 dB | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Electrical Delay (one direction) | 1.312 ns | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Manufactured by | SPEAG | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

In Collaboration with
CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42306033-2117
E-mail: cti@chinaetli.com
http://www.caict.ac.cn

Date: 2022-06-07

DASY5 Validation Report for Head TSL

Test Laboratory: CTTL, Beijing, China
DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN: 14079
 Communication System: UTD 0, CW; Frequency: 900 MHz; Duty Cycle: 1:1
 Medium parameters used: f = 900 MHz; $\sigma = 0.98$ S/m; $\epsilon_r = 42.05$; $\rho = 1000$ kg/m³
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(9.72, 9.72) @ 900 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronic: DA44 - SN1556; Calibrated: 2022-01-12
- Phantom: MFP_V5.1C (2ddeg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52.52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7) (7x7) Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 59.81 V/m; Power Drift = -0.01 dB
 Peak SAR (extrapolated) = 4.20 W/kg
 SAR(1 g) = 2.78 W/kg; SAR(10 g) = 1.78 W/kg
 Smallest distance from peaks to all points 3 dB below = 16 mm
 Ratio of SAR at M2 to SAR at M1 = 65.8%
 Maximum value of SAR (measured) = 3.71 W/kg

0 dB = 3.71 W/kg = 5.69 dBW/kg

Certificate No: Z22-60184 Page 6 of 6

In Collaboration with
CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42306033-2117
E-mail: cti@chinaetli.com
http://www.caict.ac.cn

Date: 2022-06-07

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60184 Page 6 of 6

1.6 D1800V2 - SN 2d170

In Collaboration with
CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42306033-2117
E-mail: cti@chinaetli.com
http://www.caict.ac.cn

Date: 2022-06-07

Client: SGS-CN Certificate No: Z22-60105

CALIBRATION CERTIFICATE

Object: D1800V2 - SN: 2d170

Calibration Procedure(s): FF-Z11-003-01
 Calibration Procedures for dipole validation kits

Calibration date: March 31, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration |
|------------------------|---------|--|-----------------------|
| Power Meter NRP2 | 106277 | 24-Sep-21 (CTTL No.J21X08326) | Sep-22 |
| Power sensor NRP2 | 104291 | 24-Sep-21 (CTTL No.J21X08326) | Sep-22 |
| Reference Probe EX3DV4 | SN 7307 | 26-May-21(SPEAG.No.EK3-7307_May21) | May-22 |
| DAE4 | SN 1556 | 12-Jan-22(CTTL-SPEAG.No.Z22-60007) | Jan-23 |

| Secondary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration |
|-------------------------|------------|--|-----------------------|
| Signal Generator E4438C | MY49071430 | 13-Jan-22 (CTTL No.J22X00406) | Jan-23 |
| Network Analyzer E5071C | MY46110973 | 14-Jan-22 (CTTL No.J22X00406) | Jan-23 |

Calibrated by: Zhao Jing, SAR Test Engineer, Signature: [Signature]

Reviewed by: Lin Hao, SAR Test Engineer, Signature: [Signature]

Approved by: Qi Diqian, SAR Project Leader, Signature: [Signature]

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60105 Page 1 of 6

In Collaboration with
CAICT

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42306033-2079
E-mail: cti@chinaetli.com
http://www.caict.ac.cn

Date: 2022-06-07

Glossary:

TSL: tissue simulating liquid
 ConvF: sensitivity in TSL / NORMx.y.z
 N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60105 Page 2 of 6

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@chinaeui.com http://www.chinaeui.com

Measurement Conditions
 DASYS system configuration, as far as not given on page 1.

| | | |
|------------------------------|--------------------------|-------------|
| DASY Version | DASY52 | 52.10.4 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Triple Flat Phantom 5.1C | |
| Distance Dipole Center - TSL | 10 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 1800 MHz ± 1 MHz | |

Head TSL parameters
 The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|-----------------|--------------|------------------|
| Nominal Head TSL parameters | 22.0 °C | 40.0 | 1.40 mholm |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 40.8 ± 8 % | 1.41 mholm ± 8 % |
| Head TSL temperature change during test | <1.0 °C | --- | --- |

SAR result with Head TSL

| | | |
|---|--------------------|--------------------------|
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 9.73 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 38.9 W/kg ± 18.8 % (k=2) |
| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 5.11 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 20.4 W/kg ± 18.7 % (k=2) |

Certificate No: Z22-60105 Page 3 of 6

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@chinaeui.com http://www.chinaeui.com

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

| | |
|--------------------------------------|--------------|
| Impedance, transformed to feed point | 47.90-2.54jΩ |
| Return Loss | -29.4dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.116 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

| | |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Certificate No: Z22-60105 Page 4 of 6

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@chinaeui.com http://www.chinaeui.com

DASY5 Validation Report for Head TSL Date: 2022-03-31
 Test Laboratory: CTTL, Beijing, China
 DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d170
 Communication System: UID 0, CW; Frequency: 1800 MHz; Duty Cycle: 1:1
 Medium parameters used: f = 1800 MHz; σ = 1.411 S/m; ε = 40.62; ρ = 1000 kg/m³
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(8.34, 8.34) @ 1800 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (Cube 0): Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 98.14 V/m; Power Drift = 0.03 dB
 Peak SAR (extrapolated) = 18.2 W/kg
 SAR(1 g) = 9.73 W/kg; SAR(10 g) = 5.11 W/kg
 Smallest distance from peaks to all points 3 dB below = 10 mm
 Ratio of SAR at M2 to SAR at M1 = 54%
 Maximum value of SAR (measured) = 15.2 W/kg

0 dB = 15.2 W/kg = 11.82 dBW/kg

Certificate No: Z22-60105 Page 5 of 6

In Collaboration with **TTL Speaq** CALIBRATION LABORATORY and **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504
 E-mail: cti@chinaeui.com http://www.chinaeui.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60105 Page 6 of 6

1.7 D1900V2 - SN 5d136

| <div style="display: flex; justify-content: space-between; align-items: center;"> </div> <p style="font-size: small;">In Collaboration with TTL Calibration Laboratory S P E A G Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: vt@ttslab.com http://www.caict.ac.cn</p> <p style="text-align: center;">Client: SGS-CN Certificate No: Z22-60185</p> <div style="border: 1px solid black; padding: 5px;"> <p>CALIBRATION CERTIFICATE</p> <p>Object: D1900V2 - SN: 5d136</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: June 7, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility; environment temperature (23±)°C and humidity<70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p> <table border="1" style="width: 100%; font-size: x-small;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>106277</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP6S</td> <td>104291</td> <td>24-Sep-21 (CTTL No. J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EXSDV4</td> <td>SN 7464</td> <td>28-Jan-22 (SPEAG No. EX3-7464_Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAE4</td> <td>SN 1656</td> <td>12-Jan-22 (CTTL-SPEAG No. Z22-60007)</td> <td>Jan-23</td> </tr> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> <tr> <td>Signal Generator E4438C</td> <td>MY48671430</td> <td>13-Jan-22 (CTTL No. J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyser E5071C</td> <td>MY48110673</td> <td>14-Jan-22 (CTTL No. J22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1" style="width: 100%; font-size: x-small;"> <thead> <tr> <th>Calibrated by:</th> <th>Name</th> <th>Function</th> <th>Signature</th> </tr> </thead> <tbody> <tr> <td></td> <td>Zhao Jing</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <td>Reviewed by:</td> <td>Lin Hao</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <td>Approved by:</td> <td>Qi Dianyuan</td> <td>SAR Project Leader</td> <td></td> </tr> </tbody> </table> <p style="text-align: center;">Issued: June 13, 2022</p> <p style="font-size: x-small;">This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> </div> <p style="font-size: x-small;">Certificate No: Z22-60185 Page 1 of 6</p> | Primary Standards | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration | Power Meter NRP2 | 106277 | 24-Sep-21 (CTTL No. J21X08326) | Sep-22 | Power sensor NRP6S | 104291 | 24-Sep-21 (CTTL No. J21X08326) | Sep-22 | Reference Probe EXSDV4 | SN 7464 | 28-Jan-22 (SPEAG No. EX3-7464_Jan22) | Jan-23 | DAE4 | SN 1656 | 12-Jan-22 (CTTL-SPEAG No. Z22-60007) | Jan-23 | Secondary Standards | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration | Signal Generator E4438C | MY48671430 | 13-Jan-22 (CTTL No. J22X00409) | Jan-23 | Network Analyser E5071C | MY48110673 | 14-Jan-22 (CTTL No. J22X00406) | Jan-23 | Calibrated by: | Name | Function | Signature | | Zhao Jing | SAR Test Engineer | | Reviewed by: | Lin Hao | SAR Test Engineer | | Approved by: | Qi Dianyuan | SAR Project Leader | | <div style="display: flex; justify-content: space-between; align-items: center;"> </div> <p style="font-size: small;">In Collaboration with TTL Calibration Laboratory S P E A G Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: vt@ttslab.com http://www.caict.ac.cn</p> <p>Glossary:</p> <p>TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORMx.y.z NA: not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1526: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865984, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Additional Documentation: c) DASY4/S System Handbook</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> • Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. • Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <div style="border: 1px solid black; padding: 5px; font-size: x-small;"> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> </div> <p style="font-size: x-small;">Certificate No: Z22-60185 Page 2 of 6</p> | | | | | | | | | | | | |
|--|--------------------------|---|---|-----------------------|------------------------|--------|--------------------------------|--------------------------|--------------------|------------------------------|--------------------------------|-------------|------------------------|-------------------|--------------------------------------|-----------|------------------|---------|--------------------------------------|-------------|---------------------|--------------|---|-----------------------|-------------------------|------------|--------------------------------|-----------------|-------------------------|-----------------|---|----------|----------------|------|---|-----------|--|--------------|--------------------|-----------|-------------------------------------|------------------|--------------------------|---|--------------|-------------|--------------------|--------------------|---|-------------------------------------|------------------|--------------------------|---|--------------------------------------|-----------------|-------------|---------|----------------------------------|----------|-----------------|-------|
| Primary Standards | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power Meter NRP2 | 106277 | 24-Sep-21 (CTTL No. J21X08326) | Sep-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor NRP6S | 104291 | 24-Sep-21 (CTTL No. J21X08326) | Sep-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reference Probe EXSDV4 | SN 7464 | 28-Jan-22 (SPEAG No. EX3-7464_Jan22) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| DAE4 | SN 1656 | 12-Jan-22 (CTTL-SPEAG No. Z22-60007) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Secondary Standards | ID # | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Signal Generator E4438C | MY48671430 | 13-Jan-22 (CTTL No. J22X00409) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Network Analyser E5071C | MY48110673 | 14-Jan-22 (CTTL No. J22X00406) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Calibrated by: | Name | Function | Signature | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | Zhao Jing | SAR Test Engineer | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reviewed by: | Lin Hao | SAR Test Engineer | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Approved by: | Qi Dianyuan | SAR Project Leader | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <div style="display: flex; justify-content: space-between; align-items: center;"> </div> <p style="font-size: small;">In Collaboration with TTL Calibration Laboratory S P E A G Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: vt@ttslab.com http://www.caict.ac.cn</p> <p>Measurement Conditions DASY system configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; font-size: x-small;"> <thead> <tr> <th>DASY Version</th> <th>DASY52</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>1900 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p>Head TSL parameters The following parameters and calculations were applied:</p> <table border="1" style="width: 100%; font-size: x-small;"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>40.0</td> <td>1.40 mS/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.9 ± 6 %</td> <td>1.39 mS/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><+1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p>SAR result with Head TSL</p> <table border="1" style="width: 100%; font-size: x-small;"> <thead> <tr> <th>SAR averaged over 1 cm² (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>9.65 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>40.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <th>SAR averaged over 10 cm² (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.18 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>20.8 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p style="font-size: x-small;">Certificate No: Z22-60185 Page 3 of 6</p> | DASY Version | DASY52 | 52.10.4 | Extrapolation | Advanced Extrapolation | | Phantom | Triple Flat Phantom 5.1C | | Distance Dipole Center - TSL | 10 mm | with Spacer | Zoom Scan Resolution | dx, dy, dz = 5 mm | | Frequency | 1900 MHz ± 1 MHz | | | Temperature | Permittivity | Conductivity | Nominal Head TSL parameters | 22.0 °C | 40.0 | 1.40 mS/m | Measured Head TSL parameters | (22.0 ± 0.2) °C | 39.9 ± 6 % | 1.39 mS/m ± 6 % | Head TSL temperature change during test | <+1.0 °C | --- | --- | SAR averaged over 1 cm ² (1 g) of Head TSL | Condition | | SAR measured | 250 mW input power | 9.65 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 40.0 W/kg ± 18.8 % (k=2) | SAR averaged over 10 cm ² (10 g) of Head TSL | Condition | | SAR measured | 250 mW input power | 5.18 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 20.8 W/kg ± 18.7 % (k=2) | <div style="display: flex; justify-content: space-between; align-items: center;"> </div> <p style="font-size: small;">In Collaboration with TTL Calibration Laboratory S P E A G Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42204633-2117 E-mail: vt@ttslab.com http://www.caict.ac.cn</p> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1" style="width: 100%; font-size: x-small;"> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td>51.2Ω ± 7.5Ω(j)</td> </tr> <tr> <td>Return Loss</td> <td>-22.4dB</td> </tr> </tbody> </table> <p>General Antenna Parameters and Design</p> <table border="1" style="width: 100%; font-size: x-small;"> <tbody> <tr> <td>Electrical Delay (one direction)</td> <td>1.109 ns</td> </tr> </tbody> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1" style="width: 100%; font-size: x-small;"> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table> <p style="font-size: x-small;">Certificate No: Z22-60185 Page 4 of 6</p> | Impedance, transformed to feed point | 51.2Ω ± 7.5Ω(j) | Return Loss | -22.4dB | Electrical Delay (one direction) | 1.109 ns | Manufactured by | SPEAG |
| DASY Version | DASY52 | 52.10.4 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Extrapolation | Advanced Extrapolation | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Phantom | Triple Flat Phantom 5.1C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Distance Dipole Center - TSL | 10 mm | with Spacer | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Frequency | 1900 MHz ± 1 MHz | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | Temperature | Permittivity | Conductivity | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Nominal Head TSL parameters | 22.0 °C | 40.0 | 1.40 mS/m | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 39.9 ± 6 % | 1.39 mS/m ± 6 % | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Head TSL temperature change during test | <+1.0 °C | --- | --- | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 1 cm ² (1 g) of Head TSL | Condition | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 250 mW input power | 9.65 W/kg | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 40.0 W/kg ± 18.8 % (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 10 cm ² (10 g) of Head TSL | Condition | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 250 mW input power | 5.18 W/kg | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 20.8 W/kg ± 18.7 % (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Impedance, transformed to feed point | 51.2Ω ± 7.5Ω(j) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Return Loss | -22.4dB | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Electrical Delay (one direction) | 1.109 ns | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Manufactured by | SPEAG | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62066317 E-mail: uttl@ttspeag.com http://www.caict.ac.cn

Date: 2022-06-07

DASY5 Validation Report for Head TSL
Test Laboratory: CTTL, Beijing, China
DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 54136
Communication System: UTD 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 1900 \text{ MHz}$; $\sigma = 1.385 \text{ S/m}$; $\epsilon_r = 39.85$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Right Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(R,18, 8.18, 8.18) @ 1900 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP_V5_IC (20kg probe kit); Type: QD 000 P51 Cx; Serial: 1062
- DASY52.10.4(1535); SEMCAD X.14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube D: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 99.99 V/m; Power Drift = 0.04 dB
Peak SAR (extrapolated) = 18.6 W/kg
SAR(1g) = 9.95 W/kg; SAR(10g) = 5.18 W/kg
Smallest distance from peaks to all points 3 dB below = 9.2 mm
Ratio of SAR at M2 to SAR at M1 = 54.1%

Maximum value of SAR (measured) = 15.6 W/kg

0 dB = 15.6 W/kg = 11.93 dBW/kg

Certificate No: Z22-60185 Page 5 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62066317 E-mail: uttl@ttspeag.com http://www.caict.ac.cn

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60185 Page 6 of 6

1.8 D2000V2 - SN 1041

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT** **CNAS** **中国合格评定** **认证认可** **委员会** **校准** **CNAS** **1370**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62066317 E-mail: uttl@ttspeag.com http://www.caict.ac.cn

Client: **SGS-CN** Certificate No: **Z22-60188**

CALIBRATION CERTIFICATE

Object: D2000V2 - SN: 1041

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: June 6, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (8). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (23±3)°C and humidity <70%.

Calibration Equipment used (M&E critical for calibration)

| Primary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration |
|------------------------|---------|--|-----------------------|
| Power Meter NRP2 | 106277 | 24-Sep-21 (CTTL No.J21X06326) | Sep-22 |
| Power sensor NRP5S | 104291 | 24-Sep-21 (CTTL No.J21X06326) | Sep-22 |
| Reference Probe EX3DV4 | SN 7464 | 26-Jan-22(SPEAG.No EX3-7464_Jan22) | Jan-23 |
| DAE4 | SN 1556 | 12-Jan-22(CTTL-SPEAG.No Z22-60007) | Jan-23 |

| Secondary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration |
|-------------------------|------------|--|-----------------------|
| Signal Generator E4438C | MY49071430 | 13-Jan-22 (CTTL No.J22X00409) | Jan-23 |
| Network Analyzer E5071C | MY48110673 | 14-Jan-22 (CTTL No.J22X00406) | Jan-23 |

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Dianyuan SAR Project Leader

Issued: June 13, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60188 Page 1 of 6

In Collaboration with **TTL Speag** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62066317 E-mail: uttl@ttspeag.com http://www.caict.ac.cn

Glossary:

TSL: Issue simulating liquid
ConvF: sensitivity in TSL, INORMx,y,z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 865964, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60188 Page 2 of 6

In Collaboration with **TTL S p e a g** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-4239683-2117
 E-mail: ott@china.ttl.com http://www.caict.ac.cn

Measurement Conditions
 DASYS system configuration, as far as not given on page 1.

| | | |
|------------------------------|--------------------------|-------------|
| DASY Version | DASY52 | 52.10.4 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Triple Flat Phantom 5.1C | |
| Distance Dipole Center - TSL | 10 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 2000 MHz ± 1 MHz | |

Head TSL parameters
 The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|-----------------|--------------|------------------|
| Nominal Head TSL parameters | 22.0 °C | 40.0 | 1.40 mho/m |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 40.2 ± 8 % | 1.39 mho/m ± 8 % |
| Head TSL temperature change during test | <1.0 °C | --- | --- |

SAR result with Head TSL

| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
|---|--------------------|---------------------------------|
| SAR measured | 250 mW input power | 10.4 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 41.8 W/kg ± 18.8 % (k=2) |
| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 5.30 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 21.3 W/kg ± 18.7 % (k=2) |

Certificate No: Z22-60186 Page 3 of 6

In Collaboration with **TTL S p e a g** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-4239683-2117
 E-mail: ott@china.ttl.com http://www.caict.ac.cn

Appendix (Additional assessments outside the scope of CNAS L6570)

Antenna Parameters with Head TSL

| | |
|--------------------------------------|----------------|
| Impedance, transformed to feed point | 48.4Ω ± 0.74jΩ |
| Return Loss | -34.9dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.088 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

| | |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Certificate No: Z22-60186 Page 4 of 6

In Collaboration with **TTL S p e a g** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-4239683-2117
 E-mail: ott@china.ttl.com http://www.caict.ac.cn

DASY5 Validation Report for Head TSL Date: 2022-06-06

Test Laboratory: CTTL, Beijing, China
 DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2 - SN: 1041
 Communication System: LIID 0, CW; Frequency: 2000 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 2000$ MHz; $\sigma = 1.392$ S/m; $\epsilon_r = 40.21$; $\rho = 1000$ kg/m³
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(R,2, 8.2, 8.2) @ 2000 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA4E Sn1556; Calibrated: 2022-01-12
- Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY5: S2.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0; Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 103.4 V/m; Power Drift = 0.03 dB
 Peak SAR (extrapolated) = 19.6 W/kg
 SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg
 Smallest distance from peaks to all points 3 dB below = 9.1 mm
 Ratio of SAR at M2 to SAR at M1 = 53.6%
 Maximum value of SAR (measured) = 16.3 W/kg

Certificate No: Z22-60186 Page 5 of 6

In Collaboration with **TTL S p e a g** CALIBRATION LABORATORY **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
 Tel: +86-10-4239683-2117
 E-mail: ott@china.ttl.com http://www.caict.ac.cn

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60186 Page 6 of 6

1.9 D2300V2 - SN 1096

| <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p> | | <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p> | | | | | | | | | | | | | | | | | | | |
|---|--|---|-----------------------|--|----------------|--------------|---------------|----------------------------------|-----------|-------------------------------------|--------------------------|------------------------------|--|------------|------------------|---|--------------------|-----------|-------------------------------------|------------------|--------------------------|
| <p>Client: SGS-CN Certificate No: Z22-60106</p> | | | | | | | | | | | | | | | | | | | | | |
| <p>CALIBRATION CERTIFICATE</p> | | | | | | | | | | | | | | | | | | | | | |
| Object | D2300V2 - SN 1096 | | | | | | | | | | | | | | | | | | | | |
| Calibration Procedure(s) | FF-Z11-003-01 Calibration Procedures for dipole validation kits | | | | | | | | | | | | | | | | | | | | |
| Calibration date: | March 31, 2022 | | | | | | | | | | | | | | | | | | | | |
| <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.</p> <p>Calibration Equipment used (M&TE critical for calibration)</p> | | | | | | | | | | | | | | | | | | | | | |
| Primary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | |
| Power Meter NRP2 | 108277 | 24-Sep-21 (CTTL No.J21X08328) | Sep-22 | | | | | | | | | | | | | | | | | | |
| Power sensor NRP8S | 104291 | 24-Sep-21 (CTTL No.J21X08328) | Sep-22 | | | | | | | | | | | | | | | | | | |
| Reference Probe EX3DV4 DAE4 | SN 7307 SN 1556 | 26-May-21(SPEAG.No.EK3-7307_May21) 12-Jan-22(CTTL-SPEAG.No.Z22-60007) | May-22 Jan-23 | | | | | | | | | | | | | | | | | | |
| Secondary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | |
| Signal Generator E4438C | MY49071430 | 13-Jan-22 (CTTL No.J22X00406) | Jan-23 | | | | | | | | | | | | | | | | | | |
| Network Analyzer E5071C | MY48110673 | 14-Jan-22 (CTTL No.J22X00406) | Jan-23 | | | | | | | | | | | | | | | | | | |
| Calibrated by: | Name | Function | Signature | | | | | | | | | | | | | | | | | | |
| | Zhao Jing | SAR Test Engineer | | | | | | | | | | | | | | | | | | | |
| Reviewed by: | Lin Hao | SAR Test Engineer | | | | | | | | | | | | | | | | | | | |
| Approved by: | Qi Diaryuan | SAR Project Leader | | | | | | | | | | | | | | | | | | | |
| <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> | | | | | | | | | | | | | | | | | | | | | |
| Certificate No: Z22-60106 | | Page 1 of 6 | | | | | | | | | | | | | | | | | | | |
| <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p> | | <p>Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.chinatitl.cn</p> | | | | | | | | | | | | | | | | | | | |
| <p>Measurement Conditions DASY system configuration, as far as not given on page 1</p> <table border="1"> <tr> <td>DASY Version</td> <td>DASY52</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2300 MHz ± 1 MHz</td> <td></td> </tr> </table> | | | | DASY Version | DASY52 | 52.10.4 | Extrapolation | Advanced Extrapolation | | Phantom | Triple Flat Phantom 5.1C | | Distance Dipole Center - TSL | 10 mm | with Spacer | Zoom Scan Resolution | dx, dy, dz = 5 mm | | Frequency | 2300 MHz ± 1 MHz | |
| DASY Version | DASY52 | 52.10.4 | | | | | | | | | | | | | | | | | | | |
| Extrapolation | Advanced Extrapolation | | | | | | | | | | | | | | | | | | | | |
| Phantom | Triple Flat Phantom 5.1C | | | | | | | | | | | | | | | | | | | | |
| Distance Dipole Center - TSL | 10 mm | with Spacer | | | | | | | | | | | | | | | | | | | |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | | | | | | | | | | | | | | | | | | | | |
| Frequency | 2300 MHz ± 1 MHz | | | | | | | | | | | | | | | | | | | | |
| <p>Head TSL parameters The following parameters and calculations were applied:</p> <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.5</td> <td>1.67 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.8 ± 6 %</td> <td>1.70 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>—</td> <td>—</td> </tr> </tbody> </table> | | | | | Temperature | Permittivity | Conductivity | Nominal Head TSL parameters | 22.0 °C | 39.5 | 1.67 mho/m | Measured Head TSL parameters | (22.0 ± 0.2) °C | 39.8 ± 6 % | 1.70 mho/m ± 6 % | Head TSL temperature change during test | <1.0 °C | — | — | | |
| | Temperature | Permittivity | Conductivity | | | | | | | | | | | | | | | | | | |
| Nominal Head TSL parameters | 22.0 °C | 39.5 | 1.67 mho/m | | | | | | | | | | | | | | | | | | |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 39.8 ± 6 % | 1.70 mho/m ± 6 % | | | | | | | | | | | | | | | | | | |
| Head TSL temperature change during test | <1.0 °C | — | — | | | | | | | | | | | | | | | | | | |
| <p>SAR result with Head TSL</p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm³ (1g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>12.4 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>49.2 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <th>SAR averaged over 10 cm³ (10g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.88 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>23.4 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> | | | | SAR averaged over 1 cm ³ (1g) of Head TSL | Condition | | SAR measured | 250 mW input power | 12.4 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 49.2 W/kg ± 18.8 % (k=2) | SAR averaged over 10 cm ³ (10g) of Head TSL | Condition | | SAR measured | 250 mW input power | 5.88 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 23.4 W/kg ± 18.7 % (k=2) |
| SAR averaged over 1 cm ³ (1g) of Head TSL | Condition | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 250 mW input power | 12.4 W/kg | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 49.2 W/kg ± 18.8 % (k=2) | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 10 cm ³ (10g) of Head TSL | Condition | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 250 mW input power | 5.88 W/kg | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 23.4 W/kg ± 18.7 % (k=2) | | | | | | | | | | | | | | | | | | | |
| Certificate No: Z22-60106 | | Page 3 of 6 | | | | | | | | | | | | | | | | | | | |
| <p>Glossary:</p> <p>TSL: Issue simulating liquid ConvF: sensitivity in TSL / NORMx,y,z N/A: not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Additional Documentation: c) DASY4/5 System Handbook</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> | | | | | | | | | | | | | | | | | | | | | |
| Certificate No: Z22-60106 | | Page 2 of 6 | | | | | | | | | | | | | | | | | | | |
| <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>49.20 - 4.56jΩ</td> </tr> <tr> <td>Return Loss</td> <td>-26.66dB</td> </tr> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>1.083 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table> | | | | Impedance, transformed to feed point | 49.20 - 4.56jΩ | Return Loss | -26.66dB | Electrical Delay (one direction) | 1.083 ns | Manufactured by | SPEAG | | | | | | | | | | |
| Impedance, transformed to feed point | 49.20 - 4.56jΩ | | | | | | | | | | | | | | | | | | | | |
| Return Loss | -26.66dB | | | | | | | | | | | | | | | | | | | | |
| Electrical Delay (one direction) | 1.083 ns | | | | | | | | | | | | | | | | | | | | |
| Manufactured by | SPEAG | | | | | | | | | | | | | | | | | | | | |
| Certificate No: Z22-60106 | | Page 4 of 6 | | | | | | | | | | | | | | | | | | | |

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com http://www.chinatit.com

Date: 2022-03-31

DASY5 Validation Report for Head TSL

Test Laboratory: CTTL, Beijing, China
 DUT: Dipole 2300 MHz; Type: D2300V2; Serial: D2300V2 - SN: 1096
 Communication System: UTD 0, CW; Frequency: 2300 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 2300 \text{ MHz}$; $\sigma = 1.702 \text{ S/m}$; $\epsilon = 39.77$; $\rho = 1000 \text{ kg/m}^3$
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(8.01, 8.01) @ 2300 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sst1556; Calibrated: 2022-01-12
- Phantom: MFP V5.1C (2ldag probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 S2.10.4(1535); SEMCAD X 14.6;14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 102.7 V/m; Power Drift = 0.00 dB
 Peak SAR (extrapolated) = 21.8 W/kg
 SAR(1 g) = 12.4 W/kg; SAR(10 g) = 5.88 W/kg
 Smallest distance from peaks to all points 3 dB below = 9 mm
 Ratio of SAR at M2 to SAR at M1 = 50.4%
 Maximum value of SAR (measured) = 20.3 W/kg

$0 \text{ dB} = 20.3 \text{ W/kg} = 13.07 \text{ dBW/kg}$

Certificate No: Z22-60106 Page 1 of 6

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com http://www.chinatit.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60106 Page 4 of 6

1.10 D2450V2 - SN 817

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com http://www.chinatit.com

中国认可
国家互认
校准
CALIBRATION
CNAS 10578

Certificate No: Z22-60107

Client: **SGS-CN**

CALIBRATION CERTIFICATE

Object: D2450V2 - SN: 817
 Calibration Procedure(s): FF-Z11-003-01
 Calibration Procedures for dipole validation kits
 Calibration date: April 1, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Calibrated by: Certificate No.) | Scheduled Calibration |
|-------------------------|---------|---|-----------------------|
| Power Meter: NRP2 | 108277 | 24-Sep-21 (CTTL No.J21X08320) | Sep-22 |
| Power sensor: NRP8S | 104291 | 24-Sep-21 (CTTL No.J21X08320) | Sep-22 |
| Reference Probe: EX3DV4 | SN 7307 | 26-May-21(SPEAG.No.EX3-7307_May21) | May-22 |
| DAE4 | SN 1556 | 12-Jan-22(CTTL-SPEAG.No.Z22-60007) | Jan-23 |

| Secondary Standards | ID # | Cal Date (Calibrated by: Certificate No.) | Scheduled Calibration |
|--------------------------|------------|---|-----------------------|
| Signal Generator: E4438C | MY49071430 | 13-Jan-22 (CTTL No. J22X00406) | Jan-23 |
| Network Analyzer: E5071C | MY46110873 | 14-Jan-22 (CTTL No. J22X00406) | Jan-23 |

Calibrated by: Zhao Jing, SAR Test Engineer
 Reviewed by: Lin Hao, SAR Test Engineer
 Approved by: Qi Dianyuan, SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60107 Page 1 of 6

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504
E-mail: cti@china.ttl.com http://www.chinatit.com

Glossary:

TSL: tissue simulating liquid
 ConvF: sensitivity in TSL / NORMx.yz
 N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 855664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:







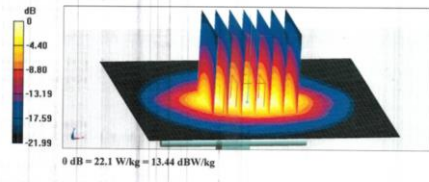



- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60107 Page 2 of 6
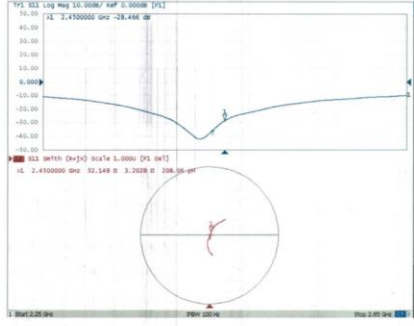
| <div style="display: flex; justify-content: space-between; align-items: center;">   </div> <p style="font-size: small;">In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p> <p>Measurement Conditions DASYS system configuration, as far as not given on page 1</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>DASYS Version</td> <td>DASYS2</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2450 MHz ± 1 MHz</td> <td></td> </tr> </table> <p>Head TSL parameters The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.2</td> <td>1.80 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>39.5 ± 6 %</td> <td>1.79 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><+1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p>SAR result with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>13.2 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>53.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <th>SAR averaged over 10 cm³ (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>6.15 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>24.7 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p style="font-size: x-small;">Certificate No: Z22-60107 Page 3 of 6</p> | DASYS Version | DASYS2 | 52.10.4 | Extrapolation | Advanced Extrapolation | | Phantom | Triple Flat Phantom 5.1C | | Distance Dipole Center - TSL | 10 mm | with Spacer | Zoom Scan Resolution | dx, dy, dz = 5 mm | | Frequency | 2450 MHz ± 1 MHz | | | Temperature | Permittivity | Conductivity | Nominal Head TSL parameters | 22.0 °C | 39.2 | 1.80 mho/m | Measured Head TSL parameters | (22.0 ± 0.2) °C | 39.5 ± 6 % | 1.79 mho/m ± 6 % | Head TSL temperature change during test | <+1.0 °C | --- | --- | SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | | SAR measured | 250 mW input power | 13.2 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 53.0 W/kg ± 18.8 % (k=2) | SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | | SAR measured | 250 mW input power | 6.15 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 24.7 W/kg ± 18.7 % (k=2) | <div style="display: flex; justify-content: space-between; align-items: center;">   </div> <p style="font-size: small;">In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Impedance, transformed to feed point</td> <td>52.10 ± 3.20jΩ</td> </tr> <tr> <td>Return Loss</td> <td>-28.5dB</td> </tr> </table> <p>General Antenna Parameters and Design</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Electrical Delay (one direction)</td> <td>1.066 ns</td> </tr> </table> <p style="font-size: x-small;">After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p style="font-size: x-small;">The dipole is made of standard serringrid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table> <p style="font-size: x-small;">Certificate No: Z22-60107 Page 4 of 6</p> | Impedance, transformed to feed point | 52.10 ± 3.20jΩ | Return Loss | -28.5dB | Electrical Delay (one direction) | 1.066 ns | Manufactured by | SPEAG |
|---|---|--------------------------|------------------|---------------|------------------------|--|---------|--------------------------|--|------------------------------|-------|-------------|----------------------|-------------------|--|-----------|------------------|--|--|-------------|--------------|--------------|-----------------------------|---------|------|------------|------------------------------|-----------------|------------|------------------|---|----------|-----|-----|---|-----------|--|--------------|--------------------|-----------|-------------------------------------|------------------|--------------------------|---|-----------|--|--------------|--------------------|-----------|-------------------------------------|------------------|--------------------------|--|--------------------------------------|----------------|-------------|---------|----------------------------------|----------|-----------------|-------|
| DASYS Version | DASYS2 | 52.10.4 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Extrapolation | Advanced Extrapolation | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Phantom | Triple Flat Phantom 5.1C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Distance Dipole Center - TSL | 10 mm | with Spacer | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Frequency | 2450 MHz ± 1 MHz | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | Temperature | Permittivity | Conductivity | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Nominal Head TSL parameters | 22.0 °C | 39.2 | 1.80 mho/m | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 39.5 ± 6 % | 1.79 mho/m ± 6 % | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Head TSL temperature change during test | <+1.0 °C | --- | --- | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 250 mW input power | 13.2 W/kg | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 53.0 W/kg ± 18.8 % (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 250 mW input power | 6.15 W/kg | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 24.7 W/kg ± 18.7 % (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Impedance, transformed to feed point | 52.10 ± 3.20jΩ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Return Loss | -28.5dB | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Electrical Delay (one direction) | 1.066 ns | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Manufactured by | SPEAG | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <div style="display: flex; justify-content: space-between; align-items: center;">   </div> <p style="font-size: small;">In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p> <p>DASYS Validation Report for Head TSL Date: 2022-04-01</p> <p>Test Laboratory: CTTL, Beijing, China DUT: Dipole 2450 MHz; Type: D2450V2 - SN: 817 Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz; σ = 1.79 S/m; ε = 39.52; ρ = 1000 kg/m³ Phantom section: Right Section Measurement Standard: DASYS (IEEE/IEC/ANSI C63.19-2007) DASYS Configuration:</p> <ul style="list-style-type: none"> • Probe: EX3DV4 - SN7307; ConvF(7.75, 7.75, 7.75) @ 2450 MHz; Calibrated: 2021-05-26 • Sensor-Surface: 1.4mm (Mechanical Surface Detection) • Electronics: DA14 Sn1556; Calibrated: 2022-01-12 • Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 • DASYS2 52.10.4(1535); SEMCAD X 14.6.14(7501) <p>Dipole Calibration Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 104.6 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 27.0 W/kg SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.15 W/kg Smallest distance from peaks to all points 3 dB below = 8.9 mm Ratio of SAR at M2 to SAR at M1 = -49.2% Maximum value of SAR (measured) = 22.1 W/kg</p>  <p style="font-size: x-small;">Certificate No: Z22-60107 Page 5 of 6</p> | <div style="display: flex; justify-content: space-between; align-items: center;">   </div> <p style="font-size: small;">In Collaboration with Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.china.ttl.com.cn</p> <p>Impedance Measurement Plot for Head TSL</p>  <p style="font-size: x-small;">Certificate No: Z22-60107 Page 6 of 6</p> | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

1.11 D2600V2 - SN 1158

| <div style="text-align: center;"> </div> <p style="font-size: small;"> Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.chinatitl.cn </p> <p> Client: SGS-CN Certificate No: Z22-60108 </p> <h3 style="text-align: center;">CALIBRATION CERTIFICATE</h3> <p> Object: D2600V2 - SN: 1158 </p> <p> Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits </p> <p> Calibration date: March 31, 2022 </p> <p> This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. </p> <p> All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%. </p> <p> Calibration Equipment used (M&TE critical for calibration) </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: x-small;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>102577</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8S</td> <td>104291</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21(SPEAG.No.EX3-7307_May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22(CTTL-SPEAG.No.Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse; font-size: x-small;"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E4438C</td> <td>MY49071430</td> <td>13-Jan-22 (CTTL No.Z22X00406)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY49110673</td> <td>14-Jan-22 (CTTL No.Z22X00406)</td> <td>Jan-23</td> </tr> </tbody> </table> <p> Calibrated by: Zhao Jing SAR Test Engineer </p> <p> Reviewed by: Lin Hao SAR Test Engineer </p> <p> Approved by: Qi Dianyuan SAR Project Leader </p> <p style="text-align: right;"> Issued: April 6, 2022 </p> <p style="font-size: x-small;"> This calibration certificate shall not be reproduced except in full without written approval of the laboratory. </p> <p style="font-size: x-small;"> Certificate No: Z22-60108 Page 1 of 6 </p> | Primary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration | Power Meter NRP2 | 102577 | 24-Sep-21 (CTTL No.J21X08326) | Sep-22 | Power sensor NRP8S | 104291 | 24-Sep-21 (CTTL No.J21X08326) | Sep-22 | Reference Probe EX3DV4 | SN 7307 | 26-May-21(SPEAG.No.EX3-7307_May21) | May-22 | DAE4 | SN 1556 | 12-Jan-22(CTTL-SPEAG.No.Z22-60007) | Jan-23 | Secondary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration | Signal Generator E4438C | MY49071430 | 13-Jan-22 (CTTL No.Z22X00406) | Jan-23 | Network Analyzer E5071C | MY49110673 | 14-Jan-22 (CTTL No.Z22X00406) | Jan-23 | <div style="text-align: center;"> </div> <p style="font-size: small;"> Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.chinatitl.cn </p> <p> Certificate No: Z22-60108 Page 2 of 6 </p> <p> Glossary: TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORMx.y.z N/A: not applicable or not measured </p> <p> Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz" </p> <p> Additional Documentation: c) DASY4/S System Handbook </p> <p> Methods Applied and Interpretation of Parameters: </p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <div style="border: 1px solid black; padding: 5px; font-size: x-small;"> The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%. </div> <p style="font-size: x-small;"> Certificate No: Z22-60108 Page 2 of 6 </p> | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
|---|--------------------------|--|--|-----------------------|------------------|---------|-------------------------------|------------------------|--------------------|---------|-------------------------------|--------|------------------------------|---------|------------------------------------|----------------------|-------------------|---------|------------------------------------|------------------|---------------------|-----------|--|-----------------------|-------------------------|-----------------------------|-------------------------------|--------|-------------------------|------------------------------|-------------------------------|------------|--|---|---------|-----|-----|---|-----------|-------|--------------|--------------------|-----------|-------------------------------------|------------------|--------------------------|---|-----------|-------|--------------|--------------------|-----------|-------------------------------------|------------------|--------------------------|---|-----------|-------|--------------------------------------|---------------|-------------|----------|-----------|-------|----------------------------------|----------|-----------|-------|-----------------|-------|
| Primary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power Meter NRP2 | 102577 | 24-Sep-21 (CTTL No.J21X08326) | Sep-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor NRP8S | 104291 | 24-Sep-21 (CTTL No.J21X08326) | Sep-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reference Probe EX3DV4 | SN 7307 | 26-May-21(SPEAG.No.EX3-7307_May21) | May-22 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| DAE4 | SN 1556 | 12-Jan-22(CTTL-SPEAG.No.Z22-60007) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Secondary Standards | ID # | Cal Date (Calibrated by Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Signal Generator E4438C | MY49071430 | 13-Jan-22 (CTTL No.Z22X00406) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Network Analyzer E5071C | MY49110673 | 14-Jan-22 (CTTL No.Z22X00406) | Jan-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <div style="text-align: center;"> </div> <p style="font-size: small;"> Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.chinatitl.cn </p> <p> Certificate No: Z22-60108 Page 3 of 6 </p> <p> Measurement Conditions DASY system configuration, as far as not given on page 1. </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: x-small;"> <thead> <tr> <th>Parameter</th> <th>Value</th> <th>Notes</th> </tr> </thead> <tbody> <tr> <td>DASY Version</td> <td>DASY52</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2600 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p> Head TSL parameters The following parameters and calculations were applied. </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: x-small;"> <thead> <tr> <th>Parameter</th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.0</td> <td>1.96 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>38.7 ± 6 %</td> <td>1.96 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p> SAR result with Head TSL </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: x-small;"> <thead> <tr> <th>SAR averaged over 1 cm² (1 g) of Head TSL</th> <th>Condition</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>13.7 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>54.8 W/kg ± 18.8 % (k=2)</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse; font-size: x-small;"> <thead> <tr> <th>SAR averaged over 10 cm² (10 g) of Head TSL</th> <th>Condition</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>6.12 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>24.6 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> | Parameter | Value | Notes | DASY Version | DASY52 | 52.10.4 | Extrapolation | Advanced Extrapolation | | Phantom | Triple Flat Phantom 5.1C | | Distance Dipole Center - TSL | 10 mm | with Spacer | Zoom Scan Resolution | dx, dy, dz = 5 mm | | Frequency | 2600 MHz ± 1 MHz | | Parameter | Temperature | Permittivity | Conductivity | Nominal Head TSL parameters | 22.0 °C | 39.0 | 1.96 mho/m | Measured Head TSL parameters | (22.0 ± 0.2) °C | 38.7 ± 6 % | 1.96 mho/m ± 6 % | Head TSL temperature change during test | <1.0 °C | --- | --- | SAR averaged over 1 cm² (1 g) of Head TSL | Condition | Value | SAR measured | 250 mW input power | 13.7 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 54.8 W/kg ± 18.8 % (k=2) | SAR averaged over 10 cm² (10 g) of Head TSL | Condition | Value | SAR measured | 250 mW input power | 6.12 W/kg | SAR for nominal Head TSL parameters | normalized to 1W | 24.6 W/kg ± 18.7 % (k=2) | <div style="text-align: center;"> </div> <p style="font-size: small;"> Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com.cn http://www.chinatitl.cn </p> <p> Certificate No: Z22-60108 Page 4 of 6 </p> <p> Appendix (Additional assessments outside the scope of CNAS L0570) </p> <p> Antenna Parameters with Head TSL </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: x-small;"> <thead> <tr> <th>Parameter</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>Impedance, transformed to feed point</td> <td>49.90- 6.49jΩ</td> </tr> <tr> <td>Return Loss</td> <td>- 23.8dB</td> </tr> </tbody> </table> <p> General Antenna Parameters and Design </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: x-small;"> <thead> <tr> <th>Parameter</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>Electrical Delay (one direction)</td> <td>1.053 ns</td> </tr> </tbody> </table> <p> After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. </p> <p> The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. </p> <p> Additional EUT Data </p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: x-small;"> <thead> <tr> <th>Parameter</th> <th>Value</th> </tr> </thead> <tbody> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </tbody> </table> | Parameter | Value | Impedance, transformed to feed point | 49.90- 6.49jΩ | Return Loss | - 23.8dB | Parameter | Value | Electrical Delay (one direction) | 1.053 ns | Parameter | Value | Manufactured by | SPEAG |
| Parameter | Value | Notes | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| DASY Version | DASY52 | 52.10.4 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Extrapolation | Advanced Extrapolation | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Phantom | Triple Flat Phantom 5.1C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Distance Dipole Center - TSL | 10 mm | with Spacer | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Frequency | 2600 MHz ± 1 MHz | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Parameter | Temperature | Permittivity | Conductivity | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Nominal Head TSL parameters | 22.0 °C | 39.0 | 1.96 mho/m | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 38.7 ± 6 % | 1.96 mho/m ± 6 % | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Head TSL temperature change during test | <1.0 °C | --- | --- | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 1 cm² (1 g) of Head TSL | Condition | Value | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 250 mW input power | 13.7 W/kg | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 54.8 W/kg ± 18.8 % (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR averaged over 10 cm² (10 g) of Head TSL | Condition | Value | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR measured | 250 mW input power | 6.12 W/kg | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| SAR for nominal Head TSL parameters | normalized to 1W | 24.6 W/kg ± 18.7 % (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Parameter | Value | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Impedance, transformed to feed point | 49.90- 6.49jΩ | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Return Loss | - 23.8dB | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Parameter | Value | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Electrical Delay (one direction) | 1.053 ns | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Parameter | Value | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Manufactured by | SPEAG | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-82304633-2079 Fax: +86-10-82304633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Date: 2022-03-31

DASY5 Validation Report for Head TSL
 Test Laboratory: CTTL, Beijing, China
 DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1158
 Communication System: UID 0, CW; Frequency: 2600 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 2600 \text{ MHz}$; $\sigma = 1.955 \text{ S/m}$; $\epsilon_r = 38.68$; $\rho = 1000 \text{ kg/m}^3$
 Phantom section: Right Section
 Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)
 DASY5 Configuration:

- Probe: EX3DV4 - SN7307; ConvF(7.5, 7.5, 7.5) @ 2600 MHz; Calibrated: 2021-05-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP_V5.1C (2dkg probe fill); Type: QD 000 P51 Cx; Serial: 1062
- DASY5 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 103.3 V/m; Power Drift = 0.04 dB
 Peak SAR (extrapolated) = 29.0 W/kg
 SAR(1 g) = 13.7 W/kg; SAR(10 g) = 6.12 W/kg
 Smallest distance from peaks to all points 3 dB below = 8.9 mm
 Ratio of SAR at M2 to SAR at M1 = 47.5%
 Maximum value of SAR (measured) = 23.4 W/kg

0 dB = 23.4 W/kg = 13.69 dBW/kg

Certificate No: Z22-60108 Page 5 of 6

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-82304633-2079 Fax: +86-10-82304633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60108 Page 6 of 6

1.12 D5GHZV2 - SN 1095

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-82304633-2079 Fax: +86-10-82304633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Certificate No: Z22-60187

CALIBRATION CERTIFICATE

Client: **SGS-CN**

Object: D5GHZV2 - SN: 1095

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: June 1, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Calibrated by: Certificate No.) | Scheduled Calibration |
|------------------------|---------|---|-----------------------|
| Power Meter NRP2 | 106277 | 24-Sep-21 (CTTL No.J21008326) | Sep-22 |
| Power sensor NRP8S | 104291 | 24-Sep-21 (CTTL No.J21008326) | Sep-22 |
| Reference Probe EX3DV4 | SN 7464 | 26-Jan-22(SPEAG No EX3-7464_Jan22) | Jan-23 |
| DAE4 | SN 1556 | 12-Jan-22(CTTL-SPEAG No.Z22-60007) | Jan-23 |

| Secondary Standards | ID # | Cal Date (Calibrated by: Certificate No.) | Scheduled Calibration |
|-------------------------|------------|---|-----------------------|
| Signal Generator E4438C | MY46071430 | 13-Jan-22 (CTTL No. J22X00406) | Jan-23 |
| Network Analyzer E5071C | MY46110673 | 14-Jan-22 (CTTL No. J22X00406) | Jan-23 |

Calibrated by: Zhao Jing, SAR Test Engineer

Reviewed by: Lin Hao, SAR Test Engineer

Approved by: Qi Dianyan, SAR Project Leader

Issued: June 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60187 Page 1 of 10

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-82304633-2079 Fax: +86-10-82304633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:

TSL: Issue simulating liquid
 ConvF: sensitivity in TSL / NORMx,y,z
 N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
- KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/G System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60187 Page 2 of 10

In Collaboration with
TTL
CALIBRATION LABORATORY

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62382117
E-mail: cti@ttsintl.com http://www.ttsintl.com

Measurement Conditions
DASY system configuration, as far as not given on page 1.

| | | |
|------------------------------|--|----------------------------------|
| DASY Version | DASY52 | 52.10.4 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Triple Flat Phantom 5.1C | |
| Distance Dipole Center - TSL | 10 mm | with Spacer |
| Zoom Scan Resolution | dx, dy = 4 mm, dz = 1.4 mm | Graded Ratio = 1.4 (Z direction) |
| Frequency | 5200 MHz ± 1 MHz 5200 MHz ± 1 MHz 5500 MHz ± 1 MHz 5800 MHz ± 1 MHz | |

Head TSL parameters at 5200MHz
The following parameters and calculations were applied.

| | | | |
|---|-----------------|--------------|------------------|
| Nominal Head TSL parameters | Temperature | Permittivity | Conductivity |
| | 22.0 °C | 35.0 | 4.66 mho/m |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 35.4 ± 6 % | 4.82 mho/m ± 6 % |
| Head TSL temperature change during test | <1.0 °C | --- | --- |

SAR result with Head TSL at 5200MHz

| | | |
|---|--------------------|--------------------------|
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 7.79 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 17.6 W/kg ± 24.4 % (k=2) |
| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
| SAR measured | 250 mW input power | 2.22 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 22.1 W/kg ± 24.2 % (k=2) |

Certificate No: Z22-60187 Page 3 of 10

In Collaboration with
TTL
CALIBRATION LABORATORY

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62382117
E-mail: cti@ttsintl.com http://www.ttsintl.com

Head TSL parameters at 5300MHz
The following parameters and calculations were applied.

| | | | |
|---|-----------------|--------------|------------------|
| Nominal Head TSL parameters | Temperature | Permittivity | Conductivity |
| | 22.0 °C | 35.9 | 4.76 mho/m |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 35.2 ± 6 % | 4.73 mho/m ± 6 % |
| Head TSL temperature change during test | <1.0 °C | --- | --- |

SAR result with Head TSL at 5300MHz

| | | |
|---|--------------------|--------------------------|
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
| SAR measured | 100 mW input power | 7.94 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 79.1 W/kg ± 24.4 % (k=2) |
| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
| SAR measured | 100 mW input power | 2.27 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 22.6 W/kg ± 24.2 % (k=2) |

Head TSL parameters at 5500MHz
The following parameters and calculations were applied.

| | | | |
|---|-----------------|--------------|------------------|
| Nominal Head TSL parameters | Temperature | Permittivity | Conductivity |
| | 22.0 °C | 35.6 | 4.96 mho/m |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 34.8 ± 6 % | 4.94 mho/m ± 6 % |
| Head TSL temperature change during test | <1.0 °C | --- | --- |

SAR result with Head TSL at 5500MHz

| | | |
|---|--------------------|--------------------------|
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
| SAR measured | 100 mW input power | 8.29 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 82.6 W/kg ± 24.4 % (k=2) |
| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
| SAR measured | 100 mW input power | 2.34 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 23.3 W/kg ± 24.2 % (k=2) |

Certificate No: Z22-60187 Page 4 of 10

In Collaboration with
TTL
CALIBRATION LABORATORY

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62382117
E-mail: cti@ttsintl.com http://www.ttsintl.com

Head TSL parameters at 5600MHz
The following parameters and calculations were applied.

| | | | |
|---|-----------------|--------------|------------------|
| Nominal Head TSL parameters | Temperature | Permittivity | Conductivity |
| | 22.0 °C | 35.5 | 5.07 mho/m |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 34.7 ± 6 % | 5.05 mho/m ± 6 % |
| Head TSL temperature change during test | <1.0 °C | --- | --- |

SAR result with Head TSL at 5600MHz

| | | |
|---|--------------------|--------------------------|
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
| SAR measured | 100 mW input power | 8.12 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 80.8 W/kg ± 24.4 % (k=2) |
| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
| SAR measured | 100 mW input power | 2.30 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 22.9 W/kg ± 24.2 % (k=2) |

Head TSL parameters at 5800MHz
The following parameters and calculations were applied.

| | | | |
|---|-----------------|--------------|------------------|
| Nominal Head TSL parameters | Temperature | Permittivity | Conductivity |
| | 22.0 °C | 35.3 | 5.27 mho/m |
| Measured Head TSL parameters | (22.0 ± 0.2) °C | 34.4 ± 6 % | 5.25 mho/m ± 6 % |
| Head TSL temperature change during test | <1.0 °C | --- | --- |

SAR result with Head TSL at 5800MHz

| | | |
|---|--------------------|--------------------------|
| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
| SAR measured | 100 mW input power | 7.71 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 76.7 W/kg ± 24.4 % (k=2) |
| SAR averaged over 10 cm ³ (10 g) of Head TSL | Condition | |
| SAR measured | 100 mW input power | 2.16 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 21.8 W/kg ± 24.2 % (k=2) |

Certificate No: Z22-60187 Page 5 of 10

In Collaboration with
TTL
CALIBRATION LABORATORY

Address: No. 52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62382117
E-mail: cti@ttsintl.com http://www.ttsintl.com

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL at 5200MHz

| | |
|--------------------------------------|--------------|
| Impedance, transformed to feed point | 46.10-5.03jΩ |
| Return Loss | -23.6dB |

Antenna Parameters with Head TSL at 5300MHz

| | |
|--------------------------------------|--------------|
| Impedance, transformed to feed point | 47.80-2.42jΩ |
| Return Loss | -28.5dB |

Antenna Parameters with Head TSL at 5500MHz

| | |
|--------------------------------------|--------------|
| Impedance, transformed to feed point | 50.30-4.26jΩ |
| Return Loss | -27.4dB |

Antenna Parameters with Head TSL at 5600MHz

| | |
|--------------------------------------|--------------|
| Impedance, transformed to feed point | 54.50-4.80jΩ |
| Return Loss | -24.0dB |

Antenna Parameters with Head TSL at 5800MHz

| | |
|--------------------------------------|--------------|
| Impedance, transformed to feed point | 51.50-5.61jΩ |
| Return Loss | -24.9dB |

Certificate No: Z22-60187 Page 6 of 10

In Collaboration with
T T L
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62302117
E-mail: ott@ttsintl.com <http://www.ttsintl.com>

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.101 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

| | |
|-----------------|-------|
| Manufactured by | SPEAG |
|-----------------|-------|

Certificate No: Z22-60187 Page 7 of 10

In Collaboration with
T T L
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62302117
E-mail: ott@ttsintl.com <http://www.ttsintl.com>

DASY5 Validation Report for Head TSL Date: 2022-06-01

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1095

Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 5200$ MHz; $\sigma = 4.62$ S/m; $\epsilon_r = 35.39$; $\rho = 1000$ kg/m³

Medium parameters used: $f = 5300$ MHz; $\sigma = 4.73$ S/m; $\epsilon_r = 35.19$; $\rho = 1000$ kg/m³

Medium parameters used: $f = 5500$ MHz; $\sigma = 4.939$ S/m; $\epsilon_r = 34.83$; $\rho = 1000$ kg/m³

Medium parameters used: $f = 5600$ MHz; $\sigma = 5.051$ S/m; $\epsilon_r = 34.69$; $\rho = 1000$ kg/m³

Medium parameters used: $f = 5800$ MHz; $\sigma = 5.247$ S/m; $\epsilon_r = 34.42$; $\rho = 1000$ kg/m³

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN7484; ConvF(5.6, 5.6, 5.6) @ 5200 MHz; ConvF(5.32, 5.32, 5.32) @ 5300 MHz; ConvF(5.11, 5.11, 5.11) @ 5500 MHz; ConvF(4.91, 4.91, 4.91) @ 5600 MHz; ConvF(5, 5, 5) @ 5800 MHz; Calibrated: 2022-01-26
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA4 Sn1556; Calibrated: 2022-01-12
- Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 60.80 V/m; Power Drift = -0.06 dB
Peak SAR (extrapolated) = 29.8 W/kg
SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.22 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 66.8%
Maximum value of SAR (measured) = 18.3 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 61.08 V/m; Power Drift = -0.07 dB
Peak SAR (extrapolated) = 31.5 W/kg
SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 65.5%
Maximum value of SAR (measured) = 19.0 W/kg

Certificate No: Z22-60187 Page 8 of 10

In Collaboration with
T T L
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62302117
E-mail: ott@ttsintl.com <http://www.ttsintl.com>

Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 61.92 V/m; Power Drift = -0.08 dB
Peak SAR (extrapolated) = 34.7 W/kg
SAR(1 g) = 8.29 W/kg; SAR(10 g) = 2.34 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 63.9%
Maximum value of SAR (measured) = 20.2 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 65.08 V/m; Power Drift = -0.07 dB
Peak SAR (extrapolated) = 35.2 W/kg
SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.3 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 62.5%
Maximum value of SAR (measured) = 19.1 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 62.13 V/m; Power Drift = -0.06 dB
Peak SAR (extrapolated) = 34.8 W/kg
SAR(1 g) = 7.71 W/kg; SAR(10 g) = 2.16 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 61.6%
Maximum value of SAR (measured) = 18.7 W/kg

0 dB = 18.7 W/kg = 12.72 dBW/kg

Certificate No: Z22-60187 Page 9 of 10

In Collaboration with
T T L
CALIBRATION LABORATORY

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62302117
E-mail: ott@ttsintl.com <http://www.ttsintl.com>

Impedance Measurement Plot for Head TSL

Certificate No: Z22-60187 Page 10 of 10

2 DAE4 - SN 1305

| <div style="display: flex; justify-content: space-between; align-items: flex-start;"> <div style="width: 45%;"> <p>Calibration Laboratory of Schmid & Partner Engineering AG Zugwegstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: Auden Tessens City, Taiwan</p> </div> <div style="width: 45%; text-align: right;"> <p>Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service</p> <p>Accreditation No.: SCS 0108</p> <p>Certificate No.: DAE4-1305_Apr23</p> </div> </div> <div style="border: 1px solid black; padding: 5px; margin-top: 10px;"> <p align="center">CALIBRATION CERTIFICATE</p> <p>Object: DAE4 - SD 000 D04 BM - SN: 1305</p> <p>Calibration procedure(s): QA CAL-06.v30 Calibration procedure for the data acquisition electronics (DAE)</p> <p>Calibration date: April 13, 2023</p> <p><small>This calibration certificate documents the traceability to national standards, which reduces the physical units of measurements (SI). The measurements and the uncertainties with confidence probability as given on the following pages are part of the certificate.</small></p> <p><small>All calibrations have been conducted in the closest laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.</small></p> <p><small>Calibration Equipment used (MATE critical for calibration)</small></p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Kettley Multimeter Type 2001</td> <td>SN: 0810278</td> <td>29-Aug-22 (No:3438)</td> <td>Aug-23</td> </tr> <tr> <td>Secondary Standards</td> <th>ID #</th> <th>Check Date (In house)</th> <th>Scheduled Check</th> </tr> <tr> <td>Auto DAE Calibration Unit</td> <td>SE UMS 003 AA 1002</td> <td>27-Jan-23 (in house check)</td> <td>In house check: Jan-24</td> </tr> <tr> <td>Calibrator Box V0.1</td> <td>SE UMS 006 AA 1002</td> <td>27-Jan-23 (in house check)</td> <td>In house check: Jan-24</td> </tr> </tbody> </table> <div style="display: flex; justify-content: space-between; margin-top: 10px;"> <div style="width: 45%;"> <p>Calibrated by: Adrian Gehring, Laboratory Technician</p> <p>Approved by: Sven Kälin, Technical Manager</p> </div> <div style="width: 45%; text-align: right;"> </div> </div> <p align="right"><small>Issued: April 13, 2023</small></p> <p><small>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</small></p> </div> | Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration | Kettley Multimeter Type 2001 | SN: 0810278 | 29-Aug-22 (No:3438) | Aug-23 | Secondary Standards | ID # | Check Date (In house) | Scheduled Check | Auto DAE Calibration Unit | SE UMS 003 AA 1002 | 27-Jan-23 (in house check) | In house check: Jan-24 | Calibrator Box V0.1 | SE UMS 006 AA 1002 | 27-Jan-23 (in house check) | In house check: Jan-24 | <div style="display: flex; justify-content: space-between; align-items: flex-start;"> <div style="width: 45%;"> <p>Calibration Laboratory of Schmid & Partner Engineering AG Zugwegstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> </div> <div style="width: 45%; text-align: right;"> <p>Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service</p> <p>Accreditation No.: SCS 0108</p> </div> </div> <p>Glossary</p> <p>DAE: data acquisition electronics Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system.</p> <p>Methods Applied and Interpretation of Parameters</p> <ul style="list-style-type: none"> • DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range. • Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required. • The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty. • DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement. • Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement. • Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage. • AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage. • Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements. • Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance. • Input resistance: Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement. • Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated. • Power consumption: Typical value for information. Supply currents in various operating modes. | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
|--|---|---------------------------------|--------------------------------|-----------------------|------------------------------|-----------------------|-----------------------|-----------------------|---------------------|-----------------------|-----------------------|-----------------------|---|--------------------|---|------------------------|---------------------|--------------------|----------------------------|------------------------|---|------|------|-------------------|----------|------|------|-------------------|-----------|------|-------|-------------------|-----------|-------|-------|-------------------|----------|-------|-------|-------------------|-----------|-------|------|-------------------|-----------|------|------|-------------------|----------|-------|-------|-------------------|-----------|-------|------|-----------|--------------|-----------------|-----------|-------------------|---------|------|------|-------------------|--------|------|------|-------------------|---------|------|-------|-------------------|---------|-------|-------|-------------------|--------|-------|-------|-------------------|---------|-------|------|-------------------|---------|-------|-------|-------------------|--------|------|------|-------------------|---------|-------|------|--|--------------------------------|---------------------------------|--------------------------------|-----------|-----|------|------|--|------|-------|-------|-----------|-----|--------|--------|--|------|-------|-------|-----------|-----|-------|-------|--|------|------|------|--|--------------------|----------------|----------------|----------------|-----------|-----|---|------|-------|-----------|-----|------|---|------|-----------|-----|-------|------|---|
| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Kettley Multimeter Type 2001 | SN: 0810278 | 29-Aug-22 (No:3438) | Aug-23 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Secondary Standards | ID # | Check Date (In house) | Scheduled Check | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Auto DAE Calibration Unit | SE UMS 003 AA 1002 | 27-Jan-23 (in house check) | In house check: Jan-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Calibrator Box V0.1 | SE UMS 006 AA 1002 | 27-Jan-23 (in house check) | In house check: Jan-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <p>Certificate No: DAE4-1305_Apr23 Page 1 of 5</p> | <p>Certificate No: DAE4-1305_Apr23 Page 2 of 5</p> | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <p>DC Voltage Measurement</p> <p><small>AD Converter Resolution nominal</small></p> <p>High Range: 1LSB = 6.1µV, full range = -100...+300 mV Low Range: 1LSB = 61mV, full range = -1...+3mV</p> <p><small>DASY measurement parameters: Auto Zero: Time: 3 sec; Measuring time: 3 sec</small></p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>Calibration Factors</th> <th>X</th> <th>Y</th> <th>Z</th> </tr> </thead> <tbody> <tr> <td>High Range</td> <td>403.819 ± 0.02% (k=2)</td> <td>403.983 ± 0.02% (k=2)</td> <td>404.309 ± 0.02% (k=2)</td> </tr> <tr> <td>Low Range</td> <td>3.98113 ± 1.50% (k=2)</td> <td>3.99190 ± 1.50% (k=2)</td> <td>3.99636 ± 1.50% (k=2)</td> </tr> </tbody> </table> <p>Connector Angle</p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <tr> <td>Connector Angle to be used in DASY system</td> <td>97.5° ± 1°</td> </tr> </table> | Calibration Factors | X | Y | Z | High Range | 403.819 ± 0.02% (k=2) | 403.983 ± 0.02% (k=2) | 404.309 ± 0.02% (k=2) | Low Range | 3.98113 ± 1.50% (k=2) | 3.99190 ± 1.50% (k=2) | 3.99636 ± 1.50% (k=2) | Connector Angle to be used in DASY system | 97.5° ± 1° | <p>Appendix (Additional assessments outside the scope of SCS0108)</p> <p>1. DC Voltage Linearity</p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>High Range</th> <th>Reading (µV)</th> <th>Difference (µV)</th> <th>Error (%)</th> </tr> </thead> <tbody> <tr><td>Channel X + Input</td><td>199995.15</td><td>1.24</td><td>0.00</td></tr> <tr><td>Channel X + Input</td><td>20002.16</td><td>0.20</td><td>0.00</td></tr> <tr><td>Channel X - Input</td><td>-19999.30</td><td>2.54</td><td>-0.01</td></tr> <tr><td>Channel Y + Input</td><td>199993.50</td><td>-0.43</td><td>-0.00</td></tr> <tr><td>Channel Y + Input</td><td>19999.85</td><td>-1.57</td><td>-0.01</td></tr> <tr><td>Channel Y - Input</td><td>-20002.21</td><td>-0.38</td><td>0.00</td></tr> <tr><td>Channel Z + Input</td><td>199995.45</td><td>1.29</td><td>0.00</td></tr> <tr><td>Channel Z + Input</td><td>20000.56</td><td>-1.24</td><td>-0.01</td></tr> <tr><td>Channel Z - Input</td><td>-20002.62</td><td>-0.64</td><td>0.00</td></tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th>Low Range</th> <th>Reading (µV)</th> <th>Difference (µV)</th> <th>Error (%)</th> </tr> </thead> <tbody> <tr><td>Channel X + Input</td><td>2001.11</td><td>0.15</td><td>0.01</td></tr> <tr><td>Channel X + Input</td><td>201.71</td><td>0.58</td><td>0.29</td></tr> <tr><td>Channel X - Input</td><td>-197.58</td><td>1.01</td><td>-0.51</td></tr> <tr><td>Channel Y + Input</td><td>1999.61</td><td>-1.08</td><td>-0.05</td></tr> <tr><td>Channel Y + Input</td><td>200.62</td><td>-0.55</td><td>-0.27</td></tr> <tr><td>Channel Y - Input</td><td>-199.48</td><td>-0.65</td><td>0.43</td></tr> <tr><td>Channel Z + Input</td><td>2000.44</td><td>-0.39</td><td>-0.02</td></tr> <tr><td>Channel Z + Input</td><td>201.23</td><td>0.18</td><td>0.08</td></tr> <tr><td>Channel Z - Input</td><td>-199.50</td><td>-0.73</td><td>0.37</td></tr> </tbody> </table> <p>2. Common mode sensitivity</p> <p><small>DASY measurement parameters: Auto Zero: Time: 3 sec; Measuring time: 3 sec</small></p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th></th> <th>Common mode Input Voltage (mV)</th> <th>High Range Average Reading (µV)</th> <th>Low Range Average Reading (µV)</th> </tr> </thead> <tbody> <tr><td>Channel X</td><td>200</td><td>7.78</td><td>6.27</td></tr> <tr><td></td><td>-200</td><td>-4.59</td><td>-6.96</td></tr> <tr><td>Channel Y</td><td>200</td><td>-22.45</td><td>-23.58</td></tr> <tr><td></td><td>-200</td><td>22.23</td><td>21.98</td></tr> <tr><td>Channel Z</td><td>200</td><td>-8.70</td><td>-8.29</td></tr> <tr><td></td><td>-200</td><td>8.76</td><td>8.65</td></tr> </tbody> </table> <p>3. Channel separation</p> <p><small>DASY measurement parameters: Auto Zero: Time: 3 sec; Measuring time: 3 sec</small></p> <table border="1" style="width: 100%; border-collapse: collapse; font-size: 8px;"> <thead> <tr> <th></th> <th>Input Voltage (mV)</th> <th>Channel X (µV)</th> <th>Channel Y (µV)</th> <th>Channel Z (µV)</th> </tr> </thead> <tbody> <tr><td>Channel X</td><td>200</td><td>-</td><td>0.51</td><td>-3.80</td></tr> <tr><td>Channel Y</td><td>200</td><td>8.86</td><td>-</td><td>2.36</td></tr> <tr><td>Channel Z</td><td>200</td><td>10.72</td><td>5.98</td><td>-</td></tr> </tbody> </table> | High Range | Reading (µV) | Difference (µV) | Error (%) | Channel X + Input | 199995.15 | 1.24 | 0.00 | Channel X + Input | 20002.16 | 0.20 | 0.00 | Channel X - Input | -19999.30 | 2.54 | -0.01 | Channel Y + Input | 199993.50 | -0.43 | -0.00 | Channel Y + Input | 19999.85 | -1.57 | -0.01 | Channel Y - Input | -20002.21 | -0.38 | 0.00 | Channel Z + Input | 199995.45 | 1.29 | 0.00 | Channel Z + Input | 20000.56 | -1.24 | -0.01 | Channel Z - Input | -20002.62 | -0.64 | 0.00 | Low Range | Reading (µV) | Difference (µV) | Error (%) | Channel X + Input | 2001.11 | 0.15 | 0.01 | Channel X + Input | 201.71 | 0.58 | 0.29 | Channel X - Input | -197.58 | 1.01 | -0.51 | Channel Y + Input | 1999.61 | -1.08 | -0.05 | Channel Y + Input | 200.62 | -0.55 | -0.27 | Channel Y - Input | -199.48 | -0.65 | 0.43 | Channel Z + Input | 2000.44 | -0.39 | -0.02 | Channel Z + Input | 201.23 | 0.18 | 0.08 | Channel Z - Input | -199.50 | -0.73 | 0.37 | | Common mode Input Voltage (mV) | High Range Average Reading (µV) | Low Range Average Reading (µV) | Channel X | 200 | 7.78 | 6.27 | | -200 | -4.59 | -6.96 | Channel Y | 200 | -22.45 | -23.58 | | -200 | 22.23 | 21.98 | Channel Z | 200 | -8.70 | -8.29 | | -200 | 8.76 | 8.65 | | Input Voltage (mV) | Channel X (µV) | Channel Y (µV) | Channel Z (µV) | Channel X | 200 | - | 0.51 | -3.80 | Channel Y | 200 | 8.86 | - | 2.36 | Channel Z | 200 | 10.72 | 5.98 | - |
| Calibration Factors | X | Y | Z | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| High Range | 403.819 ± 0.02% (k=2) | 403.983 ± 0.02% (k=2) | 404.309 ± 0.02% (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Low Range | 3.98113 ± 1.50% (k=2) | 3.99190 ± 1.50% (k=2) | 3.99636 ± 1.50% (k=2) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Connector Angle to be used in DASY system | 97.5° ± 1° | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| High Range | Reading (µV) | Difference (µV) | Error (%) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel X + Input | 199995.15 | 1.24 | 0.00 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel X + Input | 20002.16 | 0.20 | 0.00 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel X - Input | -19999.30 | 2.54 | -0.01 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Y + Input | 199993.50 | -0.43 | -0.00 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Y + Input | 19999.85 | -1.57 | -0.01 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Y - Input | -20002.21 | -0.38 | 0.00 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Z + Input | 199995.45 | 1.29 | 0.00 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Z + Input | 20000.56 | -1.24 | -0.01 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Z - Input | -20002.62 | -0.64 | 0.00 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Low Range | Reading (µV) | Difference (µV) | Error (%) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel X + Input | 2001.11 | 0.15 | 0.01 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel X + Input | 201.71 | 0.58 | 0.29 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel X - Input | -197.58 | 1.01 | -0.51 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Y + Input | 1999.61 | -1.08 | -0.05 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Y + Input | 200.62 | -0.55 | -0.27 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Y - Input | -199.48 | -0.65 | 0.43 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Z + Input | 2000.44 | -0.39 | -0.02 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Z + Input | 201.23 | 0.18 | 0.08 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Z - Input | -199.50 | -0.73 | 0.37 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | Common mode Input Voltage (mV) | High Range Average Reading (µV) | Low Range Average Reading (µV) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel X | 200 | 7.78 | 6.27 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | -200 | -4.59 | -6.96 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Y | 200 | -22.45 | -23.58 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | -200 | 22.23 | 21.98 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Z | 200 | -8.70 | -8.29 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | -200 | 8.76 | 8.65 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| | Input Voltage (mV) | Channel X (µV) | Channel Y (µV) | Channel Z (µV) | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel X | 200 | - | 0.51 | -3.80 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Y | 200 | 8.86 | - | 2.36 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Channel Z | 200 | 10.72 | 5.98 | - | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| <p>Certificate No: DAE4-1305_Apr23 Page 3 of 5</p> | <p>Certificate No: DAE4-1305_Apr23 Page 4 of 5</p> | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

4. AD-Converter Values with inputs shorted
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 15876 | 18114 |
| Channel Y | 18301 | 17045 |
| Channel Z | 15957 | 13958 |

5. Input Offset Measurement
DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec; Input: 10mV

| | Average (µV) | min. Offset (µV) | max. Offset (µV) | Std. Deviation (µV) |
|-----------|--------------|------------------|------------------|---------------------|
| Channel X | 1.73 | 0.47 | 2.81 | 0.44 |
| Channel Y | -0.21 | -2.38 | 1.70 | 0.54 |
| Channel Z | 0.13 | -1.38 | 1.54 | 0.59 |

6. Input Offset Current
Nominal input circuitry offset current on all channels: <25nA

7. Input Resistance (Typical values for information)

| | Zeroing (kOhm) | Measuring (MOhm) |
|-----------|----------------|------------------|
| Channel X | 200 | 200 |
| Channel Y | 200 | 200 |
| Channel Z | 200 | 200 |

8. Low Battery Alarm Voltage (Typical values for information)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.8 |
| Supply (- Vcc) | -7.8 |

9. Power Consumption (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.01 | +8 | +14 |
| Supply (- Vcc) | -0.01 | -8 | -9 |

Certificate No: DAE4-1005_Apr23 Page 5 of 5

3 EX3DV4 - SN 7767

| <p>Calibration Laboratory of Schmid & Partner Engineering AG Zieglerstrasse 43, 8104 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS). The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: SGS (Kunshan) Certificate No: EX-7767_Oct23</p> <p>CALIBRATION CERTIFICATE</p> <p>Object: EX3DV4 - SN.7767</p> <p>Calibration procedure(s): QA CAL-01 v10, QA CAL-12 v10, QA CAL-14 v7, QA CAL-23 v6, QA CAL-25 v6 Calibration procedure for dosimetric E-field probes</p> <p>Calibration date: October 26, 2023</p> <p><small>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3°C and humidity < 70%. Calibration Equipment used (MATE critical for calibration)</small></p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID</th> <th>Cal Date (Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP2</td> <td>SN: 104778</td> <td>30-Mar-23 (No. 217-03854/03605)</td> <td>Mar-24</td> </tr> <tr> <td>Power sensor NRP231</td> <td>SN: 103244</td> <td>28-Mar-23 (No. 217-03854)</td> <td>Mar-24</td> </tr> <tr> <td>DOF DAK-3.3 (high/low)</td> <td>SN: 1248</td> <td>05-Oct-23 (DOF-DAK3-1-1949_Oct23)</td> <td>Oct-24</td> </tr> <tr> <td>DOF DAK-12</td> <td>SN: 1018</td> <td>05-Oct-23 (DOF-DAK12-1016_Oct23)</td> <td>Oct-24</td> </tr> <tr> <td>Reference 30 dB Attenuator</td> <td>SN: C25932 (20v)</td> <td>30-Mar-23 (No. 217-03854)</td> <td>Mar-24</td> </tr> <tr> <td>EMF</td> <td>SN: 680</td> <td>16-Mar-23 (No. SAE4-490_Mar23)</td> <td>Mar-24</td> </tr> <tr> <td>Reference Probe E520V2</td> <td>SN: 3013</td> <td>05-Jan-23 (No. E52-3013_Jan23)</td> <td>Jan-24</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power meter E4119</td> <td>SN: 084126874</td> <td>06-Apr-18 (in house check Jun-20)</td> <td>in house check Jun-24</td> </tr> <tr> <td>Power sensor E4112A</td> <td>SN: 084126897</td> <td>06-Apr-18 (in house check Jun-20)</td> <td>in house check Jun-24</td> </tr> <tr> <td>Power sensor E4112A</td> <td>SN: 080112810</td> <td>06-Apr-18 (in house check Jun-20)</td> <td>in house check Jun-24</td> </tr> <tr> <td>RF generator HP 8445C</td> <td>SN: 03846591700</td> <td>04-Apr-18 (in house check Jun-20)</td> <td>in house check Jun-24</td> </tr> <tr> <td>Network Analyzer E8368A</td> <td>SN: U84188477</td> <td>31-Mar-14 (in house check Oct-22)</td> <td>in house check Oct-24</td> </tr> </tbody> </table> <p>Calibrated by: Joanna Lischka (Laboratory Technician) Signature: <i>[Signature]</i></p> <p>Approved by: Sven Kuhn (Technical Manager)</p> <p><small>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</small></p> <p>Certificate No: EX-7767_Oct23 Page 1 of 9</p> | Primary Standards | ID | Cal Date (Certificate No.) | Scheduled Calibration | Power meter NRP2 | SN: 104778 | 30-Mar-23 (No. 217-03854/03605) | Mar-24 | Power sensor NRP231 | SN: 103244 | 28-Mar-23 (No. 217-03854) | Mar-24 | DOF DAK-3.3 (high/low) | SN: 1248 | 05-Oct-23 (DOF-DAK3-1-1949_Oct23) | Oct-24 | DOF DAK-12 | SN: 1018 | 05-Oct-23 (DOF-DAK12-1016_Oct23) | Oct-24 | Reference 30 dB Attenuator | SN: C25932 (20v) | 30-Mar-23 (No. 217-03854) | Mar-24 | EMF | SN: 680 | 16-Mar-23 (No. SAE4-490_Mar23) | Mar-24 | Reference Probe E520V2 | SN: 3013 | 05-Jan-23 (No. E52-3013_Jan23) | Jan-24 | Secondary Standards | ID | Check Date (in house) | Scheduled Check | Power meter E4119 | SN: 084126874 | 06-Apr-18 (in house check Jun-20) | in house check Jun-24 | Power sensor E4112A | SN: 084126897 | 06-Apr-18 (in house check Jun-20) | in house check Jun-24 | Power sensor E4112A | SN: 080112810 | 06-Apr-18 (in house check Jun-20) | in house check Jun-24 | RF generator HP 8445C | SN: 03846591700 | 04-Apr-18 (in house check Jun-20) | in house check Jun-24 | Network Analyzer E8368A | SN: U84188477 | 31-Mar-14 (in house check Oct-22) | in house check Oct-24 | <p>Calibration Laboratory of Schmid & Partner Engineering AG Zieglerstrasse 43, 8104 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS). The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Accreditation No: SCS 0108</p> <p>Glossary</p> <p>TSL: tissue simulating liquid NORM_{x,y,z}: sensitivity in free space ConF: sensitivity in TSL / NORM_{x,y,z} DCP: disc compression point CF: crest factor (1.414₂ cycle) of the RF signal A, B, C, D: modulation dependent linearization parameters Polarization ψ: ψ rotation around probe axis Polarization θ: θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis Connector Angle: information used in DASY system to align probe sensor X to the robot coordinate system</p> <p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1:2018, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1:2018: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020. b) K08.865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> NORM_{x,y,z}: Assessed for E-field polarization $\theta = 0$ ($f \leq 900$ MHz in TEM-cell, $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E-field uncertainty inside TSL (see below ConF). NORM_{x,y,z} + NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConF. DOF_{x,y,z}: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency nor media. RAZ: RAZ is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics. A_{xx,y,z}, B_{xx,y,z}, C_{xx,y,z}, D_{xx,y,z}, VR_{xx,y,z}: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration error expressed in RMS voltage across the disc. ConF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f < 900$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 900$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, beta) of which input boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConF, whereby the uncertainty corresponds to the given ConF. A frequency dependent ConF is used in DASY version 4.4 and higher which allows extending the validity from ≤ 500 MHz to ≤ 1500 MHz. Spherical isotropy (2D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna. Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No isotropy required. Connector Angle: The angle is assessed using the information gained by determining the NORMs (no uncertainty required). <p>Certificate No: EX-7767_Oct23 Page 2 of 9</p> |
|--|-------------------|-----------------------------------|----------------------------|-----------------------|------------------|------------|---------------------------------|--------|---------------------|------------|---------------------------|--------|------------------------|----------|-----------------------------------|--------|------------|----------|----------------------------------|--------|----------------------------|------------------|---------------------------|--------|-----|---------|--------------------------------|--------|------------------------|----------|--------------------------------|--------|---------------------|----|-----------------------|-----------------|-------------------|---------------|-----------------------------------|-----------------------|---------------------|---------------|-----------------------------------|-----------------------|---------------------|---------------|-----------------------------------|-----------------------|-----------------------|-----------------|-----------------------------------|-----------------------|-------------------------|---------------|-----------------------------------|-----------------------|--|
| Primary Standards | ID | Cal Date (Certificate No.) | Scheduled Calibration | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power meter NRP2 | SN: 104778 | 30-Mar-23 (No. 217-03854/03605) | Mar-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor NRP231 | SN: 103244 | 28-Mar-23 (No. 217-03854) | Mar-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| DOF DAK-3.3 (high/low) | SN: 1248 | 05-Oct-23 (DOF-DAK3-1-1949_Oct23) | Oct-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| DOF DAK-12 | SN: 1018 | 05-Oct-23 (DOF-DAK12-1016_Oct23) | Oct-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reference 30 dB Attenuator | SN: C25932 (20v) | 30-Mar-23 (No. 217-03854) | Mar-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| EMF | SN: 680 | 16-Mar-23 (No. SAE4-490_Mar23) | Mar-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Reference Probe E520V2 | SN: 3013 | 05-Jan-23 (No. E52-3013_Jan23) | Jan-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Secondary Standards | ID | Check Date (in house) | Scheduled Check | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power meter E4119 | SN: 084126874 | 06-Apr-18 (in house check Jun-20) | in house check Jun-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor E4112A | SN: 084126897 | 06-Apr-18 (in house check Jun-20) | in house check Jun-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Power sensor E4112A | SN: 080112810 | 06-Apr-18 (in house check Jun-20) | in house check Jun-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| RF generator HP 8445C | SN: 03846591700 | 04-Apr-18 (in house check Jun-20) | in house check Jun-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Network Analyzer E8368A | SN: U84188477 | 31-Mar-14 (in house check Oct-22) | in house check Oct-24 | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

EX3DV4 - SN:7767 October 26, 2023

Parameters of Probe: EX3DV4 - SN:7767

Basic Calibration Parameters

| | Sensor X | Sensor Y | Sensor Z | Unc. (k=2) |
|----------------------|----------|----------|----------|--------------|
| Norm. $\mu(V/m)^2$ A | 0.69 | 0.72 | 0.56 | $\pm 15.1\%$ |
| DCP (mV) B | 102.4 | 102.4 | 106.6 | $\pm 4.7\%$ |

Calibration Results for Modulation Response

| UID | Communication System Name | A | B | C | D | VR | Max dev. | Max Unc. (k=2) |
|-----|---------------------------|------|------|------|------|-------|-------------|----------------|
| 0 | CW | 0.00 | 0.00 | 1.00 | 0.00 | 100.0 | $\pm 1.9\%$ | $\pm 4.7\%$ |
| | | 0.00 | 0.00 | 1.00 | | 100.0 | | |
| | | 0.00 | 0.00 | 1.00 | | 100.0 | | |

The reported uncertainty of measurement is stated as the standard uncertainty multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

A: The uncertainties of Norm. $\mu(V/m)^2$ do not show the $\pm 1\%$ field uncertainty factor 100. (See Page 6).

B: Uncertainty parameter uncertainty for maximum specified field strength.

C: Coverage is determined using the min. diameter from linear spacing applying rectangular distribution and is expressed for the square of the field value.

Certificate No: EX-7767_0023 Page 3 of 9

EX3DV4 - SN:7767 October 26, 2023

Parameters of Probe: EX3DV4 - SN:7767

Other Probe Parameters

| | |
|---|------------|
| Sensor Arrangement | Triangular |
| Connector Angle | -45.9° |
| Mechanical Surface Detection Mode | enabled |
| Optical Surface Detection Mode | disabled |
| Probe Overall Length | 337 mm |
| Probe Body Diameter | 10 mm |
| Tip Length | 9 mm |
| Tip Diameter | 2.5 mm |
| Probe Tip to Sensor X Calibration Point | 1 mm |
| Probe Tip to Sensor Y Calibration Point | 1 mm |
| Probe Tip to Sensor Z Calibration Point | 1 mm |
| Recommended Measurement Distance from Surface | 1.4 mm |

Note: Measurement distance from surface can be increased to 3.4 mm for an Area Scan job.

Certificate No: EX-7767_0023 Page 4 of 9

EX3DV4 - SN:7767 October 26, 2023

Parameters of Probe: EX3DV4 - SN:7767

Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) | Relative Permittivity ¹ | Conductivity ² (S/m) | Coeff X | Coeff Y | Coeff Z | Alpha ³ | Depth ⁴ (mm) | Unc. (k=2) |
|---------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|--------------|
| 150 | 52.3 | 0.76 | 13.37 | 13.37 | 13.37 | 0.00 | 1.25 | $\pm 13.3\%$ |
| 450 | 43.5 | 0.27 | 11.62 | 11.62 | 11.62 | 0.16 | 1.36 | $\pm 13.3\%$ |
| 750 | 41.9 | 0.89 | 10.54 | 10.16 | 10.87 | 0.36 | 1.27 | $\pm 12.0\%$ |
| 855 | 41.5 | 0.90 | 10.38 | 9.86 | 10.00 | 0.38 | 1.27 | $\pm 12.0\%$ |
| 900 | 41.5 | 0.97 | 10.23 | 9.76 | 9.99 | 0.38 | 1.27 | $\pm 12.0\%$ |
| 1750 | 40.1 | 1.37 | 9.45 | 8.73 | 9.34 | 0.24 | 1.27 | $\pm 12.0\%$ |
| 1900 | 40.0 | 1.40 | 8.54 | 7.96 | 8.42 | 0.28 | 1.27 | $\pm 12.0\%$ |
| 2100 | 39.8 | 1.49 | 8.41 | 7.82 | 8.34 | 0.28 | 1.27 | $\pm 12.0\%$ |
| 2300 | 39.6 | 1.67 | 8.70 | 8.12 | 8.81 | 0.39 | 1.27 | $\pm 12.0\%$ |
| 2450 | 39.2 | 1.80 | 8.36 | 7.75 | 8.08 | 0.28 | 1.27 | $\pm 12.0\%$ |
| 2600 | 38.0 | 1.98 | 8.01 | 7.49 | 7.92 | 0.27 | 1.27 | $\pm 12.0\%$ |
| 3300 | 38.2 | 2.71 | 7.41 | 6.83 | 7.31 | 0.33 | 1.27 | $\pm 14.0\%$ |
| 3500 | 37.9 | 2.91 | 7.64 | 7.02 | 7.52 | 0.34 | 1.27 | $\pm 14.0\%$ |
| 3700 | 37.7 | 3.12 | 7.21 | 6.62 | 7.10 | 0.34 | 1.27 | $\pm 14.0\%$ |
| 3900 | 37.5 | 3.32 | 7.17 | 6.59 | 7.08 | 0.34 | 1.27 | $\pm 14.0\%$ |
| 4100 | 37.2 | 3.53 | 6.99 | 6.39 | 6.99 | 0.35 | 1.27 | $\pm 14.0\%$ |
| 4200 | 37.1 | 3.63 | 6.64 | 6.09 | 6.55 | 0.35 | 1.27 | $\pm 14.0\%$ |
| 4400 | 36.9 | 3.94 | 6.59 | 6.06 | 6.50 | 0.36 | 1.27 | $\pm 14.0\%$ |
| 4600 | 36.7 | 4.04 | 6.65 | 6.11 | 6.67 | 0.36 | 1.27 | $\pm 14.0\%$ |
| 4900 | 36.4 | 4.25 | 6.78 | 6.23 | 6.87 | 0.36 | 1.27 | $\pm 14.0\%$ |
| 4900 | 36.3 | 4.40 | 6.43 | 5.87 | 6.30 | 0.39 | 1.36 | $\pm 14.0\%$ |
| 5200 | 36.0 | 4.96 | 6.01 | 5.50 | 5.93 | 0.30 | 1.60 | $\pm 14.0\%$ |
| 5300 | 35.9 | 4.78 | 5.89 | 5.36 | 5.75 | 0.29 | 1.67 | $\pm 14.0\%$ |
| 5500 | 35.6 | 4.46 | 5.53 | 5.07 | 5.46 | 0.32 | 1.70 | $\pm 14.0\%$ |
| 6600 | 35.5 | 5.07 | 5.25 | 4.78 | 5.16 | 0.34 | 1.79 | $\pm 14.0\%$ |
| 5600 | 35.3 | 5.27 | 5.28 | 4.79 | 5.17 | 0.34 | 1.86 | $\pm 14.0\%$ |

¹ Frequency values above 200 MHz of $\pm 10\%$ MHz only apply for DASY-4 and higher (see Page 2), else it is restricted to $\pm 30\%$ MHz. The uncertainty in the 80% of the Coeff. uncertainty at calibration frequencies and for parameters for the indicated frequency band. Frequency values below 200 MHz is $\pm 4\%$, 15, 45, 60 and 70 MHz for Coeff. measurements at 21, 66, 126, 135 and 200 MHz respectively. Uncertainty of Coeff. assessment at 8 MHz to 4 MHz, and of Coeff. assessment at 15 MHz to 30 MHz. Above 50 MHz frequency values are rounded to 1 Hz.

² The probe was calibrated using tissue simulating media (TSM) that differs for x and y by less than 0.5% from the target values (typically better than 0.5%) and are used to fit, with constraint of $\pm 0.1\%$ of TSM, with deviations from the target of less than 0.5%. We used the calibration uncertainties as 1.1% for x , y , z and 0.1% for α .

³ Alpha depth was determined during calibration. SPREAD software that the remaining deviation due to the boundary effect after compensation is always less than 1% for frequencies below 3 GHz and below $\pm 2\%$ for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.





Certificate No: EX-7767_0023 Page 5 of 9

EX3DV4 - SN:7767 October 26, 2023

Frequency Response of E-Field
(TEM-Cell#110 EXX, Waveguide#222)

Uncertainty of Frequency Response of E-Field: $\pm 0.3\%$ (k=2)

Certificate No: EX-7767_0023 Page 6 of 9

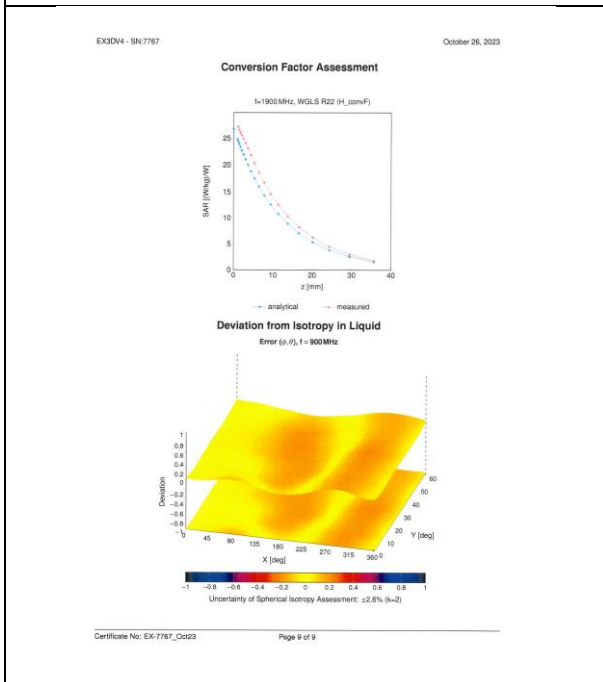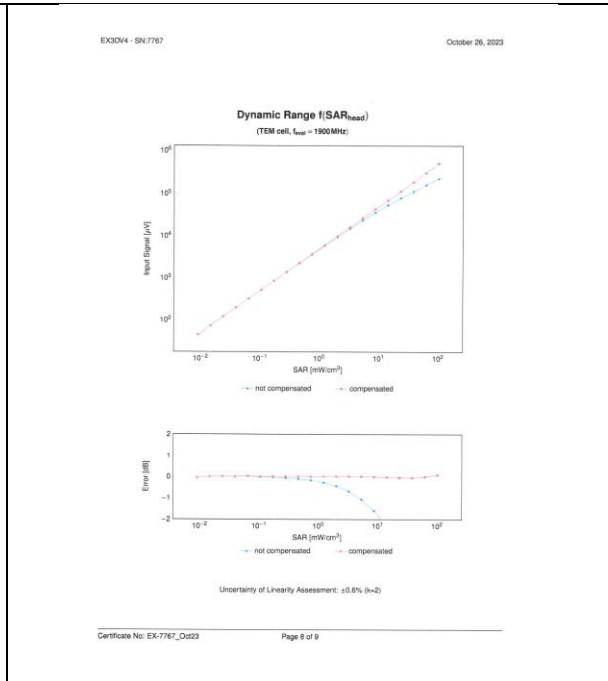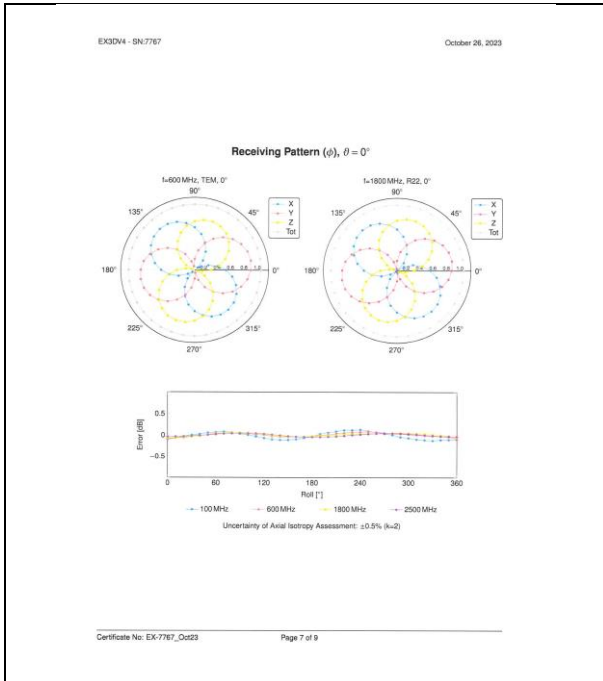

4 Impedance and return loss

| Dipole CLA150 SN 4025 | | | | |
|-------------------------|-----------------|------------|------------------------|----------------|
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2021/4/26 | -31.4 | / | 47.8 | / |
| 2022/4/26 | -32.5 | -3.5% | 47.1 | 0.7 |
| 2023/4/26 | -32.3 | -2.87% | 46.5 | 1.3 |
| Dipole D450V3 SN 1103 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2021/4/21 | -23 | / | 57.1 | / |
| 2022/4/26 | -23.4 | -1.74% | 56.6 | 0.5 |
| 2023/4/26 | -23.9 | -3.91% | 56.2 | 0.9 |
| Dipole D750V3 SN 1188 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/3/29 | -28.7 | / | 53.6 | / |
| 2023/3/29 | -28.3 | 1.39% | 53.2 | 0.4 |
| Dipole D835V2 SN 4d114 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/3/31 | -25.3 | / | 48.7 | / |
| 2023/3/31 | -24.6 | 2.77% | 49.1 | 0.4 |
| Dipole D900V2 SN 1d079 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/6/7 | -23.3 | / | 48.1 | / |
| 2023/6/7 | -23.6 | -1.29% | 48.3 | 0.2 |
| Dipole D1800V2 SN 2d170 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/3/31 | -29.4 | / | 47.9 | / |
| 2023/3/31 | -28.9 | 1.70% | 47.2 | 0.7 |
| Dipole D1900V2 SN 5d136 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/6/7 | -22.4 | / | 51.2 | / |
| 2023/6/7 | -22.9 | -2.23% | 51.6 | -0.4 |
| Dipole D2000V2 SN 1041 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/6/6 | -34.9 | / | 48.4 | / |
| 2023/6/6 | -33.5 | 4.01% | 49.1 | -0.7 |
| Dipole D2300V2 SN 1096 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |

| | | | | |
|---------------------------------|-----------------|------------|------------------------|----------------|
| 2022/3/31 | -26.6 | / | 49.2 | / |
| 2023/3/31 | -27.1 | -1.88% | 49.4 | 0.2 |
| Dipole D2450V2 SN 817 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/4/1 | -28.5 | / | 52.1 | / |
| 2023/4/1 | -28.0 | 1.75% | 51.6 | 0.5 |
| Dipole D2600V2 SN 1158 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/3/31 | -23.8 | / | 49.9 | / |
| 2023/3/31 | -23.3 | 2.10% | 50.3 | 0.4 |
| Dipole D5GHzV2 SN 1095 for 5200 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/6/1 | -23.6 | / | 46.1 | / |
| 2023/6/1 | -23.1 | 2.12% | 45.6 | 0.5 |
| Dipole D5GHzV2 SN 1095 for 5300 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/6/1 | -29.5 | / | 47.8 | / |
| 2023/6/1 | -28.8 | 2.37% | 46.9 | 0.9 |
| Dipole D5GHzV2 SN 1095 for 5500 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/6/1 | -27.4 | / | 50.3 | / |
| 2023/6/1 | -27.6 | -0.73% | 50.8 | -0.5 |
| Dipole D5GHzV2 SN 1095 for 5600 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/6/1 | -24.0 | / | 54.5 | / |
| 2023/6/1 | -23.6 | 1.67% | 54.9 | -0.4 |
| Dipole D5GHzV2 SN 1095 for 5800 | | | | |
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2022/6/1 | -24.9 | / | 51.5 | / |
| 2023/6/1 | -24.3 | 2.41% | 51.0 | 0.5 |