





TEST REPORT

No.I20N02014-SAR

For

TCL Communication Ltd.

10 inch wifi tablet

Model Name: 8092

With

Hardware Version: 1.2

Software Version: DB9

FCC ID: 2ACCJB133

Issued Date: 2020-08-14

Note:

The test results in this test report relate only to the devices specified in this report. This report shall not be reproduced except in full without the written approval of SAICT.

Test Laboratory:

SAICT, Shenzhen Academy of Information and Communications Technology

Building G, Shenzhen International Innovation Center, No.1006 Shennan Road, Futian District, Shenzhen, Guangdong, P. R. China 518026.

Tel: +86(0)755-33322000, Fax: +86(0)755-33322001

Email: yewu@caict.ac.cn. www.saict.ac.cn





REPORT HISTORY

Report Number	Revision	Description	Issue Date
I20N02014-SAR	Rev.0	1st edition	2020-08-14





TCONTENTS

1. SUMMARY OF TEST REPORT	5
1.1. TEST ITEMS	5
1.2. TEST STANDARDS	5
1.3. TEST RESULT	
1.4. TESTING LOCATION	
1.5. Project Data	
1.6. SIGNATURE	
2. STATEMENT OF COMPLIANCE	6
3. CLIENT INFORMATION	7
3.1. Applicant Information	7
3.2. MANUFACTURER INFORMATION	7
4. EQUIPMENT UNDER TEST (EUT) AND ANCILLARY EQUIPMENT (AE)	8
4.1. ABOUT EUT	
4.2. INTERNAL IDENTIFICATION OF EUT USED DURING THE TEST	
4.3. INTERNAL IDENTIFICATION OF AE USED DURING THE TEST	
5. TEST METHODOLOGY	9
5.1. APPLICABLE LIMIT REGULATIONS	
5.2. Applicable Measurement Standards	9
6. SPECIFIC ABSORPTION RATE (SAR)	10
6.1. INTRODUCTION	10
6.2. SAR DEFINITION	
7. TISSUE SIMULATING LIQUIDS	11
7.1. TARGETS FOR TISSUE SIMULATING LIQUID	11
7.2. DIELECTRIC PERFORMANCE	11
8. SYSTEM VERIFICATION	12
8.1. System Setup	
8.2. System Verification	13
9. MEASUREMENT PROCEDURES	14
9.1. Tests to be performed	
9.2. General Measurement Procedure	
9.3. BLUETOOTH & WLAN MEASUREMENT PROCEDURES FOR SAR	17
9.4. Power Drift	
10. CONDUCTED OUTPUT POWER	
10.1. BLUETOOTH AND WLAN MEASUREMENT RESULT	
11. TRANSMIT ANTENNA	19
©Copyright. All rights reserved by SAICT	Page 3 of 61





11.1. ANTENNA LOCATIONS	
11.2 SAR MEASUREMENT POSITIONS	
12. SUMMARY OF TEST RESULTS	21
12.1. TESTING ENVIRONMENT	
13. SAR MEASUREMENT VARIABILITY	23
14. MEASUREMENT UNCERTAINTY	24
14.1. MEASUREMENT UNCERTAINTY FOR NORMAL SAR TESTS (300MHz~3GHz)	24
15. MAIN TEST INSTRUMENTS	25
ANNEX A: GRAPH RESULTS	26
ANNEX B: SYSTEMVERIFICATION RESULTS	27
ANNEX C: SAR MEASUREMENT SETUP	28
C.1. MEASUREMENT SET-UP C.2. DASY5 E-FIELD PROBE SYSTEM C.3. E-FIELD PROBE CALIBRATION C.4. OTHER TEST EQUIPMENT	29 29
ANNEX D: POSITION OF THE WIRELESS DEVICE IN RELATION TO THE PHANTOM	34
D.1. GENERAL CONSIDERATIONS D.2. BODY-WORN DEVICE D.3. DESKTOP DEVICE D.4. DUT SETUP PHOTOS	35 35
ANNEX E: EQUIVALENT MEDIA RECIPES	37
ANNEX F: SYSTEM VALIDATION	38
ANNEX G: DAE CALIBRATION CERTIFICATE	39
ANNEX H: PROBE CALIBRATION CERTIFICATE	42
ANNEX I: DIPOLE CALIBRATION CERTIFICATE	52
ANNEX J: EXTENDED CALIBRATION SAR DIPOLE	60
ANNEX K: ACCREDITATION CERTIFICATE	61





1. Summary of Test Report

1.1. Test Items

Description:10 inch wifi tabletModel Name:8092Applicant's name:TCL Communication Ltd.Manufacturer's Name:TCL Communication Ltd.

1.2. Test Standards

ANSI C95.1-1992, IEEE 1528-2013

1.3. Test Result

Pass. Please refer to "13. Summary of Test Results"

1.4. Testing Location

Address: Building G, Shenzhen International Innovation Center, No.1006 Shennan Road, Futian District, Shenzhen, Guangdong, P. R. China

1.5. Project Data

Testing Start Date: 2020-08-05

Testing End Date: 2020-08-05

1.6. Signature

季田昌

Li Yongfu (Prepared this test report)

Cao Junfei (Approved this test report)

Zhang Yunzhuan (Reviewed this test report)

©Copyright. All rights reserved by SAICT





2. Statement of Compliance

The maximum results of Specific Absorption Rate (SAR) found during testing for TCL Communication Ltd. 10 inch wifi tablet 8092 are as follows:

Table 2.1: Highest Reported SAR for Body (1g)						
Exposure Configuration	Technology Band	Highest Reported SAR 1g(W/Kg)	Equipment Class			
Body	WLAN 2.4GHz	1.23	DTS			

The SAR values found for the Mobile Phone are below the maximum recommended levels of 1.6 W/Kg as averaged over any 1g tissue according to the ANSI C95.1-1992.

The EUT battery must be fully charged and checked periodically during the test to ascertain uniform power output.

The measurement together with the test system set-up is described in annex C of this test report. A detailed description of the equipment under test can be found in chapter 4 of this test report.

The highest reported SAR value is obtained at the case of (Table 2.1), and the value is: **1.23 W/kg** (1g).





3. Client Information

3.1. Applicant Information

Company Name:	TCL Communication Ltd.
Address:	5/F, Building 22E, 22 Science Park East Avenue, Hong Kong Science
Address.	Park, Shatin, NT, Hong Kong
City:	/
Country:	/
Telephone:	0086-755-36611722

3.2. Manufacturer Information

Company Name:	TCL Communication Ltd.
Address:	5/F, Building 22E, 22 Science Park East Avenue, Hong Kong Science
Address.	Park, Shatin, NT, Hong Kong
City:	/
Country:	/
Telephone:	0086-755-36611722





4. Equipment under Test (EUT) and Ancillary Equipment (AE)

4.1. About EUT

Description:	10 inch wifi tablet
Model Name:	8092
Marketing Name:	1
Operating mode(s):	Bluetooth, WLAN 2.4G
Condition of EUT as received:	No obvious damage in appearance
Tested Tx Frequency	2402 – 2480MHz (Bluetooth)
Tested Tx Frequency:	2412 – 2462MHz (WLAN 2.4G)
Test device Production information:	Production unit
Device type:	Portable device
Antenna type:	Integrated antenna
Product Dimensions:	Long 244.3mm; Wide 162.2mm; Overall Diagonal 286mm

4.2. Internal Identification of EUT used during the test

EUT ID*	UDID	HW Version	SW Version
UT05aa F05136CAEC97485		1.2	DB9
UT07aa	F05136CAEC9A933	1.2	DB9

*EUT ID: is used to identify the test sample in the lab internally.

Note: It is performed to test SAR with the UT 05aa, and conducted power with the UT07aa.

4.3. Internal Identification of AE used during the test

AE ID*	Description	Туре	Manufacturer		
AE1	Battery	TLp040M7	VEKEN		

*AE ID: is used to identify the test sample in the lab internally.





5. Test Methodology

5.1. Applicable Limit Regulations

ANSI C95.1–1992: IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz.

It specifies the maximum exposure limit of **1.60 W/kg** as averaged over any 1 gram of tissue for portable devices being used within 20 cm of the user in the uncontrolled environment.

5.2. Applicable Measurement Standards

IEEE 1528–2013: Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Experimental Techniques.

KDB 447498 D01 General RF Exposure Guidance v06: Mobile and Portable Devices RF Exposure Procedures and Equipment Authorization Policies.

KDB 616217 D04 SAR for laptop and tablets v01r02: SAR Evaluation Considerations for Laptop, Notebook, Notebook and Tablet Computers.

KDB 248227 D01 802.11 Wi-Fi SAR v02r02: SAR Guidance for IEEE 802.11 (Wi-Fi) Transmitters.

KDB 865664 D01SAR measurement 100 MHz to 6 GHz v01r04: SAR Measurement Requirements for 100 MHz to 6 GHz.

KDB 865664 D02 RF Exposure Reporting v01r02: RF Exposure Compliance Reporting and Documentation Considerations

TCB workshop April 2019; RF Exposure Procedures (Tissue Simulating Liquids)





6. Specific Absorption Rate (SAR)

6.1. Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits higher the limits for are than general population/uncontrolled.

6.2. SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density (ρ) . The equation description is as below:

$$SAR = \frac{d}{dt}(\frac{dW}{dm}) = \frac{d}{dt}(\frac{dW}{\rho dv})$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$SAR = c(\frac{\delta T}{\delta t})$$

Where: C is the specific head capacity, δT is the temperature rise and δt is the exposure duration, or related to the electrical field in the tissue by

$$SAR = \frac{\sigma |E|^2}{\rho}$$

Where: σ is the conductivity of the tissue, ρ is the mass density of tissue and *E* is the RMS electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.





7. Tissue Simulating Liquids

7.1. Targets for tissue simulating liquid

		_				
Frequency (MHz)	Liquid Type	Conductivity (σ)	± 5% Range	Permittivity (ε)	± 5% Range	
2450	Head	1.80	1.71~1.89	39.2	37.2~41.2	

note for tissue simulating liquid

7.2. Dielectric Performance

Table 7.2: Dielectric Performance of Tissue Simulating Liquid

Measurement Date (yyyy-mm-dd)	Туре	Frequency	Conductivity σ (S/m)	Drift (%)	Permittivity ε	Drift (%)
2020-08-05	2450	Head	1.853	2.94	38.32	-2.24

Note: The liquid temperature is 22.0°C.



Picture 7-1: Liquid depth in the Flat Phantom(2450MHz)






8. System verification

8.1. System Setup

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave that comes from a signal generator. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

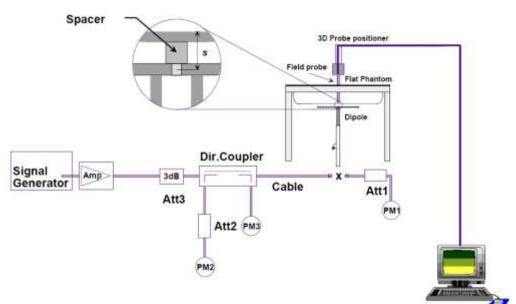

Picture 8.1 System Setup for System Evaluation



Picture 8.2 Photo of Dipole Setup





8.2. System Verification

SAR system verification is required to confirm measurement accuracy, according to the tissue dielectric media, probe calibration points and other system operating parameters required for measuring the SAR of a test device. The system verification must be performed for each frequency band and within the valid range of each probe calibration point required for testing the device.

				Cystem ver		cuu		
Measurement			Target va	lue (W/kg)	Measured v	alue (W/kg)	Deviation (%)	
	Date	Frequency	10 g	1 g	10 g	1 g	10 g	1 g
	(yyyy-mm-dd)		Average	Average	Average	Average	Average	Average
	2020-08-05	2450 MHz	24.10	52.00	24.76	54.00	2.74	3.85

Table 8.1: System Verification of Head





9. Measurement Procedures

9.1. Tests to be performed

In order to determine the highest value of the peak spatial-average SAR of a handset, all device positions, configurations and operational modes shall be tested for each frequency band according to steps 1 to 3 below. A flowchart of the test process is shown in picture 9.1.

Step 1: The tests described in 9.2 shall be performed at the channel that is closest to the center of

the transmit frequency band (f_c) for:

a) all device positions (cheek and tilt, for both left and right sides of the SAM phantom, as described in annex D),

b) all configurations for each device position in a), e.g., antenna extended and retracted, and

c) all operational modes, e.g., analogue and digital, for each device position in a) and configuration in b) in each frequency band.

If more than three frequencies need to be tested according to 11.1 (i.e., $N_c > 3$), then all


frequencies, configurations and modes shall be tested for all of the above test conditions.

Step 2: For the condition providing highest peak spatial-average SAR determined in Step 1, perform all tests described in 9.2 at all other test frequencies, i.e., lowest and highest frequencies. In addition, for all other conditions (device position, configuration and operational mode) where the peak spatial-average SAR value determined in Step 1 is within 3 dB of the applicable SAR limit, it is recommended that all other test frequencies shall be tested as well.

Step 3: Examine all data to determine the highest value of the peak spatial-average SAR found in Steps 1 to 2.



CAICT No. I20N02014-SAR

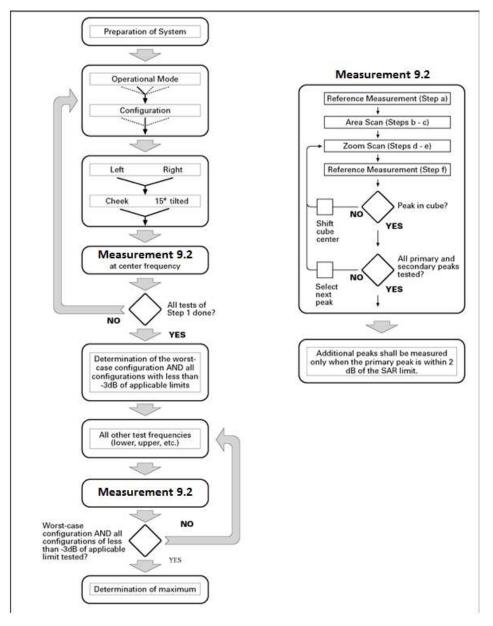

Picture 9.1 Block diagram of the tests to be performed





9.2. General Measurement Procedure

The area and zoom scan resolutions specified in the table below must be applied to the SAR measurements and fully documented in SAR reports to qualify for TCB approval. Probe boundary effect error compensation is required for measurements with the probe tip closer than half a probe tip diameter to the phantom surface. Both the probe tip diameter and sensor offset distance must satisfy measurement protocols; to ensure probe boundary effect errors are minimized and the higher fields closest to the phantom surface can be correctly measured and extrapolated to the phantom surface for computing 1-g SAR. Tolerances of the post-processing algorithms must be verified by the test laboratory for the scan resolutions used in the SAR measurements, according to the reference distribution functions specified in IEEE Std 1528-2013. The results should be documented as part of the system validation records and may be requested to support test results when all the measurement parameters in the following table are not satisfied.

			\leq 3 GHz	> 3 GHz		
Maximum distance from (geometric center of pro			$5\pm1\mathrm{mm}$	$\frac{1}{2}\cdot\delta\cdot\ln(2)\pm0.5~mm$		
Maximum probe angle normal at the measurem		axis to phantom surface 1	30°±1°	20°±1°		
			$\leq 2 \text{ GHz:} \leq 15 \text{ mm}$ $2 - 3 \text{ GHz:} \leq 12 \text{ mm}$	$\begin{array}{l} 3-4 \ \mathrm{GHz:} \leq 12 \ \mathrm{mm} \\ 4-6 \ \mathrm{GHz:} \leq 10 \ \mathrm{mm} \end{array}$		
Maximum area scan spa	atial resoluti	on: Δx _{Ares} , Δy _{Area}	When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the above, the measurement resolution must be \leq the corresponding x or y dimension of the test device with at least one measurement point on the test device.			
Maximum zoom sean sj	patial resolu	tion: Δx_{Zoom} , Δy_{Zoom}	$\leq 2 \text{ GHz} \leq 8 \text{ mm}$ 2 - 3 GHz: $\leq 5 \text{ mm}^4$	3 – 4 GHz: ≤ 5 mm 4 – 6 GHz: ≤ 4 mm		
1	uniform	grid: Δz _{Zcom} (n)	≤ 5 mm	$3 - 4 \text{ GHz}: \le 4 \text{ mm}$ $4 - 5 \text{ GHz}: \le 3 \text{ mm}$ $5 - 6 \text{ GHz}: \le 2 \text{ mm}$		
Maximum zoom scan spatial resolution, normal to phantom surface	graded	$\Delta z_{Zoom}(1)$: between 1^{st} two points closest to phantom surface	≤ 4 mm	3 – 4 GHz: ≤3 mm 4 – 5 GHz: ≤2.5 mm 5 – 6 GHz: ≤2 mm		
	grid ∆z _{Zoom} (n>1): between subsequent points		≤1.5·∆a	z _{Zeem} (n-1)		
Minimum zoom scan volume	m scan x, y, z		≥ 30 mm	3 – 4 GHz: ≥ 28 mm 4 – 5 GHz: ≥ 25 mm 5 – 6 GHz: > 22 mm		

when zoom scan is required and the <u>reported</u> SAR from the area scan based 1-g SAR estimation procedures of RDB 447498 is ≤ 1.4 W/kg, ≤ 8 mm, ≤ 7 mm and ≤ 5 mm zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.





9.3. Bluetooth & WLAN Measurement Procedures for SAR

Normal network operating configurations are not suitable for measuring the SAR of 802.11 transmitters in general. Unpredictable fluctuations in network traffic and antenna diversity conditions can introduce undesirable variations in SAR results. The SAR for these devices should be measured using chipset based test mode software to ensure that the results are consistent and reliable.

Chipset based test mode software is hardware dependent and generally varies among manufacturers. The device operating parameters established in a test mode for SAR measurements must be identical to those programmed in production units, including output power levels, amplifier gain settings and other RF performance tuning parameters. The test frequencies should correspond to actual channel frequencies defined for domestic use. SAR for devices with switched diversity should be measured with only one antenna transmitting at a time during each SAR measurement, according to a fixed modulation and data rate. The same data pattern should be used for all measurements.

9.4. Power Drift

To control the output power stability during the SAR test, DASY5 system calculates the power drift by measuring the E-field at the same location at the beginning and at the end of the measurement for each test position. These drift values can be found in Section 14 labeled as: (Power Drift [dB]). This ensures that the power drift during one measurement is within 5%.





10. Conducted Output Power

10.1. Bluetooth and WLAN Measurement result

Bluetooth	Tung un	Averaged Power (dBm)					
Mode	Tune up	Ch.0 (2402 MHz)	Ch39 (2441 MHz)	Ch78 (2480 MHz)			
GFSK	7.0	6.15	5.90	5.52			
EDR2M-4_DQPSK	6.5	5.58 5.76		5.32			
EDR3M-8DPSK	6.5	6.03	5.79	5.44			
/	1	Ch0 (2402MHz)	Ch19 (2440MHz)	Ch39 (2480MHz)			
BLE 6.0		5.15	4.94	4.48			

Table 10.1: The conducted Power measurement results for Bluetooth

Table 10.2:	The conducted Power measurement results for WLAN 2.4G

WLAN 2.4GHz	Tung un	Averaged	Power (dBm) Duty	Cycle: 100%	
Mode	Tune up	Ch.1(2412 MHz)	Ch.6(2437Mhz)	Ch.11(2462MHz)	
802.11b	15.5	14.54	14.46	14.55	
802.11g	14.5	13.41	13.46	13.49	
802.11n(20MHz)	14.5	13.37	13.51	13.42	
/	/ /		Ch.6(2437Mhz)	Ch.9(2452MHz)	
802.11n(40MHz)	02.11n(40MHz) 13.5		12.17	12.14	






BT/WLAN Antenna

11. Transmit Antenna

11.1. Antenna Locations

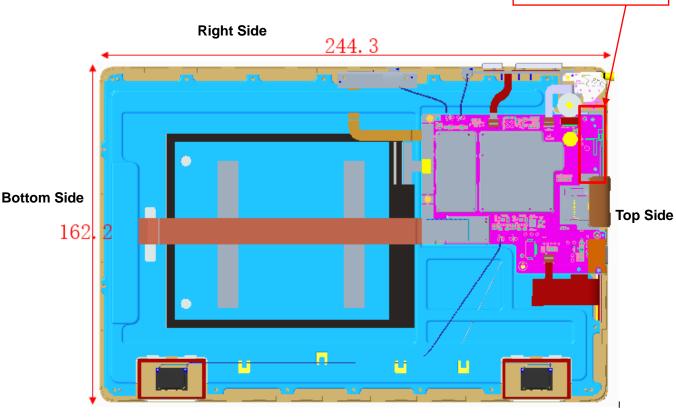

Left Side

Picture 11.1 Antenna Locations (Back View)





11.2 SAR Measurement Positions

SAR measurement positions										
Antenna	Antenna Rear Left edge Right edge Top edge Bottom edge									
WLAN Yes No Yes Yes No										

Note:

1. Per KDB 447498 D01v06, the 1-g SAR test exclusion thresholds for 100 MHz to 6 GHz at *test* separation distances \leq 50 mm are determined by:

[(max. power of channel, including tune-up tolerance, mW) / (min. test separation distance, mm)] $\cdot [\sqrt{f(GHz)}] \le 3.0$ for 1-g SAR, where

f(GHz) is the RF channel transmit frequency in GHz

Power and distance are rounded to the nearest mW and mm before calculation

2. Per KDB 447498 D01v06, For 100 MHz to 6 GHz and *test separation distances* > 50 mm, the 1-g and 10-g SAR test exclusion thresholds are determined by the following

1) {[Power allowed at *numeric threshold* for 50 mm in step a)] + [(test separation distance – 50 mm) \cdot (f(MHz)/150)]} mW, for 100 MHz to 1500 MHz

2) {[Power allowed at *numeric threshold* for 50 mm in step a)] + [(test separation distance – 50 mm) \cdot 10]} mW, for > 1500 MHz and ≤ 6 GHz

11.3. Standalone SAR Test Exclusion Considerations

Standalone 1-g head or body SAR evaluation by measurement or numerical simulation is not required when the corresponding SAR Exclusion Threshold condition, listed below, is satisfied. The 1-g SAR test exclusion threshold for 100 MHz to 6 GHz at test separation distances \leq 50 mm are determined by:

[(max. power of channel, including tune-up tolerance, mW) / (min. test separation distance, mm)] \cdot [$\sqrt{f}(GHz)$] \leq 3.0 for 1-g SAR, where

- f(GHz) is the RF channel transmit frequency in GHz
- Power and distance are rounded to the nearest mW and mm before calculation
- The result is rounded to one decimal place for comparison

Band/Mode	f(GHz)	Position	SAR test exclusion	RF outp	ut power	SAR test	
Banu/woue	((бп2)	POSILION	threshold (mW)	dBm	mW	exclusion	
Bluetooth	2.4	Body	9.60	7.0	5.01	Yes	
WLAN 2.4GHz	2.4	Body	9.58	15.5	35.48	No	

Table 11.1: Standalone SAR test exclusion considerations





12. Summary of Test Results

According to the client's decision rule in the test registration form, which is "based on the measurement results as the basis of the conformity statement", the test conclusion of this report meets the limit requirements.

The calculated SAR is obtained by the following formula:

Reported SAR = Measured SAR × $10^{(P_{Target}-P_{Measured})/10}$

Where P_{Target} is the power of manufacturing upper limit;

 $P_{Measured}$ is the measured power in chapter 10.

12.1. Testing Environment

Temperature:	18°C~25°C
Relative humidity:	30%~70%
Ground system resistance:	<4Ω
Ambient noise & Reflection:	< 0.012 W/kg





12.2. WLAN Evaluation for 2.4G

According to the KDB248227 D01, SAR is measured for 2.4GHz 802.11b DSSS using the <u>initial test</u> <u>position</u> procedure.

	Ambient Temperature: 22.0°C Liquid Temperature: 21.5°C													
Frequency MHz Ch.		Test Mode	Test Position	Figure No. / Note	Conducted Power (dBm)	Max. tune-up Power (dBm)	Measured SAR(1g) (W/kg)	Reported SAR(1g) (W/kg)	Power Drift(dB)					
	0mm Test Data													
2462	11	802.11b	Rear	11	14.55	15.5	0.992	1.23	0.02					
2462	11	802.11b	Right	/	14.55	15.5	0.105	0.13	0.07					
2462	11	802.11b	Тор	/	14.55	15.5	0.533	0.66	0.14					
2437	6	802.11b	Rear	/	14.46	15.5	0.957	1.22	0.07					
2412	1	802.11b	Rear	/	14.54	15.5	0.967	1.21	0.06					

Table 12.1: SAR Values (WLAN 2.4G - Body)

Note1: For all positions/configurations tested using the initial test position and subsequent test positions, when the reported SAR is > 0.8 W/kg, SAR is measured for these test positions/configurations on the subsequent next highest measured output power channel until the reported SAR is \leq 1.2 W/kg or all required channels are tested.

According to the KDB248227 D01, The reported SAR must be scaled to 100% transmission duty factor to determine compliance at the maximum tune-up tolerance limit.

-			•			
Frequency		Test	Actual duty	maximum	Reported SAR	Scaled reported
MHz	MHz Ch.		factor	duty factor	(1g)(W/kg)	SAR (1g)(W/kg)
2462	11	Rear	100%	100%	1.23	1.23

Table 12.2: SAR Values (WLAN - Body) – 802.11b (Scaled Reported SAR)

SAR is not required for OFDM because the 802.11b adjusted SAR \leq 1.2 W/kg.





13. SAR Measurement Variability

SAR measurement variability must be assessed for each frequency band, which is determined by the SAR probe calibration point and tissue-equivalent medium used for the device measurements. When both head and body tissue-equivalent media are required for SAR measurements in a frequency band, the variability measurement procedures should be applied to the tissue medium with the highest measured SAR, using the highest measured SAR configuration for that tissue-equivalent medium.

The following procedures are applied to determine if repeated measurements are required.

1) Repeated measurement is not required when the original highest measured SAR is < 0.80 W/kg; steps 2) through 4) do not apply.

2) When the original highest measured SAR is \geq 0.80 W/kg, repeat that measurement once.

3) Perform a second repeated measurement only if the ratio of largest to smallest SAR for the original and first repeated measurements is > 1.20 or when the original or repeated measurement is \geq 1.45 W/kg (~ 10% from the 1-g SAR limit).

4) Perform a third repeated measurement only if the original, first or second repeated measurement is \geq 1.5 W/kg and the ratio of largest to smallest SAR for the original, first and second repeated measurements is > 1.20.

Frequ	ency	Test Position	Original	1 st Repeated	Ratio	2 nd Repeated
MHz	Ch.		SAR (W/kg)	SAR (W/kg)	Ralio	SAR (W/kg)
2462	11	Rear	0.992	0.984	1.01	/

Table 13.1: SAR Measurement Variability for Body – WLAN 2.4G





14. Measurement Uncertainty

14.1. Measurement Uncertainty for Normal SAR Tests (300MHz~3GHz)

No.	No. Error Description		Uncertainty value	Probably Distribution	Div.	(Ci) 1g	(Ci) 10g	Std. Unc. (1g)	Std. Unc. (10g)	Degree of freedom				
	Measurement system													
1	Probe calibration	В	12	Ν	2	1	1	6.0	6.0	∞				
2	Axial isotropy	В	4.7	R	$\sqrt{3}$	√0.5	√0.5	4.3	4.3	8				
3	Hemispherical isotropy	В	9.6	R	$\sqrt{3}$	1	1	4.8	4.8	∞				
4	Boundary effect	В	1.1	R	$\sqrt{3}$	1	1	0.6	0.6	∞				
5	Linearity	В	4.7	R	$\sqrt{3}$	1	1	2.7	2.7	∞				
6	Detection limit	В	1.0	R	$\sqrt{3}$	1	1	0.6	0.6	8				
7	Modulation response	В	4.0	R	$\sqrt{3}$	1	1	2.3	2.3	∞				
8	Readout electronics	В	1.0	Ν	1	1	1	1.0	1.0	8				
9	Response time	В	0.8	R	$\sqrt{3}$	1	1	0.5	0.5	∞				
10	Integration time	В	1.7	R	$\sqrt{3}$	1	1	1.0	1.0	∞				
11	RF ambient conditions-noise	В	3.0	R	$\sqrt{3}$	1	1	1.7	1.7	×				
12	RF ambient conditions-reflection	В	3.0	R	$\sqrt{3}$	1	1	1.7	1.7	∞				
13	Probe positioned mech. restrictions	В	0.35	R	$\sqrt{3}$	1	1	0.2	0.2	∞				
14	Probe positioning with respect to phantom shell	В	2.9	R	$\sqrt{3}$	1	1	1.7	1.7	∞				
15	Post-processing	В	1.0	R	$\sqrt{3}$	1	1	0.6	0.6	∞				
		-	Test	sample related	-	-			-					
16	Test sample positioning	А	3.3	Ν	1	1	1	3.3	3.3	5				
17	Device holder uncertainty	А	3.4	Ν	1	1	1	3.4	3.4	5				
18	Drift of output power	В	5.0	R	$\sqrt{3}$	1	1	2.9	2.9	∞				
			Phant	om and set-up	-	1								
19	Phantom uncertainty	В	1.0	R	$\sqrt{3}$	1	1	0.6	0.6	∞				
20	Liquid conductivity (target)	В	5.0	R	$\sqrt{3}$	0.64	0.43	1.8	1.2	8				
21	Liquid conductivity (meas.)	А	1.3	Ν	1	0.64	0.43	0.83	0.56	9				
22	Liquid permittivity (target)	В	5.0	R	$\sqrt{3}$	0.6	0.49	1.7	1.4	∞				
23	Liquid permittivity (meas.)	А	1.6	Ν	1	0.6	0.49	0.96	0.78	9				
	Combined standard uncertainty $u_c^{'} = \sqrt{\sum_{i=1}^{23} c_i^2 u_i^2}$		$=\sqrt{\sum_{i=1}^{23}c_i^2u_i^2}$					11.3	11.2	95.5				
	nded uncertainty fidence interval of 95 %)	ι	$u_e = 2u_c$					22.6	22.4					





15. Main Test Instruments

No.	Name	Туре	Serial Number	Calibration Date	Valid Period
01	Network analyzer	E5071C	MY46103759	2019-11-15	One year
02	Dielectric probe	85070E	MY44300317	/	/
03	Power meter	E4418B	MY50000366	2019-12-14	
04	Power sensor	E9304A	MY50000188	2019-12-14	One year
05	Power meter	NRP			
06	Power sensor	NRP-Z91	100553	2020-01-15	One year
07	Signal Generator	E8257D	MY47461211	2020-01-15	One year
08	Amplifier	VTL5400	0404	/	/
09	E-field Probe	EX3DV4	3633	2020-04-01	One year
10	DAE	DAE4	1527	2019-11-11	One year
11	Dipole Validation Kit	D2450V2	873	2018-10-26	Three year
12	Software	DASY5	52.8.8.1222	/	/

Table 15.1: List of Main Instruments






ANNEX A: Graph Results

WLAN 2.4G Body Date: 2020-8-5 Electronics: DAE4 Sn1527 Medium: Head 2450MHz Medium parameters used: f = 2462 MHz; σ = 1.867 S/m; ϵ_r = 38.282; ρ = 1000 kg/m³ Communication System: UID 0, WiFi (0) Frequency: 2462 MHz Duty Cycle: 1:1 Probe: EX3DV4 - SN3633 ConvF (7.43, 7.43, 7.43)

Rear Side High/Area Scan (91x91x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Maximum value of SAR (interpolated) = 1.73 W/kg

Rear Side High/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 1.418 V/m; Power Drift = 0.02 dB Peak SAR (extrapolated) = 2.47 W/kg SAR(1 g) = 0.992 W/kg; SAR(10 g) = 0.428 W/kg Maximum value of SAR (measured) = 1.47 W/kg

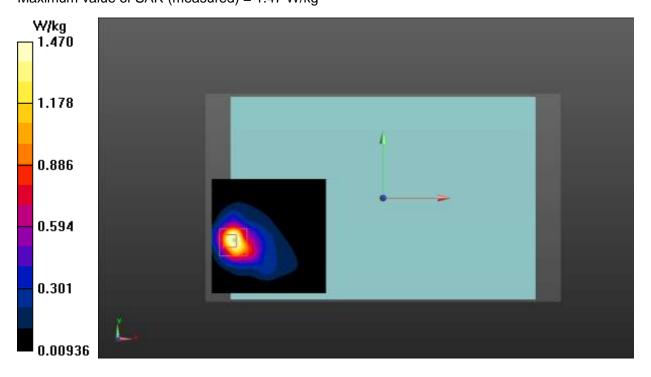








ANNEX B: SystemVerification Results

2450MHz

Date: 2020-8-5 Electronics: DAE4 Sn1527 Medium: Head 2450MHz Medium parameters used: f = 2450 MHz; σ = 1.853 S/m; ϵ_r = 38.322; ρ = 1000 kg/m³ Ambient Temperature: 22.3°C Liquid Temperature: 21.8°C Communication System: CW_TMC Frequency: 2450 MHz Duty Cycle: 1:1 Probe: EX3DV4 – SN3633 ConvF (7.43, 7.43, 7.43);

System Validation/Area Scan (81x121x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm Reference Value = 87.659 V/m; Power Drift = 0.06 dB SAR(1 g) = 13.1 W/kg; SAR(10 g) = 6.11 W/kg Maximum value of SAR (interpolated) = 15.2 W/kg

System Validation/Zoom Scan (7x7x7)/Cube0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 87.659 V/m; Power Drift = 0.06 dB Peak SAR (extrapolated) = 28.4 W/kg SAR(1 g) = 13.5 W/kg; SAR(10 g) = 6.19 W/kg Maximum value of SAR (measured) = 15.5 W/kg

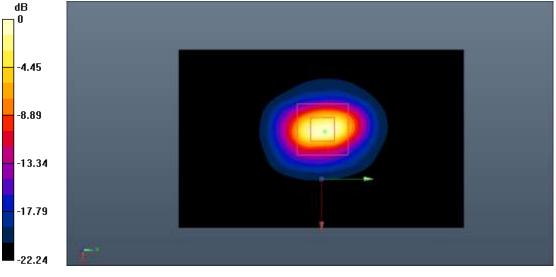

0 dB = 15.5 W/kg = 11.90 dB W/kg

Fig.B.1. Validation 2450MHz 250mW






ANNEX C: SAR Measurement Setup

C.1. Measurement Set-up

DASY5 system for performing compliance tests is illustrated above graphically. This system consists of the following items:

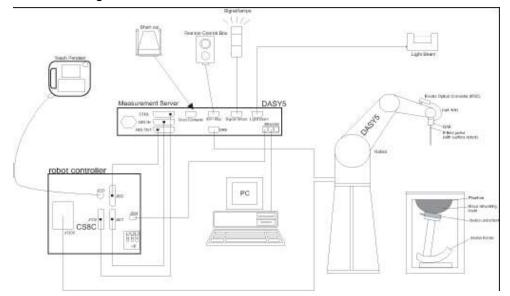

Picture C.1 SAR Lab Test Measurement Set-up

- A standard high precision 6-axis robot (Stäubli TX=RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- An isotropic field probe optimized and calibrated for the targeted measurement.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion from optical to electrical signals for the digital communication to the DAE. To use optical surface detection, a special version of the EOC is required. The EOC signal is transmitted to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
- A computer running WinXP and the DASY5 software.
- Remote control and teach pendant as well as additional circuitry for robot safety such as
- warning lamps, etc.
- The phantom, the device holder and other accessories according to the targeted measurement.





C.2. DASY5 E-field Probe System

The SAR measurements were conducted with the dosimetric probe designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multifiber line ending at the front of the probe tip. It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY5 software reads the reflection durning a software approach and looks for the maximum using 2ndord curve fitting. The approach is stopped at reaching the maximum.

Probe Specifications:

Model:	ES3DV3, EX3DV4
Frequency	10MHz — 6.0GHz(EX3DV4)
Range:	10MHz — 4GHz(ES3DV3)
Calibration:	In head and body simulating tissue at
	Frequencies from 835 up to 5800MHz
Linearity:	± 0.2 dB(30 MHz to 6 GHz) for EX3DV4
	± 0.2 dB(30 MHz to 4 GHz) for ES3DV3
Dynamic Range:	10 mW/kg — 100W/kg
Probe Length:	330 mm
Probe Tip	
Length:	20 mm
Body Diameter:	12 mm
Tip Diameter:	2.5 mm (3.9 mm for ES3DV3)
Tip-Center:	1 mm (2.0mm for ES3DV3)
Application:	SAR Dosimetry Testing
	Compliance tests of mobile phones
	Dosimetry in strong gradient fields



Picture C.2 Near-field Probe



Picture C.3 E-field Probe

C.3. E-field Probe Calibration

Each E-Probe/Probe Amplifier combination has unique calibration parameters. A TEM cell calibration procedure is conducted to determine the proper amplifier settings to enter in the probe parameters. The amplifier settings are determined for a given frequency by subjecting the probe to a known E-field density (1 mW/cm²) using an RF Signal generator, TEM cell, and RF Power Meter.

The free space E-field from amplified probe outputs is determined in a test chamber. This calibration can be performed in a TEM cell if the frequency is below 1 GHz and inn a waveguide or ©Copyright. All rights reserved by SAICT Page 29 of 61





other methodologies above 1 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees until the three channels show the maximum reading. The power density readings equates to 1 mW/ cm^2 .

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The E-field in the medium correlates with the temperature rise in the dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$SAR = C \frac{\Delta T}{\Delta t}$$

Where:

 Δt = Exposure time (30 seconds), C = Heat capacity of tissue (brain or muscle), ΔT = Temperature increase due to RF exposure.

$$SAR = \frac{\left|E\right|^2 \cdot \sigma}{\rho}$$

Where: σ = Simulated tissue conductivity, ρ = Tissue density (kg/m³).

C.4. Other Test Equipment

C.4.1. Data Acquisition Electronics (DAE)

The data acquisition electronics consist of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder with a control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information, as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE is 200 MOhm; the inputs are symmetrical and floating. Common mode rejection is above 80 dB.



PictureC.4: DAE





C.4.2. Robot

The SPEAG DASY system uses the high precision robots (DASY5: RX160L) type from Stäubli SA (France). For the 6-axis controller system, the robot controller version from Stäubli is used. The Stäubli robot series have many features that are important for our application:

- High precision (repeatability 0.02mm)
- High reliability (industrial design)
- > Low maintenance costs (virtually maintenance free due to direct drive gears; no belt drives)
- > Jerk-free straight movements (brushless synchron motors; no stepper motors)
- > Low ELF interference (motor control fields shielded via the closed metallic construction shields)



Picture C.5 DASY 5

C.4.3. Measurement Server

The Measurement server is based on a PC/104 CPU broad with CPU (DASY5: 400 MHz, Intel Celeron), chipdisk (DASY5:128MB), RAM (DASY5:128MB). The necessary circuits for communication with the DAE electronic box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY I/O broad, which is directly connected to the PC/104 bus of the CPU broad.

The measurement server performs all real-time data evaluation of field measurements and surface detection, controls robot movements and handles safety operation. The PC operating system cannot interfere with these time critical processes. All connections are supervised by a watchdog, and disconnection of any of the cables to the measurement server will automatically disarm the robot and disable all program-controlled robot movements. Furthermore, the measurement server is equipped with an expansion port which is reserved for future applications. Please note that this expansion port does not have a standardized pinout, and therefore only devices provided by SPEAG can be connected. Devices from any other supplier could seriously damage the measurement server.



Picture C.6 Server for DASY 5





C.4.4. Device Holder for Phantom

The SAR in the phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source at 5mm distance, a positioning uncertainty of ± 0.5 mm would produce a SAR uncertainty of $\pm 20\%$. Accurate device positioning is therefore crucial for accurate and repeatable measurements. The positions in which the devices must be measured are defined by the standards.

The DASY device holder is designed to cope with the different positions given in the standard. It has two scales for device rotation (with respect to the body axis) and device inclination (with respect to the line between the ear reference points). The rotation centers for both scales is the ear reference point (ERP). Thus the device needs no repositioning when changing the angles.

The DASY device holder is constructed of low-loss

POM material having the following dielectric

parameters: relative permittivity ε =3 and loss tangent δ =0.02. The amount of dielectric material


has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.

<Laptop Extension Kit>

The extension is lightweight and made of POM, acrylic glass and foam. It fits easily on the upper part of the Mounting Device in place of the phone positioner. The extension is fully compatible with the Twin-SAM and ELI phantoms.



Picture C.7-1: Device Holder



Picture C.7-2: Laptop Extension Kit

C.4.5. Phantom

The SAM Twin Phantom V4.0 is constructed of a fiberglass shell integrated in a table. The shape of the shell is based on data from an anatomical study designed to

Represent the 90th percentile of the population. The phantom enables the dissymmetric evaluation of SAR for both left and right handed handset usage, as well as body-worn usage using the flat phantom region. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. The shell phantom has a 2mm shell thickness (except the ear region where shell thickness increases to 6 mm).





Shell Thickness:2 ± 0. 2 mmFilling Volume:Approx. 25 litersDimensions:810 x l000 x 500 mm (H x L x W)Available:Special



Picture C.8: SAM Twin Phantom







ANNEX D: Position of the wireless device in relation to the phantom

D.1. General considerations

This standard specifies two handset test positions against the head phantom – the "cheek" position and the "tilt" position.

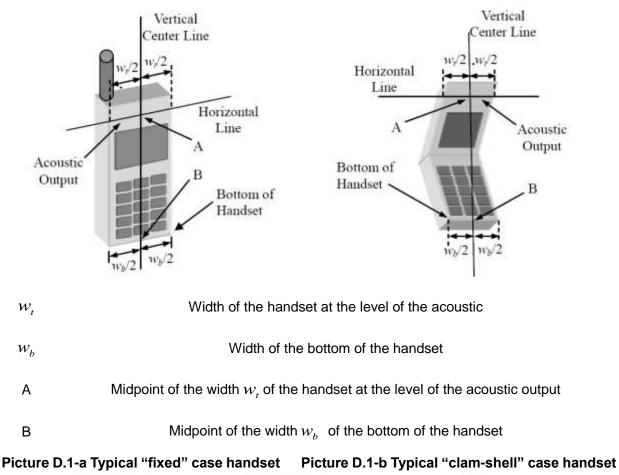


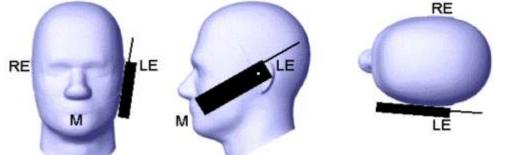

Picture D.2 Cheek position of the wireless device on the left side of SAM






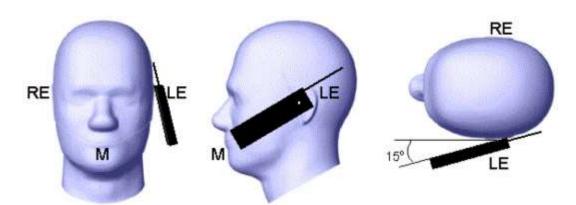

Picture D.3 Tilt position of the wireless device on the left side of SAM

D.2. Body-worn device

A typical example of a body-worn device is a mobile phone, wireless enabled PDA or other battery operated wireless device with the ability to transmit while mounted on a person's body using a carry accessory approved by the wireless device manufacturer.

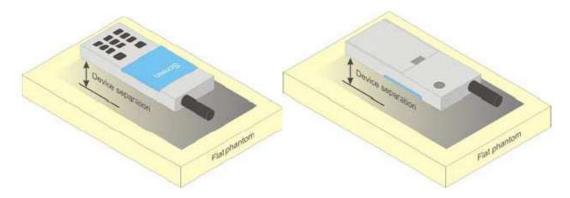

Picture D.4 Test positions for body-worn devices


D.3. Desktop device

A typical example of a desktop device is a wireless enabled desktop computer placed on a table or desk when used.

The DUT shall be positioned at the distance and in the orientation to the phantom that corresponds to the intended use as specified by the manufacturer in the user instructions. For devices that employ an external antenna with variable positions, tests shall be performed for all antenna positions specified. Picture 8.5 show positions for desktop device SAR tests. If the intended use is not specified, the device shall be tested directly against the flat phantom.





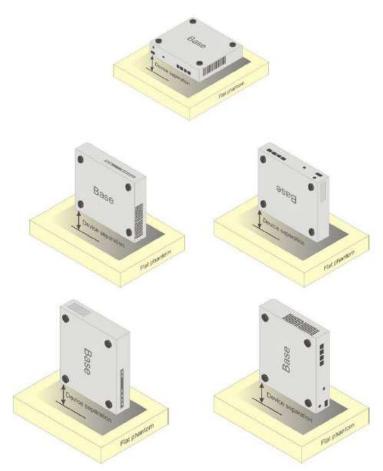

Picture D.5 Test positions for desktop devices



D.4. DUT Setup Photos

Picture D.6





ANNEX E: Equivalent Media Recipes

The liquid used for the frequency range of 700-6000 MHz consisted of water, sugar, salt, preventol, glycol monobutyl and Cellulose. The liquid has been previously proven to be suited for worst-case. The Table E.1 shows the detail solution. It's satisfying the latest tissue dielectric parameters requirements proposed by the IEEE 1528 and IEC 62209.

Frequency	835	835	1900	1900	2450	2450	5800	5800
(MHz)	Head	Body	Head	Body	Head	Body	Head	Body
Ingredients (% by	/ weight)							
Water	41.45	52.5	55.242	69.91	58.79	72.60	65.53	65.53
Sugar	56.0	45.0	١	١	١	١	١	\
Salt	1.45	1.4	0.306	0.13	0.06	0.18	١	\
Preventol	0.1	0.1	١	١	١	١	١	\
Cellulose	1.0	1.0	١	١	١	١	١	\
Glycol	1	1	44.452	29.96	41.15	27.22		
Monobutyl	ν.	١	44.452	29.90	41.15	21.22	١	\
Diethylenglycol	1	1	1	1	N	N		
monohexylether	``	١	١	١	١	١	17.24	17.24
Triton X-100	١	١	١	١	١	١	17.24	17.24
Dielectric	c=41.5	ε=55.2	ε=40.0	ε=53.3	ε=39.2	ε=52.7		
Parameters	ε=41.5 σ=0.90	ε=55.2 σ=0.97		ε=55.5 σ=1.52			ε=35.3	ε=48.2
Target Value	0-0.90	0-0.97	σ=1.40	0-1.52	σ=1.80	σ=1.95	σ=5.27	σ=6.00

Table E.1: Composition of the Tissue Equivalent Matter

Note: There is a little adjustment respectively for 750, 1800, 2600, 5200, 5300, and 5600, based on the recipe of closest frequency in table E.1





ANNEX F: System Validation

The SAR system must be validated against its performance specifications before it is deployed. When SAR probes, system components or software are changed, upgraded or recalibrated, these must be validated with the SAR system(s) that operates with such components.

Probe SN.	Liquid name	Validation date	Frequency point	Status (OK or Not)					
3633	Head 750MHz	2020-04-03	750 MHz	OK					
3633	Head 900MHz	2020-04-03	900 MHz	OK					
3633	Head 1750MHz	2020-04-03	1750 MHz	OK					
3633	Head 1900MHz	2020-04-03	1900 MHz	OK					
3633	Head 2300MHz	2020-04-04	2300 MHz	OK					
3633	Head 2450MHz	2020-04-04	2450 MHz	OK					
3633	Head 2550MHz	2020-04-04	2550 MHz	OK					
3633	Head 5200MHz	2020-04-05	5250 MHz	OK					
3633	Head 5600MHz	2020-04-05	5600 MHz	OK					
3633	Head 5750MHz	2020-04-05	5750 MHz	OK					

Table F.1: System Validation





ANNEX G: DAE Calibration Certificate

DAE4 SN: 1527 Calibration Certificate

Tell +86-10-6	2304633-2512 Fast	striet, Beijing, 100191, China 3 +86-10-62304633-2504	Madadadad		CALIBRAT CNAS L05
E-mail: ett à Client : C	TTL(South Branc	h) Cei	rtificate I	No: Z19-60419	
CALIBRATION	CERTIFICAT	TE			1.3.4
Dbject	DAE4	- SN: 1527		S-185	
Calibration Procedure(s	i)				
		1-002-01 ation Procedure for the Dat)	a Acquisit	ion Electronics	
Calibration date:	Novem	iber 11, 2019			
neasurements(SI). The pages and are part of the	measurements and e certificate.	traceability to national stands the uncertainties with confide the closed laboratory facility	nce probal	bility are given or	the following
neasurements(SI). The bages and are part of the All calibrations have t	measurements and le certificate. leen conducted in used (M&TE critical fi	the uncertainties with confide the closed laboratory facility	nce probal	bility are given or	n the following e(22±3)℃ and
neasurements(SI). The lages and are part of the salid calibrations have to umidity<70%. Calibration Equipment to	ineasurements and le certificate. leen conducted in lised (M&TE critical fi ID # Cal	the uncertainties with confide the closed laboratory facility or calibration)	nce probal r: environn te No.)	bility are given or ment temperatur	n the following e(22±3)℃ and ibration
neasurements(SI). The lages and are part of the sumidity<70%. Calibration Equipment un trimary Standards	measurements and le certificate. leen conducted in lised (M&TE critical fi ID # Cal 1971018	the uncertainties with confide the closed laboratory facility or calibration) I Date(Calibrated by, Certificat 24-Jun-19 (CTTL, No.J19X05	nce probal r: environn te No.)	bility are given or nent temperatur Scheduled Cal Jun-20	n the following e(22±3)℃ and ibration
reasurements(SI). The ages and are part of the ages and are part of the umidity<70%. alibration Equipment of rimary Standards rocess Calibrator 753	ineasurements and le certificate. leen conducted in lised (M&TE critical fi ID # Cal	the uncertainties with confide the closed laboratory facility or calibration) I Date(Calibrated by, Certificat	nce probal r: environn te No.)	bility are given or ment temperatur Scheduled Cal	n the following e(22±3)℃ and ibration
reasurements(SI). The ages and are part of the umidity<70%. alibration Equipment un rimary Standards	Name	the uncertainties with confide the closed laboratory facility or calibration) I Date(Calibrated by, Certificat 24-Jun-19 (CTTL, No.J19X05 Function	nce probal r: environn te No.)	bility are given or nent temperatur Scheduled Cal Jun-20	n the following e(22±3)℃ and ibration

Certificate No: Z19-60419

Page 1 of 3







Add: No.51 Xueywan Road, Haidian District, Beijing, 100191, China Tel: =86-10-62304633-2512 Fax: +86-10-62304633-2504 E-mail: cttl.g.chinattl.com Http://www.chinattl.cn

Glossary:

DAE Connector angle

data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters:

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.

Certificate No: Z19-60419

Page 2 of 3







Add: No.51 Xueyuun Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 E-mail: cttl/a/chinatti.com Http://www.chinatti.cn

DC Voltage Measurement

 A/D - Converter Resolution nominal High Range:
 1LSB = 6.1µV,
 full range = -100...+300 mV

 Low Range:
 1LSB = 61nV,
 full range = -1.....+3mV

 DASY measurement parameters:
 Auto Zero Time: 3 sec;
 Measuring time: 3 sec

Calibration Factors	x	Y	z
High Range	403.867 ± 0.15% (k=2)	403.590 ± 0.15% (k=2)	403.811 ± 0.15% (k=2)
Low Range	3.96119 ± 0.7% (k=2)	3.99117 ± 0.7% (k=2)	3.97030 ± 0.7% (k=2)

Connector Angle

-

P	Connector Angle to be used in DASY system	223°±1°

Certificate No: Z19-60419

Page 3 of 3





ANNEX H: Probe Calibration Certificate

Probe EX3DV4-SN: 3633 Calibration Certificate

Add: No.51 Xuey			CNAS LO
Tel: +86-10-6230 E-mail: ent@ehit		6-10-62304633-2504 www.chimattl.cn	
Client CTT	L(South Branch		Z20-60108
CALIBRATION	ERTIFICAT		1000
Object	EX3DV4	- SN : 3633	Cont .
Calibration Procedure(s)	FF-Z11- Calibrat	004-01 on Procedures for Dosimetric E-field Probes	
Calibration date:	April 01.		
pages and are part of the	certificate.	he uncertainties with confidence probability ar	
All calibrations have be humidity<70%. Calibration Equipment use	certificate. an conducted in t ad (M&TE critical fo	ne closed laboratory facility: environment to r calibration)	emperature(22±3)℃ and
All calibrations have be humidity<70%. Calibration Equipment use Primary Standards	certificate. en conducted in t ed (M&TE critical fo ID #	ne closed laboratory facility: environment to r calibration) Cal Date(Calibrated by, Certificate No.)	emperature(22±3) C and Scheduled Calibration
All calibrations have be humidity<70%. Calibration Equipment use Primary Standards Power Meter NRP2	certificate. en conducted in t ed (M&TE critical fo ID # 101919	he closed laboratory facility: environment to r calibration) Cal Date(Calibrated by, Certificate No.) 18-Jun-19(CTTL, No.J19X05125)	emperature(22±3)℃ and Scheduled Calibration Jun-20
All calibrations have be humidity<70%. Calibration Equipment use Primary Standards Power Meter NRP2 Power sensor NRP-Z9	certificate. en conducted in t ed (M&TE critical fo ID # 101919 1 01547	he closed laboratory facility: environment to r calibration) Cal Date(Calibrated by, Certificate No.) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125)	emperature(22±3)℃ and Scheduled Calibration Jun-20 Jun-20
All calibrations have be humidity<70%. Calibration Equipment use Primary Standards Power Meter NRP2	certificate. en conducted in t ed (M&TE critical fo ID # 101919 1 010547 1 01548	he closed laboratory facility: environment to r calibration) Cal Date(Calibrated by, Certificate No.) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125)	emperature(22±3)℃ and Scheduled Calibration Jun-20
All calibrations have ber humidity<70%. Calibration Equipment use Primary Standards Power Meter NRP2 Power sensor NRP-29 Power sensor NRP-29	certificate. en conducted in t ed (M&TE critical fo ID # 101919 1 101547 1 101548 ator 18N50W-10	he closed laboratory facility: environment to r calibration) Cal Date(Calibrated by, Certificate No.) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125)	emperature(22±3)℃ and Scheduled Calibration Jun-20 Jun-20 Jun-20
All calibrations have ber humidity<70%. Calibration Equipment use Primary Standards Power Meter NRP2 Power sensor NRP-29 Power sensor NRP-29 Reference 10dBAttenu	certificate. en conducted in t ed (M&TE critical fo ID # 101919 1 101547 1 101548 ator 18N50W-10 ator 18N50W-20	he closed laboratory facility: environment to r calibration) Cal Date(Calibrated by, Certificate No.) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J20X00525) 10B 10-Feb-20(CTTL, No.J20X00526) 24-May-19(SPEAG, No.EX3-7307_May1	emperature(22±3)℃ and Scheduled Calibration Jun-20 Jun-20 Jun-20 Feb-22 Feb-22 Feb-22 9/2) May-20
All calibrations have been humidity<70%. Calibration Equipment use Primary Standards Power Meter NRP2 Power sensor NRP-29 Power sensor NRP-29 Reference 10dBAttenu Reference 20dBAttenu Reference Probe EX30 DAE4	certificate. en conducted in t ed (M&TE critical fo ID # 101919 1 101547 1 101548 ator 18N50W-10 ator 18N50W-20 IV4 SN 7307 SN 1525	he closed laboratory facility: environment to r calibration) Cal Date(Calibrated by, Certificate No.) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J20X00525) dB 10-Feb-20(CTTL, No.J20X00526) 24-May-19(SPEAG, No.DAE4-1525_Aug	emperature(22±3)℃ and Jun-20 Jun-20 Jun-20 Feb-22 Feb-22 Feb-22 9/2) May-20 (19) Aug-20
All calibrations have been humidity<70%. Calibration Equipment use Primary Standards Power Meter NRP2 Power sensor NRP-Z9 Power sensor NRP-Z9 Power sensor NRP-Z9 Reference 10dBAttenu Reference 20dBAttenu Reference Probe EX3E DAE4 Secondary Standards	certificate. en conducted in t ed (M&TE critical fo ID # 101919 1 101547 1 101548 ator 18N50W-10 ator 18N50W-20 IV4 SN 7307 SN 1525 ID #	he closed laboratory facility: environment to r calibration) Cal Date(Calibrated by, Certificate No.) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J20X00525) 24-May-19(SPEAG, No.EX3-7307_May1 26-Aug-19(SPEAG, No.DAE4-1525_Aug Cel Date(Calibrated by, Certificate No.)	emperature(22±3)℃ and Jun-20 Jun-20 Jun-20 Feb-22 Feb-22 9/2) May-20 (19) Aug-20 Scheduled Calibration
All calibrations have been humidity<70%. Calibration Equipment use Primary Standards Power Meter NRP2 Power sensor NRP-29 Power sensor NRP-29 Reference 10dBAttenu Reference 20dBAttenu Reference Probe EX30 DAE4	certificate. en conducted in ti ed (M&TE critical fo ID # 101919 1 101547 1 101548 ator 18N50W-10 ator 18N50W-20 IV4 SN 7307 SN 1525 ID # 10.4 2000 620105260	he closed laboratory facility: environment to r calibration) Cal Date(Calibrated by, Certificate No.) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J20X00525) dB 10-Feb-20(CTTL, No.J20X00526) 24-May-19(SPEAG, No.EX3-7307_May1 26-Aug-19(SPEAG, No.DAE4-1525_Aug Cel Date(Calibrated by, Certificate No.) 5 18-Jun-19(CTTL, No.J19X05127)	emperature(22±3)℃ and Jun-20 Jun-20 Jun-20 Feb-22 Feb-22 Feb-22 9/2) May-20 (19) Aug-20
All calibrations have been humidity<70%. Calibration Equipment use Primary Standards Power Meter NRP2 Power sensor NRP-Z9 Power sensor NRP-Z9 Power sensor NRP-Z9 Reference 10dBAttenu Reference 20dBAttenu Reference Probe EX3E DAE4 Secondary Standards SignalGenerator MG37	certificate. en conducted in ti ed (M&TE critical fo ID # 101919 1 101547 1 101548 ator 18N50W-10 ator 18N50W-20 IV4 SN 7307 SN 1525 ID # 10.4 2000 620105260	he closed laboratory facility: environment to r calibration) Cal Date(Calibrated by, Certificate No.) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J20X00525) dB 10-Feb-20(CTTL, No.J20X00526) 24-May-19(SPEAG, No.EX3-7307_May1 26-Aug-19(SPEAG, No.DAE4-1525_Aug Cel Date(Calibrated by, Certificate No.) 5 18-Jun-19(CTTL, No.J19X05127)	emperature(22±3)℃ and Jun-20 Jun-20 Jun-20 Feb-22 Feb-22 9/2) May-20 (19) Aug-20 Scheduled Calibration Jun-20
All calibrations have ber humidity<70%. Calibration Equipment use Primary Standards Power Meter NRP2 Power sensor NRP-Z9 Power sensor NRP-Z9 Power sensor NRP-Z9 Reference 10dBAttenu Reference 20dBAttenu Reference Probe EX3E DAE4 Secondary Standards SignalGenerator MG37	certificate. en conducted in ti ed (M&TE critical fo ID # 101919 1 101547 1 101547 1 101548 ator 18N50W-10 ator 18N50W-20 IV4 SN 7307 SN 1525 ID # 00A 620105260 1C MY4611067	he closed laboratory facility: environment to r calibration) Cal Date(Calibrated by, Certificate No.) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J20X00525) 10-Feb-20(CTTL, No.J20X00526) 24-May-19(SPEAG, No.EX3-7307_May1 26-Aug-19(SPEAG, No.DAE4-1525_Aug Cel Date(Calibrated by, Certificate No.) 5 18-Jun-19(CTTL, No.J19X05127) 3 10-Feb-20(CTTL, No.J20X00515)	emperature(22±3)℃ and Jun-20 Jun-20 Jun-20 Feb-22 Feb-22 9/2) May-20 (19) Aug-20 Scheduled Calibration Jun-20 Feb-21
All calibrations have been humidity<70%. Calibration Equipment use Primary Standards Power Meter NRP2 Power sensor NRP-Z9 Power sensor NRP-Z9 Power sensor NRP-Z9 Reference 10dBAttenu Reference 20dBAttenu Reference Probe EX3E DAE4 Secondary Standards SignalGenerator MG37 Network Analyzer E507	certificate. en conducted in ti ed (M&TE critical fo ID # 101919 1 101547 1 101547 1 101548 ator 18N50W-20 IV4 SN 7307 SN 1525 ID # 00A 620105260 1C MY4611067 Name	he closed laboratory facility: environment to r calibration) Cal Date(Calibrated by, Certificate No.) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J19X05125) 18-Jun-19(CTTL, No.J20X00525) 10B 10-Feb-20(CTTL, No.J20X00526) 24-May-19(SPEAG, No.DAE4-1525_Aug Cel Date(Calibrated by, Certificate No.) 5 18-Jun-19(CTTL, No.J19X05127) 3 10-Feb-20(CTTL, No.J20X00515) Function	emperature(22±3)℃ and Jun-20 Jun-20 Jun-20 Feb-22 Feb-22 9/2) May-20 (19) Aug-20 Scheduled Calibration Jun-20 Feb-21

Certificate No: Z20-60108

Page 1 of 10





	TLspe	a g
Add: No.51	CALIBRATION LAS Xueyuan Road, Haidian District, Beij	
Tel: +86-10-	62304633-2512 Fax: +86-10-62 Behinattil.com Http://www.chi	2304633-2504
Glossary:		
TSL	tissue simulating liquid	
NORMx,y,z	sensitivity in free space	
ConvF	sensitivity in TSL / NORM	x,y,z
DCP CF	diode compression point	- Star DE - La
A.B.C.D	crest factor (1/duty_cycle) modulation dependent line	
Polarization Φ	Φ rotation around probe a	
Polarization 0		that is in the plane normal to probe axis (at measurement center)
Connector Angle	information used in DASY	system to align probe sensor X to the robot coordinate system
Calibration is	Performed According to	the Following Standards:
a) IEEE Std 15.	28-2013, "IEEE Recommer	nded Practice for Determining the Peak Spatial-Averaged
Specific Abso	rption Rate (SAR) in the	Human Head from Wireless Communications Devices:
	Techniques", June 2013	as the assessment of Country of C
hand-hald and	body-mounted devices	or the assessment of Specific Absorption Rate (SAR) from ad next to the ear (frequency range of 300 MHz to 6 GHz)",
July 2016	wwwy-mounted devices use	the next to the ear (frequency range of 300 MHz to 6 GHz)",
	Procedure to determine the	Specific Absorption Rate (SAR) for wireless communication
devices used 2010	in close proximity to the hu	iman body (frequency range of 30 MHz to 6 GHz)", March
d) KDB 865664,	*SAR Measurement Require	ements for 100 MHz to 6 GHz"
Methods Appli	ed and Interpretation of	Parameters:
 NORMx, y, z: 	Assessed for E-field polarization	ation θ=0 (f≤900MHz in TEM-cell; f>1800MHz; waveguide).
		, i.e., the uncertainties of NORMx,y,z does not effect the
E^{2} -field und	ertainty inside TSL (see belo	ow ConvF).
 NORM(I)x,y, 	z = NORMx,y,z* frequency_	response (see Frequency Response Chart). This
linearization	is implemented in DASY4 s	oftware versions later than 4.2. The uncertainty of the
 DCPx.v.z: D 	sponse is included in the sta	ated uncertainty of ConvF.
 (no uncertain 	ty required) DCP does not	on parameters assessed based on the data of power sweep depend on frequency nor media.
 PAR: PAR is 	the Peak to Average Ratio	that is not calibrated but determined based on the signal
characteristi	CS.	and to the semicined part determined pased on the signal
 Ax, y, z; Bx, y, 	z; Cx,y,z;VRx,y,z:A,B,C are	numerical linearization parameters assessed based on the
data of powe	r sweep for specific modula	tion signal. The parameters do not depend on frequency nor
media. VR is	the maximum calibration ra	ange expressed in RMS voltage across the diode
 ConvF and L 	Joundary Effect Parameters	Assessed in flat phantom using E-field (or Temperature
Transfer Sta	ndard for f≤800MHz) and ins	side waveguide using analytical field distributions based on
power meas	urements for f >800MHz. Th	e same setups are used for assessment of the parameters
These paras	teters are used in DASVA -	ha, depth) of which typical uncertainty valued are given. oftware to improve probe accuracy close to the boundary.
The sensitivi	ty in TSL corresponds to Nr	DRMx,y.z* ConvF whereby the uncertainty corresponds to
that given fo	ConvF. A frequency depen	dent ConvF is used in DASY version 4.4 and higher which
allows exten	ding the validity from±50MH	Iz to±100MHz.
 Spherical iso 	stropy (3D deviation from iso	stropy): in a field of low gradients realized using a flat
phantom exp	losed by a patch antenna.	
 Sensor Offse 	t. The sensor offset corresp	oonds to the offset of virtual measurement center from the
Galessanty	probe axis). No tolerance re	
probe tip (on	makes which a support the second second	
 probe tip (on Connector A 	ngle: The angle is assessed ity required).	l using the information gained by determining the NORMx







E-mail: cttl@chinattl.com Http://www.chinattl.cn

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3633

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm(µV/(V/m)2)^	0.37	0.37	0.39	±10.0%
DCP(mV) ^B	98.2	98.8	98.0	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dBõV	c	D dB	VR mV	Unc ^E (k=2)
0 CW	CW	X	0.0	0.0	1.0	0.00	141.5	±2.3%
		Y	0.0	0.0	1.0		141.5	
		Z	0.0	0.0	1.0		141.9	

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X, Y, Z do not affect the E²-field uncertainty inside TSL (see Page 4 and Page 5).

⁸ Numerical linearization parameter: uncertainty not required.

E Uncertainly is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No:Z20-60108

Page 3 of 10







DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3633

Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz] ^c	Relative Permittivity ⁷	Conductivity (S/m) [∓]	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	41.9	0.89	9.59	9.59	9.59	0.40	0.75	±12.1%
900	41.5	0.97	9.33	9.33	9.33	0.21	1.14	±12.1%
1640	40.3	1.29	8.17	8.17	8.17	0.16	1.22	±12.1%
1750	40.1	1.37	8.09	8.09	8.09	0.15	1.42	±12.1%
1900	40.0	1.40	7.76	7.76	7.76	0.19	1.14	±12.1%
2100	39.8	1.49	7.73	7.73	7.73	0.18	1.26	±12.1%
2300	39.5	1.67	7.69	7.69	7.69	0.48	0.78	±12.1%
2450	39.2	1.80	7.43	7.43	7.43	0.50	0.77	±12.1%
2600	39.0	1.96	7.20	7.20	7.20	0.58	0.72	±12.1%
3500	37.9	2.91	6.88	6.88	6.88	0.35	1.23	±13.3%
3700	37.7	3.12	6.57	6.57	6.57	0.44	0.98	±13.3%
3900	37.5	3.32	6.51	6.51	6.51	0.35	1.40	±13.3%
4100	37.2	3.53	6.44	6.44	6.44	0.40	1.20	±13.3%
4400	36.9	3.84	6.30	6.30	6.30	0.35	1.35	±13.3%
4600	36.7	4.04	6.10	6.10	6.10	0.45	1.40	±13.3%
4800	36.4	4.25	5.98	5.98	5.98	0.45	1.60	±13.3%
4950	36.3	4.40	5.80	5.80	5.80	0.45	1.45	±13.3%
5250	35.9	4.71	5.47	5.47	5.47	0.45	1.25	±13.3%
5600	35.5	5.07	4.72	4.72	4.72	0.45	1.50	±13.3%
5750	35.4	5.22	4.73	4.73	4.73	0.45	1.50	±13.3%

^C Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±60MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequency below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters. ^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No:Z20-60108

Page 4 of 10







DASY/EASY – Parameters of Probe: EX3DV4 – SN: 3633

Calibration Parameter Determined in Body Tissue Simulating Media

f [MHz]°	Relative Permittivity ^r	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ⁶	Depth ³ (mm)	Unct. (k=2)
750	55.5	0.96	9.57	9.57	9.57	0.40	0.80	±12.1%
900	55.0	1.05	9.34	9.34	9.34	0.25	1.11	±12.1%
1640	53.8	1.40	8.05	8.05	8.05	0.22	1.19	±12.1%
1750	53.4	1.49	7.85	7.85	7.85	0.16	1.35	±12.1%
1900	53.3	1.52	7.66	7.66	7.66	0.17	1.32	±12.1%
2100	53.2	1.62	7.69	7.69	7.69	0.21	1.30	±12.1%
2300	52.9	1.81	7.61	7.61	7.61	0.50	0.86	±12.1%
2450	52.7	1.95	7.56	7.56	7.56	0.50	0.83	±12.1%
2600	52.5	2.16	7.33	7.33	7.33	0.59	0.74	±12.1%
3500	52.3	3.31	6.28	6.28	6.28	0.40	1.30	±13.3%
3700	52.1	3.55	6.14	6.14	6.14	0.40	1.35	±13.3%
3900	50.8	3.78	6.13	6.13	6.13	0.40	1.45	±13.3%
4100	50.5	4.01	6.12	6.12	6.12	0.35	1.40	±13.3%
4400	50.1	4.37	5.93	5.93	5.93	0.35	1.70	±13.3%
4600	49.8	4.60	5.60	5.60	5.60	0.45	1.50	±13.3%
4800	49.6	4.83	5.42	5.42	5.42	0.45	1.60	±13.3%
4950	49.4	5.01	5.22	5.22	5.22	0.45	1.70	±13.3%
5250	48.9	5.36	5.04	5.04	5.04	0.50	1.45	±13.3%
5600	48.5	5.77	4.16	4.16	4.16	0.55	1.50	±13.3%
5750	48.3	5.94	4.26	4.26	4.26	0.55	1.60	±13.3%

^G Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


* At frequency below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters. ^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No:Z20-60108

Page 5 of 10






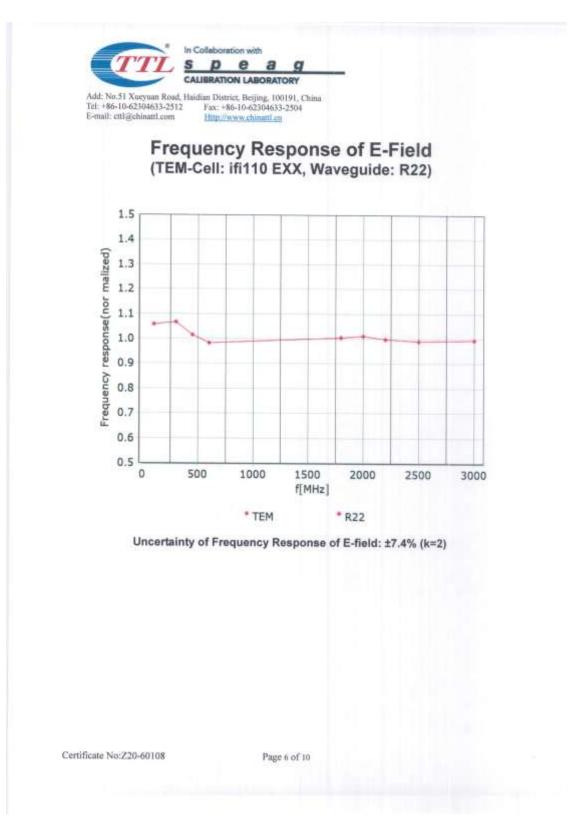






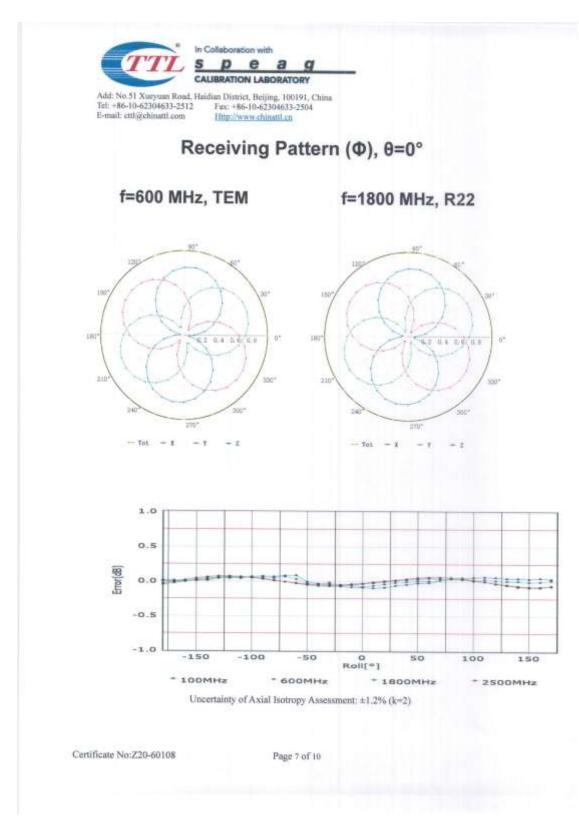






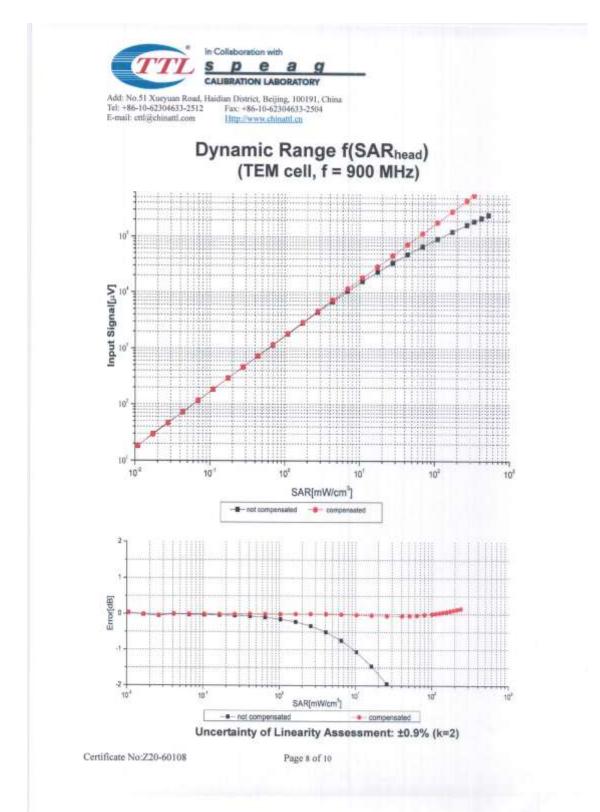





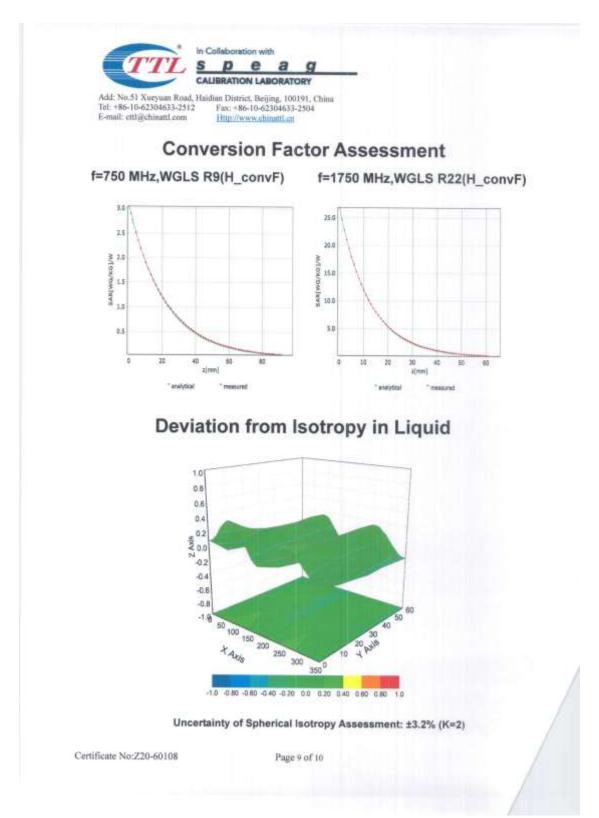







DASY/EASY - Parameters of Probe: EX3DV4 - SN:3633

Other Probe Parameters

Sensor Arrangement	Triangular	
Connector Angle (°)	71.2	
Mechanical Surface Detection Mode	enabled	
Optical Surface Detection Mode	disable	
Probe Overall Length	337mm	
Probe Body Diameter	10mm	
Tip Length	10mm	
Tip Diameter	2.5mm	
Probe Tip to Sensor X Calibration Point	1mm	
Probe Tip to Sensor Y Calibration Point	1mn	
Probe Tip to Sensor Z Calibration Point	1mm	
Recommended Measurement Distance from Surface	1.4mm	

Certificate No:Z20-60108

Page 10 of 10





ANNEX I: Dipole Calibration Certificate

2450 MHz Dipole Calibration Certificate

			C	NAS	
Tel: +86-10-62304/ F-muil: ettl.å.ehina	633-2079 Fax:+ ttl.com http://	strict, Beijing, 100191, China 866-10-62304633-2504 www.chinattl.cn		-	CALIBRATIC CNAS L057
Client CTTI	L(South Bran	ch) Certificate No:	Z18	8-60388	
CALIBRATION C	ERTIFICAT	TE			
Dbject	D2450	V2 - SN: 873			
Calibration Procedure(s)	FF-Z11	-003-01			
		tion Procedures for dipole validation kits	s		
Calibration date:	Octobe	er 26, 2018			
ages and are part of the ce	ertificate.				
All calibrations have been iumidity<70%. Calibration Equipment used		the closed laboratory facility: environ	ment	temperature(22±3)℃ and
umidity<70%. Calibration Equipment used	(M&TE critical fr	or calibration)			
umidity<70%. Calibration Equipment used Primary Standards		or calibration) Cal Date(Calibrated by, Certificate No		Scheduled	Calibration
umidity<70%. Calibration Equipment used Primary Standards Power Meter NRVD	(M&TE critical fr	or calibration)		Scheduled	
umidity<70%. Calibration Equipment used Primary Standards Power Meter NRVD Power sensor NRV-25 Reference Probe EX3DV4	(M&TE critical fr ID # 102083 100542	Cal Date(Calibrated by, Certificate No 01-Nov-17 (CTTL, No.J17X08756)	ə.)	Scheduled Oct	Calibration
umidity<70%. Calibration Equipment used Primary Standards Power Meter NRVD Power sensor NRV-25 Reference Probe EX3DV4	(M&TE critical fr ID # 102083 100542	Cal Date(Calibrated by, Certificate No 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756)	a.) g18)	Scheduled Oct Oct Aug	Calibration t-18
iumidity<70%	ID # 102083 100542 SN 7514	Cal Date(Calibrated by, Certificate No 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 27-Aug-18(SPEAG,No.EX3-7514_Aug	a.) g18) ug18)	Scheduled Oct Oct Aug	Calibration 1-18 1-18 3-19 3-19
umidity<70%. Calibration Equipment used rimary Standards Power Meter NRVD Power sensor NRV-Z5 Reference Probe EX3DV4 DAE4	(M&TE critical fi 1D # 102083 100542 SN 7514 SN 1555	Cal Date(Calibrated by, Certificate No 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 27-Aug-18(SPEAG,No.EX3-7514_Aug 20-Aug-18(SPEAG,No.DAE4-1555_Au	a.) g18) ug18)	Scheduled Oct Oct Aug Aug	Calibration t-18 t-18 g-19 g-19 Calibration
umidity<70%. Calibration Equipment used rimary Standards Power Meter NRVD Power sensor NRV-Z5 Reference Probe EX3DV4 DAE4 Secondary Standards	(M&TE critical fi 102083 100542 SN 7514 SN 1555 ID #	Cal Date(Calibrated by, Certificate No 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 27-Aug-18(SPEAG,No.EX3-7514_Aug 20-Aug-18(SPEAG,No.DAE4-1555_Au Cal Date(Calibrated by, Certificate No	a.) g18) ug18)	Scheduled Oct Oct Aug Scheduled	Calibration t-18 t-18 g-19 g-19 Calibration -19
umidity<70%. Calibration Equipment used Primary Standards Power Meter NRVD Power sensor NRV-25 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	(M&TE critical fr ID # 102083 100542 SN 7514 SN 1555 ID # MY49071430	Cal Date(Calibrated by, Certificate No 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 27-Aug-18(SPEAG,No.EX3-7514_Aug 20-Aug-18(SPEAG,No.DAE4-1555_Au Cal Date(Calibrated by, Certificate No. 23-Jan-18 (CTTL, No.J18X00560) 24-Jan-18 (CTTL, No.J18X00561)	a.) g18) ug18)	Scheduled Oct Oct Aug Scheduled Jan Jan	Calibration t-18 t-18 g-19 g-19 Calibration -19 -19
umidity<70%. Calibration Equipment used Primary Standards Power Meter NRVD Power sensor NRV-25 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	(M&TE critical fr ID # 102083 100542 SN 7514 SN 1555 ID # MY49071430 MY46110673	Cal Date(Calibrated by, Certificate No 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 27-Aug-18(SPEAG,No.EX3-7514_Aug 20-Aug-18(SPEAG,No.DAE4-1555_Au Cal Date(Calibrated by, Certificate No 23-Jan-18 (CTTL, No.J18X00560)	a.) g18) ug18)	Scheduled Oct Oct Aug Scheduled Jan	Calibration t-18 t-18 g-19 g-19 Calibration -19 -19
umidity<70%. Calibration Equipment used Primary Standards Power Meter NRVD Power sensor NRV-25 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	(M&TE critical fi 102083 100542 SN 7514 SN 1555 ID # MY49071430 MY46110673 Name	Cal Date(Calibrated by, Certificate No 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 27-Aug-18(SPEAG,No.EX3-7514_Aug 20-Aug-18(SPEAG,No.DAE4-1555_Au Cal Date(Calibrated by, Certificate No 23-Jan-18 (CTTL, No.J18X00560) 24-Jan-18 (CTTL, No.J18X00561) Function	a.) g18) ug18)	Scheduled Oct Oct Aug Scheduled Jan Jan	Calibration t-18 t-18 g-19 g-19 Calibration -19 -19

Certificate No: Z18-60388

Page 1 of a







Add: No.51 Xueyunn Roud, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304653-2504 E-mail: ettl@chinattl.com http://www.chinattl.en

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORMx,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- d) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z18-60388

Page 2 of 8







 Add: No.51 Xueyman Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2079
 Fax: +86-10-62304633-2504

 E-mail: ettl archinattl.com
 http://www.chinattl.cn

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.2.1495
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

g

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permitti	vity	Conductivity	
Nominal Head TSL parameters	22.0 °C	39.2		1.80 mho/m	
Measured Head TSL parameters	(22.0 ± 0.2) *C	39.2±0	5.%	1.80 mha/m ± 6 %	
Head TSL temperature change during test	<1.0 °C	0.02		-	
R result with Head TSL		-	11	1	
SAR averaged over 1 $\ cm^3$ (1 g) of Head TSL	Cond	ition			
SAR measured	250 mW i	nput power		13.0 mW / g	
SAR for nominal Head TSL parameters	normaliz	ed to 1W	52.0	mW /g ± 18.8 % (k=2)	
SAR averaged over 10 cm3 (10 g) of Head TS	SL Cond	ition			
SAR measured	250 mW i	nput power		6.02 mW / g	
SAR for nominal Head TSL parameters	normaliz	wt of be	24.1	mW /g ± 18.7 % (k=2)	

Body TSL parameters The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.8 ± 6 %	2.01 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C	100	

SAR result with Body TSL

SAR averaged over 1 cm3 (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.8 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	50.5 mW /g ± 18.8 % (k=2)
SAR averaged over 10 cm3 (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	5.91 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	23.5 mW /g ± 18.7 % (k=2)

Certificate No: Z18-60388

Page 3 of 8







Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.5Q+ 2.11 jQ
Return Loss	- 28.0dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	51.3Q+ 4,51 jQ		
Return Loss	- 26.7dB		

General Antenna Parameters and Design

1.024 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
manadalica of	OFENG

Certificate No: Z18-60388

Page 4 of 8







Add: No.51 Nueyuan Road, Haidian District, Beijing, 100191, China Tel: =86-10-62304633-2079 Fax: =86-10-62304633-2504 E-mail: crtl/g.chinattl.com http://www.chinattl.cn

Date: 10.26.2018

DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China


DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 873

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz; σ = 1.802 S/m; ϵ_e = 39.2; ρ = 1000 kg/m3 Phantom section: Right Section DASY5 Configuration:

- Probe: EX3DV4 SN7514; ConvF(6.95, 6.95, 6.95) @ 2450 MHz; Calibrated: 8/27/2018
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1555; Calibrated: 8/20/2018
- Phantom: MFP_V5.1C ; Type: QD 000 P51CA; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (2); SEMCAD X Version 14.6.12 (7450)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 105.0 V/m; Power Drift = 0.09 dB Peak SAR (extrapolated) = 26.8 W/kg SAR(1 g) = 13 W/kg; SAR(10 g) = 6.02 W/kg Maximum value of SAR (measured) = 21.8 W/kg

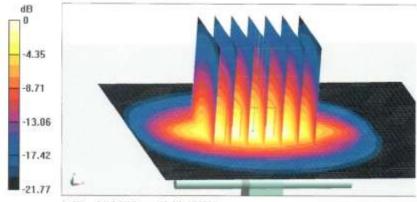

0 dB = 21.8 W/kg = 13.38 dBW/kg

Certificate No: Z18-60388

Page 5 of 8








Add: No.51 Xueyuan Road, Haidinn District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ettl.ar.ehinatti.com http://www.chinatti.en

Impedance Measurement Plot for Head TSL

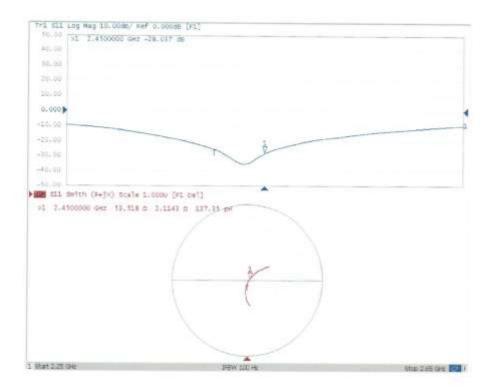

Certificate No: Z18-60388

Page 6 of 8







Add: No.51 Nueyuan Road, Ilaidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2564 E-mail: cttl.g-chinattl.con http://www.chinattl.cn

DASY5 Validation Report for Body TSL

Test Laboratory: CTTL, Beijing, China

Date: 10.26.2018

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 873 Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz; $\sigma = 2.008$ S/m; $\epsilon_r = 52.76$; $\rho = 1000$ kg/m3 Phantom section: Center Section


DASY5 Configuration:

- Probe: EX3DV4 SN7514; ConvF(7.13, 7.13, 7.13) @ 2450 MHz; Calibrated: 8/27/2018
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1555; Calibrated: 8/20/2018
- Phantom: MFP_V5.1C ; Type: QD 000 P51CA; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (2); SEMCAD X Version 14.6.12 (7450)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

```
Reference Value = 98.89 V/m; Power Drift = -0.03 dB
Peak SAR (extrapolated) = 26.4 W/kg
```

SAR(1 g) = 12.8 W/kg; SAR(10 g) = 5.91 W/kg Maximum value of SAR (measured) = 21.3 W/kg

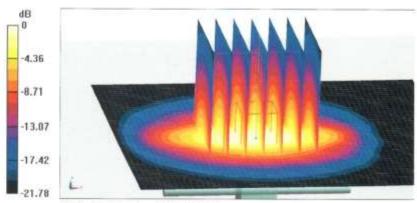

0 dB = 21.3 W/kg = 13.28 dBW/kg

Certificate No: Z18-60388

Page 7 of 8








Add: No.51 Xueyunn Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fac: +86-10-62304633-2504 E-mail: ettl@chinattl.com http://www.chinattl.cn

Impedance Measurement Plot for Body TSL

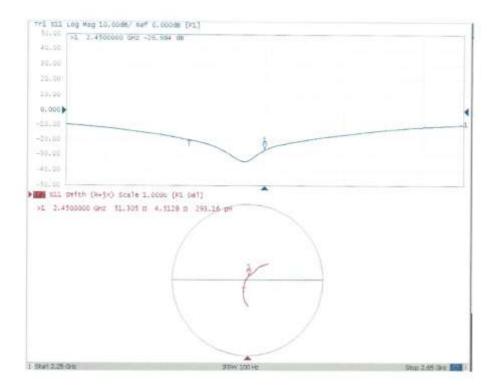

Certificate No: Z18-60388

Page 8 of 8





ANNEX J: Extended Calibration SAR Dipole

Referring to KDB865664 D01, if dipoles are verified in return loss (<-20dBm, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Justification of Extended Calibration SAR Dipole D2450V2- serial no. 873


Head						
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Imaginary Impedance (johm)	Delta (johm)
2018-10-26	-28.0	/	53.5	/	2.11	/
2019-10-22	-27.3	2.5	54.4	0.9	2.29	0.18

The Return-Loss is <-20dB, and within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the value result should support extended cabration.





ANNEX K: Accreditation Certificate

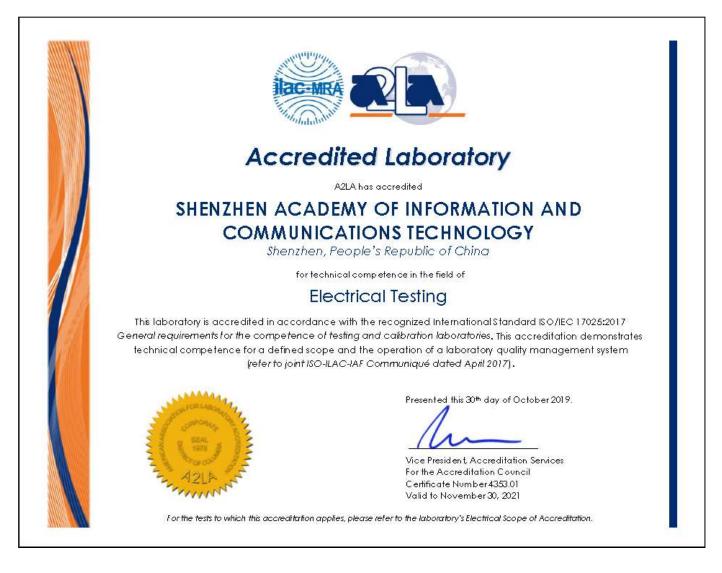

END OF REPORT