

Idle Charger CBA0059AGAC7:

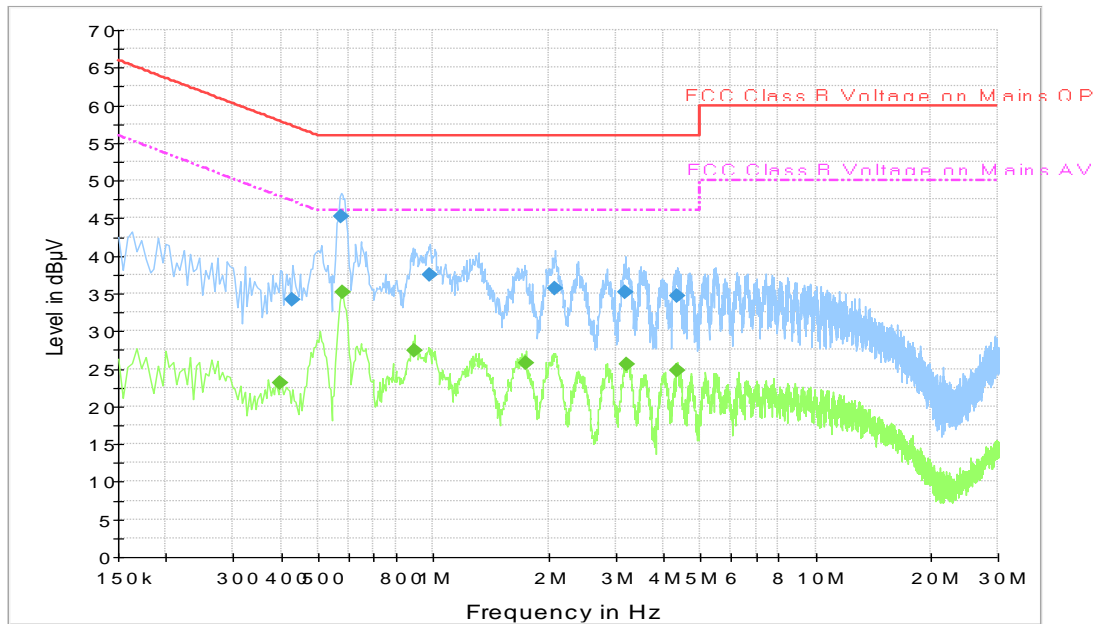


Fig.A.7.3 Conducted Emission

Final Result 1

| Frequency (MHz) | QuasiPeak (dBµV) | Meas. Time (ms) | Bandwidth (kHz) | Filter | Line | Corr. (dB) | Margin (dB) | Limit (dBµV) |
|-----------------|------------------|-----------------|-----------------|--------|------|------------|-------------|--------------|
| 0.429000 | 34.2 | 2000.0 | 9.000 | On | L1 | 19.9 | 23.0 | 57.3 |
| 0.573000 | 45.2 | 2000.0 | 9.000 | On | L1 | 19.9 | 10.8 | 56.0 |
| 0.982500 | 37.4 | 2000.0 | 9.000 | On | L1 | 19.6 | 18.6 | 56.0 |
| 2.085000 | 35.6 | 2000.0 | 9.000 | On | L1 | 19.7 | 20.4 | 56.0 |
| 3.187500 | 35.2 | 2000.0 | 9.000 | On | L1 | 19.7 | 20.8 | 56.0 |
| 4.348500 | 34.7 | 2000.0 | 9.000 | On | L1 | 19.6 | 21.3 | 56.0 |

Final Result 2

| Frequency (MHz) | Average (dBµV) | Meas. Time (ms) | Bandwidth (kHz) | Filter | Line | Corr. (dB) | Margin (dB) | Limit (dBµV) |
|-----------------|----------------|-----------------|-----------------|--------|------|------------|-------------|--------------|
| 0.397500 | 23.1 | 2000.0 | 9.000 | On | L1 | 19.9 | 24.8 | 47.9 |
| 0.577500 | 35.1 | 2000.0 | 9.000 | On | L1 | 19.9 | 10.9 | 46.0 |
| 0.892500 | 27.4 | 2000.0 | 9.000 | On | L1 | 19.7 | 18.6 | 46.0 |
| 1.747500 | 25.8 | 2000.0 | 9.000 | On | L1 | 19.7 | 20.2 | 46.0 |
| 3.210000 | 25.6 | 2000.0 | 9.000 | On | L1 | 19.7 | 20.4 | 46.0 |
| 4.353000 | 24.8 | 2000.0 | 9.000 | On | L1 | 19.6 | 21.2 | 46.0 |

ANNEX B: Accreditation Certificate

United States Department of Commerce
National Institute of Standards and Technology

NVLAP[®]

Certificate of Accreditation to ISO/IEC 17025:2005

NVLAP LAB CODE: 600118-0


Telecommunication Technology Labs, CAICT
Beijing
China


*is accredited by the National Voluntary Laboratory Accreditation Program for specific services,
listed on the Scope of Accreditation, for:*

Electromagnetic Compatibility & Telecommunications

*This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2005.
This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory quality
management system (refer to joint ISO-ILAC-IAF Communique dated January 2009).*

2017-08-22 through 2018-09-30
Effective Dates




For the National Voluntary Laboratory Accreditation Program

END OF REPORT