




Appendix D







Photographs

| |
|--|
| 1. SAR measurement System |
| 2. Photographs of Tissue Simulate Liquid |
| 3. Photographs of EUT test position |
| 4. EUT Constructional Details |



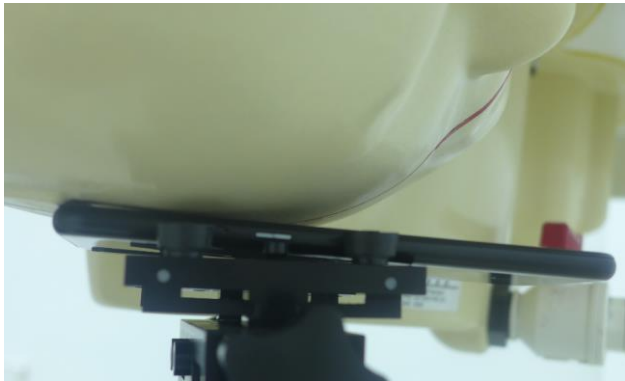
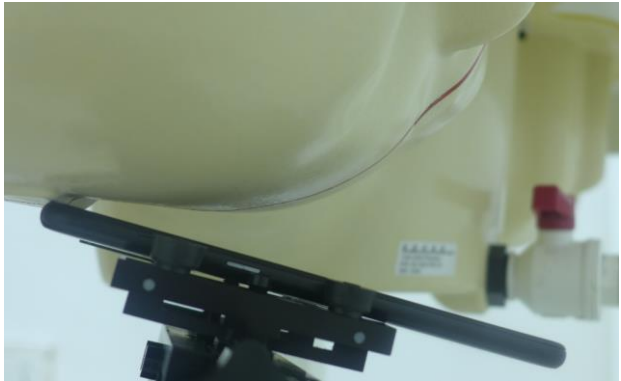
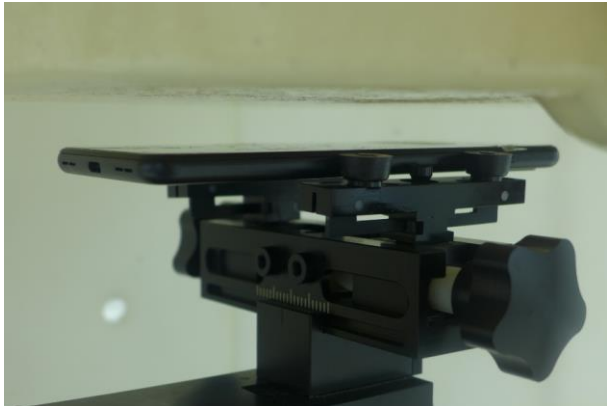

1. SAR measurement System

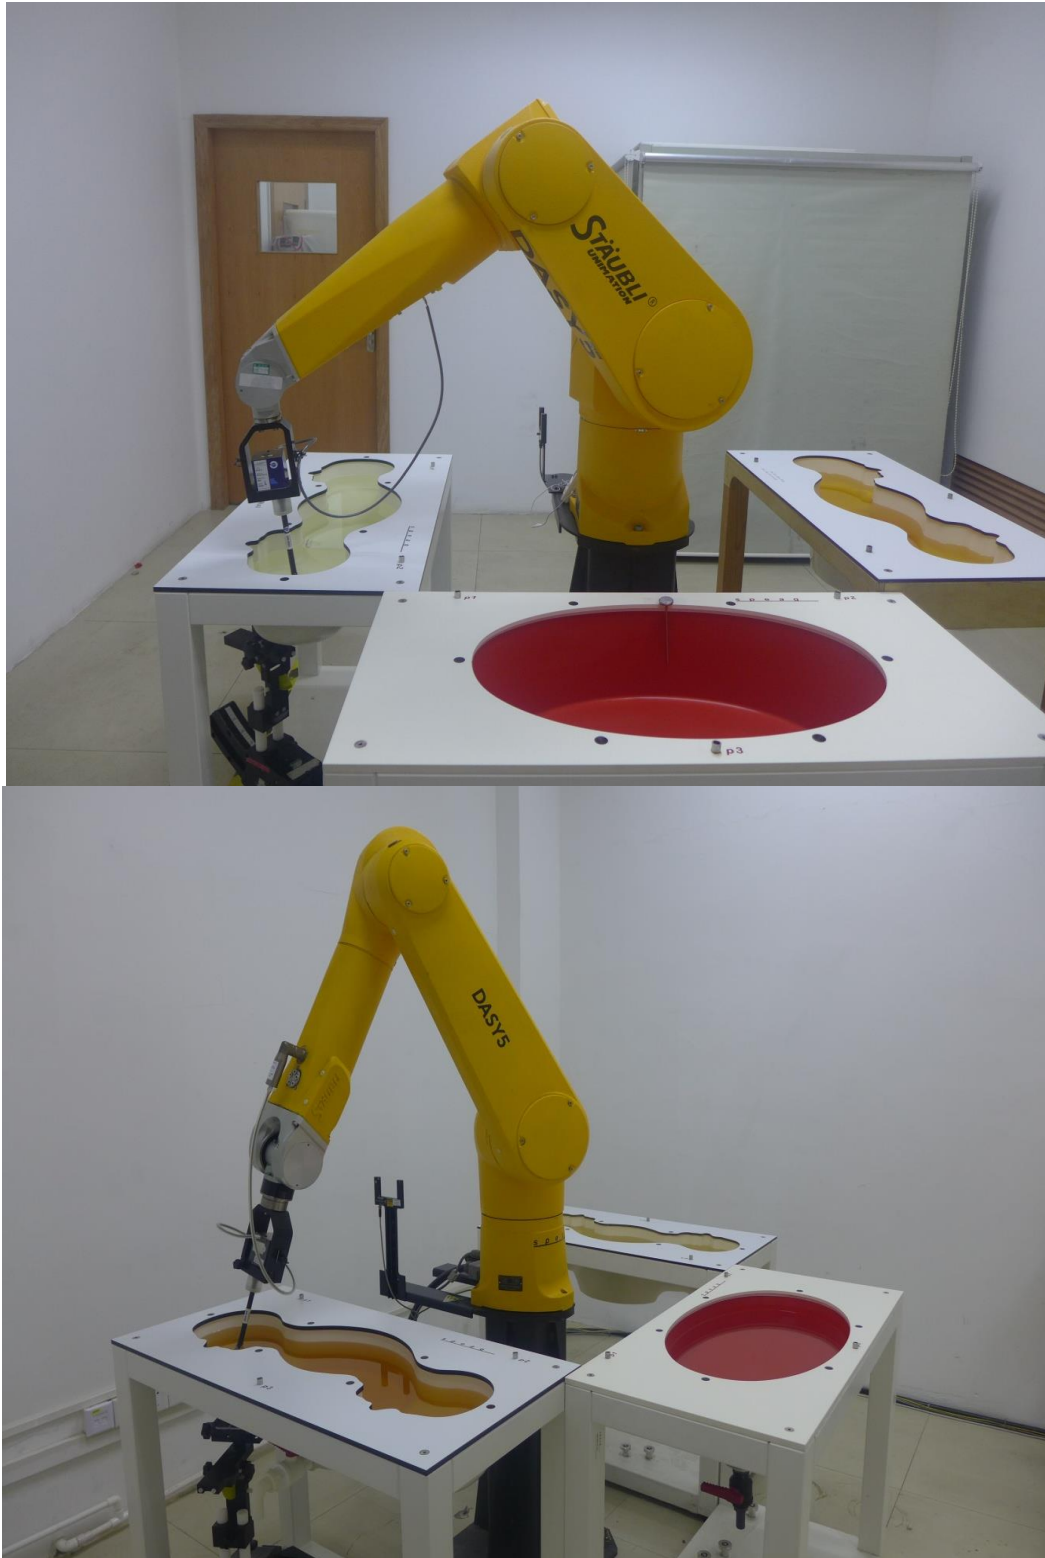



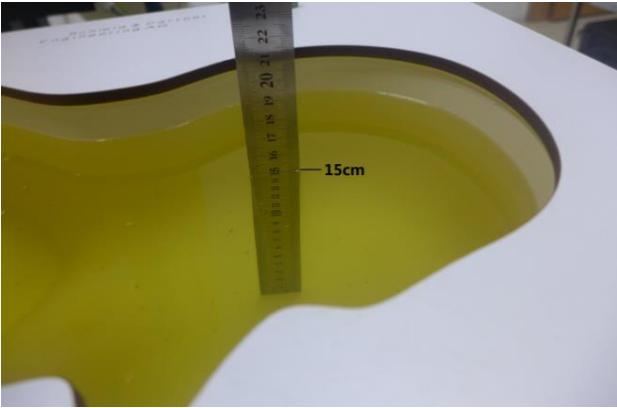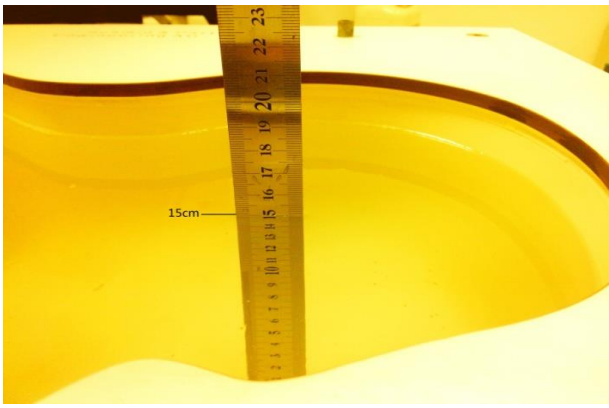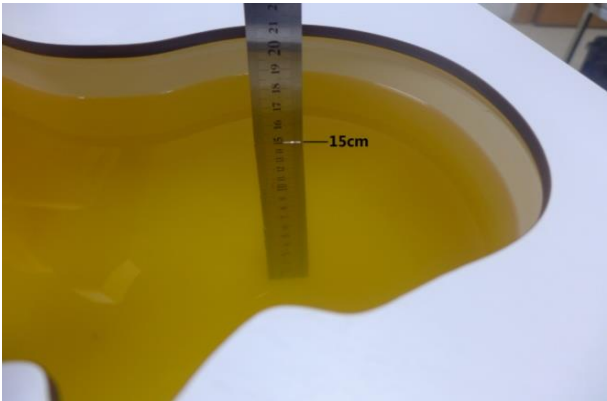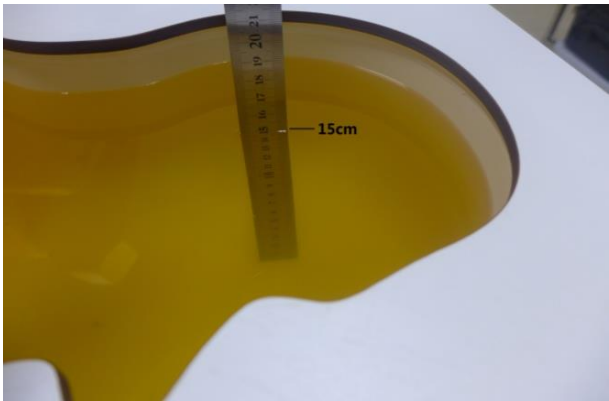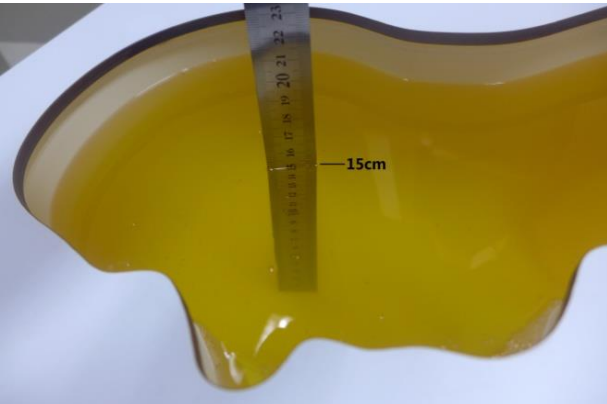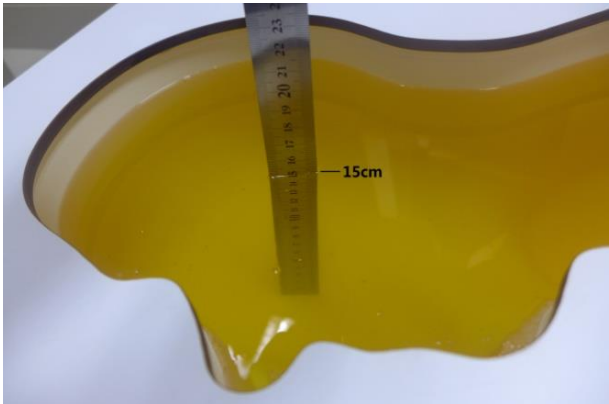

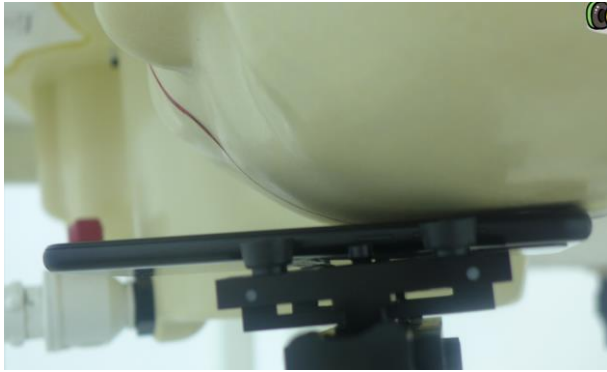


2. Photographs of Tissue Simulate Liquid

| | |
|---|--|
| <p>Photo 1: Tissue Simulant Liquid for Head 750</p> | <p>Photo 2: Tissue Simulant Liquid for Head 835</p> |
|  |  |
| <p>Photo 3: Tissue Simulant Liquid for Head 1750</p> | <p>Photo 4: Tissue Simulant Liquid for Head 1900</p> |
|  |  |
| <p>Photo 5: Tissue Simulant Liquid for Head 2450</p> | <p>Photo 6: Tissue Simulant Liquid for Head 2600</p> |
|  |  |



3. Photographs of EUT test position

| | |
|---|--|
| <p align="center">Photo 7: Left cheek</p> | <p align="center">Photo 8: Left tilted</p> |
|  |  |
| <p align="center">Photo 9: Right cheek</p> | <p align="center">Photo 10: Right tilted</p> |
|  |  |
| <p align="center">Photo 11: Front side 15mm</p> | <p align="center">Photo 12: Back side 15mm</p> |
|  |  |

| | |
|---|--|
| <p>Photo 13: Front side 10mm</p> | <p>Photo 14: Back side 10mm</p> |
|  |  |
| <p>Photo 15: Left side 10mm</p> | <p>Photo 16: Right side 10mm</p> |
|  |  |
| <p>Photo 17: Top side 10mm</p> | <p>Photo 18: Bottom side 10mm</p> |
|  |  |

| Photo 19: Back side 0mm | NA |
|---|-----------|
|  | <p>NA</p> |

4. EUT Constructional Details

| Photo 20: Front View | Photo 21: Back View |
|---|--|
|  |  |