

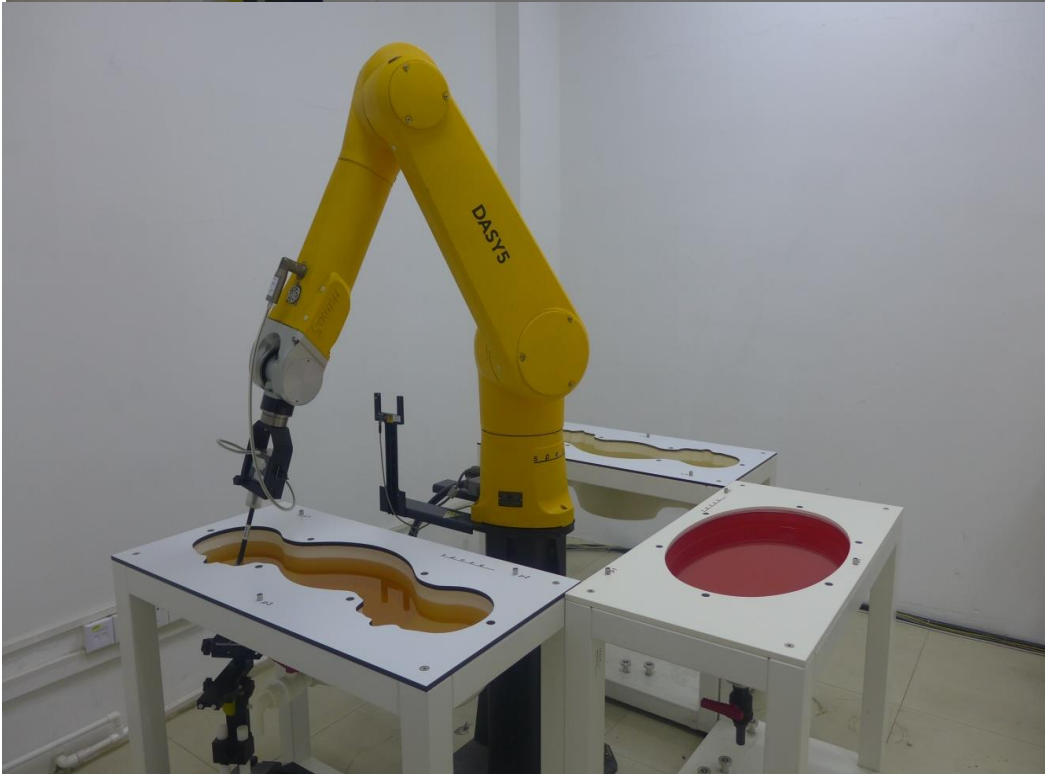
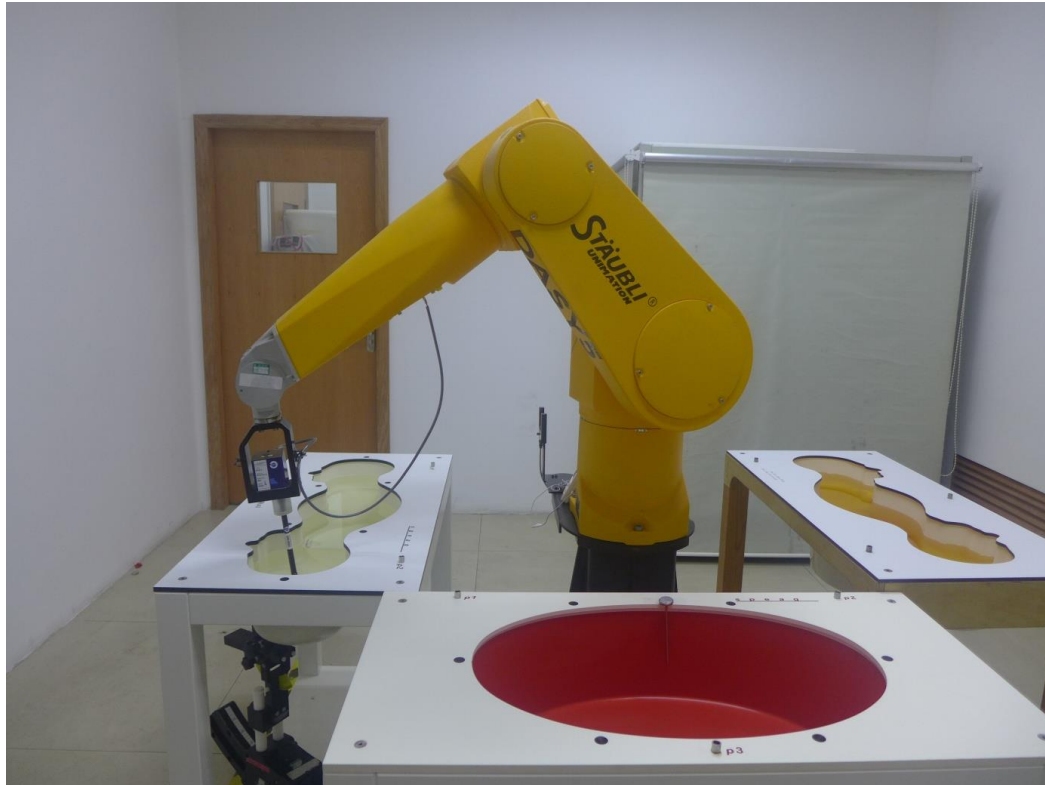


Appendix D

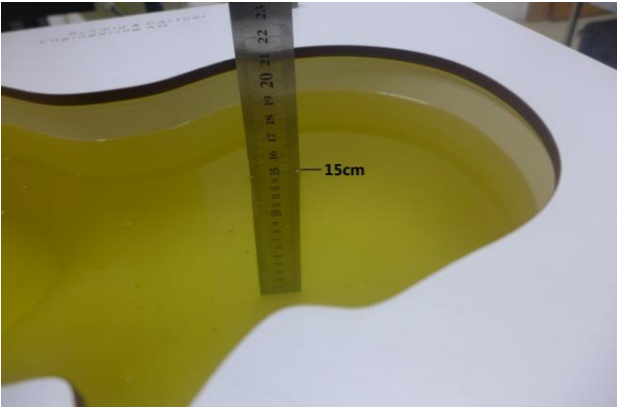
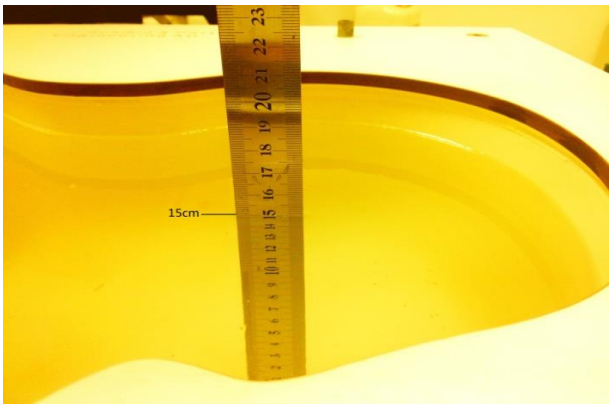
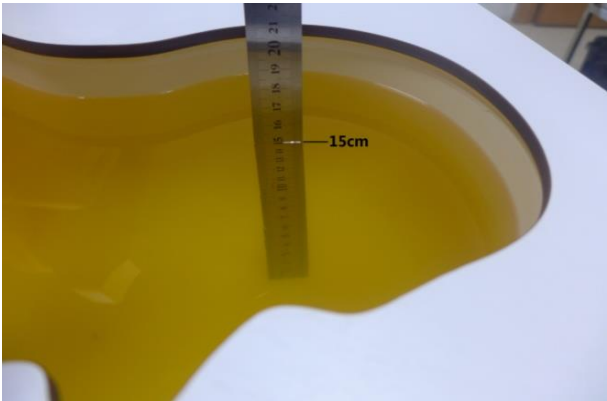
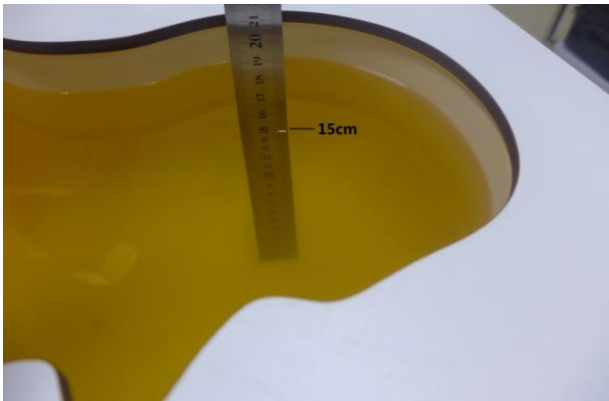
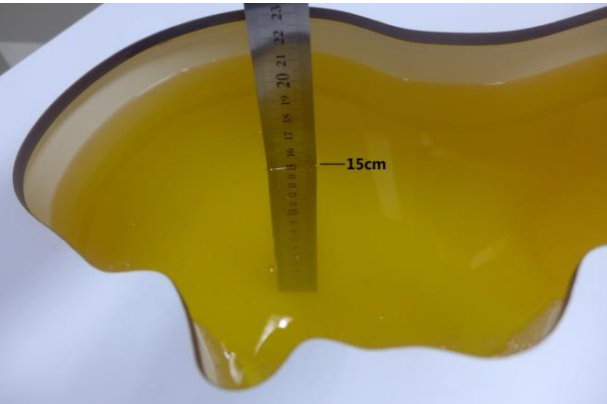
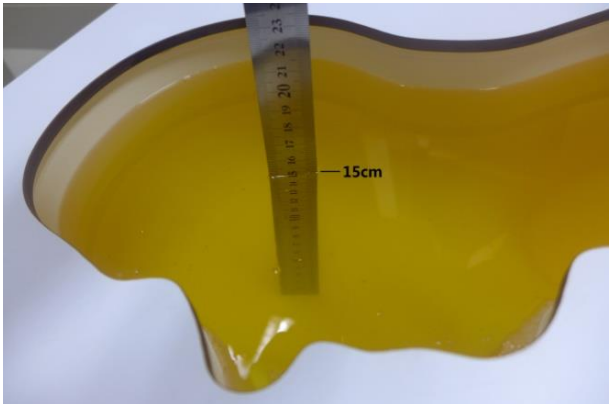
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	Photo 6: Tissue Simulant Liquid for Head 2600
	

3. Photographs of EUT test position

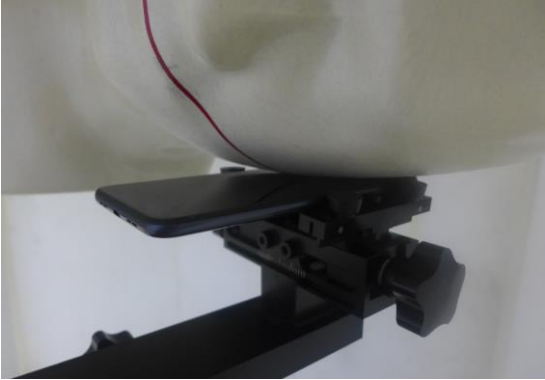





<p>Photo 7: Left cheek</p>	<p>Photo 8: Left tilted</p>
	
<p>Photo 9: Right cheek</p>	<p>Photo 10: Right tilted</p>
	
<p>Photo 11: Front side 15mm</p>	<p>Photo 12: Back side 15mm</p>
	






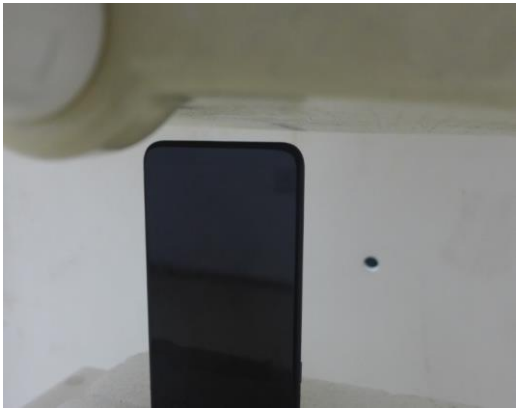

Photo 13: Front side 10mm	Photo 14: Back side 10mm
	
Photo 15: Left side 10mm	Photo 16: Right side 10mm
	
Photo 17: Top side 10mm	Photo 18: Bottom side 10mm
	

Photo 19: Back side 0mm	NA
	<p>NA</p>

4. EUT Constructional Details

Photo 20: Front View	Photo 21: Back View
