

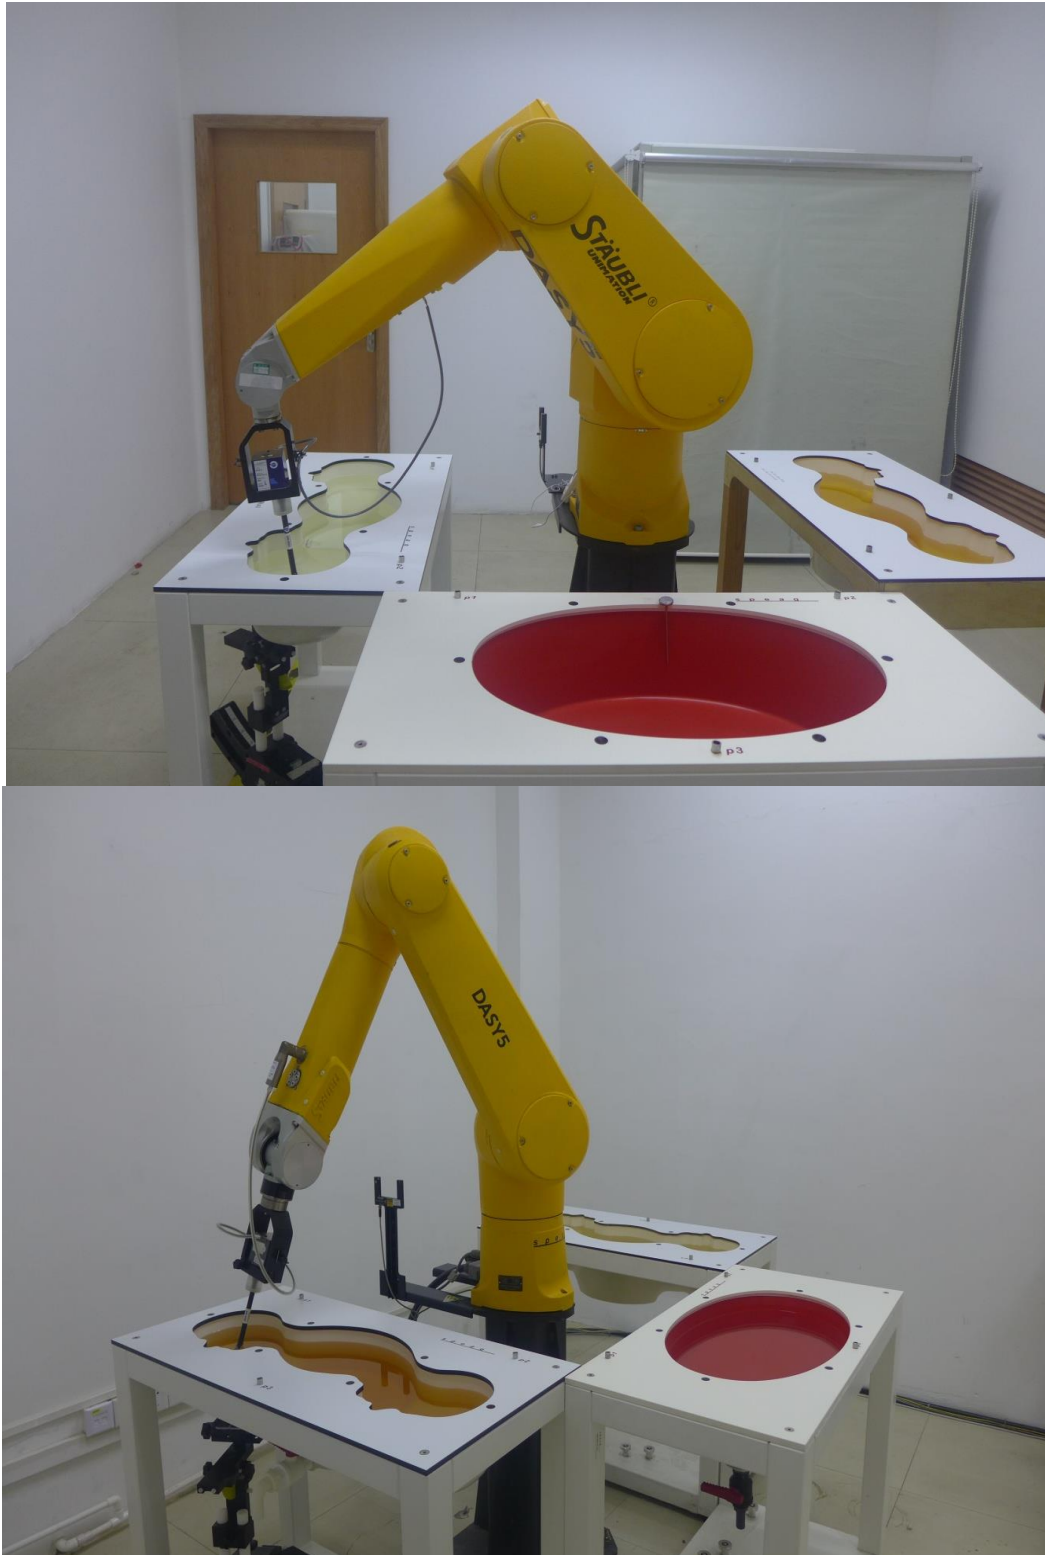


# **Appendix D**

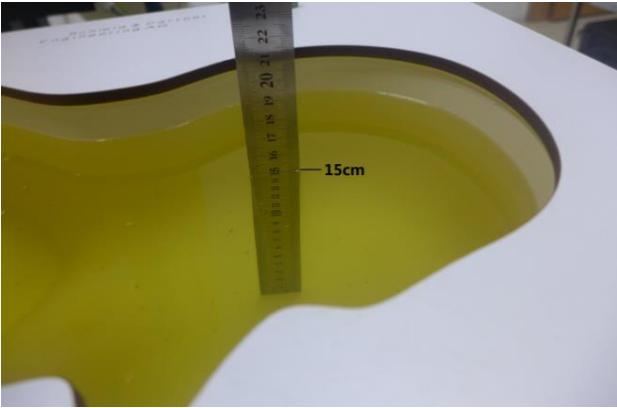
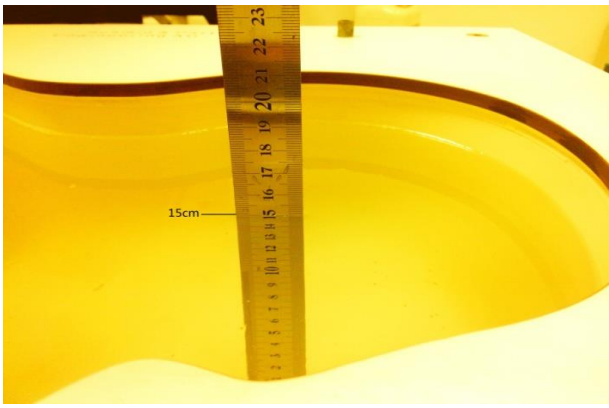
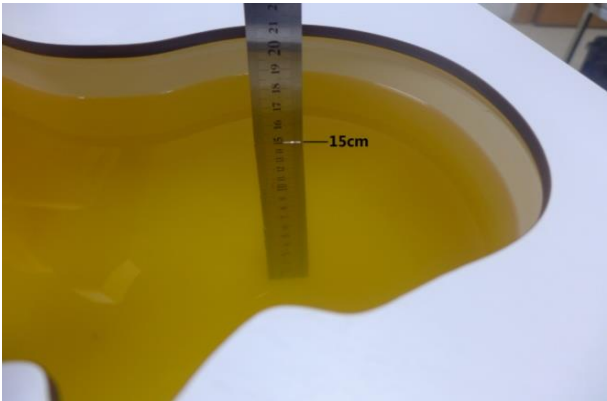
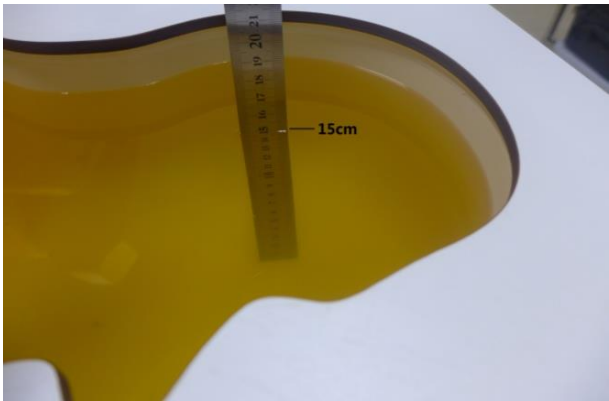
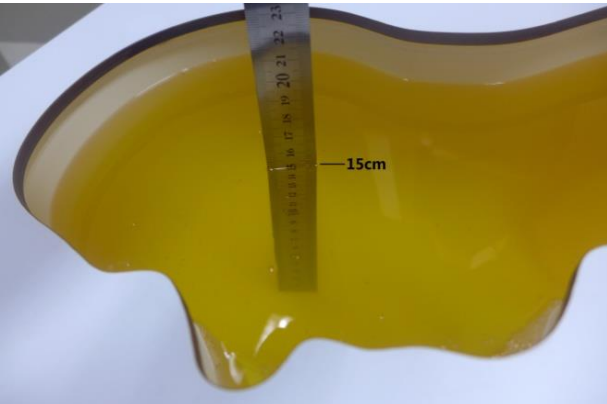
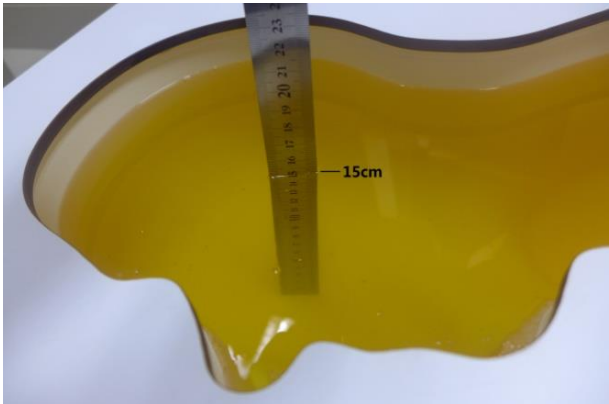
## **Photographs**

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## 1. SAR measurement System



## 2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 750</p>	<p>Photo 2: Tissue Simulant Liquid for Head 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1750</p>	<p>Photo 4: Tissue Simulant Liquid for Head 1900</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 6: Tissue Simulant Liquid for Head 2600</p>
	

### 3. Photographs of EUT test position

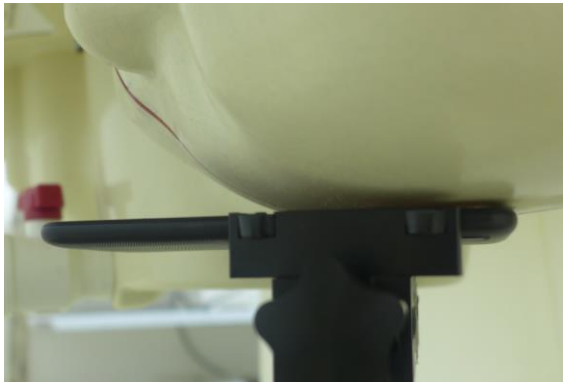

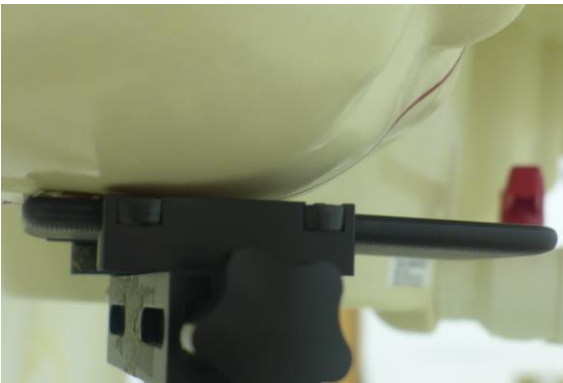



<p align="center"><b>Photo 7: Left cheek</b></p>	<p align="center"><b>Photo 8: Left tilted</b></p>
	
<p align="center"><b>Photo 9: Right cheek</b></p>	<p align="center"><b>Photo 10: Right tilted</b></p>
	
<p align="center"><b>Photo 11: Front side 15mm</b></p>	<p align="center"><b>Photo 12: Back side 15mm</b></p>
	

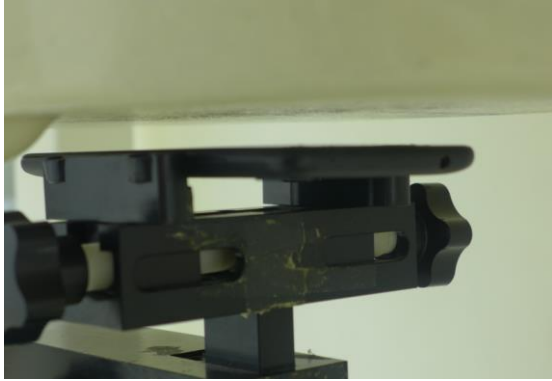
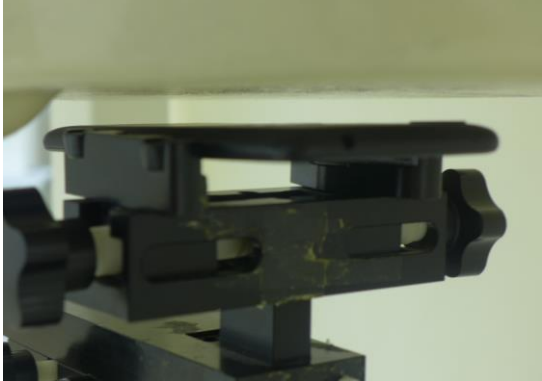




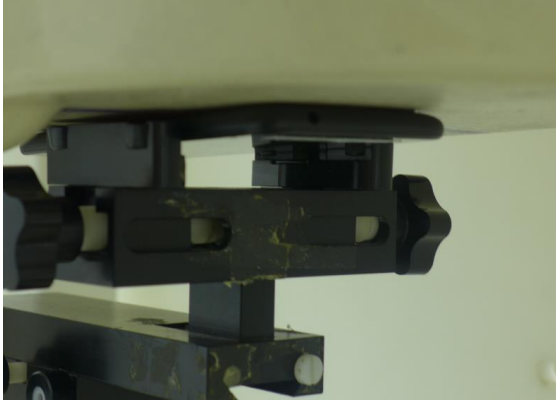

Photo 13: Front side 10mm	Photo 14: Back side 10mm
	
Photo 15: Left side 10mm	Photo 16: Right side 10mm
	
Photo 17: Top side 10mm	Photo 18: Bottom side 10mm
	

Photo 19: Back side 0mm	Photo 20: Back side 0mm
	

#### 4. EUT Constructional Details

Photo 21: Front View	Photo 22: Back View
