

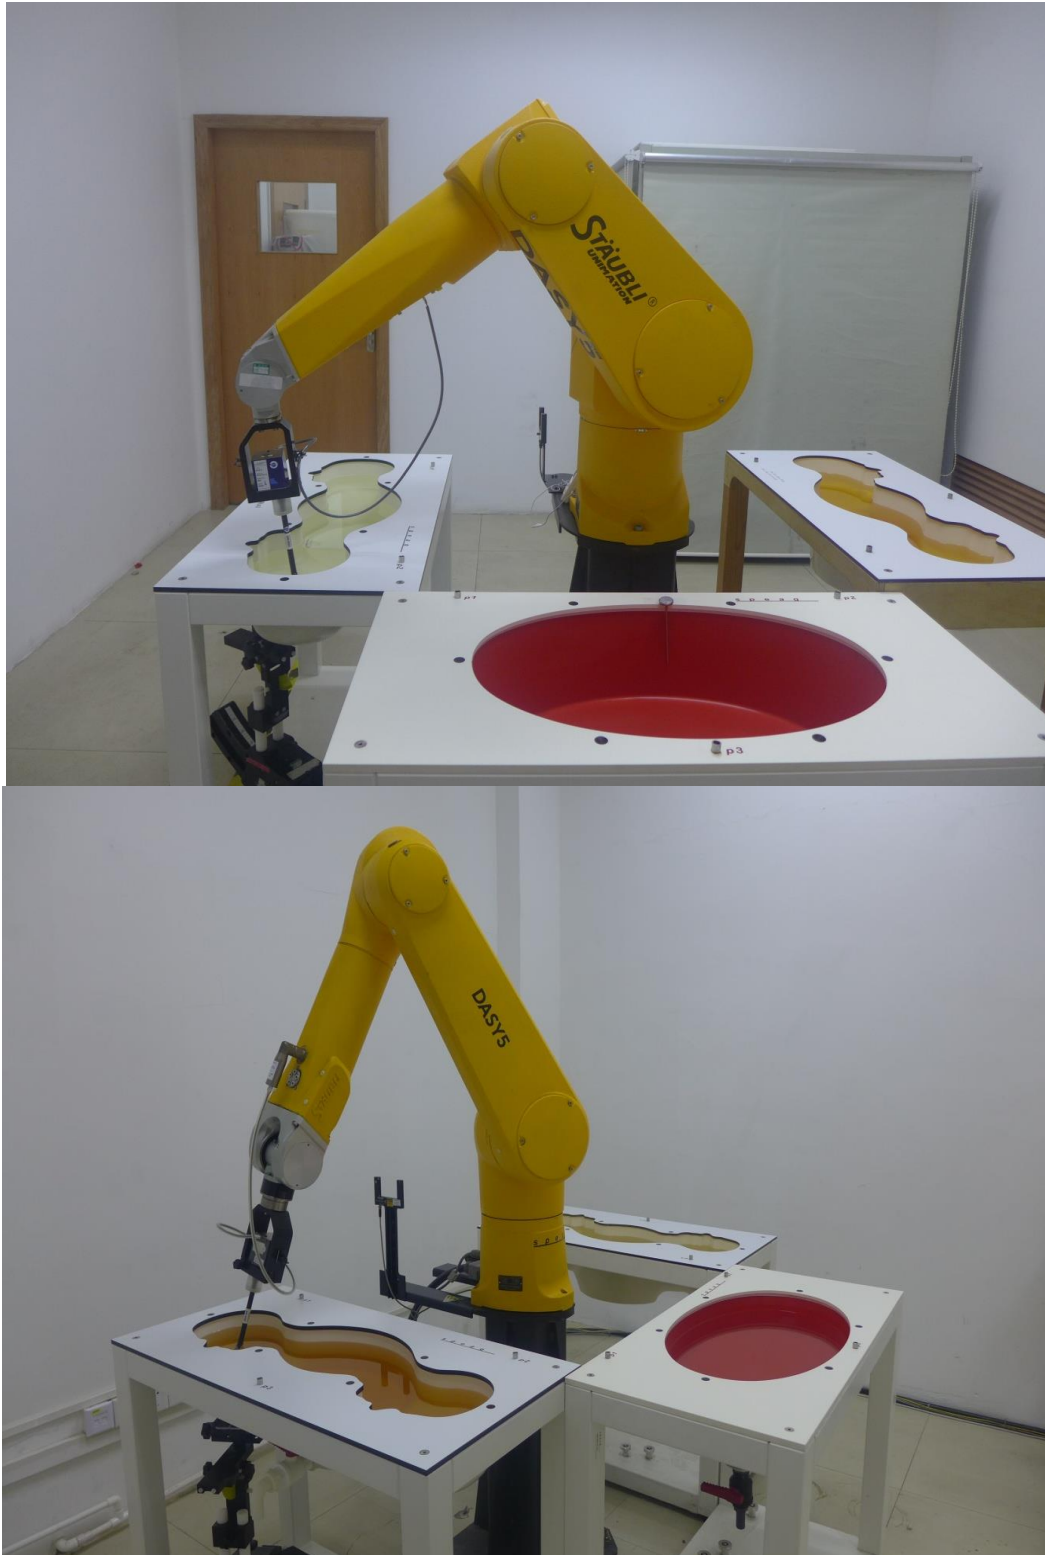


Appendix D

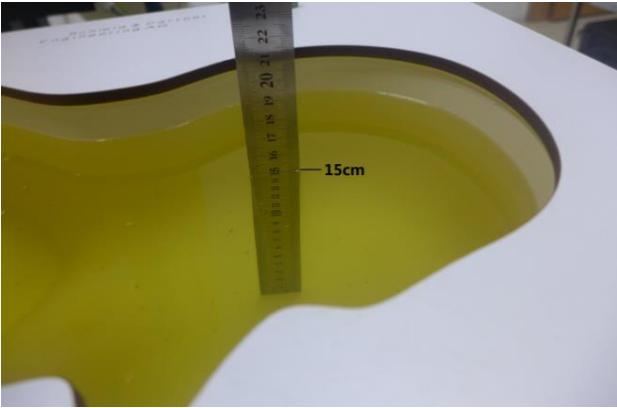
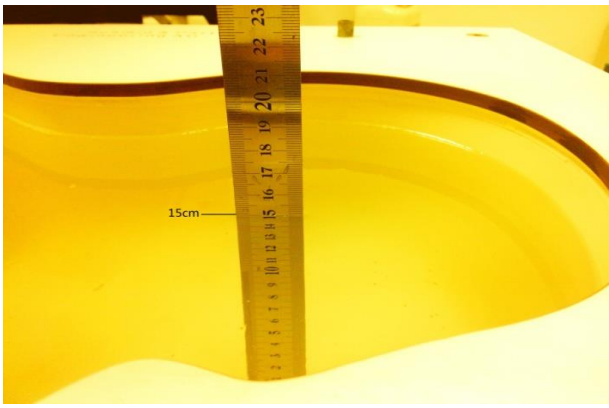
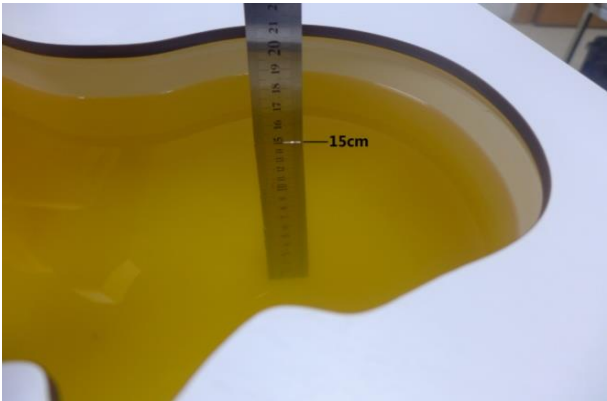
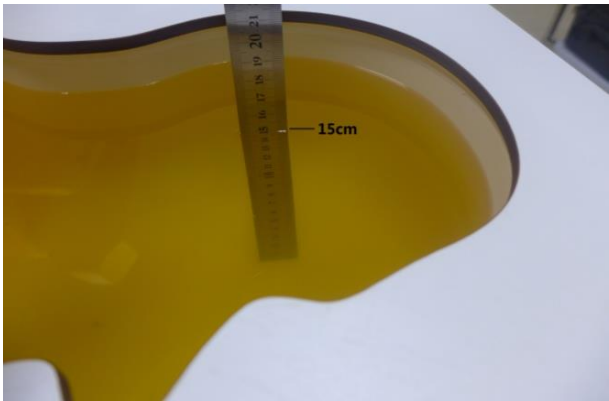
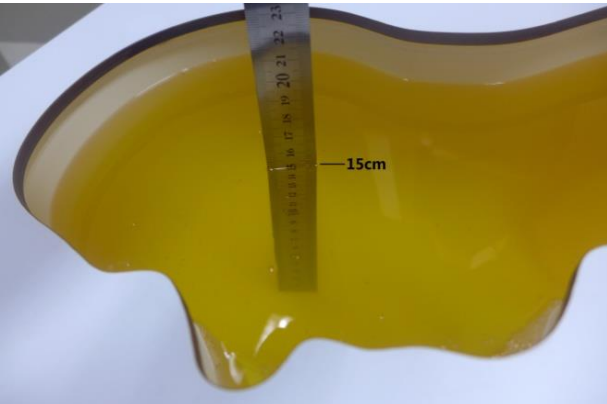
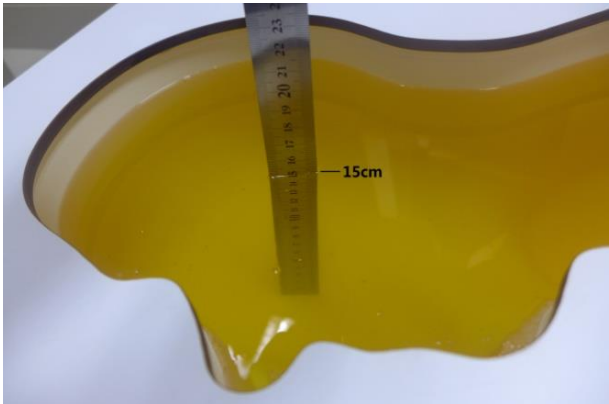
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 750</p>	<p>Photo 2: Tissue Simulant Liquid for Head 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1750</p>	<p>Photo 4: Tissue Simulant Liquid for Head 1900</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 6: Tissue Simulant Liquid for Head 2600</p>
	

3. Photographs of EUT test position

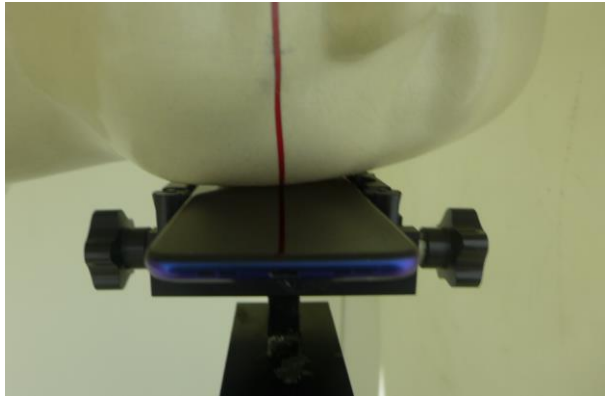
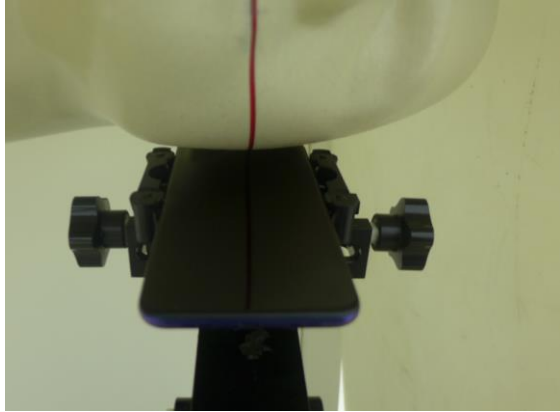
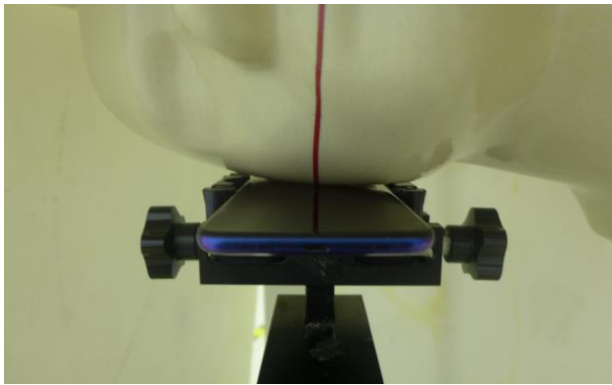
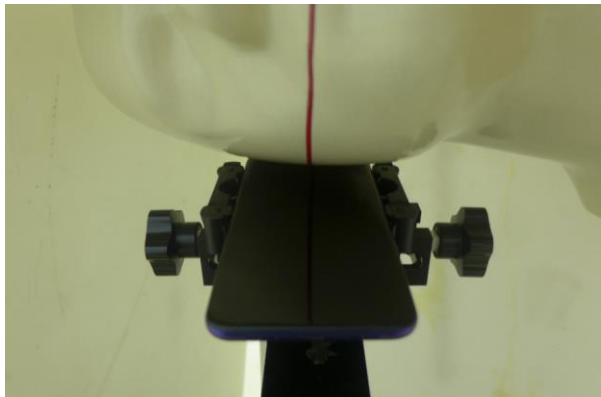
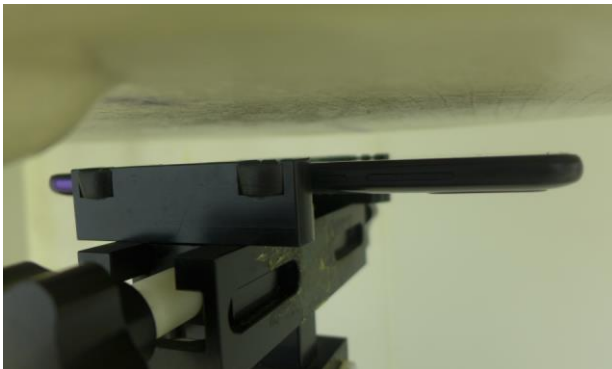
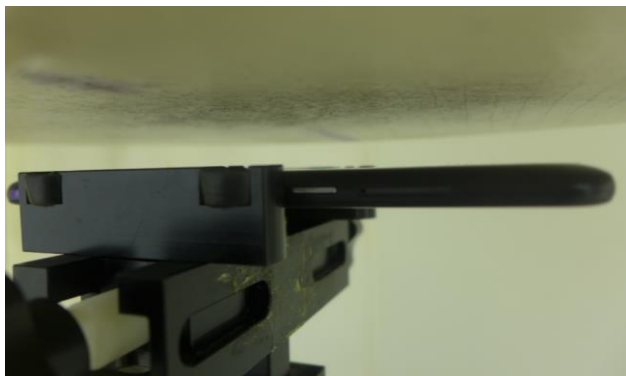
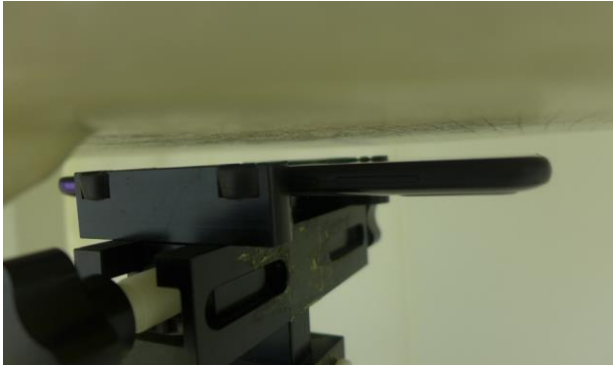


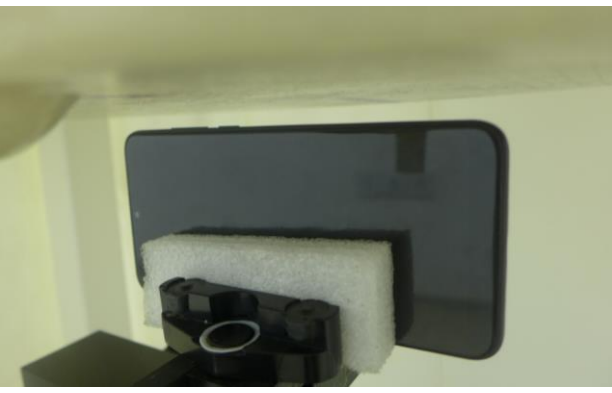


<p align="center">Photo 7: Left cheek</p>	<p align="center">Photo 8: Left tilted</p>
	
<p align="center">Photo 9: Right cheek</p>	<p align="center">Photo 10: Right tilted</p>
	
<p align="center">Photo 11: Front side 15mm</p>	<p align="center">Photo 12: Back side 15mm</p>
	

Photo 13: Front side 10mm	Photo 14: Back side 10mm
	
Photo 15: Left side 10mm	Photo 16: Right side 10mm
	
Photo 17: Top side 10mm	Photo 18: Bottom side 10mm
	

4. EUT Constructional Details

Photo 19: Front View	Photo 20: Back View
