





HAC RF TEST REPORT

No. I20Z60681-SEM01

For

TCL Communication Ltd.

GSM/UMTS/LTE Mobile phone

Model Name: 5004S

With

Hardware Version: 08

Software Version: 5H6EUFE0

FCC ID: 2ACCJH127

Results Summary: M Category = M3

Issued Date: 2020-7-10

Note:

The test results in this test report relate only to the devices specified in this report. This report shall not be reproduced except in full without the written approval of CTTL.

The report must not be used by the client to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S.Government.

Test Laboratory:

CTTL, Telecommunication Technology Labs, CAICT

No. 51, Xueyuan Road, Haidian District, Beijing, P. R. China 100191. Tel:+86(0)10-62304633-2512, Fax:+86(0)10-62304633-2504 Email: cttl_terminals@caict.ac.cn, website: www.caict.ac.cn





REPORT HISTORY

Report Number	Revision	Issue Date	Description	
I20Z60681-SEM01	Rev.0	2020-7-1	Initial creation of test report	
I20Z60681-SEM01	SEM01 Rev.1 2020-7-10	2020-7-10	Update the version of KDB285076	
		2020 0	D01 on page 9	





TABLE OF CONTENT

1 TEST LABORATORY	5
1.1 TESTING LOCATION	
1.2 TESTING ENVIRONMENT	
1.3 PROJECT DATA	
1.4 Signature	
2 CLIENT INFORMATION	6
2.1 APPLICANT INFORMATION	
2.2 MANUFACTURER INFORMATION	.6
3 EQUIPMENT UNDER TEST (EUT) AND ANCILLARY EQUIPMENT (AE)	7
3.1 About EUT	
3.2 INTERNAL IDENTIFICATION OF EUT USED DURING THE TEST	
3.3 INTERNAL IDENTIFICATION OF AE USED DURING THE TEST	
3.4 AIR INTERFACES / BANDS INDICATING OPERATING MODES	.7
4 MAXIMUM OUTPUT POWER	8
5 REFERENCE DOCUMENTS	9
5.1 Reference Documents for testing	.9
6 OPERATIONAL CONDITIONS DURING TEST 1	10
6.1 HAC MEASUREMENT SET-UP	10
6.2 PROBE SPECIFICATION	
6.3Test Arch Phantom & Phone Positioner	
6.4ROBOTIC SYSTEM SPECIFICATIONS	12
7 EUT ARRANGEMENT 1	13
7.1 WD RF EMISSION MEASUREMENTS REFERENCE AND PLANE	13
8 SYSTEM VALIDATION 1	14
8.1 VALIDATION PROCEDURE	14
8.2 VALIDATION RESULT	
9 EVALUATION OF MIF 1	15
9.1 INTRODUCTION	15
9.1 INTRODUCTION	
9.3 TEST EQUIPMENT FOR THE MIF MEASUREMENT	
9.4 TEST EQUI MENTION	
9.5 DUT MIF RESULTS.	
10 EVALUATION FOR LOW-POWER EXEMPTION 1	18
10.1 Product testing threshold	18
10.2 CONDUCTED POWER	
10.3 CONCLUSION	



CAICT No.I20Z60681-SEM01

11 RF TEST	PROCEDUERES 20
12 MEASUR	EMENT RESULTS (E-FIELD)
13 ANSIC 63	3.19-2011 LIMITS
14 MEASUR	EMENT UNCERTAINTY 22
15 MAIN TES	ST INSTRUMENTS
16 CONCLU	SION
ANNEX A 1	TEST LAYOUT
ANNEX B	TEST PLOTS
ANNEX C	SYSTEM VALIDATION RESULT 29
ANNEX D	PROBE CALIBRATION CERTIFICATE
	DIPOLE CALIBRATION CERTIFICATE 40





1 Test Laboratory

1.1 Testing Location

CompanyName:	CTTL(Shouxiang)	
Address:	No. 51 Shouxiang Science Building, Xueyuan Road, Haidian District,	
	Beijing, P. R. China100191	

1.2 Testing Environment

Temperature:	18°C~25°C,			
Relative humidity: 30%~ 70%				
Ground system resistance: $< 0.5 \Omega$				
Ambient noise is checked and found very low and in compliance with requirement of standards.				
Reflection of surrounding objects is minimized and in compliance with requirement of standards.				

1.3 Project Data

Project Leader:	Qi Dianyuan
Test Engineer:	Lin Hao
Testing Start Date:	June 17, 2020
Testing End Date:	June 18, 2020

1.4 Signature

Lin Xiaojun (Prepared this test report)

Qi Dianyuan (Reviewed this test report)

Lu Bingsong Deputy Director of the laboratory (Approved this test report)





2 Client Information

2.1 Applicant Information

Company Name:	TCL Communication Ltd.		
Address/Post:	5/F, Building 22E, 22 Science Park East Avenue, Hong Kong Science		
	Park, Shatin, NT, Hong Kong		
Contact Person:	Gong Zhizhou		
Contact Email:	zhizhou.gong@tcl.com		
Telephone:	0086-755-36611722		
Fax	0086-755-36612000-81722		

2.2 Manufacturer Information

Company Name:	TCL Communication Ltd.	
Address/Post:	5/F, Building 22E, 22 Science Park East Avenue, Hong Kong Science	
	Park, Shatin, NT, Hong Kong	
Contact Person:	Gong Zhizhou	
Contact Email:	zhizhou.gong@tcl.com	
Telephone:	0086-755-36611722	
Fax	0086-755-36612000-81722	





3 Equipment Under Test (EUT) and Ancillary Equipment (AE)

3.1 About EUT

Description: GSM/UMTS/LTE Mobile phone		
Model name: 5004S		
Operating mode(s):	GSM 850/900/1800/1900, UMTS FDD 1/2/4/5/8, BT, Wi-Fi,	
	LTE Band 2/3/4/5/7/12/13/66	

3.2 Internal Identification of EUT used during the test

EUT ID*	IMEI	HW Version	SW Version
EUT1	355952110203877	08	5H6EUFE0

*EUT ID: is used to identify the test sample in the lab internally.

Note: It is performed to test HAC with the EUT1

3.3 Internal Identification of AE used during the test

AE ID*	Description	Model	SN	Manufacturer
AE1	Battery	CAC2900028C1	/	BYD

*AE ID: is used to identify the test sample in the lab internally.

3.4 Air Interfaces / Bands Indicating Operating Modes

Air-interface	Band(MHz)	Туре	C63.19/tested	Simultaneous Transmissio ns	Name of Voice Service
GSM	850	VO	Voc		
GSIM	1900	vo	Yes		CMRS Voice
GPRS/EDGE	850	DT	Mar	BT, WLAN	
GPR5/EDGE	1900		Yes		Google duo
	850				
WCDMA	1700	VO	Yes	BT, WLAN	CMRS Voice
(UMTS)	1900				
	HSPA	DT	Yes		Google duo
LTE FDD	Band2/5/7/12/13/66	V/D	Yes	BT, WLAN	VoLTE, Google
	Danuz/5/7/12/13/00	V/D	162	DI, WLAN	duo
ВТ	2450	DT	NA	GSM,	NA
Ы	2430		NA NA	WCDMA, LTE	INA
WLAN	2450	V/D	Yes	GSM,	VoWiFi, Google
	2430	v/D	165	WCDMA, LTE	duo
WLAN	5G V/D		Yes	GSM,	VoWiFi, Google
		v/D		WCDMA, LTE	duo

NA: Not Applicable VO: Voice Only V/D: CMRS and IP Voice Service over Digital Transport DT: Digital Transport

* HAC Rating was not based on concurrent voice and data modes, Non current mode was found to represent worst case rating for both M and T rating

Note1 = No Associated T-Coil measurement has been made in accordance with 285076 D02 T-Coil testing for CMRS IP

©Copyright. All rights reserved by CTTL.





4 Maximum Output Power

GSM		Tune up (dBm)					
850MHz	Channel 251(848.8MHz)	Channel 190(836.6MHz)	Channel 128(824.2MHz)				
Voice	32	32	32				
EDGE	29.5	29.5	29.5				
GSM		Tune up(dBm)					
1900MHz	Channel 810(1909.8MHz)	Channel 661(1880MHz)	Channel 512(1850.2MHz)				
Voice	29.5	29.5	29.5				
EDGE	25	25	25				
WCDMA		Tune up (dBm)					
850MHz	Channel 4233(846.6MHz)	Channel 4132(826.4MHz)					
RMC	23.5	23.5	23.5				
HSPA	23	23	23				
		Tune up (dBm)					
	Channel 1513	Channel 1412 (1732.4MHz)	Channel 1312				
1700MHz	(1752.6MHz)		(1712.4MHz)				
RMC	23.2	23.2					
HSPA	SPA 23 23		23				
	Tune up (dBm)						
	Channel 9538(1907.6MHz)	Channel 9400(1880MHz)	Channel				
1900MHz			9262(1852.4MHz)				
RMC	23.2	23.2	23.2				
HSPA	23	23	23				
LTE Band2		Tune up (dBm)					
LIE Danuz	Channel 19100(1900MHz)	Channel18900(1880MHz)	Channel 18700(1860MHz)				
QPSK	23	23	23				
16QAM	22	22	22				
LTE Band5		Tune up (dBm)					
LIE Ballus	Channel 20600(844MHz)	Channel 20525(836.5MHz)	Channel20450(829MHz)				
QPSK	23.5	23.5	23.5				
16QAM	22.5	22.5	22.5				
LTE Band7		Tune up (dBm)					
	Channel 21350(2560Hz)	Channel 21100(2535MHz)	Channel20850(2510MHz)				
QPSK	23.5	23.5	23.5				
16QAM	22.5	22.5	22.5				
		Tune up (dBm)					
LTE Band12	Channel 23130(711MHz)	Channel 23095(707.5MHz)	Channel23060(704MHz)				
QPSK	23.6	23.6	23.6				
16QAM	22.6	22.6	22.6				
LTE Band13		Tune up (dBm)					
LIE Dallu 13	Channel 23230(782MHz)						



CAICT No.I20Z60681-SEM01

QPSK	23.6							
16QAM	22.6							
		Tune up (dBm)						
LTE Band66	Channel 132572(1770MHz)	Channel 132322(1745MHz)	Channel 133072(1720MHz)					
QPSK	23.8	23.8						
16QAM	22.8	22.8						
2 4011-	Tune up (dBm)							
2.4GHz 802.11b	Channel 11 (2462MHz)	Channel 6 (2437MHz)	Channel 1 (2412MHz)					
002.110	18	18	18					
5011-		Tune up (dBm)						
5GHz 802.11a	Channel 100 (5500MHz)	Channel 124 (5620MHz)	Channel 144 (5720MHz)					
ouz.11a	14	14	14					

5 Reference Documents

5.1 Reference Documents for testing

The following document listed in this section is referred for testing.

Reference	Title	Version
ANSI C63.19-2011	American National Standard for Methods of Measurement of	2011
	Compatibility between Wireless Communication Devices and	Edition
	Hearing Aids	
FCC 47 CFR §20.19	Hearing Aid Compatible Mobile Headsets	2015
		Edition
KDB 285076 D01	Equipment Authorization Guidance for Hearing Aid Compatibility	v05r01






6 OPERATIONAL CONDITIONS DURING TEST

6.1 HAC MEASUREMENT SET-UP

These measurements are performed using the DASY5 NEO automated dosimetric assessment system. It is made by Schmid & Partner Engineering AG (SPEAG) in Zurich, Switzerland. It consists of high precision robotics system (Stäubli), robot controller, Intel Core2 computer, near-field probe, probe alignment sensor. The robot is a six-axis industrial robot performing precise movements. A cell controller system contains the power supply, robot controller, teach pendant (Joystick), and remote control, is used to drive the robot motors. The PC consists of the HP Intel Core21.86 GHz computer with Windows XP system and HAC Measurement Software DASY5 NEO, A/D interface card, monitor, mouse, and keyboard. The Stäubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE)circuit performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. is connected to the Electro-optical coupler (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the PC plug-in card.

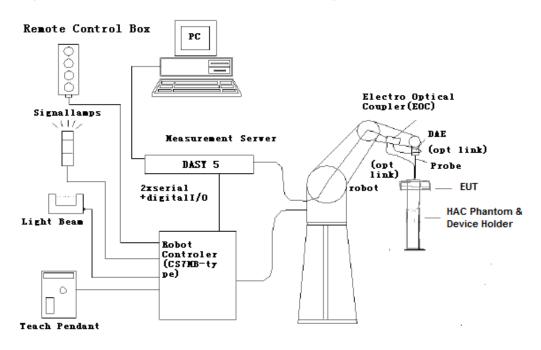



The DAE4 consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe mounting device includes two different sensor systems for frontal and sidewise probe contacts. They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built in VME-bus computer.





6.2 Probe Specification

E-Field Probe Description

Construction	One dipole parallel, two dipoles normal to probe axis	
	Built-in shielding against static charges	
	PEEK enclosure material	E
Calibration	In air from 100 MHz to 3.0 GHz (absolute accuracy $\pm 6.0\%$, k=2)	
		[ER3DV6]
Frequency	40 MHz to > 6 GHz (can be extended to < 20 MHz)	
	Linearity: ± 0.2 dB (100 MHz to 3 GHz)	
Directivity	± 0.2 dB in air (rotation around probe axis)	
	± 0.4 dB in air (rotation normal to probe axis)	
Dynamic Range	2 V/m to > 1000 V/m; Linearity: \pm 0.2 dB	
Dimensions	Overall length: 330 mm (Tip: 16 mm)	
	Tip diameter: 8 mm (Body: 12 mm)	
	Distance from probe tip to dipole centers: 2.5 mm	
Application	General near-field measurements up to 6 GHz	
	Field component measurements	
	Fast automatic scanning in phantoms	





6.3Test Arch Phantom & Phone Positioner

The Test Arch phantom should be positioned horizontally on a stable surface. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. It enables easy and well defined positioning of the phone and validation dipoles as well as simple teaching of the robot (Dimensions: 370 x 370 x 370 mm).

The Phone Positioner supports accurate and reliable positioning of any phone with effect on near field < \pm 0.5 dB.




Fig. 2 HAC Phantom & Device Holder

6.4 Robotic System Specifications

Specifications

Positioner: Stäubli Unimation Corp. Robot Model: RX160L Repeatability: ±0.02 mm No. of Axis: 6 Data Acquisition Electronic (DAE) System Cell Controller Processor: Intel Core2 Clock Speed: 1.86GHz Operating System: Windows XP Data Converter Features:Signal Amplifier, multiplexer, A/D converter, and control logic Software: DASY5 software Connecting Lines: Optical downlink for data and status info. Optical uplink for commands and clock





7 EUT ARRANGEMENT

7.1 WD RF Emission Measurements Reference and Plane

Figure 4 illustrates the references and reference plane that shall be used in the WD emissions measurement.

- The grid is 5 cm by 5 cm area that is divided into 9 evenly sized blocks or sub-grids.
- The grid is centered on the audio frequency output transducer of the WD (speaker or T-coil).

The grid is located by reference to a reference plane. This reference plane is the planar area that contains the highest point in the area of the WD that normally rests against the user's ear
The measurement plane is located parallel to the reference plane and 15 mm from it, out from the phone. The grid is located in the measurement plane.

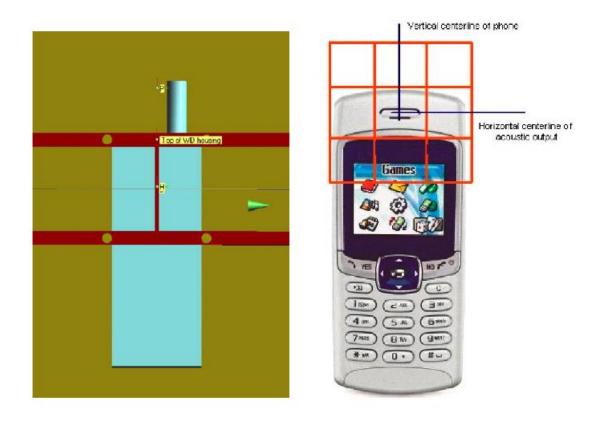


Fig. 3 WD reference and plane for RF emission measurements





8 SYSTEM VALIDATION

8.1 Validation Procedure

Place a dipole antenna meeting the requirements given in ANSI C63.19 in the position normally occupied by the WD. The dipole antenna serves as a known source for an electrical output. Position the E-field probes so that:

•The probes and their cables are parallel to the coaxial feed of the dipole antenna

•The probe cables and the coaxial feed of the dipole antenna approach the measurement area from opposite directions

• The center point of the probe element(s) are 15 mm from the closest surface of the dipole elements.

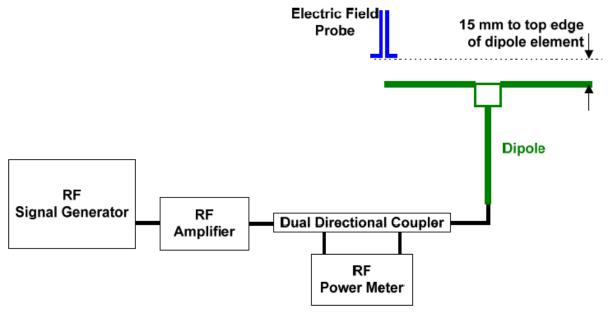


Fig. 4 Dipole Validation Setup

8.2 Validation Result

	E-Field Scan								
Mada	Frequency	Input Power Measured		Target ²	Deviation ³	Limit ⁴			
Mode	(MHz)	(mW)	Value(dBV/m)	Value(dBV/m)	(%)	(%)			
CW	835	100	40.58	40.56	0.23	±25			
CW	1880	100	38.92	38.89	0.35	±25			

Notes:

1. Please refer to the attachment for detailed measurement data and plot.

2. Target value is provided by SPEAD in the calibration certificate of specific dipoles.

3. Deviation (%) = 100 * (Measured value minus Target value) divided by Target value.

4. ANSI C63.19 requires values within \pm 25% are acceptable, of which 12% is deviation and 13% is measurement uncertainty. Values independently validated for the dipole actually used in the measurements should be used, when available.





9 Evaluation of MIF

9.1 Introduction

The MIF (Modulation Interference Factor) is used to classify E-field emission to determine Hearing Aid Compatibility (HAC). It scales the power-averaged signal to the RF audio interference level and is characteristic to a modulation scheme. The HAC standard preferred "indirect" measurement method is based on average field measurement with separate scaling by the MIF. With an Audio Interference Analyzer (AIA) designed by SPEAG specifically for the MIF measurement, these values have been verified by practical measurements on an RF signal modulated with each of the waveforms. The resulting deviations from the simulated values are within the requirements of the HAC standard.

The AIA (Audio Interference Analyzer) is an USB powered electronic sensor to evaluate signals in the frequency range 698MHz - 6 GHz. It contains RMS detector and audio frequency circuits for sampling of the RF envelope.

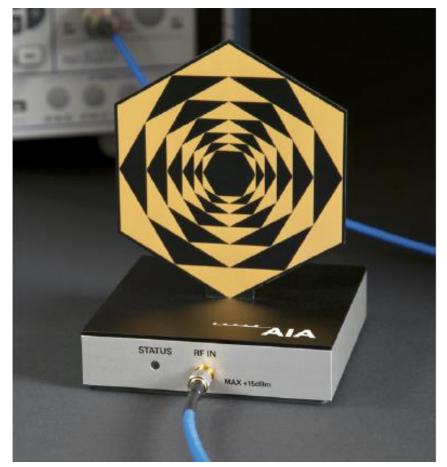


Fig. 5 AIA Front View





9.2 MIF measurement with the AIA

The MIF is measured with the AIA as follows:

- 1. Connect the AIA via USB to the DASY5 PC and verify the configuration settings.
- 2. Couple the RF signal to be evaluated to an AIA via cable or antenna.
- 3. Generate a MIF measurement job for the unknown signal and select the measurement port and timing settings.
- 4. Document the results via the post processor in a report.

9.3 Test equipment for the MIF measurement

No.	Name	Туре	Serial Number	Manufacturer
01	Signal Generator	E4438C	MY49071430	Agilent
02	AIA	SE UMS 170 CB	1029	SPEAG
03	BTS	E5515C	MY50263375	Agilent

9.4 Test signal validation

The signal generator (E4438C) is used to generate a 1GHz signal with different modulation in the below table based on the ANSI C63.19-2011. The measured MIF with AIA are compared with the target values given in ANSI C63.19-2011 table D.3, D.4 and D5.

Pulse modulation	Target MIF	Measured MIF	Deviation
0.5ms pulse, 1000Hz repetition rate	-0.9 dB	-0.9 dB	0 dB
1ms pulse, 100Hz repetition rate	+3.9 dB	+3.7 dB	0.2 dB
0.1ms pulse, 100Hz repetition rate	+10.1 dB	+10.0 dB	0.1 dB
10ms pulse, 10Hz repetition rate	+1.6 dB	+1.7 dB	0.1 dB
Sine-wave modulation	Target MIF	Measured MIF	Deviation
1 kHz, 80% AM	-1.2 dB	-1.3 dB	0.1 dB
1 kHz, 10% AM	-9.1 dB	-9.0 dB	0.1 dB
1 kHz, 1% AM	-19.1 dB	-18.9 dB	0.2 dB
100 Hz, 10% AM	-16.1 dB	-16.0 dB	0.1 dB
10 kHz, 10% AM	-21.5 dB	-21.6 dB	0.1 dB
Transmission protocol	Target MIF	Measured MIF	Deviation
GSM; full-rate version 2; speech codec/handset low	+3.5 dB	+3.47 dB	0.03 dB
WCDMA; speech; speech codec low; AMR 12.2 kb/s	-20.0 dB	-19.8 dB	0.2 dB
CDMA; speech; SO3; RC3; full frame rate; 8kEVRC	-19.0 dB	-19.1 dB	0.1 dB
CDMA; speech; SO3; RC1; 1/8 th frame rate; 8kEVRC	+3.3 dB	+3.44 dB	0.14 dB





9.5 DUT MIF results

Based on the KDB285076D01v05, the handset can also use the MIF values predetermined by the test equipment manufacturer. MIF values applied in this test report were provided by the HAC equipment provider of SPEAG, and the worst values for all air interface are listed below to be determine the Low-power Exemption.

Typical MIF levels in ANSI C63.19-2011					
Transmission protocol	Modulation interference factor				
GSM-FDD (TDMA, GMSK)	+3.63 dB				
EDGE-FDD (TDMA, 8PSK, TN 0-1)	+1.23dB				
EDGE-FDD (TDMA, 8PSK, TN 0-1-2)	-0.52dB				
UMTS-FDD(WCDMA, AMR)	-25.43dB				
UMTS-FDD (HSPA)	-20.75dB				
LTE-FDD (SC-FDMA, 1RB, 20MHz, QPSK)	-15.63 dB				
LTE-FDD (SC-FDMA, 1RB, 20MHz, 16QAM)	-9.76 dB				
IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	-5.90 dB				
IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps)	-5.17 dB				
IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps)	-3.37 dB				
IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps)	-2.02 dB				
IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps)	-0.36dB				
IEEE 802.11n (HT Greenfield, 6.5 Mbps, BPSK)	-15.80 dB				
IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps)	-5.82 dB				





10 Evaluation for low-power exemption

10.1 Product testing threshold

There are two methods for exempting an RF air interface technology from testing. The first method requires evaluation of the MIF for the worst-case operating mode. An RF air interface technology of a device is exempt from testing when its average antenna input power plus its MIF is \leq 17 dBm for any of its operating modes. The second method does not require determination of the MIF. The RF emissions testing exemption shall be applied to an RF air interface technology in a device whose peak antenna input power, averaged over intervals \leq 50 μ s20, is \leq 23 dBm. An RF air interface technology that is exempted from testing by either method shall be rated as M4. The first method is used to be exempt from testing for the RF air interface technology in this report.

Band	Average power (dBm)	MIF (dB)	Sum (dBm)	C63.19 Tested
GSM 850 - Voice	32	3.63	35.63	Yes
GSM 850 - EDGE	29.5	1.23	30.73	Yes*
GSM 1900 - Voice	29.5	3.63	33.13	Yes
GSM 1900 - EDGE	25	-0.52	24.48	Yes*
WCDMA 850 - RMC	23.5	-25.43	-1.93	No
WCDMA 850 - HSPA	23	-20.75	2.25	No
WCDMA 1700 - RMC	23.2	-25.43	-2.23	No
WCDMA 1700 - HSPA	23	-20.75	2.25	No
WCDMA 1900 - RMC	23.2	-25.43	-2.23	No
WCDMA 1900 - HSPA	23	-20.75	2.25	No
LTE Band 2 QPSK	23	-15.63	7.37	No
LTE Band 5 QPSK	23.5	-15.63	7.87	No
LTE Band 7 QPSK	23.5	-15.63	7.87	No
LTE Band 12 QPSK	23.6	-15.63	7.97	No
LTE Band 13 QPSK	23.6	-15.63	7.97	No
LTE Band 66 QPSK	23.8	-15.63	8.17	No
LTE Band 2 16QAM	22	-9.76	12.24	No
LTE Band 5 16QAM	22.5	-9.76	12.74	No
LTE Band 7 16QAM	22.5	-9.76	12.74	No
LTE Band 12 16QAM	22.6	-9.76	12.84	No
LTE Band 13 16QAM	22.6	-9.76	12.84	No
LTE Band 66 16QAM	22.8	-9.76	13.04	No
WiFi-2.4G	18	-5.90	12.1	No
WiFi-5G	14	-5.82	8.18	No

10.2 Conducted power

*Note: For GSM bands, EDGE modes were not evaluated as Voice modes were found to the worst-case modes for the GSM air interface.





10.3 Conclusion

According to the above table, the sums of average power and MIF for WCDMA, LTE FDD and WiFi are less than 17dBm. So it is measured for GSM bands. The WCDMA, LTE FDD and WiFi are exempt from testing and rated as M4.





11 RF TEST PROCEDUERES

The evaluation was performed with the following procedure:

- 1) Confirm proper operation of the field probe, probe measurement system and other instrumentation and the positioning system.
- 2) Position the WD in its intended test position. The gauge block can simplify this positioning.
- 3) Configure the WD normal operation for maximum rated RF output power, at the desired channel and other operating parameters (e.g., test mode), as intended for the test.
- 4) The center sub-grid shall centered on the center of the T-Coil mode axial measurement point or the acoustic output, as appropriate. Locate the field probe at the initial test position in the50 mm by 50 mm grid, which is contained in the measurement plane. If the field alignment method is used, align the probe for maximum field reception.
- 5) Record the reading.
- 6) Scan the entire 50 mm by 50 mm region in equally spaced increments and record the reading at each measurement point. The distance between measurement points shall be sufficient to assure the identification of the maximum reading.
- 7) Identify the five contiguous sub-grids around the center sub-grid whose maximum reading is the lowest of all available choices. This eliminates the three sub-grids with the maximum readings. Thus, the six areas to be used to determine the WD's highest emissions are identified.
- 8) Identify the maximum field reading within the non-excluded sub-grids identified in Step 7)
- 9) Evaluate the MIF and add to the maximum steady-state rms field-strength reading to obtain the RF audio interference level.
- 10) Compare this RF audio interference level with the categories and record the resulting WD category rating.





Freq	luency	Measured		Cotomorra			
MHz	Channel	Value(dBV/m)	Power Drift (dB)	Category			
	GSM 850						
848.8	251	36.35	-0.07	M4			
836.6	190	36.92	-0.04	M4			
824.2	128	37.03	-0.08	M4 (see Fig B.1)			
		GSM 19	00				
1909.8	810	30.73	-0.08	M3			
1880	661	31.08	0.03	M3			
1850.2	512	31.12	-0.12	M3 (see Fig B.2)			

12 Measurement Results (E-Field)

13 ANSIC 63.19-2011 LIMITS

WD RF audio interference level categories in logarithmic units

Emission categories	< 960 MHz E	-field emissions
Category M1	50 to 55	dB (V/m)
Category M2	45 to 50	dB (V/m)
Category M3	40 to 45	dB (V/m)
Category M4	< 40	dB (V/m)
Emission categories	> 960 MHz E	-field emissions
Category M1	40 to 45	dB (V/m)
Category M2	35 to 40	dB (V/m)
Category M3	30 to 35	dB (V/m)
Category M4	< 30	dB (V/m)





14 MEASUREMENT UNCERTAINTY

No.	Error source	Туре	Uncertainty Value(%)	Prob. Dist.	k	ciE	Standard Uncertainty (%) $\mu_i^{(*)}$ (%)E	Degree of freedom V _{eff} or <i>v</i> i	
Meas	Measurement System								
1	Probe Calibration	В	5.	Ν	1	1	5.1	∞	
2	Axial Isotropy	В	4.7	R	$\sqrt{3}$	1	2.7	∞	
3	Sensor Displacement	В	16.5	R	$\sqrt{3}$	1	9.5	∞	
4	Boundary Effects	В	2.4	R	$\sqrt{3}$	1	1.4	∞	
5	Linearity	В	4.7	R	$\sqrt{3}$	1	2.7	ø	
6	Scaling to Peak Envelope Power	В	2.0	R	$\sqrt{3}$	1	1.2	ø	
7	System Detection Limit	В	1.0	R	$\sqrt{3}$	1	0.6	∞	
8	Readout Electronics	В	0.3	N	1	1	0.3	∞	
9	Response Time	В	0.8	R	$\sqrt{3}$	1	0.5	×	
10	Integration Time	В	2.6	R	$\sqrt{3}$	1	1.5	ø	
11	RF Ambient Conditions	В	3.0	R	$\sqrt{3}$	1	1.7	ø	
12	RF Reflections	В	12.0	R	$\sqrt{3}$	1	6.9	ø	
13	Probe Positioner	В	1.2	R	$\sqrt{3}$	1	0.7	∞	
14	Probe Positioning	А	4.7	R	$\sqrt{3}$	1	2.7	×	
15	Extra. And Interpolation	В	1.0	R	$\sqrt{3}$	1	0.6	ø	
Test	Sample Related		I	1					
16	Device Positioning Vertical	В	4.7	R	$\sqrt{3}$	1	2.7	ø	
17	Device Positioning Lateral	В	1.0	R	$\sqrt{3}$	1	0.6	×	
18	Device Holder and Phantom	В	2.4	R	$\sqrt{3}$	1	1.4	×	
19	Power Drift	В	5.0	R	$\sqrt{3}$	1	2.9	×	





20	AIA measurement	В	12	R	$\sqrt{3}$	1	6.9	∞	
Pha	Phantom and Setup related								
21	Phantom Thickness	В	2.4	R	$\sqrt{3}$	1	1.4	×	
Comb	pined standard uncertainty(%)						16.2		
Expanded uncertainty (confidence interval of 95 %)		ı	<i>u_e</i> = 2 <i>u_c</i> N k		k=2		32.4		

15 MAIN TEST INSTRUMENTS

Table 1: List of Main Instruments

No.	Name	Туре	Serial Number	Calibration Date	Valid Period
01	Signal Generator	E4438C	MY49071430	February 25, 2020	One Year
02	Power meter	NRP2	106277	Soptombor 4, 2010	
03	Power sensor	NRP8S	104291	September 4, 2019	One year
04	Amplifier	60S1G4	0331848	No Calibration Requested	
05	E-Field Probe	ER3DV6	2344	June 24, 2019	One year
06	DAE	SPEAG DAE4	777	January 8, 2020	One year
07	HAC Dipole	CD835V3	1023	August 26, 2019	One year
08	HAC Dipole	CD1880V3	1018	August 26, 2019	One year
09	BTS	CMW500	166370	June 27, 2019	One year
10	AIA	SE UMS 170 CB	1029	No Calibration Requested	

16 CONCLUSION


The HAC measurement indicates that the EUT complies with the HAC limits of the ANSIC63.19-2011. The total M-rating is **M3.**

END OF REPORT BODY





ANNEX A TEST LAYOUT

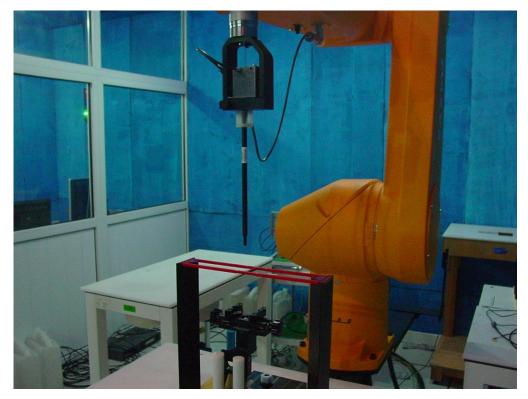

Picture A1:HAC RF System Layout





ANNEX B TEST PLOTS

HAC RF E-Field GSM 850 Low Date: 2020-6-17

Electronics: DAE4 Sn777 Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon_r = 1$; $\rho = 1000$ kg/m³ Ambient Temperature: 22.0°C Communication System: GSM 850; Frequency: 824.2 MHz; Duty Cycle: 1:8.3 Probe: ER3DV6 - SN2344;ConvF(1, 1, 1)

GSM850/E Scan - ER3DV6 - 2011: 15 mm from Probe Center to the Device

3/Hearing Aid Compatibility Test (101x101x1): Interpolated grid:

dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 58.25 V/m; Power Drift = -0.08 dB Applied MIF = 3.48 dB RF audio interference level = 37.03 dBV/m

Emission category: M4

MIL SCALEU E ITELU					
Grid 1 M4	Grid 2 M4	Grid 3 M4			
36.07 dBV/m	36.91 dBV/m	36.71 dBV/m			
Grid 4 M4	Grid 5 M4	Grid 6 M4			
36.2 dBV/m	37.03 dBV/m	36.83 dBV/m			
Grid 7 M4	Grid 8 M4	Grid 9 M4			
36.16 dBV/m	36.9 dBV/m	36.7 dBV/m			

MIF scaled E-field





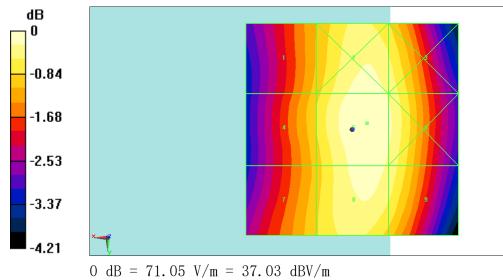


Fig B.1 HAC RF E-Field GSM 850 Low





HAC RF E-Field GSM 1900 Low Date: 2020-6-18 Electronics: DAE4 Sn777 Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\varepsilon_r = 1$; $\rho = 1000$ kg/m³ Ambient Temperature: 22.0°C Communication System: PCS 1900; Frequency: 1850.2 MHz; Duty Cycle: 1:8.3 Probe: ER3DV6 - SN2344;ConvF(1, 1, 1)

GSM1900/E Scan - ER3DV6 - 2011: 15 mm from Probe Center to the Device

3/Hearing Aid Compatibility Test (101x101x1): Interpolated grid:

dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 26.10 V/m; Power Drift = -0.12 dB Applied MIF = 3.49 dB RF audio interference level = 31.12 dBV/m

Emission category: M3

Grid 1 M4	Grid 2 M3	Grid 3 M3
27.26 dBV/m	31.28 dBV/m	31.78 dBV/m
Grid 4 M4	Grid 5 M3	Grid 6 M3
27.96 dBV/m	31.12 dBV/m	31.3 dBV/m
Grid 7 M4	Grid 8 M3	Grid 9 M3
28.02 dBV/m	30.74 dBV/m	30.75 dBV/m

MIF scaled E-field





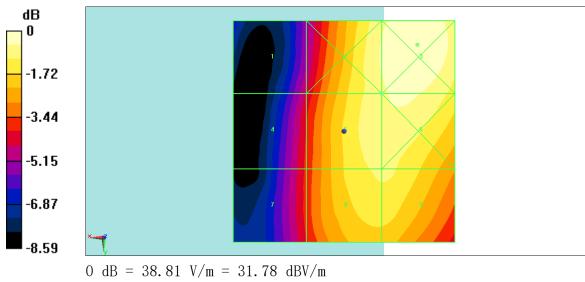


Fig B.2 HAC RF E-Field GSM 1900 Low







ANNEX C SYSTEM VALIDATION RESULT

E SCAN of Dipole 835 MHz Date: 2020-6-17 Electronics: DAE4 Sn777 Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\epsilon r = 1$; $\rho = 1000$ kg/m3 Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1 Probe: ER3DV6 - SN2344;ConvF(1, 1, 1) E Scan - measurement distance from the probe sensor center to CD835 Dipole = 15mm/Hearing Aid Compatibility Test (41x361x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm Reference Value = 130.7 V/m; Power Drift = 0.05 dB Applied MIF = 0.00 dB RF audio interference level = 40.58 dBV/m Emission category: M3

MIF scaled E-field

Grid 1 M3	Grid 2 M3	Grid 3 M3
40.11 dBV/m	40.58 dBV/m	40.69 dBV/m
Grid 4 M4	Grid 5 M4	Grid 6 M4
35.38 dBV/m	35.13 dBV/m	35.11 dBV/m
Grid 7 M3	Grid 8 M3	Grid 9 M3
40.34 dBV/m	40.73 dBV/m	40.59 dBV/m

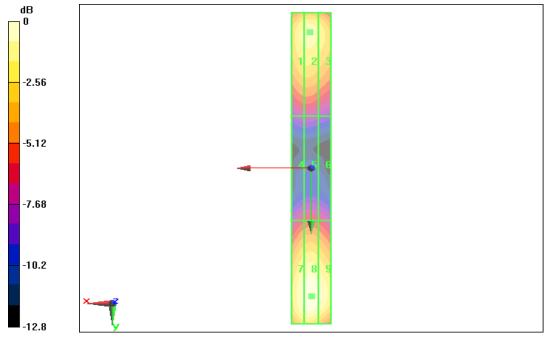







E SCAN of Dipole 1880 MHz Date: 2020-6-18

Electronics: DAE4 Sn777 Medium: Air Medium parameters used: $\sigma = 0$ mho/m, $\varepsilon_r = 1$; $\rho = 1000$ kg/m³ Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1 Probe: ER3DV6 - SN2344;ConvF(1, 1, 1) E Scan - measurement distance from the probe sensor center to CD1880 Dipole = 15mm/Hearing Aid Compatibility Test (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 149.7 V/m; Power Drift = 0.04 dB


Applied MIF = 0.00 dB

RF audio interference level = 38.92 dBV/m

Emission category: M2

MIF scaled E-field

Grid 1 M2	Grid 2 M2	Grid 3 M2
38.61 dBV/m	38.92 dBV/m	38.79 dBV/m
Grid 4 M2	Grid 5 M2	Grid 6 M2
36.02 dBV/m	36.01 dBV/m	36.14 dBV/m
Grid 7 M2	Grid 8 M2	Grid 9 M2
38.65 dBV/m	38.87 dBV/m	38.76 dBV/m

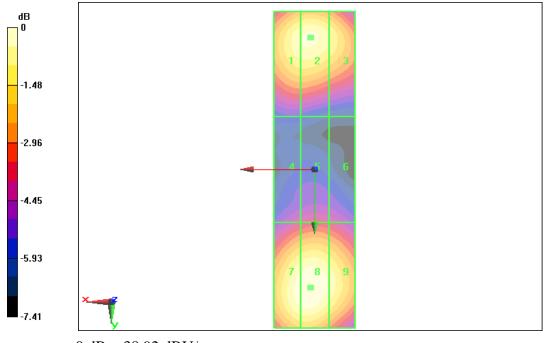

0 dB = 38.92 dBV/m






ANNEX D PROBE CALIBRATION CERTIFICATE

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 2 Accredited by the Swiss Accre			Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
The Swiss Accreditation Se	rvice is one of the signatories in the recognition of calibration of	n the EA	ccreditation No.: SCS 0108
Client Auden			o: ER3-2344_Jun19
CALIBRATION	CERTIFICATE		
Object	ER3DV6- SN:2344		
Calibration procedure(s)	QA CAL-02.v9, QA Calibration procedu evaluations in air	CAL-25.v7 ire for E-field probes optimized	for close near field
Calibration date:	June 24, 2019		
All calibrations have been con Calibration Equipment used (h	ducted in the closed laboratory fa	children on the following pages and children on the following pages and children on the following pages and children of the ch	and humidity < 70%.
All calibrations have been con	ducted in the closed laboratory fa A&TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: S5277 (20x)	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893)	and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Apr-20
All calibrations have been con Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator	ducted in the closed laboratory fa 18 TE critical for calibration) 10 SN: 104778 SN: 103244 SN: 103245	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893)	and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20
All calibrations have been con Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ER3DV6 Secondary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A RF generator HP 8648C	ducted in the closed laboratory fa 4&TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: 55277 (20x) SN: 789	Call Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 14-Jan-19 (No. DAE4-789_Jan19) 09-Oct-18 (No. ER3-2328_Oct18) Check Date (in house) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18)	and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Jan-20 Jan-20 Oct-19 Scheduled Check In house check: Jun-20 In house check: Jun-20 In house check: Jun-20
All calibrations have been con Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ER3DV6 Secondary Standards Power meter E4419B Power sensor E4412A	ducted in the closed laboratory fa M&TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: 55277 (20x) SN: 789 SN: 2328 ID SN: GB41293874 SN: MY41498087 SN: 000110210	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. DAE4-789_Jan19) 09-Oct-18 (No. ER3-2328_Oct18) Check Date (in house) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18)	and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Jan-20 Jan-20 Oct-19 Scheduled Check In house check: Jun-20 In house check: Jun-20
All calibrations have been con Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ER3DV6 Secondary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A RF generator HP 8648C	ducted in the closed laboratory fa M&TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: 55277 (20x) SN: 789 SN: 2328 ID SN: GB41293874 SN: MY41498087 SN: 000110210 SN: US3642U01700	Cility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02892) 04-Apr-19 (No. 217-02893) 04-Apr-19 (No. DAE4-789_Jan19) 09-Oct-18 (No. ER3-2328_Oct18) Check Date (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18)	and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Jan-20 Oct-19 Scheduled Check In house check: Jun-20 In house check: Jun-20 In house check: Jun-20 In house check: Jun-20
All calibrations have been con Calibration Equipment used (M Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ER3DV6 Secondary Standards Power meter E44198 Power sensor E4412A RF generator HP 8648C Network Analyzor E8358A	ducted in the closed laboratory fa 46.TE critical for calibration) ID SN: 104778 SN: 103244 SN: 103245 SN: 23245 SN: 2328 ID SN: GB41293874 SN: GB41293874 SN: MY41498087 SN: 000110210 SN: US3642U01700 SN: US41080477 Name	Cility: environment temperature (22 ± 3)*C Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 14-Jan-19 (No. DAE4-789_Jan19) 09-Oct-18 (No. ER3-2328_Oct18) Check Date (in house) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 04-Aug-99 (in house check Jun-18) 31-Mar-14 (in house check Oct-18) Function	and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Jan-20 Cct-19 Scheduled Check In house check: Jun-20 In house check: Cot-19
All calibrations have been con Calibration Equipment used (h Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator DAE4 Reference Probe ER3DV6 Secondary Standards Power meter E44198 Power sensor E4412A RF generator HP 8648C Network Analyzor E8358A Calibrated by:	ID ID ID SN: 104778 SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 55277 (20x) SN: 2328 ID SN: 6B41293874 SN: 000110210 SN: WY41498087 SN: US3642U01700 SN: US41080477 Name Maru Setz Katja Pokovic: Katja Pokovic:	Cility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 04-Apr-19 (No. 217-02892) 04-Apr-19 (No. 217-02894) 14-Jan-19 (No. DAE4-789_Jan19) 09-Oct-18 (No. ER3-2328_Oct18) Check Date (in house) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 06-Apr-16 (in house check Jun-18) 04-Aug-99 (in house check Jun-18) 31-Mar-14 (in house check Oct-18) Function Laboratory Technician	and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Jan-20 Cct-19 Scheduled Check In house check: Jun-20 In house check: Cot-19





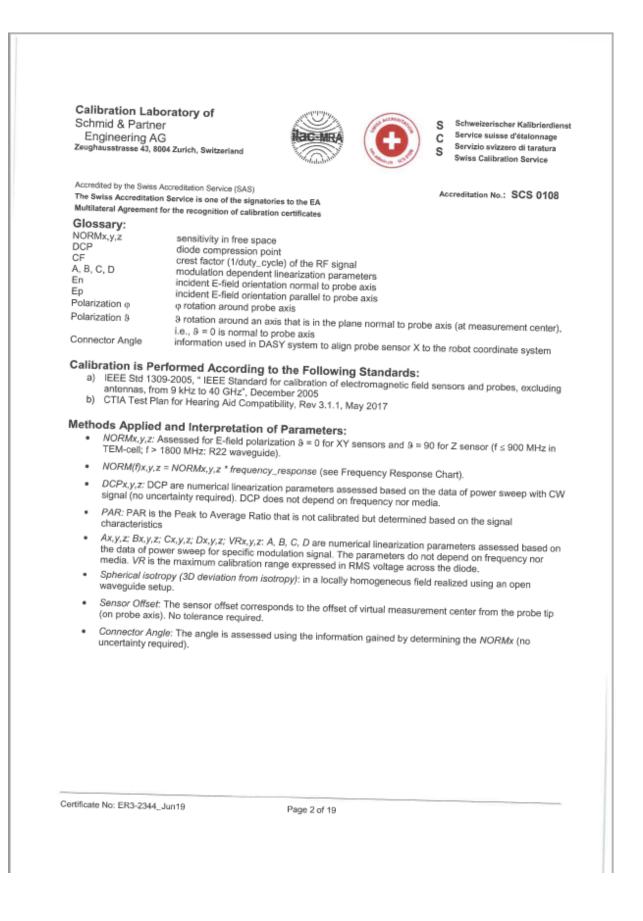



ER3DV6 - SN:2344

June 24, 2019

DASY/EASY - Parameters of Probe: ER3DV6 - SN:2344

Basic Calibration Parameters

	Conces V			
	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m) ²)	1.63	1.76	1.68	
DCP (mV) ⁸	99.6			± 10.1 %
	33.0	100.3	98.2	

Calibration results for Frequency Response (30 MHz - 3 GHz)

Frequency MHz	Target E-Field V/m	Measured E-field (En) V/m	Deviation E-normal in %	Measured E-field (Ep) V/m	Deviation E-normal	Unc (k≈2) %
30	77.3	76.6	-0.9%	77.4	in %	
100	77.4	78.7	1.7%		0.2%	± 5.1%
450	76.9	78.3		77.9	0.7%	± 5.1%
600	77.1		1.8%	77.8	1.1%	± 5.1 %
750		78.2	1.4%	77.5	0.5%	± 5.1 %
750	77.2	78.2	1.2%	77.5	0.4%	± 5.1 %
1800	143.1	141.6	4.00/			
2000	135.2		-1.0%	141.0	-1.4%	± 5.1 %
2200		134.5	-0.5%	133.6	-1.2%	± 5.1 %
	127.7	126.2	-1.2%	127.7	0.0%	± 5.1 %
2500	125.5	126.0	0.4%	127.3	1.4%	the second se
3000	79.4	78.2	-1.4%	81.1		± 5.1 %
			- 1470	01.1	2.1%	± 5.1 %

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^a Numerical linearization parameter: uncertainty not required.
^c Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the

Certificate No: ER3-2344_Jun19

Page 3 of 19





ER3DV6 - SN:2344

June 24, 2019

DASY/EASY - Parameters of Probe: ER3DV6 - SN:2344

Calibration Results for Modulation Response

UID	Communication System Name		A dB	B dBõV	с	D dB	VR mV	Max dev.	Max Unc ^E
0	CW	X	0.00	0.00	1.00	0.00	216.3	± 2.5 %	(k=2) ± 4.7 %
		Y	0.00	0.00	1.00	0.000	214.3	12.5 /0	2 4.7 26
40050		Z	0.00	0.00	1.00	1	200.5	1	
10352- AAA	Pulse Waveform (200Hz, 10%)	X	10.38	83.10	20.80	10.00	60.0	+20%	± 9.6 %
AAA		Y	10.36	82.67	21.43	10.00	60.0	12.0 %	± 9.0 %
40050	B	Z	10.52	82.75	22.13	1	60.0	-	
10353- AAA	Pulse Waveform (200Hz, 20%)	X	10.36	83.87	19.67	6.99	80.0	±2.7% ±9.6	± 9.6 %
AAA		Y	10.21	83.68	20.34	0.00	80.0		± 9.6 %
10001		Z	11.16	85.20	21.53		80.0	-	
10354-	Pulse Waveform (200Hz, 40%)	X	15.00	89.57	19.84	3.98	95.0	+30%	± 9.6 %
AAA		Y	15.00	90.39	20.82	0.00	95.0	4 0.0 %	1 0.0 %
		Z	15.00	91.07	21.62		95.0	1	
10355-	Pulse Waveform (200Hz, 60%)	X	15.00	86.11	16.33	2.22	120.0	± 3.8 %	± 9.6 %
AAA		Y	15.00	89.66	18.67		120.0		
1.0.0.00		Z	15.00	91.98	20.24		120.0		
10387-	QPSK Waveform, 1 MHz	X	1.12	65.47	12.08	0.00	150.0		± 9.6 %
AAA		Y	1.24	66.47	13.07	0.00	150.0	± 2.2 %	± 9.6 %
		Z	0.94	64.22	11.03		150.0		
10388-	QPSK Waveform, 10 MHz	X	2.55	69.49	16.18	0.00	150.0	44.0.0/	1000
AAA		Y	2.63	69.83	16.35	0.00	150.0	± 1.3 %	± 9.6 %
		Z	2.54	69.81	16.49		150.0		
10396-	64-QAM Waveform, 100 kHz	X	4.36	76.16	21.88	3.01	150.0	+0.0 W	± 9.6 %
AAA		Y	4.54	76.35	21.88	0.01	150.0	± 0.0 %	± 9.6 %
		Z	5.29	79.05	23.00		150.0		
10399-	64-QAM Waveform, 40 MHz	X	3.63	67.41	15.88	0.00	150.0	+ 1 7 9/	±9.6%
4.A.A		Y	3.66	67.50	15.92	0.00	150.0	± 1.7 %	I 9.0 %
		Z	3.64	67.59	16.05	-	150.0		
10414-	WLAN CCDF, 64-QAM, 40MHz	X	5.08	65.84	15.67	0.00	150.0	+20%	+0.0.0
AAA		Y	5.12	65.84	15.65	0.00	150.0	x 3.3 %	±9.6 %
	tetails on LIID parameters and Ann	Z	4.85	65.27	15.42	-	150.0	± 3.9 %	

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^a Numerical linearization parameter: uncertainty not required.
^c Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: ER3-2344_Jun19

Page 4 of 19





ER3DV6 - SN:2344

June 24, 2019

DASY/EASY - Parameters of Probe: ER3DV6 - SN:2344

Sensor Frequency Model Parameters

Soneor V	A H		
	Sensor Y	Sensor Z	
-1.67	-1.70	0.00	
0.00		0.36	
0.00	0.00	0.00	
	Sensor X -1.67 0.00	-1.67 -1.70	

Sensor Model Parameters

	C1 fF	C2 fF	α V ⁻¹	T1 ms.V ⁻²	T2 ms.V ⁻¹	T3 ms	T4 V-2	T5 V~1	Т6
Х	93.3	450.60	36.87	27.36	1.75				
Y	103.5	496.01				5.10	0.00	0.67	1.02
7	the second se		36.42	28.88	2.49	5.10	0.00	0.72	1.02
2	80.8	390.98	37.12	29.73	3.30	5.10	0.00	0.82	1.02
					0.00	0.10	0.00	0.62	1.0

Other Probe Parameters

Sensor Arrangement	Rectangular
Connector Angle (°)	
Mechanical Surface Detection Mode	-22
Optical Surface Detection Mode	enabled
	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	
Fip Diameter	10 mm
Probe Tip to Sensor X Calibration Point	8 mm
	2.5 mm
Probe Tip to Sensor Y Calibration Point	2.5 mm
Probe Tip to Sensor Z Calibration Point	2.5 mm

Certificate No: ER3-2344_Jun19

Page 5 of 19






ER3DV6 - SN:2344 June 24, 2019 Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$ f=600 MHz,TEM,0° f=2500 MHz,R22,0° Tet z × 0 e Z Tot Receiving Pattern (ϕ), $\vartheta = 90^{\circ}$ f=600 MHz, TEM, 90° f=2500 MHz,R22,90° 52 0.4 0.0 × °, . Tet x . Tot z Certificate No: ER3-2344_Jun19 Page 6 of 19



CAICT No.I20Z60681-SEM01

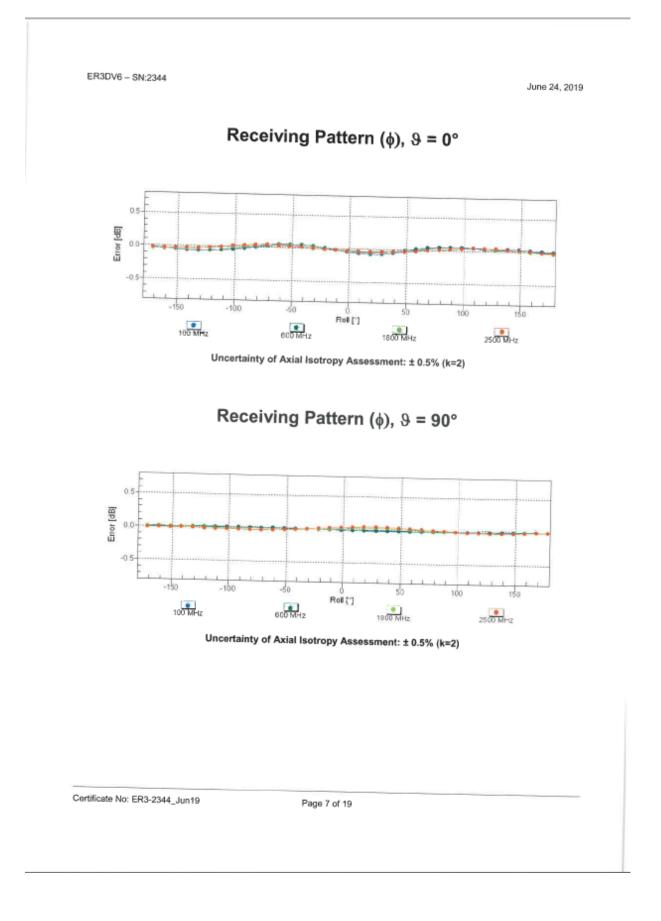







ER3DV6 - SN:2344

June 24, 2019

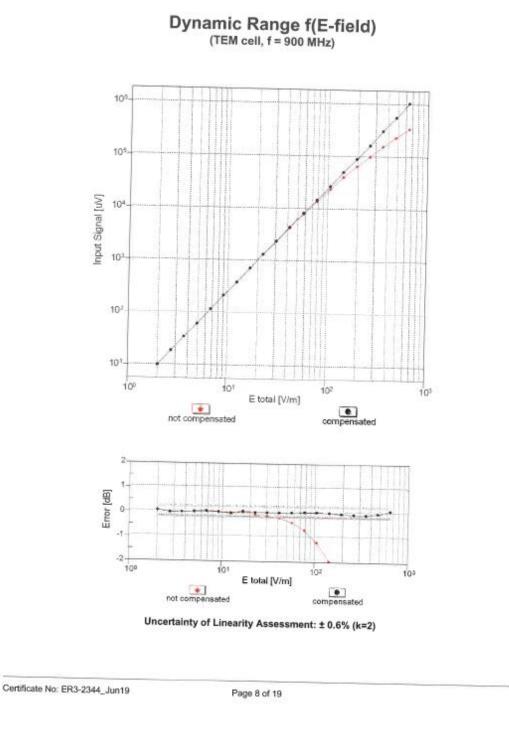





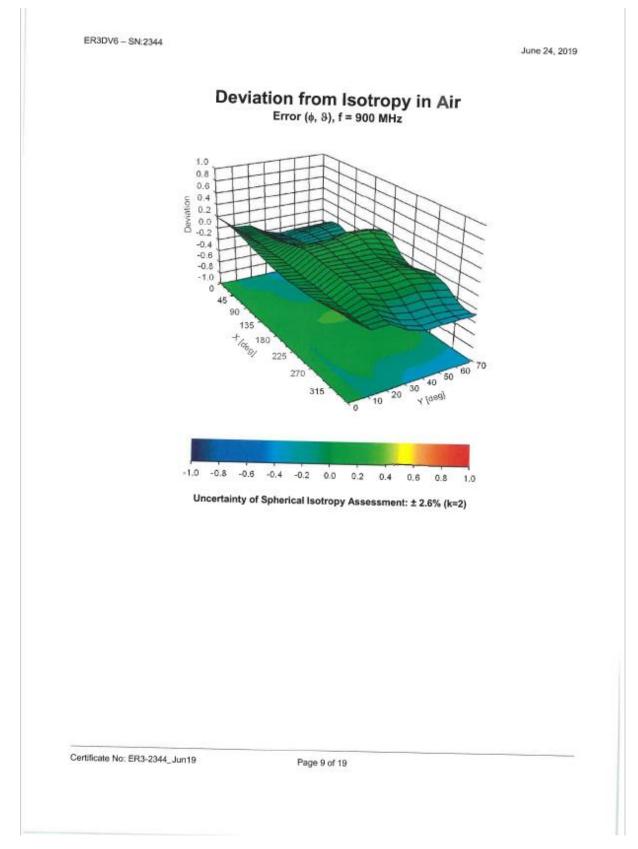





ANNEX E DIPOLE CALIBRATION CERTIFICATE

Dipole 835 MHz

Engineering AG eughausstrasse 43, 8004 Zurich, S	Switzerland	SC MRA	Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
ccredited by the Swiss Accreditation he Swiss Accreditation Service is ultilateral Agreement for the reco	one of the signatories	to the EA	ccreditation No.: SCS 0108
lient CTTL (Auden)		Certificate No	: CD835V3-1023_Aug19
CALIBRATION C	ERTIFICATE		
Object	CD835V3 - SN: 1	023	
	QA CAL-20.v7 Calibration Proce	dure for Validation Sources in ai	r
Calibration date:	August 26, 2019		
Calibration Equipment used (M&TE	critical for calibration)		
Primany Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Primary Standards	ID # SN: 104778	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893)	Scheduled Calibration Apr-20
Power meter NRP	ID # SN: 104778 SN: 103244	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892)	
Power meter NRP Power sensor NRP-Z91	SN: 104778	03-Apr-19 (No. 217-02892/02893)	Apr-20
Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91	SN: 104778 SN: 103244	03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892)	Apr-20 Apr-20
Power meter NRP Power sensor NRP-Z91	SN: 104778 SN: 103244 SN: 103245	03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893)	Apr-20 Apr-20 Apr-20
Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator	SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k)	03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894)	Apr-20 Apr-20 Apr-20 Apr-20
Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination	SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327	03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 04-Apr-19 (No. 217-02895)	Apr-20 Apr-20 Apr-20 Apr-20 Apr-20
Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Probe EF3DV3	SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 4013 SN: 781	03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 04-Apr-19 (No. 217-02895) 03-Jan-19 (No. EF3-4013_Jan19) 09-Jan-19 (No. DAE4-781_Jan19) Check Date (in house)	Apr-20 Apr-20 Apr-20 Apr-20 Jan-20 Jan-20 Scheduled Check
Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Probe EF3DV3 DAE4 Secondary Standards Power meter Agilent 4419B	SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 4013 SN: 781 ID # SN: GB42420191	03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 04-Apr-19 (No. 217-02895) 03-Jan-19 (No. EF3-4013_Jan19) 09-Jan-19 (No. DAE4-781_Jan19) Check Date (in house) 09-Oct-09 (in house check Oct-17)	Apr-20 Apr-20 Apr-20 Apr-20 Jan-20 Jan-20 Scheduled Check In house check: Oct-20
Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Probe EF3DV3 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP E4412A	SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 4013 SN: 781 ID # SN: GB42420191 SN: US38485102	03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 04-Apr-19 (No. 217-02895) 03-Jan-19 (No. EF3-4013_Jan19) 09-Jan-19 (No. DAE4-781_Jan19) Check Date (in house) 09-Oct-09 (in house check Oct-17) 05-Jan-10 (in house check Oct-17)	Apr-20 Apr-20 Apr-20 Apr-20 Jan-20 Jan-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Probe EF3DV3 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP E4412A Power sensor HP 8482A	SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 4013 SN: 781 ID # SN: GB42420191 SN: US38485102 SN: US37295597	03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 04-Apr-19 (No. 217-02895) 03-Jan-19 (No. 217-02895) 03-Jan-19 (No. DAE4-781_Jan19) 09-Jan-19 (No. DAE4-781_Jan19) Check Date (in house) 09-Oct-09 (in house check Oct-17) 05-Jan-10 (in house check Oct-17) 09-Oct-09 (in house check Oct-17)	Apr-20 Apr-20 Apr-20 Apr-20 Jan-20 Jan-20 Scheduled Check In house check: Oct-20 In house check: Oct-20 In house check: Oct-20
Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Probe EF3DV3 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP E4412A Power sensor HP 8482A RF generator R&S SMT-06	SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 4013 SN: 781 ID # SN: GB42420191 SN: US38485102 SN: US37295597 SN: 837633/005	03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02895) 03-Jan-19 (No. 217-02895) 03-Jan-19 (No. DAE4-781_Jan19) 09-Jan-19 (No. DAE4-781_Jan19) Check Date (in house) 09-Oct-09 (in house check Oct-17) 05-Jan-10 (in house check Oct-17) 09-Oct-09 (in house check Oct-17) 10-Jan-19 (in house check Jan-19)	Apr-20 Apr-20 Apr-20 Apr-20 Jan-20 Jan-20 Scheduled Check In house check: Oct-20 In house check: Oct-20 In house check: Oct-20 In house check: Oct-20 In house check: Oct-22
Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Probe EF3DV3 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP E4412A	SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 4013 SN: 781 ID # SN: GB42420191 SN: US38485102 SN: US37295597 SN: 837633/005 SN: US41080477	03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 04-Apr-19 (No. 217-02895) 03-Jan-19 (No. 2F3-4013_Jan19) 09-Jan-19 (No. DAE4-781_Jan19) 09-Oct-09 (in house check Oct-17) 05-Jan-10 (in house check Oct-17) 09-Oct-09 (in house check Oct-17) 10-Jan-19 (in house check Oct-17) 31-Mar-14 (in house check Oct-18)	Apr-20 Apr-20 Apr-20 Apr-20 Jan-20 Jan-20 Scheduled Check In house check: Oct-20 In house check: Oct-19
Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Probe EF3DV3 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP E4412A Power sensor HP E442A RF generator R&S SMT-06	SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 4013 SN: 781 ID # SN: GB42420191 SN: US38485102 SN: US37295597 SN: 837633/005	03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02895) 03-Jan-19 (No. 217-02895) 03-Jan-19 (No. DAE4-781_Jan19) 09-Jan-19 (No. DAE4-781_Jan19) Check Date (in house) 09-Oct-09 (in house check Oct-17) 05-Jan-10 (in house check Oct-17) 09-Oct-09 (in house check Oct-17) 10-Jan-19 (in house check Jan-19)	Apr-20 Apr-20 Apr-20 Apr-20 Jan-20 Jan-20 Scheduled Check In house check: Oct-20 In house check: Oct-20 In house check: Oct-20 In house check: Oct-20 In house check: Oct-20
Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Probe EF3DV3 DAE4 Secondary Standards Power meter Agilent 4419B Power sensor HP E4412A Power sensor HP E4412A RF generator R&S SMT-06 Network Analyzer Agilent E8358A	SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 4013 SN: 781 ID # SN: GB42420191 SN: US38485102 SN: US37295597 SN: 837633/005 SN: US41080477 Name	03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 04-Apr-19 (No. 217-02895) 03-Jan-19 (No. 2F3-4013_Jan19) 09-Jan-19 (No. DAE4-781_Jan19) 09-Jan-19 (No. DAE4-781_Jan19) 09-Oct-09 (in house check Oct-17) 05-Jan-10 (in house check Oct-17) 05-Jan-10 (in house check Oct-17) 10-Jan-19 (in house check Oct-17) 31-Mar-14 (in house check Oct-18) Function	Apr-20 Apr-20 Apr-20 Apr-20 Jan-20 Jan-20 Scheduled Check In house check: Oct-20 In house check: Oct-20 In house check: Oct-20 In house check: Oct-20 In house check: Oct-21 In house check: Oct-22 In house check: Oct-19

Certificate No: CD835V3-1023_Aug19

Page 1 of 5





Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst C Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

References

- [1] ANSI-C63.19-2011
 - American National Standard, Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

Methods Applied and Interpretation of Parameters:

- Coordinate System: y-axis is in the direction of the dipole arms. z-axis is from the basis of the antenna (mounted on the table) towards its feed point between the two dipole arms. x-axis is normal to the other axes. In coincidence with the standards [1], the measurement planes (probe sensor center) are selected to be at a distance of 15 mm above the top metal edge of the dipole arms.
- Measurement Conditions: Further details are available from the hardcopies at the end of the certificate. All
 figures stated in the certificate are valid at the frequency indicated. The forward power to the dipole connector
 is set with a calibrated power meter connected and monitored with an auxiliary power meter connected to a
 directional coupler. While the dipole under test is connected, the forward power is adjusted to the same level.
- Antenna Positioning: The dipole is mounted on a HAC Test Arch phantom using the matching dipole positioner with the arms horizontal and the feeding cable coming from the floor. The measurements are performed in a shielded room with absorbers around the setup to reduce the reflections. It is verified before the mounting of the dipole under the Test Arch phantom, that its arms are perfectly in a line. It is installed on the HAC dipole positioner with its arms parallel below the dielectric reference wire and able to move elastically in vertical direction without changing its relative position to the top center of the Test Arch phantom. The vertical distance to the probe is adjusted after dipole mounting with a DASY5 Surface Check job. Before the measurement, the distance between phantom surface and probe tip is verified. The proper measurement distance is selected by choosing the matching section of the HAC Test Arch phantom with the proper device reference point (upper surface of the dipole) and the matching grid reference point (tip of the probe) considering the probe sensor offset. The vertical distance to the probe is essential for the accuracy.
- Feed Point Impedance and Return Loss: These parameters are measured using a Vector Network Analyzer. The impedance is specified at the SMA connector of the dipole. The influence of reflections was eliminating by applying the averaging function while moving the dipole in the air, at least 70cm away from any obstacles.
- E-field distribution: E field is measured in the x-y-plane with an isotropic E-field probe with 100 mW forward
 power to the antenna feed point. In accordance with [1], the scan area is 20mm wide, its length exceeds the
 dipole arm length (180 or 90mm). The sensor center is 15 mm (in z) above the metal top of the dipole arms.
 Two 3D maxima are available near the end of the dipole arms. Assuming the dipole arms are perfectly in one
 line, the average of these two maxima (in subgrid 2 and subgrid 8) is determined to compensate for any nonparallelity to the measurement plane as well as the sensor displacement. The E-field value stated as
 calibration value represents the maximum of the interpolated 3D-E-field, in the plane above the dipole surface.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: CD835V3-1023_Aug19

Page 2 of 5





Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.2
Phantom	HAC Test Arch	
Distance Dipole Top - Probe Center	15 mm	
Scan resolution	dx, dy = 5 mm	
Frequency	835 MHz ± 1 MHz	
Input power drift	< 0.05 dB	

Maximum Field values at 835 MHz

E-field 15 mm above dipole surface	condition	Interpolated maximum
Maximum measured above high end	100 mW input power	106.7 V/m = 40.56 dBV/m
Maximum measured above low end	100 mW input power	106.6 V/m = 40.56 dBV/m
Averaged maximum above arm	100 mW input power	106.7 V/m ± 12.8 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters

Frequency	Return Loss	Impedance
800 MHz	17.2 dB	41.4 Ω - 9.3 jΩ
835 MHz	25.2 dB	52.6 Ω + 5.0 jΩ
880 MHz	16.4 dB	62.6 Ω - 11.7 jΩ
900 MHz	16.2 dB	52.8 Ω - 15.9 jΩ
945 MHz	24.1 dB	45.6 Ω + 4.0 jΩ

3.2 Antenna Design and Handling

The calibration dipole has a symmetric geometry with a built-in two stub matching network, which leads to the enhanced bandwidth.

The dipole is built of standard semirigid coaxial cable. The internal matching line is open ended. The antenna is therefore open for DC signals.

Do not apply force to dipole arms, as they are liable to bend. The soldered connections near the feedpoint may be damaged. After excessive mechanical stress or overheating, check the impedance characteristics to ensure that the internal matching network is not affected.


After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

Page 3 of 5





Impedance Measurement Plot

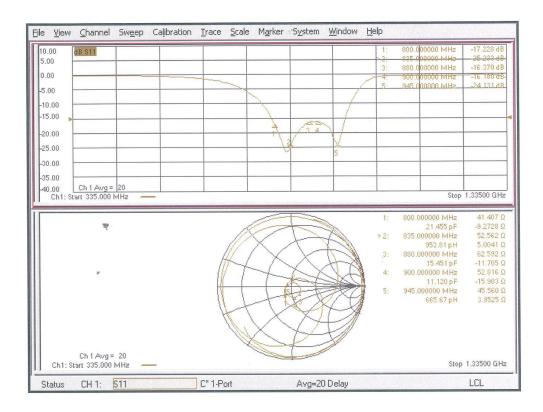

Page 4 of 5





DASY5 E-field Result

Date: 26.08.2019

Test Laboratory: SPEAG Lab2

DUT: HAC-Dipole 835 MHz; Type: CD835V3; Serial: CD835V3 - SN: 1023

 $\begin{array}{l} Communication \ System: \ UID \ 0 \ - \ CW \ ; \ Frequency: \ 835 \ MHz \\ Medium \ parameters \ used: \ \sigma = 0 \ S/m, \ \epsilon_r = 1; \ \rho = 0 \ kg/m^3 \\ Phantom \ section: \ RF \ Section \\ Measurement \ Standard: \ DASY5 \ (IEEE/IEC/ANSI \ C63.19-2011) \\ \end{array}$

DASY52 Configuration:


- Probe: EF3DV3 SN4013; ConvF(1, 1, 1) @ 835 MHz; Calibrated: 03.01.2019
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn781; Calibrated: 09.01.2019
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- DASY52 52.10.2(1504); SEMCAD X 14.6.12(7470)

Dipole E-Field measurement @ 835MHz/E-Scan - 835MHz d=15mm/Hearing Aid Compatibility Test (41x361x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm

Reference Value = 127.9 V/m; Power Drift = -0.01 dB Applied MIF = 0.00 dB RF audio interference level = 40.56 dBV/m Emission category: M3

MIF scaled E-field

Grid 1 M3	Grid 2 M3	Grid 3 M3
40.08 dBV/m	40.56 dBV/m	40.51 dBV/m
Grid 4 M4	Grid 5 M4	Grid 6 M4
35.34 dBV/m	35.68 dBV/m	35.67 dBV/m
Grid 7 M3	Grid 8 M3	Grid 9 M3
40.23 dBV/m	40.56 dBV/m	40.49 dBV/m

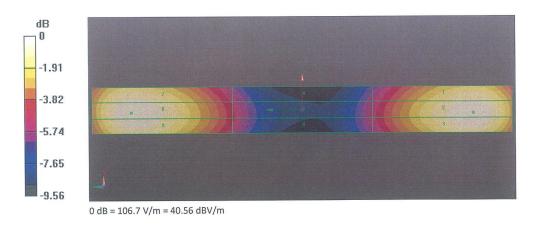

Certificate No: CD835V3-1023_Aug19

Page 5 of 5





Dipole 1880 MHz

Calibration Laboratory Schmid & Partner Engineering AG eughausstrasse 43, 8004 Zurich, S		BIC MEA	Sonvizio evizzoro di taratura
ccredited by the Swiss Accreditation he Swiss Accreditation Service is Iultilateral Agreement for the reco	one of the signatories	to the EA	ccreditation No.: SCS 0108
ilient CTTL (Auden)	gintion of calibration of		: CD1880V3-1018_Aug19
CALIBRATION CI	ERTIFICATI		
Object	CD1880V3 - SN:	1018	
Calibration procedure(s)	QA CAL-20.v7 Calibration Proce	dure for Validation Sources in a	ir
Calibration date:	August 26, 2019		
All calibrations have been conducte Calibration Equipment used (M&TE		ry facility: environment temperature (22 \pm 3)'	°C and humidity < 70%.
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	03-Apr-19 (No. 217-02892/02893)	Apr-20
Power sensor NRP-Z91	SN: 103244	03-Apr-19 (No. 217-02892)	Apr-20
Power sensor NRP-Z91	SN: 103245	03-Apr-19 (No. 217-02893)	Apr-20
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-19 (No. 217-02894)	Apr-20
Type-N mismatch combination	SN: 5047.2 / 06327	04-Apr-19 (No. 217-02895)	Apr-20
Probe EF3DV3	SN: 4013	03-Jan-19 (No. EF3-4013_Jan19)	Jan-20
DAE4	SN: 781	09-Jan-19 (No. DAE4-781_Jan19)	Jan-20
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter Agilent 4419B	SN: GB42420191	09-Oct-09 (in house check Oct-17)	In house check: Oct-20
Power sensor HP E4412A	SN: US38485102	05-Jan-10 (in house check Oct-17)	In house check: Oct-20
Power sensor HP 8482A	SN: US37295597	09-Oct-09 (in house check Oct-17)	In house check: Oct-20
RF generator R&S SMT-06	SN: 837633/005	10-Jan-19 (in house check Jan-19)	In house check: Oct-22
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19
Collington but	Name	Function	Signature
Calibrated by:	Leif Klysner	Laboratory Technician	Set Illen
			/
Approved by:	Katja Pokovic	Technical Manager	flet

Certificate No: CD1880V3-1018_Aug19

Page 1 of 5





Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S

C

S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

References

- [1] ANSI-C63.19-2011
 - American National Standard, Methods of Measurement of Compatibility between Wireless Communications Devices and Hearing Aids.

Methods Applied and Interpretation of Parameters:

- Coordinate System: y-axis is in the direction of the dipole arms. z-axis is from the basis of the antenna (mounted on the table) towards its feed point between the two dipole arms. x-axis is normal to the other axes. In coincidence with the standards [1], the measurement planes (probe sensor center) are selected to be at a distance of 15 mm above the top metal edge of the dipole arms.
- Measurement Conditions: Further details are available from the hardcopies at the end of the certificate. All
 figures stated in the certificate are valid at the frequency indicated. The forward power to the dipole connector
 is set with a calibrated power meter connected and monitored with an auxiliary power meter connected to a
 directional coupler. While the dipole under test is connected, the forward power is adjusted to the same level.
- Antenna Positioning: The dipole is mounted on a HAC Test Arch phantom using the matching dipole positioner with the arms horizontal and the feeding cable coming from the floor. The measurements are performed in a shielded room with absorbers around the setup to reduce the reflections. It is verified before the mounting of the dipole under the Test Arch phantom, that its arms are perfectly in a line. It is installed on the HAC dipole positioner with its arms parallel below the dielectric reference wire and able to move elastically in vertical direction without changing its relative position to the top center of the Test Arch phantom. The vertical distance to the probe is adjusted after dipole mounting with a DASY5 Surface Check job. Before the measurement, the distance between phantom surface and probe tip is verified. The proper measurement distance is selected by choosing the matching section of the HAC Test Arch phantom with the proper device reference point (upper surface of the dipole) and the matching grid reference point (tip of the probe) considering the probe sensor offset. The vertical distance to the probe is essential for the accuracy.
- Feed Point Impedance and Return Loss: These parameters are measured using a Vector Network Analyzer. The impedance is specified at the SMA connector of the dipole. The influence of reflections was eliminating by applying the averaging function while moving the dipole in the air, at least 70cm away from any obstacles.
- E-field distribution: E field is measured in the x-y-plane with an isotropic E-field probe with 100 mW forward
 power to the antenna feed point. In accordance with [1], the scan area is 20mm wide, its length exceeds the
 dipole arm length (180 or 90mm). The sensor center is 15 mm (in z) above the metal top of the dipole arms.
 Two 3D maxima are available near the end of the dipole arms. Assuming the dipole arms are perfectly in one
 line, the average of these two maxima (in subgrid 2 and subgrid 8) is determined to compensate for any nonparallelity to the measurement plane as well as the sensor displacement. The E-field value stated as
 calibration value represents the maximum of the interpolated 3D-E-field, in the plane above the dipole surface.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: CD1880V3-1018_Aug19

Page 2 of 5





Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.2
Phantom	HAC Test Arch	
Distance Dipole Top - Probe Center	15 mm	
Scan resolution	dx, dy = 5 mm	
Frequency	1880 MHz ± 1 MHz	
Input power drift	< 0.05 dB	

Maximum Field values at 1880 MHz

E-field 15 mm above dipole surface	condition	Interpolated maximum
Maximum measured above high end	100 mW input power	88.0 V/m = 38.89 dBV/m
Maximum measured above low end	100 mW input power	86.5 V/m = 38.74 dBV/m
Averaged maximum above arm	100 mW input power	87.3 V/m ± 12.8 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters

Frequency	Return Loss	Impedance
1730 MHz	27.8 dB	54.3 Ω + 0.3 jΩ
1880 MHz	21.6 dB	55.4 Ω + 7.0 jΩ
1900 MHz	22.8 dB	56.3 Ω + 4.5 jΩ
1950 MHz	33.3 dB	52.2 Ω - 0.1 jΩ
2000 MHz	19.4 dB	47.6 Ω + 10.2 jΩ

3.2 Antenna Design and Handling

The calibration dipole has a symmetric geometry with a built-in two stub matching network, which leads to the enhanced bandwidth.

The dipole is built of standard semirigid coaxial cable. The internal matching line is open ended. The antenna is therefore open for DC signals.

Do not apply force to dipole arms, as they are liable to bend. The soldered connections near the feedpoint may be damaged. After excessive mechanical stress or overheating, check the impedance characteristics to ensure that the internal matching network is not affected.


After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

Page 3 of 5





Impedance Measurement Plot

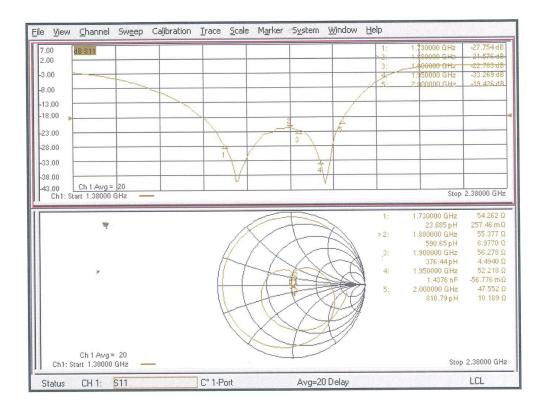

Page 4 of 5





DASY5 E-field Result

Date: 26.08.2019

Test Laboratory: SPEAG Lab2

DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: CD1880V3 - SN: 1018

 $\begin{array}{l} \mbox{Communication System: UID 0 - CW ; Frequency: 1880 MHz \\ \mbox{Medium parameters used: } \sigma = 0 \ S/m, \ \epsilon_r = 1; \ \rho = 0 \ kg/m^3 \\ \mbox{Phantom section: RF Section} \\ \mbox{Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)} \\ \end{array}$

DASY52 Configuration:

- Probe: EF3DV3 SN4013; ConvF(1, 1, 1) @ 1880 MHz; Calibrated: 03.01.2019
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn781; Calibrated: 09.01.2019
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA; Serial: 1070
- DASY52 52.10.2(1504); SEMCAD X 14.6.12(7470)


Dipole E-Field measurement @ 1880MHz/E-Scan - 1880MHz d=15mm/Hearing Aid Compatibility Test (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm Device Reference Point: 0, 0, -6.3 mm

Reference Value = 151.1 V/m; Power Drift = -0.01 dB Applied MIF = 0.00 dB RF audio interference level = 38.89 dBV/m

Emission category: M2

MIF scaled E-field

Grid 1 M2	Grid 2 M2	Grid 3 M2
38.47 dBV/m	38.89 dBV/m	38.86 dBV/m
Grid 4 M2	Grid 5 M2	Grid 6 M2
35.88 dBV/m	36.02 dBV/m	35.97 dBV/m
Grid 7 M2	Grid 8 M2	Grid 9 M2
38.51 dBV/m	38.74 dBV/m	38.6 dBV/m

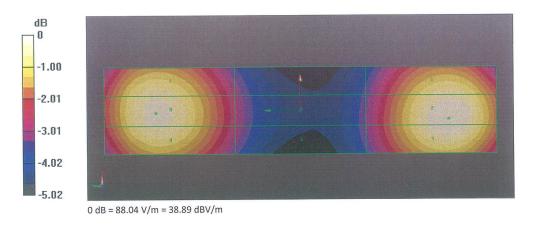

Certificate No: CD1880V3-1018_Aug19

Page 5 of 5





The photos of HAC test are presented in the additional document:

Appendix to test report No.I20Z60681-SEM01

The photos of HAC test