

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL at 5200 MHz

Impedance, transformed to feed point	50.5 Ω - 6.6 jΩ
Return Loss	- 23.7 dB

Antenna Parameters with Head TSL at 5300 MHz

Impedance, transformed to feed point	47.5 Ω - 2.8 jΩ
Return Loss	- 28.3 dB

Antenna Parameters with Head TSL at 5500 MHz

Impedance, transformed to feed point	51.1 Ω - 3.7 jΩ	_
Return Loss	- 28.5 dB	

Antenna Parameters with Head TSL at 5600 MHz

Impedance, transformed to feed point	54.0 Ω + 2.0 jΩ	
Return Loss	- 27.4 dB	

Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	52.3 Ω - 2.9 jΩ	
Return Loss	- 28.9 dB	

Antenna Parameters with Body TSL at 5200 MHz

Impedance, transformed to feed point	49.7 Ω - 4.7 jΩ
Return Loss	- 26.5 dB

Antenna Parameters with Body TSL at 5300 MHz

Impedance, transformed to feed point	46.8 Ω - 1.9 jΩ	
Return Loss	- 28.3 dB	

Antenna Parameters with Body TSL at 5500 MHz

Impedance, transformed to feed point	50.7 Ω - 2.2 jΩ	
Return Loss	- 32.8 dB	

Antenna Parameters with Body TSL at 5600 MHz

Impedance, transformed to feed point	55.1 Ω + 1.2 jΩ	
Return Loss	- 26.1 dB	

Certificate No: D5GHzV2-1060_Jul17

Page 9 of 16



Antenna Parameters with Body TSL at 5800 MHz

Impedance, transformed to feed point	52.5 Ω - 1.9 jΩ
Return Loss	- 30.1 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.202 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	November 27, 2006	

Certificate No: D5GHzV2-1060_Jul17

Page 10 of 16



DASY5 Validation Report for Head TSL

Date: 25.07.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1060

Communication System: UID 0 - CW; Frequency: 5200 MHz, Frequency: 5300 MHz, Frequency: 5500 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz Medium parameters used: f = 5200 MHz; $\sigma = 4.51$ S/m; $\varepsilon_r = 36.3$; $\rho = 1000$ kg/m³, Medium parameters used: f = 5500 MHz; $\sigma = 4.61$ S/m; $\varepsilon_r = 36.1$; $\rho = 1000$ kg/m³, Medium parameters used: f = 5500 MHz; $\sigma = 4.81$ S/m; $\varepsilon_r = 35.8$; $\rho = 1000$ kg/m³, Medium parameters used: f = 5800 MHz; $\sigma = 5.14$ S/m; $\varepsilon_r = 35.4$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN3503; ConvF(5.76, 5.76, 5.76); Calibrated: 31.12.2016, ConvF(5.35, 5.35, 5.35); Calibrated: 31.12.2016, ConvF(5.2, 5.2, 5.2); Calibrated: 31.12.2016, ConvF(5.09, 5.09); Calibrated: 31.12.2016, ConvF(5.01, 5.01, 5.01); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.03.2017
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 70.18 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 29.8 W/kg SAR(1 g) = 8.05 W/kg; SAR(10 g) = 2.30 W/kg Maximum value of SAR (measured) = 18.4 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 69.70 V/m; Power Drift = -0.01 dB Peak SAR (extrapolated) = 30.5 W/kg SAR(1 g) = 8.38 W/kg; SAR(10 g) = 2.4 W/kg Maximum value of SAR (measured) = 19.4 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 68.97 V/m; Power Drift = -0.02 dB Peak SAR (extrapolated) = 33.3 W/kg SAR(1 g) = 8.48 W/kg; SAR(10 g) = 2.41 W/kg Maximum value of SAR (measured) = 20.2 W/kg


Certificate No: D5GHzV2-1060_Jul17

Page 11 of 16



Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 69.72 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 33.6 W/kg SAR(1 g) = 8.45 W/kg; SAR(10 g) = 2.41 W/kg Maximum value of SAR (measured) = 20.2 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 67.66 V/m; Power Drift = -0.02 dB Peak SAR (extrapolated) = 33.2 W/kg SAR(1 g) = 8.10 W/kg; SAR(10 g) = 2.29 W/kg Maximum value of SAR (measured) = 19.6 W/kg

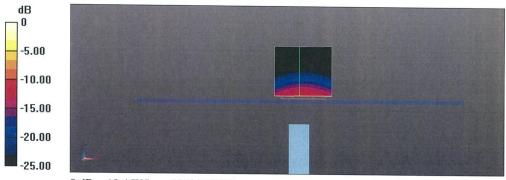


0 dB = 18.4 W/kg = 12.66 dBW/kg

Certificate No: D5GHzV2-1060_Jul17

Page 12 of 16



Impedance Measurement Plot for Head TSL

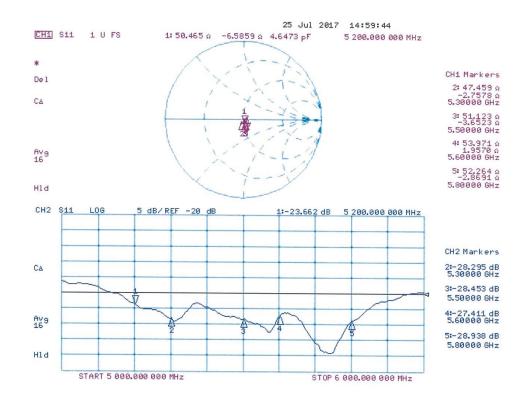

Certificate No: D5GHzV2-1060_Jul17

Page 13 of 16



DASY5 Validation Report for Body TSL

Date: 17.07.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1060

Communication System: UID 0 - CW; Frequency: 5200 MHz, Frequency: 5300 MHz, Frequency: 5500 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz Medium parameters used: f = 5200 MHz; $\sigma = 5.45$ S/m; $\varepsilon_r = 47.4$; $\rho = 1000$ kg/m³, Medium parameters used: f = 5500 MHz; $\sigma = 5.85$ S/m; $\varepsilon_r = 47.2$; $\rho = 1000$ kg/m³, Medium parameters used: f = 5500 MHz; $\sigma = 5.85$ S/m; $\varepsilon_r = 46.9$; $\rho = 1000$ kg/m³, Medium parameters used: f = 5800 MHz; $\sigma = 6.28$ S/m; $\varepsilon_r = 46.4$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN3503; ConvF(5.29, 5.29, 5.29); Calibrated: 31.12.2016, ConvF(5.04, 5.04, 5.04); Calibrated: 31.12.2016, ConvF(4.62, 4.62, 4.62); Calibrated: 31.12.2016, ConvF(4.57, 4.57, 4.57); Calibrated: 31.12.2016, ConvF(4.48, 4.48, 4.48); Calibrated: 31.12.2016;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.03.2017
- Phantom: Flat Phantom 5.0 (back); Type: QD 000 P50 AA; Serial: 1002
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5200MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 64.89 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 29.2 W/kg SAR(1 g) = 7.56 W/kg; SAR(10 g) = 2.13 W/kg Maximum value of SAR (measured) = 18.0 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 64.82 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 30.7 W/kg SAR(1 g) = 7.75 W/kg; SAR(10 g) = 2.18 W/kg Maximum value of SAR (measured) = 18.6 W/kg

```
Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan,
dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
Reference Value = 66.03 V/m; Power Drift = -0.05 dB
Peak SAR (extrapolated) = 34.2 W/kg
SAR(1 g) = 8.19 W/kg; SAR(10 g) = 2.27 W/kg
Maximum value of SAR (measured) = 19.9 W/kg
```


Certificate No: D5GHzV2-1060_Jul17

Page 14 of 16



Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 65.05 V/m; Power Drift = -0.04 dB Peak SAR (extrapolated) = 34.5 W/kg SAR(1 g) = 8.1 W/kg; SAR(10 g) = 2.28 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 63.30 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 35.2 W/kg SAR(1 g) = 7.84 W/kg; SAR(10 g) = 2.19 W/kg Maximum value of SAR (measured) = 19.7 W/kg

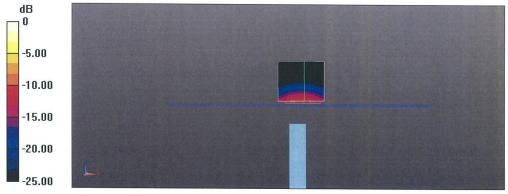


0 dB = 18.0 W/kg = 12.55 dBW/kg

Certificate No: D5GHzV2-1060_Jul17

Page 15 of 16



Impedance Measurement Plot for Body TSL

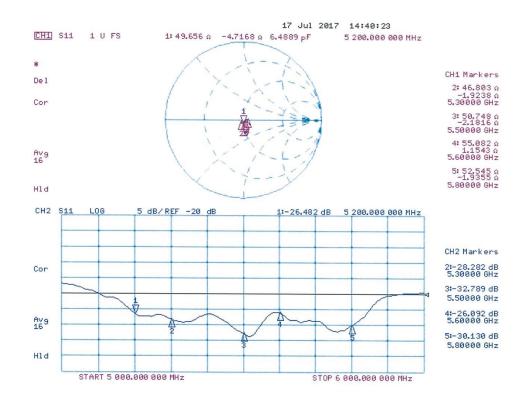

Certificate No: D5GHzV2-1060_Jul17

Page 16 of 16



ANNEX I Accreditation Certificate

