




PLANAR CONICAL
INDUCTOR

WIDEBAND DIPOLE

2

1

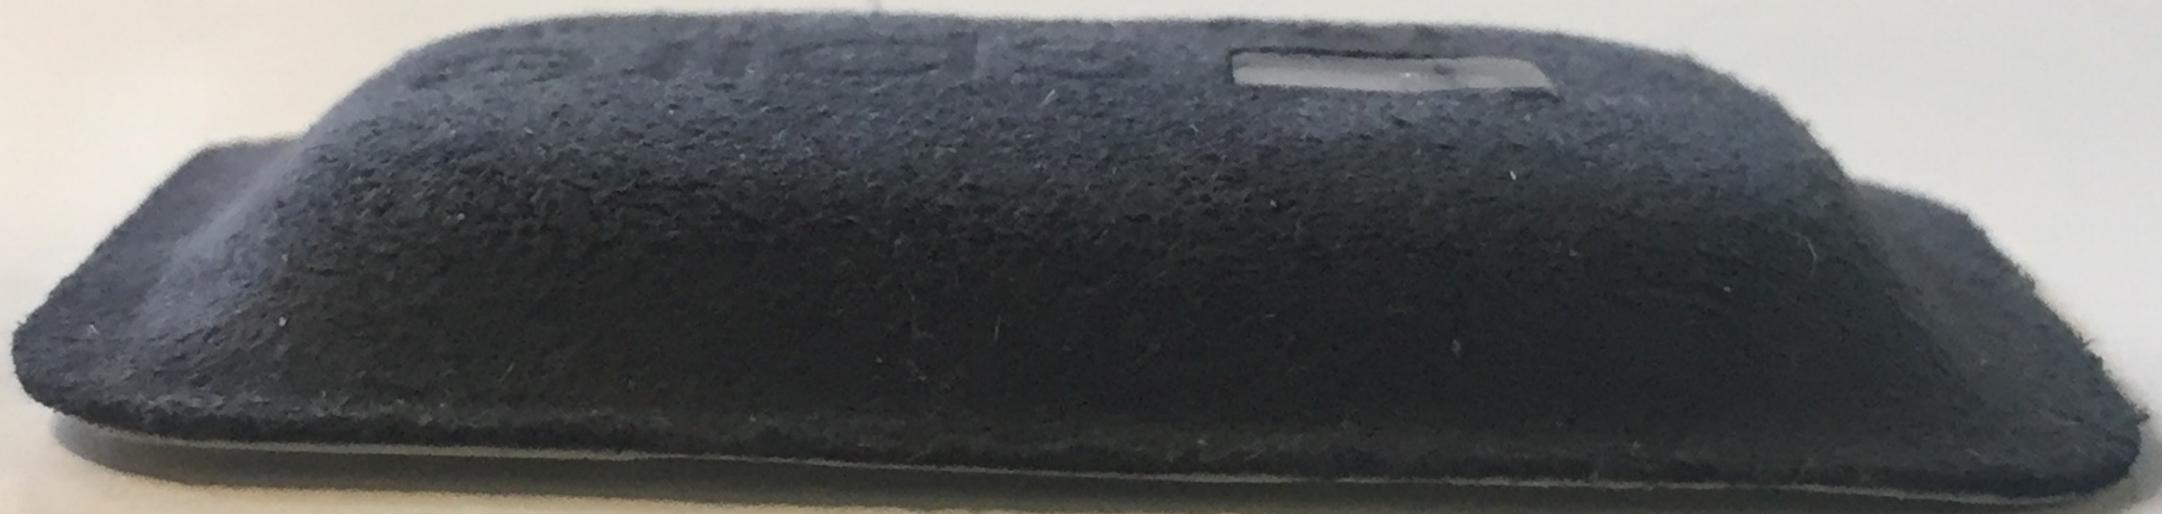

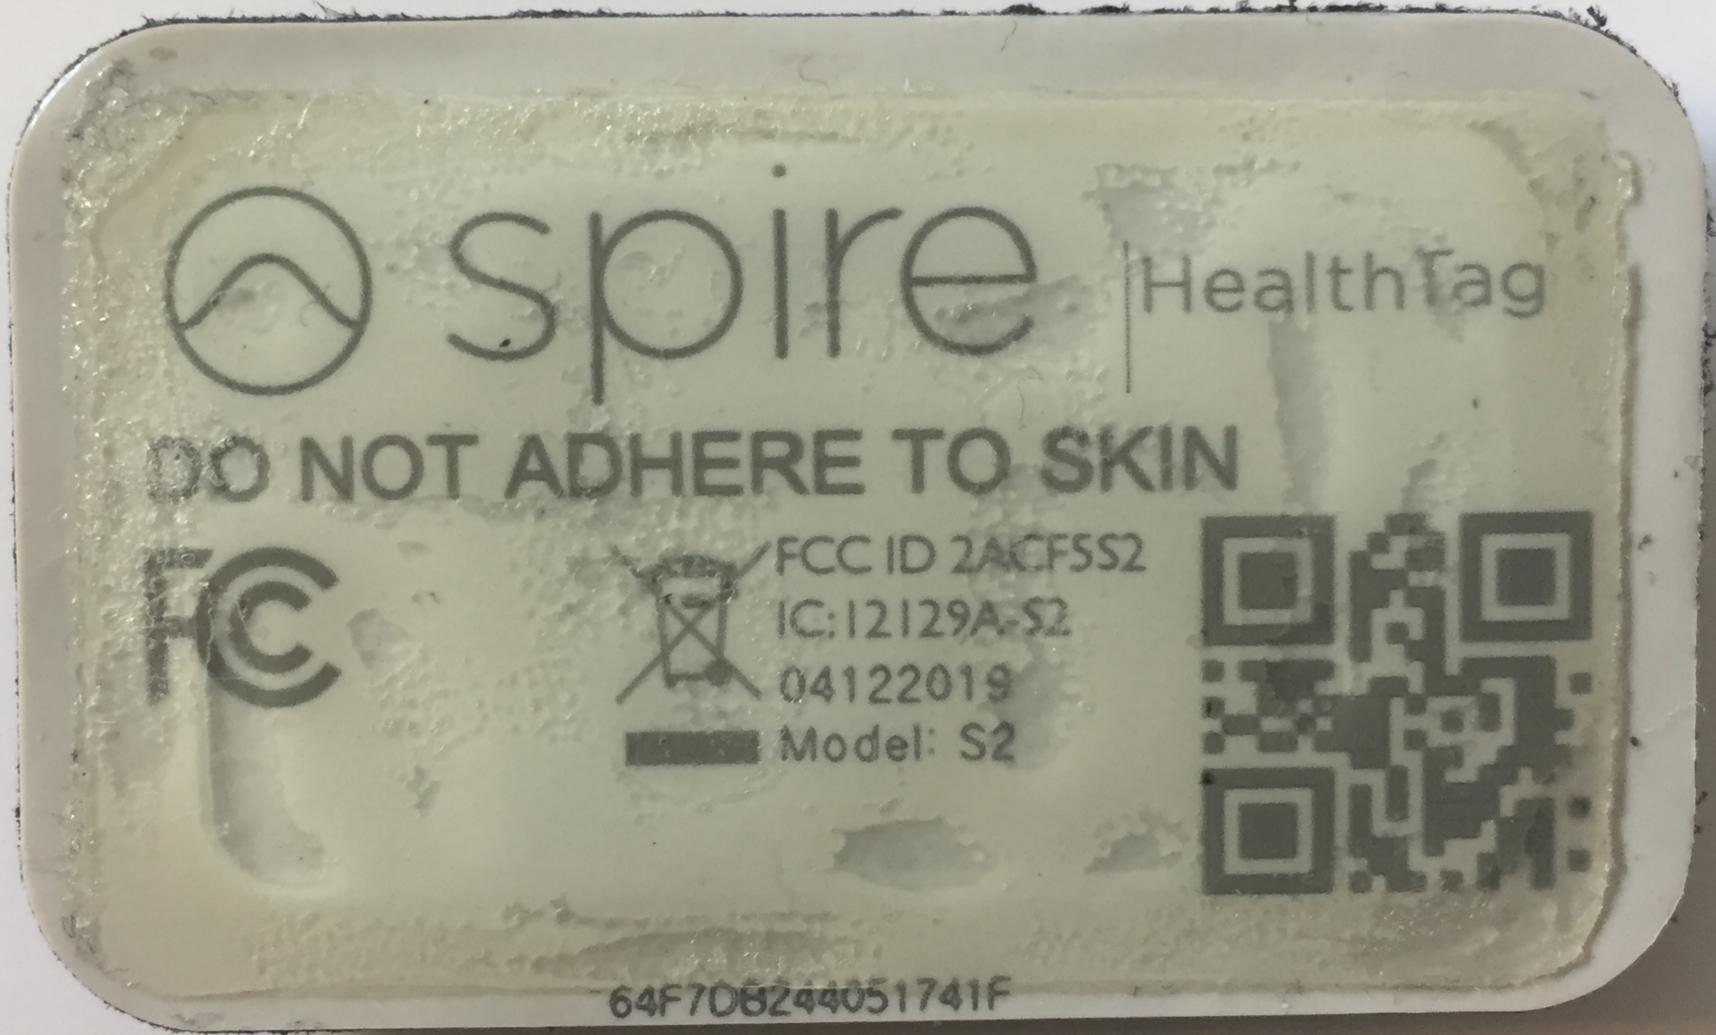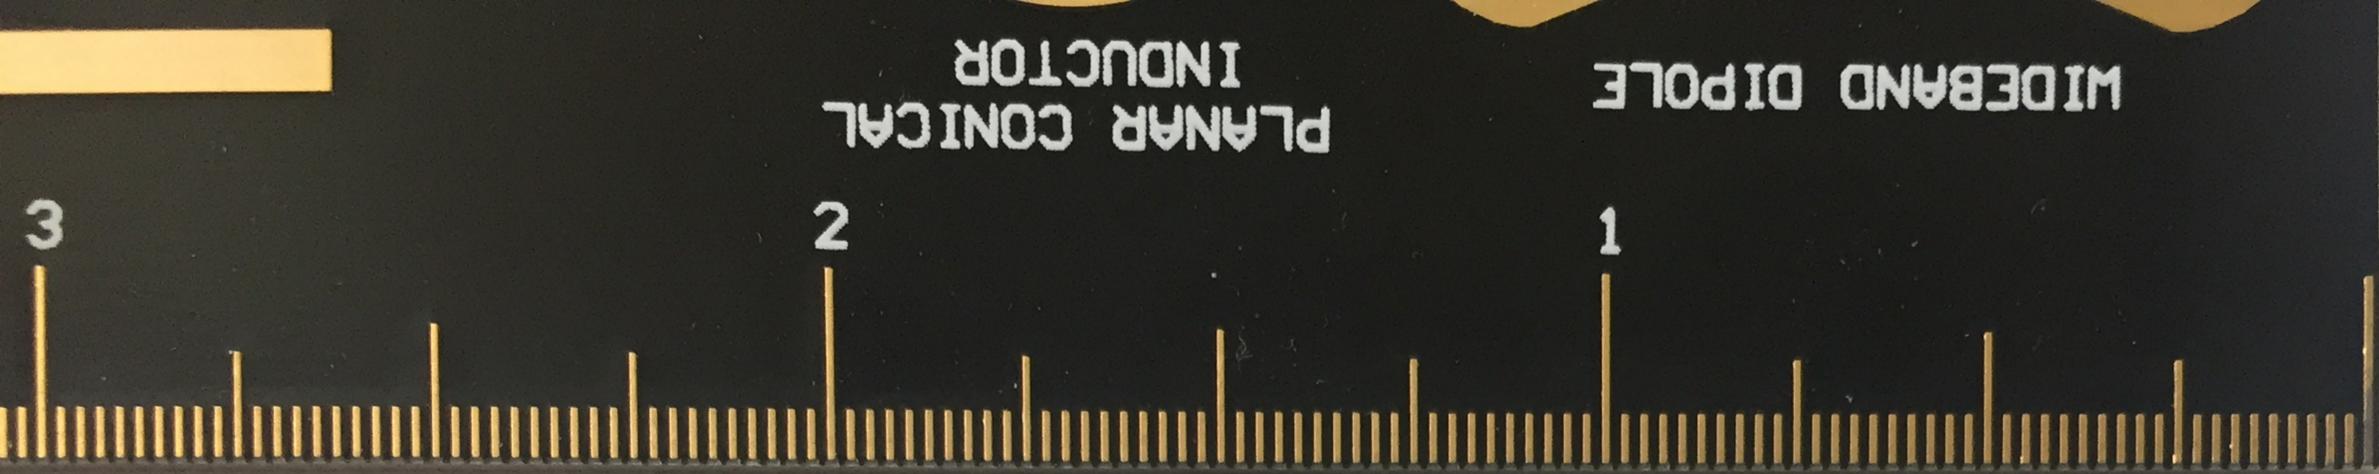


PLANAR CONICAL
INDUCTOR

WIDEBAND DIPOLE

3

2

1

 spire

HealthTag

DO NOT ADHERE TO SKIN

FCC



FCC ID 2ACF552



IC:12129A-S2

04122019

Model: S2





64F708244051741F

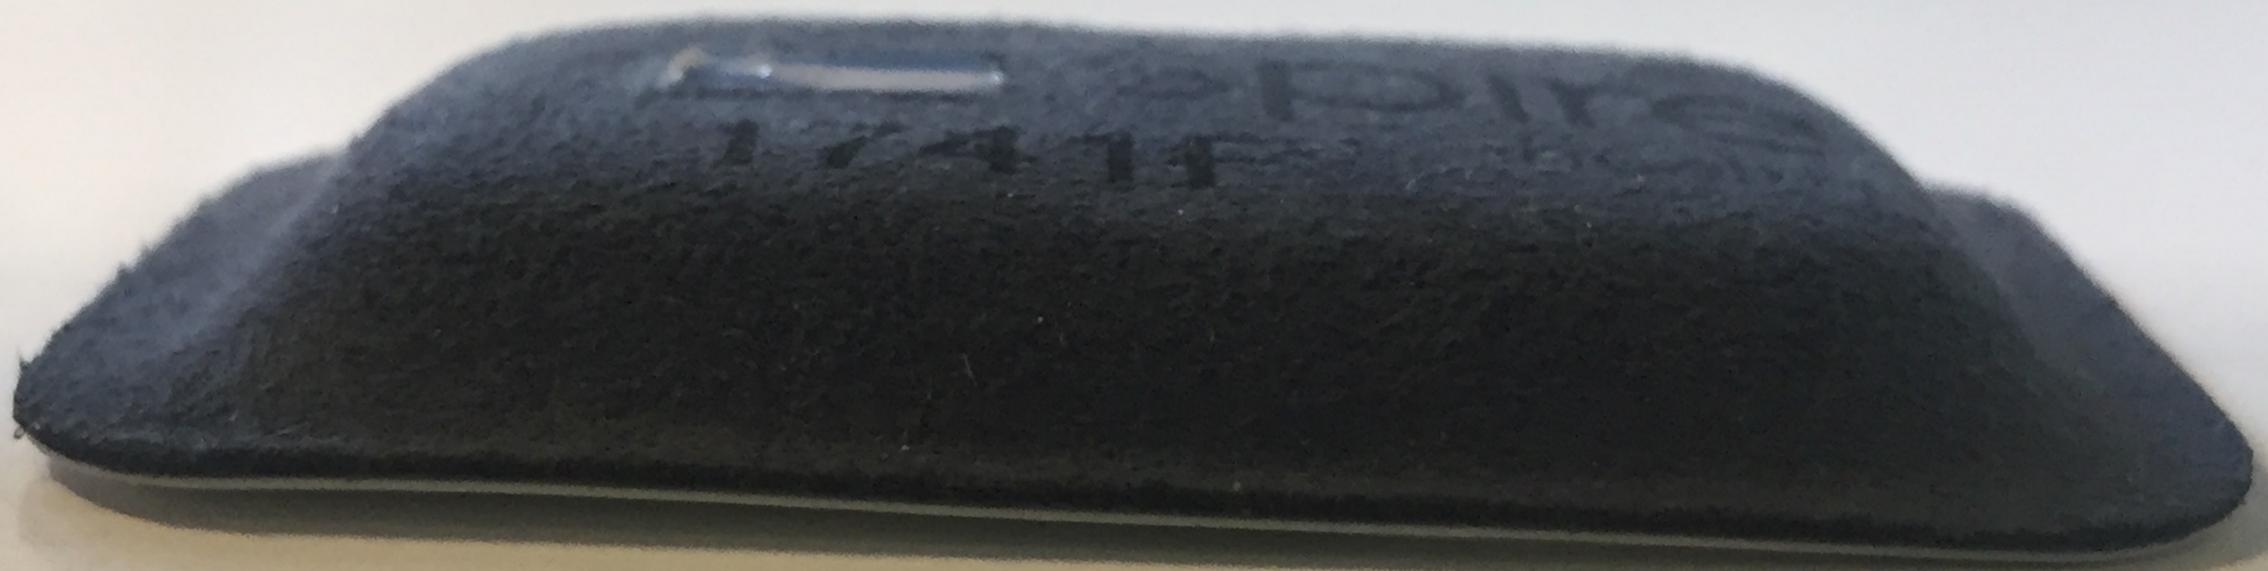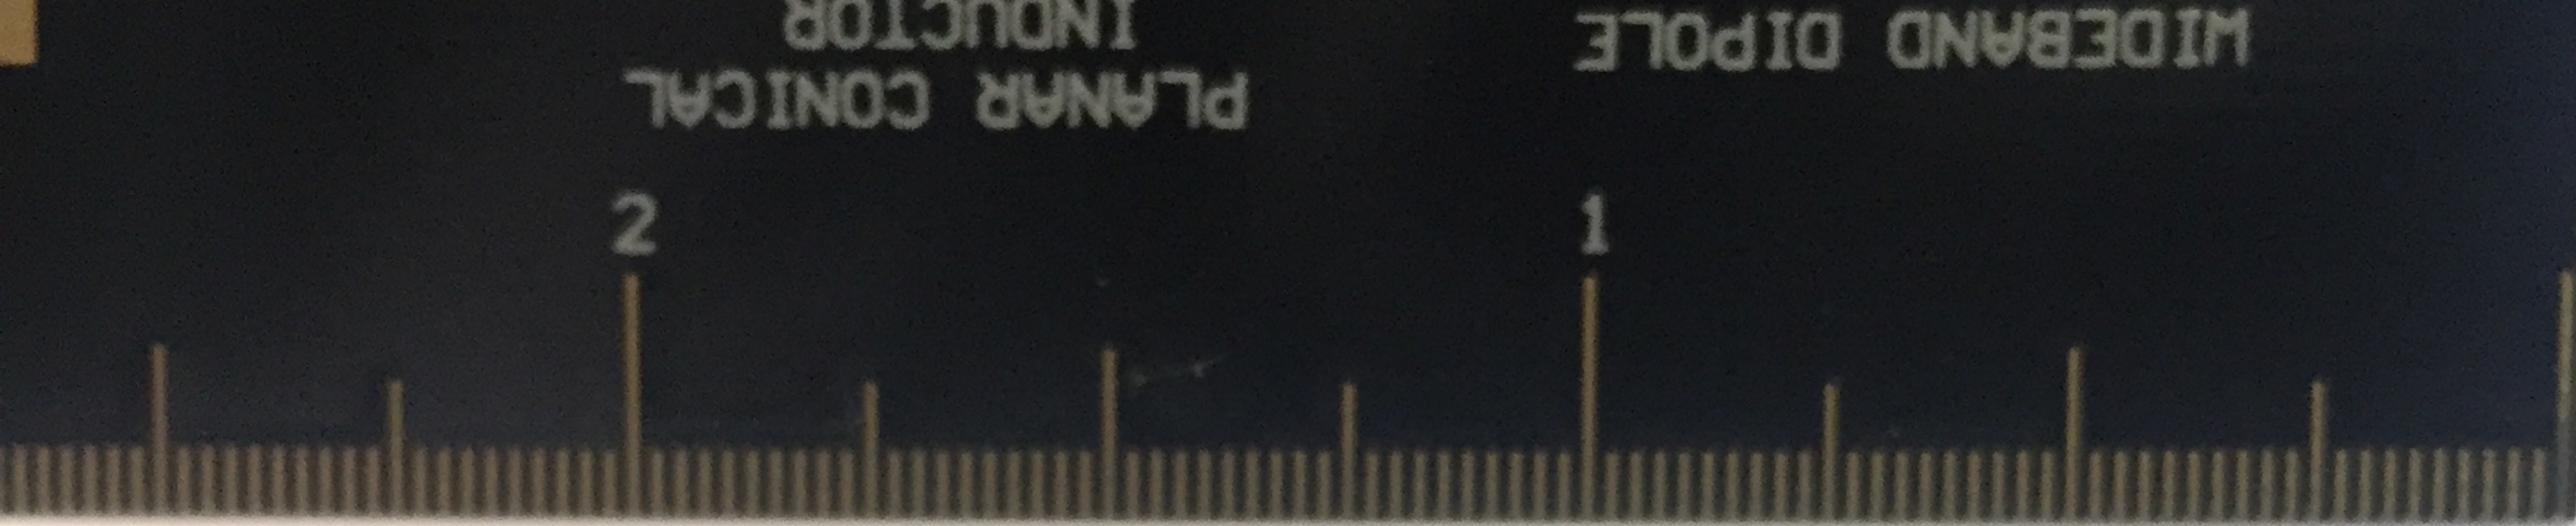

PI ANAB CONINCA

1

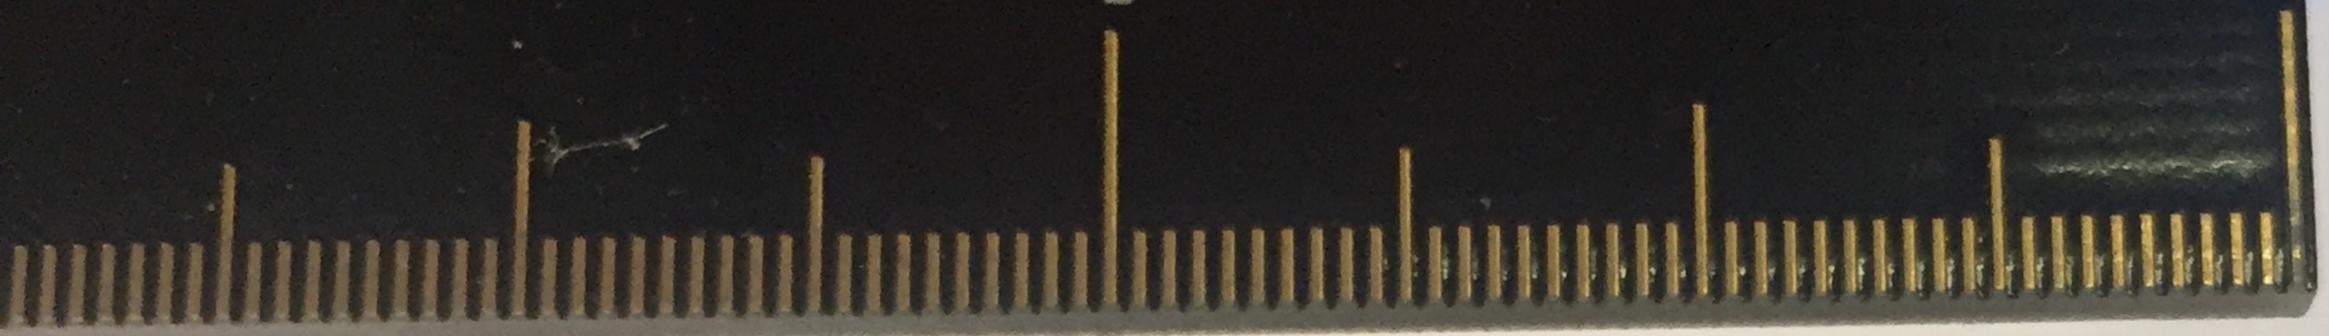

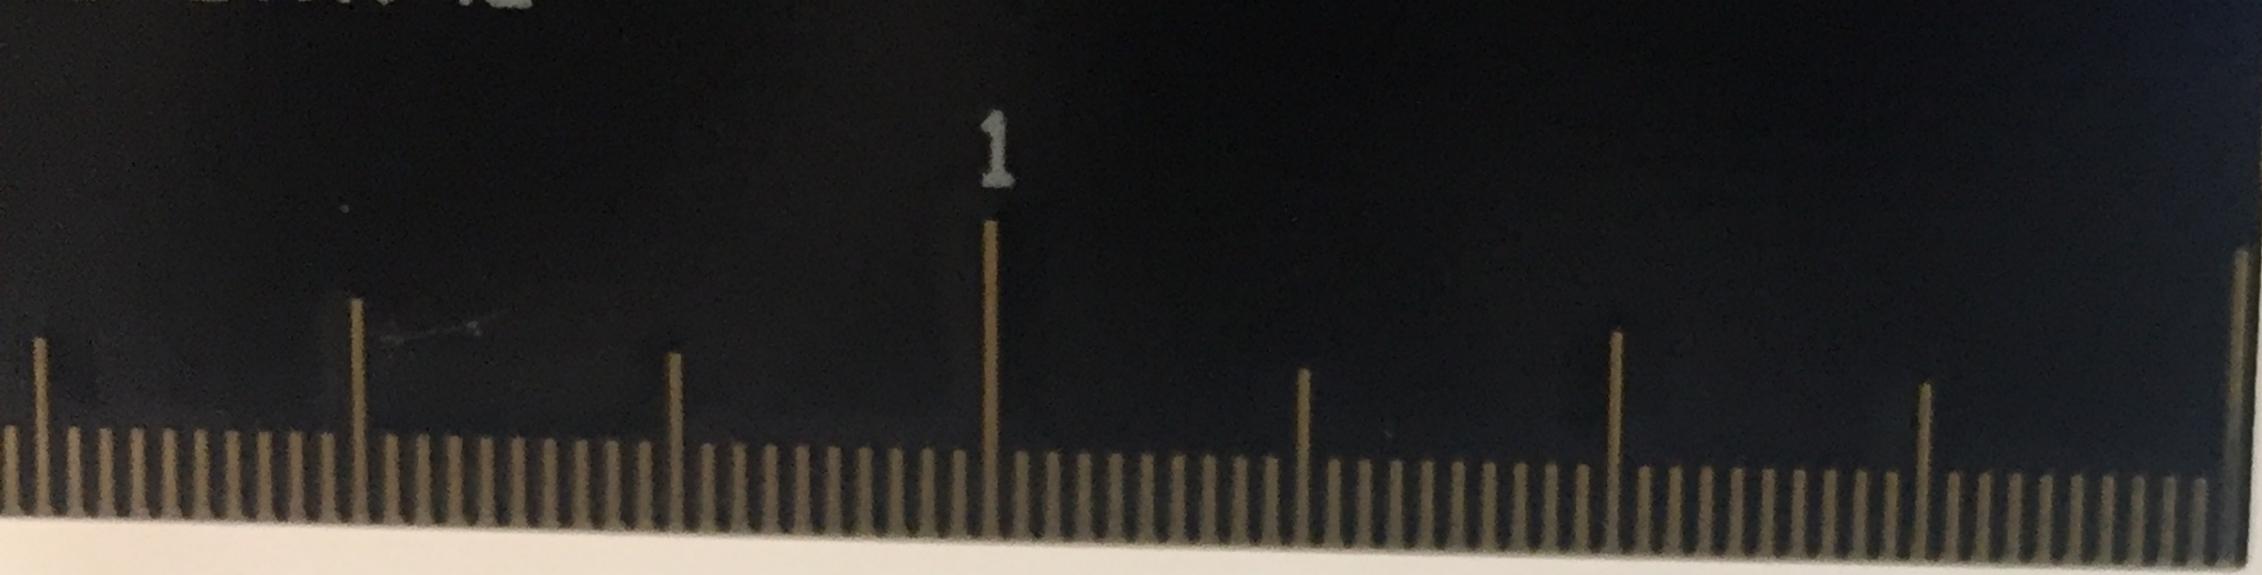



spire
health
1741F