

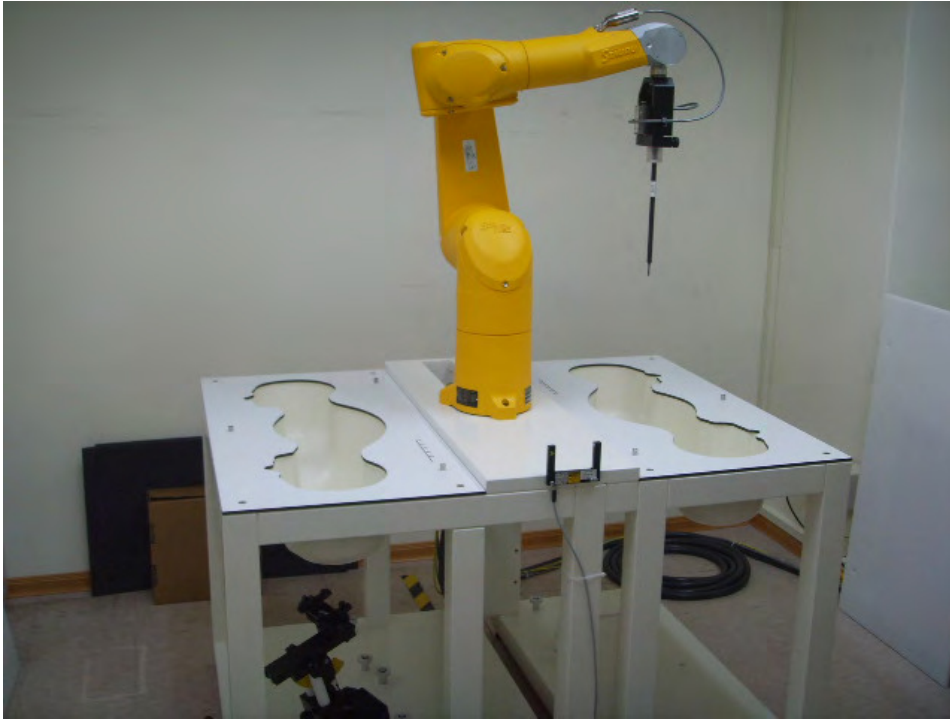
APPENDIX**10. Photographs of Test Setup**

Fig.1 Photograph of the SAR measurement system

Photograph of the tissue simulant fluid liquid depth (Body)

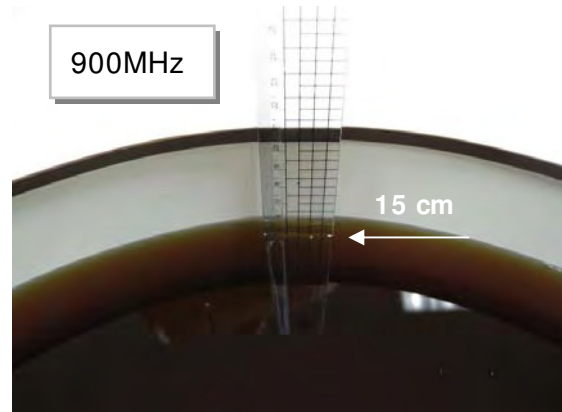


Fig.2

Cover Closed - distance between flat phantom and EUT is 5 mm

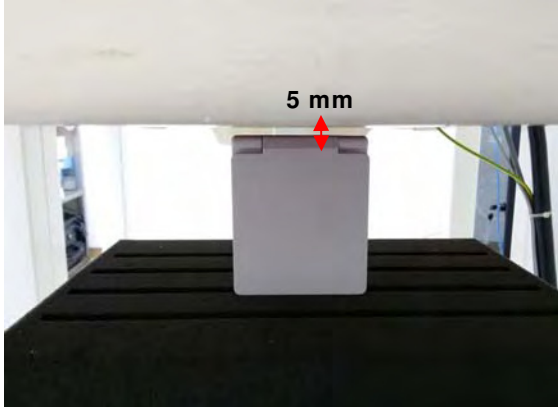


Fig.3 EUT Top side mode to flat phantom

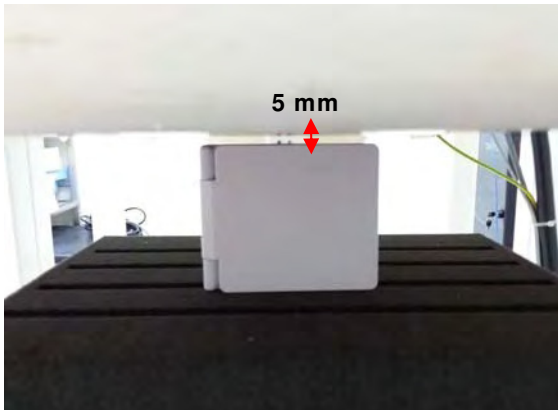


Fig.4 EUT Right side to flat phantom

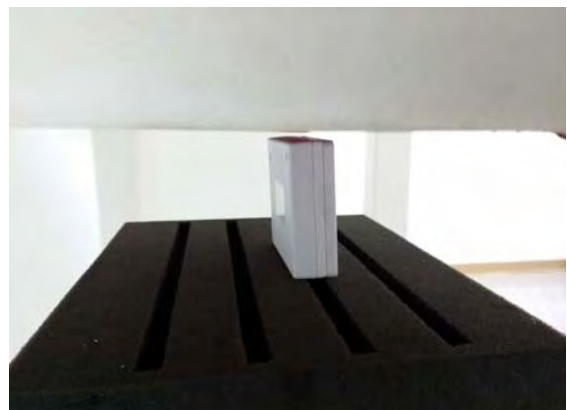
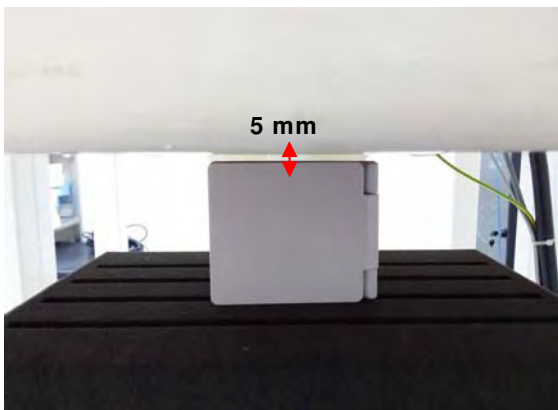


Fig.5 EUT Left side to flat phantom

Cover Closed - distance between flat phantom and EUT is 5 mm

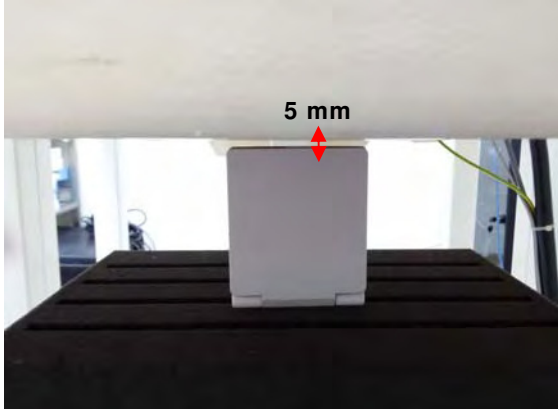


Fig.6 EUT Bottom side to flat phantom


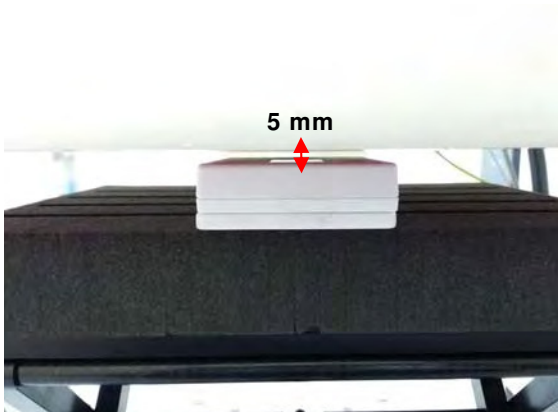


Fig.7 EUT Back side to flat phantom



Fig.8 EUT Front side to flat phantom

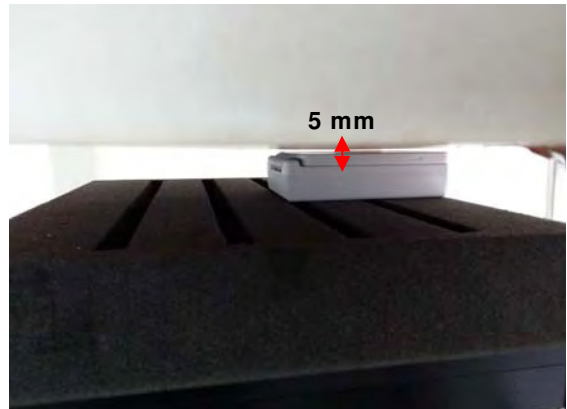

Cover Open - distance between flat phantom and EUT is 10 mm

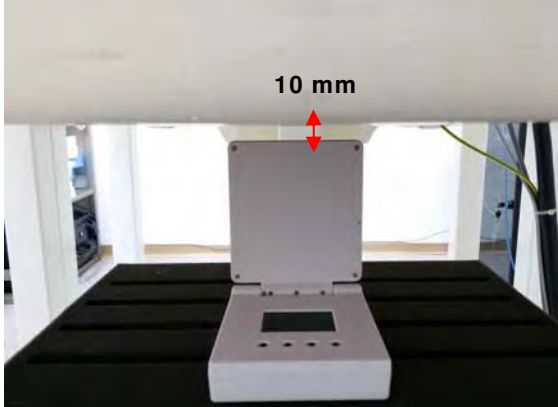


Fig.9 EUT Top side mode to flat phantom


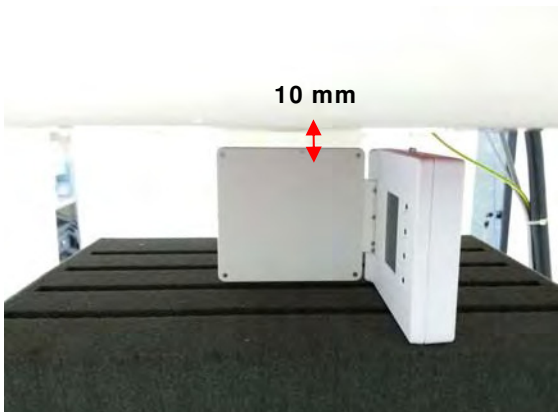


Fig.10 EUT Right side to flat phantom



Fig.11 EUT Left side to flat phantom

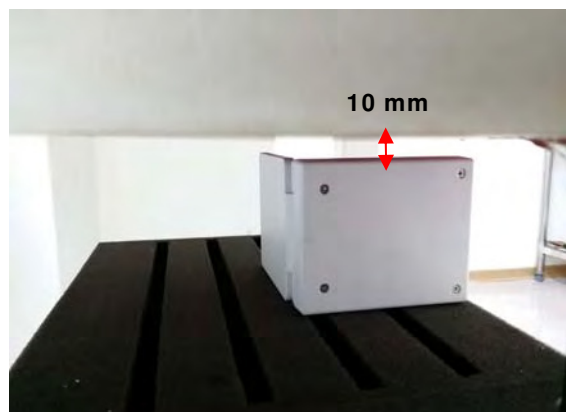

Cover Open - distance between flat phantom and EUT is 10 mm

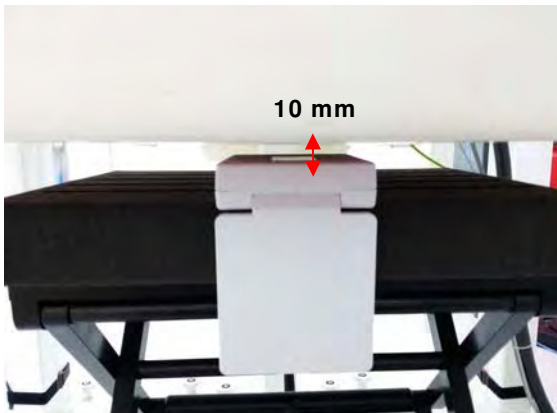


Fig.12 EUT Bottom side to flat phantom



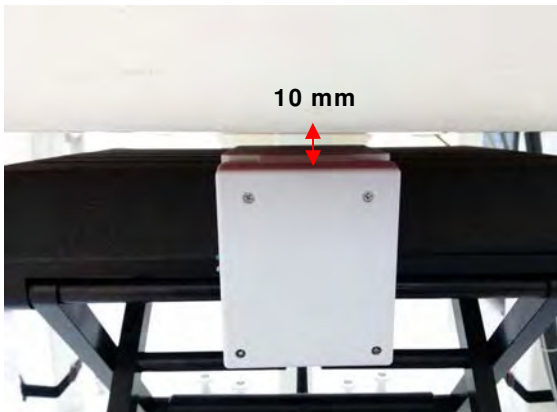


Fig.13 EUT Back side to flat phantom



Fig.14 EUT Front side to flat phantom

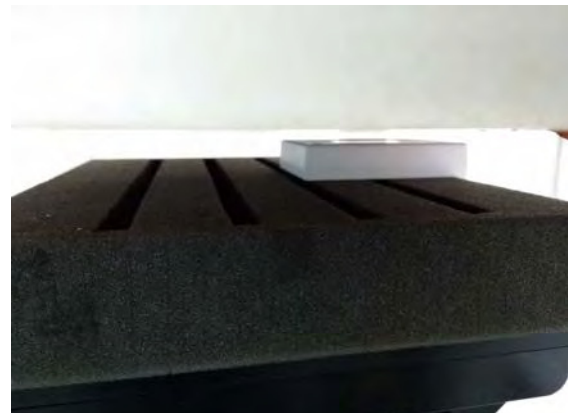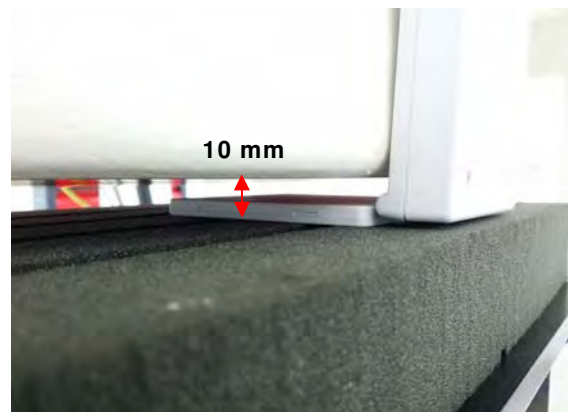

12. Photographs of the EUT



Fig.15 Front view of EUT

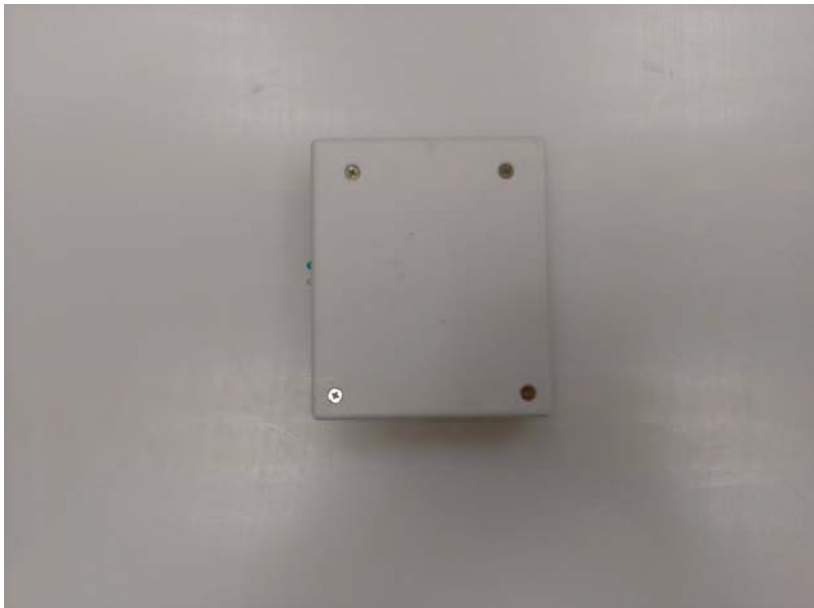


Fig.16 Back view of EUT

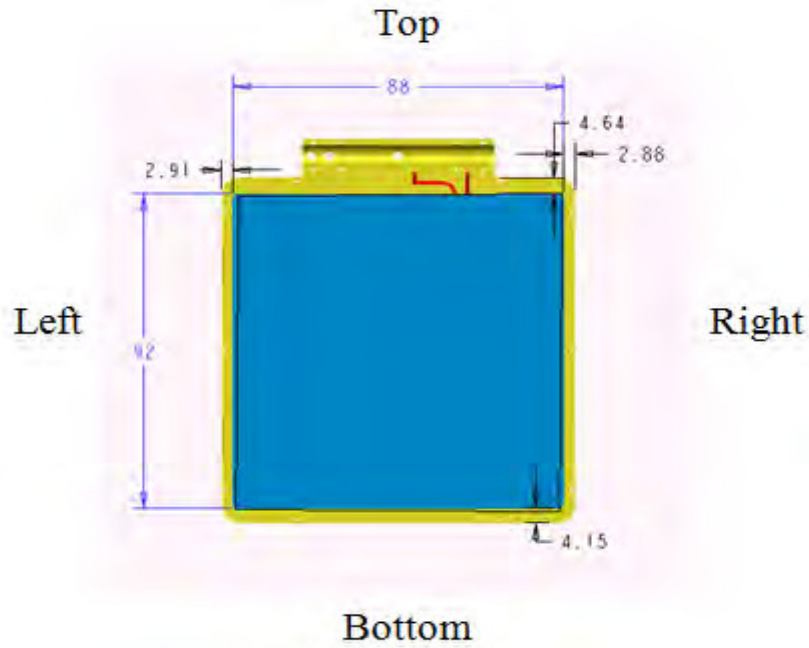


Fig.17 Antenna position of EUT (Front view / Cover closed)

- End of Report -