


## **Appendix 4. Photographs**


This appendix contains the following photographs:

<b>Photo Reference Number</b>	<b>Title</b>
001	Test configuration for the measurement of Specific Absorption Rate (SAR)
002	Front of EUT Facing Phantom at 10mm
003	Back of EUT Facing Phantom at 10mm
004	Left Hand Side of EUT Facing Phantom at 10mm
005	Right Hand Side of EUT Facing Phantom at 10mm
006	Top of EUT Facing Phantom at 10mm
007	Bottom of EUT Facing Phantom at 10mm
008	Front View of EUT
009	Back View of EUT
010	Left Hand Side View of EUT
011	Right Hand Side View of EUT
012	Top View of EUT
013	Bottom View of EUT
014	Internal View of Conducted Sample
015	Internal View of Radiated EUT
016	EUT Dimensions
017	900 Body Fluid Level
018	1900 Body Fluid Level
019	2450 Body Fluid Level


**001: Test configuration for the measurement of Specific Absorption Rate (SAR)**

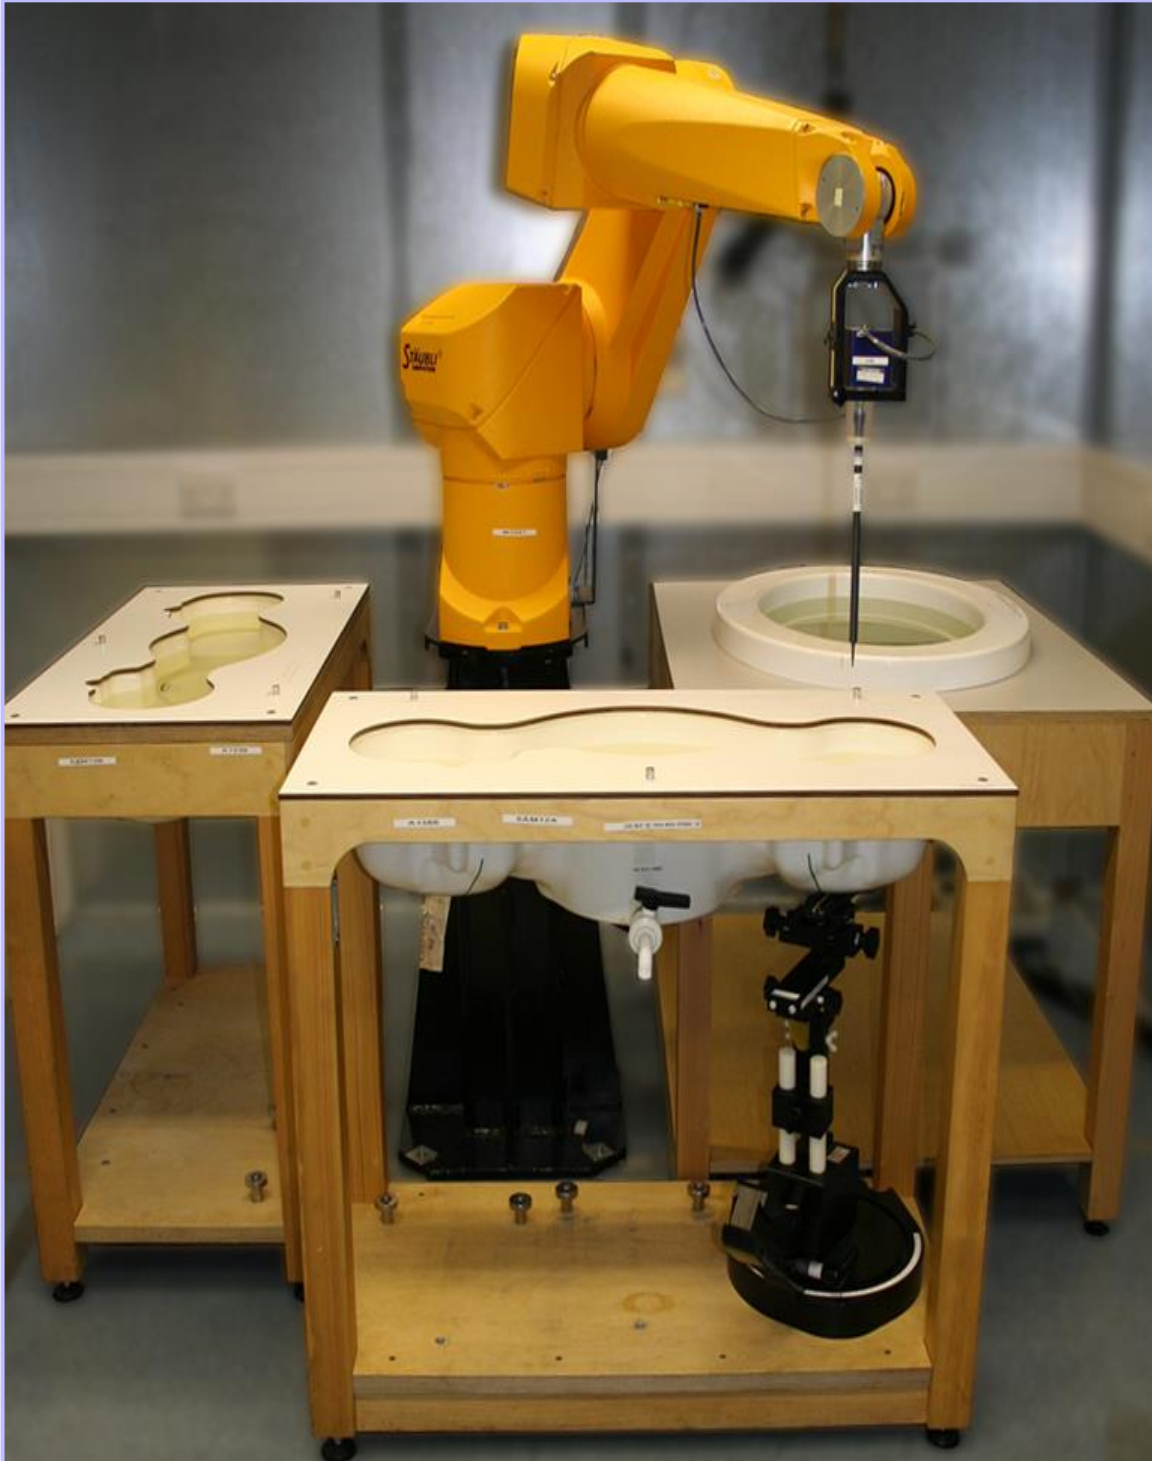

**002: Front of EUT Facing Phantom at 10mm**

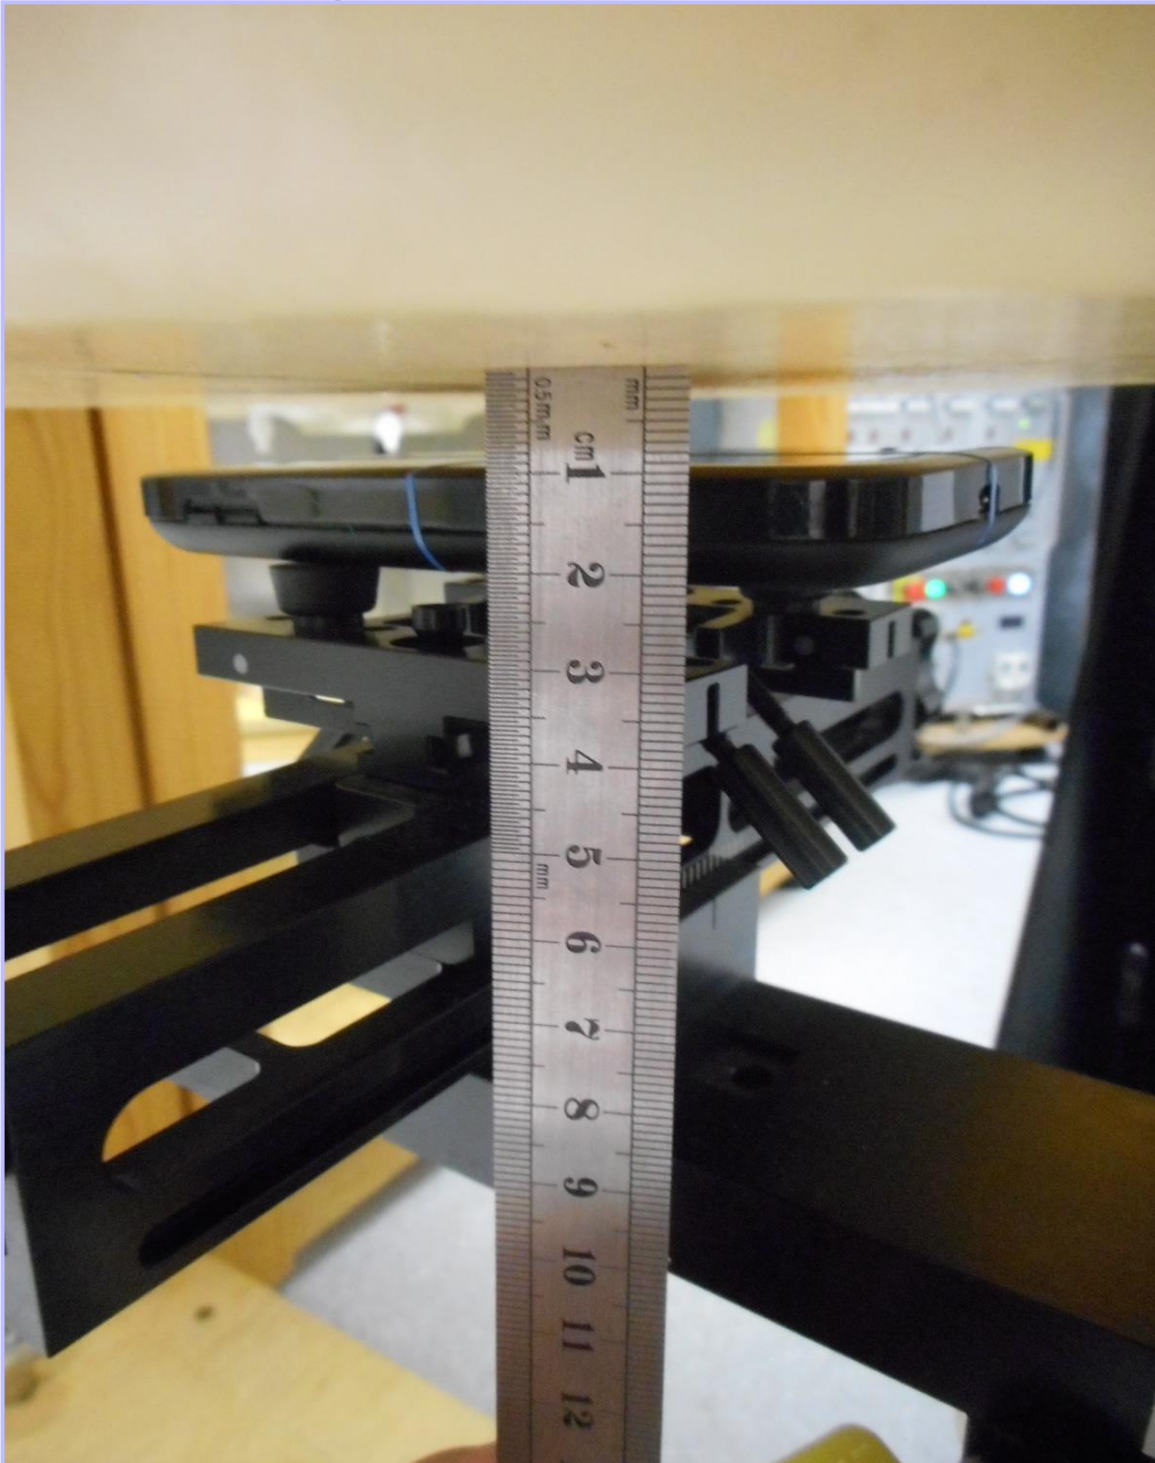

**003: Back of EUT Facing Phantom at 10mm**

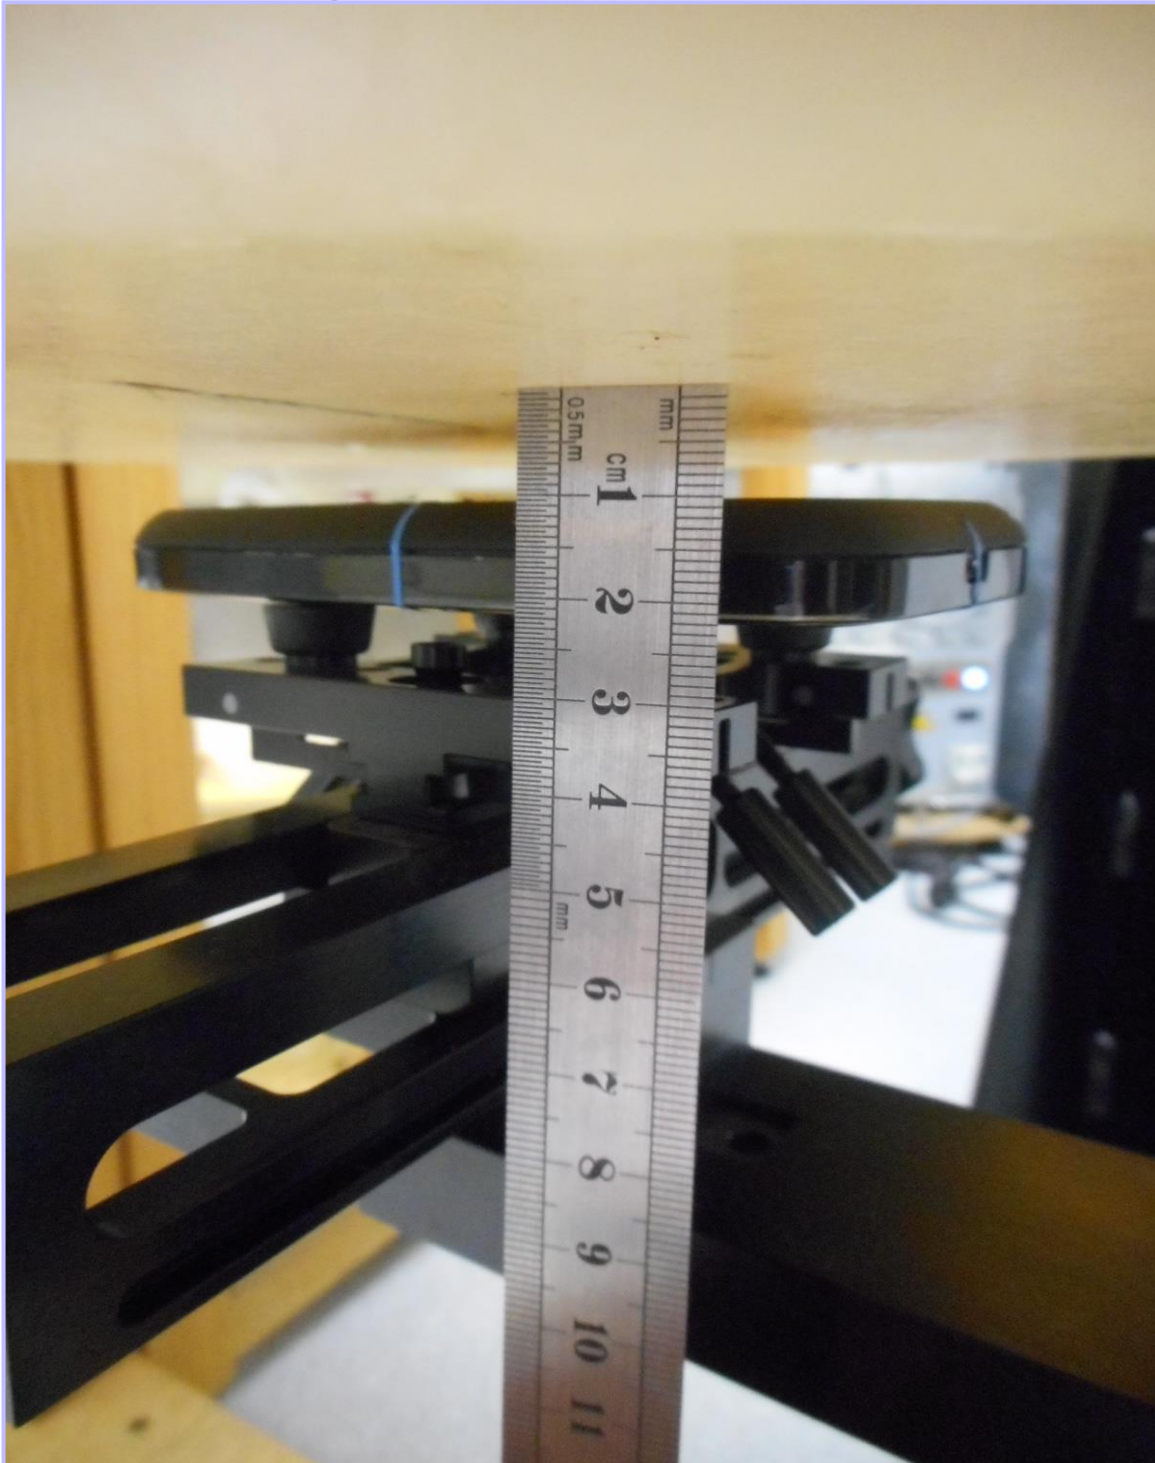




**004: Left Hand Side of EUT Facing Phantom at 10mm**



**005: Right Hand Side of EUT Facing Phantom at 10mm**




**006: Top of EUT Facing Phantom at 10mm**

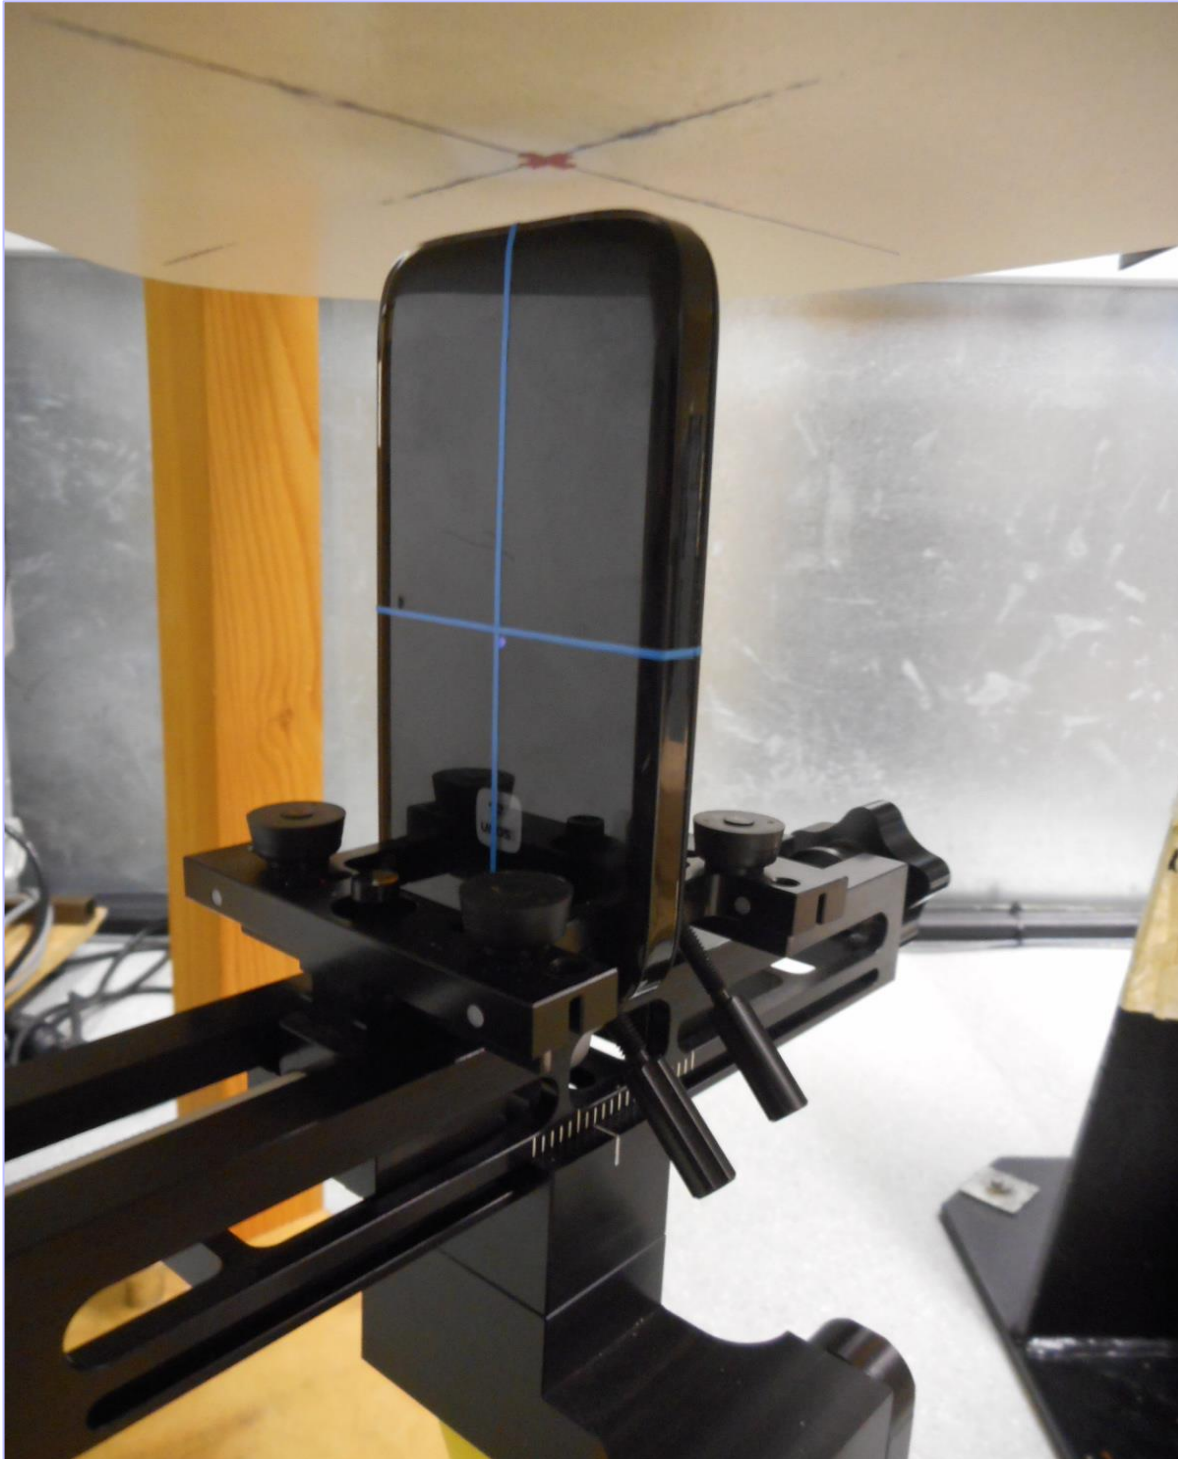



**007: Bottom of EUT Facing Phantom at 10mm**

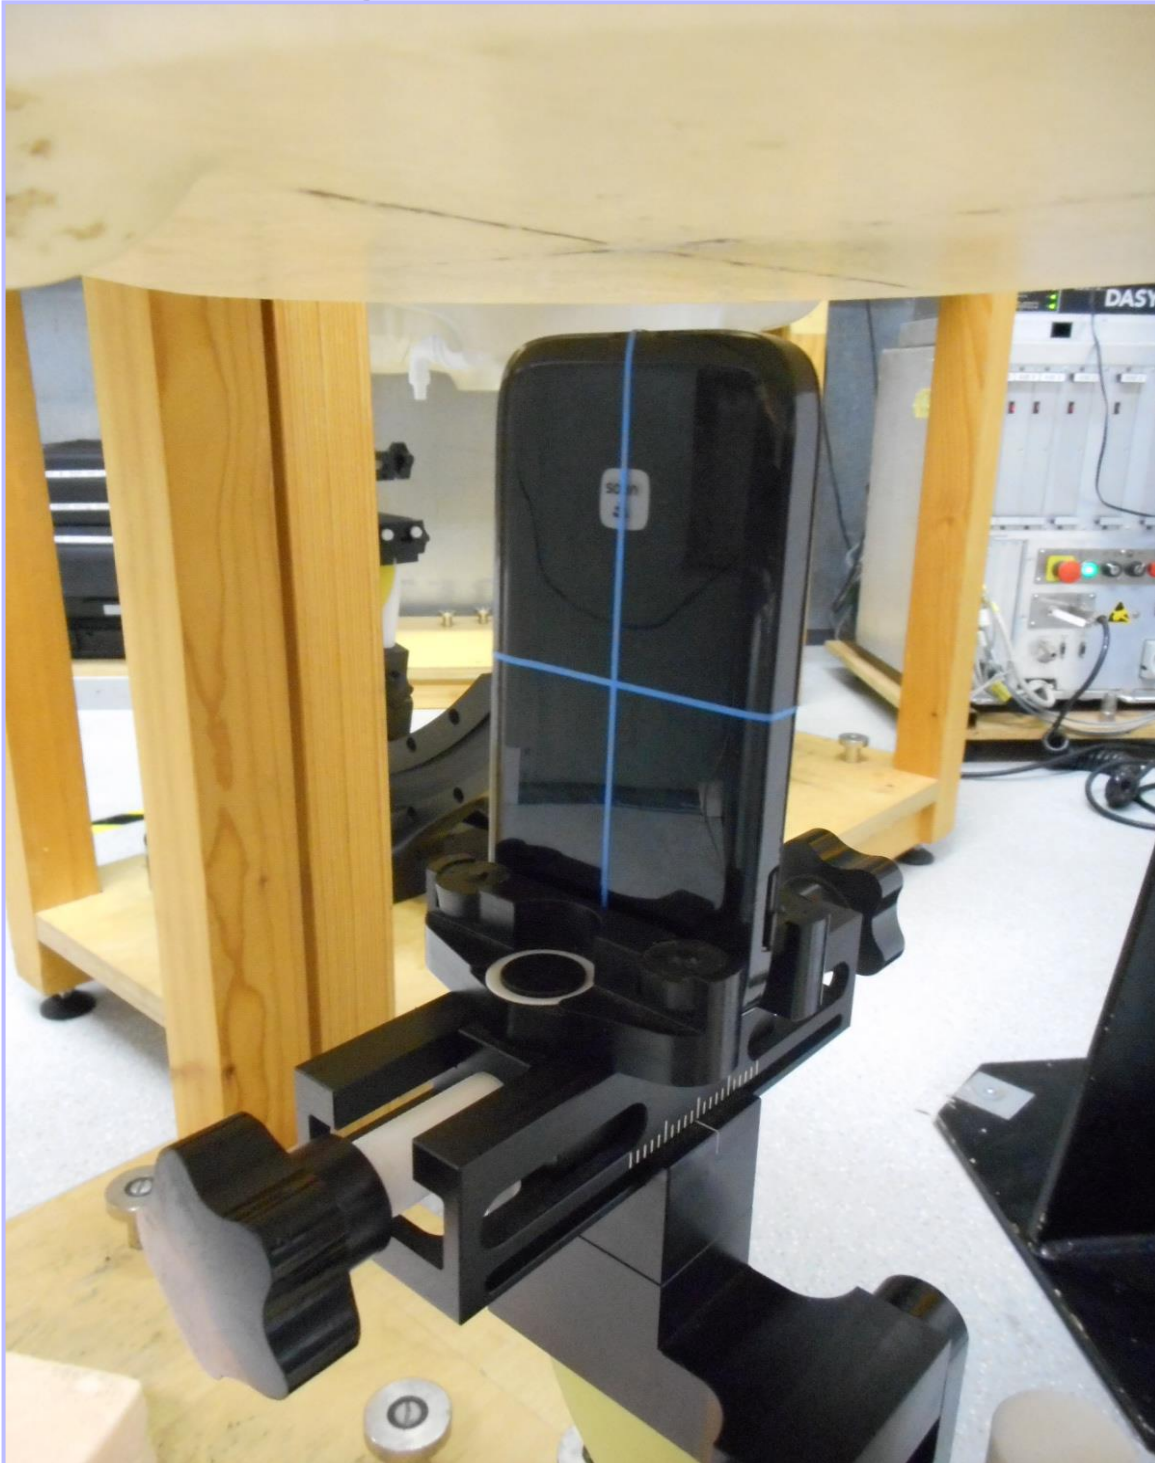




**008: Front View of EUT**



**009: Back View of EUT**




**010: Left Hand Side View of EUT**

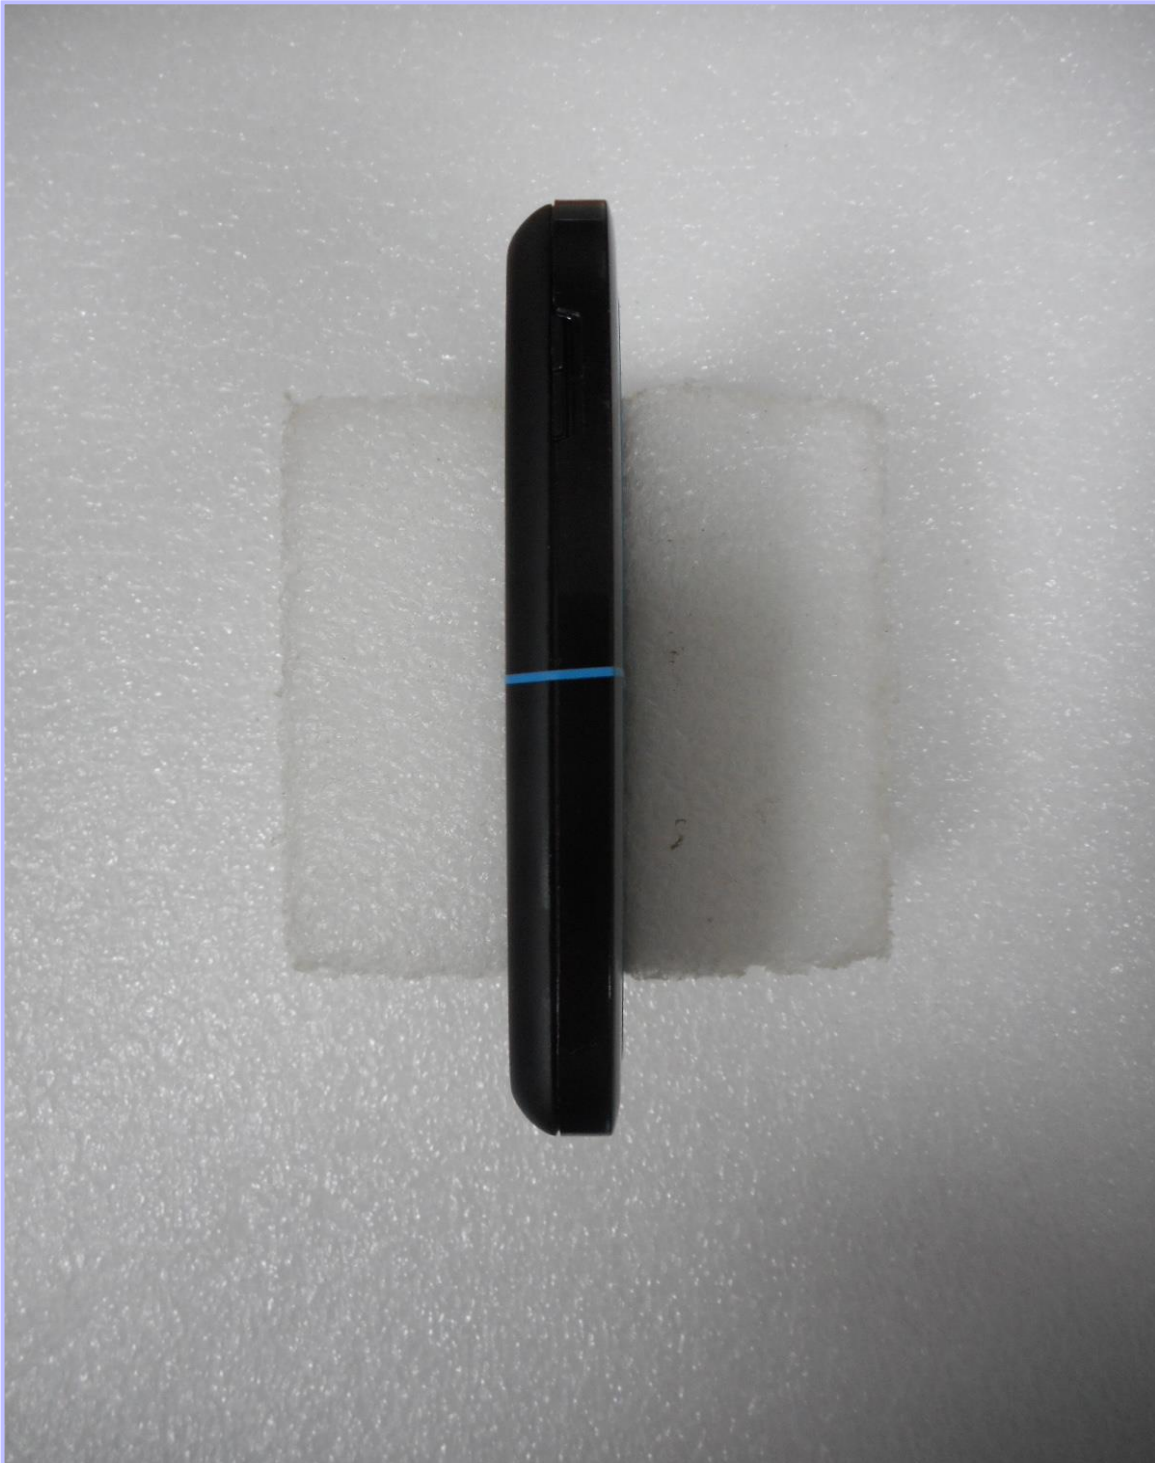





**011: Right Hand Side View of EUT**

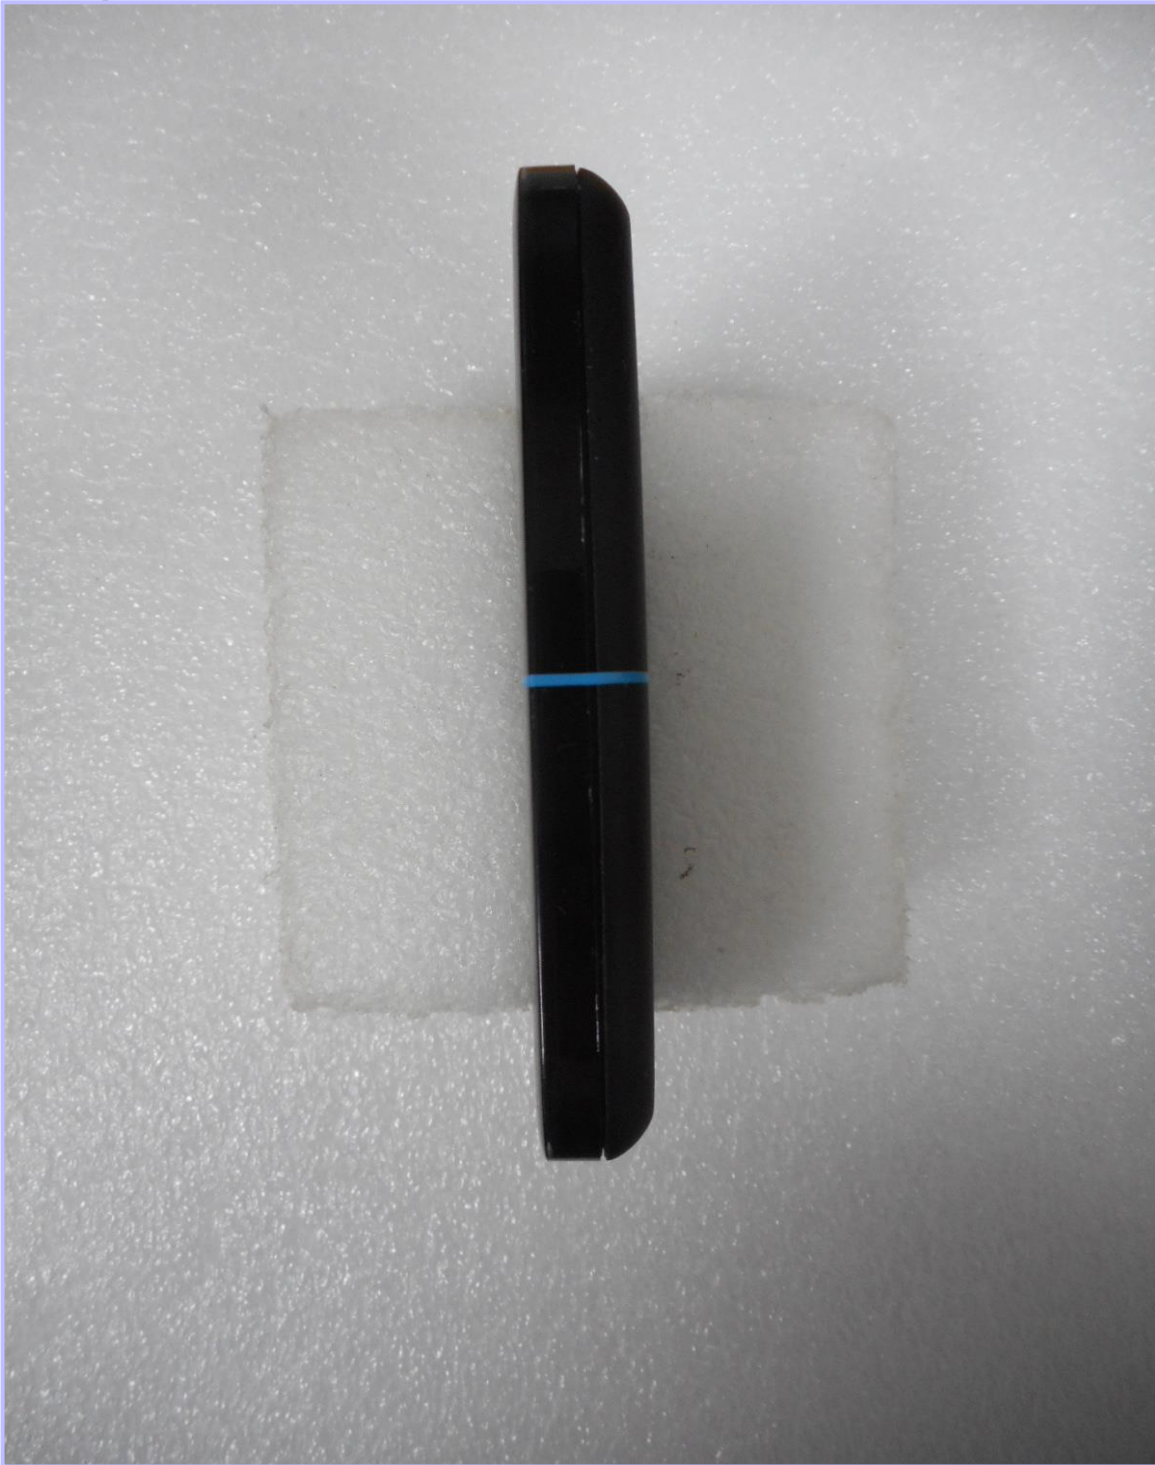

**012: Top View of EUT**

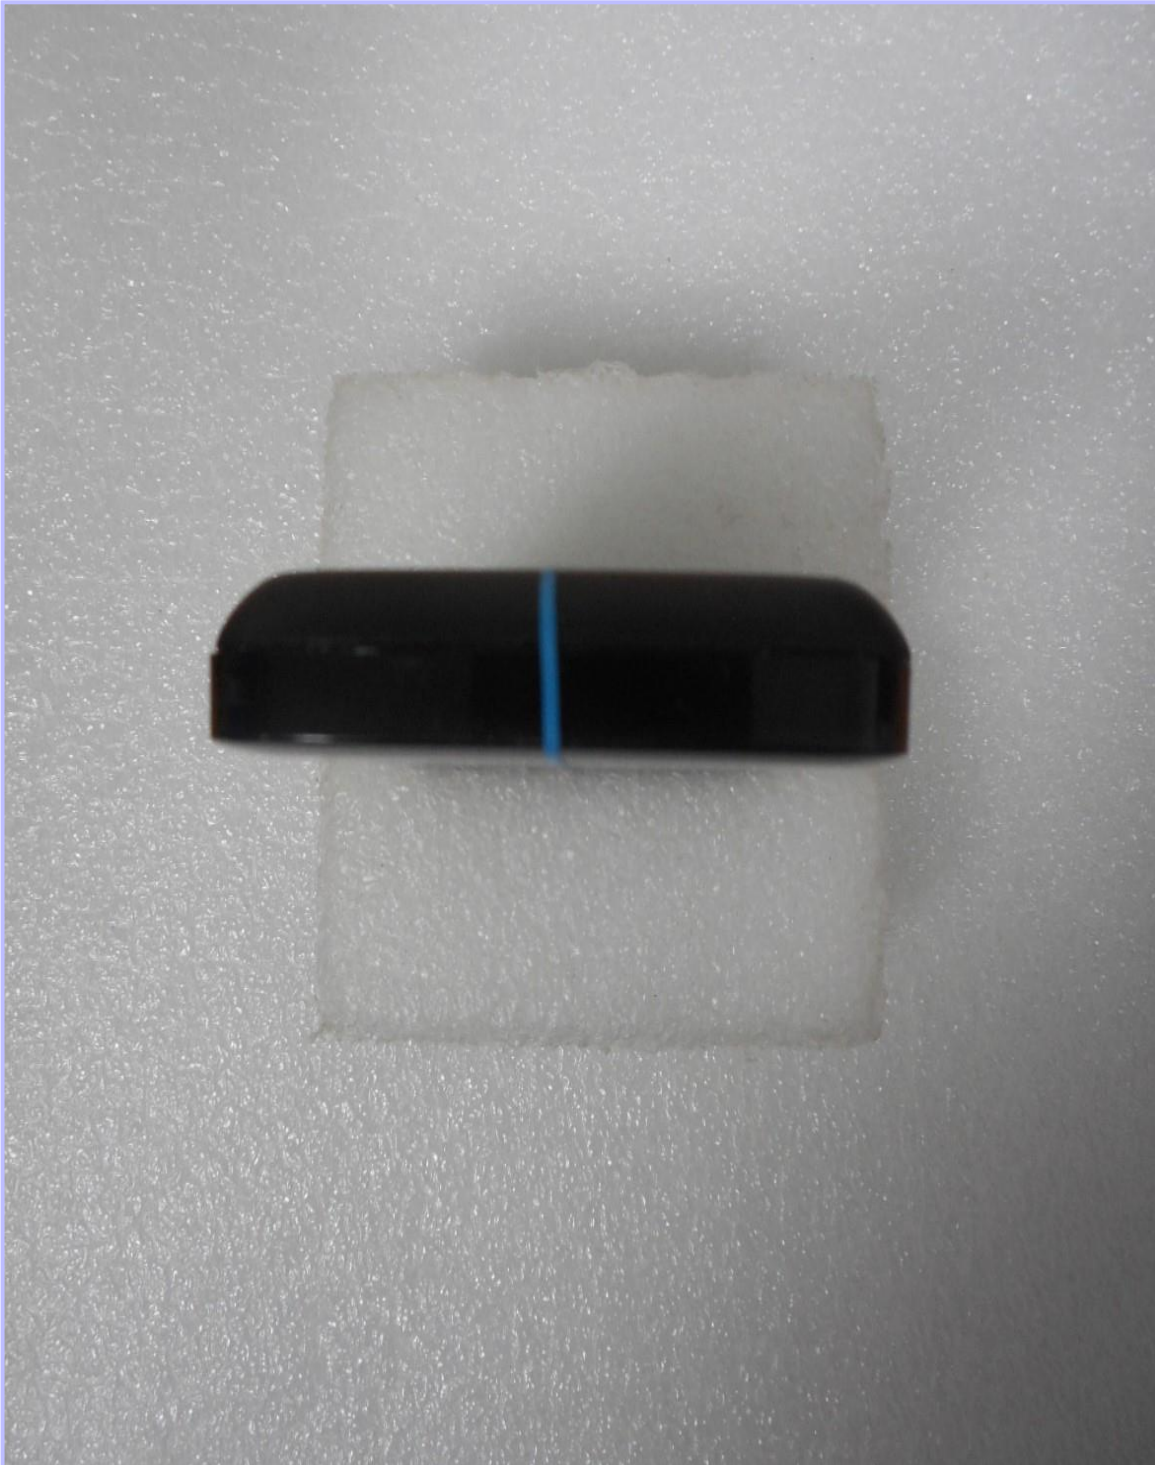

**013: Bottom View of EUT**

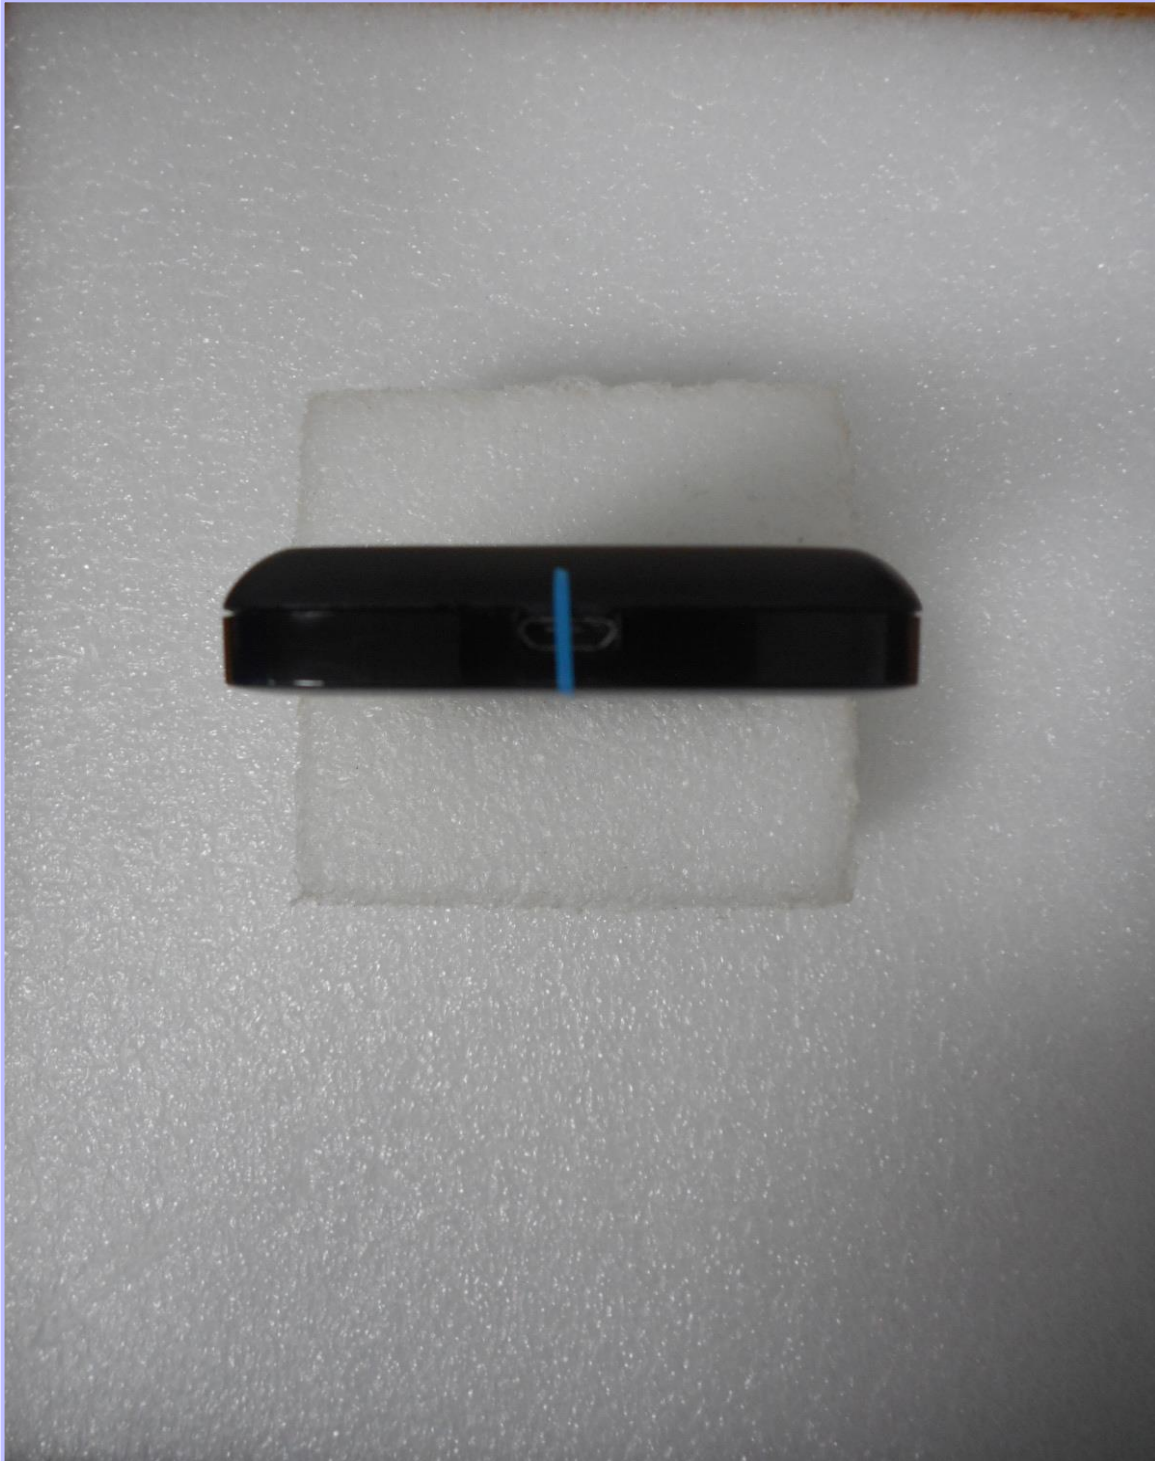



**014: Internal View of Conducted Sample**



**015: Internal View of Radiated EUT**




**016: EUT Dimensions**






**017: 900 Body Fluid Level**

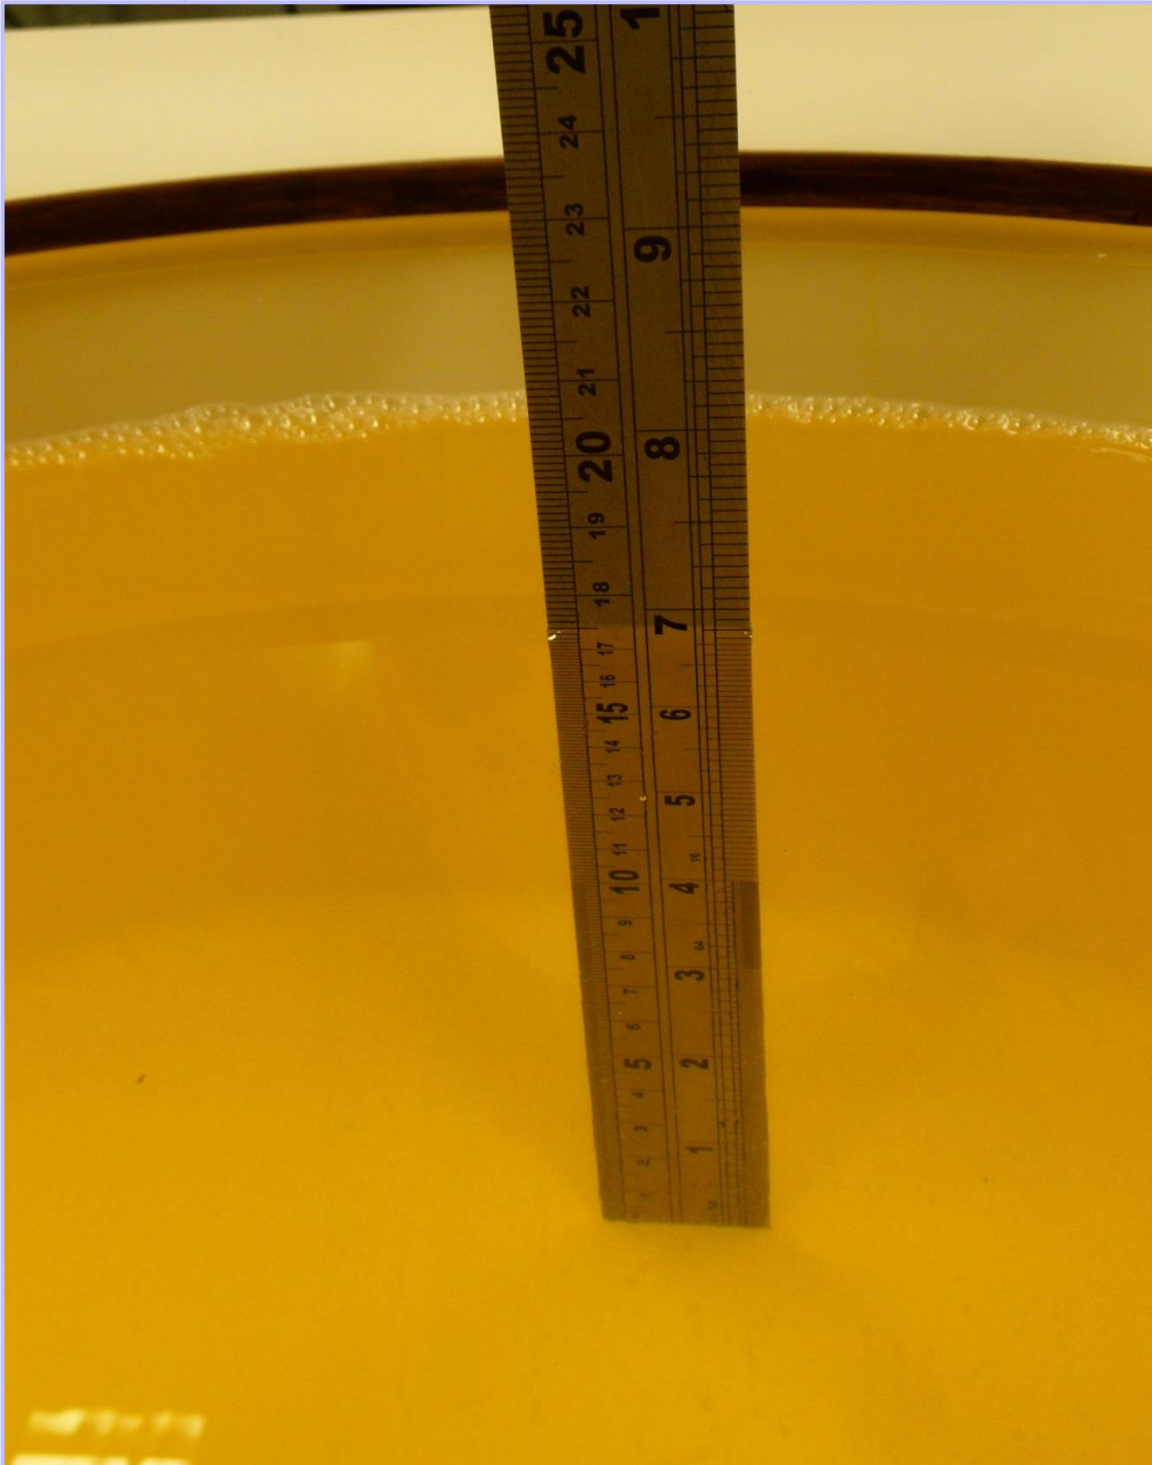

**018: 1900 Body Fluid Level**

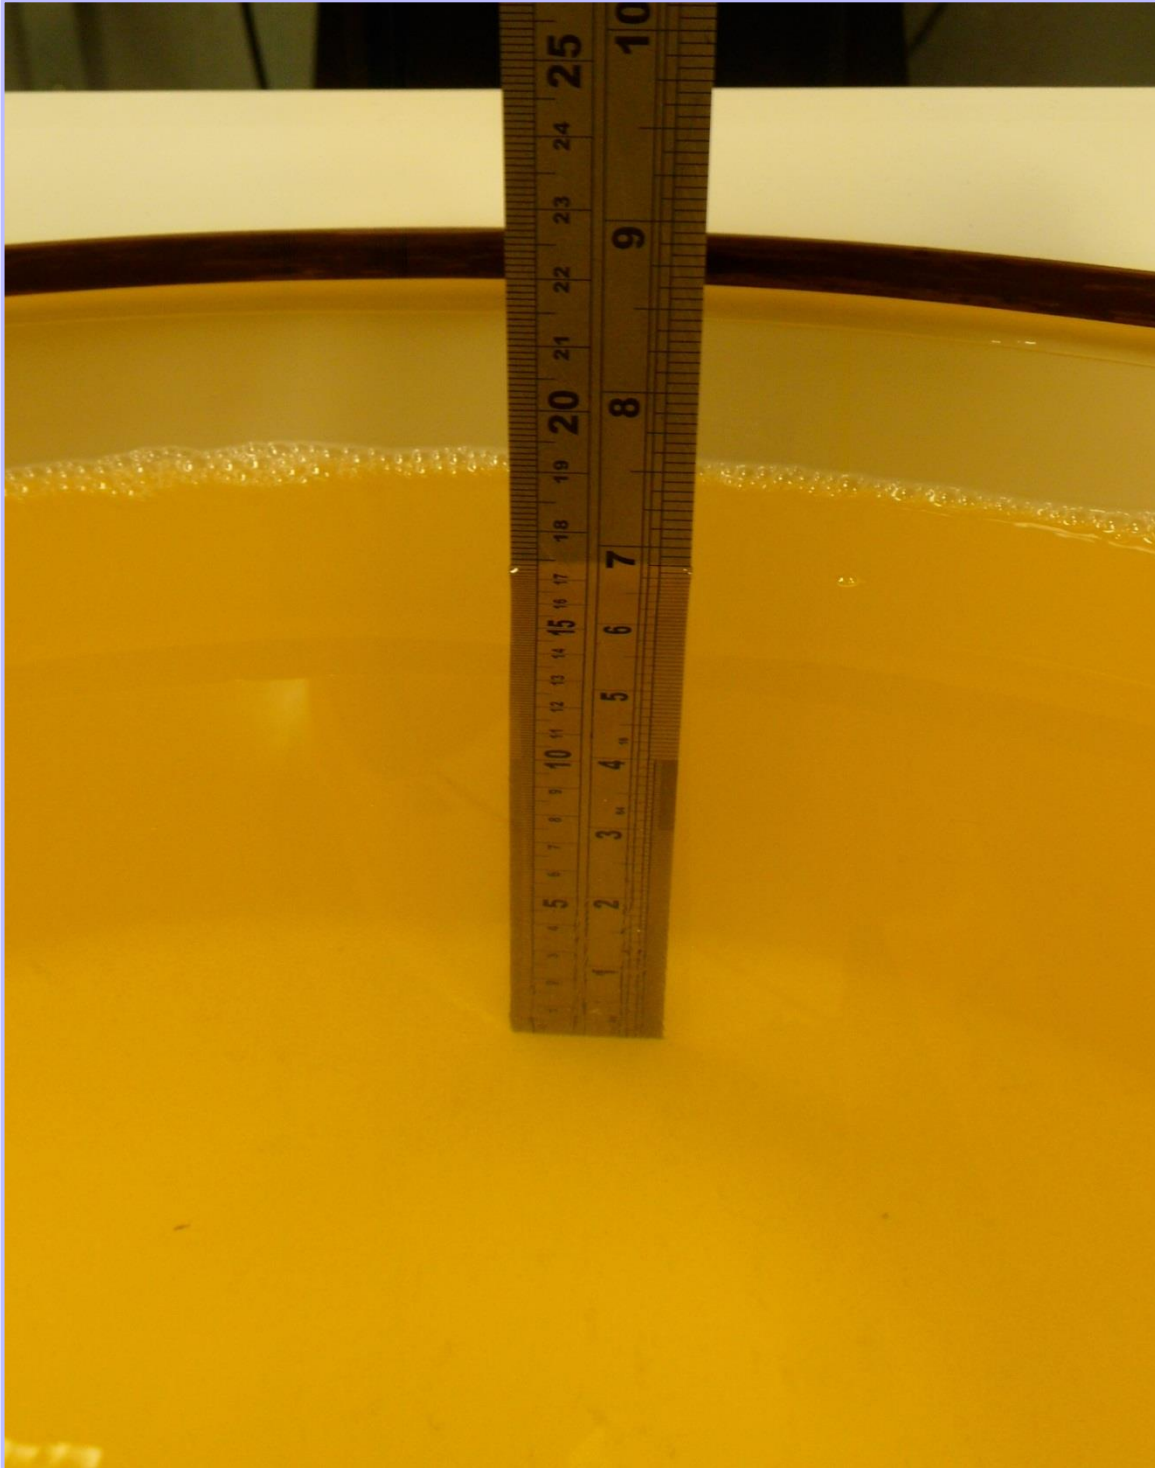

**019: 2450 Body Fluid Level**

