Report NO: TS201510006 Page 1 / 96

# FCC SAR TEST REPORT

For

## **MOVILTELCO TRADE, S.L**

Street: ABTAO, 25-1 Floor A-office MADRID-SPAIN, MADRID, Spain

**Product Name**: Smartphone

**Model No.** : A53

FCC ID : 2ACQKTELCO008

Date of Receipt: 17th Oct. 2015

**Date of Test** : 18th ~20th Oct. 2015

**Issued Date**: 27th Oct. 2015

**Report No.** : TS201510006

**Report Version**: V1.0

## Issue By

Shenzhen Sunway Communication CO.,LTD Testing Center

1/F,BuildingA, SDG Info Port, KefengRoad, Hi-Tech Park, Nanshan District,
Shenzhen, Guangdong, China 518104,

**Note:** The test results relate only to the samples tested. This report shall not be reproduced in full, without the written approval of SUNWAY Testing Center.



# SHENZHEN SUNWAY COMMUNICATION CO.,LTD Report NO: TS201510006 Page 2 / 96

## **TABLE OF CONTENS**

1. Statement of Compliance	4
2. SAR Evaluation compliance	5
3. General Information:	6
3.1 EUT Description:	6
3.2 Test Environment:	7
4. SAR Measurement System:	8
4.1 Dasy4 System Description:	8
5. System Components:	9
6. Tissue Simulating Liquid	11
6.1 The composition of the tissue simulating liquid:	11
6.2 Tissue Calibration Result:	11
7. SAR System Validation	16
7.1 Validation System:	16
7.2 Validation Dipoles:	16
7.3 Validation Result:	17
8. SAR Evaluation Procedures:	18
9. SAR Exposure Limits	20
9.1 Uncontrolled Environment	20
9.2 Controlled Environment	20
10. Measurement Uncertainty:	21
11. Conducted Power Measurement:	23
12. Antenna Location	29
13. Results and Test photos :	30
13.1 SAR result summary:	30
13.2 Evaluation of Simultaneous :	33
13.3 DUT and setup photos photos	34
14. Equipment List:	37
Appendix A. System validation plots:	38
Appendix B. SAR Test plots:	44



Report NO: TS201510006	Page 3 / 96
Appendix C. Probe Calibration Data:	54
Appendix D. DAE Calibration Data:	66
Appendix E. Dipole Calibration Data:	69



Report NO: TS201510006 Page 4 / 96

# 1. Statement of Compliance

The maximum results of Specific Absorption Rate (SAR) found during testing are as follows.

#### <Highest SAR Summary>

Exposure Position	Frequency Band	1g-SAR (W/kg)	Highest 1g-SAR (W/kg)
	GSM850	0.340	
	GSM1900	0.231	
Head	WCDMA V	0.375	0.382
	WCDMA II	0.382	]
	WLAN 2.4GHz Band	0.0931	]
	GSM850	0.746	
Hatamat	GSM1900	0.589	
Hotspot	WCDMA V	0.581	0.746
(1cm Gap)	WCDMA II	0.643	
	WLAN 2.4GHz Band	0.0802	
	GSM850	0.746	
Body Worn (1cm Gap)	GSM1900	0.589	
	WCDMA V	0.581	0.746
(Tolli Gap)	WCDMA II	0.643	
	WLAN 2.4GHz Band	0.0802	

This device is in compliance with Specific Absorption Rate (SAR) for general population/uncontrolled exposure limits (1.6 W/kg) specified in FCC 47 CFR part 2 (2.1093) and ANSI/IEEE C95.1-1992, and had been tested in accordance with the measurement methods and procedures specified in IEEE 1528-2013.

#### <Highest simultaneous transmission SAR>

	Position	Main antenna (W/kg)	WLAN 2.4G (W/kg)	Bluetooth (W/kg)	Max Sum (W/kg)
Highest SAR value for Head	Right Cheek	0.375	0.0931	0.053	0.468
Highest SAR value for Body	Back	0.746	0.0802	0.026	0.826

According to the above table, the maximum sum of reported SAR values for GSM/WCDMA and BT/WIFI is **0.826**W/kg (1g).



Report NO: TS201510006 Page 5 / 96

# 2. SAR Evaluation compliance

Product Name:	Smartphone		
Brand Name:	mtt		
Model Name:	A53		
Applicant:	MOVILTELCO TRADE, S.L		
Address:	Street:ABTAO,25-1Floor A-office MADRID-SPAIN, MADRID, Spain		
Manufacturer:	Shenzhen Gotron Electronic Co., LTD		
Address:	518, 5F, R&D building,Tsinghua Hi-Tech Park, Hi-Tech park(North) Nanshan district, Shenzhen		
Applicable Standard:	FCC 47 CFR Part 2 (2.1093) ANSI/IEEE C95.1-1992 IEEE 1528-2013 FCC KDB 865664 D01 SAR Measurement 100 MHz to 6 GHz v01r04 FCC KDB 865664 D02 SAR Reporting v01r01 FCC KDB 447498 D01 General RF Exposure Guidance v05r02 FCC KDB 941225 D06 Hotspot Mode v02 FCC KDB 648474 D04 Handset SAR v01r02 FCC KDB 248227 D01 SAR meas for 802 11abg v02r01 FCC KDB 941225 D01 3G SAR Procedures v03		
Test Engineer:	Li.zhao		
Reviewed By	Li.Zhao Tomy. Lirl		
Performed Location:	Shenzhen Sunway Communication CO.,LTD Testing Center 1/F,BuildingA, SDG Info Port, KefengRoad, Hi-Tech Park, Nanshan District,Shenzhen, Guangdong, China 518104 Tel: +86-755- 36615880 Fax: +86-755- 86525532		



Report NO: TS201510006 Page 6 / 96

# 3. General Information:

# 3.1 EUT Description:

	EUT Information				
Product Name	Smartphone				
Brand Name	mtt				
Model Name	A53				
Hardware Version	S509 V1.1				
Software Version	S509_GQ3021_K1_MTT_A53_20150730				
	GSM 850: 2 dBi				
	PCS 1900: 2dBi				
Antenna gain:	WCDMA 850:2 dBi				
Antenna gam.	WCDMA 1900:2 dBi				
	WIFI: 1 dBi				
	BT:1 dBi				
	GSM850: 824.2 MHz ~ 848.8 MHz				
	GSM1900: 1850.2 MHz ~ 1909.8 MHz				
Tx Frequency	WCDMA Band V: 826.4 MHz ~ 846.6 MHz				
1 x 1 requericy	WCDMA Band II: 1852.4 MHz ~ 1907.6 MHz				
	WLAN 2.4GHz Band: 2412 MHz ~ 2462 MHz				
	Bluetooth: 2402 MHz ~ 2480 MHz				
	GSM/GPRS				
	RMC/AMR 12.2Kbps				
Mode	HSDPA				
Wiode	HSUPA				
	802.11b/g/n HT20/HT40				
	Bluetooth v3.0+EDR				
GSM//E\GDDS Transfer	Class B - EUT cannot support Packet Switched and Circuit Switched				
GSM/(E)GPRS Transfer mode	Network simultaneously but can automatically switch between Packet and				
mode	Circuit Switched Network.				



Report NO: TS201510006 Page 7 / 96

## 3.2 Test Environment:

Ambient conditions in the SAR laboratory:


Items	Required	Actual
Temperature (°C)	18-25	22~23
Humidity (%RH)	30-70	55~65



Report NO: TS201510006 Page 8 / 96

## 4. SAR Measurement System:

### 4.1 Dasy4 System Description:

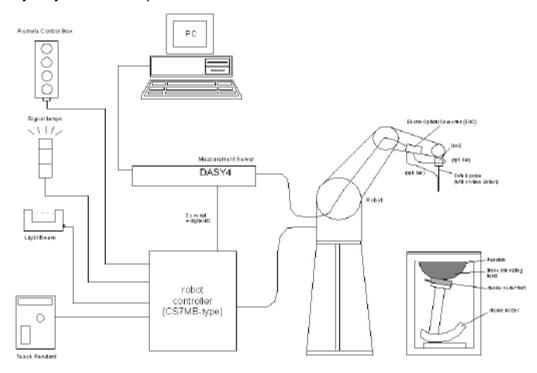

The DASY4 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc.
- ➤ The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- ➤ A computer operating Windows 2000 or Windows XP.
- DASY4 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM twin phantom enabling testing left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- > Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing to validate the proper functioning of the system.



Report NO: TS201510006 Page 9 / 96

## 5. System Components:

#### DASY4 Measurement Server:



Calibration: No calibration required.

The DASY4 measurement server is based on a PC/104 CPU board with a 166MHz low-power pentium, 32MB chipdisk and 64MB RAM. The necessary circuits for communication with either the DAE4 (or DAE3) electronic box as well as the 16-bit AD-converter system for optical detection and digital I/O interface are contained on the DASY4 I/O-board, which is directly connected to the PC/104 bus of the CPU board.

### DATA Acquisition Electronics (DAE):



Calibration: Recommended once a year

The data acquisition electronics consists of a highly sensitive electrometer grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD converter and a command decoder and control logic unit.

Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

#### Dosimetric Probes:



Calibration: Recommended once a year

Model: ES3DV3,

Frequency: 10MHz to 3G, Linearity:±0.2dB, Dynamic Range: 10 µW/g to100 mW/g

Directivity:

± 0.3 dB in HSL (rotation around probe axis) ± 0.5 dB in tissue material (rotation normal to

probe axis)

These probes are specially designed and calibrated for use in liquids with high permittivities. They should not be used in air, since the spherical isotropy in air is poor (±2 dB). The dosimetric probes have special calibrations in various liquids at different frequencies.



Report NO: TS201510006 Page 10 / 96

### Light Beam unit:



Calibration: No calibration required.

The light beam switch allows automatic "tooling" of the probe. During the process, the actual position of the probe tip with respect to the robot arm is measured, as well as the probe length and the horizontal probe offset. The software then corrects all movements, such that the robot coordinates are valid for the probe tip. The repeatability of this process is better than 0.1 mm.

#### SAM Twin Phantom:



The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- Left hand
- Right hand
- Flat phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

#### Device Holder for SAM Twin Phantom:



The DASY device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation centers for both scales is the ear reference point (ERP). Thus the device needs no repositioning when changing the angles.

The DASY device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity "=3 and loss tangent \_=0.02. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered



Report NO: TS201510006 Page 11 / 96

# 6. Tissue Simulating Liquid

## 6.1 The composition of the tissue simulating liquid:

The following tissue formulations are provided for reference only as some of the parameters have not been thoroughly verified. The composition of ingredients may be modified accordingly to achieve the desired target tissue parameters required for routine SAR evaluation.

Frequency	Water	Sugar	Cellulose	Salt	Preventol	DGBE	Conductivity	Permittivity
(MHz)	(%)	(%)	(%)	(%)	(%)	(%)	(σ)	(εr)
				For H	ead			
900	40.3	57.9	0.2	1.4	0.2	0	0.97	41.5
1750	55.2	0	0	0.3	0	44.5	1.37	40.1
1800,1900,2000	55.2	0	0	0.3	0	44.5	1.40	40.0
2450	55.0	0	0	0	0	45.0	1.80	39.2
				For B	ody			
900	50.8	48.2	0	0.9	0.1	0	0.97	55.2
1750	70.2	0	0	0.4	0	29.4	1.49	53.4
1800,1900,2000	70.2	0	0	0.4	0	29.4	1.52	53.3
2450	68.6	0	0	0	0	31.4	1.95	52.7

#### 6.2 Tissue Calibration Result:

Eroguanav	Fraguency		Parameters	Tiggue Tomp	
Frequency	Description	Permittivity	Conductivity	Tissue Temp.	Date
(MHz)		(εr )	(σ)	(℃)	
200	Reference	41.50±5%	$0.97\!\pm\!5\%$	NA	
900	Reference	(39.425~43.574)	(0.9215~1.0185)	NA .	2015/10/18
(Head)	Measurement	42.12	0.98	22.5	
1000	Reference	40.00±5%	1.40±5%	NA	
1900	Reference	(38.00~42.00)	(1.33~1.47)	INA	2015/10/18
(Head)	Measurement	40.4	1.45	22.7	
	Reference	39.2±5%	1.80±5%	NA	
	Reference	(37.24~41.16)	(1.71~1.89)	INA	2015/10/18
(Head)	Measurement	38.1	1.84	22.1	



Report NO: TS201510006 Page 12 / 96

Eroguanav	Fraguency		Dielectric Parameters		
Frequency (MHz)	Description	Permittivity	Conductivity	Tissue Temp. (°C)	Date
` ′		(ɛr )	(σ)	` ,	
900	Reference	55.2±5%	$0.97\!\pm\!5\%$	NA	
	Reference	(52.44~57.96)	(0.9215~1.0185)	INA	2015/10/19
(Body)	Measurement	54.6	0.95	22.4	
1000	Reference	53.3±5%	1.52±5%	NA	
1900	Reference	(50.635~55.965)	(1.444~1.596)	INA	2015/10/20
(Body)	Measurement	53.5	1.51	22.8	
2450	Reference	52.7±5%	1.95±5%	NA	
	Reference	(50.065~55.335)	(1.8525~2.0475)	INA	2015/10/20
(Body)	Measurement	50.6	1.87	22.6	



Report NO: TS201510006 Page 13 / 96



Liquid depth in the Head Phantom (900 MHz) (depth>15cm)



Liquid depth in the Flat Phantom (900 MHz) (depth>15cm)



Report NO: TS201510006 Page 14 / 96



Liquid depth in the Head Phantom (1900 MHz) (depth>15cm)



Liquid depth in the Body Phantom (1900 MHz) (depth>15cm)



Report NO: TS201510006 Page 15 / 96



Liquid depth in the Head Phantom (2450 MHz) (depth>15cm)



Liquid depth in the Flat Phantom (2450 MHz) (depth>15cm)




Report NO: TS201510006 Page 16 / 96

## 7. SAR System Validation

#### 7.1 Validation System:

In the simplified setup for system evaluation, the EUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave that comes from a signal generator. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

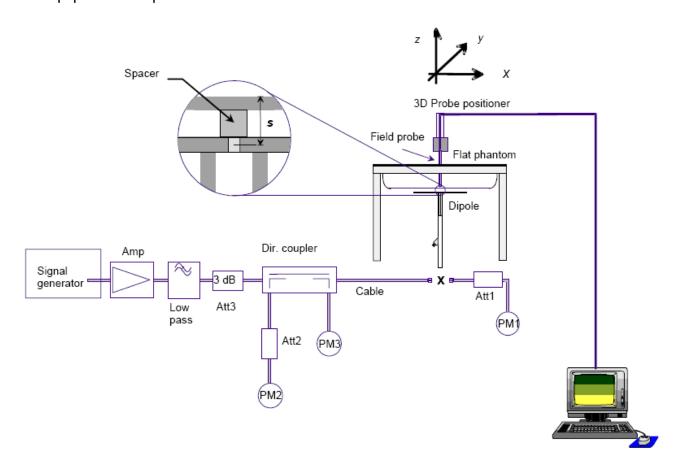

## 7.2 Validation Dipoles:

The dipoles used is based on the IEEE-1528/EN62209-1 standard, and is complied with mechanical and electrical specifications in line with the requirements of both IEEE-1528/EN62209-1 and FCC Supplement C.



Report NO: TS201510006 Page 17 / 96

## 7.3 Validation Result:

Frequency (MHz)	Description	SAR(1g) W/Kg	SAR(10g) W/Kg	Tissue Temp. (°C)	Date
900	Reference	10.7±10%	6.87±10%	NA	
(Head)	Reference	(9.63~11.77)	(6.18~7.49)	IVA	2015/10/18
(Fleau)	Measurement	10.68	6.92	22.5	
1900	Reference	40.6±10%	21.3±10%	NA	
	Reference	(36.54~44.66)	(19.17~23.43)	INA	2015/10/18
(Head)	Measurement	39.4	21.04	22.7	
2450	Deference	52.4±10%	24.4±10%	NA	
2450	Reference	(47.16~57.64)	(21.96~26.84)		2015/10/18
(Head)	Measurement	53.6	25.8	22.1	
000	Defenses	10.7±10%	6.94±10%	NA	
900 (Rody)	Reference	(9.63~11.77)	(6.246~7.634)	INA	2015/10/19
(Body)	Measurement	9.72	6.4	22.4	
1000	Deference	40.1±10%	21.3±10%	NA	
1900	Reference	(36.09~44.11)	(19.17~23.43)	NA	2015/10/20
(Body)	Measurement	40.4	21.68	22.8	
2450	Reference	53.7±10%	25.0±10%	NA	
2450	Reference	(48.33~59.07)	(22.5~27.5)	INA	2015/10/20
(Body)	Measurement	54.4	25.4	22.6	



Report NO: TS201510006 Page 18 / 96

#### 8. SAR Evaluation Procedures:

The procedure for assessing the average SAR value consists of the following steps:

#### Power Reference Measurement

The Power Reference Measurement and Power Drift Measurement jobs are useful jobs for monitoring the power drift of the device under test in the batch process. Both jobs measure the field at a specified reference position, at a selectable distance from the phantom surface. The reference position can be either the selected section's grid reference point or a user point in this section. The reference job projects the selected point onto the phantom surface, orients the probe perpendicularly to the surface, and approaches the surface using the selected detection method.

### > Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values, before doing a finer measurement around the hot spot. The sophisticated interpolation routines implemented in DASY4 software can find the maximum locations even in relatively coarse grids. The scanning area is defined by an editable grid. This grid is anchored at the grid reference point of the selected section in the phantom. When the Area Scan's property sheet is brought-up, grid settings can be edited by a user.

### Zoom Scan


Zoom Scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The default Zoom Scan measures 7 x 7 x 7 points (5mmx5mmx5mm) within a cube whose base faces are centered on the maxima found in a preceding area scan job within the same procedure.

#### Power Drift Measurement

The Power Drift Measurement job measures the field at the same location as the most recent power reference measurement job within the same procedure, and with the same settings. The Power Drift Measurement gives the field difference in dB from the reading conducted within the last Power Reference Measurement.



Report NO: TS201510006 Page 19 / 96

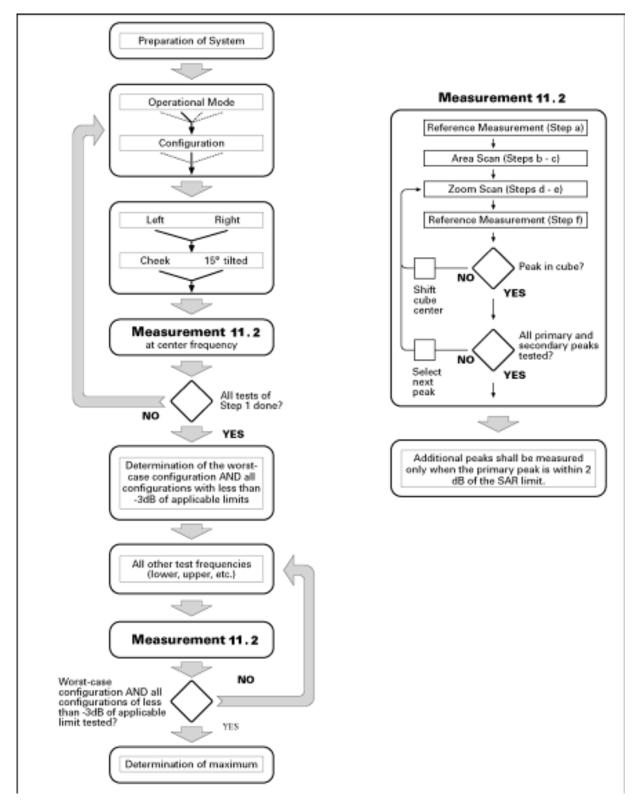

Block diagram of the tests to be performed



Report NO: TS201510006 Page 20 / 96

## 9. SAR Exposure Limits

#### 9.1 Uncontrolled Environment

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

#### 9.2 Controlled Environment

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. The exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

### Limits for Occupational/Controlled Exposure (W/kg)

Whole-Body	Partial-Body	Hands, Wrists, Feet and Ankles
0.4	8.0	20.0

#### Limits for General Population/Uncontrolled Exposure (W/kg)

Whole-Body	Partial-Body	Hands, Wrists, Feet and Ankles
0.08	1.6	4.0

Whole-Body SAR is averaged over the entire body, partial-body SAR is averaged over any 1gram of tissue defined as a tissue volume in the shape of a cube. SAR for hands, wrists, feet and ankles is averaged over any 10 grams of tissue defined as a tissue volume in the shape of a cube.



Report NO: TS201510006 Page 21 / 96

# 10. Measurement Uncertainty:

NO	Source	Uncert.	Prob. Dist.	Div. k	ci (1g)	ci (10g)	Stand. Uncert. ui (1g)	Stand. Uncert. ui (10g)	Veff	
1	Repeat	0.04	N	1	1	1	0.04	0.04	9	
Instru	nstrument									
2	Probe calibration	7	N	2	1	1	3.5	3.5	∞	
3	Axial isotropy	4.7	R	√3	0.7	0.7	1.9	1.9	∞	
4	Hemispherical isotropy	9.6	R	√3	0.7	0.7	3.9	3.9	∞	
5	Boundary effect	1.0	R	<sub>1</sub> /2	1	1	0.6	0.6	∞	
6	Linearity	4.7	R	$\sqrt{3}$	1	1	2.7	2.7	∞	
7	Detection limits	1.0	R	<del>√</del> 3	1	1	0.6	0.6	∞	
8	Readout electronics	0.3	N	1	1	1	0.3	0.3	∞	
9	Response time	0.8	R	√3	1	1	0.5	0.5	∞	
10	Integration time	2.6	R	$\sqrt{3}$	1	1	1.5	1.5	∞	
11	Ambient noise	3.0	R	$\sqrt{3}$	1	1	1.7	1.7	∞	
12	Ambient reflections	3.0	R	$\sqrt{3}$	1	1	1.7	1.7	∞	
13	Probe positioner mech. restrictions	0.4	R	√3	1	1	0.2	0.2	∞	
14	Probe positioning with respect to phantom shell	2.9	R	√3	1	1	1.7	1.7	∞	
15	Max.SAR evaluation	1.0	R	√3	1	1	0.6	0.6	∞	
Test s	sample related									
16	Device positioning	3.8	N	1	1	1	3.8	3.8	99	



Report NO: TS201510006 Page 22 / 96

17	Device holder	5.1	N	1	1	1	5.1	5.1	5	
18	Drift of output power	5.0	R	√3	1	1	2.9	2.9	∞	
Phan	Phantom and set-up									
19	Phantom uncertainty	4.0	R	$\sqrt{3}$	1	1	2.3	2.3	∞	
20	Liquid conductivity (target)	5.0	R	√3	0.64	0.43	1.8	1.2	∞	
21	Liquid conductivity (meas)	2.5	N	1	0.64	0.43	1.6	1.2	∞	
22	Liquid Permittivity (target)	5.0	R	√3	0.6	0.49	1.7	1.5	∞	
23	3 Liquid Permittivity (meas) 2.5		N	1	0.6	0.49	1.5	1.2	∞	
Combined standard			RSS	$U_C = \sqrt{\sum_{i=1}^{n} C_i^2 U_i^2}$		12.2%	11.9%	236		
Expanded uncertainty (P=95%)			U = k U	$U_{c}$ ,k=2			24.4%	23.8%		



Report NO: TS201510006 Page 23 / 96

### 11. Conducted Power Measurement:

#### <GSM Conducted Power>

General Note:

- 1. Per KDB 447498 D01v05r02, the maximum output power channel is used for SAR testing and for further SAR test reduction.
- 2. According to October 2013TCB Workshop, for GSM / GPRS, the number of time slots to test for SAR should correspond to the highest frame-average maximum output power configuration, considering the possibility of e.g. 3rd party VoIP operation for head and body-worn SAR testing, the EUT was set in GPRS (4Tx slot) for GSM850/GSM1900 band due to their highest frame-average power.
- 3. For hotspot mode SAR testing, GPRS should be evaluated, therefore the EUT was set in GPRS 4 Tx slots for GSM850/GSM1900 band due to its highest frame-average power.

Band GSM850	Burst Av	erage Pow	er (dBm)	Frame-Av	erage Pov	ver (dBm)
TX Channel	128	189	251	128	189	251
Frequency (MHz)	824.2	836.4	848.8	824.2	836.4	848.8
GSM (GMSK, 1 Tx slot)	32.08	32.06	32.07	23.08	23.06	23.07
GPRS (GMSK, 1 Tx slot) – CS1	32.04	32.05	32.06	23.04	23.05	23.06
GPRS (GMSK, 2 Tx slots) – CS1	31.12	31.09	31.06	25.12	25.09	25.06
GPRS (GMSK, 3 Tx slots) – CS1	29.23	29.18	29.18	24.97	24.92	24.92
GPRS (GMSK, 4 Tx slots) – CS1	28.3	28.27	28.21	25.30	25.27	25.21
Band GSM1900	Burst Av	erage Pow	er (dBm)	Frame-A	erage Pov	ver (dBm)
Band GSM1900 TX Channel	Burst Av 512	erage Pow 661	ver (dBm) 810	Frame-Av	erage Pov 661	ver (dBm) 810
			. ,			. ,
TX Channel	512	661	810	512	661	810
TX Channel Frequency (MHz)	512 1850.2	661 1880	810 1909.8	512 1850.2	661 1880	810 1909.8
TX Channel Frequency (MHz) GSM (GMSK, 1 Tx slot)	<b>512 1850.2</b> 29.07	661 1880 29.1	810 1909.8 29.25	<b>512</b> <b>1850.2</b> 20.07	661 1880 20.10	810 1909.8 20.25
TX Channel Frequency (MHz) GSM (GMSK, 1 Tx slot) GPRS (GMSK, 1 Tx slot) – CS1	<b>512 1850.2</b> 29.07 29.06	661 1880 29.1 29.08	810 1909.8 29.25 29.22	512 1850.2 20.07 20.06	661 1880 20.10 20.08	810 1909.8 20.25 20.22

Remark: The frame-averaged power is linearly scaled the maximum burst averaged power over 8 time slots.

The calculated method are shown as below:

Frame-averaged power = Maximum burst averaged power (1 Tx Slot) - 9 dB

Frame-averaged power = Maximum burst averaged power (2 Tx Slots) - 6 dB

Frame-averaged power = Maximum burst averaged power (3 Tx Slots) - 4.26 dB

Frame-averaged power = Maximum burst averaged power (4 Tx Slots) - 3 dB

# 7

## SHENZHEN SUNWAY COMMUNICATION CO.,LTD

Report NO: TS201510006 Page 24 / 96

#### <WCDMA Conducted Power>

The following tests were conducted according to the test requirements outlines in 3GPP TS 34.121 specification. A summary of these settings are illustrated below:

#### **HSDPA Setup Configuration:**

- a. The EUT was connected to Base Station Agilent E5515C referred to the Setup Configuration.
- b. The RF path losses were compensated into the measurements.
- c. A call was established between EUT and Base Station with following setting:
  - i. Set Gain Factors ( $\beta_c$  and  $\beta_d$ ) and parameters were set according to each
  - ii. Specific sub-test in the following table, C10.1.4, quoted from the TS 34.121
  - iii. Set RMC 12.2Kbps + HSDPA mode.
  - iv. Set Cell Power = -86 dBm
  - v. Set HS-DSCH Configuration Type to FRC (H-set 1, QPSK)
  - vi. Select HSDPA Uplink Parameters
  - vii. Set Delta ACK, Delta NACK and Delta CQI = 8
  - viii. Set Ack-Nack Repetition Factor to 3
  - ix. Set CQI Feedback Cycle (k) to 4 ms
  - x. Set CQI Repetition Factor to 2
  - xi. Power Ctrl Mode = All Up bits
- d. The transmitted maximum output power was recorded.

Table C.10.1.4: β values for transmitter characteristics tests with HS-DPCCH

Sub-test	βο	βd	β <sub>d</sub> (SF)	βc/βd	βнs (Note1, Note 2)	CM (dB) (Note 3)	MPR (dB) (Note 3)
1	2/15	15/15	64	2/15	4/15	0.0	0.0
2	12/15	15/15	64	12/15	24/15	1.0	0.0
	(Note 4)	(Note 4)		(Note 4)			
3	15/15	8/15	64	15/8	30/15	1.5	0.5
4	15/15	4/15	64	15/4	30/15	1.5	0.5

- Note 1:  $\Delta_{ACK}$ ,  $\Delta_{NACK}$  and  $\Delta_{CQI} = 30/15$  with  $\beta_{hs} = 30/15 * \beta_c$ .
- Note 2: For the HS-DPCCH power mask requirement test in clause 5.2C, 5.7A, and the Error Vector Magnitude (EVM) with HS-DPCCH test in clause 5.13.1A, and HSDPA EVM with phase discontinuity in clause 5.13.1AA,  $\Delta_{\rm ACK}$  and  $\Delta_{\rm NACK}$  = 30/15 with  $\beta_{hs}$  = 30/15 \*  $\beta_c$ , and  $\Delta_{\rm CQI}$  = 24/15 with  $\beta_{hs}$  = 24/15 \*  $\beta_c$ .
- Note 3: CM = 1 for  $\beta_0/\beta_d$  =12/15,  $\beta_{hs}/\beta_c$ =24/15. For all other combinations of DPDCH, DPCCH and HSDPCH the MPR is based on the relative CM difference. This is applicable for only UEs that support HSDPA in release 6 and later releases.
- Note 4: For subtest 2 the  $\beta_c/\beta_d$  ratio of 12/15 for the TFC during the measurement period (TF1, TF0) is achieved by setting the signalled gain factors for the reference TFC (TF1, TF1) to  $\beta_c$  = 11/15 and  $\beta_d$  = 15/15.

**Setup Configuration** 

# 7

## SHENZHEN SUNWAY COMMUNICATION CO.,LTD

Report NO: TS201510006 Page 25 / 96

#### **HSUPA Setup Configuration:**

- a. The EUT was connected to Base Station Agilent E5515C referred to the Setup Configuration.
- b. The RF path losses were compensated into the measurements.
- c. A call was established between EUT and Base Station with following setting \*:
  - i. Call Configs = 5.2B, 5.9B, 5.10B, and 5.13.2B with QPSK
  - ii. Set the Gain Factors ( $\beta_c$  and  $\beta_d$ ) and parameters (AG Index) were set according to each specific sub-test in the following table, C11.1.3, quoted from the TS 34.121
  - iii. Set Cell Power = -86 dBm
  - iv. Set Channel Type = 12.2k + HSPA
  - v. Set UE Target Power
  - vi. Power Ctrl Mode= Alternating bits
  - vii. Set and observe the E-TFCI
  - viii. Confirm that E-TFCI is equal to the target E-TFCI of 75 for sub-test 1, and other subtest's E-TFCI
- d. The transmitted maximum output power was recorded.

Table C.11.1.3: β values for transmitter characteristics tests with HS-DPCCH and E-DCH

Sub- test	βε	βa	β <sub>d</sub> (SF)	βc/βd	βнs (Note1)	βес	β <sub>ed</sub> (Note 5) (Note 6)	β <sub>ed</sub> (SF)	β <sub>ed</sub> (Codes)	CM (dB) (Note 2)	MPR (dB) (Note 2)	AG Index (Note 6)	E- TFCI
1	11/15 (Note 3)	15/15 (Note 3)	64	11/15 (Note 3)	22/15	209/2 25	1309/225	4	1	1.0	0.0	20	75
2	6/15	15/15	64	6/15	12/15	12/15	94/75	4	1	3.0	2.0	12	67
3	15/15	9/15	64	15/9	30/15	30/15	β <sub>ed</sub> 1: 47/15 β <sub>ed</sub> 2: 47/15	4 4	2	2.0	1.0	15	92
4	2/15	15/15	64	2/15	4/15	2/15	56/75	4	1	3.0	2.0	17	71
5	15/15 (Note 4)	15/15 (Note 4)	64	15/15 (Note 4)	30/15	24/15	134/15	4	1	1.0	0.0	21	81

Note 1:  $\Delta_{ACK}$ ,  $\Delta_{NACK}$  and  $\Delta_{CQI}$  = 30/15 with  $\beta_{hs}$  = 30/15 \*  $\beta_c$ .

Note 2: CM = 1 for  $\beta_c/\beta_d$  =12/15,  $\beta_{ns}/\beta_c$ =24/15. For all other combinations of DPDCH, DPCCH, HS- DPCCH, E-DPDCH and E-DPCCH the MPR is based on the relative CM difference.

Note 3: For subtest 1 the  $\beta_c/\beta_d$  ratio of 11/15 for the TFC during the measurement period (TF1, TF0) is achieved by setting the signalled gain factors for the reference TFC (TF1, TF1) to  $\beta_c$  = 10/15 and  $\beta_d$  = 15/15.

Note 4: For subtest 5 the  $\beta_c/\beta_d$  ratio of 15/15 for the TFC during the measurement period (TF1, TF0) is achieved by setting the signalled gain factors for the reference TFC (TF1, TF1) to  $\beta_c$  = 14/15 and  $\beta_d$  = 15/15.

Note 5: In case of testing by UE using E-DPDCH Physical Layer category 1, Sub-test 3 is omitted according to TS25.306 Table 5.1g.

Note 6:  $\beta_{ed}$  can not be set directly, it is set by Absolute Grant Value.

**Setup Configuration** 



Report NO: TS201510006 Page 26 / 96

#### **General Note**

- Per KDB 941225 D01 v02, RMC 12.2kbps setting is used to evaluate SAR. If AMR 12.2kbps power is < 0.25dB higher than RMC 12.2kbps, SAR tests with AMR 12.2kbps can be excluded.
- 2. By design, AMR and HSDPA/HSUPA RF power will not be larger than RMC 12.2kbps, detailed information is included in Tune-up Procure exhibit.
- 3. It is expected by the manufacturer that MPR for some HSDPA/HSUPA subtests may differ from the specification of 3GPP, according to the chipset implementation in this model. The implementation and expected deviation are detailed in tune-up procedure exhibit.

Band		WCDMA I	I		WCDMA V	
TX Channel	9262	9400	9538	4132	4183	4233
Rx Channel	9662	9800	9938	4357	4408	4458
Frequency (MHz)	1852.4	1880	1907.6	826.4	836.6	846.6
AMR 12.2Kbps	21.68	21.53	21.55	22.49	22.50	22.36
RMC 12.2Kbps	21.69	21.61	21.56	22.50	22.51	22.37
HSDPA Subtest-1	20.70	20.69	20.58	21.54	21.58	21.40
HSDPA Subtest-2	20.34	20.28	20.16	21.08	21.09	20.90
HSDPA Subtest-3	18.65	18.59	18.55	19.36	19.48	19.29
HSDPA Subtest-4	18.77	18.61	18.60	19.54	19.39	19.19
HSUPA Subtest-1	20.64	20.54	20.49	21.40	21.41	21.22
HSUPA Subtest-2	20.60	20.63	20.52	21.48	21.50	21.30
HSUPA Subtest-3	18.67	18.68	18.42	19.23	19.51	19.36
HSUPA Subtest-4	20.67	20.71	20.55	21.54	21.50	21.39
HSUPA Subtest-5	19.70	19.58	19.53	20.41	20.37	20.27



Report NO: TS201510006 Page 27 / 96

#### <WLAN 2.4GHz Conducted Power>

Mode	Channel	Frequency (MHz)	Conducted Output Power(dBm)	Test Rate Data
	1	2412	11.80	1 Mbps
802.11b	6	2437	12.36	1 Mbps
	11	2462	12.82	1 Mbps
	1	2412	8.57	6 Mbps
802.11g	6	2437	11.20	6 Mbps
	11	2462	9.52	6 Mbps
	1	2412	8.48	6.5 Mbps
802.11n(20MHz)	6	2437	11.06	6.5 Mbps
	11	2462	9.60	6.5 Mbps
	1	2412	6.89	13.5Mbps
802.11n(40MHz)	6	2437	11.12	13.5Mbps
	11	2462	7.79	13.5Mbps

#### Note:

1. Per KDB 447498 D01v05r02, the 1-g SAR test exclusion thresholds for 100 MHz to 6 GHz at *test* separation distances ≤ 50 mm are determined by:

[(max. power of channel, including tune-up tolerance, mW) / (min. test separation distance, mm)] · [ $\sqrt{f(GHz)}$ ]  $\leq 3.0$  for 1-g SAR, where

- · f(GHz) is the RF channel transmit frequency in GHz
- · Power and distance are rounded to the nearest mW and mm before calculation
- · The result is rounded to one decimal place for comparison

Channel	Frequency (GHz)	Tune-up Power (dBm)	Max. Power (mW)	Test distance (mm)	Result	exclusion thresholds for 1-g SAR
b/CH 11	2.462	13.5	22.39	5	7.05	3.0
g/CH 6	2.437	12.0	15.85	5	4.99	3.0

- 2. Base on the result of note1, RF exposure evaluation of 802.11 b mode is required.
- 3. Per KDB 248227 D01v02, choose the highest output power channel to test SAR and determine further SAR exclusion.
- 4. Per KDB 248227 D01v02, In the 2.4 GHz band, separate SAR procedures are applied to DSSS and OFDM configurations to simplify DSSS test requirements. SAR is not required for the following 2.4 GHz OFDM conditions:
  - 1) When KDB Publication 447498 SAR test exclusion applies to the OFDM configuration.
  - 2) When the highest reported SAR for DSSS is adjusted by the ratio of OFDM to DSSS specified maximum output power and the adjusted SAR is ≤ 1.2 W/kg.
- 5. The output power of all data rate were pre-scan, just the worst case (the lowest data rate) of all mode were shown in report.
- 6. Per KDB 248227 D01V02 section 2.2, when the EUT in continuously transmitting mode, the actual duty cycle is 98.4%, so the duty cycle factor is 1.02.



Report NO: TS201510006 Page 28 / 96

#### <Bluetooth Conducted Power>

Mada Band	Average power(dBm)
Mode Band	Bluetooth v3.0+EDR
2.4GHz Bluetooth	-0.36

Per KDB 447498 D01v05r02, the 1-g and 10-g SAR test exclusion thresholds for 100 MHz to 6 GHz at test separation distances  $\leq$  50 mm are determined by:

[(max. power of channel, including tune-up tolerance, mW)/(min. test separation distance,

mm)]  $\cdot [\sqrt{f(GHz)}] \le 3.0$  for 1-g SAR and  $\le 7.5$  for 10-g extremity SAR

- · f(GHz) is the RF channel transmit frequency in GHz
- · Power and distance are rounded to the nearest mW and mm before calculation
- · The result is rounded to one decimal place for comparison

Bluetooth Turn up Power (dBm)	Separation Distance (mm)	Frequency (GHz)	exclusion thresholds	
1	0	2.48	0.4	


Per KDB 447498 D01v05r02, when the minimum test separation distance is < 5 mm, a distance of 5 mm is applied to determine SAR test exclusion. The test exclusion threshold is 0.4 which is <= 3, SAR testing is not required.



Report NO: TS201510006 Page 29 / 96

## 12. Antenna Location

**Top Side** 

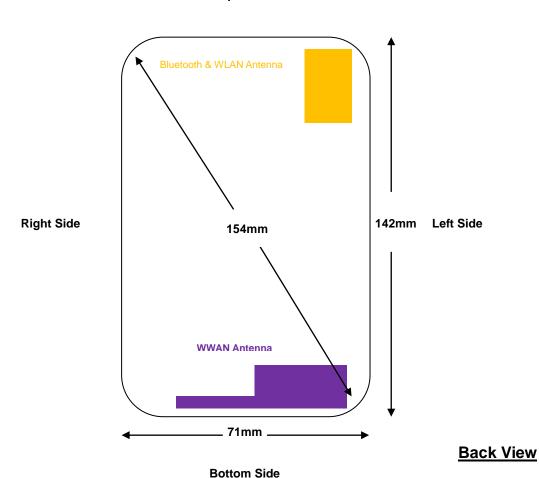

	Distance of The Antenna to the EUT surface and edge									
Antennas	Front	Back	Top Side	<b>Bottom Side</b>	Left Side	Right Side				
WWAN	/	/	>25mm	/	/	<25mm				
BT&WLAN	/	/	/	>25mm	/	>25mm				

Positions for SAR tests; Hotspot mode										
Antennas	Antennas Front Back Top Side Bottom Side Left Side Right Side									
WWAN	Yes	Yes	No	Yes	Yes	Yes				
BT&WLAN	Yes	Yes	Yes	No	Yes	No				

**General Note:** Referring to KDB 941225 D06 v02, When the overall device length and width are ≥9cm\*5cm, the test distance is 10mm, SAR must be measured for all sides and surfaces with a transmitting antenna located with 25mm from that surface or edge.



Report NO: TS201510006 Page 30 / 96

# 13. Results and Test photos:

13.1 SAR result summary:

Head

Test Case of Head		Meas.	Target		Meas. SAR	Scale	Power		
Band	Test Position	СН	Power (dBm)	Power (dBm)	Factor	(W/kg) 1g Avg.	SAR (W/kg)	Drift <±0.2 dB	Plot
	Right Cheek	Ch128	32.08	32.50	1.102	0.309	0.340	0.064	#1
GSM	Right Tilt	Ch128	32.08	32.50	1.102	0.164	0.181	0.038	
850	Left Cheek	Ch128	32.08	32.50	1.102	0.265	0.292	-0.113	
	Left Tilt	Ch128	32.08	32.50	1.102	0.157	0.173	0.054	
	Right Cheek	Ch810	29.25	30.00	1.189	0.151	0.179	0.044	
GSM	Right Tilt	Ch810	29.25	30.00	1.189	0.0566	0.067	0.011	
1900	Left Cheek	Ch810	29.25	30.00	1.189	0.194	0.231	0.118	#2
	Left Tilt	Ch810	29.25	30.00	1.189	0.0557	0.066	0.088	
	Right Cheek	Ch4183	22.51	23.00	1.119	0.335	0.375	-0.150	#3
WCDM A Band	Right Tilt	Ch4183	22.51	23.00	1.119	0.172	0.193	0.149	
V	Left Cheek	Ch4183	22.51	23.00	1.119	0.284	0.318	0.130	
	Left Tilt	Ch4183	22.51	23.00	1.119	0.166	0.186	0.063	
	Right Cheek	Ch9262	21.69	22.00	1.074	0.333	0.358	-0.086	
WCDM	Right Tilt	Ch9262	21.69	22.00	1.074	0.154	0.165	0.000	
A Band II	Left Cheek	Ch9262	21.69	22.00	1.074	0.356	0.382	0.192	#4
	Left Tilt	Ch9262	21.69	22.00	1.074	0.132	0.142	-0.134	

Test Case of Head		Meas.	Target			Meas.	Scale			
Band	Test Position	СН	Power (dBm)	Power Factor	D.C Factor	SAR (W/kg) 1g	SAR (W/kg)	Power Drift(dB)	Plot	
	Right Cheek	Ch11	12.82	13.50	1.169	1.02	0.0781	0.0931	-0.052	#5
WLA	Right Tilt	Ch11	12.82	13.50	1.169	1.02	0.0663	0.0791	-0.028	
N2.4 G	Left Cheek	Ch11	12.82	13.50	1.169	1.02	0.044	0.0525	0.140	
	Left Tilt	Ch11	12.82	13.50	1.169	1.02	0.028	0.0333	0.051	



Report NO: TS201510006 Page 31 / 96

# Body Hotspot (10mm between DUT and Flat Phantom)

Test Case of Head		Meas.	Target		Meas. SAR	Scale	Power		
Band	Test Position	СН	Power (dBm)	Power (dBm)	Factor	(W/kg) 1g Avg.	SAR (W/kg)	Drift <±0.2 dB	Plot
	Front	Ch128	28.30	28.50	1.047	0.414	0.434	0.130	
GPRS 850(4	Back	Ch128	28.30	28.50	1.047	0.712	0.746	-0.006	#6
7x	Left Side	Ch128	28.30	28.50	1.047	0.351	0.368	0.110	
slots)	Right Side	Ch128	28.30	28.50	1.047	0.449	0.470	0.076	
	Bottom Side	Ch128	28.30	28.50	1.047	0.237	0.248	0.175	
	Front	Ch810	25.38	26.00	1.153	0.331	0.382	0.006	
GPRS	Back	Ch810	25.38	26.00	1.153	0.511	0.589	-0.099	#7
1900(4 Tx	Left Side	Ch810	25.38	26.00	1.153	0.139	0.160	0.026	
slots)	Right Side	Ch810	25.38	26.00	1.153	0.076	0.088	0.177	
	Bottom Side	Ch810	25.38	26.00	1.153	0.423	0.488	0.144	
	Front	Ch4183	22.51	23.00	1.119	0.265	0.297	0.086	
WCDM	Back	Ch4183	22.51	23.00	1.119	0.519	0.581	-0.020	#8
А	Left Side	Ch4183	22.51	23.00	1.119	0.227	0.254	-0.062	
Band V	Right Side	Ch4183	22.51	23.00	1.119	0.316	0.354	0.156	
	Bottom Side	Ch4183	22.51	23.00	1.119	0.134	0.150	-0.172	
	Front	Ch9262	21.69	22.00	1.074	0.426	0.458	0.151	
WCDM	Back	Ch9262	21.69	22.00	1.074	0.599	0.643	-0.094	#9
А	Left Side	Ch9262	21.69	22.00	1.074	0.239	0.257	0.053	
Band II	Right Side	Ch9262	21.69	22.00	1.074	0.117	0.126	0.162	
	Bottom Side	Ch9262	21.69	22.00	1.074	0.462	0.496	-0.159	



Report NO: TS201510006 Page 32 / 96

Те	Test Case of Head		Meas.	Target			Meas.	Scale		
Band	Test Position	СН	Power (dBm)	Power (dBm)	Factor	D.C Factor	SAR (W/kg) 1g	SAR (W/kg)	Power Drift(dB)	Plot
	Front	Ch11	12.82	13.50	1.169	1.02	0.036	0.0429	0.094	
WLA N	Back	Ch11	12.82	13.50	1.169	1.02	0.0673	0.0802	0.114	#10
2.4G	Left Side	Ch11	12.82	13.50	1.169	1.02	0.012	0.0143	0.166	
	Тор	Ch11	12.82	13.50	1.169	1.02	0.032	0.0376	0.058	



Report NO: TS201510006 Page 33 / 96

Body Worn (10mm between DUT and Flat Phantom

Те	Test Case of Head			Target		Meas. SAR	Scale	Power Drift
Band	Test Position	СН	Power (dBm)	Power (dBm)	Factor	(W/kg) 1g Avg.	SAR (W/kg)	<±0.2 dB
GPRS 850(4	Front	Ch128	28.30	28.50	1.047	0.414	0.434	0.130
Tx slots)	Back	Ch128	28.30	28.50	1.047	0.712	0.746	-0.006
GPRS 1900(4	Front	Ch810	25.38	26.00	1.153	0.331	0.382	-0.164
Tx slots)	Back	Ch810	25.38	26.00	1.153	0.511	0.589	0.141
WCDM	Front	Ch4183	22.51	23.00	1.119	0.265	0.297	0.086
A Band V	Back	Ch4183	22.51	23.00	1.119	0.519	0.581	-0.020
WCDM	Front	Ch9262	21.69	22.00	1.074	0.426	0.458	0.151
A Band II	Back	Ch9262	21.69	22.00	1.074	0.599	0.643	-0.094

#### 13.2 Evaluation of Simultaneous:

#### BT\* - Estimated SAR for Bluetooth

(max. power of channel, including tune-up tolerance, mW)/(min. test separation distance, mm)]·[ $\sqrt{f_{\text{(GHz)}}}/x$ ] W/kg for test separation distances  $\leq$  50 mm;

where x = 7.5 for 1-g SAR, and x = 18.75 for 10-g SAR.

Maximum Turn	Exposure Position	Head	Hotspot	Body-worn	
up Power	Test separation	0 mm	10 mm	10 mm	
1dBm	Estimated SAR (W/kg)	0.053W/kg	0.026W/kg	0.026W/kg	

### **Conclusion:**

According to the above table, the sum of reported SAR values for GSM/WCDMA and WIFI/BT <1.6W/kg. So the simultaneous transmission SAR is not required for WIFI/BT transmitter.



Report NO: TS201510006

Page 34 / 96

# 13.3 DUT and setup photos photos:



Front



Back



Report NO: TS201510006 Page 35 / 96



Left Cheek Left Tilt



Right Cheek Right Tilt



Report NO: TS201510006 Page 36 / 96



Front of the EUT with 1 cm Gap



Back of the EUT with 1 cm Gap



Left of the EUT with 1 cm Gap

Right of the EUT with 1 cm Gap



Top of the EUT with 1 cm Gap

Bottom of the EUT with 1 cm Gap



Report NO: TS201510006 Page 37 / 96

### 14. Equipment List:

NO.	Instrument	Manufacturer	Model	S/N	Cal. Date	Cal. Due Date
1	Communication Tester	Agilent	E5515C	MY502672 64	Dec 26 <sup>th</sup> 2015	Dec 25 <sup>th</sup> 2016
2	E-field Probe	Speag	ES3DV3	3028	Oct 22 <sup>th</sup> 2014	Oct 21 <sup>th</sup> 2015
3	Dielectric Probe Kit	Speag	DAK	1038	N/A	N/A
4	DAE	Speag	DAE4	905	Jul 16 <sup>th</sup> 2015	Jul 15 <sup>th</sup> 2016
5	SAM TWIN phantom	Speag	SAM	1360/1432	N/A	N/A
6	Robot	Stabuli	TX60L	N/A	N/A	N/A
7	Device Holder	Speag	SD000H0 1HA	N/A	N/A	N/A
8	Vector Network	Agilent	E5071C	MY461076 15	Jan 6 <sup>th</sup> 2015	Jan 7 <sup>th</sup> 2016
9	Signal Generator	Agilent	E4438C	MY490722 79	Nov 27 <sup>th</sup> 2014	Nov 26 <sup>th</sup> 2015
10	Amplifier	Mini-circult	ZHL-42W	QA098002	N/A	N/A
11	Power Meter	Agilent	N1419A	MY500015 63	Nov 27 <sup>th</sup> 2014	Nov 26 <sup>th</sup> 2015
12	Power Sensor	Agilent	N8481H	MY510200 10	Nov 27 <sup>th</sup> 2014	Nov 26 <sup>th</sup> 2015
13	Directional Coupler	Agilent	772D	MY461512 75	Nov 27 <sup>th</sup> 2014	Nov 26 <sup>th</sup> 2015
14	Directional Coupler	Agilent	778D	MY482206 07	Nov 27 <sup>th</sup> 2014	Nov 26 <sup>th</sup> 2015
15	Dipole 900MHz	Speag	D900V2	1d086	Aug 9 <sup>th</sup> 2013	Aug 8 <sup>th</sup> 2016
16	Dipole 1900MHz	Speag	D1900V2	5d194	Jan 7 <sup>th</sup> 2015	Aug 6 <sup>th</sup> 2018
18	Dipole 2450MHz	Speag	D2450V2	955	Jan 8 <sup>th</sup> 2015	Jan 7 <sup>th</sup> 2018



Report NO: TS201510006 Page 38 / 96

#### Appendix A. System validation plots:

DUT: Dipole 900MHz; Type: D900V2; Serial: D900V2 - SN: 1d086 Program Name: System Performance Check at 900 MHz Head

Communication System: CW; Frequency: 900 MHz; Duty Cycle: 1:1

Medium parameters used: f = 900 MHz;  $\sigma = 0.98 \text{ mho/m}$ ;  $\varepsilon_r = 42.12$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(6.19, 6.19, 6.19); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015

- Phantom: SAM 2; Type: SAM; Serial: TP-1432

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172


**d=15mm, Pin=250mW/Area Scan (61x61x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 2.82 mW/g

**d=15mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 54.523 V/m; Power Drift = -0.01dB

Peak SAR (extrapolated) = 4.068 W/kg

SAR(1 g) = 2.67 mW/g; SAR(10 g) = 1.73 mW/gMaximum value of SAR (measured) = 2.90 mW/g

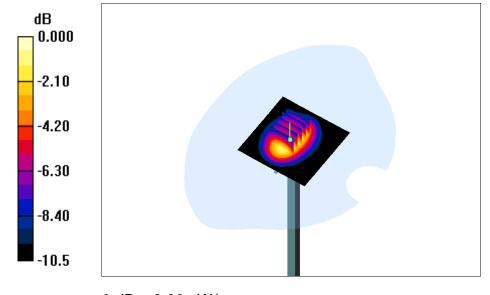

0 dB = 2.90 mW/g



Report NO: TS201510006 Page 39 / 96

DUT: Dipole 1900MHz; Type: D1900V2; Serial: 5d194

Program Name: System Performance Check at 1900 MHz Head

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium parameters used: f = 1900 MHz;  $\sigma = 1.45 \text{ mho/m}$ ;  $\epsilon_r = 40.4$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(4.68, 4.68, 4.68); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 7/16/2015
- Phantom: SAM 1; Type: SAM; Serial: TP-1360
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172


**d=10mm, Pin=250mW/Area Scan (91x91x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 11.3 mW/g

**d=10mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 80.6 V/m; Power Drift = -0.005 dB

Peak SAR (extrapolated) = 17.5 W/kg

SAR(1 g) = 9.87 mW/g; SAR(10 g) = 5.26 mW/gMaximum value of SAR (measured) = 11.2 mW/g

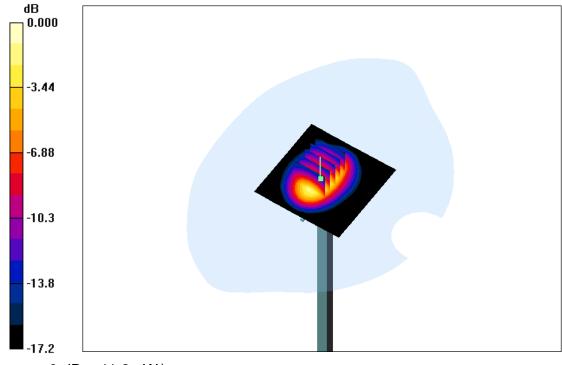

0 dB = 11.2 mW/g



Report NO: TS201510006 Page 40 / 96

**DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 955** 

Program Name: System Performance Check at 2450 MHz Head

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2450 MHz;  $\sigma = 1.84 \text{ mho/m}$ ;  $\varepsilon_r = 38.1$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(4.21, 4.21, 4.21); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015

- Phantom: SAM 1; Type: SAM; Serial: TP-1360

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172


**d=10mm, Pin=250mW/Area Scan (61x61x1):** Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (interpolated) = 16.7 mW/g

**d=10mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 87.0 V/m; Power Drift = 0.019 dB

Peak SAR (extrapolated) = 30.7 W/kg

SAR(1 g) = 13.4 mW/g; SAR(10 g) = 6.45 mW/g Maximum value of SAR (measured) = 16.2 mW/g

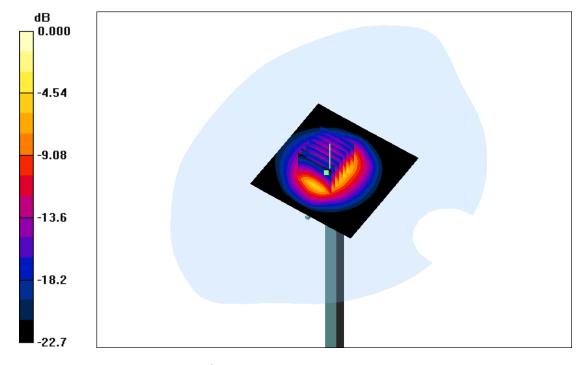

0 dB = 16.2 mW/g



Report NO: TS201510006 Page 41 / 96

DUT: Dipole 900MHz; Type: D900V2; Serial: D900V2 - SN: 1d086 Program Name: System Performance Check at 900 MHz Body

Communication System: CW; Frequency: 900 MHz; Duty Cycle: 1:1

Medium parameters used: f = 900 MHz;  $\sigma = 0.95 \text{ mho/m}$ ;  $\epsilon_r = 54.6$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

#### DASY4 Configuration:

- Probe: ES3DV3 SN3028; ConvF(6.02, 6.02, 6.02); Calibrated:10/22/2014
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 7/16/2015
- Phantom: SAM 2; Type: SAM; Serial: TP-1432
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

**d=15mm, Pin=250mW/Area Scan (61x61x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 2.72 mW/g


**d=15mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 54.523 V/m; Power Drift = -0.01dB

Peak SAR (extrapolated) = 4.068 W/kg

SAR(1 g) = 2.43 mW/g; SAR(10 g) = 1.6 mW/g

Maximum value of SAR (measured) = 2.80 mW/g

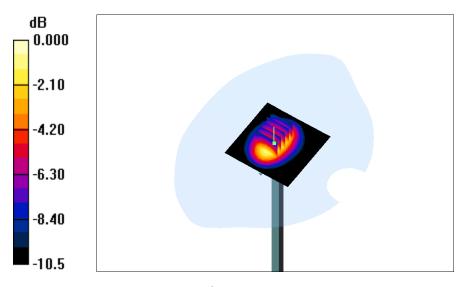

0 dB = 2.90 mW/g



Report NO: TS201510006 Page 42 / 96

DUT: Dipole 1900MHz; Type: D1900V2; Serial: 5d194

Program Name: System Performance Check at 1900 MHz Body

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium parameters used: f = 1900 MHz;  $\sigma = 1.51 \text{ mho/m}$ ;  $\varepsilon_r = 53.5$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

#### DASY4 Configuration:

- Probe: ES3DV3 SN3028; ConvF(4.48, 4.48, 4.48); Calibrated: 10/22/2014
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn905; Calibrated: 7/16/2015
- Phantom: SAM 1; Type: SAM; Serial: TP-1360
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172


**d=10mm, Pin=250mW/Area Scan (91x91x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 12.8 mW/g

**d=10mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 85.9 V/m; Power Drift = 0.109 dB

Peak SAR (extrapolated) = 19.7 W/kg

**SAR(1 g) = 10.1 mW/g; SAR(10 g) = 5.42 mW/g** Maximum value of SAR (measured) = 12.5 mW/g

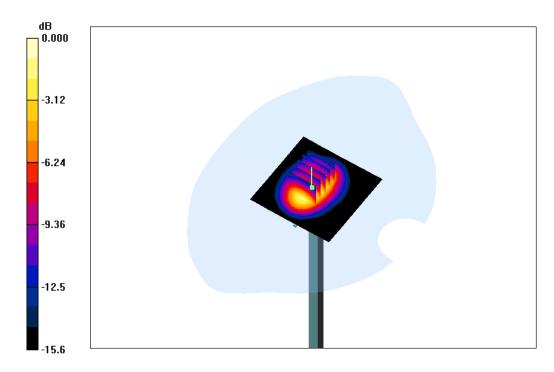

0 dB = 12.5 mW/g



Report NO: TS201510006 Page 43 / 96

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 955

Program Name: System Performance Check at 2450 MHz Body

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2450 MHz;  $\sigma$  = 1.87 mho/m;  $\varepsilon_r$  = 50.6;  $\rho$  = 1000 kg/m<sup>3</sup>

Phantom section: Flat Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(4.14, 4.14, 4.14); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015

- Phantom: SAM 1; Type: SAM; Serial: TP-1360

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172


**d=10mm, Pin=250mW/Area Scan (91x91x1):** Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (interpolated) = 16.2 mW/g

**d=10mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 89.5 V/m; Power Drift = 0.017 dB

Peak SAR (extrapolated) = 27.0 W/kg

SAR(1 g) = 13.6 mW/g; SAR(10 g) = 6.35 mW/g Maximum value of SAR (measured) = 15.4 mW/g

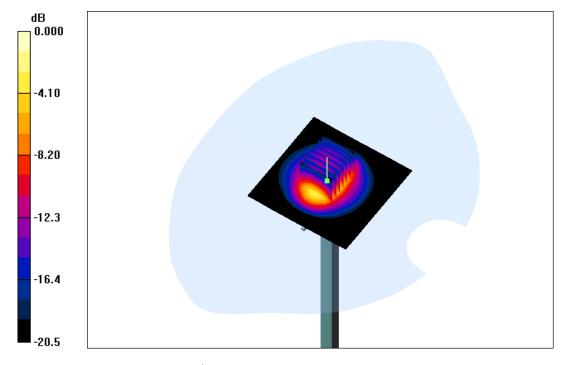

0 dB = 15.4 mW/g



Report NO: TS201510006 Page 44 / 96

#### **Appendix B. SAR Test plots:**

#1

Date: 10/18/2015

DUT: A53; Type: SI PIN; Serial: IMEI Number

Communication System: GSM 850; Frequency: 824.2 MHz; Duty Cycle: 1:8.3

Medium parameters used (interpolated): f = 824.2 MHz;  $\sigma = 0.907 \text{ mho/m}$ ;  $\varepsilon_r = 41.4$ ;  $\rho = 1000$ 

kg/m<sup>3</sup>

Phantom section: Right Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(6.19, 6.19, 6.19); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015


- Phantom: SAM 2; Type: SAM; Serial: TP-1432

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

**Right Cheek/Area Scan (71x111x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.330 mW/g

**Right Cheek/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 5.96 V/m; Power Drift = 0.064 dB Peak SAR (extrapolated) = 0.408 W/kg

SAR(1 g) = 0.309 mW/g; SAR(10 g) = 0.230 mW/gMaximum value of SAR (measured) = 0.326 mW/g

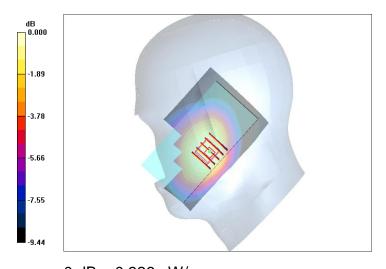

0 dB = 0.326 mW/g



Report NO: TS201510006 Page 45 / 96

#2

Date: 10/18/2015

Test Laboratory: SUNWAY COMMUNICATION CO.,LTD.

DUT: A53; Type: SI PIN; Serial: IMEI Number

Communication System: GSM 1900; Frequency: 1909.8 MHz;Duty Cycle: 1:8.3 Medium parameters used: f = 1910 MHz;  $\sigma$  = 1.42 mho/m;  $\epsilon_r$  = 39.6;  $\rho$  = 1000 kg/m<sup>3</sup>

Phantom section: Left Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(4.68, 4.68, 4.68); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015

- Phantom: SAM 1; Type: SAM; Serial: TP-1360

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

**Left Cheek/Area Scan (71x111x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.204 mW/g

**Left Cheek/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 3.65 V/m; Power Drift = 0.118 dB Peak SAR (extrapolated) = 0.326 W/kg

SAR(1 g) = 0.194 mW/g; SAR(10 g) = 0.114 mW/g Maximum value of SAR (measured) = 0.210 mW/g



0 dB = 0.210 mW/g



Report NO: TS201510006 Page 46 / 96

#### #3

Date: 10/18/2015

Test Laboratory: SUNWAY COMMUNICATION CO.,LTD.

**DUT: A53; Type: SI PIN; Serial: IMEI Number** 

Communication System: W850; Frequency: 836.6 MHz; Duty Cycle: 1:1

Medium parameters used: f = 837 MHz;  $\sigma$  = 0.919 mho/m;  $\epsilon_r$  = 41.3;  $\rho$  = 1000 kg/m<sup>3</sup>

Phantom section: Right Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(6.19, 6.19, 6.19); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015


- Phantom: SAM 2; Type: SAM; Serial: TP-1432

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

**Right Cheek/Area Scan (71x111x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.364 mW/g

**Right Cheek/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 6.40 V/m; Power Drift = -0.150 dB Peak SAR (extrapolated) = 0.441 W/kg

SAR(1 g) = 0.335 mW/g; SAR(10 g) = 0.248 mW/g Maximum value of SAR (measured) = 0.353 mW/g

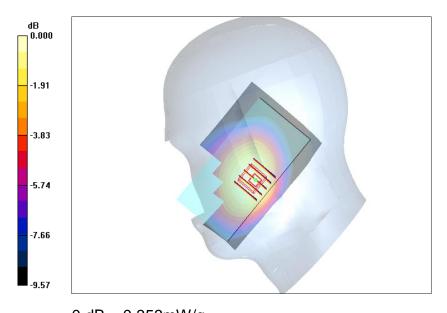

0 dB = 0.353 mW/g



Report NO: TS201510006 Page 47 / 96

#### #4

Date: 10/18/2015

Test Laboratory: SUNWAY COMMUNICATION CO.,LTD.

DUT: A53; Type: SI PIN; Serial: IMEI Number

Communication System: W1900; Frequency: 1852.4 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated): f = 1852.4 MHz;  $\sigma = 1.36$  mho/m;  $\varepsilon_r = 39.8$ ;  $\rho = 1000$ 

kg/m<sup>3</sup>

Phantom section: Left Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(4.68, 4.68, 4.68); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015


- Phantom: SAM 1; Type: SAM; Serial: TP-1360

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

**Left Cheek/Area Scan (71x111x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.388 mW/g

**Left Cheek/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 6.15 V/m; Power Drift = 0.192 dB Peak SAR (extrapolated) = 0.572 W/kg

SAR(1 g) = 0.356 mW/g; SAR(10 g) = 0.214 mW/g Maximum value of SAR (measured) = 0.390 mW/g

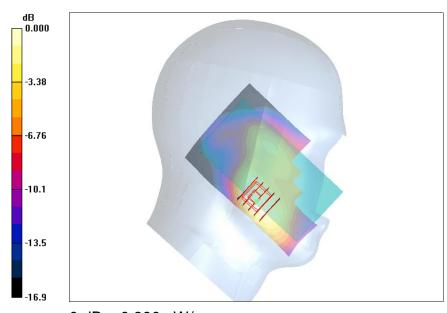

0 dB = 0.390 mW/g



Report NO: TS201510006 Page 48 / 96

#### #5

Date: 10/18/2015

Test Laboratory: SUNWAY COMMUNICATION CO.,LTD.

**DUT: A53; Type: SI PIN; Serial: IMEI Number** 

Communication System: 802.11; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2462 MHz;  $\sigma = 1.82 \text{ mho/m}$ ;  $\epsilon_r = 37.5$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Right Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(4.21, 4.21, 4.21); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015


- Phantom: SAM 1; Type: SAM; Serial: TP-1360

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

**Right Cheek/Area Scan (71x111x1):** Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (interpolated) = 0.081 mW/g

**Right Cheek/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 4.03 V/m; Power Drift = -0.052 dB Peak SAR (extrapolated) = 0.173 W/kg

SAR(1 g) = 0.0781 mW/g; SAR(10 g) = 0.041 mW/g Maximum value of SAR (measured) = 0.085 mW/g

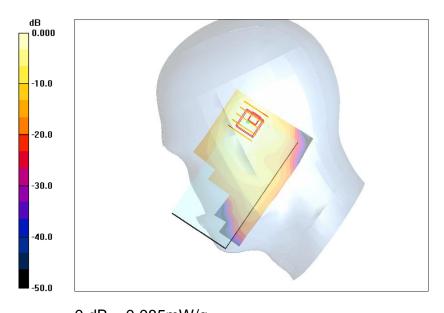

0 dB = 0.085 mW/g



Report NO: TS201510006 Page 49 / 96

#### #6

Date: 10/19/2015

Test Laboratory: SUNWAY COMMUNICATION CO.,LTD.

**DUT: A53; Type: SI PIN; Serial: IMEI Number** 

Communication System: GPRS850; Frequency: 824.2 MHz; Duty Cycle: 1:2

Medium parameters used (interpolated): f = 824.2 MHz;  $\sigma = 0.96 \text{ mho/m}$ ;  $\varepsilon_r = 56.6$ ;  $\rho = 1000$ 

kg/m<sup>3</sup>

Phantom section: Flat Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(6.02, 6.02, 6.02); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015

- Phantom: SAM 2; Type: SAM; Serial: TP-1432


- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

**Back/Area Scan (71x111x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.92 mW/g

**Back/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 25.7 V/m; Power Drift = -0.006 dB

Peak SAR (extrapolated) = 1.10 W/kg

SAR(1 g) = 0.712 mW/g; SAR(10 g) = 0.584 mW/gMaximum value of SAR (measured) = 0.91 mW/g

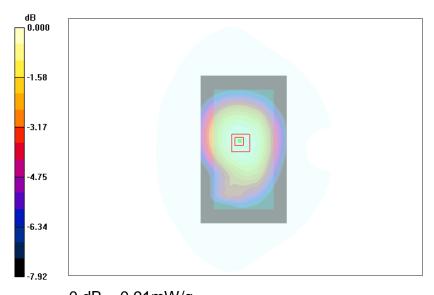

0 dB = 0.91 mW/g



Report NO: TS201510006 Page 50 / 96

#### #7

Date: 10/20/2015

Test Laboratory: SUNWAY COMMUNICATION CO.,LTD.

**DUT: A53; Type: SI PIN; Serial: IMEI Number** 

Communication System: GPRS1900; Frequency: 1909.8 MHz;Duty Cycle: 1:2 Medium parameters used: f = 1910 MHz;  $\sigma = 1.55$  mho/m;  $\epsilon_r = 52.7$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(4.48, 4.48, 4.48); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015


- Phantom: SAM 1; Type: SAM; Serial: TP-1360

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

**Back/Area Scan (71x111x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.565 mW/g

**Back/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 10.8 V/m; Power Drift = -0.099 dB Peak SAR (extrapolated) = 0.904 W/kg

SAR(1 g) = 0.511 mW/g; SAR(10 g) = 0.290 mW/g Maximum value of SAR (measured) = 0.573 mW/g

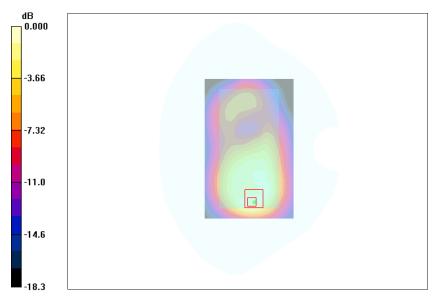

0 dB = 0.573 mW/g



Report NO: TS201510006 Page 51 / 96

#### #8

Date: 10/19/2015

Test Laboratory: SUNWAY COMMUNICATION CO.,LTD.

**DUT: A53; Type: SI PIN; Serial: IMEI Number** 

Communication System: W850; Frequency: 836.6 MHz; Duty Cycle: 1:1

Medium parameters used: f = 837 MHz;  $\sigma$  = 0.972 mho/m;  $\epsilon_r$  = 56.5;  $\rho$  = 1000 kg/m<sup>3</sup>

Phantom section: Flat Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(6.02, 6.02, 6.02); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015


- Phantom: SAM 2; Type: SAM; Serial: TP-1432

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

**Back/Area Scan (71x111x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.579 mW/g

**Back/Zoom Scan (5x5x7)/Cube 0:** Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 23.6 V/m; Power Drift = -0.020 dB Peak SAR (extrapolated) = 0.811 W/kg

SAR(1 g) = 0.519 mW/g; SAR(10 g) = 0.361 mW/g Maximum value of SAR (measured) = 0.562 mW/g

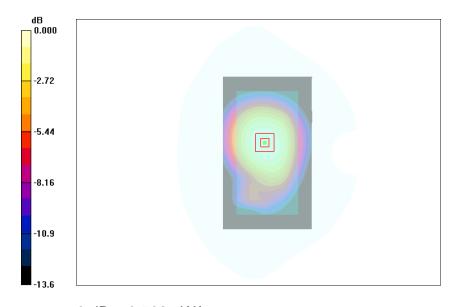

0 dB = 0.562 mW/g



Report NO: TS201510006 Page 52 / 96

#### #9

Date: 10/20/2015

Test Laboratory: SUNWAY COMMUNICATION CO.,LTD.

**DUT: A53; Type: SI PIN; Serial: IMEI Number** 

Communication System: W1900; Frequency: 1852.4 MHz; Duty Cycle: 1:1

Medium parameters used (interpolated): f = 1852.4 MHz;  $\sigma = 1.48$  mho/m;  $\varepsilon_r = 52.9$ ;  $\rho = 1000$ 

kg/m<sup>3</sup>

Phantom section: Flat Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(4.48, 4.48, 4.48); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015

- Phantom: SAM 1; Type: SAM; Serial: TP-1360

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

**Back/Area Scan (71x111x1):** Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.690 mW/g


Back/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 12.5 V/m; Power Drift = -0.094 dB

Peak SAR (extrapolated) = 1.02 W/kg

SAR(1 g) = 0.599 mW/g; SAR(10 g) = 0.352 mW/g

Maximum value of SAR (measured) = 0.663 mW/g

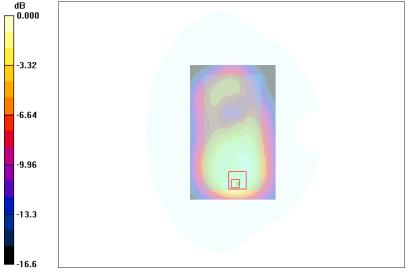

0 dB = 0.663 mW/g



Report NO: TS201510006 Page 53 / 96

#### #10

Date: 10/20/2015

Test Laboratory: SUNWAY COMMUNICATION CO.,LTD.

DUT: A53; Type: SI PIN; Serial: IMEI Number

Communication System: 802.11; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2462 MHz;  $\sigma = 1.98 \text{ mho/m}$ ;  $\epsilon_r = 53.8$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

#### DASY4 Configuration:

- Probe: ES3DV3 - SN3028; ConvF(4.14, 4.14, 4.14); Calibrated: 10/22/2014

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE4 Sn905; Calibrated: 7/16/2015


- Phantom: SAM 1; Type: SAM; Serial: TP-1360

- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

**Back/Area Scan (71x111x1):** Measurement grid: dx=12mm, dy=12mm Maximum value of SAR (interpolated) = 0.077 mW/g

**Back/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 3.78 V/m; Power Drift = 0.114 dB Peak SAR (extrapolated) = 0.150 W/kg

**SAR(1 g) = 0.0673 mW/g; SAR(10 g) = 0.034 mW/g**Maximum value of SAR (measured) = 0.073 mW/g

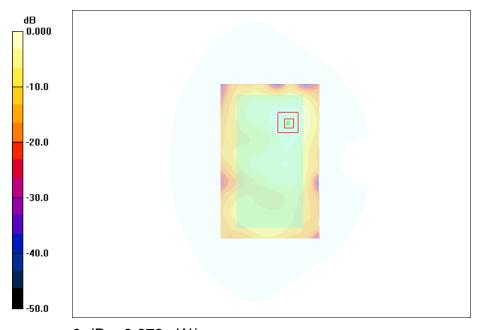

0 dB = 0.073 mW/g



Report NO: TS201510006 Page 54 / 96

#### **Appendix C. Probe Calibration Data:**



Add: No.51 Xneyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com Hitp://www.chinattl.com

CALIBRATION No. L0570

AUDEN Certificate No: Z14-97115

#### CALIBRATION CERTIFICATE

Object ES3DV3 - SN:3028

Calibration Procedure(s) TMC-OS-E-02-195

Calibration Procedures for Dosimetric E-field Probes

Calibration date: October 22, 2014

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)% and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration	
Power Meter NRP2	101919	01-Jul-14 (CTTL, No.J14X02146)	Jun-15	
Power sensor NRP-Z91	101547	01-Jul-14 (CTTL, No.J14X02146)	Jun-15	
Power sensor NRP-Z91	101548	01-Jul-14 (CTTL, No.J14X02146)	Jun-15	
Reference10dBAttenuator	BT0520	12-Dec-12(TMC,No.JZ12-867)	Dec-14	
Reference20dBAttenuator BT0267		12-Dec-12(TMC,No.JZ12-866)	Dec-14	
Reference Probe EX3DV4 SN 3617		28-Aug-14(SPEAG,No.EX3-3617_Aug14)	Aug-15	
DAE4 SN 1331		23-Jan-14 (SPEAG, DAE4-1331_Jan14)	Jan -15	
Secondary Standards ID#		Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration	
SignalGeneratorMG3700A	6201052605	01-Jul-14 (CTTL, No.J14X02145)	Jun-15	
Network Analyzer E5071C	MY46110673	15-Feb-14 (TMC, No.JZ14-781)	Feb-15	
	Name	Function	Signature	
Calibrated by:	Yu Zongying	SAR Test Engineer		
Reviewed by: Qi Dianyuan		SAR Project Leader		
Approved by:	Lu Bingsong	Deputy Director of the laboratory		
Issued: October 23, 2014				

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z14-97115 Page 1 of 11



Report NO: TS201510006 Page 55 / 96



Add: No.51 Xneyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com Http://www.chinattl.com

Glossarv:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty\_cycle) of the RF signal A,B,C,D modulation dependent linearization parameters

Polarization Φ Φ rotation around probe axis

Polarization θ θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.

θ=0 is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization θ=0 (f≤900MHz in TEM-cell; f>1800MHz: waveguide).
   NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z\* frequency\_response (see Frequency Response Chart). This
  linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the
  frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- Ax,y,z; Bx,y,z; Cx,y,z; VRx,y,z:A,B,C are numerical linearization parameters assessed based on the
  data of power sweep for specific modulation signal. The parameters do not depend on frequency nor
  media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f≤800MHz) and inside waveguide using analytical field distributions based on power measurements for f >800MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z\* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from±50MHz to±100MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the
  probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Page 2 of 11

Certificate No: Z14-97115

# 7

### SHENZHEN SUNWAY COMMUNICATION CO.,LTD

Report NO: TS201510006 Page 56 / 96



Add: No.51 Xneyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com Http://www.chinattl.com

## Probe ES3DV3

SN: 3028

Calibrated: October 22, 2014

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: Z14-97115

Page 3 of 11



Report NO: TS201510006 Page 57 / 96



Add: No.51 Xneyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com Http://www.chinattl.com

DASY - Parameters of Probe: ES3DV3 - SN: 3028

#### **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm(μV/(V/m) <sup>2</sup> ) <sup>A</sup>	1.16	1.27	1.21	±10.8%
DCP(mV) <sup>8</sup>	105.8	103.2	103.8	

#### Modulation Calibration Parameters

UID	Communication		Α	В	С	D	VR	Unc E
	System Name		dB	dB√μV		dB	mV	(k=2)
0	CW	Х	0.0	0.0	1.0	0.00	282.9	±2.2%
		Υ	0.0	0.0	1.0		292.0	
		Z	0.0	0.0	1.0		290.3	

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z14-97115

<sup>&</sup>lt;sup>A</sup> The uncertainties of Norm X, Y, Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 5 and Page 6).

<sup>&</sup>lt;sup>B</sup> Numerical linearization parameter: uncertainty not required.

Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



Report NO: TS201510006 Page 58 / 96



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com Http://www.chinattl.cn

DASY - Parameters of Probe: ES3DV3 - SN: 3028

#### Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz] <sup>©</sup>	Relative Permittivity F	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
750	41.9	0.89	6.36	6.36	6.36	0.37	1.44	±12%
835	41.5	0.90	6.19	6.19	6.19	0.39	1.42	±12%
1750	40.1	1.37	4.97	4.97	4.97	0.55	1.34	±12%
1900	40.0	1.40	4.68	4.68	4.68	0.70	1.23	±12%
2300	39.5	1.67	4.52	4.52	4.52	0.80	1.17	±12%
2450	39.2	1.80	4.21	4.21	4.21	0.98	1.04	±12%
2600	39.0	1.96	4.06	4.06	4.06	0.86	1.11	±12%

<sup>&</sup>lt;sup>c</sup> Frequency validity of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. 
<sup>F</sup> At frequency below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.
<sup>a</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-8 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: Z14-97115



Report NO: TS201510006 Page 59 / 96



Add: No.51 Xneyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ctil@chinatd.com Http://www.chinatd.cn

DASY - Parameters of Probe: ES3DV3 - SN: 3028

#### Calibration Parameter Determined in Body Tissue Simulating Media

f [MHz] <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (\$/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
750	55.5	0.96	6.02	6.02	6.02	0.33	1.68	±12%
835	55.2	0.97	6.02	6.02	6.02	0.34	1.79	±12%
1750	53.4	1.49	4.69	4.69	4.69	0.63	1.30	±12%
1900	53.3	1.52	4.48	4.48	4.48	0.60	1.34	±12%
2300	52.9	1.81	4.37	4.37	4.37	0.74	1.25	±12%
2450	52.7	1.95	4.14	4.14	4.14	0.68	1.35	±12%
2600	52.5	2.16	4.02	4.02	4.02	0.84	1.16	±12%

 $<sup>^{\</sup>circ}$  Frequency validity of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.  $^{\#}$  At frequency below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Certificate No: Z14-97115

Page 6 of 11

 $<sup>^{\</sup>circ}$  Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than  $\pm$  1% for frequencies below 3 GHz and below  $\pm$  2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.




Report NO: TS201510006 Page 60 / 96



Add: No.51 Xneyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ctt@chinatd.com Http://www.chinatd.com

## Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

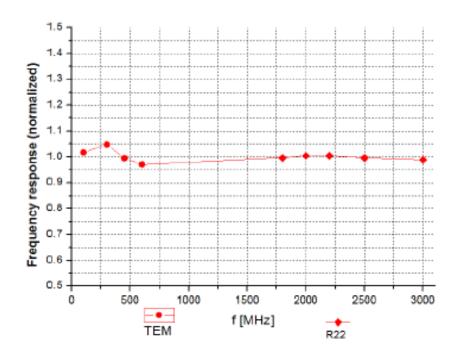


Uncertainty of Frequency Response of E-field: ±7.5% (k=2)

Certificate No: Z14-97115 Page 7 of 11



Report NO: TS201510006 Page 61 / 96

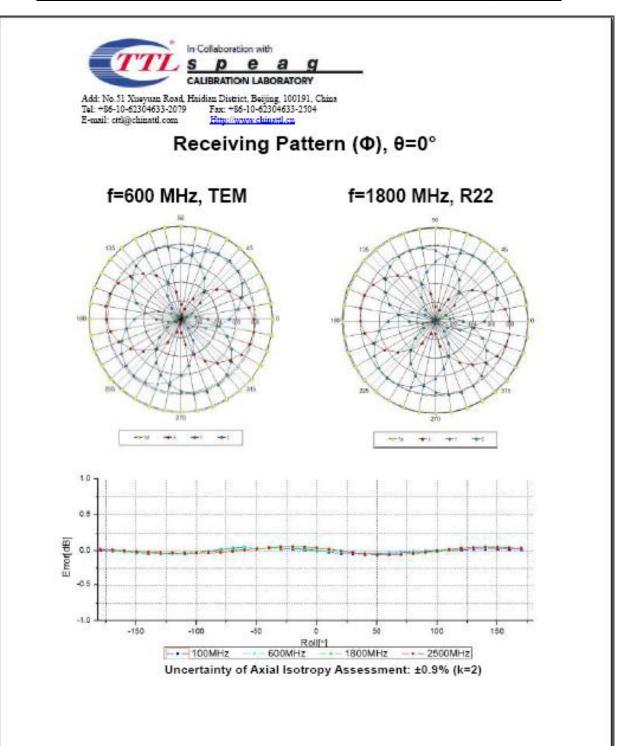


Certificate No: Z14-97115

Page 8 of 11




Report NO: TS201510006 Page 62 / 96

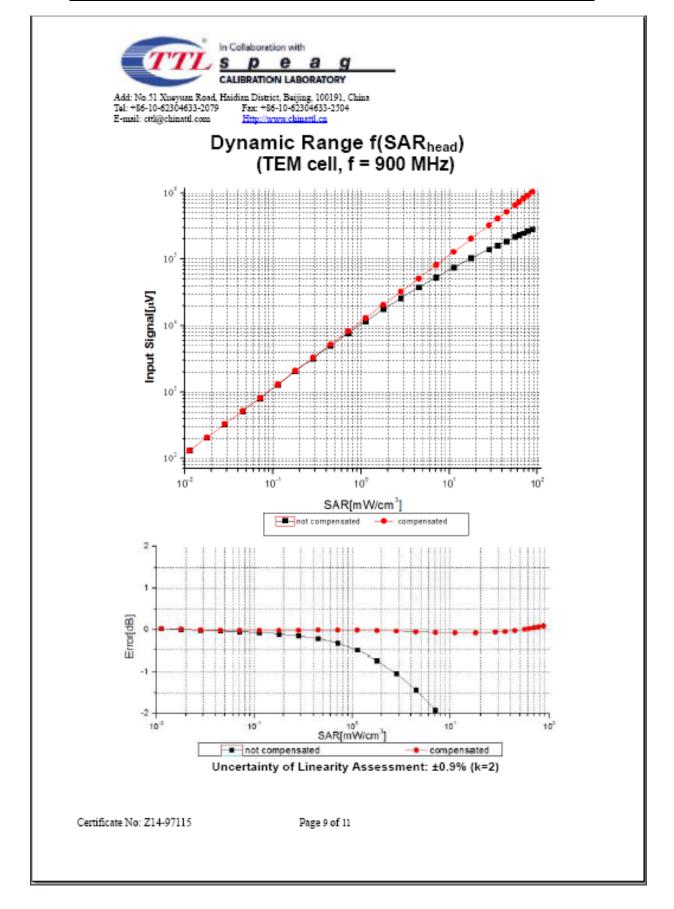



Report NO: TS201510006 Page 63 / 96




Add: No.51 Xneyuan Road, Haidian District, Beijing, 100191, China Tal: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ctt@chinattl.com Http://www.chinattl.cn


#### **Conversion Factor Assessment**

#### f=835 MHz, WGLS R9(H\_convF)

#### f=1750 MHz, WGLS R22(H\_convF)

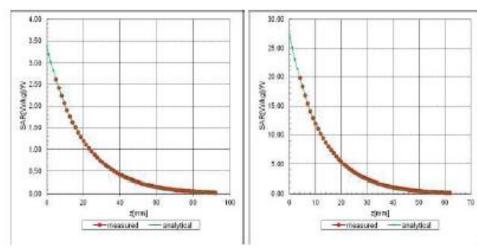

### Deviation from Isotropy in Liquid

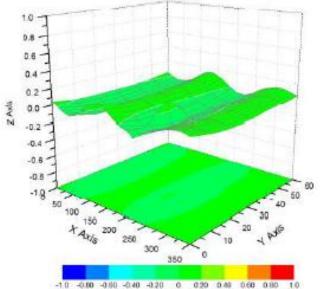

Uncertainty of Spherical Isotropy Assessment: ±2.8% (K=2)

Certificate No: Z14-97115

Page 10 of 11



Report NO: TS201510006 Page 64 / 96



Add: No.51 Xneyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ctt@chinatd.com Http://www.chinatd.com

### DASY - Parameters of Probe: ES3DV3 - SN: 3208

### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	54.8
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	10mm
Tip Diameter	4mm
Probe Tip to Sensor X Calibration Point	2mm
Probe Tip to Sensor Y Calibration Point	2mm
Probe Tip to Sensor Z Calibration Point	2mm
Recommended Measurement Distance from Surface	3mm

Certificate No: Z14-97115 Page 11 of 11



Report NO: TS201510006 Page 65 / 96



#### Acceptable Conditions for SAR Measurements Using Probes and Dipoles Calibrated under the SPEAG-TMC Dual-Logo Calibration Program to Support FCC Equipment Certification

The acceptable conditions for SAR measurements using probes, dipoles and DAEs calibrated by TMC (*Telecommunication Metrology Center of MITT in Beijing, China*), under thé Dual-Logo Calibration Certificate program and quality assurance (QA) protocols established between SPEAG (*Schmid & Partner Engineering AG, Switzerland*) and TMC, to support FCC (*U.S. Federal Communications Commission*) equipment certification are defined and described in the following.

- The agreement established between SPEAG and TMC is only applicable to calibration services performed by TMC where its clients (companies and divisions of such companies) are headquartered in the Greater China Region, including Taiwan and Hong Kong. This agreement is subject to renewal at the end of each calendar year between SPEAG and TMC. TMC shall inform the FCC of any changes or early termination to the agreement.
- 2) Only a subset of the calibration services specified in the SPEAG-TMC agreement, while it remains valid, are applicable to SAR measurements performed using such equipment for supporting FCC equipment certification. These are identified in the following.
  - a) Calibration of dosimetric (SAR) probes EX3DVx, ET3DVx and ES3DVx.
    - i) Free-space E-field and H-field probes, including those used for HAC (hearing aid compatibility) evaluation, temperature probes, other probes or equipment not identified in this document, when calibrated by TMC, are excluded and cannot be used for measurements to support FCC equipment certification.
    - ii) Signal specific and bundled probe calibrations based on PMR (probe modulation response) characteristics are handled according to the requirements of KDB 865664; that is, "Until standardized procedures are available to make such determination, the applicability of a signal specific probe calibration for testing specific wireless modes and technologies is determined on a case-by-case basis through KDB inquiries, including SAR system verification requirements."
  - b) Calibration of SAR system validation dipoles, excluding HAC dipoles.
  - c) Calibration of data acquisition electronics DAE3Vx, DAE4Vx and DAEasyVx.
  - d) For FCC equipment certification purposes, the frequency range of SAR probe and dipole calibrations is limited to 700 MHz - 6 GHz and provided it is supported by the equipment identified in the TMC QA protocol (a separate attachment to this document).
  - e) The identical system and equipment setup, measurement configurations, hardware, evaluation algorithms, calibration and QA protocols, including the format of calibration certificates and reports used by SPEAG shall be applied by TMC.
  - f) The calibrated items are only applicable to SPEAG DASY 4 and DASY 5 or higher version systems.



Report NO: TS201510006 Page 66 / 96

#### Appendix D. DAE Calibration Data:



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2218 Fax: +86-10-62304633-2209 E-mail: ettl@chinattl.com Http://www.chinattl.cn

Certificate No: Z15-97093 Auden Client :

#### **CALIBRATION CERTIFICATE** Object DAE4 - SN: 905 Calibration Procedure(s) FD-Z11-2-002-01 Calibration Procedure for the Data Acquisition Electronics Calibration date: July 16, 2015 This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%. Calibration Equipment used (M&TE critical for calibration) Scheduled Calibration Primary Standards ID# Cal Date(Calibrated by, Certificate No.) 06-July-15 (CTTL, No:J15X04257) July-16 Process Calibrator 753 1971018 Function Name Calibrated by: Yu Zongying SAR Test Engineer Reviewed by: SAR Project Leader Qi Dianyuan Approved by: Deputy Director of the laboratory Lu Bingsong Issued: July 17, 2015 This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: Z15-97093

Page 1 of 3



Report NO: TS201510006 Page 67 / 96



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2218 Fax: +86-10-62304633-2209 E-mail: ettl@chinattl.com Http://www.chinattl.cn

Glossary:

DAE data acquisition electronics

Connector angle information used in DASY system to align probe sensor X

to the robot coordinate system.

#### Methods Applied and Interpretation of Parameters:

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.

Certificate No: Z15-97093

Page 2 of 3



Report NO: TS201510006 Page 68 / 96



DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 µV, full range = -100...+300 mV

Low Range: 1LSB = 61 nV, full range = -1......+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	x	Y	Z
High Range	404.672 ± 0.15% (k=2)	405.235 ± 0.15% (k=2)	404.825 ± 0.15% (k=2)
Low Range	3.98116 ± 0.7% (k=2)	4.00286 ± 0.7% (k=2)	3.99735 ± 0.7% (k=2)

#### Connector Angle


Connector Angle to be used in DASY system	269° ± 1 °

Certificate No: Z15-97093 Page 3 of 3



Report NO: TS201510006 Page 69 / 96

#### Appendix E. Dipole Calibration Data:

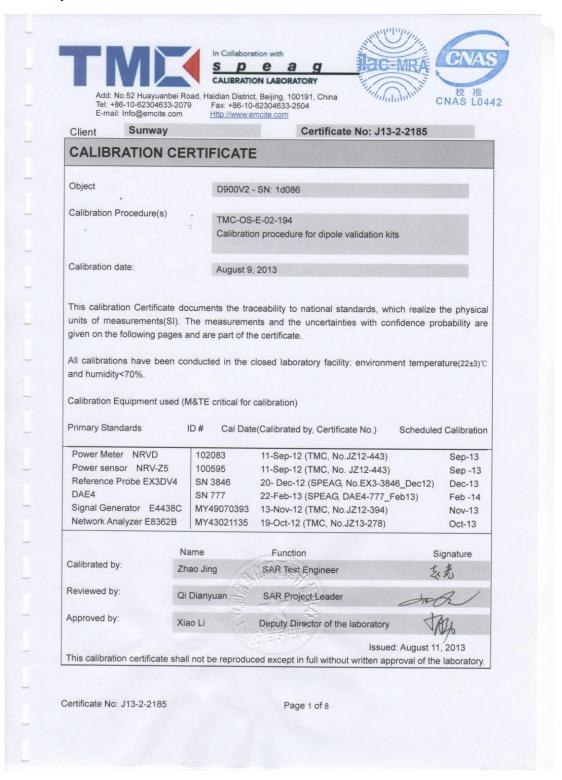



Report NO: TS201510006 Page 70 / 96



p e

E-mail: Info@emcite.com

Add: No 52 Huayuanbei Road, Haidian District, Beijing, 100191, China Fax: +86-10-62304633-2504 Http://www.emcite.com

Glossary:

TSL ConvF N/A

tissue simulating liquid sensitivity in TSL / NORMx,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005

c) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: J13-2-2185

Page 2 of 8



Report NO: TS201510006 Page 71 / 96



DASY Version	DASY52	52.8.7.1137
Extrapolation	Advanced Extrapolation	
Phantom	Twin Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.6 ± 6 %	0.98 mho/m ± 6 %
Head TSL temperature change during test	<0.5 °C		

SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.67 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	10.7 mW /g ± 20.8 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.72 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	6.87 mW /g ± 20.4 % (k=2)

**Body TSL parameters** 

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.0	1.05 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.2 ± 6 %	1.02 mho/m ± 6 %
Body TSL temperature change during test	<0.5 °C		

SAR result with Body TSL


SAR averaged over 1 $\ cm^3$ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.63 mW / g 10.7mW /g ± 20.8 % (k=2)
SAR for nominal Body TSL parameters	normalized to 1W	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.71 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	6.94 mW /g ± 20.4 % (k=2

Certificate No: J13-2-2185

Page 3 of 8




<u>Report NO: TS201510006</u> <u>Page 72</u> / 96

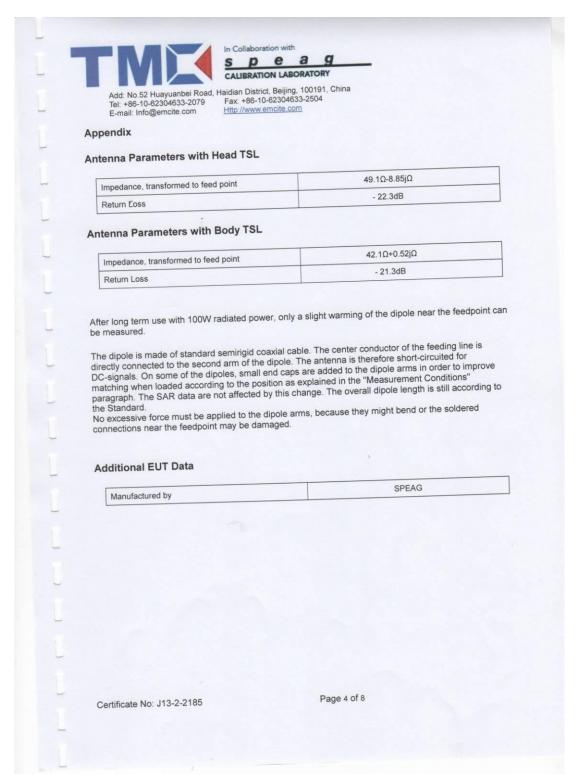




Report NO: TS201510006 Page 73 / 96

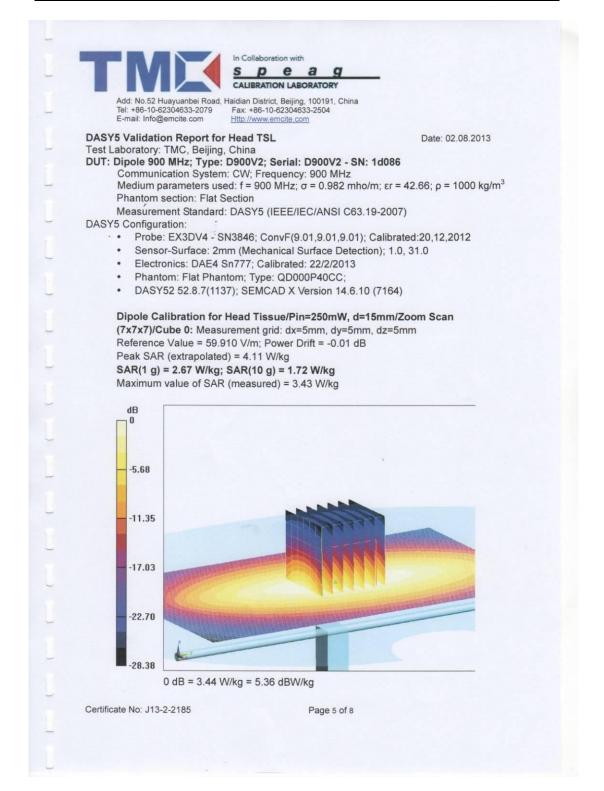




Report NO: TS201510006 Page 74 / 96

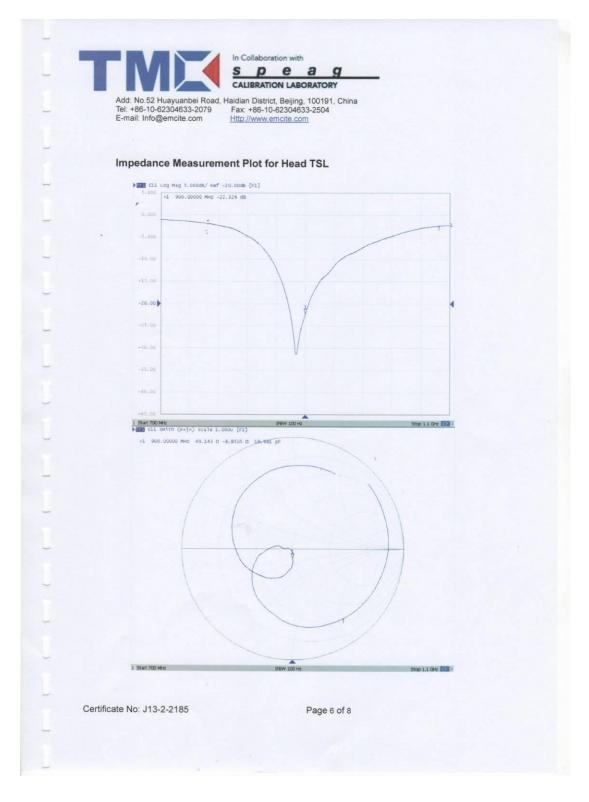




Report NO: TS201510006 Page 75 / 96

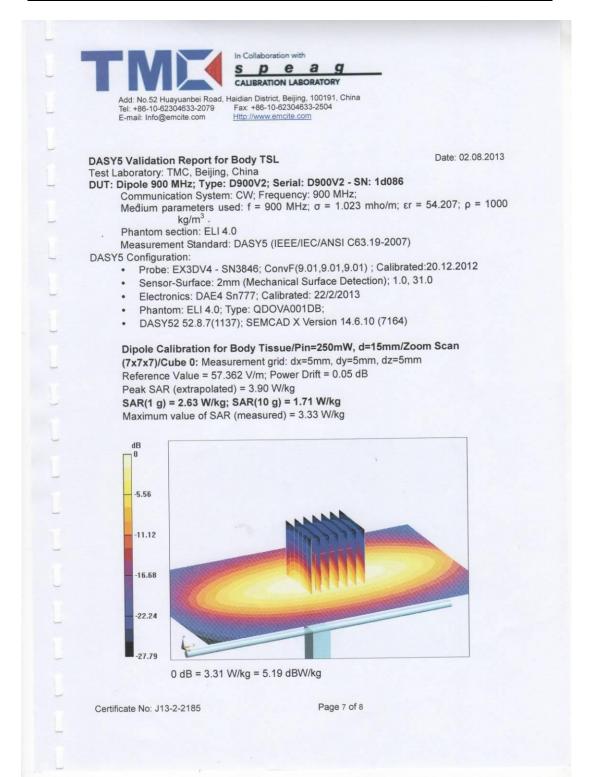



Report NO: TS201510006 Page 76 / 96

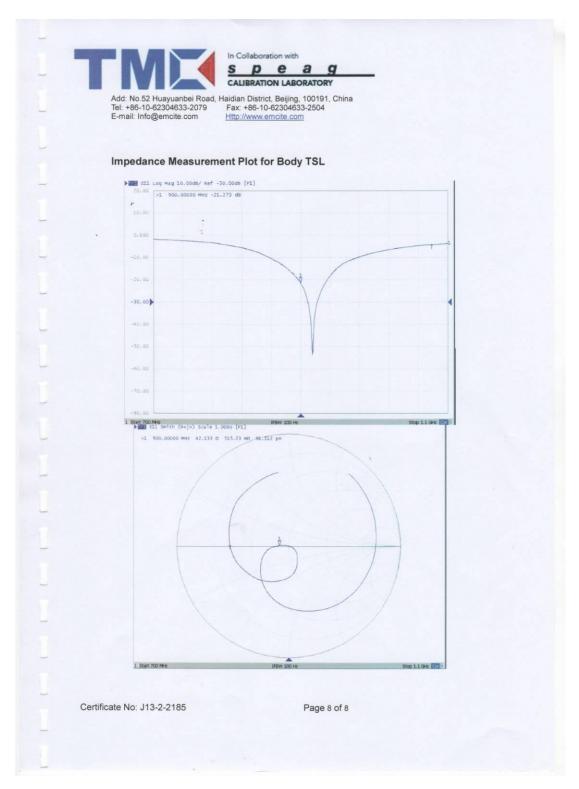



Report NO: TS201510006 Page 77 / 96




Acceptable Conditions for SAR Measurements Using Probes and Dipoles Calibrated under the SPEAG-TMC Dual-Logo Calibration Program to Support FCC Equipment Certification

The acceptable conditions for SAR measurements using probes, dipoles and DAEs calibrated by TMC (Telecommunication Metrology Center of MITT in Beijing, China), under the Dual-Logo Calibration Certificate program and quality assurance (QA) protocols established between SPEAG (Schmid & Partner Engineering AG, Switzerland) and TMC, to support FCC (U.S. Federal Communications Commission) equipment certification are defined and described in the following.

- The agreement established between SPEAG and TMC is only applicable to
  calibration services performed by TMC where its clients (companies and divisions of
  such companies) are headquartered in the Greater China Region, including Taiwan
  and Hong Kong. This agreement is subject to renewal at the end of each calendar
  year between SPEAG and TMC. TMC shall inform the FCC of any changes or early
  termination to the agreement.
- 2) Only a subset of the calibration services specified in the SPEAG-TMC agreement, while it remains valid, are applicable to SAR measurements performed using such equipment for supporting FCC equipment certification. These are identified in the following.
  - a) Calibration of dosimetric (SAR) probes EX3DVx, ET3DVx and ES3DVx.
    - Free-space E-field and H-field probes, including those used for HAC (hearing aid compatibility) evaluation, temperature probes, other probes or equipment not identified in this document, when calibrated by TMC, are excluded and cannot be used for measurements to support FCC equipment certification.
    - ii) Signal specific and bundled probe calibrations based on PMR (probe modulation response) characteristics are handled according to the requirements of KDB 865664; that is, "Until standardized procedures are available to make such determination, the applicability of a signal specific probe calibration for testing specific wireless modes and technologies is determined on a case-by-case basis through KDB inquiries, including SAR system verification requirements."
  - b) Calibration of SAR system validation dipoles, excluding HAC dipoles.
  - c) Calibration of data acquisition electronics DAE3Vx, DAE4Vx and DAEasyVx.
  - d) For FCC equipment certification purposes, the frequency range of SAR probe and dipole calibrations is limited to 700 MHz - 6 GHz and provided it is supported by the equipment identified in the TMC QA protocol (a separate attachment to this document).
  - The identical system and equipment setup, measurement configurations, hardware, evaluation algorithms, calibration and QA protocols, including the format of calibration certificates and reports used by SPEAG shall be applied by TMC.
  - f) The calibrated items are only applicable to SPEAG DASY 4 and DASY 5 or higher version systems.



Report NO: TS201510006 Page 78 / 96

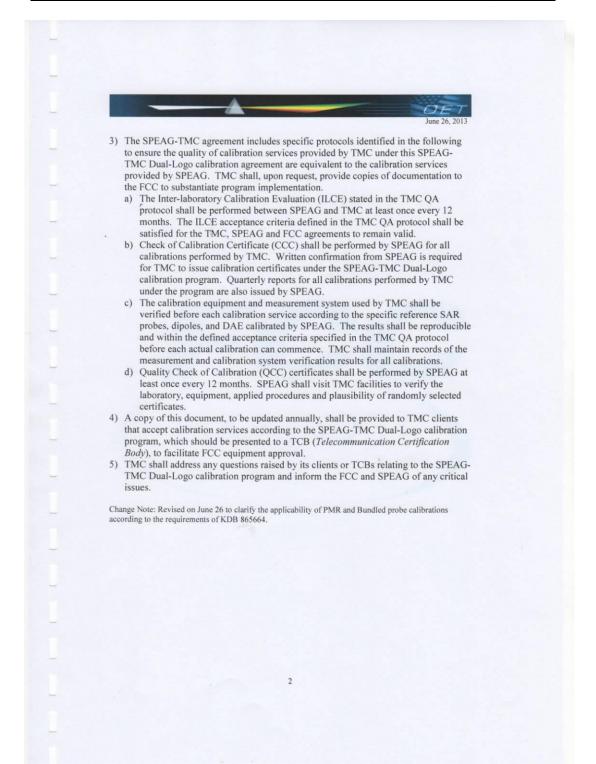



Report NO: TS201510006 Page 79 / 96

#### D900V2, serial no. 1d086 Extended Dipole Calibrations


Referring to KDB 865664D01V01r03, if dipoles are verified in return loss (<-20dB, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

			D900V2, se	rial no. 1	d086			
	900 Head			900 Body				
Date of Measurement	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)	Return-Loss (dB)	Delta (%)	Real Impedance (ohm)	Delta (ohm)
2013-8-9	-22.3		49.2		-21.3		42.1	
2014-8-8	-22.21	0.41	49.12	-0.08	-21.1	0.94	42.25	-0.15
2015-8-4	-22.1	0.9	48.4	-0.8	-21.4	-0.5	43.1	1.0


The return loss is < -20dB, within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

<Dipole Verification Data>- D900V2, serial no. 1d086





900MHz Body





Report NO: TS201510006 Page 80 / 96

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.  All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.  Calibration Equipment used (M&TE critical for calibration)  Primary Standards    D #   Calibration (Calibration)   Scheduled Calibration    Primary Standards   ID #   Calibration (Calibration)   Oct-15    Power meter EPM-442A   GB37480704   07-Oct-14 (No. 217-02020)   Oct-15    Power sensor HP 8481A   US37292783   07-Oct-14 (No. 217-02020)   Oct-15    Power sensor HP 8481A   MY41092317   07-Oct-14 (No. 217-02021)   Oct-15    Reference 20 dB Attenuator   SN: 5058 (20k)   03-Apr-14 (No. 217-01921)   Apr-15    Type-N mismatch combination   SN: 5047.2 / 06327   00-Apr-14 (No. 217-01921)   Apr-15    Reference Probe ES30V3   SN: 3205   30-Dec-14 (No. ES3-3205_Dec14)   Dec-15    SN: 601   18-Aug-14 (No. DAE4-601_Aug14)   Aug-15    Secondary Standards   ID #   Check Date (in house)   Scheduled Check    RF generator R&S SMT-06   100005   04-Aug-99 (in house check Oct-13)   In house check: Oct-16    Name   Function   Signature    Calibrated by: Cloudio Leubler   Laboratory Technician   Signature    Calibrated by: Calibrated   Signature   Signature    Calibrated   Signature   Si	OALIBITATION C	CERTIFICATE		
Calibration procedure for dipole validation kits above 700 MHz  January 07, 2015  This calibration cartificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.  All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.  Calibration Equipment used (M&TE critical for calibration)  Primary Standards    D #	Object	D1900V2 - SN: 5	id194	
Calibration procedure for dipole validation kits above 700 MHz  January 07, 2015  This calibration cartificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.  All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.  Calibration Equipment used (M&TE critical for calibration)  Primary Standards    D #				
Calibration date:  January 07, 2015  This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (St). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.  All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.  Calibration Equipment used (M&TE critical for calibration)  Primary Standards    D #   Cal Date (Certificate No.)   Scheduled Calibration    Power meter EPM-442A   CB37480704   07-0ct-14 (No. 217-02020)   Oct-15    Power sensor HP 8481A   US37292783   07-0ct-14 (No. 217-0200)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-02021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-02021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-02021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (No. 217-03021)   Oct-15    Power sensor HP 8481A   MY41082317   07-0ct-14 (N	Calibration procedure(s)	QA CAL-05.v9		
This calibration certificate documents the braceability to national standards, which realize the physical units of measurements (Si). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.  All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.  Calibration Equipment used (M&TE critical for calibration)  Primary Standards  ID # Cali Date (Certificate No.) Scheduled Calibration  Power meter EPM-442A GB37480704 07-Oct-14 (No. 217-02020) Oct-15  Power sensor HP 8481A US37292783 07-Oct-14 (No. 217-02020) Oct-15  Power sensor HP 8481A MY41092317 07-Oct-14 (No. 217-02021) Oct-15  Reference 20 dB Attenuator SN: 5058 (20k) 03-Apr-14 (No. 217-0918) Apr-15  Type-N mismatch combination SN: 5047.2 / 06327 03-Apr-14 (No. 217-01921) Apr-15  Reference Probe ES30V3 SN: 3205 30-Dec-14 (No. ES3-3205, Dec-14) Dec-15  Becondary Standards  ID # Check Date (in house) Scheduled Check  RF generator R&S SMT-06 100005 04-Aug-99 (in house check Oct-13) In house check: Oct-16  Network Analyzer HP 8753E US37390685 S4206 18-Oct-01 (in house check Oct-14) In house check: Oct-15  Name Function Signature  Calibrated by:		Calibration proce	edure for dipole validation kits abo	ove 700 MHz
This calibration certificate documents the braceability to national standards, which realize the physical units of measurements (Si). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.  All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.  Calibration Equipment used (M&TE critical for calibration)  Primary Standards  ID # Calibration (Calibration)  Primary Standards  ID # Calibration (Calibration)  Power meter EPM-442A GB37480704 07-Oct-14 (No. 217-02020) Oct-15  Power sensor HP 8481A US37292783 07-Oct-14 (No. 217-02020) Oct-15  Power sensor HP 8481A MY41092317 07-Oct-14 (No. 217-02021) Oct-15  Power sensor HP 8481A MY41092317 07-Oct-14 (No. 217-02021) Oct-15  Reference 20 dB Attenuator SN: 5088 (20k) 03-Apr-14 (No. 217-01918) Apr-15  Type-N mismatch combination SN: 5047.2 / 06327 03-Apr-14 (No. 217-01921) Apr-15  Reference Probe ES30V3 SN: 3205 30-Dec-14 (No. ES3-3205, Dec-14) Dec-15  Belerence Probe ES30V3 SN: 3205 30-Dec-14 (No. DAE4-601_Aug14) Aug-15  Secondary Standards  ID # Check Date (in house) Scheduled Check  RF generator R&S SMT-06 100005 04-Aug-99 (in house check Oct-13) In house check: Oct-16  Name Function Signature  Calibrated by: Claudio Leubler Laboratory Technician	Calibration date:	January 07, 2015	5	
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.  All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.  Calibration Equipment used (M&TE critical for calibration)  Primary Standards  ID # Calibration (Calibration)  Primary Standards  ID # Calibration (Calibration)  Scheduled Calibration  Power meter EPM-442A  GB37480704  07-Oct-14 (No. 217-02020)  Oct-15  Power sensor HP 8481A  MY41092317  07-Oct-14 (No. 217-02020)  Oct-15  Reference 20 dB Attorustor  SN: 5058 (20k)  03-Apr-14 (No. 217-02021)  Oct-15  Type-N mismatch combination  SN: 5047.2 / 06327  03-Apr-14 (No. 217-01921)  Apr-15  Reference Probe ES3OV3  SN: 3205  30-Dec-14 (No. ES3-3205_Dec14)  Dec-15  Aug-15  Secondary Standards  ID # Check Date (in house)  Scheduled Check  RF generator R&S SMT-06  Network Analyzer HP 8753E  Name  Function  Signature  Calibrated by:  Calibrated by:				
All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.  Calibration Equipment used (M&TE critical for calibration)  Primary Standards   ID #   Calibratic No.)   Scheduled Calibration    Power meter EPM-442A   GB37480704   07-Oct-14 (No. 217-02020)   Oct-15    Power sensor HP 8481A   US37292783   07-Oct-14 (No. 217-02020)   Oct-15    Power sensor HP 8481A   MY41092317   07-Oct-14 (No. 217-02021)   Oct-15    Reference 20 dB Attenuator   SN: 5058 (20k)   03-Apr-14 (No. 217-01921)   Apr-15    Type-N mismatch combination   SN: 5047 2 / 06327   03-Apr-14 (No. 217-01921)   Apr-15    Reference Probe ES3DV3   SN: 3205   30-Dec-14 (No. ES3-3205_Dec14)   Dec-15    DAE4   SN: 601   18-Aug-14 (No. DAE4-601_Aug14)   Aug-15    Secondary Standards   ID #   Check Date (in house)   Scheduled Check    RF generator R&S SMT-06   100005   04-Aug-99 (in house check Oct-13)   In house check: Oct-16    Network Analyzer HP 8753E   US37390685 S4205   18-Oct-01 (in house check Oct-14)   In house check: Oct-15    Name   Function   Signature    Calibrated by:   Cloudio Leublier   Leboratory Technician   Signature    Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Leboratory Technician   Signature   Signat	This calibration certificate docum	ents the traceability to nat	ional standards, which realize the physical un	nits of measurements (Si).
Primary Standards	The measurements and the unce	ertainties with confidence p	robability are given on the following pages ar	nd are part of the certificate.
Primary Standards	All calibrations have been condu	cted in the closed laborato	or facility aminonment temperature (22 - 200)	C and humidity - 200
Primary Standards				
Power meter EPM-442A   GB37480704   O7-Oct-14 (No. 217-02020)   Oct-15			y many, announced to paramete (az 2 g)	a programment of reserving
Power meter EPM-442A   GB37480704   O7-Oct-14 (No. 217-02020)   Oct-15			y looniy. Simonian da garana (az 2 s) l	
Power sensor HP 8481A	Calibration Equipment used (M&		y coords of the constraint (at 2 of the	
Power sensor HP 8481A   MY41092317   O7-Oct-14 (No. 217-02021)   Oct-15	Calibration Equipment used (M&	TE critical for calibration)	Cal Date (Certificate No.)	
Reference 20 dB Attenuator   SN: 5058 (20k)   O3-Apr-14 (No. 217-01918)   Apr-15	Calibration Equipment used (M& Primary Standards Power meter EPM-442A	TE critical for calibration)  ID #  GB37480704	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020)	Scheduled Celibration Oct-15
Type-N mismatch combination Reference Probe ES3DV3 SN: 3205 SN: 3205 SN: 3205 SN: 3205 SN: 601	Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	ID # GB37480704 US37292783	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02020)	Scheduled Celibration Oct-15
Secondary Standards	Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A	ID # GB37480704 US37292783	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02020)	Scheduled Calibration Oct-15 Oct-15
DAE4	Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator	TE critical for calibration)  ID #  GB37480704  US37292783  MY41092317	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02021)	Scheduled Calibration Oct-15 Oct-15 Oct-15
Secondary Standards ID # Check Date (in house) Scheduled Check  RF generator R&S SMT-06 100005 04-Aug-99 (in house check Oct-13) In house check: Oct-16  Network Analyzer HP 8753E US37390885 S4205 18-Oct-01 (in house check Oct-14) In house check: Oct-15  Name Function Signature  Calibrated by: Claudio Leubler Laboratory Technician	Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination	TE critical for calibration)  ID #  GB37480704  US37296783  MY41092317  SN: 5058 (20k)	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02021) 03-Apr-14 (No. 217-01918)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15
RF generator R&S SMT-06 100005 04-Aug-99 (in house check Oct-13) In house check: Oct-16 Network Analyzer HP 8753E US37390685 S4205 18-Oct-01 (in house check Oct-14) In house check: Oct-15  Name Function Signature Calibrated by: Claudio Leublier Leiboratory Technician	Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	TE critical for calibration)  ID #  GB37480704  US37292783  MY41092317  SN: 5058 (20k)  SN: 5047.2 / 06327	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02021) 03-Apr-14 (No. 217-01918) 03-Apr-14 (No. 217-01921)	Scheduled Calibration Oct-15 Oct-15 Apr-15 Apr-15
Network Analyzer HP 8753E US37390685 S4205 18-Oct-01 (in house check Oct-14) In house check: Oct-15  Name Function Signature Calibrated by: Claudio Leubler Leiboratory Technician	Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	ID #  GB37480704  US37292783  MY41092317  SN: 5058 (20k)  SN: 5047.2 / 06327  SN: 3205	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02021) 03-Apr-14 (No. 217-01918) 03-Apr-14 (No. 217-01921) 30-Dec-14 (No. ES3-3205_Dec14)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Dec-15
Calibrated by:  Name Function Signature  Claudio Leublier Laboratory Technician	Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4	TE critical for calibration)  ID #  GB37480704  US37292783  MY41092317  SN: 5058 (20k)  SN: 5047.2 / 06327  SN: 3205  SN: 601	Cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02021)  03-Apr-14 (No. 217-01918)  03-Apr-14 (No. 217-01921)  30-Dec-14 (No. ES3-3205_Dec14)  18-Aug-14 (No. DAE4-601_Aug14)  Check Date (in house)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Dec-15 Aug-15
Calibrated by: Claudio Leubiler Laboratory Technician	Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4	TE critical for calibration)  ID #  GB37480704  US37292783  MY41092317  SN: 5058 (20k)  SN: 5047.2 / 06327  SN: 3205  SN: 601	Cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02021)  03-Apr-14 (No. 217-01918)  03-Apr-14 (No. 217-01921)  30-Dec-14 (No. ES3-3205_Dec14)  18-Aug-14 (No. DAE4-601_Aug14)  Check Date (in house)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Dec-15 Aug-15 Scheduled Check
Caribrated by: Claudio Leubler Leiboratory Technician	Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06	TE critical for calibration)  ID #  GB37480704  US37296783  MY41092317  SN: 5058 (20k)  SN: 5047.2 / 06327  SN: 3206  SN: 601  ID #  100005	Cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02021)  03-Apr-14 (No. 217-01918)  03-Apr-14 (No. 217-01921)  30-Dec-14 (No. ES3-3205_Dec14)  18-Aug-14 (No. DAE4-601_Aug14)  Check Date (In house)  04-Aug-99 (in house check Oct-13)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Apr-15 Dec-15 Aug-15 Scheduled Check In house check: Oct-16
	Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06	TE critical for calibration)  ID #  GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3205 SN: 601  ID #  100005 US37390685 S4206	Cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02021)  03-Apr-14 (No. 217-01918)  03-Apr-14 (No. ES3-3205_Dec14)  18-Aug-14 (No. DAE4-601_Aug14)  Check Date (in house)  04-Aug-99 (in house check Oct-13)  18-Oct-01 (in house check Oct-14)	Scheduled Celibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Dec-15 Aug-15 Scheduled Check In house check: Oct-16 In house check: Oct-15
Approved by: Katja Pokovic Technical Manager	Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attonuator Type-N mismatch combination Reference Probe ES30V3 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E	TE critical for calibration)  ID #  GB37480704 US37292783 MY41092317 SN: 5056 (20k) SN: 5047.2 / 06327 SN: 3205 SN: 601  ID #  100005 US37390685 S4206	Cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02021)  03-Apr-14 (No. 217-01918)  03-Apr-14 (No. E33-3205_Dec14)  18-Aug-14 (No. DAE4-601_Aug14)  Check Date (in house)  04-Aug-99 (in house check Oct-13)  18-Oct-01 (in house check Oct-14)	Scheduled Celibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Dec-15 Aug-15 Scheduled Check In house check: Oct-16 In house check: Oct-15
	Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attonuator Type-N mismatch combination Reference Probe ES30V3 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E	TE critical for calibration)  ID #  GB37480704 US37292783 MY41092317 SN: 5056 (20k) SN: 5047.2 / 06327 SN: 3205 SN: 601  ID #  100005 US37390685 S4206	Cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02021)  03-Apr-14 (No. 217-01918)  03-Apr-14 (No. E33-3205_Dec14)  18-Aug-14 (No. DAE4-601_Aug14)  Check Date (in house)  04-Aug-99 (in house check Oct-13)  18-Oct-01 (in house check Oct-14)	Scheduled Celibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Dec-15 Aug-15 Scheduled Check In house check: Oct-16 In house check: Oct-15

Certificate No: D1900V2-5d194\_Jan15

Page 1 of 8



Report NO: TS201510006 Page 81 / 96

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z

not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- EC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- · SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D1900V2-5d194\_Jan15

Page 2 of 8



Report NO: TS201510006 Page 82 / 96

#### Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied.

**	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.1 ± 6 %	1.39 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	****	

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.1 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.6 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.32 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 16.5 % (k=2)

### **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.3 ± 6 %	1.50 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

#### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.95 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	40.1 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.31 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.3 W/kg ± 16.5 % (k=2)



Report NO: TS201510006 Page 83 / 96

### Appendix (Additional assessments outside the scope of SCS108)

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.7 Ω + 4.9  Ω	
Return Loss	- 24.5 dB	

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.9 Ω + 5.1 jΩ
Return Loss	- 25.6 dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.201 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	May 06, 2014

Certificate No: D1900V2-5d194\_Jan15

Page 4 of 8



Report NO: TS201510006 Page 84 / 96

#### **DASY5 Validation Report for Head TSL**

Date: 07.12.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d194

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz;  $\sigma = 1.39$  S/m;  $\epsilon_r = 40.1$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

#### DASY52 Configuration:


- Probe: ES3DV3 SN3205; ConvF(5, 5, 5); Calibrated: 30.12.2014;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

### Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 98.35 V/m; Power Drift = 0.04 dB Peak SAR (extrapolated) = 18.5 W/kg

SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.32 W/kg

Maximum value of SAR (measured) = 12.7 W/kg



0 dB = 12.7 W/kg = 11.04 dBW/kg


Certificate No: D1900V2-5d194\_Jan15



Report NO: TS201510006

Page 85 / 96

### Impedance Measurement Plot for Head TSL

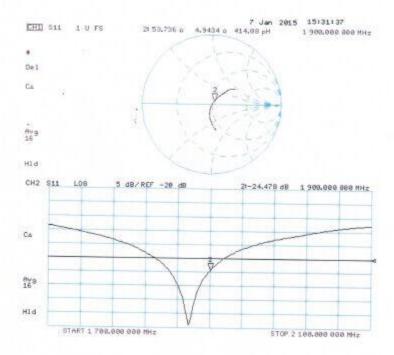

Certificate No: D1900V2-5d194\_Jan15

Page 6 of 8



Report NO: TS201510006 Page 86 / 96

### **DASY5 Validation Report for Body TSL**

Date: 07.01.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d194

Communication System: UID 0 - CW; Frequency: 1900 MHz Medium parameters used: f = 1900 MHz;  $\sigma = 1.5$  S/m;  $\epsilon_c = 53.3$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)


#### DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.65, 4.65, 4.65); Calibrated: 30.12.2014;
- · Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 95.88 V/m; Power Drift = -0.00 dB Peak SAR (extrapolated) = 16.8 W/kg SAR(1 g) = 9.95 W/kg; SAR(10 g) = 5.31 W/kg

Maximum value of SAR (measured) = 12.6 W/kg




0 dB = 12.6 W/kg = 11.00 dBW/kg



Report NO: TS201510006 Page 87 / 96



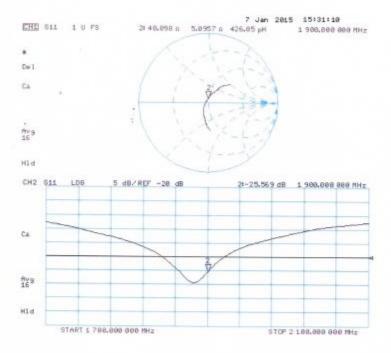



Report NO: TS201510006 Page 88 / 96

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

CALIBRATION	CERTIFICATE	E (Replacement of No: D	2450V2-955_Jan15)
Object	D2450V2 - SN: 9	955	
Calibration procedure(s)	QA CAL-05.v9 Calibration proce	dure for dipole validation kits abo	ove 700 MHz
Calibration date:	January 08, 2015	3	
This calibration certificate docum The measurements and the unco	nents the traceability to nat artainties with confidence p	ional standards, which realize the physical un robability are given on the following pages an	nits of measurements (SI). nd are part of the certificate.
		Valer to the state of	2 10 10 10
All calibrations have been condu	cted in the closed laborator	ry facility: environment temperature (22 $\pm$ 3) $^{\circ}$	C and humidity < 70%.
		ry facility: environment temperature (22 ± 3)*(	C and humidity < 70%.
Calibration Equipment used (M&			
Calibration Equipment used (M&	TE critical for calibration)	cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)	Scheduled Calibration Oct-15
Calibration Equipment used (M& Primary Standards Power meter EPM-442A	TE critical for calibration)	Cal Date (Certificate No.)	Scheduled Calibration
Calibration Equipment used (M& Primary Standards Power master EPM-442A Power sensor HP 8481A	TE critical for calibration)  ID #  GB37480704	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020)	Scheduled Calibration Oct-15
Calibration Equipment used (M& Primary Standards Power mater EPM-442A Power sensor HP 8481A Power sensor HP 8481A	TE critical for calibration)  ID #  GB37480704  US37292783	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02020)	Scheduled Calibration Oct-15 Oct-15
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator	TE critical for calibration)  ID #  G837480704  US37292783  MY41092317	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02021)	Scheduled Calibration Oct-15 Oct-15
Calibration Equipment used (M& Primary Standards Prower meter EPM-442A Prower sensor HP 8481A Prower sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination	TE critical for calibration)  ID #  G837480704  US37292783  MY41092317  SN: 5058 (20k)	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02021) 03-Apr-14 (No. 217-01918)	Scheduled Calibration Oct-15 Oct-15 Apr-15
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	ID #  GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02021) 03-Apr-14 (No. 217-01918) 03-Apr-14 (No. 217-01921)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards	TE critical for calibration)  ID #  G837480704  US37292783  MY41092317  SN: 5058 (20k)  SN: 5047.2 / 06327  SN: 3206  SN: 601	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02021) 03-Apr-14 (No. 217-01918) 03-Apr-14 (No. 217-01921) 30-Dec-14 (No. ES3-3205_Dec14)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Dec-15
Calibration Equipment used (M& Primary Standards Power meter EPM-642A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06	TE critical for calibration)  ID #  GB37480704  US37292783  MY41092317  SN: 5058 (20k)  SN: 5047.2 / 06327  SN: 3206  SN: 601	Cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02021)  03-Apr-14 (No. 217-01918)  03-Apr-14 (No. 217-01918)  30-Dec-14 (No. ES3-3205_Dec14)  18-Aug-14 (No. DAE4-601_Aug14)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Dec-15 Aug-15
All celibrations have been condu- Calibration Equipment used (M& Primary Standards Power moter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4  Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E	TE critical for calibration)  ID #  G837480704  US37292783  MY41092317  SN: 5058 (20k)  SN: 5047.2 / 06327  SN: 3206  SN: 601	Cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02021)  03-Apr-14 (No. 217-01918)  03-Apr-14 (No. 217-01921)  30-Dec-14 (No. ES3-3205_Dec14)  18-Aug-14 (No. DAE4-601_Aug14)  Check Date (in house)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Apr-15 Dec-15 Aug-15 Scheduled Check
Calibration Equipment used (M& Primary Standards Power meter EPM-642A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06	TE critical for calibration)  ID #  GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5058 (20k) SN: 5042/ 06327 SN: 3206 SN: 601  ID #  100005 US37390585 S4206	Cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02021)  03-Apr-14 (No. 217-01918)  03-Apr-14 (No. 217-01918)  03-Dec-14 (No. ESS-3205_Dec14)  18-Aug-14 (No. DAE4-601_Aug14)  Check Date (in house)  04-Aug-99 (in house check Oct-13)  18-Oct-01 (in house check Oct-14)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Dec-15 Aug-15 Scheduled Check In house check: Oct-16 In house check: Oct-16
Calibration Equipment used (M& Primary Standards Power mater EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E	TE critical for calibration)  ID #  GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3206 SN: 601  ID #  100005 US37390565 S4205	Cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02021)  03-Apr-14 (No. 217-01918)  03-Apr-14 (No. 217-01918)  30-Dec-14 (No. ES3-3205_Dec14)  18-Aug-14 (No. DAE4-601_Aug14)  Check Date (in house)  04-Aug-99 (in house check Oct-13)  18-Oct-01 (in house check Oct-14)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Apr-15 Dec-15 Aug-15 Scheduled Check In house check: Oct-18
Calibration Equipment used (M& Primary Standards Power meter EPM-642A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06	TE critical for calibration)  ID #  GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5058 (20k) SN: 5042/ 06327 SN: 3206 SN: 601  ID #  100005 US37390585 S4206	Cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02021)  03-Apr-14 (No. 217-01918)  03-Apr-14 (No. 217-01918)  03-Dec-14 (No. ESS-3205_Dec14)  18-Aug-14 (No. DAE4-601_Aug14)  Check Date (in house)  04-Aug-99 (in house check Oct-13)  18-Oct-01 (in house check Oct-14)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Dec-15 Aug-15 Scheduled Check In house check: Oct-16 In house check: Oct-16
Calibration Equipment used (M& Primary Standards Power mater EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E	TE critical for calibration)  ID #  GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3206 SN: 601  ID #  100005 US37390565 S4205	Cal Date (Certificate No.)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02020)  07-Oct-14 (No. 217-02021)  03-Apr-14 (No. 217-01918)  03-Apr-14 (No. 217-01918)  30-Dec-14 (No. ES3-3205_Dec14)  18-Aug-14 (No. DAE4-601_Aug14)  Check Date (in house)  04-Aug-99 (in house check Oct-13)  18-Oct-01 (in house check Oct-14)	Scheduled Calibration Oct-15 Oct-15 Oct-15 Apr-15 Apr-15 Dec-15 Aug-15 Scheduled Check In house check: Oct-16 In house check: Oct-16

Certificate No: D2450V2-955\_Jan15/2

Page 1 of 8



Report NO: TS201510006 Page 89 / 96

#### Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdiens C Service suisse d'étalonnage

Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

#### Glossary:

TSL

tissue simulating liquid

ConvF N/A sensitivity in TSL / NORM x,y,z

not applicable or not measured

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- EC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-955\_Jan15/2

Page 2 of 8



Report NO: TS201510006 Page 90 / 96

# Measurement Conditions DASY system configuration, a

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied.

- F	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.7 ± 6 %	1.84 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	****	****

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.2 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.4 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm3 (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.12 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.4 W/kg ± 16.5 % (k=2)

Body TSL parameters
The following parameters and calculations were applied.

200 PO 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.0 ± 6 %	2.03 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

#### SAR result with Body TSL

SAR averaged over 1 cm3 (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.8 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	53.7 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm3 (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.36 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	25.0 W/kg ± 16.5 % (k=2)

Certificate No: D2450V2-955\_Jan15/2



Report NO: TS201510006 Page 91 / 96

### Appendix (Additional assessments outside the scope of SCS108)

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	$54.8 \Omega + 3.5 j\Omega$	
Return Loss	- 24.9 dB	

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	51.2 Ω + 4.9 jΩ
Return Loss	- 26.0 dB

#### General Antenna Parameters and Design

Electrical Delay (one direction)	1.165 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	August 05, 2014

Certificate No: D2450V2-955\_Jan15/2

Page 4 of 8



Report NO: TS201510006 Page 92 / 96

#### **DASY5 Validation Report for Head TSL**

Date: 08.01.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 955

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz;  $\sigma = 1.84 \text{ S/m}$ ;  $\epsilon_r = 39.7$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)


#### DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.45, 4.45, 4.45); Calibrated: 30.12.2014;
- · Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

#### Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 101.2 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 27.5 W/kg SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.12 W/kg

Maximum value of SAR (measured) = 17.5 W/kg

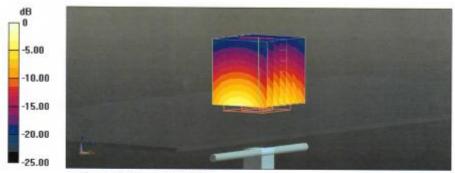


0 dB = 17.5 W/kg = 12.43 dBW/kg



Report NO: TS201510006 Page 93 / 96

#### Impedance Measurement Plot for Head TSL

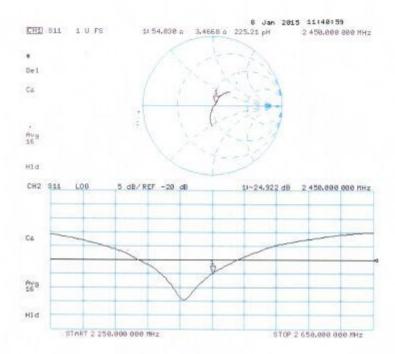

Certificate No: D2450V2-955\_Jan15/2

Page 6 of 8



Report NO: TS201510006 Page 94 / 96

#### **DASY5 Validation Report for Body TSL**

Date: 08.01.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 955

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz;  $\sigma = 2.03 \text{ S/m}$ ;  $\epsilon_r = 51$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)


#### DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.17, 4.17, 4.17); Calibrated: 30.12.2014;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 97.96 V/m; Power Drift = 0.01 dB Peak SAR (extrapolated) = 28.8 W/kg SAR(1 g) = 13.8 W/kg; SAR(10 g) = 6.36 W/kg

Maximum value of SAR (measured) = 18.3 W/kg

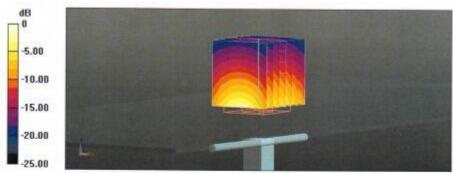


0 dB = 18.3 W/kg = 12.62 dBW/kg



Report NO: TS201510006 Page 95 / 96

### Impedance Measurement Plot for Body TSL

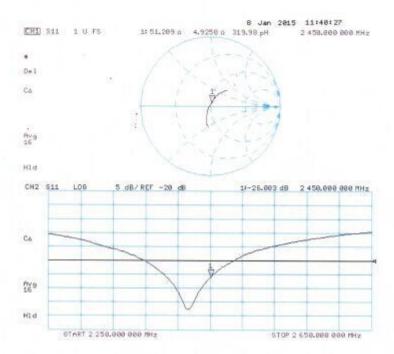



Report NO: TS201510006 Page 96 / 96



China National Accreditation Service for Conformity Assessment

# LABORATORY ACCREDITATION CERTIFICATE

(Registration No. CNAS L6487)

Shenzhen Sunway Communication Co., Ltd. Testing Center

1/F., Building A, SDG Info Port, Kefeng Road, Hi-Tech Park,

Nanshan District, Shenzhen, Guangdong, China

is accredited to ISO/IEC 17025:2005 General Requirements for the Competence of Testing and Calibration Laboratories(CNAS-CL01 Accreditation Criteria for the Competence of Testing and Calibration Laboratories) for the competence of testing.

The scope of accreditation is detailed in the attached appendices bearing the same registration number as above. The appendices form an integral part of this certificate.

Date of Issue: 2013-10-29

Date of Expiry: 2016-10-28

Date of Initial Accreditation: 2013-10-29

Date of Update: 2013-10-29

其建学

Signed on behalf of China National Accreditation Service for Conformity Assessment

China National Accreditation Service for Conformity Assessment (CNAS) is authorized by Certification and Accreditation Administration of the People's Republic of China (CNCA) to operate the national accreditation schemes for conformity assessment, CNAS is the signatory to International Laboratory Accreditation Cooperation Multilateral Recognition Arrangement (ILAC MRA) and Asia Pacific Laboratory Accreditation Cooperation Multilateral Recognition Arrangement (APLAC MRA).

No.CNASAL2

0008227