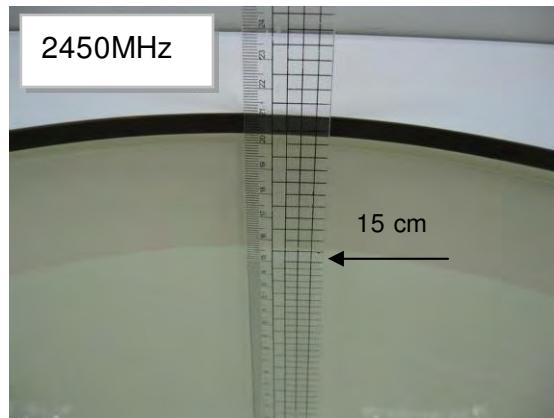


APPENDIX**11. Photographs of Test Setup****Fig.1 Photograph of the SAR measurement system**

Photograph of the Tissue Simulant Fluid Liquid (Body)**Fig.2****Extremity exposure - distance between flat phantom and backside of device is 0 mm****Fig.3 EUT Back side to flat phantom**

12. Photographs of the EUT



Fig.4 Front view of EUT



Fig.5 Back view of EUT

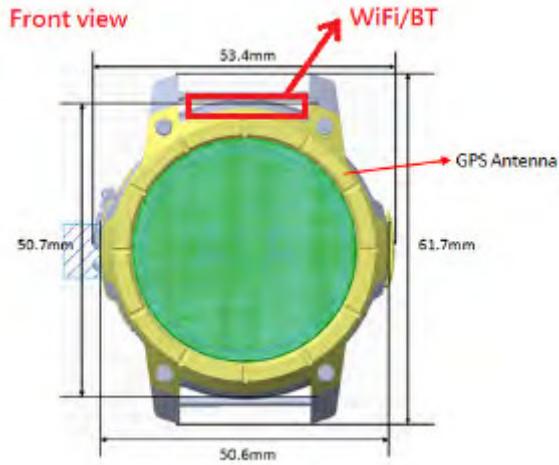


Fig.6 Antenna position of EUT (front view)

- End of Report -