

# Appendix D





## Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## 1. SAR measurement System




## 2. Photographs of Tissue Simulate Liquid

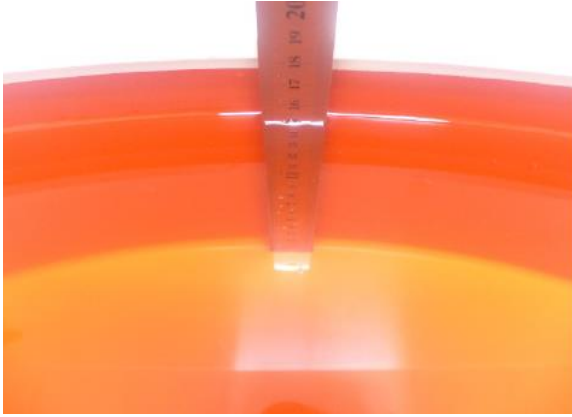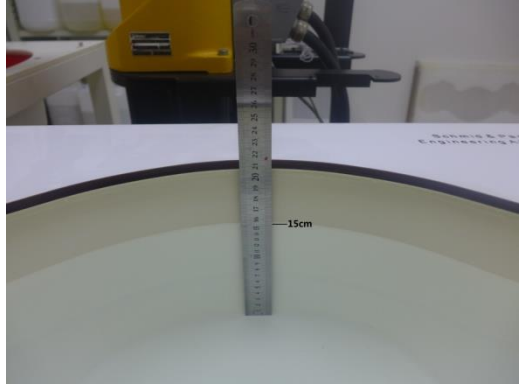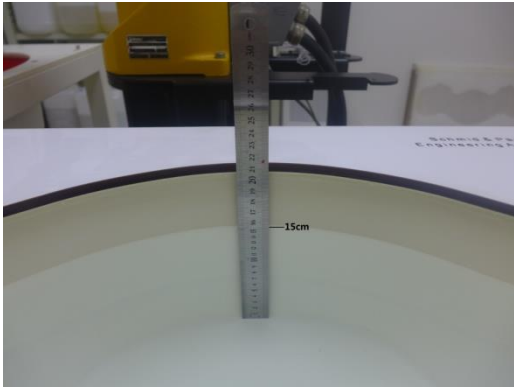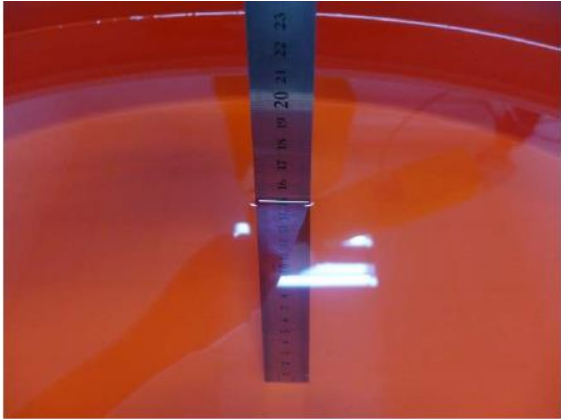


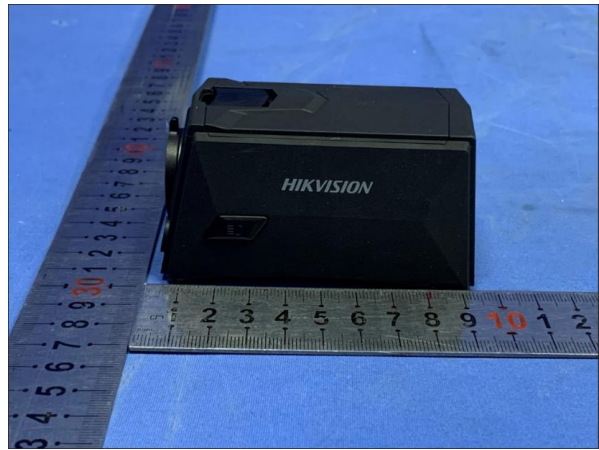
<p><b>Photo 1: Tissue Simulant Liquid for Head 835</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Head 1800</b></p>
	
<p><b>Photo 3: Tissue Simulant Liquid for Head 1900</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Head 2450</b></p>
	

### 3. Photographs of EUT test position

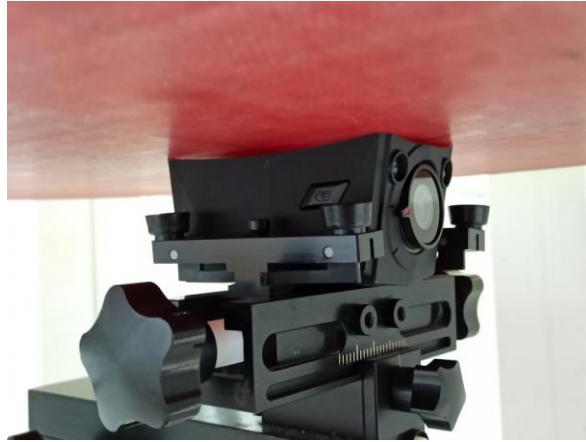Photo 5: Bottom side 0mm



### 4. EUT Constructional Details

<p>Photo 6: Front View</p>	<p>Photo 7: Back View</p>
	
<p>Photo 8: Left View</p>	<p>Photo 9: Right View</p>
	
<p>Photo 10: Top View</p>	<p>Photo 11: Bottom View</p>
