

# TEST REPORT

**Product Name** : Electronic Blood Pressure Monitor  
**Brand Mark** : Jumper  
**Model No.** : HAA21  
**Report Number** : BLA-EMC-202401-A5102  
**FCC ID** : 2ADYL-HAA21  
**Date of Sample Receipt** : 2024/1/19  
**Date of Test** : 2024/1/19 to 2024/3/25  
**Date of Issue** : 2024/3/25  
**Test Standard** : 47 CFR Part 15, Subpart C 15.247  
**Test Result** : Pass

Prepared for:

**Shenzhen Jumper Medical Equipment Co., Ltd.**  
**D Building, No.71, Xintian Road, Fuyong Street, Baoan, Shenzhen,**  
**Guangdong, China 518103**

Prepared by:

**BlueAsia of Technical Services(Shenzhen) Co.,Ltd.**  
**Building C, No. 107, Shihuan Road, Shiyuan Sub-District, Baoan District,**  
**Shenzhen, Guangdong Province, China**  
**TEL: +86-755-23059481**

Compiled by:

*Jozu*

Review by:

*Sueels*

Approved by:

*Blue Zheng*

Date:

2024/3/25



## REPORT REVISE RECORD

| Version No. | Date      | Description |
|-------------|-----------|-------------|
| 00          | 2024/3/25 | Original    |

BlueAsia

## TABLE OF CONTENTS

|           |  |           |
|-----------|--|-----------|
| <b>1</b>  | <b>TEST SUMMARY .....</b>  | <b>5</b>  |
| <b>2</b>  | <b>GENERAL INFORMATION .....</b>                                   | <b>6</b>  |
| <b>3</b>  | <b>GENERAL DESCRIPTION OF E.U.T. ....</b>                          | <b>6</b>  |
| <b>4</b>  | <b>TEST ENVIRONMENT .....</b>                                      | <b>8</b>  |
| <b>5</b>  | <b>TEST MODE .....</b>   | <b>8</b>  |
| <b>6</b>  | <b>MEASUREMENT UNCERTAINTY .....</b>                               | <b>8</b>  |
| <b>7</b>  | <b>DESCRIPTION OF SUPPORT UNIT .....</b>                           | <b>9</b>  |
| <b>8</b>  | <b>TEST FACILITY .....</b>   | <b>9</b>  |
| <b>9</b>  | <b>LABORATORY LOCATION .....</b>                                   | <b>9</b>  |
| <b>10</b> | <b>TEST INSTRUMENTS LIST .....</b>                                 | <b>10</b> |
| <b>11</b> | <b>CONDUCTED EMISSIONS AT AC POWER LINE (150KHZ-30MHZ) .....</b>   | <b>12</b> |
| 11.1      | LIMITS .....   | 12        |
| 11.2      | BLOCK DIAGRAM OF TEST SETUP .....                                  | 12        |
| 11.3      | PROCEDURE .....  | 12        |
| 11.4      | TEST DATA .....  | 14        |
| <b>12</b> | <b>CONDUCTED BAND EDGES MEASUREMENT .....</b>                      | <b>17</b> |
| 12.1      | LIMITS .....   | 17        |
| 12.2      | BLOCK DIAGRAM OF TEST SETUP .....                                  | 17        |
| 12.3      | TEST DATA .....  | 17        |
| <b>13</b> | <b>RADIATED SPURIOUS EMISSIONS .....</b>                           | <b>18</b> |
| 13.1      | LIMITS .....   | 18        |
| 13.2      | BLOCK DIAGRAM OF TEST SETUP .....                                  | 19        |
| 13.3      | PROCEDURE .....  | 19        |
| 13.4      | TEST DATA .....  | 21        |
| <b>14</b> | <b>RADIATED EMISSIONS WHICH FALL IN THE RESTRICTED BANDS .....</b> | <b>30</b> |
| 14.1      | LIMITS .....   | 30        |
| 14.2      | BLOCK DIAGRAM OF TEST SETUP .....                                  | 31        |
| 14.3      | PROCEDURE .....  | 31        |
| 14.4      | TEST DATA .....  | 33        |
| <b>15</b> | <b>CONDUCTED SPURIOUS EMISSIONS .....</b>                          | <b>38</b> |

|  |  |           |
|--|--|-----------|
| 15.1   | LIMITS .....                             | 38        |
| 15.2   | BLOCK DIAGRAM OF TEST SETUP .....        | 38        |
| 15.3   | TEST DATA .....                          | 38        |
| <b>16</b>  | <b>POWER SPECTRUM DENSITY .....</b>      | <b>39</b> |
| 16.1   | LIMITS .....                             | 39        |
| 16.2   | BLOCK DIAGRAM OF TEST SETUP .....        | 39        |
| 16.3   | TEST DATA .....                          | 39        |
| <b>17</b>  | <b>CONDUCTED PEAK OUTPUT POWER .....</b> | <b>40</b> |
| 17.1   | LIMITS .....                             | 40        |
| 17.2   | BLOCK DIAGRAM OF TEST SETUP .....        | 40        |
| 17.3   | TEST DATA .....                          | 40        |
| <b>18</b>  | <b>MINIMUM 6DB BANDWIDTH .....</b>       | <b>41</b> |
| 18.1   | LIMITS .....                             | 41        |
| 18.2   | BLOCK DIAGRAM OF TEST SETUP .....        | 41        |
| 18.3   | TEST DATA .....                          | 41        |
| <b>19</b>  | <b>ANTENNA REQUIREMENT .....</b>         | <b>42</b> |
| 19.1   | CONCLUSION .....                         | 42        |
| <b>20</b>  | <b>APPENDIX1 .....</b>                   | <b>43</b> |
| <b>APPENDIX A: PHOTOGRAPHS OF TEST SETUP .....</b> |  | <b>58</b> |
| <b>APPENDIX B: PHOTOGRAPHS OF EUT .....</b>        |  | <b>60</b> |

## 1 TEST SUMMARY

| Test item   | Test Requirement                 | Test Method  | Class/Severity                               | Result |
|---|----------------------------------|--|--|--------|
| Conducted Emissions at AC Power Line (150kHz-30MHz)   | 47 CFR Part 15, Subpart C 15.247 | ANSI C63.10 (2013) Section 6.2                       | 47 CFR Part 15, Subpart C 15.207             | Pass   |
| Conducted Band Edges Measurement                      | 47 CFR Part 15, Subpart C 15.247 | ANSI C63.10 (2013) Section 7.8.8 & Section 11.13.3.2 | 47 CFR Part 15, Subpart C 15.247(d)          | Pass   |
| Radiated Spurious Emissions                           | 47 CFR Part 15, Subpart C 15.247 | ANSI C63.10 (2013) Section 6.4,6.5,6.6               | 47 CFR Part 15, Subpart C 15.209 & 15.247(d) | Pass   |
| Radiated Emissions which fall in the restricted bands | 47 CFR Part 15, Subpart C 15.247 | ANSI C63.10 (2013) Section 6.10.5                    | 47 CFR Part 15, Subpart C 15.209 & 15.247(d) | Pass   |
| Conducted Spurious Emissions                          | 47 CFR Part 15, Subpart C 15.247 | ANSI C63.10 (2013) Section 7.8.6 & Section 11.11     | 47 CFR Part 15, Subpart C 15.247(d)          | Pass   |
| Power Spectrum Density                                | 47 CFR Part 15, Subpart C 15.247 | ANSI C63.10 (2013) Section 11.10.2                   | 47 CFR Part 15, Subpart C 15.247(e)          | Pass   |
| Conducted Peak Output Power                           | 47 CFR Part 15, Subpart C 15.247 | ANSI C63.10 (2013) Section 7.8.5                     | 47 CFR Part 15, Subpart C 15.247(b)(3)       | Pass   |
| Minimum 6dB Bandwidth                                 | 47 CFR Part 15, Subpart C 15.247 | ANSI C63.10 (2013) Section 11.8.1                    | 47 CFR Part 15, Subpart C 15.247a(2)         | Pass   |
| Antenna Requirement                                   | 47 CFR Part 15, Subpart C 15.247 | N/A  | 47 CFR Part 15, Subpart C 15.203 & 15.247(c) | Pass   |

Remark:

N/A: Not Applicable

## 2 GENERAL INFORMATION

|                       |  |
|-----------------------|--|
| <b>Applicant</b>      | Shenzhen Jumper Medical Equipment Co., Ltd.  |
| <b>Address</b>        | D Building, No.71, Xintian Road, Fuyong Street, Baoan, Shenzhen, Guangdong, China 518103 |
| <b>Manufacturer</b>   | Shenzhen Jumper Medical Equipment Co., Ltd.  |
| <b>Address</b>        | D Building, No.71, Xintian Road, Fuyong Street, Baoan, Shenzhen, Guangdong, China 518103 |
| <b>Factory</b>        | Shenzhen Jumper Medical Equipment Co., Ltd.  |
| <b>Address</b>        | D Building, No.71, Xintian Road, Fuyong Street, Baoan, Shenzhen, Guangdong, China 518103 |
| <b>Product Name</b>   | Electronic Blood Pressure Monitor  |
| <b>Test Model No.</b> | HAA21  |

## 3 GENERAL DESCRIPTION OF E.U.T.

|                             |                                  |
|-----------------------------|----------------------------------|
| <b>Hardware Version</b>     | V1.2                             |
| <b>Software Version</b>     | V1.0                             |
| <b>Operation Frequency:</b> | 2402MHz-2480MHz                  |
| <b>Modulation Type:</b>     | GFSK                             |
| <b>Rate data:</b>           | 1Mbps                            |
| <b>Channel Spacing:</b>     | 2MHz                             |
| <b>Number of Channels:</b>  | 40                               |
| <b>Antenna Type:</b>        | PCB Antenna                      |
| <b>Antenna Gain:</b>        | 0dBi (Provided by the applicant) |

| Operation Frequency each of channel |           |         |           |         |           |         |           |
|-------------------------------------|-----------|---------|-----------|---------|-----------|---------|-----------|
| Channel                             | Frequency | Channel | Frequency | Channel | Frequency | Channel | Frequency |
| 1                                   | 2402MHz   | 11      | 2422MHz   | 21      | 2442MHz   | 31      | 2462MHz   |
| 2                                   | 2404MHz   | 12      | 2424MHz   | 22      | 2444MHz   | 32      | 2464MHz   |
| ⋮                                   | ⋮         | ⋮       | ⋮         | ⋮       | ⋮         | ⋮       | ⋮         |
| 9                                   | 2418MHz   | 19      | 2438MHz   | 29      | 2458MHz   | 39      | 2478MHz   |
| 10                                  | 2420MHz   | 20      | 2440MHz   | 30      | 2460MHz   | 40      | 2480MHz   |

Note:

In section 15.31(m), regards to the operating frequency range over 10 MHz, the Lowest frequency, the middle frequency, and the highest frequency of channel were selected to perform the test, and the selected channel see below:

| Channel             | Frequency |
|---------------------|-----------|
| The lowest channel  | 2402MHz   |
| The middle channel  | 2442MHz   |
| The Highest channel | 2480MHz   |

#### 4 TEST ENVIRONMENT

| Environment | Temperature | Voltage |
|-------------|-------------|---------|
| Normal      | 25°C        | 6Vdc    |

#### 5 TEST MODE

| TEST MODE         | TEST MODE DESCRIPTION   |
|-------------------|---|
| Transmitting mode | Keep the EUT in continuously transmitting mode with modulation. |

#### 6 MEASUREMENT UNCERTAINTY

| Parameter                                      | Expanded Uncertainty (Confidence of 95%) |
|--|--|
| Occupied Channel Bandwidth                     | ±5 %                                     |
| RF output power, conducted                     | ±1.5 dB                                  |
| Power Spectral Density, conducted              | ±3.0 dB                                  |
| Unwanted Emissions, conducted                  | ±3.0 dB                                  |
| Temperature                                    | ±3 °C                                    |
| Supply voltages                                | ±3 %                                     |
| Time   | ±5 %                                     |
| Unwanted Radiated Emission (30MHz ~ 1000MHz)   | ±4.35 dB                                 |
| Unwanted Radiated Emission (1GHz ~ 18GHz)      | ±4.44 dB                                 |
| AC Power Line Conducted Emission(150kHz-30MHz) | ±3.45dB                                  |



## 7 DESCRIPTION OF SUPPORT UNIT

| Device Type | Manufacturer | Model Name | Serial No. | Remark |
|-------------|--------------|------------|------------|--------|
| AC Adapter  | UGREEN       | CD112      | N/A        | N/A    |

## 8 TEST FACILITY

The test facility is recognized, certified, or accredited by the following organizations:

- FCC — Designation No.: CN1252

BlueAsia of Technical Services(Shenzhen) Co., Ltd has been registered and fully described in a report filed with the (FCC) Federal Communications Commission. The acceptance letter from the FCC is maintained in files. Designation CN1252.

- ISED — CAB identifier No.: CN0028

BlueAsia of Technical Services(Shenzhen) Co., Ltd has been registered by Certification and Engineering Bureau of ISED for radio equipment testing with CAB identifier CN0028.

## 9 LABORATORY LOCATION

All tests were performed at:

BlueAsia of Technical Services(Shenzhen) Co.,Ltd.

Building C, No. 107, Shihuan Road, Shiyuan Sub-District, Baoan District, Shenzhen, Guangdong Province, China

Telephone: TEL: +86-755-28682673 FAX: +86-755-28682673

## 10 TEST INSTRUMENTS LIST

| Test Equipment Of Radiated Spurious Emissions |              |                        |                  |            |            |
|---|--------------|------------------------|------------------|------------|------------|
| Equipment                                     | Manufacturer | Model                  | S/N              | Cal.Date   | Cal.Due    |
| Chamber 1                                     | SKET         | 966                    | N/A              | 2023/11/16 | 2026/11/15 |
| Chamber 2                                     | SKET         | 966                    | N/A              | 2021/07/20 | 2024/07/19 |
| Spectrum                                      | R&S          | FSP40                  | 100817           | 2023/08/30 | 2024/08/29 |
| Receiver                                      | R&S          | ESR7                   | 101199           | 2023/08/30 | 2024/08/29 |
| Receiver                                      | R&S          | ESPI7                  | 101477           | 2023/07/07 | 2024/07/06 |
| broadband Antenna                             | Schwarzbeck  | VULB9168               | 00836<br>P:00227 | 2022/10/12 | 2025/10/11 |
| Horn Antenna                                  | Schwarzbeck  | BBHA9120D              | 01892<br>P:00331 | 2022/09/13 | 2025/09/12 |
| Horn Antenna                                  | Schwarzbeck  | BBHA 9170              | 1106             | 2022/04/24 | 2024/04/23 |
| Amplifier                                     | SKET         | LNPA_30M01G-30         | SK2021060801     | 2023/07/07 | 2024/07/06 |
| Amplifier                                     | SKET         | PA-000318G-45          | N/A              | 2023/08/30 | 2024/08/29 |
| Amplifier                                     | SKET         | LNPA_18G40G-50         | SK2022071301     | 2023/07/14 | 2024/07/13 |
| Filter group                                  | SKET         | 2.4G/5G Filter group r | N/A              | 2023/07/07 | 2024/07/06 |
| EMI software                                  | EZ           | EZ-EMC                 | EEMC-3A1         | N/A        | N/A        |
| Loop antenna                                  | SCHNARZBECK  | FMZB1519B              | 00102            | 2022/09/14 | 2025/09/13 |
| 1kHz calibration audio source                 | SKET         | MCS-ABT-C35            | N/A              | 2023/09/04 | 2024/09/03 |
| Free Field Microphone                         | SKET         | MGS MP 663             | 0414             | 2023/09/04 | 2024/09/03 |
| Audio shielding box                           | SKET         | SB-ABT-C35             | N/A              | 2023/03/30 | 2024/03/29 |
| Controller                                    | SKET         | N/A                    | N/A              | N/A        | N/A        |
| Coaxial Cable                                 | BlueAsia     | BLA-XC-02              | N/A              | N/A        | N/A        |
| Coaxial Cable                                 | BlueAsia     | BLA-XC-03              | N/A              | N/A        | N/A        |
| Coaxial Cable                                 | BlueAsia     | BLA-XC-01              | N/A              | N/A        | N/A        |
| Signal Generator DTV                          | ECREDIX      | DSG-1000               | N/A              | N/A        | N/A        |

| <b>Test Equipment Of RF Conducted Test</b> |                     |              |                 |                 |                |
|--|---------------------|--------------|-----------------|-----------------|----------------|
| <b>Equipment</b>                           | <b>Manufacturer</b> | <b>Model</b> | <b>S/N</b>      | <b>Cal.Date</b> | <b>Cal.Due</b> |
| Spectrum                                   | R&S                 | FSP40        | 100817          | 2023/08/30      | 2024/08/29     |
| Spectrum                                   | Agilent             | N9020A       | MY49100060      | 2023/08/30      | 2024/08/29     |
| Spectrum                                   | Agilent             | N9020A       | MY54420161      | 2023/08/30      | 2024/08/29     |
| Signal Generator                           | Agilent             | N5182A       | MY47420955      | 2023/08/30      | 2024/08/29     |
| Signal Generator                           | Agilent             | N5181A       | MY46240904      | 2023/07/07      | 2024/07/06     |
| Signal Generator                           | R&S                 | CMW500       | 132429          | 2023/08/30      | 2024/08/29     |
| BluetoothTester                            | Anritsu             | MT8852B      | 06262047872     | 2023/08/30      | 2024/08/29     |
| Power probe                                | DARE                | RPR3006W     | 14I00889SN042   | 2023/09/01      | 2024/08/31     |
| Power detection box                        | CDKMV               | MW100-PSB    | MW201020JYT     | 2023/07/07      | 2024/07/06     |
| DCPowersupply                              | zhaoxin             | KXN-305D     | 20K305D1221363  | 2023/08/30      | 2024/08/29     |
| DCPowersupply                              | zhaoxin             | RXN-1505D    | 19R1505D050168  | 2023/08/30      | 2024/08/29     |
| 2.4GHz/5GHz RF Test software               | MTS                 | MTS 8310     | Version 2.0.0.0 | N/A             | N/A            |
| Audio Analyzer                             | Audio Precision     | ATS-1        | ATS141094       | 2023/07/07      | 2024/07/06     |

| <b>Test Equipment Of Conducted Emissions at AC Power Line (150kHz-30MHz)</b> |                     |              |               |                 |                |
|--|---------------------|--------------|---------------|-----------------|----------------|
| <b>Equipment</b>   | <b>Manufacturer</b> | <b>Model</b> | <b>S/N</b>    | <b>Cal.Date</b> | <b>Cal.Due</b> |
| Shield room  | SKET                | 833          | N/A           | 2023/11/16      | 2025/11/15     |
| Receiver   | R&S                 | ESPI3        | 101082        | 2023/08/30      | 2024/08/29     |
| LISN   | R&S                 | ENV216       | 3560.6550.15  | 2023/08/30      | 2024/08/29     |
| LISN   | AT                  | AT166-2      | AKK1806000003 | 2023/08/30      | 2024/08/29     |
| ISN  | TESEQ               | ISNT8-cat6   | 53580         | 2023/08/30      | 2024/08/29     |
| Single-channel vehicle artificial power network                              | Schwarzbeck         | NNBM 8124    | 01045         | 2023/07/07      | 2024/07/06     |
| Single-channel vehicle artificial power network                              | Schwarzbeck         | NNBM 8124    | 01075         | 2023/07/07      | 2024/07/06     |
| EMI software   | EZ                  | EZ-EMC       | EEMC-3A1      | N/A             | N/A            |
| Coaxial Cable  | BlueAsia            | BLA-XC-05    | N/A           | N/A             | N/A            |

## 11 CONDUCTED EMISSIONS AT AC POWER LINE (150KHZ-30MHZ)


|                        |                                  |
|------------------------|----------------------------------|
| Test Standard          | 47 CFR Part 15, Subpart C 15.247 |
| Test Method            | ANSI C63.10 (2013) Section 6.2   |
| Test Mode (Pre-Scan)   | TX                               |
| Test Mode (Final Test) | TX                               |
| Tester                 | Jozu                             |
| Temperature            | 25°C                             |
| Humidity               | 60%                              |

### 11.1 LIMITS

| Frequency of emission(MHz) | Conducted limit(dB $\mu$ V) |           |
|----------------------------|-----------------------------|-----------|
|                            | Quasi-peak                  | Average   |
| 0.15-0.5                   | 66 to 56*                   | 56 to 46* |
| 0.5-5                      | 56                          | 46        |
| 5-30                       | 60                          | 50        |

\*Decreases with the logarithm of the frequency.

### 11.2 BLOCK DIAGRAM OF TEST SETUP

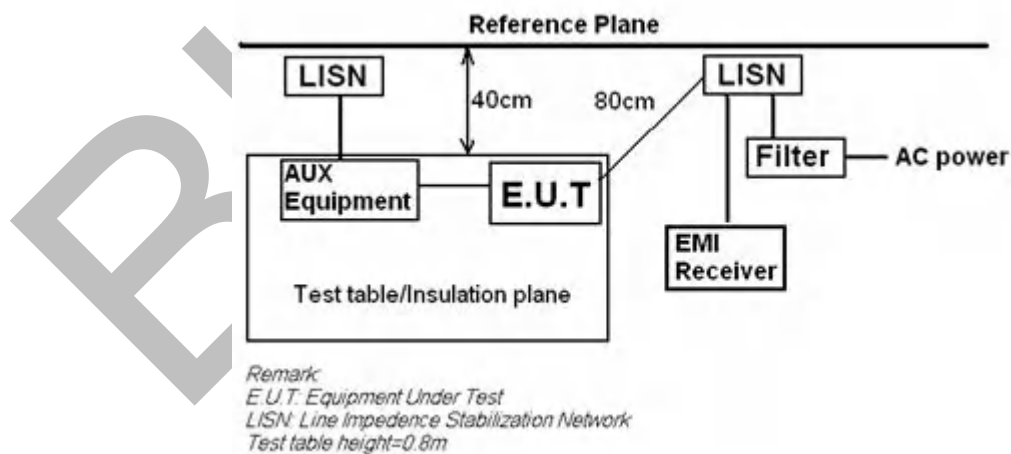

### 11.3 PROCEDURE

- 1) The mains terminal disturbance voltage test was conducted in a shielded room.
- 2) The EUT was connected to AC power source through a LISN 1 (Line Impedance Stabilization Network) which provides a 50ohm/50H + 5ohm linear impedance. The power cables of all other units of the EUT were connected to a second LISN 2, which was bonded to the ground reference plane in the same way as the LISN 1 for the unit being measured. A multiple socket outlet strip was used to connect multiple power cables to a single LISN provided the rating of the LISN was not exceeded.

3) The tabletop EUT was placed upon a non-metallic table 0.8m above the ground reference plane. And for floor-standing arrangement, the EUT was placed on the horizontal ground reference plane,

4) The test was performed with a vertical ground reference plane. The rear of the EUT shall be 0.4 m from the vertical ground reference plane. The vertical ground reference plane was bonded to the horizontal ground reference plane. The LISN 1 was placed 0.8 m from the boundary of the unit under test and bonded to a ground reference plane for LISNs mounted on top of the ground reference plane. This distance was between the closest points of the LISN 1 and the EUT. All other units of the EUT and associated equipment was at least 0.8 m from the LISN 2.


5) In order to find the maximum emission, the relative positions of equipment and all of the interface cables must be changed according to ANSI C63.10 on conducted measurement.

Remark: LISN=Read Level+ Cable Loss+ LISN Factor

BlueAsia

### 11.4 TEST DATA

[TestMode: Tx]; [Line: Line] ;[Power:AC120V/60Hz]

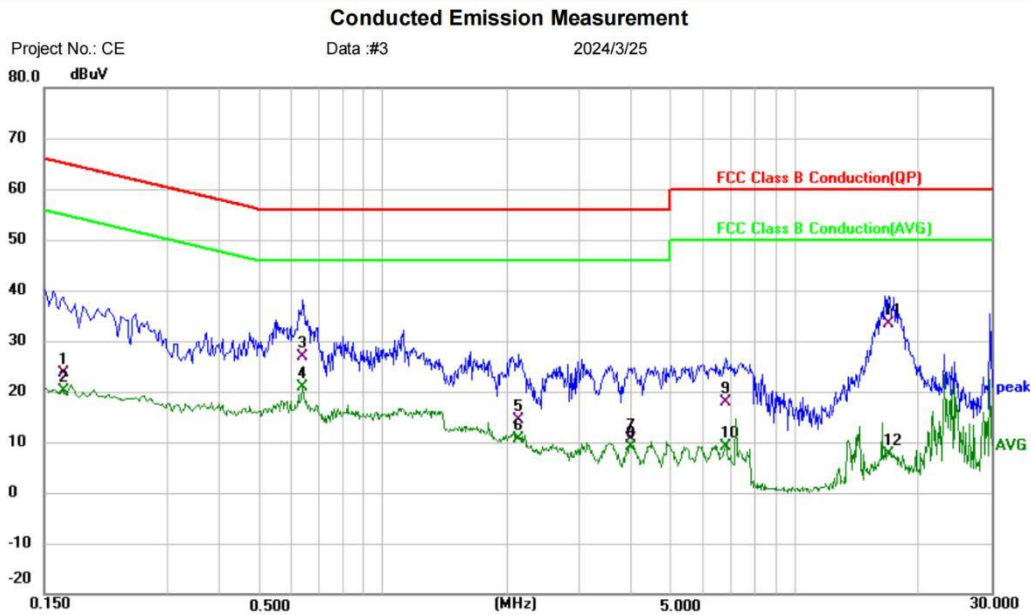

|  |                      |                   |
|--|----------------------|-------------------|
| Site                                   | Phase: <b>L1</b>     | Temperature: (C)  |
| Limit: FCC Class B Conduction(QP)      | Power:               | Humidity: %RH     |
| EUT: Electronic Blood Pressure Monitor | Distance: RBW: 9 KHz | Sweep Time: 10 ms |
| M/N: HAA21                             | VBW: 30 KHz          |                   |
| Mode: TX mode                          |                      |                   |
| Note:                                  |                      |                   |

| No. | Mk. | Freq.   | Reading Level | Correct Factor | Measurement | Limit | Over   | Antenna Height | Table Degree |         |
|-----|-----|---------|---------------|----------------|-------------|-------|--------|----------------|--------------|---------|
|     |     | MHz     | dBuV          | dB             | dBuV        | dBuV  | dB     | cm             | degree       | Comment |
| 1   |     | 0.1660  | 13.54         | 10.15          | 23.69       | 65.16 | -41.47 | QP             |              |         |
| 2   |     | 0.1660  | 9.87          | 10.15          | 20.02       | 55.16 | -35.14 | AVG            |              |         |
| 3   |     | 0.6380  | 16.82         | 9.96           | 26.78       | 56.00 | -29.22 | QP             |              |         |
| 4   | *   | 0.6380  | 10.84         | 9.96           | 20.80       | 46.00 | -25.20 | AVG            |              |         |
| 5   |     | 2.1380  | 4.23          | 10.14          | 14.37       | 56.00 | -41.63 | QP             |              |         |
| 6   |     | 2.1380  | 0.60          | 10.14          | 10.74       | 46.00 | -35.26 | AVG            |              |         |
| 7   |     | 3.9980  | 0.72          | 9.95           | 10.67       | 56.00 | -45.33 | QP             |              |         |
| 8   |     | 3.9980  | -0.74         | 9.95           | 9.21        | 46.00 | -36.79 | AVG            |              |         |
| 9   |     | 6.7940  | 7.04          | 10.84          | 17.88       | 60.00 | -42.12 | QP             |              |         |
| 10  |     | 6.7940  | -1.70         | 10.84          | 9.14        | 50.00 | -40.86 | AVG            |              |         |
| 11  |     | 16.8980 | 19.65         | 13.75          | 33.40       | 60.00 | -26.60 | QP             |              |         |
| 12  |     | 16.8980 | -6.06         | 13.75          | 7.69        | 50.00 | -42.31 | AVG            |              |         |

\*:Maximum data    x:Over limit    !:over margin      <Reference Only

Receiver: ESPL\_1      Spectrum Analyzer: ESPI


L.I.S.N:      Engineer Signature:

**Test Result: Pass**



[TestMode: Tx]; [Line: Neutral] ;[Power:AC120V/60Hz]

### Conducted Emission Measurement

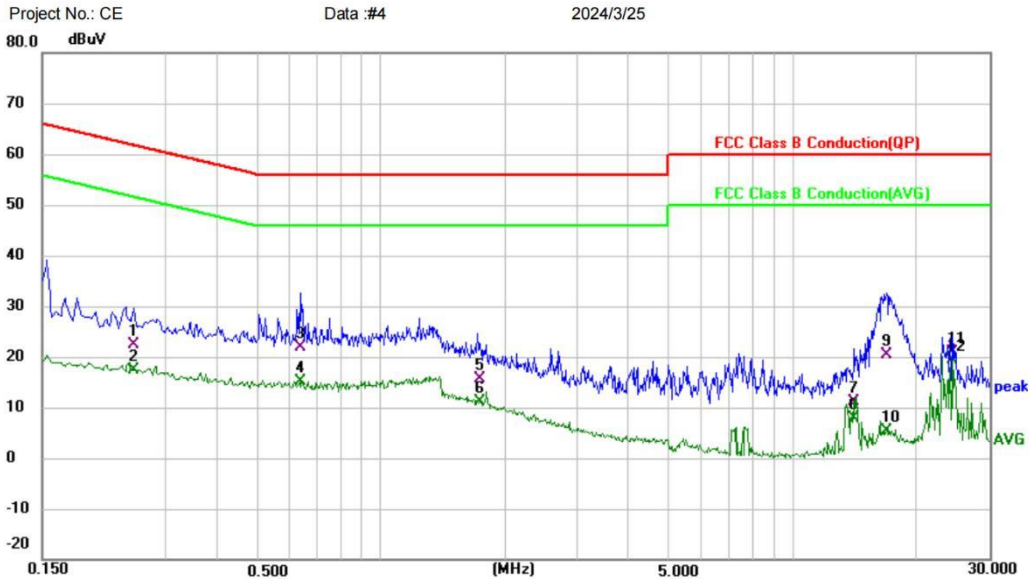

|  |                 |                   |
|--|-----------------|-------------------|
| Site                                   | Phase: <b>N</b> | Temperature: (C)  |
| Limit: FCC Class B Conduction(QP)      | Power:          | Humidity: %RH     |
| EUT: Electronic Blood Pressure Monitor | Distance:       | RBW: 9 KHz        |
| M/N: HAA21                             |                 | VBW: 30 KHz       |
| Mode: TX mode                          |                 | Sweep Time: 10 ms |
| Note:                                  |                 |                   |

| No. | Mk. | Freq.   | Reading Level | Correct Factor | Measurement | Limit | Over   | Antenna Height | Table Degree |         |
|-----|-----|---------|---------------|----------------|-------------|-------|--------|----------------|--------------|---------|
|     |     | MHz     | dBuV          | dB             | dBuV        | dBuV  | dB     | cm             | degree       | Comment |
| 1   |     | 0.2500  | 12.02         | 10.37          | 22.39       | 61.76 | -39.37 |                |              | QP      |
| 2   |     | 0.2500  | 7.12          | 10.37          | 17.49       | 51.76 | -34.27 |                |              | AVG     |
| 3   |     | 0.6340  | 12.10         | 9.89           | 21.99       | 56.00 | -34.01 |                |              | QP      |
| 4   |     | 0.6340  | 5.12          | 9.89           | 15.01       | 46.00 | -30.99 |                |              | AVG     |
| 5   |     | 1.7379  | 5.58          | 9.98           | 15.56       | 56.00 | -40.44 |                |              | QP      |
| 6   |     | 1.7379  | 1.13          | 9.98           | 11.11       | 46.00 | -34.89 |                |              | AVG     |
| 7   |     | 14.0900 | 12.46         | -1.33          | 11.13       | 60.00 | -48.87 |                |              | QP      |
| 8   |     | 14.0900 | 9.27          | -1.33          | 7.94        | 50.00 | -42.06 |                |              | AVG     |
| 9   |     | 16.8419 | 6.77          | 13.63          | 20.40       | 60.00 | -39.60 |                |              | QP      |
| 10  |     | 16.8419 | -8.24         | 13.63          | 5.39        | 50.00 | -44.61 |                |              | AVG     |
| 11  |     | 24.3500 | 6.06          | 14.88          | 20.94       | 60.00 | -39.06 |                |              | QP      |
| 12  | *   | 24.3500 | 4.41          | 14.88          | 19.29       | 50.00 | -30.71 |                |              | AVG     |

\*:Maximum data    x:Over limit    !:over margin      <Reference Only

Receiver: ESPI\_1      Spectrum Analyzer: ESPI

L.I.S.N:      Engineer Signature:

**Test Result: Pass**

Notes:

1. An initial pre-scan was performed on the line and neutral lines with peak detector.
2. Quasi-Peak and Average measurement were performed at the frequencies with maximized peak emission.
3. Final Level =Receiver Read level + LISN Factor + Cable Loss.

BlueAsia




## 12 CONDUCTED BAND EDGES MEASUREMENT

|                               |  |
|-------------------------------|--|
| <b>Test Standard</b>          | 47 CFR Part 15, Subpart C 15.247                     |
| <b>Test Method</b>            | ANSI C63.10 (2013) Section 7.8.8 & Section 11.13.3.2 |
| <b>Test Mode (Pre-Scan)</b>   | TX   |
| <b>Test Mode (Final Test)</b> | TX   |
| <b>Tester</b>                 | Jozu   |
| <b>Temperature</b>            | 25°C   |
| <b>Humidity</b>               | 60%  |

### 12.1 LIMITS

|               |   |
|---------------|---|
| <b>Limit:</b> | <p>In any 100 kHz bandwidth outside the frequency band in which the spread spectrum or digitally modulated intentional radiator is operating, the radio frequency power that is produced by the intentional radiator shall be at least 20 dB below that in the 100 kHz bandwidth within the band that contains the highest level of the desired power, based on either an RF conducted or a radiated measurement, provided the transmitter demonstrates compliance with the peak conducted power limits. If the transmitter complies with the conducted power limits based on the use of RMS averaging over a time interval, as permitted under paragraph (b)(3) of this section, the attenuation required under this paragraph shall be 30 dB instead of 20 dB. Attenuation below the general limits specified in §15.209(a) is not required. In addition, radiated emissions which fall in the restricted bands, as defined in §15.205(a), must also comply with the radiated emission limits specified in §15.209(a) (see §15.205(c)).</p> |
|---------------|---|

### 12.2 BLOCK DIAGRAM OF TEST SETUP

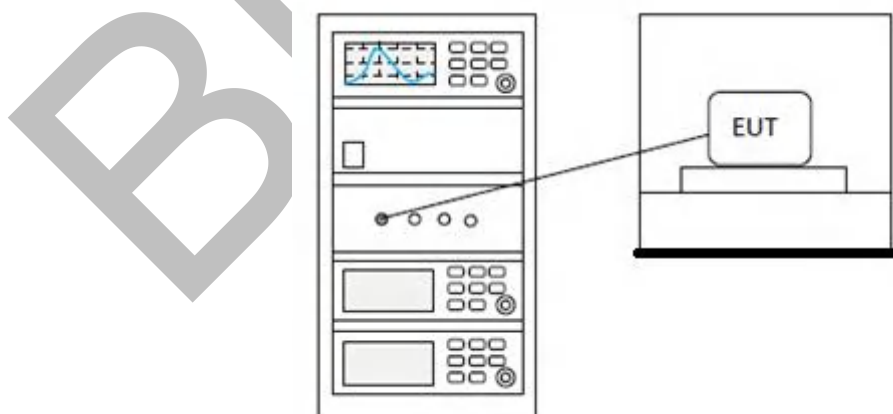

### 12.3 TEST DATA

**Pass: Please Refer To Appendix: Appendix1 For Details**

### 13 RADIATED SPURIOUS EMISSIONS


|                               |  |
|-------------------------------|--|
| <b>Test Standard</b>          | 47 CFR Part 15, Subpart C 15.247       |
| <b>Test Method</b>            | ANSI C63.10 (2013) Section 6.4,6.5,6.6 |
| <b>Test Mode (Pre-Scan)</b>   | TX                                     |
| <b>Test Mode (Final Test)</b> | TX                                     |
| <b>Tester</b>                 | Jozu                                   |
| <b>Temperature</b>            | 25°C                                   |
| <b>Humidity</b>               | 60%                                    |

#### 13.1 LIMITS

| <b>Frequency(MHz)</b> | <b>Field strength(microvolts/meter)</b> | <b>Measurement distance(meters)</b> |
|-----------------------|---|-------------------------------------|
| 0.009-0.490           | 2400/F(kHz)                             | 300                                 |
| 0.490-1.705           | 24000/F(kHz)                            | 30                                  |
| 1.705-30.0            | 30                                      | 30                                  |
| 30-88                 | 100                                     | 3                                   |
| 88-216                | 150                                     | 3                                   |
| 216-960               | 200                                     | 3                                   |
| Above 960             | 500                                     | 3                                   |

Remark: The emission limits shown in the above table are based on measurements employing a CISPR quasi-peak detector except for the frequency bands 9-90kHz, 110-490kHz and above 1000 MHz. Radiated emission limits in these three bands are based on measurements employing an average detector, the peak field strength of any emission shall not exceed the maximum permitted average limits specified above by more than 20 dB under any condition of modulation.

### 13.2 BLOCK DIAGRAM OF TEST SETUP

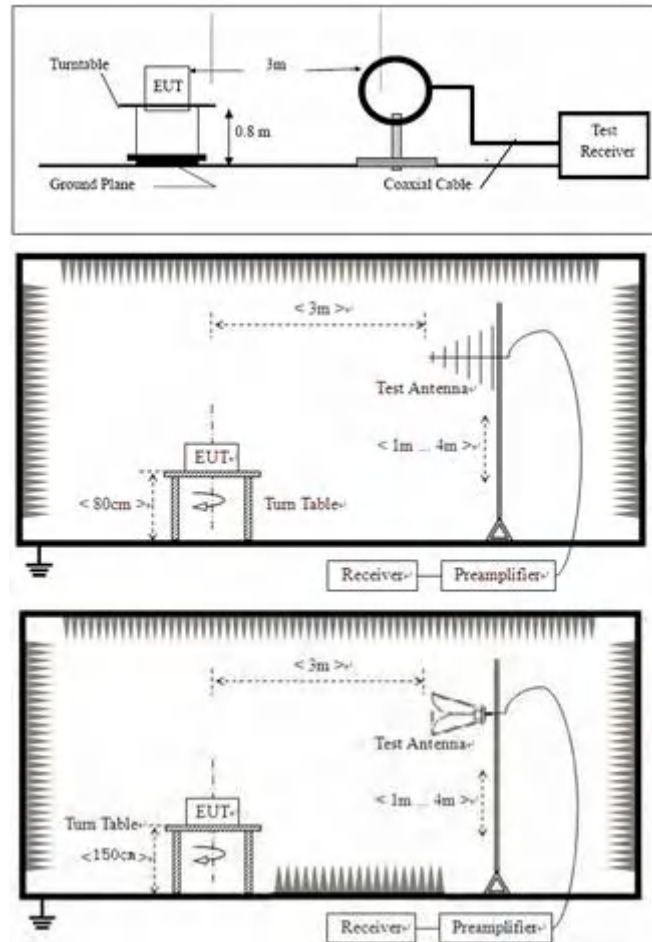

### 13.3 PROCEDURE

- For below 1GHz, the EUT was placed on the top of a rotating table 0.8 meters above the ground at a 3 or 10 meter semi-anechoic chamber. The table was rotated 360 degrees to determine the position of the highest radiation.
- For above 1GHz, the EUT was placed on the top of a rotating table 1.5 meters above the ground at a 3 meter fully-anechoic chamber. The table was rotated 360 degrees to determine the position of the highest radiation.
- The EUT was set 3 or 10 meters away from the interference-receiving antenna, which was mounted on the top of a variable-height antenna tower.
- The antenna height is varied from one meter to four meters above the ground to determine the maximum value of the field strength. Both horizontal and vertical polarizations of the antenna are set to make the measurement.
- For each suspected emission, the EUT was arranged to its worst case and then the antenna was tuned to heights from 1 meter to 4 meters (for the test frequency of below 30MHz, the antenna was tuned to heights 1 meter) and the rotatable table was turned from 0 degrees to 360 degrees to find the maximum reading.
- The test-receiver system was set to Peak Detect Function and Specified Bandwidth with Maximum Hold Mode.
- If the emission level of the EUT in peak mode was 10dB lower than the limit specified, then testing could be stopped and the peak values of the EUT would be reported. Otherwise the emissions that did not have 10dB margin would be re-tested one by one using peak, quasi-peak or average method as specified and then reported in a data sheet.


- h. Test the EUT in the lowest channel, the middle channel, the Highest channel.
- i. The radiation measurements are performed in X, Y, Z axis positioning for Transmitting mode, and found the X axis positioning which it is the worst case.
- j. Repeat above procedures until all frequencies measured was complete.

Remark:

- 1) For emission below 1GHz, through pre-scan found the worst case is the lowest channel. Only the worst case is recorded in the report.
- 2) The field strength is calculated by adding the Antenna Factor, Cable Factor & Preamplifier. The basic equation with a sample calculation is as follows:  
Final Test Level = Receiver Reading + Antenna Factor + Cable Factor - Preamplifier Factor
- 3) Scan from 9kHz to 25GHz, the disturbance above 12.75GHz and below 30MHz was very low. The points marked on above plots are the highest emissions could be found when testing, so only above points had been displayed. The amplitude of spurious emissions from the radiator which are attenuated more than 20dB below the limit need not be reported. fundamental frequency is blocked by filter, and only spurious emission is shown.
- 4) For frequencies above 1GHz, the field strength limits are based on average limits. However, the peak field strength of any emission shall not exceed the maximum permitted average limits specified above by more than 20 dB under any condition of modulation. For the emissions whose peak level is lower than the average limit, only the peak measurement is shown in the report.




[TestMode: TX below 1G]; [Polarity: Vertical]

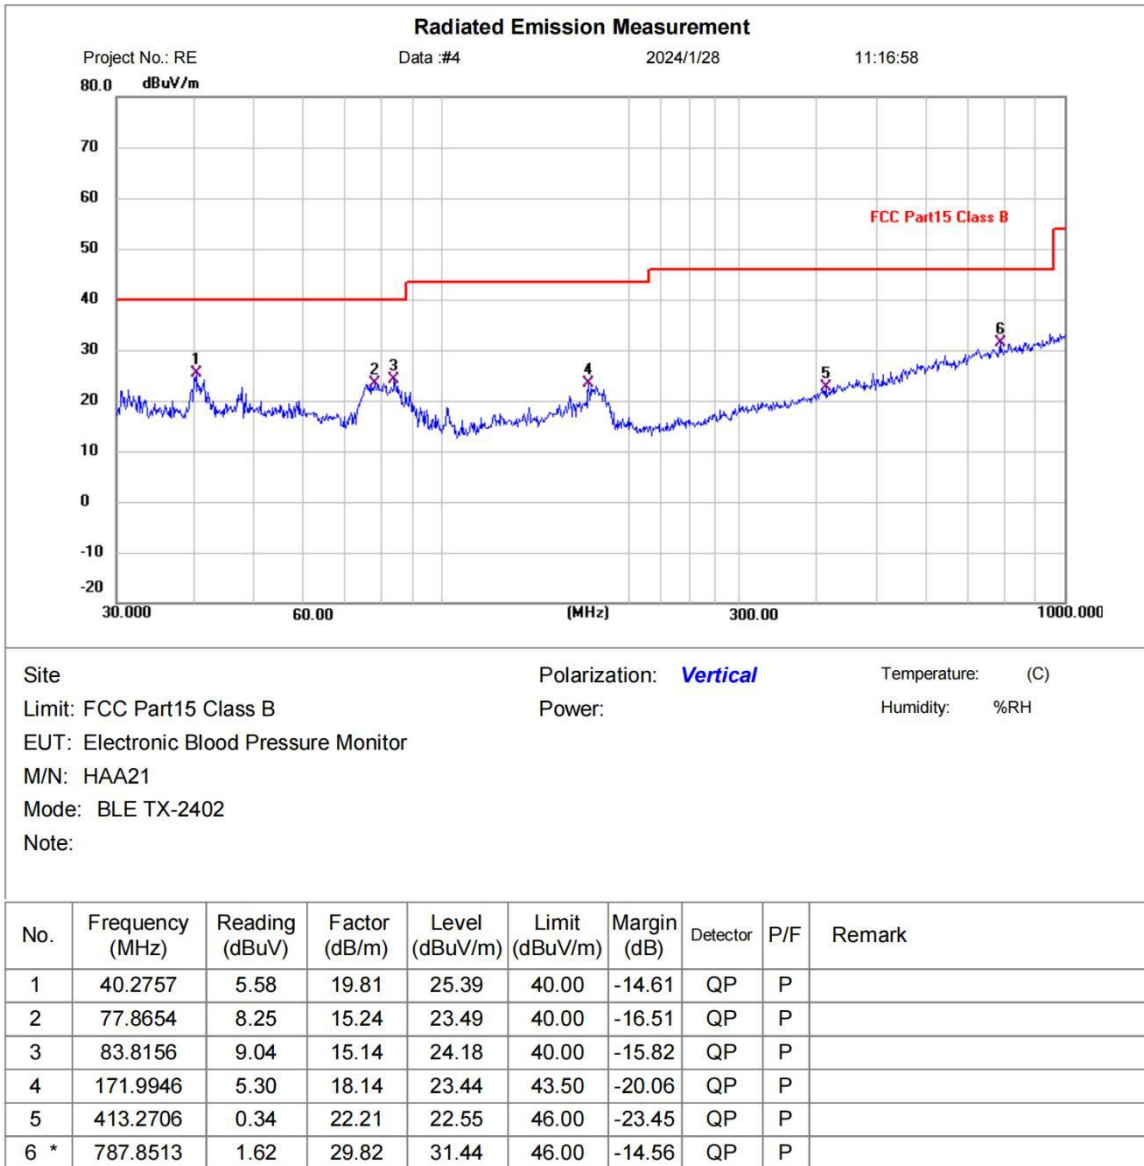

\*:Maximum data    x:Over limit    !:over margin

**Test Result: Pass**

[TestMode: TX low channel]; [Polarity: Horizontal]

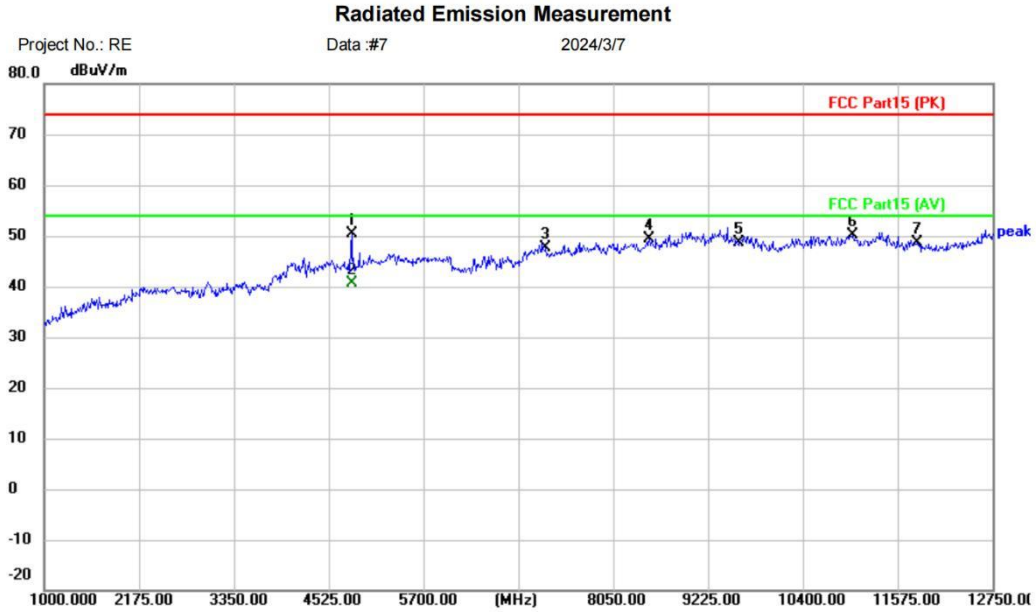

|  |                                 |                  |
|--|---------------------------------|------------------|
| Site                                   | Polarization: <b>Horizontal</b> | Temperature: (C) |
| Limit: FCC Part15 (PK)                 | Power:                          | Humidity: %RH    |
| EUT: Electronic Blood Pressure Monitor |                                 |                  |
| M/N: HAA21                             |                                 |                  |
| Mode: TX-2402                          |                                 |                  |
| Note:                                  |                                 |                  |

| No. | Mk. | Freq.<br>MHz | Reading<br>Level<br>dBuV | Correct<br>Factor<br>dB | Measure-<br>ment<br>dBuV/m | Limit<br>dBuV/m | Over<br>dB | Detector | Comment |
|-----|-----|--------------|--------------------------|-------------------------|----------------------------|-----------------|------------|----------|---------|
| 1   |     | 4807.000     | 44.70                    | 5.64                    | 50.34                      | 74.00           | -23.66     | peak     |         |
| 2   | *   | 4807.000     | 35.00                    | 5.64                    | 40.64                      | 54.00           | -13.36     | AVG      |         |
| 3   |     | 7206.000     | 38.36                    | 9.24                    | 47.60                      | 74.00           | -26.40     | peak     |         |
| 4   |     | 8496.500     | 38.37                    | 10.90                   | 49.27                      | 74.00           | -24.73     | peak     |         |
| 5   |     | 9608.000     | 36.31                    | 12.31                   | 48.62                      | 74.00           | -25.38     | peak     |         |
| 6   |     | 11022.75     | 36.75                    | 13.32                   | 50.07                      | 74.00           | -23.93     | peak     |         |
| 7   |     | 11810.00     | 37.00                    | 11.73                   | 48.73                      | 74.00           | -25.27     | peak     |         |

\*:Maximum data    x:Over limit    !:over margin                      <Reference Only


Receiver: ESR\_1                      Spectrum Analyzer: FSP40

Antenna: EZ 9120D 1G-18G                      Engineer Signature:

**Test Result: Pass**



[TestMode: TX low channel]; [Polarity: Vertical]

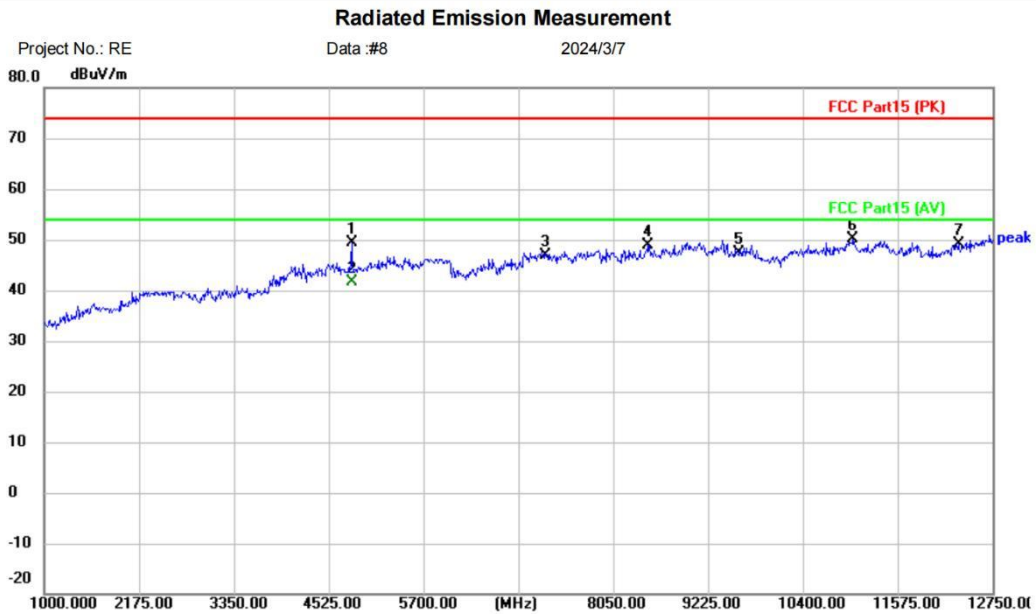

Site:      Polarization: **Vertical**      Temperature: (C)  
 Limit: FCC Part15 (PK)      Power:      Humidity: %RH  
 EUT: Electronic Blood Pressure Monitor  
 M/N: HAA21  
 Mode: TX-2402  
 Note:

| No. | Mk. | Freq.<br>MHz | Reading<br>Level<br>dBuV | Correct<br>Factor<br>dB | Measure-<br>ment<br>dBuV/m | Limit<br>dBuV/m | Over<br>dB | Detector | Comment |
|-----|-----|--------------|--------------------------|-------------------------|----------------------------|-----------------|------------|----------|---------|
| 1   |     | 4807.000     | 43.81                    | 5.64                    | 49.45                      | 74.00           | -24.55     | peak     |         |
| 2   | *   | 4807.000     | 35.93                    | 5.64                    | 41.57                      | 54.00           | -12.43     | AVG      |         |
| 3   |     | 7206.000     | 37.73                    | 9.24                    | 46.97                      | 74.00           | -27.03     | peak     |         |
| 4   |     | 8484.750     | 38.10                    | 10.84                   | 48.94                      | 74.00           | -25.06     | peak     |         |
| 5   |     | 9608.000     | 35.06                    | 12.31                   | 47.37                      | 74.00           | -26.63     | peak     |         |
| 6   |     | 11022.75     | 36.84                    | 13.32                   | 50.16                      | 74.00           | -23.84     | peak     |         |
| 7   |     | 12327.00     | 36.99                    | 12.13                   | 49.12                      | 74.00           | -24.88     | peak     |         |


\*:Maximum data    x:Over limit    !:over margin      (Reference Only)

Receiver:      ESR\_1      Spectrum Analyzer:      FSP40  
 Antenna:      EZ 9120D 1G-18G      Engineer Signature:

**Test Result: Pass**



[TestMode: TX mid channel]; [Polarity: Horizontal]

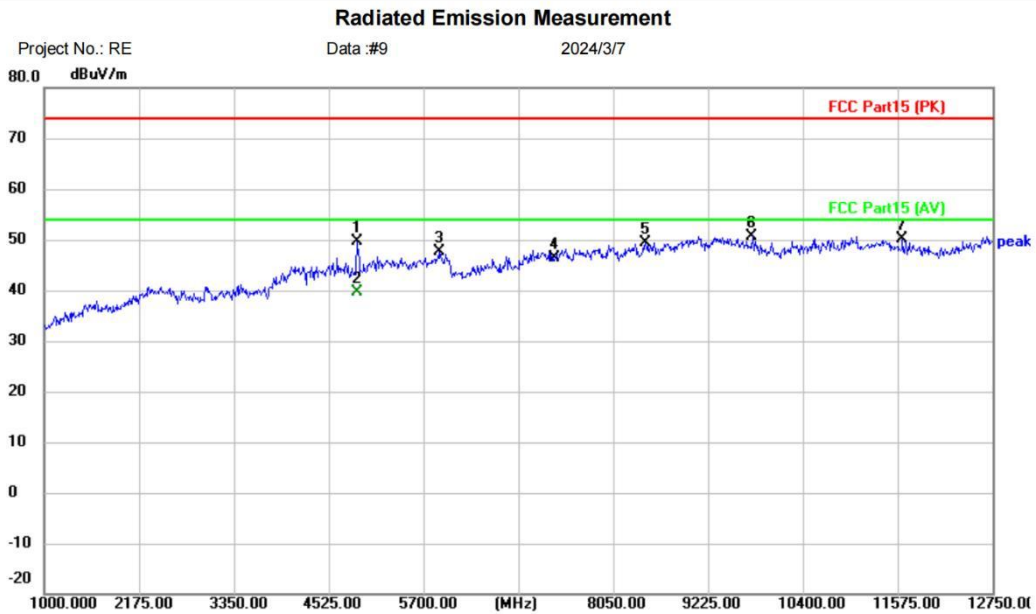

Site:      Polarization: **Horizontal**      Temperature: (C)  
 Limit: FCC Part15 (PK)      Power:      Humidity: %RH  
 EUT: Electronic Blood Pressure Monitor  
 M/N: HAA21  
 Mode: TX-2442  
 Note:


| No. | Mk. | Freq.<br>MHz | Reading<br>Level<br>dBuV | Correct<br>Factor<br>dB | Measure-<br>ment<br>dBuV/m | Limit<br>dBuV/m | Over<br>dB | Detector | Comment |
|-----|-----|--------------|--------------------------|-------------------------|----------------------------|-----------------|------------|----------|---------|
| 1   |     | 4877.500     | 43.86                    | 5.72                    | 49.58                      | 74.00           | -24.42     | peak     |         |
| 2   | *   | 4877.500     | 33.94                    | 5.72                    | 39.66                      | 54.00           | -14.34     | AVG      |         |
| 3   |     | 5888.000     | 38.98                    | 8.60                    | 47.58                      | 74.00           | -26.42     | peak     |         |
| 4   |     | 7326.000     | 36.98                    | 9.43                    | 46.41                      | 74.00           | -27.59     | peak     |         |
| 5   |     | 8449.500     | 38.65                    | 10.63                   | 49.28                      | 74.00           | -24.72     | peak     |         |
| 6   |     | 9768.000     | 38.39                    | 12.22                   | 50.61                      | 74.00           | -23.39     | peak     |         |
| 7   |     | 11633.75     | 38.03                    | 12.03                   | 50.06                      | 74.00           | -23.94     | peak     |         |

\*:Maximum data    x:Over limit    !:over margin      (Reference Only)

Receiver:      ESR\_1      Spectrum Analyzer:      FSP40  
 Antenna:      EZ 9120D 1G-18G      Engineer Signature:

**Test Result: Pass**

[TestMode: TX mid channel]; [Polarity: Vertical]

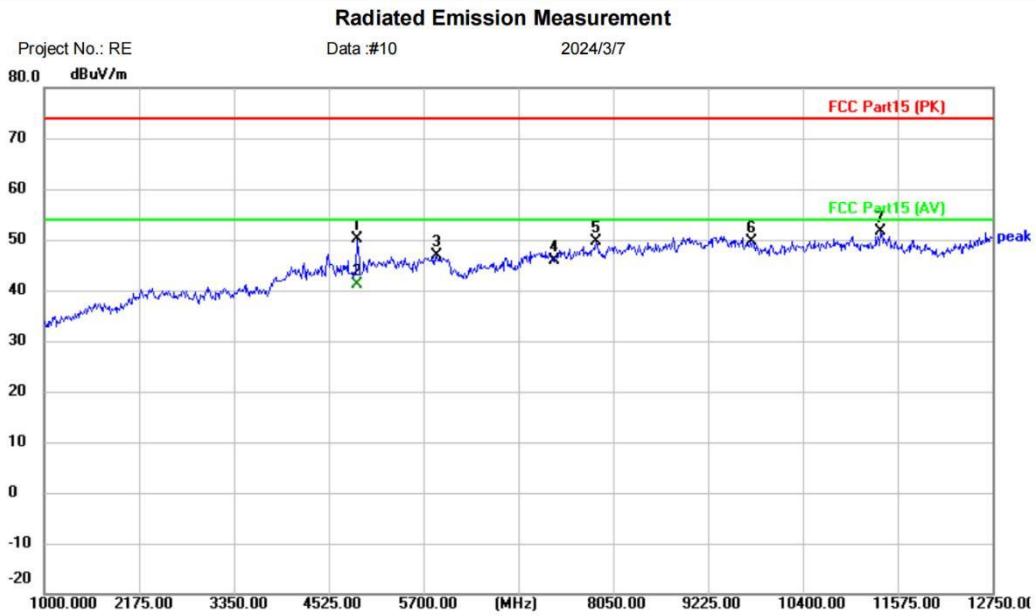

Site:      Polarization: **Vertical**      Temperature: (C)  
 Limit: FCC Part15 (PK)      Power:      Humidity: %RH  
 EUT: Electronic Blood Pressure Monitor  
 M/N: HAA21  
 Mode: TX-2442  
 Note:

| No. | Mk. | Freq.<br>MHz | Reading<br>Level<br>dBuV | Correct<br>Factor<br>dB | Measure-<br>ment<br>dBuV/m | Limit<br>dBuV/m | Over<br>dB | Detector | Comment |
|-----|-----|--------------|--------------------------|-------------------------|----------------------------|-----------------|------------|----------|---------|
| 1   |     | 4877.500     | 44.32                    | 5.72                    | 50.04                      | 74.00           | -23.96     | peak     |         |
| 2   | *   | 4877.500     | 35.42                    | 5.72                    | 41.14                      | 54.00           | -12.86     | AVG      |         |
| 3   |     | 5864.500     | 38.51                    | 8.48                    | 46.99                      | 74.00           | -27.01     | peak     |         |
| 4   |     | 7326.000     | 36.57                    | 9.43                    | 46.00                      | 74.00           | -28.00     | peak     |         |
| 5   |     | 7838.500     | 39.80                    | 9.86                    | 49.66                      | 74.00           | -24.34     | peak     |         |
| 6   |     | 9768.000     | 37.47                    | 12.22                   | 49.69                      | 74.00           | -24.31     | peak     |         |
| 7   |     | 11363.50     | 38.95                    | 12.65                   | 51.60                      | 74.00           | -22.40     | peak     |         |


\*:Maximum data    x:Over limit    !:over margin      (Reference Only)

Receiver: ESR\_1      Spectrum Analyzer: FSP40

Antenna: EZ 9120D 1G-18G      Engineer Signature:

**Test Result: Pass**

[TestMode: TX high channel]; [Polarity: Horizontal]

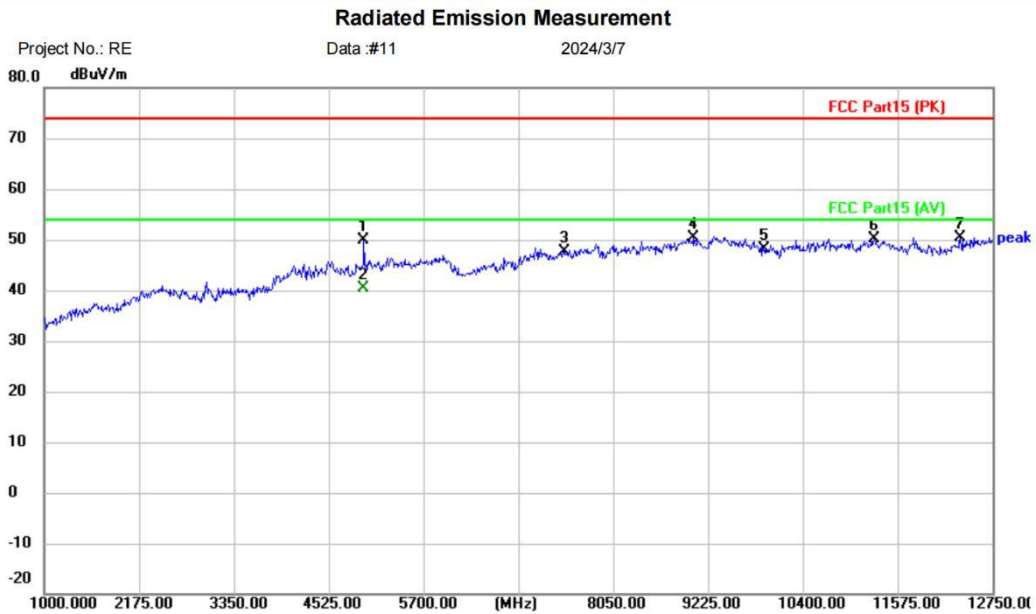

Site:      Polarization: **Horizontal**      Temperature: (C)  
 Limit: FCC Part15 (PK)      Power:      Humidity: %RH  
 EUT: Electronic Blood Pressure Monitor  
 M/N: HAA21  
 Mode: TX-2480  
 Note:


| No. | Mk. | Freq.<br>MHz | Reading<br>Level<br>dBuV | Correct<br>Factor<br>dB | Measure-<br>ment<br>dBuV/m | Limit<br>dBuV/m | Over<br>dB | Detector | Comment |
|-----|-----|--------------|--------------------------|-------------------------|----------------------------|-----------------|------------|----------|---------|
| 1   |     | 4959.750     | 43.30                    | 6.60                    | 49.90                      | 74.00           | -24.10     | peak     |         |
| 2   | *   | 4959.750     | 33.77                    | 6.60                    | 40.37                      | 54.00           | -13.63     | AVG      |         |
| 3   |     | 7440.000     | 37.91                    | 9.64                    | 47.55                      | 74.00           | -26.45     | peak     |         |
| 4   |     | 9048.750     | 38.24                    | 12.12                   | 50.36                      | 74.00           | -23.64     | peak     |         |
| 5   |     | 9920.000     | 36.02                    | 12.14                   | 48.16                      | 74.00           | -25.84     | peak     |         |
| 6   |     | 11281.25     | 37.35                    | 12.70                   | 50.05                      | 74.00           | -23.95     | peak     |         |
| 7   |     | 12350.50     | 38.27                    | 12.15                   | 50.42                      | 74.00           | -23.58     | peak     |         |

\*:Maximum data    x:Over limit    !:over margin      (Reference Only)

Receiver:      ESR\_1      Spectrum Analyzer:      FSP40  
 Antenna:      EZ 9120D 1G-18G      Engineer Signature:

**Test Result: Pass**

[TestMode: TX high channel]; [Polarity: Vertical]

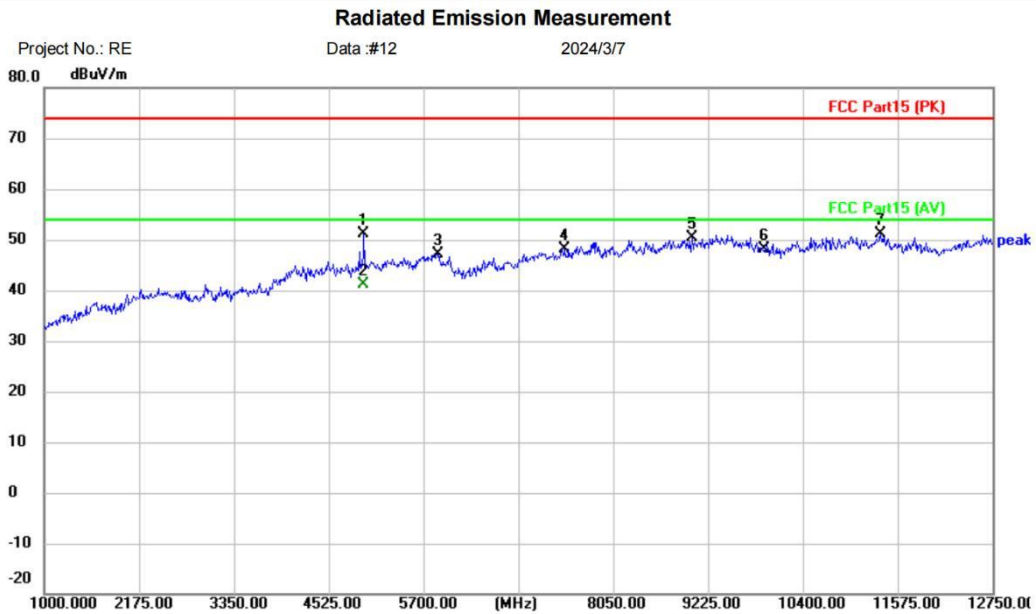

Site:      Polarization: **Vertical**      Temperature: (C)  
 Limit: FCC Part15 (PK)      Power:      Humidity: %RH  
 EUT: Electronic Blood Pressure Monitor  
 M/N: HAA21  
 Mode: TX-2480  
 Note:

| No. | Mk. | Freq.<br>MHz | Reading<br>Level<br>dBuV | Correct<br>Factor<br>dB | Measure-<br>ment<br>dBuV/m | Limit<br>dBuV/m | Over<br>dB | Detector | Comment |
|-----|-----|--------------|--------------------------|-------------------------|----------------------------|-----------------|------------|----------|---------|
| 1   |     | 4959.750     | 44.42                    | 6.60                    | 51.02                      | 74.00           | -22.98     | peak     |         |
| 2   | *   | 4959.750     | 34.48                    | 6.60                    | 41.08                      | 54.00           | -12.92     | AVG      |         |
| 3   |     | 5876.250     | 38.67                    | 8.54                    | 47.21                      | 74.00           | -26.79     | peak     |         |
| 4   |     | 7440.000     | 38.50                    | 9.64                    | 48.14                      | 74.00           | -25.86     | peak     |         |
| 5   |     | 9025.250     | 38.12                    | 12.28                   | 50.40                      | 74.00           | -23.60     | peak     |         |
| 6   |     | 9920.000     | 36.11                    | 12.14                   | 48.25                      | 74.00           | -25.75     | peak     |         |
| 7   |     | 11363.50     | 38.50                    | 12.65                   | 51.15                      | 74.00           | -22.85     | peak     |         |

\*:Maximum data    x:Over limit    !:over margin      (Reference Only)

Receiver:      ESR\_1      Spectrum Analyzer:      FSP40  
 Antenna:      EZ 9120D 1G-18G      Engineer Signature:

**Test Result: Pass**

Remark:

1. Final Level = Receiver Read level + Correct factor
2. Correct factor = Antenna Factor + Cable Loss – Preamplifier Factor
3. The emission levels of other frequencies are very lower than the limit and not show in test report.

BlueAsia

## 14 RADIATED EMISSIONS WHICH FALL IN THE RESTRICTED BANDS


|                               |                                   |
|-------------------------------|-----------------------------------|
| <b>Test Standard</b>          | 47 CFR Part 15, Subpart C 15.247  |
| <b>Test Method</b>            | ANSI C63.10 (2013) Section 6.10.5 |
| <b>Test Mode (Pre-Scan)</b>   | TX                                |
| <b>Test Mode (Final Test)</b> | TX                                |
| <b>Tester</b>                 | Jozu                              |
| <b>Temperature</b>            | 25°C                              |
| <b>Humidity</b>               | 60%                               |

### 14.1 LIMITS

| <b>Frequency(MHz)</b> | <b>Field strength(microvolts/meter)</b> | <b>Measurement distance(meters)</b> |
|-----------------------|---|-------------------------------------|
| 0.009-0.490           | 2400/F(kHz)                             | 300                                 |
| 0.490-1.705           | 24000/F(kHz)                            | 30                                  |
| 1.705-30.0            | 30                                      | 30                                  |
| 30-88                 | 100                                     | 3                                   |
| 88-216                | 150                                     | 3                                   |
| 216-960               | 200                                     | 3                                   |
| Above 960             | 500                                     | 3                                   |

Remark: The emission limits shown in the above table are based on measurements employing a CISPR quasi-peak detector except for the frequency bands 9-90kHz, 110-490kHz and above 1000 MHz. Radiated emission limits in these three bands are based on measurements employing an average detector, the peak field strength of any emission shall not exceed the maximum permitted average limits specified above by more than 20 dB under any condition of modulation.

## 14.2 BLOCK DIAGRAM OF TEST SETUP

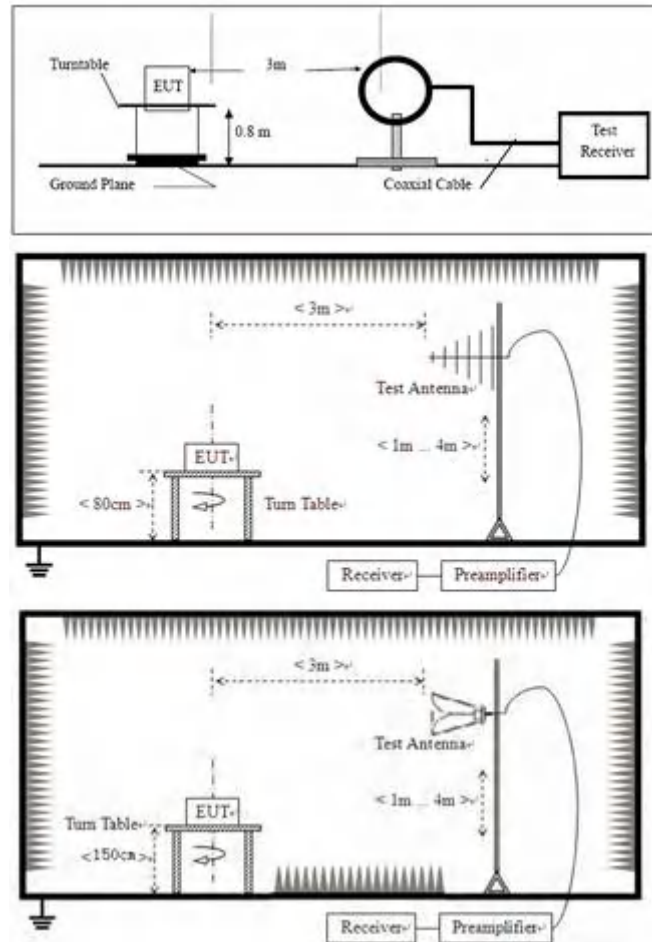

## 14.3 PROCEDURE

- For below 1GHz, the EUT was placed on the top of a rotating table 0.8 meters above the ground at a 3 or 10 meter semi-anechoic chamber. The table was rotated 360 degrees to determine the position of the highest radiation.
- For above 1GHz, the EUT was placed on the top of a rotating table 1.5 meters above the ground at a 3 meter fully-anechoic chamber. The table was rotated 360 degrees to determine the position of the highest radiation.
- The EUT was set 3 or 10 meters away from the interference-receiving antenna, which was mounted on the top of a variable-height antenna tower.
- The antenna height is varied from one meter to four meters above the ground to determine the maximum value of the field strength. Both horizontal and vertical polarizations of the antenna are set to make the measurement.
- For each suspected emission, the EUT was arranged to its worst case and then the antenna was tuned to heights from 1 meter to 4 meters (for the test frequency of below 30MHz, the antenna was tuned to heights 1 meter) and the rotatable table was turned from 0 degrees to 360 degrees to find the maximum reading.
- The test-receiver system was set to Peak Detect Function and Specified Bandwidth with Maximum Hold Mode.
- If the emission level of the EUT in peak mode was 10dB lower than the limit specified, then testing could be stopped and the peak values of the EUT would be reported. Otherwise the emissions that did not have 10dB margin would be re-tested one by one using peak, quasi-peak or average method as specified and then reported in a data sheet.



- h. Test the EUT in the lowest channel, the middle channel, the Highest channel.
- i. The radiation measurements are performed in X, Y, Z axis positioning for Transmitting mode, and found the X axis positioning which it is the worst case.
- j. Repeat above procedures until all frequencies measured was complete.

Remark 1:  $Level = Read\ Level + Cable\ Loss + Antenna\ Factor - Preamp\ Factor$


Remark 2: For frequencies above 1GHz, the field strength limits are based on average limits. However, the peak field strength of any emission shall not exceed the maximum permitted average limits specified above by more than 20 dB under any condition of modulation. For the emissions whose peak level is lower than the average limit, only the peak measurement is shown in the report.

BlueAsia



### 14.4 TEST DATA

[TestMode: TX low channel]; [Polarity: Horizontal]

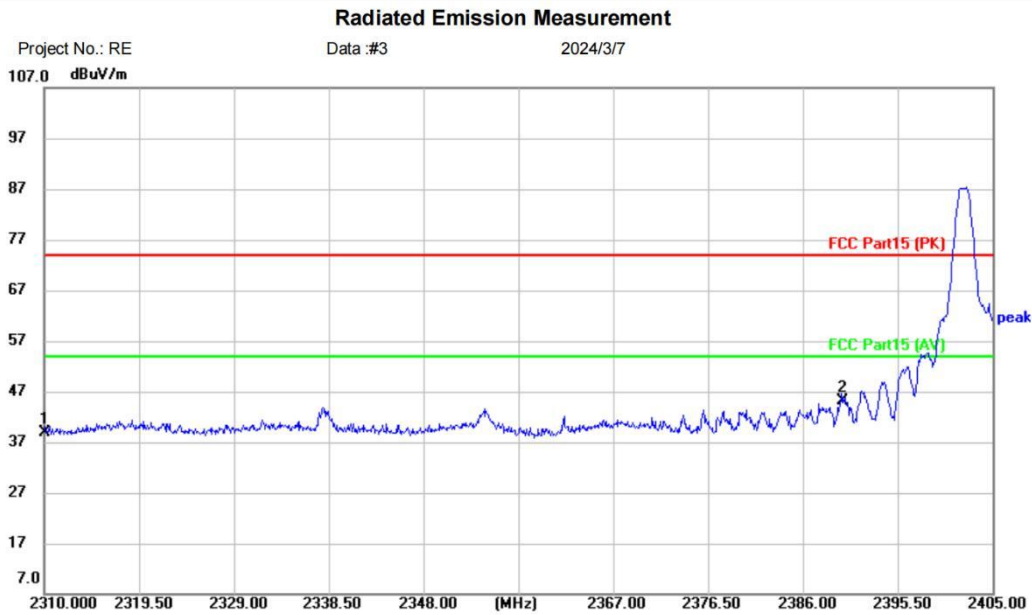

|  |                                 |                  |
|--|---------------------------------|------------------|
| Site                                   | Polarization: <b>Horizontal</b> | Temperature: (C) |
| Limit: FCC Part15 (PK)                 | Power:                          | Humidity: %RH    |
| EUT: Electronic Blood Pressure Monitor |                                 |                  |
| M/N: HAA21                             |                                 |                  |
| Mode: TX-2402                          |                                 |                  |
| Note:                                  |                                 |                  |

| No. | Mk. | Freq.    | Reading Level | Correct Factor | Measurement | Limit  | Over   | Detector | Comment |
|-----|-----|----------|---------------|----------------|-------------|--------|--------|----------|---------|
|     |     | MHz      | dBuV          | dB             | dBuV/m      | dBuV/m | dB     |          |         |
| 1   |     | 2310.000 | 41.76         | -2.89          | 38.87       | 74.00  | -35.13 | peak     |         |
| 2   | *   | 2390.000 | 47.86         | -2.70          | 45.16       | 74.00  | -28.84 | peak     |         |


\*:Maximum data    x:Over limit    !:over margin                      (Reference Only)

Receiver:            ESR\_1                      Spectrum Analyzer:            FSP40

Antenna:            EZ 9120D 1G-18G            Engineer Signature:

**Test Result: Pass**

[TestMode: TX low channel]; [Polarity: Vertical]

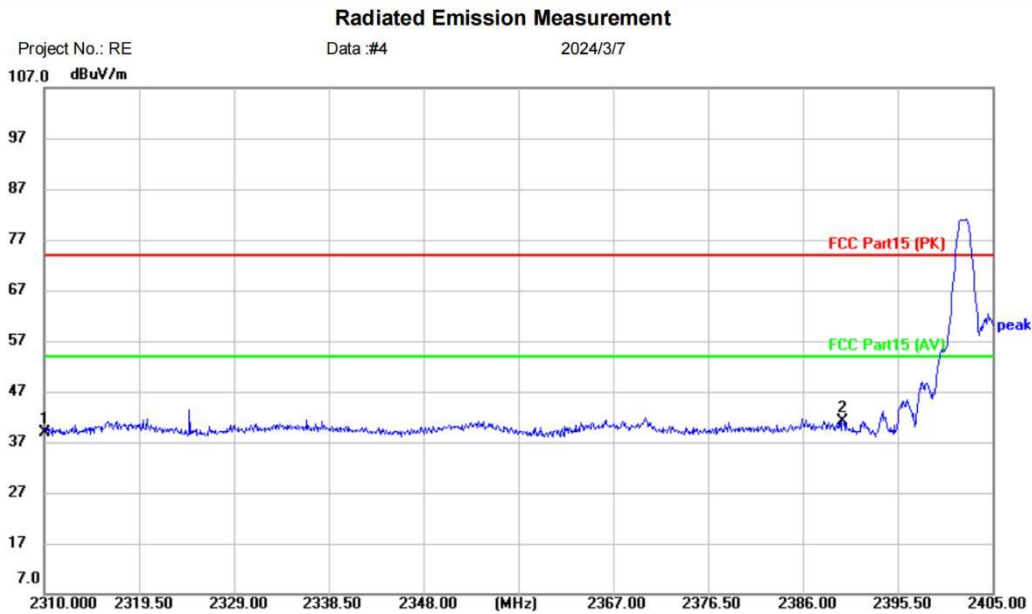

|  |                               |                  |
|--|-------------------------------|------------------|
| Site                                   | Polarization: <b>Vertical</b> | Temperature: (C) |
| Limit: FCC Part15 (PK)                 | Power:                        | Humidity: %RH    |
| EUT: Electronic Blood Pressure Monitor |                               |                  |
| M/N: HAA21                             |                               |                  |
| Mode: TX-2402                          |                               |                  |
| Note:                                  |                               |                  |

| No. | Mk. | Freq.    | Reading Level | Correct Factor | Measurement | Limit  | Over   | Detector | Comment |
|-----|-----|----------|---------------|----------------|-------------|--------|--------|----------|---------|
|     |     | MHz      | dBuV          | dB             | dBuV/m      | dBuV/m | dB     |          |         |
| 1   |     | 2310.000 | 41.79         | -2.89          | 38.90       | 74.00  | -35.10 | peak     |         |
| 2   | *   | 2390.000 | 43.80         | -2.70          | 41.10       | 74.00  | -32.90 | peak     |         |


\*:Maximum data    x:Over limit    !:over margin      (Reference Only)

Receiver:      ESR\_1      Spectrum Analyzer:      FSP40

Antenna:      EZ 9120D 1G-18G      Engineer Signature:

**Test Result: Pass**

[TestMode: TX high channel]; [Polarity: Horizontal]

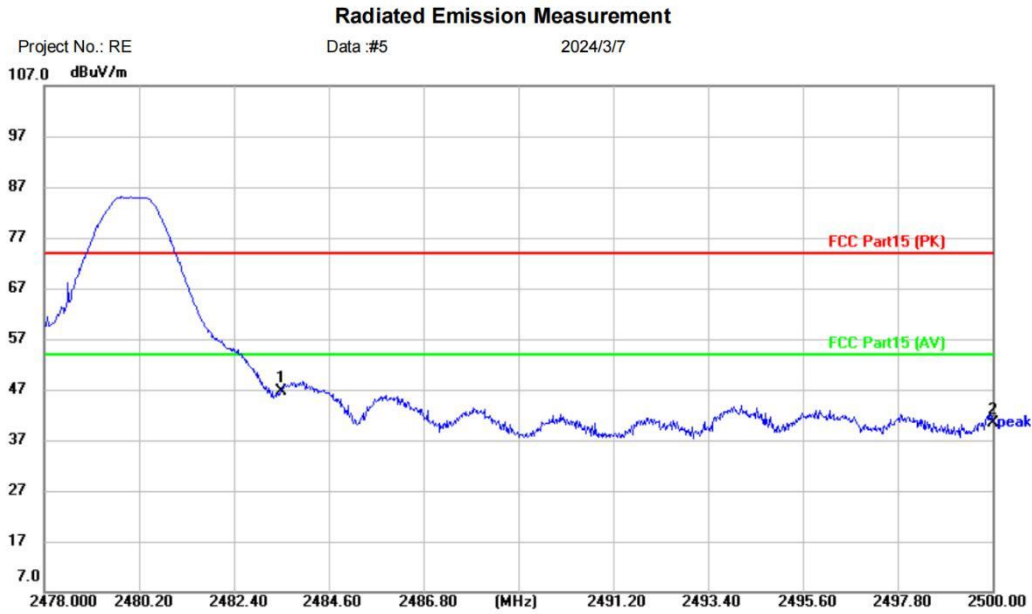

Site:      Polarization: **Horizontal**      Temperature: (C)  
 Limit: FCC Part15 (PK)      Power:      Humidity: %RH  
 EUT: Electronic Blood Pressure Monitor  
 M/N: HAA21  
 Mode: TX-2480  
 Note:


| No. | Mk. | Freq.<br>MHz | Reading<br>Level<br>dBuV | Correct<br>Factor<br>dB | Measure-<br>ment<br>dBuV/m | Limit<br>dBuV/m | Over<br>dB | Detector | Comment |
|-----|-----|--------------|--------------------------|-------------------------|----------------------------|-----------------|------------|----------|---------|
| 1   | *   | 2483.500     | 49.43                    | -2.91                   | 46.52                      | 74.00           | -27.48     | peak     |         |
| 2   |     | 2500.000     | 43.46                    | -3.00                   | 40.46                      | 74.00           | -33.54     | peak     |         |

\*:Maximum data    x:Over limit    !:over margin      (Reference Only)

Receiver:      ESR\_1      Spectrum Analyzer:      FSP40  
 Antenna:      EZ 9120D 1G-18G      Engineer Signature:

**Test Result: Pass**

[TestMode: TX high channel]; [Polarity: Vertical]

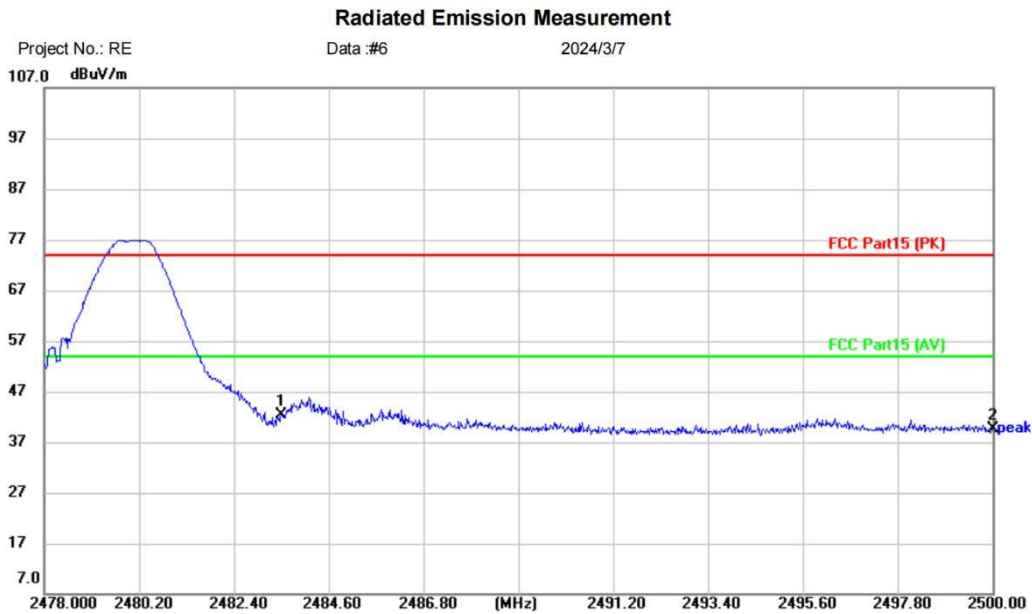

Site:      Polarization: **Vertical**      Temperature: (C)  
 Limit: FCC Part15 (PK)      Power:      Humidity: %RH  
 EUT: Electronic Blood Pressure Monitor  
 M/N: HAA21  
 Mode: TX-2480  
 Note:

| No. | Mk. | Freq.<br>MHz | Reading<br>Level<br>dBuV | Correct<br>Factor<br>dB | Measure-<br>ment<br>dBuV/m | Limit<br>dBuV/m | Over<br>dB | Detector | Comment |
|-----|-----|--------------|--------------------------|-------------------------|----------------------------|-----------------|------------|----------|---------|
| 1   | *   | 2483.500     | 45.27                    | -2.91                   | 42.36                      | 74.00           | -31.64     | peak     |         |
| 2   |     | 2500.000     | 42.52                    | -3.00                   | 39.52                      | 74.00           | -34.48     | peak     |         |

\*:Maximum data    x:Over limit    !:over margin      (Reference Only)

Receiver:      ESR\_1      Spectrum Analyzer:      FSP40  
 Antenna:      EZ 9120D 1G-18G      Engineer Signature:

**Test Result: Pass**

Remark:

1. Final Level = Receiver Read level + Correct factor
2. Correct factor = Antenna Factor + Cable Loss – Preamplifier Factor
3. The emission levels of other frequencies are very lower than the limit and not show in test report.

BlueAsia


## 15 CONDUCTED SPURIOUS EMISSIONS

|                               |  |
|-------------------------------|--|
| <b>Test Standard</b>          | 47 CFR Part 15, Subpart C 15.247                 |
| <b>Test Method</b>            | ANSI C63.10 (2013) Section 7.8.6 & Section 11.11 |
| <b>Test Mode (Pre-Scan)</b>   | TX   |
| <b>Test Mode (Final Test)</b> | TX   |
| <b>Tester</b>                 | Jozu   |
| <b>Temperature</b>            | 25°C   |
| <b>Humidity</b>               | 60%  |

### 15.1 LIMITS

|               |   |
|---------------|---|
| <b>Limit:</b> | <p>In any 100 kHz bandwidth outside the frequency band in which the spread spectrum or digitally modulated intentional radiator is operating, the radio frequency power that is produced by the intentional radiator shall be at least 20 dB below that in the 100 kHz bandwidth within the band that contains the highest level of the desired power, based on either an RF conducted or a radiated measurement, provided the transmitter demonstrates compliance with the peak conducted power limits. If the transmitter complies with the conducted power limits based on the use of RMS averaging over a time interval, as permitted under paragraph (b)(3) of this section, the attenuation required under this paragraph shall be 30 dB instead of 20 dB. Attenuation below the general limits specified in §15.209(a) is not required. In addition, radiated emissions which fall in the restricted bands, as defined in §15.205(a), must also comply with the radiated emission limits specified in §15.209(a) (see §15.205(c)).</p> |
|---------------|---|

### 15.2 BLOCK DIAGRAM OF TEST SETUP

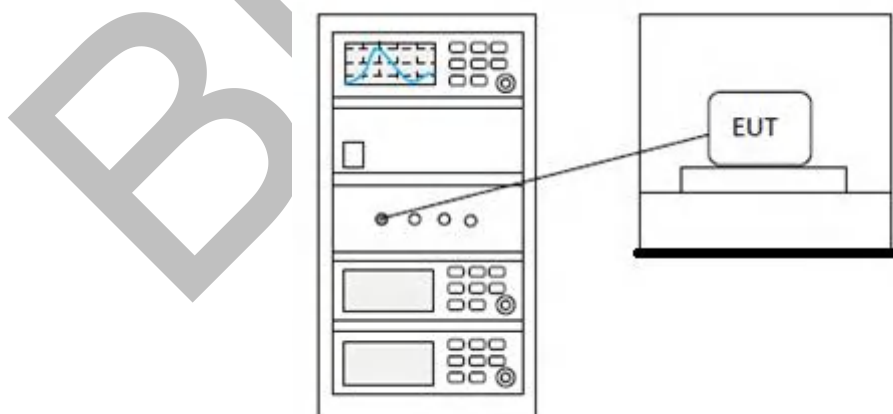

### 15.3 TEST DATA

**Pass: Please Refer To Appendix: Appendix1 For Details**


## 16 POWER SPECTRUM DENSITY

|                        |                                    |
|------------------------|------------------------------------|
| Test Standard          | 47 CFR Part 15, Subpart C 15.247   |
| Test Method            | ANSI C63.10 (2013) Section 11.10.2 |
| Test Mode (Pre-Scan)   | TX                                 |
| Test Mode (Final Test) | TX                                 |
| Tester                 | Jozu                               |
| Temperature            | 25°C                               |
| Humidity               | 60%                                |

### 16.1 LIMITS

**Limit:**  $\leq 8\text{dBm}$  in any 3 kHz band during any time interval of continuous transmission

### 16.2 BLOCK DIAGRAM OF TEST SETUP

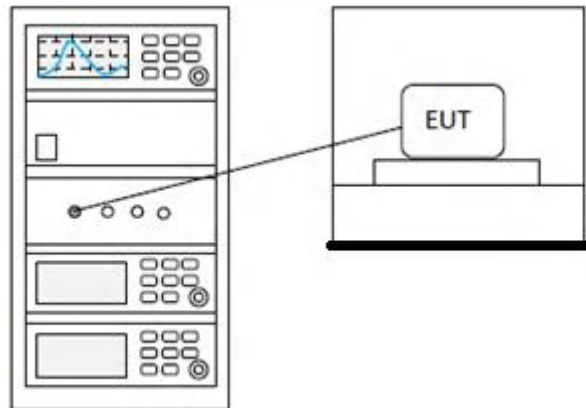

### 16.3 TEST DATA

**Pass: Please Refer To Appendix: Appendix1 For Details**


## 17 CONDUCTED PEAK OUTPUT POWER

|                               |                                  |
|-------------------------------|----------------------------------|
| <b>Test Standard</b>          | 47 CFR Part 15, Subpart C 15.247 |
| <b>Test Method</b>            | ANSI C63.10 (2013) Section 7.8.5 |
| <b>Test Mode (Pre-Scan)</b>   | TX                               |
| <b>Test Mode (Final Test)</b> | TX                               |
| <b>Tester</b>                 | Jozu                             |
| <b>Temperature</b>            | 25°C                             |
| <b>Humidity</b>               | 60%                              |

### 17.1 LIMITS

| Frequency range(MHz) | Output power of the intentional radiator(watt)         |
|----------------------|--|
| 902-928              | 1 for $\geq 50$ hopping channels                       |
|                      | 0.25 for $25 \leq$ hopping channels $< 50$             |
|                      | 1 for digital modulation                               |
| 2400-2483.5          | 1 for $\geq 75$ non-overlapping hopping channels       |
|                      | 0.125 for all other frequency hopping systems          |
|                      | 1 for digital modulation                               |
| 5725-5850            | 1 for frequency hopping systems and digital modulation |

### 17.2 BLOCK DIAGRAM OF TEST SETUP

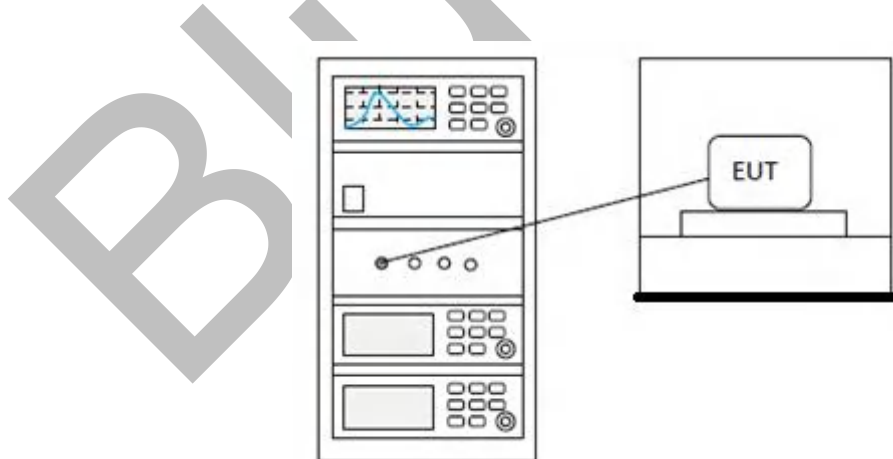

### 17.3 TEST DATA

**Pass: Please Refer To Appendix: Appendix1 For Details**




## 18 MINIMUM 6DB BANDWIDTH

|                        |                                   |
|------------------------|-----------------------------------|
| Test Standard          | 47 CFR Part 15, Subpart C 15.247  |
| Test Method            | ANSI C63.10 (2013) Section 11.8.1 |
| Test Mode (Pre-Scan)   | TX                                |
| Test Mode (Final Test) | TX                                |
| Tester                 | Jozu                              |
| Temperature            | 25°C                              |
| Humidity               | 60%                               |

### 18.1 LIMITS

|        |                |
|--------|----------------|
| Limit: | $\geq 500$ kHz |
|--------|----------------|

### 18.2 BLOCK DIAGRAM OF TEST SETUP

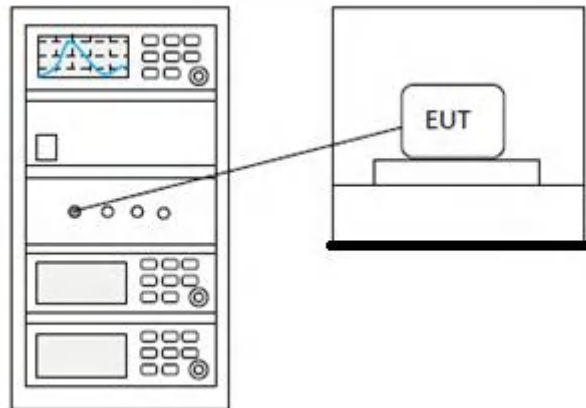

### 18.3 TEST DATA

**Pass: Please Refer To Appendix: Appendix1 For Details**

## 19 ANTENNA REQUIREMENT

|               |                                  |
|---------------|----------------------------------|
| Test Standard | 47 CFR Part 15, Subpart C 15.247 |
| Test Method   | N/A                              |

### 19.1 CONCLUSION

Standard Requirement:

An intentional radiator shall be designed to ensure that no antenna other than that furnished by the responsible party shall be used with the device. The use of an antenna that uses a unique coupling to the intentional radiator, the manufacturer may design the unit permanently attached antenna or of an so that a broken antenna can be replaced by the user, but the use of a standard antenna jack or electrical connector is prohibited.

EUT Antenna:


The best case gain of the antenna is 0dBi.

## 20 APPENDIX1


### Maximum Conducted Output Power

| Condition | Mode | Frequency (MHz) | Antenna | Conducted Power (dBm) | Limit (dBm) | Verdict |
|-----------|------|-----------------|---------|-----------------------|-------------|---------|
| NVNT      | BLE  | 2402            | Ant1    | -2.92                 | 30          | Pass    |
| NVNT      | BLE  | 2442            | Ant1    | -3.649                | 30          | Pass    |
| NVNT      | BLE  | 2480            | Ant1    | -3.424                | 30          | Pass    |


Power NVNT BLE 2402MHz Ant1

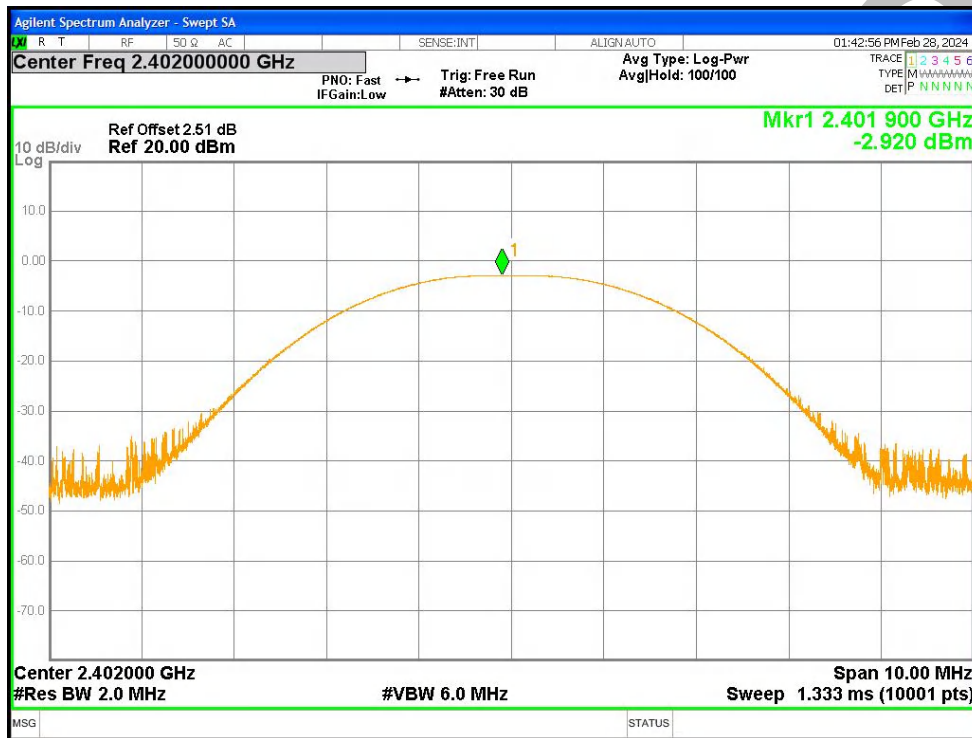

Power NVNT BLE 2442MHz Ant1

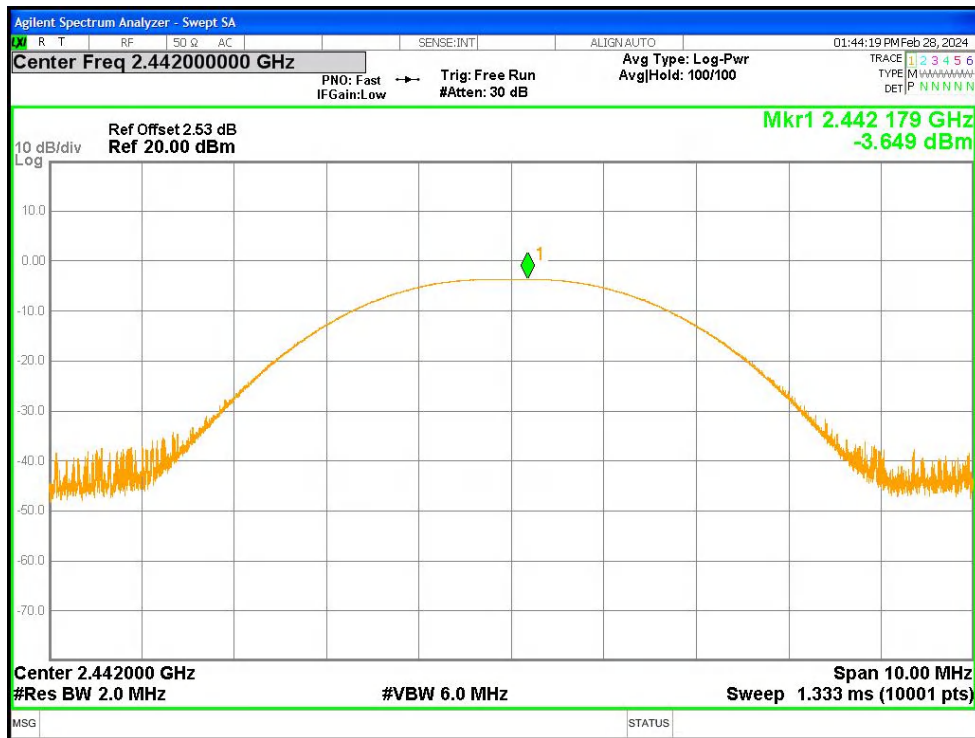



Power NVNT BLE 2480MHz Ant1

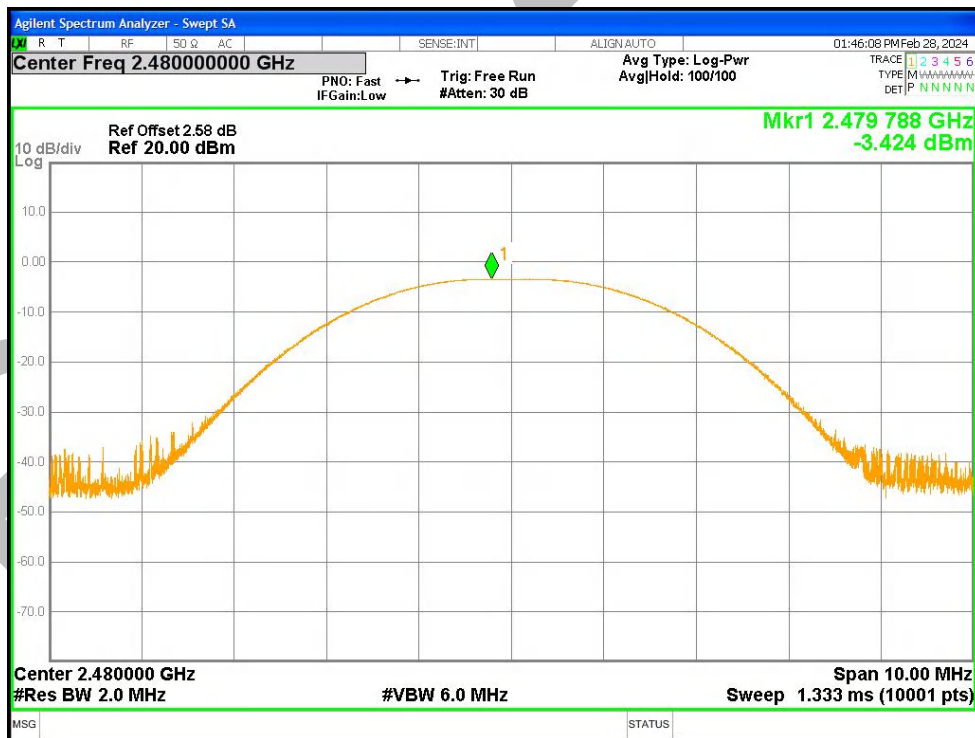


**-6dB Bandwidth**

| Condition | Mode | Frequency (MHz) | Antenna | -6 dB Bandwidth (MHz) | Limit -6 dB Bandwidth (MHz) | Verdict |
|-----------|------|-----------------|---------|-----------------------|-----------------------------|---------|
| NVNT      | BLE  | 2402            | Ant1    | 0.673                 | 0.5                         | Pass    |
| NVNT      | BLE  | 2442            | Ant1    | 0.675                 | 0.5                         | Pass    |
| NVNT      | BLE  | 2480            | Ant1    | 0.697                 | 0.5                         | Pass    |

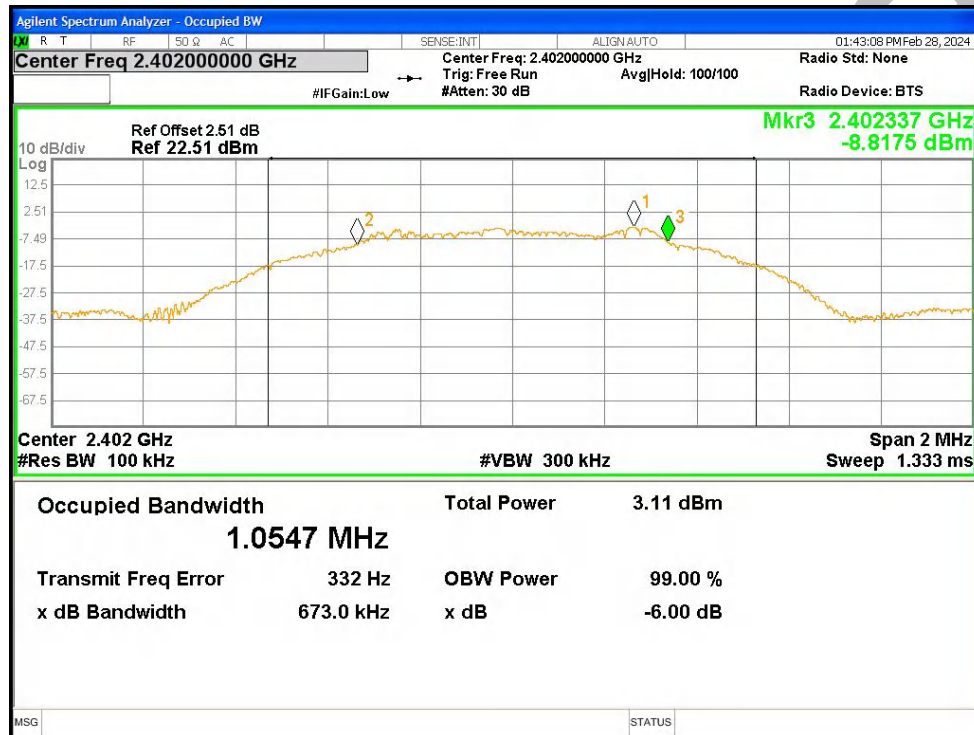**-6dB Bandwidth NVNT BLE 2402MHz Ant1**

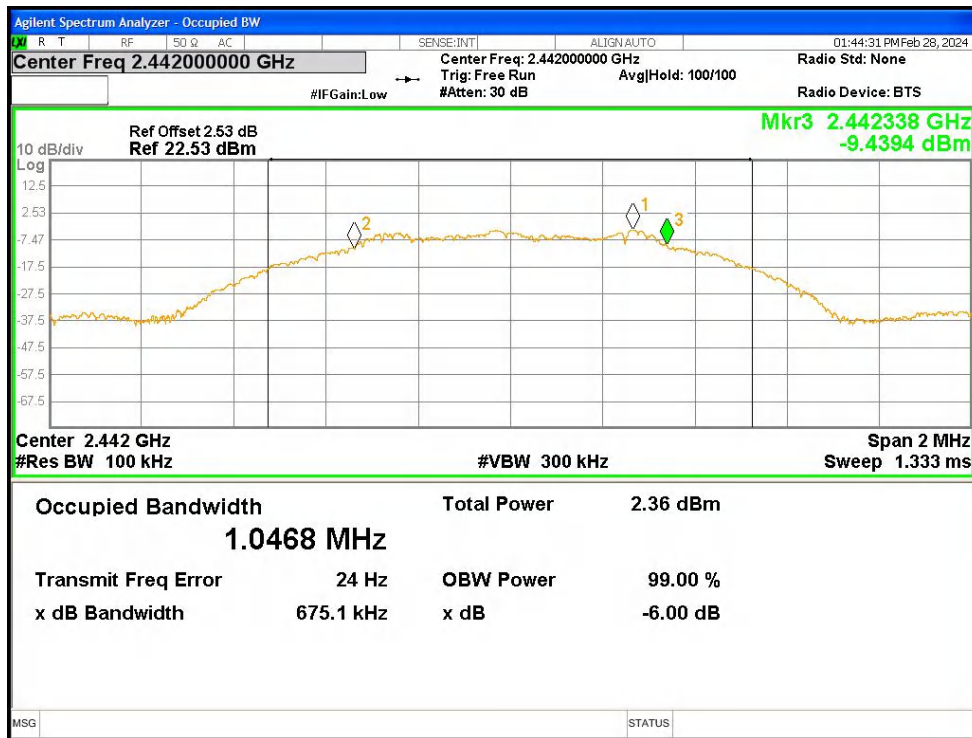**-6dB Bandwidth NVNT BLE 2442MHz Ant1**

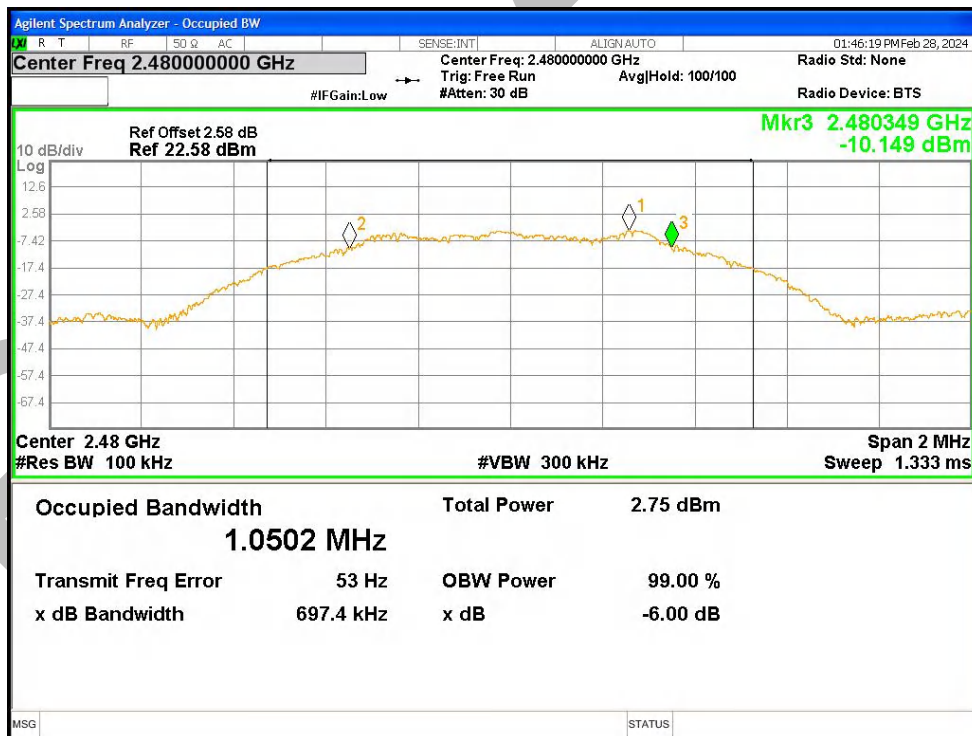


-6dB Bandwidth NVNT BLE 2480MHz Ant1



**Occupied Channel Bandwidth**


| Condition | Mode | Frequency (MHz) | Antenna | 99% OBW (MHz) |
|-----------|------|-----------------|---------|---------------|
| NVNT      | BLE  | 2402            | Ant1    | 1.0369        |
| NVNT      | BLE  | 2442            | Ant1    | 1.0345        |
| NVNT      | BLE  | 2480            | Ant1    | 1.0350        |

OBW NVNT BLE 2402MHz Ant1

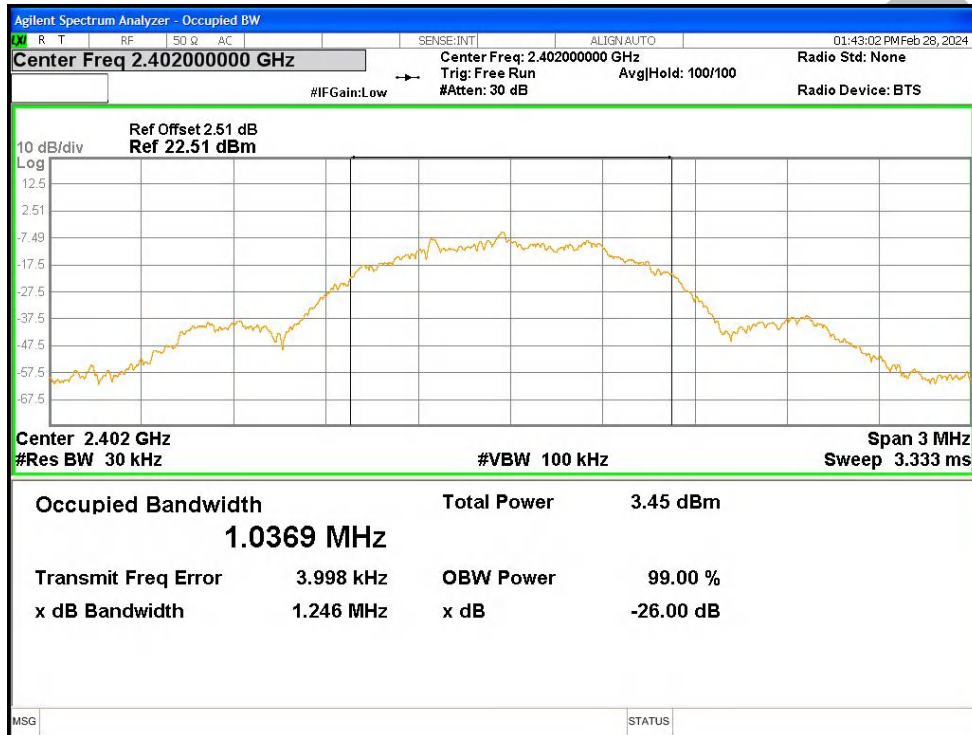


OBW NVNT BLE 2442MHz Ant1



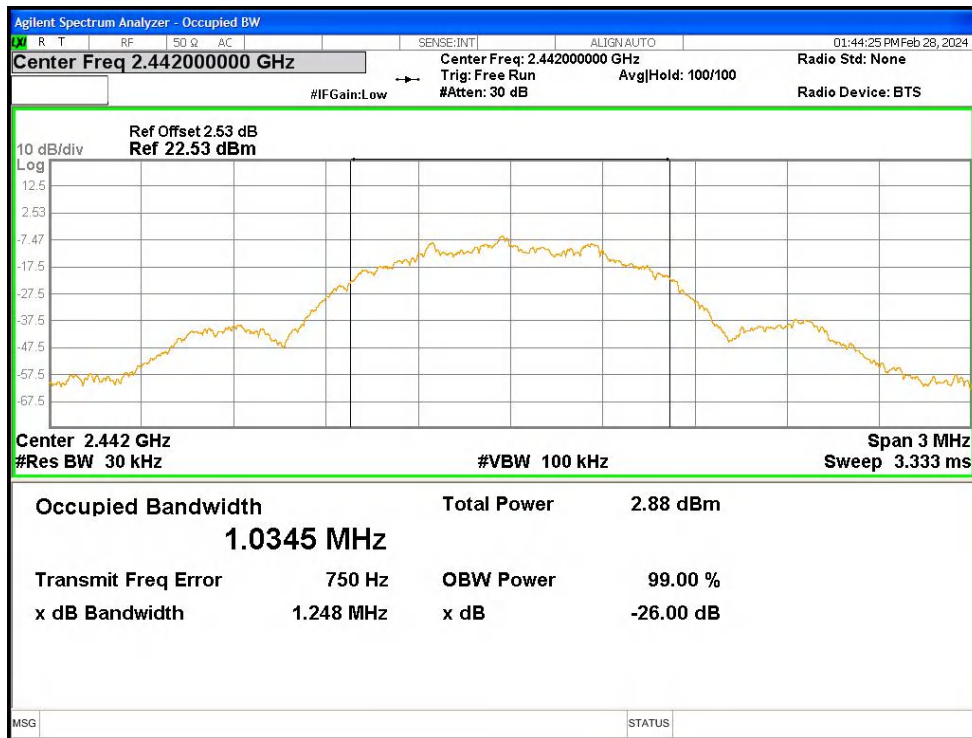

OBW NVNT BLE 2480MHz Ant1

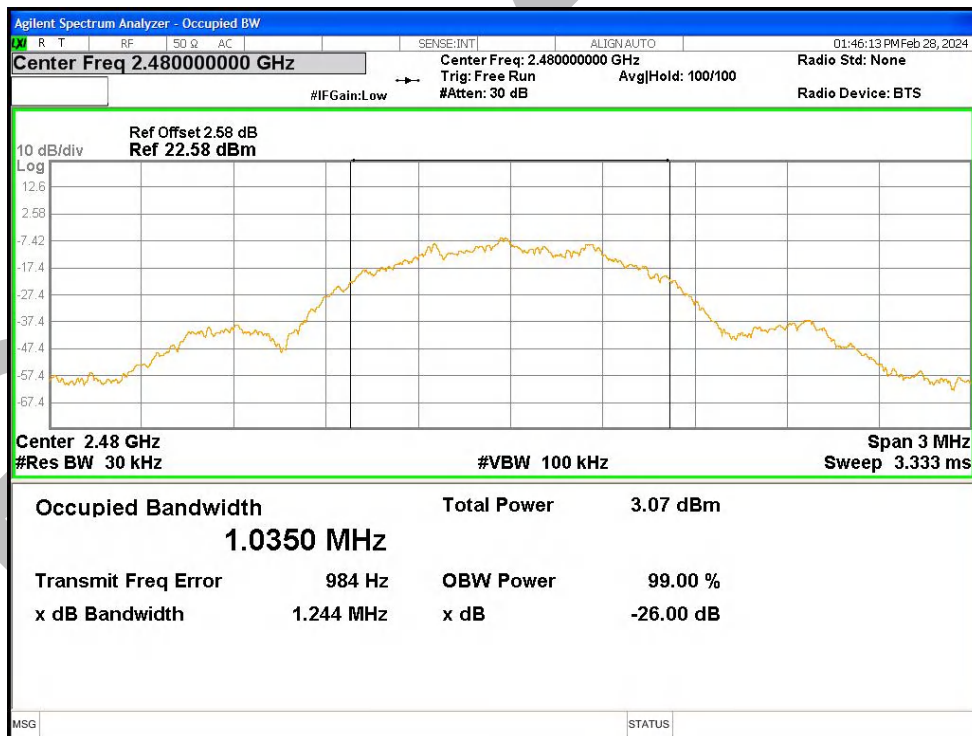



**Maximum Power Spectral Density Level**

| Condition | Mode | Frequency (MHz) | Antenna | Max PSD (dBm) | Limit (dBm) | Verdict |
|-----------|------|-----------------|---------|---------------|-------------|---------|
| NVNT      | BLE  | 2402            | Ant1    | -18.765       | 8           | Pass    |
| NVNT      | BLE  | 2442            | Ant1    | -19.485       | 8           | Pass    |
| NVNT      | BLE  | 2480            | Ant1    | -19.185       | 8           | Pass    |


PSD NVNT BLE 2402MHz Ant1



PSD NVNT BLE 2442MHz Ant1



PSD NVNT BLE 2480MHz Ant1

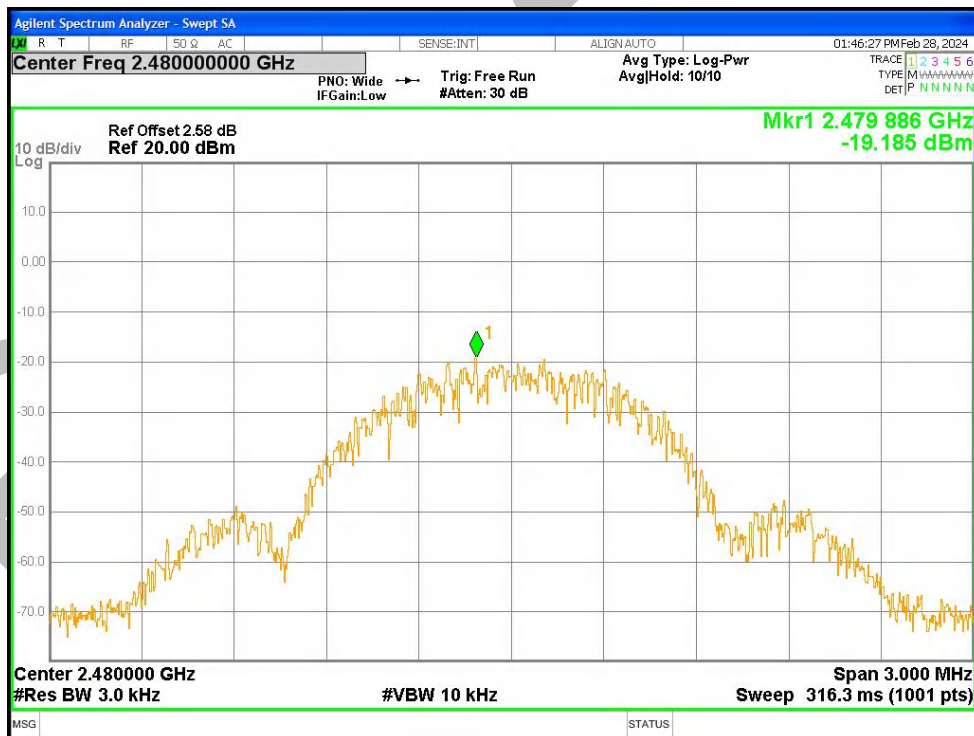


**Band Edge**

| Condition | Mode | Frequency (MHz) | Antenna | Max Value (dBc) | Limit (dBc) | Verdict |
|-----------|------|-----------------|---------|-----------------|-------------|---------|
| NVNT      | BLE  | 2402            | Ant1    | -48.88          | -20         | Pass    |
| NVNT      | BLE  | 2480            | Ant1    | -46.4           | -20         | Pass    |

Band Edge NVNT BLE 2402MHz Ant1 Ref




Band Edge NVNT BLE 2402MHz Ant1 Emission

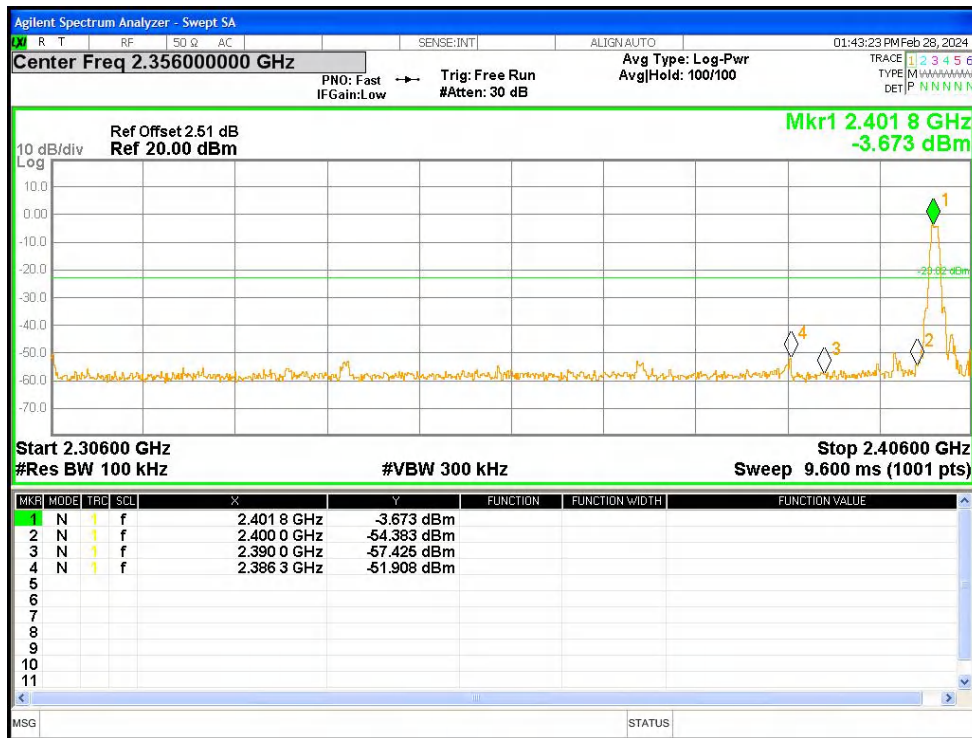

Band Edge NVNT BLE 2480MHz Ant1 Ref



Band Edge NVNT BLE 2480MHz Ant1 Emission

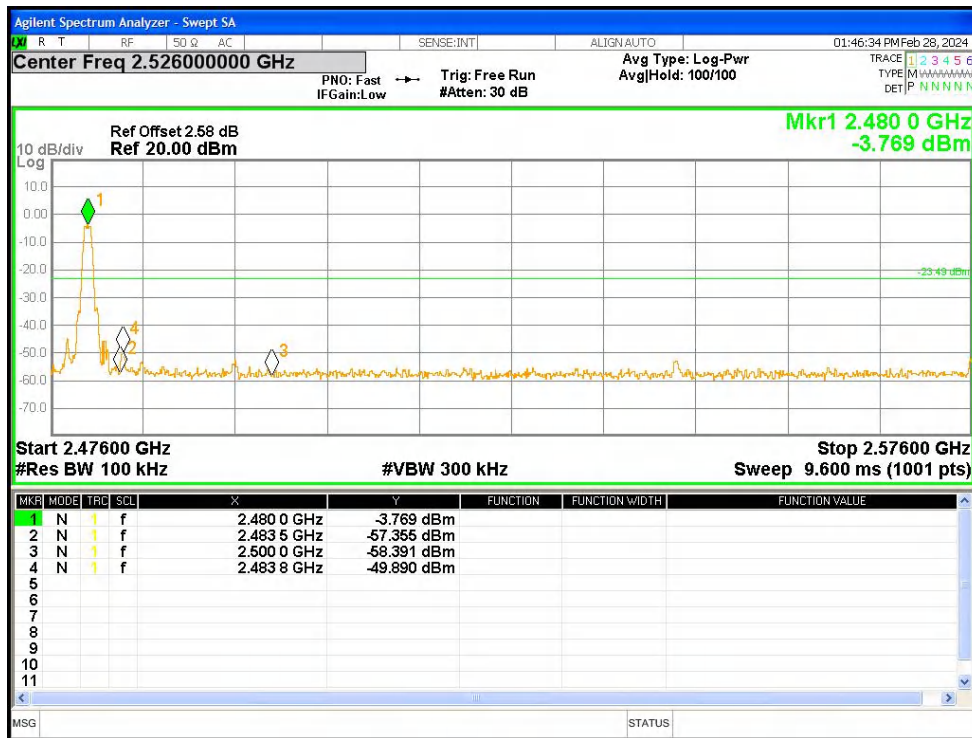


BlueAsia

**Conducted RF Spurious Emission**


| Condition | Mode | Frequency (MHz) | Antenna | Max Value (dBc) | Limit (dBc) | Verdict |
|-----------|------|-----------------|---------|-----------------|-------------|---------|
| NVNT      | BLE  | 2402            | Ant1    | -40.83          | -20         | Pass    |
| NVNT      | BLE  | 2442            | Ant1    | -40.48          | -20         | Pass    |
| NVNT      | BLE  | 2480            | Ant1    | -41.16          | -20         | Pass    |

Tx. Spurious NVNT BLE 2402MHz Ant1 Ref

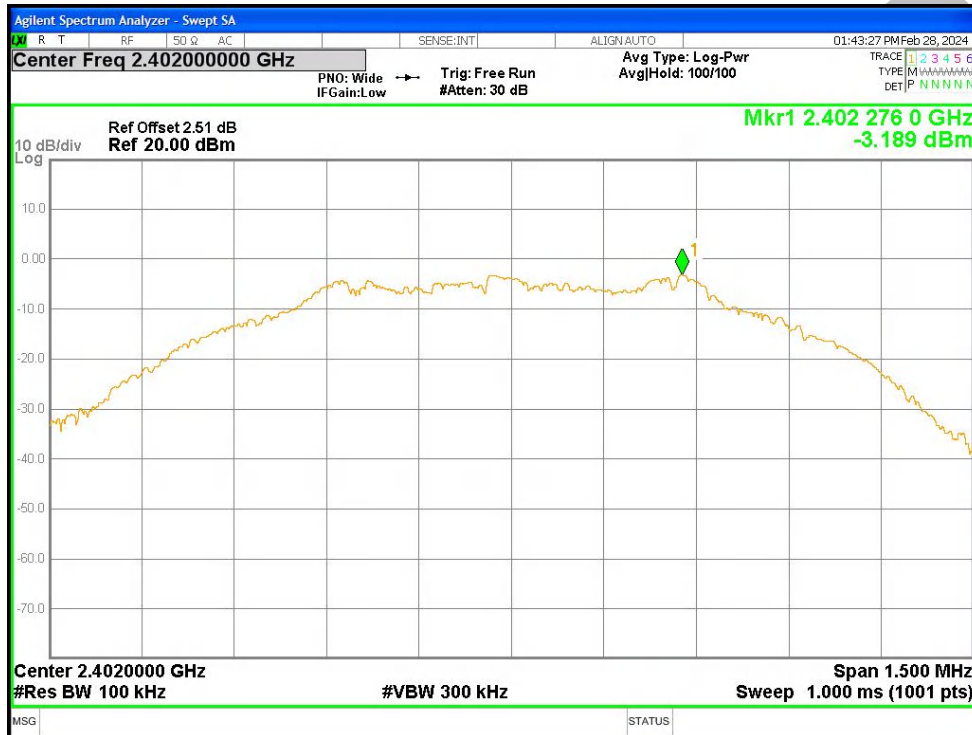


Tx. Spurious NVNT BLE 2402MHz Ant1 Emission




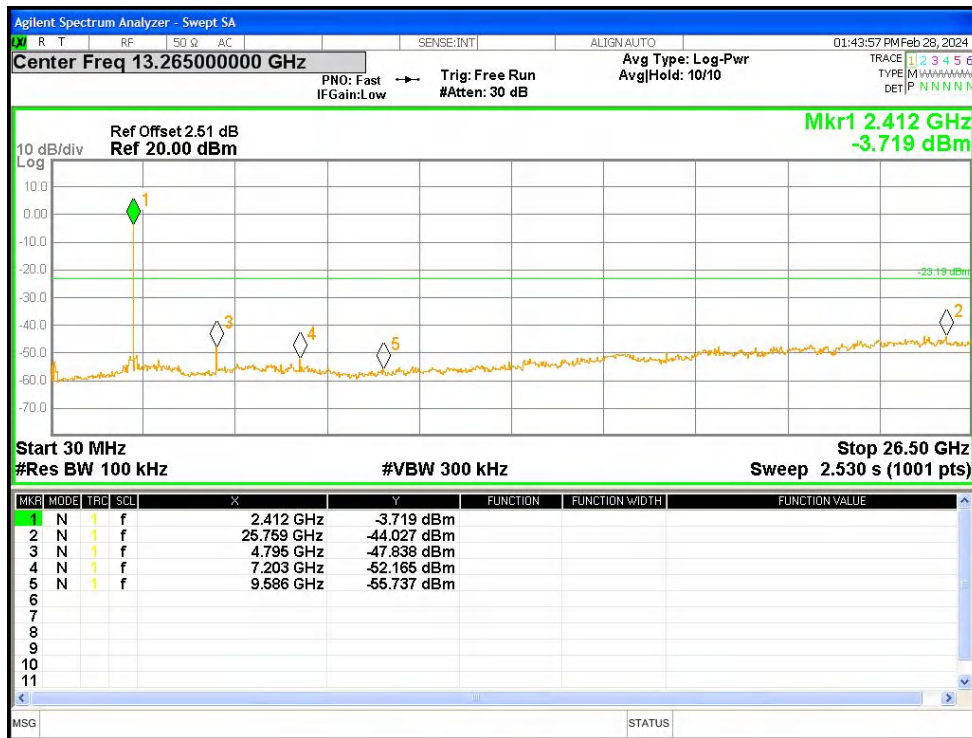


Tx. Spurious NVNT BLE 2442MHz Ant1 Ref

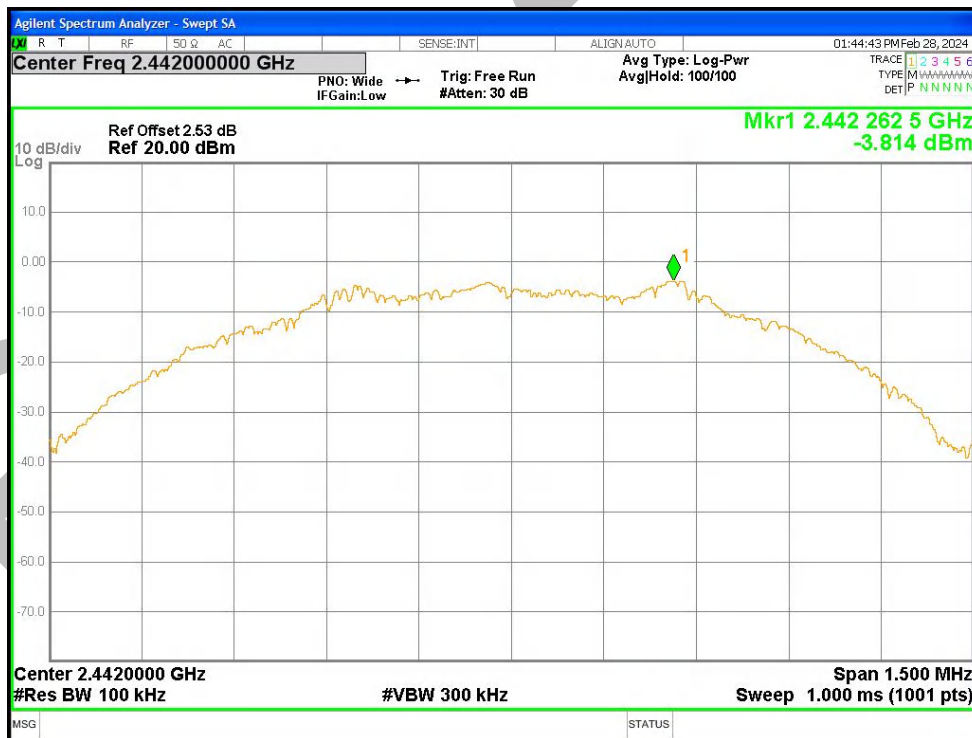

Tx. Spurious NVNT BLE 2442MHz Ant1 Emission

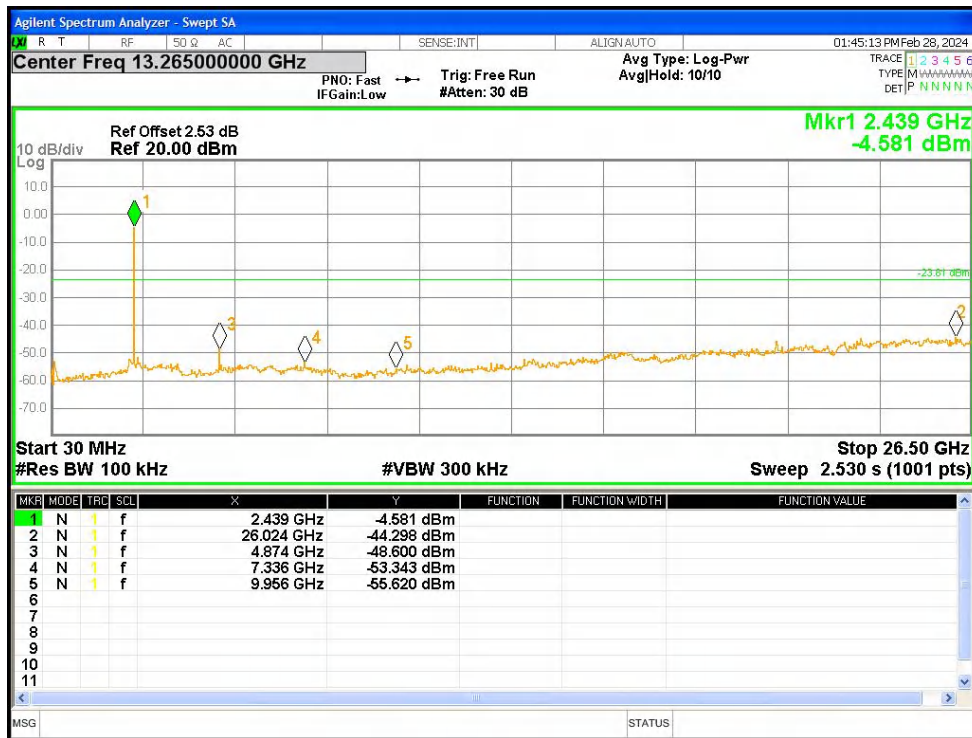


Tx. Spurious NVNT BLE 2480MHz Ant1 Ref

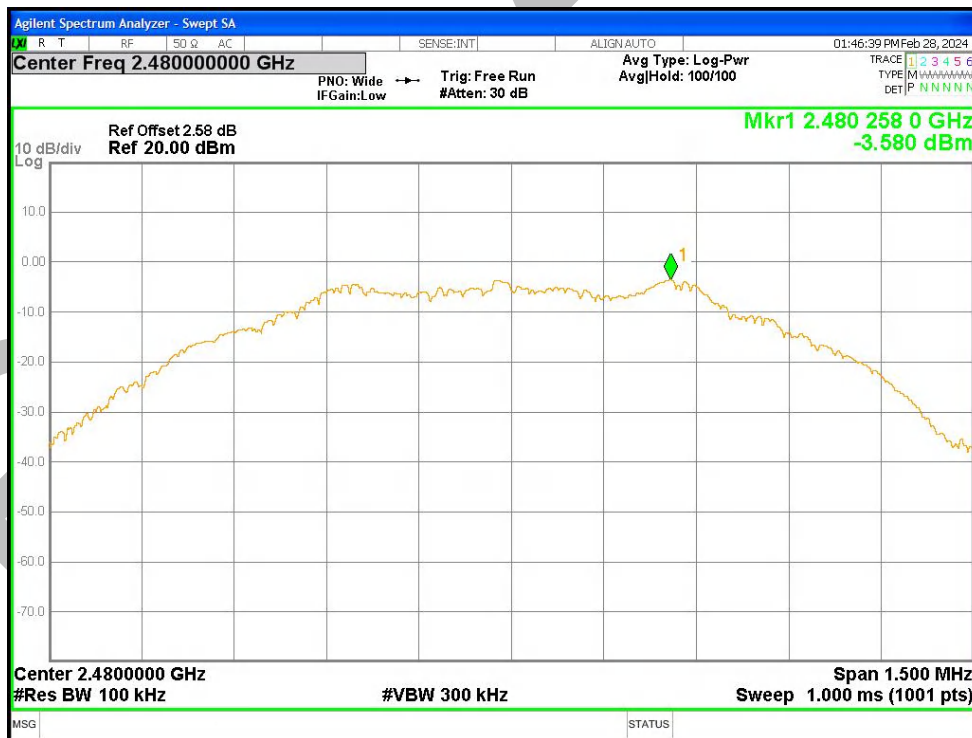

Tx. Spurious NVNT BLE 2480MHz Ant1 Emission




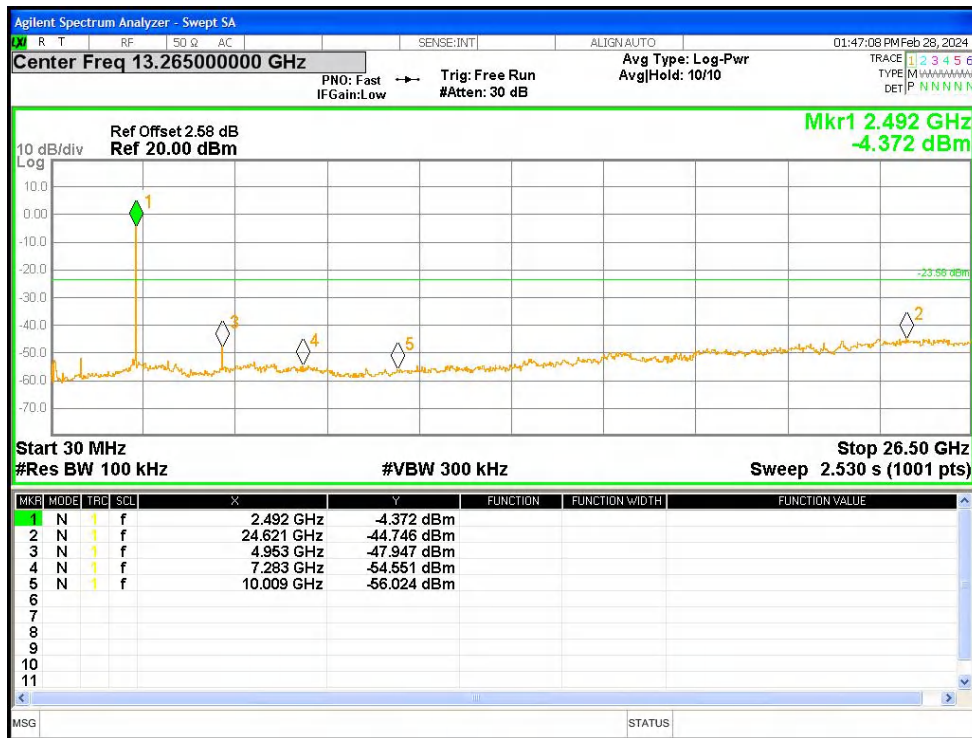

BlueAsia

## APPENDIX A: PHOTOGRAPHS OF TEST SETUP

### Radiated Spurious Emissions

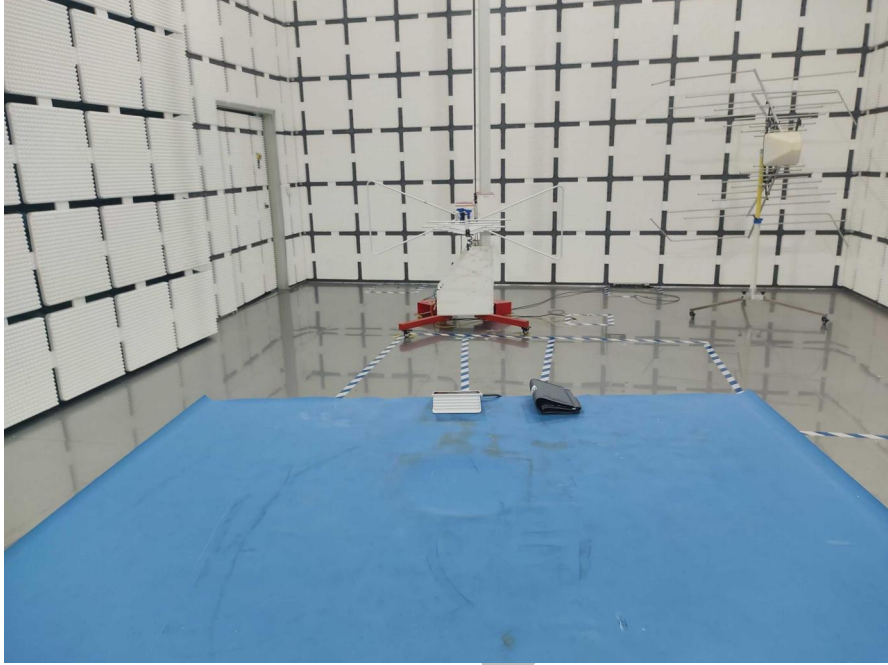

**Conducted Emissions at AC Power Line (150kHz-30MHz)**



BlueAsia

**APPENDIX B: PHOTOGRAPHS OF EUT**

Reference to the test report No. BLA-EMC-202401-A5101

**----END OF REPORT----**

The test report is effective only with both signature and specialized stamp, The result(s) shown in this report refer only to the sample(s) tested. Without written approval of BlueAsia, this report can't be reproduced except in full.

BlueAsia