

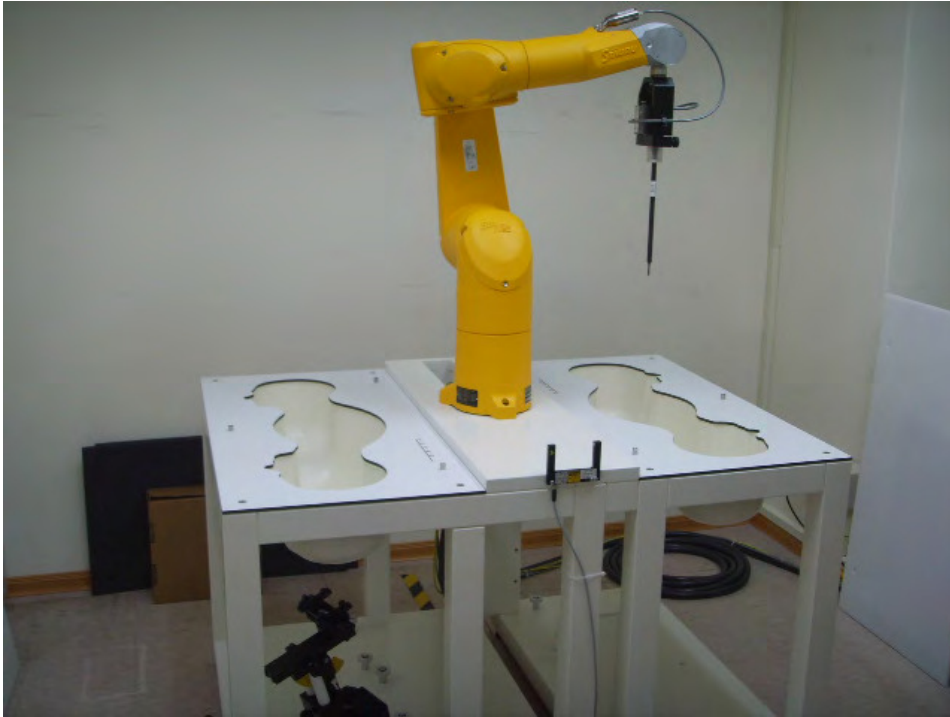
APPENDIX**10. Photographs of Test Setup**

Fig.1 Photograph of the SAR measurement system

Photograph of the tissue simulant fluid liquid depth (Body)

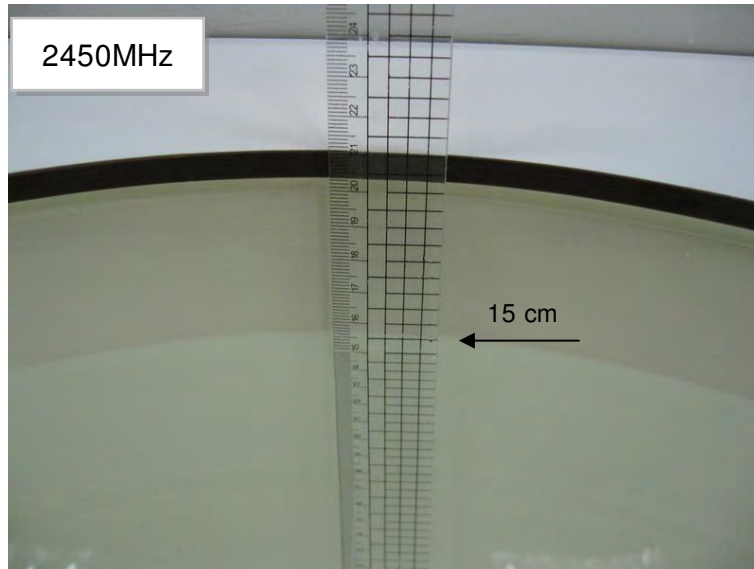


Fig.2.1

Body - distance between flat phantom and EUT is 0 mm

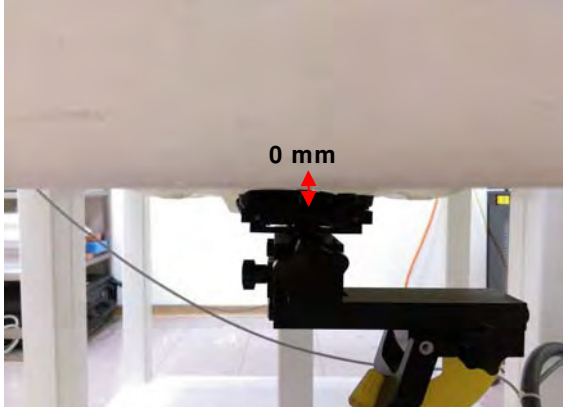


Fig.3 EUT Front side_1 to flat phantom



Fig.4 EUT Front side_1 with headset to flat phantom

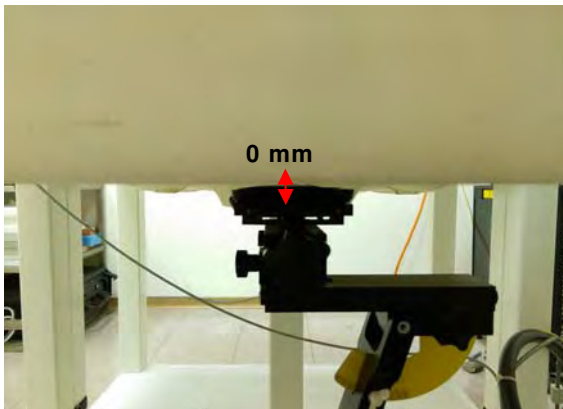


Fig.5 EUT Front side_2 to flat phantom

Body - distance between flat phantom and EUT is 0 mm

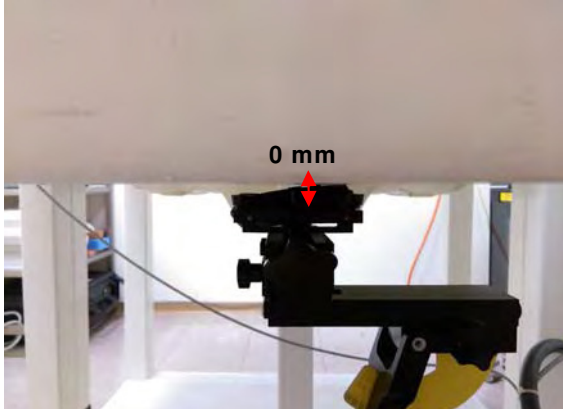


Fig.6 EUT Front side_3 to flat phantom

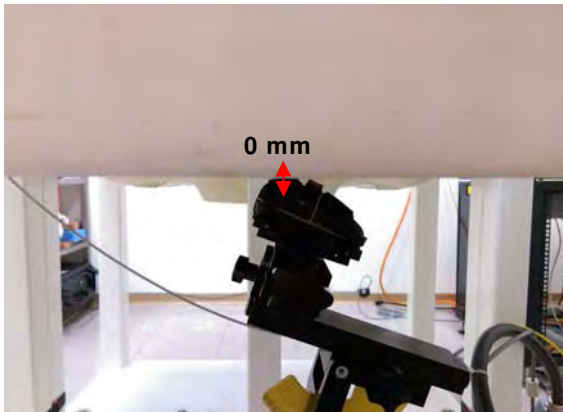


Fig.7 EUT Bottom side_1 to flat phantom

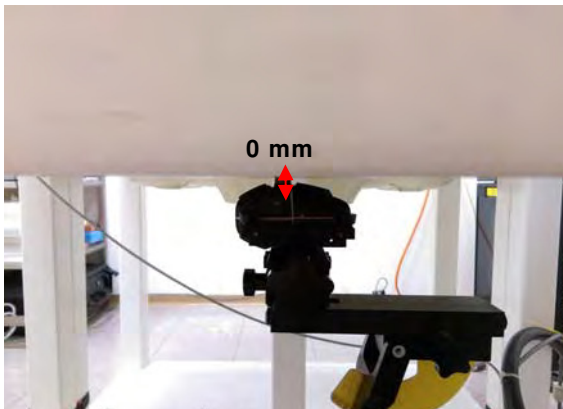


Fig.8 EUT Bottom side_2 to flat phantom

Body - distance between flat phantom and EUT is 0 mm



Fig.9 EUT Bottom side_3 to flat phantom

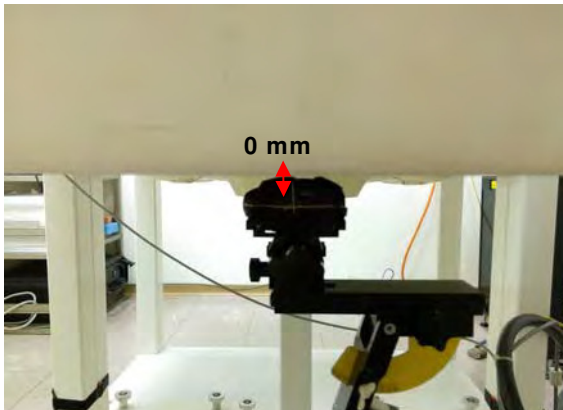


Fig.10 EUT Top side to flat phantom

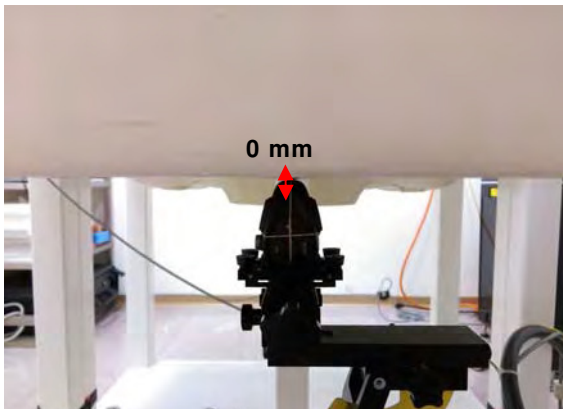


Fig.11 EUT Left side to flat phantom

Body - distance between flat phantom and EUT is 0 mm

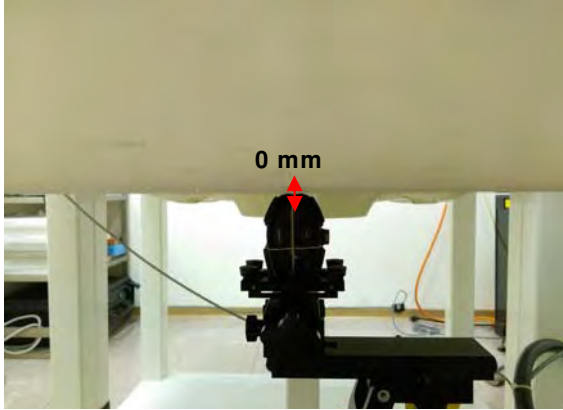


Fig.12 EUT Right side to flat phantom

Body - distance between flat phantom and EUT is 25 mm

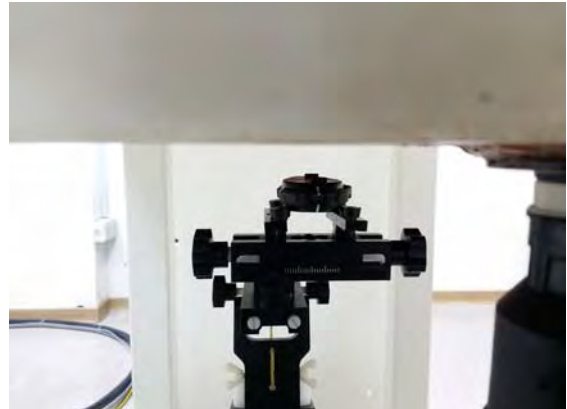
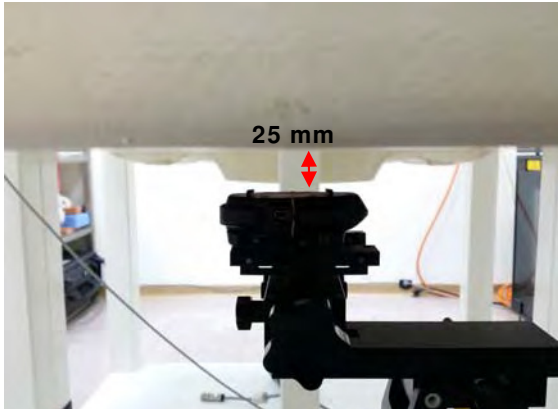


Fig.13 EUT Back side to flat phantom



Fig.14 EUT Back side with headset to flat phantom

11. Photographs of the EUT



Fig.15 Front view of EUT



Fig.16 Back view of EUT



Fig.17 Headset



Fig.18 Antenna position of EUT (Front view)

- End of Report -