

Fig.6-1 Z-Scan at power reference point (1900 MHz CH810)



# **GSM 1900 Body Rear**

Date/Time: 2015/10/28 Electronics: DAE4 Sn786 Medium: Body1900 MHz

Medium parameters used: f = 1880 MHz;  $\sigma = 1.555 \text{ S/m}$ ;  $\varepsilon_r = 53.496$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Ambient Temperature:22.0°C Liquid Temperature:21.5°C

Communication System: UID 0, 4 slot GPRS (0) Frequency: 1880 MHz Duty Cycle: 1:2.0

Probe: EX3DV4 - SN3633 ConvF(7.18, 7.18, 7.18);

Rear side Middle/Area Scan (31x41x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm

Maximum value of SAR (interpolated) = 2.85 W/kg

Rear side Middle/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 37.00 V/m; Power Drift = 0.07 dB

Peak SAR (extrapolated) = 6.30 W/kg

SAR(1 g) = 2.52 W/kg; SAR(10 g) = 1.34 W/kg Maximum value of SAR (measured) = 2.67 W/kg

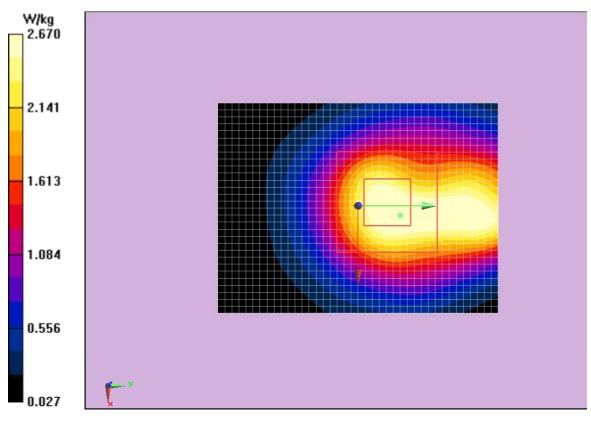


Fig.7 1900 MHz CH661



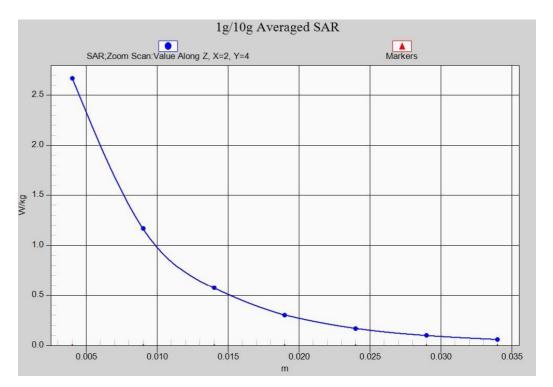


Fig.7-1 Z-Scan at power reference point (1900 MHz CH661)



# **GSM 1900 Body Rear**

Date/Time: 2015/10/28 Electronics: DAE4 Sn786 Medium: Body1900 MHz

Medium parameters used (interpolated): f = 1850.2 MHz;  $\sigma = 1.512 \text{ S/m}$ ;  $\varepsilon_r = 51.527$ ;  $\rho = 1000 \text{ MHz}$ 

kg/m<sup>3</sup>

Ambient Temperature:22.0°C Liquid Temperature:21.5°C

Communication System: UID 0, 4 slot GPRS Frequency: 1850.2 MHz Duty Cycle: 1:2.0

Probe: EX3DV4 - SN3633 ConvF(7.18, 7.18, 7.18);

Rear side Low/Area Scan (31x41x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm

Maximum value of SAR (interpolated) = 3.12 W/kg

Rear side Low/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 43.48 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 6.96 W/kg

SAR(1 g) = 2.72 W/kg; SAR(10 g) = 1.46 W/kg

Maximum value of SAR (measured) = 2.99 W/kg

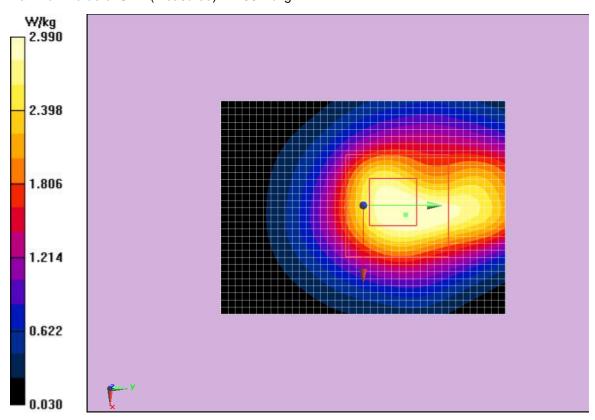


Fig.8 1900 MHz CH512



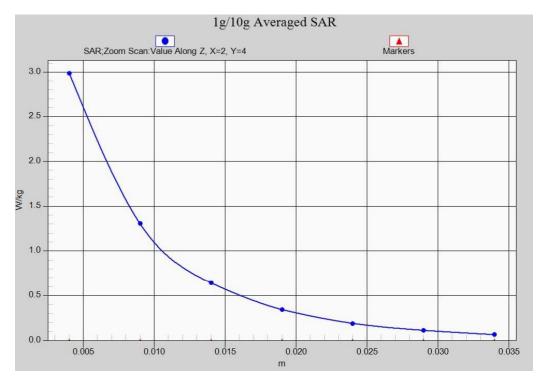


Fig.8-1 Z-Scan at power reference point (1900 MHz CH512)



# **ANNEX B** System Verification Results

Date/Time: 2015-10-29 Electronics: DAE4 Sn786 Medium: Head 850 MHz

Medium parameters used (interpolated): f = 835 MHz;  $\sigma$  = 0.929 S/m;  $\varepsilon_r$  = 41.315;  $\rho$  = 1000 kg/m<sup>3</sup>

Ambient Temperature:22.0°C Liquid Temperature:21.5°C

Communication System: CW\_TMC Frequency: 835 MHz Duty Cycle: 1:1

Probe: EX3DV4 - SN3633 ConvF(9.31, 9.31, 9.31);

Configuration/Area Scan (31x91x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm

Fast SAR:SAR(1 g) = 2.42 W/kg; SAR(10 g) = 1.49 W/kg

Maximum value of SAR (interpolated) = 2.48 W/kg


Configuration/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 54.349 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.75 W/kg

SAR(1 g) = 2.44 W/kg; SAR(10 g) = 1.55 W/kg

Maximum value of SAR (measured) = 2.66 W/kg

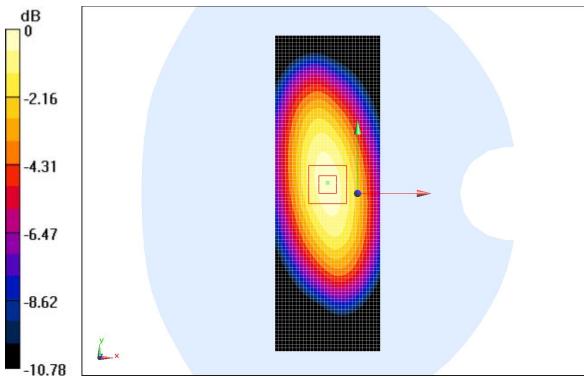

0 dB = 2.66 W/kg = 4.25 dBW/kg

Fig.B.1 validation 835MHz 250mW



## 835MHz

Date/Time: 2015-10-29 Electronics: DAE4 Sn786 Medium: Body850 MHz

Medium parameters used (interpolated): f = 835 MHz;  $\sigma$  = 0.97 S/m;  $\varepsilon_r$  = 53.498;  $\rho$  = 1000 kg/m<sup>3</sup>

Ambient Temperature:22.0°C Liquid Temperature:21.5°C

Communication System: CW\_TMC Frequency: 835 MHz Duty Cycle: 1:1 Probe: EX3DV4 - SN3633 ConvF(9.29, 9.29, 9.29); Calibrated: 2015/9/9

Configuration/Area Scan (61x181x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm

Reference Value = 51.989 V/m; Power Drift = 0.06 dB

Fast SAR: SAR(1 g) = 2.47 W/kg; SAR(10 g) = 1.62 W/kg

Maximum value of SAR (interpolated) = 2.67 W/kg

Configuration/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 51.989 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 3.60 W/kg

SAR(1 g) = 2.45 W/kg; SAR(10 g) = 1.6 W/kg Maximum value of SAR (measured) = 2.66 W/kg

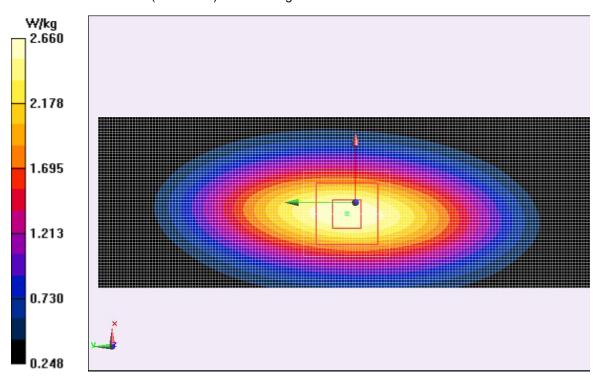


Fig.B.1 validation 835MHz 250mW



## 1900MHz

Date/Time: 2015-10-28 Electronics: DAE4 Sn786 Medium: 1900 Head

Medium parameters used: f = 1900 MHz;  $\sigma$  = 1.421 S/m;  $\varepsilon_r$  = 38.838;  $\rho$  = 1000 kg/m<sup>3</sup>

Ambient Temperature:22.0°C Liquid Temperature:21.5°C

Communication System: CW\_TMC Frequency: 1900 MHz Duty Cycle: 1:1

Probe: EX3DV4 - SN3633 ConvF(7.55, 7.55, 7.55);

Configuration/Area Scan (61x121x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm

SAR(1 g) = 9.89 W/kg; SAR(10 g) = 5.04 W/kg Maximum value of SAR (interpolated) = 11.0 W/kg


Configuration/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 81.837 V/m; Power Drift = 0.18 dB

Peak SAR (extrapolated) = 18.8 W/kg

SAR(1 g) = 9.93 W/kg; SAR(10 g) = 5.13 W/kg

Maximum value of SAR (measured) = 11.2 W/kg

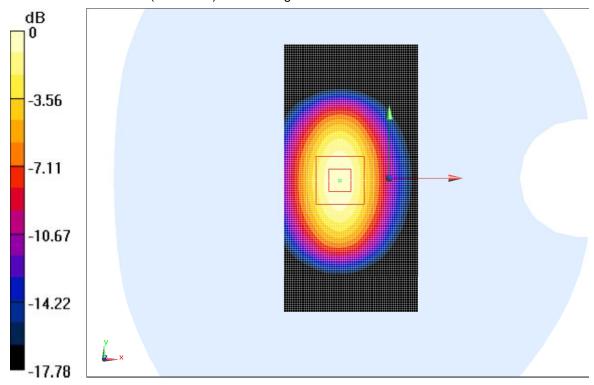

0 dB = 11.2 W/kg = 10.49 dBW/kg

Fig.B.3 validation 1900MHz 250mW



## 1900MHz

Date/Time: 2015-10-28 Electronics: DAE4 Sn786 Medium: 1900 Body

Medium parameters used: f = 1900 MHz;  $\sigma = 1.543 \text{ S/m}$ ;  $\varepsilon_r = 50.79$ ;  $\rho = 1000 \text{ kg/m}^3$ 

Ambient Temperature:22.0°C Liquid Temperature:21.5°C

Communication System: CW\_TMC Frequency: 1900 MHz Duty Cycle: 1:1

Probe: EX3DV4 - SN3633 ConvF(7.18, 7.18, 7.18);

Configuration/1900 Body/Area Scan (61x121x1): Interpolated grid: dx=1.000 mm, dy=1.000 mm

Reference Value = 84.945 V/m; Power Drift = 0.10 dBFast SAR: SAR(1 g) = 10.2 W/kg; SAR(10 g) = 5.3 W/kg

Maximum value of SAR (interpolated) = 11.6 W/kg

Configuration/1900 Body/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 84.945 V/m; Power Drift = 0.10 dB

Peak SAR (extrapolated) = 18.2 W/kg

SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.27 W/kg Maximum value of SAR (measured) = 11.4 W/kg

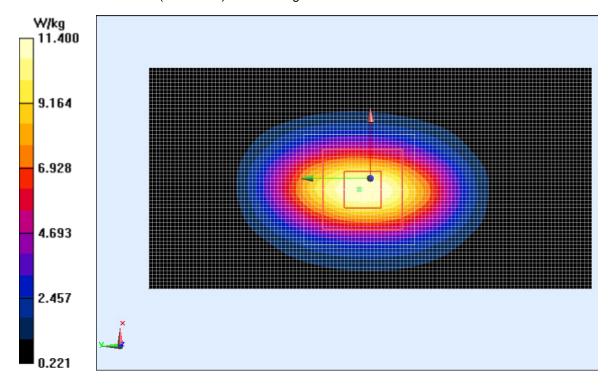


Fig.B.2 validation 835MHz 250mW



The SAR system verification must be required that the area scan estimated 1-g SAR is within 3% of the zoom scan 1-g SAR.

Table B.1 Comparison between area scan and zoom scan for system verification


Band	Position	Area scan (1g)	Zoom scan (1g)	Drift (%)
835	Head	2.42	2.44	-0.82
835	Body	2.47	2.45	0.82
1900	Head	9.89	9.93	-0.40
1900	Body	10.2	10.1	0.99



# **ANNEX C** SAR Measurement Setup

# C.1 Measurement Set-up

The Dasy4 or DASY5 system for performing compliance tests is illustrated above graphically. This system consists of the following items:

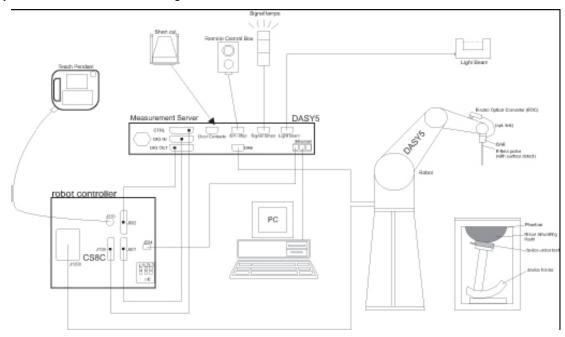

Picture C.1 SAR Lab Test Measurement Set-up

- A standard high precision 6-axis robot (Stäubli TX=RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- An isotropic field probe optimized and calibrated for the targeted measurement.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc.
   The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion from optical to electrical signals
  for the digital communication to the DAE. To use optical surface detection, a special version of
  the EOC is required. The EOC signal is transmitted to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
- A computer running WinXP and the DASY4 or DASY5 software.
- Remote control and teach pendant as well as additional circuitry for robot safety such as
- warning lamps, etc.
- The phantom, the device holder and other accessories according to the targeted measurement.



# C.2 Dasy4 or DASY5 E-field Probe System

The SAR measurements were conducted with the dosimetric probe designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multifiber line ending at the front of the probe tip. It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY4 or DASY5 software reads the reflection durning a software approach and looks for the maximum using 2<sup>nd</sup> ord curve fitting. The approach is stopped at reaching the maximum.

# **Probe Specifications:**

Model: EX3DV4, EX3DV4

Frequency 10MHz — 6.0GHz(EX3DV4) Range: 10MHz — 4GHz(EX3DV4)

Calibration: In head and body simulating tissue at

Frequencies from 835 up to 5800MHz

Linearity:  $\pm 0.2 \text{ dB}(30 \text{ MHz to 6 GHz})$  for EX3DV4

± 0.2 dB(30 MHz to 4 GHz) for EX3DV4

Dynamic Range: 10 mW/kg — 100W/kg

Probe Length: 330 mm

**Probe Tip** 

Length: 20 mm Body Diameter: 12 mm

Tip Diameter: 2.5 mm (3.9 mm for EX3DV4)

Tip-Center: 1 mm (2.0mm for EX3DV4)

Application: SAR Dosimetry Testing

Compliance tests of mobile phones

Dosimetry in strong gradient fields



Picture C.2 Near-field Probe



Picture C.3 E-field Probe

## C.3 E-field Probe Calibration

Each E-Probe/Probe Amplifier combination has unique calibration parameters. A TEM cell calibration procedure is conducted to determine the proper amplifier settings to enter in the probe parameters. The amplifier settings are determined for a given frequency by subjecting the probe to a known E-field density (1 mW/cm²) using an RF Signal generator, TEM cell, and RF Power Meter. The free space E-field from amplified probe outputs is determined in a test chamber. This calibration can be performed in a TEM cell if the frequency is below 1 GHz and inn a waveguide or other methodologies above 1 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then



rotated 360 degrees until the three channels show the maximum reading. The power density readings equates to 1 mW/ cm<sup>2</sup>.

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The E-field in the medium correlates with the temperature rise in the dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$SAR = C \frac{\Delta T}{\Delta t}$$

Where: C = Heat capacity of tissue (brain or muscle),  $\Delta T$  = Temperature increase due to RF exposure,  $\Delta t$  = Exposure time (30 seconds).

$$SAR = \frac{\left|E\right|^2 \cdot \sigma}{\rho}$$

Where:  $\sigma$  = Simulated tissue conductivity,  $\rho$  = Tissue density (kg/m<sup>3</sup>).

# **C.4 Other Test Equipment**

# C.4.1 Data Acquisition Electronics(DAE)

The data acquisition electronics consist of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder with a control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information, as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE is 200 MOhm; the inputs are symmetrical and floating. Common mode rejection is above 80 dB.



PictureC.4: DAE

## C.4.2 Robot

The SPEAG DASY system uses the high precision robots (DASY4: RX90XL; DASY5: RX160L) type from Stäubli SA (France). For the 6-axis controller system, the robot controller version from Stäubli is used. The Stäubli robot series have many features that are important for our application:

High precision (repeatability 0.02mm)



- High reliability (industrial design)
- Low maintenance costs (virtually maintenance free due to direct drive gears; no belt drives)
- Jerk-free straight movements (brushless synchron motors; no stepper motors)
- Low ELF interference (motor control fields shielded via the closed metallic construction shields)



Picture C.6 DASY 5

# C.4.3 Measurement Server

The Measurement server is based on a PC/104 CPU broad with CPU (dasy4: 166 MHz, Intel Pentium; DASY5: 400 MHz, Intel Celeron), chipdisk (DASY4: 32 MB; DASY5: 128MB), RAM (DASY4: 64 MB, DASY5: 128MB). The necessary circuits for communication with the DAE electronic box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY I/O broad, which is directly connected to the PC/104 bus of the CPU broad.

The measurement server performs all real-time data evaluation of field measurements and surface detection, controls robot movements and handles safety operation. The PC operating system cannot interfere with these time critical processes. All connections are supervised by a watchdog, and disconnection of any of the cables to the measurement server will automatically disarm the robot and disable all program-controlled robot movements. Furthermore, the measurement server is equipped with an expansion port which is reserved for future applications. Please note that this expansion port does not have a standardized pinout, and therefore only devices provided by SPEAG can be connected. Devices from any other supplier could seriously damage the measurement server.





Picture C.7 Server for DASY 4

Picture C.8 Server for DASY 5

## C.4.4 Device Holder for Phantom

The SAR in the phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source at 5mm distance, a positioning uncertainty of ±0.5mm would produce a SAR uncertainty of ±20%. Accurate device positioning is therefore crucial for accurate and repeatable measurements. The positions in which the devices must be



measured are defined by the standards.

The DASY device holder is designed to cope with the different positions given in the standard. It has two scales for device rotation (with respect to the body axis) and device inclination (with respect to the line between the ear reference points). The rotation centers for both scales is the ear reference point (ERP). Thus the device needs no repositioning when changing the angles.

The DASY device holder is constructed of low-loss POM material having the following dielectric parameters: relative permittivity  $\mathcal{E}$ =3 and loss tangent  $\delta$ =0.02. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.

<Laptop Extension Kit>

The extension is lightweight and made of POM, acrylic glass and foam. It fits easily on the upper part of the Mounting Device in place of the phone positioned. The extension is fully compatible with the Twin-SAM and ELI phantoms.



Picture C.9-1: Device Holder



Picture C.9-2: Laptop Extension Kit

## C.4.5 Phantom

The SAM Twin Phantom V4.0 is constructed of a fiberglass shell integrated in a table. The shape of the shell is based on data from an anatomical study designed to

Represent the 90<sup>th</sup> percentile of the population. The phantom enables the dissymmetric evaluation of SAR for both left and right handed handset usage, as well as body-worn usage using the flat phantom region. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. The shell phantom has a 2mm shell thickness (except the ear region where shell thickness increases to 6 mm).

Shell Thickness:  $2 \pm 0.2$  mm Filling Volume: Approx. 25 liters

Dimensions: 810 x 1000 x 500 mm (H x L x W)

Available: Special




Picture C.10: SAM Twin Phantom



# ANNEX D Position of the wireless device in relation to the phantom

# D.1 Body-worn device

A typical example of a body-worn device is a mobile phone, wireless enabled PDA or other battery operated wireless device with the ability to transmit while mounted on a person's body using a carry accessory approved by the wireless device manufacturer.

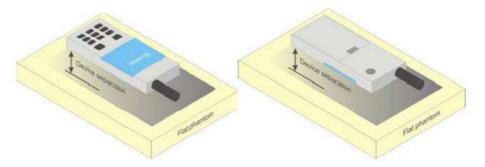


Picture D.1 Test positions for body-worn devices

# D.2 Limb-worn device

A limb-worn device is a unit whose intended use includes being strapped to the arm or leg of the user while transmitting (except in idle mode). It is similar to a body-worn device.

The strap shall be opened so that it is divided into two parts as shown in Picture D.2. The device shall be positioned directly against the phantom surface with the strap straightened as much as possible and the back of the device towards the phantom.

If the strap cannot normally be opened to allow placing in direct contact with the phantom surface, it may be necessary to break the strap of the device but ensuring to not damage the antenna.

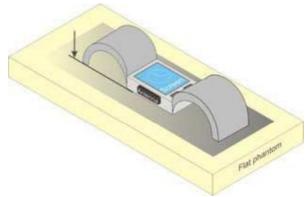

Picture D.2 Test position for limb-worn devices



# **ANNEX E Equivalent Media Recipes**

The liquid used for the frequency range of 800-3000 MHz consisted of water, sugar, salt, preventol, glycol monobutyl and Cellulose. The liquid has been previously proven to be suited for worst-case. The Table E.1 shows the detail solution. It's satisfying the latest tissue dielectric parameters requirements proposed by the IEEE 1528 and IEC 62209.

Table E.1: Composition of the Tissue Equivalent Matter

Frequency	835	835	1900	1900	2450	2450	5800	5800			
(MHz)	Head	Body	Head	Body	Head	Body	Head	Body			
Ingredients (% by	Ingredients (% by weight)										
Water	41.45	52.5	55.242	69.91	58.79	72.60	65.53	65.53			
Sugar	56.0	45.0	\	\	\	\	\	/			
Salt	1.45	1.4	0.306	0.13	0.06	0.18	\	/			
Preventol	0.1	0.1	\	\	\	\	\	\			
Cellulose	1.0	1.0	\	\	\	\	\	/			
Glycol	,	\	44.452	20.06	44 4E	27.22	\	\			
Monobutyl	\	\	44.452	29.96	41.15	21.22	\	\			
Diethylenglycol	\	\	\	\	\	\	17.24	17.24			
monohexylether	\	\	\	\	\	\	17.24	17.24			
Triton X-100	\	\	\	\	\	\	17.24	17.24			
Dielectric	c=41 E	c=EE 2	c=40.0	c=E2 2	ε=39.2	ε=52.7	ε=35.3	ε=48.2			
Parameters	ε=41.5	ε=55.2	ε=40.0	ε=53.3							
Target Value	σ=0.90	σ=0.97	σ=1.40	σ=1.52	σ=1.80	σ=1.95	σ=5.27	σ=6.00			

# ANNEX F System Validation

The SAR system must be validated against its performance specifications before it is deployed. When SAR probes, system components or software are changed, upgraded or recalibrated, these must be validated with the SAR system(s) that operates with such components.


**Table F.1: System Validation** 

Probe SN.	Liquid name	Validation date	Frequency point	Status (OK or Not)
3633	Head 850MHz	September 12, 2015	850 MHz	OK
3633	Head 1900MHz	September 12, 2015	1900 MHz	OK



# ANNEX G Probe Calibration Certificate

## Probe EX3DV4-SN:3633 Calibration Certificate

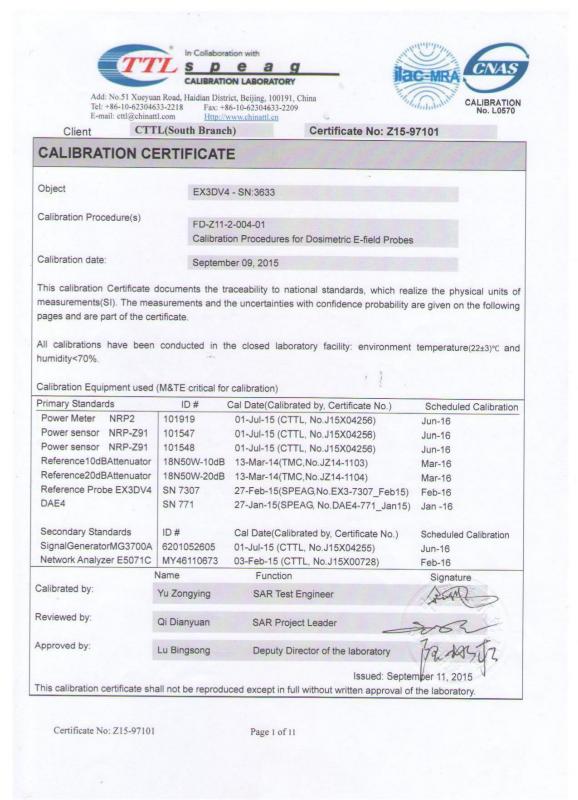





Glossarv:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty\_cycle) of the RF signal A,B,C,D modulation dependent linearization parameters

Polarization Φ rotation around probe axis

Polarization θ θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i

 $\theta$ =0 is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

 b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005

Methods Applied and Interpretation of Parameters:

NORMx,y,z: Assessed for E-field polarization θ=0 (f≤900MHz in TEM-cell; f>1800MHz: waveguide).
 NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).

NORM(f)x,y,z = NORMx,y,z\* frequency\_response (see Frequency Response Chart). This
linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the
frequency response is included in the stated uncertainty of ConvF.

 DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.

 PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.

Ax, y, z; Bx, y, z; Cx, y, z; VRx, y, z:A,B,C are numerical linearization parameters assessed based on the
data of power sweep for specific modulation signal. The parameters do not depend on frequency nor
media. VR is the maximum calibration range expressed in RMS voltage across the diode.


• ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f≤800MHz) and inside waveguide using analytical field distributions based on power measurements for f >800MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z\* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from±50MHz to±100MHz.

 Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.

 Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

 Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).





# Probe EX3DV4

SN: 3633

Calibrated: September 09, 2015

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: Z15-97101

Page 3 of 11





# DASY/EASY - Parameters of Probe: EX3DV4 - SN: 3633

# **Basic Calibration Parameters**

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
$Norm(\mu V/(V/m)^2)^A$	0.39	0.42	0.40	±10.8%
DCP(mV) <sup>B</sup>	98.0	99.2	99.7	

# **Modulation Calibration Parameters**

UID	Communication System Name		A dB	B dBõV	С	D dB	VR mV	Unc E (k=2)
0 CW	0	X	0.0	0.0	1.0	0.00	175.5	±2.2%
		Y	0.0	0.0	1.0		179.7	
		Z	0.0	0.0	1.0		175.1	


The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

A The uncertainties of Norm X, Y, Z do not affect the E2-field uncertainty inside TSL (see Page 5 and Page 6).

E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.





# DASY/EASY - Parameters of Probe: EX3DV4 - SN: 3633

# Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz] <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
750	41.9	0.89	9.31	9.31	9.31	0.25	1.00	±12%
900	41.5	0.97	8.85	8.85	8.85	0.11	1.62	±12%
1750	40.1	1.37	7.76	7.76	7.76	0.15	1.26	±12%
1900	40.0	1.40	7.55	7.55	7.55	0.17	1.27	±12%
2300	39.5	1.67	7.37	7.37	7.37	0.37	0.77	±12%
2450	39.2	1.80	7.02	7.02	7.02	0.30	0.97	±12%
2600	39.0	1.96	6.79	6.79	6.79	0.40	0.83	±12%
5200	36.0	4.66	5.23	5.23	5.23	0.39	1.37	±13%
5300	35.9	4.76	5.01	5.01	5.01	0.36	1.42	±13%
5500	35.6	4.96	4.75	4.75	4.75	0.39	1.43	±13%
5600	35.5	5.07	4.57	4.57	4.57	0.39	1.50	±13%
5800	35.3	5.27	4.61	4.61	4.61	0.42	1.55	±13%

<sup>&</sup>lt;sup>C</sup> Frequency validity of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. F At frequency below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters. G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.





# DASY/EASY - Parameters of Probe: EX3DV4 - SN: 3633

# Calibration Parameter Determined in Body Tissue Simulating Media

f [MHz] <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
750	55.5	0.96	9.29	9.29	9.29	0.25	0.98	±12%
900	55.0	1.05	8.91	8.91	8.91	0.16	1.33	±12%
1750	53.4	1.49	7.45	7.45	7.45	0.13	1.60	±12%
1900	53.3	1.52	7.18	7.18	7.18	0.16	1.39	±12%
2300	52.9	1.81	6.97	6.97	6.97	0.27	1.30	±12%
2450	52.7	1.95	6.92	6.92	6.92	0.28	1.29	±12%
2600	52.5	2.16	6.76	6.76	6.76	0.32	1.10	±12%
5200	49.0	5.30	4.49	4.49	4.49	0.45	1.60	±13%
5300	48.9	5.42	4.29	4.29	4.29	0.45	1.60	±13%
5500	48.6	5.65	3.98	3.98	3.98	0.45	1.60	±13%
5600	48.5	5.77	3.83	3.83	3.83	0.45	1.60	±13%
5800	48.2	6.00	4.03	4.03	4.03	0.45	1.60	±13%


<sup>&</sup>lt;sup>C</sup> Frequency validity of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. 
<sup>F</sup> At frequency below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.





# Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

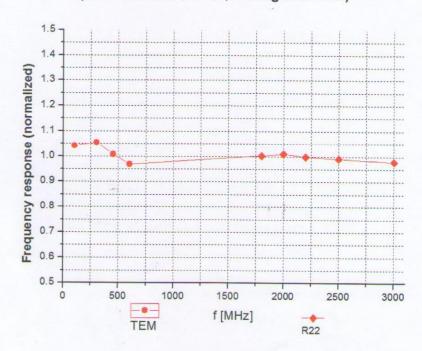


Uncertainty of Frequency Response of E-field: ±7.5% (k=2)


Certificate No: Z15-97101

Page 7 of 11




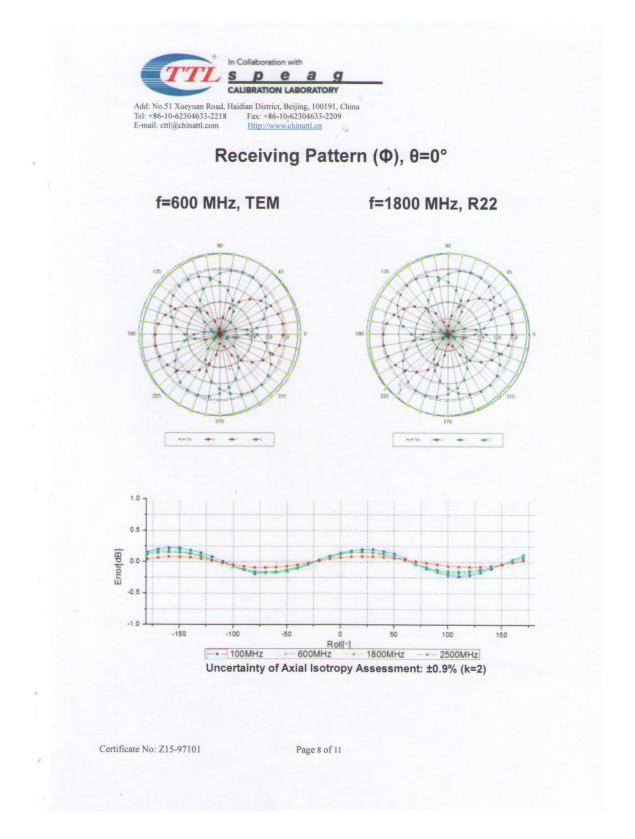



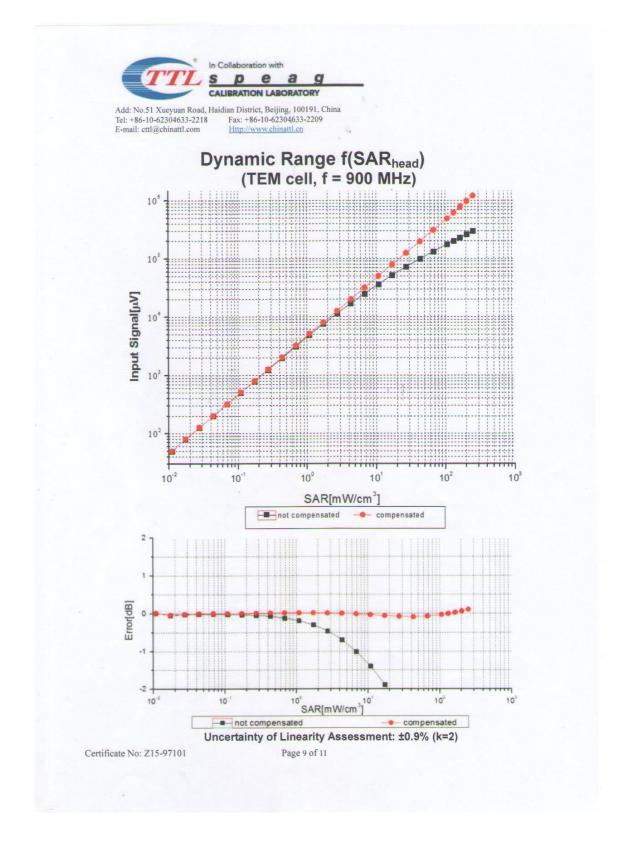



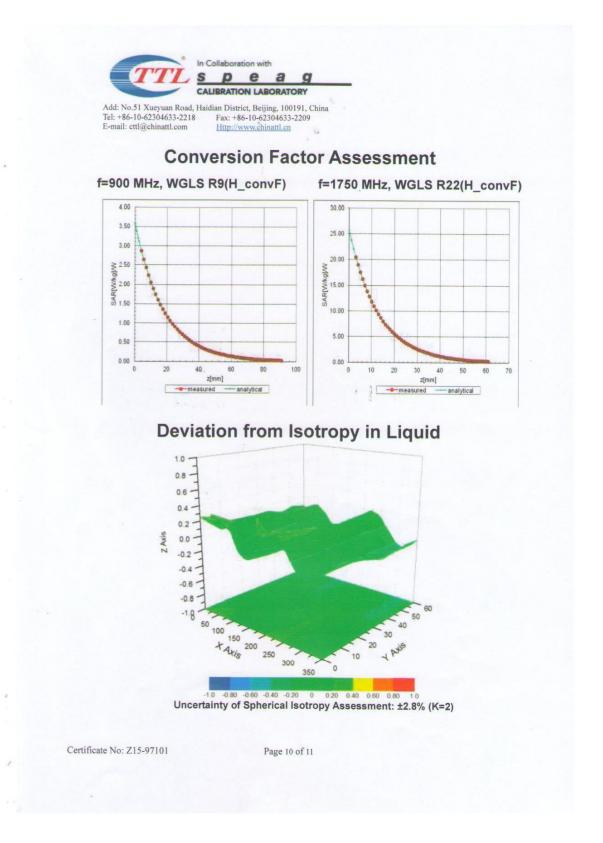





# DASY/EASY - Parameters of Probe: EX3DV4 - SN: 3633

# Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	163.5
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	9mm
Tip Diameter	2.5mm
Probe Tip to Sensor X Calibration Point	1mm
Probe Tip to Sensor Y Calibration Point	1mm
Probe Tip to Sensor Z Calibration Point	1mm
Recommended Measurement Distance from Surface	1.4mm



# ANNEX H DIPOLE CALIBRATION CERTIFICATE

# 835 MHz Dipole Calibration Certificate



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 Http://www.chinattl.cn

IBC MRA

CALIBRATION
No. L0570

lient CTTL(South Branch) Certificate No: Z14-97127

**CALIBRATION CERTIFICATE** 

D835V2 - SN: 4d057

Calibration Procedure(s)

TMC-OS-E-02-194

Calibration Procedures for dipole validation kits

Calibration date:

Object

November 4, 2014

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22 $\pm$ 3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
101919	01-Jul-14 (CTTL, No.J14X02146)	Jun-15
101547	01-Jul-14 (CTTL, No.J14X02146)	Jun-15
SN 3617	28-Aug-14(SPEAG,No.EX3-3617_Aug14)	Aug-15
SN 1331	23-Jan-14 (SPEAG, DAE4-1331_Jan14)	Jan-15
ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
6201052605	01-Jul-14 (CTTL, No.J14X02145)	Jun-15
MY4614d0573	15-Feb-14 (TMC, No.JZ14-781)	Feb-15
	101919 101547 SN 3617 SN 1331 ID # 6201052605	101919 01-Jul-14 (CTTL, No.J14X02146) 101547 01-Jul-14 (CTTL, No.J14X02146) SN 3617 28-Aug-14(SPEAG,No.EX3-3617_Aug14) SN 1331 23-Jan-14 (SPEAG, DAE4-1331_Jan14)  ID# Cal Date(Calibrated by, Certificate No.) 6201052605 01-Jul-14 (CTTL, No.J14X02145)

Name Function Signature

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Qi Dianyuan SAR Project Leader

Approved by: Lu Bingsong Deputy Director of the laboratory

Issued: November 6, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.





Glossary:

TSL ConvF N/A tissue simulating liquid sensitivity in TSL / NORMx,y,z not applicable or not measured

# Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

#### Additional Documentation:

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.





#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.8.8.1222
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

## **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.8 ± 6 %	0.92 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

## SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.41 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	9.48 mW /g ± 20.8 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.57 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	6.20 mW /g ± 20.4 % (k=2)

# **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.3 ± 6 %	0.99 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

## SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.42 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	9.53 mW /g ± 20.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	1.61 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	6.36 mW /g ± 20.4 % (k=2)

Page 3 of 8





#### **Appendix**

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.4Ω- 3.05jΩ	
Return Loss	- 30.3dB	

# Antenna Parameters with Body TSL

Impedance, transformed to feed point	45.3Ω- 4.70jΩ	
Return Loss	- 23.1dB	

# General Antenna Parameters and Design

3

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

# **Additional EUT Data**

Manufactured by	SPEAG	





# **DASY5 Validation Report for Head TSL**

Date: 04.11.2014

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d057

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium parameters used: f = 835 MHz;  $\sigma = 0.916$  S/m;  $\varepsilon_r = 40.82$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 SN3617; ConvF(9.67, 9.67, 9.67); Calibrated: 2014-08-28;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 2014-01-23
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

System Performance Check at Frequencies above 1 GHz/d=15mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid:


dx=5mm, dy=5mm, dz=5mm

Reference Value = 58.60 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.68 W/kg

SAR(1 g) = 2.41 W/kg; SAR(10 g) = 1.57 W/kg

Maximum value of SAR (measured) = 3.08 W/kg

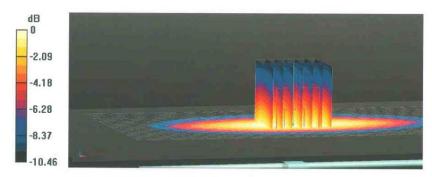


0 dB = 3.08 W/kg = 4.89 dBW/kg





## Impedance Measurement Plot for Head TSL

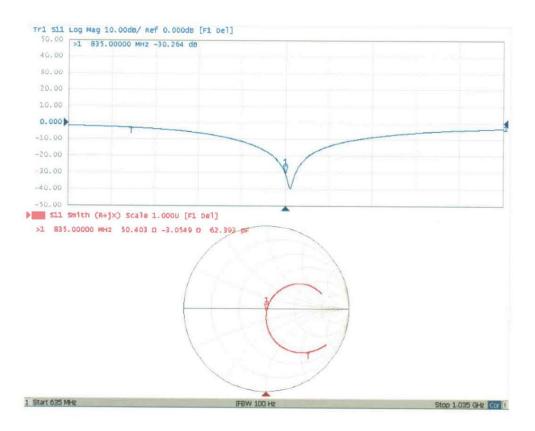





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2079
 Fax: +86-10-62304633-2504

 E-mail: cttl@chinattl.com
 Http://www.chinattl.cn

# DASY5 Validation Report for Body TSL

Date: 04.11.2014

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d057

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium parameters used: f = 835 MHz;  $\sigma = 0.991$  S/m;  $\epsilon_r = 55.34$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Center Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:

- Probe: EX3DV4 SN3617; ConvF(9.48, 9.48, 9.48); Calibrated: 2014-08-28;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 2014-01-23
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

System Performance Check at Frequencies above 1 GHz/d=15mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid:


dx=5mm, dy=5mm, dz=5mm

Reference Value = 55.94 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.60 W/kg

SAR(1 g) = 2.42 W/kg; SAR(10 g) = 1.61 W/kg

Maximum value of SAR (measured) = 3.05 W/kg

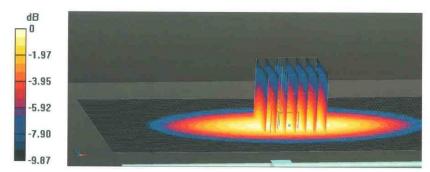


0 dB = 3.05 W/kg = 4.84 dBW/kg





# Impedance Measurement Plot for Body TSL

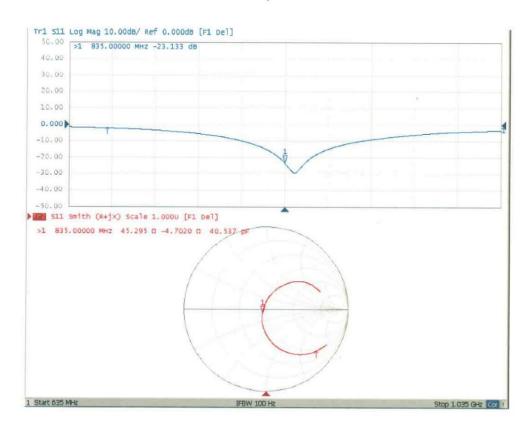



# 1900 MHz Dipole Calibration Certificate



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504



Client

E-mail: cttl@chinattl.com Http://www.chinattl.cn

CTTL(South Branch)

Certificate No:

Z14-97130

# **CALIBRATION CERTIFICATE**

Object

D1900V2 - SN: 5d088

Calibration Procedure(s)

TMC-OS-E-02-194

Calibration Procedures for dipole validation kits

Calibration date:

November 5, 2014

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)℃ and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	101919	01-Jul-14 (CTTL, No.J14X02146)	Jun-15
Power sensor NRP-Z91	101547	01-Jul-14 (CTTL, No.J14X02146)	Jun-15
Reference Probe EX3DV4	SN 3617	28-Aug-14(SPEAG,No.EX3-3617_Aug14)	Aug-15
DAE4	SN 1331	23-Jan-14 (SPEAG, DAE4-1331_Jan14)	Jan-15
Secondary Standards	ID#	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
SignalGeneratorMG3700A	6201052605	01-Jul-14 (CTTL, No.J14X02145)	Jun-15
Network Analyzer E5071C	MY46110673	15-Feb-14 (TMC, No.JZ14-781)	Feb-15

Calibrated by:

Name Function

Signature

Zhao Jing SAR Test Engineer

NO

Reviewed by:

Qi Dianyuan SAR Project Leader

202

Approved by:

Lu Bingsong Deputy Director of the laboratory

Issued: November 8, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.





Glossary:

TSL ConvF

N/A

tissue simulating liquid sensitivity in TSL / NORMx,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

#### **Additional Documentation:**

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
   No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.





#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.8.8.1222
Extrapolation	Advanced Extrapolation	4
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

### **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.9 ± 6 %	1.37 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

## SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.97 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	40.5 mW /g ± 20.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.18 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	20.9 mW /g ± 20.4 % (k=2)

# **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.1 ± 6 %	1.51 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

## SAR result with Head TSL

SAR averaged over 1 $cm^3$ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.2 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	41.1 mW /g ± 20.8 % (k=2)
SAR averaged over 10 $cm^3$ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	5.35 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	21.5 mW /g ± 20.4 % (k=2)

Page 3 of 8





## **Appendix**

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.0Ω+ 6.31jΩ	
Return Loss	- 22.9dB	

## Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.5Ω+ 6.01jΩ	
Return Loss	- 24.1dB	

# General Antenna Parameters and Design

Electrical Delay (one direction)	1.299 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

# **Additional EUT Data**

The second secon	
Manufactured by	SPEAG





# DASY5 Validation Report for Head TSL

Date: 05.11.2014

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d088

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1 Medium parameters used: f = 1900 MHz;  $\sigma$  = 1.365 S/m;  $\epsilon_r$  = 39.92;  $\rho$  = 1000 kg/m<sup>3</sup>

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 SN3617; ConvF(7.9, 7.9, 7.9); Calibrated: 2014-08-28;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 2014-01-23
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid:


dx=5mm, dy=5mm, dz=5mm

Reference Value = 103.0 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 18.7 W/kg

SAR(1 g) = 9.97 W/kg; SAR(10 g) = 5.18 W/kg

Maximum value of SAR (measured) = 14.5 W/kg

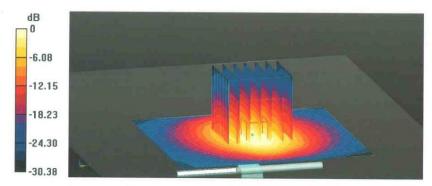


0 dB = 15.3 W/kg = 11.84 dBW/kg





# Impedance Measurement Plot for Head TSL

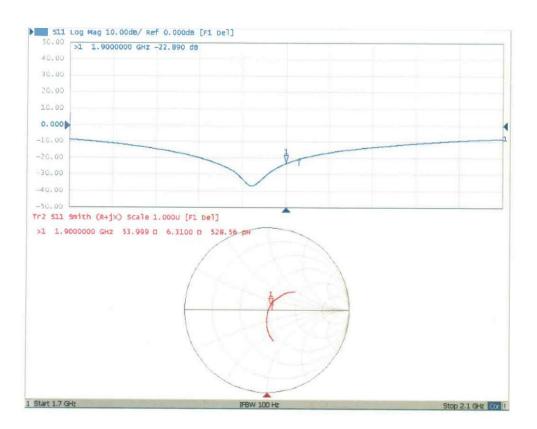





DASY5 Validation Report for Body TSL

Date: 05.11.2014

Test Laboratory: CTTL, Beijing, China

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d088** Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1 Medium parameters used: f = 1900 MHz;  $\sigma = 1.511$  S/m;  $\varepsilon_r = 54.12$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Left Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 SN3617; ConvF(7.58, 7.58, 7.58); Calibrated: 2014-08-28;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1331; Calibrated: 2014-01-23
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=2.0mm (EX-Probe)/Zoom Scan (7x7x7) (8x7x7)/Cube 0: Measurement grid:


dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.67 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 18.4 W/kg

SAR(1 g) = 10.2 W/kg; SAR(10 g) = 5.35 W/kg

Maximum value of SAR (measured) = 14.6 W/kg

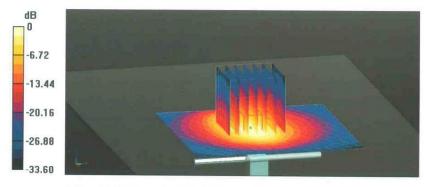


0 dB = 15.7 W/kg = 11.96 dBW/kg





# Impedance Measurement Plot for Body TSL

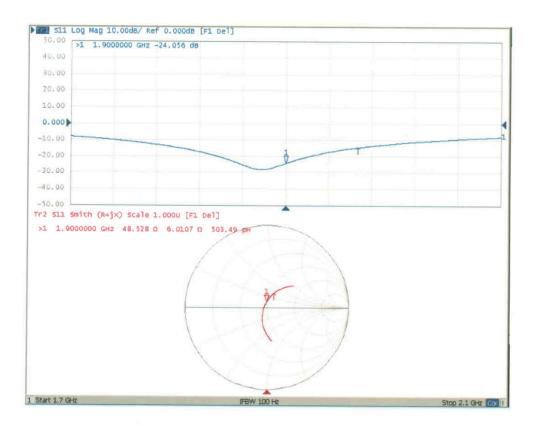

Certificate No: Z14-97130

Page 8 of 8