




# **Appendix D**






## **Photographs**

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details




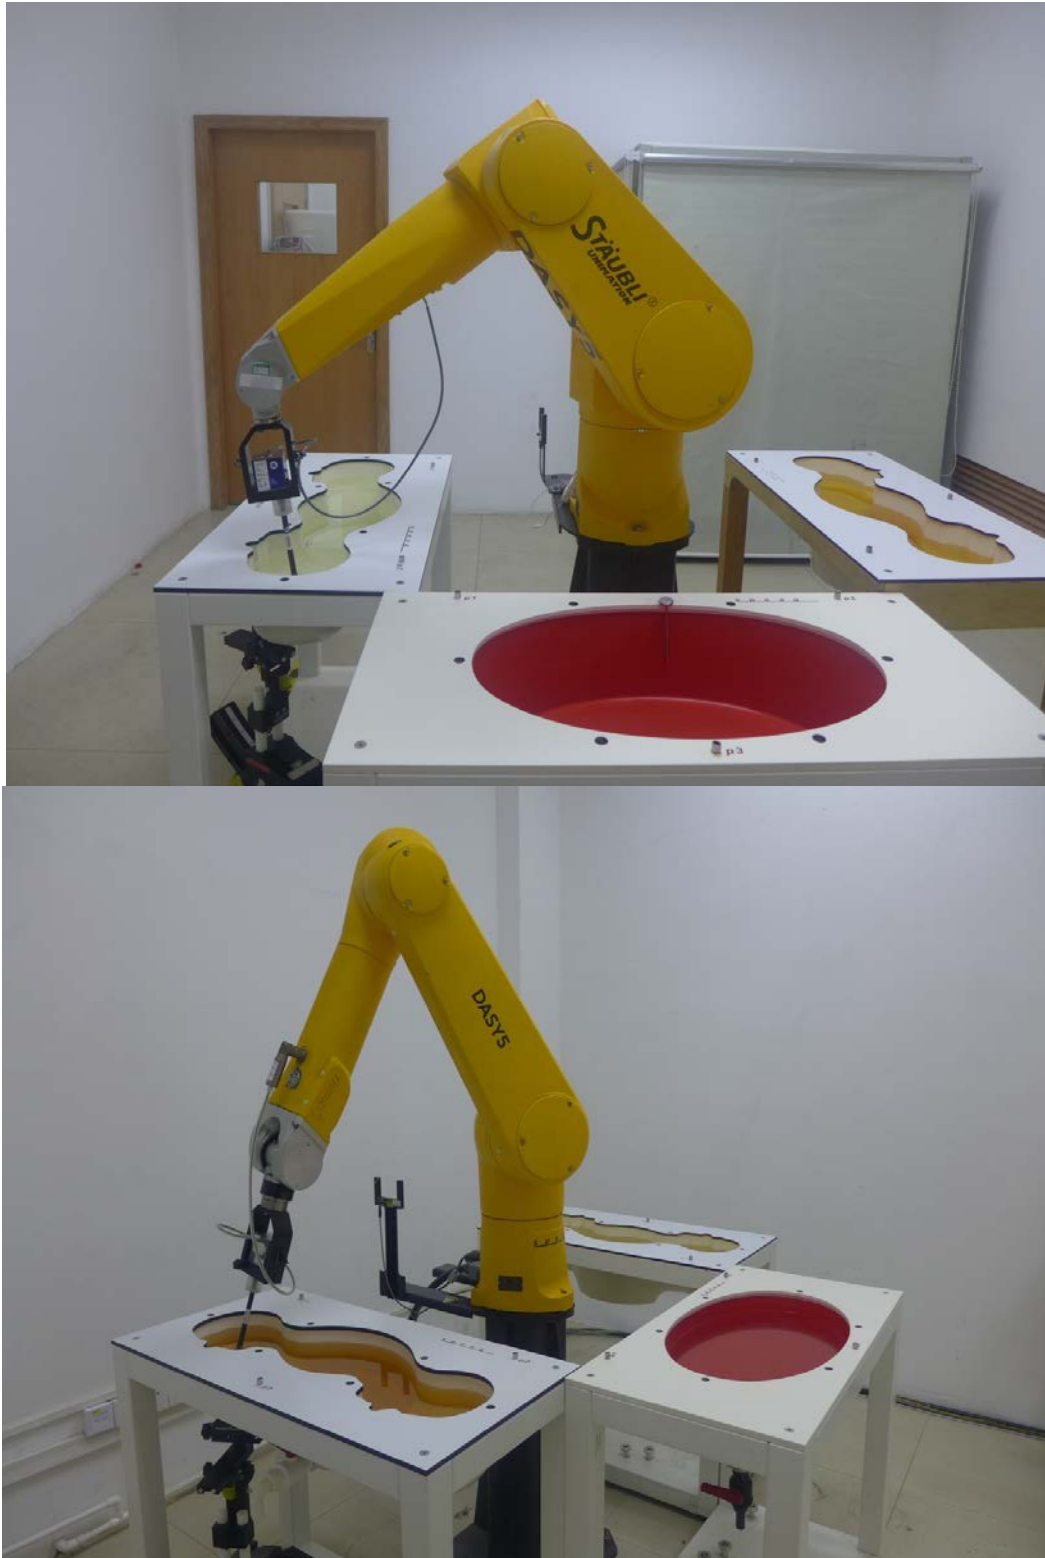


## 1. SAR measurement System

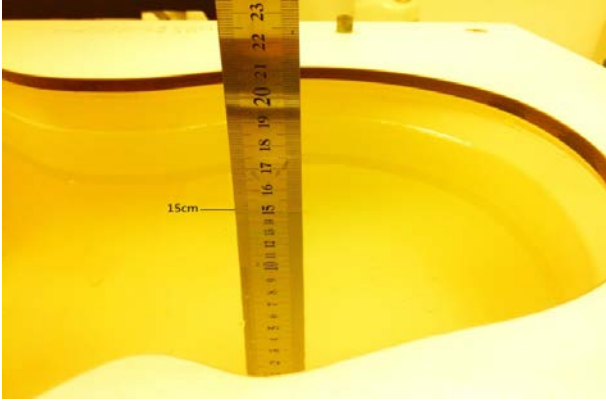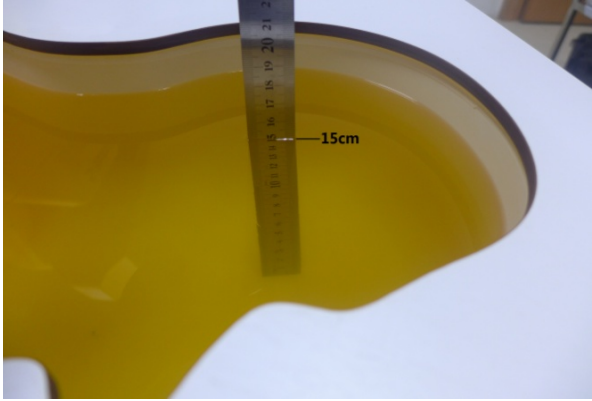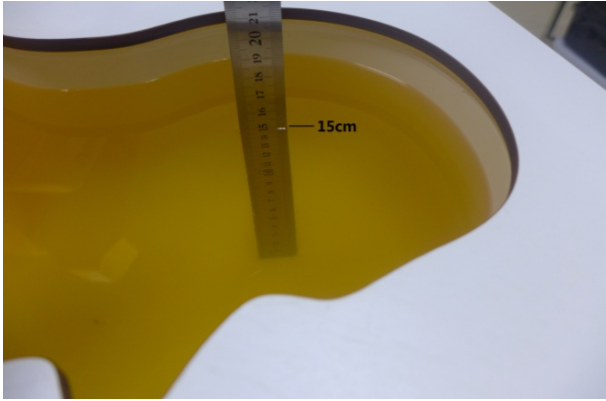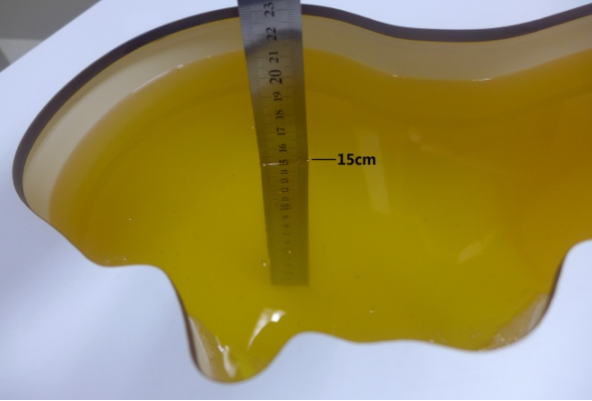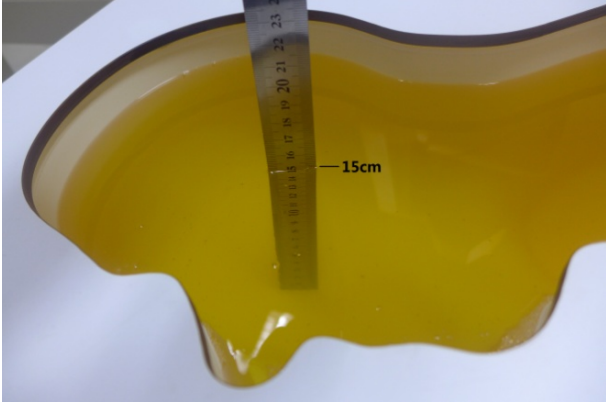

## 2. Photographs of Tissue Simulate Liquid

<p><b>Photo 1: Tissue Simulant Liquid for Head 835</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Head 1750</b></p>
	
<p><b>Photo 3: Tissue Simulant Liquid for Head 1900</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Head 2450</b></p>
	
<p><b>Photo 5: Tissue Simulant Liquid for Head 2600</b></p>	<p><b>NA</b></p>
	<p><b>NA</b></p>
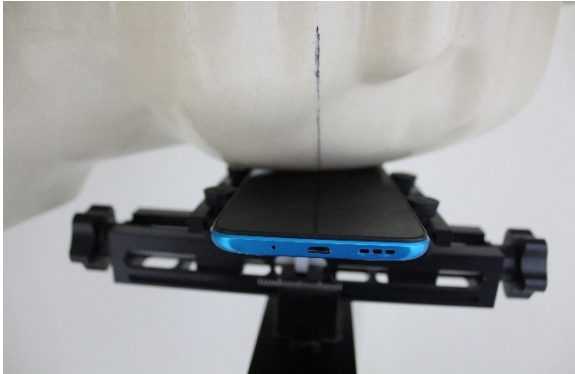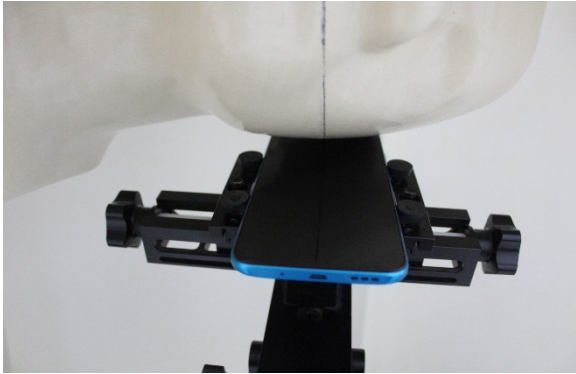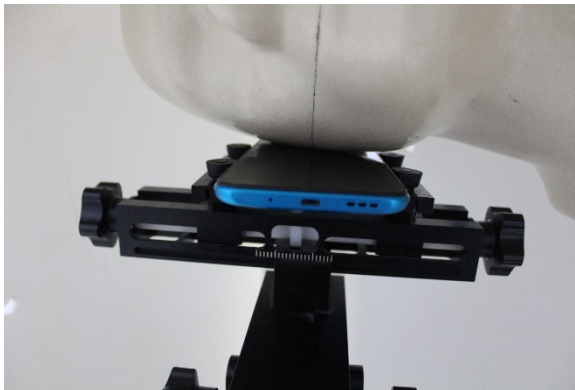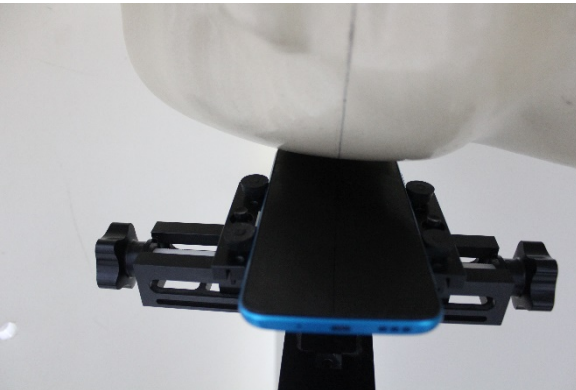
### 3. Photographs of EUT test position

<p>Photo 6: Left cheek</p>	<p>Photo 7: Left tilted</p>
	
<p>Photo 8: Right cheek</p>	<p>Photo 9: Right tilted</p>
	
<p>Photo 10: Front side 10mm</p>	<p>Photo 11: Back side 10mm</p>
	






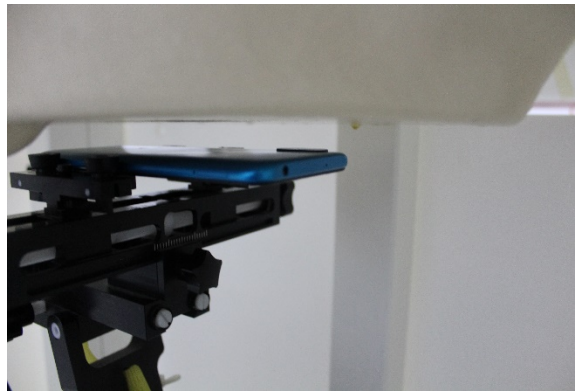

<p><b>Photo 12: Left side 10mm</b></p>	<p><b>Photo 13: Right side 10mm</b></p>
	
<p><b>Photo 14: Top side 10mm</b></p>	<p><b>Photo 15: Bottom side 10mm</b></p>
	
<p><b>Photo 16: Front side 15mm</b></p>	<p><b>Photo 17: Back side 15mm</b></p>
	

Photo 18: Bottom side 15mm	NA
	NA

#### 4. EUT Constructional Details

Photo 19: Front View	Photo 20: Back View
