

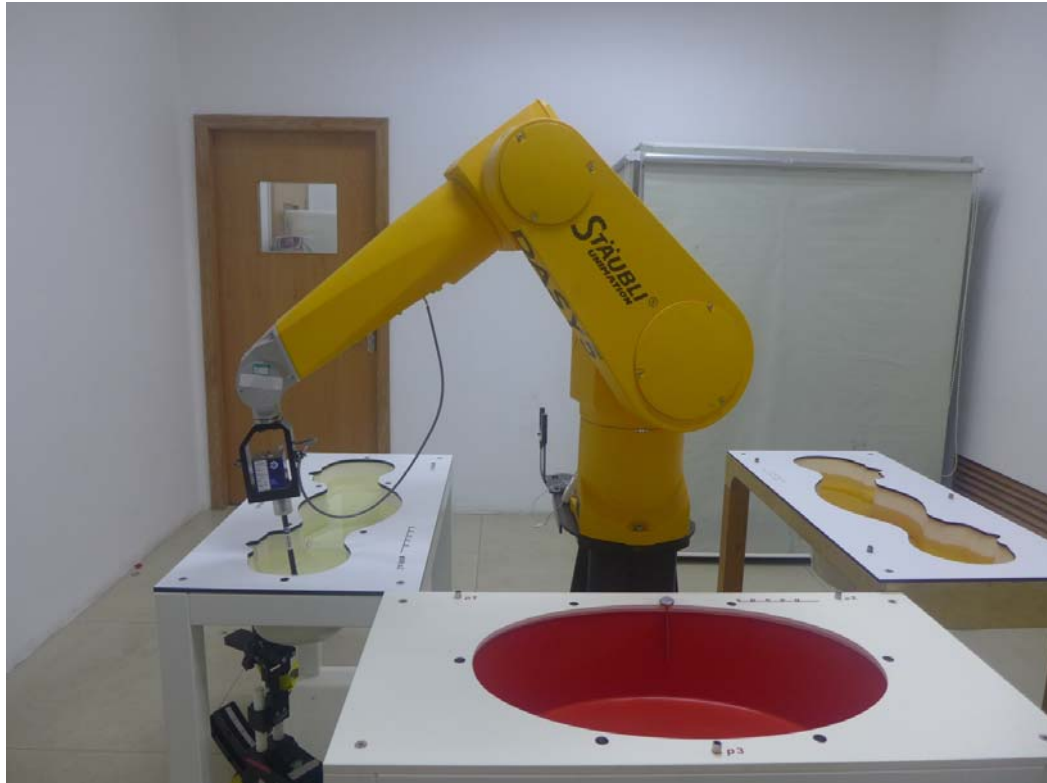


Appendix D

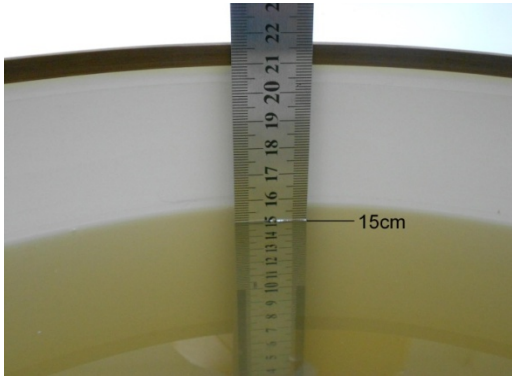
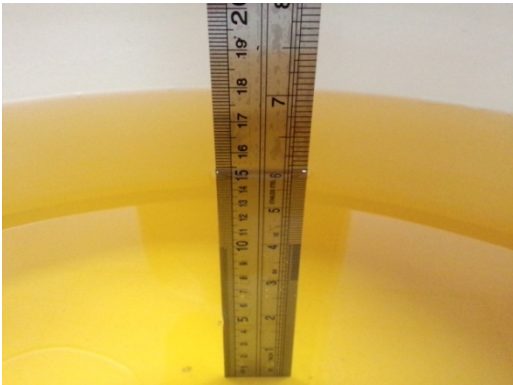
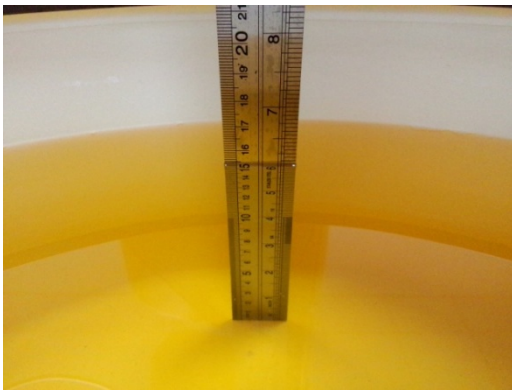

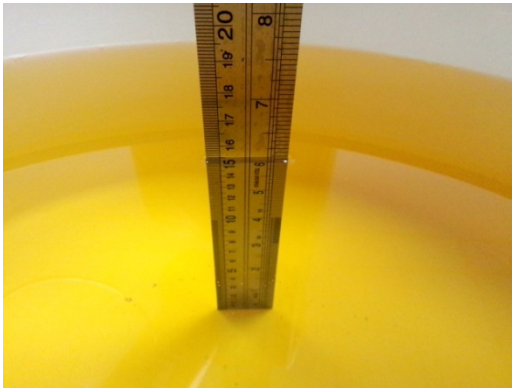
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Head 1750</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1900</p>	<p>Photo 4: Tissue Simulant Liquid for Head 2450</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2600</p>	<p>NA</p>
	<p>NA</p>

3. Photographs of EUT test position

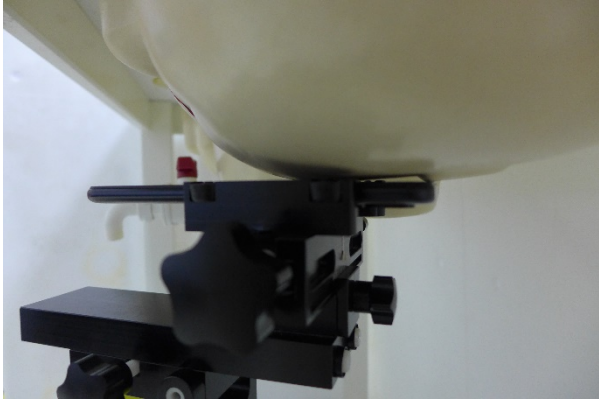
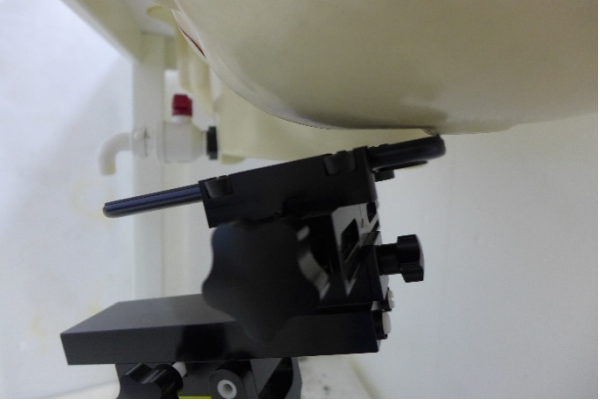
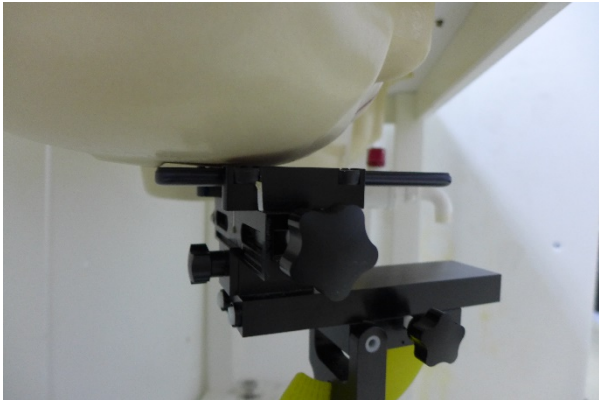



<p>Photo 6: Left touch cheek</p>	<p>Photo 7: Left tilted 15 degree</p>
	
<p>Photo 8: Right touch cheek</p>	<p>Photo 9: Right tilted 15 degree</p>
	
<p>Photo 10: Front side 10mm</p>	<p>Photo 11: Back side 10mm</p>
	



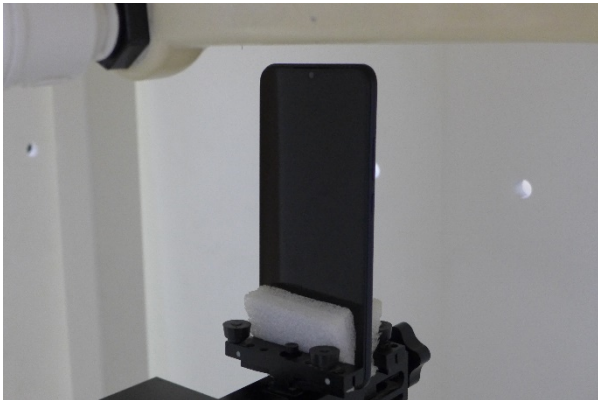
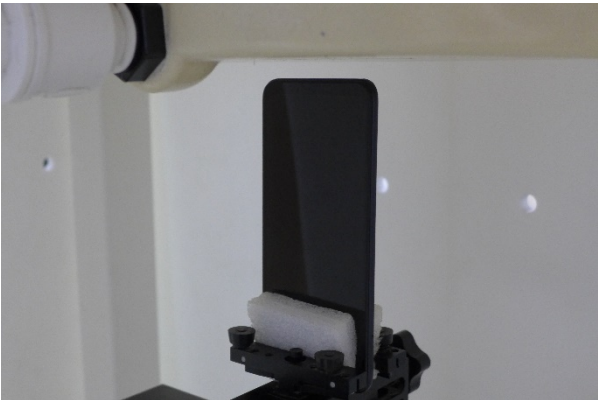



Photo 12: Left side 10mm	Photo 13: Right side 10mm
	
Photo 14: Top side 10mm	Photo 15: Bottom side 10mm
	
Photo 16: Front side 15mm	Photo 17: Back side 15mm
	

Photo 18: Bottom side 15mm	NA
	NA

4. EUT Constructional Details

