




Appendix D







Photographs

| |
|--|
| 1. SAR measurement System |
| 2. Photographs of Tissue Simulate Liquid |
| 3. Photographs of EUT test position |
| 4. EUT Constructional Details |



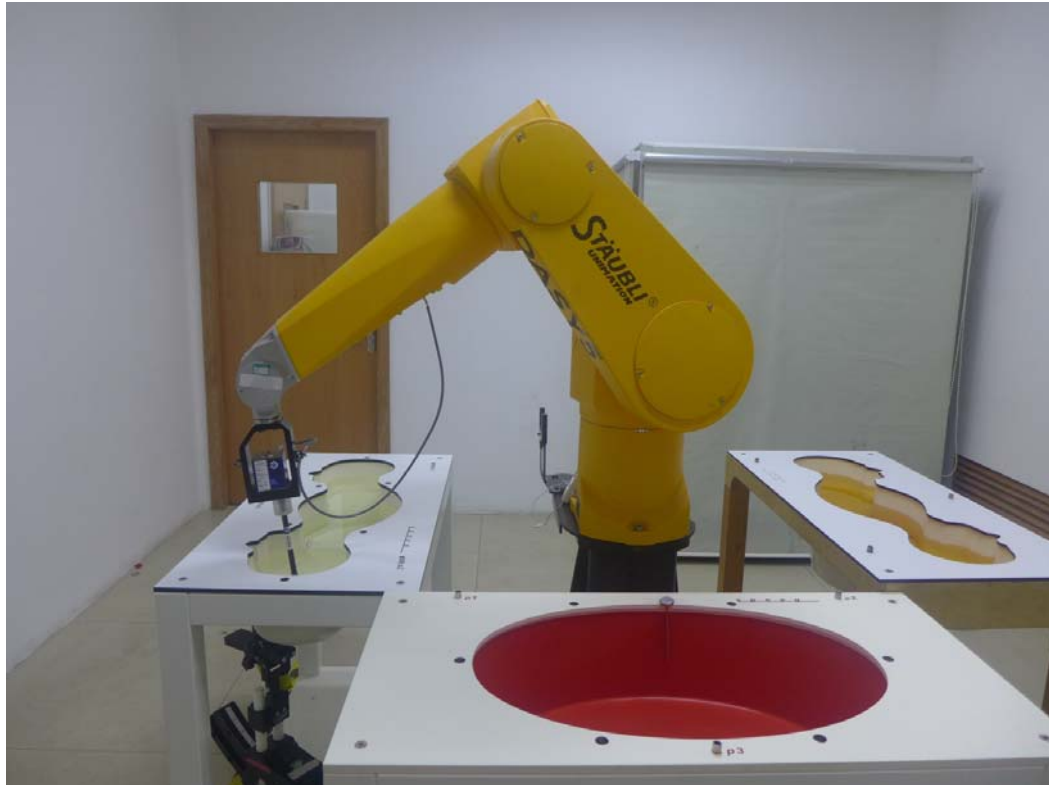


1. SAR measurement System



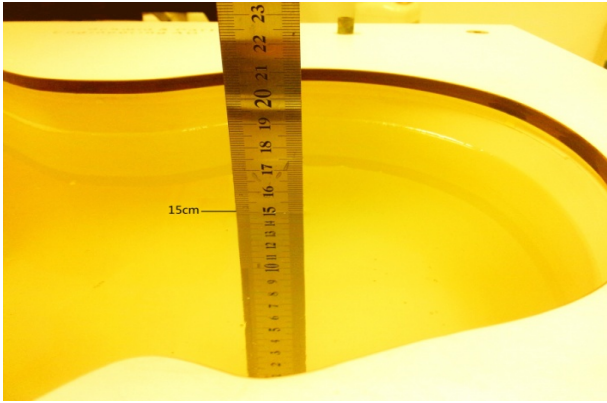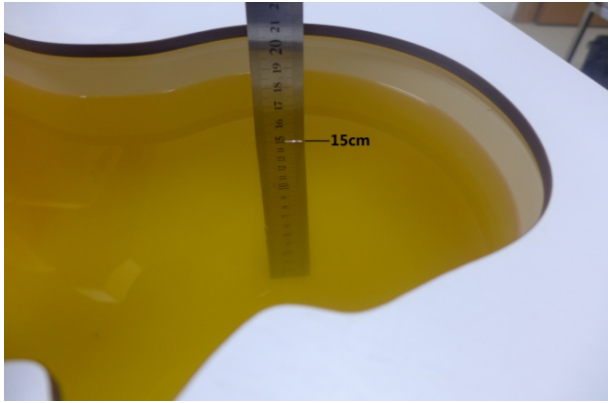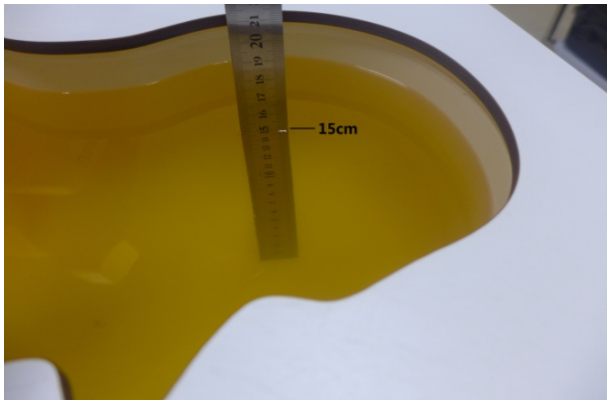
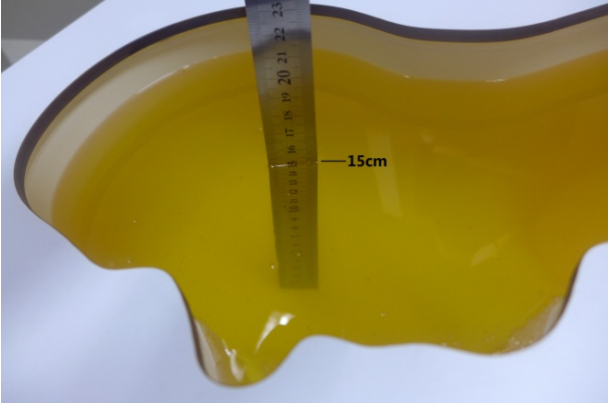
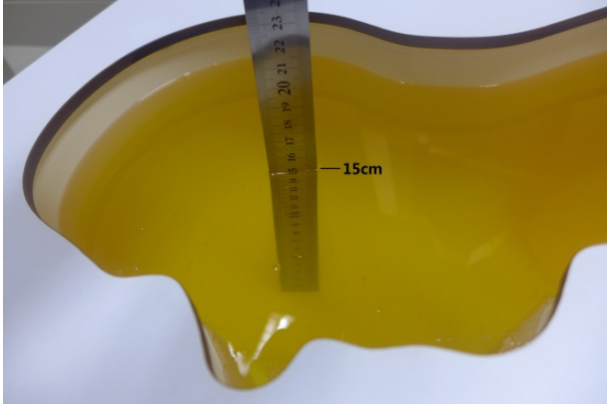
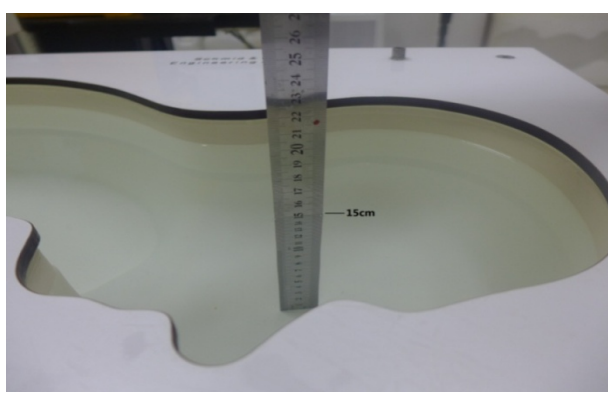



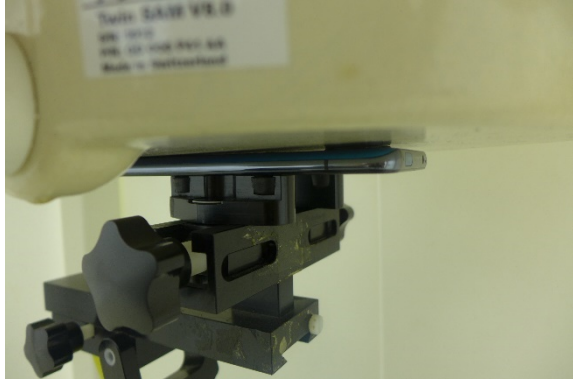
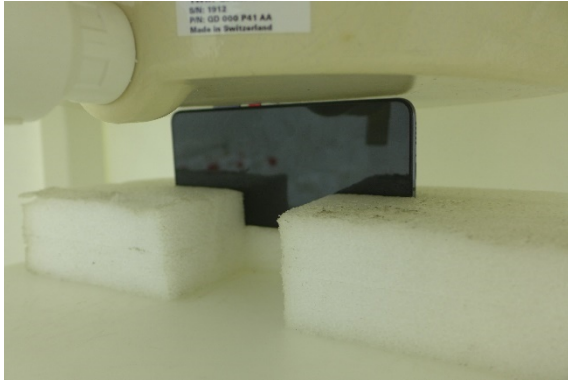
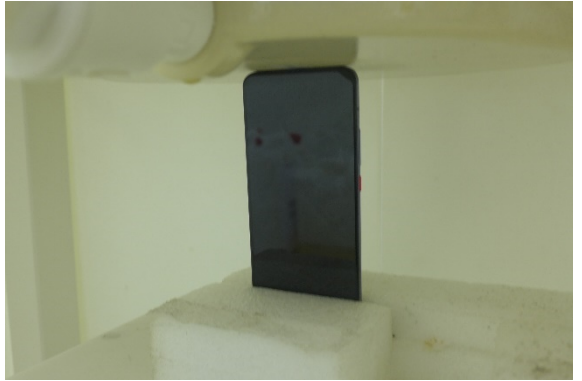
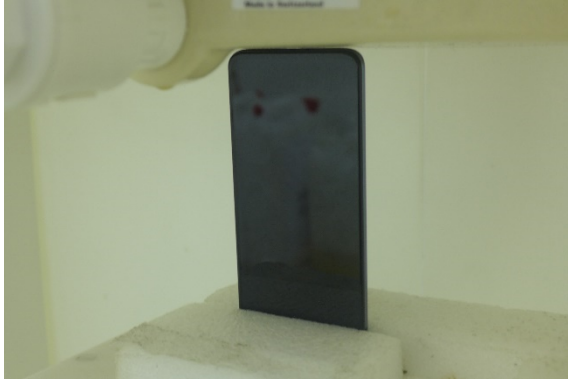
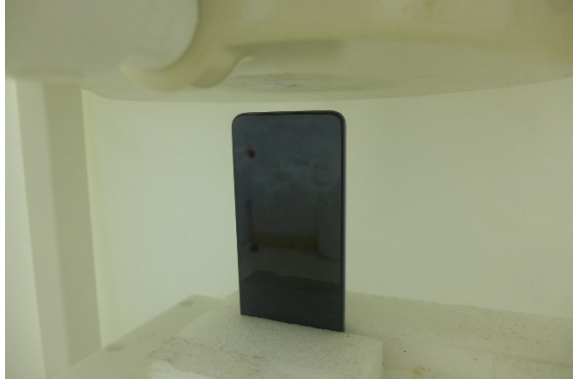
2. Photographs of Tissue Simulate Liquid
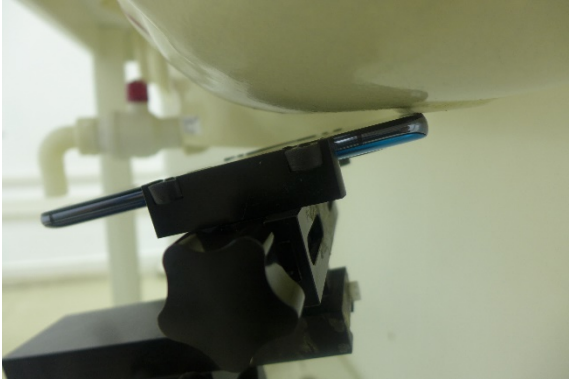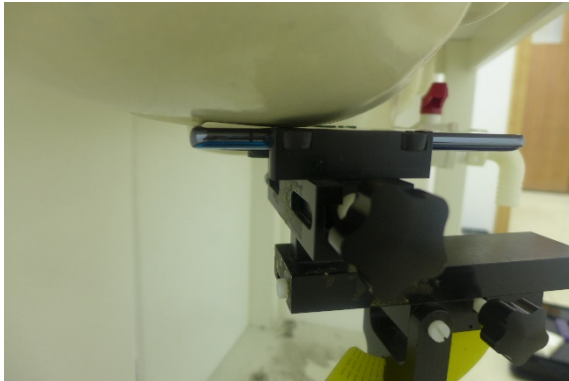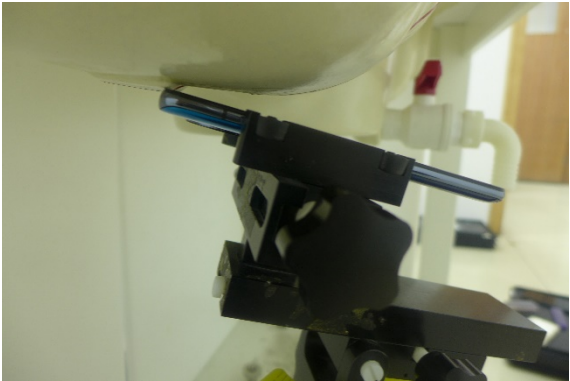
| | |
|---|--|
| <p>Photo 1: Tissue Simulant Liquid for Head 835</p> | <p>Photo 2: Tissue Simulant Liquid for Head 1750</p> |
|  |  |
| <p>Photo 3: Tissue Simulant Liquid for Head 1900</p> | <p>Photo 4: Tissue Simulant Liquid for Head 2450</p> |
|  |  |
| <p>Photo 5: Tissue Simulant Liquid for Head 2600</p> | <p>Photo 6: Tissue Simulant Liquid for Head 5G</p> |
|  |  |


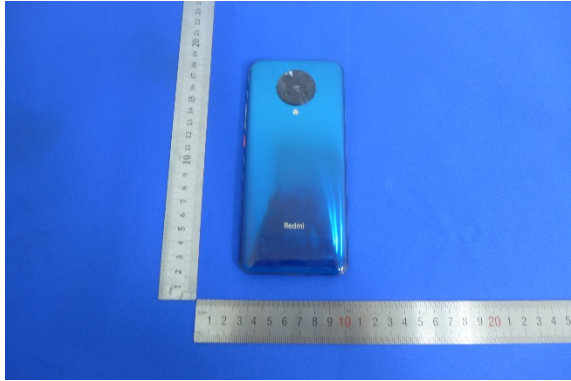
3. Photographs of EUT test position

| | |
|---|--|
| <p align="center">Photo 7: Left cheek</p> | <p align="center">Photo 8: Left tilted</p> |
|  |  |
| <p align="center">Photo 9: Right cheek</p> | <p align="center">Photo 10: Right tilted</p> |
|  |  |
| <p align="center">Photo 11: Front side 15mm</p> | <p align="center">Photo 12: Back side 15mm</p> |
|  |  |
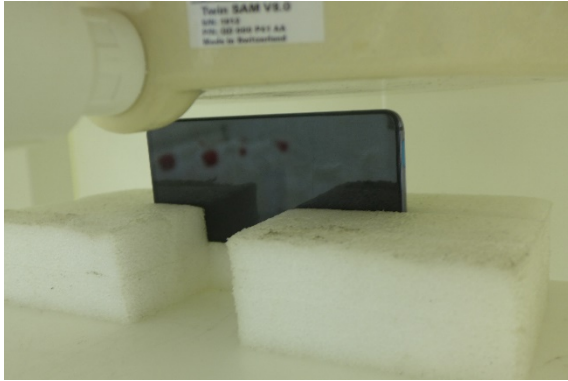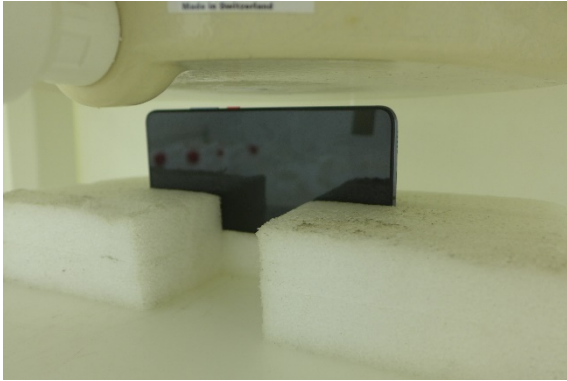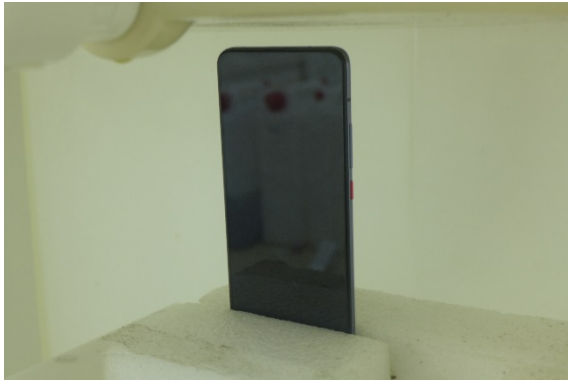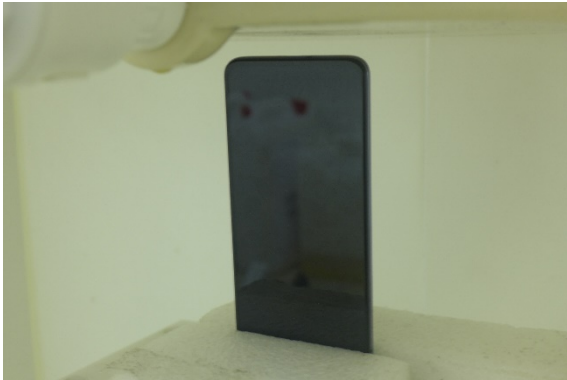
| Photo 13: Front side 10mm | Photo 14: Back side 10mm |
|---|--|
|  |  |
| Photo 15: Left side 10mm | Photo 16: Right side 10mm |
|  |  |
| Photo 17: Top side 10mm | Photo 18: Bottom side 10mm |
|  |  |

| | |
|---|--|
| <p>Photo 19: Front side 0mm</p> | <p>Photo 20: Back side 0mm</p> |
|  |  |
| <p>Photo 21: Right side 0mm</p> | <p>Photo 22: Top side 0mm</p> |
|  |  |
| <p>Photo 23: Bottom side 0mm</p> | <p>Photo 24: Bottom side 15mm</p> |
|  |  |

4. EUT Constructional Details

| Photo 25: Front View | Photo 26: Back View |
|---|--|
|  |  |