

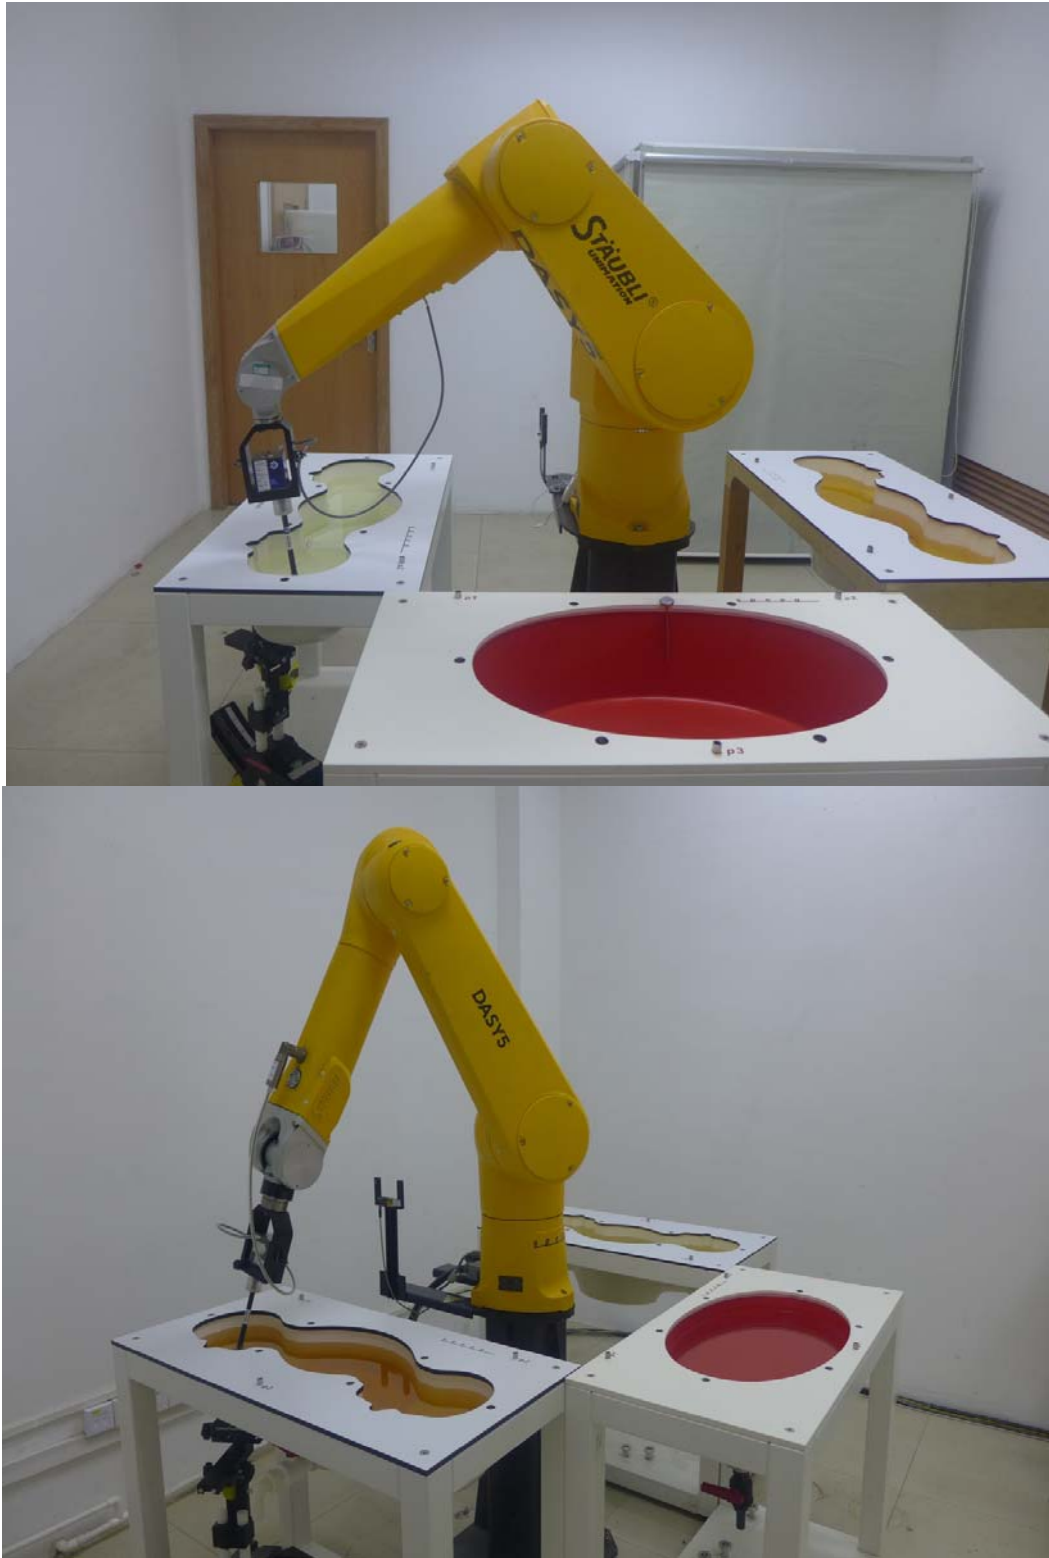


Appendix D

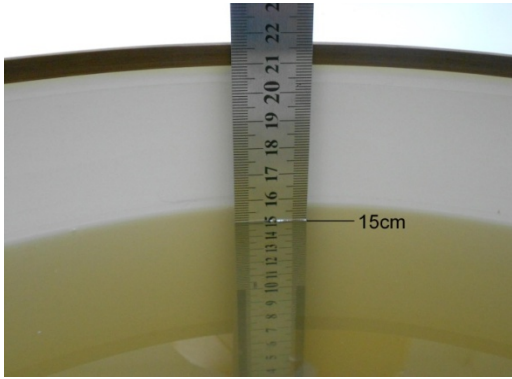
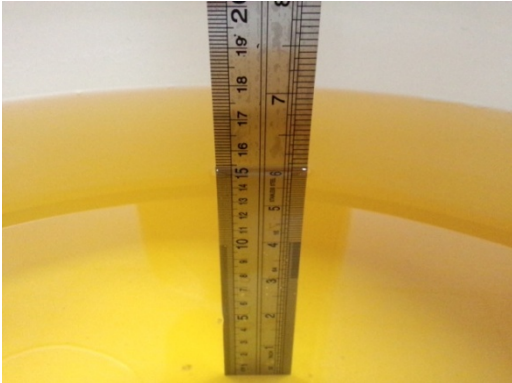

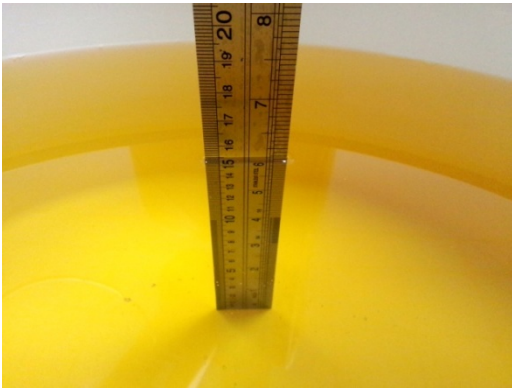

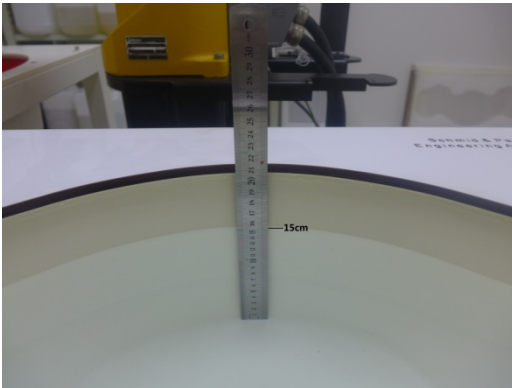
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

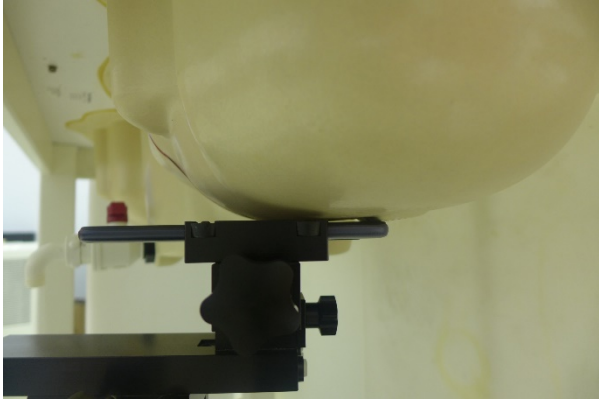
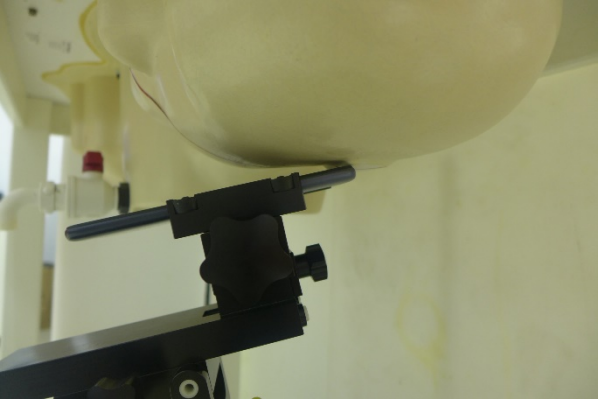
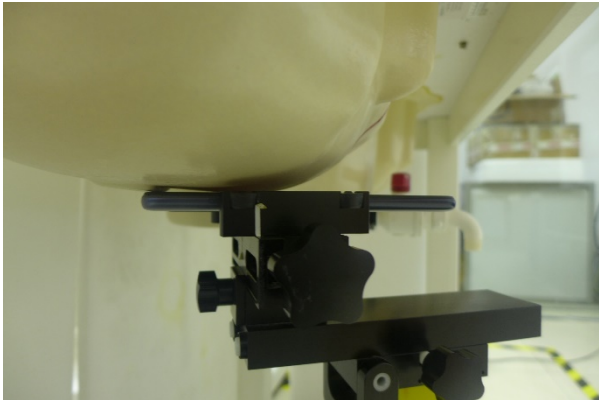
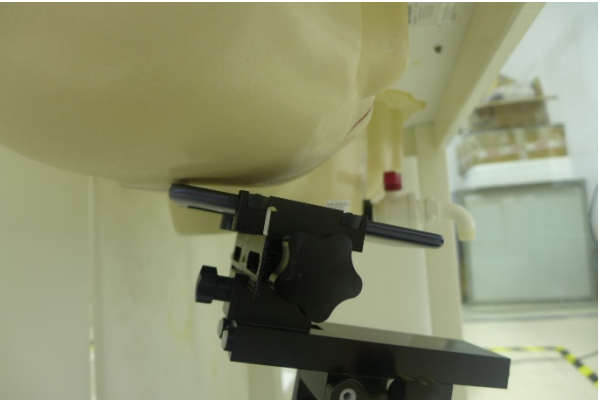


1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Head 1750
	
Photo 3: Tissue Simulant Liquid for Head 1900	Photo 4: Tissue Simulant Liquid for Head 2450
	
Photo 5: Tissue Simulant Liquid for Head 2600	Photo 6: Tissue Simulant Liquid for Head 5G
	

3. Photographs of EUT test position

<p>Photo 7: Left touch cheek</p>	<p>Photo 8: Left tilted 15 degree</p>
	
<p>Photo 9: Right touch cheek</p>	<p>Photo 10: Right tilted 15 degree</p>
	
<p>Photo 11: Front side 10mm</p>	<p>Photo 12: Back side 10mm</p>
	

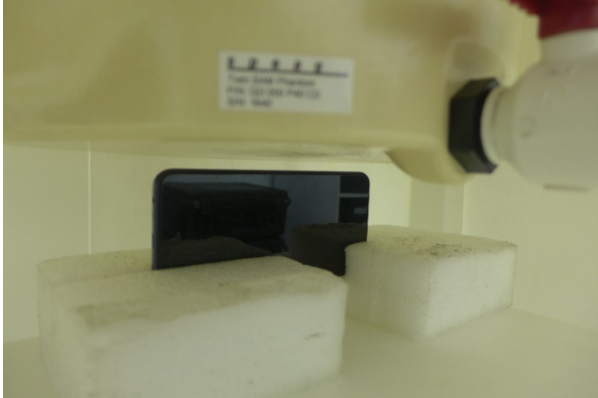

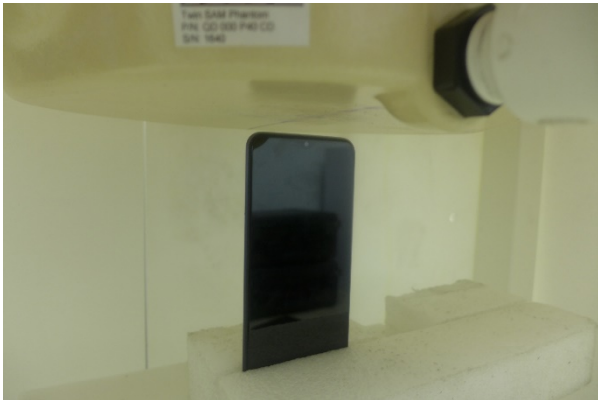


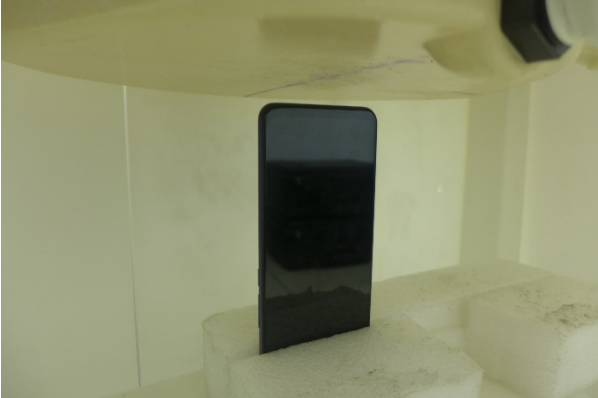


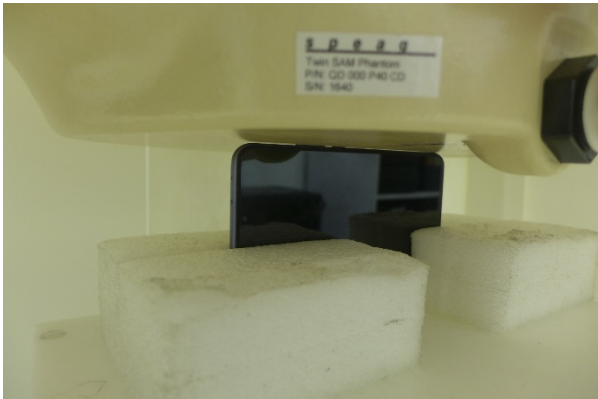

<p>Photo 13: Left side 10mm</p>	<p>Photo 14: Right side 10mm</p>
	
<p>Photo 15: Top side 10mm</p>	<p>Photo 16: Bottom side 10mm</p>
	
<p>Photo 17: Back side 15mm</p>	<p>Photo 18: Bottom side 15mm</p>
	

Photo 19: Front side 0mm	Photo 20: Back side 0mm
	
Photo 21: Right side 0mm	Photo 22: Top side 0mm
 <p>Label text: SGS Two SAM Phasor PN: QD 000 P40 CD SN: 1642</p>	

4. EUT Constructional Details

