

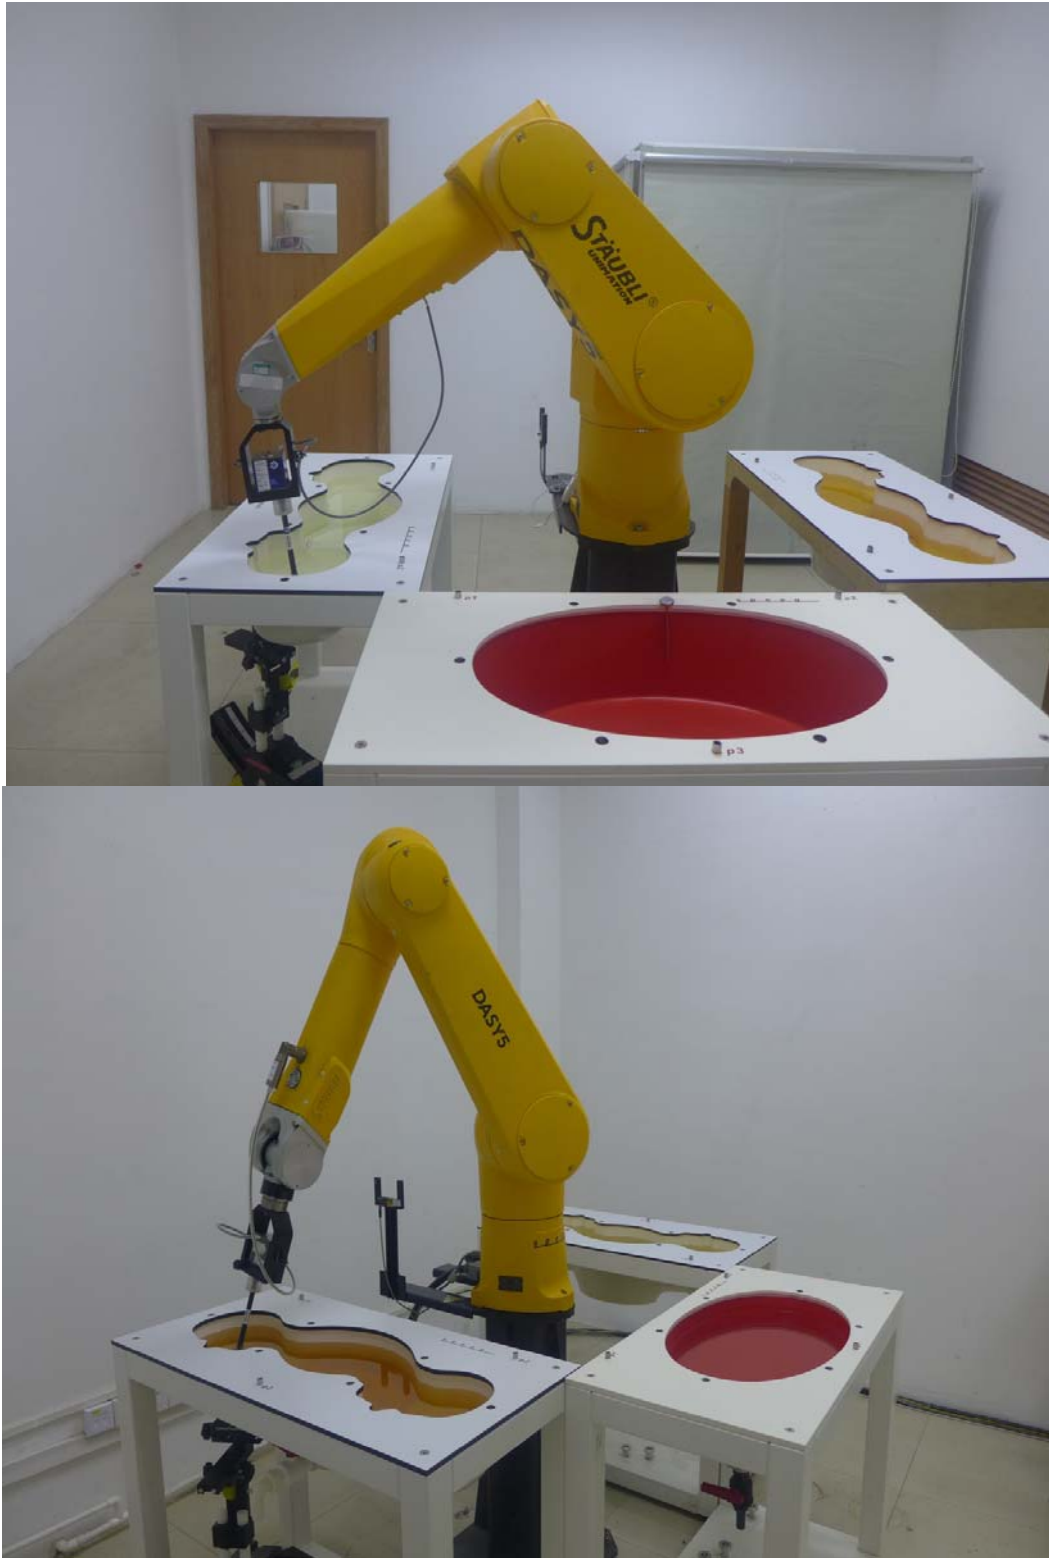


# **Appendix D**

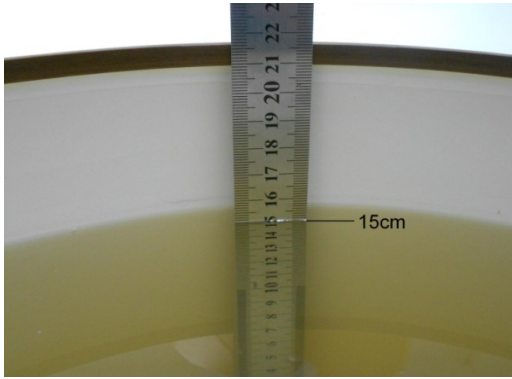
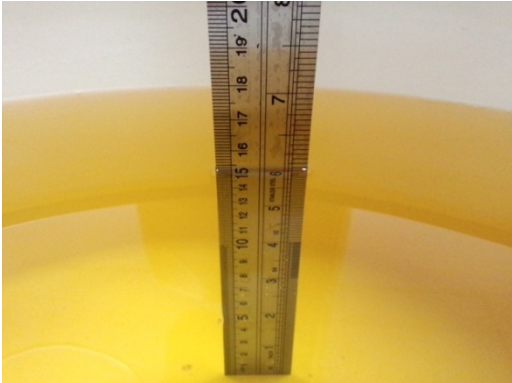

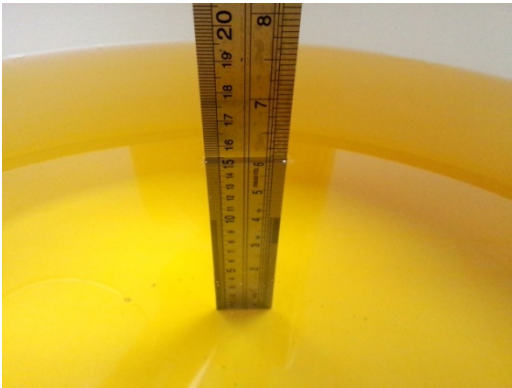

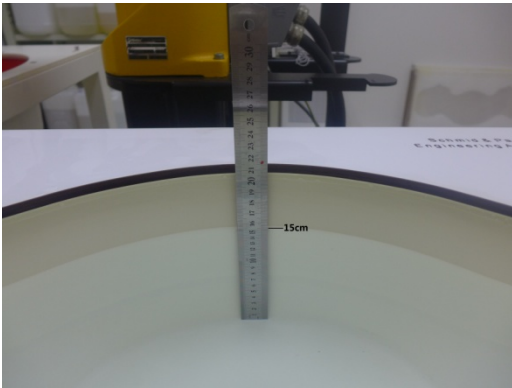
## **Photographs**

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## 1. SAR measurement System



## 2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Head 1750</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1900</p>	<p>Photo 4: Tissue Simulant Liquid for Head 2450</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2600</p>	<p>Photo 6: Tissue Simulant Liquid for Head 5G</p>
	

### 3. Photographs of EUT test position

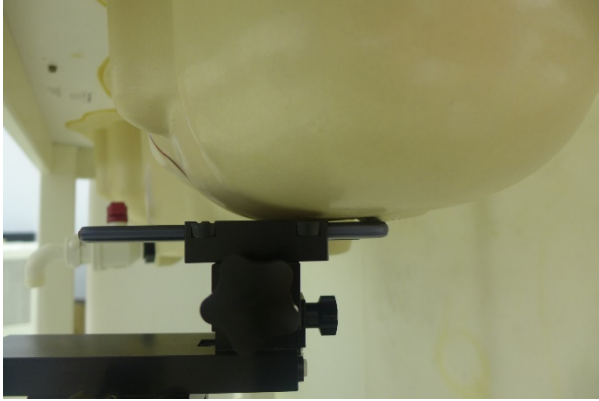
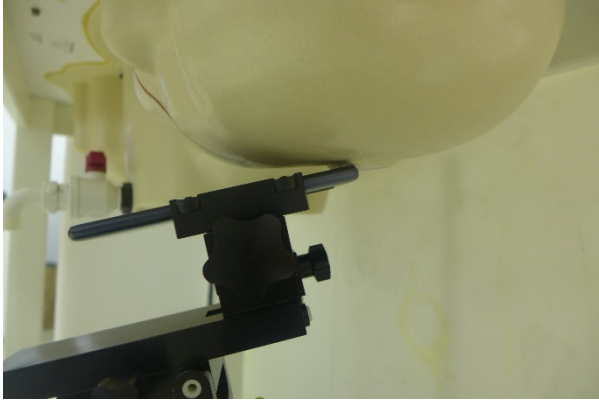
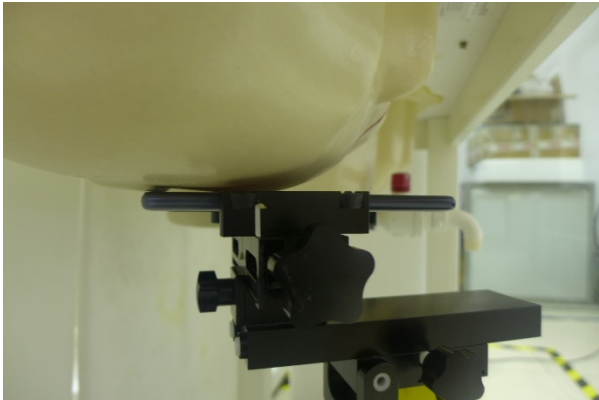



<p><b>Photo 7: Left touch cheek</b></p>	<p><b>Photo 8: Left tilted 15 degree</b></p>
	
<p><b>Photo 9: Right touch cheek</b></p>	<p><b>Photo 10: Right tilted 15 degree</b></p>
	
<p><b>Photo 11: Front side 10mm</b></p>	<p><b>Photo 12: Back side 10mm</b></p>
	



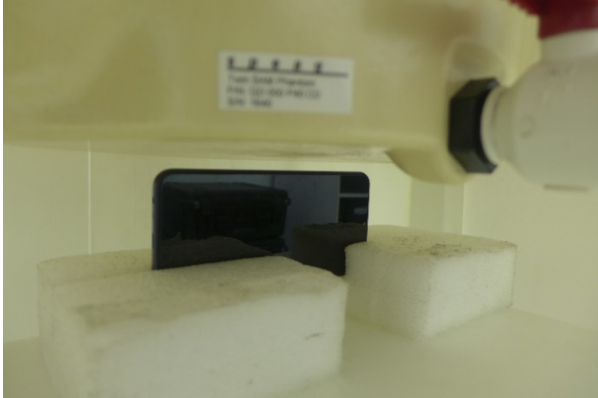

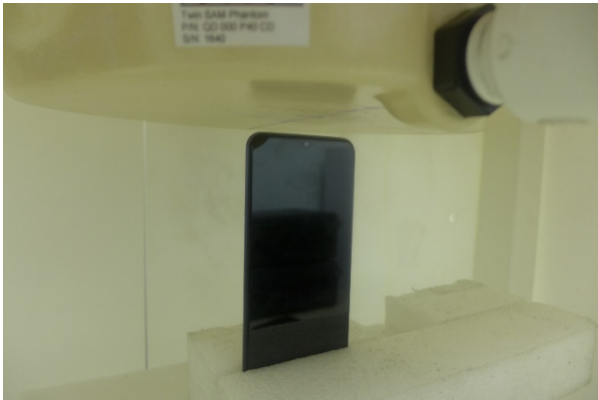


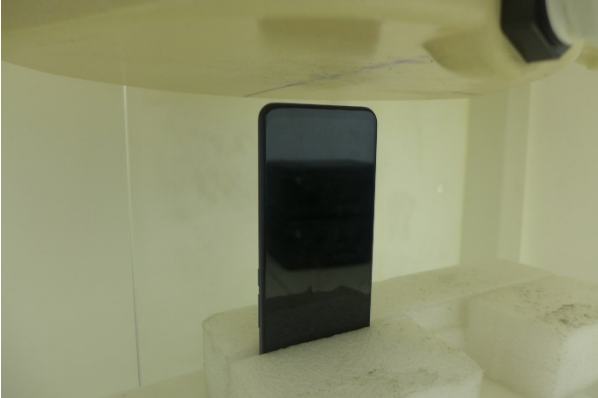


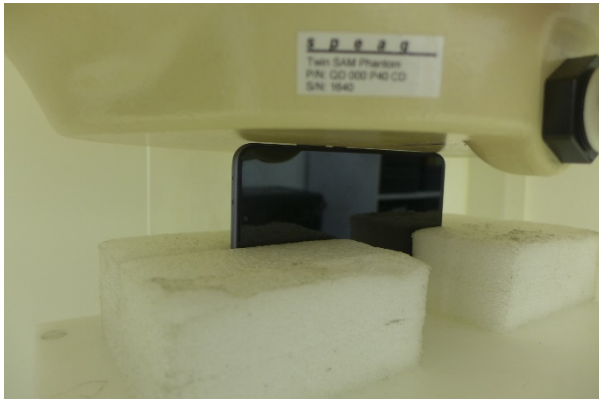

Photo 13: Left side 10mm	Photo 14: Right side 10mm
	
Photo 15: Top side 10mm	Photo 16: Bottom side 10mm
	
Photo 17: Back side 15mm	Photo 18: Bottom side 15mm
	

Photo 19: Front side 0mm	Photo 20: Back side 0mm
	
Photo 21: Right side 0mm	Photo 22: Top side 0mm
	

#### 4. EUT Constructional Details

