



## DASY/EASY – Parameters of Probe: EX3DV4 – SN:3923

### Calibration Parameter Determined in Head Tissue Simulating Media

f [MHz] <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unct. (k=2)
750	41.9	0.89	10.67	10.67	10.67	0.40	0.75	± 12.1%
835	41.5	0.90	10.35	10.35	10.35	0.17	1.16	± 12.1%
1750	40.1	1.37	8.90	8.90	8.90	0.22	1.13	± 12.1%
1900	40.0	1.40	8.55	8.55	8.55	0.24	1.09	± 12.1%
2300	39.5	1.67	8.29	8.29	8.29	0.50	0.69	± 12.1%
2450	39.2	1.80	7.95	7.95	7.95	0.55	0.69	± 12.1%
2600	39.0	1.96	7.70	7.70	7.70	0.37	0.89	± 12.1%
3300	38.2	2.71	7.36	7.36	7.36	0.42	0.91	± 13.3%
3500	37.9	2.91	7.03	7.03	7.03	0.40	0.98	± 13.3%
3700	37.7	3.12	6.73	6.73	6.73	0.41	1.00	± 13.3%
3900	37.5	3.32	6.75	6.75	6.75	0.35	1.41	± 13.3%
4100	37.2	3.53	6.70	6.70	6.70	0.40	1.15	± 13.3%
4400	36.9	3.84	6.47	6.47	6.47	0.30	1.50	± 13.3%
4600	36.7	4.04	6.30	6.30	6.30	0.40	1.35	± 13.3%
4800	36.4	4.25	6.22	6.22	6.22	0.40	1.45	± 13.3%
4950	36.3	4.40	5.90	5.90	5.90	0.40	1.45	± 13.3%
5250	35.9	4.71	5.45	5.45	5.45	0.40	1.70	± 13.3%
5600	35.5	5.07	4.92	4.92	4.92	0.50	1.30	± 13.3%
5750	35.4	5.22	4.91	4.91	4.91	0.50	1.47	± 13.3%

<sup>C</sup> Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequency below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.


<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.





Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

## Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

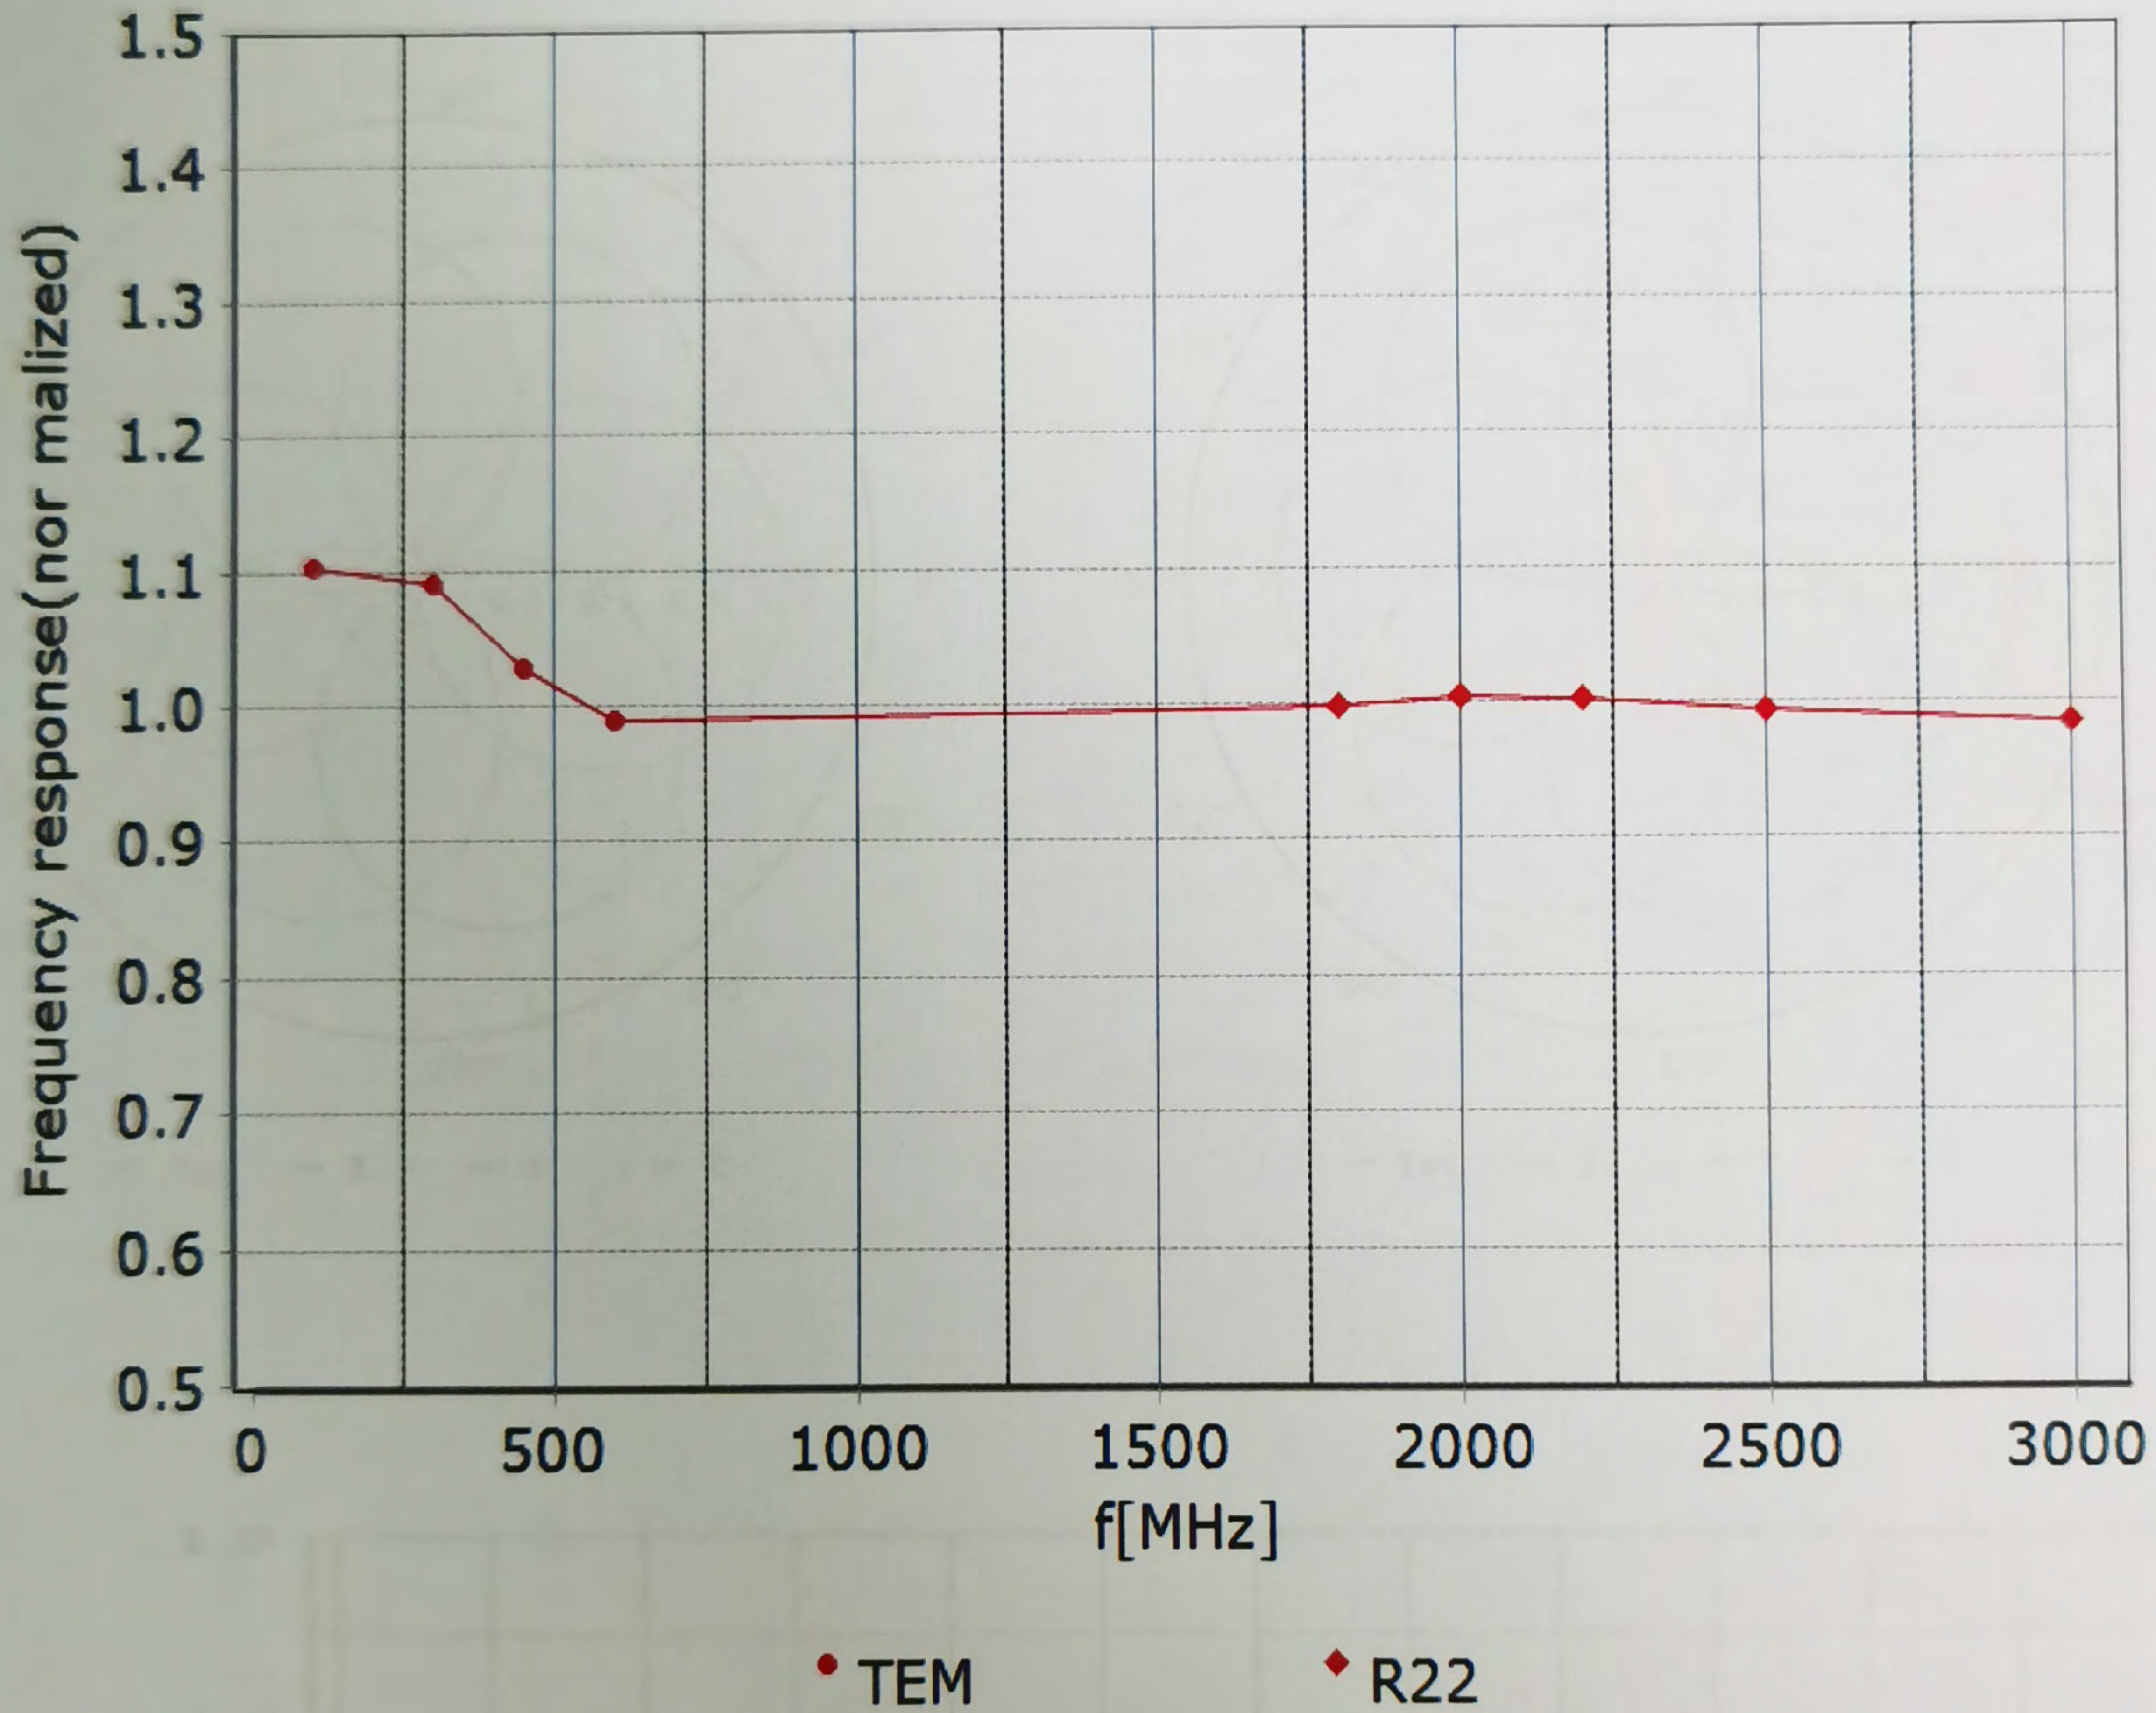

Uncertainty of Frequency Response of E-field:  $\pm 7.4\%$  ( $k=2$ )








## Receiving Pattern ( $\Phi$ ), $\theta=0^\circ$

**f=600 MHz, TEM**

**f=1800 MHz, R22**

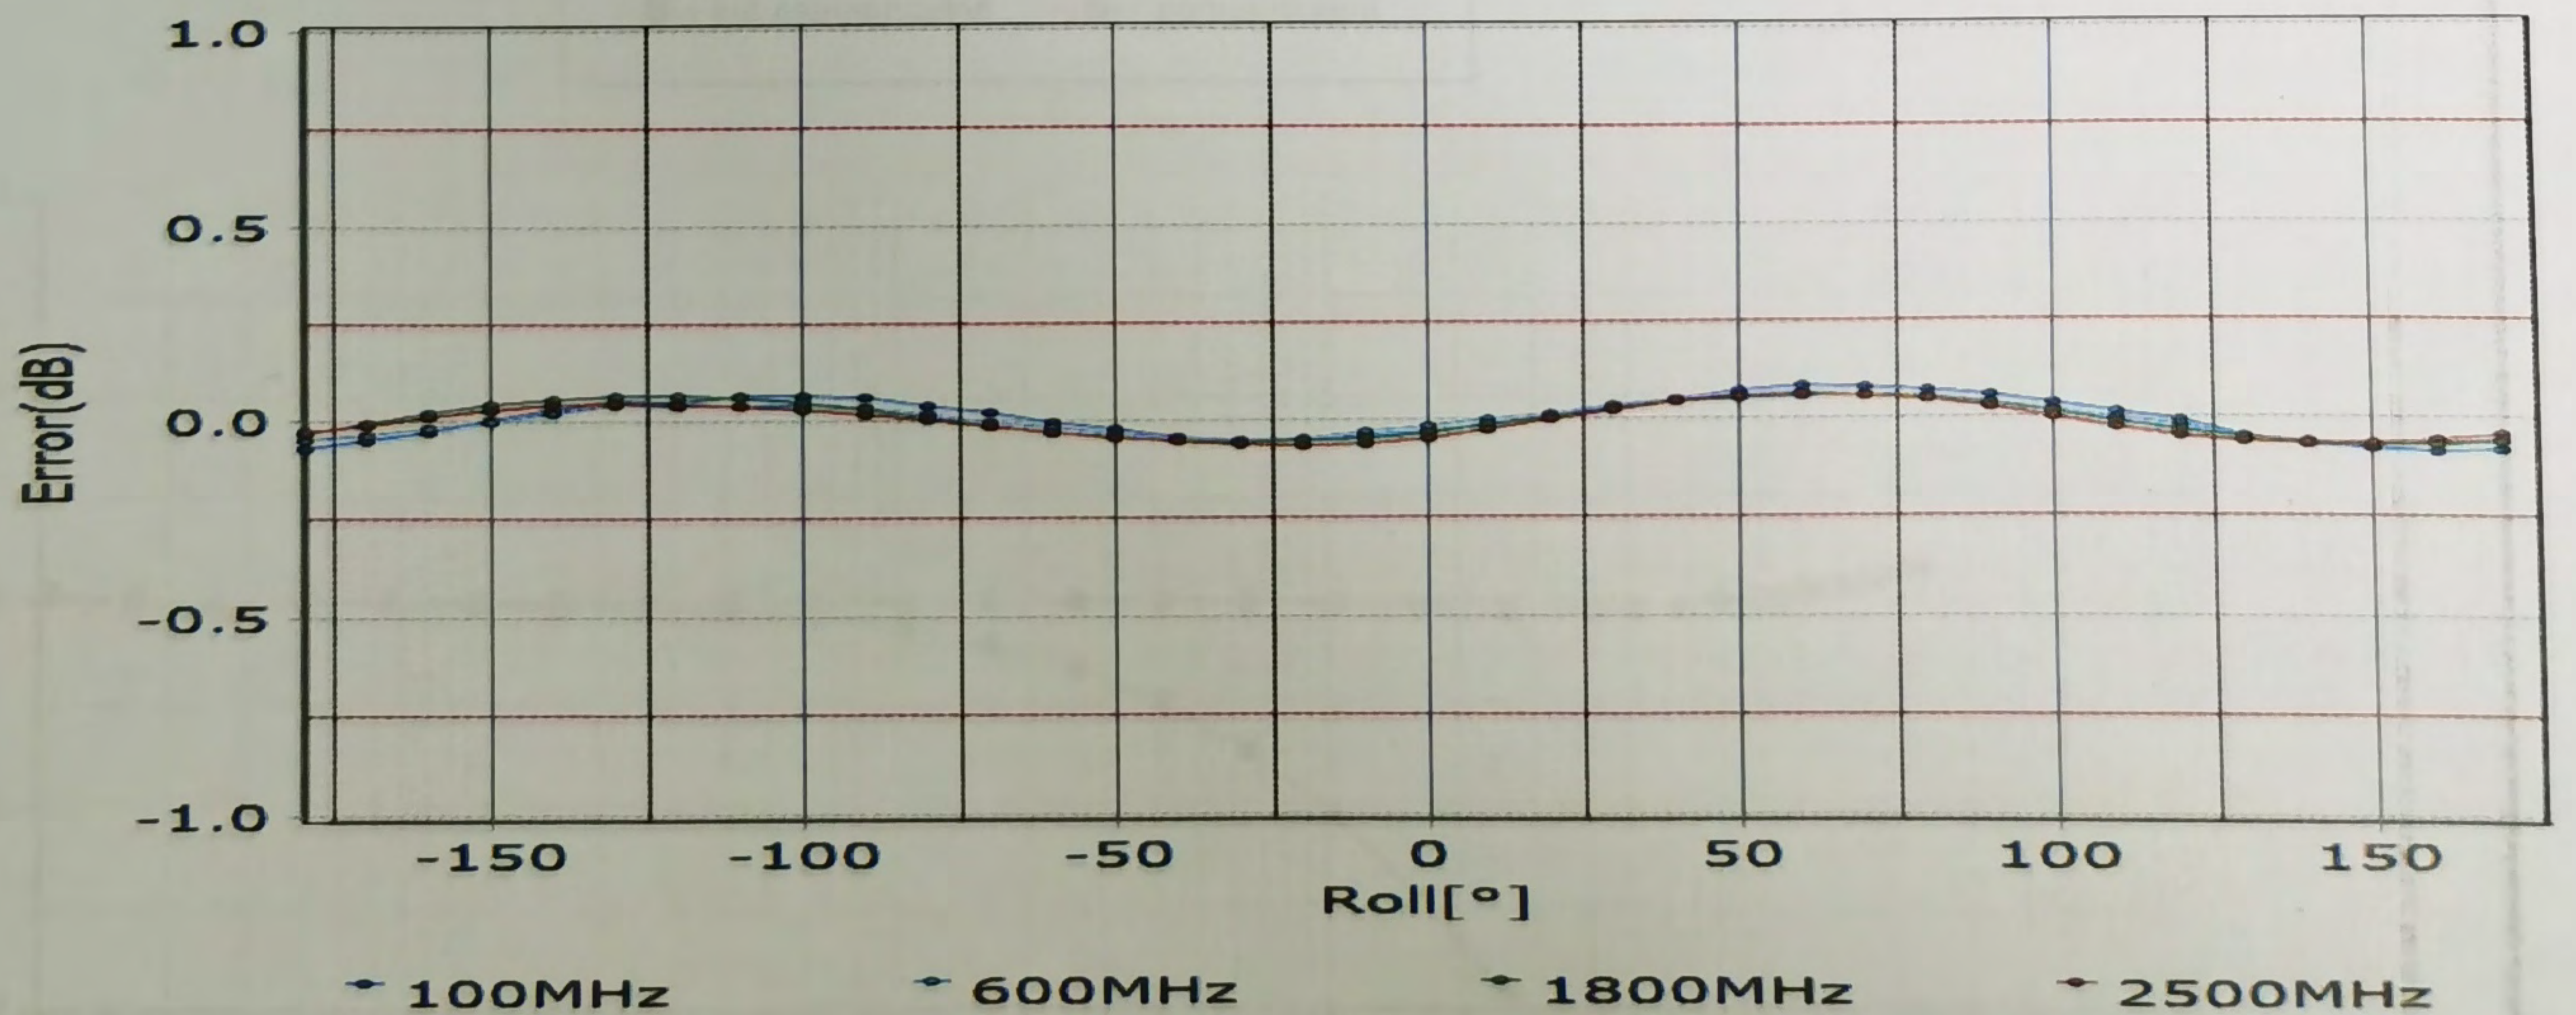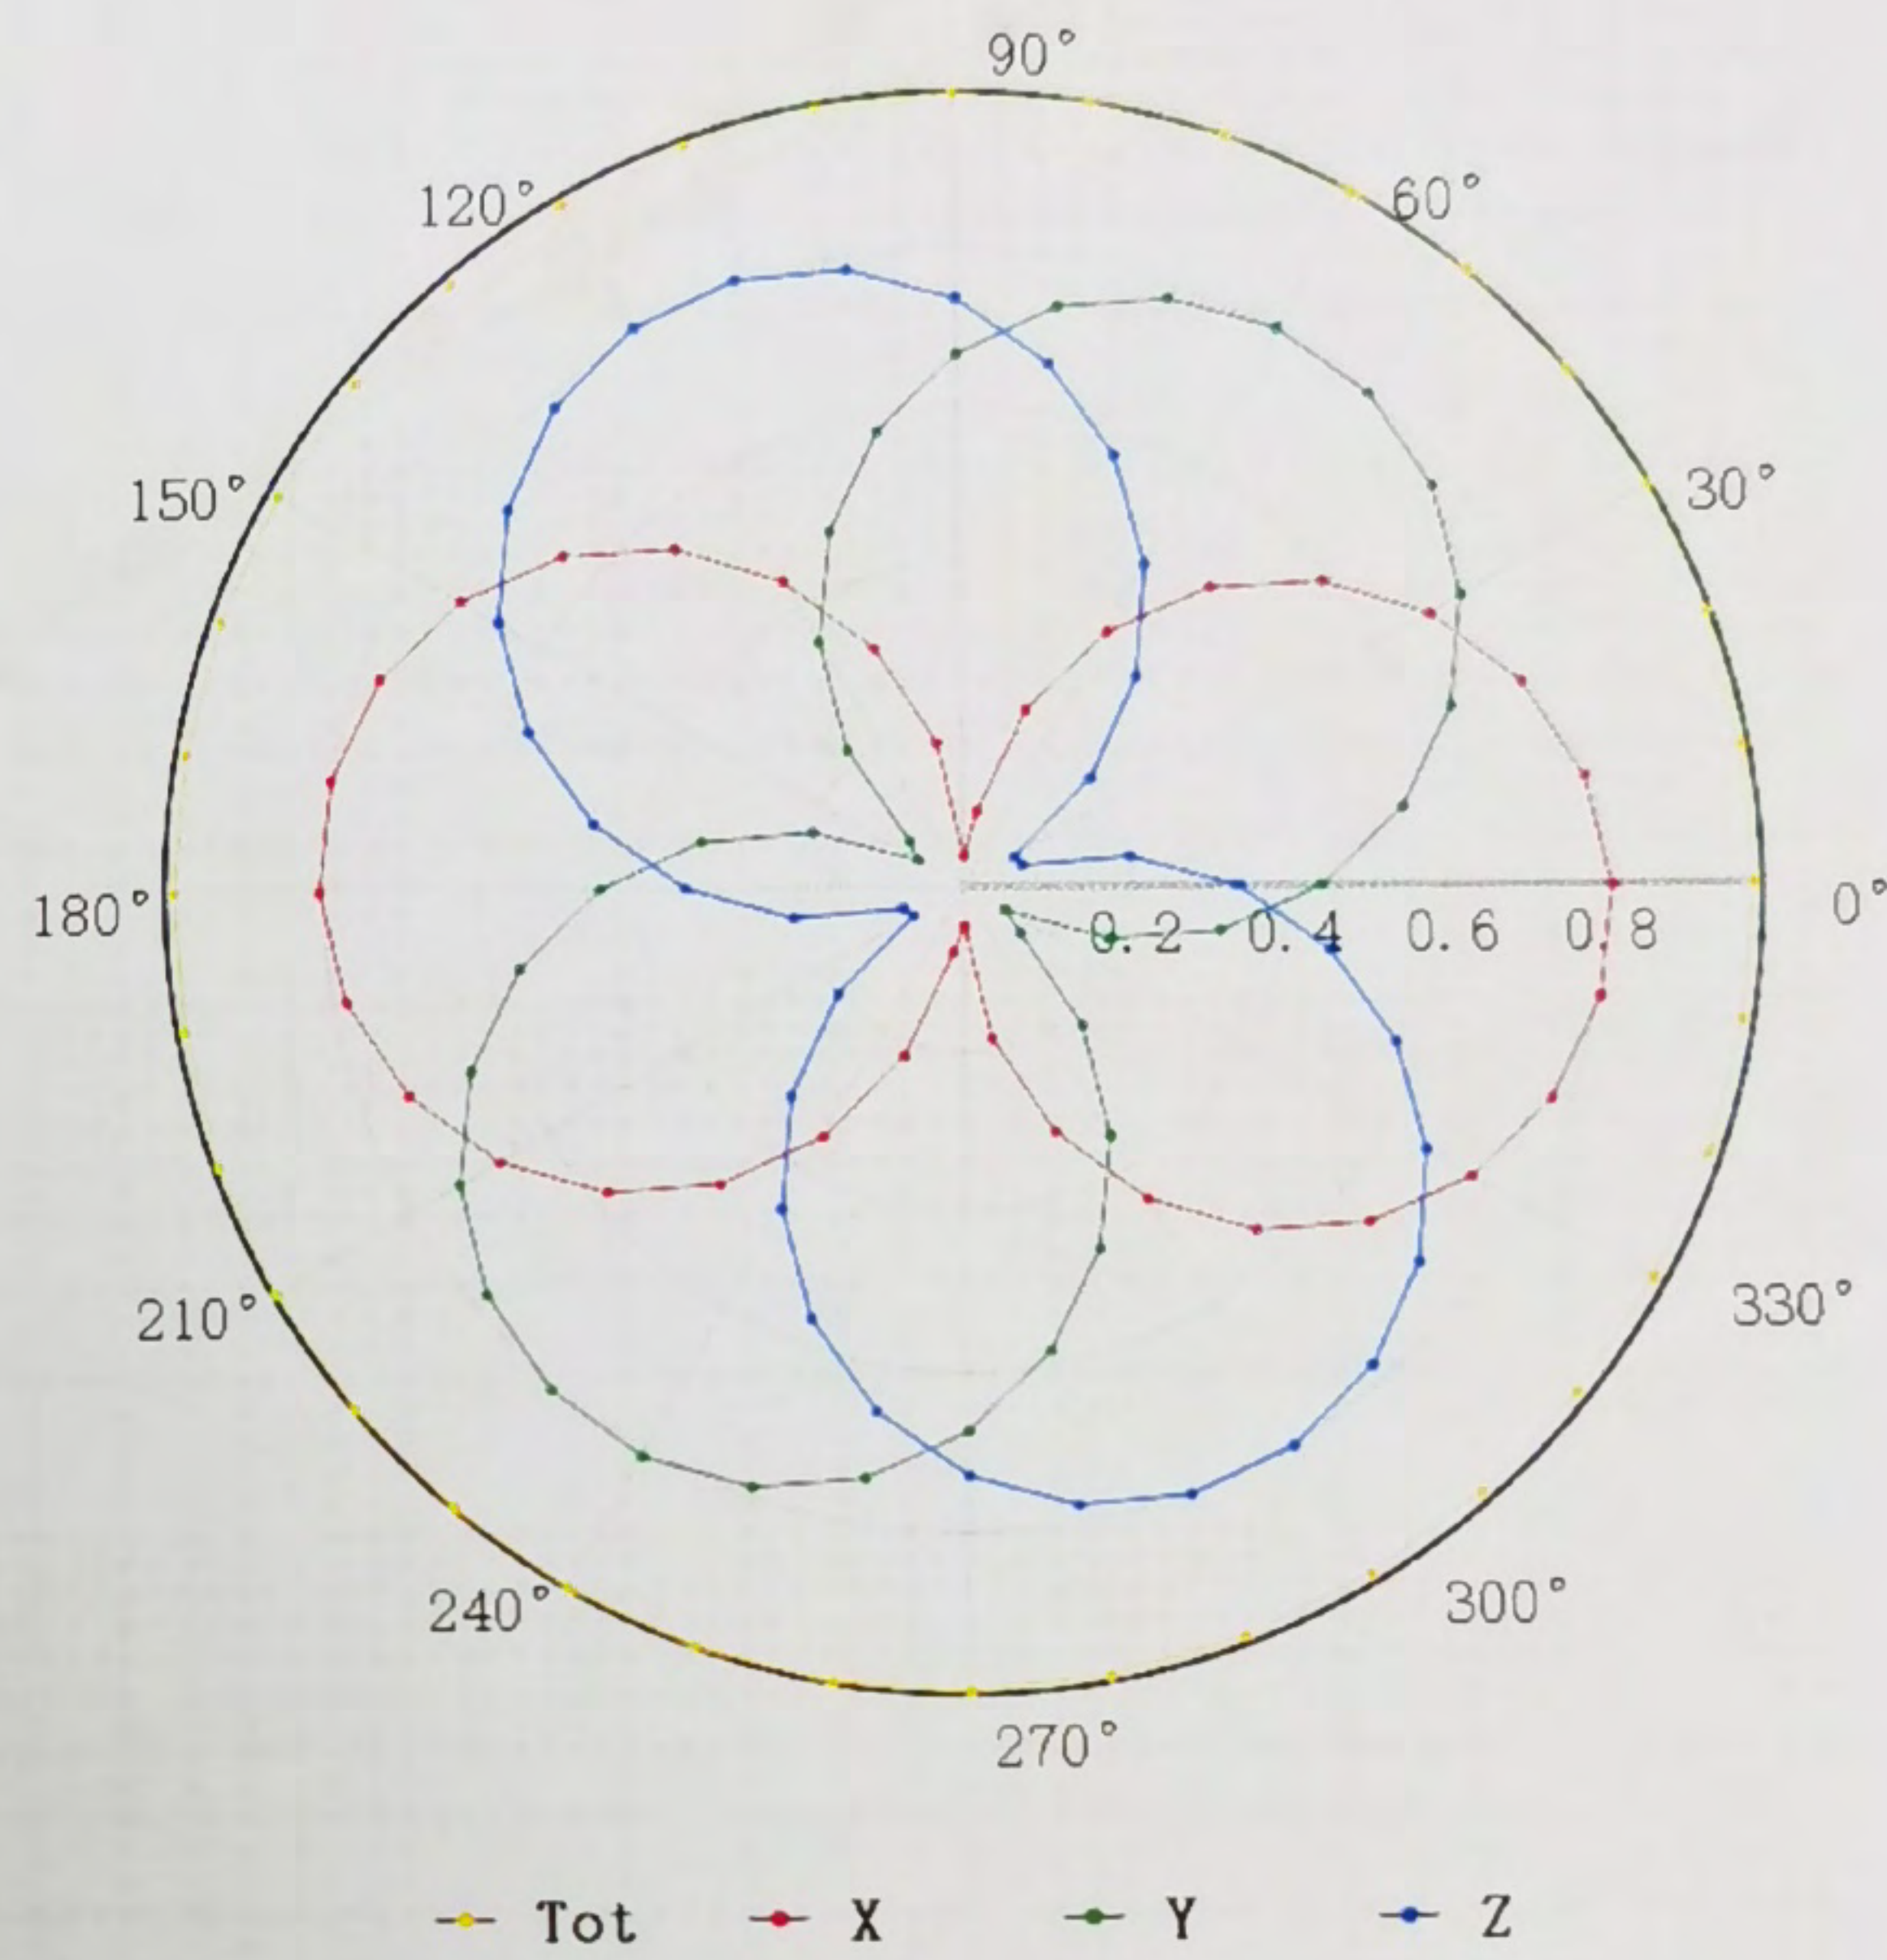
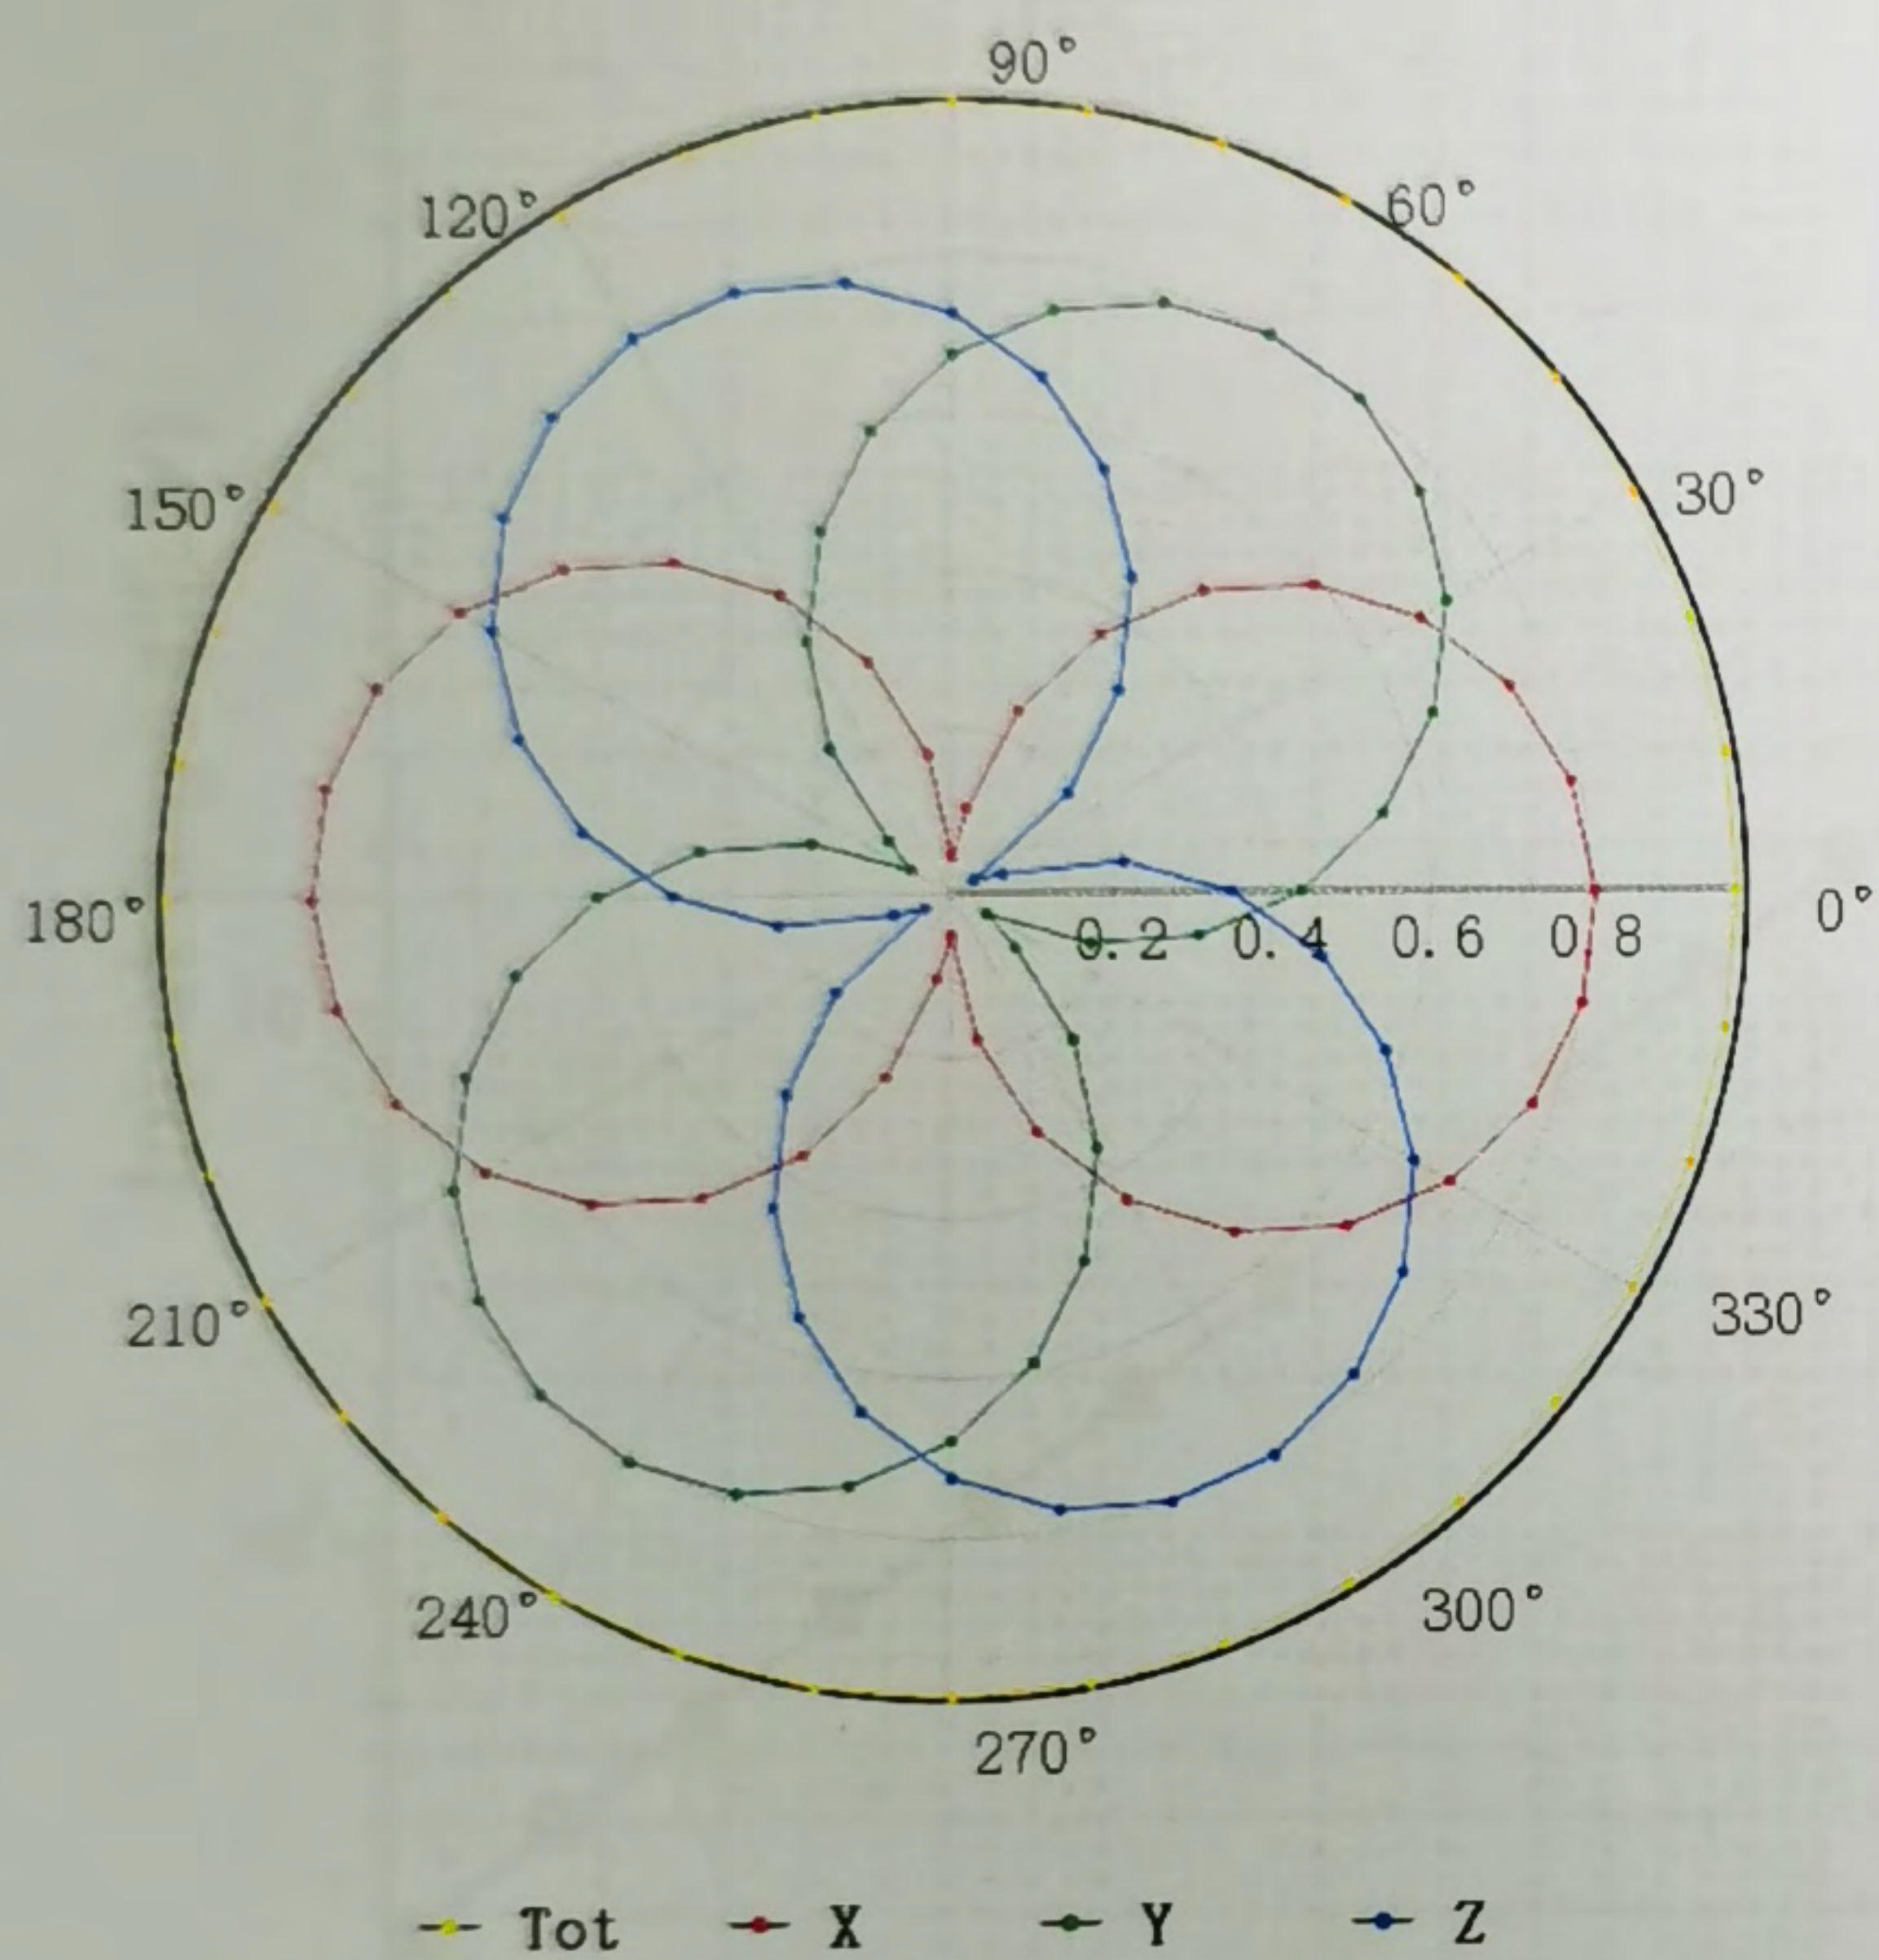


Uncertainty of Axial Isotropy Assessment:  $\pm 1.2\%$  ( $k=2$ )





## Dynamic Range f(SAR<sub>head</sub>) (TEM cell, f = 900 MHz)

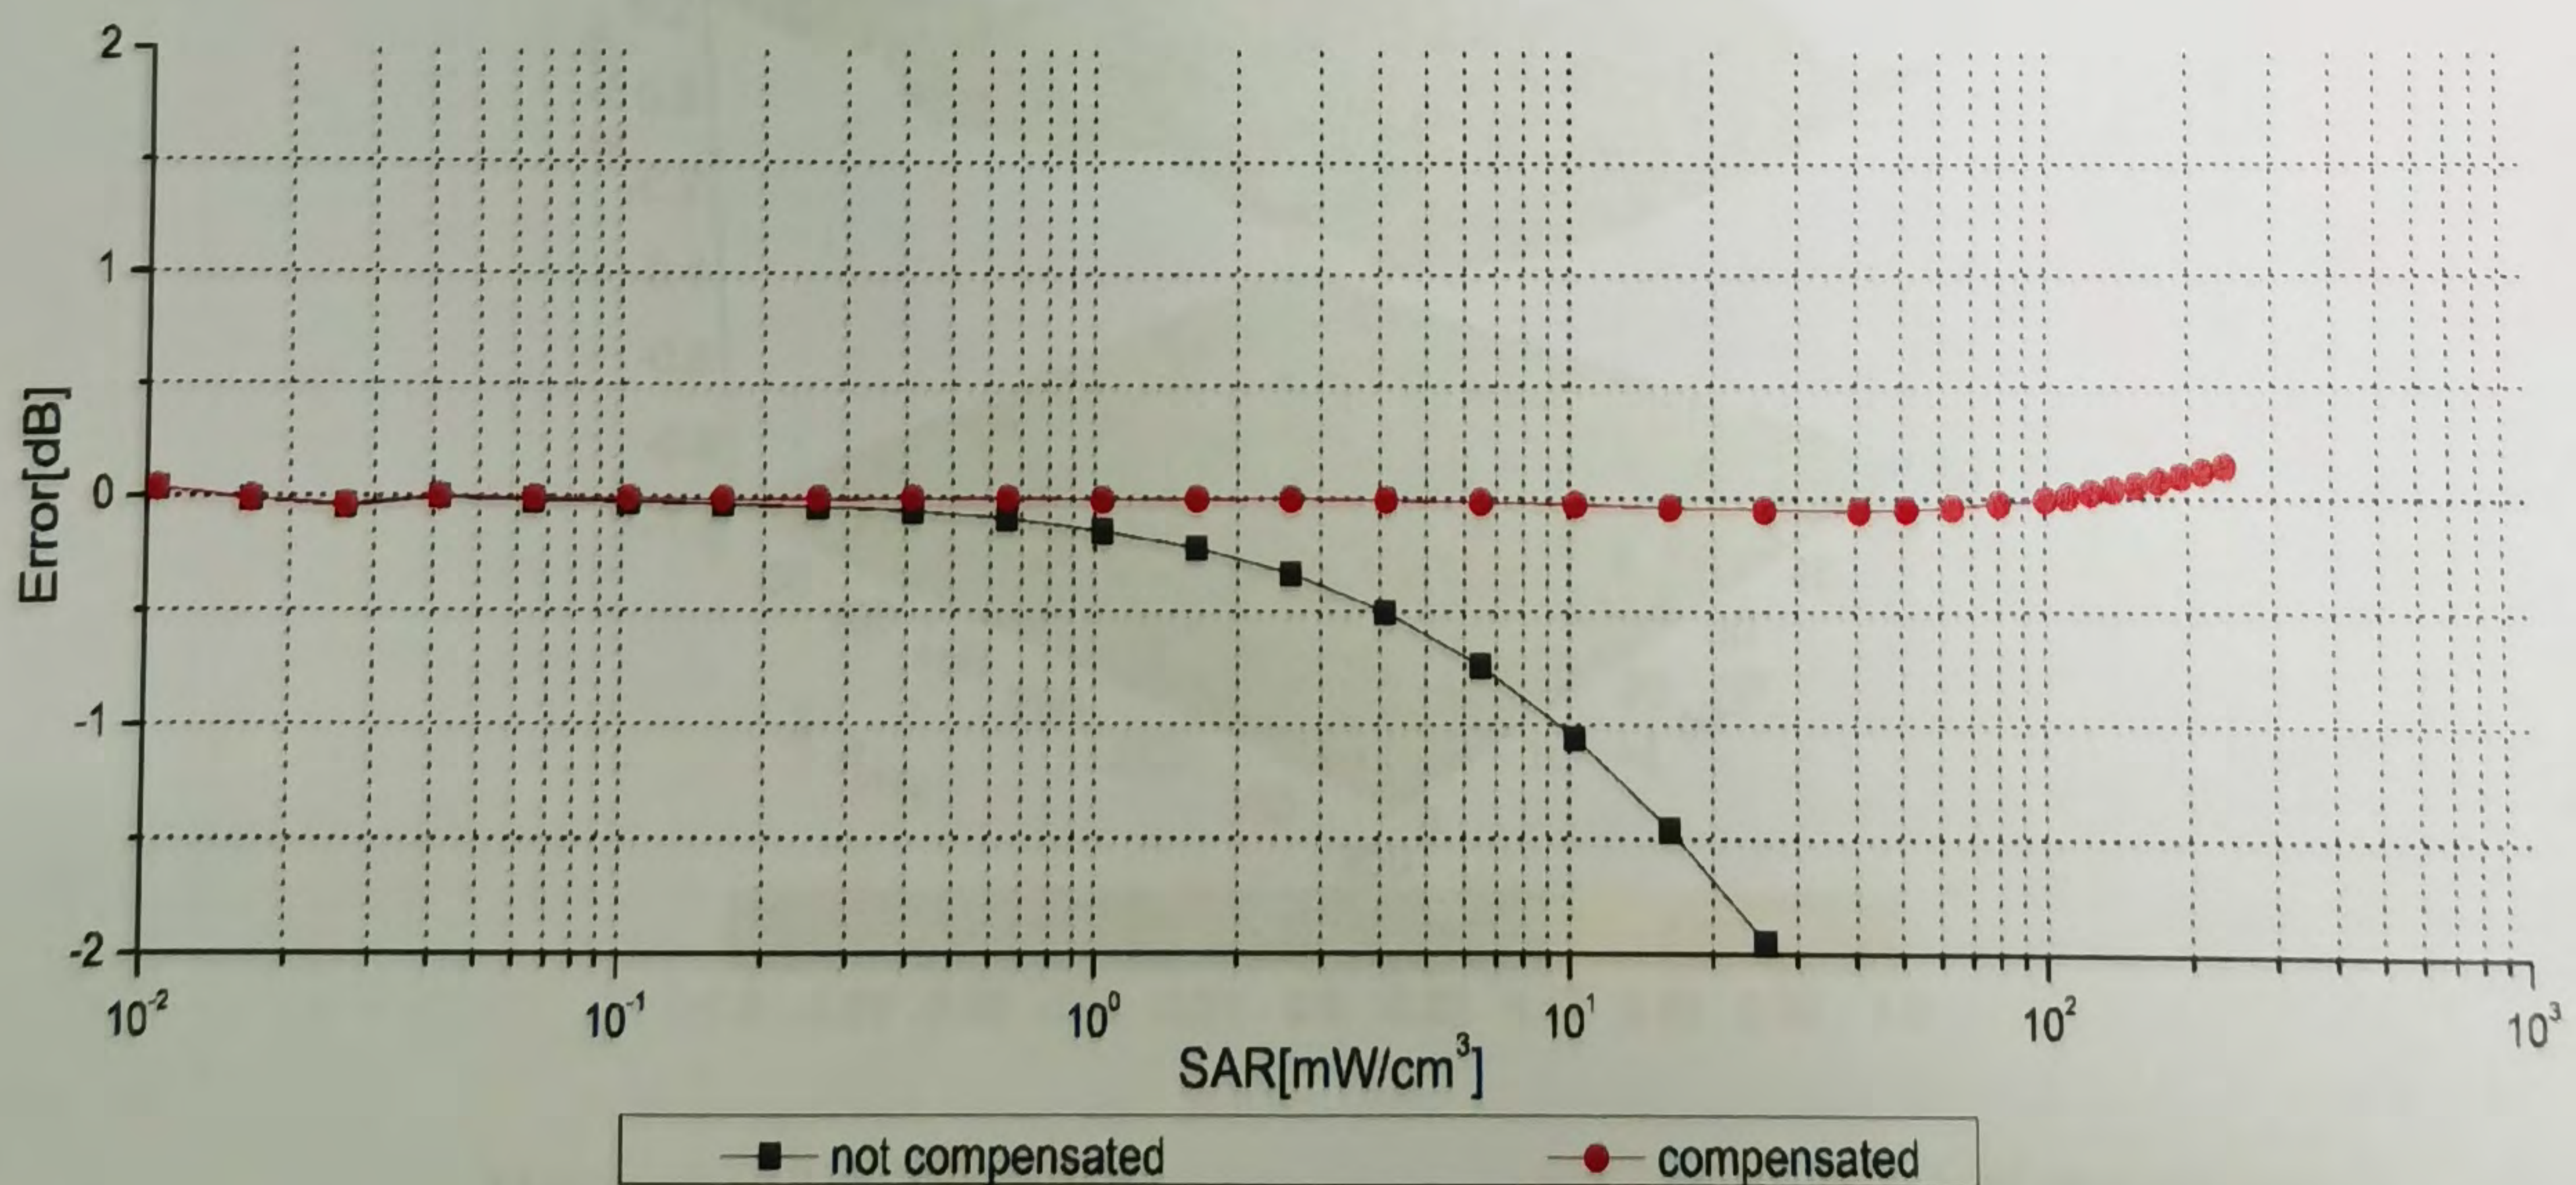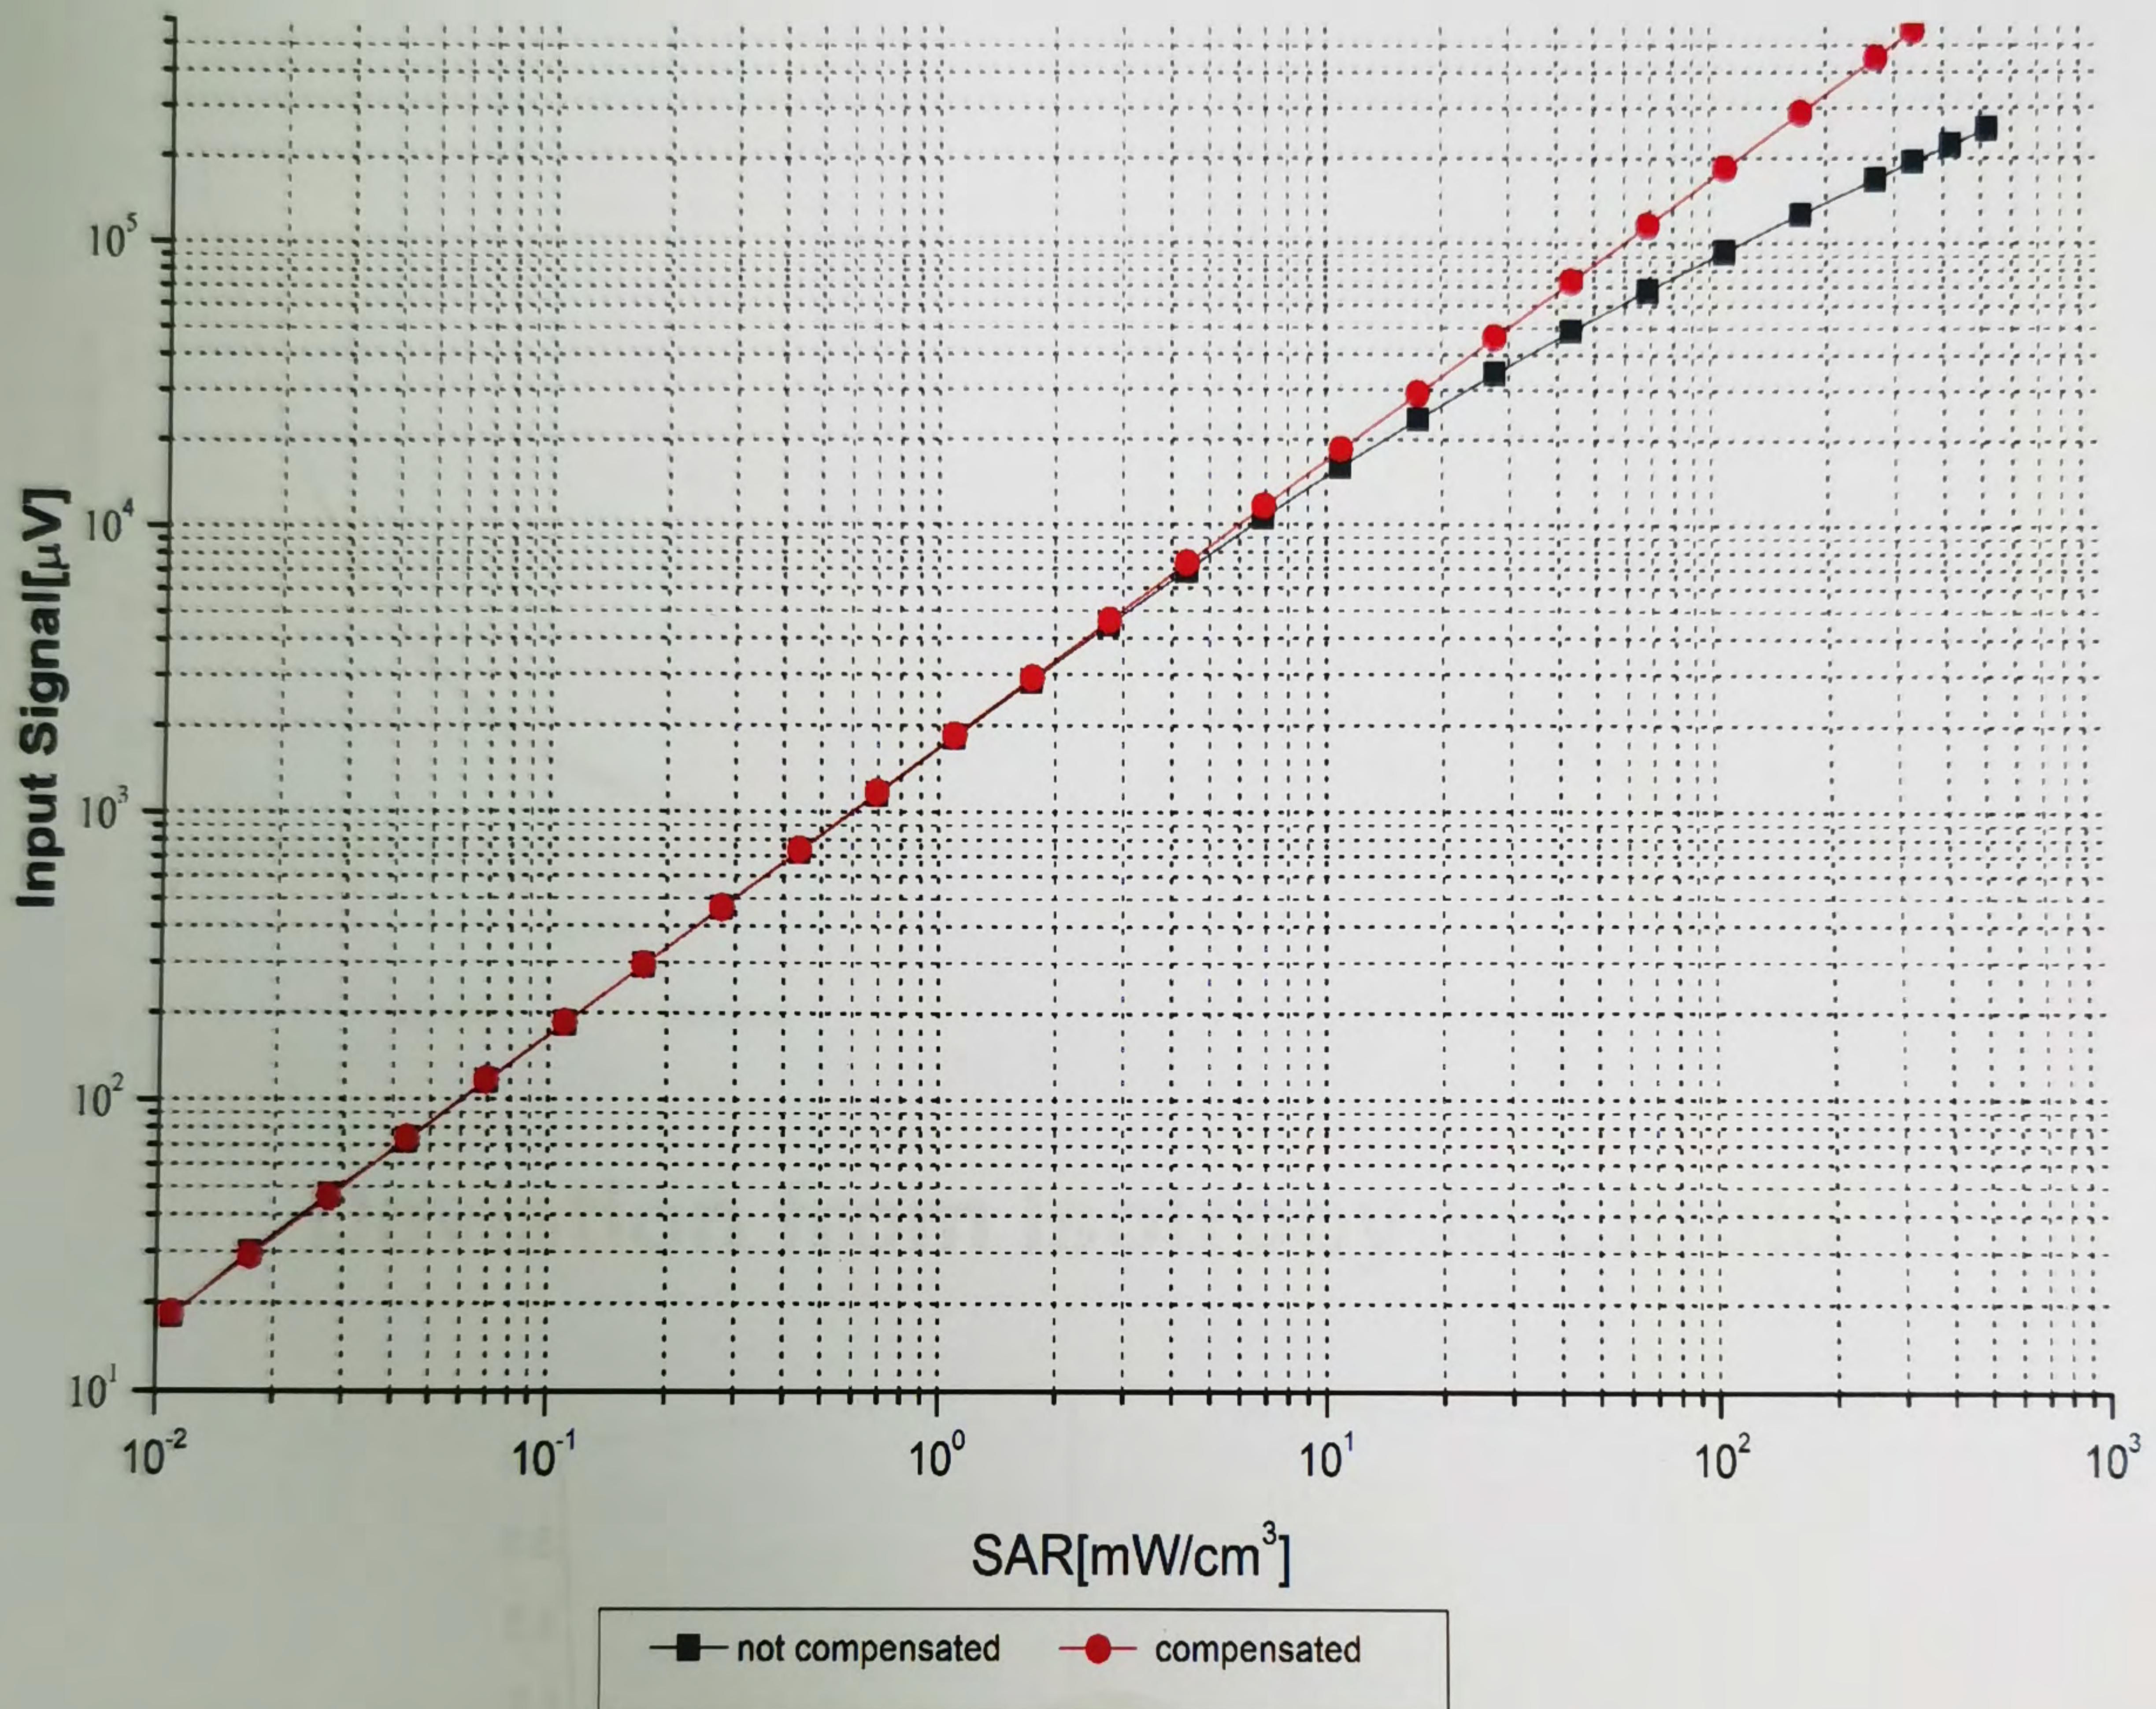

Uncertainty of Linearity Assessment: ±0.9% (k=2)







## Conversion Factor Assessment

f=750 MHz,WGLS R9(H\_convF)


f=1750 MHz,WGLS R22(H\_convF)

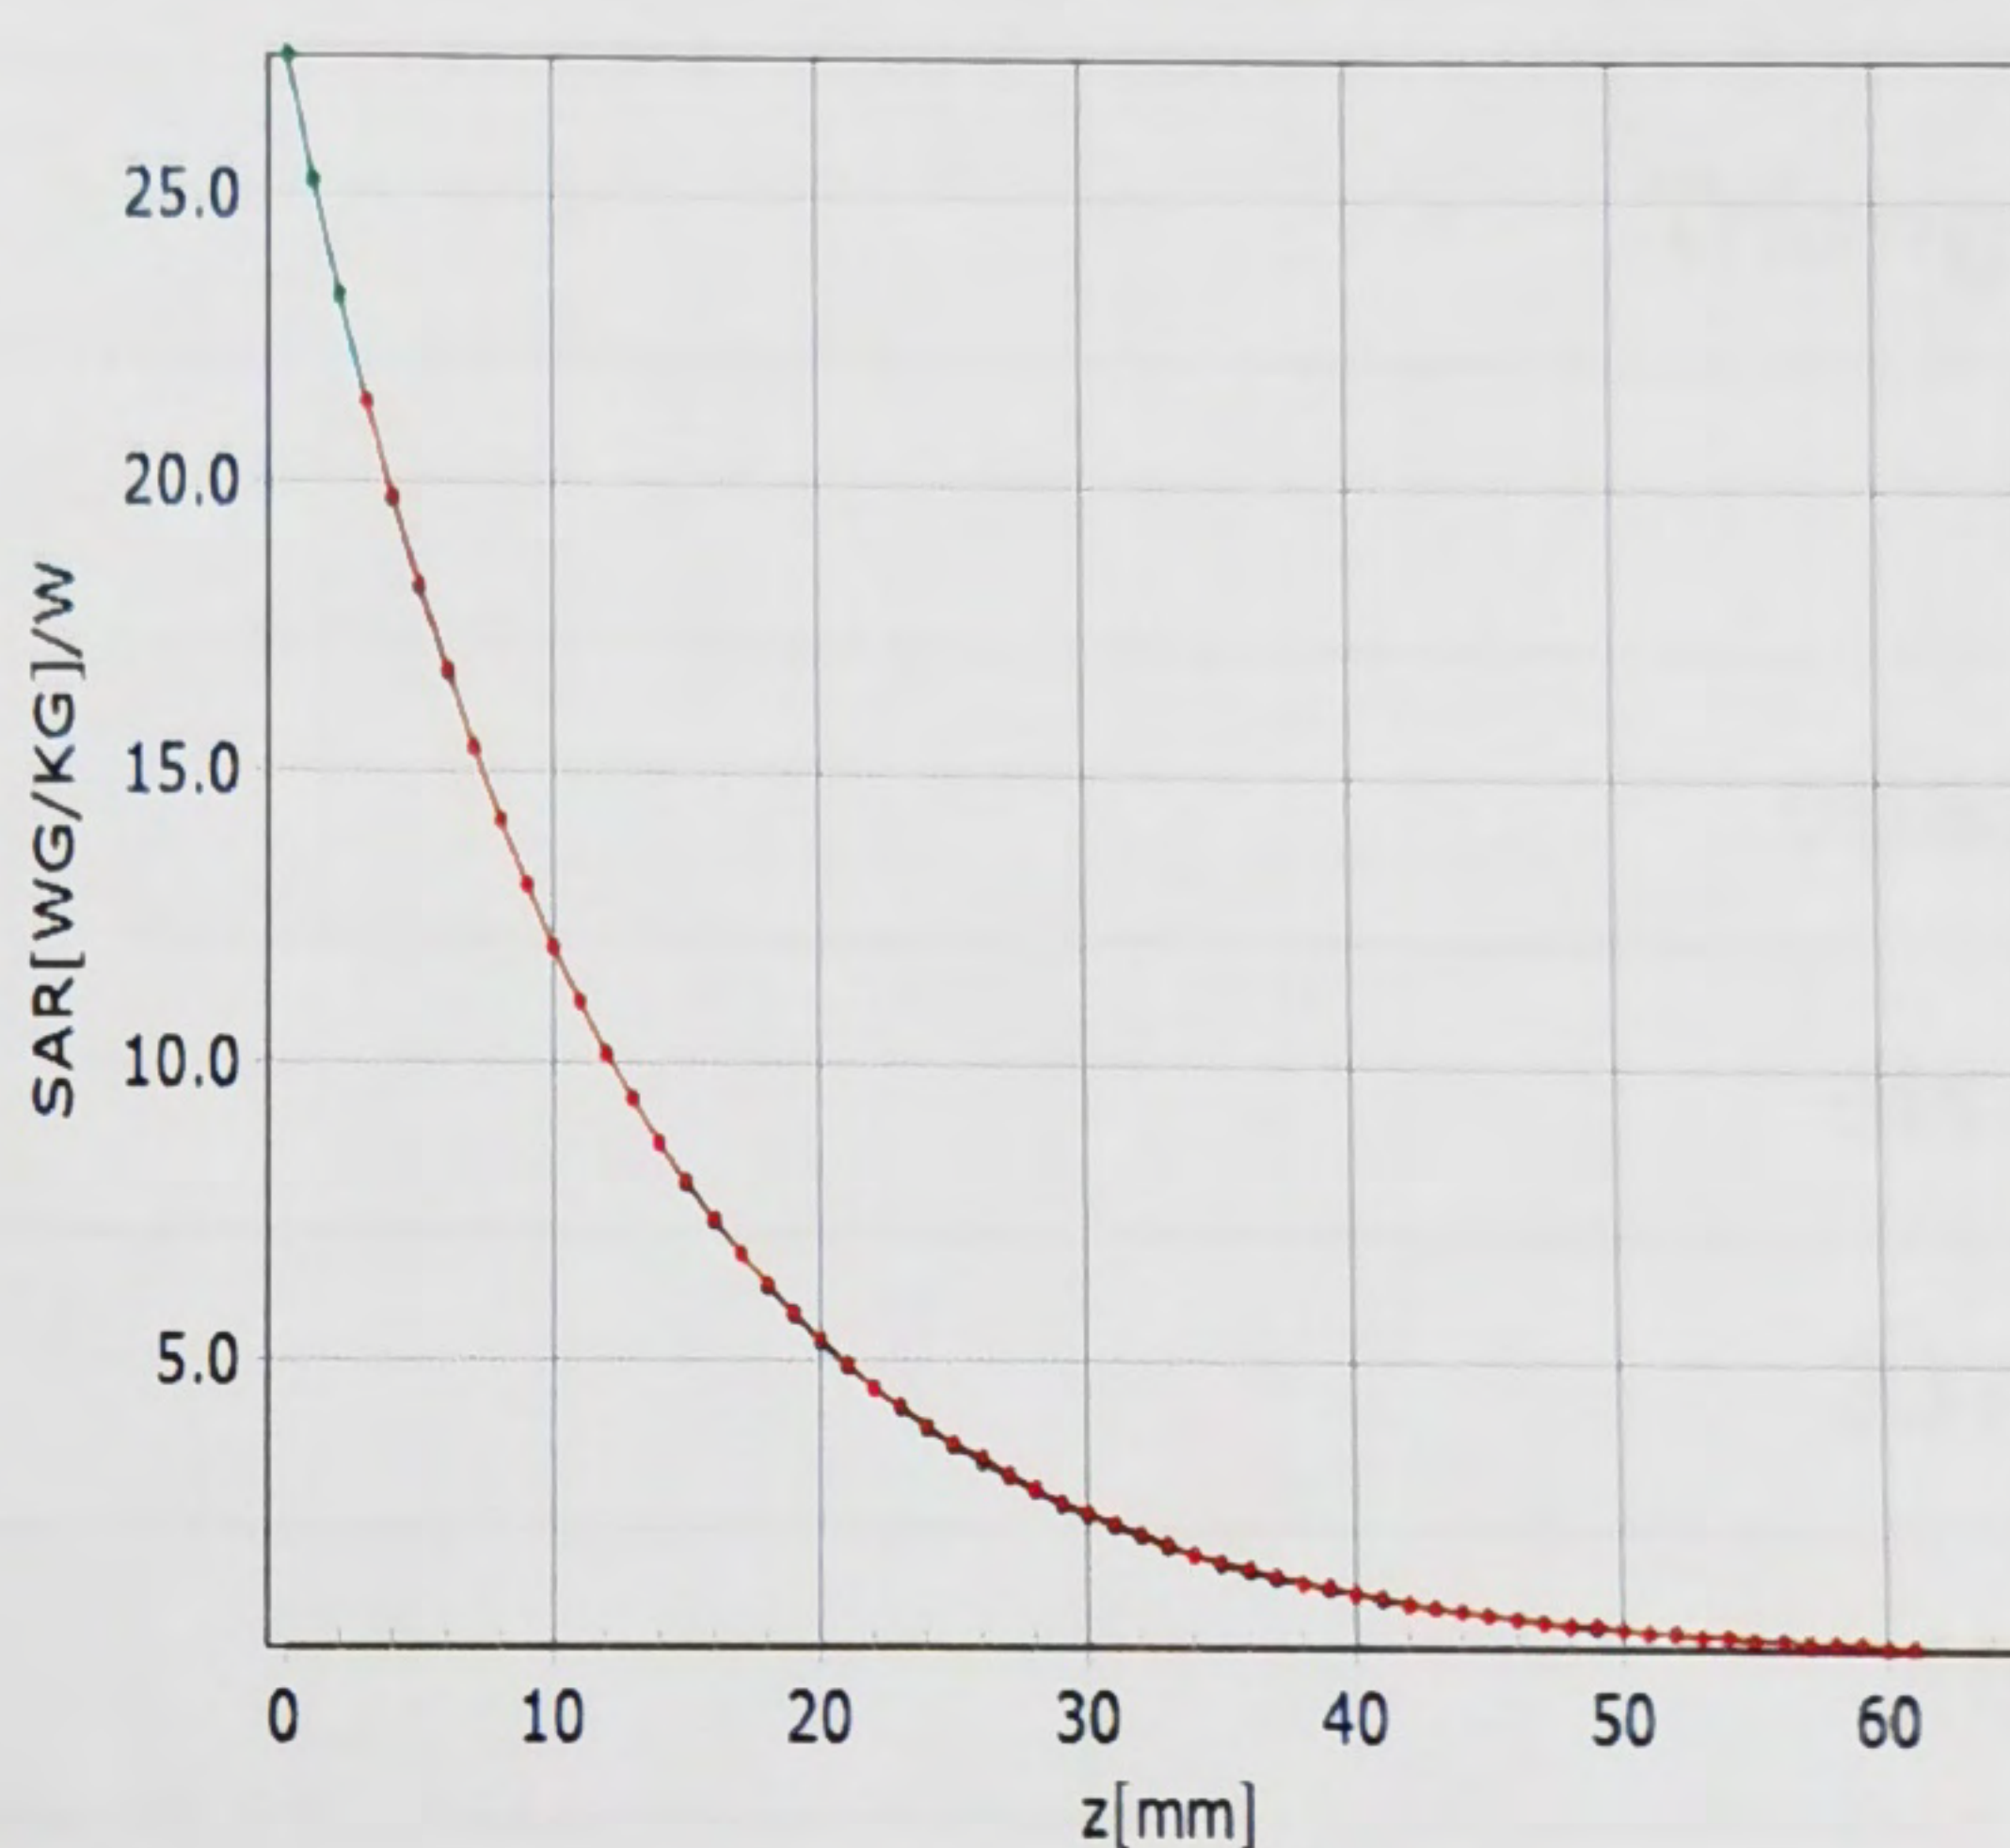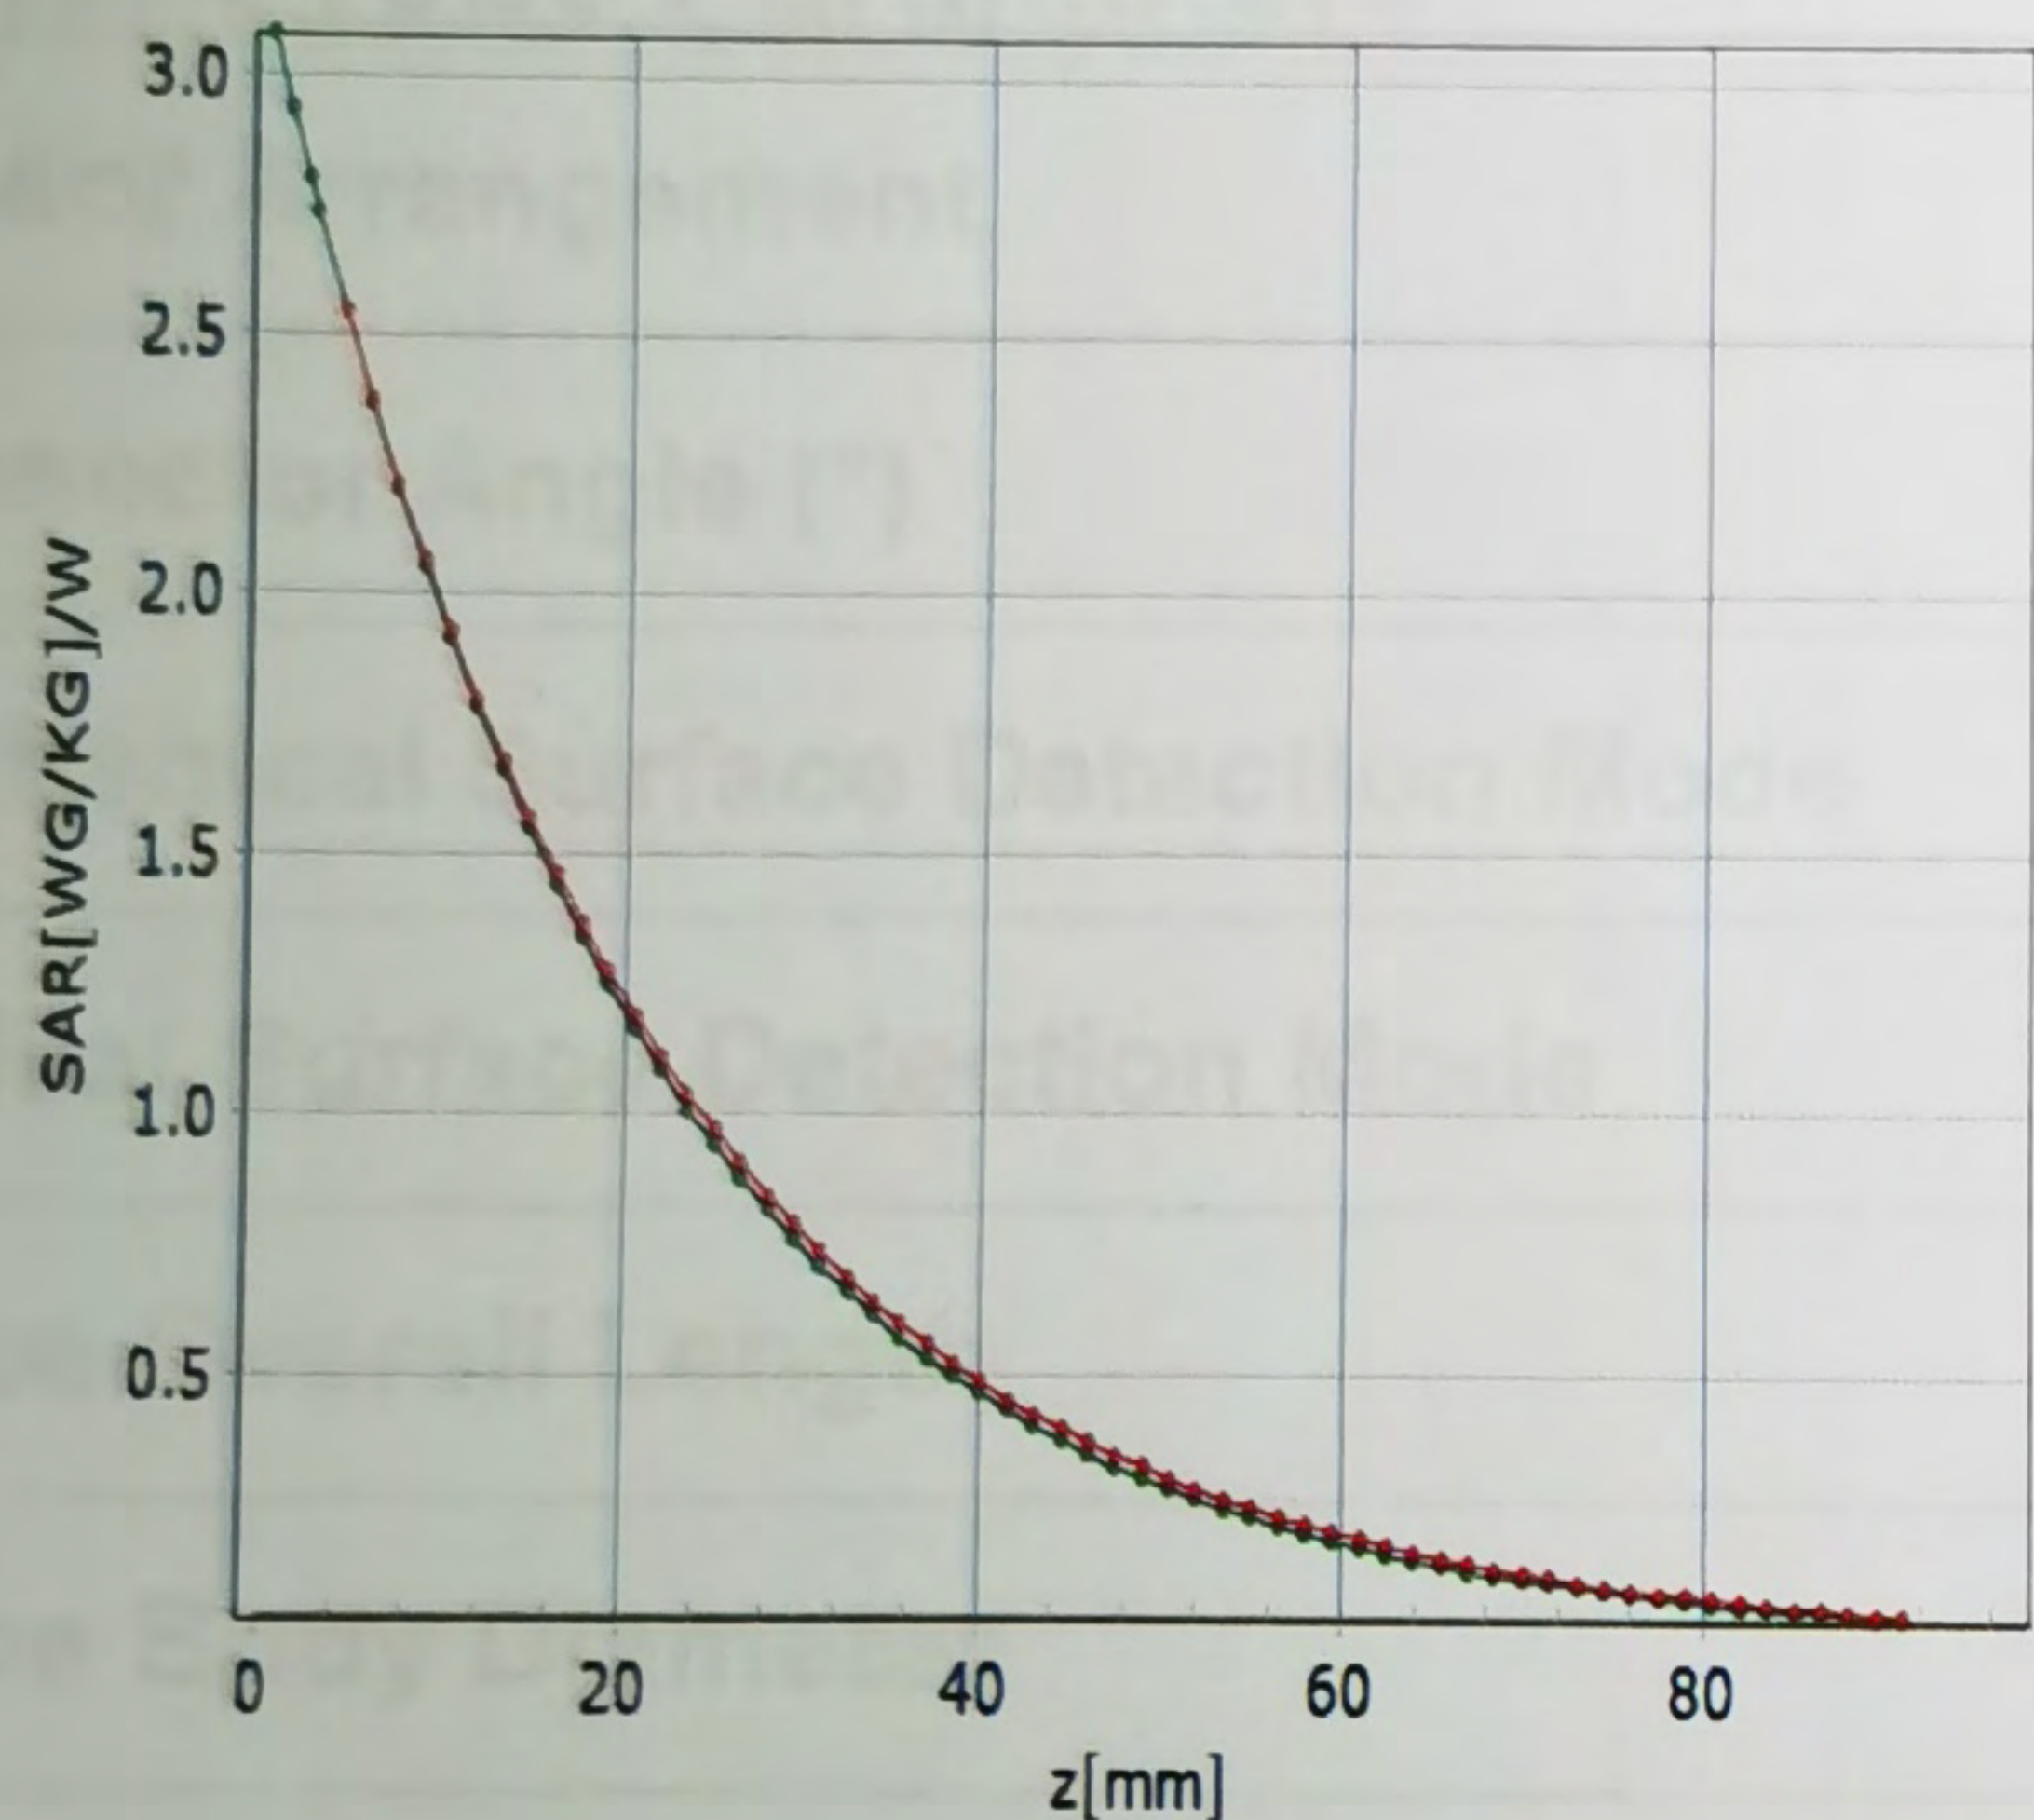

\* analytical \* measured

\* analytical \* measured

## Deviation from Isotropy in Liquid

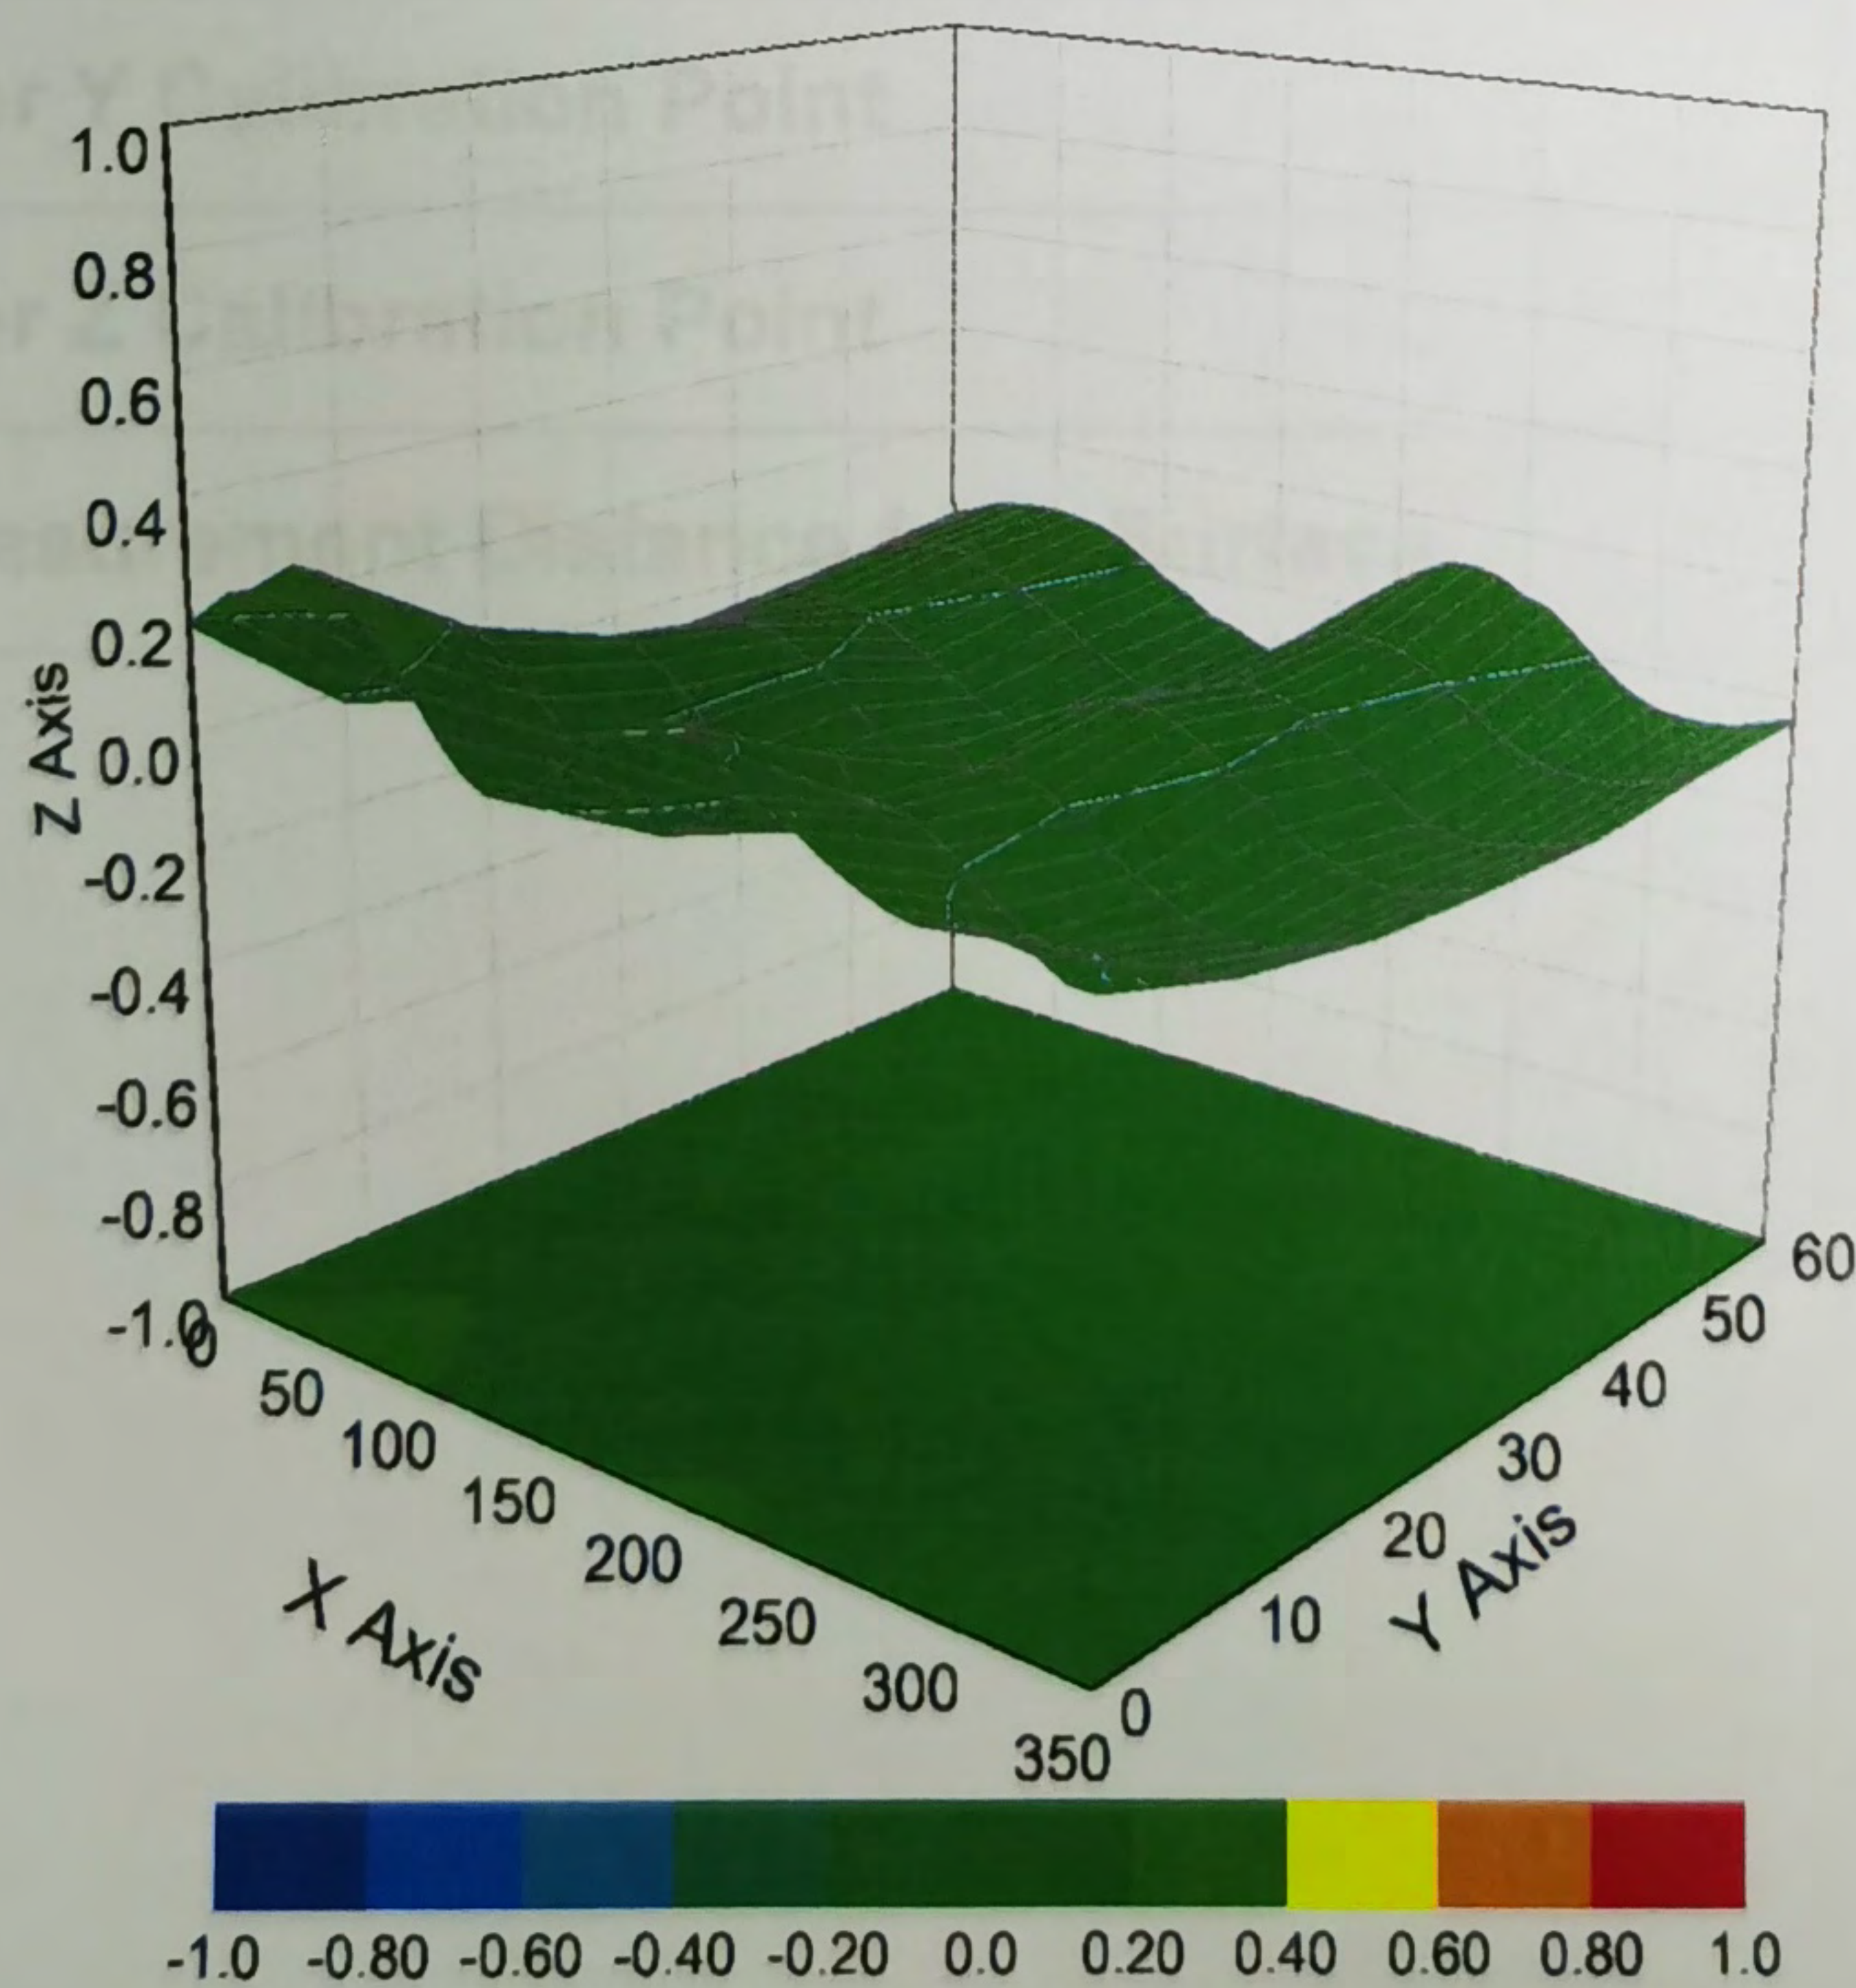

Uncertainty of Spherical Isotropy Assessment:  $\pm 3.2\%$  ( $k=2$ )





Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: [cttl@chinattl.com](mailto:cttl@chinattl.com) [Http://www.chinattl.cn](http://www.chinattl.cn)

## DASY/EASY – Parameters of Probe: EX3DV4 – SN:3923

### Other Probe Parameters

<b>Sensor Arrangement</b>	<b>Triangular</b>
<b>Connector Angle (°)</b>	<b>25.7</b>
<b>Mechanical Surface Detection Mode</b>	<b>enabled</b>
<b>Optical Surface Detection Mode</b>	<b>disable</b>
<b>Probe Overall Length</b>	<b>337mm</b>
<b>Probe Body Diameter</b>	<b>10mm</b>
<b>Tip Length</b>	<b>10mm</b>
<b>Tip Diameter</b>	<b>2.5mm</b>
<b>Probe Tip to Sensor X Calibration Point</b>	<b>1mm</b>
<b>Probe Tip to Sensor Y Calibration Point</b>	<b>1mm</b>
<b>Probe Tip to Sensor Z Calibration Point</b>	<b>1mm</b>
<b>Recommended Measurement Distance from Surface</b>	<b>1.4mm</b>



Dipole D750V3 SN 1160				
Head Liquid				
Date of Measurement	Return Loss(dB)	$\Delta$ %	Impedance ( $\Omega$ )	$\Delta\Omega$
2019-05-22	-29.1	/	51.8	/
2020-05-21	-29.4	1.03%	52.2	0.4 $\Omega$

Dipole D835V2 SN 4d105				
Head Liquid				
Date of Measurement	Return Loss(dB)	$\Delta$ %	Impedance ( $\Omega$ )	$\Delta\Omega$
2019-12-17	-26.0	/	49.5	/
2020-12-16	-27.0	3.85%	51.4	1.9 $\Omega$

Dipole D1750V2 SN 1149				
Head Liquid				
Date of Measurement	Return Loss(dB)	$\Delta$ %	Impedance ( $\Omega$ )	$\Delta\Omega$
2019-05-21	-31.8	/	47.6	/
2020-05-20	-32.3	1.57%	48.9	1.3 $\Omega$

Dipole D1900V2 SN 5d028				
Head Liquid				
Date of Measurement	Return Loss(dB)	$\Delta$ %	Impedance ( $\Omega$ )	$\Delta\Omega$
2019-12-17	-22.2	/	51.2	/
2020-12-16	-23.0	3.60%	53.3	2.1 $\Omega$

Dipole D2450V2 SN 733				
Head Liquid				
Date of Measurement	Return Loss(dB)	$\Delta$ %	Impedance ( $\Omega$ )	$\Delta\Omega$
2019-12-17	-27.2	/	52.2	/
2020-12-16	-27.8	2.21%	53.4	1.2 $\Omega$

Dipole D2600V2 SN 1125				
Head Liquid				
Date of Measurement	Return Loss(dB)	$\Delta$ %	Impedance ( $\Omega$ )	$\Delta\Omega$
2019-05-20	-25.7	/	48.9	/
2020-05-19	-26.6	3.50%	50.8	1.9 $\Omega$

Dipole D5GHzV2 SN 1165				
5250MHz Head Liquid				
Date of Measurement	Return Loss(dB)	$\Delta$ %	Impedance ( $\Omega$ )	$\Delta\Omega$
2019-12-20	-25.5	/	45.2	/
2020-12-19	-26.3	3.14%	47.1	1.9 $\Omega$
5600MHz Head Liquid				
Date of Measurement	Return Loss(dB)	$\Delta$ %	Impedance ( $\Omega$ )	$\Delta\Omega$
2019-12-20	26.8	/	52.0	/
2020-12-19	-27.6	2.99%	53.7	1.7 $\Omega$
5750MHz Head Liquid				
Date of Measurement	Return Loss(dB)	$\Delta$ %	Impedance ( $\Omega$ )	$\Delta\Omega$
2019-12-20	-27.5	/	50.0	/
2020-12-19	-28.4	3.27%	52.6	2.6 $\Omega$