



DASY/EASY – Parameters of Probe: EX3DV4 – SN:3982

Basic Calibration Parameters

| | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|----------------------------------------------------------|----------|----------|----------|--------------|
| Norm($\mu\text{V}/(\text{V}/\text{m})^2$) ^A | 0.55 | 0.56 | 0.50 | $\pm 10.0\%$ |
| DCP(mV) ^B | 102.2 | 104.8 | 102.5 | |

Modulation Calibration Parameters

| UID | Communication System Name | | A dB | B dB $\sqrt{\mu\text{V}}$ | C | D dB | VR mV | Unc ^E (k=2) |
|-----|---------------------------|---|---------|------------------------------|-----|---------|----------|---------------------------|
| 0 | CW | X | 0.0 | 0.0 | 1.0 | 0.00 | 176.8 | $\pm 2.3\%$ |
| | | Y | 0.0 | 0.0 | 1.0 | | 181.5 | |
| | | Z | 0.0 | 0.0 | 1.0 | | 167.8 | |

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor $k=2$, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X, Y, Z do not affect the E²-field uncertainty inside TSL (see Page 4).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Probe shall not be used for SAR compliance testing if measured SAR value of the DUT is below 0.025 mW/g.



DASY/EASY – Parameters of Probe: EX3DV4 – SN:3982

Frequency Response of E-Field

Calibration Parameter Determined in Head Tissue Simulating Media

| f [MHz] ^C | Relative Permittivity ^F | Conductivity (S/m) ^F | ConvF X | ConvF Y | ConvF Z | Alpha ^G | Depth ^G (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|--------------------|-------------------------|-------------|
| 750 | 41.9 | 0.89 | 10.73 | 10.73 | 10.73 | 0.40 | 0.75 | ± 12.1% |
| 835 | 41.5 | 0.90 | 10.32 | 10.32 | 10.32 | 0.28 | 1.03 | ± 12.1% |
| 1750 | 40.1 | 1.37 | 8.78 | 8.78 | 8.78 | 0.22 | 1.05 | ± 12.1% |
| 1900 | 40.0 | 1.40 | 8.40 | 8.40 | 8.40 | 0.26 | 0.98 | ± 12.1% |
| 3300 | 38.2 | 2.71 | 7.41 | 7.41 | 7.41 | 0.40 | 1.01 | ± 13.3% |
| 3500 | 37.9 | 2.91 | 7.10 | 7.10 | 7.10 | 0.45 | 0.93 | ± 13.3% |
| 3700 | 37.7 | 3.12 | 6.78 | 6.78 | 6.78 | 0.41 | 1.05 | ± 13.3% |
| 4100 | 37.2 | 3.53 | 6.71 | 6.71 | 6.71 | 0.40 | 1.20 | ± 13.3% |
| 4400 | 36.9 | 3.84 | 6.48 | 6.48 | 6.48 | 0.35 | 1.35 | ± 13.3% |
| 4600 | 36.7 | 4.04 | 6.34 | 6.34 | 6.34 | 0.45 | 1.25 | ± 13.3% |
| 4800 | 36.4 | 4.25 | 6.30 | 6.30 | 6.30 | 0.45 | 1.30 | ± 13.3% |
| 4950 | 36.3 | 4.40 | 5.99 | 5.99 | 5.99 | 0.45 | 1.30 | ± 13.3% |
| 5250 | 35.9 | 4.71 | 5.70 | 5.70 | 5.70 | 0.45 | 1.30 | ± 13.3% |
| 5600 | 35.5 | 5.07 | 5.12 | 5.12 | 5.12 | 0.50 | 1.20 | ± 13.3% |
| 5750 | 35.4 | 5.22 | 5.14 | 5.14 | 5.14 | 0.50 | 1.20 | ± 13.3% |

^C Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequency below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.


^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.



In Collaboration with
s p e a g
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504
E-mail: cttl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

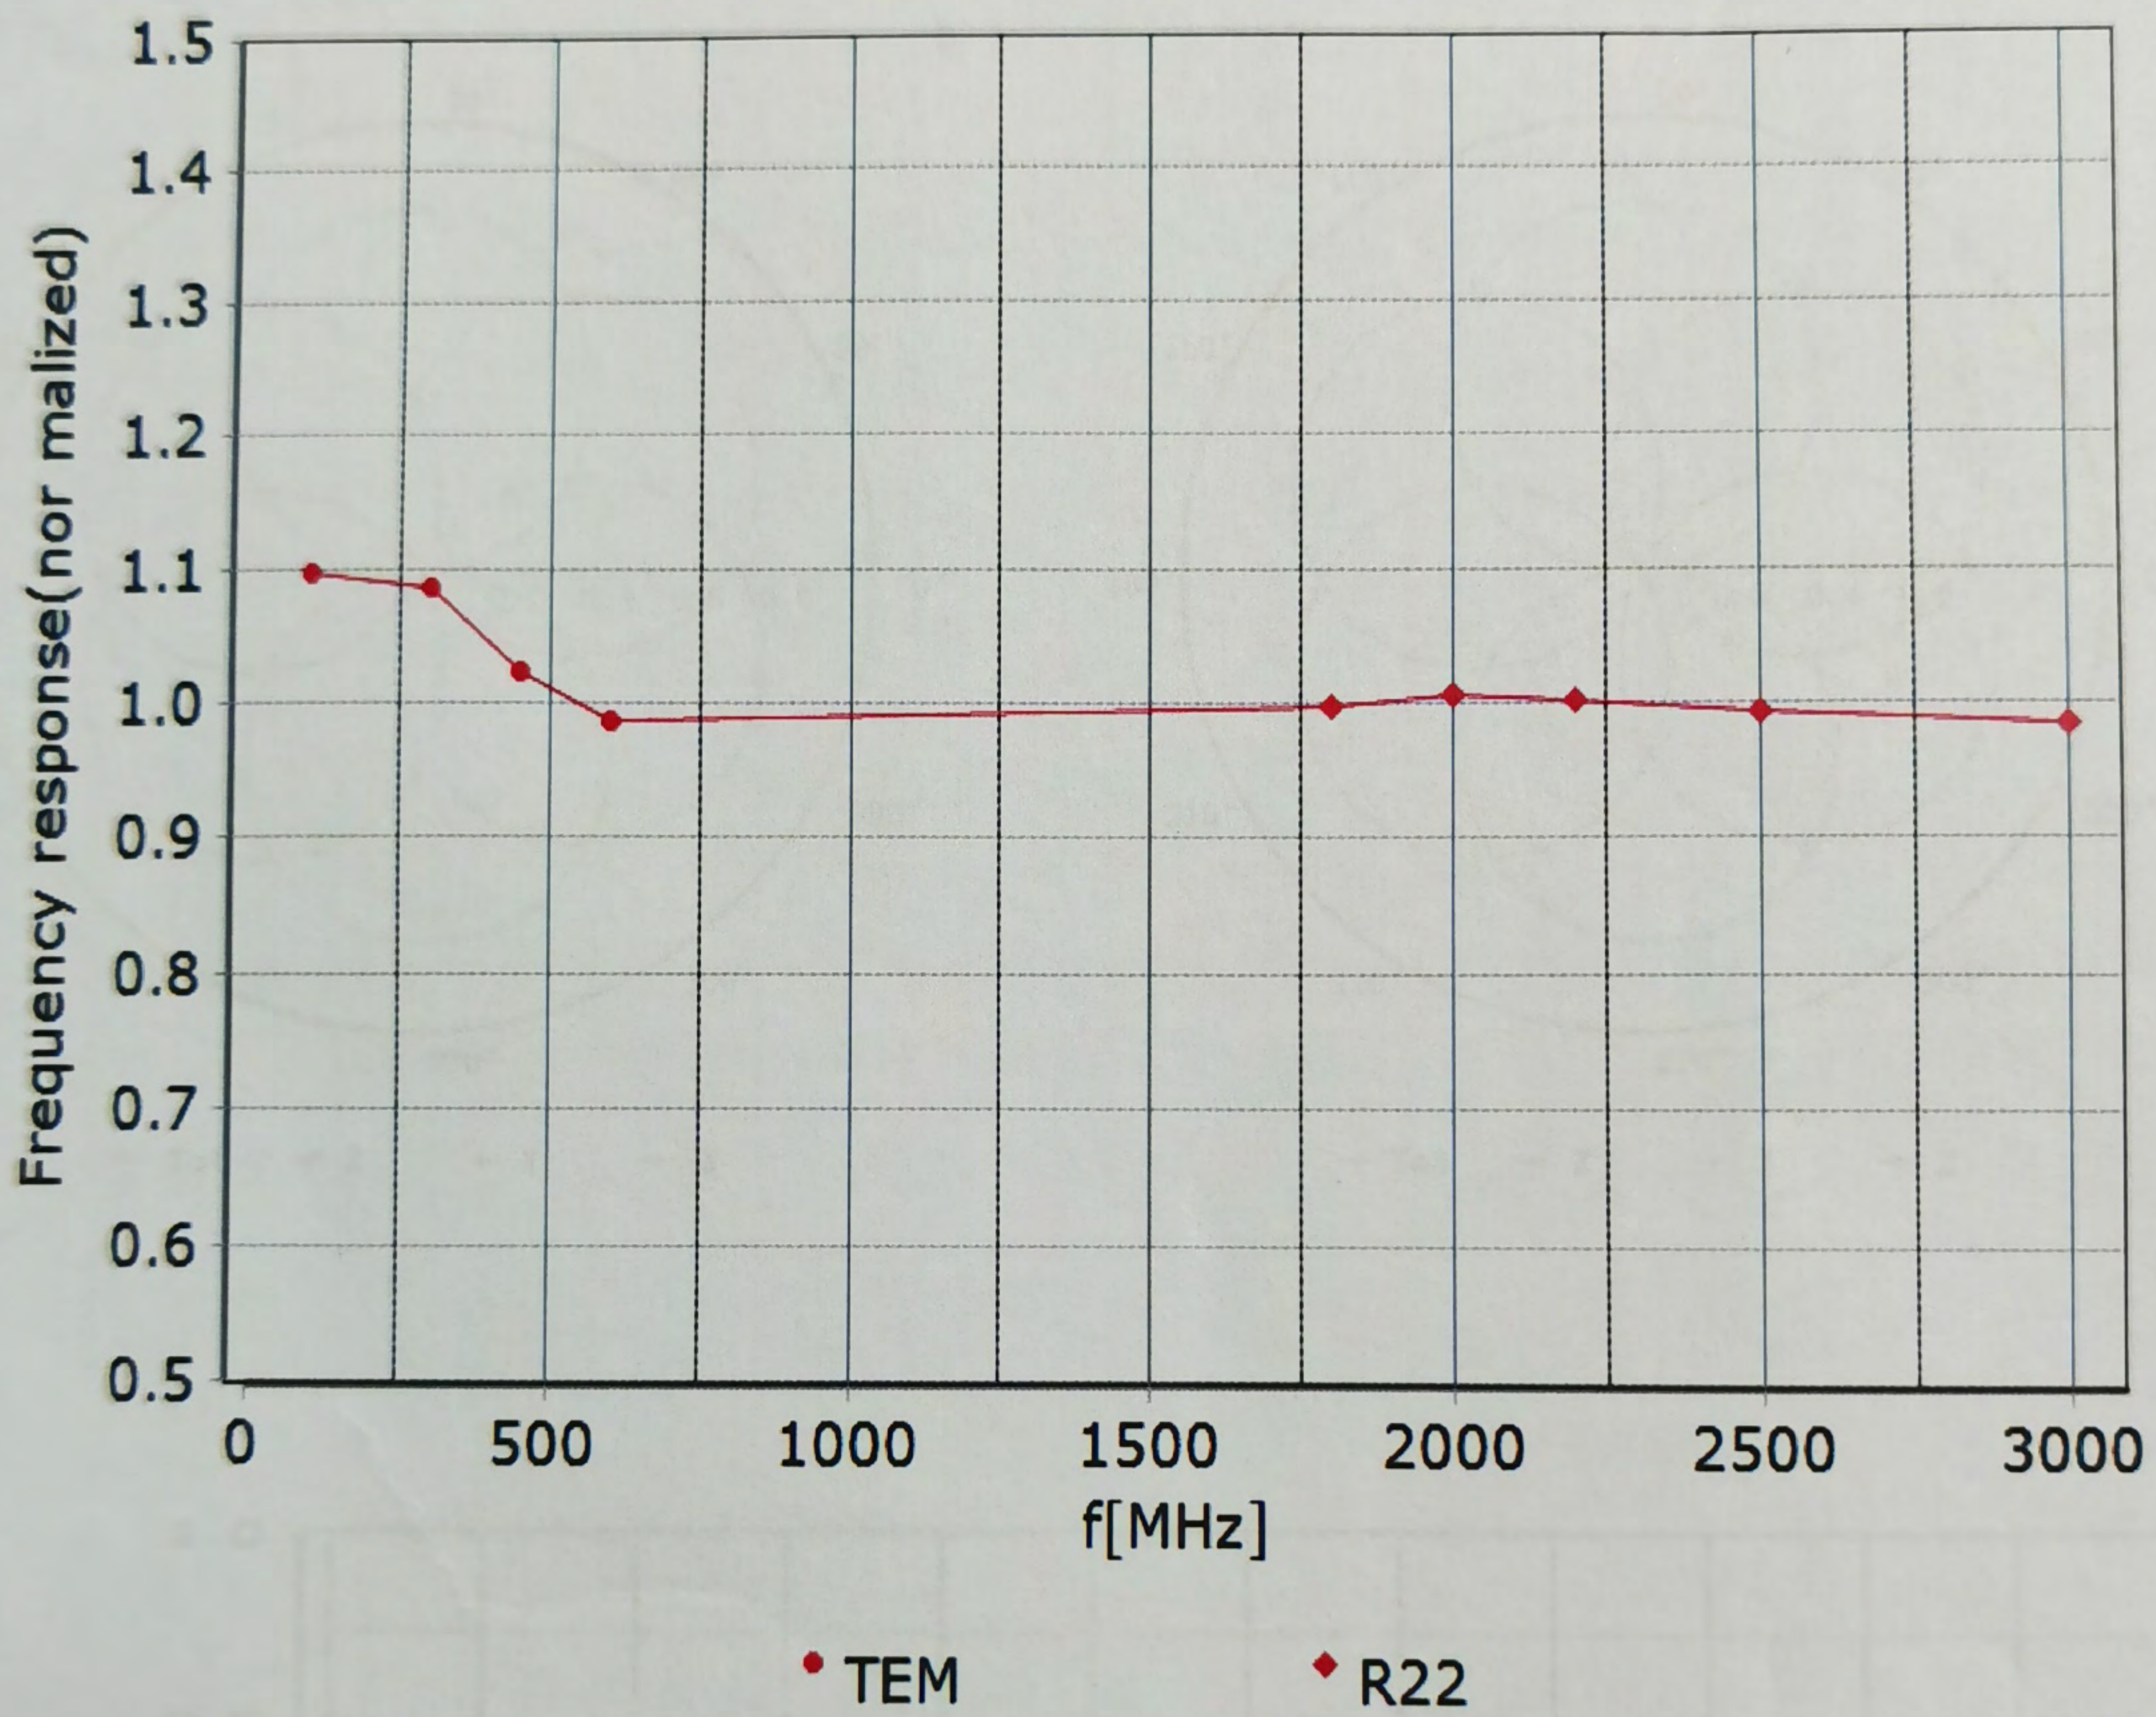

Uncertainty of Frequency Response of E-field: $\pm 7.4\%$ ($k=2$)






In Collaboration with
s p e a g
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504
E-mail: cttl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

Receiving Pattern (Φ), $\theta=0^\circ$

f=600 MHz, TEM



f=1800 MHz, R22

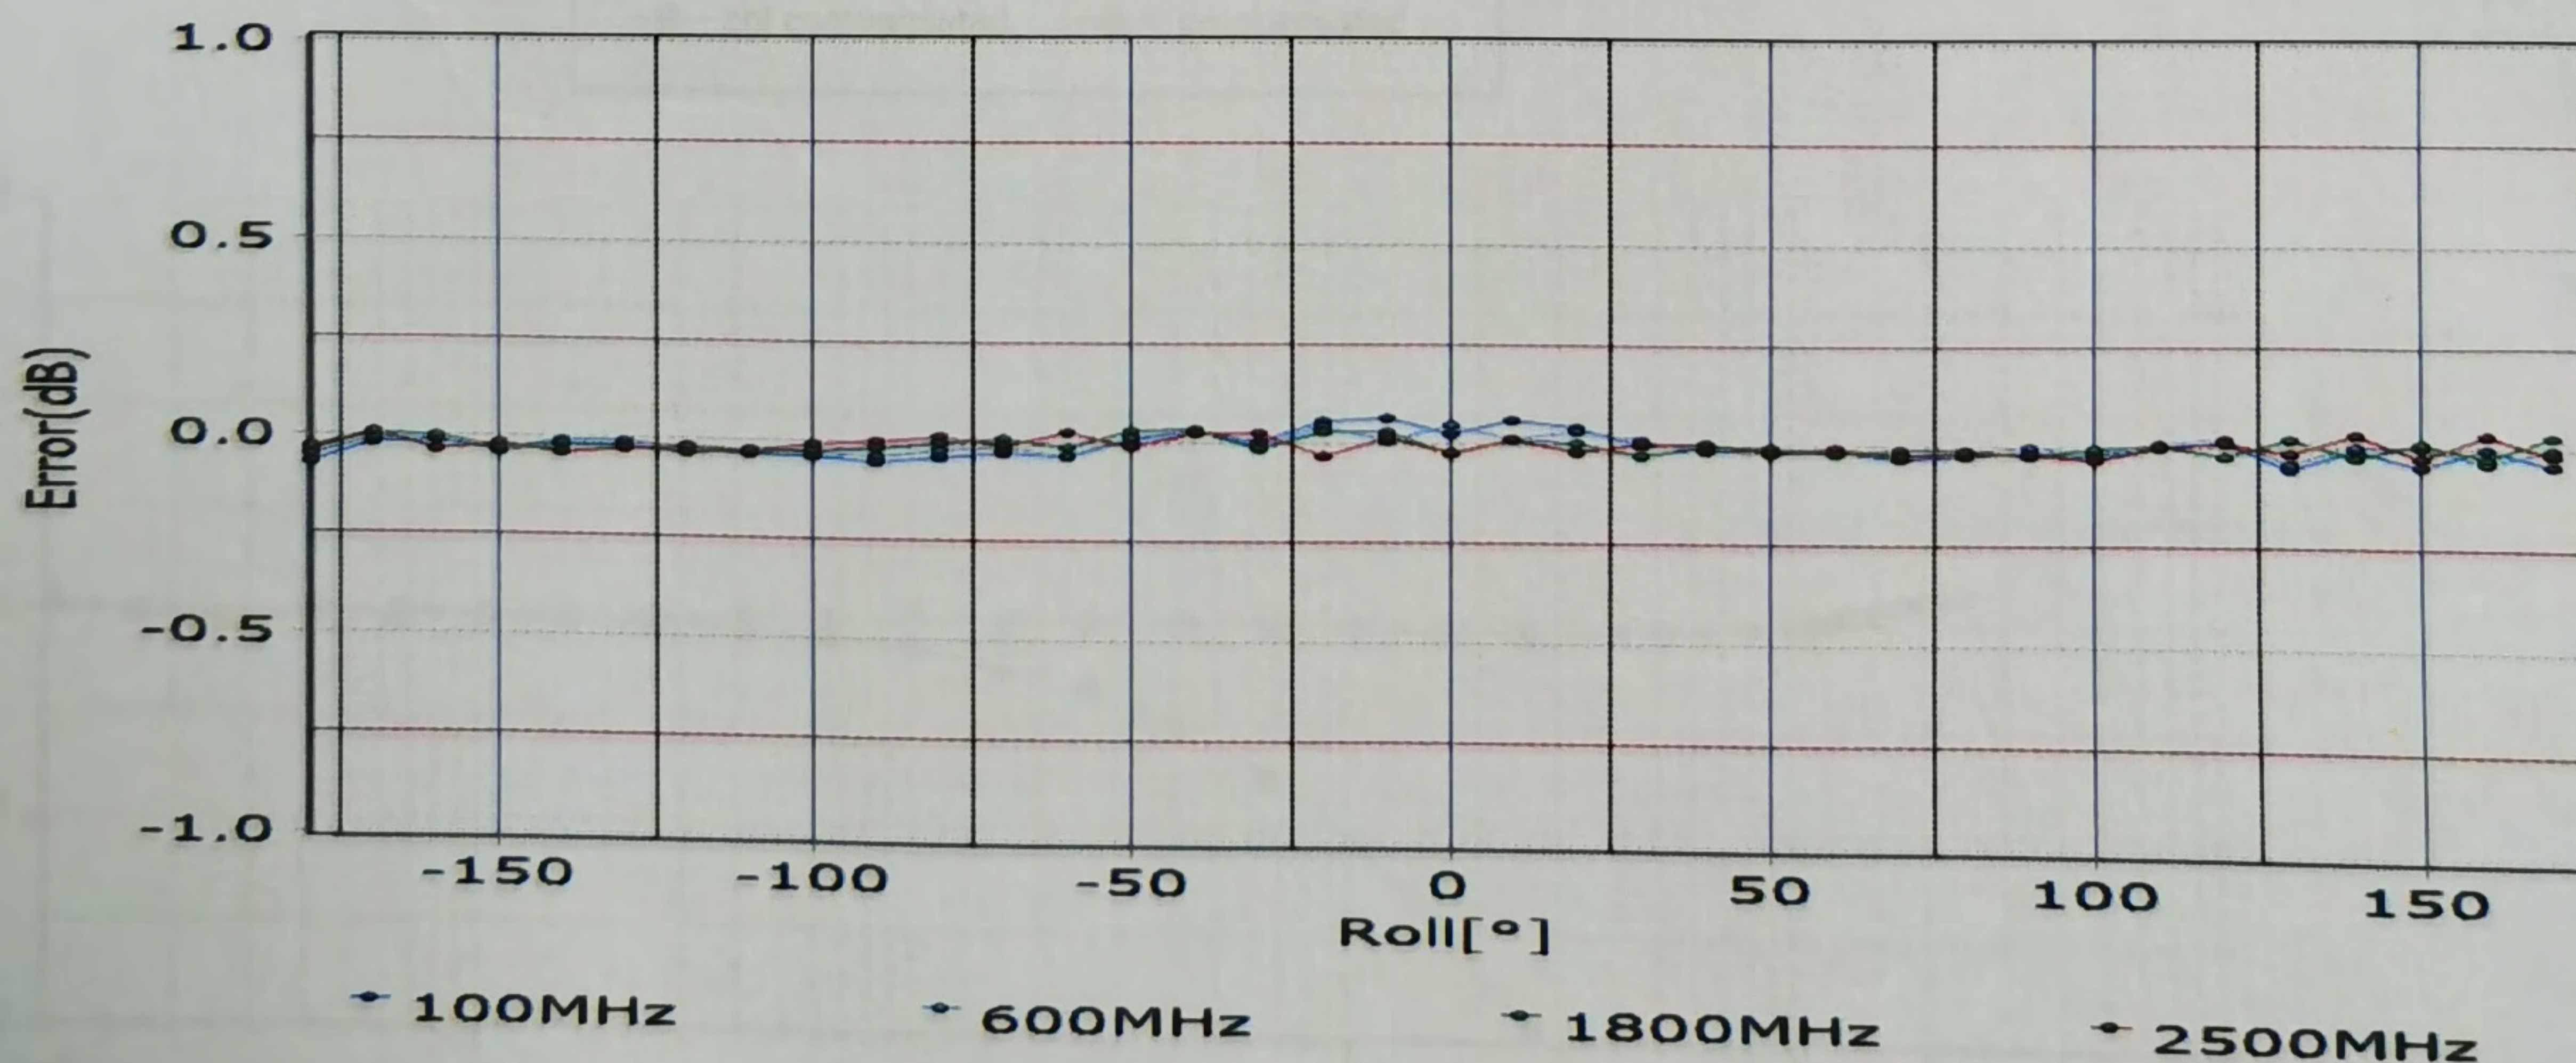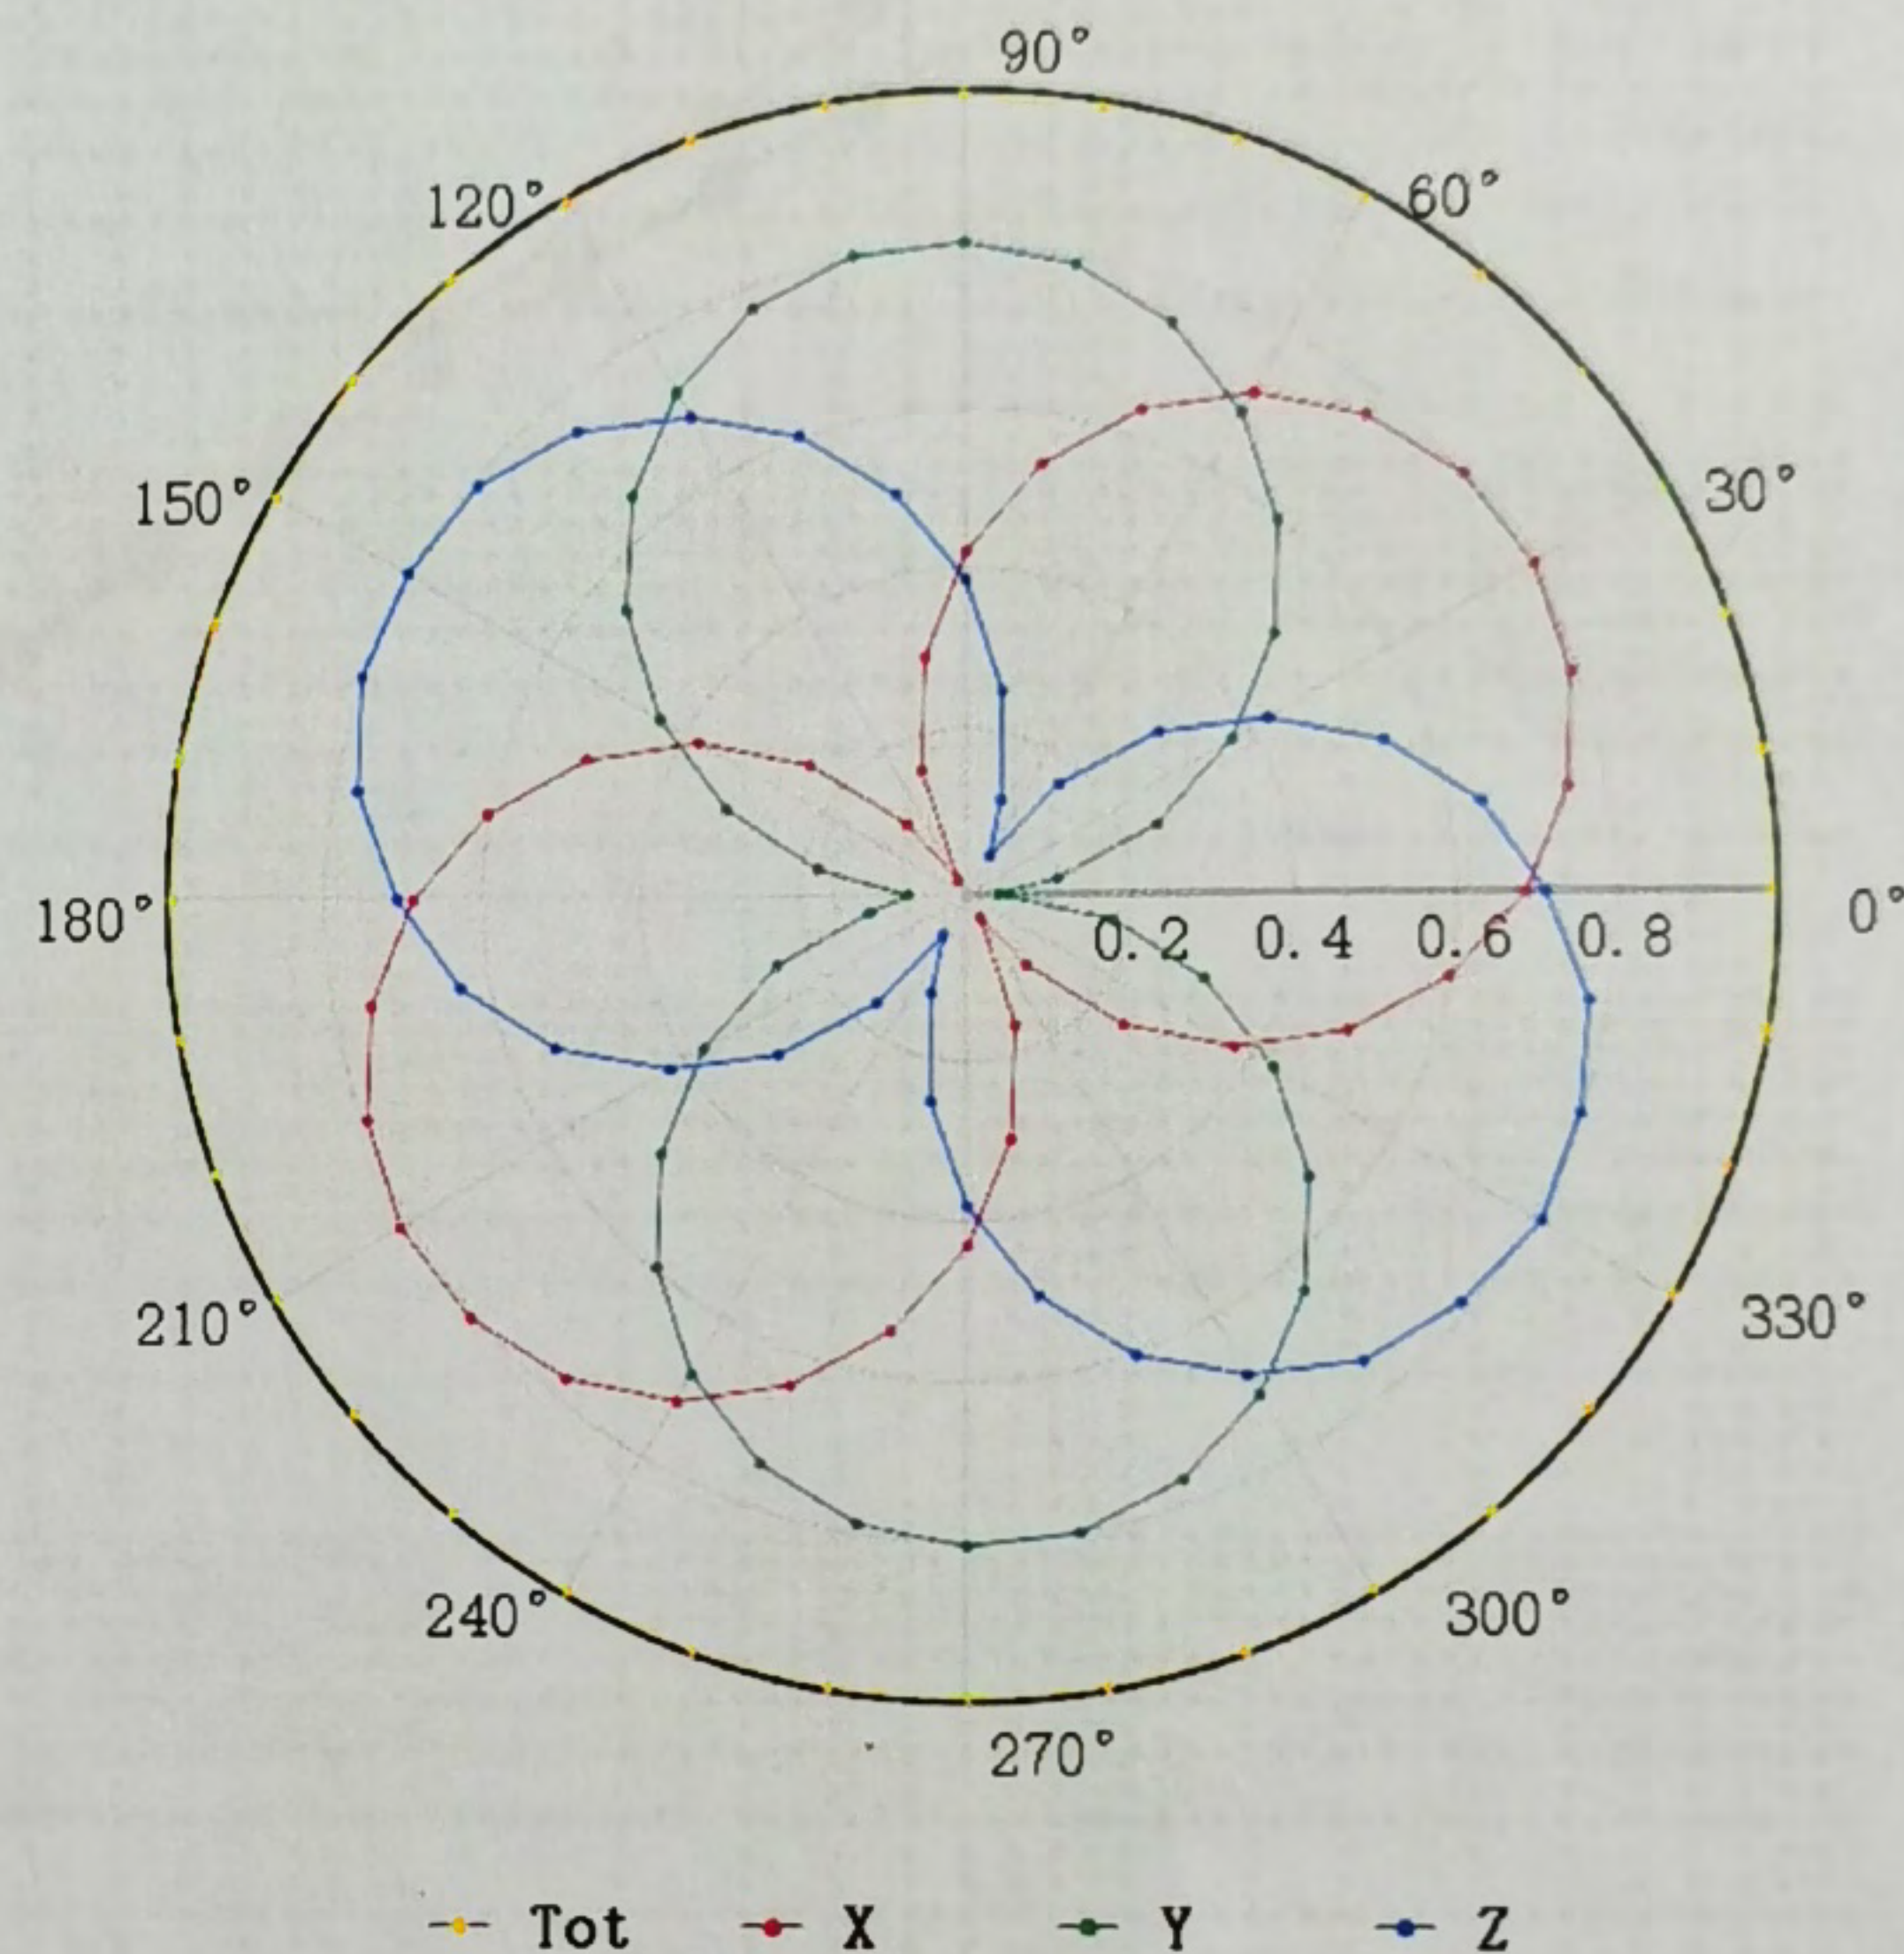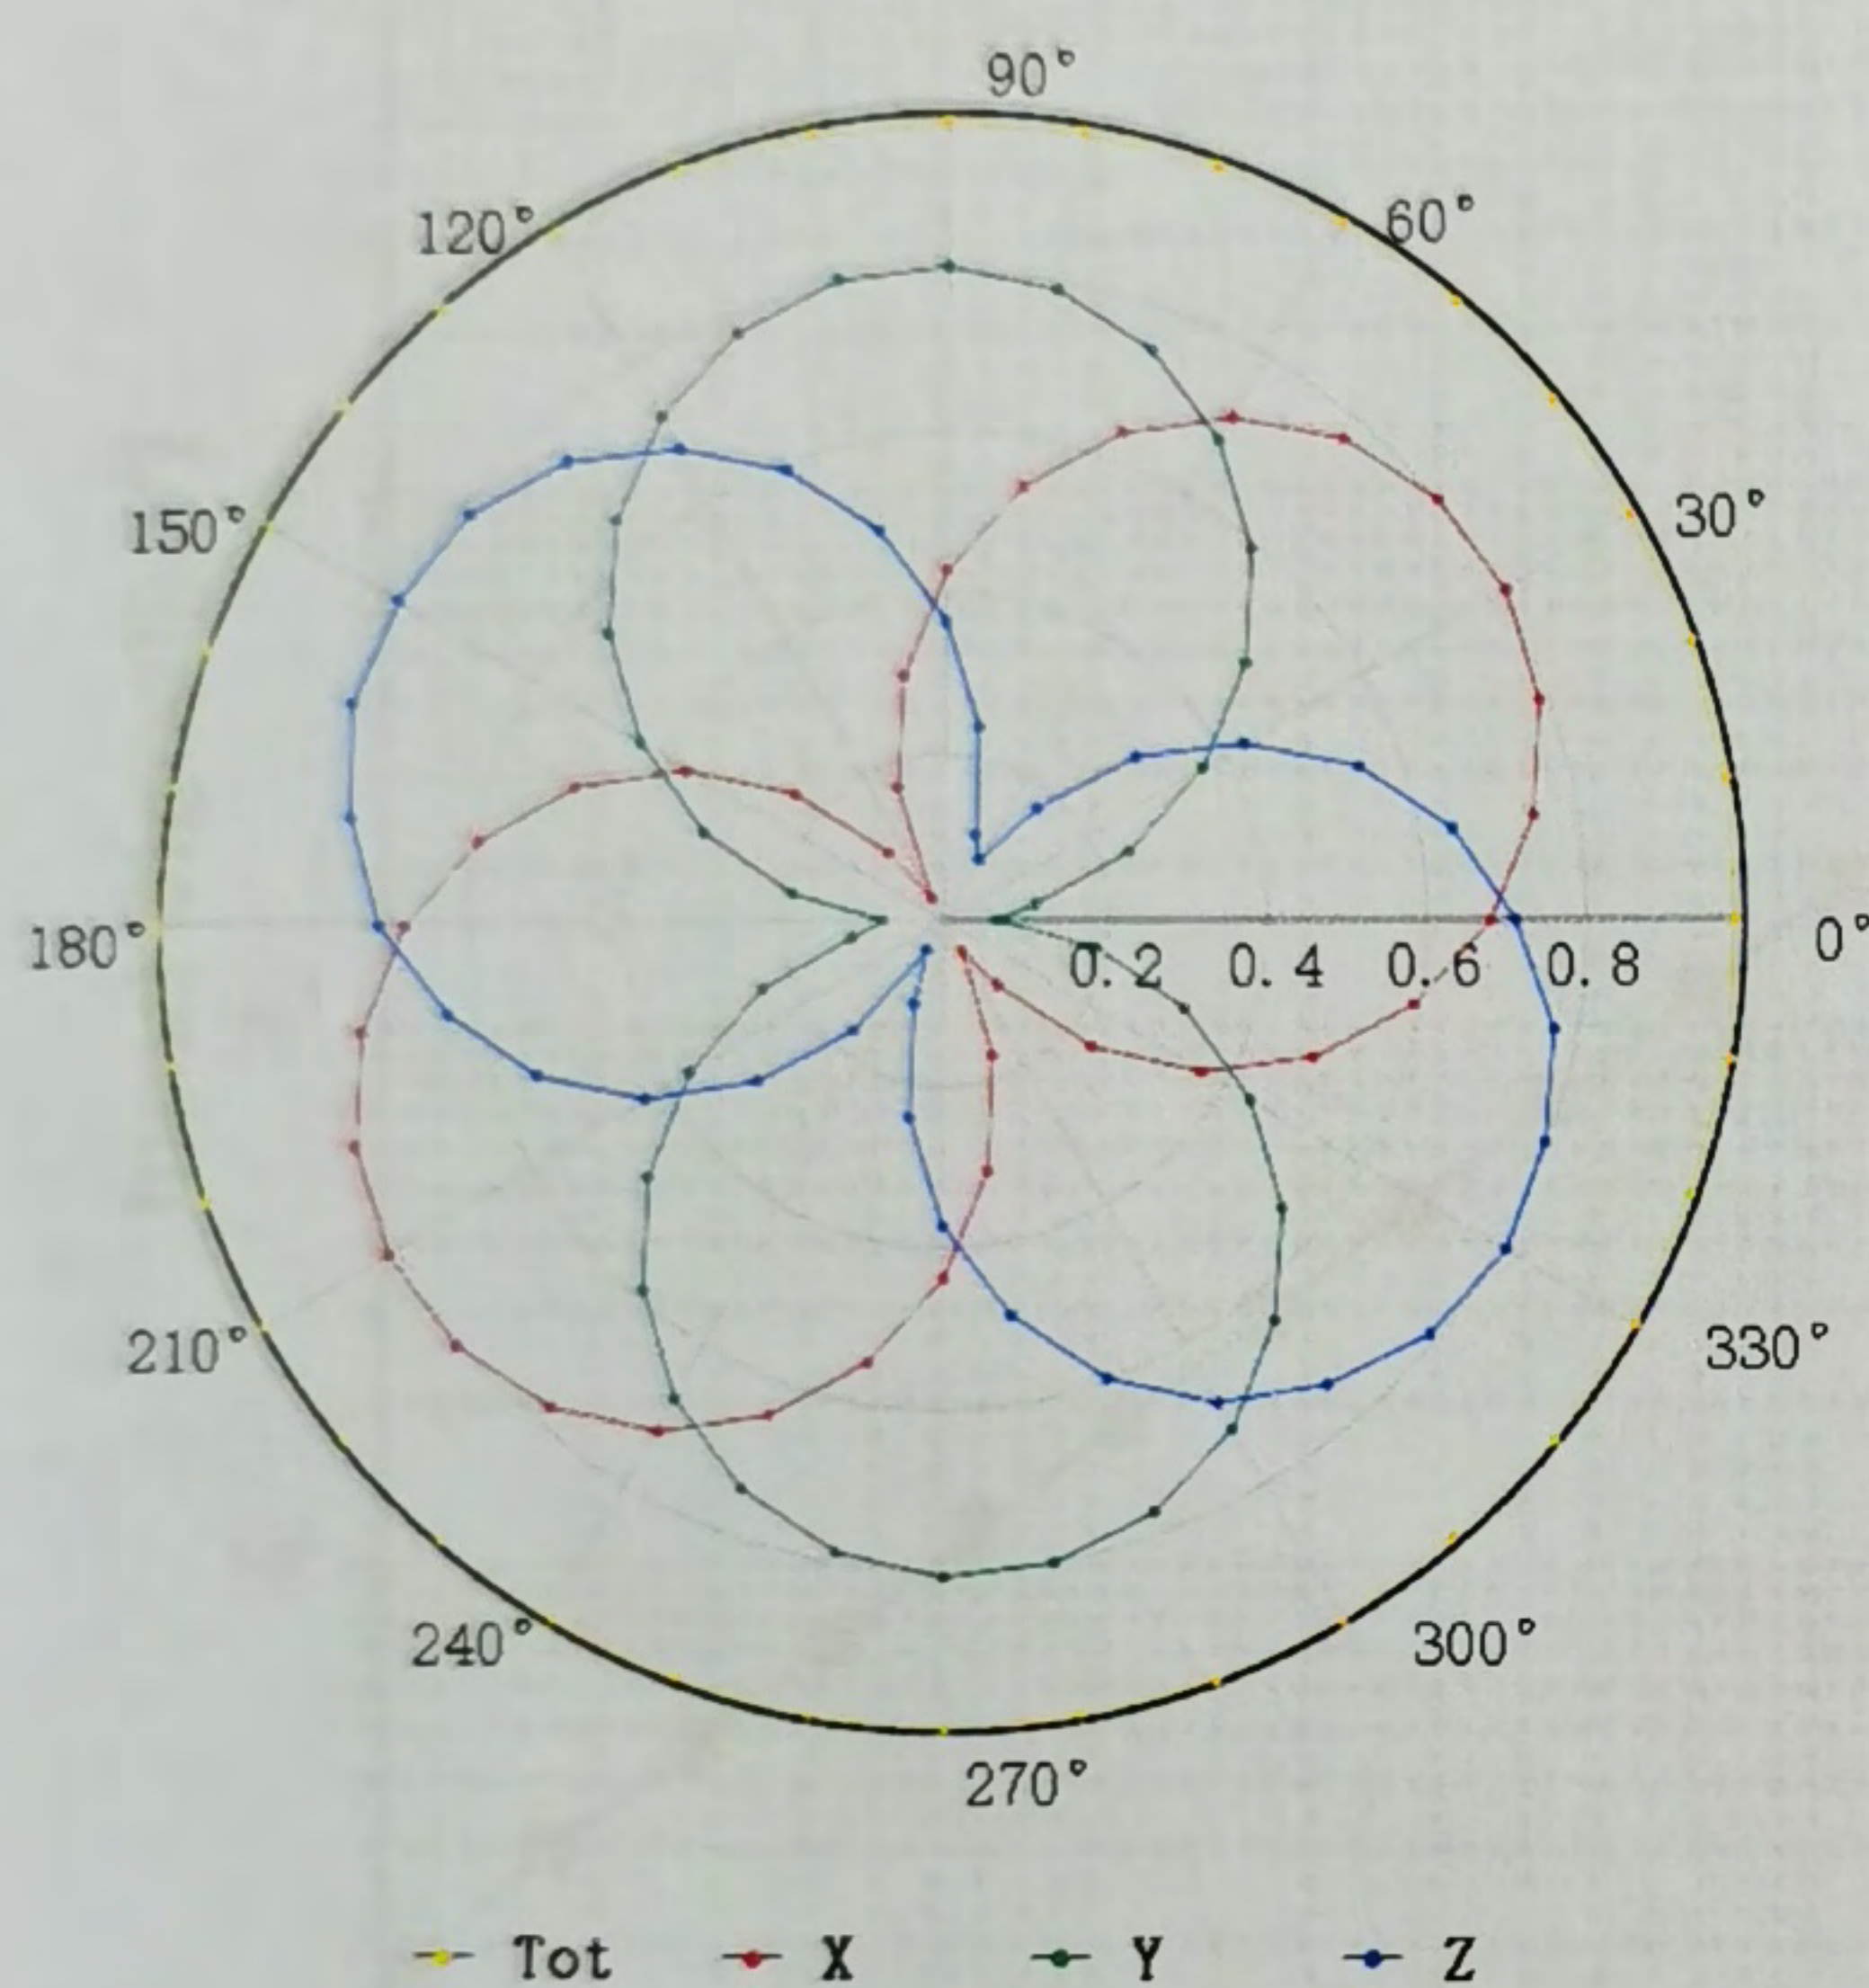

Uncertainty of Axial Isotropy Assessment: $\pm 1.2\%$ ($k=2$)



Dynamic Range f(SAR_{head}) (TEM cell, f = 900 MHz)

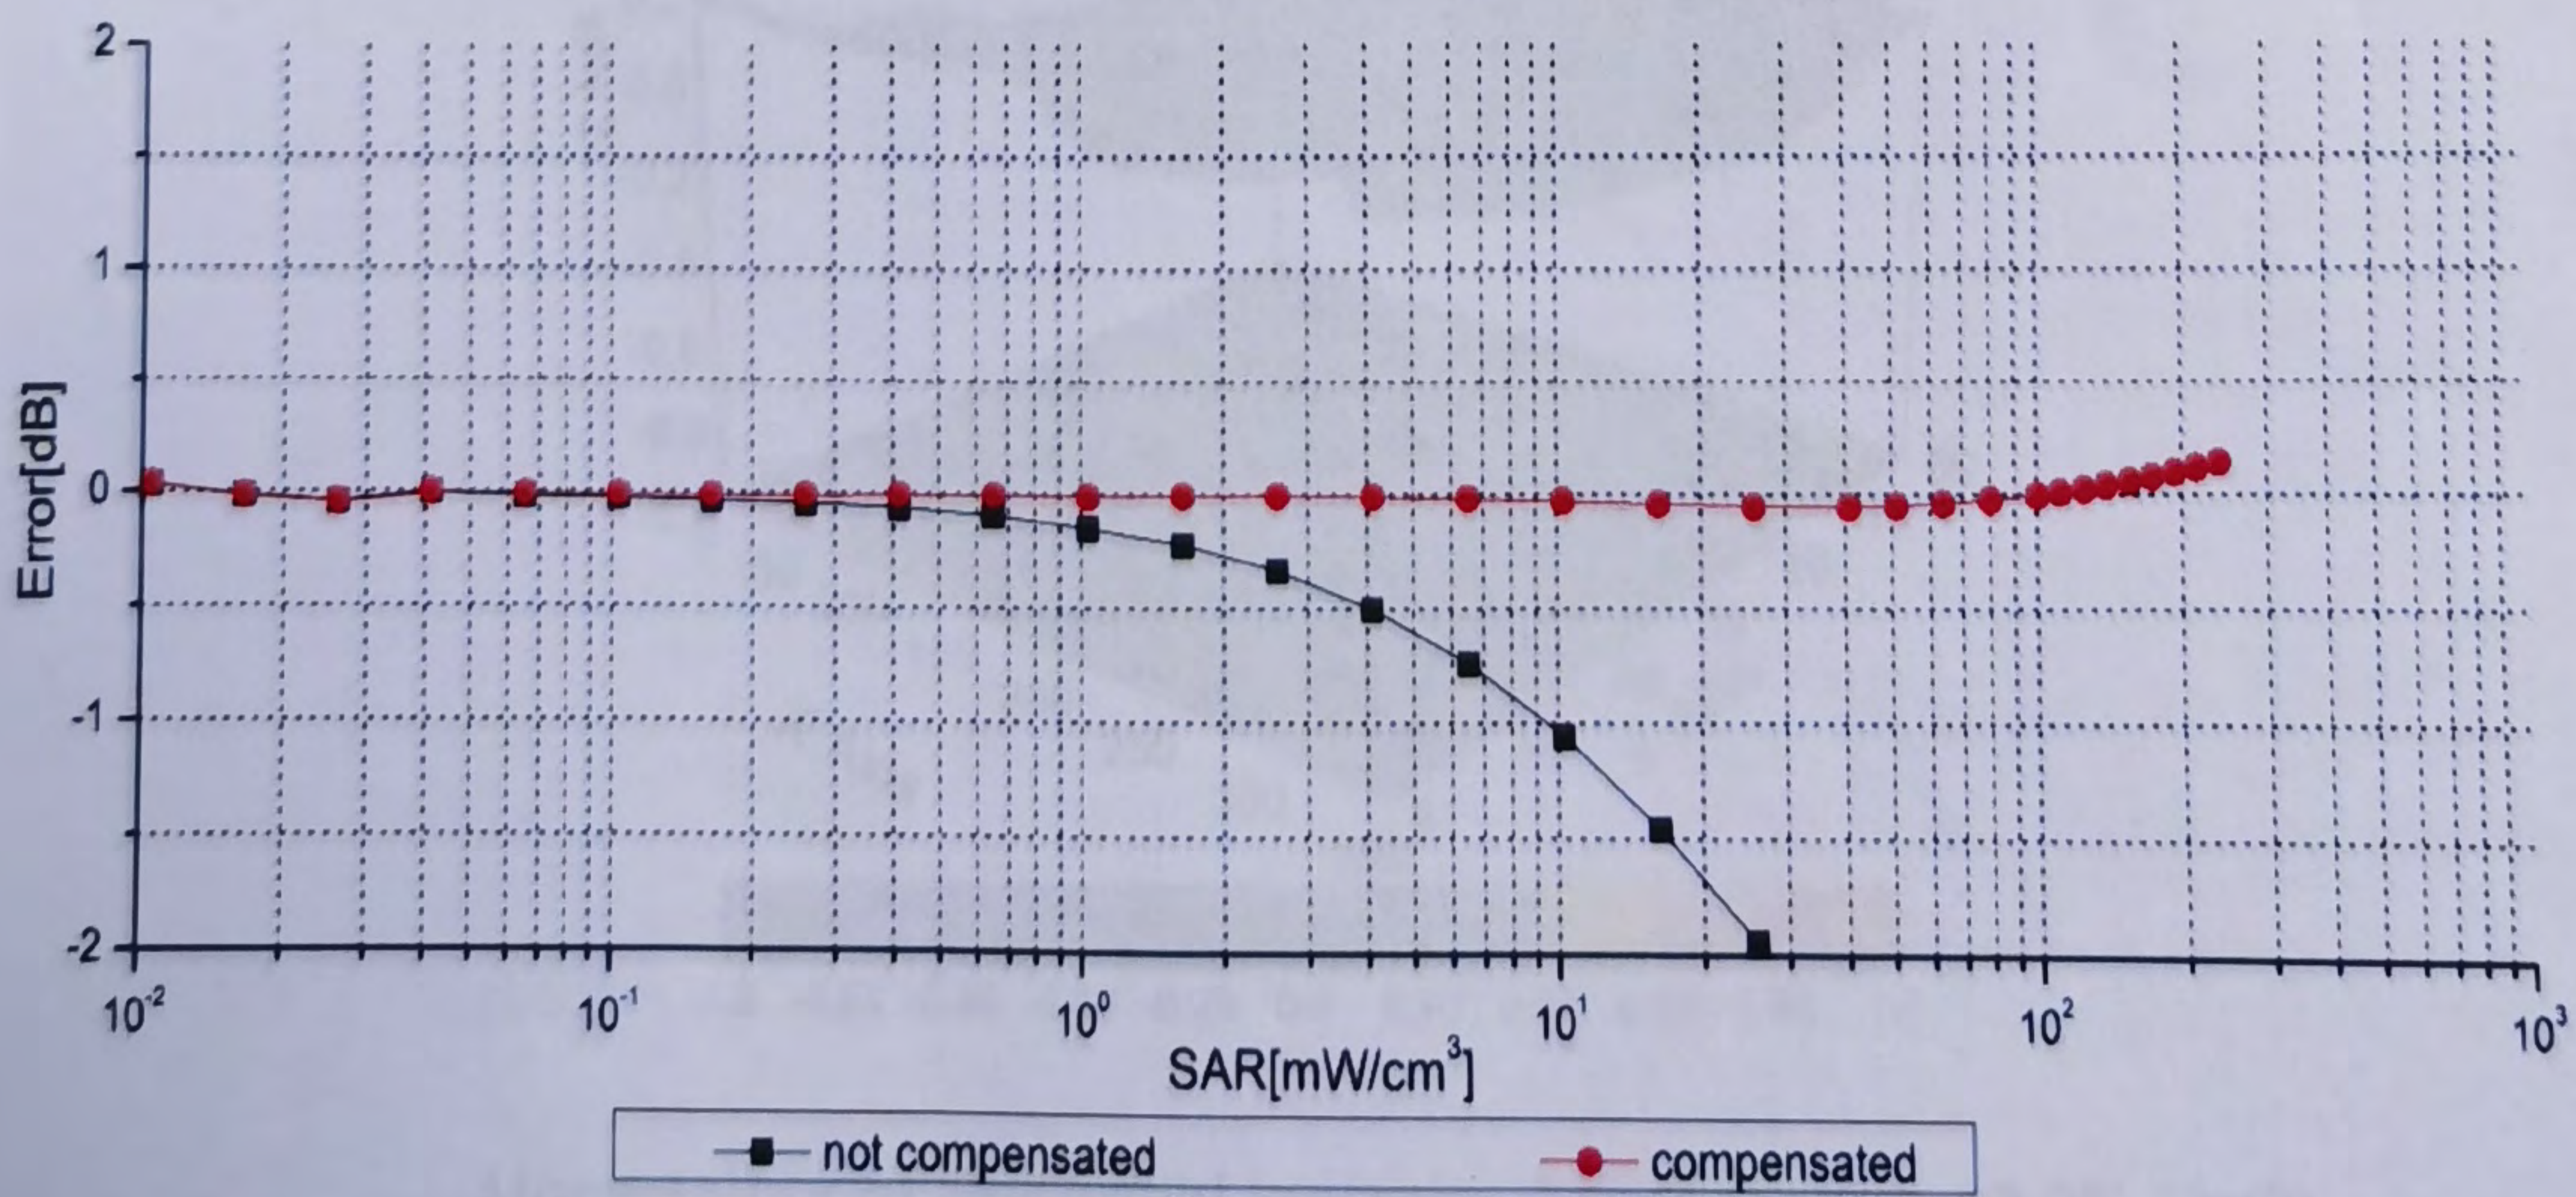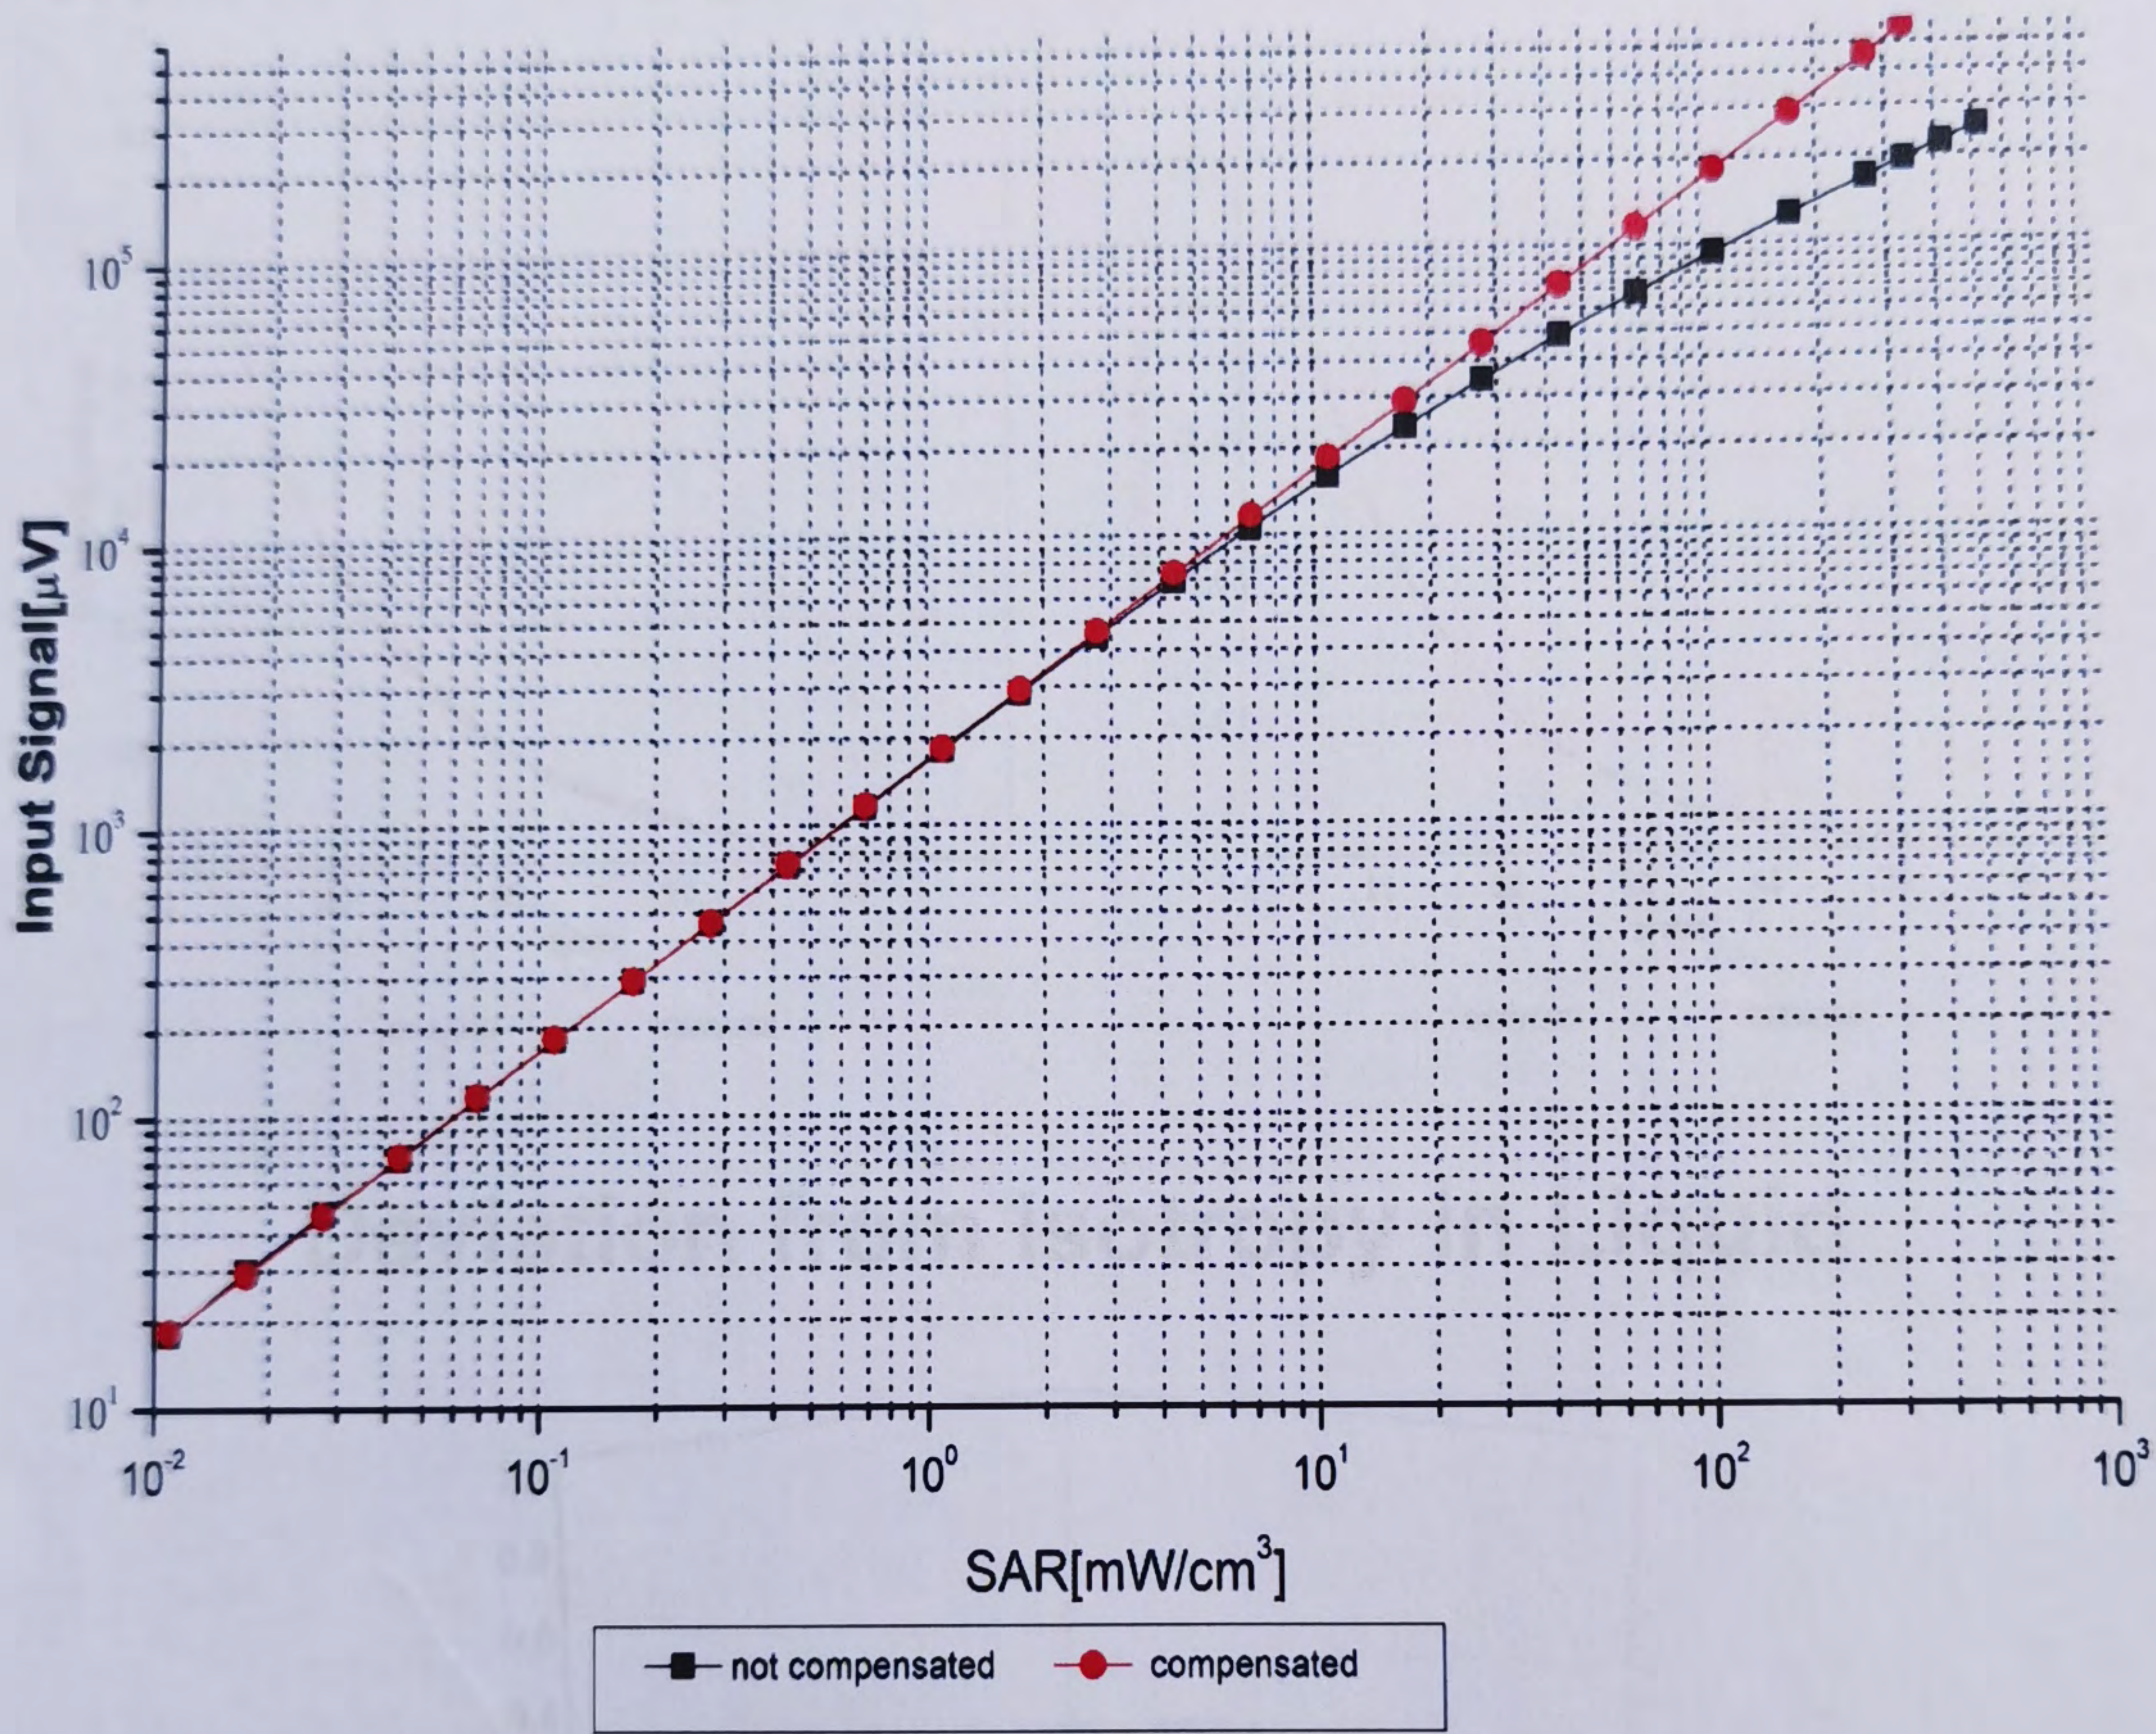

Uncertainty of Linearity Assessment: ±0.9% (k=2)





In Collaboration with
s p e a g
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504
E-mail: cttl@chinattl.com Http://www.chinattl.cn

Conversion Factor Assessment

f=750 MHz,WGLS R9(H_convF)


f=1750 MHz,WGLS R22(H_convF)

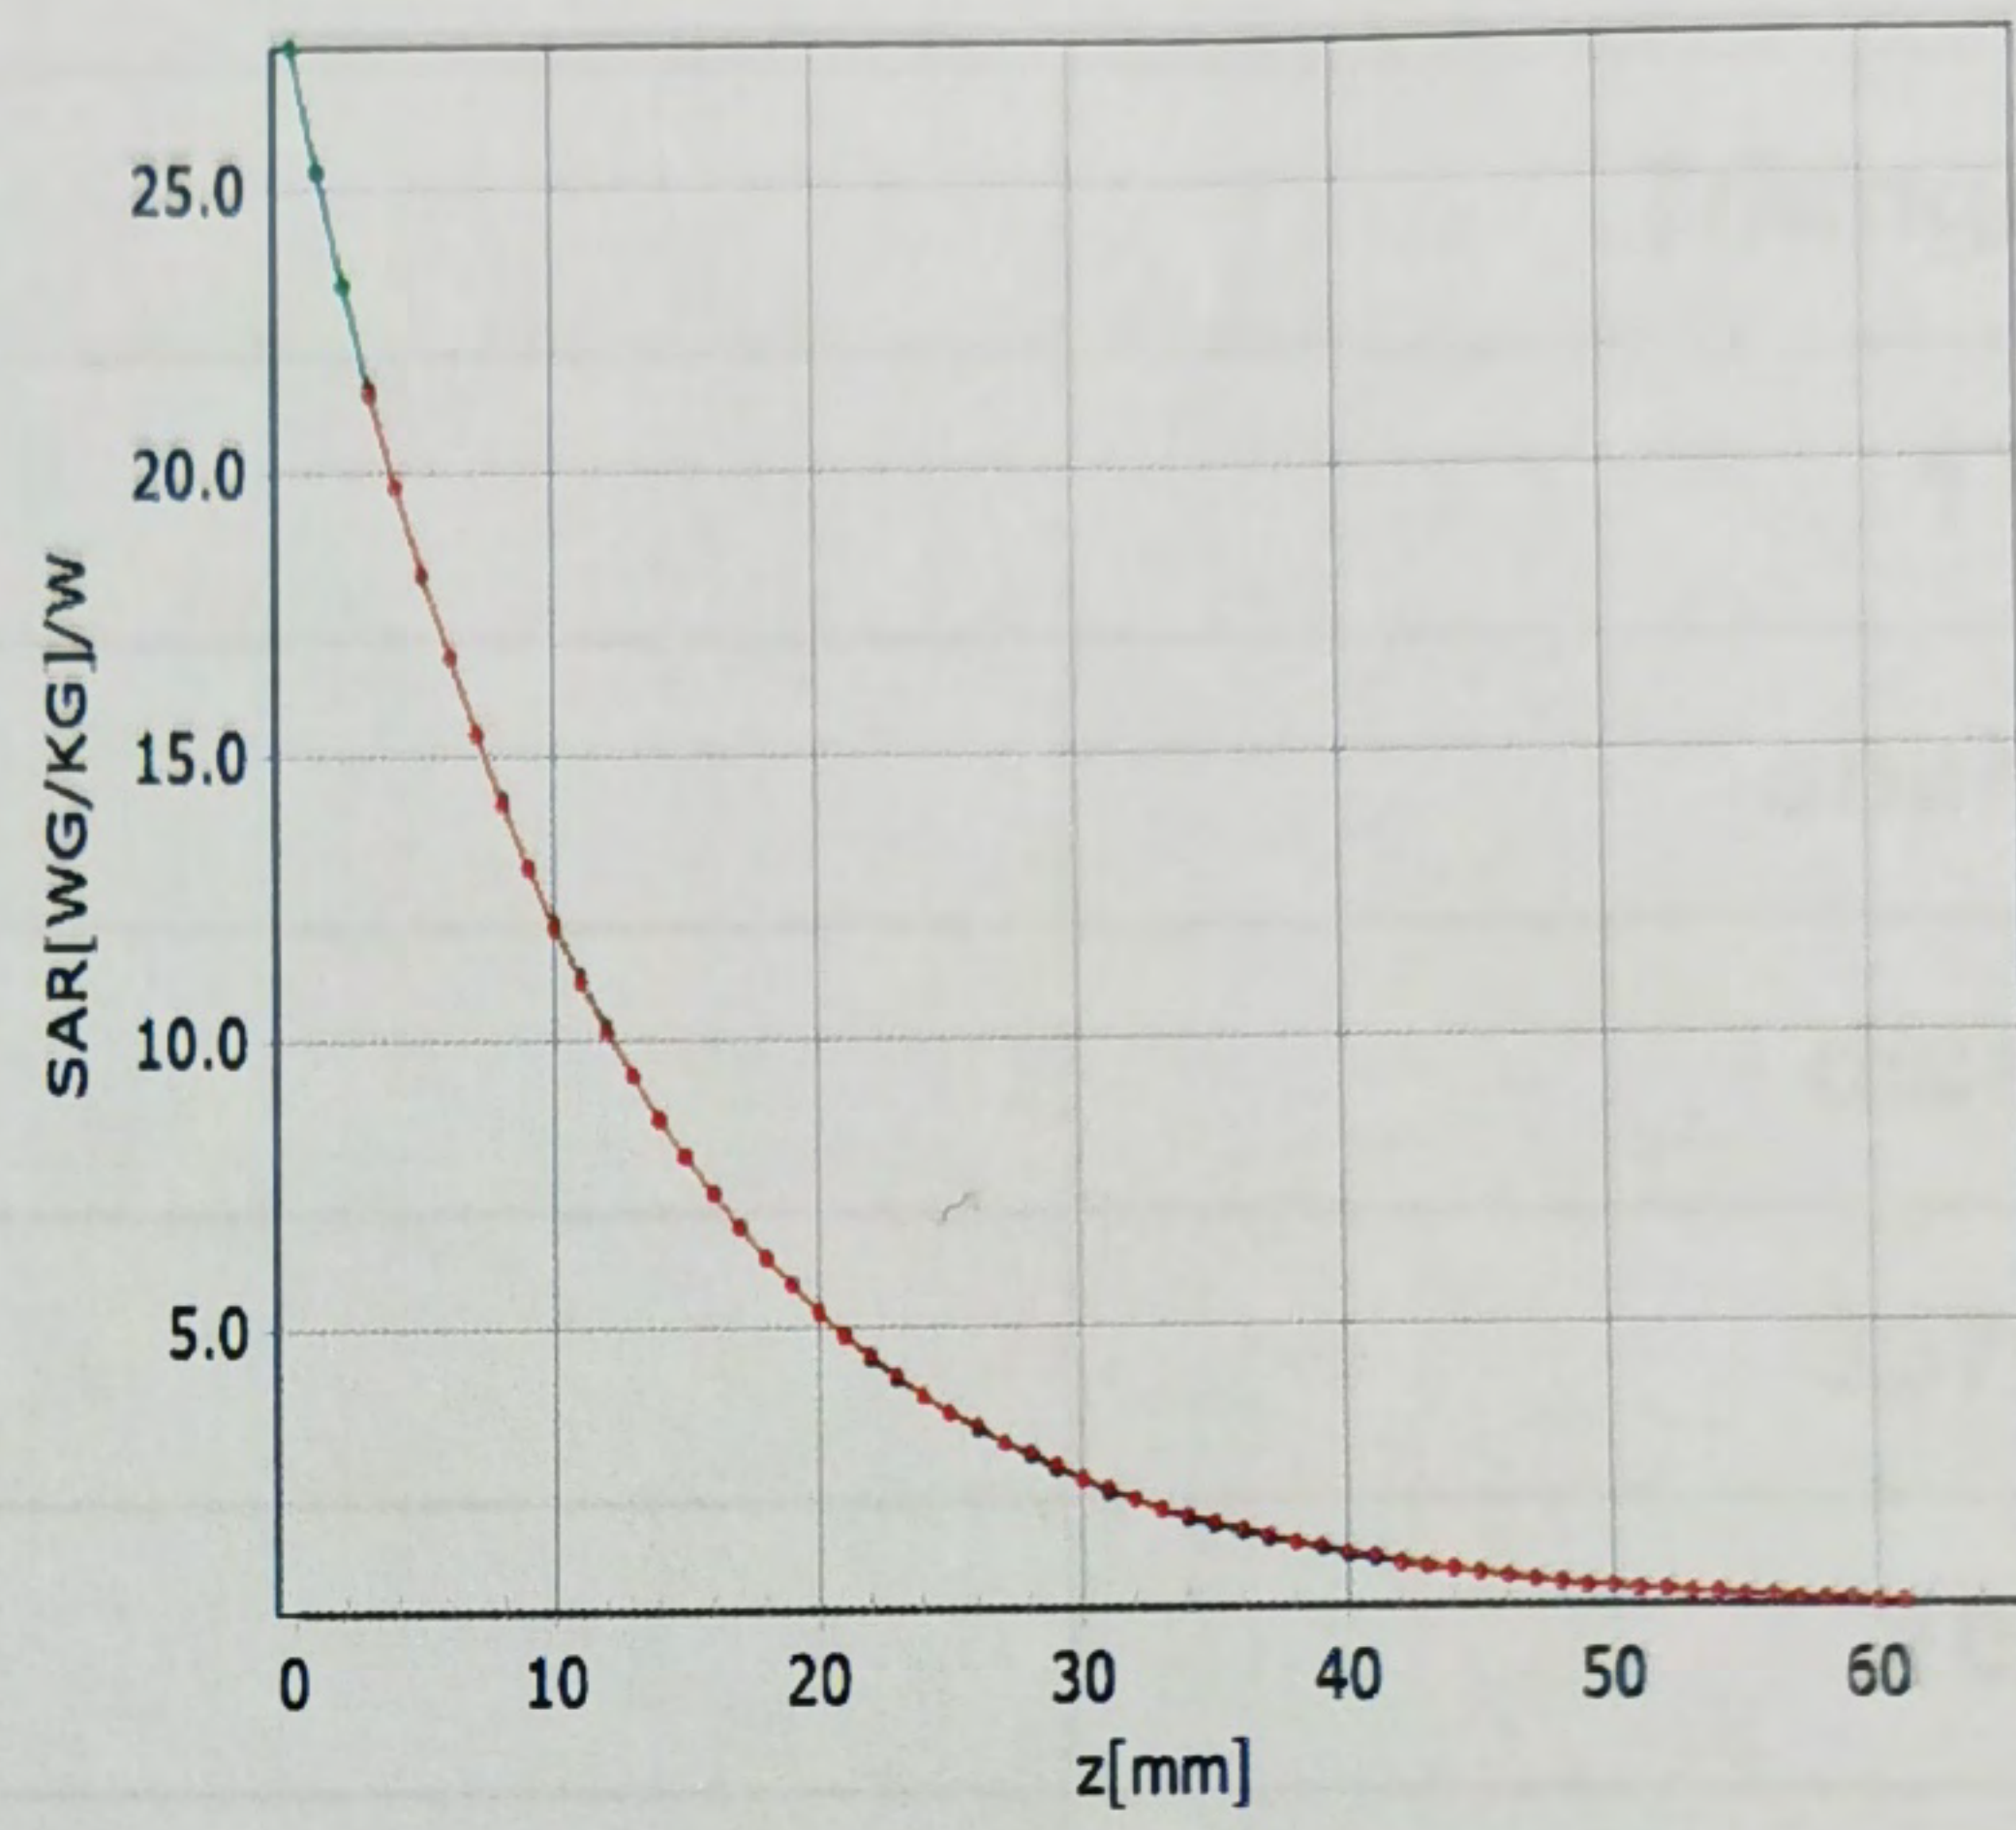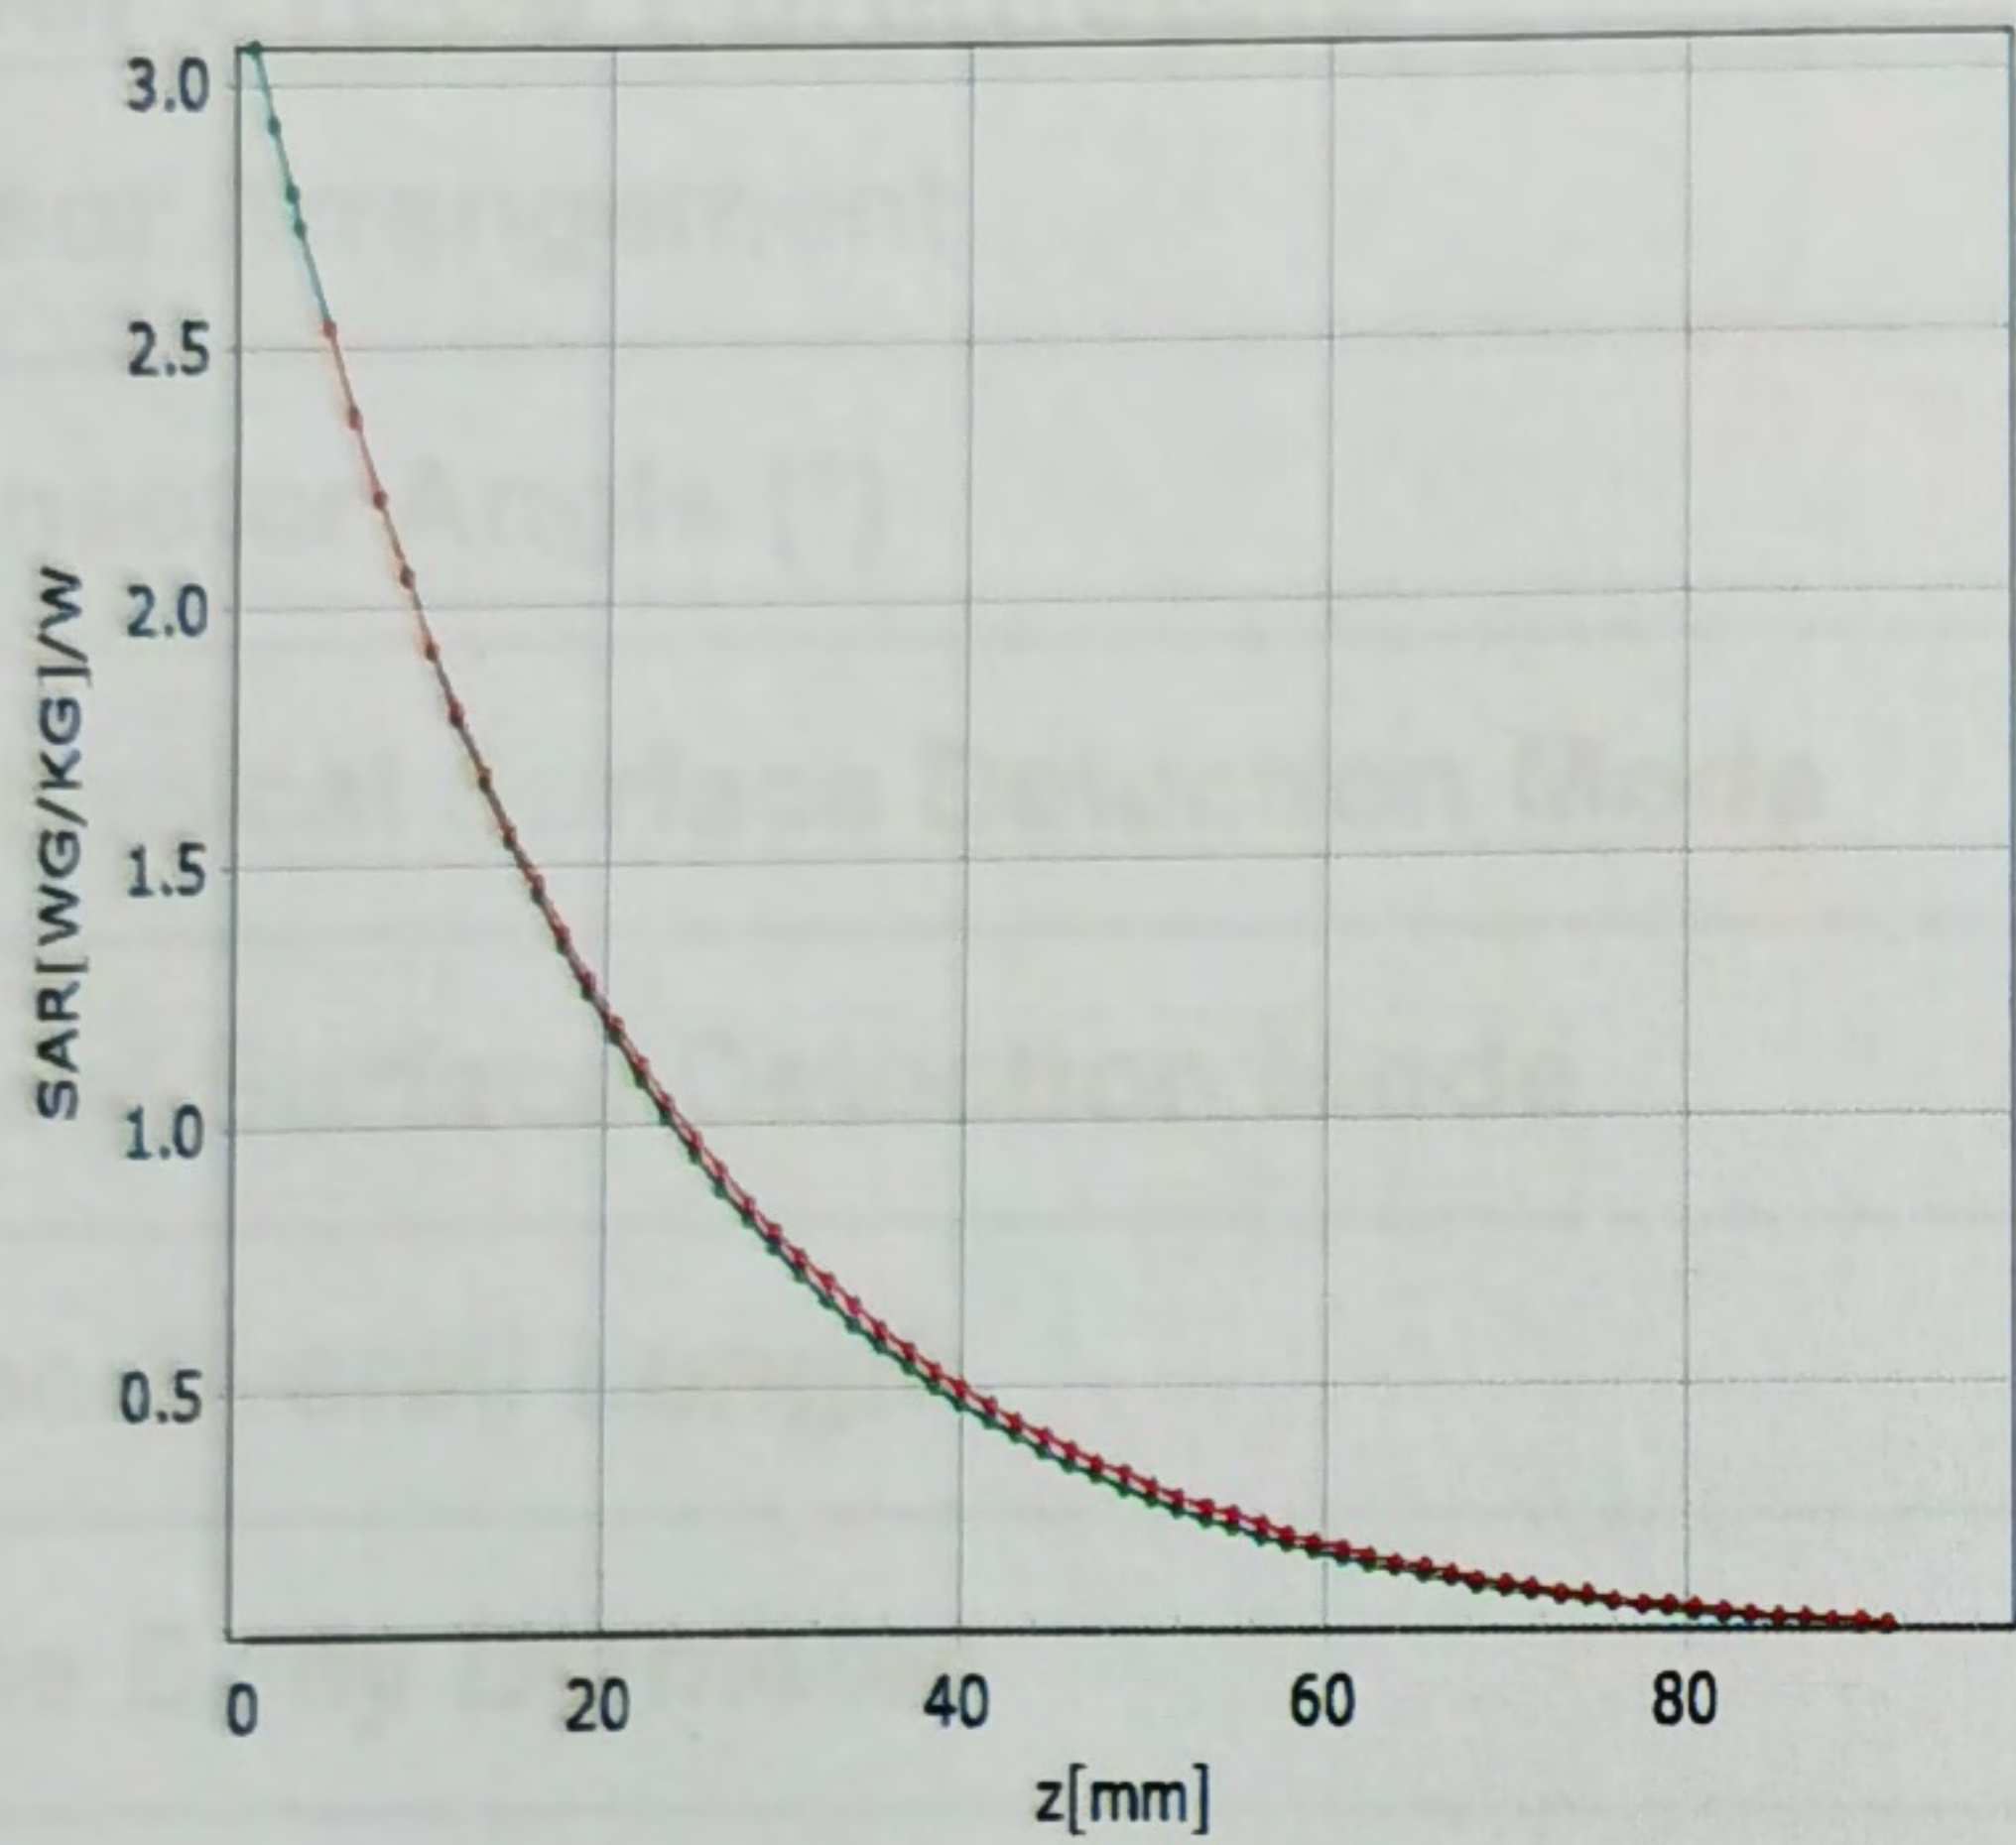

* analytical * measured

* analytical * measured

Deviation from Isotropy in Liquid

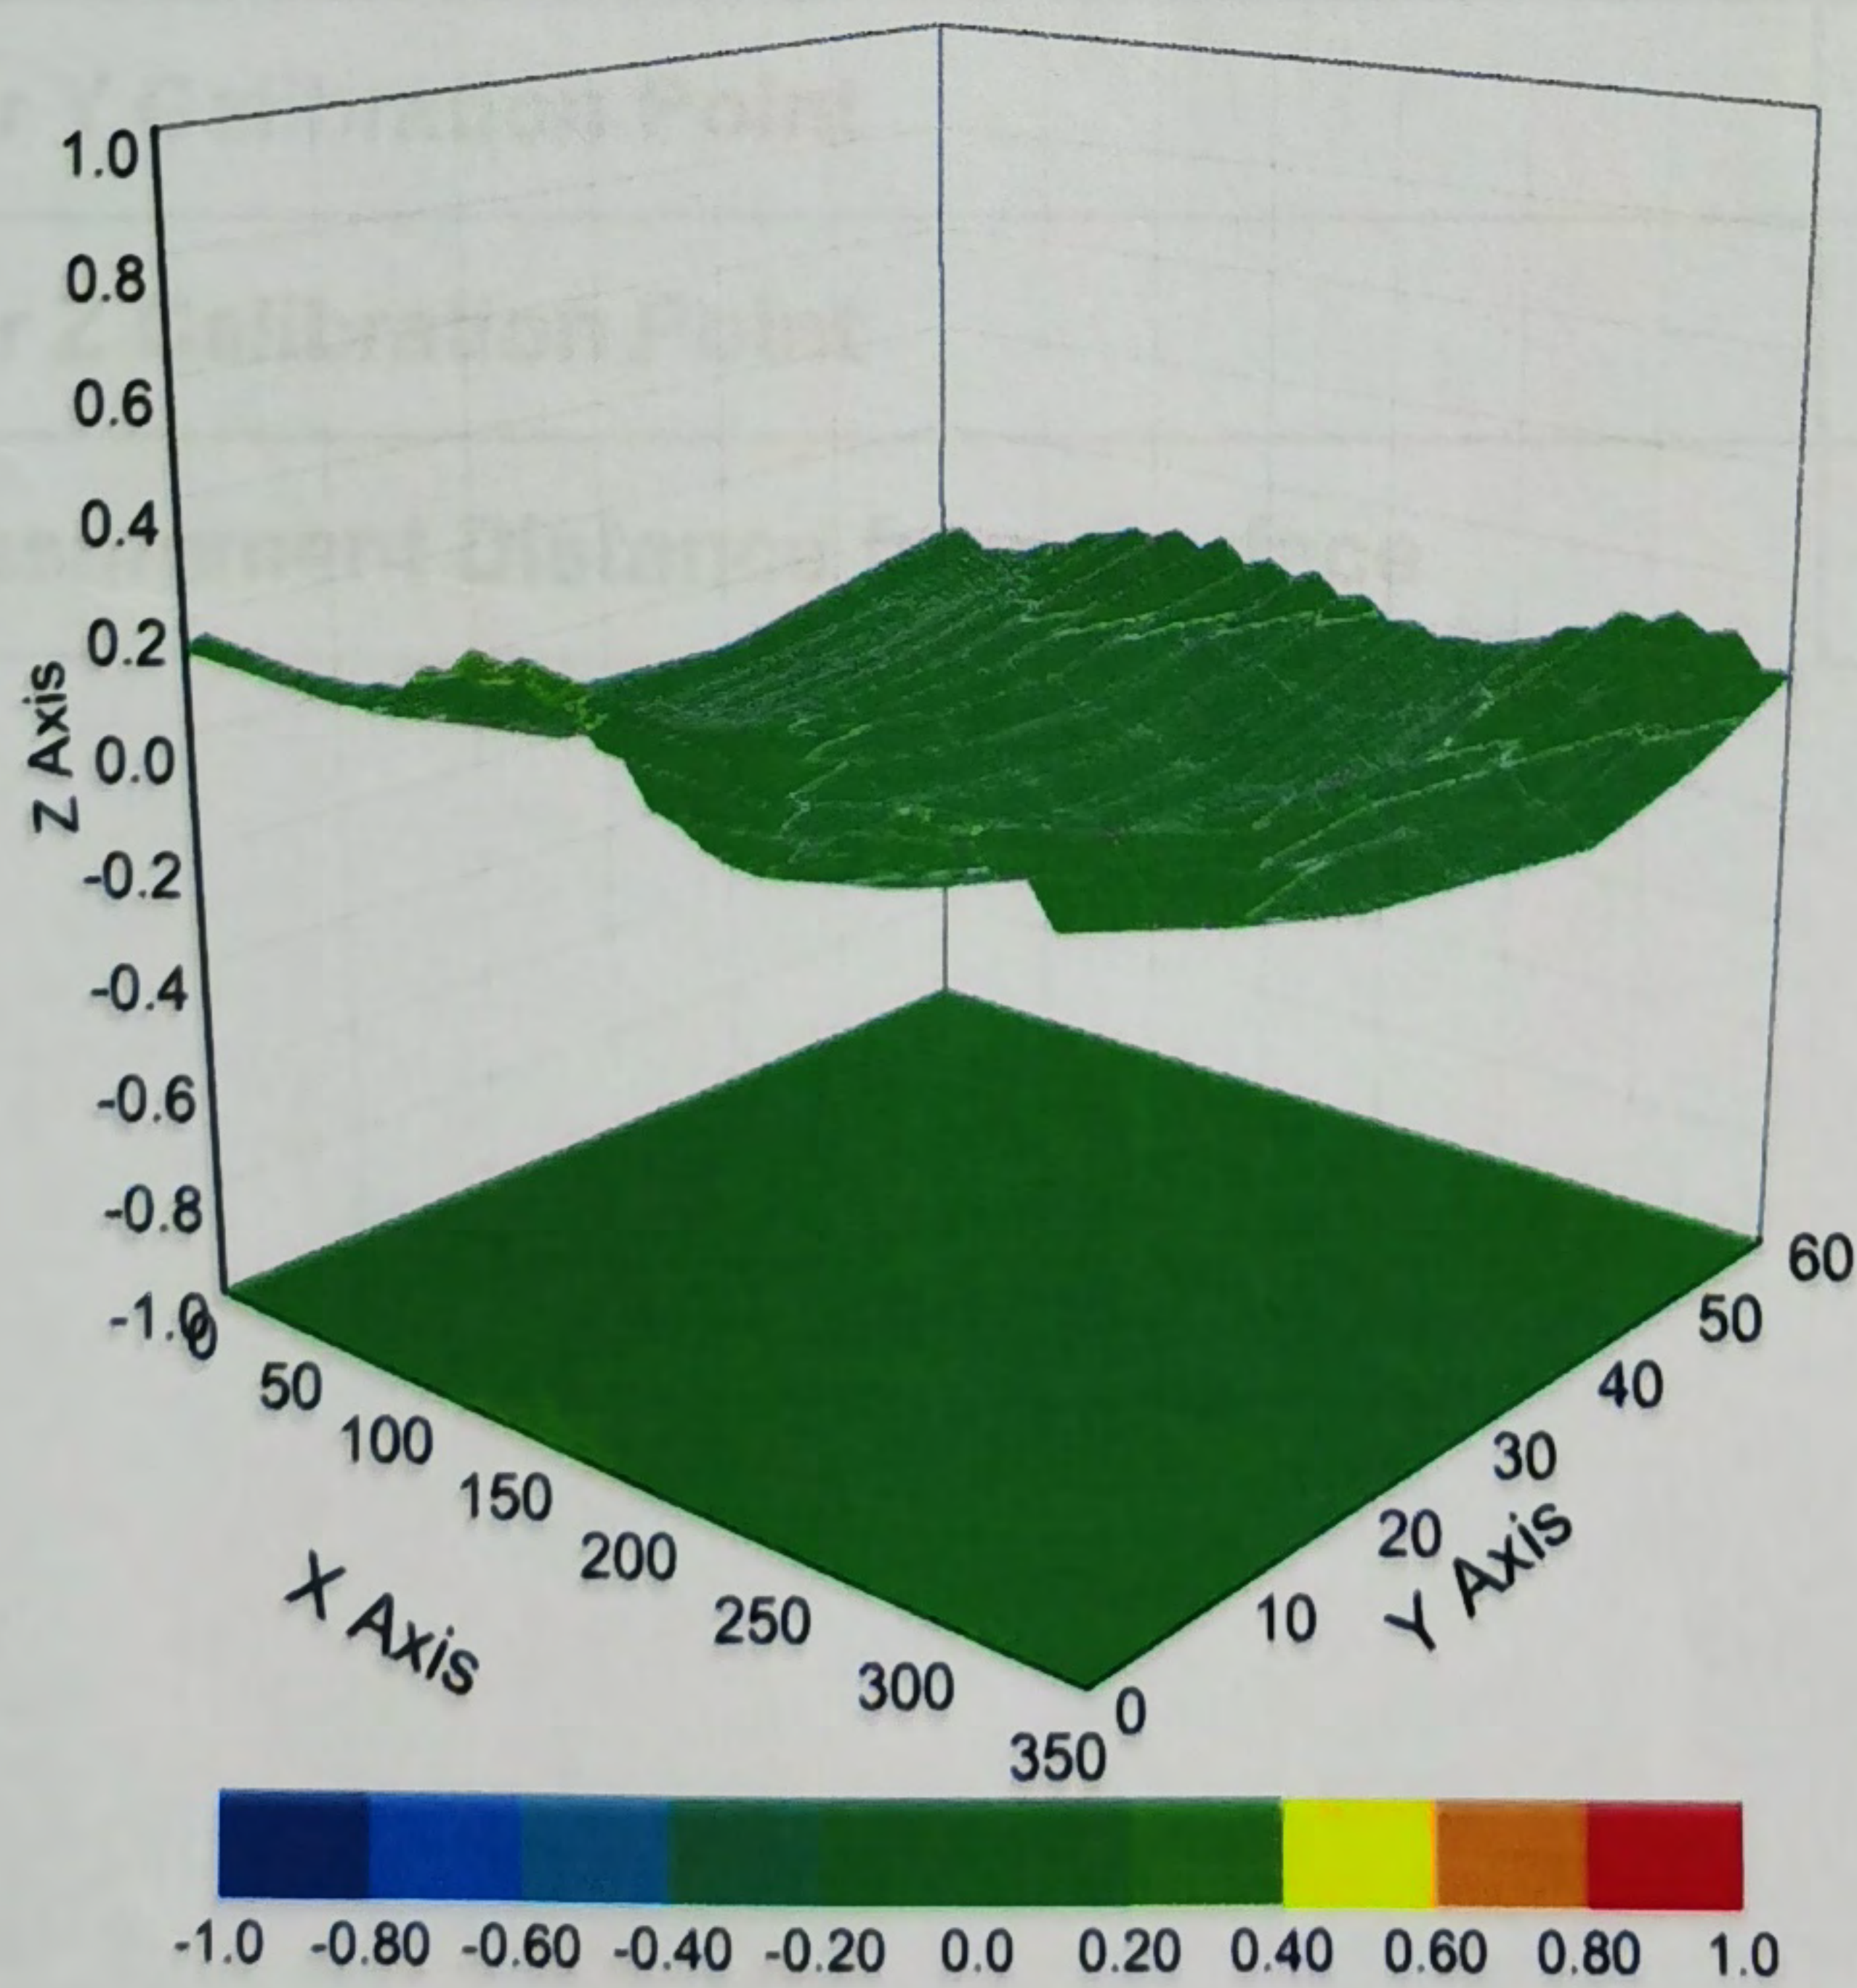

Uncertainty of Spherical Isotropy Assessment: $\pm 3.2\%$ ($k=2$)



In Collaboration with
s p e a g
CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504
E-mail: cttl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

DASY/EASY – Parameters of Probe: EX3DV4 – SN:3982

Other Probe Parameters

| | |
|-----------------------------------------------|------------|
| Sensor Arrangement | Triangular |
| Connector Angle (°) | 170.7 |
| Mechanical Surface Detection Mode | enabled |
| Optical Surface Detection Mode | disable |
| Probe Overall Length | 337mm |
| Probe Body Diameter | 10mm |
| Tip Length | 10mm |
| Tip Diameter | 2.5mm |
| Probe Tip to Sensor X Calibration Point | 1mm |
| Probe Tip to Sensor Y Calibration Point | 1mm |
| Probe Tip to Sensor Z Calibration Point | 1mm |
| Recommended Measurement Distance from Surface | 1.4mm |

| Dipole D835V2 SN 4d105 | | | | |
|------------------------|-----------------|------------|------------------------|----------------|
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2019-12-17 | -26.0 | / | 49.5 | / |
| 2020-12-16 | -27.0 | 3.85% | 51.4 | 1.9 Ω |

| Dipole D1750V2 SN 1149 | | | | |
|------------------------|-----------------|------------|------------------------|----------------|
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2019-05-21 | -31.8 | / | 47.6 | / |
| 2020-05-20 | -32.3 | 1.57% | 48.9 | 1.3 Ω |

| Dipole D1900V2 SN 5d028 | | | | |
|-------------------------|-----------------|------------|------------------------|----------------|
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2019-12-17 | -22.2 | / | 51.2 | / |
| 2020-12-16 | -23.0 | 3.60% | 53.3 | 2.1 Ω |

| Dipole D2450V2 SN 733 | | | | |
|-----------------------|-----------------|------------|------------------------|----------------|
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2019-12-17 | -27.2 | / | 52.2 | / |
| 2020-12-16 | -27.8 | 2.21% | 53.4 | 1.2 Ω |

| Dipole D2600V2 SN 1125 | | | | |
|------------------------|-----------------|------------|------------------------|----------------|
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2019-05-20 | -25.7 | / | 48.9 | / |
| 2020-05-19 | -26.6 | 3.50% | 50.8 | 1.9 Ω |

| Dipole D3700V2 SN 1046 | | | | |
|------------------------|-----------------|------------|------------------------|----------------|
| Head Liquid | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 2019-09-06 | -28.2 | / | 43.3 | / |
| 2020-09-05 | -29.1 | 3.19% | 44.7 | 1.4 Ω |

| Dipole D3900V2 SN 1026 | | | | | |
|------------------------|---------------------|-----------------|------------|------------------------|----------------|
| Head Liquid | | | | | |
| Frequency(MHz) | Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ |
| 3900 | 2019-09-03 | -23.4 | / | 46.7 | / |
| | 2020-09-02 | -24.2 | 3.42% | 47.8 | 1.1 Ω |
| 4100 | 2019-09-03 | -21.7 | / | 59.0 | / |
| | 2020-09-02 | -22.2 | 2.30% | 59.6 | 0.6 Ω |

| Dipole D5GHzV2 SN 1165 | | | | | |
|------------------------|-----------------|------------|------------------------|----------------|--|
| 5250MHz Head Liquid | | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ | |
| 2019-12-20 | -25.5 | / | 45.2 | / | |
| 2020-12-19 | -26.3 | 3.14% | 47.1 | 1.9 Ω | |
| 5600MHz Head Liquid | | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ | |
| 2019-12-20 | 26.8 | / | 52.0 | / | |
| 2020-12-19 | -27.6 | 2.99% | 53.7 | 1.7 Ω | |
| 5750MHz Head Liquid | | | | | |
| Date of Measurement | Return Loss(dB) | Δ % | Impedance (Ω) | $\Delta\Omega$ | |
| 2019-12-20 | -27.5 | / | 50.0 | / | |
| 2020-12-19 | -28.4 | 3.27% | 52.6 | 2.6 Ω | |