


# Appendix D

## Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

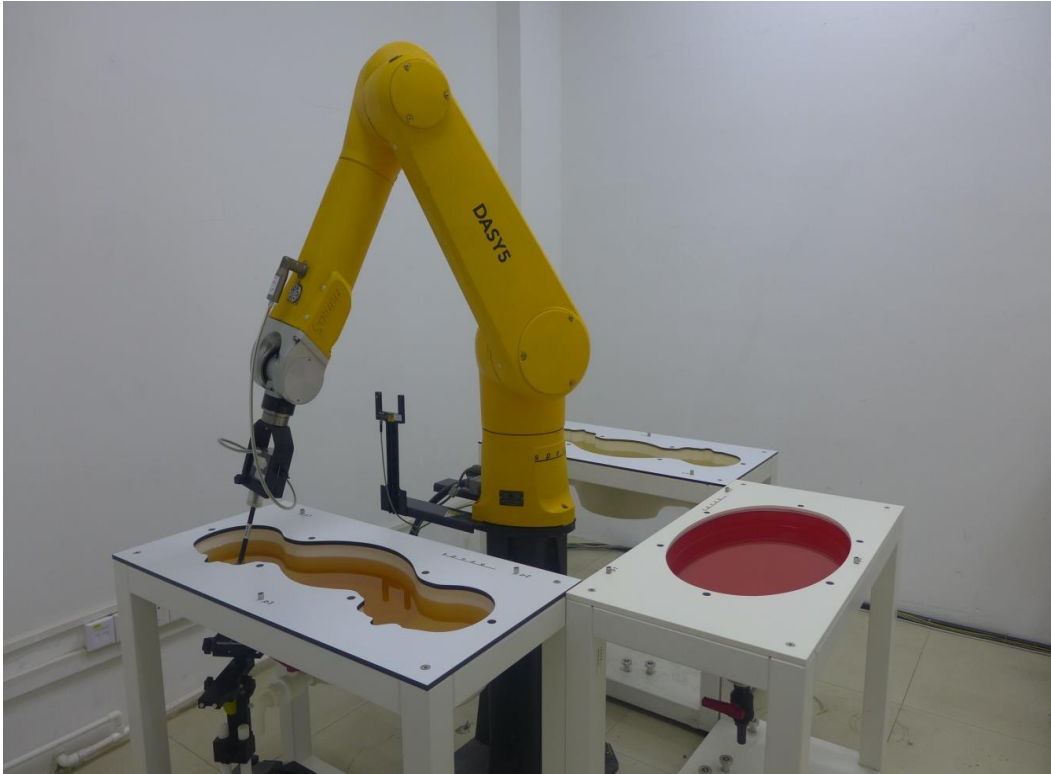


## 1. SAR measurement System







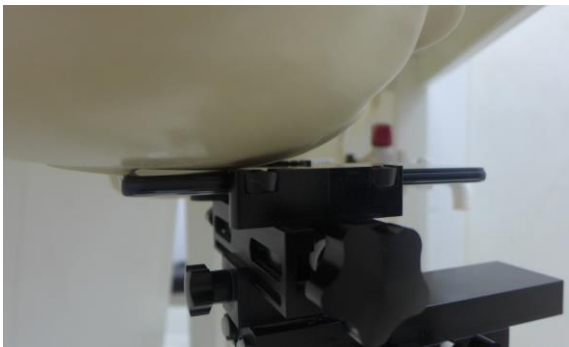



## 2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
 A photograph showing a cross-section of a container filled with a yellowish, translucent liquid. A metal ruler is placed vertically next to the container, with the 10 cm mark visible. The container has a blue outer rim and a white inner lining. The liquid level is approximately 8 cm high.	NA

### 3. Photographs of EUT test position

<p><b>Photo 2: Left cheek</b></p>	<p><b>Photo 3: Left tilted</b></p>
	
<p><b>Photo 4: Right cheek</b></p>	<p><b>Photo 5: Right tilted</b></p>
	
<p><b>Photo 6: Front side 15mm</b></p>	<p><b>Photo 7: Back side 15mm</b></p>
	

<p><b>Photo 8: Front side 10mm</b></p>	<p><b>Photo 9: Back side 10mm</b></p>
	
<p><b>Photo 10: Left side 10mm</b></p>	<p><b>Photo 11: Right side 10mm</b></p>
	
<p><b>Photo 12: Top side 10mm</b></p>	<p><b>Photo 13: Bottom side 10mm</b></p>
	

<p><b>Photo 14: Front side 0mm</b></p>	<p><b>Photo 15: Back side 0mm</b></p>
	
<p><b>Photo 16: Right side 0mm</b></p>	<p><b>Photo 17: Top side 0mm</b></p>
	
<p><b>Photo 18: Top side 5mm</b></p>	<p><b>NA</b></p>
	<p><b>NA</b></p>

## 4. EUT Constructional Details

