


Appendix D


Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details



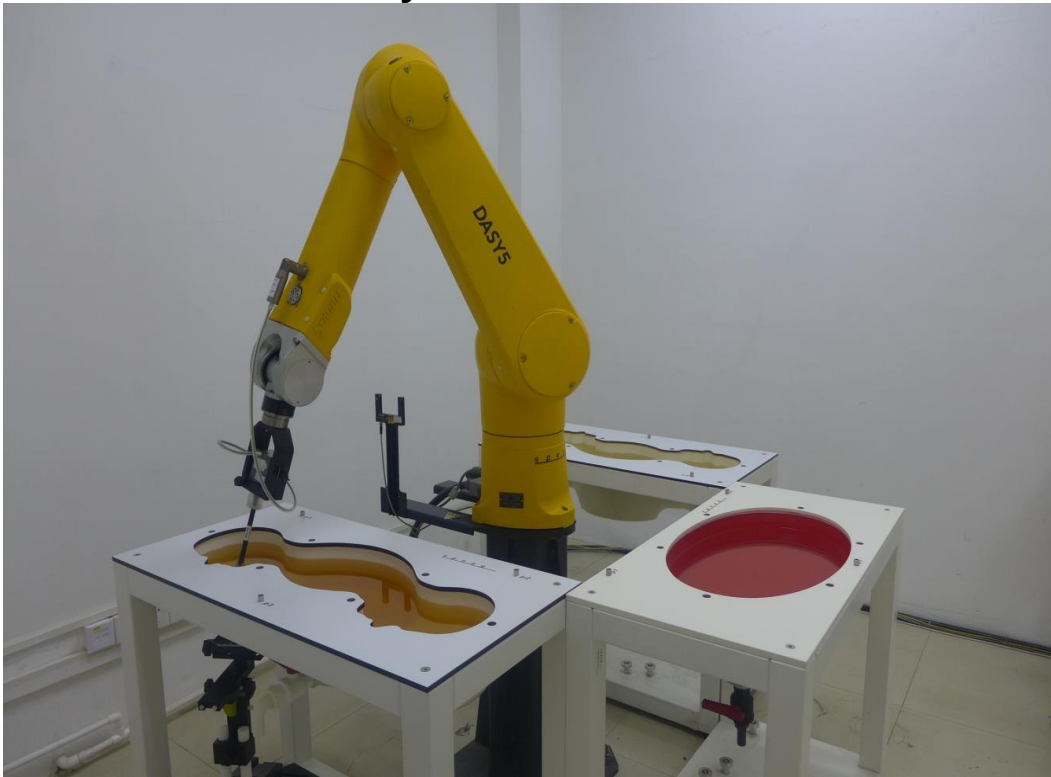

1. SAR measurement System

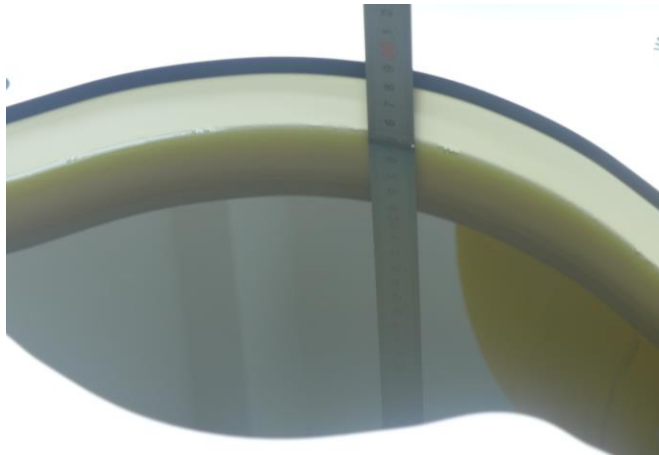



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
	NA

3. Photographs of EUT test position

<p>Photo 2: Front side 5mm</p>	<p>Photo 3: Back side 5mm</p>
	
<p>Photo 4: Left side 5mm</p>	<p>Photo 5: Right side 5mm</p>
	
<p>Photo 6: Top side 5mm</p>	<p>Photo 7: Bottom side 5mm</p>
	

4. EUT Constructional Details

Photo 8: Front View	Photo 9: Back View
 A photograph showing the front view of a white, rectangular electronic device. The device has rounded corners and a small, dark rectangular slot at the top. It is placed on a blue background. A vertical ruler is positioned to the left of the device, and a horizontal ruler is positioned below it. The vertical ruler shows the device is approximately 10 cm high. The horizontal ruler shows the device is approximately 4 cm wide.	 A photograph showing the back view of the same white, rectangular electronic device. The back view shows a small, dark rectangular slot at the top, similar to the front view. There are four small circular indentations or screws on the back surface, two on the left and two on the right. The device is placed on a blue background. A vertical ruler is positioned to the left of the device, and a horizontal ruler is positioned below it. The vertical ruler shows the device is approximately 10 cm high. The horizontal ruler shows the device is approximately 4 cm wide.