

Inspire Model 2500 ID Label/Location Info

FCC ID: 2AGO22500

Device dimensions: 4.7" x 2.7" x 1.1"


Label dimensions: 2.0" x 2.3"

Underside surface of device:



FCC ID in diagram is for info only, see page 1 for actual FCC ID


		REVISION			
REV	DESCRIPTION	ECO NUMBER	DATE	DRFT	APRV
01	INITIAL RELEASE	15-00208	7/7/2015	TY	KV
02	MATERIAL CHANGE	15-00211	7/22/2015	TY	KV
03	ARTWORK CHANGE	15-00215	8/27/2015	TY	KV
04	MULTIPLE DRAWING CHANGES	15-00215	9/4/2015	TY	KV
05	ARTWORK CHANGE, ADDED PRINTING DETAILS	15-00230	10/12/2015	TY	KV

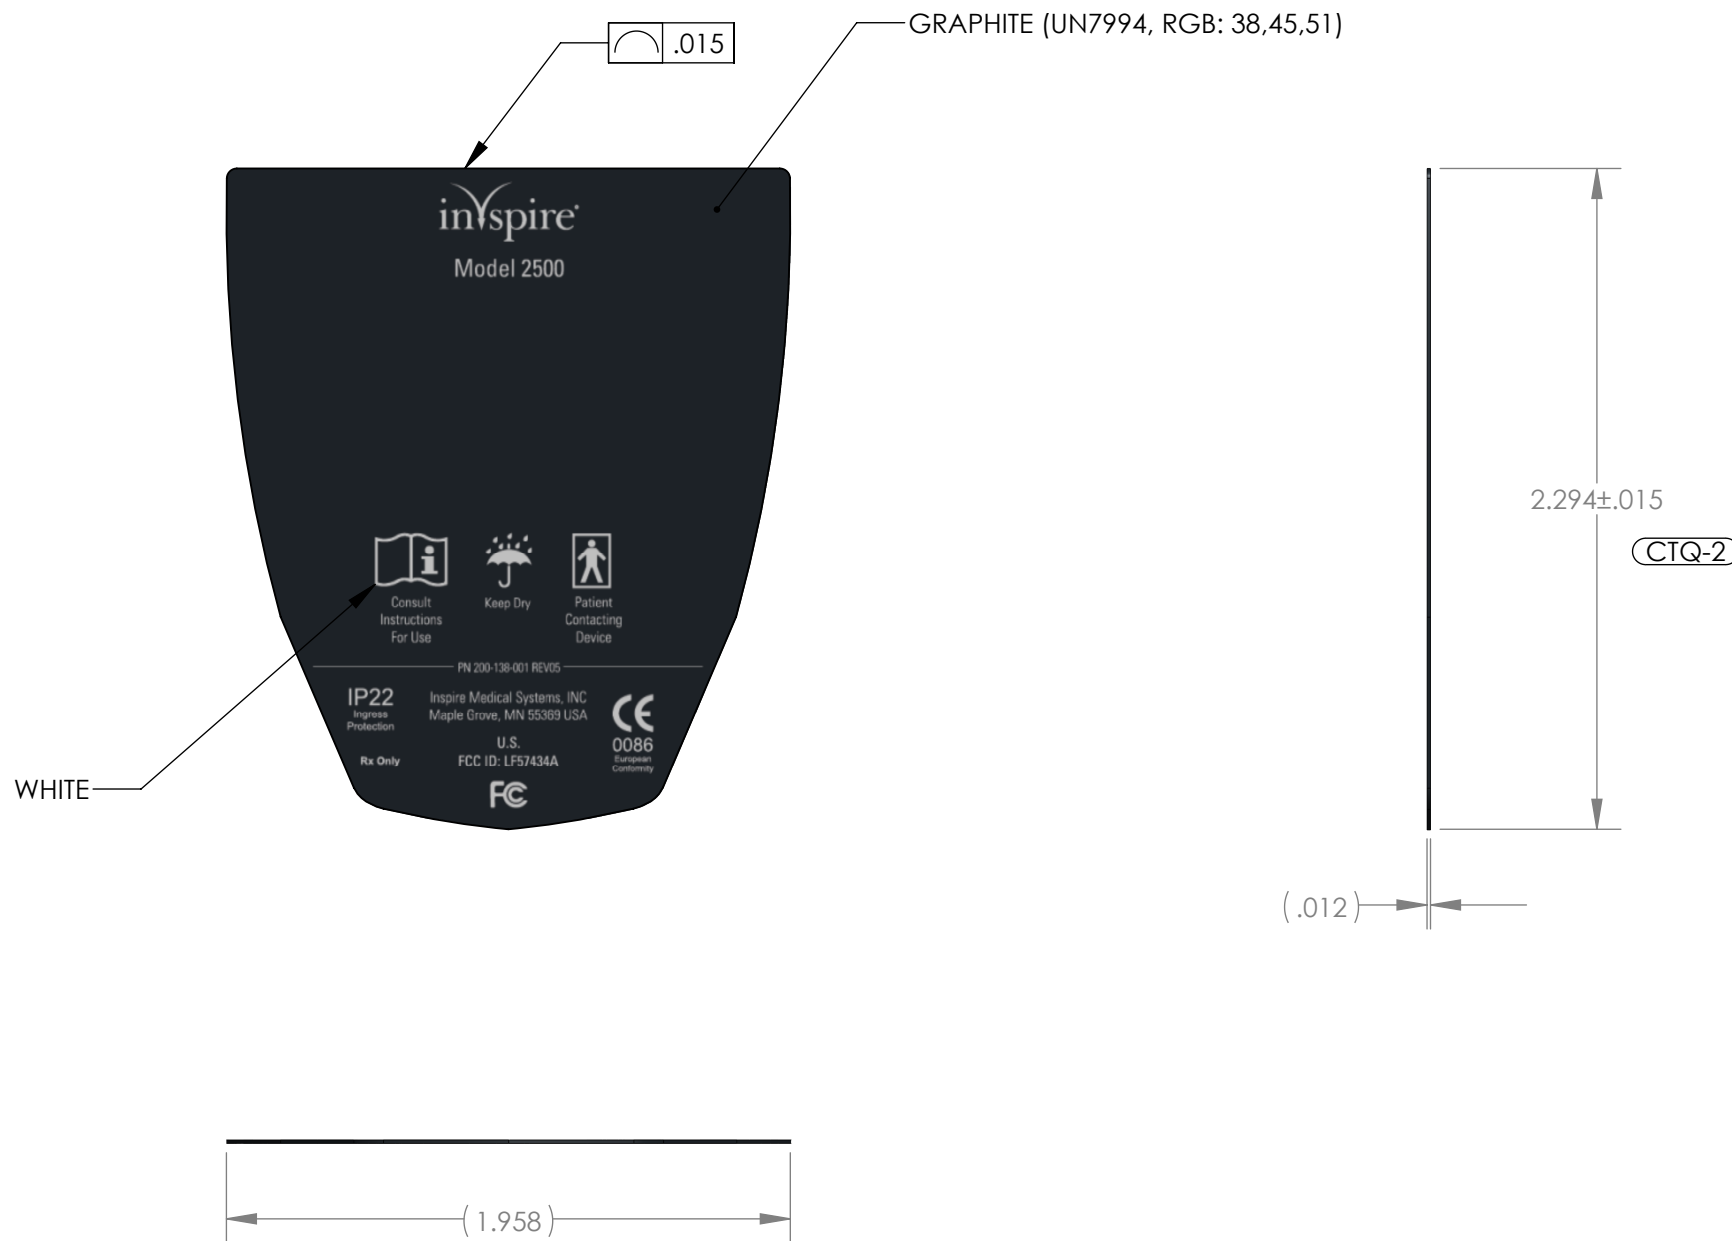

NOTES:

- (CTQ-1) 1. MATERIAL: .010 LEXAN 8B35V FILM WITH 3M 7952MP REAR ADHESIVE (.002). SCREEN PRINT GRAPHICS ON SECOND SURFACE PER THE PROVIDED ILLUSTRATOR FILE USING SERICOL TECHMARK INKS (OR EQUIVALENT). MATERIAL CERTIFICATION TO BE PROVIDED WITH EACH LOT.
- 2. UNTOLERANCED DIMENSIONS ARE REFERENCE DIMENSIONS. SEE CAD MODEL FOR COMPLETE GEOMETRY DEFINITION. CTQ ARE CRITICAL INSPECTION DIMENSIONS FOR SUPPLIER (2).
- 3. THE PARTS SHALL BE PACKAGED IN A MANNER THAT PREVENTS DAMAGE OR CONTAMINATION FROM FOREIGN MATERIAL. EACH MANUFACTURING LOT SHALL BE LABELED IN ACCORDANCE WITH INSPIRE SPEC 700-006-000.
- 4. UPON APPROVAL BY INSPIRE MEDICAL SYSTEMS OF THE INITIAL DESIGN, ANY PROCESS CHANGES, DESIGN CHANGES, PACKAGING CHANGES, RAW MATERIAL CHANGES, OR DEVIATIONS CONSIDERED BY THE MANUFACTURER MUST BE SUBMITTED TO INSPIRE IN WRITING FOR PRE-APPROVAL. THE INFORMATION SUBMITTED SHALL INCLUDE A COMPLETE DESCRIPTION OF THE CHANGE AND THE EFFECT THE CHANGE WILL HAVE ON ALL THE CHARACTERISTICS OF THE DEVICE/MATERIAL. UPON REQUEST, THE MANUFACTURER SHALL SUBMIT SAMPLES OF THE PROPOSED DEVICE/MATERIAL FOR EVALUATION AND APPROVAL BY INSPIRE MEDICAL SYSTEMS.

IMS P/N	REV	DESCRIPTION
200-138-001	05	LABEL, BATTERY DOOR, MODEL 2500

PROPERTY AND CONFIDENTIAL The information contained in this drawing is the sole property of Inspire. Any reproduction in part or as a whole without the express written permission of Inspire is strictly prohibited.	 Inspire Medical Systems, Inc. Maple Grove, MN USA	
	TITLE: LABEL, BATTERY DOOR, MODEL 2500	
X.X ± .1 X.XX ± .01 X.XXX ± .005 ANGLES ± 2.0°	DOCUMENT CREATED BY: T. YOCH	DATE: 06/10/2015
SIZE: B	DWG NO.: 200-138-000	APPROVED: K. VERZAL
		DATE: 07/07/2015
		REV. SHEET: 05 1 OF 1