



# element

## Inspire Medical Systems

Inspire Remote Model 2580

FCC 15.209:2021

Inductive Radio

Report: INSP0027.3 Rev. 1, Issue Date: May 13, 2021



NVLAP LAB CODE: 200881-0



*This report must not be used to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. Government. This Report shall not be reproduced, except in full without written approval of the laboratory.*



# CERTIFICATE OF TEST

Last Date of Test: March 18, 2021  
Inspire Medical Systems  
EUT: Inspire Remote Model 2580

## Radio Equipment Testing

### Standards

Specification	Method
FCC 15.209:2021	ANSI C63.10:2013

### Results

Method Clause	Test Description	Applied	Results	Comments
6.2	Powerline Conducted Emissions	No	N/A	Not required for a battery powered EUT.
6.4	Field Strength of Fundamental	Yes	Pass	
6.4, 6.5	Spurious Radiated Emissions	Yes	Pass	

### Deviations From Test Standards

None

### Approved By:

Eric Brandon, Department Manager

*Product compliance is the responsibility of the client; therefore, the tests and equipment modes of operation represented in this report were agreed upon by the client, prior to testing. The results of this test pertain only to the sample(s) tested. The specific description is noted in each of the individual sections of the test report supporting this certificate of test. This report reflects only those tests from the referenced standards shown in the certificate of test. It does not include inspection or verification of labels, identification, marking or user information. As indicated in the Statement of Work sent with the quotation, Element's standard process is to always use the latest published version of the test methods even when earlier versions are cited in the test specification. Issuance of a purchase order was de facto acceptance of this approach. Otherwise, the client would have advised Element in writing of the specific version of the test methods they wanted applied to the subject testing.*

# REVISION HISTORY



<b>Revision Number</b>	<b>Description</b>	<b>Date (yyyy-mm-dd)</b>	<b>Page Number</b>
01	Added note to TD, worst case orientation was determined at 3m and remeasured at 10m	2021-05-13	13
	Added details about how the radio was operating during testing	2021-05-13	13, 14, 16 and 17
	Added power table	2021-05-13	all

# ACCREDITATIONS AND AUTHORIZATIONS



---

## United States

**FCC** - Designated by the FCC as a Telecommunications Certification Body (TCB). Certification chambers, Open Area Test Sites, and conducted measurement facilities are listed with the FCC.

**A2LA** - Accredited by A2LA to ISO / IEC 17065 as a product certifier. This allows Element to certify transmitters to FCC and IC specifications.

**NVLAP** - Each laboratory is accredited by NVLAP to ISO 17025

---

## Canada

**ISED** - Recognized by Innovation, Science and Economic Development Canada as a Certification Body (CB) and as a CAB for the acceptance of test data.

---

## European Union

**European Commission** – Recognized as an EU Notified Body validated for the EMCD and RED Directives.

---

## United Kingdom

**BEIS** – Recognized by the UK as an Approved Body under the UK Radio Equipment and UK EMC Regulations.

---

## Australia/New Zealand

**ACMA** - Recognized by ACMA as a CAB for the acceptance of test data.

---

## Korea

**MSIT / RRA** - Recognized by KCC's RRA as a CAB for the acceptance of test data.

---

## Japan

**VCCI** - Associate Member of the VCCI. Conducted and radiated measurement facilities are registered.

---

## Taiwan

**BSMI** – Recognized by BSMI as a CAB for the acceptance of test data.

**NCC** - Recognized by NCC as a CAB for the acceptance of test data.

---

## Singapore

**IDA** – Recognized by IDA as a CAB for the acceptance of test data.

---

## Israel

**MOC** – Recognized by MOC as a CAB for the acceptance of test data.

---

## Hong Kong

**OFCA** – Recognized by OFCA as a CAB for the acceptance of test data.

---

## Vietnam

**MIC** – Recognized by MIC as a CAB for the acceptance of test data.

---


## SCOPE

For details on the Scopes of our Accreditations, please visit:  
<https://www.nwemc.com/emc-testing-accreditations>

# FACILITIES



<b>California</b> Labs OC01-17 41 Tesla Irvine, CA 92618 (949) 861-8918	<b>Minnesota</b> Labs MN01-11 9349 W Broadway Ave. Brooklyn Park, MN 55445 (612)-638-5136	<b>Oregon</b> Labs EV01-12 6775 NE Evergreen Pkwy #400 Hillsboro, OR 97124 (503) 844-4066	<b>Texas</b> Labs TX01-09 3801 E Plano Pkwy Plano, TX 75074 (469) 304-5255	<b>Washington</b> Labs NC01-05 19201 120 <sup>th</sup> Ave NE Bothell, WA 98011 (425)984-6600
<b>NVLAP</b>				
NVLAP Lab Code: 200676-0	NVLAP Lab Code: 200881-0	NVLAP Lab Code: 200630-0	NVLAP Lab Code:201049-0	NVLAP Lab Code: 200629-0
<b>Innovation, Science and Economic Development Canada</b>				
2834B-1, 2834B-3	2834E-1, 2834E-3	2834D-1	2834G-1	2834F-1
<b>BSMI</b>				
SL2-IN-E-1154R	SL2-IN-E-1152R	SL2-IN-E-1017	SL2-IN-E-1158R	SL2-IN-E-1153R
<b>VCCI</b>				
A-0029	A-0109	A-0108	A-0201	A-0110
<b>Recognized Phase I CAB for ISED, ACMA, BSMI, IDA, KCC/RRA, MIC, MOC, NCC, OFCA</b>				
US0158	US0175	US0017	US0191	US0157

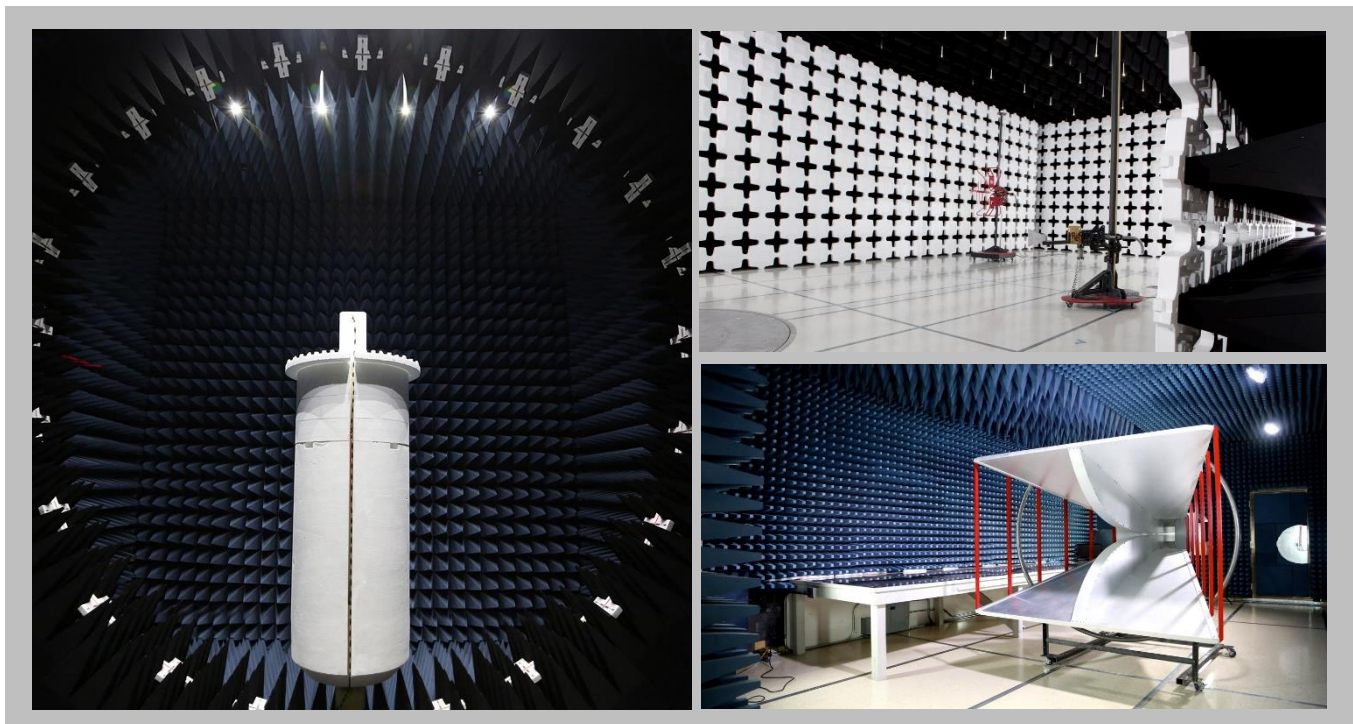

# MEASUREMENT UNCERTAINTY



## Measurement Uncertainty

When a measurement is made, the result will be different from the true or theoretically correct value. The difference is the result of tolerances in the measurement system that cannot be completely eliminated. To the extent that technology allows us, it has been our aim to minimize this error. Measurement uncertainty is a statistical expression of measurement error qualified by a probability distribution.


A measurement uncertainty estimation has been performed for each test per our internal quality document QM205.4.6. The estimation is used to compare the measured result with its "true" or theoretically correct value. The expanded measurement uncertainty (K=2) can be found in the table below. A lab specific value may also be found in the applicable test description section. Our measurement data meets or exceeds the measurement uncertainty requirements of the applicable specification; therefore, the test data can be compared directly to the specification limit to determine compliance. The calculations for estimating measurement uncertainty are based upon ETSI TR 100 028 (or CISPR 16-4-2 as applicable), and are available upon request.

The following table represents the Measurement Uncertainty (MU) budgets for each of the tests that may be contained in this report.

<b>Test</b>	<b>+ MU</b>	<b>- MU</b>
Frequency Accuracy	0.0007%	-0.0007%
Amplitude Accuracy (dB)	1.2 dB	-1.2 dB
Conducted Power (dB)	1.2 dB	-1.2 dB
Radiated Power via Substitution (dB)	0.7 dB	-0.7 dB
Temperature (degrees C)	0.7°C	-0.7°C
Humidity (% RH)	2.5% RH	-2.5% RH
Voltage (AC)	1.0%	-1.0%
Voltage (DC)	0.7%	-0.7%
Field Strength (dB)	5.2 dB	-5.2 dB
AC Powerline Conducted Emissions (dB)	2.6 dB	-2.6 dB

# Test Setup Block Diagrams


## Antenna Port Conducted Measurements

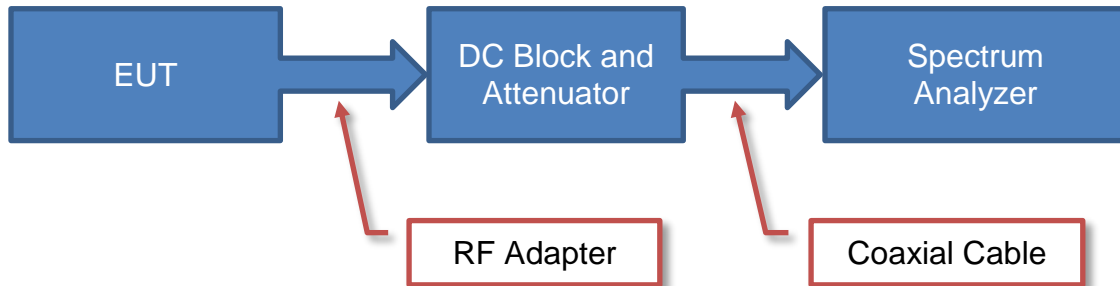

## Near Field Test Fixture Measurements




## Spurious Radiated Emissions

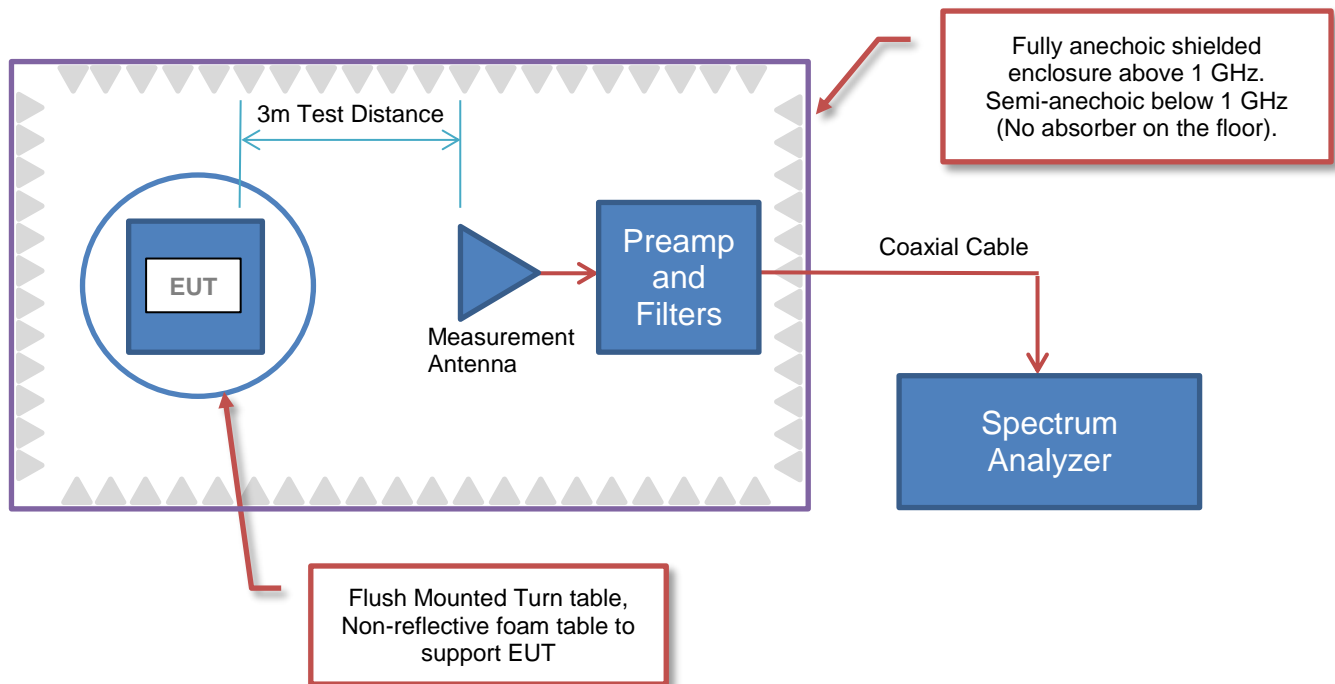

# Test Setup Block Diagrams

## Bore Siting (>1GHz)

The diameter of the illumination area is the dimension of the line tangent to the EUT formed by 3 dB beamwidth of the measurement antenna at the measurement distance. At a 3 meter test distance, the diameter of the illumination area was 3.8 meters at 1 GHz and greater than 2.1 meters up to 6 GHz. Above 1 GHz, when required by the measurement standard, the antenna is pointed for both azimuth and elevation to maintain the receive antenna within the cone of radiation from the EUT. The specified measurement detectors were used for comparison of the emissions to the peak and average specification limits.

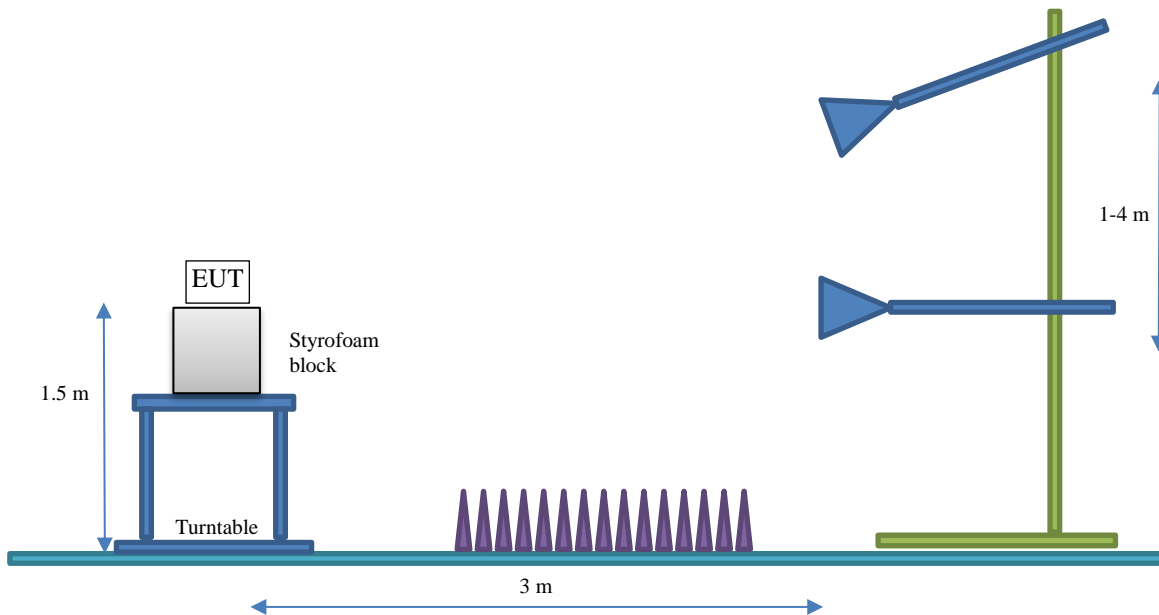





# PRODUCT DESCRIPTION

## Client and Equipment Under Test (EUT) Information

<b>Company Name:</b>	Inspire Medical Systems
<b>Address:</b>	5500 Wayzata Blvd., Suite 1600
<b>City, State, Zip:</b>	Golden Valley, MN 55416
<b>Test Requested By:</b>	Charles Steaderman
<b>EUT:</b>	Inspire Remote Model 2580
<b>First Date of Test:</b>	March 18, 2021
<b>Last Date of Test:</b>	March 18, 2021
<b>Receipt Date of Samples:</b>	March 11, 2021
<b>Equipment Design Stage:</b>	Production
<b>Equipment Condition:</b>	No Damage
<b>Purchase Authorization:</b>	Verified

## Information Provided by the Party Requesting the Test

<b>Functional Description of the EUT:</b>
Medical device programmer with BLE and inductive.
<b>Testing Objective:</b>
To demonstrate compliance of the inductive portion of the device to FCC Part 15.209 specifications.

# CONFIGURATIONS



## Configuration INSP0027- 6

<b>EUT</b>			
<b>Description</b>	<b>Manufacturer</b>	<b>Model/Part Number</b>	<b>Serial Number</b>
Inspire Remote	Inspire Medical Systems	2580	REM000098

<b>Peripherals in test setup boundary</b>			
<b>Description</b>	<b>Manufacturer</b>	<b>Model/Part Number</b>	<b>Serial Number</b>
Battery Pack	Unknown	None	None

<b>Cables</b>					
<b>Cable Type</b>	<b>Shield</b>	<b>Length (m)</b>	<b>Ferrite</b>	<b>Connection 1</b>	<b>Connection 2</b>
Battery Leads (x2)	No	0.1m	No	Inspire Remote	Battery Pack

# MODIFICATIONS



## Equipment Modifications

Item	Date	Test	Modification	Note	Disposition of EUT
1	2021-03-18	Field Strength of Fundamental	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	EUT remained at Element following the test.
2	2021-03-18	Spurious Radiated Emissions	Tested as delivered to Test Station.	No EMI suppression devices were added or modified during this test.	Scheduled testing was completed.

# POWER SETTINGS AND ANTENNAS



The power settings, antenna gain value(s) and cable loss (if applicable) used for the testing contained in this report were provided by the customer and will affect the validity of the results. Element assumes no responsibility for the accuracy of this information.

## ANTENNA GAIN (dBi)

Type	Provided by:	Frequency Range (kHz)	Gain (dBi)
34 loop, 1.92" x 1.80" coil	Inspire Medical Systems	175	Unknown

No adjustable power settings were provided. The EUT was tested using power settings pre-defined by the manufacturer.

# FIELD STRENGTH OF FUNDAMENTAL



PSA-ESCI 2021.01.22.0

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data. The test data represents the configuration / operating mode/ model that produced the highest emission levels as compared to the specification limit.

## MODES OF OPERATION

Inductive radio: Transmitting 175 kHz with 100% duty cycle

## POWER SETTINGS INVESTIGATED

Battery

## CONFIGURATIONS INVESTIGATED

INSP0027 - 6

## FREQUENCY RANGE INVESTIGATED

Start Frequency 9 kHz Stop Frequency 490 kHz

## SAMPLE CALCULATIONS

Radiated Emissions: Field Strength = Measured Level + Antenna Factor + Cable Factor - Amplifier Gain + Distance Adjustment Factor + External Attenuation

## TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Cal. Due
Analyzer - Spectrum Analyzer	Keysight	N9010A	AFM	2020-04-14	2021-04-14
Cable	ESM Cable Corp.	Antenna Loop Cable	MNE	2021-02-17	2022-02-17
Antenna - Loop	ETS Lindgren	6502	AOB	2019-05-21	2021-05-21

## MEASUREMENT BANDWIDTHS

Frequency Range (MHz)	Peak Data (kHz)	Quasi-Peak Data (kHz)	Average Data (kHz)
0.01 - 0.15	1.0	0.2	0.2
0.15 - 30.0	10.0	9.0	9.0
30.0 - 1000	100.0	120.0	120.0
Above 1000	1000.0	N/A	1000.0

## TEST DESCRIPTION

The antennas to be used with the EUT were tested. The EUT was continuously transmitting while set to the channel specified.

The fundamental carrier of the EUT was maximized by rotating the EUT on a turntable, adjusting the position of the EUT and EUT antenna in three orthogonal axis, and adjusting the measurement antenna polarization (per ANSI C63.10). A calibrated active loop antenna was used for this test in order to provide sufficient measurement sensitivity. The reference point of the loop antenna was maintained at 1m above the ground plane during the testing.

Measurements were made with the required detectors and annotated on the data for each individual point using the following annotation:

QP = Quasi-Peak Detector  
PK = Peak Detector  
AV = RMS Detector

As outlined in 15.209(e), 15.31(f)(2), and RSS-GEN, 6.5, measurements may be performed at a distance closer than what is specified with the limit. The limit at the specified distance is shown on the data sheet. Measurements are made at a closer distance and the data is adjusted using a distance correction factor of 40dB/decade for comparison to the limit. Worst case orientation was determined at 3 m and remeasured at 10 m.


# FIELD STRENGTH OF FUNDAMENTAL



Work Order:	INSP0027	Date:	2021-03-18	<i>Chris Patterson</i>
Project:	None	Temperature:	23 °C	
Job Site:	MN04	Humidity:	26.6% RH	
Serial Number:	REM000098	Barometric Pres.:	1028 mbar	
EUT:	Inspire Remote Model 2580			
Configuration:	6			
Customer:	Inspire Medical Systems			
Attendees:	Tom Haider			
EUT Power:	Battery			
Operating Mode:	Inductive radio: Transmitting 175 kHz with 100% duty cycle			
Deviations:	None			
Comments:	None			

Test Specifications	Test Method
FCC 15.209:2021	ANSI C63.10:2013

Run #	3	Test Distance (m)	3	Antenna Height(s)	1(m)	Results	Pass
-------	---	-------------------	---	-------------------	------	---------	------

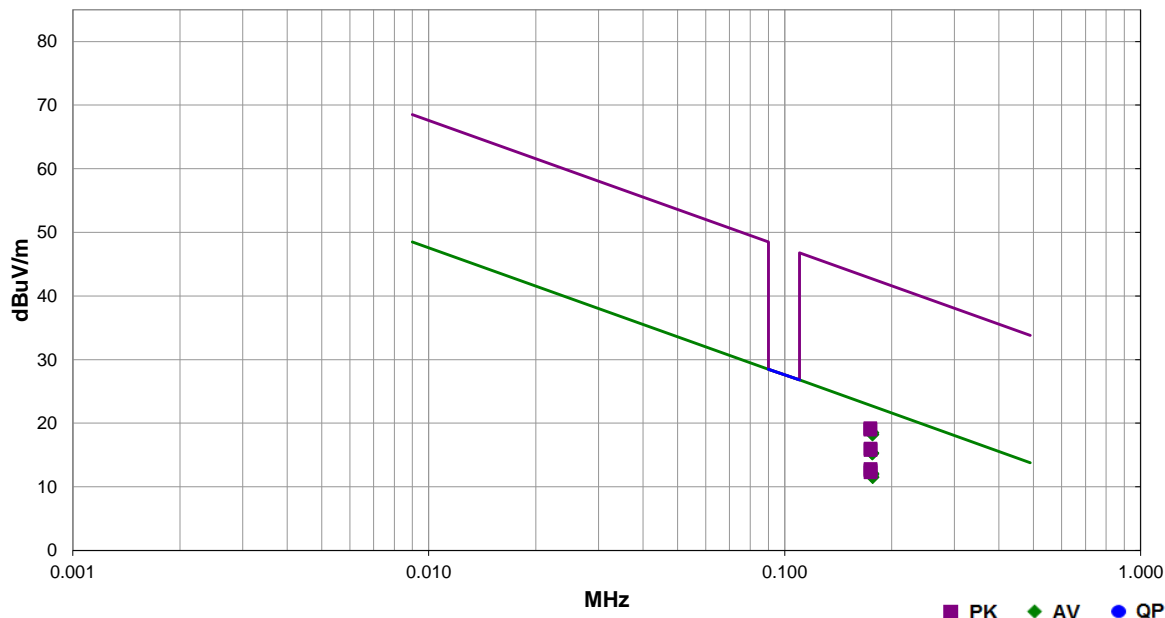

Freq (MHz)	Amplitude (dBuV)	Factor (dB)	Antenna Height (meters)	Azimuth (degrees)	Test Distance (meters)	External Attenuation (dB)	Polarity/Transducer Type	Detector	Distance Adjustment (dB)	Adjusted (dBuV/m)	Spec. Limit (dBuV/m)	Compared to Spec. (dB)	Comments
0.177	87.0	11.5	1.0	277.0	3.0	0.0	Para to EUT	AV	-80.0	18.5	22.7	-4.2	EUT Vert
0.177	86.7	11.5	1.0	274.0	3.0	0.0	Para to EUT	AV	-80.0	18.2	22.7	-4.5	EUT On Side
0.177	83.8	11.5	1.0	189.0	3.0	0.0	Perp to EUT	AV	-80.0	15.3	22.7	-7.4	EUT On Side
0.176	83.7	11.5	1.0	191.0	3.0	0.0	Perp to EUT	AV	-80.0	15.2	22.7	-7.5	EUT Vert
0.177	80.6	11.5	1.0	97.0	3.0	0.0	Para to GND	AV	-80.0	12.1	22.7	-10.6	EUT Horz
0.177	80.4	11.5	1.0	276.0	3.0	0.0	Para to GND	AV	-80.0	11.9	22.7	-10.8	EUT Vert
0.177	80.0	11.5	1.0	261.0	3.0	0.0	Para to GND	AV	-80.0	11.5	22.7	-11.2	EUT On Side
0.174	87.7	11.5	1.0	277.0	3.0	0.0	Para to EUT	PK	-80.0	19.2	42.8	-23.6	EUT Vert
0.174	87.5	11.5	1.0	274.0	3.0	0.0	Para to EUT	PK	-80.0	19.0	42.8	-23.8	EUT On Side
0.174	84.5	11.5	1.0	189.0	3.0	0.0	Perp to EUT	PK	-80.0	16.0	42.8	-26.8	EUT On Side
0.174	84.3	11.5	1.0	191.0	3.0	0.0	Perp to EUT	PK	-80.0	15.8	42.8	-27.0	EUT Vert
0.174	81.3	11.5	1.0	97.0	3.0	0.0	Para to GND	PK	-80.0	12.8	42.8	-30.0	EUT Horz
0.174	81.1	11.5	1.0	276.0	3.0	0.0	Para to GND	PK	-80.0	12.6	42.8	-30.2	EUT Vert
0.174	80.8	11.5	1.0	261.0	3.0	0.0	Para to GND	PK	-80.0	12.3	42.8	-30.5	EUT On Side
0.177	57.9	11.5	1.0	196.0	3.0	0.0	Para to EUT	AV	-80.0	-10.6	22.7	-33.3	EUT Horz
0.177	50.6	11.5	1.0	159.0	3.0	0.0	Perp to EUT	AV	-80.0	-17.9	22.7	-40.6	EUT Horz
0.176	59.7	11.5	1.0	196.0	3.0	0.0	Para to EUT	PK	-80.0	-8.8	42.7	-51.5	EUT Horz
0.176	53.8	11.5	1.0	159.0	3.0	0.0	Perp to EUT	PK	-80.0	-14.7	42.7	-57.4	EUT Horz

# FIELD STRENGTH OF FUNDAMENTAL




EmiR5 2021.01.08.0 PSA-ESCI 2021.01.22.0

<b>Work Order:</b>	INSP0027	<b>Date:</b>	2021-03-18	
<b>Project:</b>	None	<b>Temperature:</b>	24 °C	
<b>Job Site:</b>	MN04	<b>Humidity:</b>	26% RH	
<b>Serial Number:</b>	REM000098	<b>Barometric Pres.:</b>	1029 mbar	
<b>Tested by:</b>	Chris Patterson			
<b>EUT:</b>	Inspire Remote Model 2580			
<b>Configuration:</b>	6			
<b>Customer:</b>	Inspire Medical Systems			
<b>Attendees:</b>	Tom Haider			
<b>EUT Power:</b>	Battery			
<b>Operating Mode:</b>	Inductive radio: Transmitting 175 kHz with 100% duty cycle			
<b>Deviations:</b>	None			
<b>Comments:</b>	Worst case was determined at 3 m and remeasured at 10 m.			

Test Specifications	Test Method
FCC 15.209:2021	ANSI C63.10:2013

Run #	4	Test Distance (m)	10	Antenna Height(s)	1(m)	Results	Pass
-------	---	-------------------	----	-------------------	------	---------	------

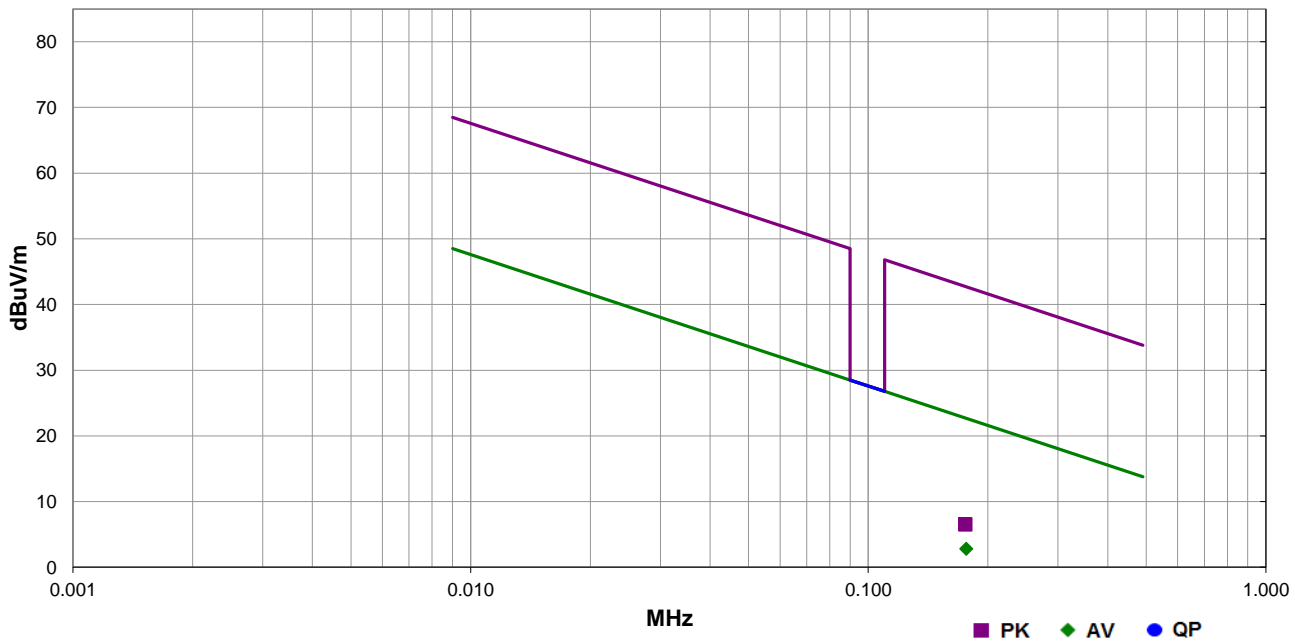

Freq (MHz)	Amplitude (dBuV)	Factor (dB)	Antenna Height (meters)	Azimuth (degrees)	Test Distance (meters)	External Attenuation (dB)	Polarity/Transducer Type	Detector	Distance Adjustment (dB)	Adjusted (dBuV/m)	Spec. Limit (dBuV/m)	Compared to Spec. (dB)	Comments
0.177	50.4	11.5	1.0	102.0	10.0	0.0	Para to EUT	AV	-59.1	2.8	22.7	-19.9	EUT Vert
0.176	54.1	11.5	1.0	102.0	10.0	0.0	Para to EUT	PK	-59.1	6.5	42.7	-36.2	EUT Vert

# SPURIOUS RADIATED EMISSIONS



PSA-ESCI 2021.01.22.0

Testing was performed using the mode(s) of operation and configuration(s) noted within the report. The individuals and/or the organization requesting the test provided the modes, configurations and settings used to complete the evaluation. The actual test parameters are specified in the test data, this includes items such as investigated frequency range (scanned) and test levels. The testing methods and performance specifications, as well as the test site used for the evaluation are indicated in the test data. The test data represents the configuration / operating mode/ model that produced the highest emission levels as compared to the specification limit.

## MODES OF OPERATION

Inductive radio: Transmitting 175 kHz with 100% duty cycle

## POWER SETTINGS INVESTIGATED

Battery

## CONFIGURATIONS INVESTIGATED

INSP0027 - 6

## FREQUENCY RANGE INVESTIGATED

Start Frequency	9 kHz	Stop Frequency	30 MHz
-----------------	-------	----------------	--------

## SAMPLE CALCULATIONS

Radiated Emissions: Field Strength = Measured Level + Antenna Factor + Cable Factor - Amplifier Gain + Distance Adjustment Factor + External Attenuation

## TEST EQUIPMENT

Description	Manufacturer	Model	ID	Last Cal.	Cal. Due
Analyzer - Spectrum Analyzer	Keysight	N9010A	AFM	2020-04-14	2021-04-14
Cable	ESM Cable Corp.	Antenna Loop Cable	MNE	2021-02-17	2022-02-17
Antenna - Loop	ETS Lindgren	6502	AOB	2019-05-21	2021-05-21

## MEASUREMENT BANDWIDTHS

Frequency Range (MHz)	Peak Data (kHz)	Quasi-Peak Data (kHz)	Average Data (kHz)
0.01 - 0.15	1.0	0.2	0.2
0.15 - 30.0	10.0	9.0	9.0
30.0 - 1000	100.0	120.0	120.0
Above 1000	1000.0	N/A	1000.0

## TEST DESCRIPTION

The antennas to be used with the EUT were tested. The EUT was continuously transmitting while set to the channel specified.

For each configuration, the spectrum was scanned throughout the specified range as part of the exploratory investigation of the emissions. These "pre-scans" are not included in the report. Final measurements on individual emissions were then made and included in this test report.

The individual emissions from the EUT were maximized by rotating the EUT on a turntable, adjusting the position of the EUT and EUT antenna in three orthogonal axis, and adjusting the measurement antenna height (where applicable) and polarization (per ANSI C63.10). A calibrated active loop antenna was used for this test in order to provide sufficient measurement sensitivity. The reference point of the loop antenna was maintained at 1m above the ground plane during the testing.

Measurements were made with the required detectors and annotated on the data for each individual point using the following annotation:

QP = Quasi-Peak Detector  
 PK = Peak Detector  
 AV = RMS Detector

If there are no detectable emissions above the noise floor, the data included may show noise floor measurements for reference only.

As outlined in 15.209(e), 15.31(f)(2), and RSS-GEN, 6.5, measurements may be performed at a distance closer than what is specified with the limit. The limit at the specified distance is shown on the data sheet. Measurements are made at a closer distance and the data is adjusted using a distance correction factor of 40dB/decade for comparison to the limit.



# SPURIOUS RADIATED EMISSIONS




EmiR5 2021.01.08.0      PSA-ESCI 2021.01.22.0

<b>Work Order:</b>	INSP0027	<b>Date:</b>	2021-03-18	
<b>Project:</b>	None	<b>Temperature:</b>	24 °C	
<b>Job Site:</b>	MN04	<b>Humidity:</b>	26% RH	
<b>Serial Number:</b>	REM000098	<b>Barometric Pres.:</b>	1029 mbar	<b>Tested by:</b> Chris Patterson
<b>EUT:</b>	Inspire Remote Model 2580			
<b>Configuration:</b>	6			
<b>Customer:</b>	Inspire Medical Systems			
<b>Attendees:</b>	Tom Haider			
<b>EUT Power:</b>	Battery			
<b>Operating Mode:</b>	Inductive radio: Transmitting 175 kHz with 100% duty cycle			
<b>Deviations:</b>	None			
<b>Comments:</b>	Worst case antenna position and EUT orientation used from Field Strength of Fundamental testing.			

<b>Test Specifications</b>	<b>Test Method</b>
FCC 15.209:2021	ANSI C63.10:2013

<b>Run #</b>	8	<b>Test Distance (m)</b>	10	<b>Antenna Height(s)</b>	1(m)	<b>Results</b>	Pass
--------------	---	--------------------------	----	--------------------------	------	----------------	------

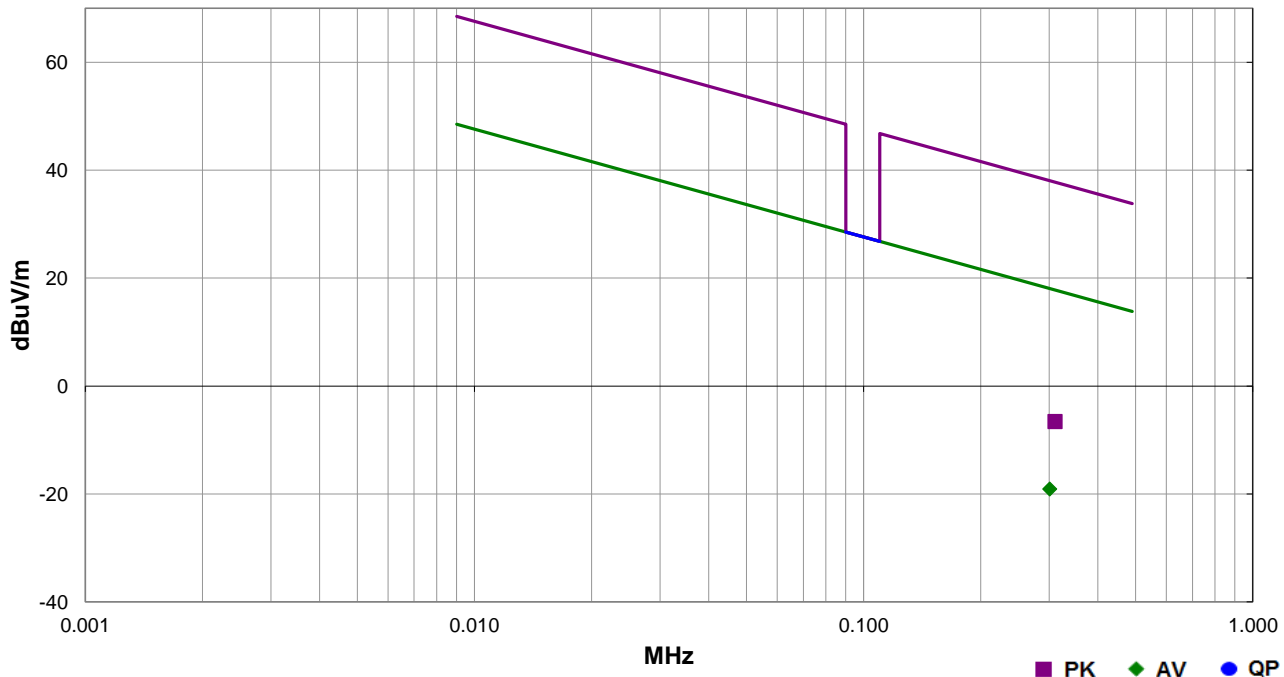

Freq (MHz)	Amplitude (dBuV)	Factor (dB)	Antenna Height (meters)	Azimuth (degrees)	Test Distance (meters)	External Attenuation (dB)	Polarity/ Transducer Type	Detector	Distance Adjustment (dB)	Adjusted (dBuV/m)	Spec. Limit (dBuV/m)	Compared to Spec. (dB)	Comments
0.301	28.5	11.5	1.0	302.0	10.0	0.0	Para to EUT	AV	-59.1	-19.1	18.0	-37.1	EUT Vert
0.310	41.0	11.5	1.0	302.0	10.0	0.0	Para to EUT	PK	-59.1	-6.6	37.8	-44.4	EUT Vert




# SPURIOUS RADIATED EMISSIONS

EmiR5 2021.01.08.0      PSA-ESCI 2021.01.22.0

<b>Work Order:</b>	INSP0027	<b>Date:</b>	2021-03-18	
<b>Project:</b>	None	<b>Temperature:</b>	24 °C	
<b>Job Site:</b>	MN04	<b>Humidity:</b>	26% RH	
<b>Serial Number:</b>	REM000098	<b>Barometric Pres.:</b>	1029 mbar	<b>Tested by:</b> Chris Patterson
<b>EUT:</b>	Inspire Remote Model 2580			
<b>Configuration:</b>	6			
<b>Customer:</b>	Inspire Medical Systems			
<b>Attendees:</b>	Tom Haider			
<b>EUT Power:</b>	Battery			
<b>Operating Mode:</b>	Inductive radio: Transmitting 175 kHz with 100% duty cycle			
<b>Deviations:</b>	None			
<b>Comments:</b>	Worst case antenna position and EUT orientation used from Field Strength of Fundamental testing.			

<b>Test Specifications</b>	<b>Test Method</b>
FCC 15.209:2021	ANSI C63.10:2013

<b>Run #</b>	9	<b>Test Distance (m)</b>	10	<b>Antenna Height(s)</b>	1(m)	<b>Results</b>	Pass
--------------	---	--------------------------	----	--------------------------	------	----------------	------

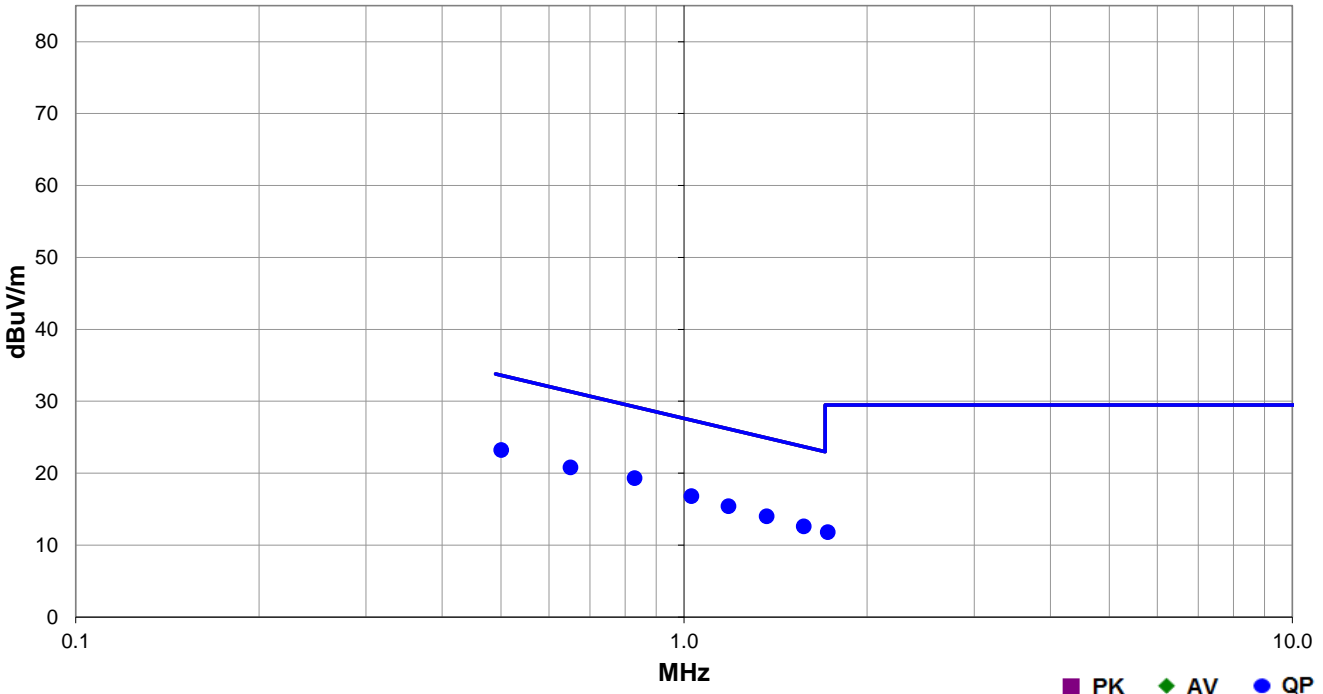

Freq (MHz)	Amplitude (dBuV)	Factor (dB)	Antenna Height (meters)	Azimuth (degrees)	Test Distance (meters)	External Attenuation (dB)	Polarity/Transducer Type	Detector	Distance Adjustment (dB)	Adjusted (dBuV/m)	Spec. Limit (dBuV/m)	Compared to Spec. (dB)
0.829	26.6	11.8	1.0	126.0	10.0	0.0	Para to EUT	QP	-19.1	19.3	29.2	-9.9
0.501	30.6	11.7	1.0	196.0	10.0	0.0	Para to EUT	QP	-19.1	23.2	33.6	-10.4
0.651	28.2	11.7	1.0	32.0	10.0	0.0	Para to EUT	QP	-19.1	20.8	31.3	-10.5
1.028	23.7	12.2	1.0	330.0	10.0	0.0	Para to EUT	QP	-19.1	16.8	27.4	-10.6
1.183	22.3	12.2	1.0	113.0	10.0	0.0	Para to EUT	QP	-19.1	15.4	26.2	-10.8
1.367	20.9	12.2	1.0	7.0	10.0	0.0	Para to EUT	QP	-19.1	14.0	24.9	-10.9
1.573	19.5	12.2	1.0	15.0	10.0	0.0	Para to EUT	QP	-19.1	12.6	23.7	-11.1
1.723	18.7	12.2	1.0	187.0	10.0	0.0	Para to EUT	QP	-19.1	11.8	29.5	-17.7