


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

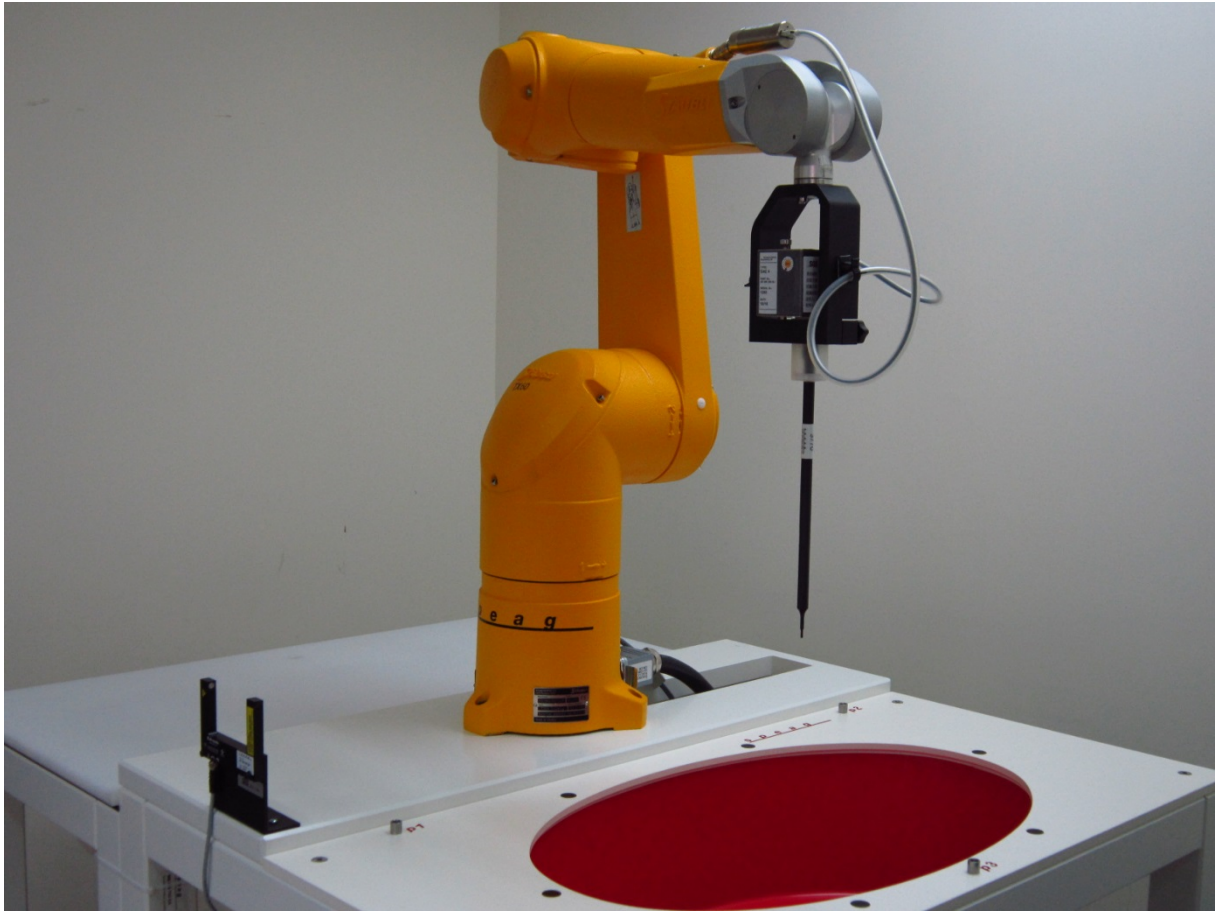

2. Photographs of Tissue Simulate Liquid

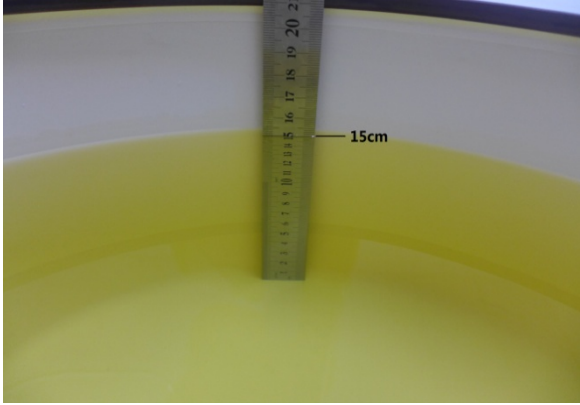
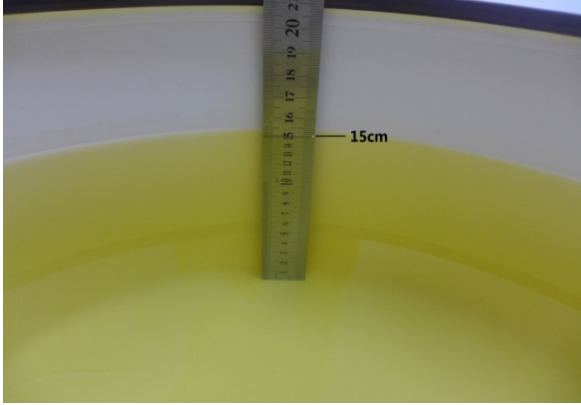
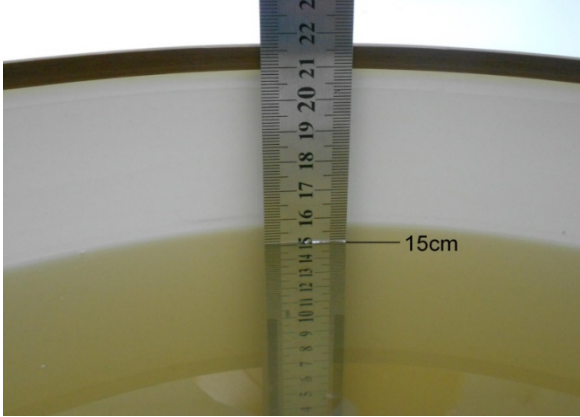
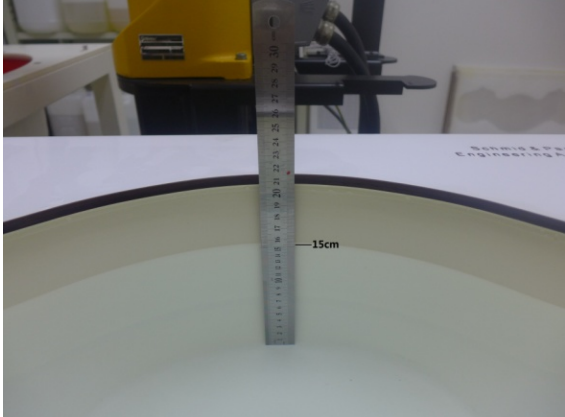
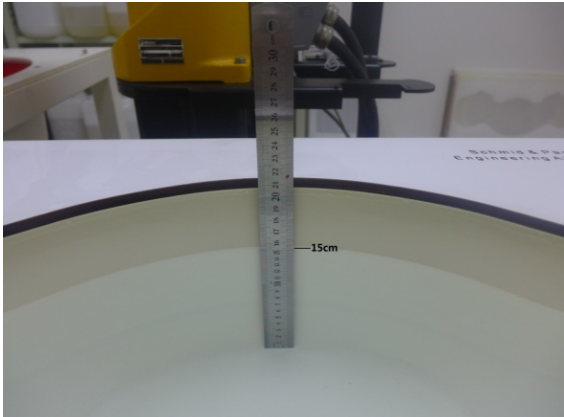
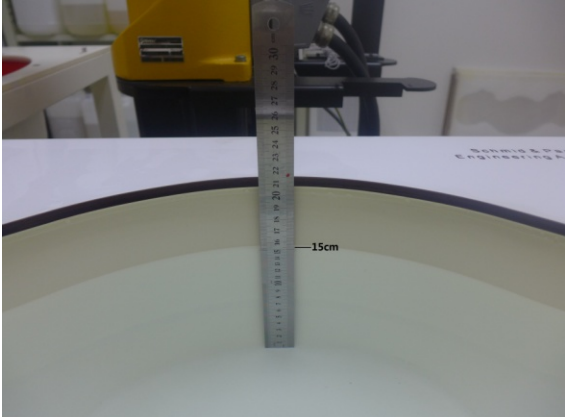
<p>Photo 1: Tissue Simulant Liquid for Head 750</p>	<p>Photo 2: Tissue Simulant Liquid for Head 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 900</p>	<p>Photo 4: Tissue Simulant Liquid for Head 1800</p>
	
<p>Photo 5: Tissue Simulant Liquid for Head 2000</p>	<p>Photo 6: Tissue Simulant Liquid for Head 2300</p>
	

Photo 7: Tissue Simulant Liquid for Head 2450

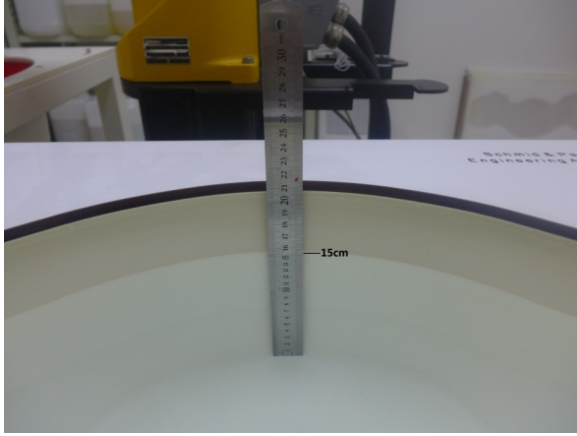


Photo 8: Tissue Simulant Liquid for Head 2600


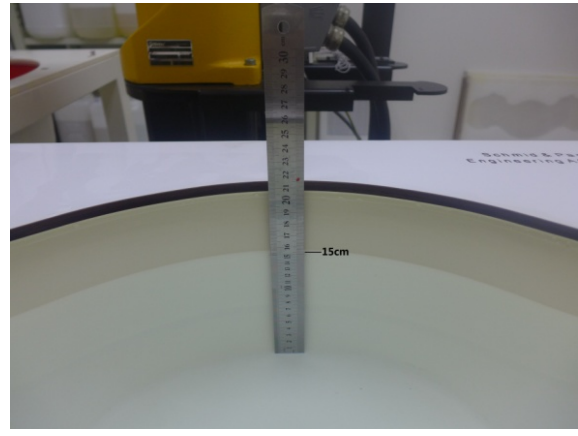



Photo 9: Tissue Simulant Liquid for Head 5GHz

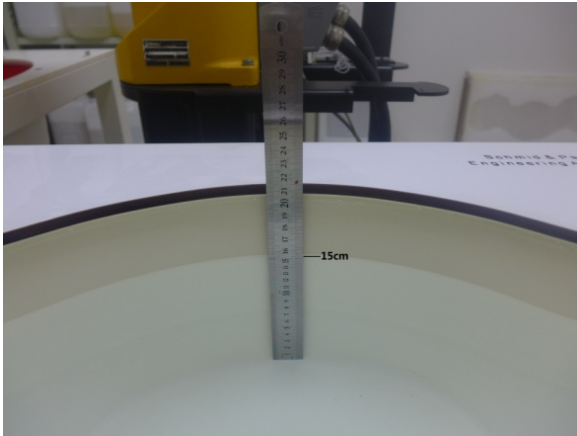

3. Photographs of EUT test position

<p>Photo 10: Front side 0mm</p>	<p>Photo 11: Back side 0mm</p>
	
<p>Photo 12: Left side 0mm</p>	<p>Photo 13: Right side 0mm</p>
	
<p>Photo 14: Top side 0mm</p>	<p>Photo 15: Bottom side 0mm</p>
	

Photo 16: Handheld Back 0mm

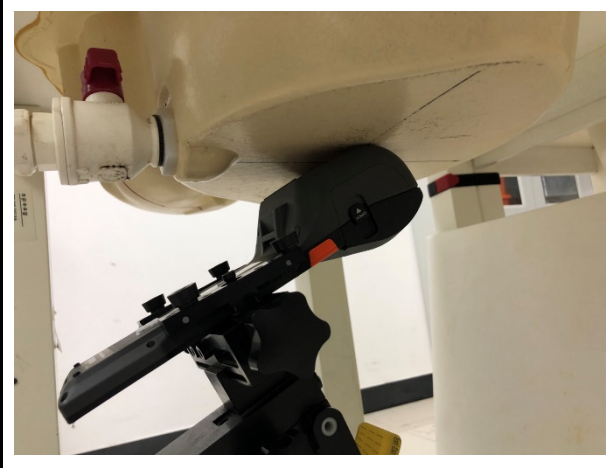

4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.