

UBTECH ROBOTICS CORP

TEST REPORT

SCOPE OF WORK FCC TESTING- IPSWSTS

REPORT NUMBER SZHH01201042-006


ISSUE DATE

28 December 2017

PAGES 57

DOCUMENT CONTROL NUMBER FCC SAR_b © 2017 INTERTEK







SAR TEST REPORT

For

UBTECH ROBOTICS CORP

First Order Stormtrooper[™] Robot with companion app

Model No.: IPSWSTS

FCC ID: 2AHJX-IPSWSTS

Report No.: SZHH01201042-006

Issue Date: 28 December 2017

Prepared by

Intertek Testing Services Shenzhen Ltd. Longhua Branch 1F/2F, Building B, QiaoAn Scientific Technology Park, Shangkeng Community, Guanhu Subdistrict, Longhua District, Shenzhen, P.R. China Telephone: 86-755-8601 6288 Fax: 86-755-8601 6751

• The test report only allows to be revised only within the report defined retention period unless further standard or the requirement was noticed

This report is for the exclusive use of Intertek's Client and is provided pursuant to the agreement between Intertek and its Client. Intertek's responsibility
and liability are limited to the terms and conditions of the agreement. Intertek assumes no liability to any party, other than to the Client in accordance with
the agreement, for any loss, expense or damage occasioned by the use of this report. Only the Client is authorized to copy or distribute this report. Any
use of the Intertek name or one of its marks for the sale or advertisement of the tested material, product or service must first be approved in writing by
Intertek. The observations and test results referenced from this report are relevant only to the sample tested. This report by itself does not imply that the
material, product, or service is or has ever been under an Intertek certification program.



Table of Contents

1	GEN	VERAL INFORMATION	
2	STA	TEMENT OF COMPLIANCE	4
3	EQU	JIPMENT UNDER TEST (EUT) TECHNICAL DESCRIPTION	6
4	AU	XILIARY EQUIPMENT DETAILS	7
5	TES	T FACILITY	7
6	EUT	Γ ANTENNA LOCATIONS	
7	GUI	IDANCE STANDARD	
8		EXPOSURE	
Ũ	8.1	LIMITS	
	8.2	EVALUATION	
9	SPE	CIFIC ABSORPTION RATE (SAR)	
	9.1	INTRODUCTION	
	9.2	SAR DEFINITION	
10	SAF	R MEASUREMENTS SYSTEM CONFIGURATION	
	10.1	SAR MEASUREMENT SET-UP	
	10.2	DASY5 E-FIELD PROBE SYSTEM	
	10.3	E-FIELD PROBE CALIBRATION	
	10.4	OTHER TEST EQUIPMENT	
	10.5	SCANNING PROCEDURE	
	10.6	DATA STORAGE AND EVALUATION	
	10.7	TISSUE-EQUIVALENT LIQUID	
	10.8	SYSTEM CHECK	
11	ME.	ASUREMENT PROCEDURES	
	11.1	GENERAL DESCRIPTION OF TEST PROCEDURES	
	11.2	MEASUREMENT VARIABILITY	
	11.3	TEST RESULTS	
12	ME.	ASUREMENT UNCERTAINTY	
13	MA	IN TEST INSTRUMENT	
AN	INEX	A: TEST LAYOUT	32
AN	INEX	B: SYSTEM CHECK RESULTS	33
AN	INEX	C: MAXIMUM GRAPH RESULTS	34
AN	INEX	D: SYSTEM VALIDATION	34
		E: PROBE, DAE AND DIPOLE CALIBRATION CERTIFICATE	
<i>i</i> 11			



1 GENERAL INFORMATION

Applicant:	UBTECH ROBOTICS CORP Nanshan I Park, No.1001 Xueyuan Road, Nanshan Dist,Shenzhen City, PR. CHINA
Product Description:	First Order Stormtrooper™ Robot with companion app
Model Number:	IPSWSTS
FCC ID	2AHJX-IPSWSTS
File Number:	SZHH01201042-006
Date of Test:	28 November 2017

The above equipment was tested by Intertek Testing Services Shenzhen Ltd. Longhua Branch. The test data, data evaluation, test procedures, and equipment configurations shown in this report were made in accordance with the procedures given in IEEE 1528-2013 and KDB 865664. This device is in compliance with Specific Absorption Rate (SAR) for general population/uncontrolled exposure limits (1.6 W/kg) specified in ANSI/IEEE C95.1-1992.

The test results of this report relate only to the tested sample identified in this report.

Prepared and Checked by:

Approved by:

Sign on file

Terry Tang Senior Engineer Kidd Yang Senior Project Engineer Date: 28 December 2017



2 STATEMENT OF COMPLIANCE

Max. Reported SAR (1g)

Test Position				Limit of SAR1g: 1.6 W/kg		
		Mode	Channel/Frequency(MHz)	Measured SAR1g (W/kg)	Reported SAR1g (W/kg)	
Body	Top Side	802.11b	11/2462	0.324	0.505	

The SAR values found for the First Order Stormtrooper[™] Robot with companion app is below the maximum recommended levels of 1.6 W/kg as averaged over any 1g tissue according to the ANSI C95.1-1992.

The maximum reported SAR value is: 0.505W/kg (1g).



Modified Information

Rev.	Summary	Date of Rev.	Report No.	
Ver.1.0	Original Report	28 November 2017	SZHH01201042-006	



3 EQUIPMENT UNDER TEST (EUT) TECHNICAL DESCRIPTION

Characteristics	Description
Description:	First Order Stormtrooper [™] Robot with companion app
Model name:	IPSWSTS
Exposure Category:	Uncontrolled Environment/General Population
Test Mode(s):	802.11 b/g/n-HT20
Operating Frequency Range:	802.11 b/g/n-HT20: 2412MHz – 2462MHz
Modulation:	BPSK, QPSK, 16QAM, 64QAM, CCK
Power Level:	IEEE 802.11b: 16dBm(max.) IEEE 802.11g/n-HT20:10dBm(max.)
Antenna Type:	Integral Antenna
Antenna Gain:	2.0dBi max
Dimensions:	28.0cmX11.0cmX14.0cm
Power supply:	DC supply: DC 3.7V internal rechargeable Li-ion Polymer battery × 2.
	Switching Adapter supply: N/A
Product Software Version:	Storm Trooper PCB V1
Product Hardware Version:	Wifi_V18, M4_r505, M0_V107

Note:

1. For more details, please refer to the User's manual of the EUT.

2. The sample under test was selected by the Client.



4 AUXILIARY EQUIPMENT DETAILS

AE: Battery	Description
Manufacturer:	/
Model:	/
S/N:	/
capacity:	1200mAh
Voltage:	3.7V

5 TEST FACILITY

Site Description		
EMC Lab.	:	Intertek Testing Services Shenzhen Ltd. Longhua Branch was accredited by China National Accreditation Service for Conformity Assessment (CNAS) with registration no.: L0327 and Taiwan Accreditation Foundation (TAF) with registration no.: L2342-151102 according to ISO/IEC 17025: 2005. Effective Date of TAF Accreditation: June 28, 2017 to August 31, 2019
		Accredited by FCC
		The Certificate Registration Number is CN1188
		Accredited by Industry Canada The Certificate Registration Number is 2055C
Name of Firm	:	Intertek Testing Services Shenzhen Ltd. Longhua Branch
Site Location	:	1F/2F, Building B, QiaoAn Scientific Technology Park, Shangkeng Community, Guanhu Subdistrict, Longhua District, Shenzhen, P.R. China



6 EUT ANTENNA LOCATIONS



All	Sides	for	SAR	Testing	Evaluation:
	~		~	1000000	

Mode	Front Side	Rear Side	Left Side	Right Side	Top Side	Bottom Side
Distance from the antenna (mm)	2	46	36	36	10	70
Exemption with Max. Allowed Power	9.6 mW	87.9 mW	68.8 mW	68.8 mW	19.1 mW	295.6 mW
802.11b	YES	N/A	N/A	N/A	YES	N/A

Note: Exemption with Max. Allowed Power Calculation according to KDB 447498 D01 Clause 4.3.1 with the following fomula.

a) For 100 MHz to 6 GHz and test separation distances \leq 50 mm, the 1-g SAR test exclusion thresholds are determined by the following:

 $[(max. power of channel, including tune-up tolerance, mW) / (min. test separation distance, mm)] \cdot [\sqrt{f_{(GHz)}}] \le 3.0$ for 1-g SAR,

*where f_(GHz) is the RF channel transmit frequency in GHz



*When the minimum test separation distance is < 5 mm, a distance of 5 mm is applied to determine SAR test exclusion.

b) For 100 MHz to 6 GHz and *test separation distances* > 50 mm, the 1-g *SAR test exclusion thresholds* are determined by the following

{[Power allowed at *numeric threshold* for 50 mm in step a)] + [(test separation distance – 50 mm) \cdot 10]} mW, for > 1500 MHz and \leq 6 GHz

c)EuT maximum power level: 16dBm=39.81mW (Duty factor = 1)



7 GUIDANCE STANDARD

The Specific Absorption Rate (SAR) testing specification, method, and procedure for this device is in accordance with the following standards:

FCC 47CFR §2.1093 Radiofrequency Radiation Exposure Evaluation: Portable Devices

ANSI C95.1, 1992: Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz.(IEEE Std C95.1-1991)

□ IEEE Std 1528[™]-2013: IEEE Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques.

KDB 865664 D01 SAR measurement 100 MHz to 6 GHz v01r04: SAR Measurement Requirements for 100 MHz to 6 GHz

KDB 865664 D02 RF Exposure Reporting v01r02: RF Exposure Compliance Reporting and Documentation Considerations

KDB 447498 D01 General RF Exposure Guidance v06: RF Exposure Procedures and Equipment Authorization Policies For Mobile and Portable Table Device

KDB 248227 D01 802.11 Wi-Fi SAR v02r02: SAR Guidance for IEEE 802.11 (Wi-Fi) Transmotters

Remark:

This portable wireless equipment has been measured in all cases requested by the relevant standards. Test results in Chapter 11 of this test report are below limits specified in the relevant standards for the tested bands only.



8 **RF EXPOSURE**

8.1 LIMITS

Uncontrolled Environment

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

Limits for General Population/Uncontrolled Exposure (W/kg)

Whole-Body	Partial-Body	Hands, Wrists, Feet and ankles	
0.08	1.6	4.0	

Whole-Body SAR is averaged over the entire body, partial-body SAR is averaged over any 1gram of tissue defined as a tissue volume in the shape of a cube. SAR for hands, wrists, feet and ankles is averaged over any 10 grams of tissue defined as a tissue volume in the shape of a cube.

8.2 EVALUATION

According to FCC KDB447498 D01 and §1.1310, systems operating under the provisions of this section shall be operated in a manner that ensures that the public is not exposed to radio frequency energy level in excess of the Commission's guidelines.

Routine SAR evaluation refers to that specifically required by § 2.1093, using measurements or computer simulation. Portable transmitters with output power greater than the applicable low threshold require SAR testing to qualify for TCB approval.



9 SPECIFIC ABSORPTION RATE (SAR)

9.1 INTRODUCTION

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

9.2 SAR DEFINITION

The SAR definition is the time derivative (rate) of the incremental energy $(^{dW})$ absorbed by (dissipated in) an incremental mass $(^{dm})$ contained in a volume element $(^{dv})$ of a given density $(^{\rho})$. The equation description is as below:

$$SAR = \frac{d}{dt}(\frac{dW}{dm}) = \frac{d}{dt}(\frac{dW}{\rho dv})$$

SAR is expressed in units of Watts per kilogram (W/kg) SAR measurement can be either related to the temperature elevation in tissue by

$$SAR = c(\frac{\delta T}{\delta t})$$

Where: C is the specific head capacity, δT is the temperature rise and δt is the exposure duration, or related to the electrical field in the tissue by

$$SAR = \frac{\sigma |E|^2}{\rho}$$

Where: σ is the conductivity of the tissue ρ is the mass density of tissue and E is the RMS electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.




10 SAR MEASUREMENTS SYSTEM CONFIGURATION

10.1 SAR MEASUREMENT SET-UP

The DASY5 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Stäubli TX=RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- An isotropic field probe optimized and calibrated for the targeted measurement.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion from optical to electrical signals for the digital communication to the DAE. To use optical surface detection, a special version of the EOC is required. The EOC signal is transmitted to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
- A computer running Win 7 profesional operating system and the DASY5 software.
- Remote control and teach pendant as well as additional circuitry for robot safety such as warning lamps, etc.
- The phantom, the device holder and other accessories according to the targeted measurement.

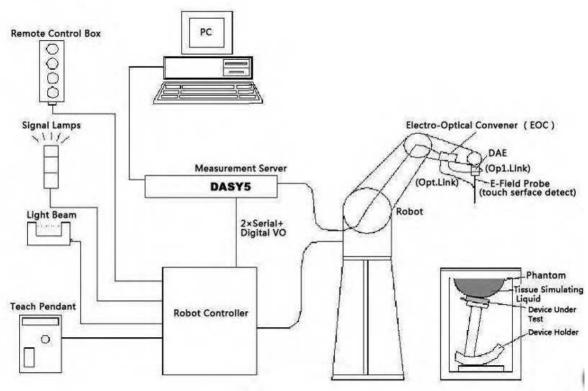

Picture 1. SAR Lab Test Measurement Set-up



10.2 DASY5 E-FIELD PROBE SYSTEM

The SAR measurements were conducted with the dosimetric probe designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multifiber line ending at the front of the probe tip. It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY5 software reads the reflection turning a software approach and looks for the maximum using 2nd ord curve fitting. The approach is stopped at reaching the maximum.

Probe Specifications:

Frequency	10 MHz - >6 GHz Linearity: ±0.2 dB (30 MHz - 6 GHz)
Directivity	±0.3 dB in TSL (rotation around probe axis) ±0.5 dB in TSL (rotation normal to probe axis)
Dynamic Range	10 μW/g – >100 mW/g Linearity: ±0.2 dB (noise: typically <1 μW/g)
Dimensions	Overall length: 337 mm (tip: 20 mm) Tip diameter: 2.5 mm (body: 10 mm) Typical distance from probe tip to dipole centers: 1 mm
Applications	High precision dosimetric measurements in any exposure scenario (e.g., very strong gradient fields); the only probe that enables compliance testing for frequencies up to 6 GHz with precision of better than 30%



Picture 2 E-field Probe



10.3 E-FIELD PROBE CALIBRATION

Each E-Probe/Probe Amplifier combination has unique calibration parameters. A TEM cell calibration procedure is conducted to determine the proper amplifier settings to enter in the probe parameters. The amplifier settings are determined for a given frequency by subjecting the probe to a known E-field density (1 mW/cm²) using an RF Signal generator, TEM cell, and RF Power Meter.

The free space E-field from amplified probe outputs is determined in a test chamber. This calibration can be performed in a TEM cell if the frequency is below 1 GHz and inn a waveguide or other methodologies above 1 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees until the three channels show the maximum reading. The power density readings equates to 1 mw/ cm².

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The E-field in the medium correlates with the temperature rise in the dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

$$SAR = C \frac{\Delta T}{\Delta t}$$

Where:

 $\begin{array}{l} \Delta t = \text{Exposure time (30 seconds)}, \\ \text{C} = \text{Heat capacity of tissue (brain or muscle)}, \\ \Delta \text{T} = \text{Temperature increase due to RF exposure.} \end{array}$

$$SAR = \frac{\left|E\right|^2 \cdot \sigma}{\rho}$$

Where: σ = Simulated tissue conductivity, ρ = Tissue density (kg/m³).

10.4 OTHER TEST EQUIPMENT

10.4.1 Data Acquisition Electronics (DAE)

The data acquisition electronics consist of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder with a control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information, as well as an optical uplink for commands and the clock. The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE is 200 MOhm; the inputs are symmetrical and floating. Common mode rejection is above 80 dB.



Picture 3: DAE



10.4.2 Robot

The SPEAG DASY system uses the high precision robots (DASY5: TX90XL) type from Stäubli SA (France). For the 6-axis controller system, the robot controller version from Stäubli is used. The Stäubli robot series have many features that are important for our application:

- High precision (repeatability 0.02mm)
- High reliability (industrial design)
- > Low maintenance costs (virtually maintenance free due to direct drive gears; no belt drives)
- > Jerk-free straight movements (brushless synchron motors; no stepper motors)
- > Low ELF interference (motor control fields shielded via the closed metallic construction shields)



Picture 4 DASY 5

10.4.3 Measurement Server

The Measurement server is based on a PC/104 CPU broad with CPU (DASY5: 400 MHz, Intel Celeron), chip disk (DASY5: 128MB), RAM (DASY5: 128MB). The necessary circuits for communication with the DAE electronic box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY I/O broad, which is directly connected to the PC/104 bus of the CPU broad.



Picture 5 Server for DASY 5



The measurement server performs all real-time data evaluation of field measurements and surface detection, controls robot movements and handles safety operation. The PC operating system cannot interfere with these time critical processes. All connections are supervised by a watchdog, and disconnection of any of the cables to the measurement server will automatically disarm the robot and disable all program-controlled robot movements. Furthermore, the measurement server is equipped with an expansion port which is reserved for future applications. Please note that this expansion port does not have a standardized pinout, and therefore only devices provided by SPEAG can be connected. Devices from any other supplier could seriously damage the measurement server.

10.4.4 Device Holder for Phantom

The SAR in the phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface.. Accurate device positioning is therefore crucial for accurate and repeatable measurements. The positions in which the devices must be measured are defined by the standards.

The DASY device holder is designed to cope with the different positions given in the standard. It has two scales for device rotation (with respect to the body axis) and device inclination (with respect to the line between the ear reference points). The rotation centers for both scales are the ear reference point (ERP). Thus the device needs no repositioning when changing the angles.

The DASY device holder is constructed of low-loss POM material having the following dielectric parameters: relative permittivity $\mathcal{E}=3$ and loss tangent $\delta=0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.

<Laptop Extension Kit>

The extension is lightweight and made of POM, acrylic glass and foam. It fits easily on the upper part of the Mounting Device in place of the phone positioner. The extension is fully compatible with the Twin-SAM and ELI phantoms.




Picture 6: Device Holder

10.4.5 Phantom

The SAM Twin Phantom V4.0 is constructed of a fiberglass shell integrated in a table. The shape of the shell is based on data from an anatomical study designed to Represent the 90th percentile of the population. The phantom enables the dissymmetric evaluation of SAR for both left and right handed handset usage, as well as body-worn usage using the flat phantom region. Reference markings on the Phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot. The shell phantom has a 2mm shell thickness (except the ear region where shell thickness increases to 6 mm).

Shell Thickness:	2 ± 0. 2 mm
Filling Volume:	Approx. 25 liters
Dimensions:	810 x 1000 x 500 mm (H x L x W)
Available:	Special





Picture 7: SAM Twin Phantom

10.5 SCANNING PROCEDURE

The DASY5 installation includes predefined files with recommended procedures for measurements and validation. They are read-only document files and destined as fully defined but unmeasured masks. All test positions (head or body-worn) are tested with the same configuration of test steps differing only in the grid definition for the different test positions.

The "reference" and "drift" measurements are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the DUT's output power and should vary max. ± 5 %.

The "surface check" measurement tests the optical surface detection system of the DASY5 system by repeatedly detecting the surface with the optical and mechanical surface detector and comparing the results. The output gives the detecting heights of both systems, the difference between the two systems and the standard deviation of the detection repeatability. Air bubbles or refraction in the liquid due to separation of the sugar-water mixture gives poor repeatability (above ± 0.1 mm). To prevent wrong results tests are only executed when the liquid is free of air bubbles. The difference between the optical surface detection and the actual surface depends on the probe and is specified with each probe. (It does not depend on the surface reflectivity or the probe angle to the surface within $\pm 30^{\circ}$.)

Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values before running a detailed measurement around the hot spot. Before starting the area scan a grid spacing is set according to FCC KDB Publication 865664. During scan the distance of the probe to the phantom remains unchanged. After finishing area scan, the field maxima within a range of 2 dB will be ascertained.

Zoom Scan

After the maximum interpolated values were calculated between the points in the cube, the SAR was averaged over the spatial volume (1g or 10g) using a 3D-Spline interpolation algorithm. The 3D-spline is composed of three one-dimensional splines with the "Not a knot" condition (in x, y, and z directions). The volume was then integrated with the trapezoidal algorithm.

Spatial Peak Detection

The procedure for spatial peak SAR evaluation has been implemented and can determine values of masses of 1g and 10g, as well as for user-specific masses. The DASY5 system allows evaluations that combine measured data and robot positions, such as:

- maximum search
- extrapolation
- boundary correction
- peak search for averaged SAR

During a maximum search, global and local maxima searches are automatically performed in 2-D after each Area Scan measurement with at least 6 measurement points. It is based on the evaluation of the local SAR gradient calculated by the Quadratic Shepard's method. The algorithm will find the global maximum and all local maxima within -2 dB of the global maxima for all SAR distributions.



Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. Several measurements at different distances are necessary for the extrapolation. Extrapolation routines require at least 10 measurement points in 3-D space.

They are used in the Zoom Scan to obtain SAR values between the lowest measurement points and the inner phantom surface. The routine uses the modified Quadratic Shepard's method for extrapolation.

A Z-axis scan measures the total SAR value at the x-and y-position of the maximum SAR value found during the cube scan. The probe is moved away in z-direction from the bottom of the SAM phantom in 5mm steps.

Frequency	Maximum Area Scan Resolution (mm) (Δxarea, Δyarea)	Maximum Zoom Scan Resolution (mm) (Δxzoom, Δyzoom)	Maximum Zoom Scan Spatial Resolution (mm) Δzzoom(n)	Minimum Zoom Scan Volume (mm) (x,y,z)
≤2 GHz	≤15	≤8	≤5	≥ 30
2-3 GHz	≤12	≤5	≤5	≥30
3-4 GHz	≤12	≤5	≤4	≥28
4-5 GHz	≤10	≤4	≤3	≥25
5-6 GHz	≤10	≤4	≤2	≥22

Table 1: Area and Zoom Scan Resolutions per FCC KDB Publication 865664 D01

10.6 DATA STORAGE AND EVALUATION

10.6.1 Data Storage

The DASY5 software stores the acquired data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension ".DAE4". The software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of incorrect parameter settings. For example, if a measurement has been performed with a wrong crest factor parameter in the device set up, the parameter can be corrected afterwards and the data can be re-evaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type ([V/m], [A/m], [°C], [mW/g], [mW/cm²], [dBrel], etc.). Some of these units are not available in certain situations or show meaningless results, e.g., a SAR output in a loss less media will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

10.6.2 Data Evaluation by SEMCAD

The SEMCAD software automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters:

- Sensitivity	Normi, ai0, ai1, ai2
Considivity	
 Conversion factor 	ConvFi
- Diode compression point	Dcpi
Device parameters:	
- Frequency	f
- Crest factor	cf



Media parameters:

- Conductivity

- Density

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY5 components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics.

If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$V_i = U_i + U_i^2 \cdot c f / dcp_i$

With V_i = compensated signal of channel i (i = x, y, z)

 \mathbf{U}_i = input signal of channel i (i = x, y, z)

cf = crest factor of exciting field (DASY parameter)

dcp_i = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be

evaluated:

E-field probes: $E_i = (V_i / Norm_i \cdot ConvF)^{1/2}$

H-field probes: $H_i = (V_i)^{1/2} \cdot (a_{i0} + a_{i1} f + a_{i2} f^2) / f$

With V_i = compensated signal of channel i (i = x, y, z)

Norm_i = sensor sensitivity of channel i (i = x, y, z)

[mV/(V/m)2] for E-field Probes

ConvF = sensitivity enhancement in solution

a_{ij} = sensor sensitivity factors for H-field probes

f = carrier frequency [GHz]

 E_i = electric field strength of channel i in V/m

 H_i = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

 $E_{tot} = (E_x^2 + E_y^2 + E_z^2)^{1/2}$

The primary field data are used to calculate the derived field units.

SAR = (E_{tot}) 2 · σ / (ρ · 1000)

with SAR = local specific absorption rate in mW/g

Etot = total field strength in V/m

- = conductivity in [mho/m] or [Siemens/m]
- = equivalent tissue density in g/cm³

Note that the density is normally set to 1 (or 1.06), to account for actual brain density rather than the density of the simulation liquid. The power flow density is calculated assuming the excitation field to be a free space field.

 $P_{pwe} = E_{tot}^2 / 3770 \text{ or } P_{pwe} = H_{tot}^2 \cdot 37.7$

with P_{pwe} = equivalent power density of a plane wave in mW/cm² E_{tot} = total electric field strength in V/m ; H_{tot} = total magnetic field strength in A/m



10.7 TISSUE-EQUIVALENT LIQUID

10.7.1 Tissue-equivalent Liquid Ingredients

The liquid is consisted of water, salt and Glycol. The liquid has previously been proven to be suited for worst-case. The Table 2 shows the detail solution. It's satisfying the latest tissue dielectric parameters requirements proposed by the KDB 865664 D01.

Table 2: Composition of the Body Tissue Equivalent Matter

MIXTURE%	FREQUENCY (Body) 2450MHz
Water	73.2
Glycol	26.7
Salt	0.1
Dielectric Parameters Target Value	f=2450MHz ε=52.7 σ=1.95

10.7.2 Tissue-equivalent Liquid Properties

Table 3: Dielectric Performance of Tissue Simulating Liquid


Test Date	Frequ ency (MHz)	Tissue Type	Liquid Temp. (℃)	Conductivity (σ)	Permittivity (εr)	Conductivity Target (σ)	Permittivity Target (ɛr)	Delta (σ) (%)	Delta (εr) (%)	Limit (%)
2017-11-28	2450	Body	21.5	2.016	52.379	1.95	52.7	3.4	-0.61	±5



10.8 SYSTEM CHECK

10.8.1 Description of System Check

The manufacturer calibrates the probes annually. Dielectric parameters of the tissue simulants were measured every day using the dielectric probe kit and the network analyzer. A system check measurement was made following the determination of the dielectric parameters of the simulant, using the dipole validation kit. A power level of 250 mW was supplied to the dipole antenna, which was placed under the flat section of the twin SAM phantom. The system check results (dielectric parameters and SAR values) are given in the table 4. System check results have to be equal or near the values determined during dipole calibration with the relevant liquids and test system (±10 %). System check is performed regularly on all frequency bands where tests are performed with the DASY5 system.

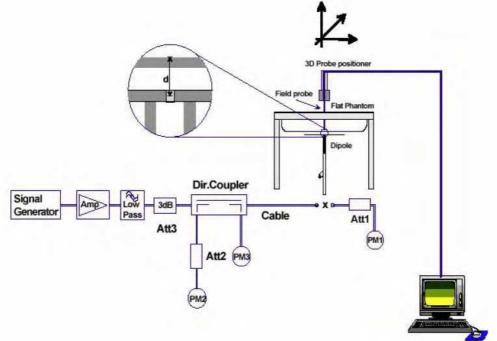

Picture 9. System Check Set-up



10.8.2 System Check Results

Table 5: System Check for Body Tissue Simulating Liquid

Frequency	Test Date	Dielectric Parameters		250mW	1W	1W Target	Limit(±10%	
				Measured	Normalized	SAR1g	Deviation)	
				SAR1g	SAR1g			
		٤r	σ (s/m)	(W/kg)				
2450MHz	2017-11-28	52.379	2.016	13.2	52.8	52.1	1.34	
Note: 1. Th	Note: 1. The graph results see ANNEX B.							
2.Ta	rget Values us	ed derive from	n the calibrati	on certificate.				



11 MEASUREMENT PROCEDURES

11.1 GENERAL DESCRIPTION OF TEST PROCEDURES

For WLAN SAR testing, WLAN engineering testing software installed on the DUT can provide continuous transmitting RF signal. This RF signal utilized in SAR measurement has almost 100% duty cycle and its crest factor is 1.

For the 802.11b/g/n SAR tests, a communication link is set up with the test mode software for WIFI mode test. During the test, at the each test frequency channel, the EUT is operated at the RF continuous emission mode. Provided higher maximum output power is not specified for the other channels, channels 1, 6 and 11 are used to configure 22 MHz DSSS and 20 MHz OFDM channels for SAR measurements; otherwise, the closest adjacent channel with the highest maximum output power specified for production units should be tested instead of channels 1, 6 or 11. When 40 MHz channels are supported, and provided higher maximum output power is not specified for other applicable 40 MHz channels, channel 6 is used to measure SAR; otherwise, the channel with highest specified maximum output power should be tested instead. In addition, SAR test reduction with respect to reported SAR and transmission band width according to 4.3.3 of KDB Publication 447498 D01 may also be applied

802.11b/g/n operating modes are tested independently according to the service requirements in each frequency band. 802.11b/g/n modes are tested on the maximum average output channel.

SAR is measured for 2.4 GHz 802.11b DSSS using either a fixed test position or, when applicable, the initial test position procedure. SAR test reduction is determined according to the following:

a) When the reported SAR of the highest measured maximum output power channel (see 3.1) for the exposure configuration is \leq 0.8 W/kg, no further SAR testing is required for 802.11b DSSS in that exposure configuration.

b) When the reported SAR is > 0.8 W/kg, SAR is required for that exposure configuration using the next highest measured output power channel. When any reported SAR is > 1.2 W/kg, SAR is required for the third channel; i.e., all channels require testing.

When SAR measurement is required for 2.4 GHz 802.11g/n OFDM configurations, the measurement and test reduction procedures for OFDM are applied (see 5.3, including subclauses). SAR is not required for the following 2.4 GHz OFDM conditions.

a) When KDB Publication 447498 D01 SAR test exclusion applies to the OFDM configuration. b) When the highest reported SAR for DSSS is adjusted by the ratio of OFDM to DSSS specified maximum output power and the adjusted SAR is ≤ 1.2 W/kg.

11.2 MEASUREMENT VARIABILITY

Per FCC KDB Publication 865664 D01, SAR measurement variability was assessed for each frequency band, which was determined by the SAR probe calibration point and tissue-equivalent medium used for the device measurements. When both head and body tissue-equivalent media were required for SAR measurements in a frequency band, the variability measurement procedures were applied to the tissue medium with the highest measured SAR, using the highest measured SAR configuration for that tissue-equivalent medium. These additional measurements were repeated after the completion of all measurements requiring the same head or body tissue-equivalent medium in a frequency band. The test device was returned to ambient conditions (normal room temperature) with the battery fully charged before it was re-mounted on the device holder for the repeated measurement(s) to minimize any unexpected variations in the repeated results.

SAR Measurement Variability was assessed using the following procedures for each frequency band:

1) Repeated measurement is not required when the original highest measured SAR is < 0.80 W/kg; steps 2) through 4) do not apply.



- 2) When the original highest measured SAR is \geq 0.80 W/kg, repeat that measurement once.
- Perform a second repeated measurement only if the ratio of largest to smallest SAR for the original and first repeated measurements is > 1.20 or when the original or repeated measurement is ≥ 1.45 W/kg (~ 10% from the 1-g SAR limit).
- Perform a third repeated measurement only if the original, first or second repeated measurement is ≥
 1.5 W/kg and the ratio of largest to smallest SAR for the original, first and second repeated
 measurements is > 1.20.



11.3 TEST RESULTS

11.3.1 Conducted Power Results

Mode	Channel / Frequency (MHz)	Data rate (Mbps)	AV Power (dBm)
		1	13.0
	1 / 2/12	2	12.4
	1 / 2412	5.5	12.3
		11	12.1
		1	13.62
11b	6 / 2437	2	13.41
110	67 2437	5.5	13.12
		11	13.02
		1	14.07
	11 / 24/22	2	13.84
	11 / 2462	5.5	13.8
		11	13.9
		6	7.97
		9	7.9
		12	7.9
	1 / 2412	18	7.8
		24	7.9
		36	7.7
		48	7.7
		54	7.6
		6	8.55
		9	8.41
		12	8.29
11	6 / 0 107	18	8.24
11g	6 / 2437	24	8.3
		36	8.22
		48	8.19
		54	8.17
		6	9.0
		9	8.91
		12	8.88
	11 / 24/22	18	8.82
	11 / 2462	24	8.78
		36	8.76
		48	8.76
		54	8.71



Mode	Channel / Frequency (MHz)	Data rate (Mbps)	AV Power (dBm)		
		MCS0	8.2		
		MCS1	8.15		
		MCS2	8.11		
	1 / 2412	MCS3	8.06		
	1 / 2412	MCS4	8.03		
		MCS5	7.94		
		MCS6 8.			
		MCS7	7.97		
		MCS0	8.62		
		MCS1	8.58		
	6 / 2437	MCS2	8.51		
11n-HT20		MCS3	8.51		
1111-H120	0/243/	MCS4	8.53		
		MCS5	8.49		
		MCS6	8.44		
		MCS7	8.41		
		MCS0	8.85		
		MCS1	8.81		
		MCS2	8.78		
	11 / 2462	MCS3	8.72		
	11 / 2402	MCS4	8.7		
		MCS5	8.7		
		MCS6	8.68		
		MCS7	8.65		



11.3.2 SAR TEST RESULTS

2.4GHz WiFi-802.11b DSSS SAR Value

Toot Channel		Channel/	Max.	Conducte	Drift ±0.21dB		Limit SAR1g: 1.6 W/kg				
Test Position	Frequency (MHz)	Mode	Allowed Power (dBm)	d Power (dBm)	Drift(dB)	Measured SAR1g (W/kg)	Scaling Factor	Reported SAR1g (W/kg)	Figure No.		
	Test Position of Body (Distance Between EUT and Flat Phatom:0mm)										
Front Side	11/2462	DSSS	16.0	14.07	0.07	0.062	1.56	0.097	-		
Rear Side	11/2462	DSSS	16.0	14.07	N/A	N/A	N/A	N/A	-		
Left Side	11/2462	DSSS	16.0	14.07	N/A	N/A	N/A	N/A	-		
Right Side	11/2462	DSSS	16.0	14.07	N/A	N/A	N/A	N/A	-		
Top Side	11/2462	DSSS	16.0	14.07	-0.11	0.324	1.56	0.505	Fig.1		
Bottom Side	11/2462	DSSS	16.0	14.07	N/A	N/A	N/A	N/A	-		
Top Side	1/2412	DSSS	16.0	13.00	N/A	N/A	N/A	N/A	-		
Top Side	6/2437	DSSS	16.0	13.62	N/A	N/A	N/A	N/A	-		

Note:

1. The value with blue color is the maximum SAR Value of each test band.

2 When the reported SAR of the highest measured maximum output power channel for the exposure configuration is ≤ 0.8 W/kg, no further SAR testing is required for 802.11b DSSS in that exposure configuration.

- 3 When the reported SAR is > 0.8 W/kg, SAR is required for that exposure configuration using the next highest measured output power channel. When any reported SAR is > 1.2 W/kg, SAR is required for the third channel; i.e., all channels require testing.
- 4 The EUT exercise program (provided by client) used during SAR testing was designed to exercise the various system components in a manner similar to a typical use. During the test, Channel and test mode software provided by the applicant was used to control the operating channel as well as the test mode. The worst case configuration is used in all specified testing.

SAR Measurement Variability Results

Test Position	Channel/ Frequency (MHz)	Measured SAR (1g)	1st Repeated SAR (1g)	Ratio	2nd Repeated SAR (1g)	3rd Repeated SAR (1g)
Top Side	11/2462	0.324	N/A	N/A	N/A	N/A
Note:						

NULE.

1 When the original highest measured SAR is \geq 0.80 W/kg, the measurement was repeated once.

2 A second repeated measurement was preformed only if the ratio of largest to smallest SAR for the original and first repeated measurements was > 1.20 or when the original or repeated measurement was ≥ 1.45 W/kg (~ 10% from the 1-g SAR limit).

3 A third repeated measurement was performed only if the original, first or second repeated measurement was ≥ 1.5 W/kg and the ratio of largest to smallest SAR for the original, first and second repeated measurements is > 1.20.

4 Repeated measurements are not required when the original highest measured SAR is < 0.80 W/kg



2.4 GHz 802.11g/n-HT20 OFDM SAR Test Exclusion Requirements

Test	Channel/	802.11b Max. Allowed	802.11g/n Max. Allowed		Limit SAR1g : 1.6W/kg			
Position	Frequency (MHz)	Power (dBm)	Power (dBm)	802.11b Report SAR1g (W/kg)	Scaling Factor	Adjusted SAR1g (W/kg)		
Top Side	11/2462	16	10	0.324	4.0	0.081		
Note: SAR is not required for the 2.4 GHz OFDM conditions if When the highest reported SAR for DSSS is adjusted by the ratio of OFDM to DSSS specified maximum output power and the adjusted SAR is \leq 1.2 W/kg.								

11.3.3 MAXIMUM GRAPH RESULTS

The graph results see ANNEX C.



12 MEASUREMENT UNCERTAINTY

The measured SAR were <1.5 W/kg for all frequency bands, therefore per KDB Publication 865664 D01v01r04, the extensive SAR measurement uncertainty analysis described in IEEE Std 1528-2013 is not required in SAR reports.




13 MAIN TEST INSTRUMENT


	Equipment No.	Equipment	Manufacturer	Model No.	Serial No.	Last Cal.	Cal. Interval
\boxtimes	SZ060-01	SAR Test System	SPEAG	DASY52 SAR TX90XL	F14/5YJ0B1/ A/01	6/23/2017	1 year
	SZ060-01- 01	E-Field Probe	SPEAG	EX3DV4	7322	6/29/2017	1 year
	SZ060-01- 10	System Validation Dipole	SPEAG	D2450V2	966	6/10/2015	3 year
	SZ060-01- 13	Data Acquisition Unit	SPEAG	DAE4	1473	6/23/2017	1 year
	SZ060-01- 14	Dielectric Assessment Kit	SPEAG	DAKS 3.5	1056	N/A	N/A
	SZ060-01- 15	Vector Reflectometer	Copper Mountain Technologies	Planar R140	0090614	N/A	N/A
\boxtimes	SZ060-01- 16	Thermometer	LKM electronics GmbH	DTM3000	3477	8/9/2017	1 year
	SZ060-01- 17	Power Amplifier	Mini Circuits	ZHL-42W+	QA1449003	N/A	N/A
	SZ060-01- 18	Power Amplifier	Mini Circuits	ZVE-8G+	111701437	N/A	N/A
\boxtimes	SZ060-01- 21	ELI Phantom	SPEAG	ELI Phantom V6.0	2033	N/A	N/A
\boxtimes	SZ180-15	Signal Generator	R&S	SMB100A	113589	11/15/2017	1 year
	SZ070-04	Directional Bridge	Agilent	86205A	MY31402141	12/27/2016	1 year
	SZ182-02	RF Power Meter	Anritsu	ML2496A	1302005	6/1/2017	1 year
\boxtimes	SZ182-03	Average power sensor	R&S	NRP-Z22	101689	7/20/2017	1 year
	SZ070-01	Attenuator	Huber Suhner	10dB	N/A	N/A	N/A
	SZ070-02	Attenuator	Huber Suhner	30dB	N/A	N/A	N/A
	N/A	Device Holder	SPEAG	N/A	N/A	N/A	N/A
	SZ060-01- 22	SAR Test System Software	SPEAG	DASY5.2 SW: 52.8.8.1222	N/A	N/A	N/A



ANNEX A: TEST LAYOUT

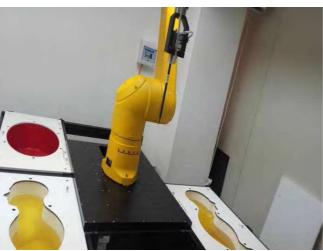

Specific Absorption Rate Test Layout

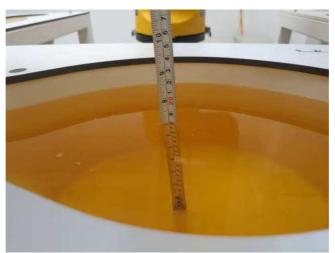

Liquid Depth in the flat phantom (2450MHz, 18.2cm)



Front Side (distance 0mm with Flat Phatom)



Top Side (distance 0mm with Flat Phatom)



ANNEX B: SYSTEM CHECK RESULTS

Date: 11/28/2017

Test Laboratory: Intertek Service

System Check 2450


Communication System: UID 0, CW (0); Frequency: 2450 MHz;Duty Cycle: 1:1 Medium: 2450 Body Medium parameters used: f = 2450 MHz; σ = 2.016 S/m; ϵ_r = 52.379; ρ = 1000 kg/m³ Phantom section: Flat Section Ambient Temperature: 22.0 °C; Liquid Temperature: 21.5 °C

DASY Configuration:

- Probe: EX3DV4 SN7322; ConvF(7.15, 7.15, 7.15); Calibrated: 6/29/2017;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1473; Calibrated: 6/23/2017
- Phantom: ELI V6.0 (20deg probe tilt); Type: QD OVA 003 AA; Serial: 2033
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7373)

Area Scan (51x61x1): Interpolated grid: dx=1.500 mm, dy=1.500 mm Maximum value of SAR (interpolated) = 20.8 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 70.14 V/m; Power Drift = -0.00 dBPeak SAR (extrapolated) = 31.0 W/kg SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.4 W/kg Maximum value of SAR (measured) = 19.9 W/kg

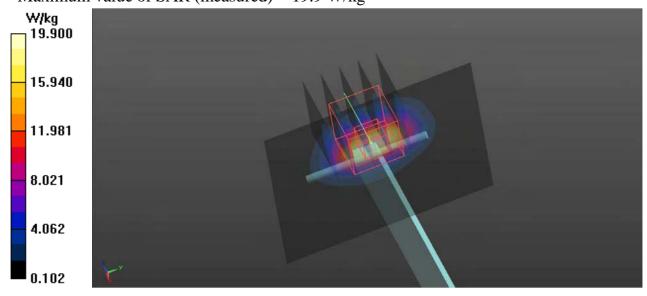



ANNEX C: MAXIMUM GRAPH RESULTS

Date: 11/28/2017

Test Laboratory: Intertek Service

802.11b_Top Side_CH11


Communication System: UID 0, WiFi 802.11 b (0); Frequency:2462 MHz;Duty Cycle: 1:1 Medium: 2450 Body Medium parameters used: f = 2462 MHz; $\sigma = 2.031$ S/m; $\epsilon r = 52.34$; $\rho = 1000$ kg/m3 Phantom section: Flat Section Ambient Temperature: 22.0 °C; Liquid Temperature: 21.5 °C

DASY Configuration:

- Probe: EX3DV4 SN7322; ConvF(7.15, 7.15, 7.15); Calibrated: 6/29/2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1473; Calibrated: 6/23/2017
- Phantom: ELI V6.0 (20deg probe tilt); Type: QD OVA 003 AA; Serial: 2033
- DASY52 52.8.8(1258); SEMCAD X 14.6.10(7373)

Area Scan (91x91x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm Maximum value of SAR (interpolated) = 0.506 W/kg

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 12.85 V/m; Power Drift = -0.11dB Peak SAR (extrapolated) = 0.604 W/kg SAR(1 g) = 0.324 W/kg; SAR(10 g) = 0.159 W/kg Maximum value of SAR (measured) = 0.494 W/kg

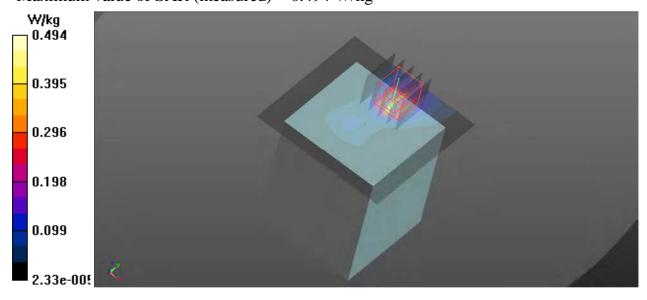



ANNEX D: SYSTEM VALIDATION

The SAR system must be validated against its performance specifications before it is deployed. When SAR probes, system components or software are changed, upgraded or recalibrated, these must be validated with the SAR system(s) that operates with such components.

Justification for Extended SAR Dipole Calibrations

Usage of SAR dipoles calibrated less than 3 years ago but more than 1 year ago were confirmed in maintaining return loss (≤20 dB, within 20% of prior calibration) and impedance (within 5 ohm from prior calibration) requirements per extended calibrations in KDB 865664 D01: Table D.1: Antenna Parameters with Body Tissue Simulating Liquid

Table D.1: System Validation Part 1

	Dipole D2450V2 SN: 966								
		Body Liquid							
Date of	Return Loss(dB)	Δ%	Impedance (Ω)	ΔΩ					
Measurement		_ / *							
2015-06-10	-28.2	-	50.1+3.9j	-					
2016-06-09	-27.7	1.8	51.2+4.1j	1.1					
2017-07-30	-29.7	5.3	50.7+3.3j	0.6					

Table D.2: System Validation Part 2

Probe SN: 7322							
Liquid name	Measured Date	Description	Dielectric Parameters		Verdict		
			٦3	σ(s/m)	Verdict		
2450MHz (Body)	2017-7-30	Target Value	52.70	1.95			
		±5% window	50.07 — 55.34	1.85 — 2.05	PASS		
		Measurement Value	51.338	1.97			

Table D.3: System Validation Part 3

CW	Sensitivity	PASS	PASS
Validation	Probe linearity	PASS	PASS
	Probe Isotropy	PASS	PASS
Mod	MOD.type	QPSK	QPSK
Validation	Duty factor	PASS	PASS
	PAR	PASS	PASS

Temperature: 21°C



ANNEX E: PROBE, DAE and DIPOLE CALIBRATION CERTIFICATE

and the second s		Stranger Stranger	CNAS 校准 CALIBRA
Add: No.51 Xueyı Tel: +86-10-6230- E-mail: cttl/@china	1633-2218 Fax: +1	rict. Beijing, 100191. China 86-10-6230-1633-2209 www.chinattl.cn	CNAS LO
Client Inte	ertek	Certificate No: Z17	-97087
CALIBRATION C	ERTIFICAT	E	
Object	EX3DV4	4 - SN:7322	
Calibration Procedure(s)	FF-Z11-	004-01	
		ion Procedures for Dosimetric E-field Probes	
Calibration date:	June 29		
	June 29	, 2017	
		he uncertainties with confidence probability a	- and the following
ages and are part of the contract of the contr		he closed laboratory facility: environment	temperature(22±3) © and
bages and are part of the co All calibrations have beer numidity<70%. Calibration Equipment used	n conducted in th	r calibration)	
bages and are part of the co All calibrations have beer numidity<70%. Calibration Equipment used	n conducted in th	r calibration) Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
bages and are part of the constraints have been aumidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2	n conducted in th I (M&TE critical for ID #	r calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05857)	Scheduled Calibration Jun-18
bages and are part of the contract of the cont	n conducted in th I (M&TE critical for ID # 101919	r calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857)	Scheduled Calibration Jun-18 Jun-18
bages and are part of the control of	I (M&TE critical for ID # 101919 101547	r calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05857)	Scheduled Calibration Jun-18
bages and are part of the constraints have been aumidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator	I (M&TE critical for ID # 101919 101547 101548	r calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857)	Scheduled Calibration Jun-18 Jun-18 Jun-18
bages and are part of the control of	I (M&TE critical for ID # 101919 101547 101548 18N50W-10dB	r calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 13-Mar-16(CTTL,No.J16X01547) 13-Mar-16(CTTL, No.J16X01548)	Scheduled Calibration Jun-18 Jun-18 Jun-18 Mar-18 Mar-18 Mar-18
Calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4	Conducted in the conducted in the conducted in the critical for ID # 101919 101547 101548 18N50W-10dB 18N50W-20dB	r calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 13-Mar-16(CTTL,No.J16X01547)	Scheduled Calibration Jun-18 Jun-18 Jun-18 Mar-18
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator	I (M&TE critical for ID # 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7433	r calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) 26-Sep-16(SPEAG, No.EX3-7433_Sep16) 13-Dec-16(SPEAG, No.DAE4-549_Dec16)	Scheduled Calibration Jun-18 Jun-18 Jun-18 Mar-18 Mar-18 Sep-17 Dec -17
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4	n conducted in the I (M&TE critical for ID # 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7433 SN 549 ID #	r calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) 26-Sep-16(SPEAG,No.EX3-7433_Sep16) 13-Dec-16(SPEAG, No.DAE4-549_Dec16) Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration Jun-18 Jun-18 Jun-18 Mar-18 Mar-18 Sep-17 Dec -17 Scheduled Calibration
ages and are part of the ca All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGeneratorMG3700A	n conducted in the I (M&TE critical for ID# 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7433 SN 549 ID # 6201052605	r calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) 26-Sep-16(SPEAG,No.EX3-7433_Sep16) 13-Dec-16(SPEAG, No.DAE4-549_Dec16) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05858)	Scheduled Calibration Jun-18 Jun-18 Jun-18 Mar-18 Mar-18 Sep-17 Dec -17 Scheduled Calibration Jun-18
bages and are part of the ca All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGeneratorMG3700A Network Analyzer E5071C	n conducted in the I (M&TE critical for ID# 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7433 SN 549 ID # 6201052605	r calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) 26-Sep-16(SPEAG,No.EX3-7433_Sep16) 13-Dec-16(SPEAG, No.DAE4-549_Dec16) Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration Jun-18 Jun-18 Jun-18 Mar-18 Mar-18 Sep-17 Dec -17 Scheduled Calibration
bages and are part of the ca All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGeneratorMG3700A Network Analyzer E5071C	n conducted in the I (M&TE critical for ID# 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7433 SN 549 ID # 6201052605 MY46110673	r calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 13-Mar-16(CTTL, No.J17X05857) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) 26-Sep-16(SPEAG,No.EX3-7433_Sep16) 13-Dec-16(SPEAG, No.DAE4-549_Dec16) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05858) 13-Jan-17 (CTTL, No.J17X00285)	Scheduled Calibration Jun-18 Jun-18 Jun-18 Mar-18 Mar-18 Sep-17 Dec -17 Scheduled Calibration Jun-18 Jan -18
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference10dBAttenuator Reference20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGeneratorMG3700A Network Analyzer E5071C	n conducted in the I (M&TE critical for ID # 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7433 SN 549 ID # 6201052605 MY46110673 Name	r calibration) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05857) 27-Jun-17 (CTTL, No.J17X05857) 13-Mar-16(CTTL, No.J16X01547) 13-Mar-16(CTTL, No.J16X01548) 26-Sep-16(SPEAG,No.EX3-7433_Sep16) 13-Dec-16(SPEAG, No.DAE4-549_Dec16) Cal Date(Calibrated by, Certificate No.) 27-Jun-17 (CTTL, No.J17X05858) 13-Jan-17 (CTTL, No.J17X00285) Function	Scheduled Calibration Jun-18 Jun-18 Jun-18 Mar-18 Mar-18 Sep-17 Dec -17 Scheduled Calibration Jun-18 Jan -18

Certificate No: Z17-97087

Page 1 of 11



Intertek Report No.: SZHH01201042-006



Tel: +86-10-62304633-2218 E-mail: cttl@chinattl.com

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Fax: +86-10-62304633-2209 Http://www.chinattl.cn

Glossary

choosary.	
TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A,B,C,D	modulation dependent linearization parameters
Polarization Φ	Φ rotation around probe axis
Polarization θ	θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i
	θ =0 is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORMx, y,z: Assessed for E-field polarization θ=0 (f≤900MHz in TEM-cell; f>1800MHz: waveguide). 0 NORMx, y,z are only intermediate values, i.e., the uncertainties of NORMx, y,z does not effect the E^2 -field uncertainty inside TSL (see below ConvF).
- NORM(f)x, y, z = NORMx, y, z* frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx, y, z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- Ax, y, z; Bx, y, z; Cx, y, z; VRx, y, z: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature 0 Transfer Standard for f≤800MHz) and inside waveguide using analytical field distributions based on power measurements for f >800MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from±50MHz to±100MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: Z17-97087

Page 2 of 11





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209

 E-mail: cttl@chinattl.com
 <u>Http://www.chinattl.cn</u>

Probe EX3DV4

SN: 7322

Calibrated: June 29, 2017

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: Z17-97087

Page 3 of 11





DASY/EASY – Parameters of Probe: EX3DV4 – SN: 7322

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm(µV/(V/m) ²) ^A	0.45	0.55	0.52	±10.0%
DCP(mV) ^B	97.4	98.3	98.6	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dBõV	c	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	176.7	±2.0%
		Y	0.0	0.0	1.0		198.0	
		Ζ	0.0	0.0	1.0		195.2	

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X, Y, Z do not affect the E²-field uncertainty inside TSL (see Page 5 and Page 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainly is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No: Z17-97087

Page 4 of 11





DASY/EASY – Parameters of Probe: EX3DV4 – SN: 7322

f [MHz] ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
835	41.5	0.90	9.55	9.55	9.55	0.11	1.66	±12.1%
1750	40.1	1.37	8.41	8.41	8.41	0.25	1.00	±12.1%
1900	40.0	1.40	7.88	7.88	7.88	0.28	0.97	±12.1%
2300	39.5	1.67	7.64	7.64	7.64	0.46	0.76	±12.1%
2450	39.2	1.80	7.36	7.36	7.36	0.31	1.09	±12.1%
2600	39.0	1.96	7.09	7.09	7.09	0.40	0.88	±12.1%
5250	35.9	4.71	5.25	5.25	5.25	0.36	1.40	±13.3%
5600	35.5	5.07	4.73	4.73	4.73	0.40	1.35	±13.3%
5750	35.4	5.22	4.77	4.77	4.77	0.40	1.40	±13.3%

Calibration Parameter Determined in Head Tissue Simulating Media

^c Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequency below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters. ^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: Z17-97087

Page 5 of 11





DASY/EASY - Parameters of Probe: EX3DV4 - SN: 7322

f [MHz] ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
835	55.2	0.97	9.68	9.68	9.68	0.17	1.46	±12.1%
1750	53.4	1.49	8.00	8.00	8.00	0.23	1.06	±12.1%
1900	53.3	1.52	7.73	7.73	7.73	0.18	1.23	±12.1%
2300	52.9	1.81	7.40	7.40	7.40	0.37	1.01	±12.1%
2450	52.7	1.95	7.15	7.15	7.15	0.31	1.25	±12.1%
2600	52.5	2.16	7.04	7.04	7.04	0.50	0.90	±12.1%
5250	48.9	5.36	4.72	4.72	4.72	0.45	1.70	±13.3%
5600	48.5	5.77	4.06	4.06	4.06	0.45	1.75	±13.3%
5750	48.3	5.94	4.27	4.27	4.27	0.50	1.97	±13.3%

Calibration Parameter Determined in Body Tissue Simulating Media

^c Frequency validity above 300 MHz of \pm 100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to \pm 50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is \pm 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to \pm 110 MHz.

^F At frequency below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters. ^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: Z17-97087

Page 6 of 11



Intertek Report No.: SZHH01201042-006




 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209

 E-mail: cttl@chinattl.com
 <u>Http://www.chinattl.cn</u>

Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

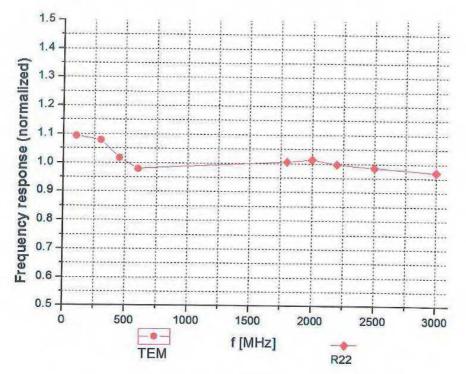

Uncertainty of Frequency Response of E-field: ±7.4% (k=2)

Certificate No: Z17-97087

Page 7 of 11






 Add: No.51 Xueyuan Road, Ilaidian District, Beijing, 100191, China


 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209


 E-mail: cttl@chinattl.com
 Http://www.chinattl.cn

Receiving Pattern (Φ), θ=0°

f=600 MHz, TEM



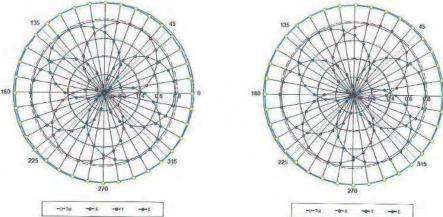


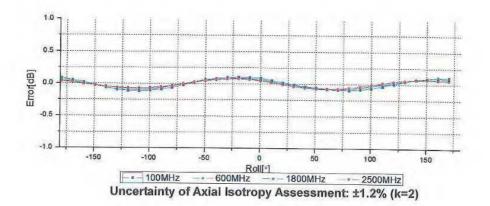

Certificate No: Z17-97087

Page 8 of 11



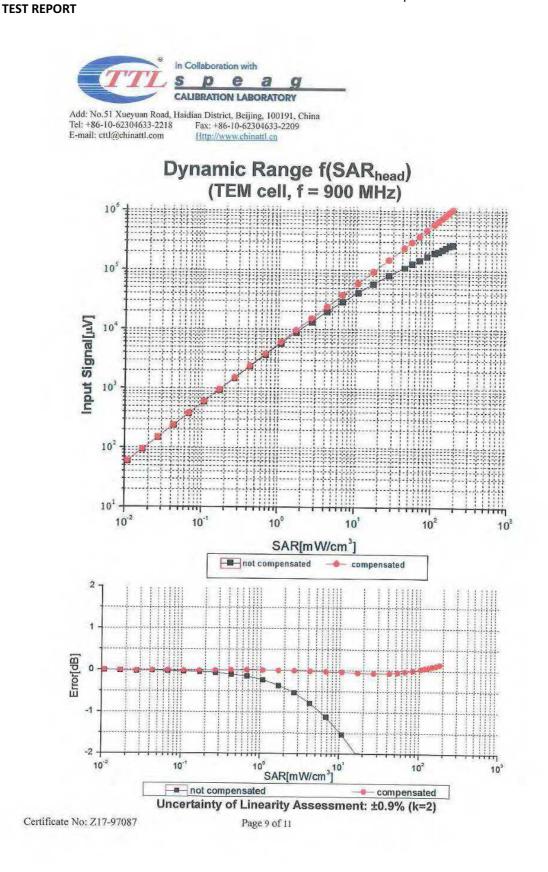



Intertek Report No.: SZHH01201042-006



 Add: No.51 Xueyuan Road, Ilaidian District, Beijing, 100191, China


 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209

 E-mail: cttl@chinattl.com
 <u>Http://www.chinattl.cn</u>

Conversion Factor Assessment

f=835 MHz, WGLS R9(H_convF) f=1750 MHz, WGLS R22(H_convF) 3.50 30.00 3.00 25.00 2.50 20.00 20.00 MIGN/MBIS 2.00 SAR[WI 1.50 10.00 1.00 5.00 0.50 0.00 0.00 0 20 40 60 80 100 0 10 20 30 40 50 60 70 z[mm] z[mm] ----measured -analytical Ę ---measured analytical

Deviation from Isotropy in Liquid

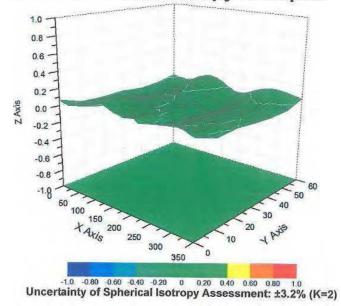

Certificate No: Z17-97087

Page 10 of 11





DASY/EASY – Parameters of Probe: EX3DV4 – SN: 7322

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	41.9
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	9mm
Tip Diameter	2.5mm
Probe Tip to Sensor X Calibration Point	1mm
Probe Tip to Sensor Y Calibration Point	1mm
Probe Tip to Sensor Z Calibration Point	1mm
Recommended Measurement Distance from Surface	1.4mm

Certificate No: Z17-97087

Page 11 of 11

Quality. Assured. EST REPORT	•	Ir	tertek Report No.: SZI	HH0120104
2	CALIB	aboration with D C a g RATION LABORATORY	Hac MRA CN/	中国认行 国际互信 校准 CALIBRA
Tel: +86-10-6 E-mail: ettl <i>ä</i> .	2304633-2218 F	District. Beijing, 100191. China ax: +86-10-62304633-2209 ttp://www.chinattl.cn	Certificate No: Z17-9708	CNAS LO
CALIBRATION	CERTIFIC			
Object	DAE	E4 - SN: 1473		
Calibration Procedure(s	FF-2	Z11-002-01 bration Procedure for the [Ex)	Data Acquisition Electronics	5
Calibration date:		23, 2017		
This calibration Certifica measurements(SI). The pages and are part of the	ate documents th measurements a e certificate.	23, 2017 te traceability to national stand the uncertainties with conf nd the closed laboratory fac	dence probability are given o	on the following
This calibration Certifica measurements(SI). The pages and are part of the All calibrations have be	ate documents th measurements a e certificate. een conducted i	e traceability to national sta nd the uncertainties with conf n the closed laboratory fac	dence probability are given o	on the following
This calibration Certifica measurements(SI). The pages and are part of the All calibrations have be humidity<70%.	ate documents th measurements a e certificate. een conducted i sed (M&TE critica	e traceability to national sta nd the uncertainties with conf n the closed laboratory fac	dence probability are given o lity: environment temperatu	on the following ire(22±3)℃ and
This calibration Certifica measurements(SI). The pages and are part of the All calibrations have be humidity<70%. Calibration Equipment us	ate documents th measurements a e certificate. een conducted i sed (M&TE critica	e traceability to national sta nd the uncertainties with conf n the closed laboratory fac Il for calibration)	dence probability are given of lity: environment temperatu	on the following ire(22±3)℃ and
This calibration Certifica measurements(SI). The pages and are part of the All calibrations have be humidity<70%. Calibration Equipment us Primary Standards Process Calibrator 753	ate documents th measurements a e certificate. een conducted i sed (M&TE critica ID # C	e traceability to national sta nd the uncertainties with conf n the closed laboratory fac Il for calibration) Cal Date(Calibrated by, Certifi	dence probability are given of lity: environment temperatu	on the following rre(22±3)℃ and alibration
This calibration Certifica measurements(SI). The pages and are part of the All calibrations have be humidity<70%. Calibration Equipment us Primary Standards	ate documents th measurements a e certificate. een conducted i sed (M&TE critica ID # (1971018	e traceability to national sta nd the uncertainties with conf n the closed laboratory fac Il for calibration) Cal Date(Calibrated by, Certifi 27-June-16 (CTTL, No:J16	dence probability are given (lity: environment temperatu cate No.) Scheduled Ca X04778) Jun	on the following rre(22±3)℃ and alibration
This calibration Certifica measurements(SI). The pages and are part of the All calibrations have be humidity<70%. Calibration Equipment us Primary Standards Process Calibrator 753	ate documents th measurements a e certificate. een conducted i sed (M&TE critica ID # C 1971018	e traceability to national sta nd the uncertainties with conf n the closed laboratory fac al for calibration) Cal Date(Calibrated by, Certifi 27-June-16 (CTTL, No:J16 Function	dence probability are given (lity: environment temperatu cate No.) Scheduled Ca X04778) Jun	on the following rre(22±3)℃ and alibration

Certificate No: Z17-97086

Page 1 of 3



Intertek Report No.: SZHH01201042-006



Add: No.51 Xueyuan Road. Haidian District. Beijing. 100191, China Tel: 186-10-62301633-2218 Fax: =86-10-62304633-2209 E-mail: cttl@chinattl.com Http://www.chinattl.en

Glossary: DAE Connector angle

data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters:

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.

Certificate No: Z17-97086

Page 2 of 3



Intertek Report No.: SZHH01201042-006



 Add: No.51 Xueyuan Road. Haidian District. Beijing, 100191. China

 Tel: +86-10-62304633-2218
 Fax: +86-10-62304633-2209

 E-mail: cttl@chinattl.com
 Http://www.chinattl.en

DC Voltage Measurement

 A/D - Converter Resolution nominal

 High Range:
 1LSB =
 6.1μV ,
 full range =
 -100...+300 mV

 Low Range:
 1LSB =
 61nV ,
 full range =
 -1.....+3mV

 DASY measurement parameters:
 Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	Х	Y	Z
High Range	403.995 ± 0.15% (k=2)	$404.595 \pm 0.15\% \ (k{=}2)$	404.448 ± 0.15% (k=2)
Low Range	3.96487 ± 0.7% (k=2)	3.99568 ± 0.7% (k=2)	3.99012 ± 0.7% (k=2)

Connector Angle

46.5° ± 1 °	
3	346.5°±1°

Certificate No: Z17-97086

Page 3 of 3



Calibration Laboratory of

TEST REPORT

Intertek Report No.: SZHH01201042-006

Schweizerischer Kalibrierdienst

S

Schmid & Partner Service suisse d'étalonnage C **Engineering AG** Servizio svizzero di taratura Zeughausstrasse 43, 8004 Zurich, Switzerland S Swiss Calibration Service Accredited by the Swiss Accreditation Service (SAS) Accreditation No.: SCS 0108 The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Client Intertek HK (Auden) Certificate No: D2450V2-966 Jun15 **CALIBRATION CERTIFICATE** D2450V2 - SN: 966 Object QA CAL-05.v9 Calibration procedure(s) Calibration procedure for dipole validation kits above 700 MHz Calibration date: June 10, 2015 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (M&TE critical for calibration) Primary Standards ID # Cal Date (Certificate No.) Scheduled Calibration Power meter EPM-442A GB37480704 07-Oct-14 (No. 217-02020) Oct-15 Power sensor HP 8481A US37292783 07-Oct-14 (No. 217-02020) Oct-15 Power sensor HP 8481A MY41092317 07-Oct-14 (No. 217-02021) Oct-15 SN: 5058 (20k) Reference 20 dB Attenuator 01-Apr-15 (No. 217-02131) Mar-16 Type-N mismatch combination SN: 5047.2 / 06327 01-Apr-15 (No. 217-02134) Mar-16 Reference Probe ES3DV3 SN: 3205 30-Dec-14 (No. ES3-3205_Dec14) Dec-15 DAE4 SN: 601 18-Aug-14 (No. DAE4-601_Aug14) Aug-15 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator R&S SMT-06 100005 04-Aug-99 (in house check Oct-13) In house check: Oct-16 Network Analyzer HP 8753E US37390585 S4206 18-Oct-01 (in house check Oct-14) In house check: Oct-15 Name Function Signature Calibrated by: Israe Elnaoug Laboratory Technician Ward Approved by: Katja Pokovic Technical Manager

Issued: June 10, 2015

Certificate No: D2450V2-966_Jun15

Page 1 of 8

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Intertek Report No.: SZHH01201042-006

S

S

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power. 0
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-966 Jun15



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.9 ± 6 %	1.84 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.7 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	53.8 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured	condition 250 mW input power	6.41 W/kg

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	50.7 ± 6 %	2.03 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	(22) (22)	

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.4 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	52.1 W/kg ± 17.0 % (k=2)
		CALL AND
SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR averaged over 10 cm ³ (10 g) of Body TSL SAR measured	condition 250 mW input power	6.22 W/kg

Certificate No: D2450V2-966_Jun15



Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.3 Ω + 2.0 jΩ
Return Loss	- 28.6 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.1 Ω + 3.9 jΩ
Return Loss	- 28.2 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.156 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	November 19, 2014

Certificate No: D2450V2-966_Jun15

Page 4 of 8



DASY5 Validation Report for Head TSL

Date: 10.06.2015

Test Laboratory: SPEAG, Zurich, Switzerland


DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 966

Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz; $\sigma = 1.84$ S/m; $\varepsilon_r = 37.9$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.54, 4.54, 4.54); Calibrated: 30.12.2014;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 102.4 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 28.2 W/kg SAR(1 g) = 13.7 W/kg; SAR(10 g) = 6.41 W/kg Maximum value of SAR (measured) = 17.9 W/kg

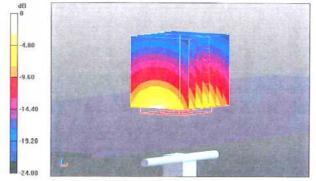


0 dB = 17.9 W/kg = 12.53 dBW/kg

Certificate No: D2450V2-966_Jun15

Page 5 of 8



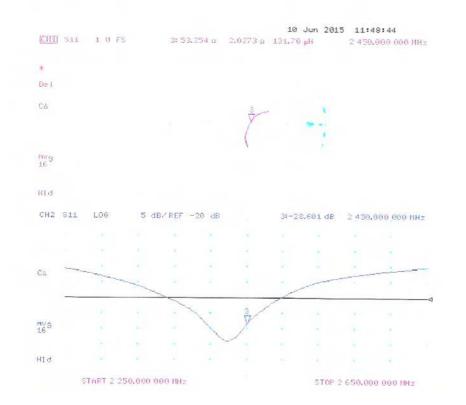

Impedance Measurement Plot for Head TSL

Certificate No: D2450V2-966_Jun15

Page 6 of 8



DASY5 Validation Report for Body TSL

Date: 10.06.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 966


Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz; $\sigma = 2.03$ S/m; $\epsilon_r = 50.7$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.32, 4.32, 4.32); Calibrated: 30.12.2014;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 95.29 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 27.6 W/kg SAR(1 g) = 13.4 W/kg; SAR(10 g) = 6.22 W/kg Maximum value of SAR (measured) = 17.3 W/kg

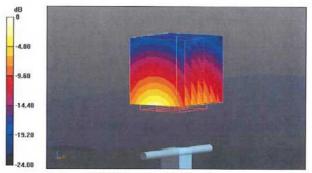


0 dB = 17.3 W/kg = 12.38 dBW/kg

Certificate No: D2450V2-966_Jun15

Page 7 of 8



Impedance Measurement Plot for Body TSL

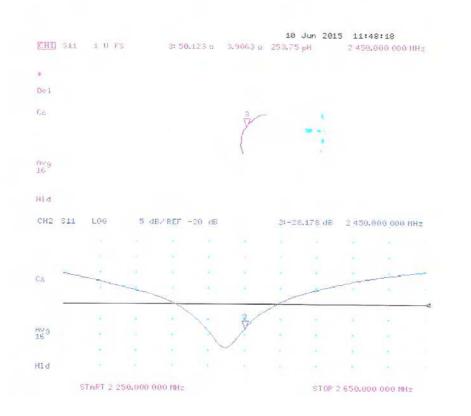

Certificate No: D2450V2-966_Jun15

Page 8 of 8